



US00D580281S

(12) **United States Design Patent**
Lewis

(10) **Patent No.:** **US D580,281 S**
(45) **Date of Patent:** **** Nov. 11, 2008**

(54) **DOSIMETER BADGE**

(57) **CLAIM**

(75) Inventor: **David Fairhurst Lewis**, Monroe, CT
(US)

The ornamental design for a dosimeter badge, as shown and described.

(73) Assignee: **ISP Investments Inc.**, Wilmington, DE
(US)

DESCRIPTION

(**) Term: **14 Years**

FIG. 1 is a front view of one embodiment of the dosimeter badge of the present invention;

(21) Appl. No.: **29/296,855**

FIG. 2 is a right-side elevational view of the dosimeter badge thereof, the left-side elevational view being identical thereto;

(22) Filed: **Oct. 30, 2007**

FIG. 3 is a front elevational view of the dosimeter badge thereof; the rear elevational view being identical thereto;

(51) **LOC (8) Cl.** **10-04**

FIG. 4 is a rear view of the dosimeter badge thereof;

(52) **U.S. Cl.** **D10/47**

FIG. 5 is a front view of a second embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4;

(58) **Field of Classification Search** D10/47;
250/370.01, 370.07, 370 P, 473.1, 474.1,
250/484.3-484.5; 356/319, 328

See application file for complete search history.

FIG. 6 is a front view of a third embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4;

(56) **References Cited**

FIG. 7 is a front view of a fourth embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4;

U.S. PATENT DOCUMENTS

5,051,597	A	9/1991	Lewis et al.	
5,084,623	A	1/1992	Lewis et al.	
D325,171	S *	4/1992	Laffaille D10/47
5,173,609	A *	12/1992	Lacoste et al. 250/370.07
5,359,200	A	10/1994	Donahue et al.	
5,637,876	A	6/1997	Donahue et al.	
5,767,520	A	6/1998	Donahue et al.	
5,777,341	A	7/1998	Seiwatz et al.	
6,268,602	B1	7/2001	Seiwatz et al.	
D539,177	S *	3/2007	Widener et al. D10/47
7,227,158	B1	6/2007	Patel et al.	
7,420,187	B1 *	9/2008	Klemic et al. 250/484.5

FIG. 8 is a front view of a fifth embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4; and

OTHER PUBLICATIONS

U.S. Appl. No. 29/271,271, filed Jan. 12, 2007, Lewis et al.
Wavelengths Online Press Release entitled "Division Researchers Are Awarded Terrorism-Related Project" (May 17, 2005).

FIG. 9 is a front view of a sixth embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4.

FIG. 10 is a front view of a seventh embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4; and,

FIG. 11 is a front view of an eighth embodiment of the dosimeter badge of the present invention, the remaining views being the same as set forth in FIGS. 2-4.


(Continued)

The broken lines, including those forming the numerals and text, have been shown for illustrative purposes only and form no part of the claimed design. Shading has been shown to represent that portions of the claimed design have different colors.

Primary Examiner—Antoine D Davis

(74) *Attorney, Agent, or Firm*—William J. Davis

1 Claim, 10 Drawing Sheets

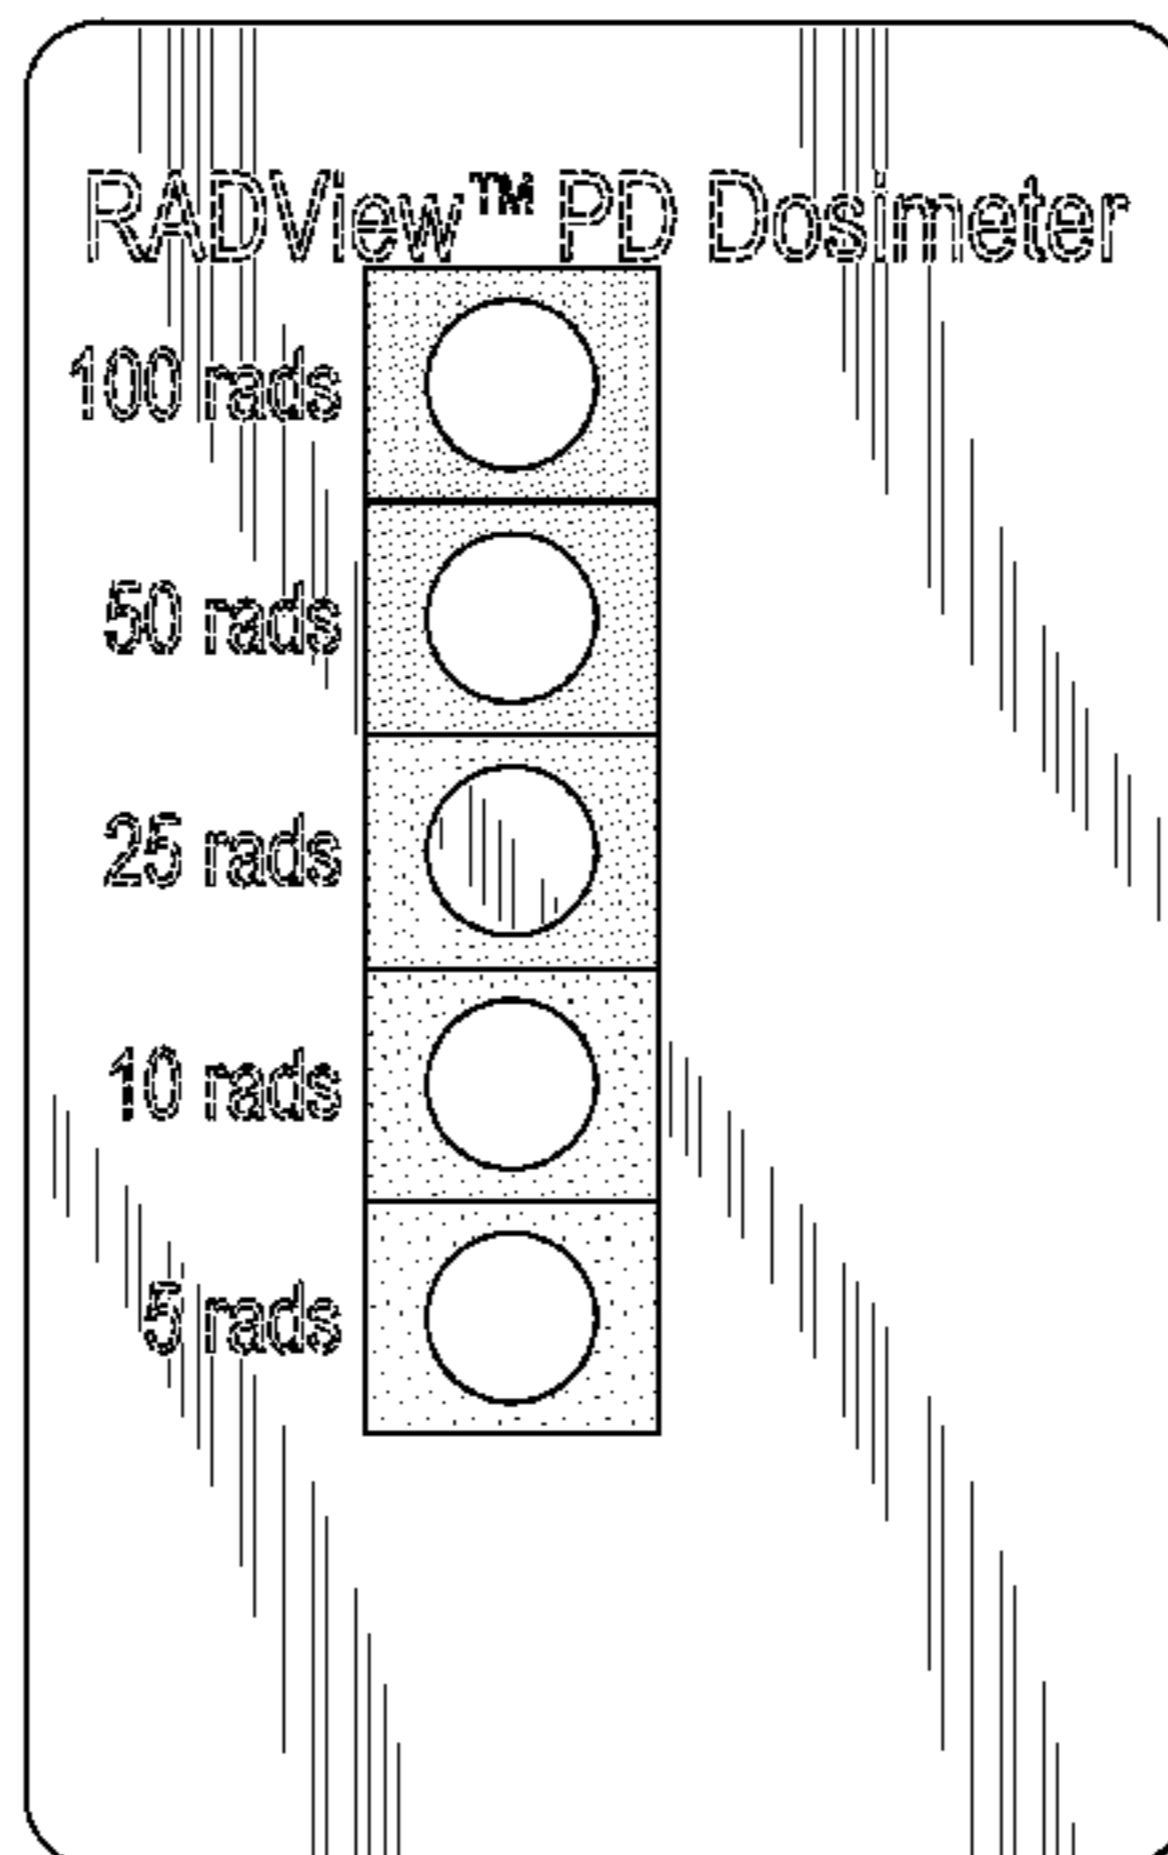

OTHER PUBLICATIONS

“RADTriage—A Dual Sensor Personal Smart Dosimeter,” by JP Laboratories, Inc. (date of first publication unknown).

“RadTag—An innovative way to confirm your blood products were irradiated,” by RadTag Technologies (date of first publication unknown).

Abstract for Irie, S. et al., “The Radiation-Induced Coloration of Amorphous Photochromic Dithienylethene Films,” *Bulletin of the Chemical Society of Japan*, vol. 77, No. 5, pp. 1037-1040 (2004).

Petkov, I. et al., “New Two-Functional UVR Sunscreen Protector and Dosimeter” (date of first publication unknown).

Press Release by International Specialty Products entitled “A New Radiation Monitoring Badge for Emergency and Disaster Response Personnel” (Jan. 16, 2006).

“What is SIRAD—Self-indicating Instant Radiation Alert Dosimeter” (date of first publication unknown).

* cited by examiner

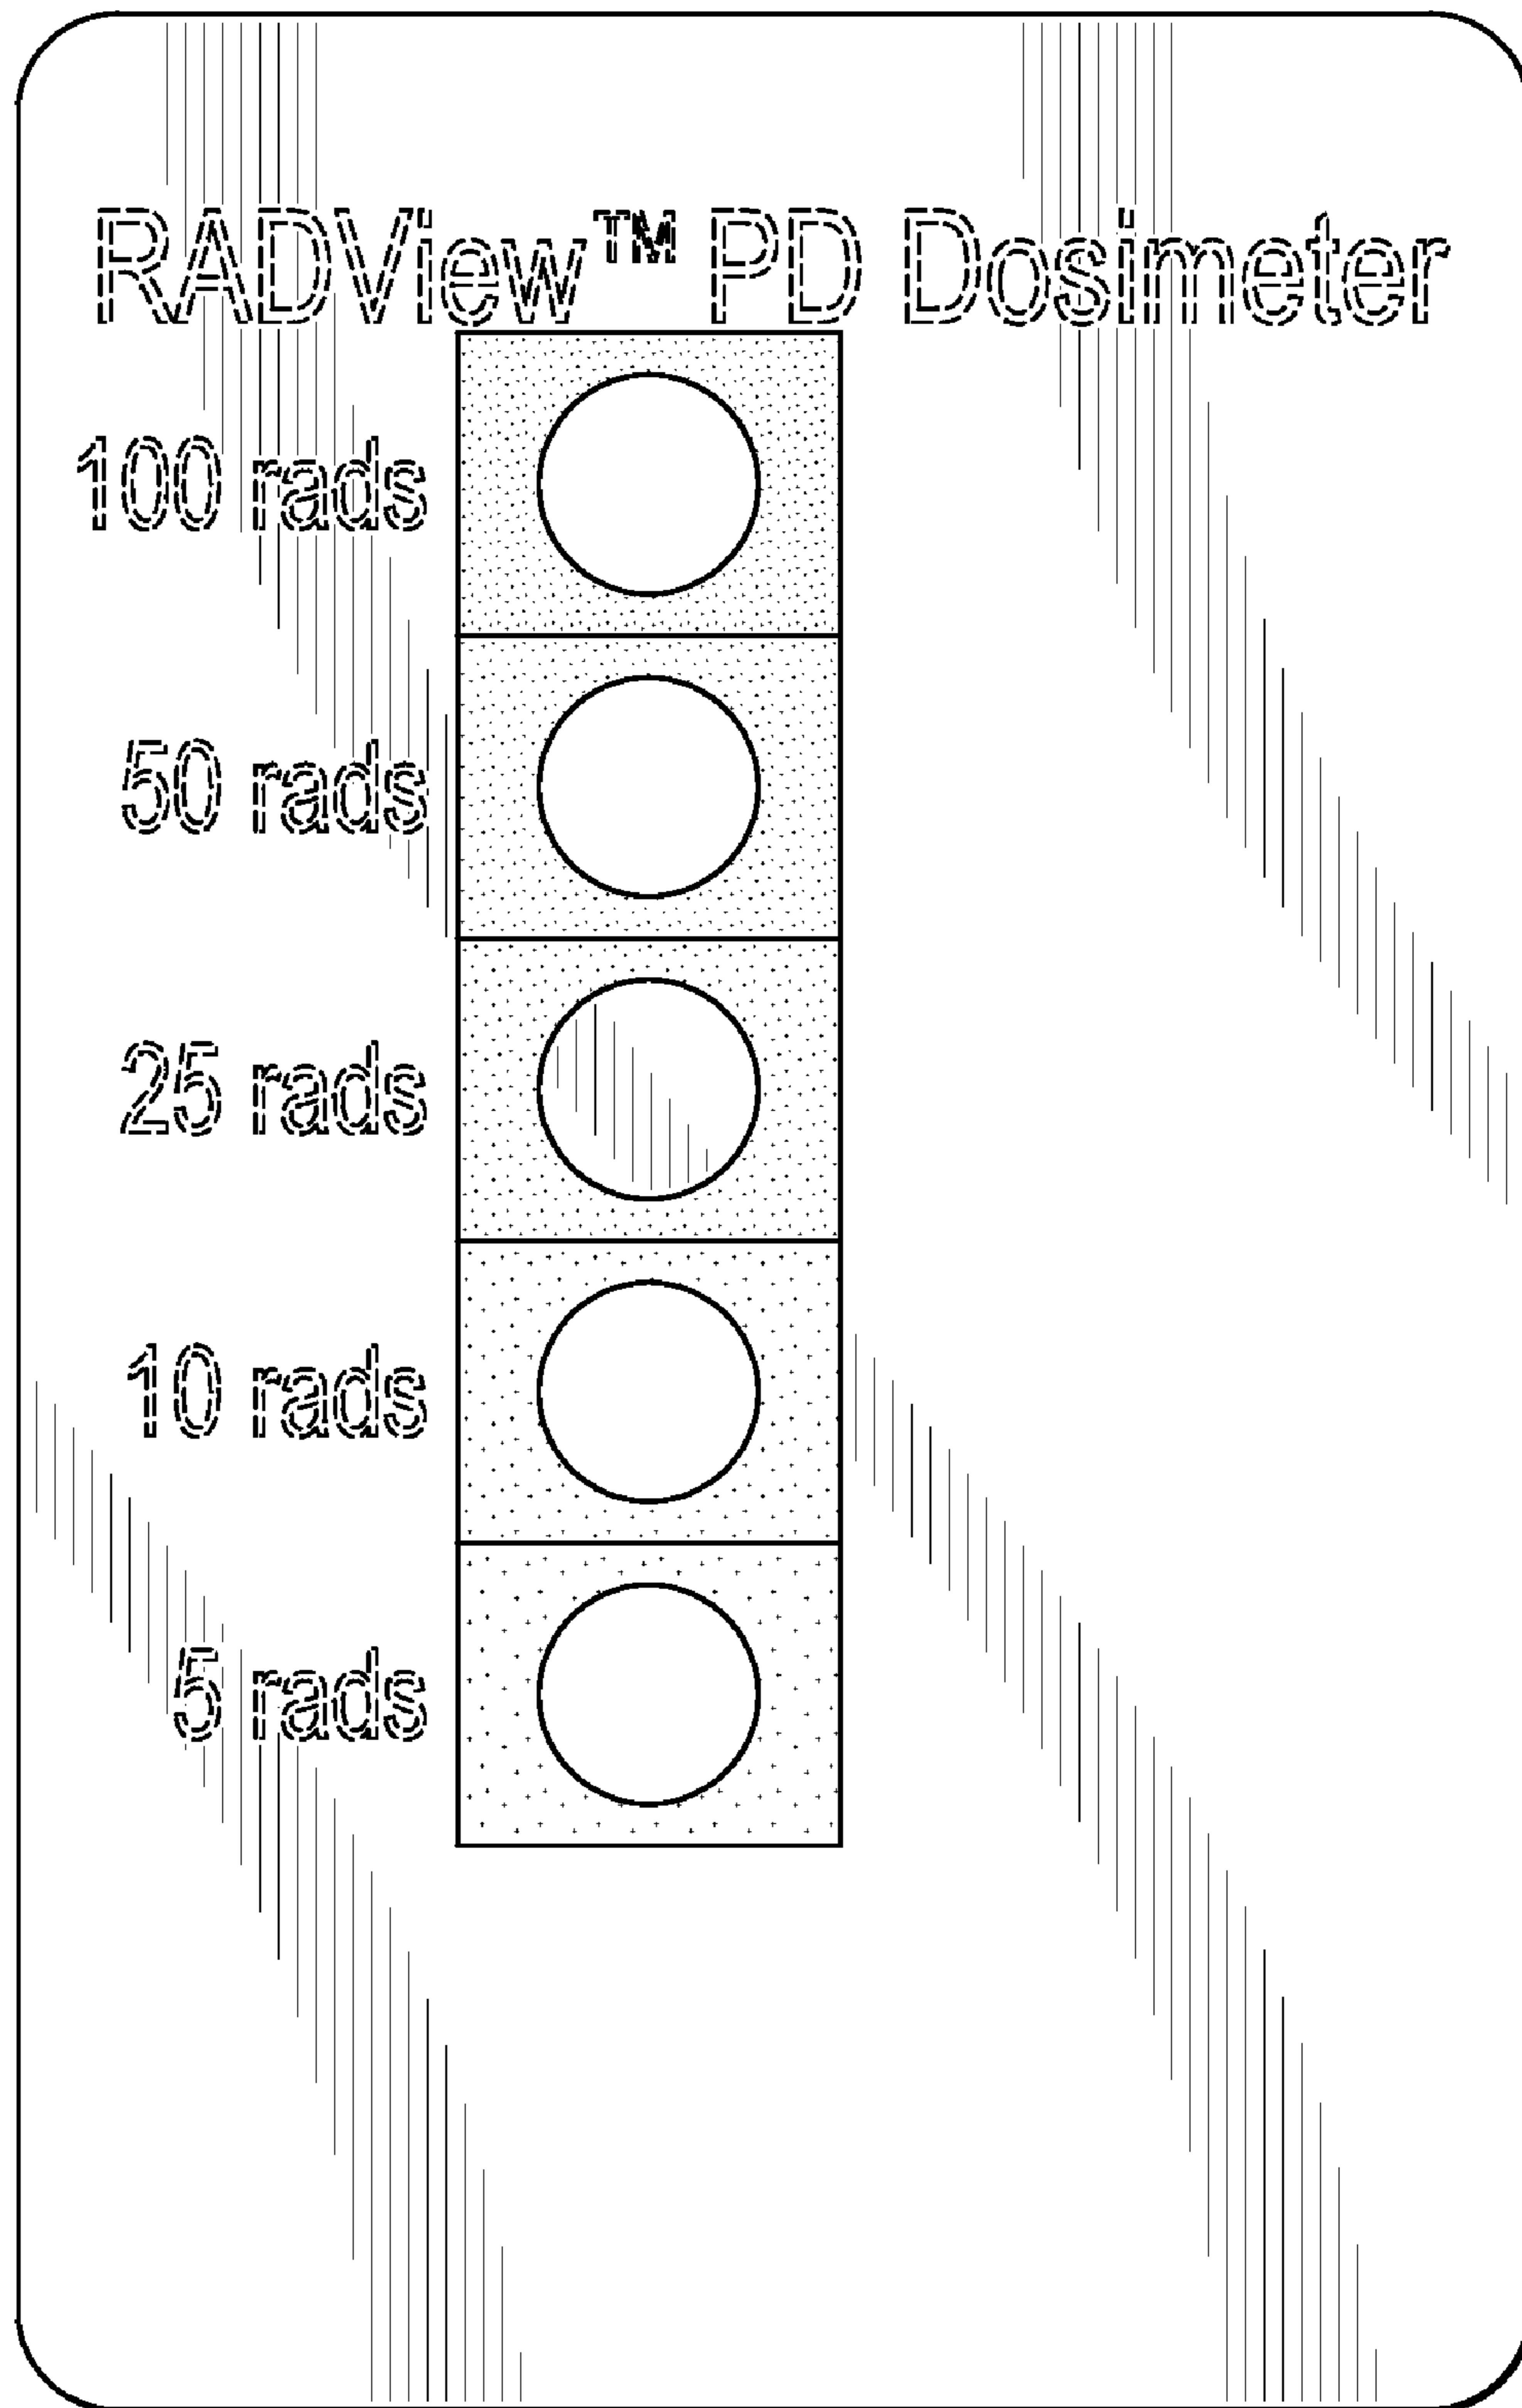


FIG. 1



FIG. 2



FIG. 3

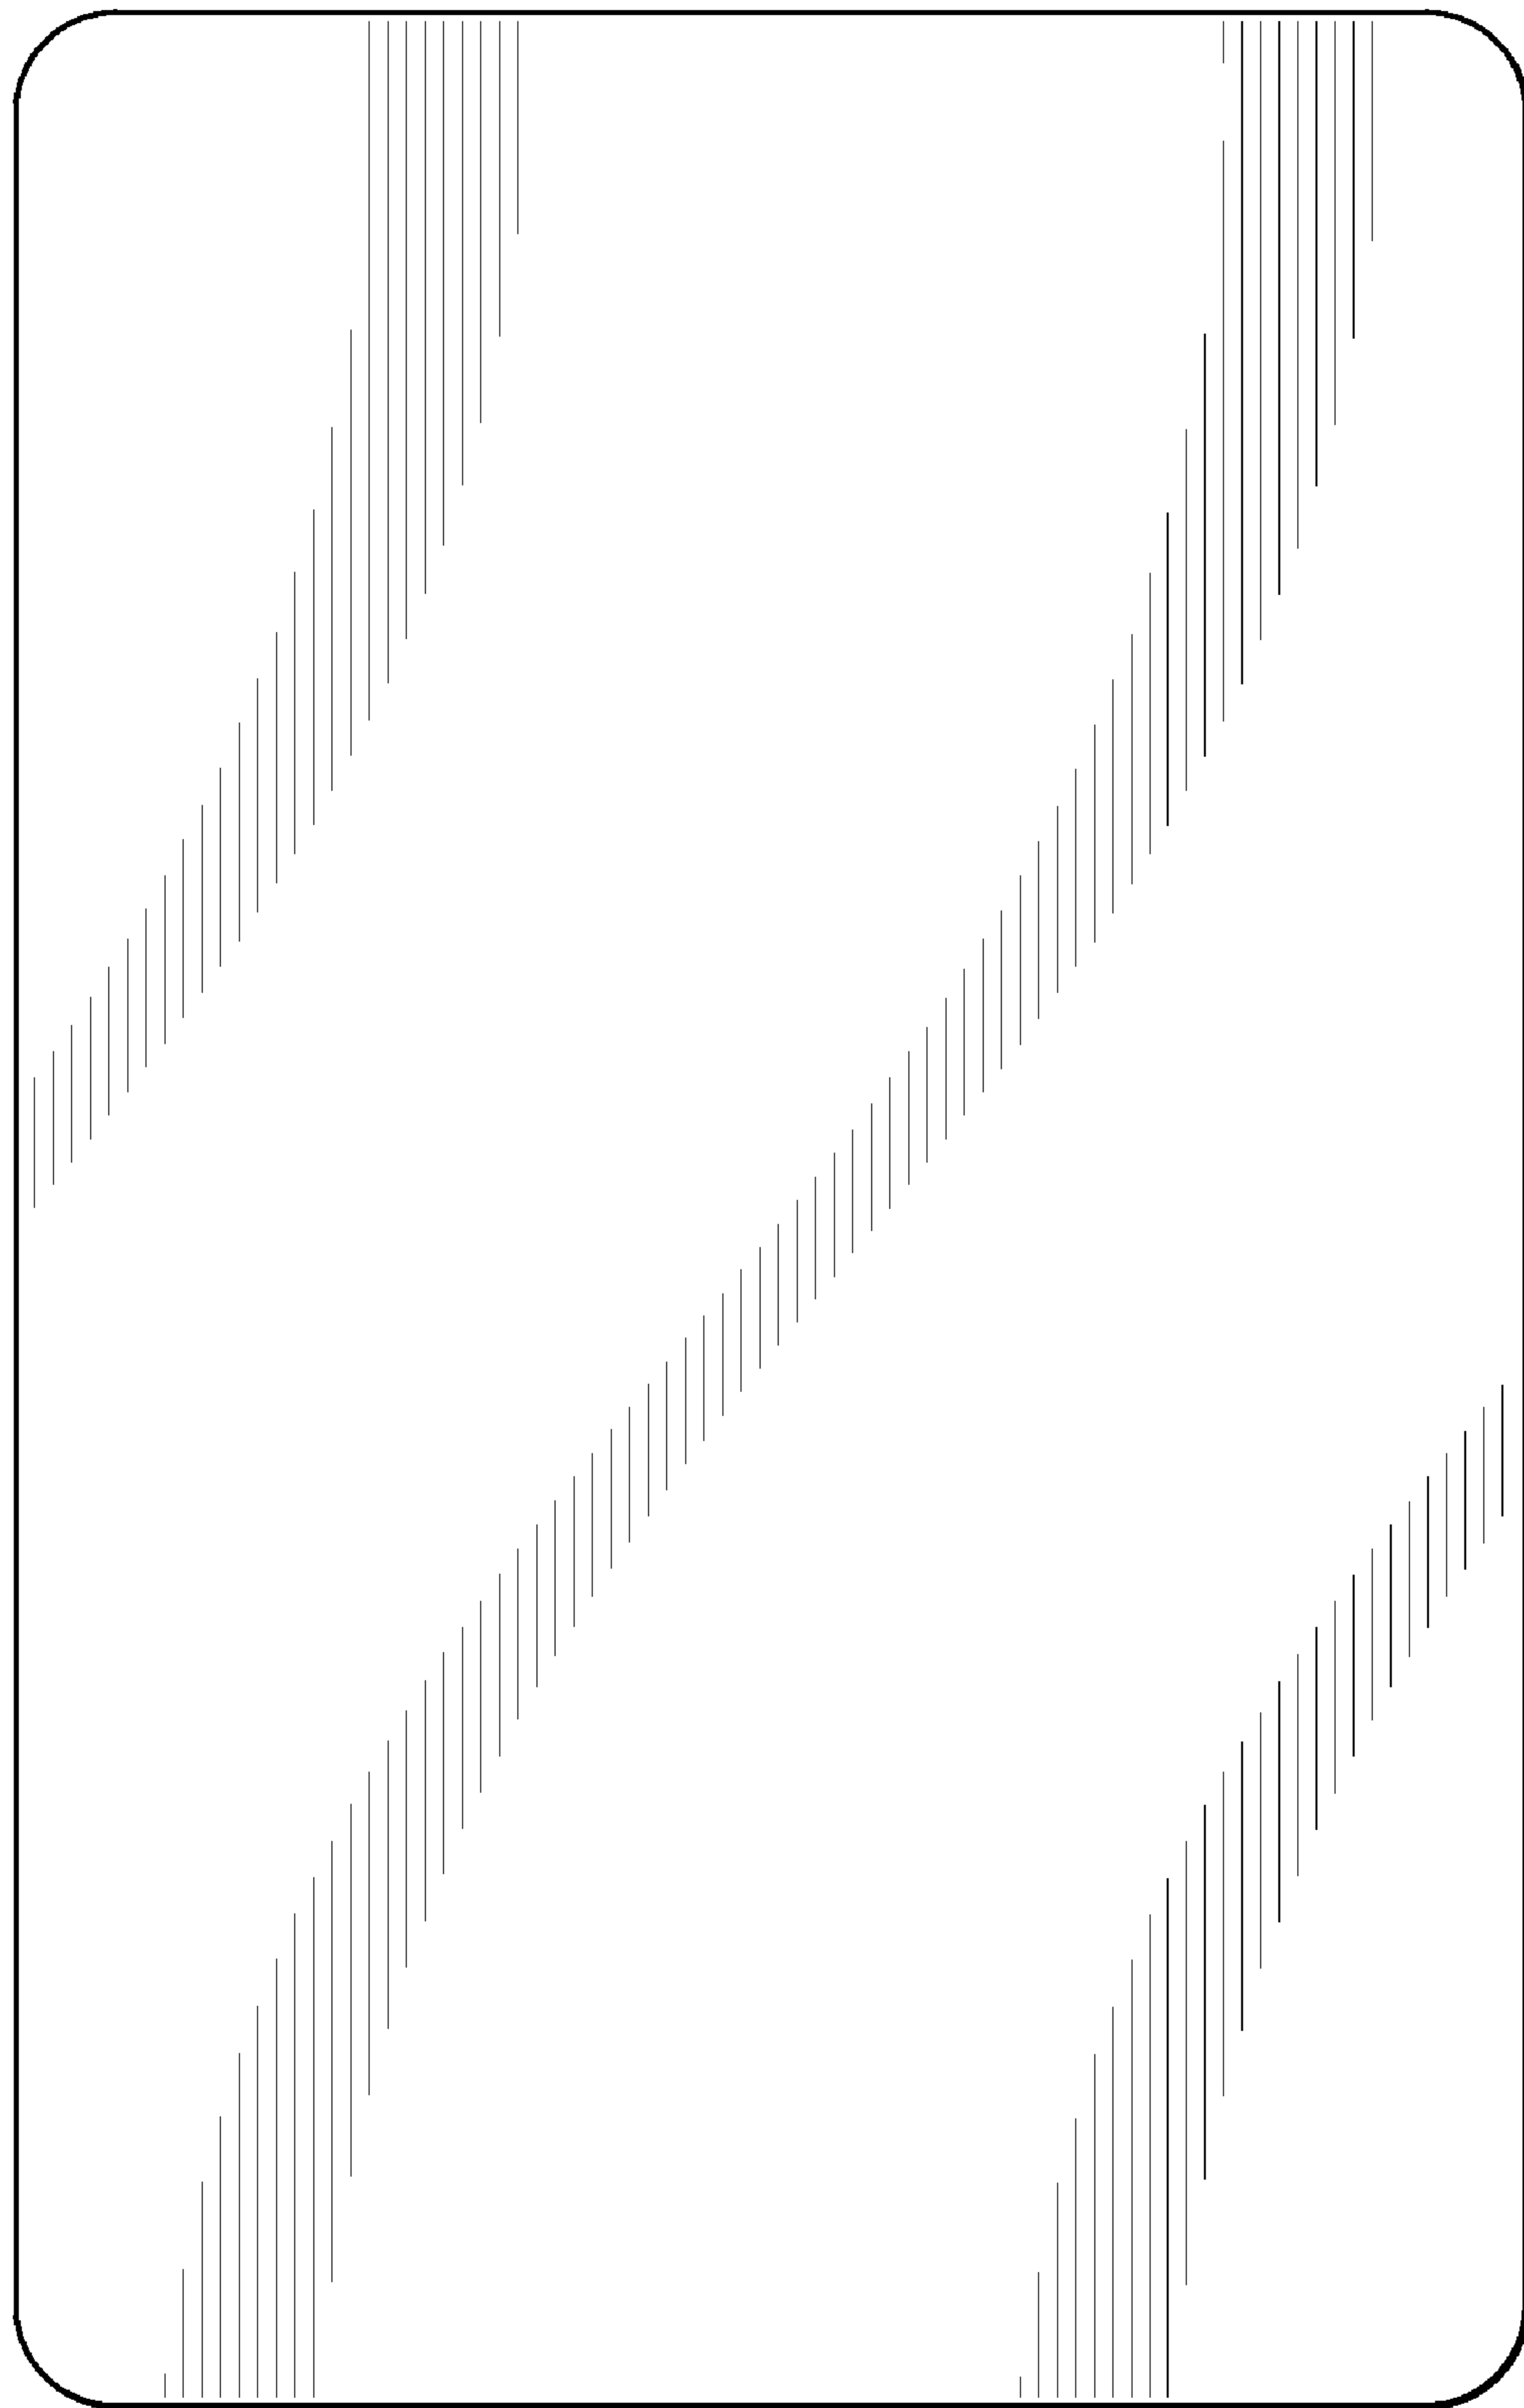


FIG. 4

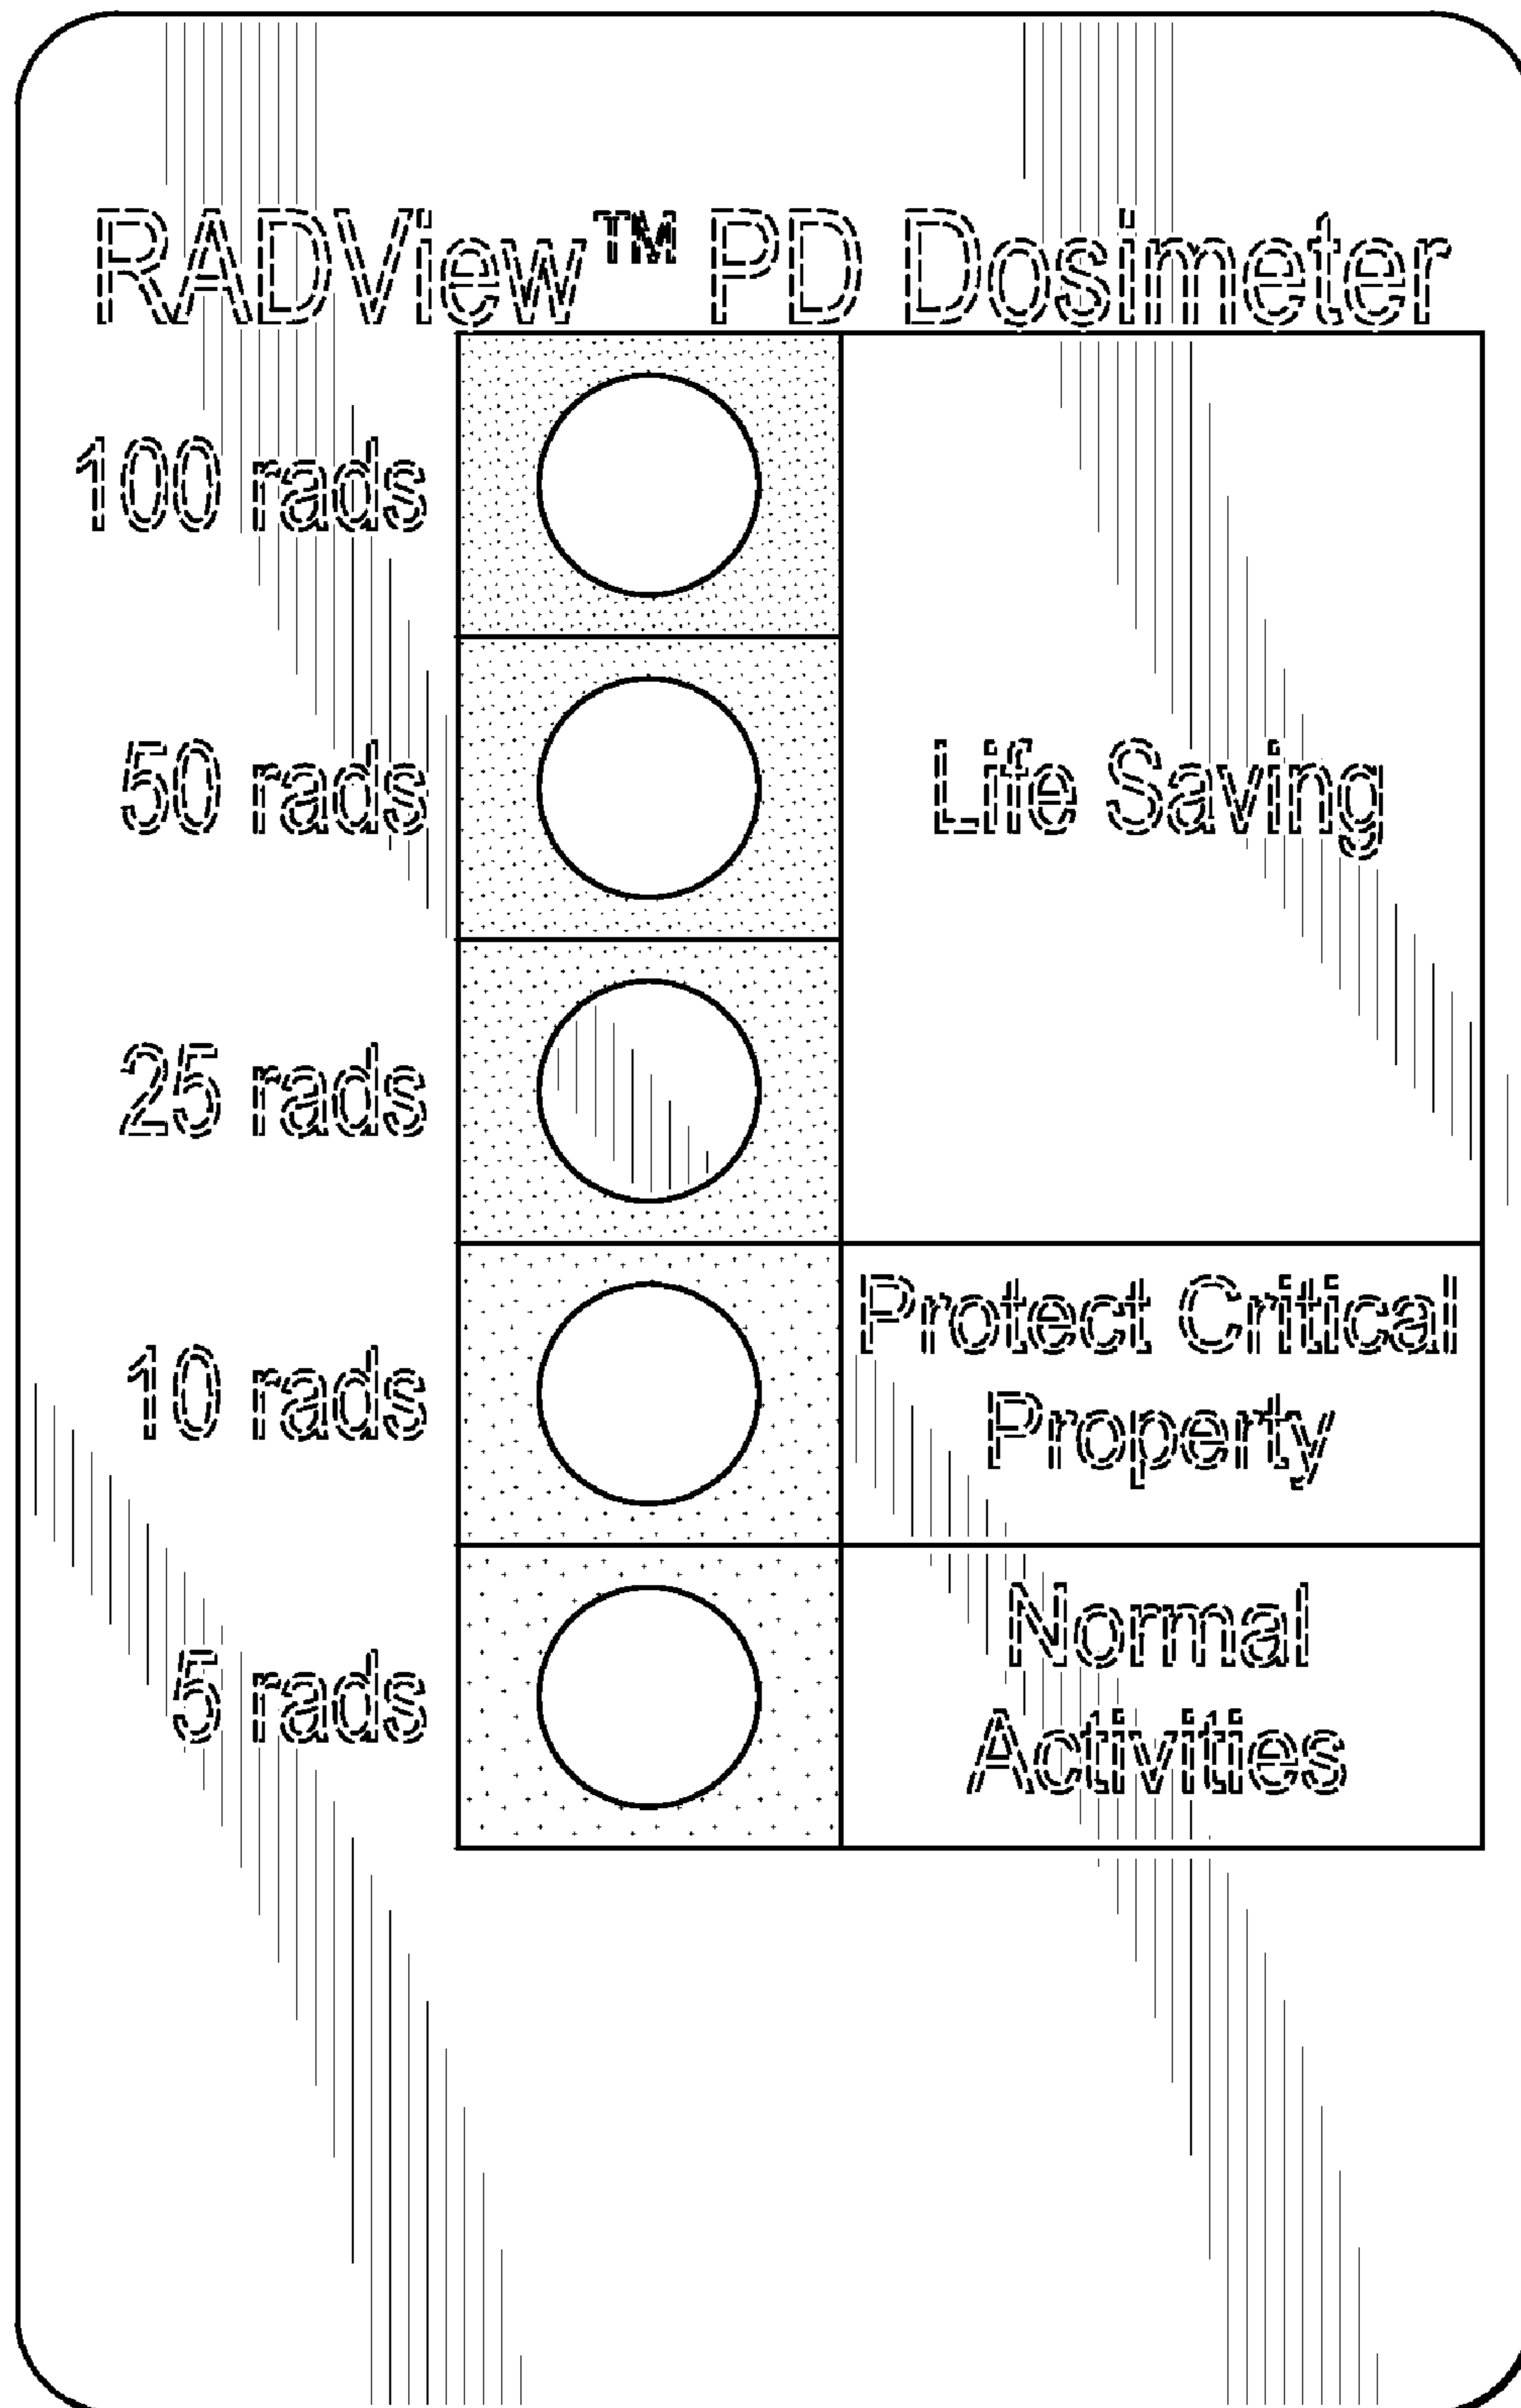


FIG. 5

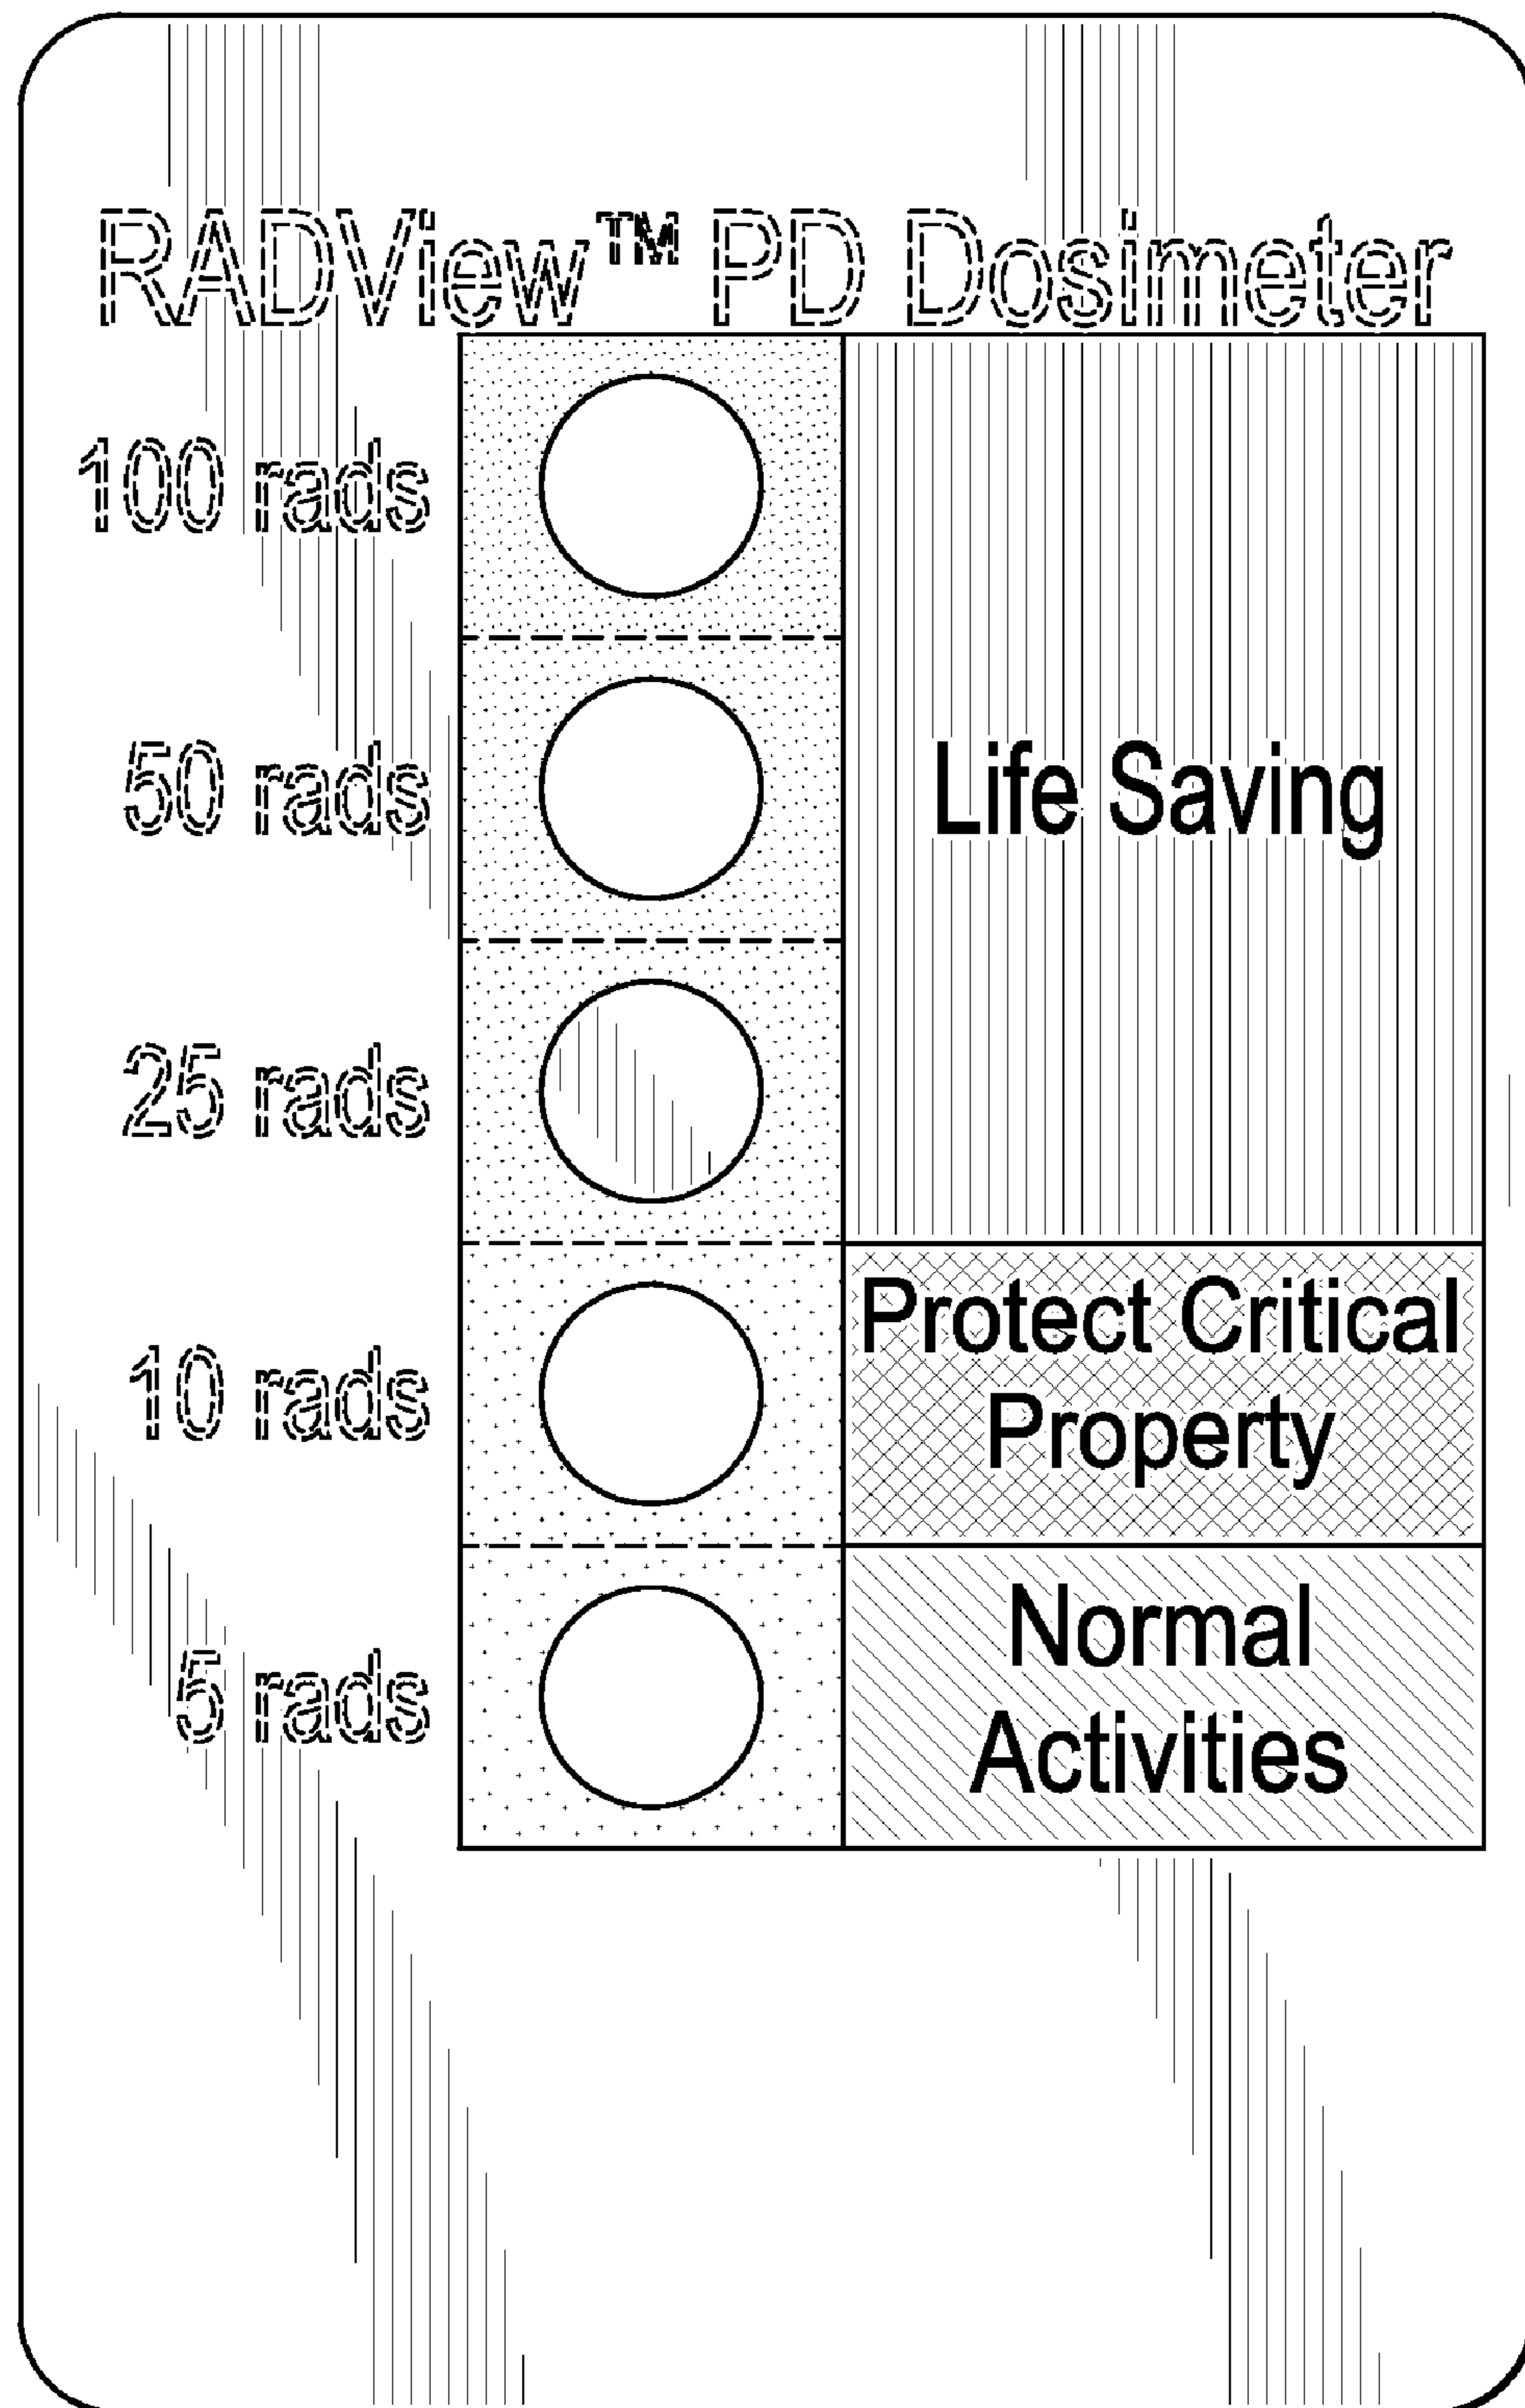


FIG. 6

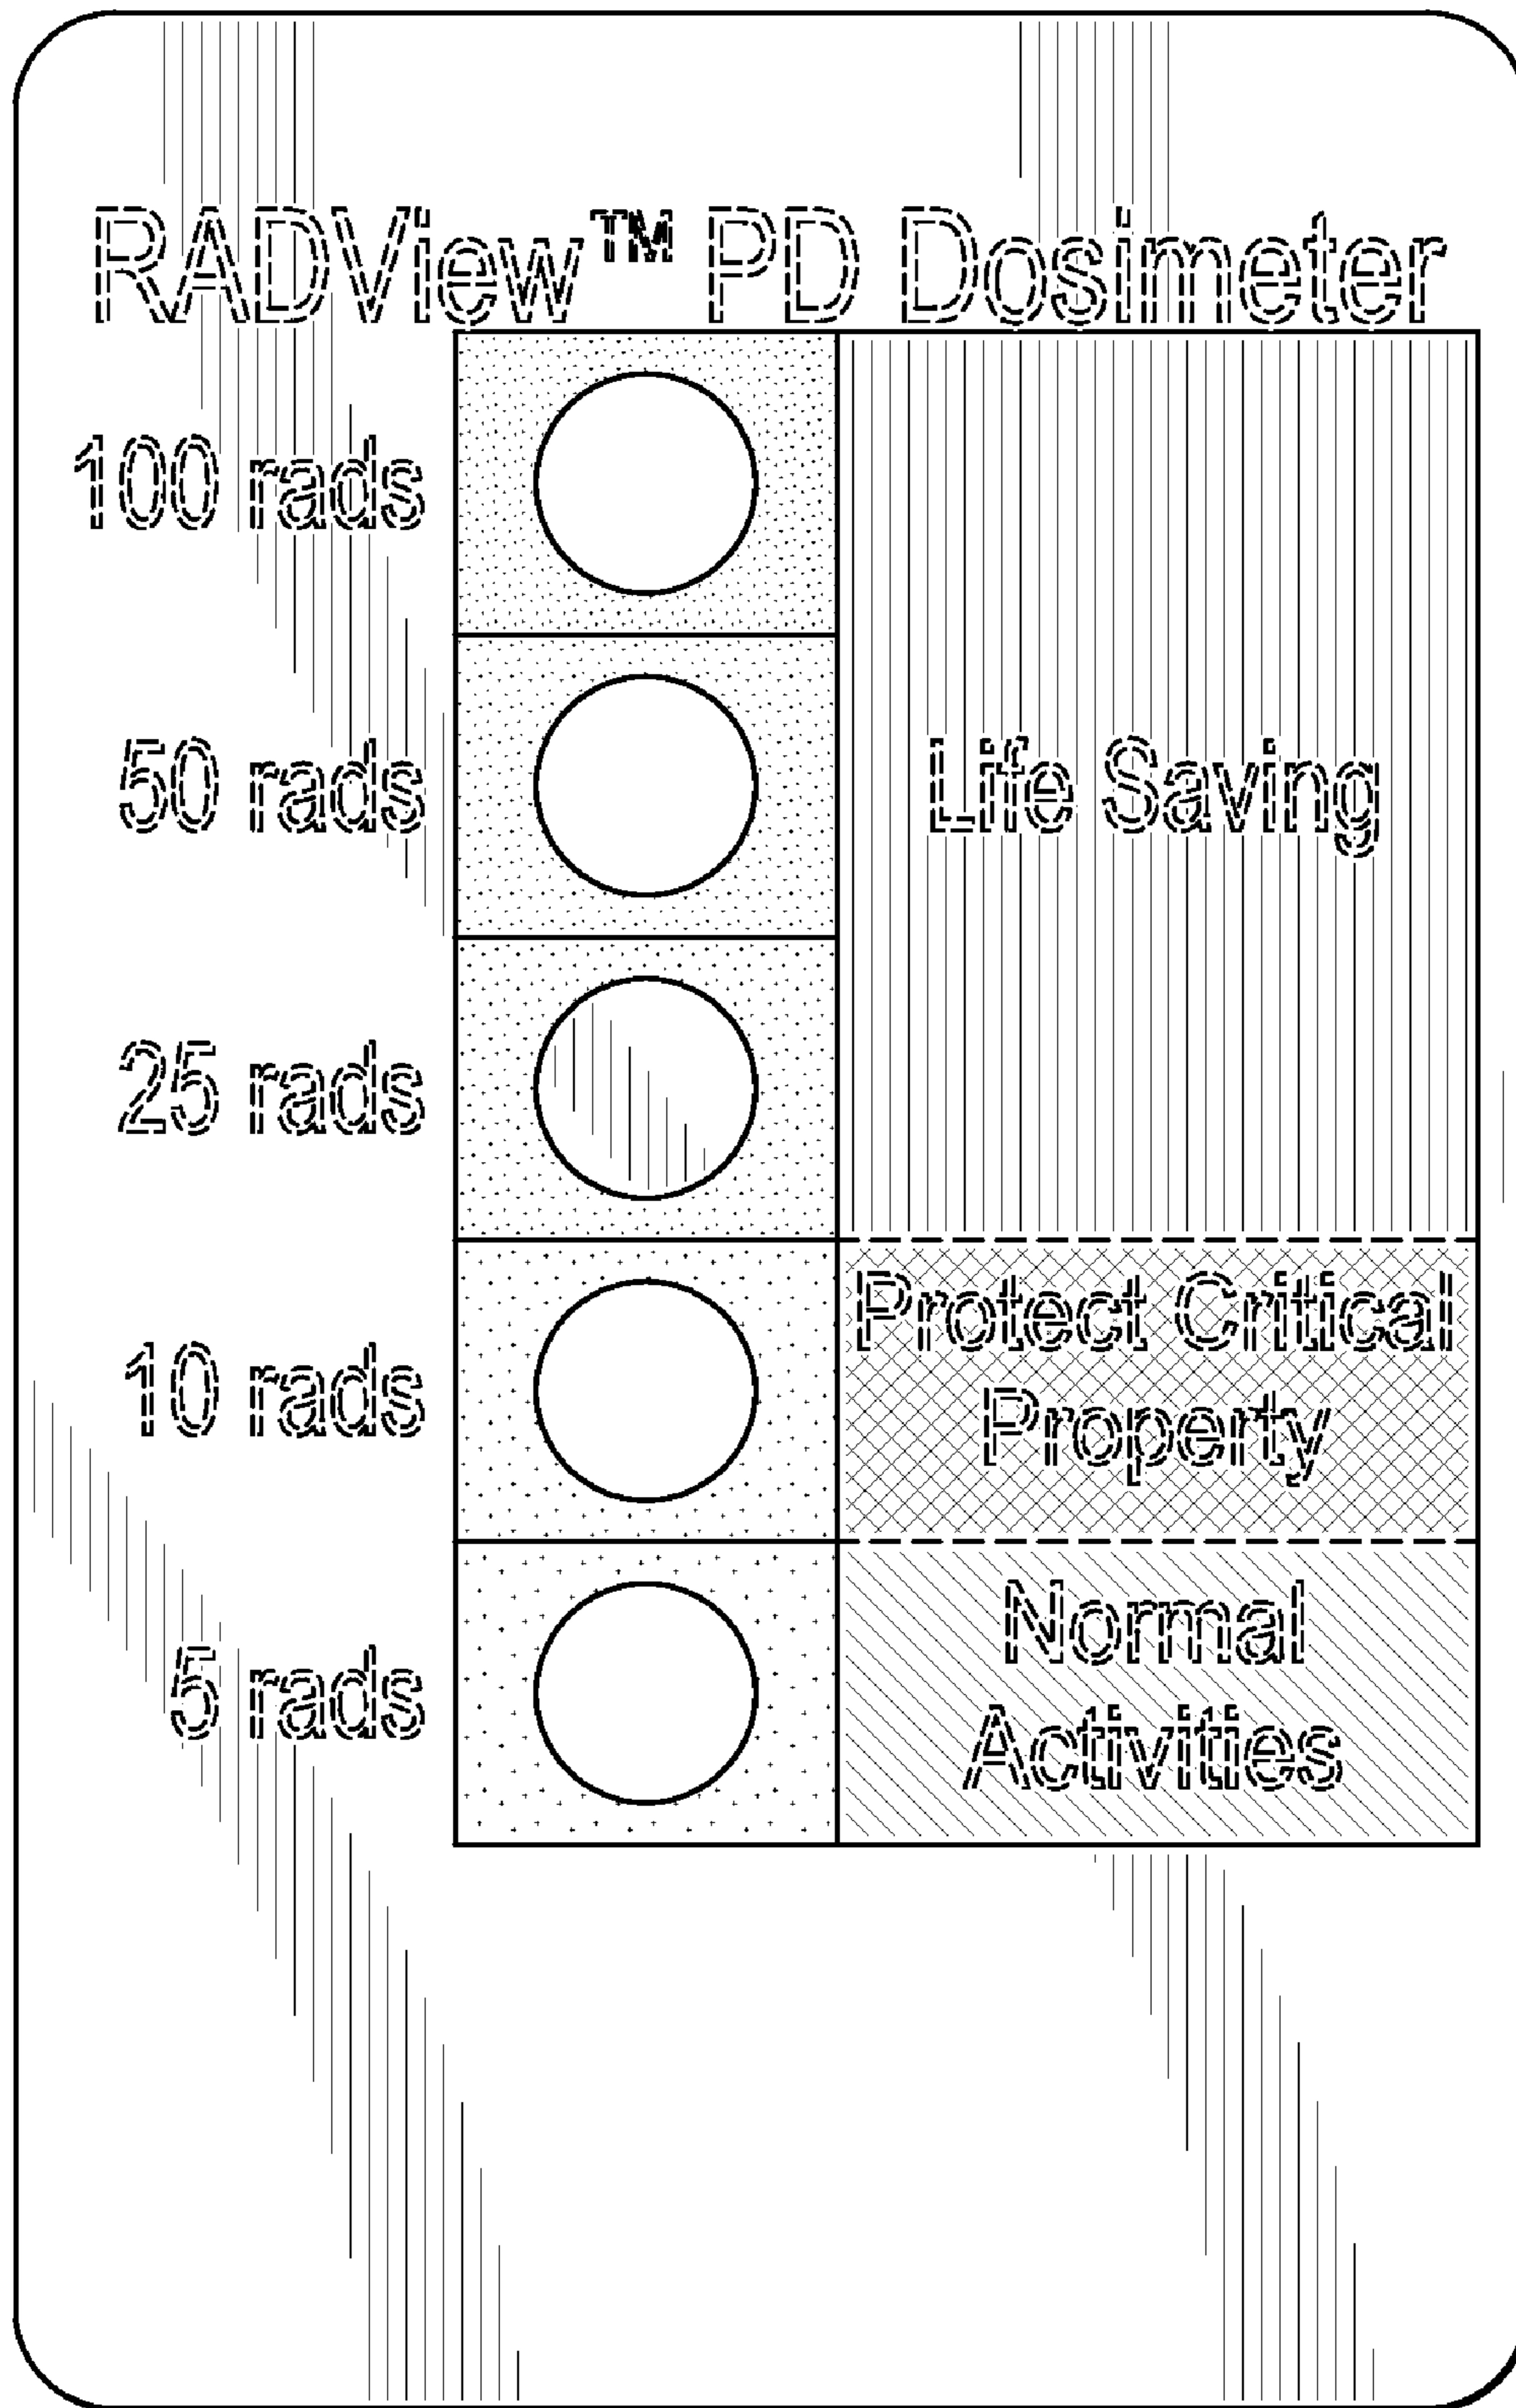


FIG. 7

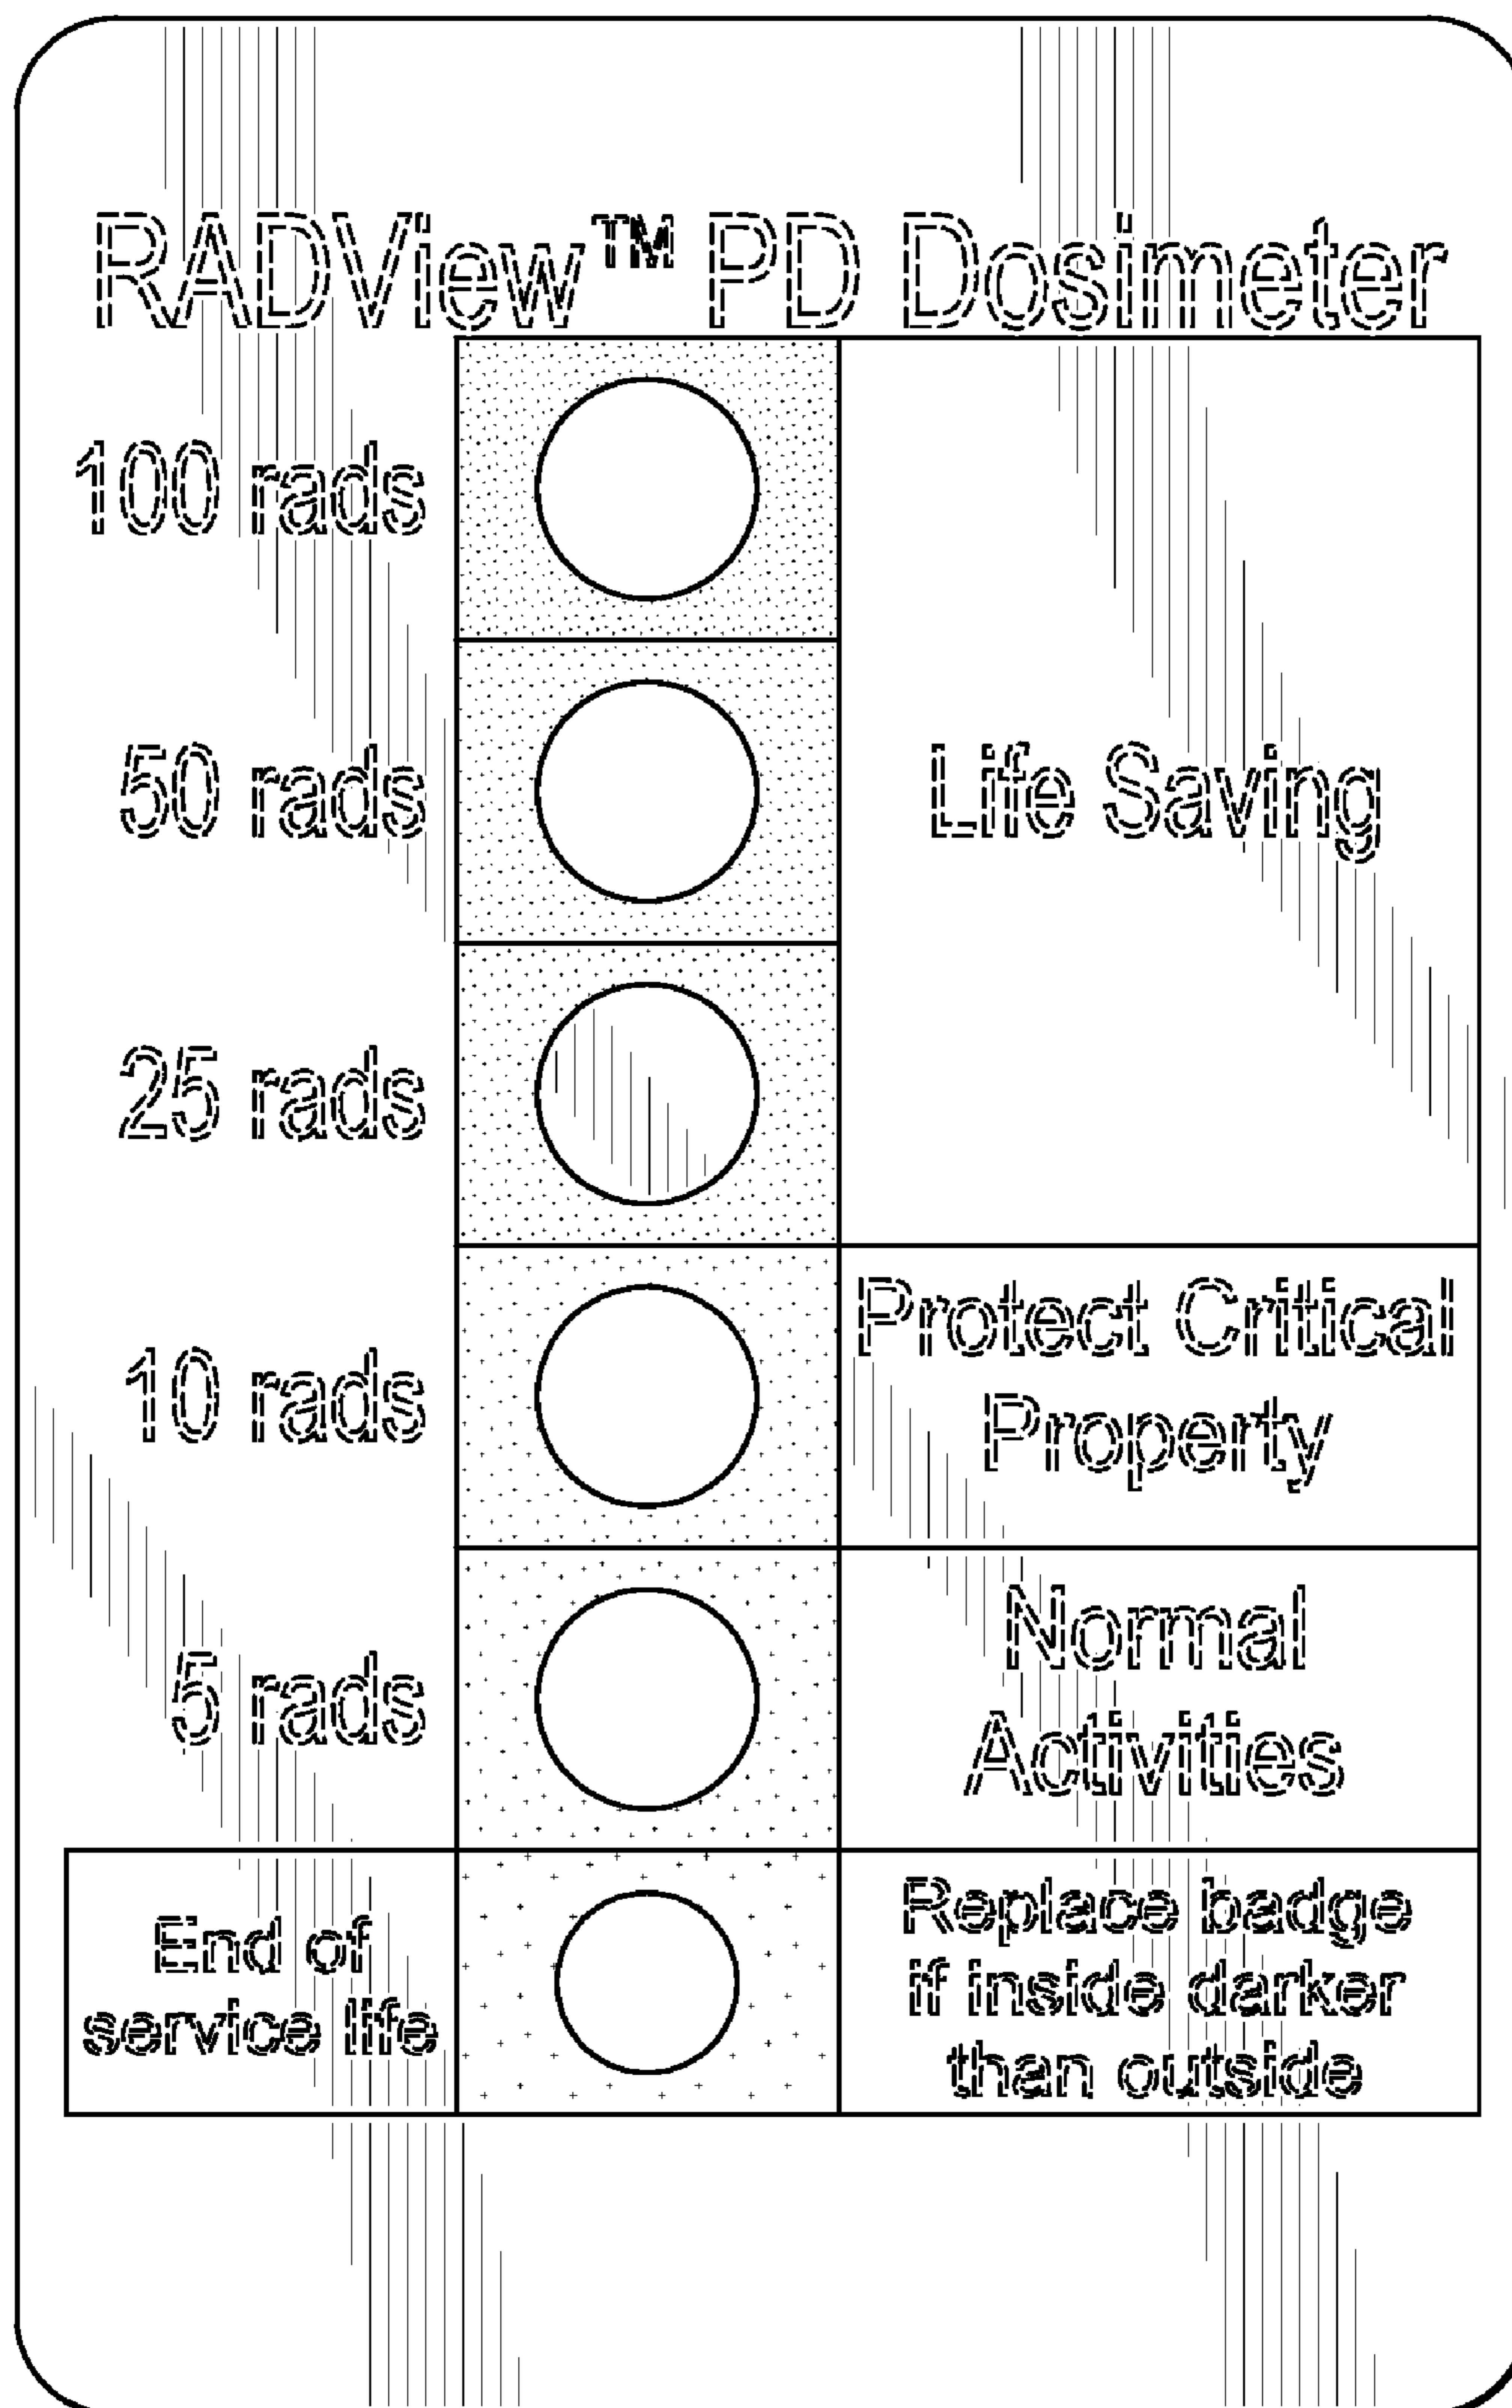


FIG. 8

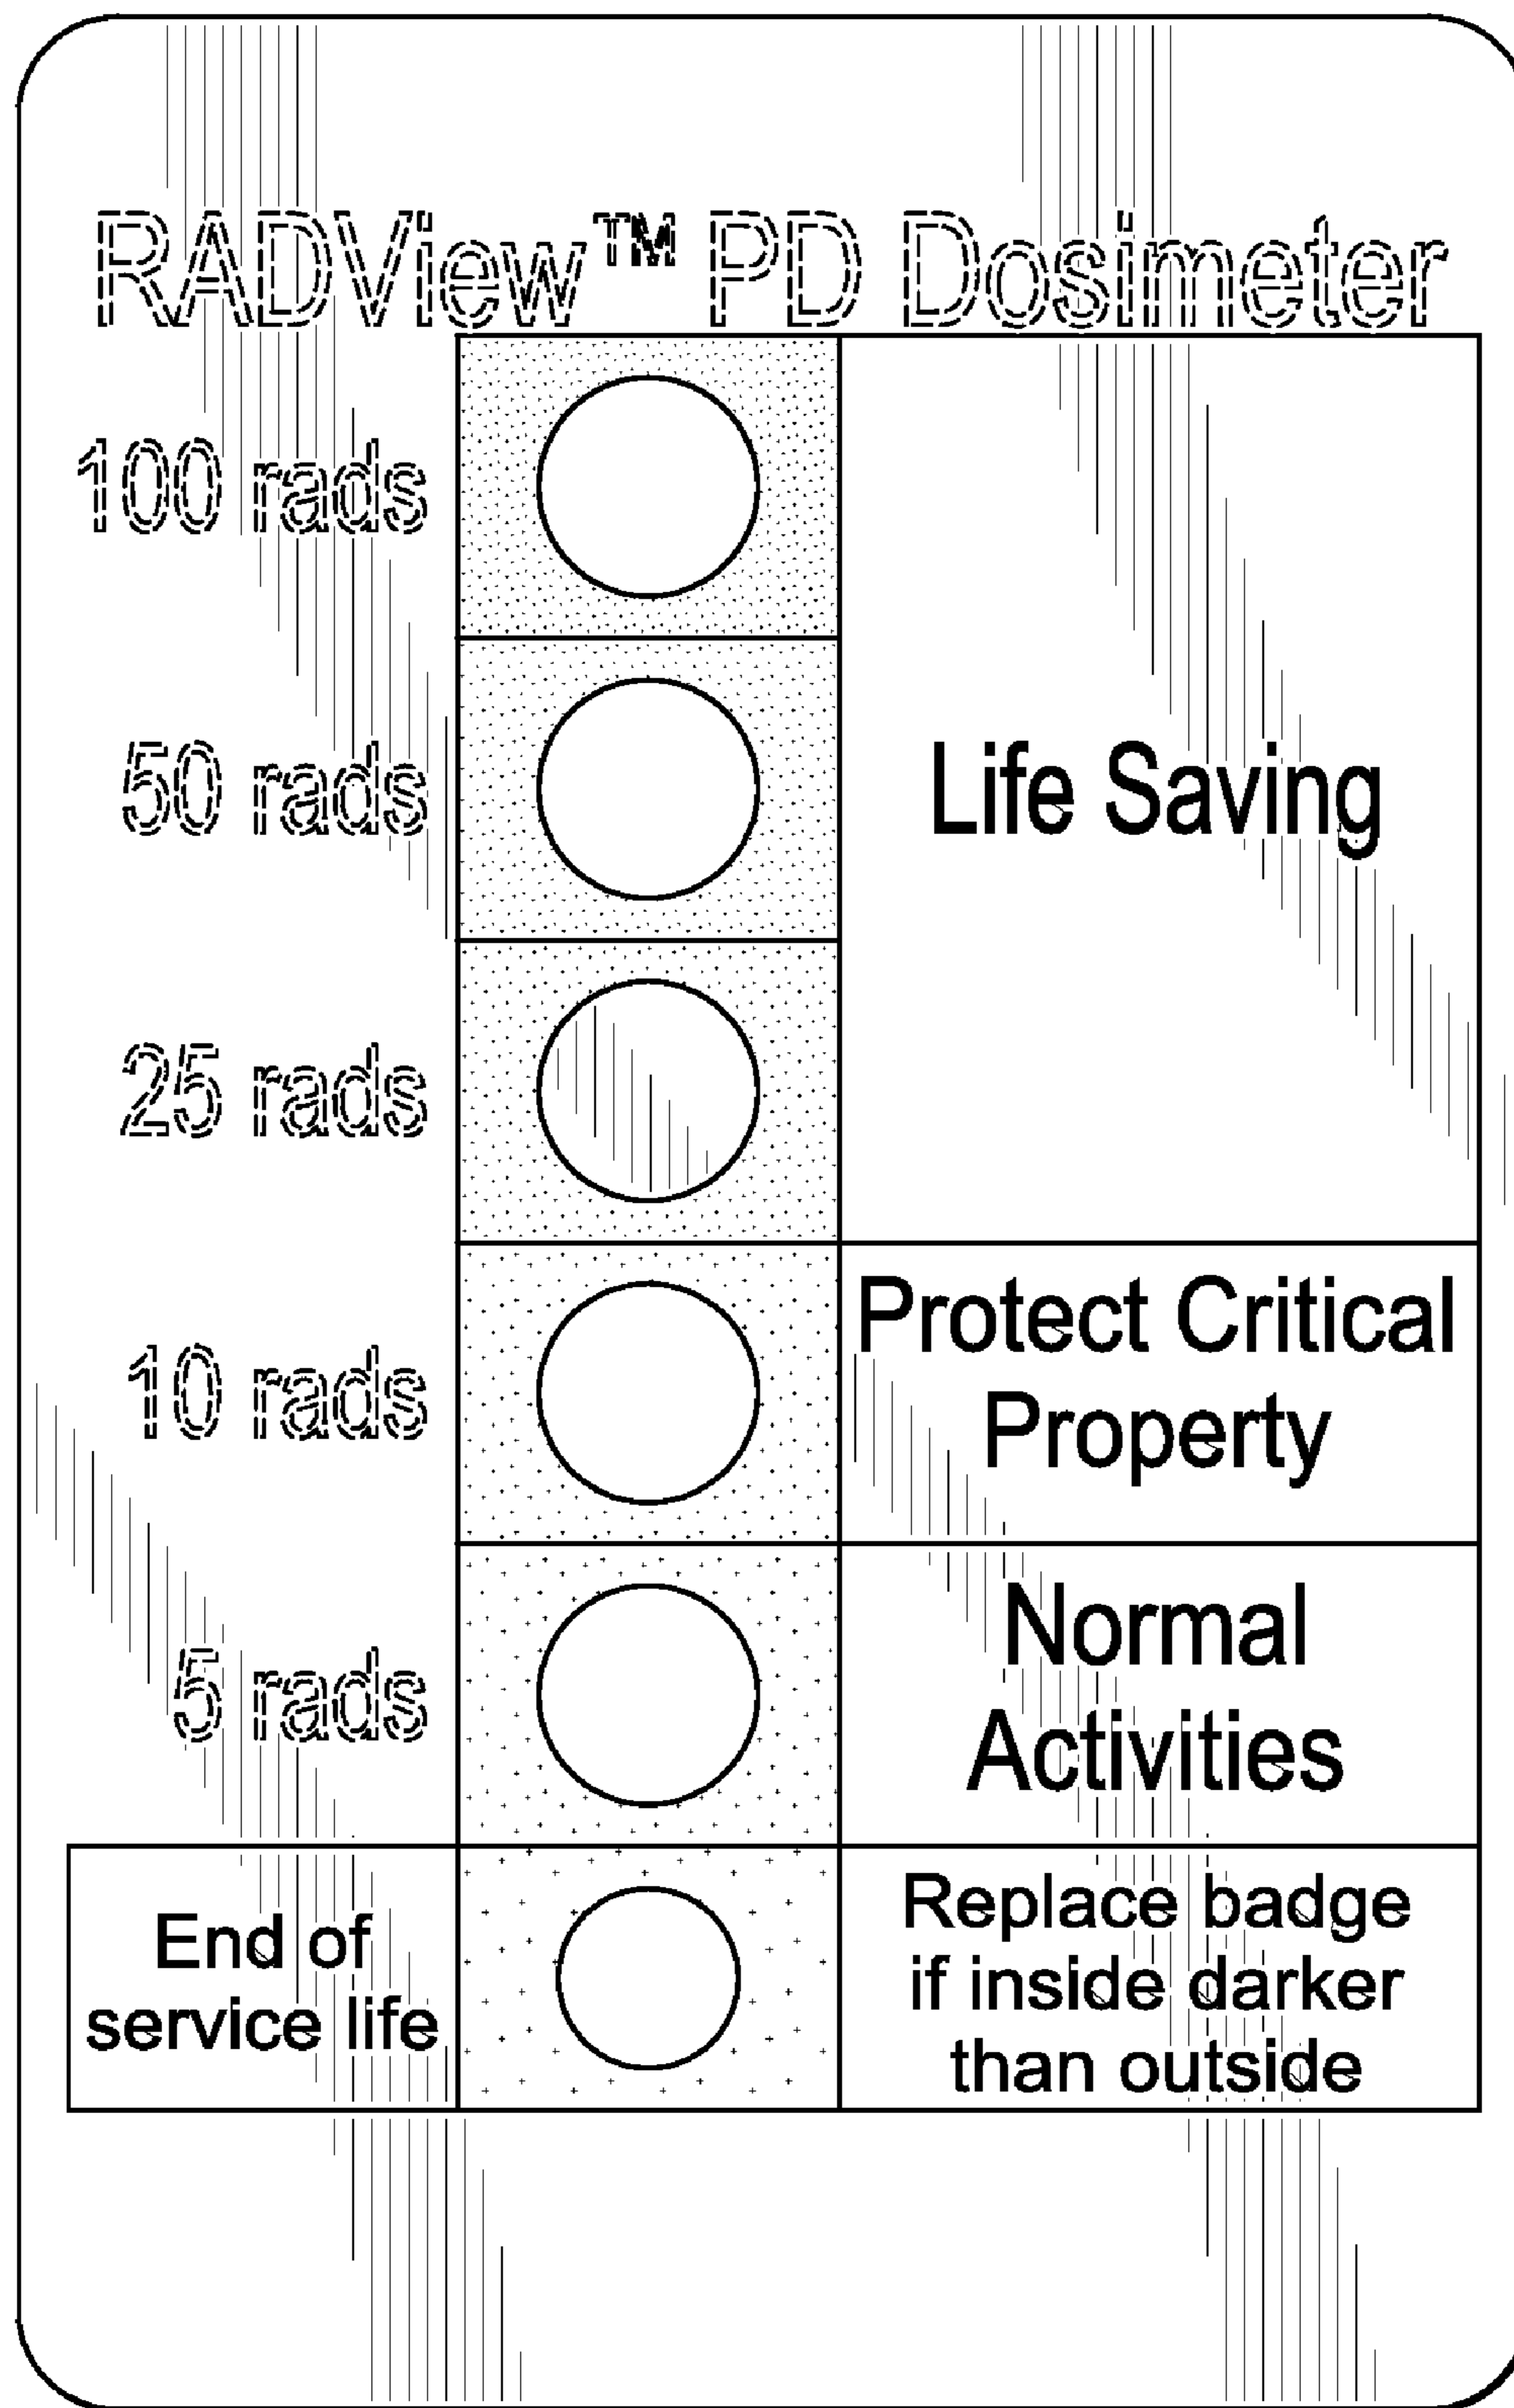


FIG. 9

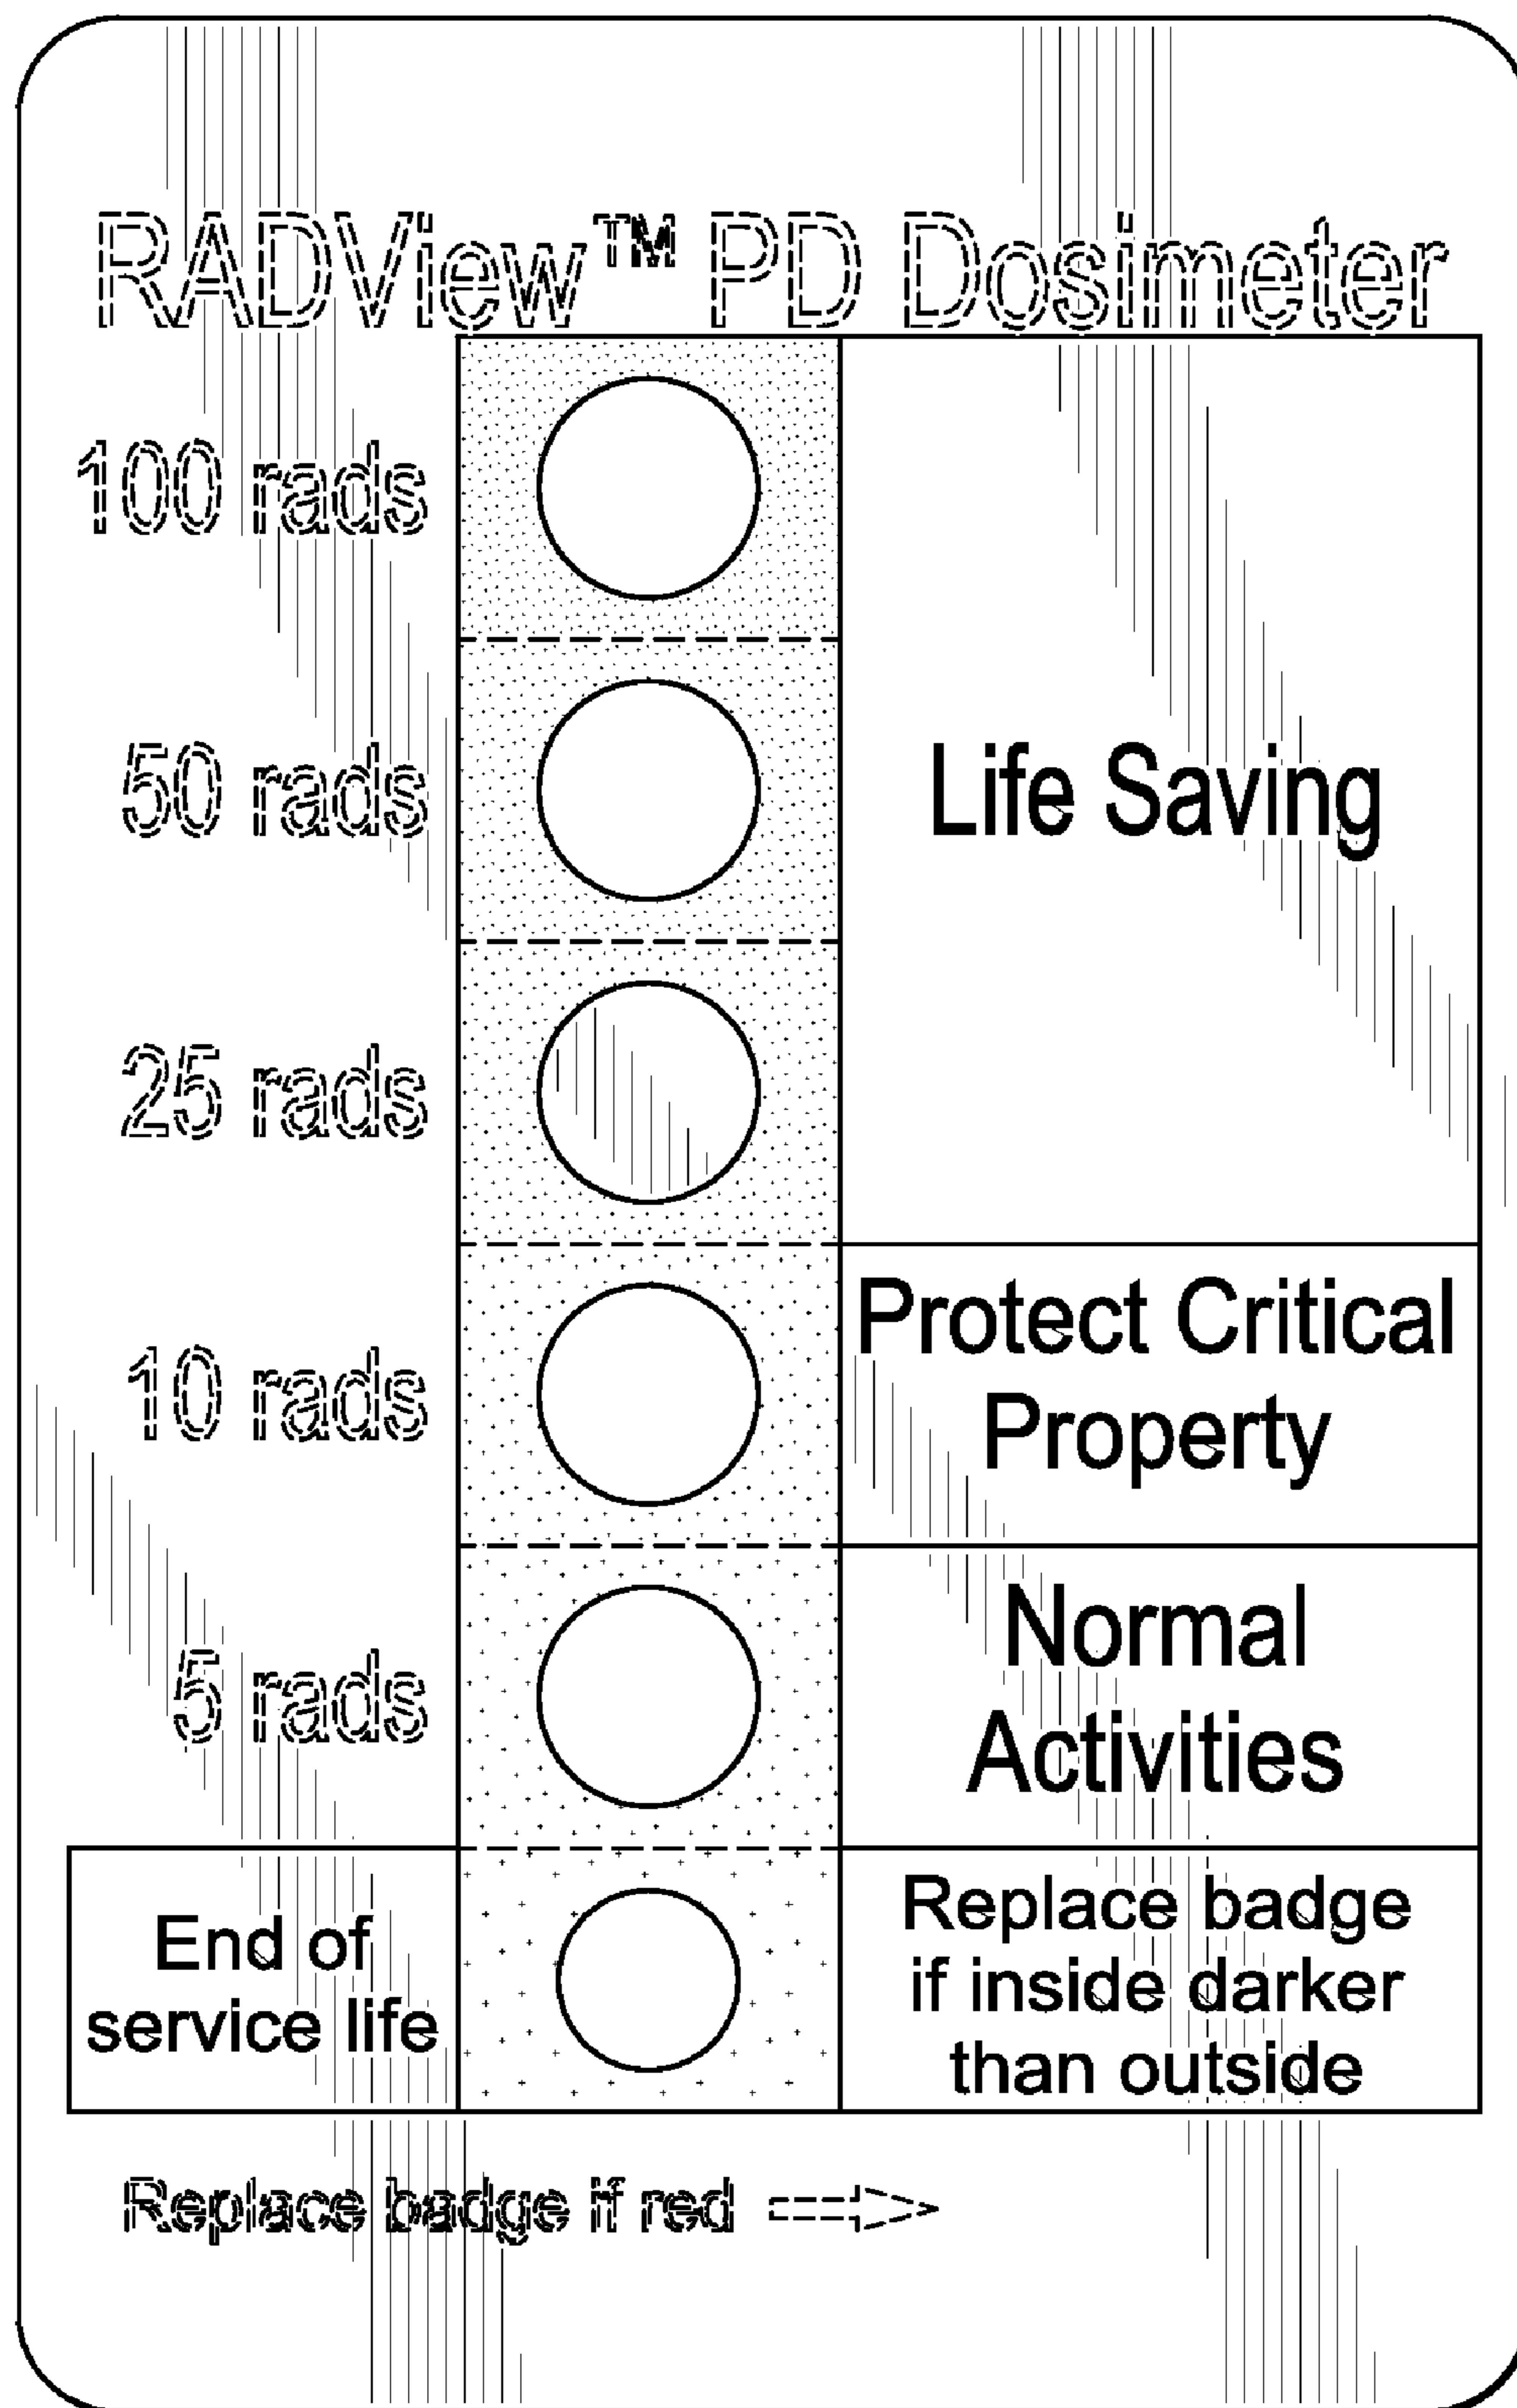


FIG. 10

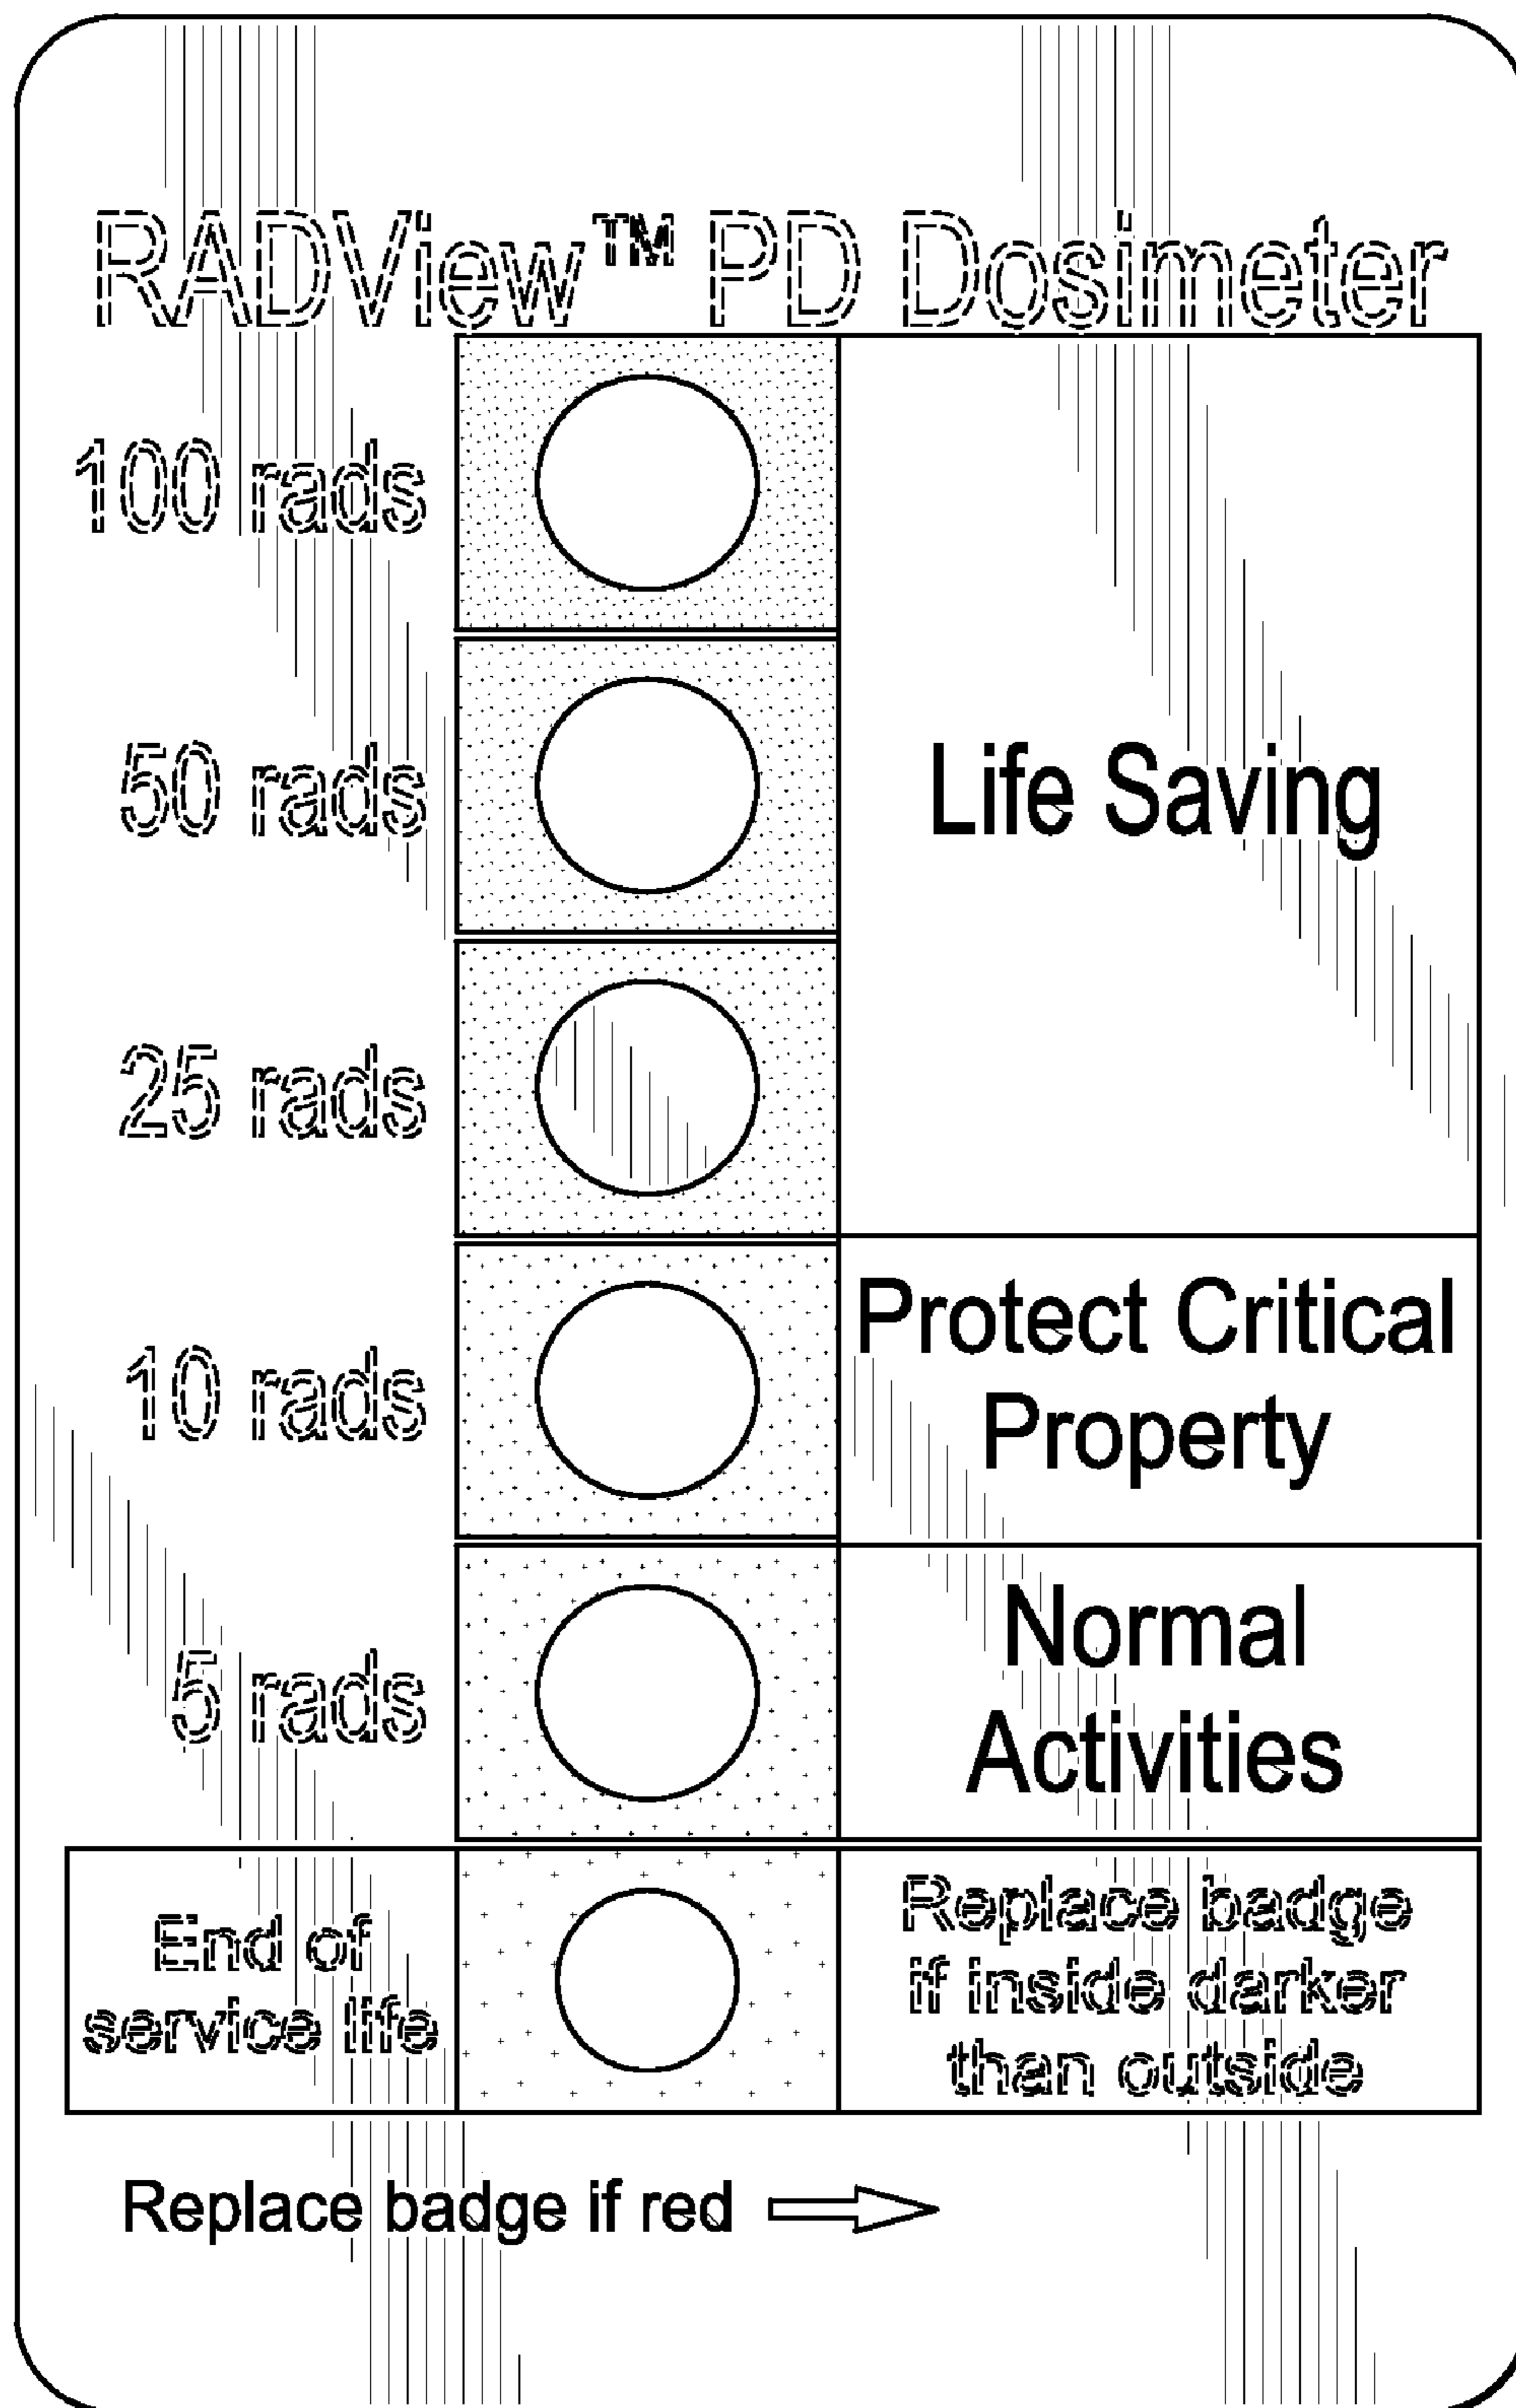


FIG. 11