



US00D583057S

(12) **United States Design Patent**  
**Kojima et al.**

(10) **Patent No.:** **US D583,057 S**  
(45) **Date of Patent:** **\*\* Dec. 16, 2008**

- (54) **DENTAL IMPLANT FIXTURE**
- (75) Inventors: **Norio Kojima**, Tokyo (JP); **Kiyoshi Watanabe**, Tokyo (JP)
- (73) Assignee: **GC Corporation**, Tokyo (JP)
- (\*\*) Term: **14 Years**
- (21) Appl. No.: **29/303,402**
- (22) Filed: **Feb. 7, 2008**

5,435,723 A	7/1995	O'Brien	
D362,720 S *	9/1995	Holmen et al. ....	D24/155
5,772,437 A	6/1998	Rangert et al.	
5,816,812 A	10/1998	Kownacki et al.	
5,829,978 A	11/1998	Day	
5,842,865 A	12/1998	Bassett et al.	
5,885,079 A	3/1999	Niznick	
5,906,489 A	5/1999	Khazzam et al.	
6,261,097 B1 *	7/2001	Schmutz et al. ....	433/173
6,358,050 B1	3/2002	Bergstrom et al.	
6,402,515 B1	6/2002	Palti et al.	
6,626,911 B1	9/2003	Engman et al.	
6,857,874 B2 *	2/2005	Kim .....	433/173
D567,947 S *	4/2008	Lerner et al. ....	D24/156
2003/0158554 A1	8/2003	Hall	

**Related U.S. Application Data**

- (63) Continuation of application No. 11/075,852, filed on Mar. 10, 2005.

**Foreign Application Priority Data**

- (30) Mar. 29, 2004 (JP) ..... 2004-094816

- (51) **LOC (8) Cl.** ..... **24-03**
- (52) **U.S. Cl.** ..... **D24/156**
- (58) **Field of Classification Search** ..... D24/155, D24/156, 107; 433/173, 176  
See application file for complete search history.

**References Cited**

**U.S. PATENT DOCUMENTS**

2,112,007 A	3/1938	Adams	
3,579,831 A	5/1971	Stevens et al.	
3,589,011 A	6/1971	Sneer	
4,552,532 A	11/1985	Mozsary	
4,872,839 A	10/1989	Brajnovic	
4,988,299 A	1/1991	Branemark	
5,007,835 A	4/1991	Valen	
D317,200 S *	5/1991	Jorneus .....	D24/156
5,088,926 A	2/1992	Lang	
D350,395 S *	9/1994	Håkansson .....	D24/173
D353,674 S *	12/1994	Jorneus .....	D24/156

**FOREIGN PATENT DOCUMENTS**

EP	0 343 135 A1	11/1989
JP	8-510400	11/1996
WO	WO 95/17135	6/1995

\* cited by examiner

*Primary Examiner*—Charles A Rademaker  
(74) *Attorney, Agent, or Firm*—Oblon, Spivak, McClelland, Maier & Neustadt, P.C.


(57) **CLAIM**


The ornamental design for a dental implant fixture, as shown.

**DESCRIPTION**


FIG. 1 is a front elevational view of a dental implant fixture, showing our new design;  
FIG. 2 is a right side elevational view thereof; and,  
FIG. 3 is a left side elevational view thereof.  
The broken lines shown in the figure drawings are used to illustrate environmental structure and form no part of the claimed design.

**1 Claim, 2 Drawing Sheets**

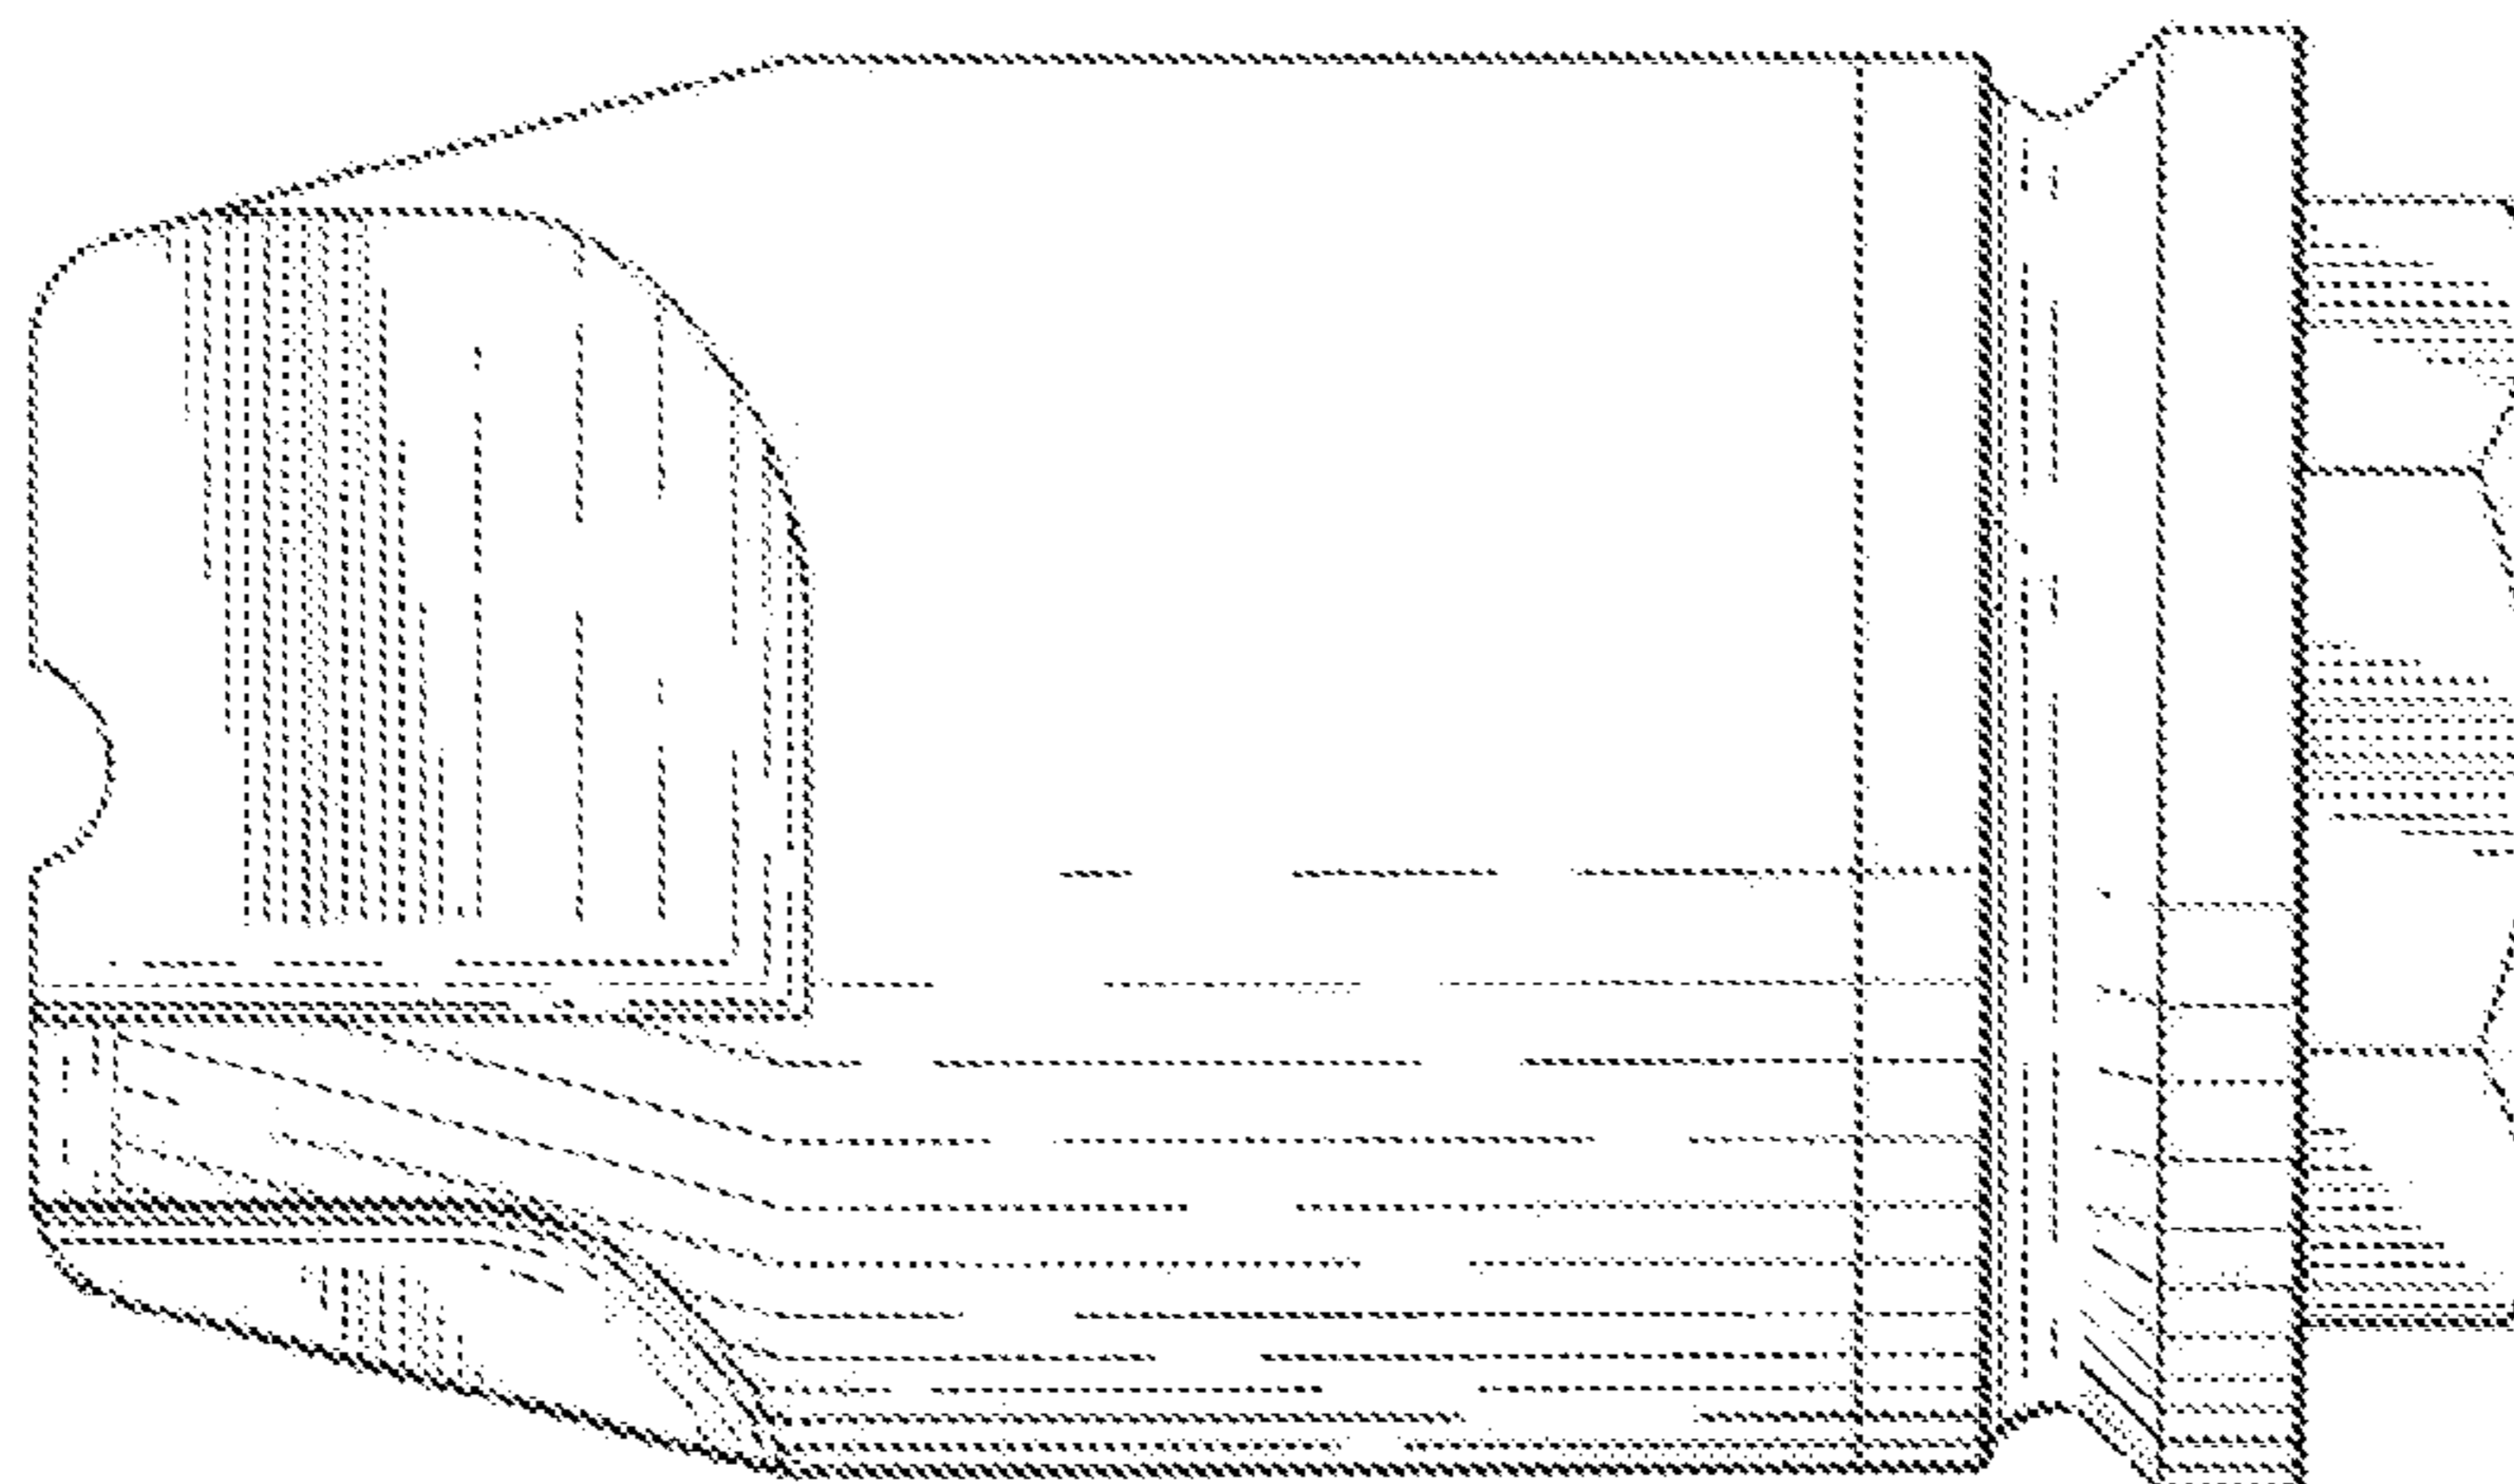


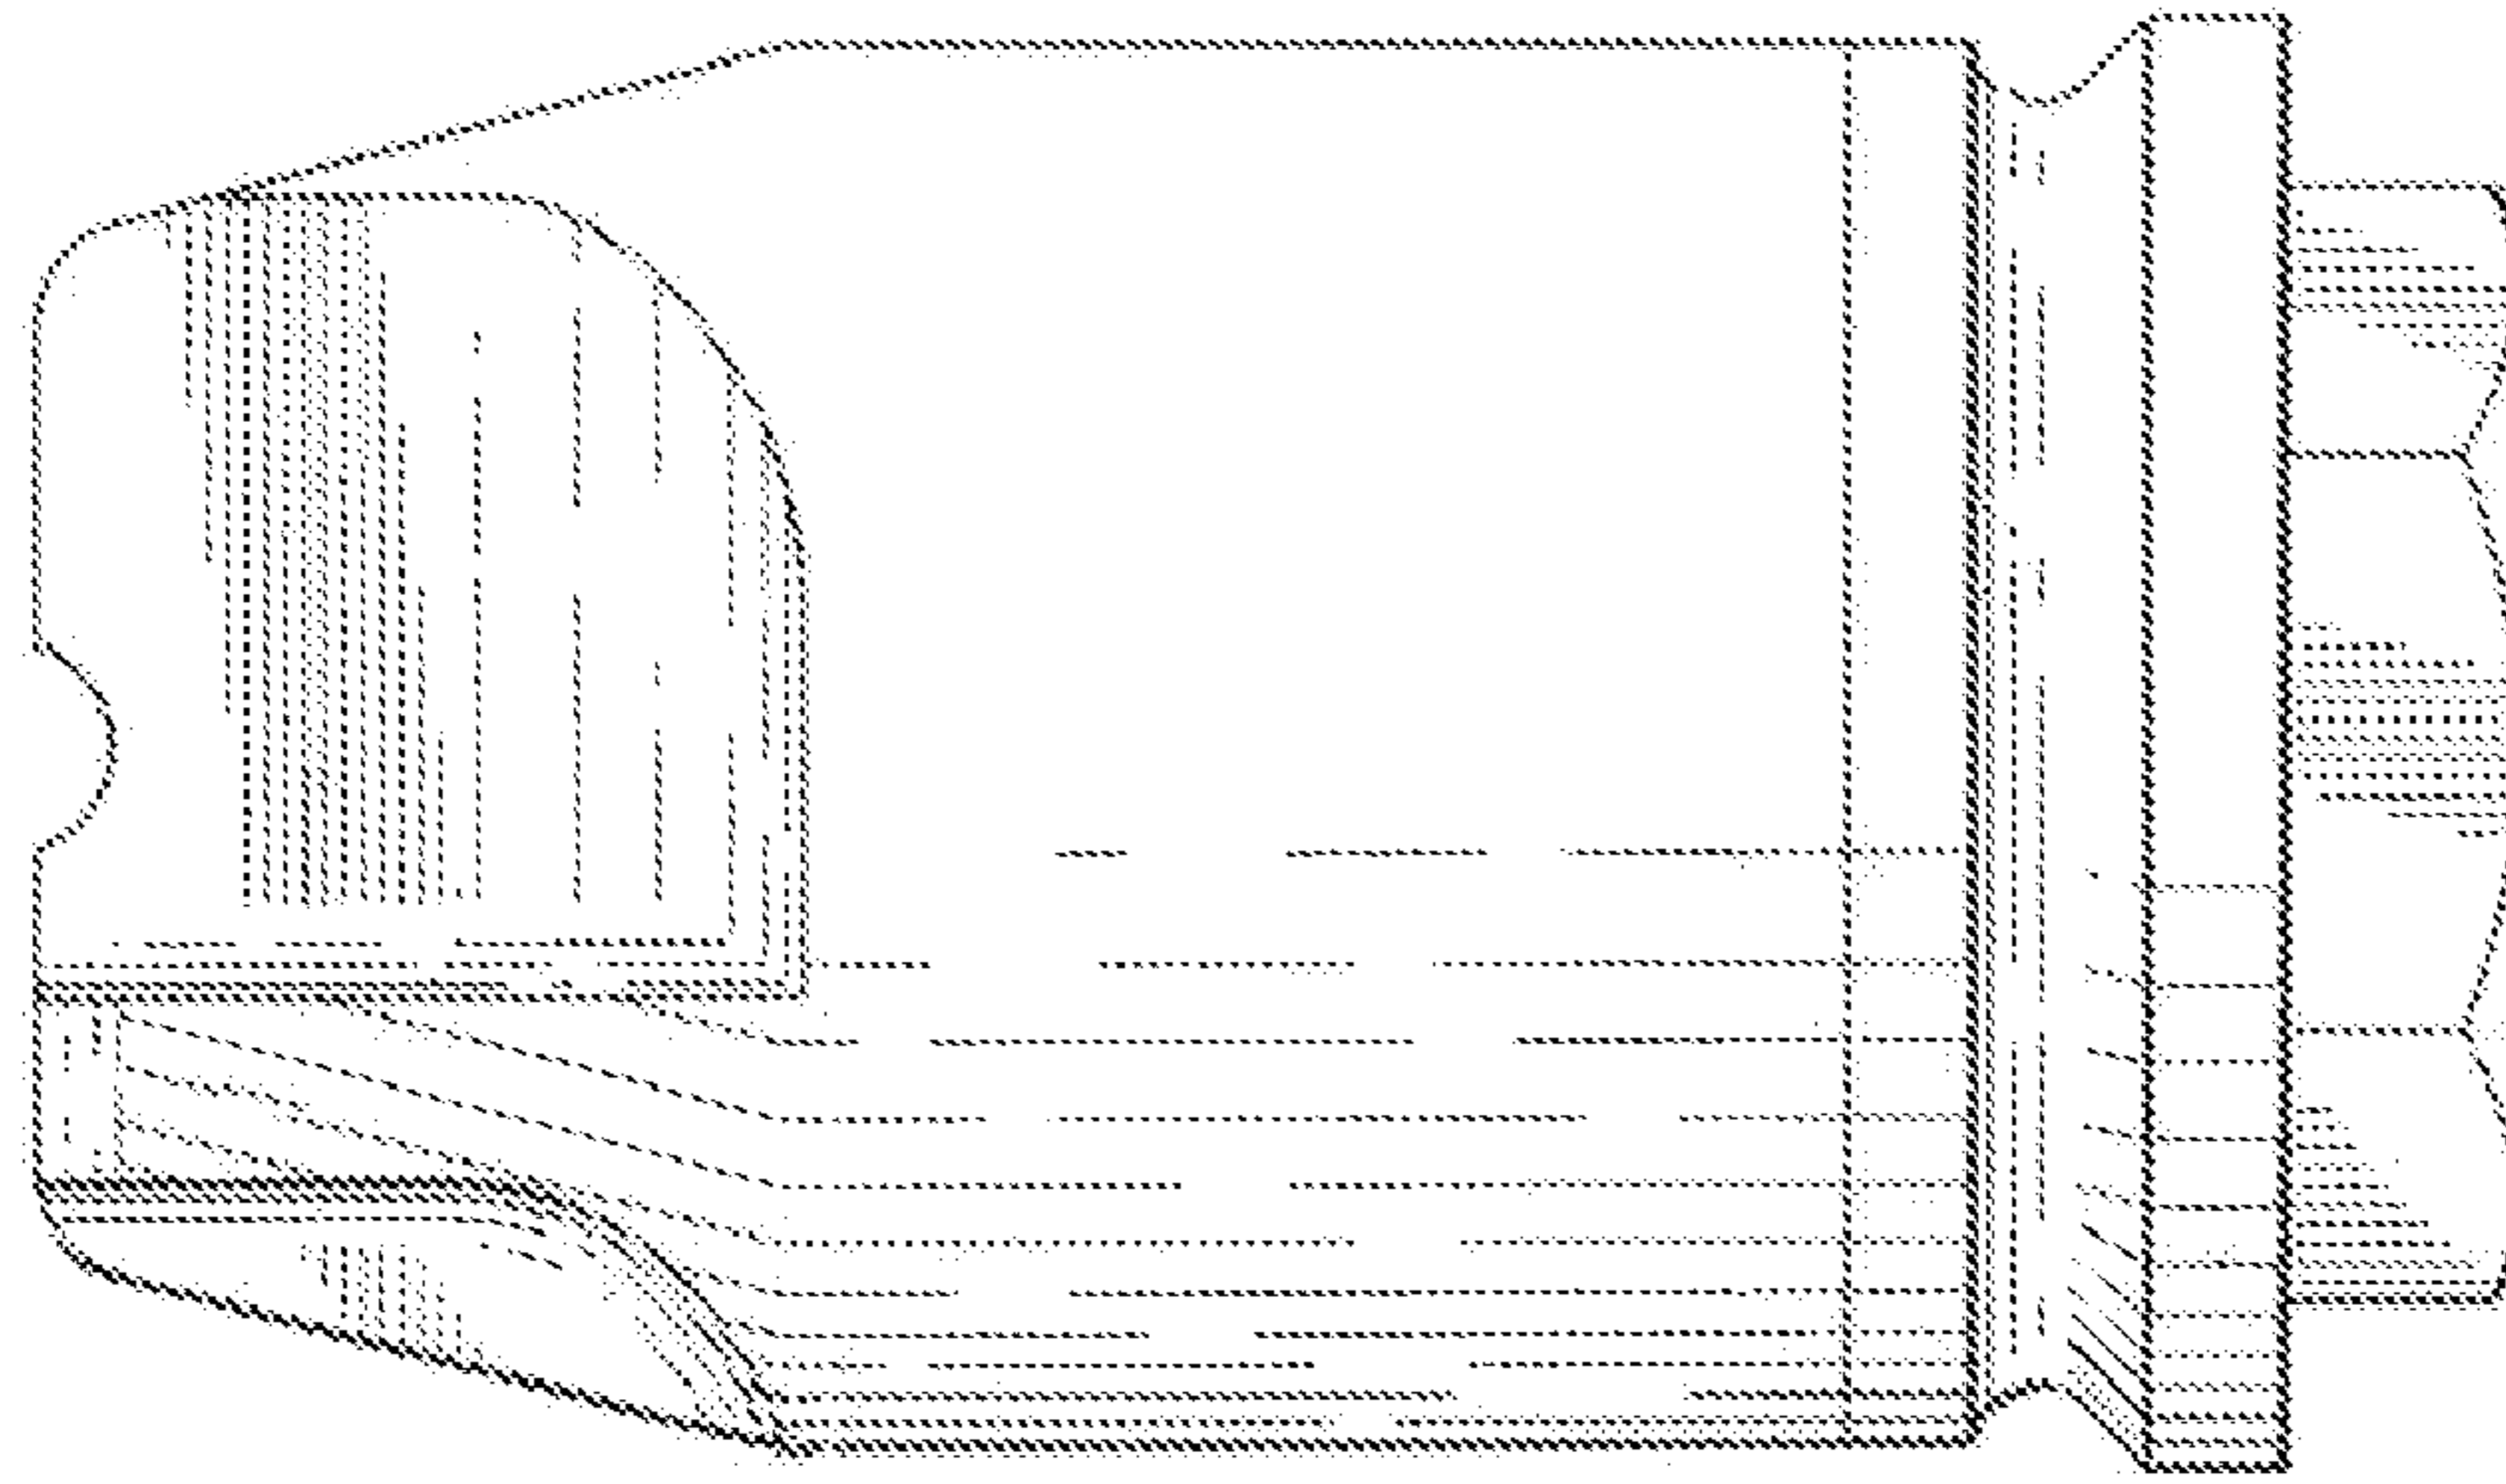

*Fig. 1*

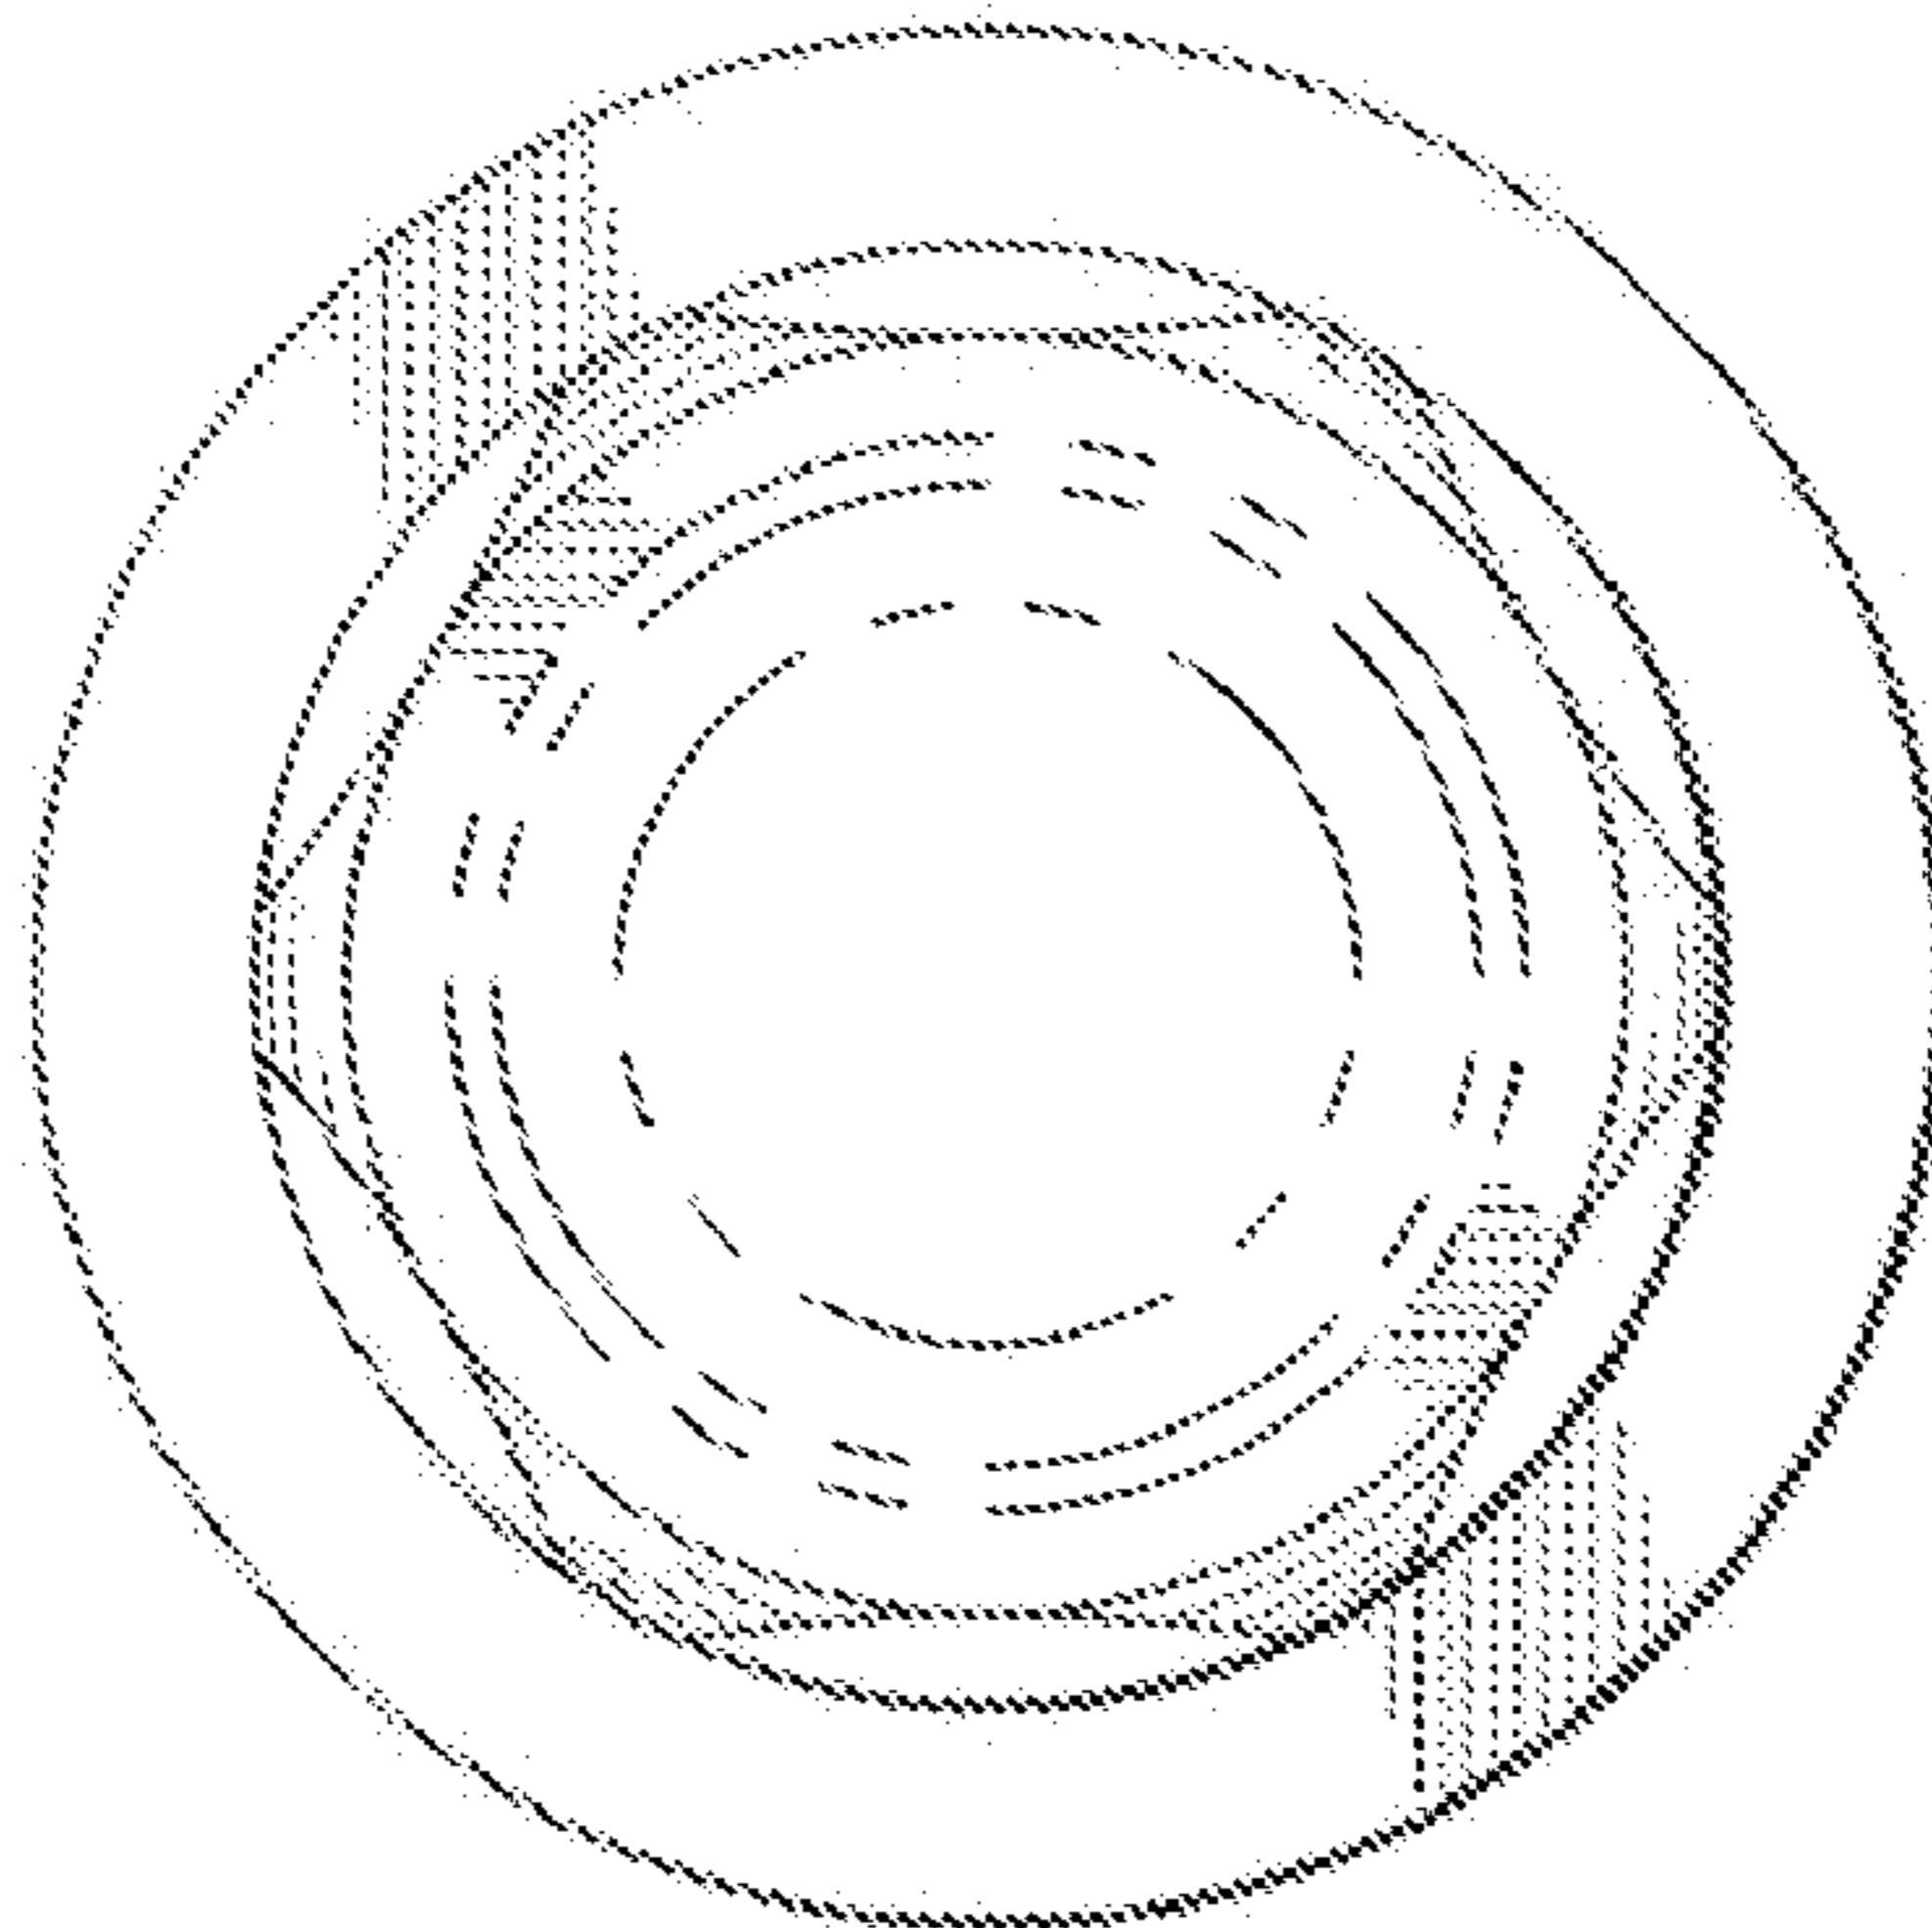

*Fig. 2*

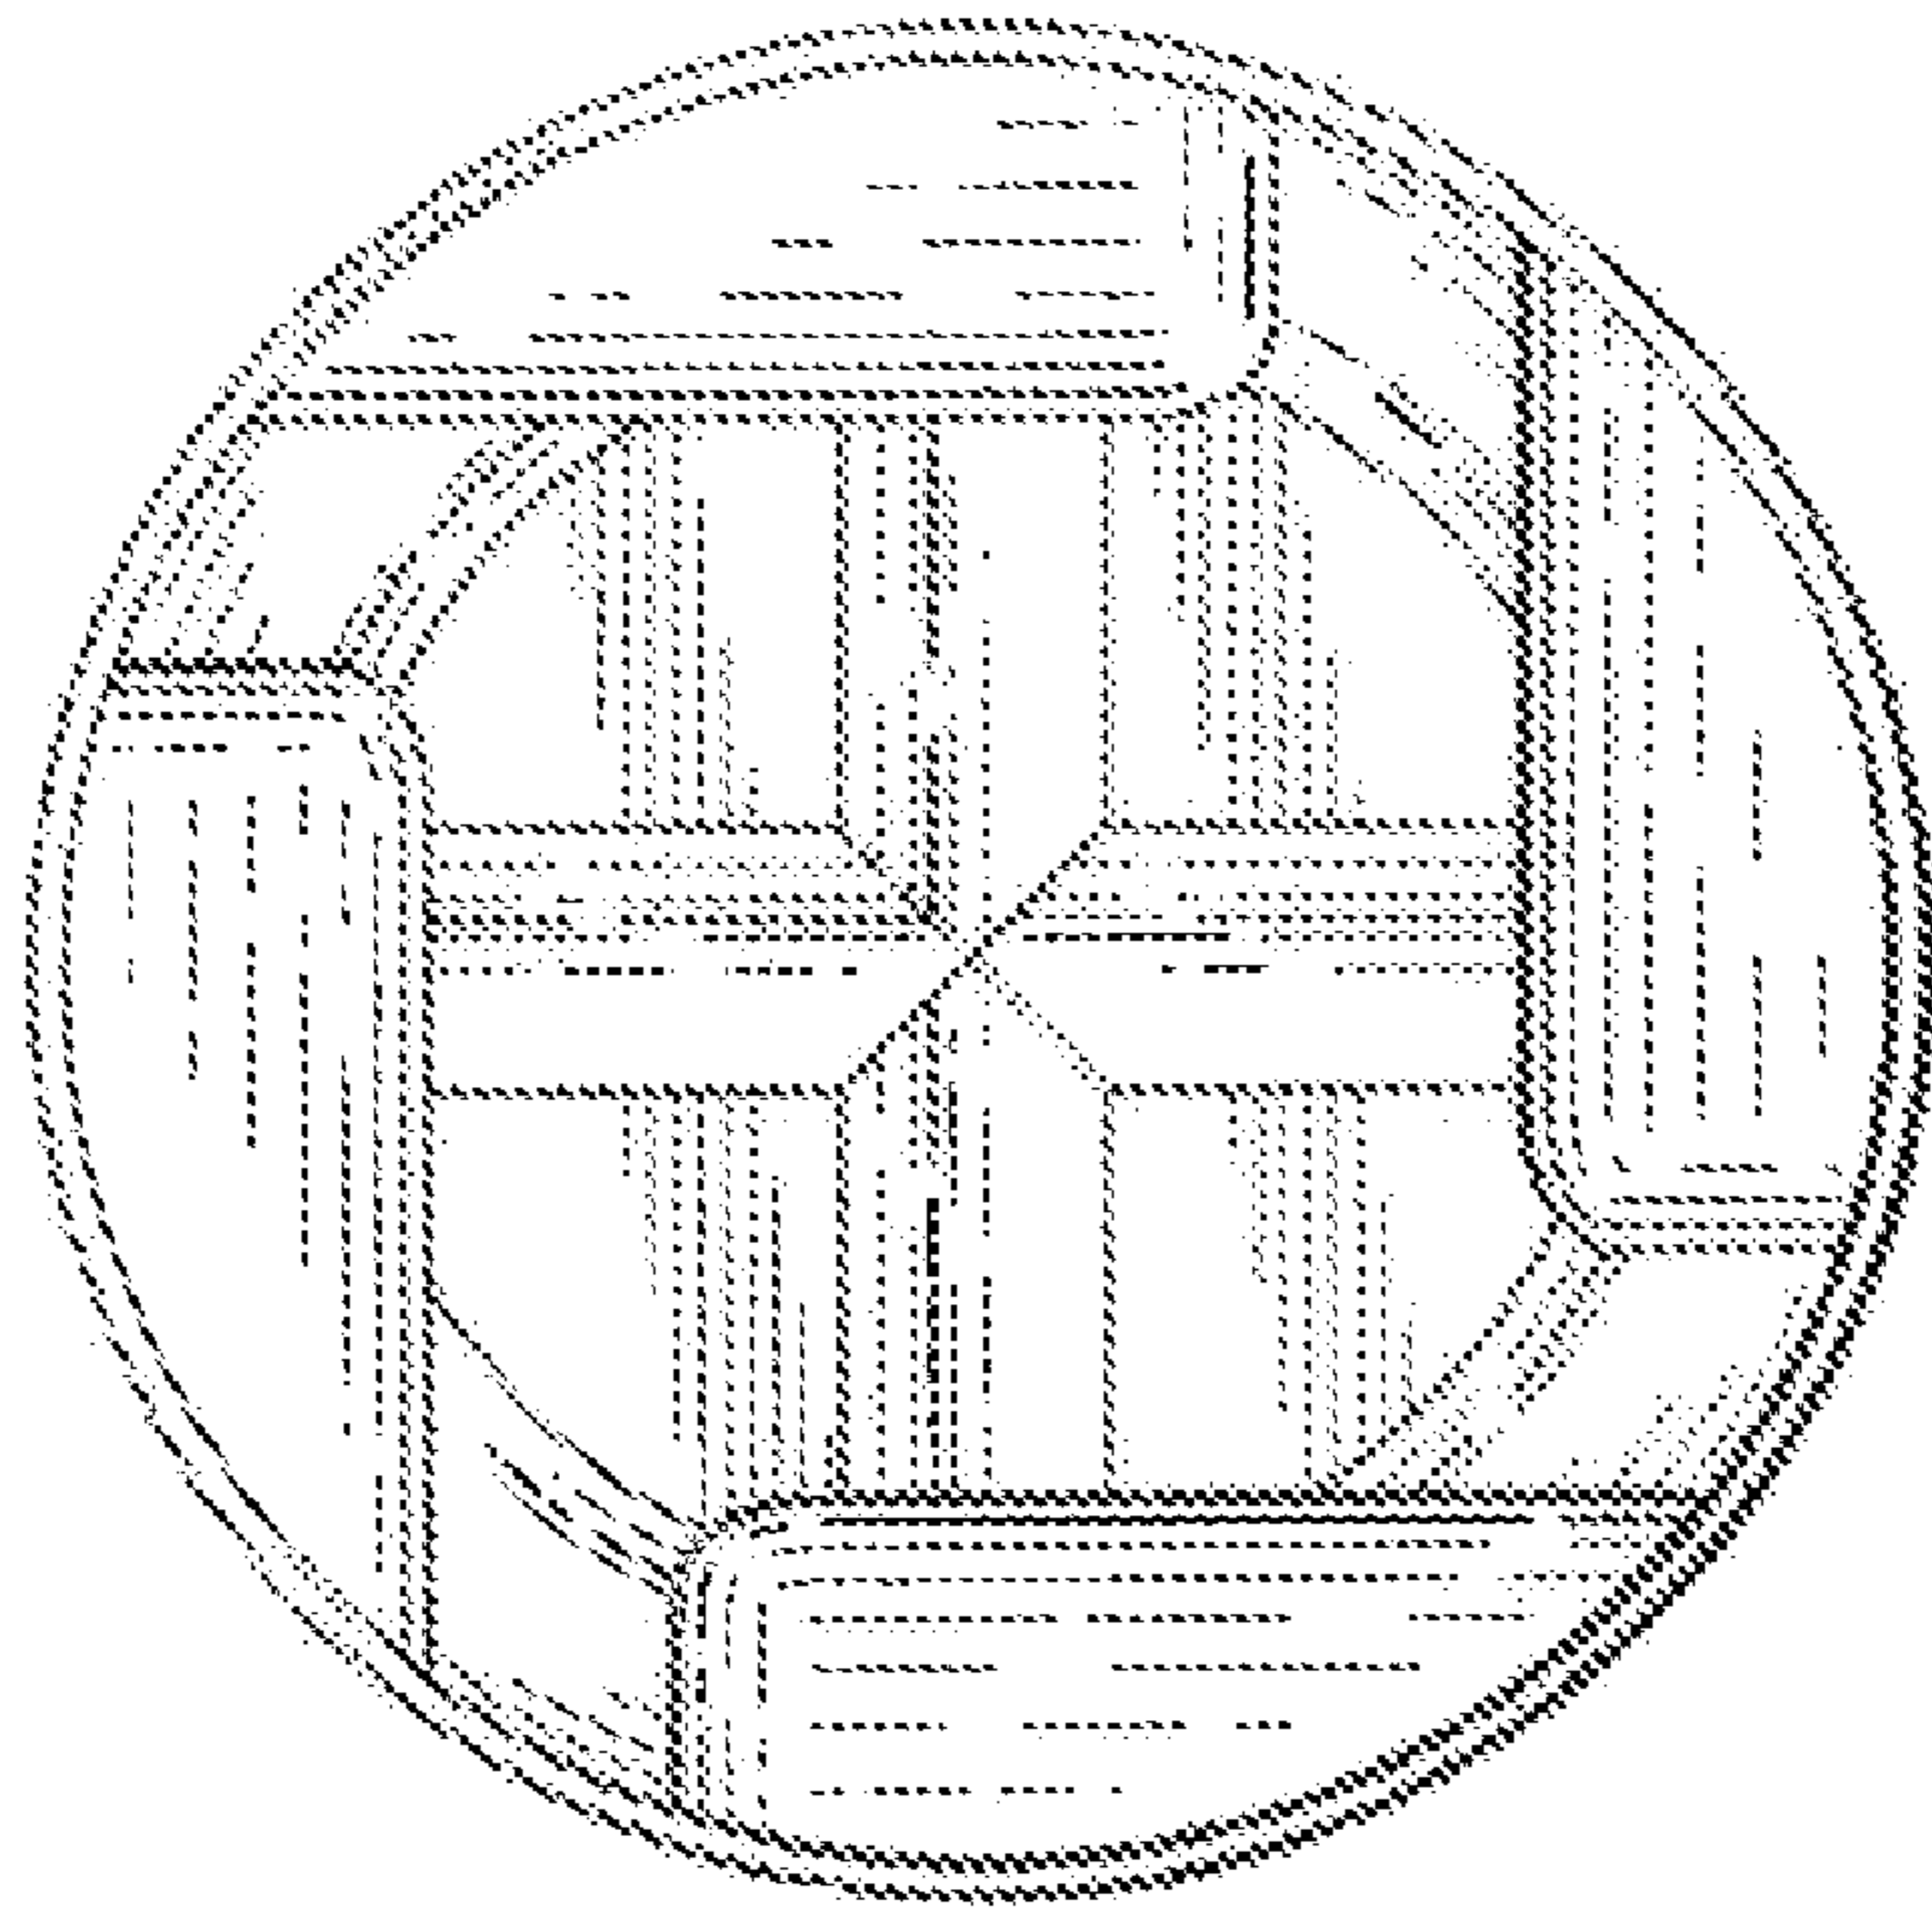

*Fig. 3*

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. 583,057 S  
APPLICATION NO. : 29/303402  
DATED : December 16, 2008  
INVENTOR(S) : Kojima et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page, Item (63), the Related U.S. Application Data information is incorrect. Item (63) should read:

**Related U.S. Application Data**

--(63) Division of Application No. 11/075,852, filed on  
Mar. 10, 2005.--

Signed and Sealed this

Tenth Day of February, 2009



JOHN DOLL  
*Acting Director of the United States Patent and Trademark Office*