



US00D583057S

(12) **United States Design Patent**
Kojima et al.

(10) **Patent No.:** **US D583,057 S**

(45) **Date of Patent:** **** Dec. 16, 2008**

(54) **DENTAL IMPLANT FIXTURE**

(75) Inventors: **Norio Kojima**, Tokyo (JP); **Kiyoshi Watanabe**, Tokyo (JP)

(73) Assignee: **GC Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/303,402**

(22) Filed: **Feb. 7, 2008**

Related U.S. Application Data

(63) Continuation of application No. 11/075,852, filed on Mar. 10, 2005.

(30) **Foreign Application Priority Data**

Mar. 29, 2004 (JP) 2004-094816

(51) **LOC (8) Cl.** **24-03**

(52) **U.S. Cl.** **D24/156**

(58) **Field of Classification Search** D24/155,
D24/156, 107; 433/173, 176

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | |
|--------------|---------|----------------|---------|
| 2,112,007 A | 3/1938 | Adams | |
| 3,579,831 A | 5/1971 | Stevens et al. | |
| 3,589,011 A | 6/1971 | Sneer | |
| 4,552,532 A | 11/1985 | Mozsary | |
| 4,872,839 A | 10/1989 | Brajnovic | |
| 4,988,299 A | 1/1991 | Branemark | |
| 5,007,835 A | 4/1991 | Valen | |
| D317,200 S * | 5/1991 | Jorneus | D24/156 |
| 5,088,926 A | 2/1992 | Lang | |
| D350,395 S * | 9/1994 | Håkansson | D24/173 |
| D353,674 S * | 12/1994 | Jorneus | D24/156 |

| | | | |
|-----------------|---------|------------------|---------|
| 5,435,723 A | 7/1995 | O'Brien | |
| D362,720 S * | 9/1995 | Holmen et al. | D24/155 |
| 5,772,437 A | 6/1998 | Rangert et al. | |
| 5,816,812 A | 10/1998 | Kownacki et al. | |
| 5,829,978 A | 11/1998 | Day | |
| 5,842,865 A | 12/1998 | Bassett et al. | |
| 5,885,079 A | 3/1999 | Niznick | |
| 5,906,489 A | 5/1999 | Khazzam et al. | |
| 6,261,097 B1 * | 7/2001 | Schmutz et al. | 433/173 |
| 6,358,050 B1 | 3/2002 | Bergstrom et al. | |
| 6,402,515 B1 | 6/2002 | Palti et al. | |
| 6,626,911 B1 | 9/2003 | Engman et al. | |
| 6,857,874 B2 * | 2/2005 | Kim | 433/173 |
| D567,947 S * | 4/2008 | Lerner et al. | D24/156 |
| 2003/0158554 A1 | 8/2003 | Hall | |

FOREIGN PATENT DOCUMENTS

| | | |
|----|--------------|---------|
| EP | 0 343 135 A1 | 11/1989 |
| JP | 8-510400 | 11/1996 |
| WO | WO 95/17135 | 6/1995 |

* cited by examiner

Primary Examiner—Charles A Rademaker

(74) *Attorney, Agent, or Firm*—Oblon, Spivak, McClelland, Maier & Neustadt, P.C.

(57) **CLAIM**

The ornamental design for a dental implant fixture, as shown.

DESCRIPTION


FIG. 1 is a front elevational view of a dental implant fixture, showing our new design;

FIG. 2 is a right side elevational view thereof; and,

FIG. 3 is a left side elevational view thereof.

The broken lines shown in the figure drawings are used to illustrate environmental structure and form no part of the claimed design.

1 Claim, 2 Drawing Sheets

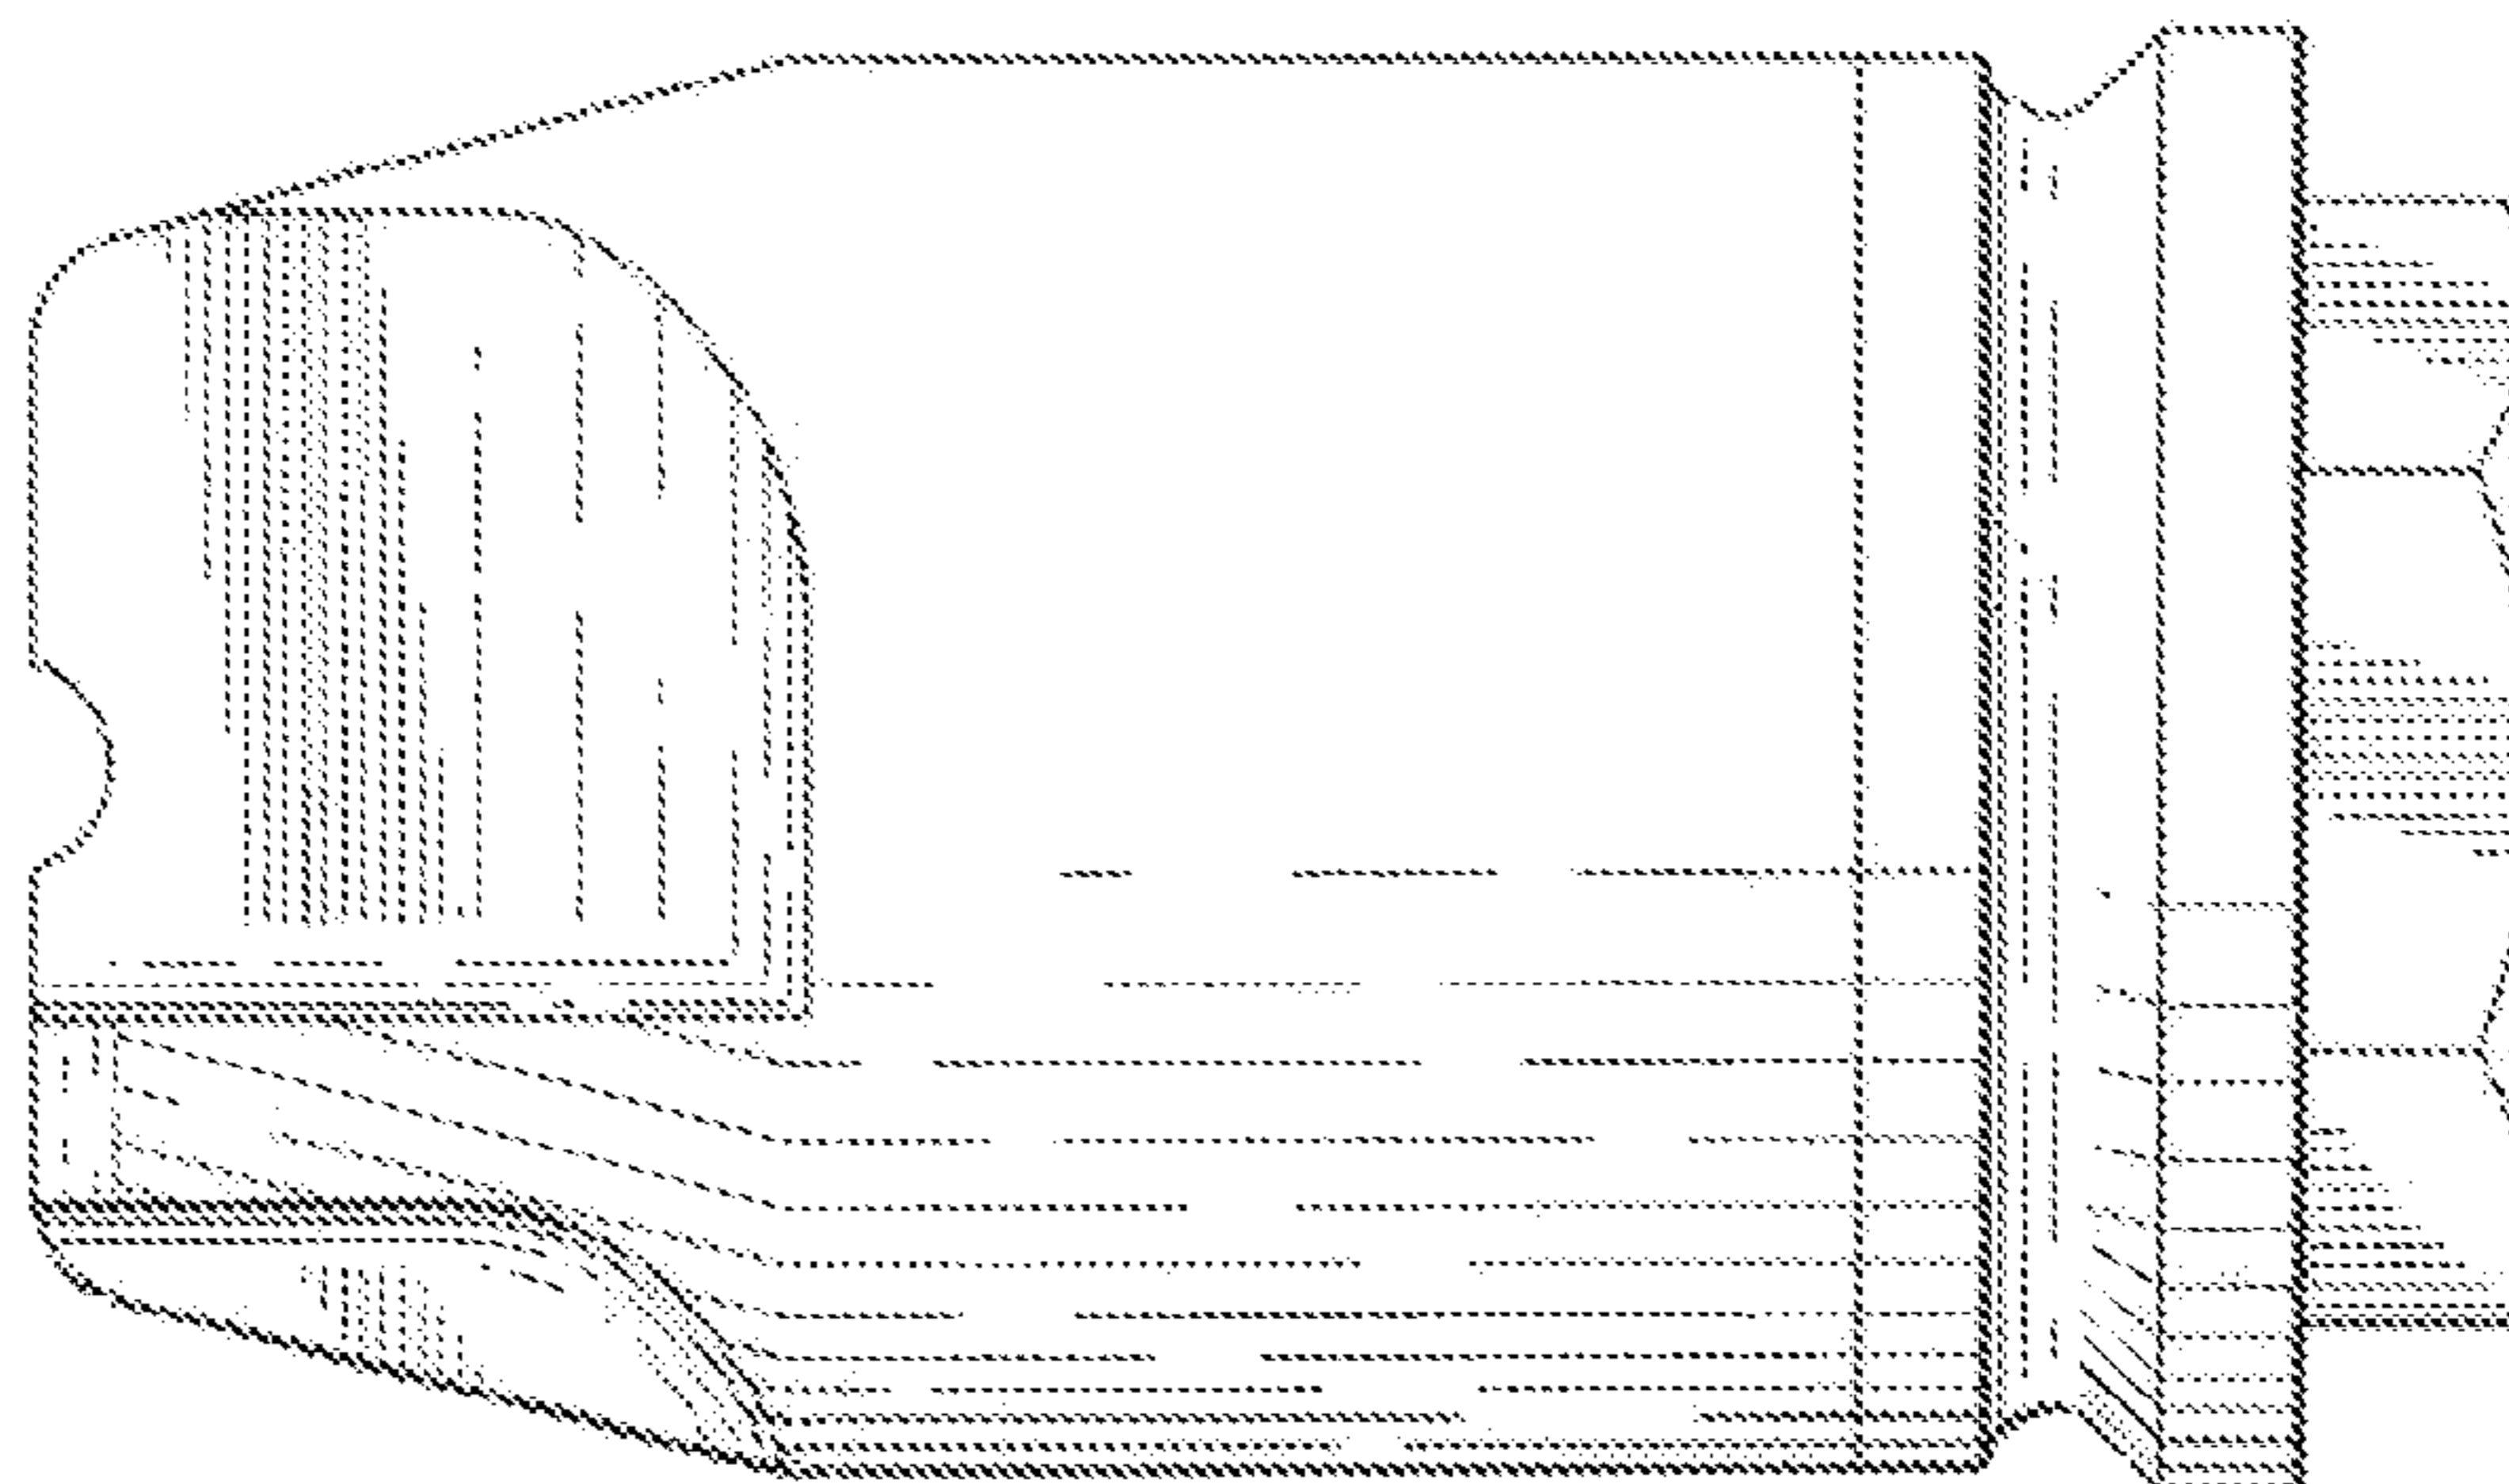

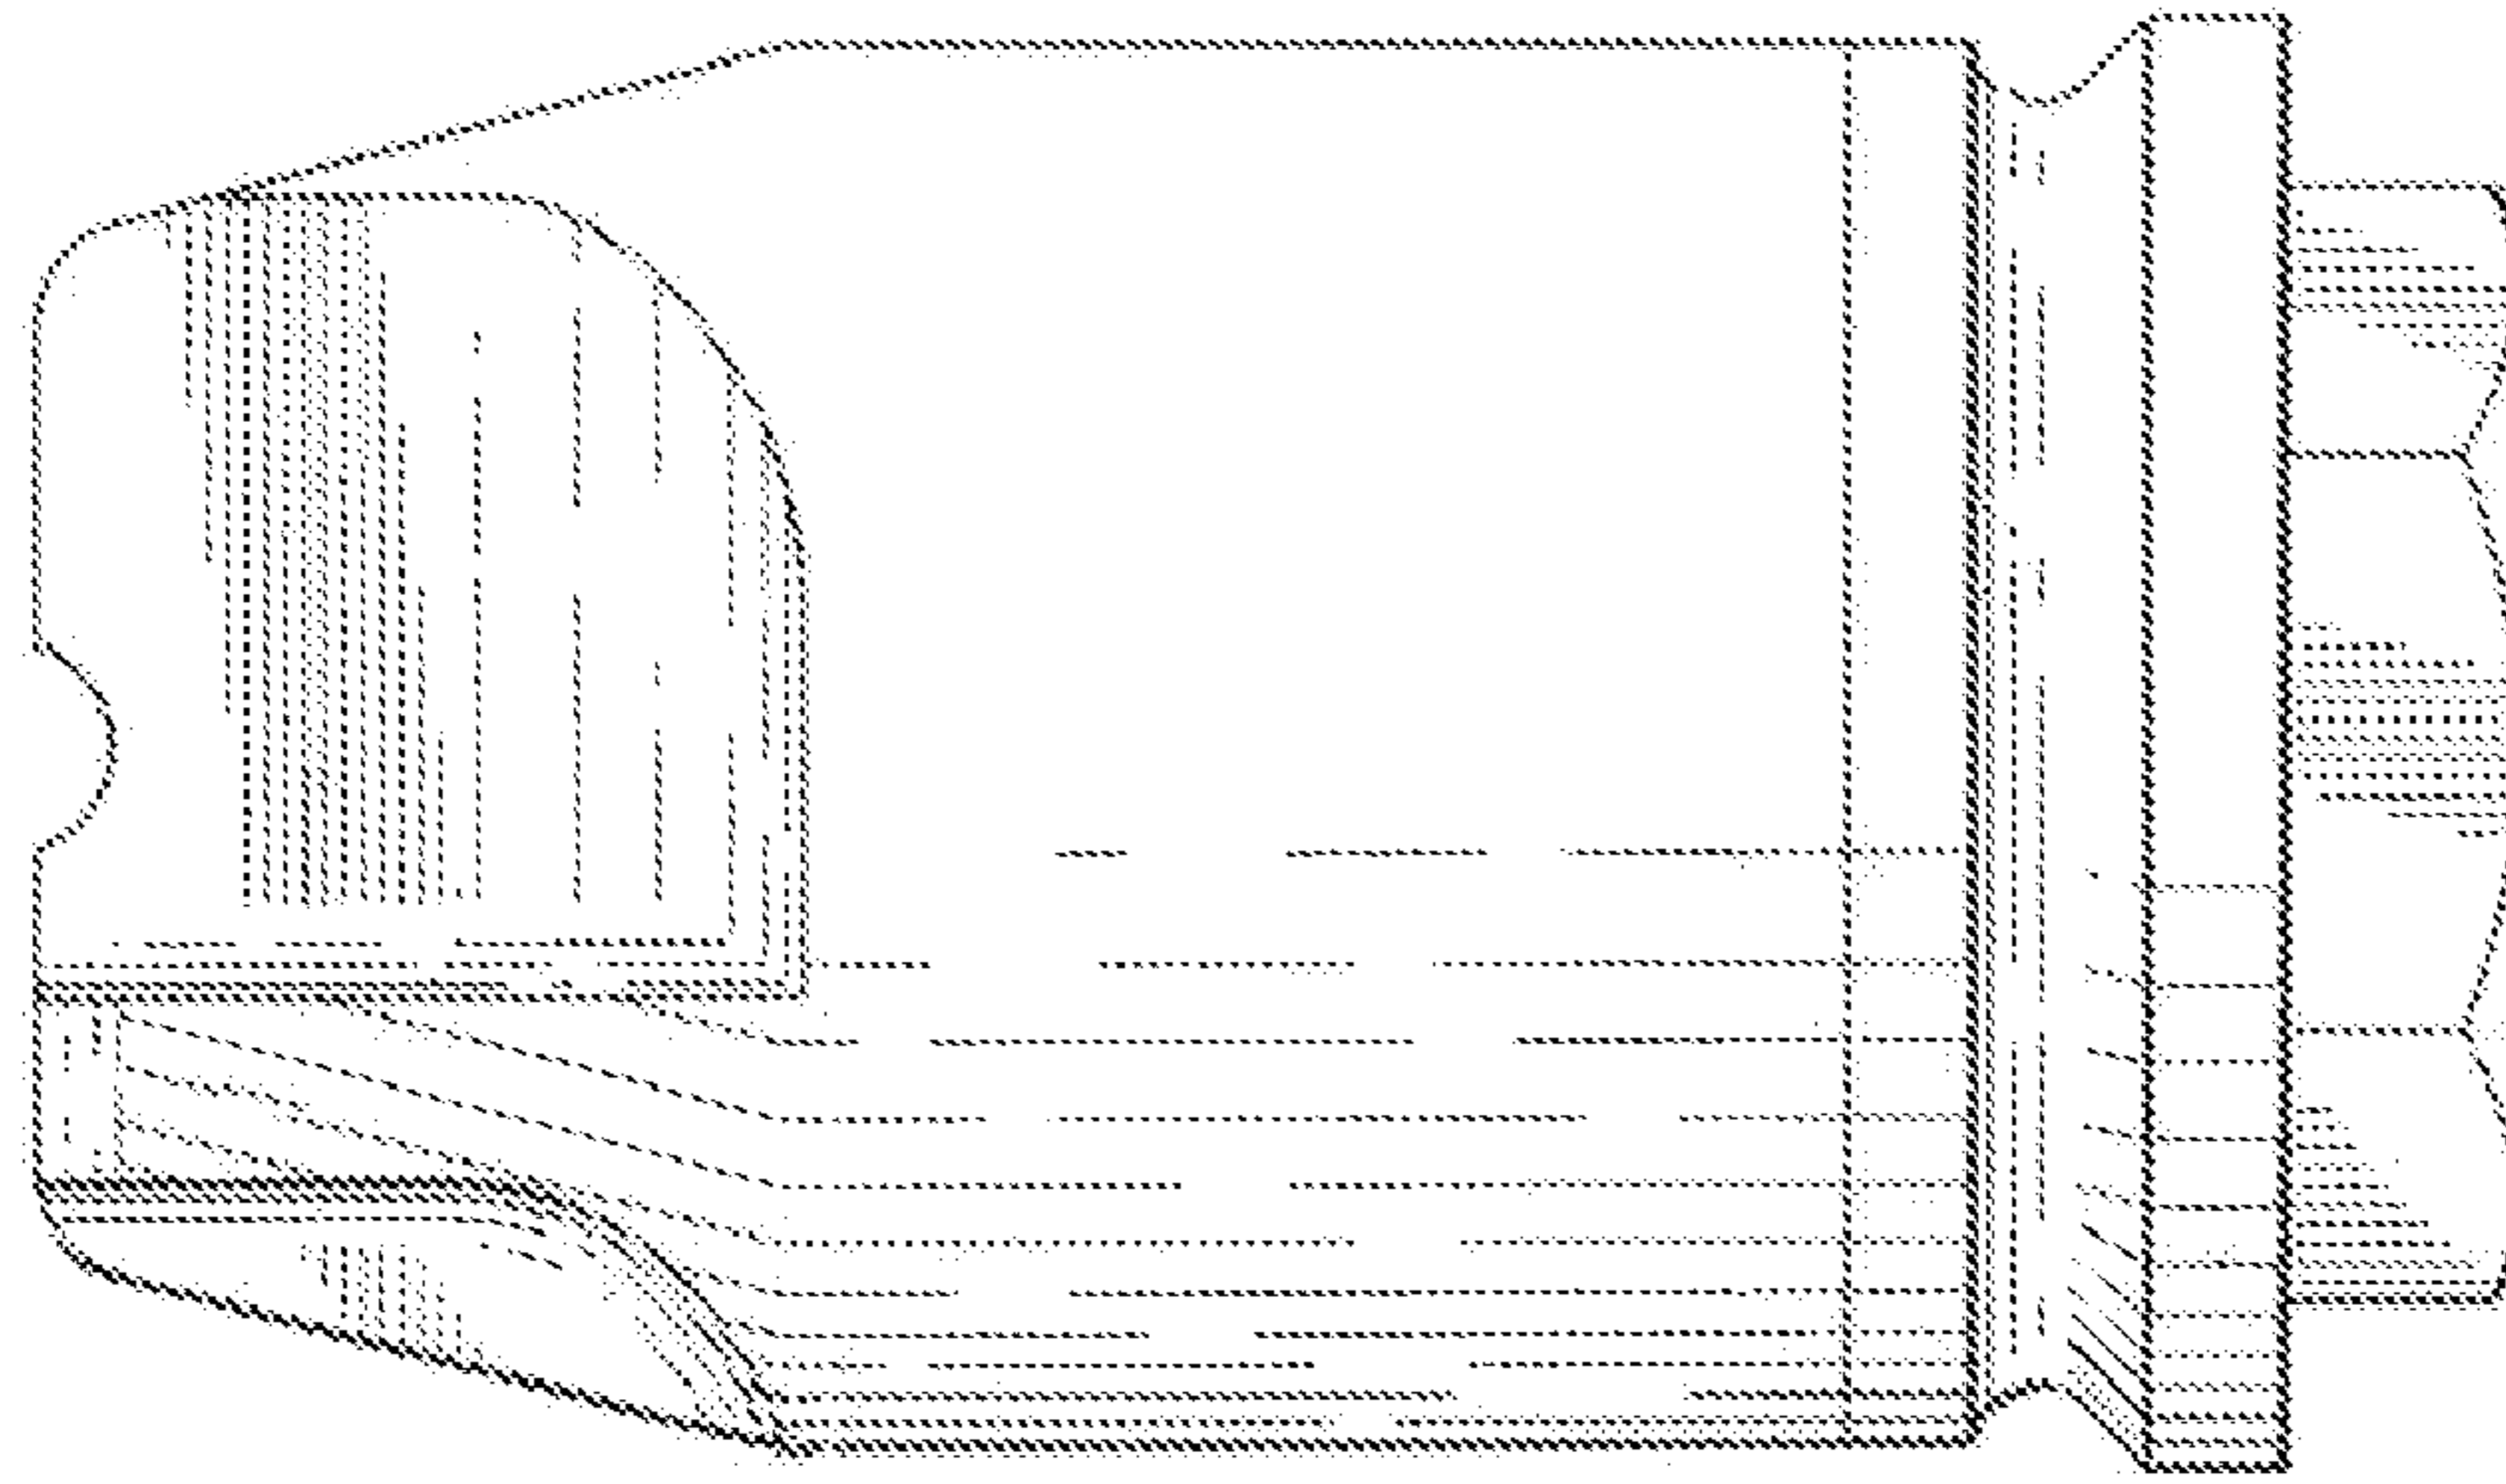


Fig. 1

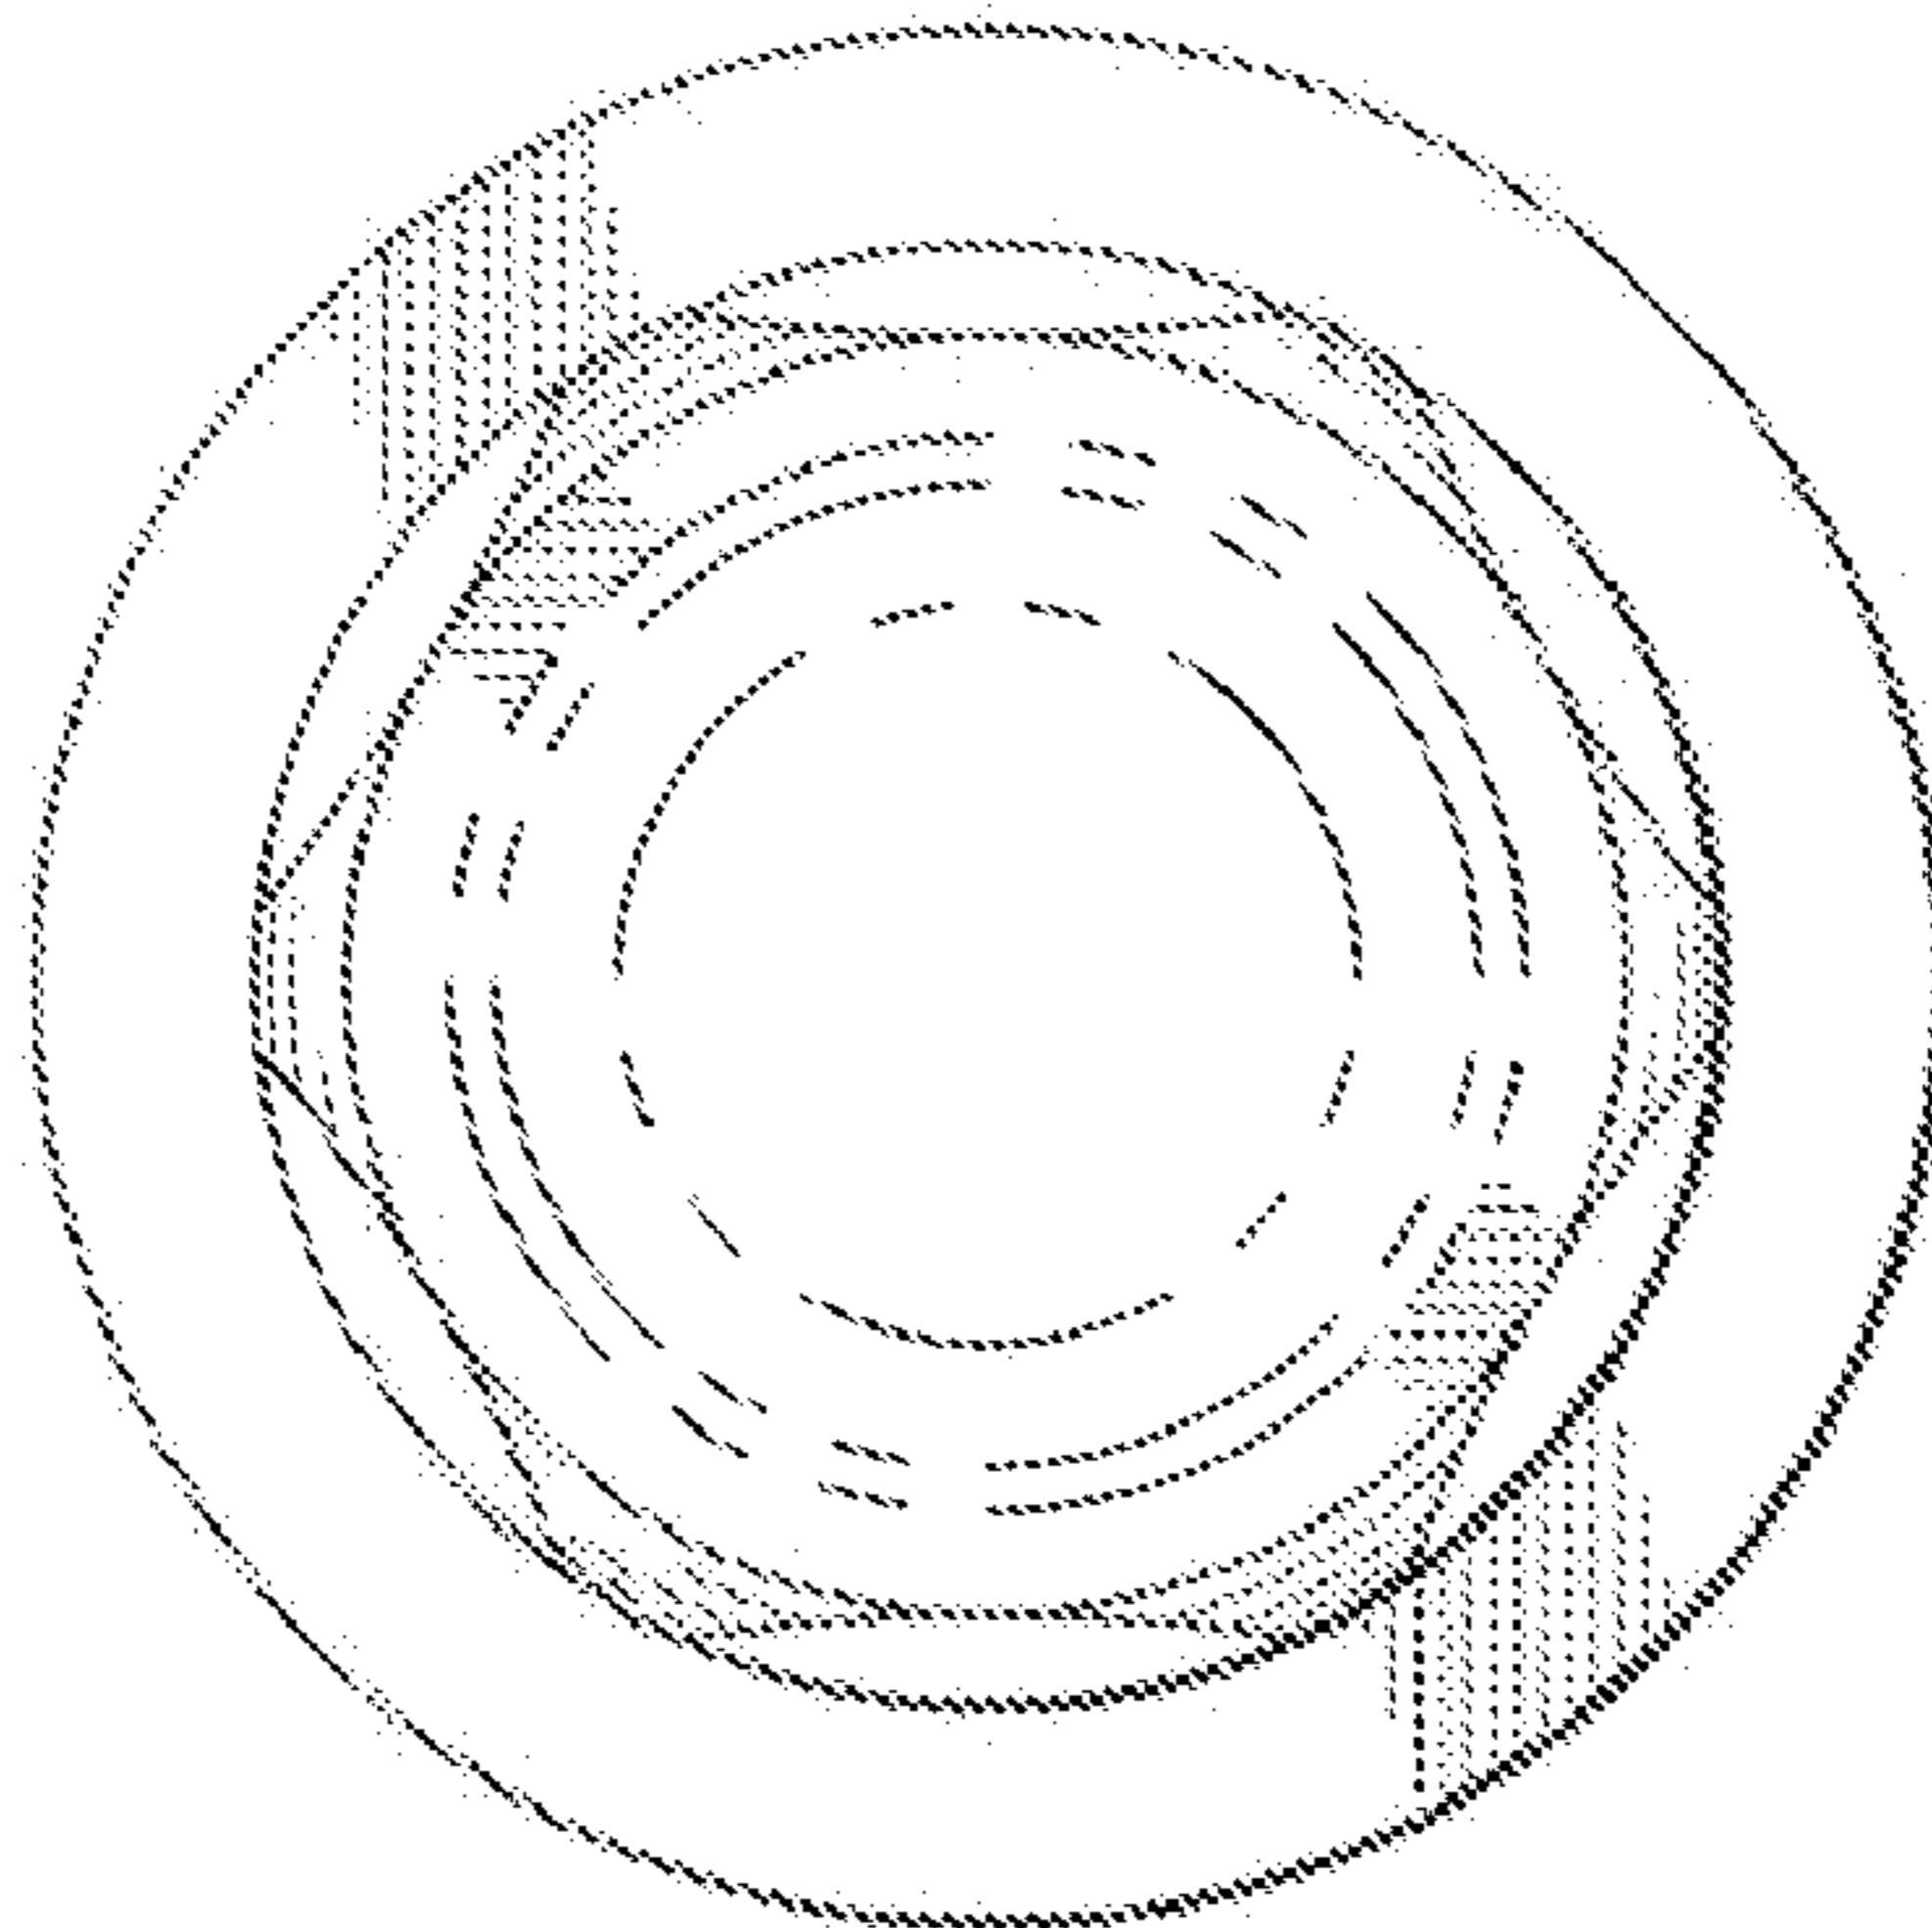


Fig. 2

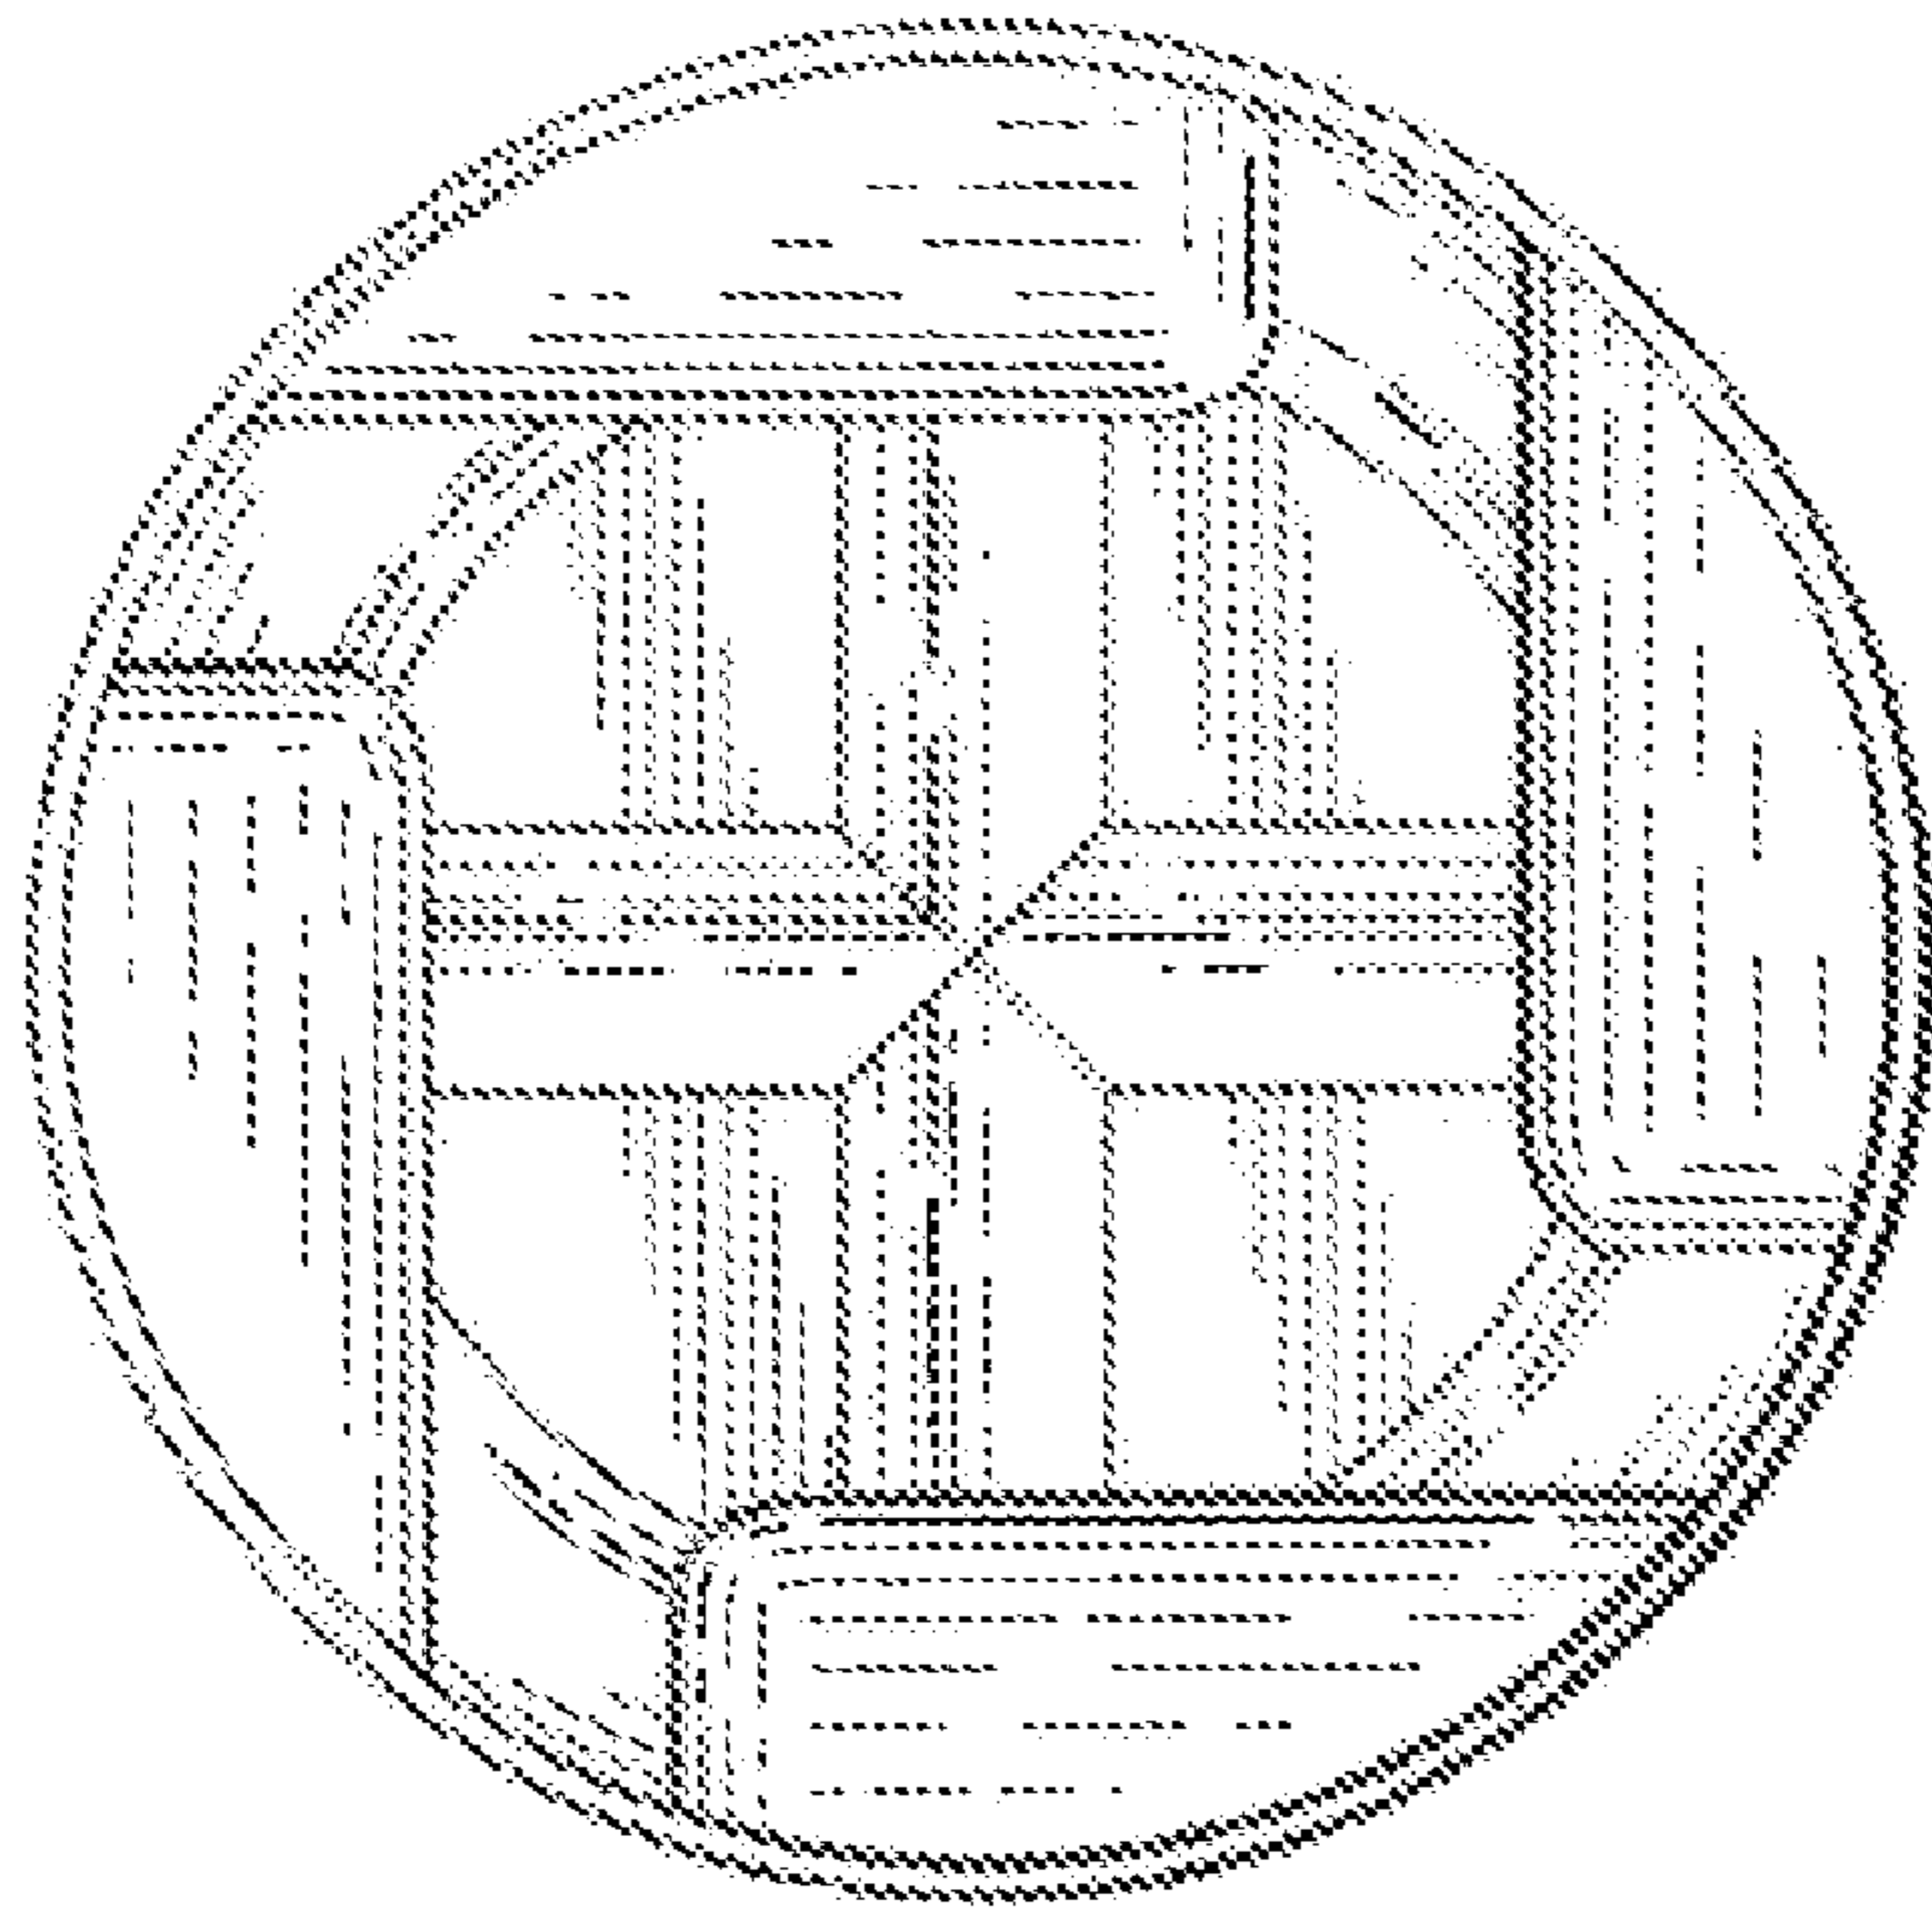


Fig. 3

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 583,057 S
APPLICATION NO. : 29/303402
DATED : December 16, 2008
INVENTOR(S) : Kojima et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page, Item (63), the Related U.S. Application Data information is incorrect. Item (63) should read:

Related U.S. Application Data

--(63) Division of Application No. 11/075,852, filed on
Mar. 10, 2005.--

Signed and Sealed this

Tenth Day of February, 2009



JOHN DOLL
Acting Director of the United States Patent and Trademark Office