



US00D583060S

(12) **United States Design Patent**  
**Kitamura et al.**

(10) **Patent No.:** **US D583,060 S**  
(45) **Date of Patent:** **\*\* Dec. 16, 2008**

- (54) **SPHYGMOMANOMETER**
- (75) Inventors: **Masashi Kitamura**, Matsusaka (JP);  
**Tadashi Koike**, Kyoto (JP); **Yukiko Mitsunami**, Otsu (JP); **Takahide Tanaka**, Otsu (JP); **Hiroyuki Kato**, Kyoto (JP); **Masayuki Fukutsuka**, Uji (JP); **Takashi Shigeno**, Kawasaki (JP); **Kazuya Andachi**, Kawasaki (JP)
- (73) Assignee: **Omron Healthcare Co., Ltd.**, Kyoto (JP)
- (\*\*) Term: **14 Years**
- (21) Appl. No.: **29/287,648**
- (22) Filed: **Sep. 4, 2007**

- D446,306 S \* 8/2001 Ochi et al. .... D24/165
- D473,945 S 4/2003 Nakanishi et al.
- 6,547,741 B2 4/2003 Mori et al.
- D484,980 S 1/2004 Hartwein et al.
- D496,104 S 9/2004 Eda et al.
- D532,518 S 11/2006 Eda et al.
- D533,279 S 12/2006 Kobayashi et al.
- D533,666 S 12/2006 Kobayashi et al.
- D537,944 S 3/2007 Eda et al.

**FOREIGN PATENT DOCUMENTS**

- KR 30-0256390 4/2000
- KR 30-0348509 3/2004

**OTHER PUBLICATIONS**

Japanese Office Action dated Feb. 27, 2007.

\* cited by examiner

*Primary Examiner*—Joel Sincavage

*Assistant Examiner*—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Harness, Dickey & Pierce PLC

**Related U.S. Application Data**

- (62) Division of application No. 29/277,672, filed on Mar. 6, 2007, now Pat. No. Des. 561,340.

**Foreign Application Priority Data**

- (30) Sep. 7, 2006 (JP) ..... D2006-023887
- Sep. 7, 2006 (JP) ..... D2006-023888
- Sep. 7, 2006 (JP) ..... D2006-023889
- Sep. 7, 2006 (JP) ..... D2006-023890
- Sep. 7, 2006 (JP) ..... D2006-023891
- Sep. 7, 2006 (JP) ..... D2006-023892

**CLAIM**

(57) The ornamental design for a sphygmomanometer, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of another embodiment of a sphygmomanometer showing our new design;

FIG. 2 is front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a bottom plan view thereof;

FIG. 6 is a right side elevational view thereof; and,

FIG. 7 is a left side elevational view thereof.

The broken lines in FIG. 5 are included for the purpose of illustrating a portion of the sphygmomanometer that forms no part of the claimed design.


- (51) **LOC (8) Cl.** ..... **24-02**
- (52) **U.S. Cl.** ..... **D24/165**
- (58) **Field of Classification Search** ..... D24/165-169, D24/186; D10/96, 98; 600/480, 485, 500, 600/502, 503, 490-496, 499; 128/900  
See application file for complete search history.

**References Cited**

**U.S. PATENT DOCUMENTS**

- D283,916 S \* 5/1986 Akiyama ..... D24/165
- D315,020 S \* 2/1991 Sakaguchi et al. .... D24/165
- D330,594 S \* 10/1992 Koshino ..... D24/165
- D338,271 S \* 8/1993 Yoshikawa et al. .... D24/165
- D344,338 S 2/1994 Yoshikawa et al.
- D373,419 S 9/1996 Muramatsu et al.
- D437,414 S \* 2/2001 Kern et al. .... D24/165

**1 Claim, 5 Drawing Sheets**

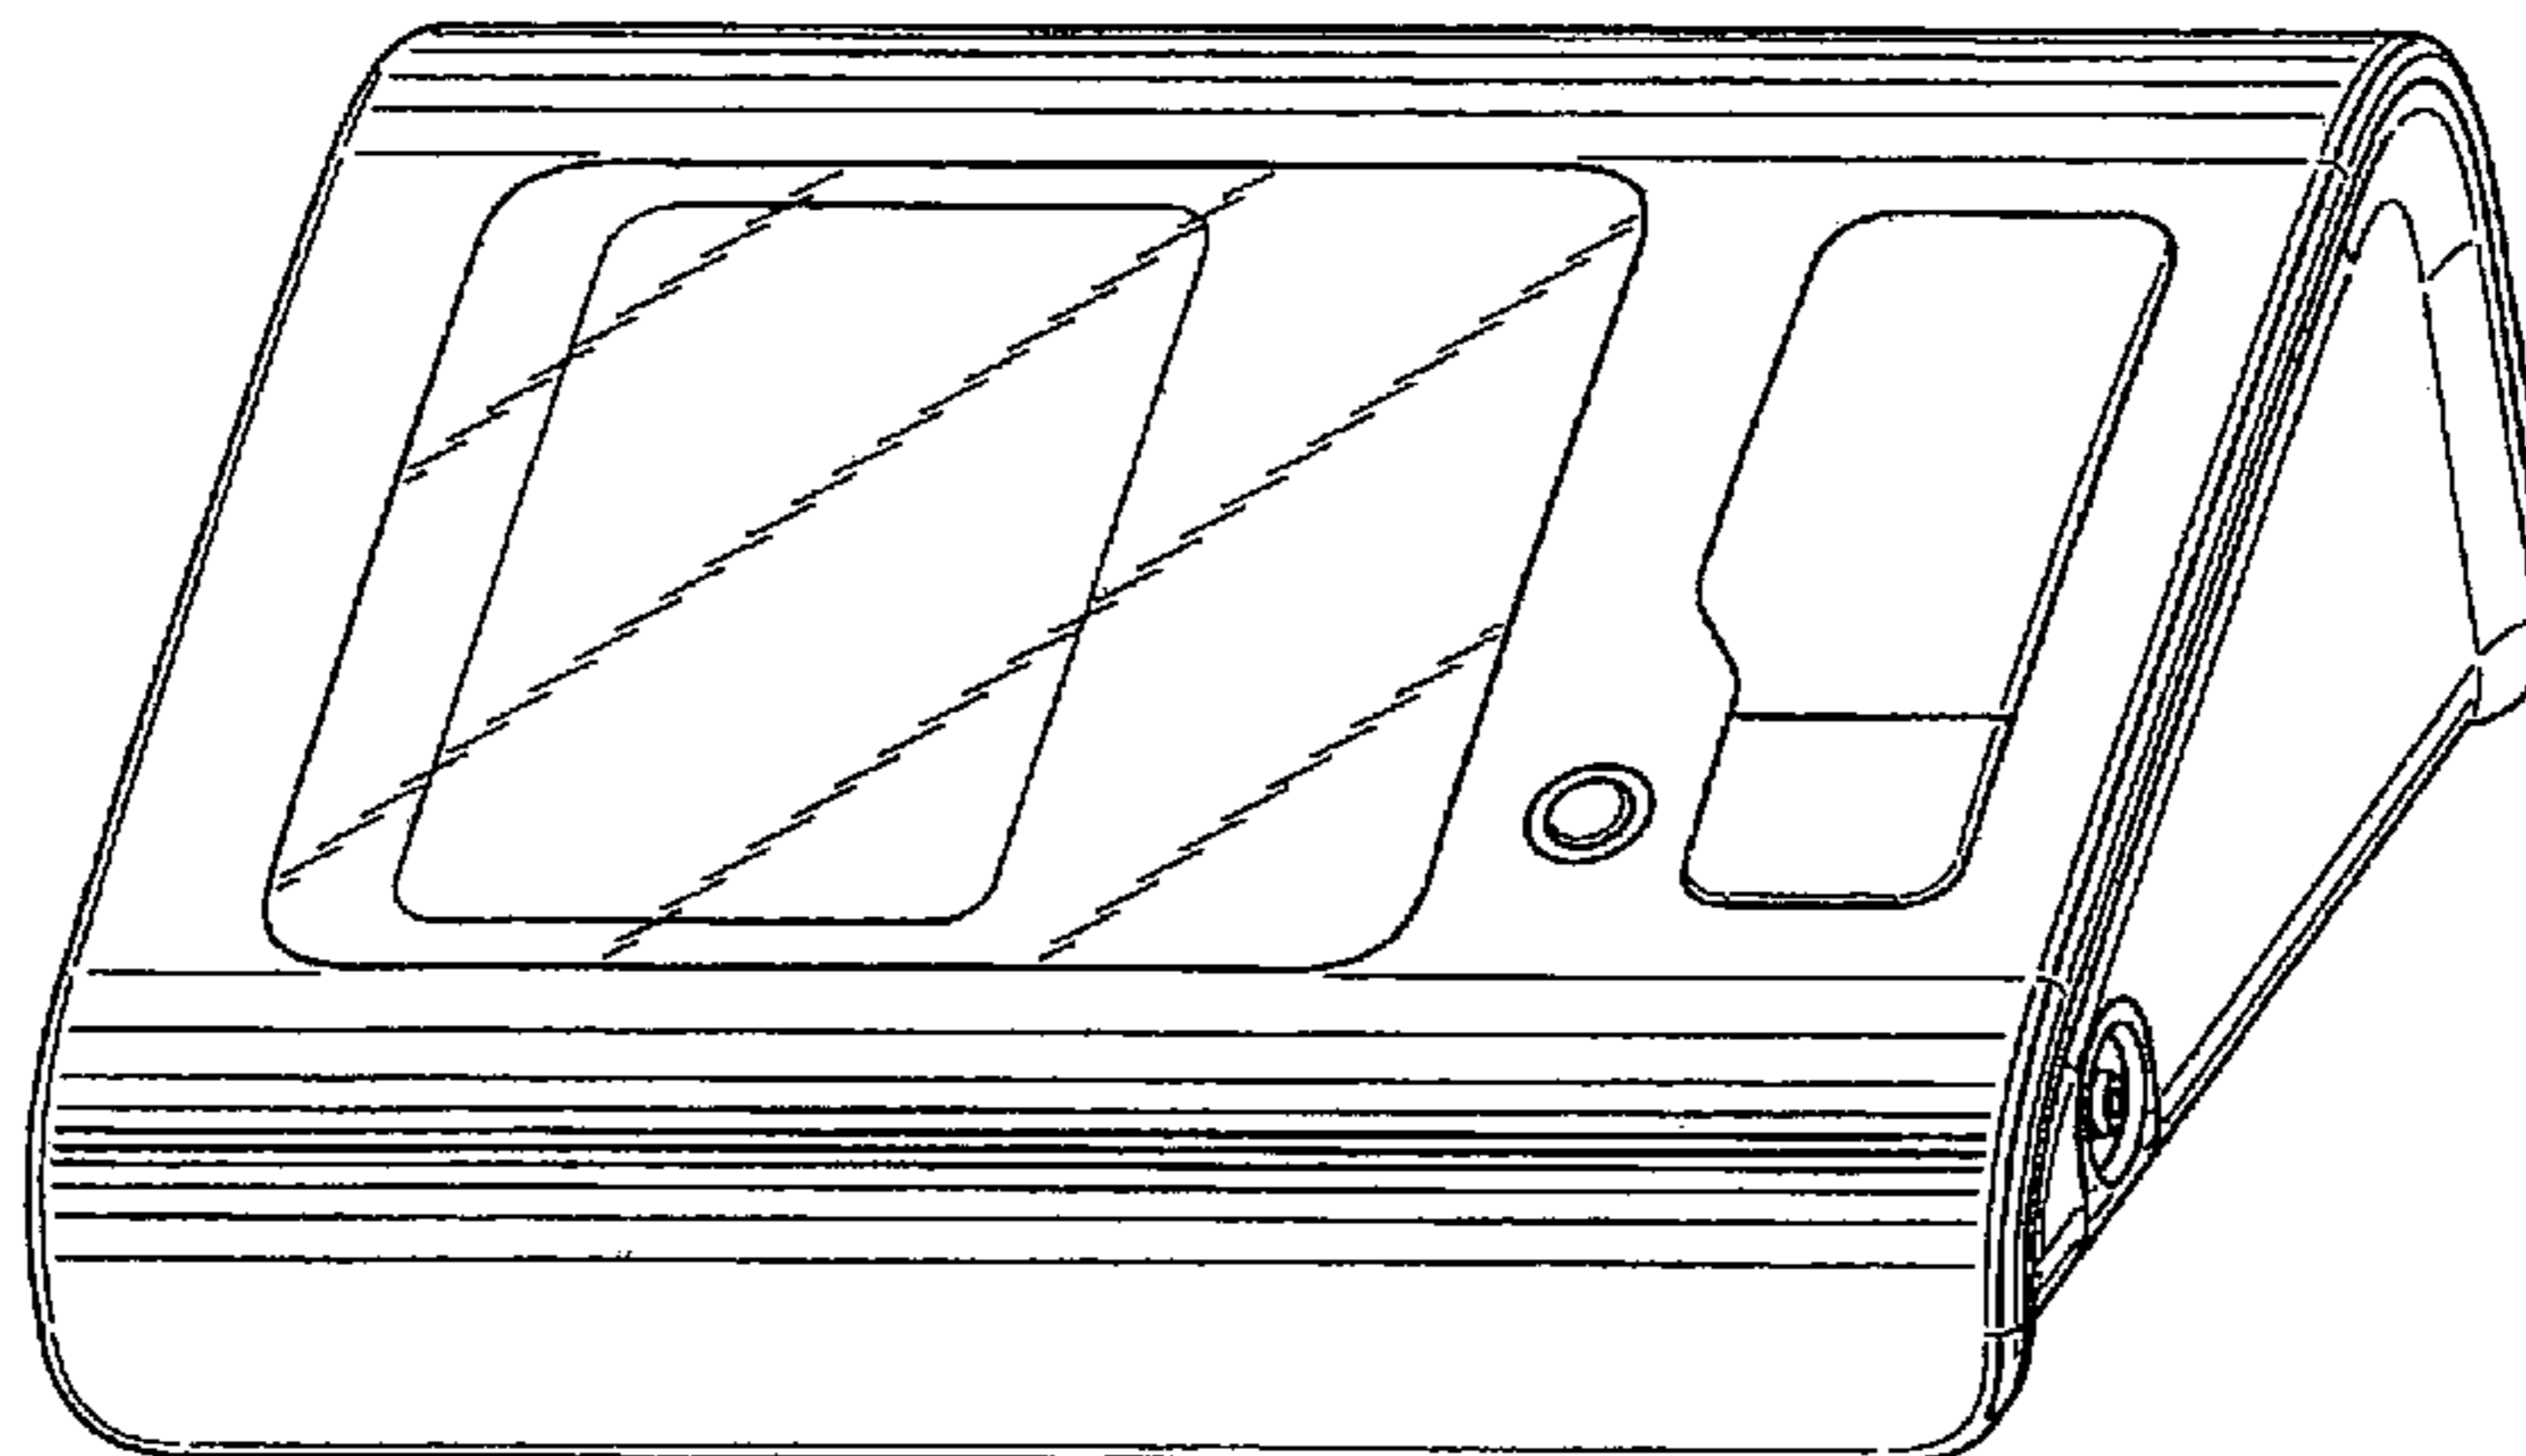

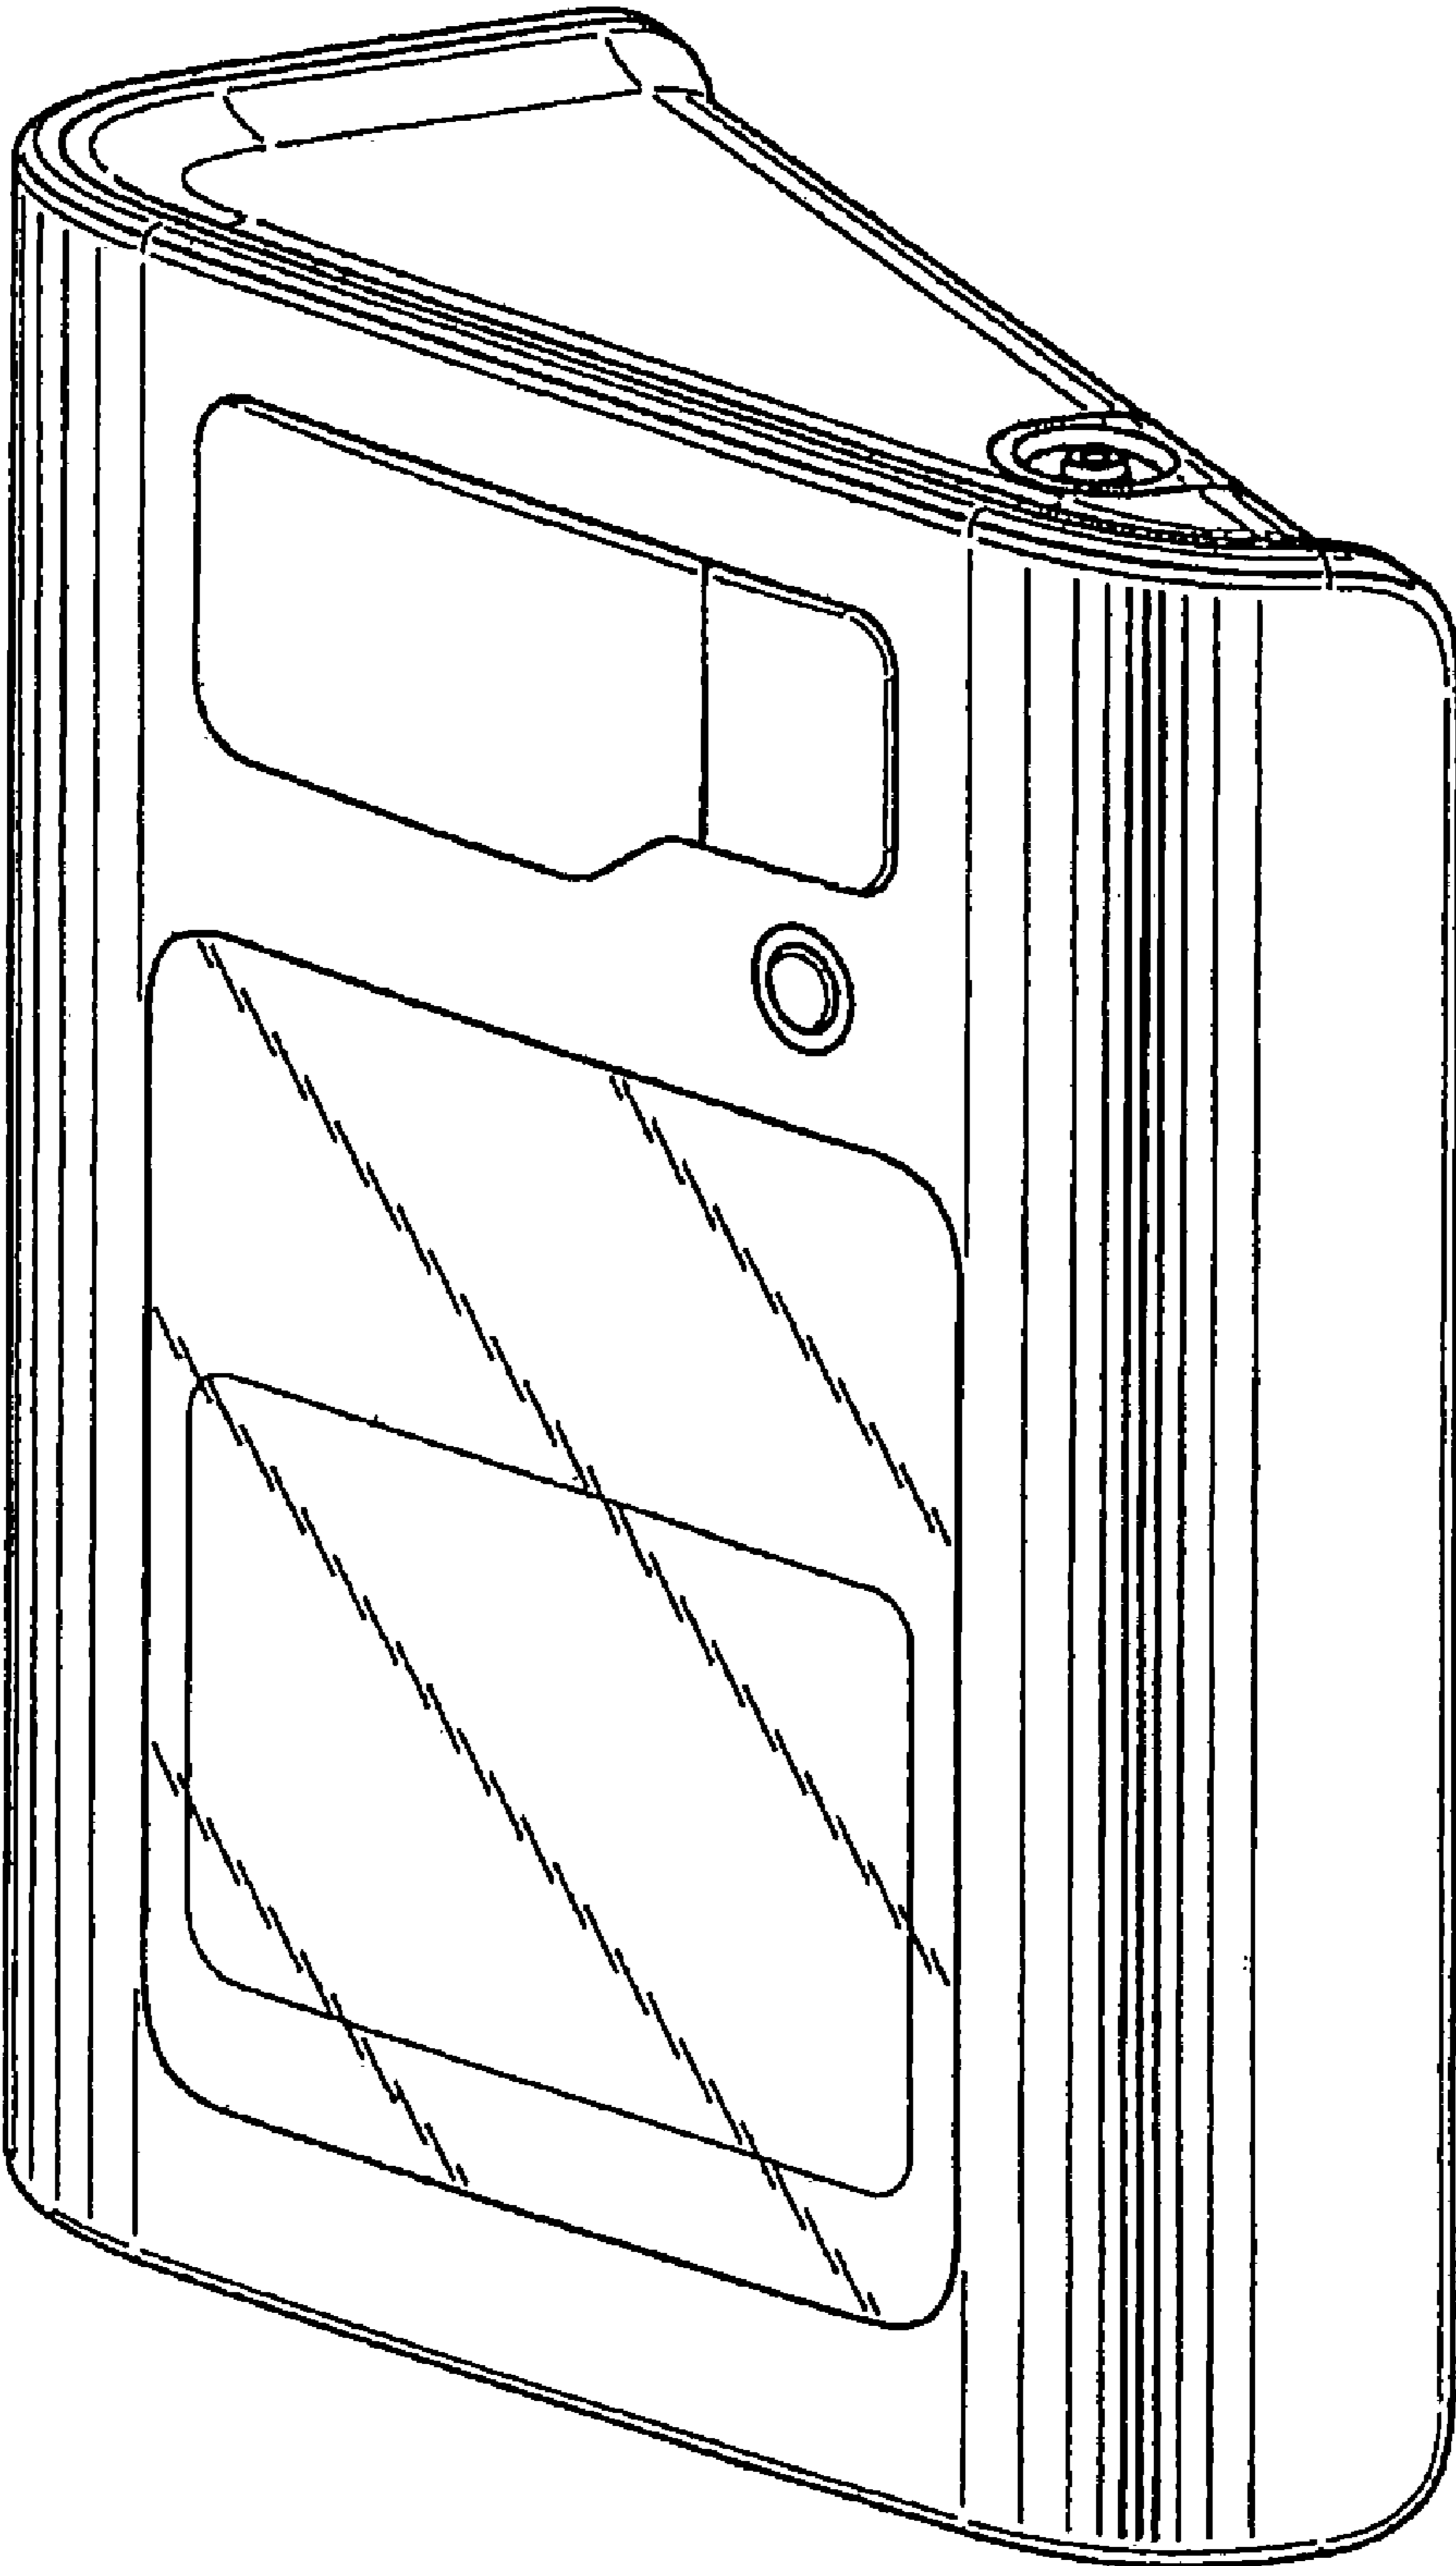


FIG. 1

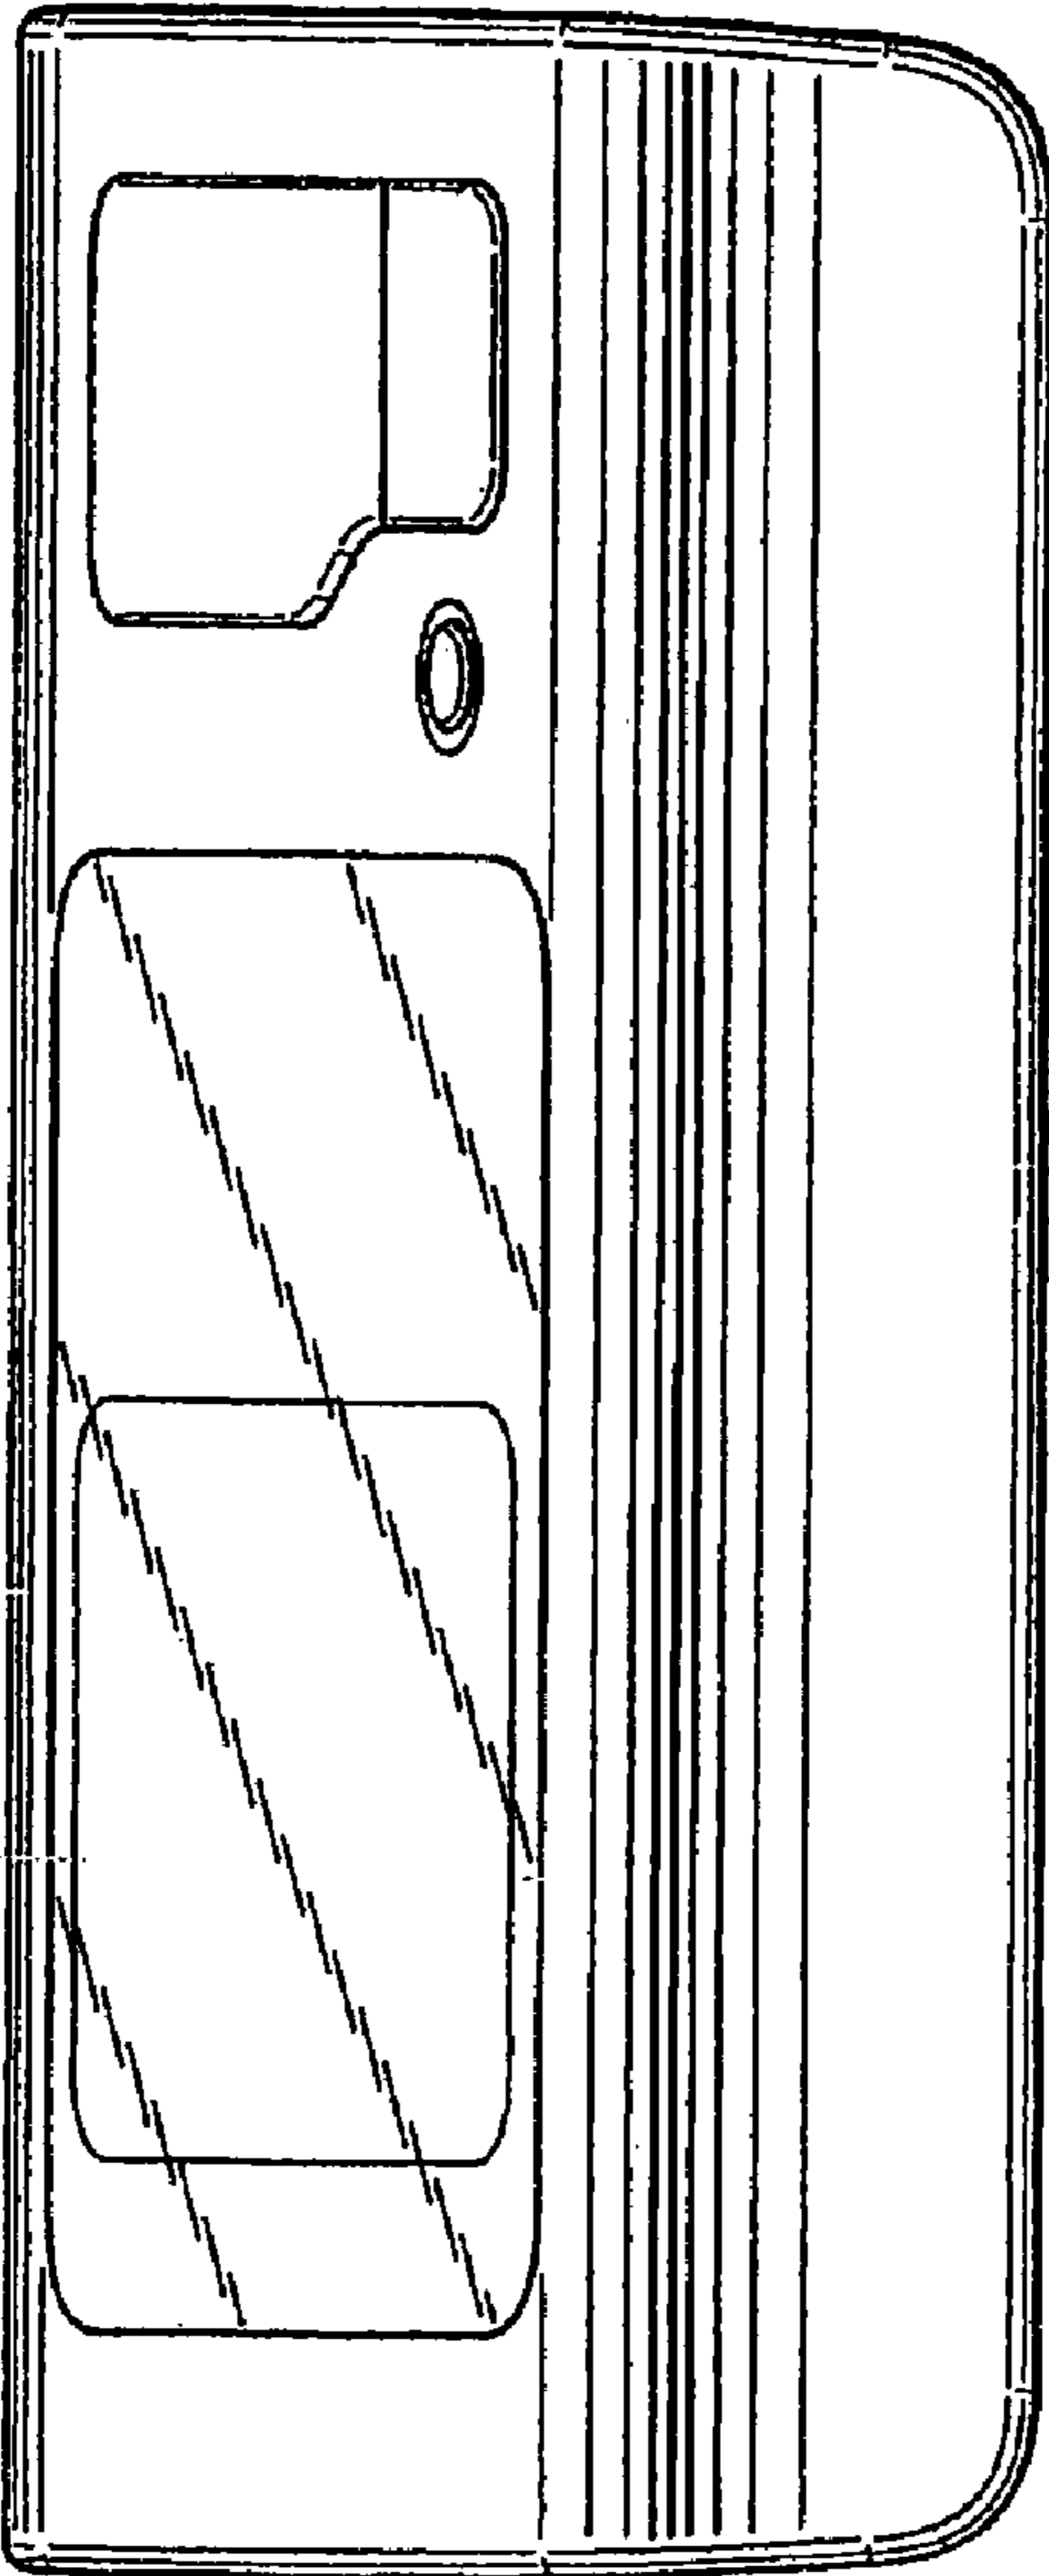


FIG. 2

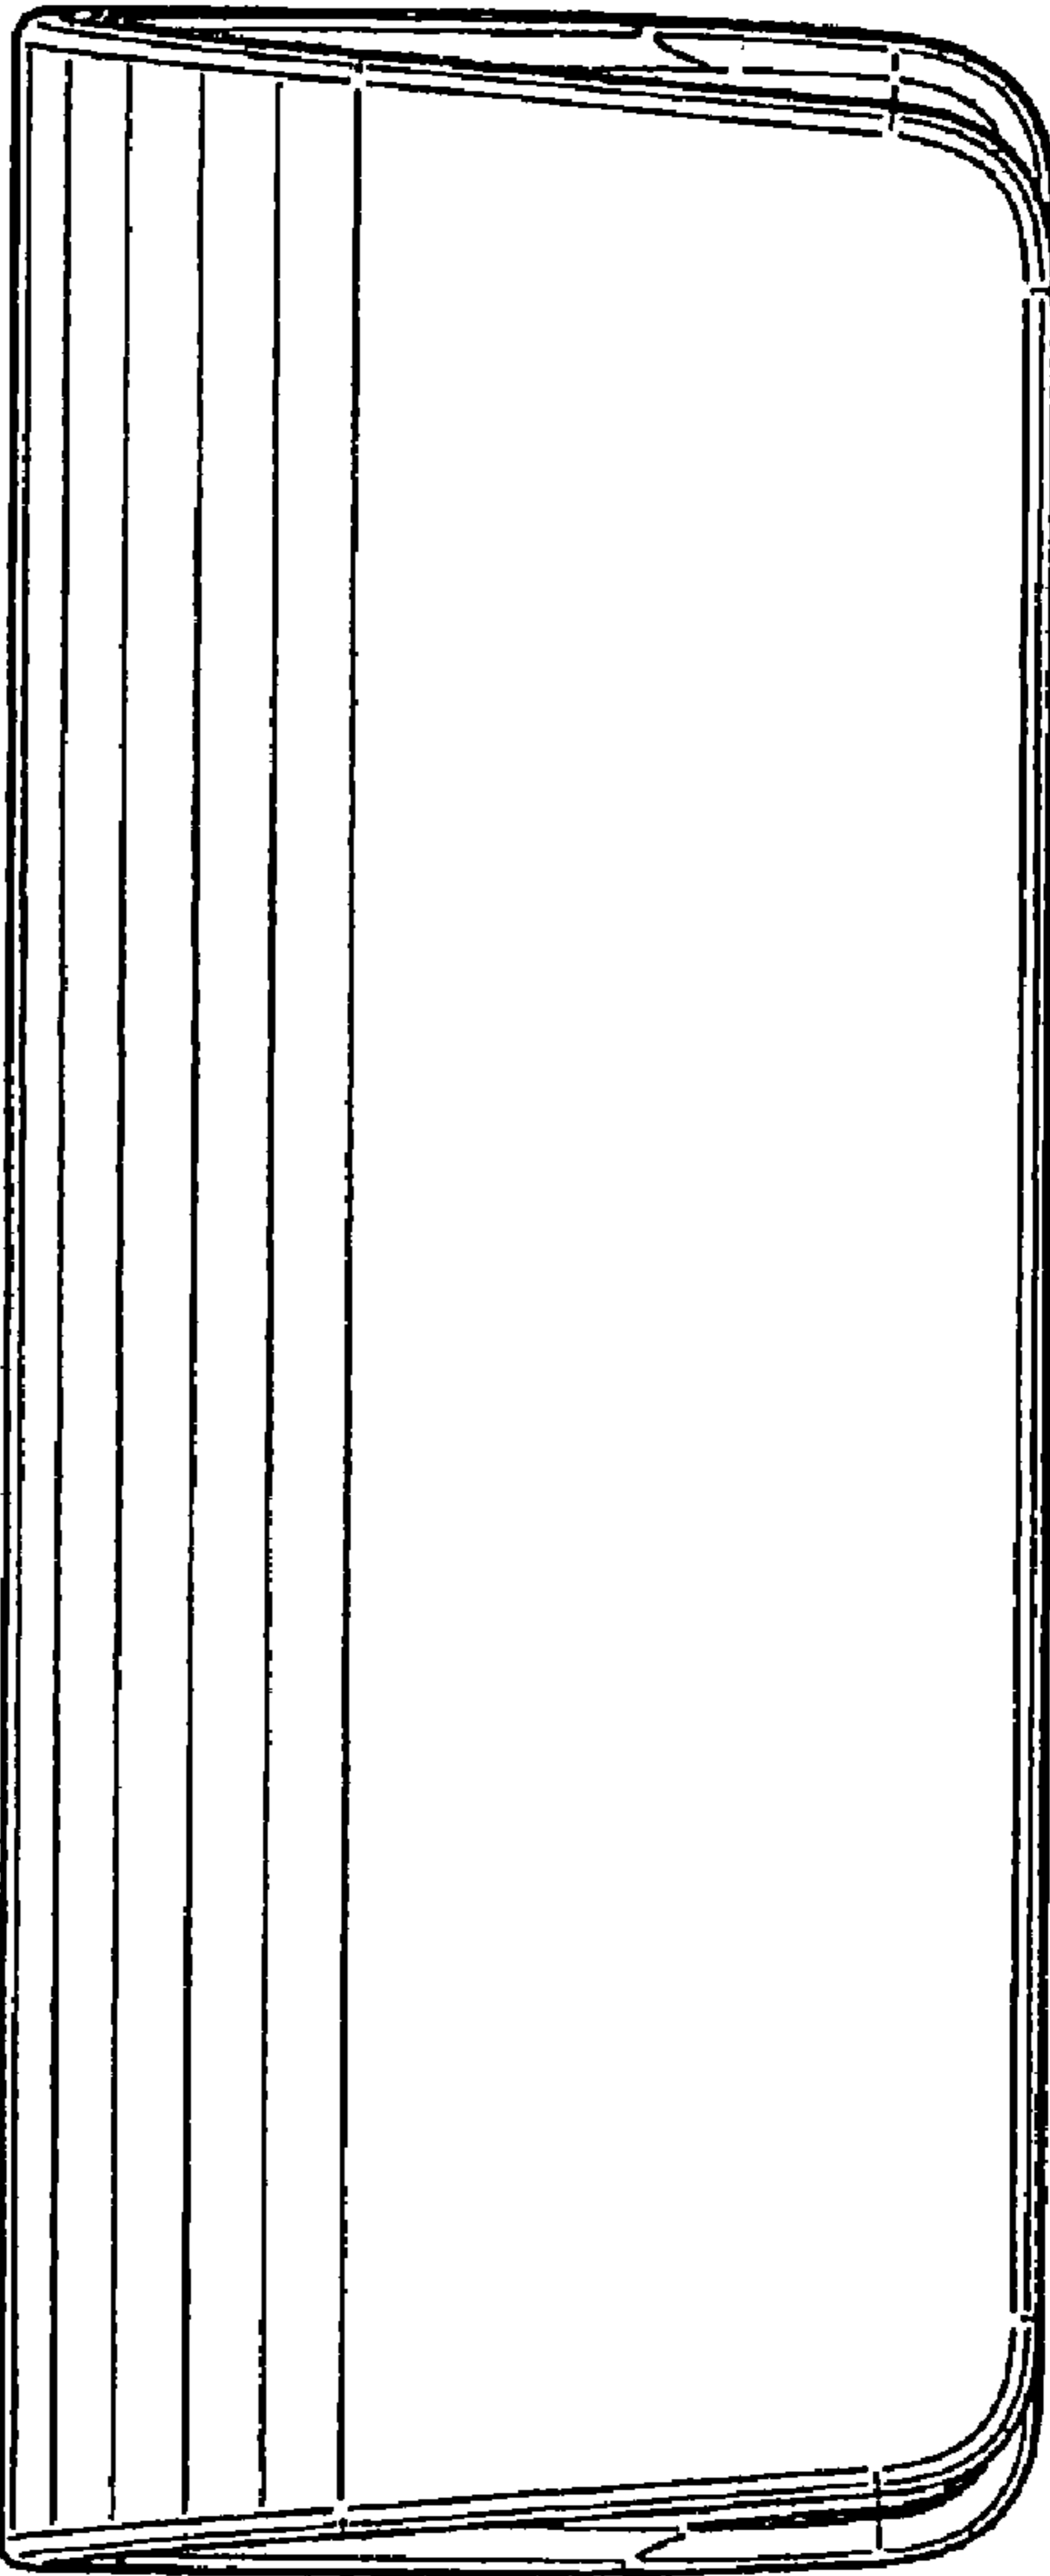


FIG. 3

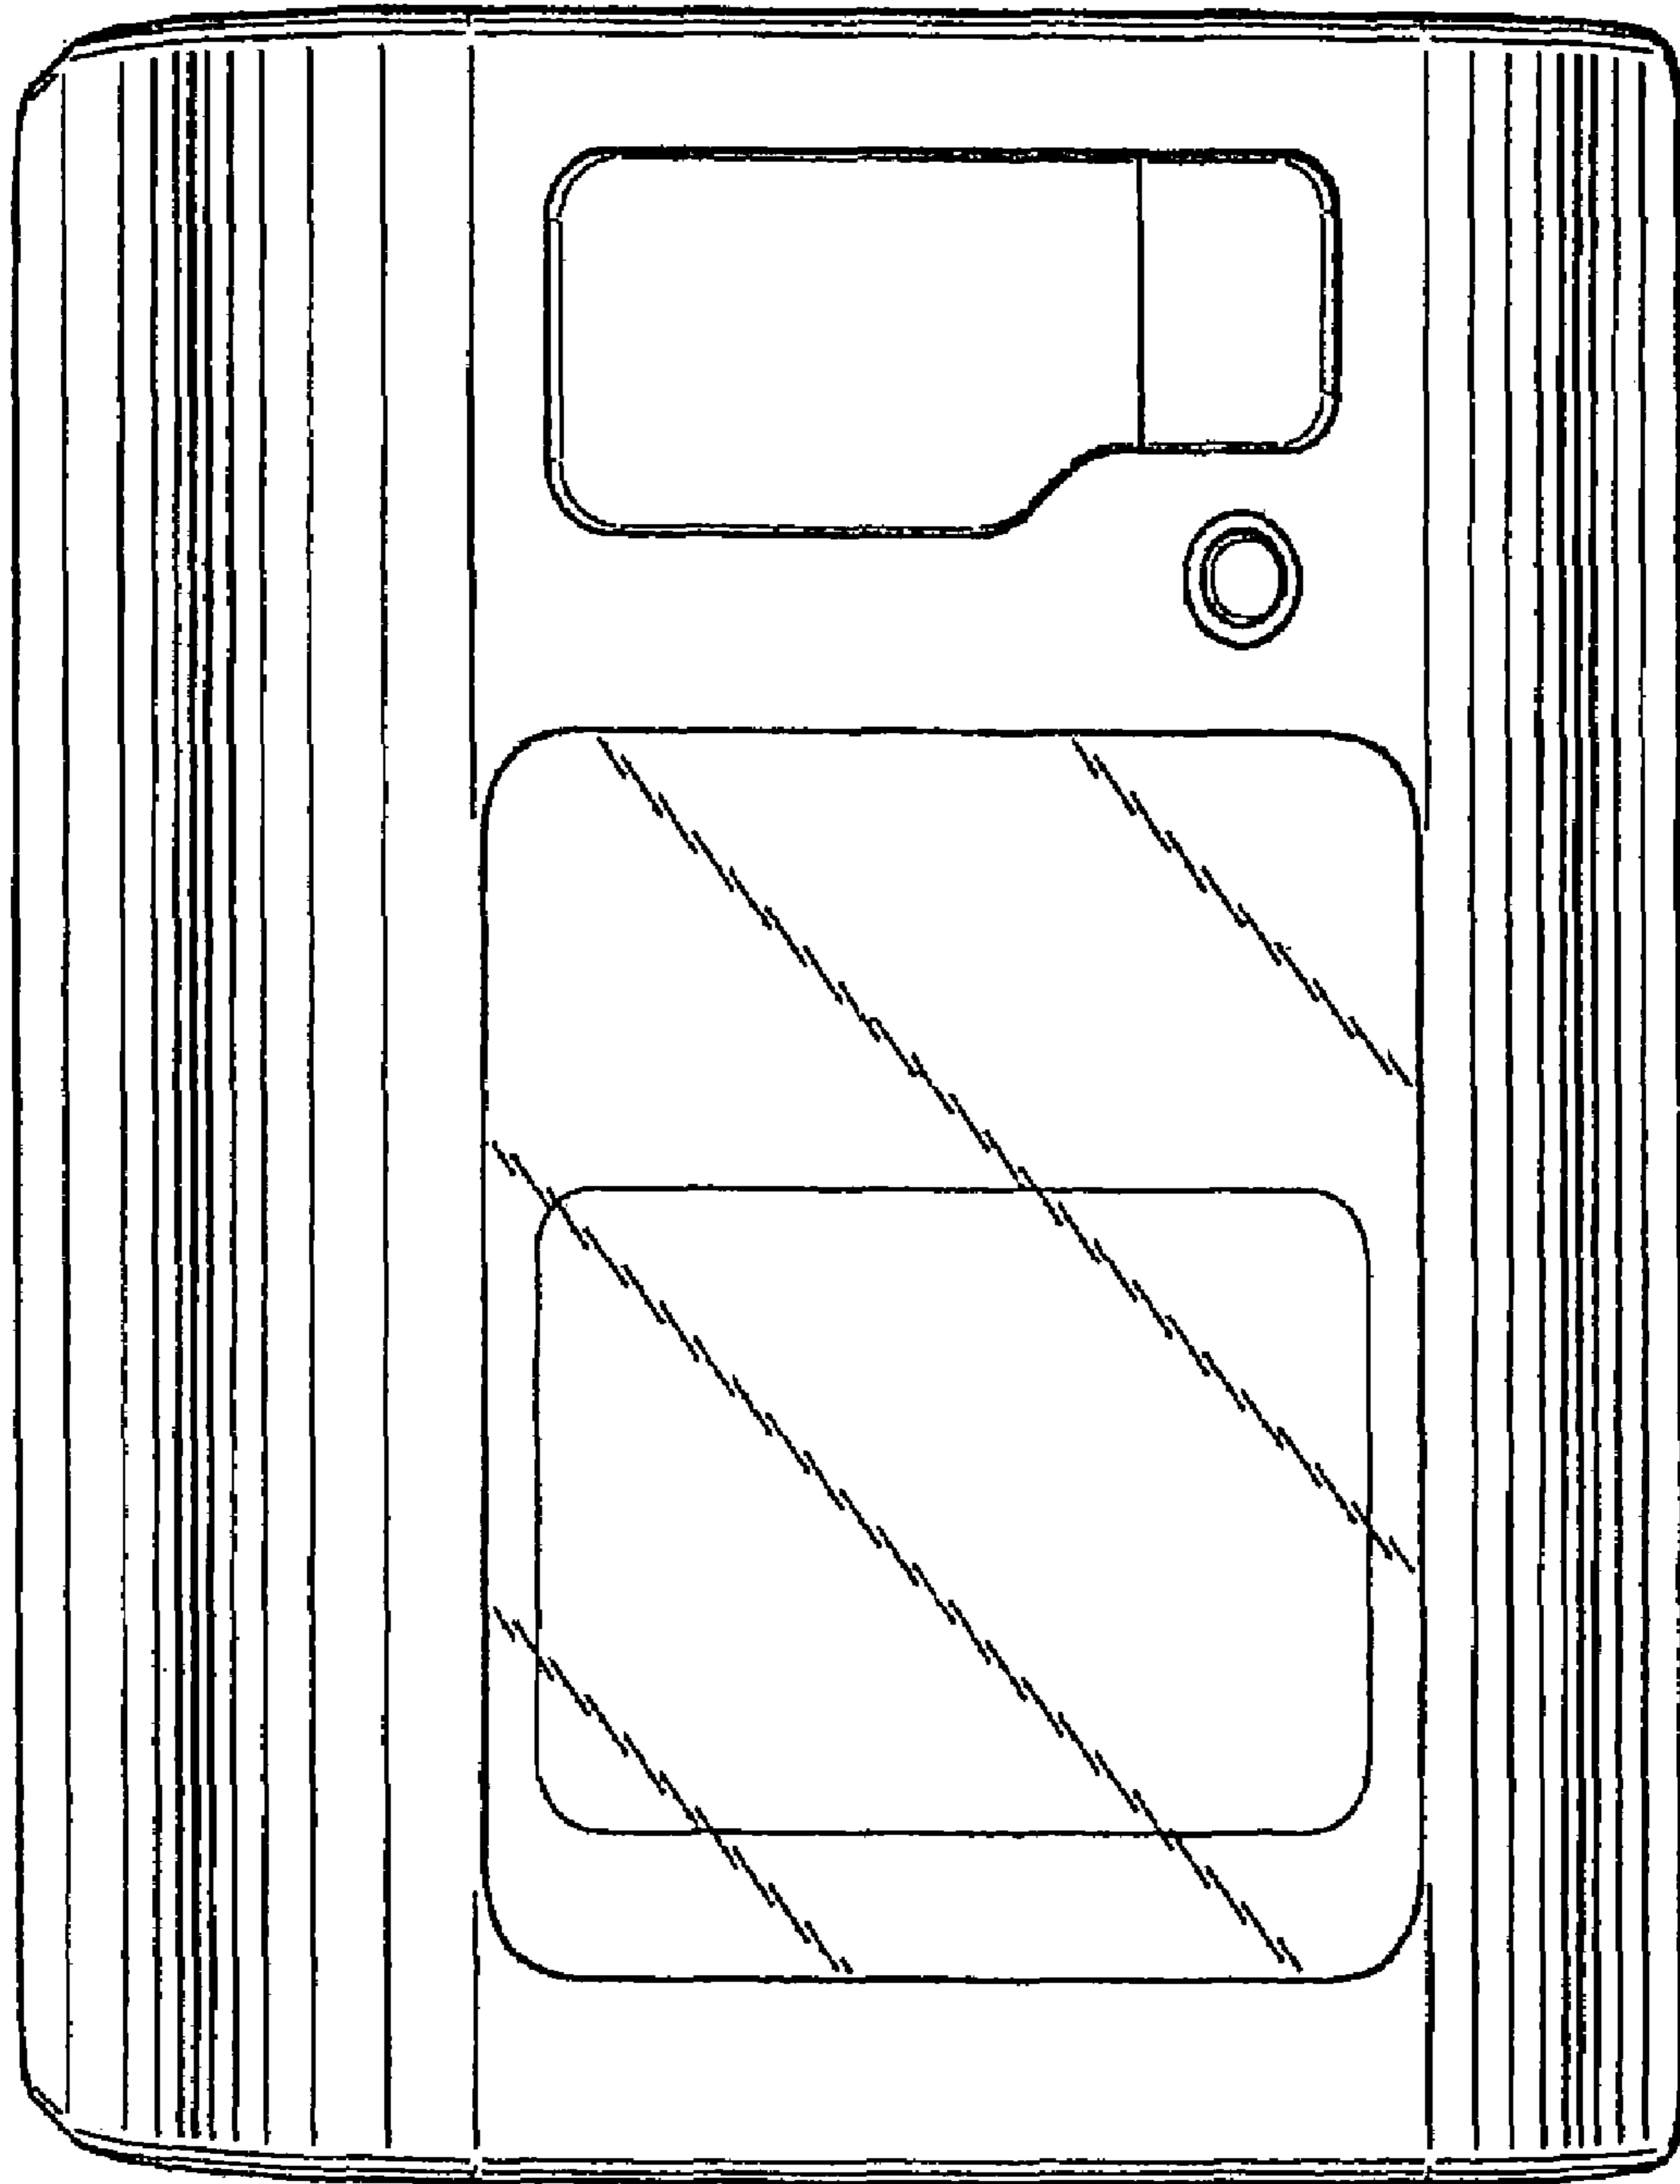


FIG. 4

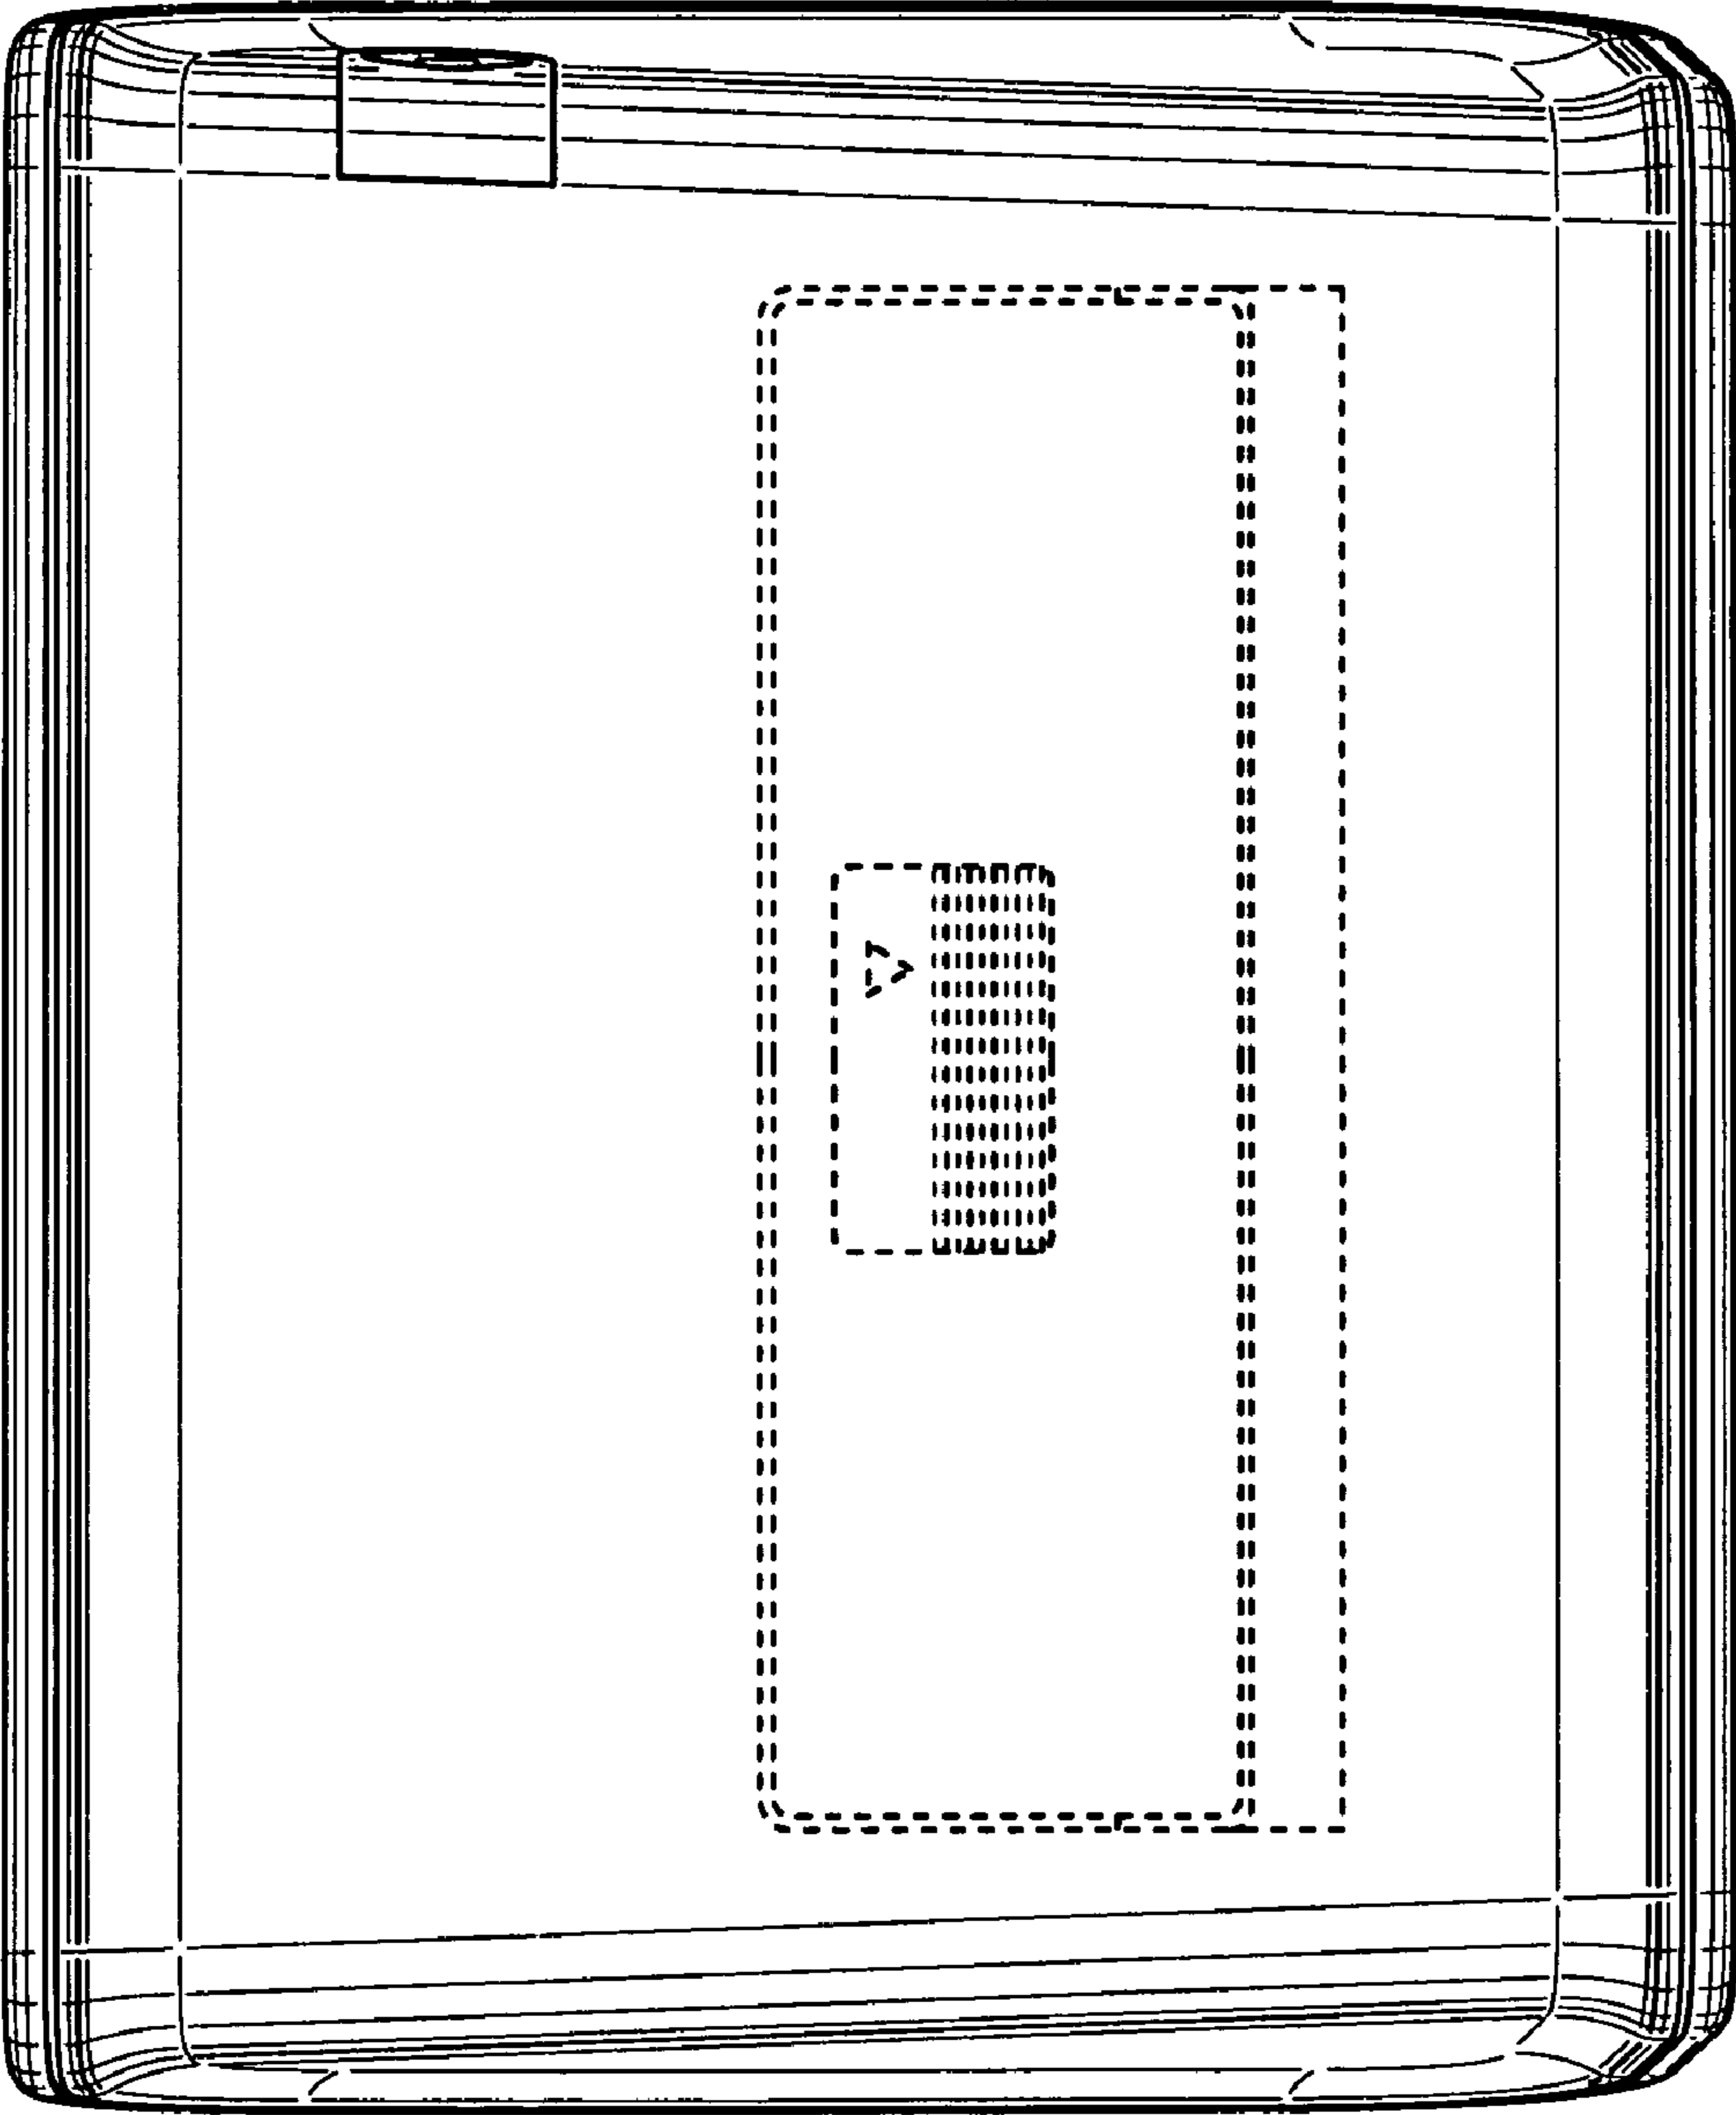


Fig. 5

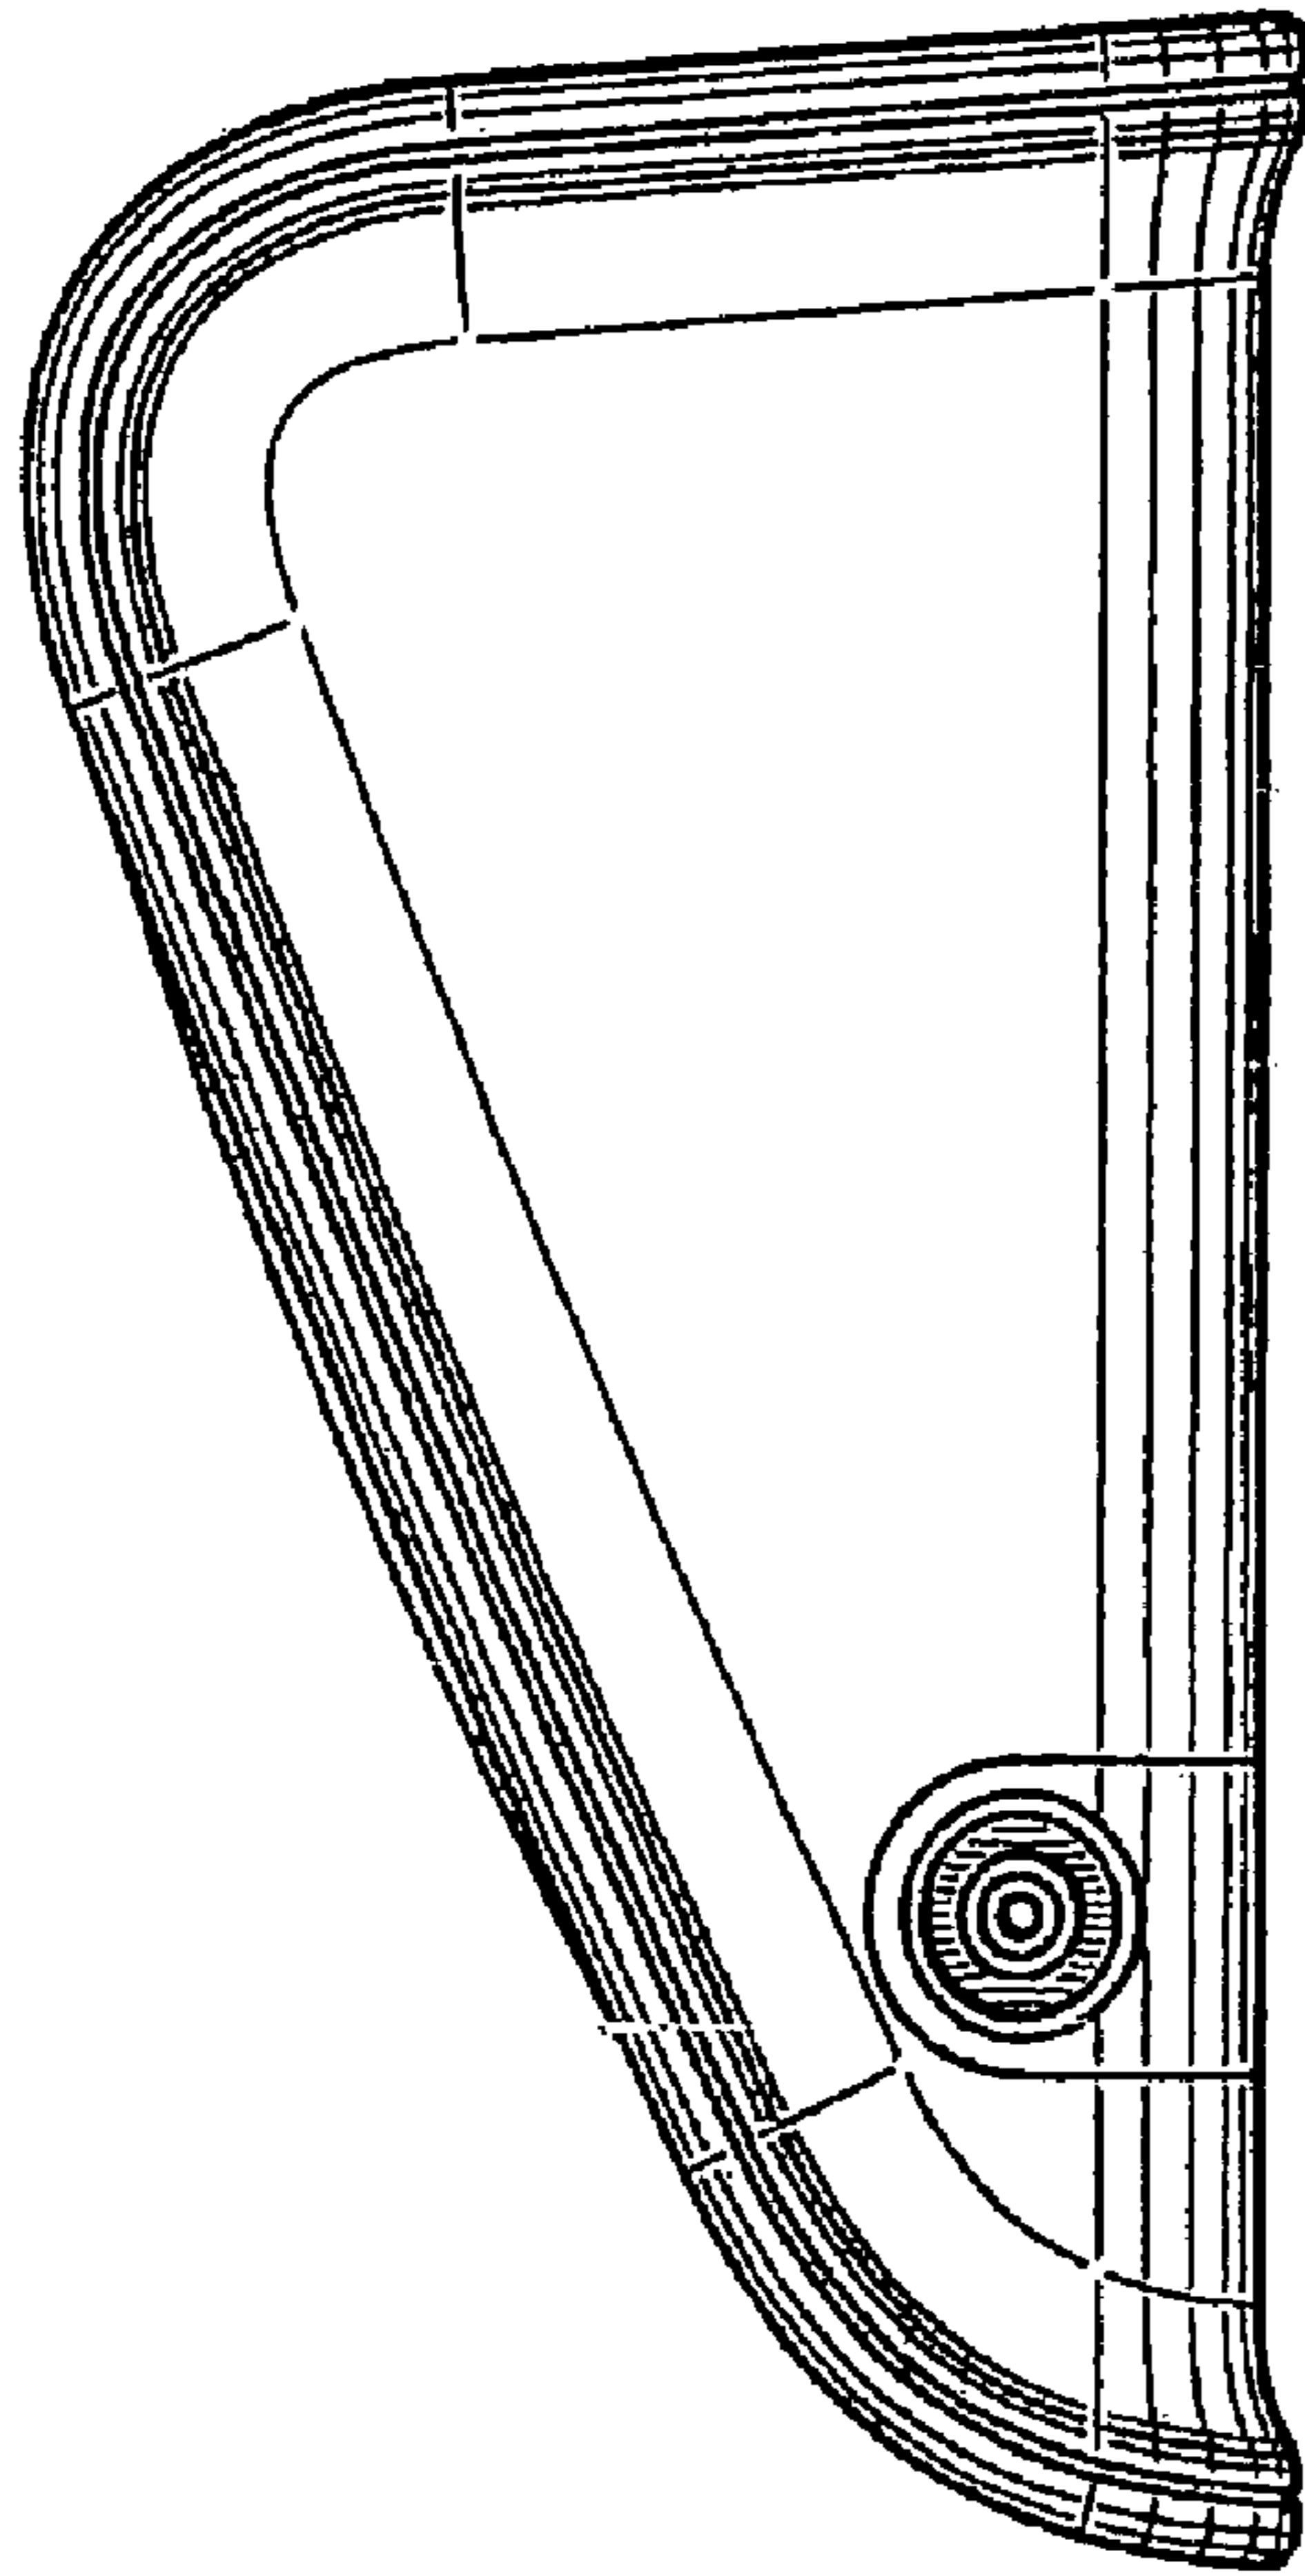


FIG. 6

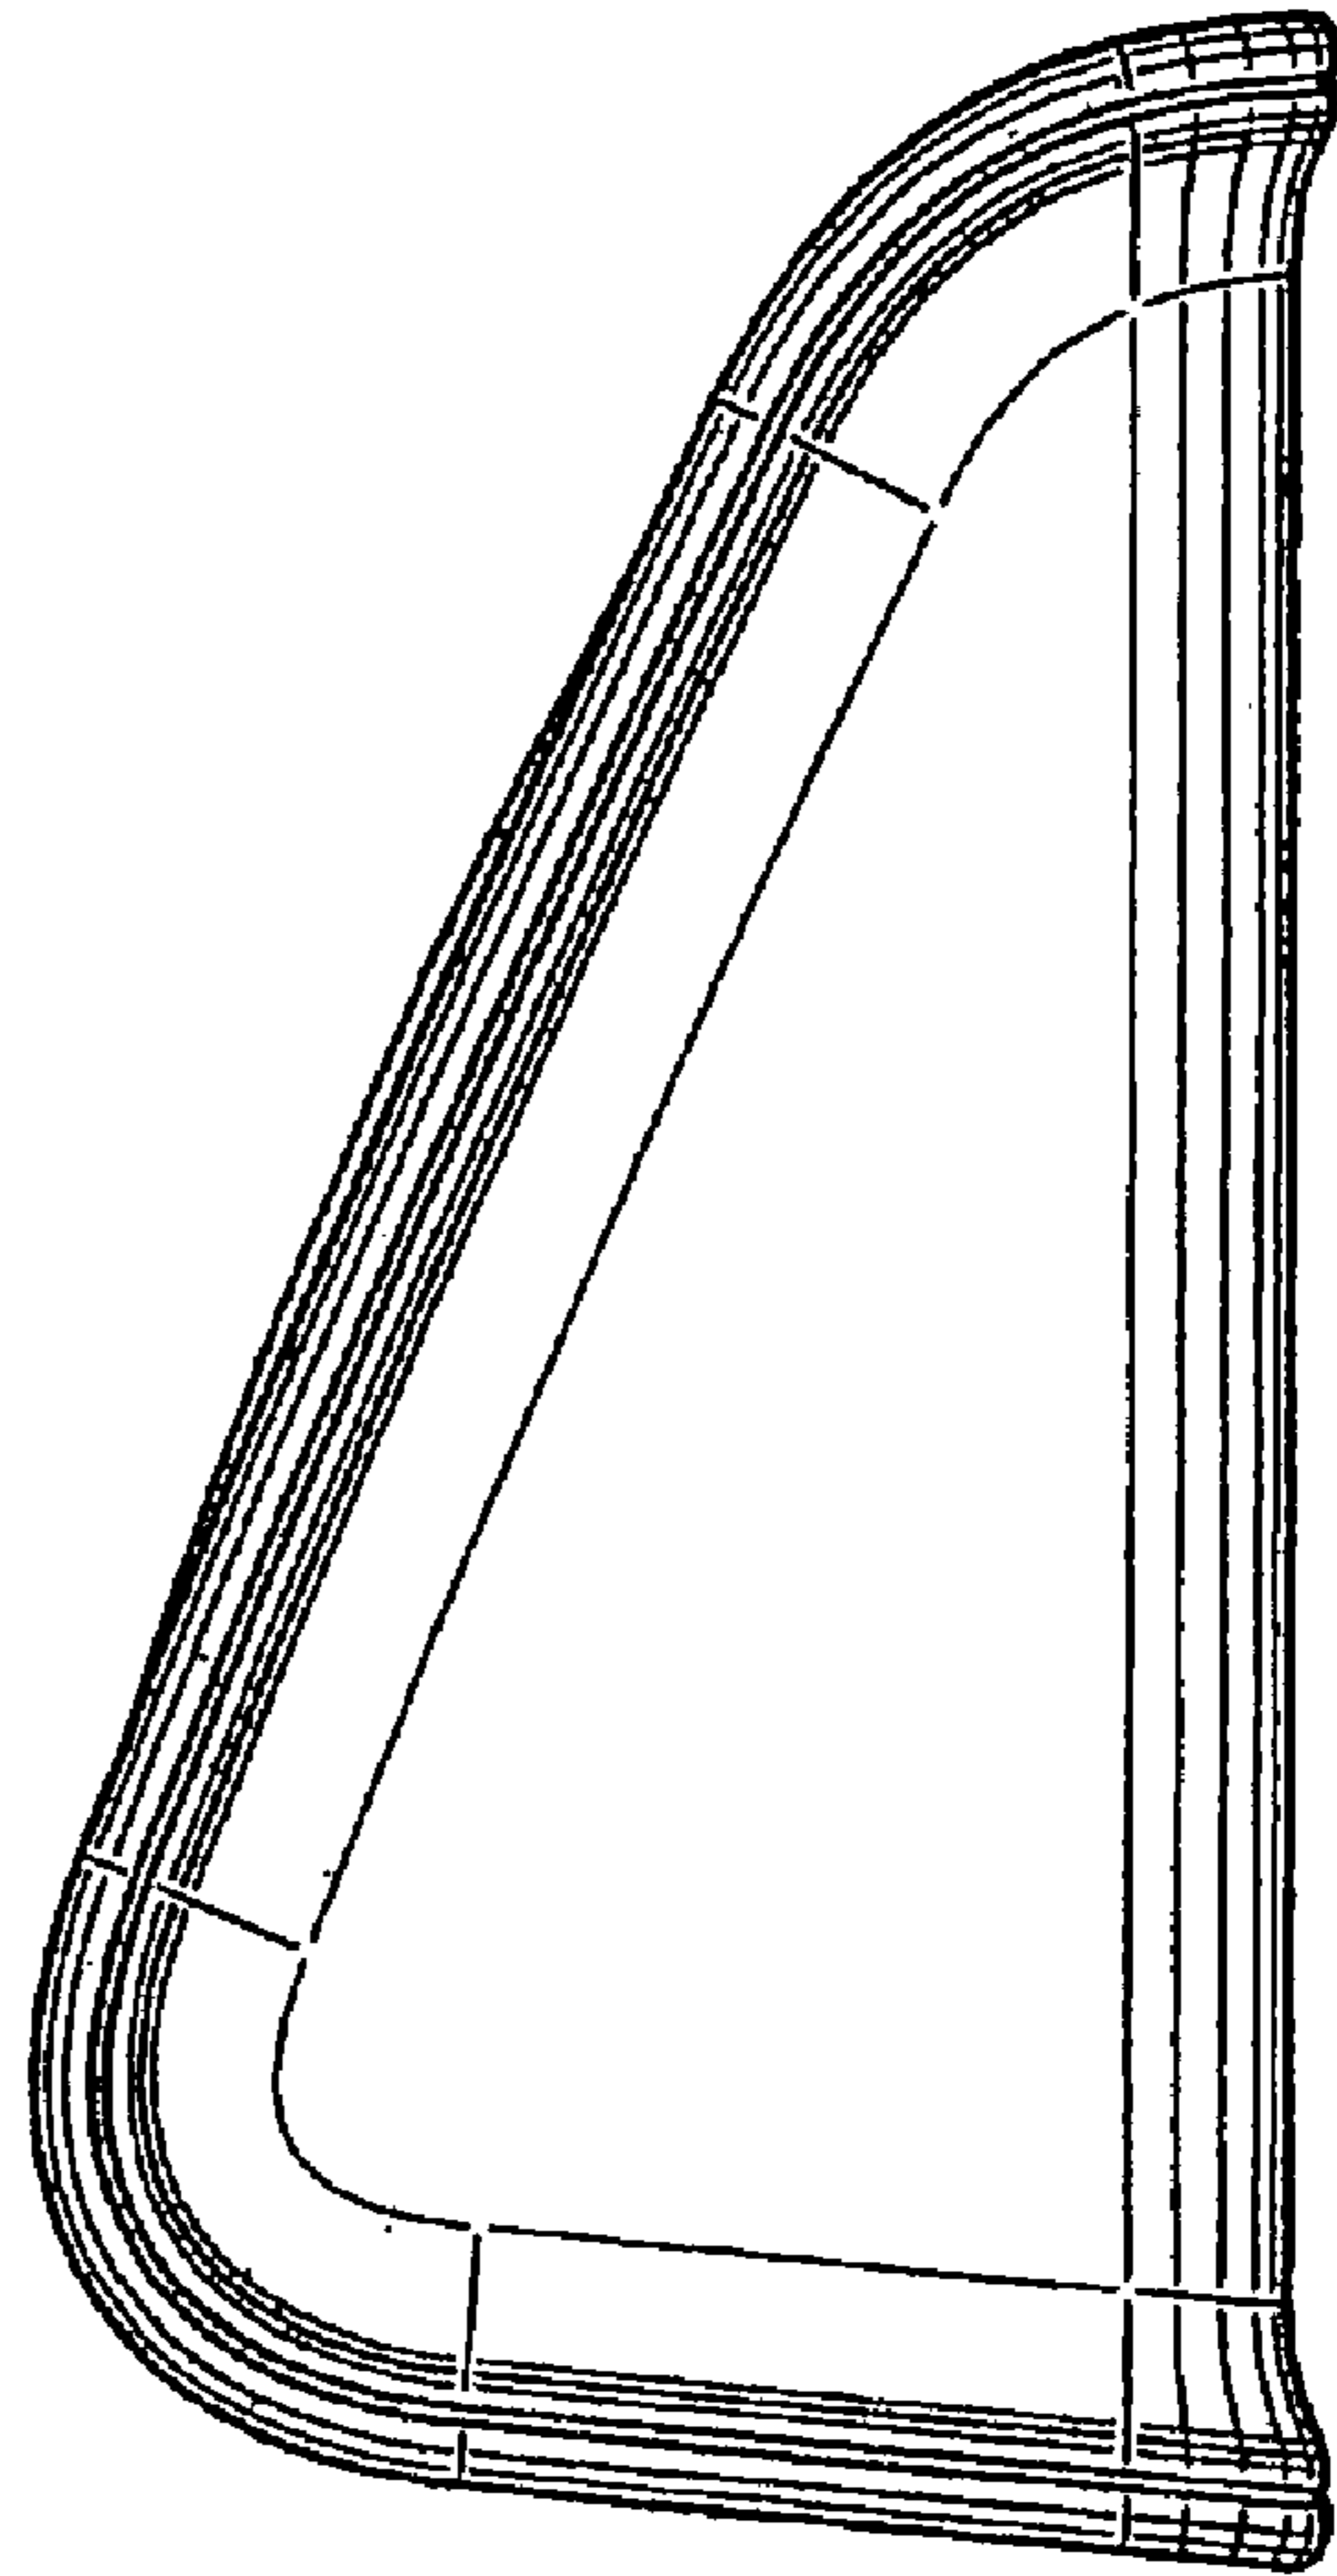


FIG. 7