



US00D585992S

(12) **United States Design Patent**
Kousuge

(10) **Patent No.:** **US D585,992 S**
(45) **Date of Patent:** **** Feb. 3, 2009**

(54) **URINE GLUCOSE METER**

(75) Inventor: **Rie Kousuge**, Yashio (JP)

(73) Assignee: **Tanita Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/292,646**

(22) Filed: **Oct. 22, 2007**

(30) **Foreign Application Priority Data**

Apr. 25, 2007 (JP) 2007-011230

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D10/78,
D10/81; D24/169, 183–187, 216–234; 422/68.1,
422/63, 65, 99, 56, 58, 61, 67, 102, 104;
436/180, 43, 46, 50, 55; 600/309, 318, 322,
600/368, 583; 204/403.03, 406, 407
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D388,519 S * 12/1997 Skiffington et al. D24/223
D390,667 S * 2/1998 Nazareth D24/223
D403,975 S * 1/1999 Douglas et al. D24/225
D408,082 S * 4/1999 Skiffington et al. D24/223
D432,244 S * 10/2000 Anderson et al. D24/223
D470,240 S * 2/2003 Niedbala et al. D24/223
D474,271 S * 5/2003 Iori et al. D24/216
D530,825 S * 10/2006 Lee et al. D24/223

D531,735 S * 11/2006 Lee et al. D24/223
D536,798 S * 2/2007 Lee et al. D24/223
D545,439 S * 6/2007 Draudt et al. D24/186
D569,982 S * 5/2008 Loerwald D24/186

* cited by examiner

Primary Examiner—Robert A. Delehanty

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Frishauf, Holtz, Goodman & Chick, P.C.

(57) **CLAIM**

The ornamental design for a urine glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a front, left side, top perspective view of a urine glucose meter showing my new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;


FIG. 6 is a top plan view thereof;

FIG. 7 is a bottom plan view thereof; and,

FIG. 8 is a reference perspective view thereof showing a state in which this article is fold and a cap is attached.

The portions of the urine glucose meter in broken lines are shown for illustrative purposes only and form no part of the claimed design.

1 Claim, 7 Drawing Sheets

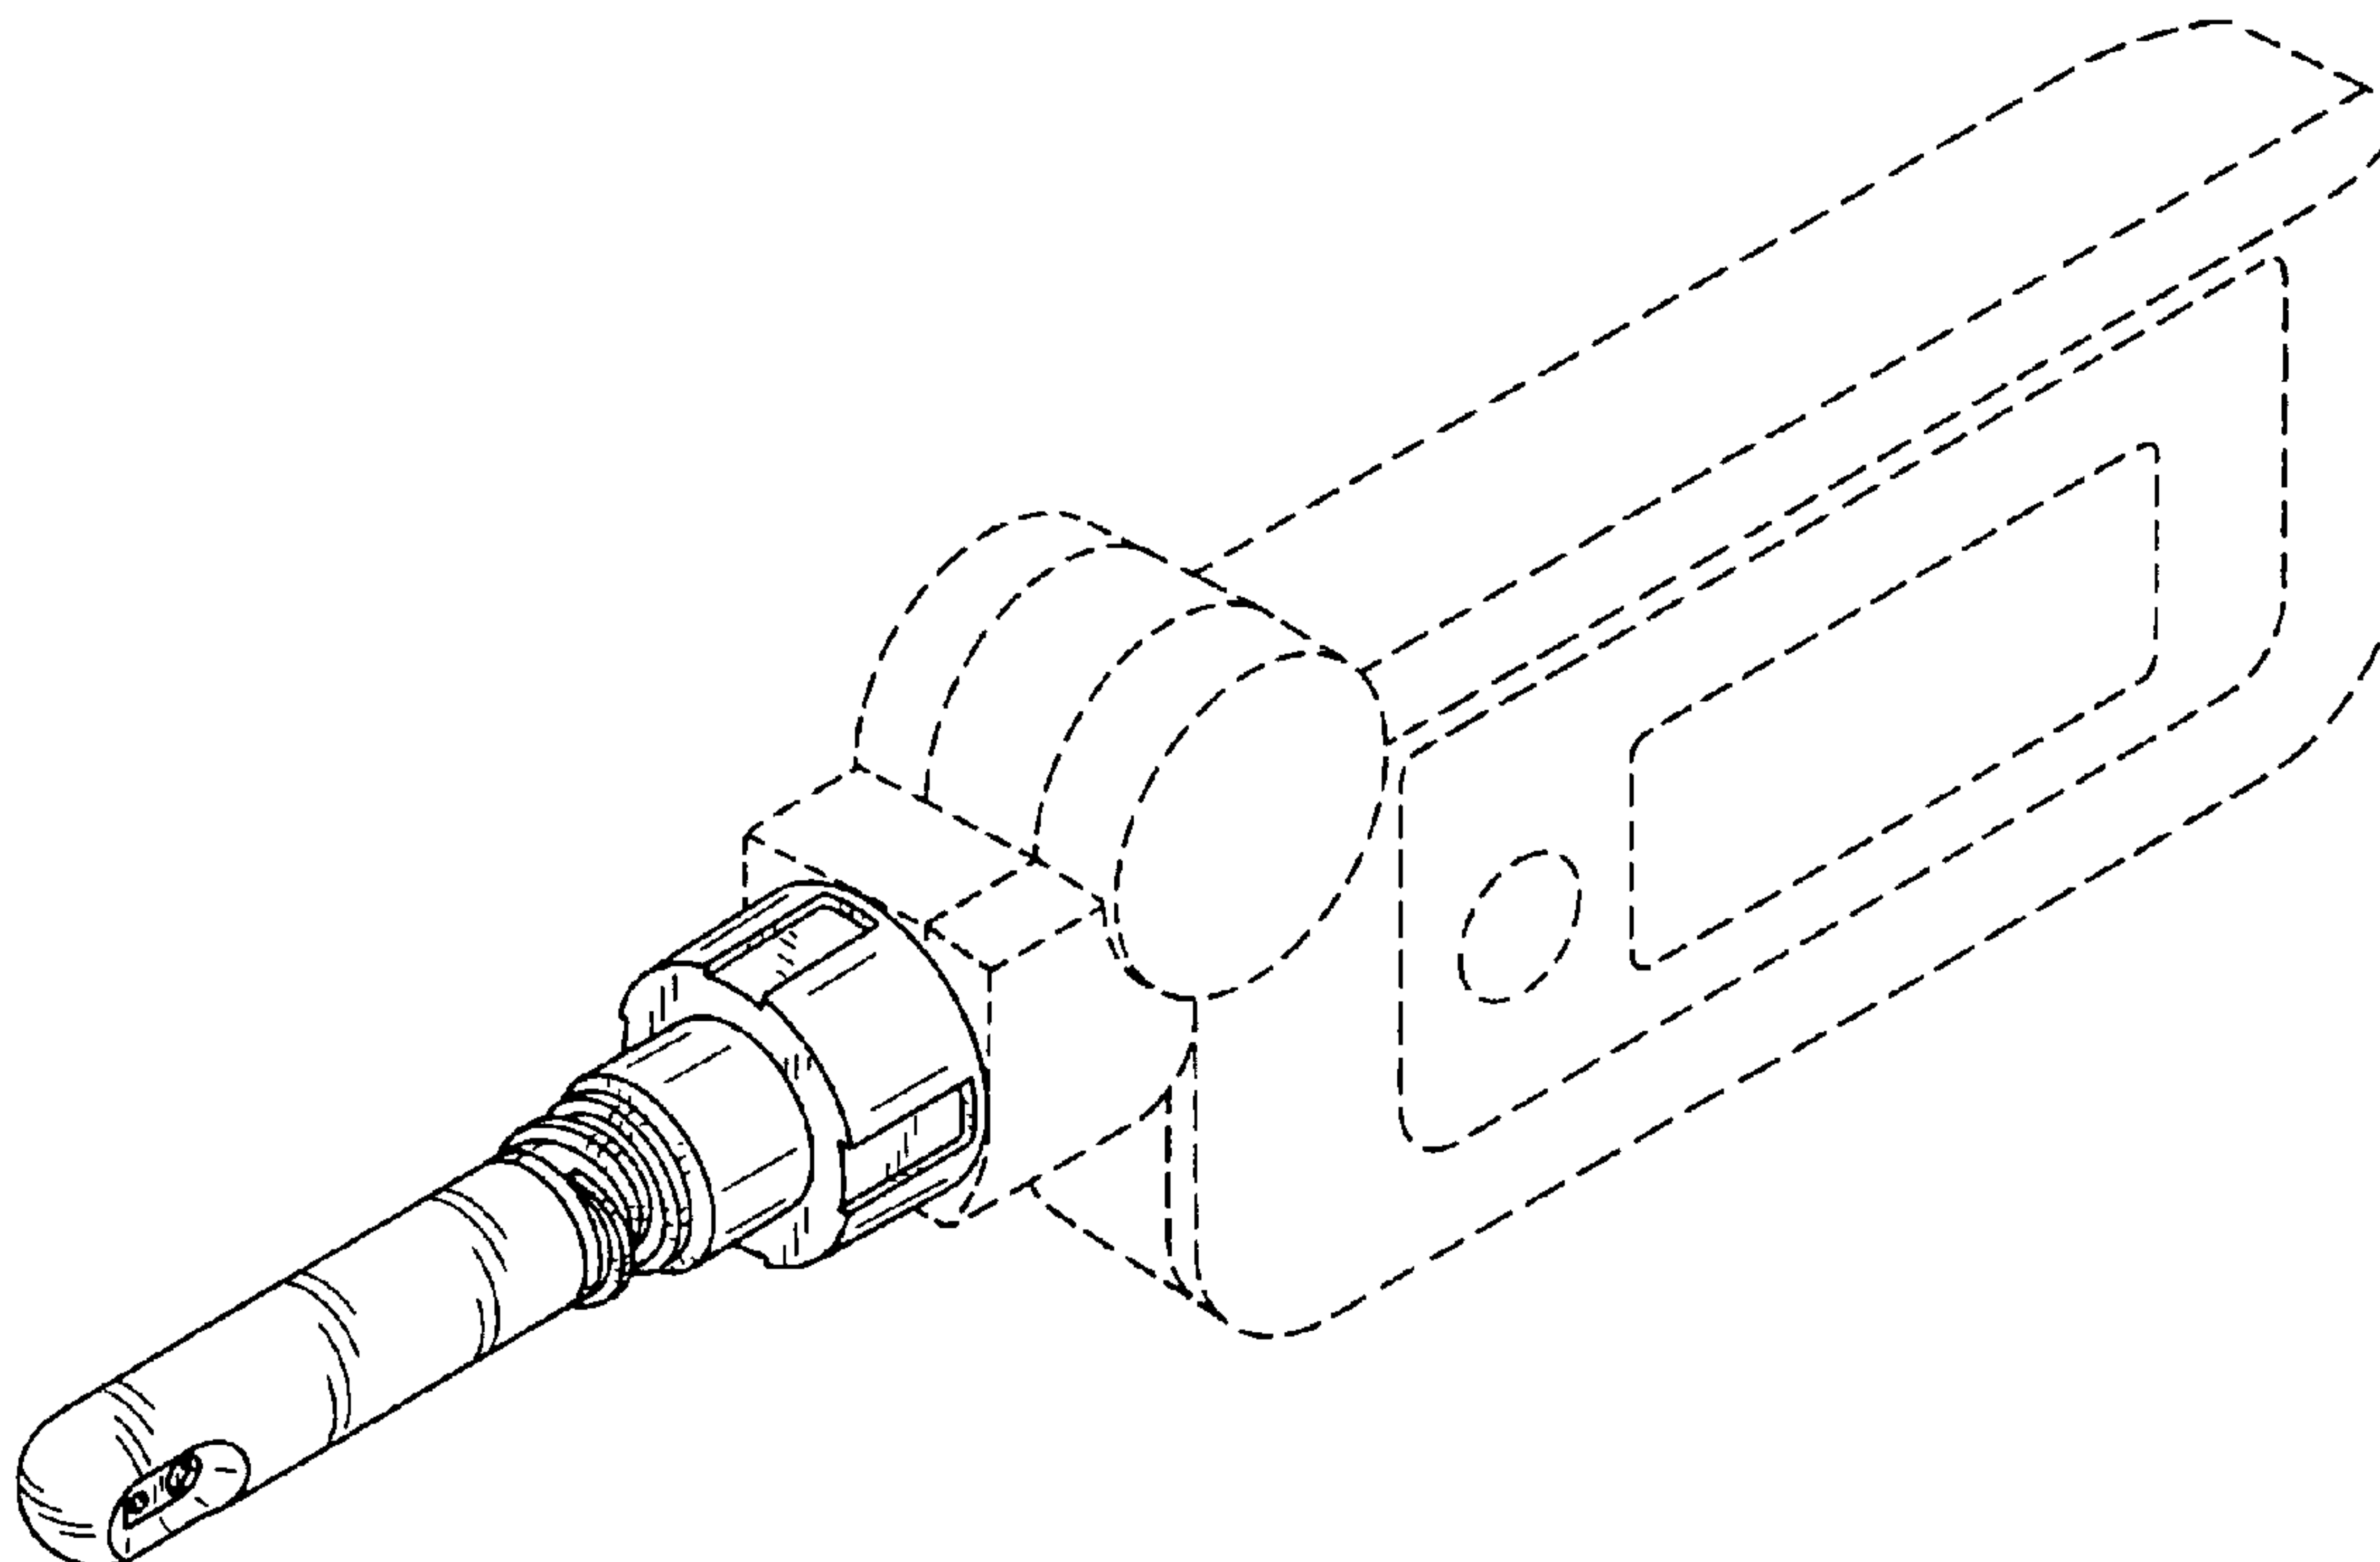

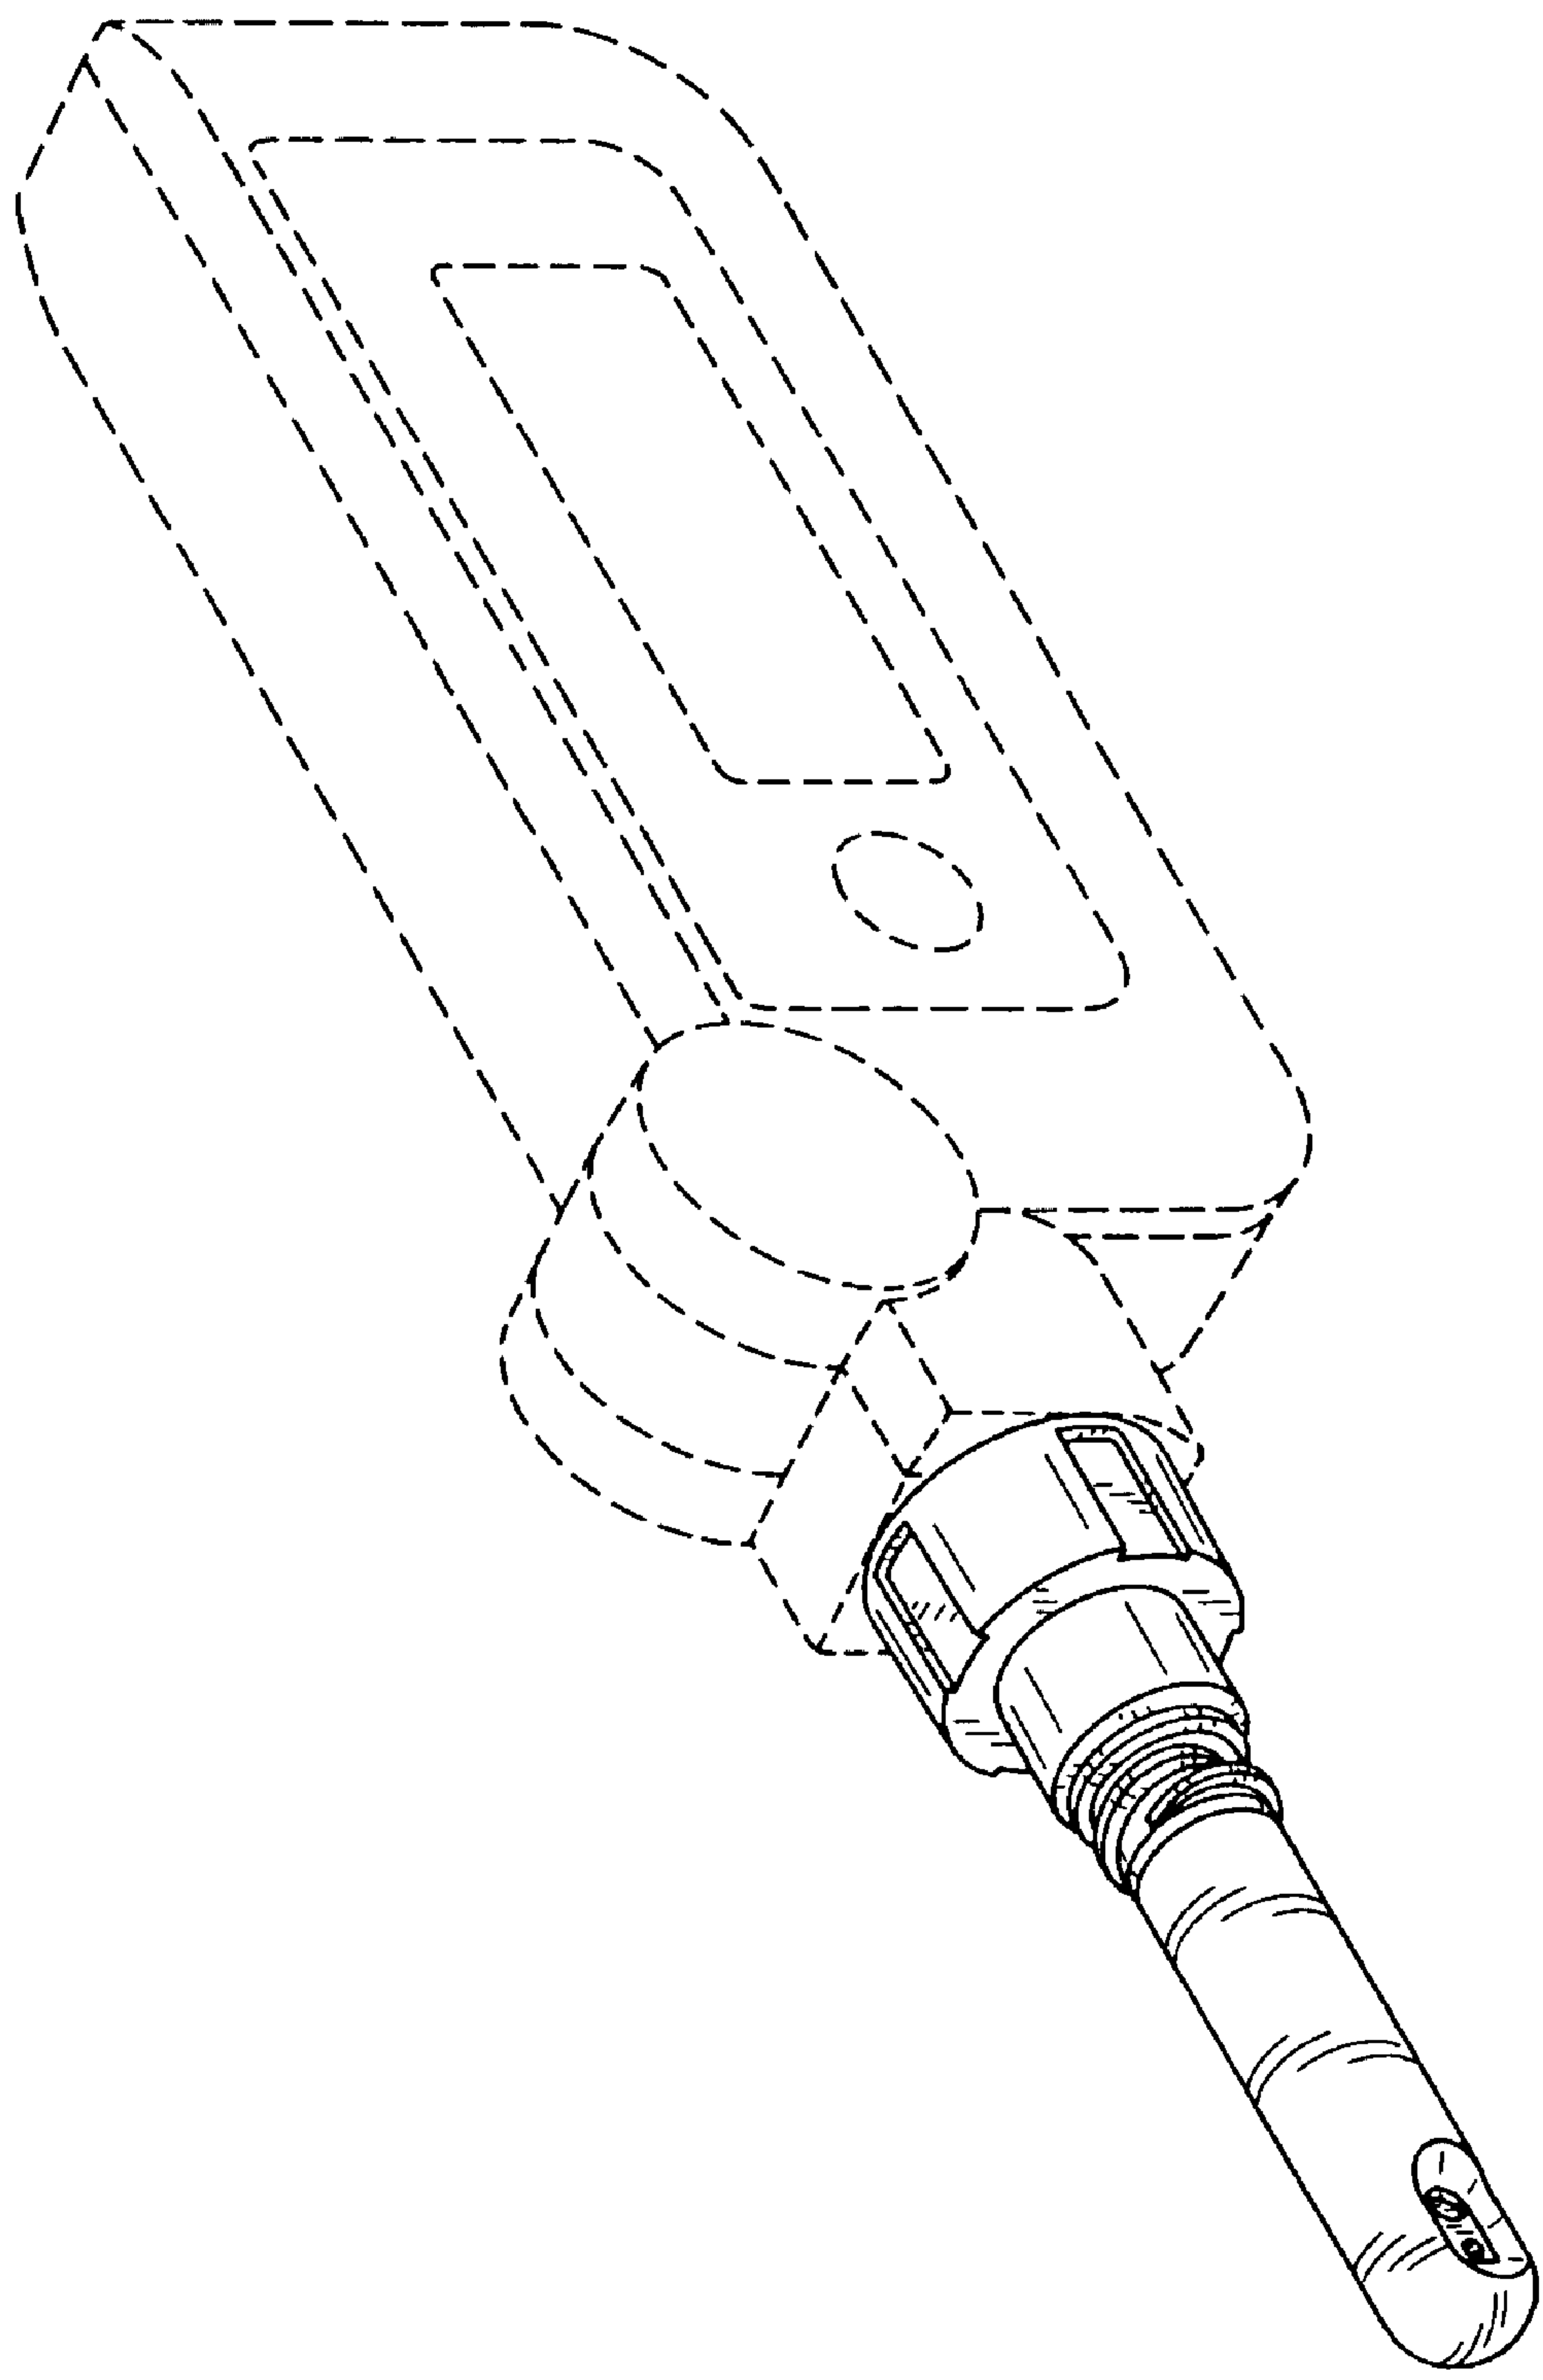


FIG. 1

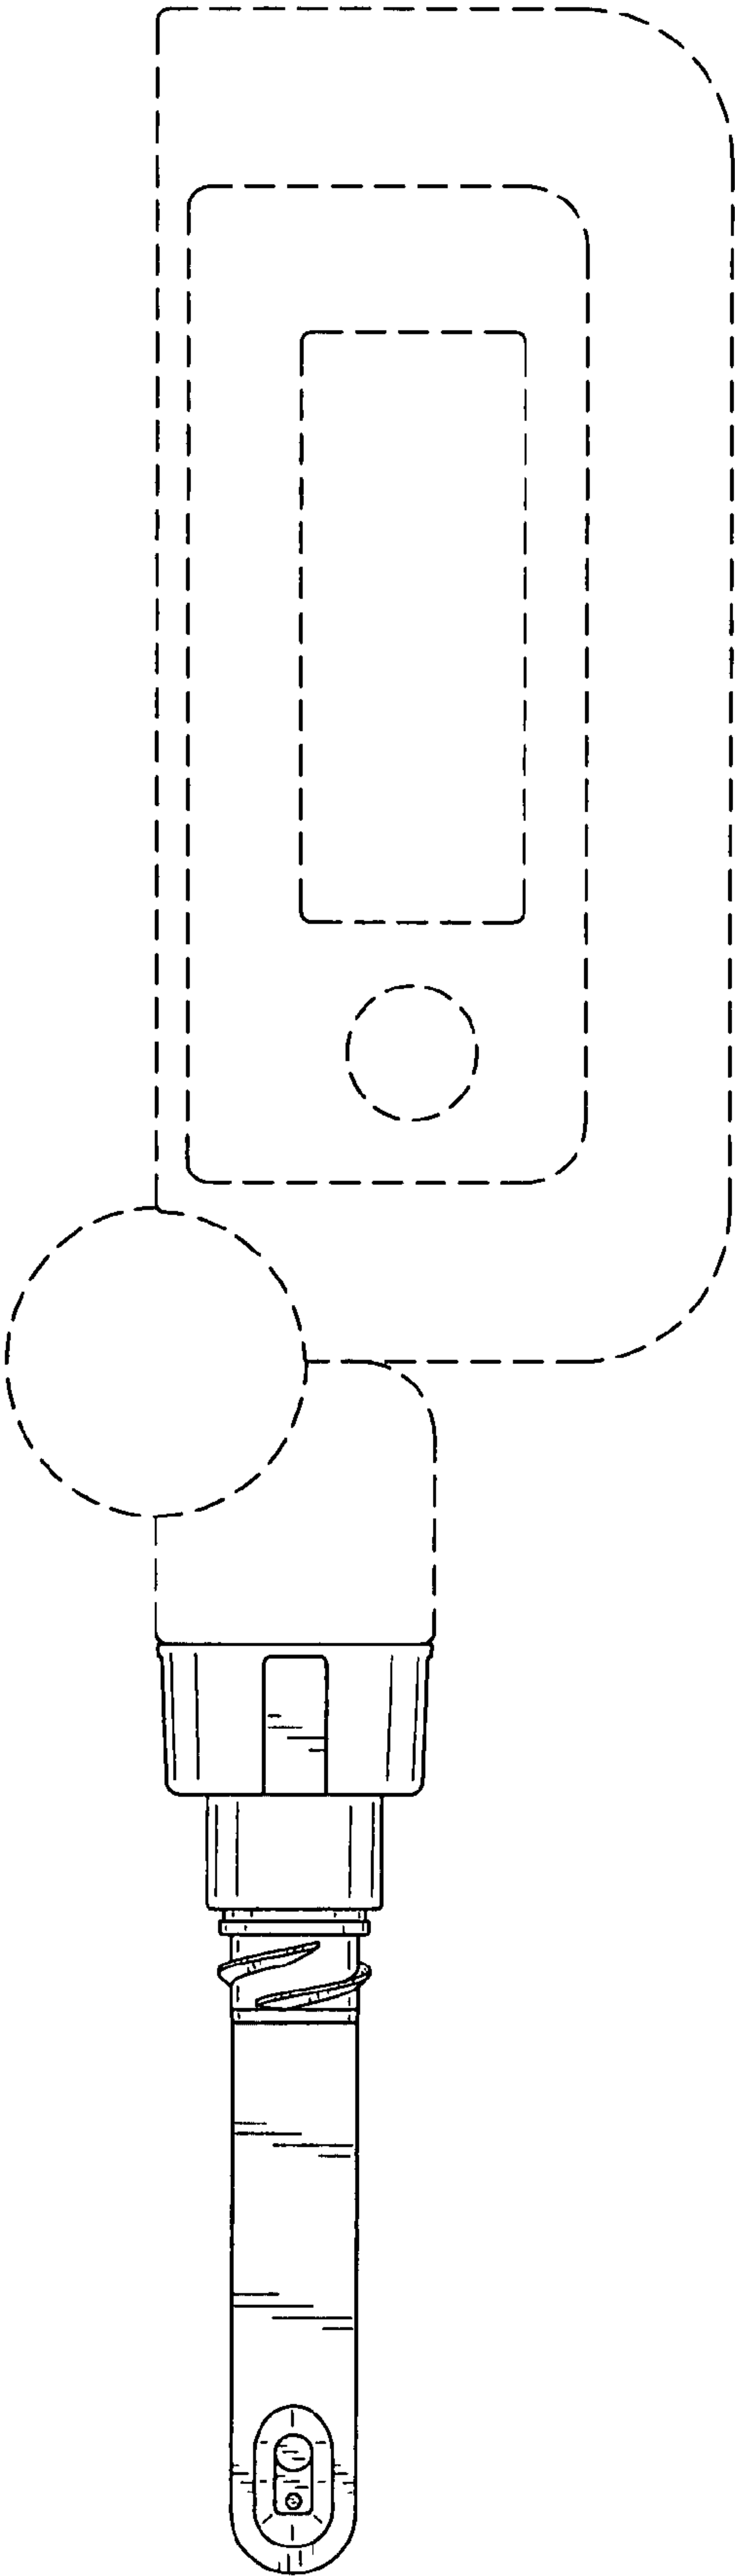


FIG. 2

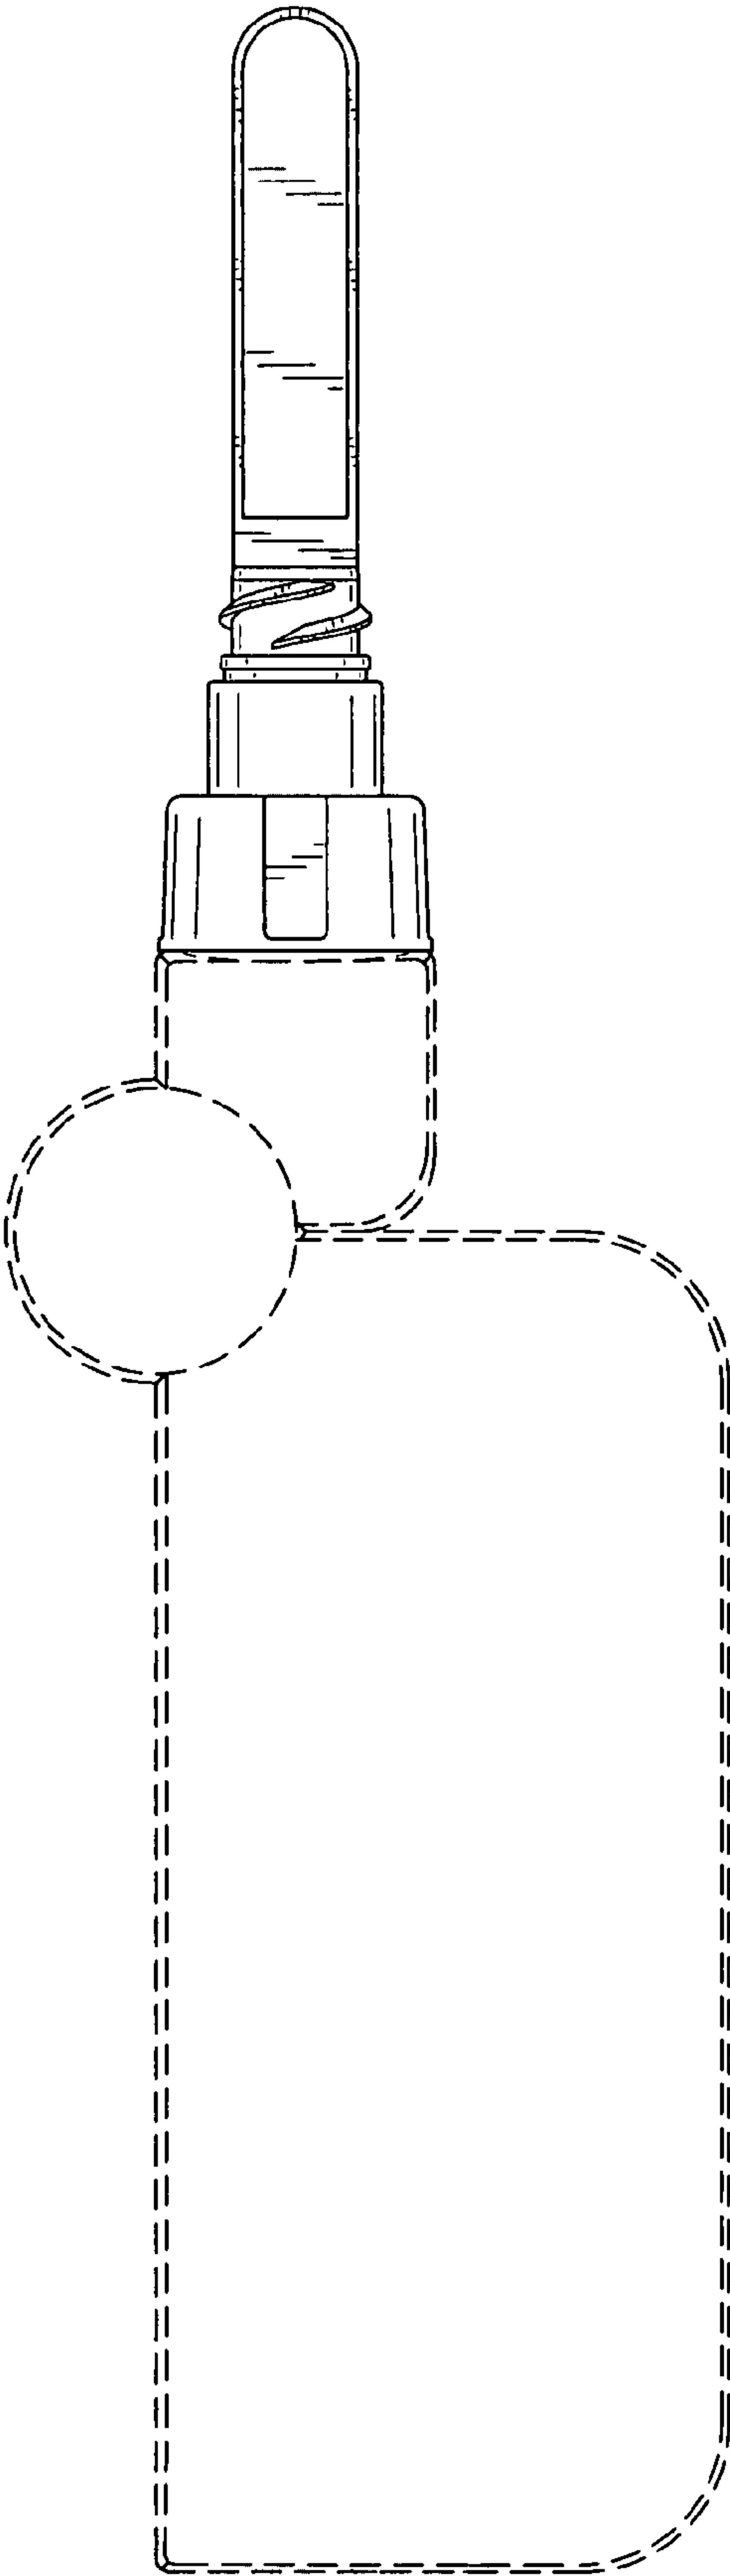


FIG. 3

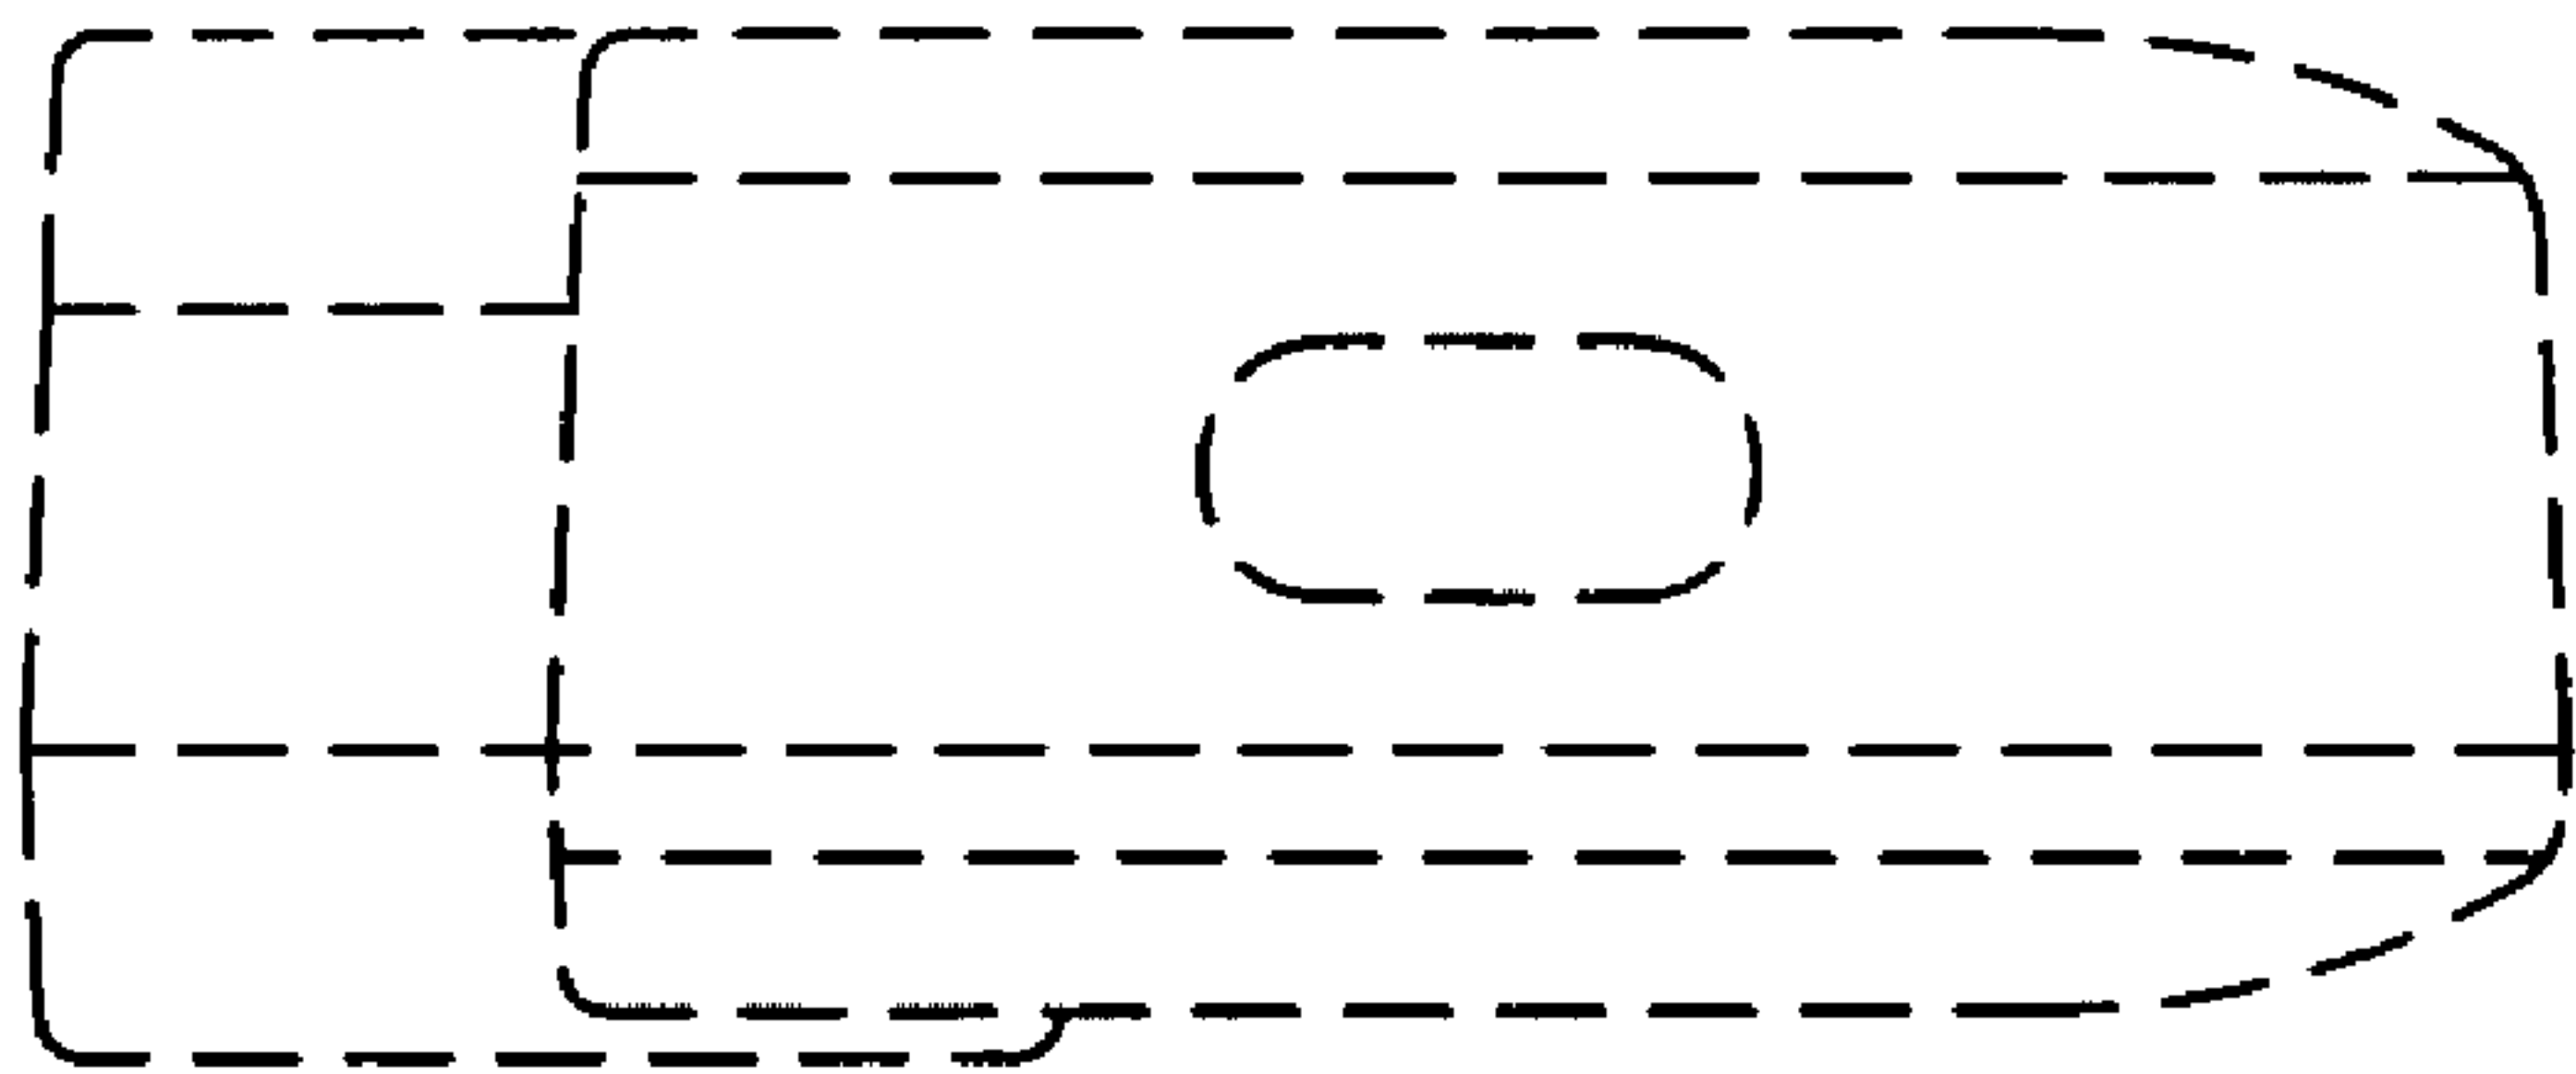


FIG. 4

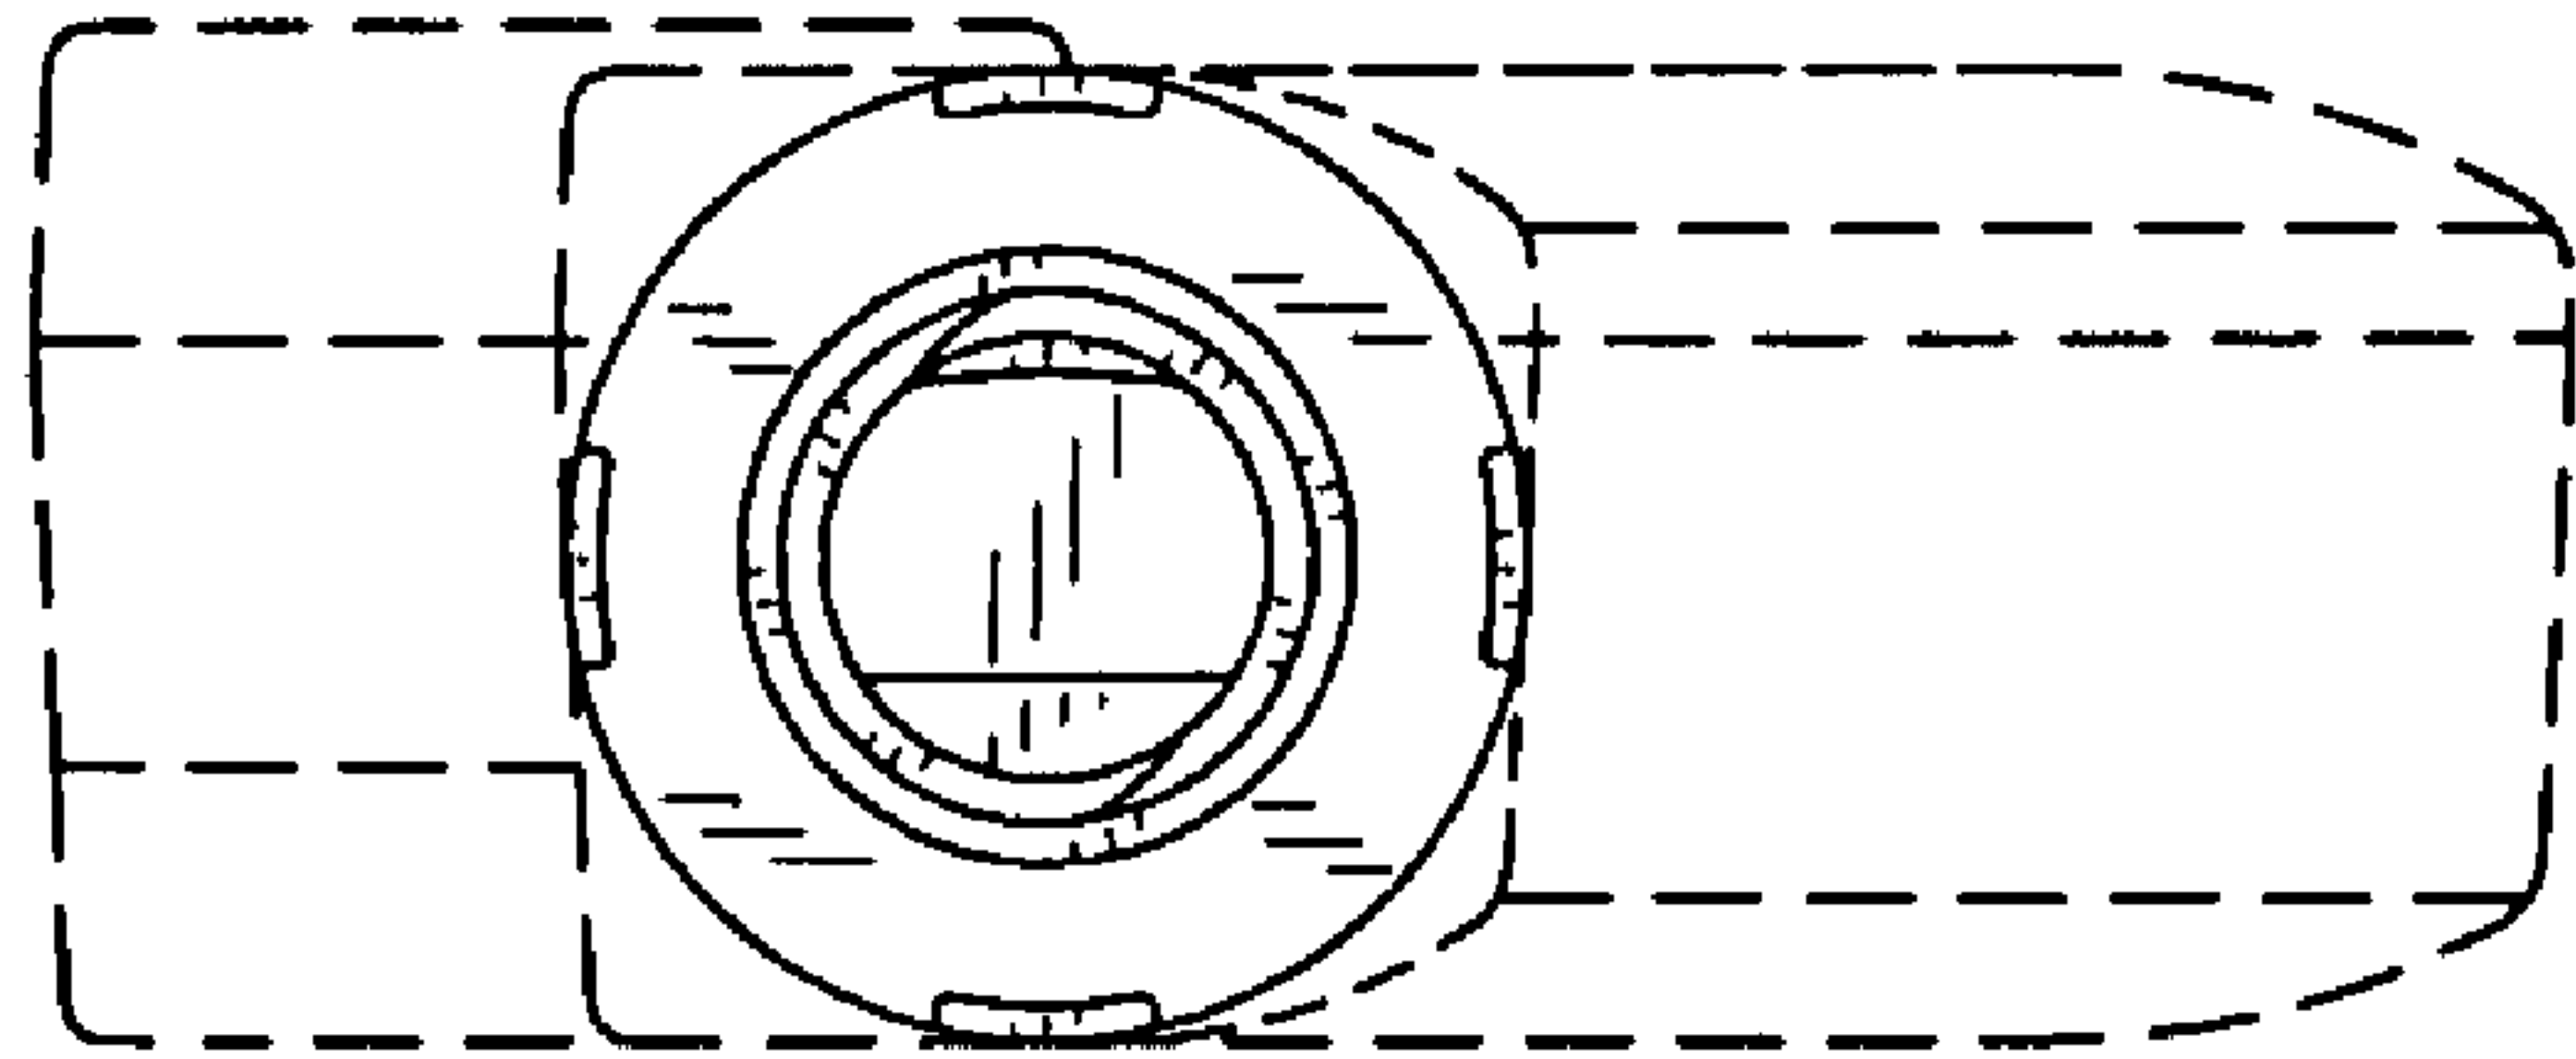


FIG. 5

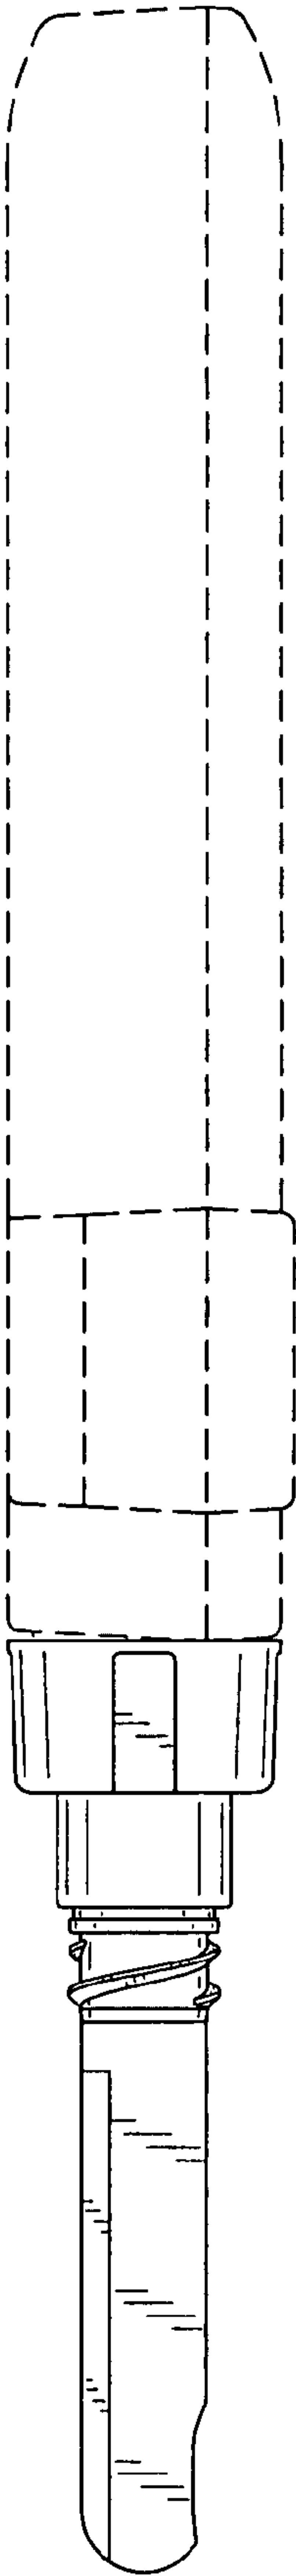


FIG. 6

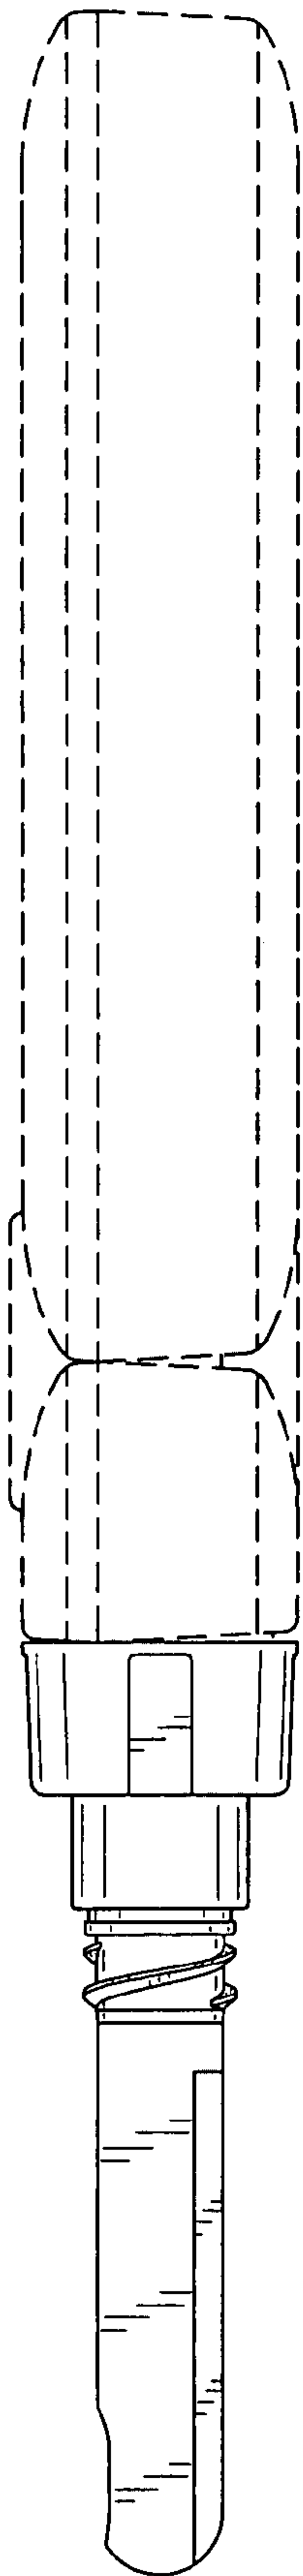


FIG. 7

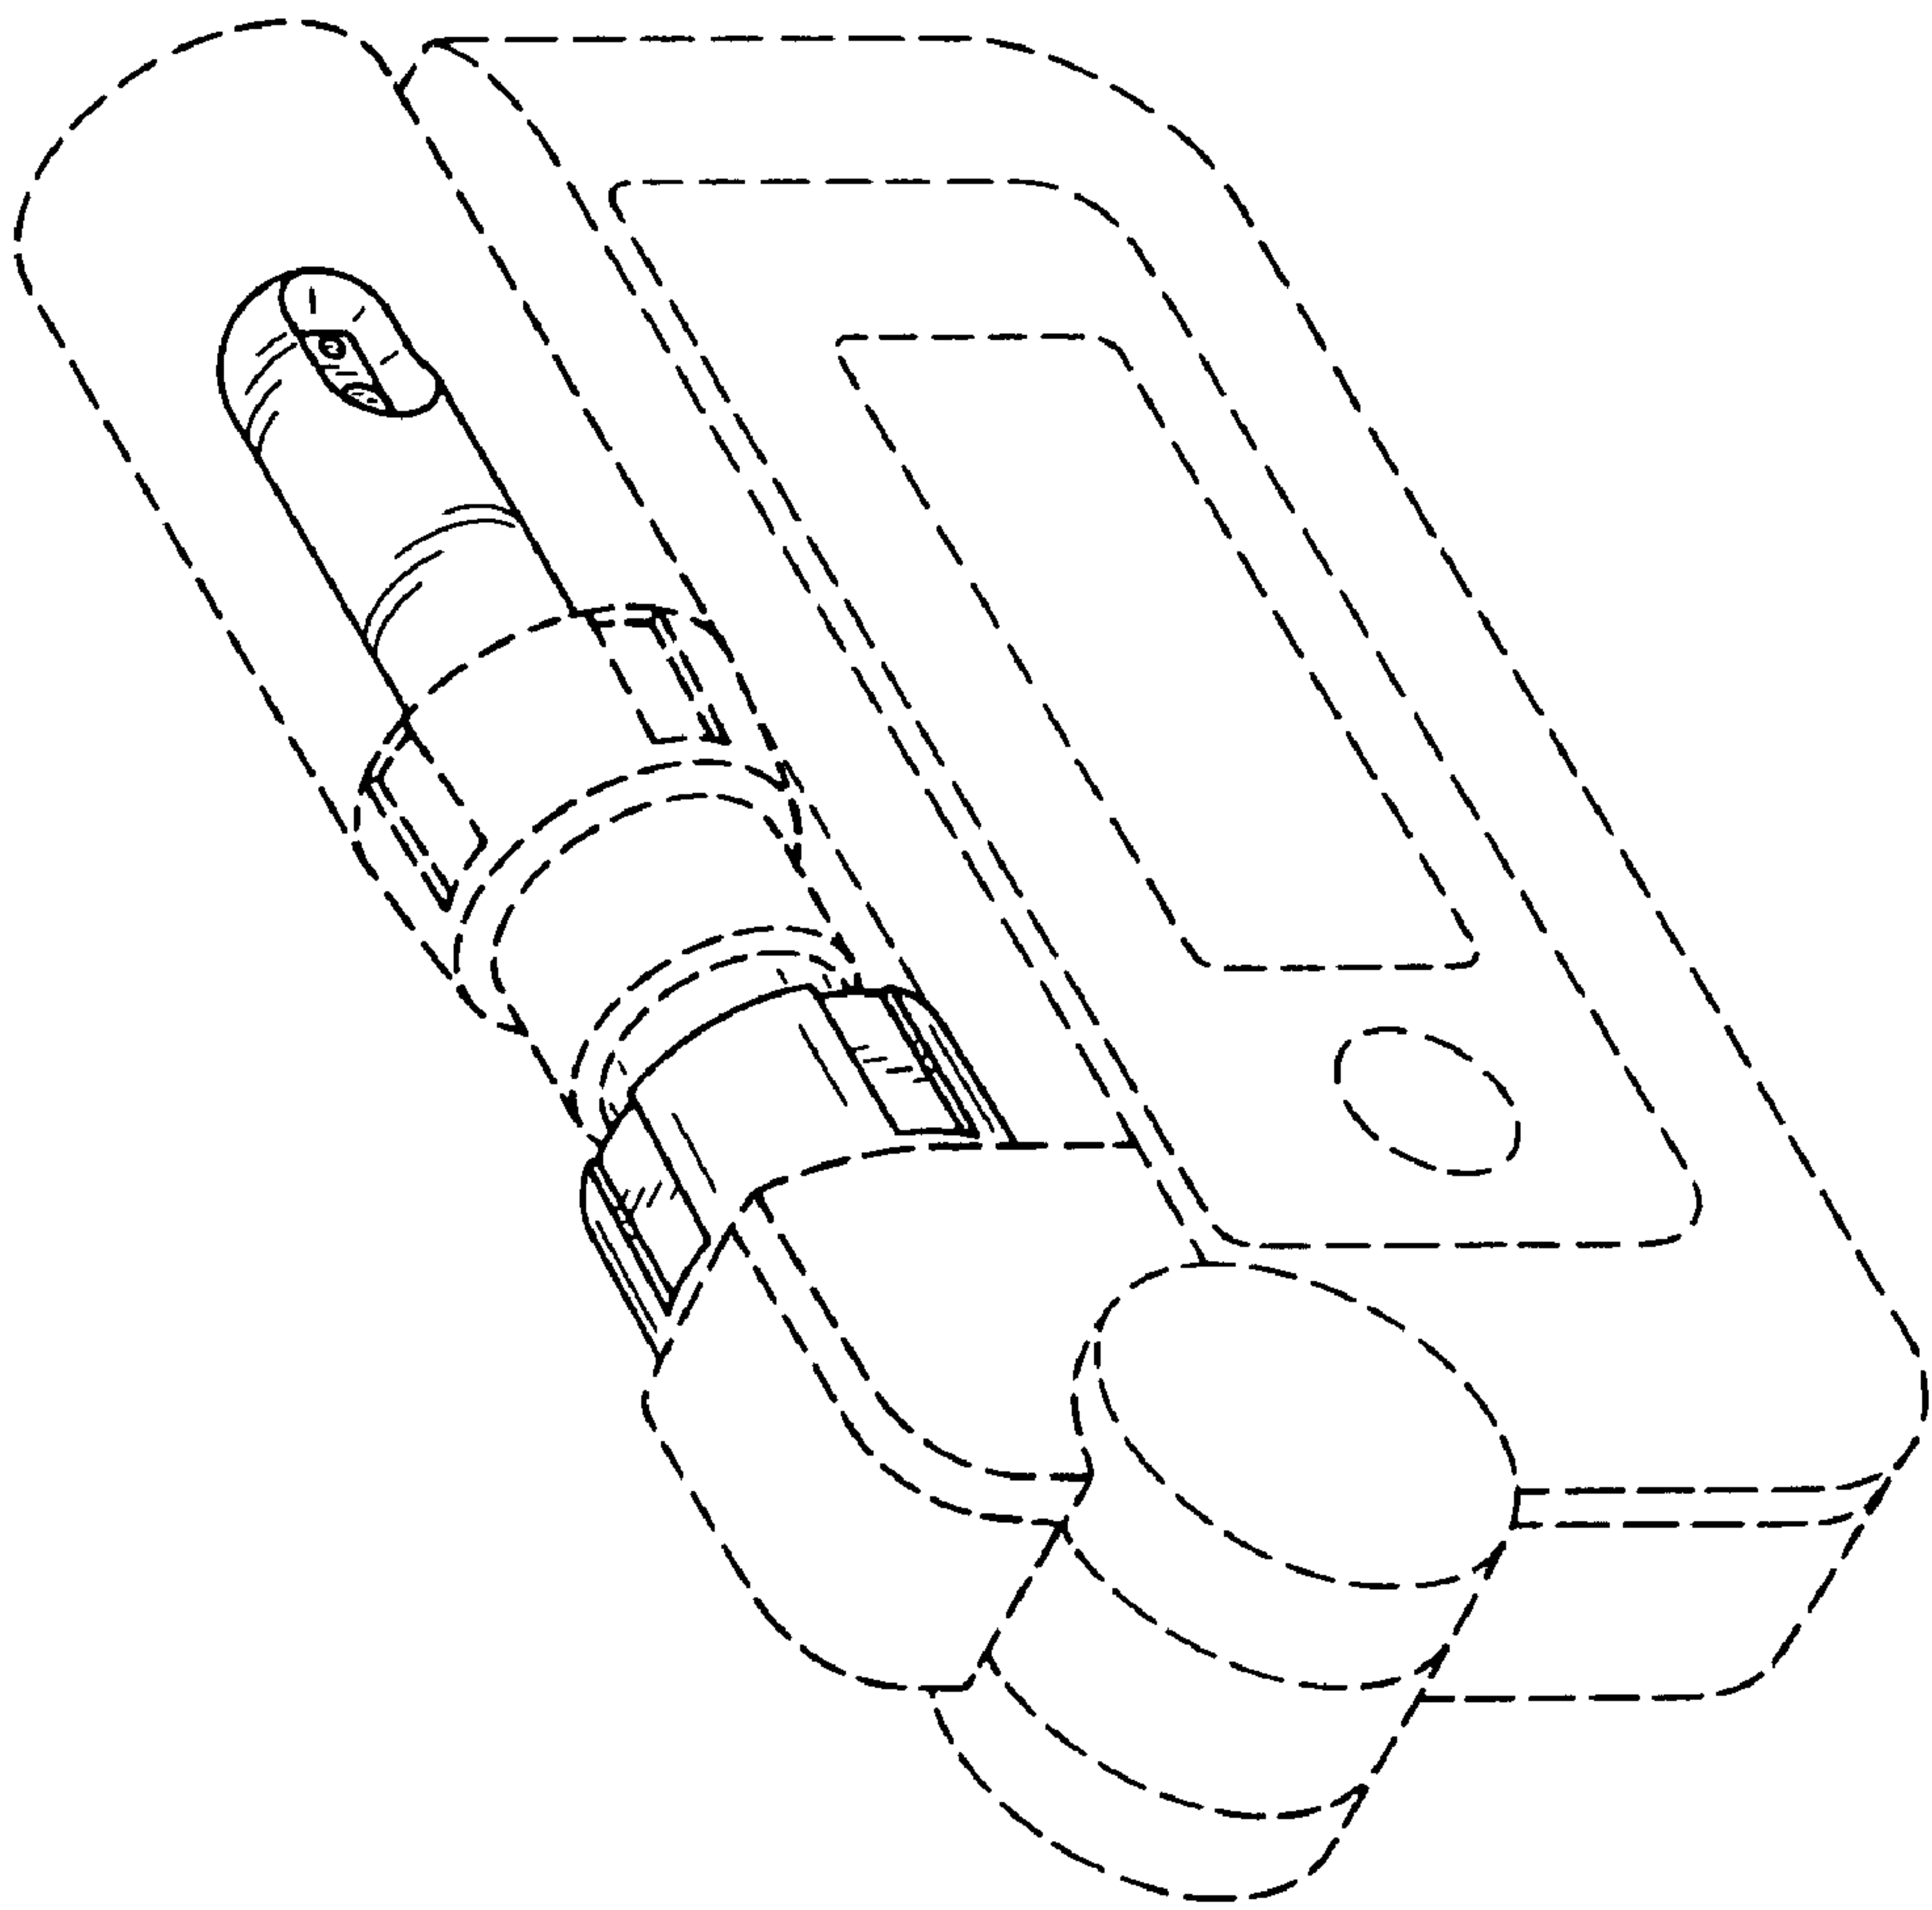


FIG. 8