



US00D594127S

(12) **United States Design Patent**
Causevic et al.

(10) **Patent No.:** **US D594,127 S**
(45) **Date of Patent:** **** Jun. 9, 2009**

(54) **ELECTRODE ARRAY**

(75) Inventors: **Elvir Causevic**, New York, NY (US);
Christian Christiansen, Norresundby
(DK); **Daniel Metzger**, Belleville, IL
(US); **Greg Holderfield**, Oak Park, IL
(US); **Elliot Hsu**, Raleigh, NC (US)

(73) Assignee: **BrainScope Company, Inc.**,
Chesterfield, MO (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/298,138**

(22) Filed: **Nov. 29, 2007**

Related U.S. Application Data

(62) Division of application No. 29/238,840, filed on Sep.
22, 2005, now Pat. No. Des. 560,809.

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/187**

(58) **Field of Classification Search** D24/168,
D24/187, 200, 215, 206-207; D2/878; 600/109,
600/139, 383, 372, 382, 386, 388, 393; 607/54,
607/59, 60, 62, 72-74, 109, 139, 121
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,849,745	A *	3/1932	Hoffman	607/139
2,426,958	A *	9/1947	Ulett, Jr. et al.	600/383
2,549,836	A	4/1951	McIntyre et al.	
D277,787	S *	2/1985	Corbett	D24/187
D326,717	S *	6/1992	Henderson et al.	D24/168
D348,520	S *	7/1994	Wolf	D24/200
D368,141	S	3/1996	Rabin et al.	
D405,538	S *	2/1999	Chih	D24/215

D417,282	S *	11/1999	Allen	D24/206
6,126,683	A *	10/2000	Momtaheni	607/109
D446,863	S *	8/2001	Carroll	D24/206
D456,908	S *	5/2002	Cunningham et al.	D24/200
D474,577	S *	5/2003	Rohde	D2/878
D501,558	S *	2/2005	Chastain et al.	D24/187
D505,206	S *	5/2005	Chastain et al.	D24/187
D560,809	S *	1/2008	Causevic et al.	D24/187
D565,735	S *	4/2008	Washbon	D24/187
D578,221	S *	10/2008	Sakurai et al.	D24/187
D578,222	S *	10/2008	Sakurai et al.	D24/187

* cited by examiner

Primary Examiner—Robert A. Delehanty

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Finnegan Henderson
Farabow Garrett & Dunner LLP

(57) **CLAIM**

The ornamental design for an electrode array, as shown and
described.

DESCRIPTION

FIG. 1 is a perspective side view of the electrode array show-
ing our new design;

FIG. 2 is a top plan view;


FIG. 3 is a bottom plan view thereof,

FIG. 4 is a front plan view thereof. The back plan view is
substantially identical, and a duplicative back plan view is
correspondingly not shown; and,

FIG. 5 is a left side plan view thereof. The right side is
substantially identical, and a duplicative right side view is
correspondingly not shown.

The broken line showing of the electrical coupling and the
head of the human subject is included for illustrative purposes
only and forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

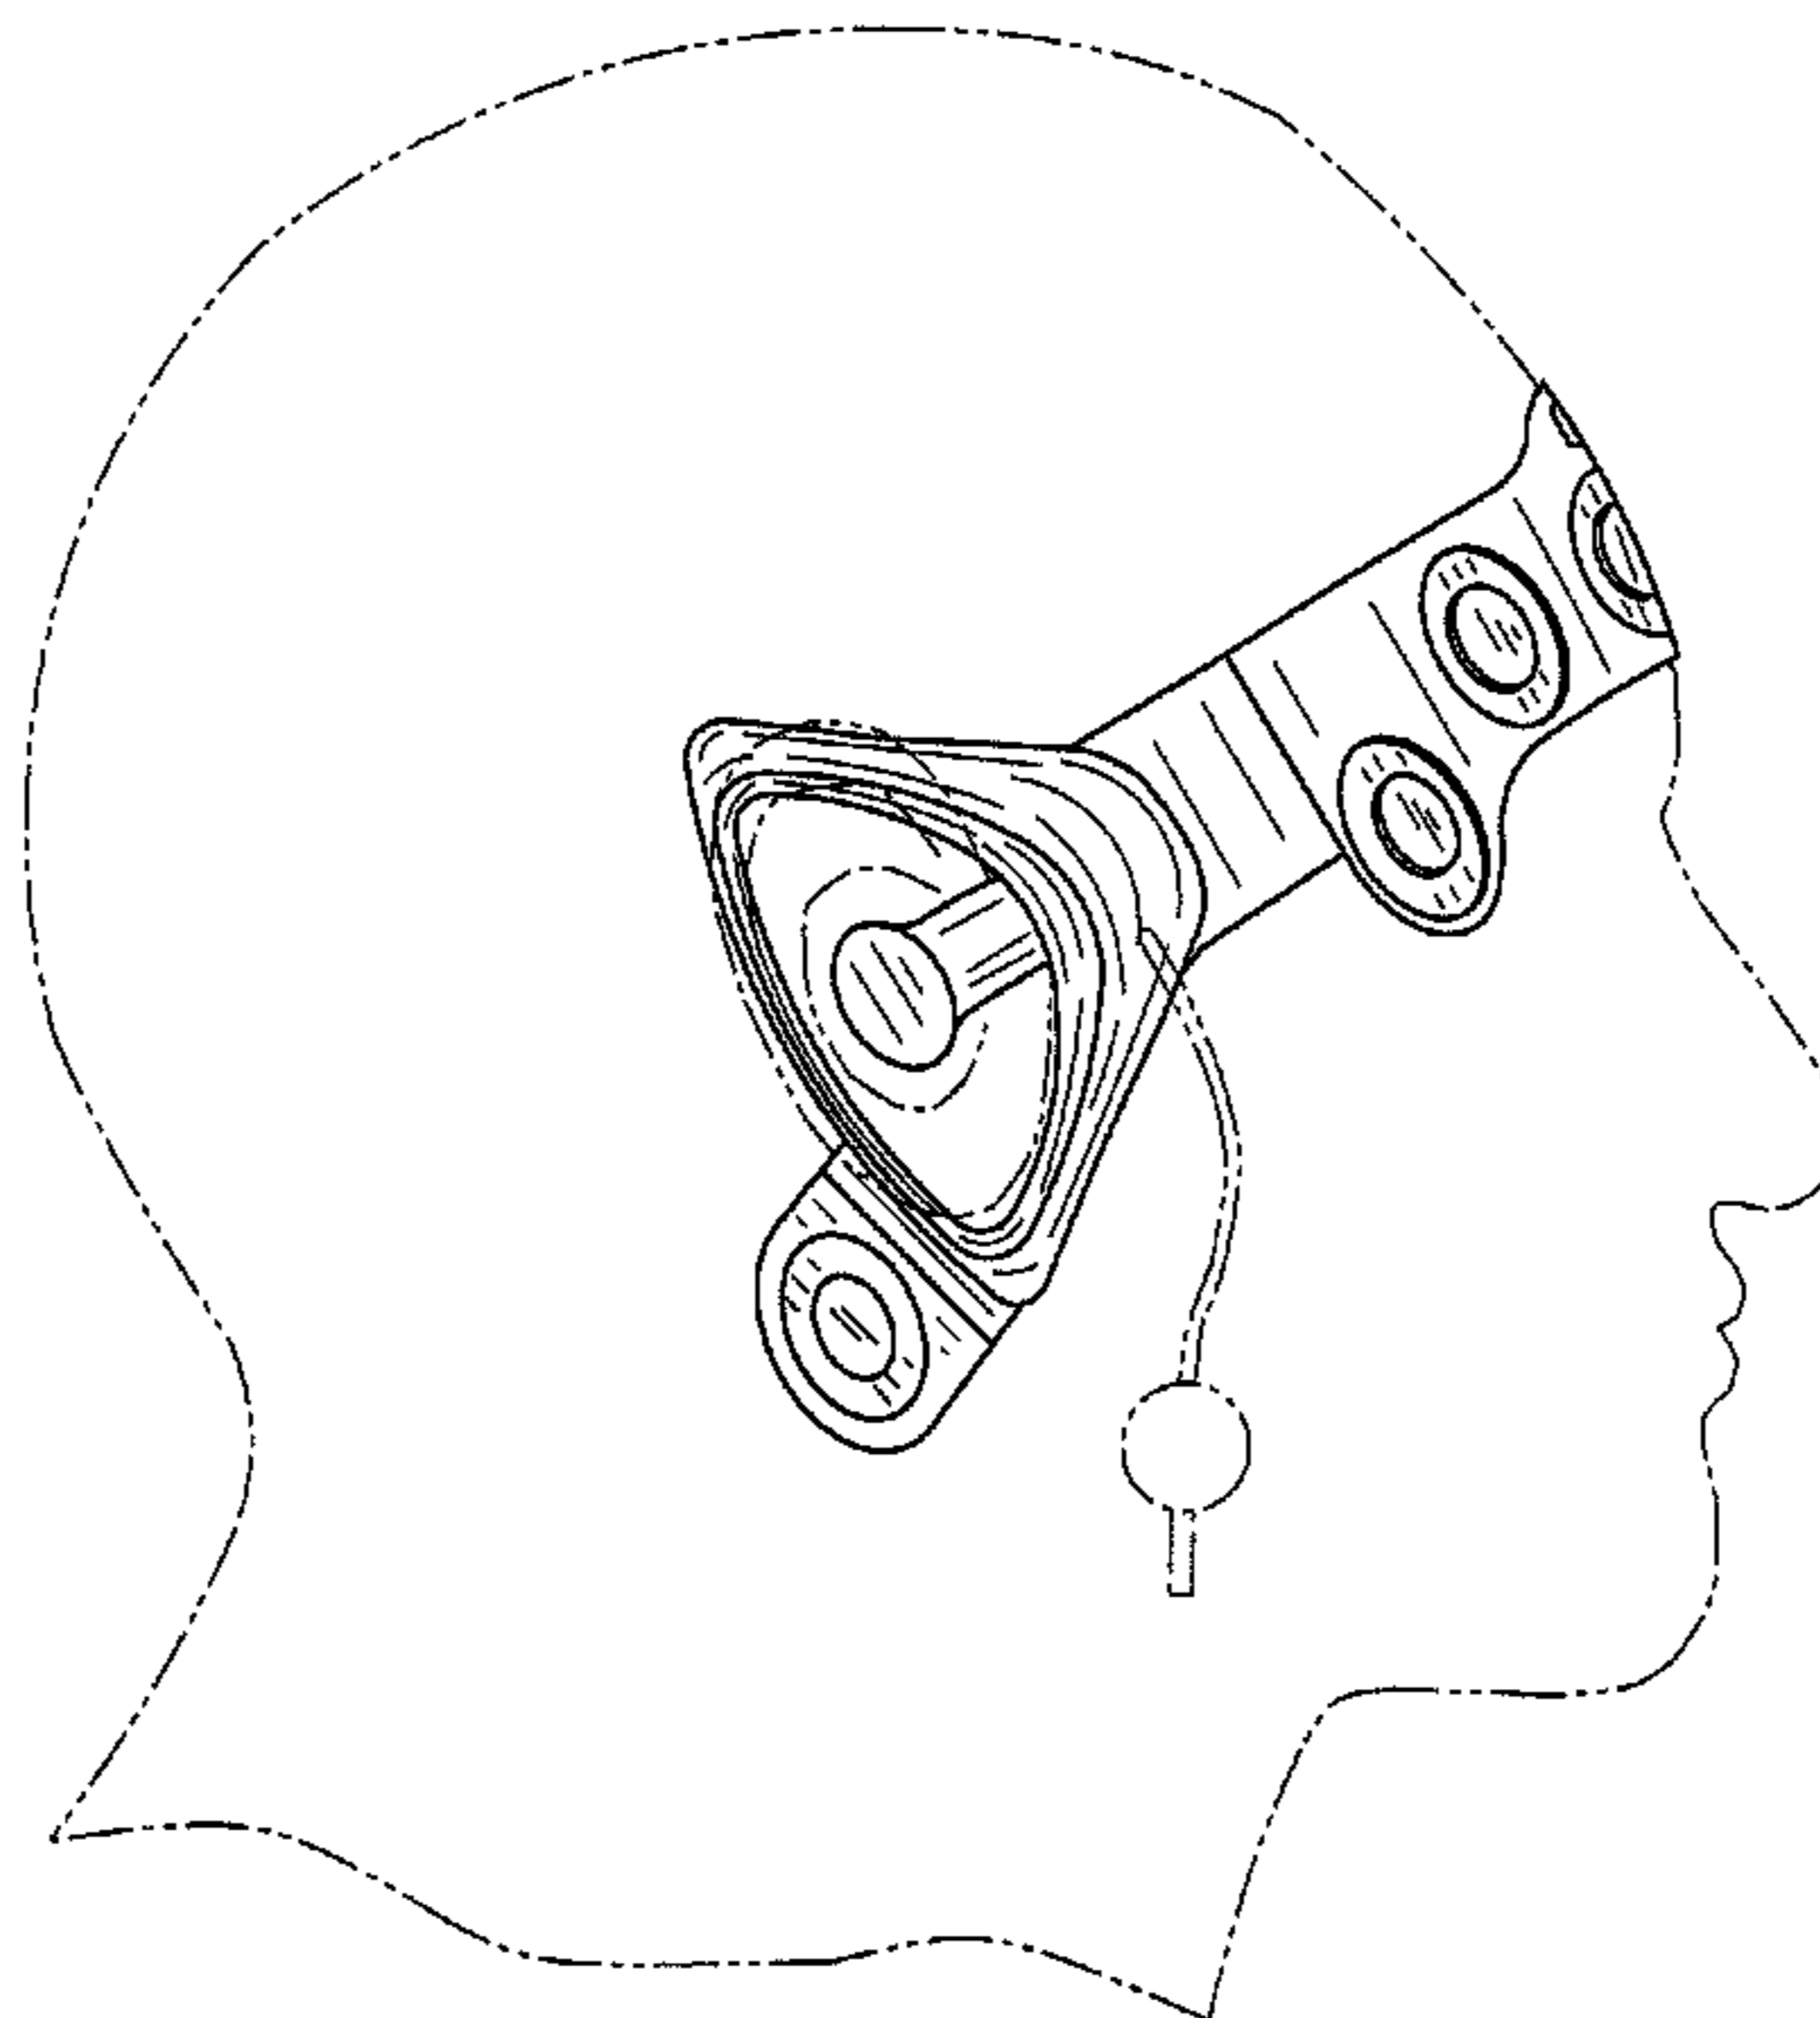

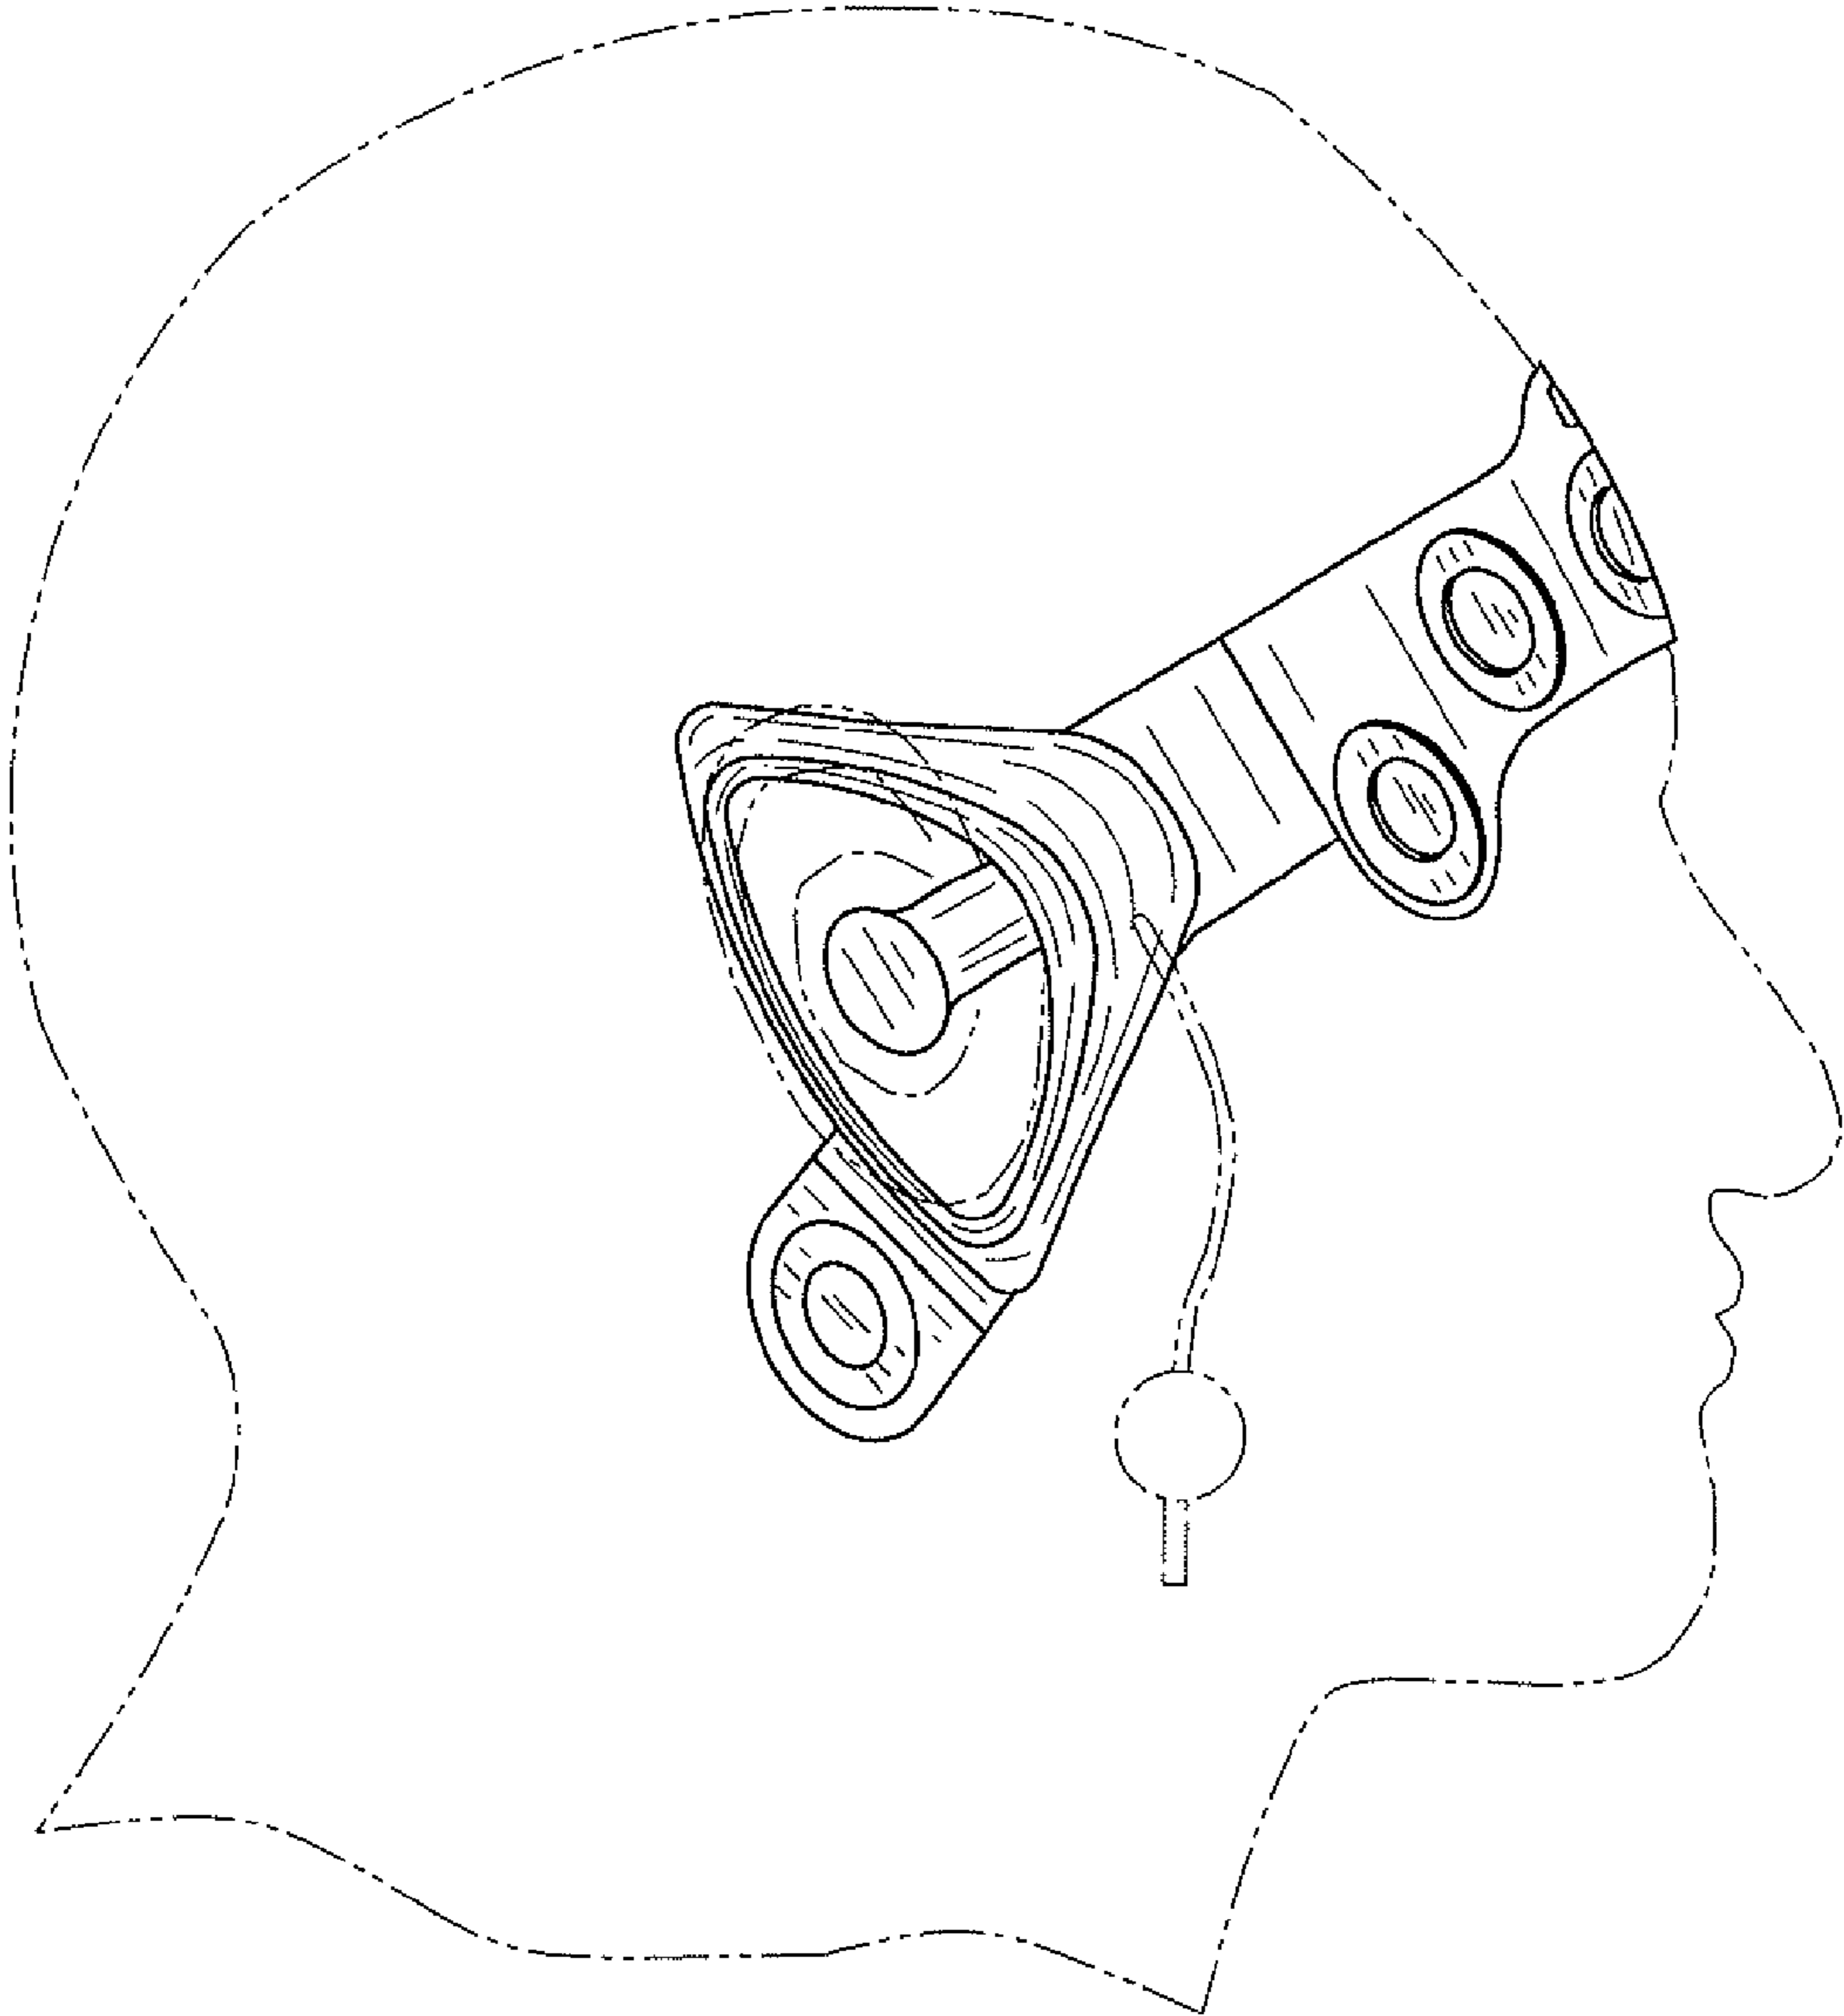


FIG. 1

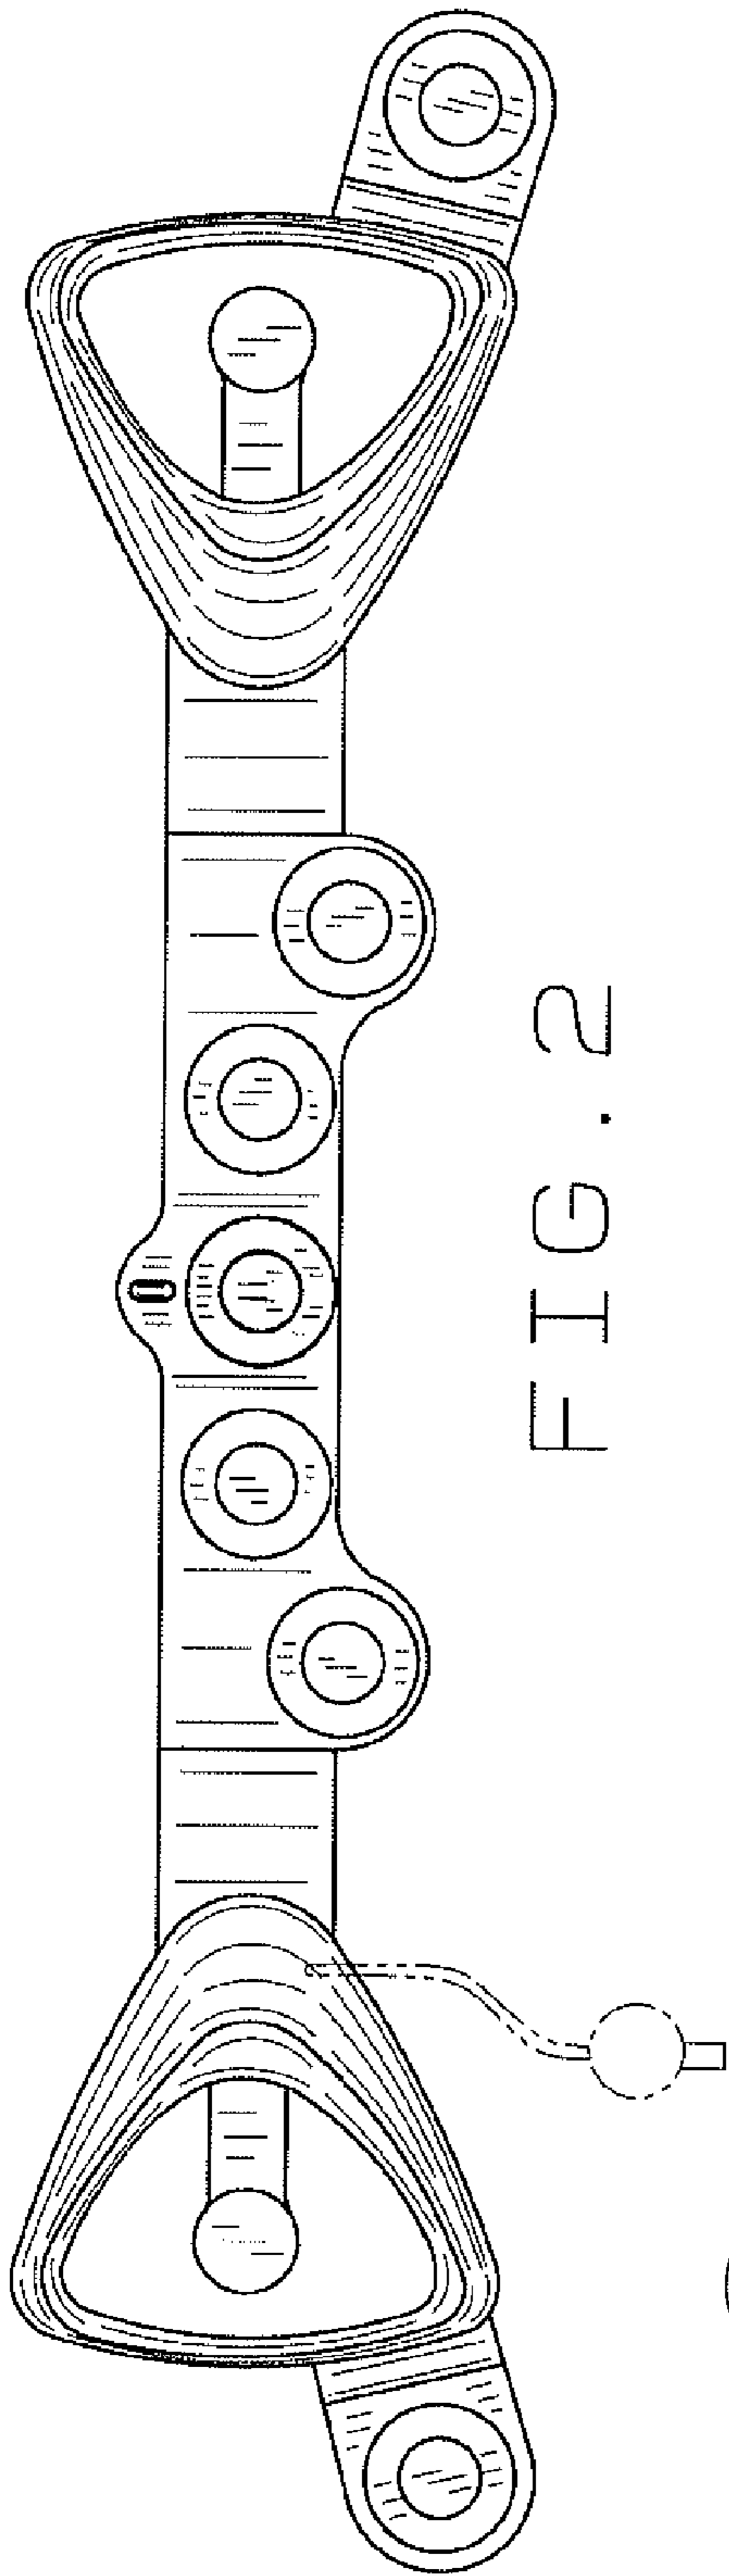


FIG. 2

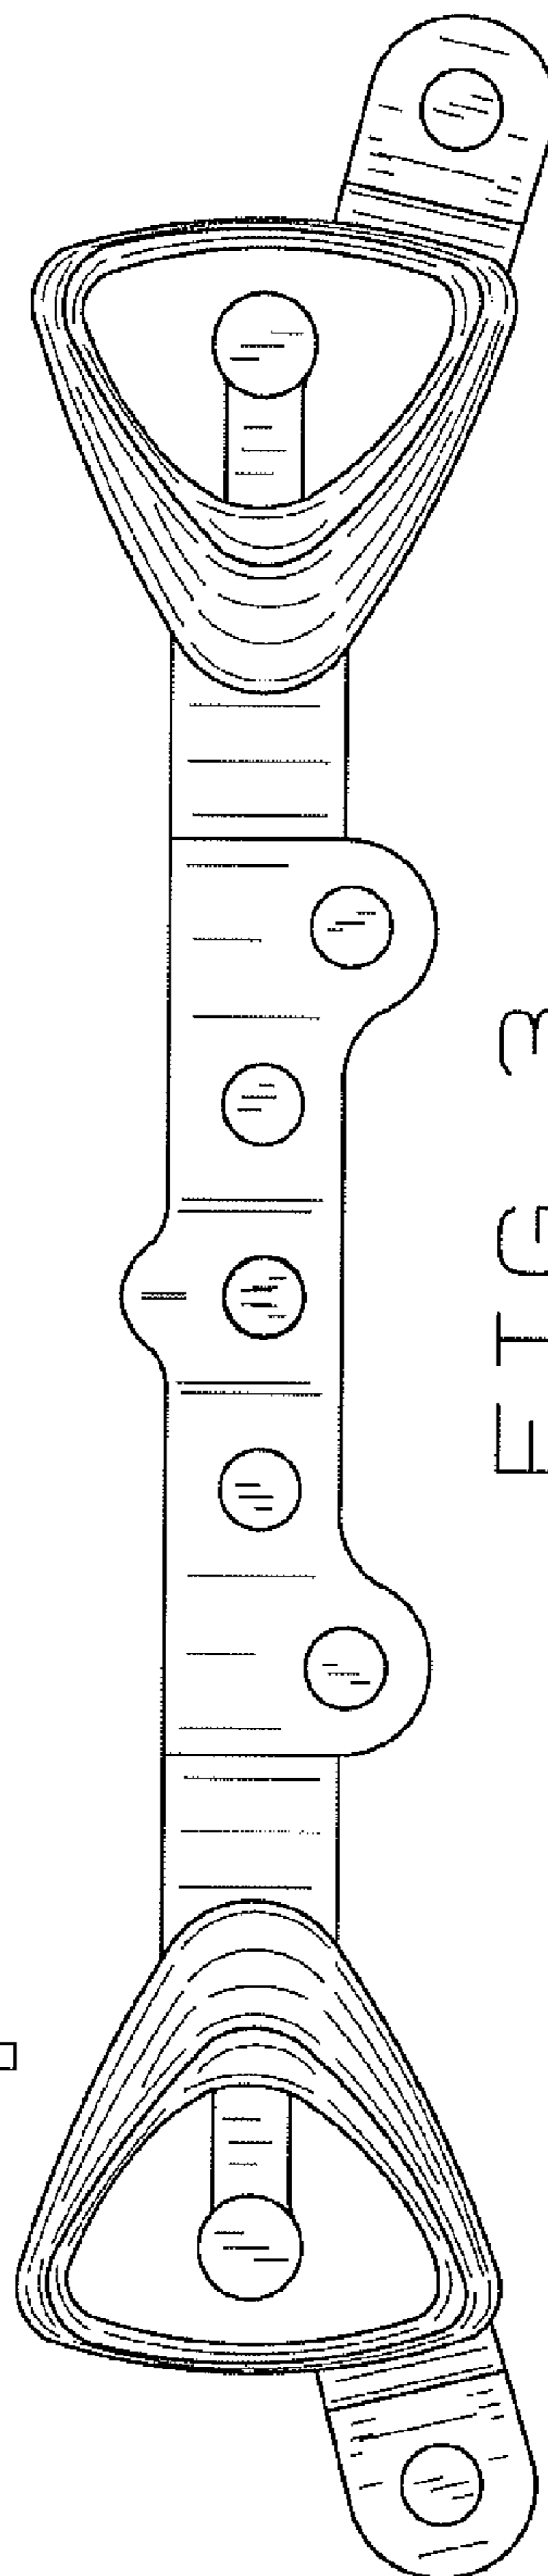


FIG. 3



FIG. 4

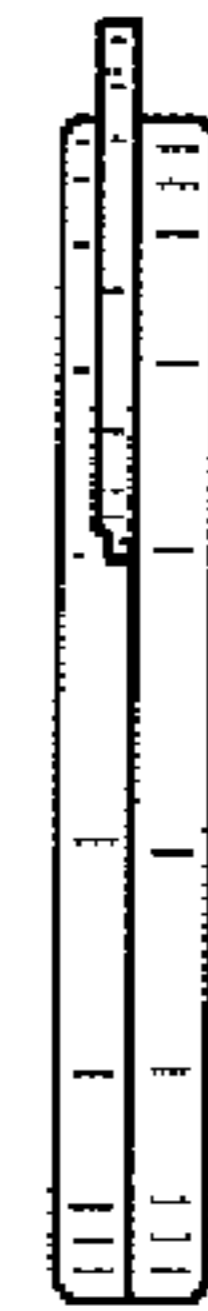


FIG. 5