



US00D596300S

(12) **United States Design Patent**
Han et al.

(10) **Patent No.:** **US D596,300 S**
(45) **Date of Patent:** **** Jul. 14, 2009**

(54) **MEDICAL ULTRASOUND TRANSDUCER**

(75) Inventors: **Jin Ha Han**, Gyeonggi-do (KR); **Dong Hyun Kim**, Gyeongbuk (KR); **Ji Whan Moon**, Busan (KR); **In Seong Song**, Daegu (KR)

(73) Assignee: **Prosonic Co., Ltd.**, Gyeongbuk (KR)

(**) Term: **14 Years**

(21) Appl. No.: **29/274,638**

(22) Filed: **May 11, 2007**

(30) **Foreign Application Priority Data**

Nov. 13, 2006 (KR) 30-2006-0045148

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/141,
D24/144, 158, 186–187, 200; D10/78; 600/407,
600/461, 459; 378/98.7, 98.8, 189
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D369,307 S * 4/1996 Imling et al. D10/78
- D387,867 S * 12/1997 Henderson et al. D24/187
- D389,918 S * 1/1998 Ninomiya et al. D24/186
- D389,919 S * 1/1998 Ninomiya et al. D24/186
- D390,959 S * 2/1998 Mesaros et al. D24/186
- D392,044 S * 3/1998 Mesaros et al. D24/186
- 5,897,503 A * 4/1999 Lyon et al. 600/459
- D462,446 S * 9/2002 Felix et al. D24/187

- D544,606 S * 6/2007 Hasegawa et al. D24/186
- D545,433 S * 6/2007 Messerly et al. D24/158
- D546,460 S * 7/2007 Hasegawa D24/186
- D550,365 S * 9/2007 Kitayama D24/186
- D555,252 S * 11/2007 Kitayama et al. D24/186

* cited by examiner

Primary Examiner—Robert A. Delehanty

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Venable LLP; Michael A. Sartori; Kyle D. Petaja

(57) **CLAIM**

The ornamental design for a medical ultrasound transducer, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the medical ultrasound transducer;

FIG. 2 is a front view of the medical ultrasound transducer;

FIG. 3 is a left side view of the medical ultrasound transducer;

FIG. 4 is a right side view of the medical ultrasound transducer;

FIG. 5 is a top view of the medical ultrasound transducer;

FIG. 6 is a bottom view of the medical ultrasound transducer; and,

FIG. 7 is a back view of the medical ultrasound transducer.

The broken line in the interior of the circular element in FIG. 6 is included for the purpose of illustrating environment and forms no part of the claimed design.

1 Claim, 6 Drawing Sheets

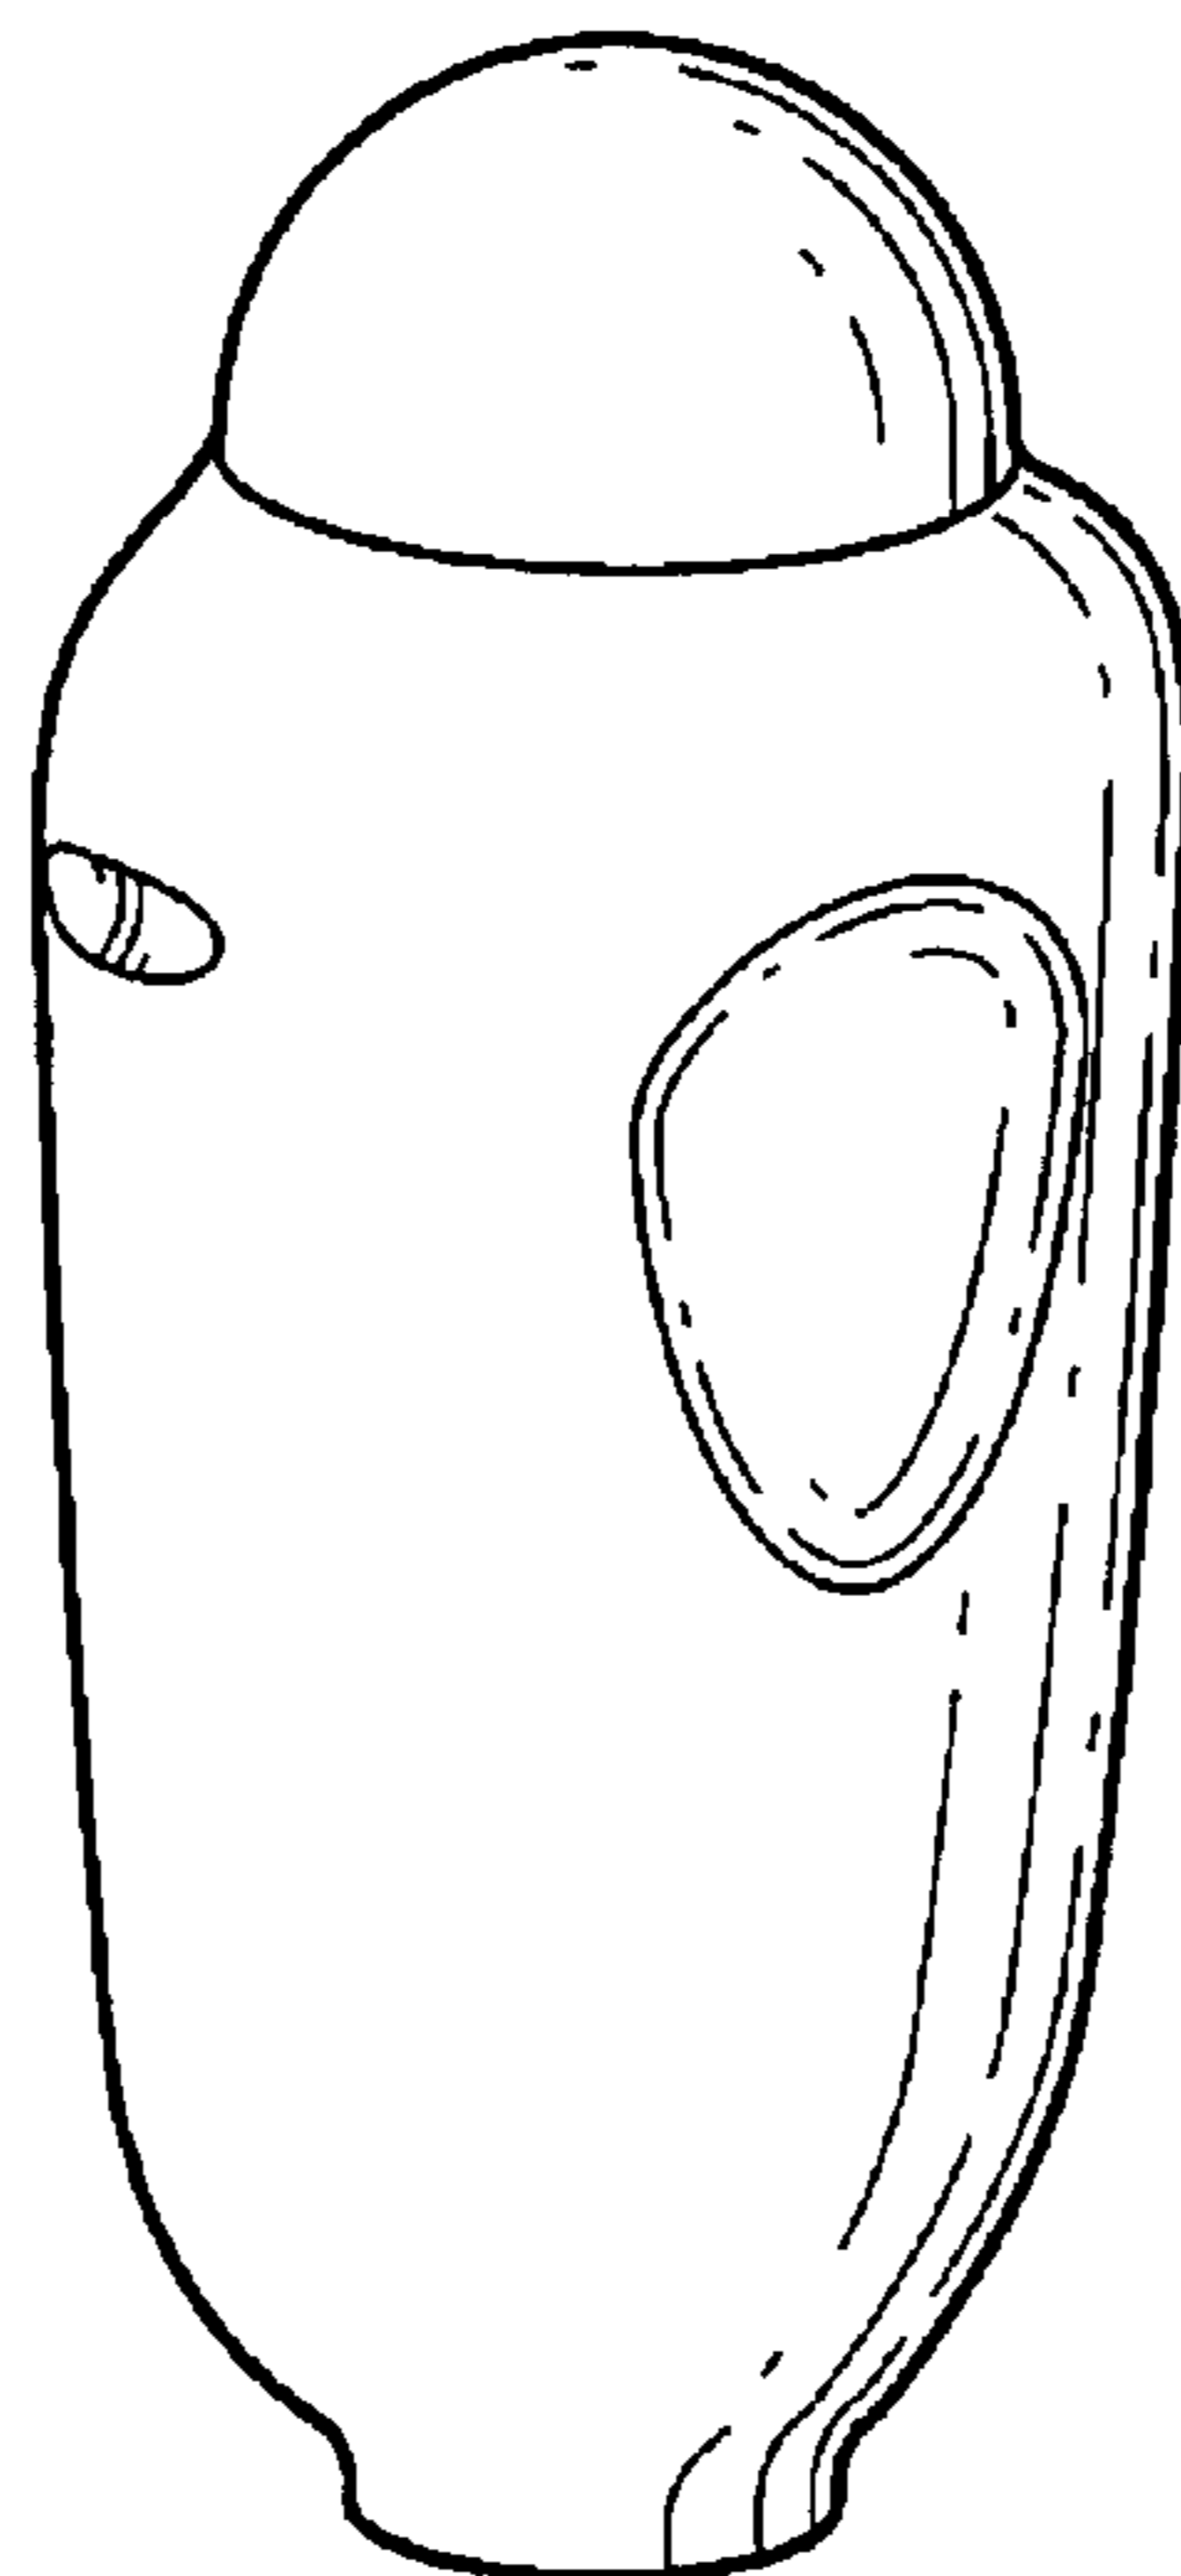


FIG. 1

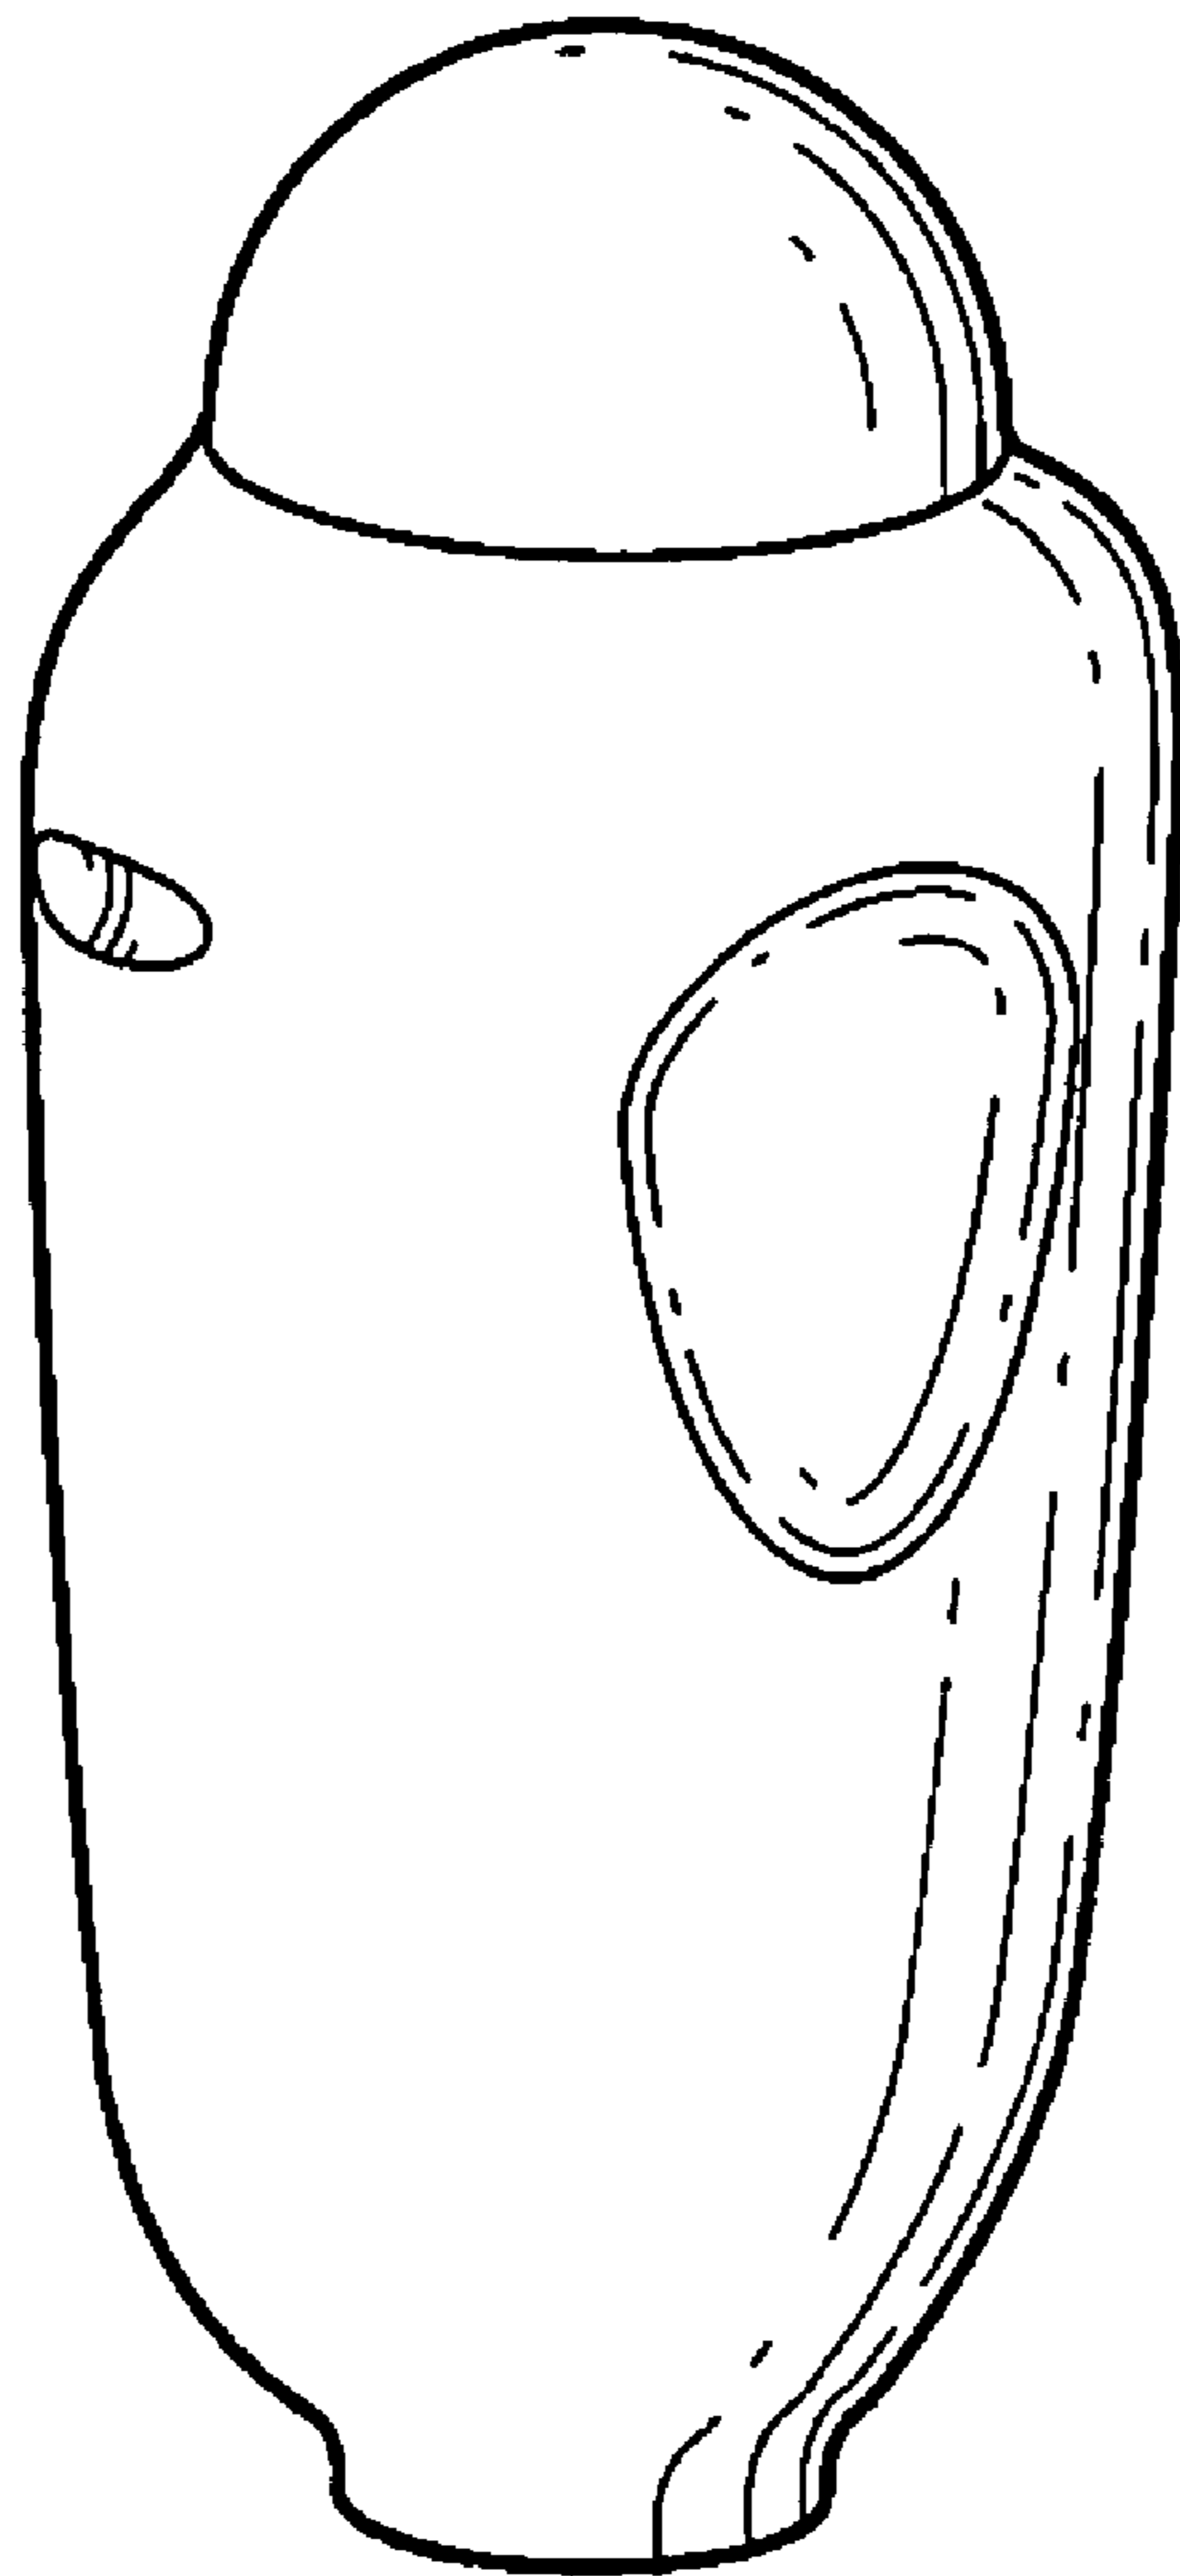


FIG. 2

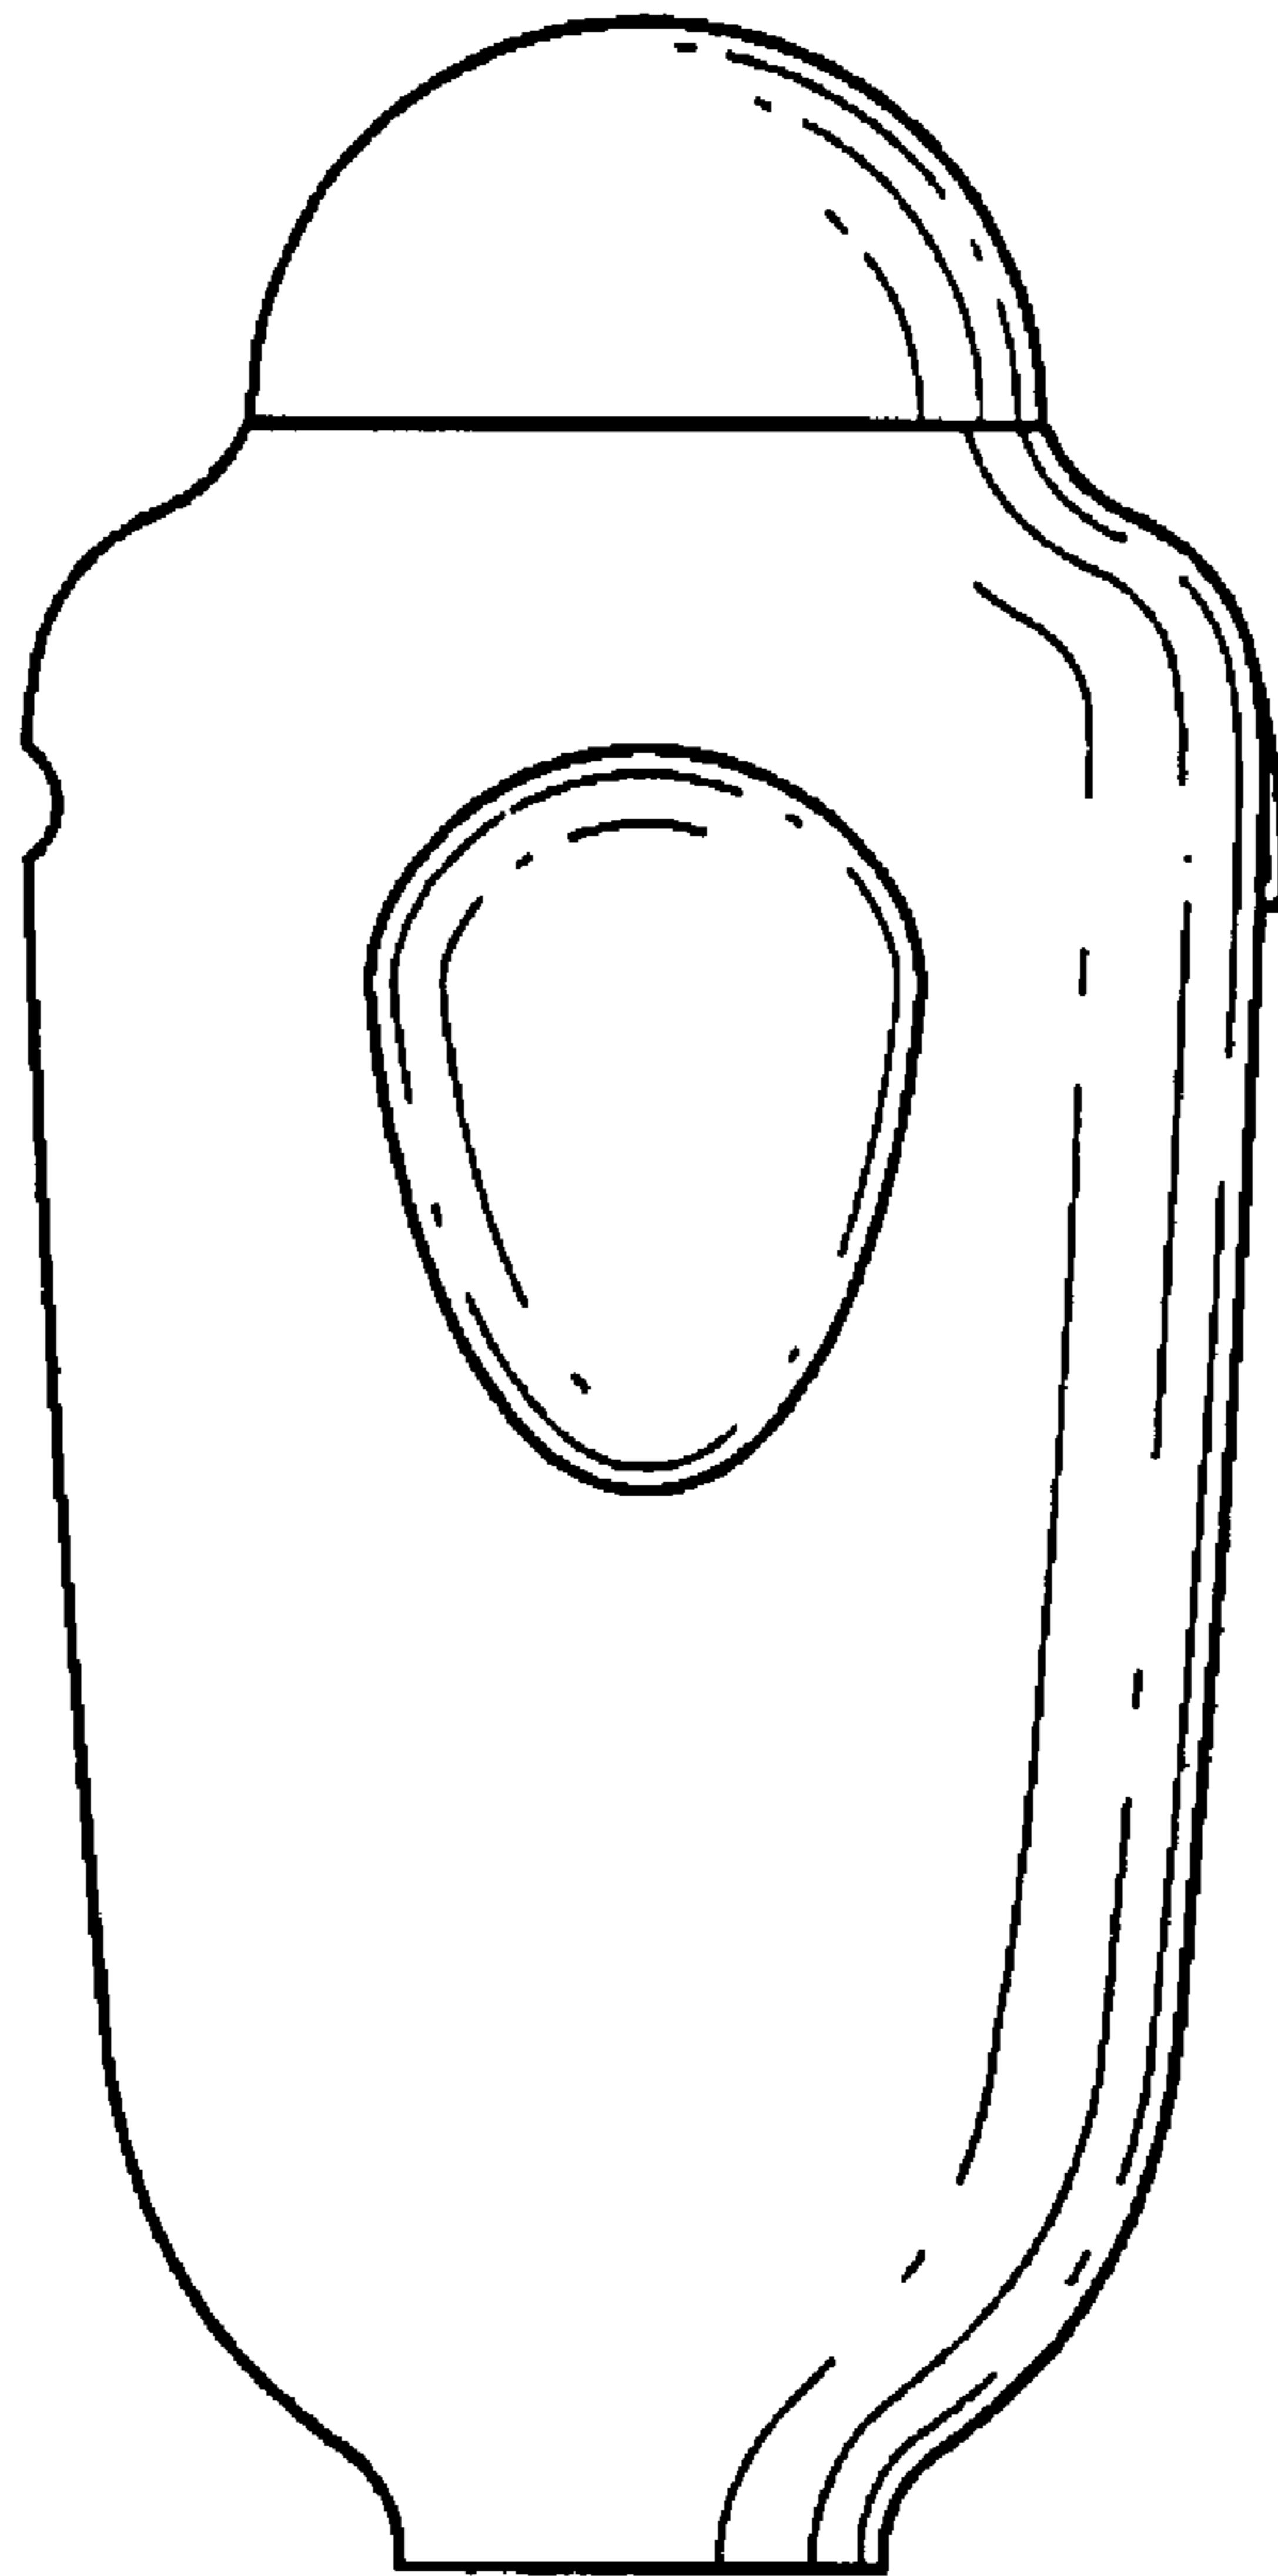


FIG. 3

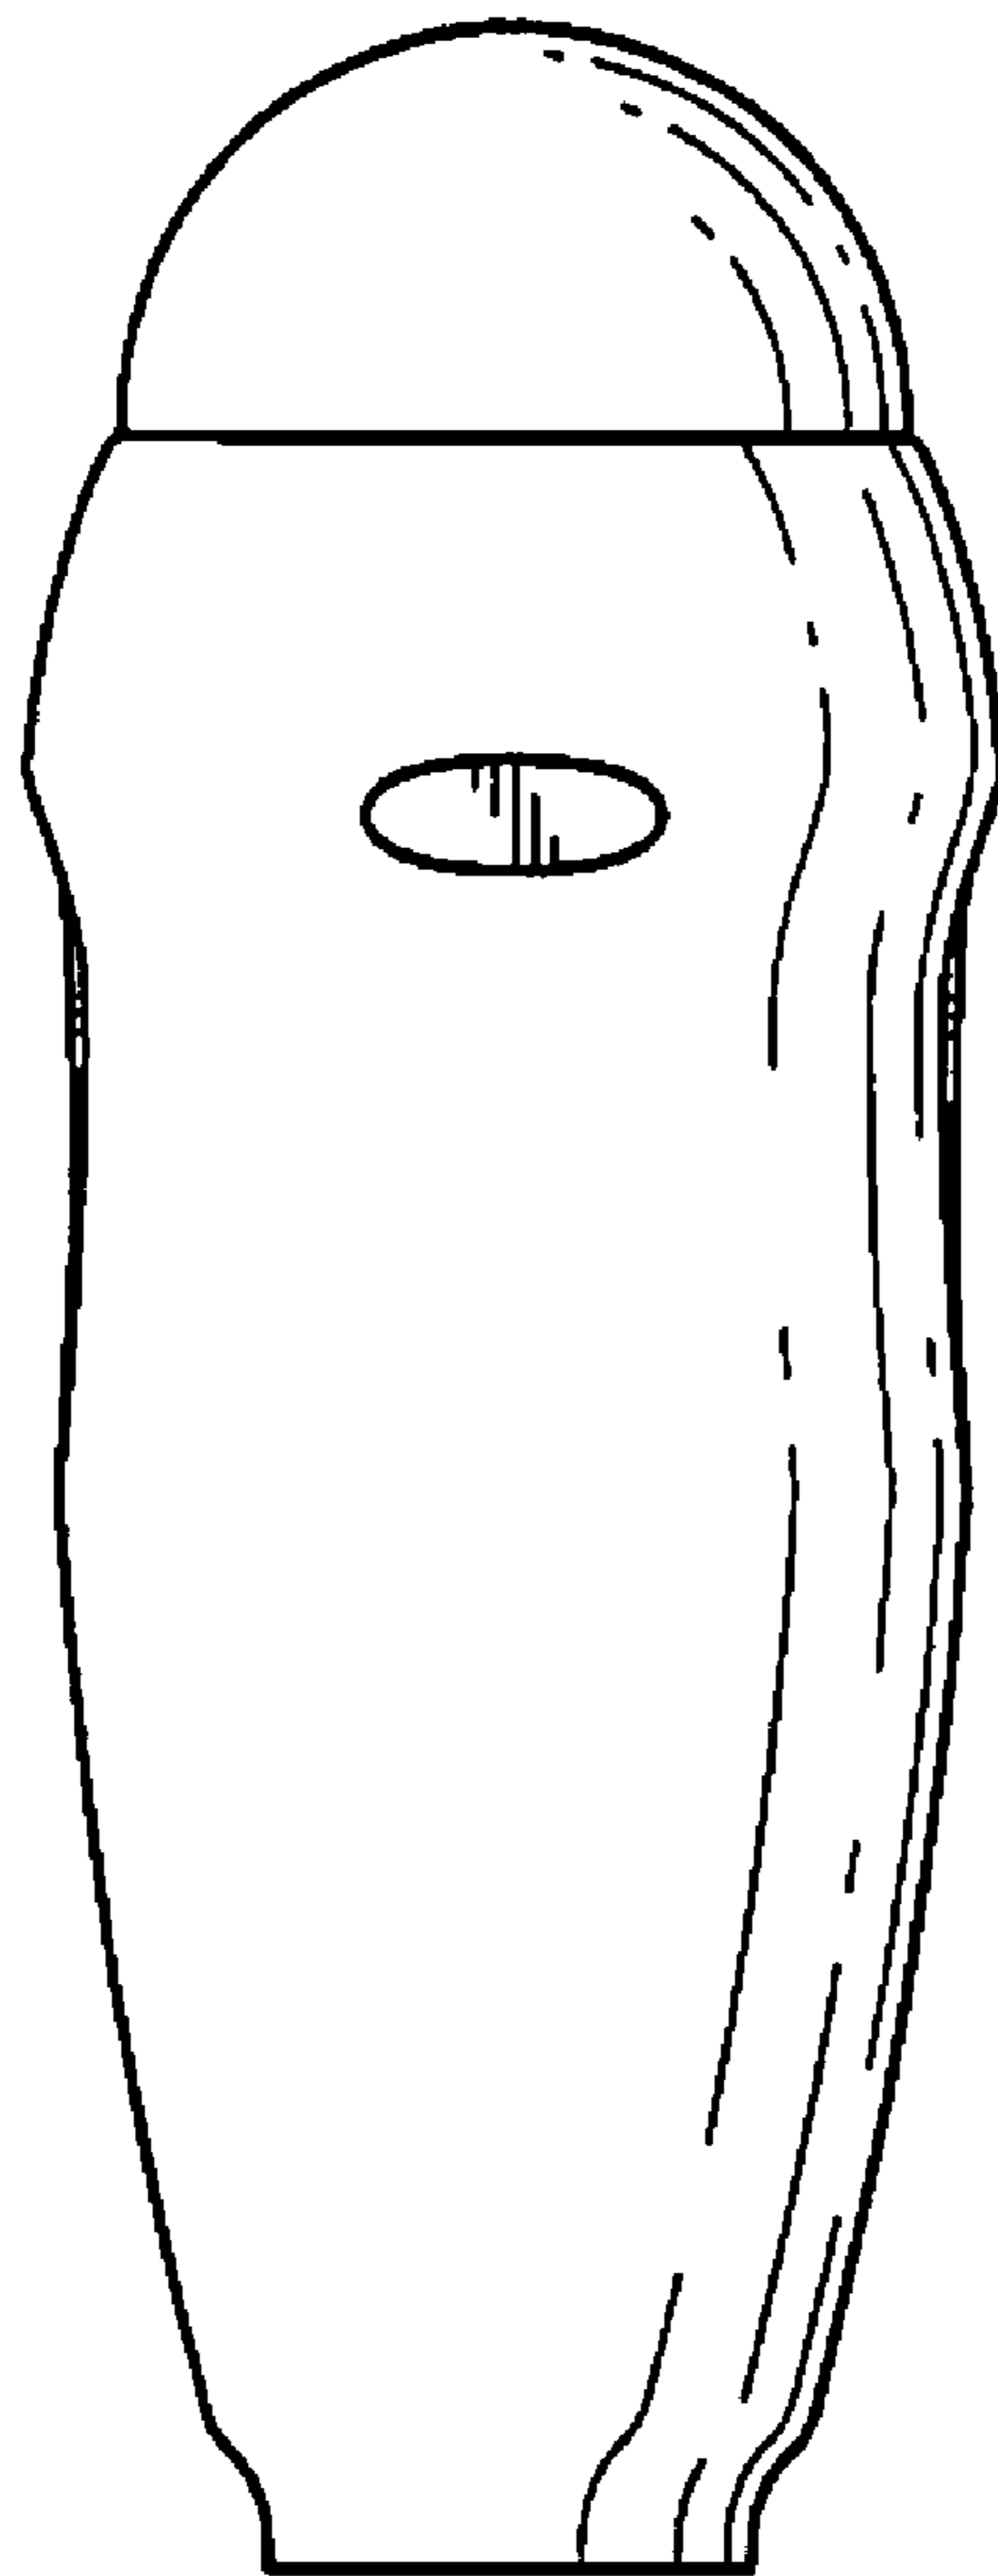


FIG. 4

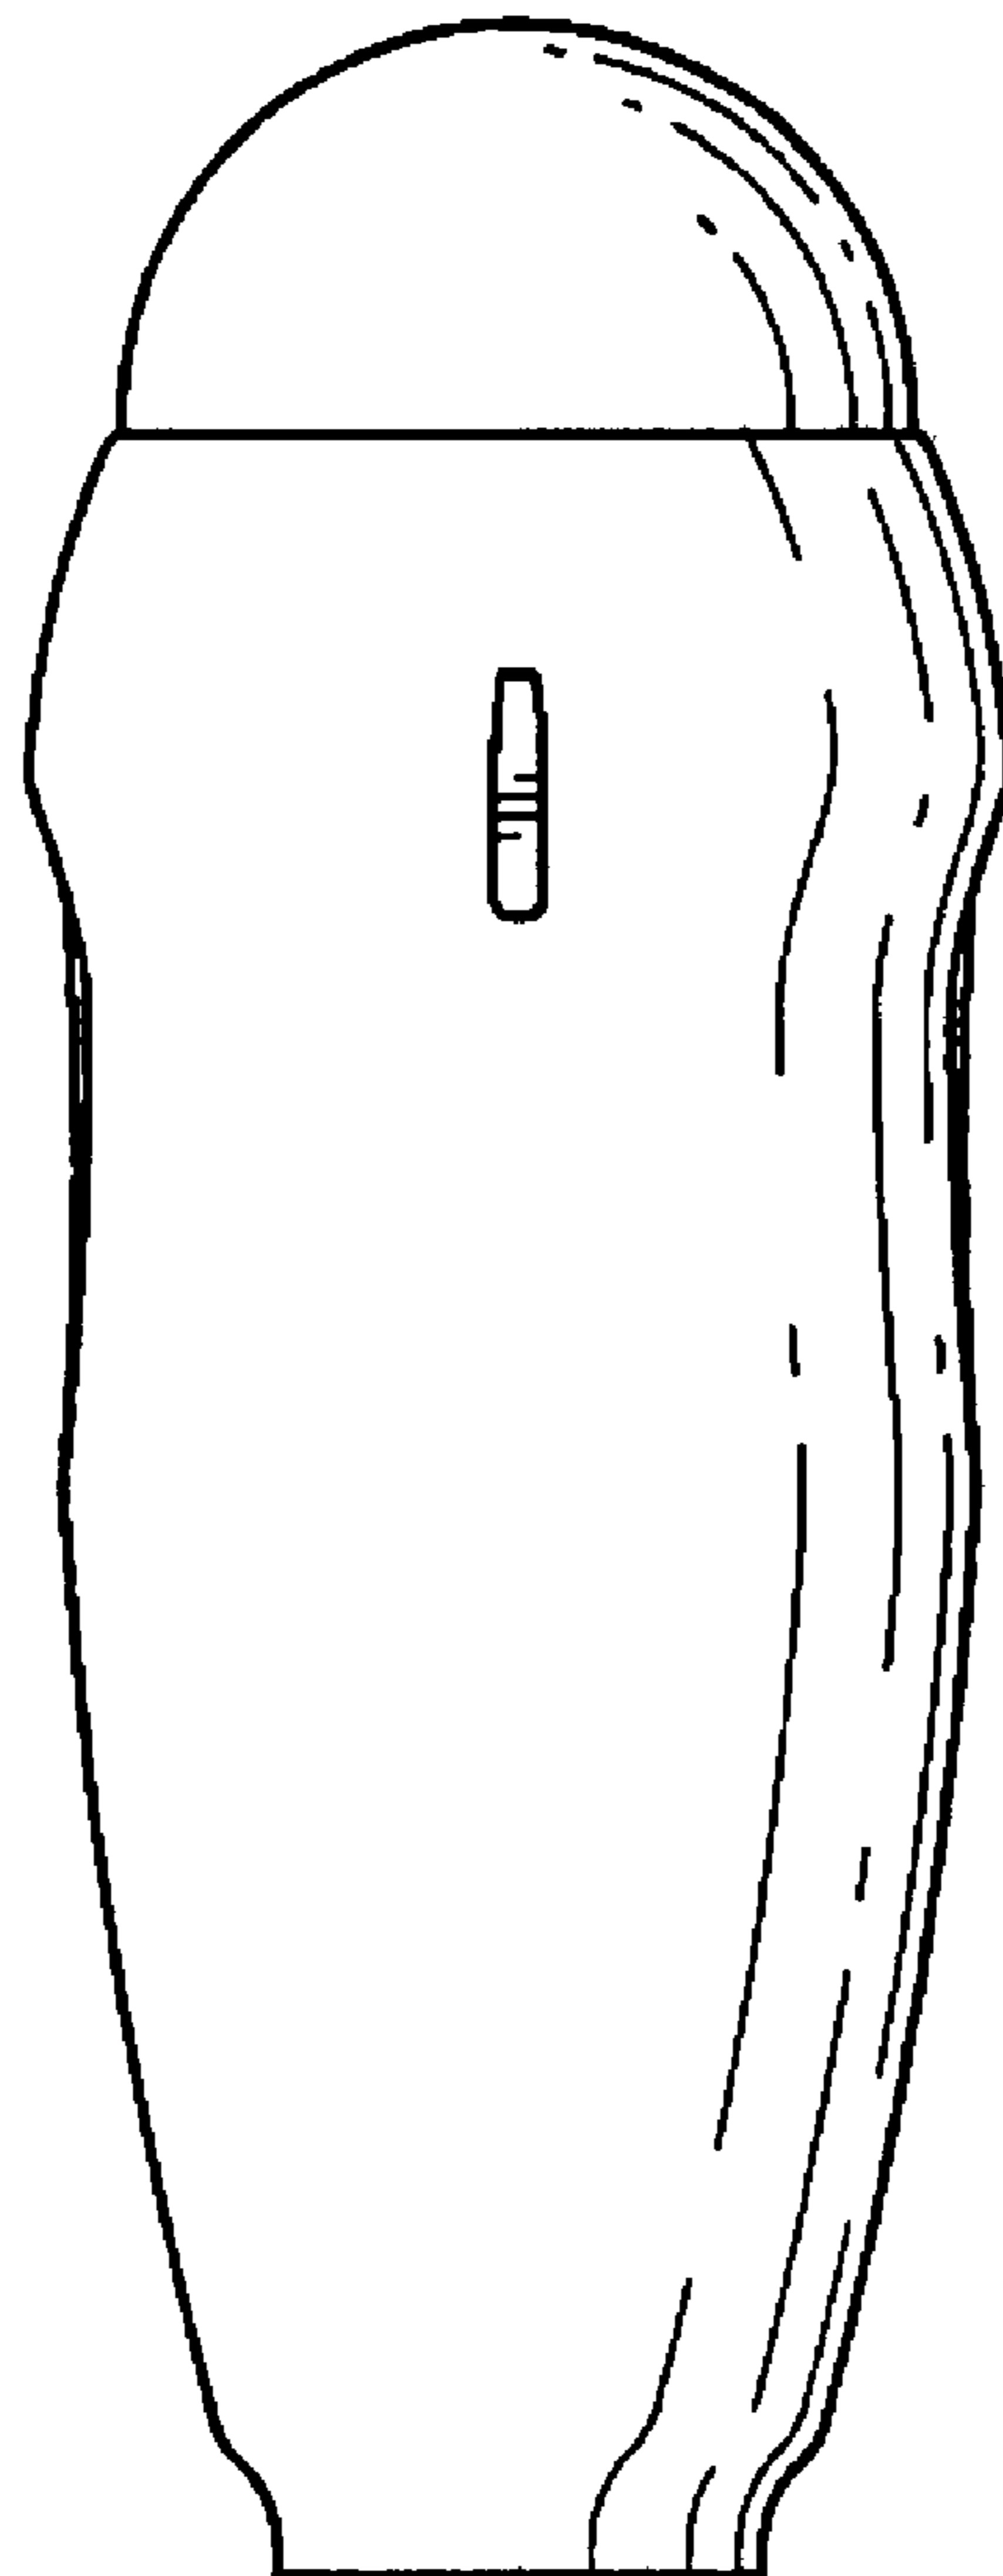


FIG. 5

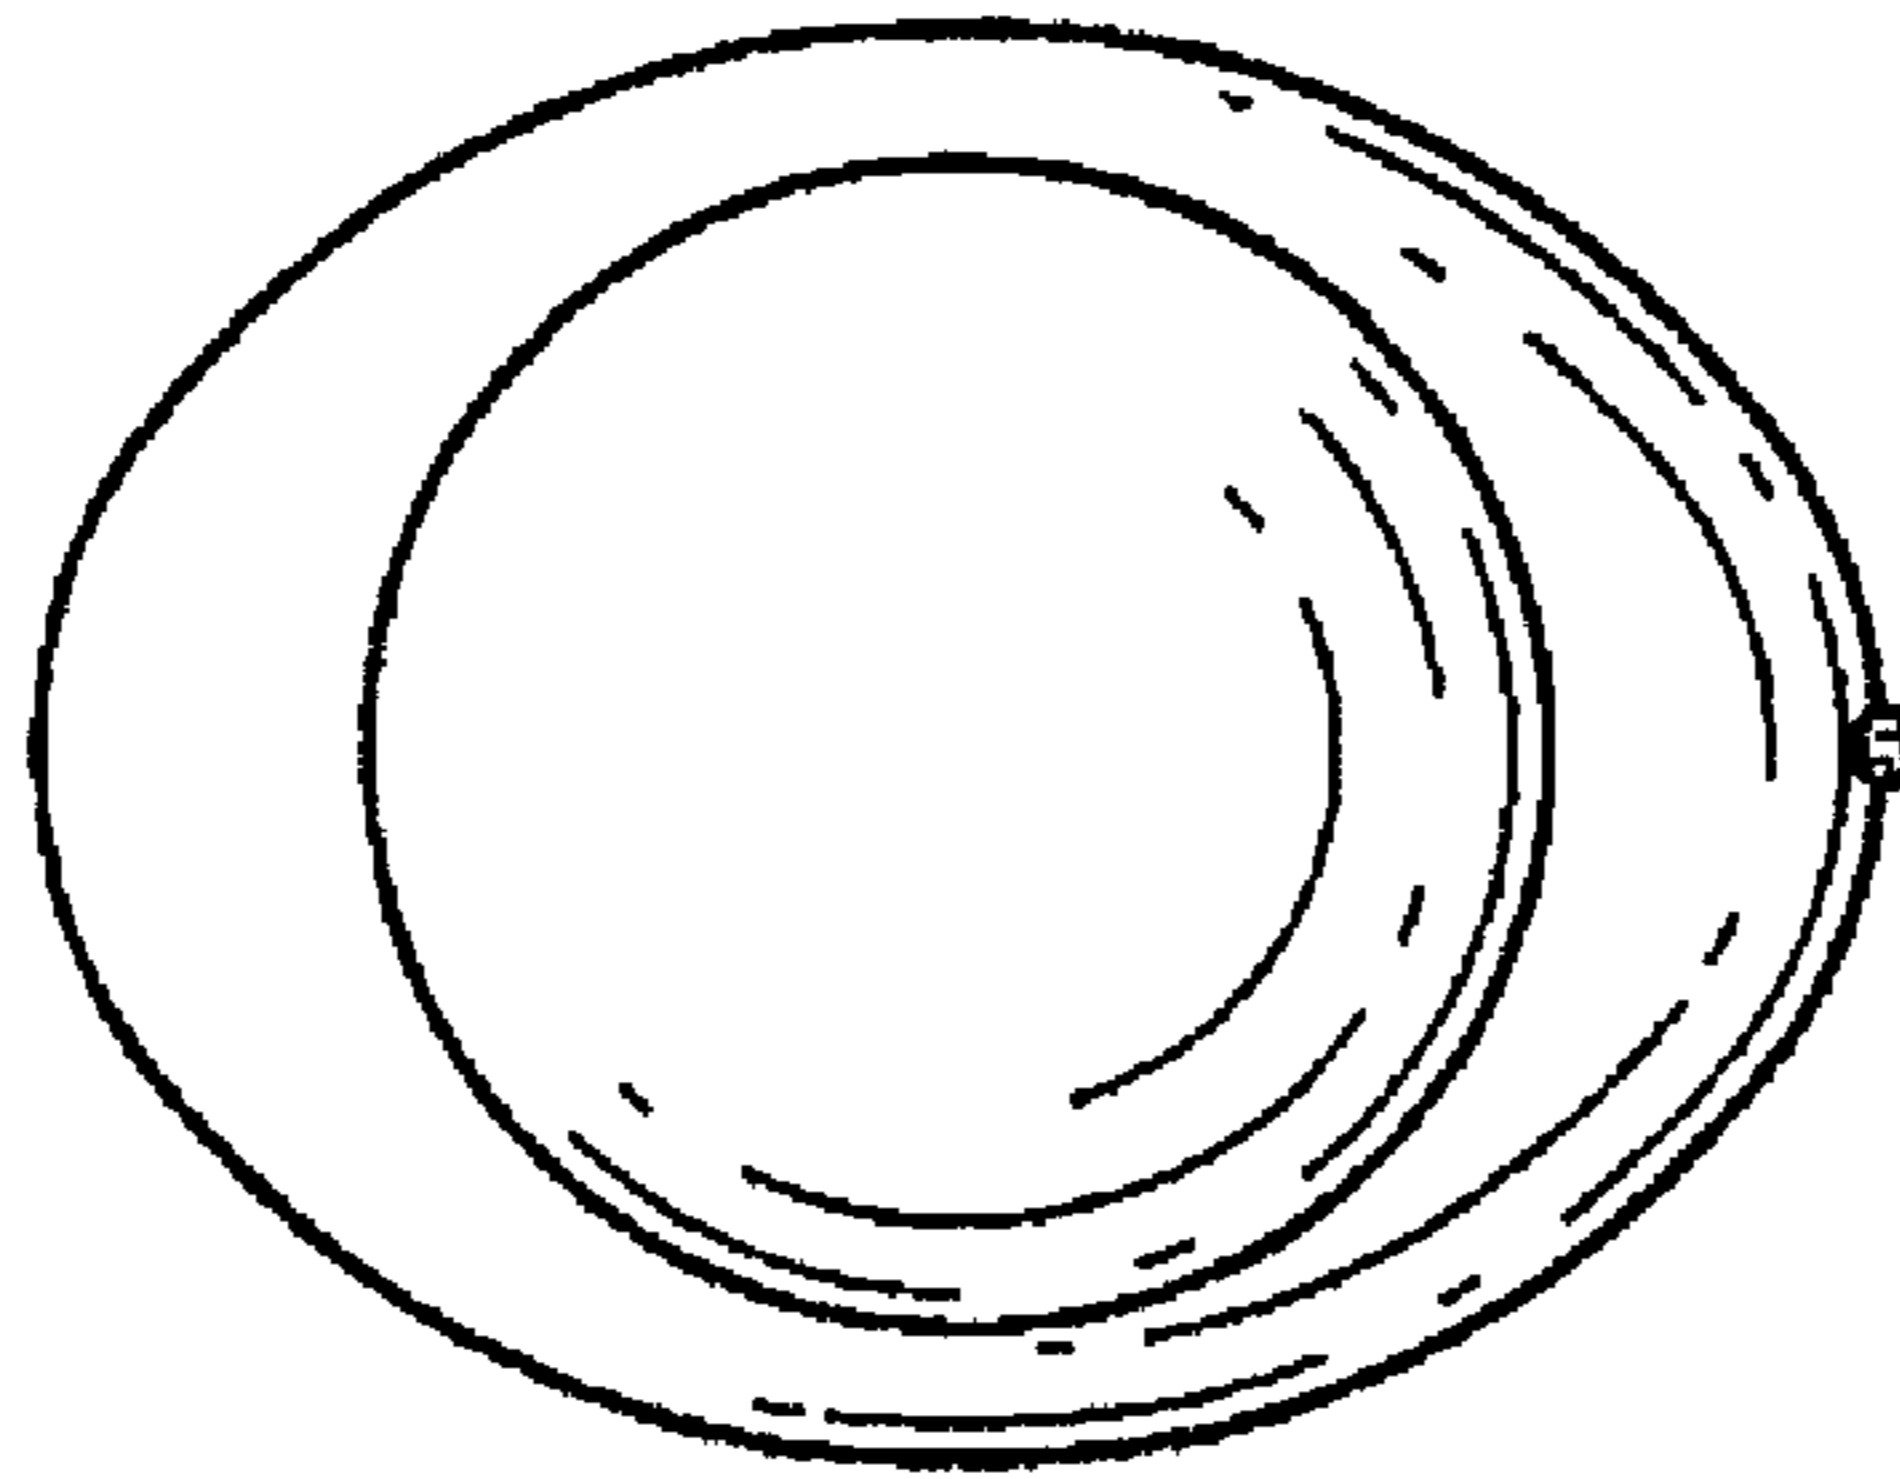


FIG. 6

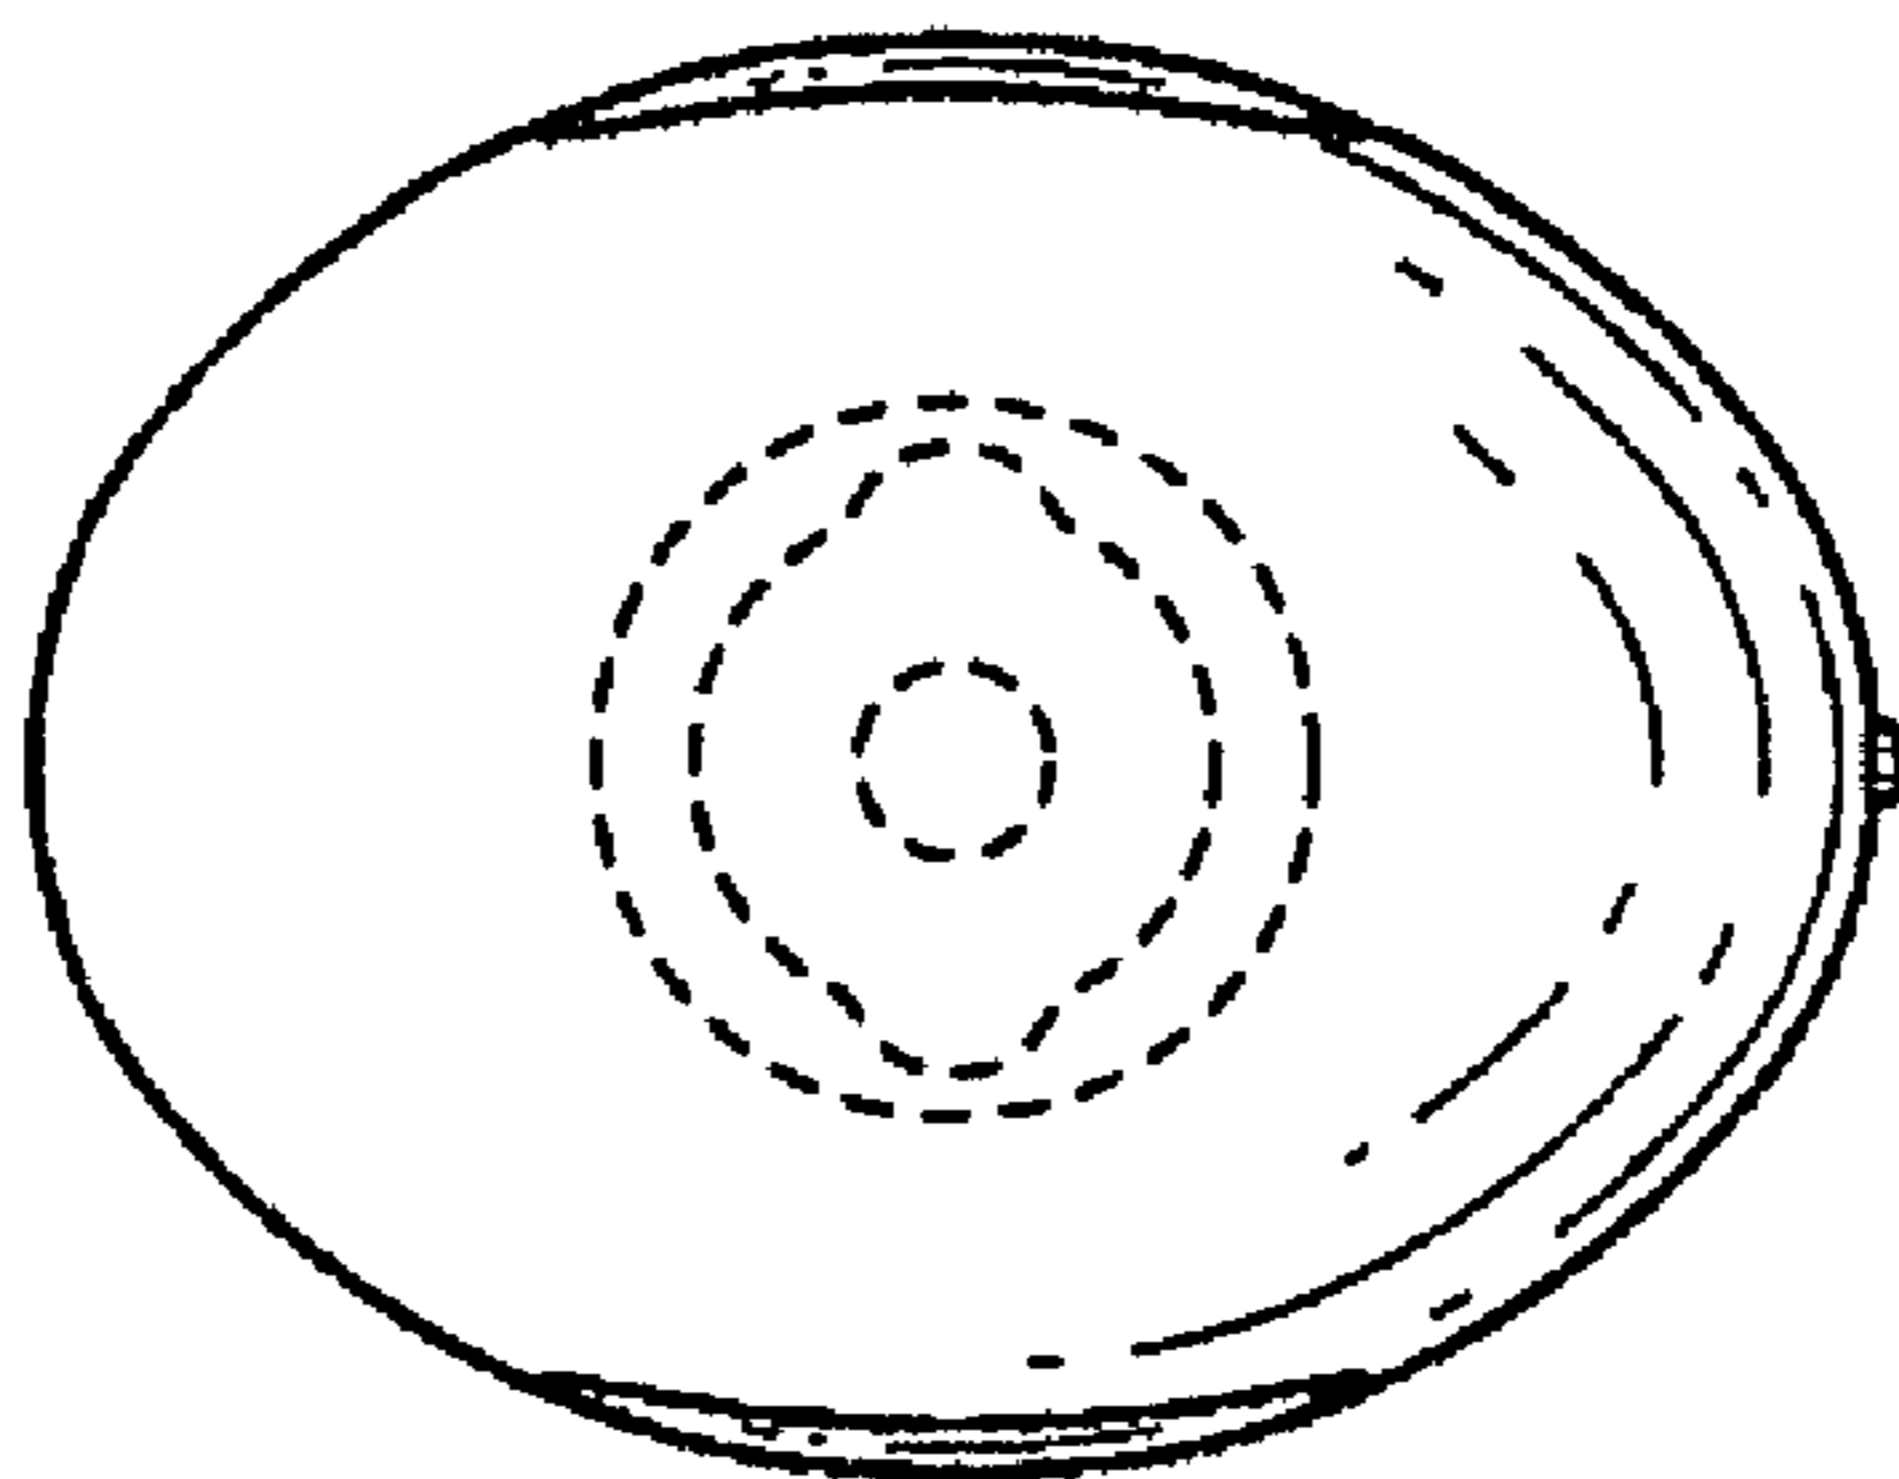


FIG. 7

