



US00D596300S

(12) **United States Design Patent**  
**Han et al.**

(10) **Patent No.:** **US D596,300 S**  
(45) **Date of Patent:** **\*\* Jul. 14, 2009**

(54) **MEDICAL ULTRASOUND TRANSDUCER**

(75) Inventors: **Jin Ha Han**, Gyeonggi-do (KR); **Dong Hyun Kim**, Gyeongbuk (KR); **Ji Whan Moon**, Busan (KR); **In Seong Song**, Daegu (KR)

(73) Assignee: **Prosonic Co., Ltd.**, Gyeongbuk (KR)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/274,638**

(22) Filed: **May 11, 2007**

(30) **Foreign Application Priority Data**

Nov. 13, 2006 (KR) ..... 30-2006-0045148

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/186**

(58) **Field of Classification Search** ..... D24/141, D24/144, 158, 186-187, 200; D10/78; 600/407, 600/461, 459; 378/98.7, 98.8, 189  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

- D369,307 S \* 4/1996 Imling et al. .... D10/78
- D387,867 S \* 12/1997 Henderson et al. .... D24/187
- D389,918 S \* 1/1998 Ninomiya et al. .... D24/186
- D389,919 S \* 1/1998 Ninomiya et al. .... D24/186
- D390,959 S \* 2/1998 Mesaros et al. .... D24/186
- D392,044 S \* 3/1998 Mesaros et al. .... D24/186
- 5,897,503 A \* 4/1999 Lyon et al. .... 600/459
- D462,446 S \* 9/2002 Felix et al. .... D24/187

- D544,606 S \* 6/2007 Hasegawa et al. .... D24/186
- D545,433 S \* 6/2007 Messerly et al. .... D24/158
- D546,460 S \* 7/2007 Hasegawa ..... D24/186
- D550,365 S \* 9/2007 Kitayama ..... D24/186
- D555,252 S \* 11/2007 Kitayama et al. .... D24/186

\* cited by examiner

*Primary Examiner*—Robert A. Delehanty

*Assistant Examiner*—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Venable LLP; Michael A. Sartori; Kyle D. Petaja

(57) **CLAIM**

The ornamental design for a medical ultrasound transducer, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the medical ultrasound transducer;

FIG. 2 is a front view of the medical ultrasound transducer;

FIG. 3 is a left side view of the medical ultrasound transducer;

FIG. 4 is a right side view of the medical ultrasound transducer;


FIG. 5 is a top view of the medical ultrasound transducer;

FIG. 6 is a bottom view of the medical ultrasound transducer; and,


FIG. 7 is a back view of the medical ultrasound transducer.

The broken line in the interior of the circular element in FIG. 6 is included for the purpose of illustrating environment and forms no part of the claimed design.


**1 Claim, 6 Drawing Sheets**

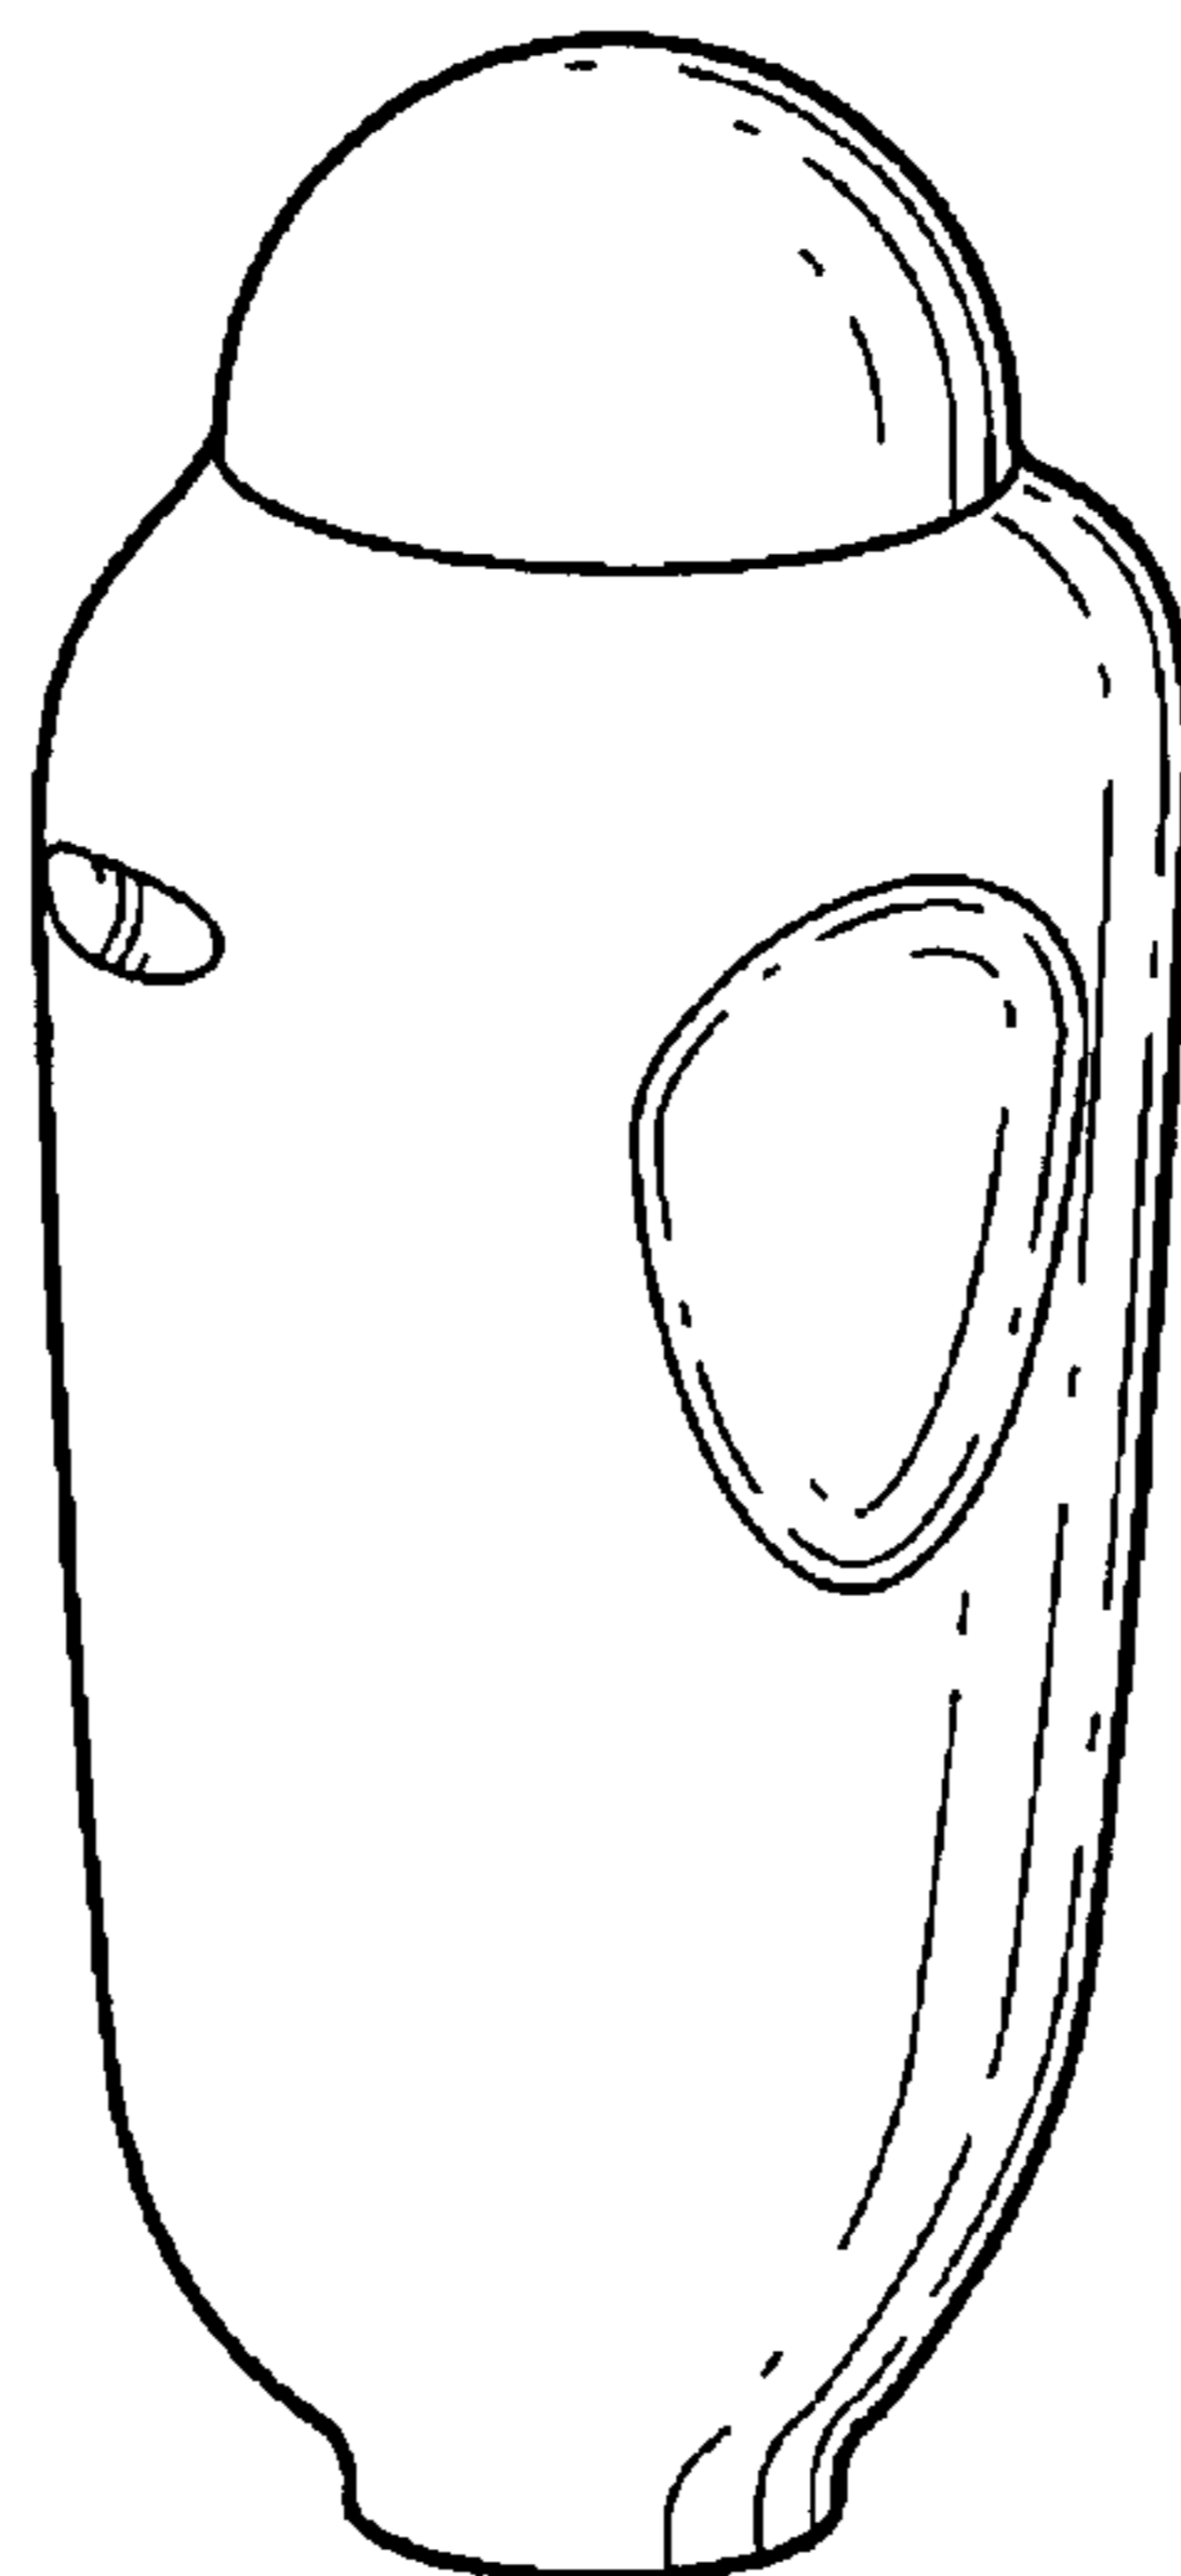


**FIG. 1**

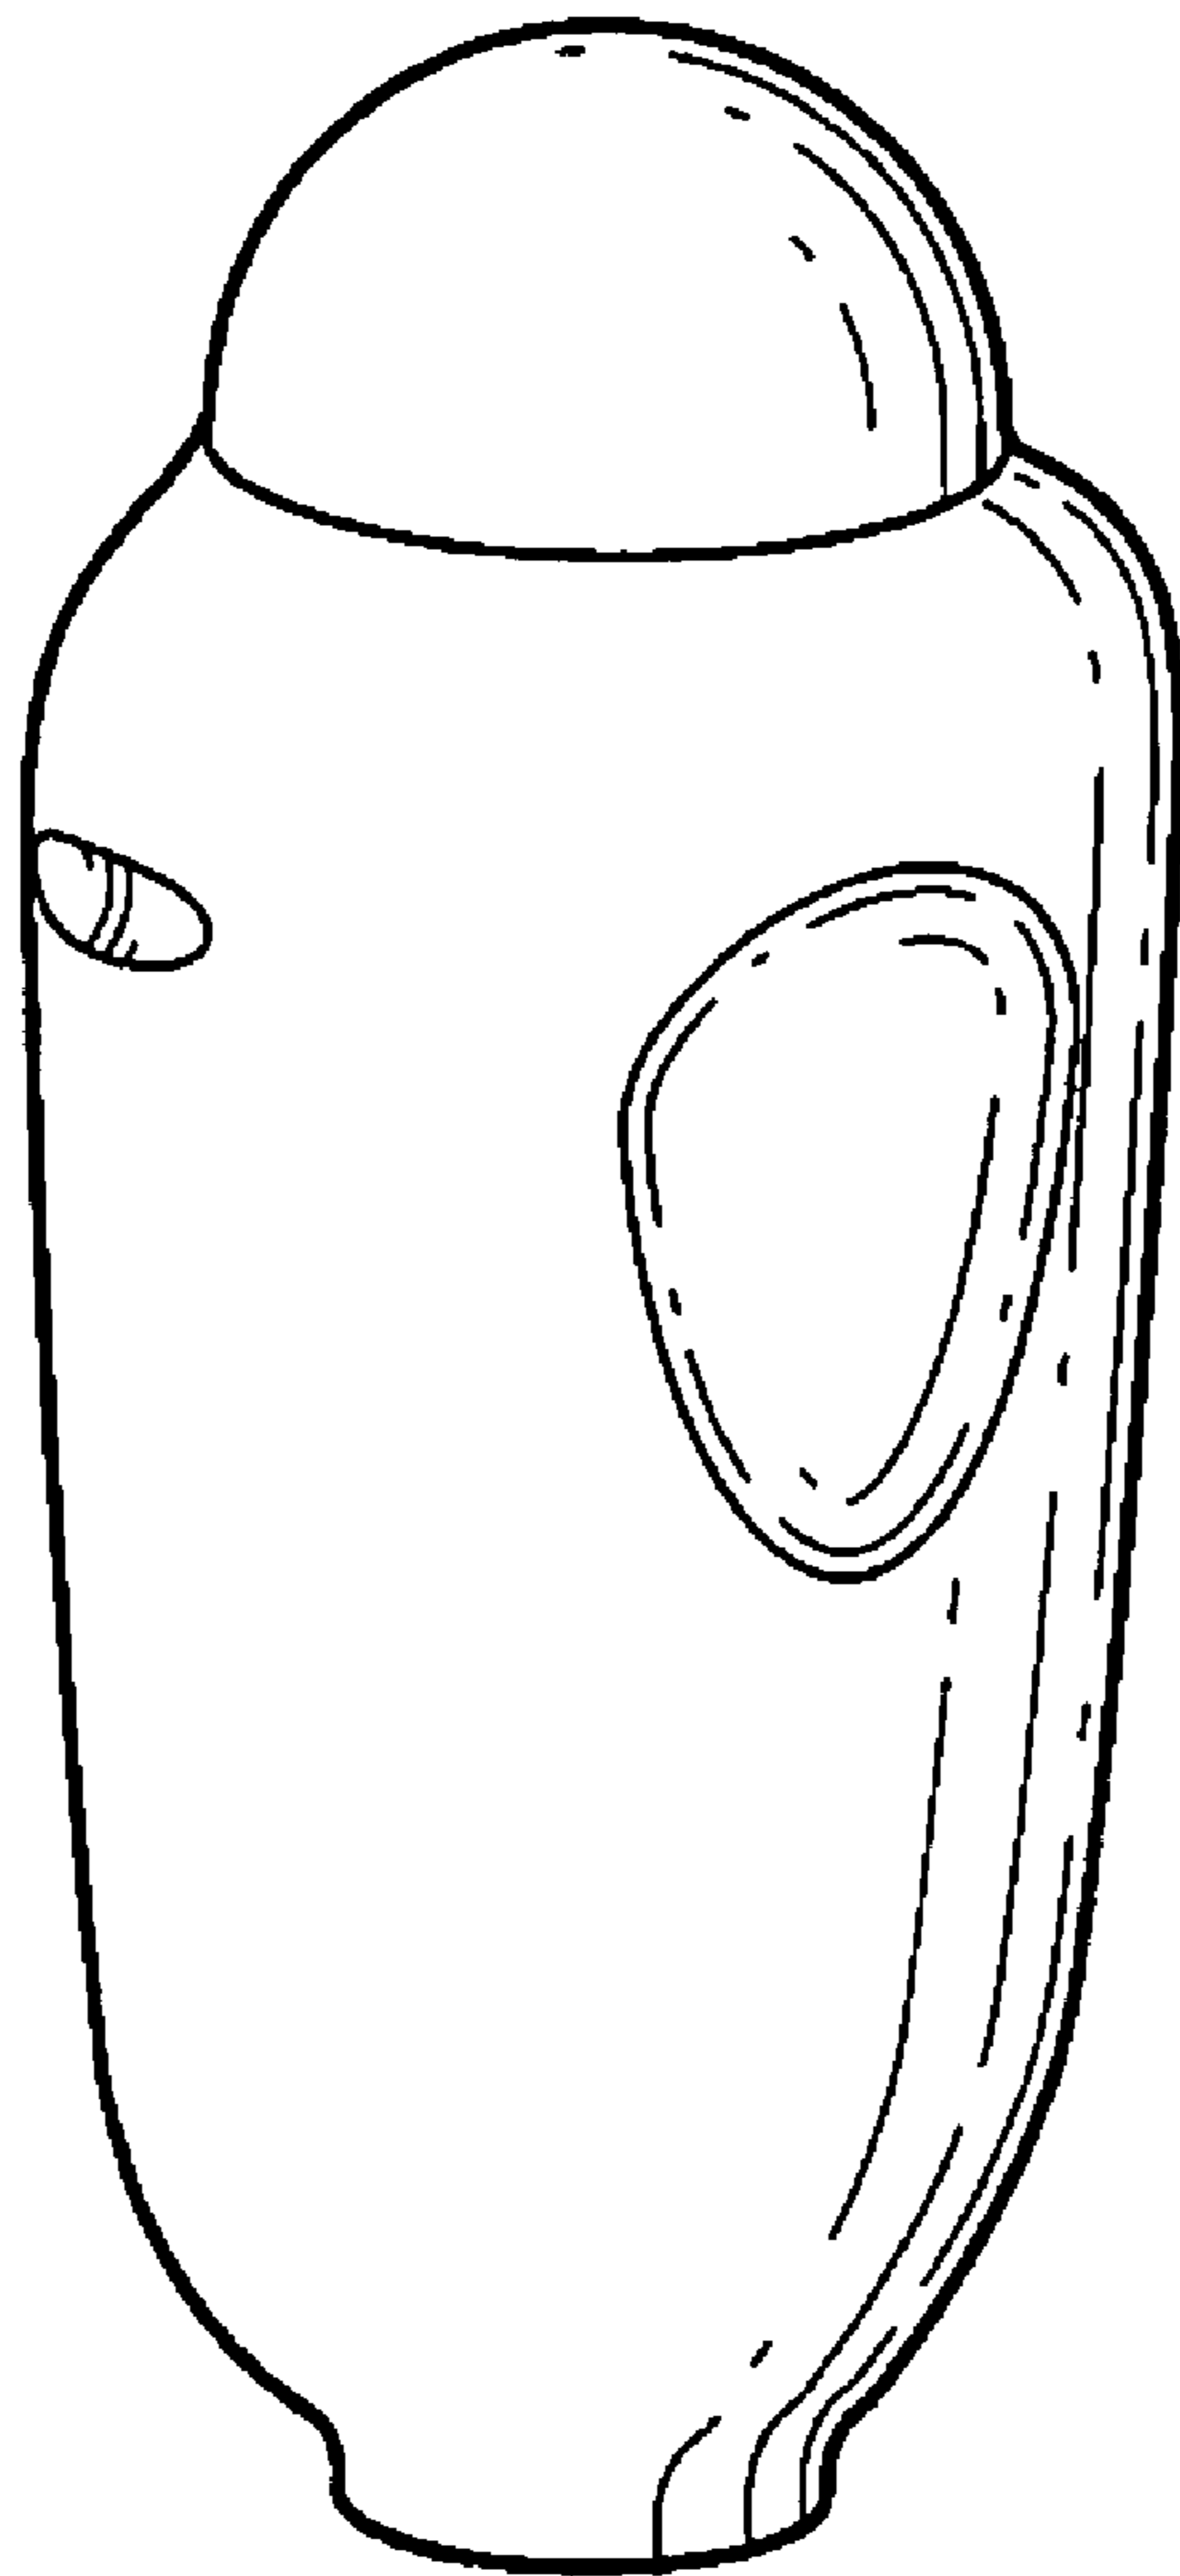


**FIG. 2**

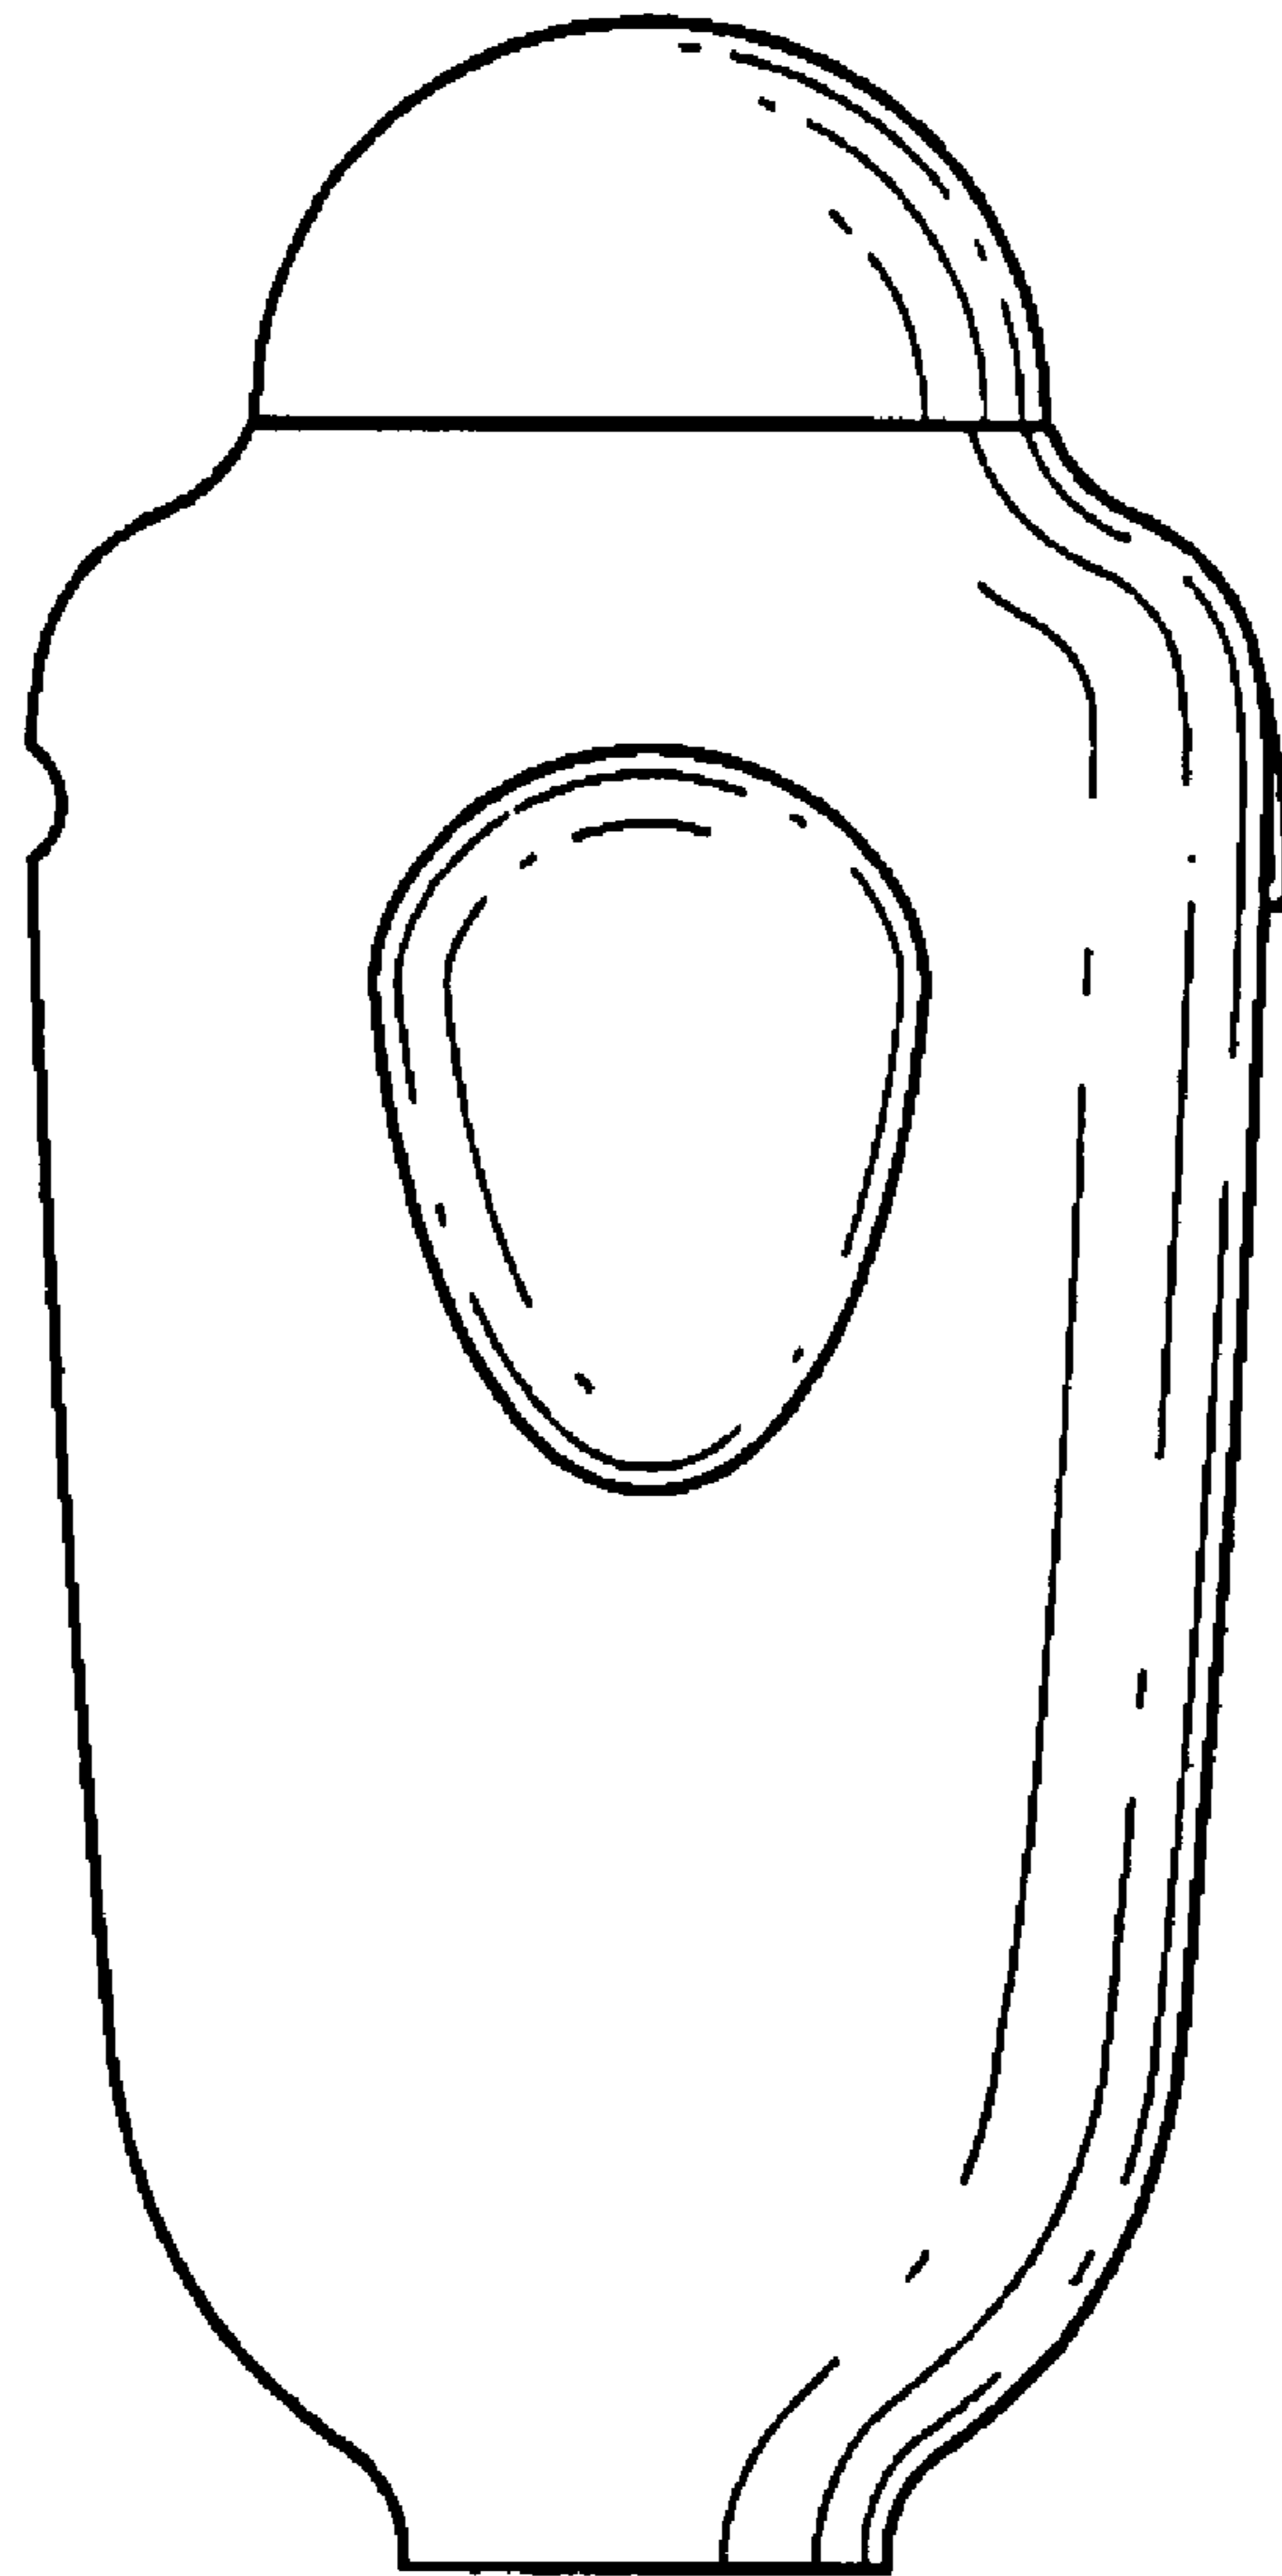


**FIG. 3**

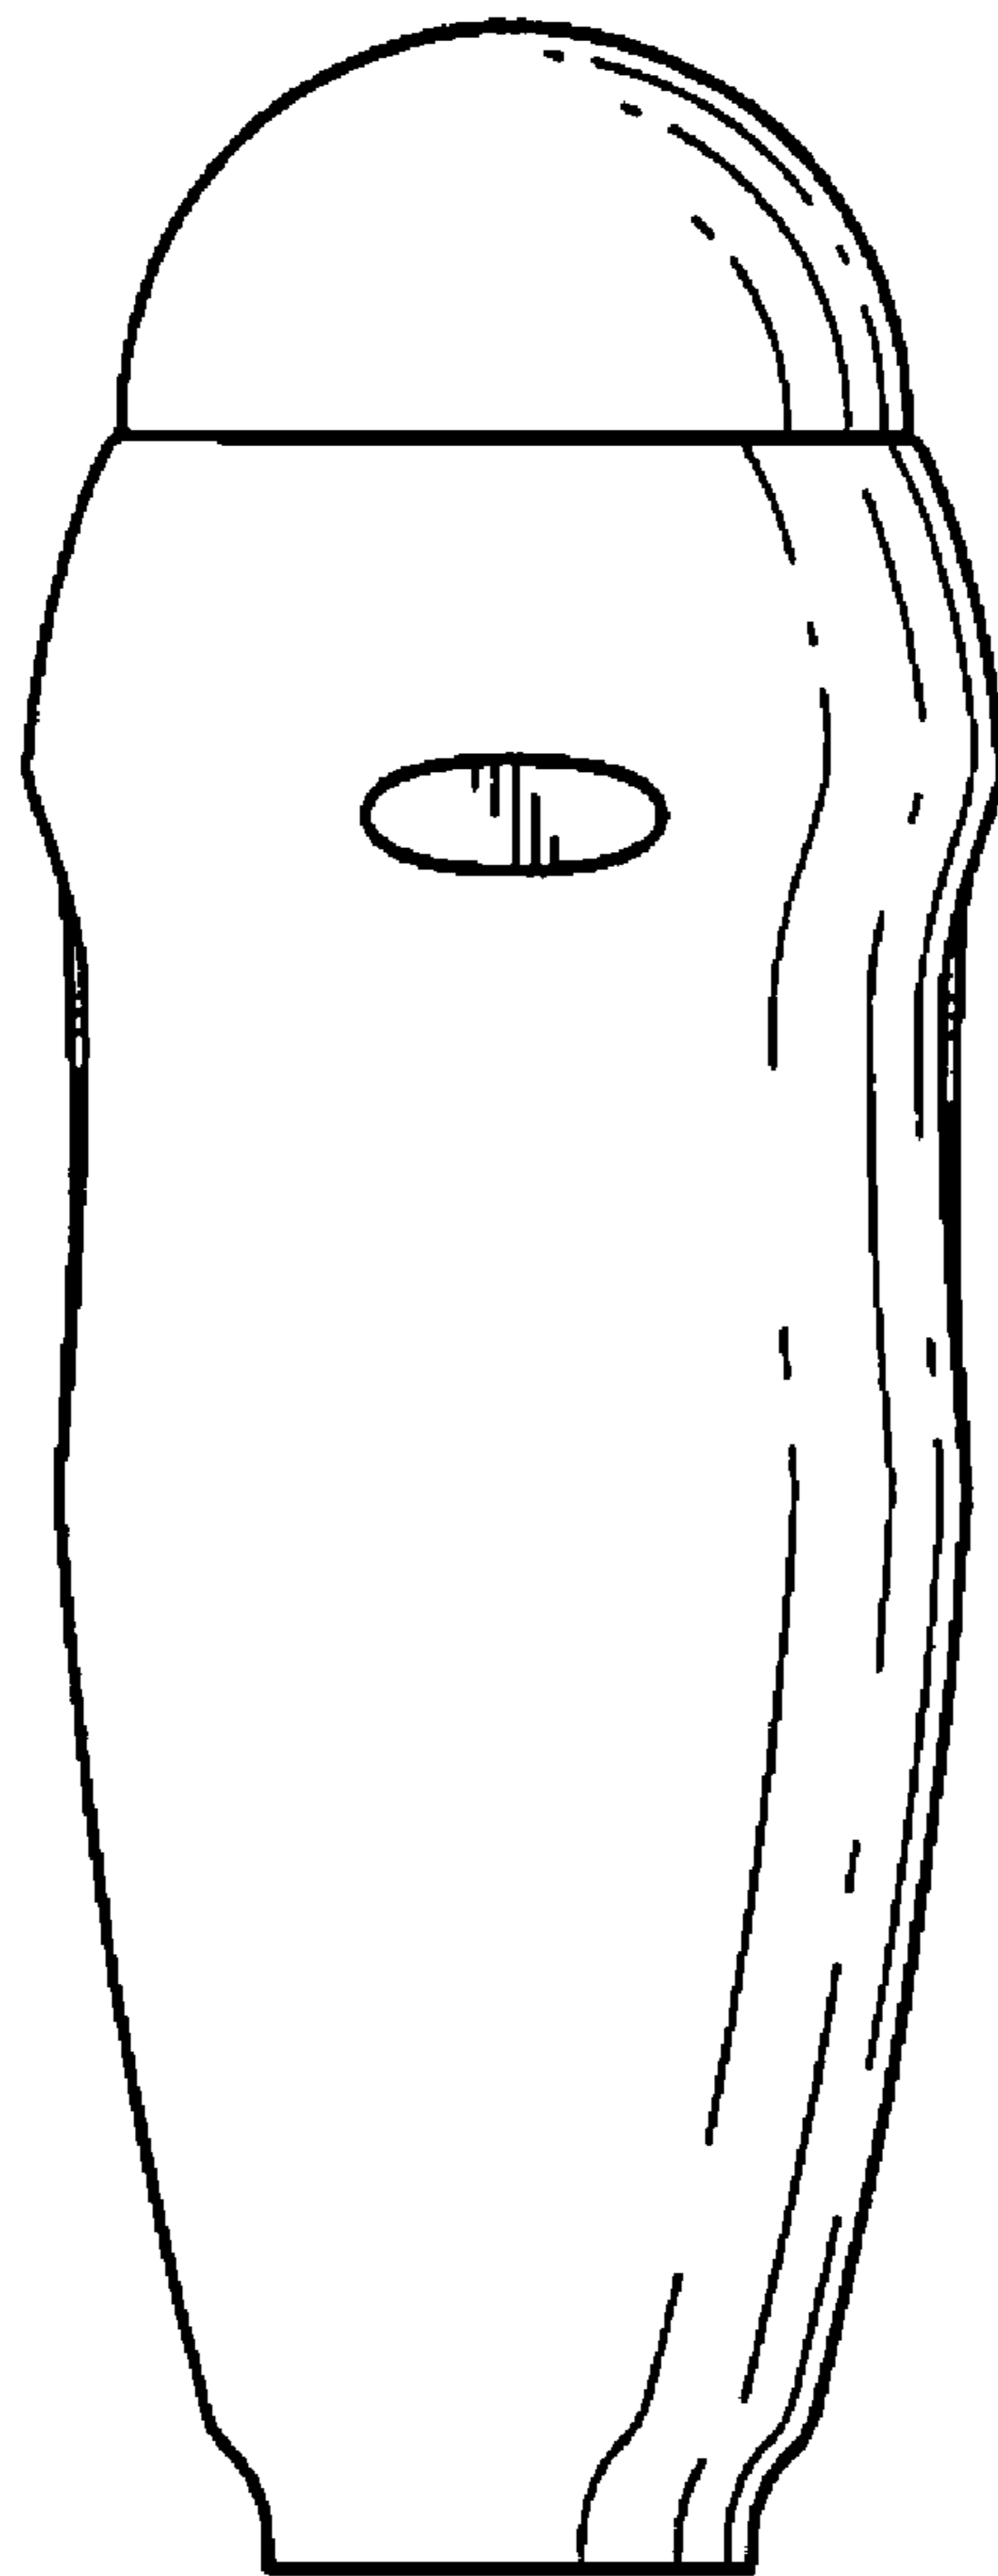


**FIG. 4**

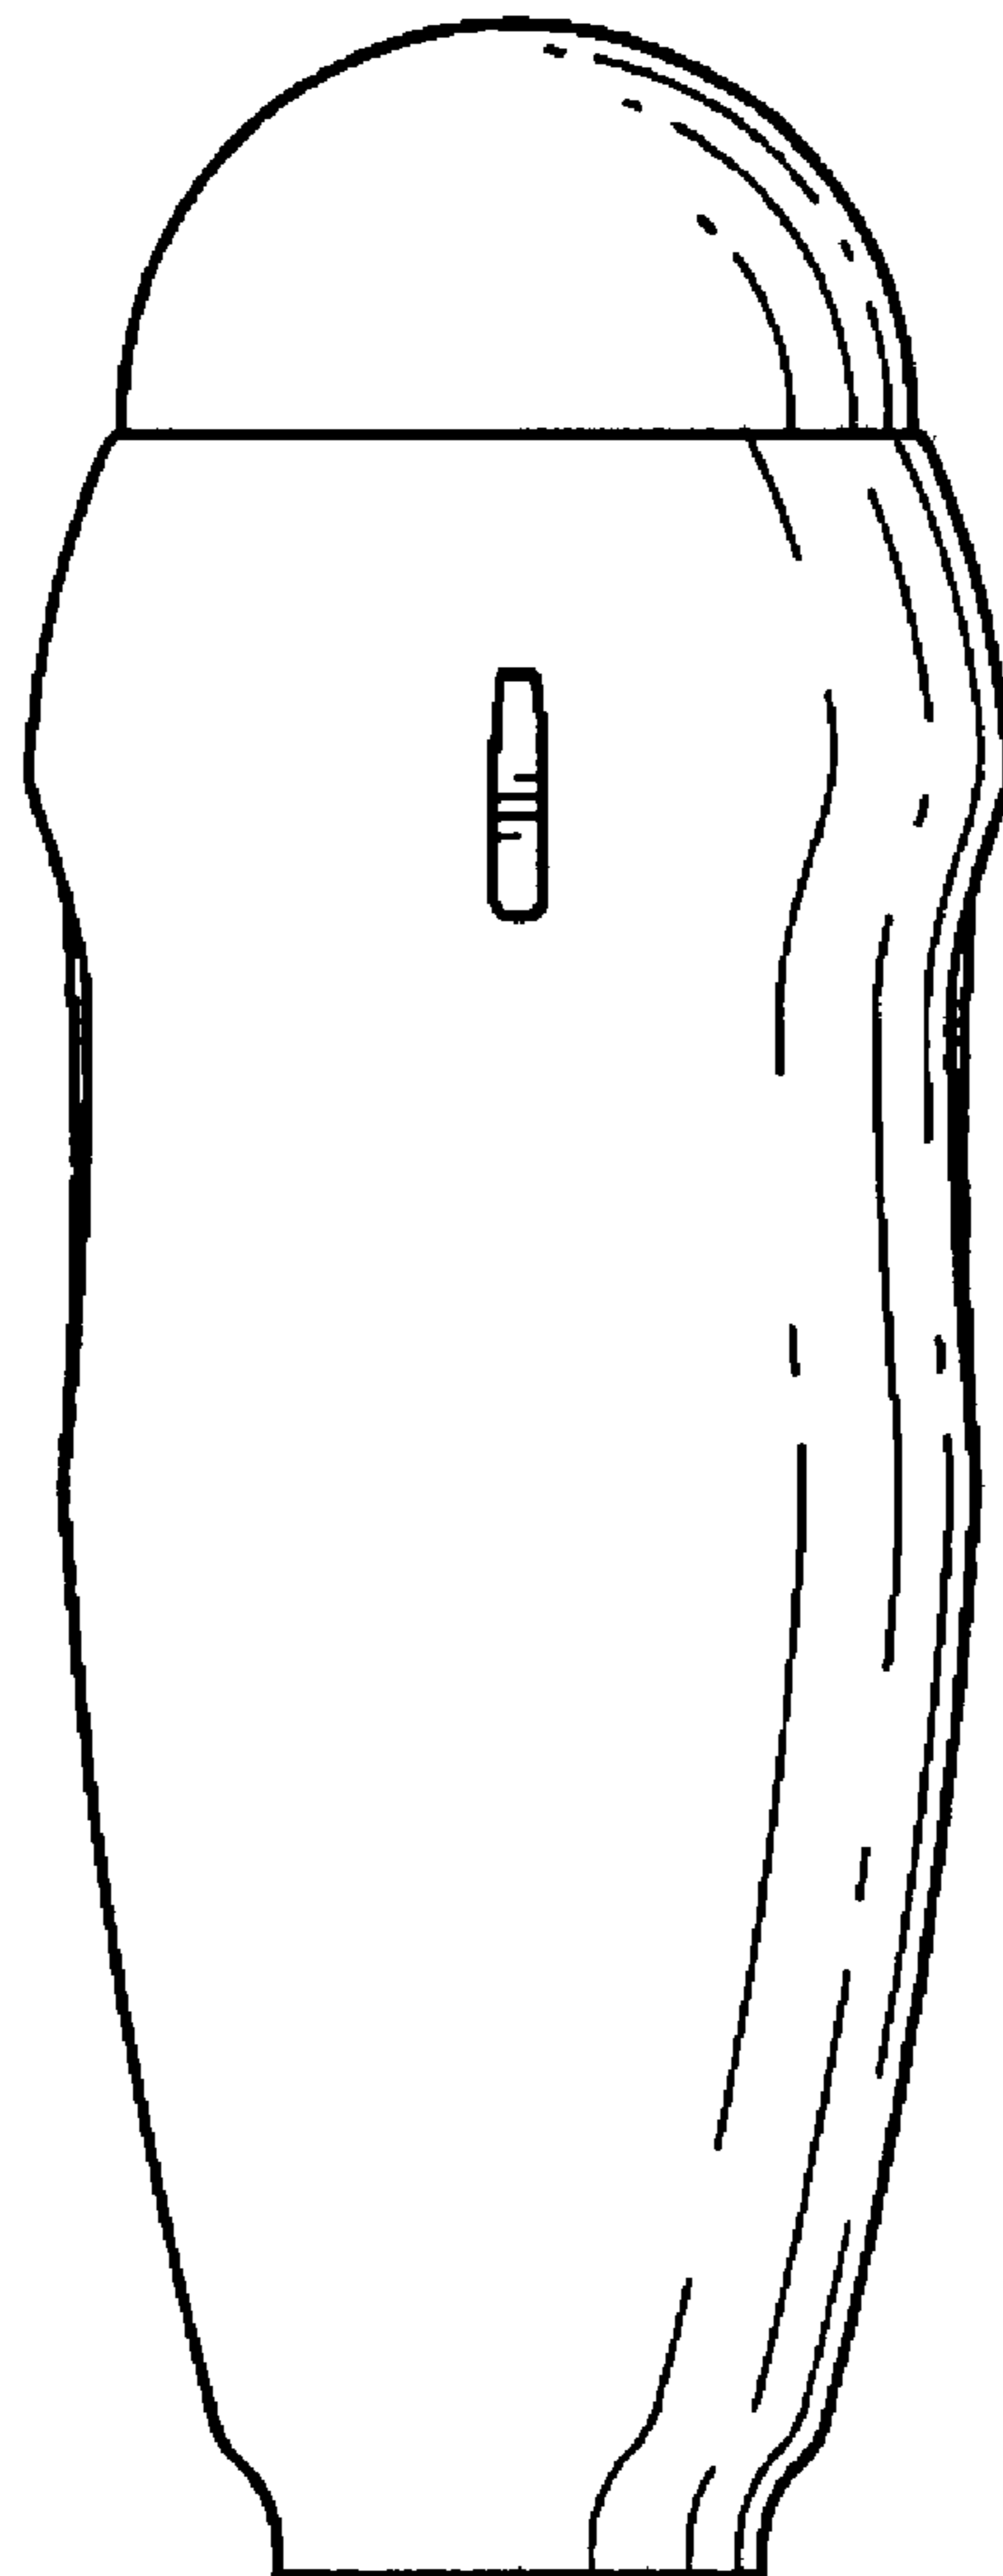

**FIG. 5**

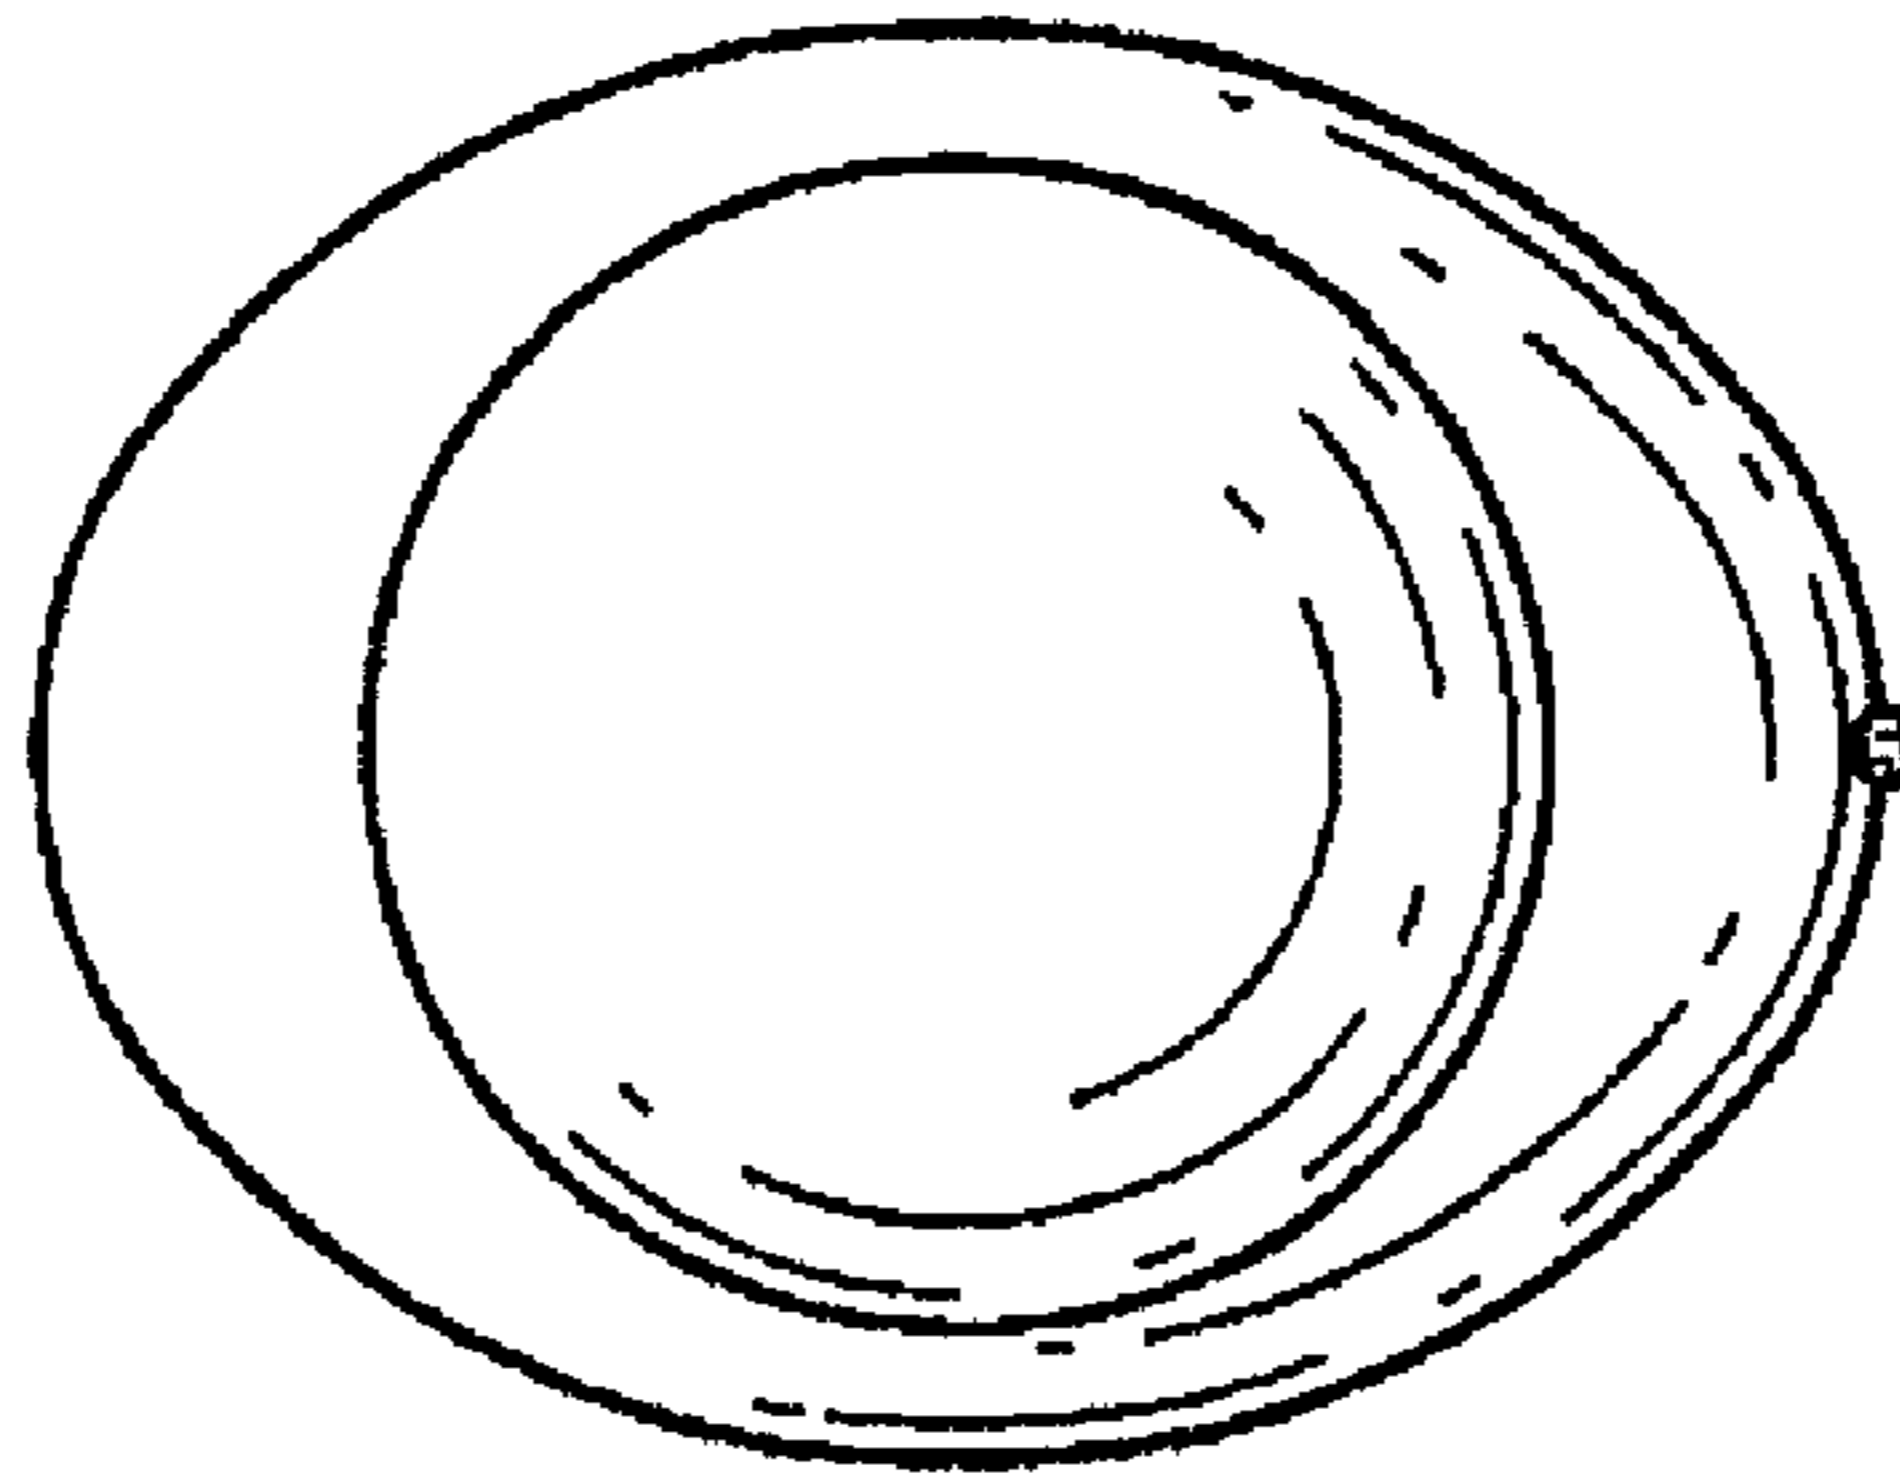

**FIG. 6**

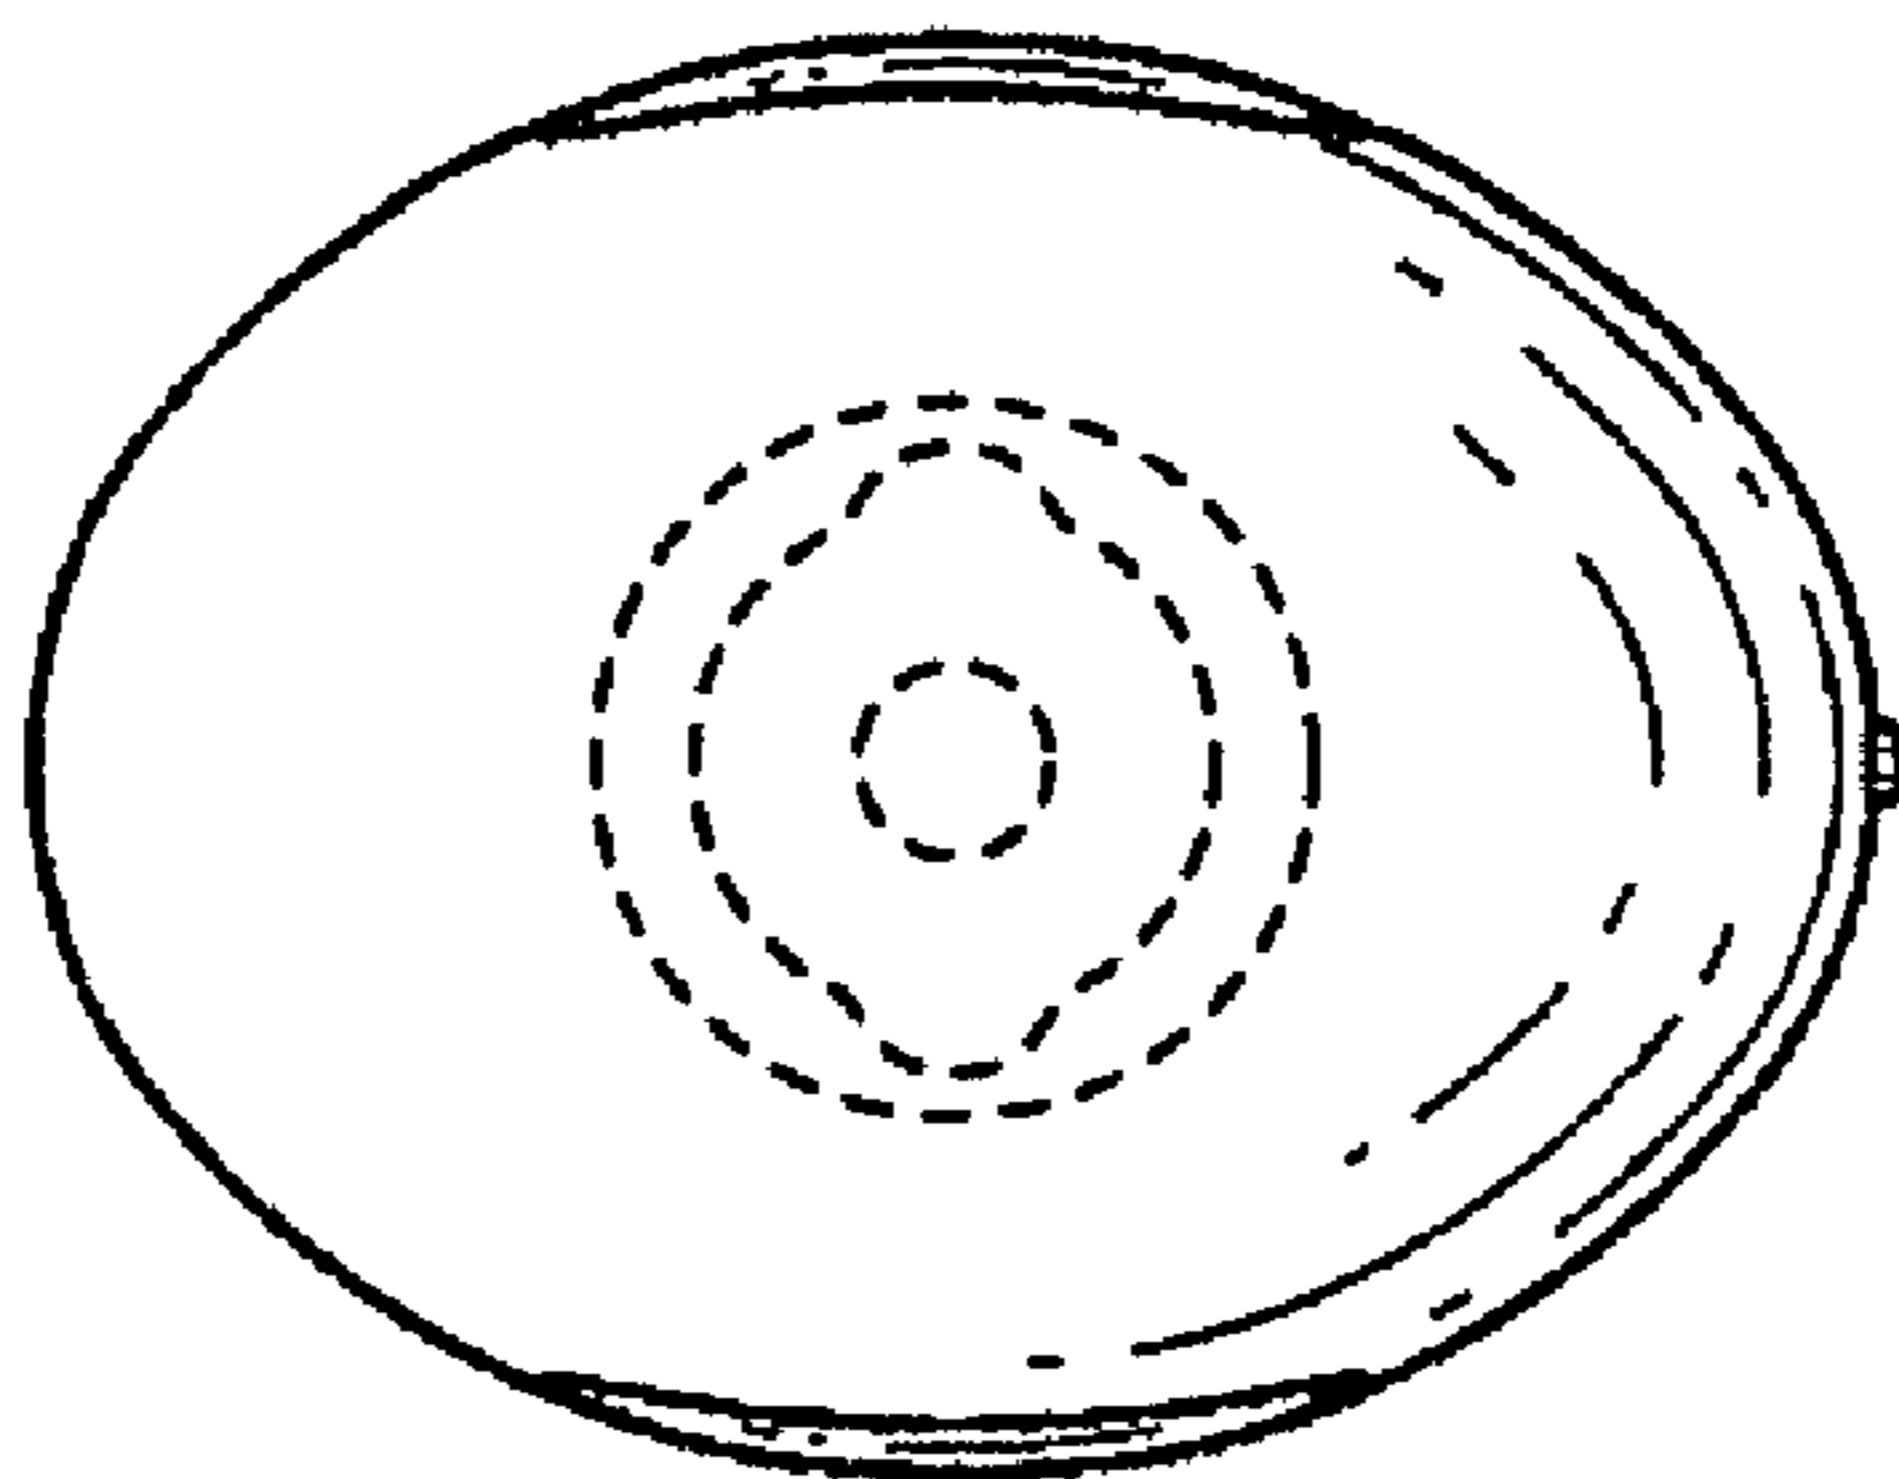

**FIG. 7**

