



US00D597037S

(12) **United States Design Patent**
Lampropoulos et al.

(10) **Patent No.:** **US D597,037 S**
(45) **Date of Patent:** **** Jul. 28, 2009**

(54) **INFLATION DEVICE DISPLAY**

(75) Inventors: **Fred P. Lampropoulos**, Salt Lake City, UT (US); **Brian W. Stevens**, Pleasant Grove, UT (US)

(73) Assignee: **Merit Medical Systems, Inc.**, South Jordan, UT (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/321,794**

(22) Filed: **Jul. 23, 2008**

Related U.S. Application Data

(63) Continuation-in-part of application No. 12/118,442, filed on May 9, 2008.

(51) **LOC (9) Cl.** **13-03**

(52) **U.S. Cl.** **D13/162**

(58) **Field of Classification Search** D13/152, D13/158–168, 172, 174, 177, 184, 199; D14/137–139, D14/151, 167, 168, 172, 174, 191–193, 214, D14/217, 218, 240; 361/600, 622, 678, 681; 345/173; 338/153; 174/66; 200/5 A
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D373,571 S * 9/1996 Zambelli et al. D13/162
D412,157 S * 7/1999 Stevenson D14/443
D422,545 S * 4/2000 Palalau et al. D12/192
D445,745 S * 7/2001 Norman D12/192

* cited by examiner

Primary Examiner—Daniel D Bui
Assistant Examiner—Thomas J Johannes

(74) *Attorney, Agent, or Firm*—Ryan D. Benson; Stoel Rives LLP

(57) **CLAIM**

The ornamental design for an inflation device display, substantially as shown and described.

DESCRIPTION

FIG. 1 is a front plan view of a first embodiment of an inflation device display, showing our new design;

FIG. 2 is a front perspective view thereof;

FIG. 3 is a front perspective view thereof, in a typical usage environment;

FIG. 4 is a front plan view thereof, showing an alternate usage configuration;

FIG. 5 is a front perspective view thereof;

FIG. 6 is a front perspective view thereof, in a typical usage environment;

FIG. 7 is a front plan view thereof, showing an alternate usage configuration;

FIG. 8 is a front perspective view thereof;

FIG. 9 is a front perspective view thereof, in a typical usage environment;

FIG. 10 is a front plan view thereof, showing an alternate usage configuration;

FIG. 11 is a front perspective view thereof;


FIG. 12 is a front perspective view thereof, in a typical usage environment;

FIG. 13 is a front plan view of a second embodiment of an inflation device display, showing our new design;

FIG. 14 is a front perspective view thereof; and,

FIG. 15 is a front perspective view thereof, in a typical usage environment.

1 Claim, 15 Drawing Sheets

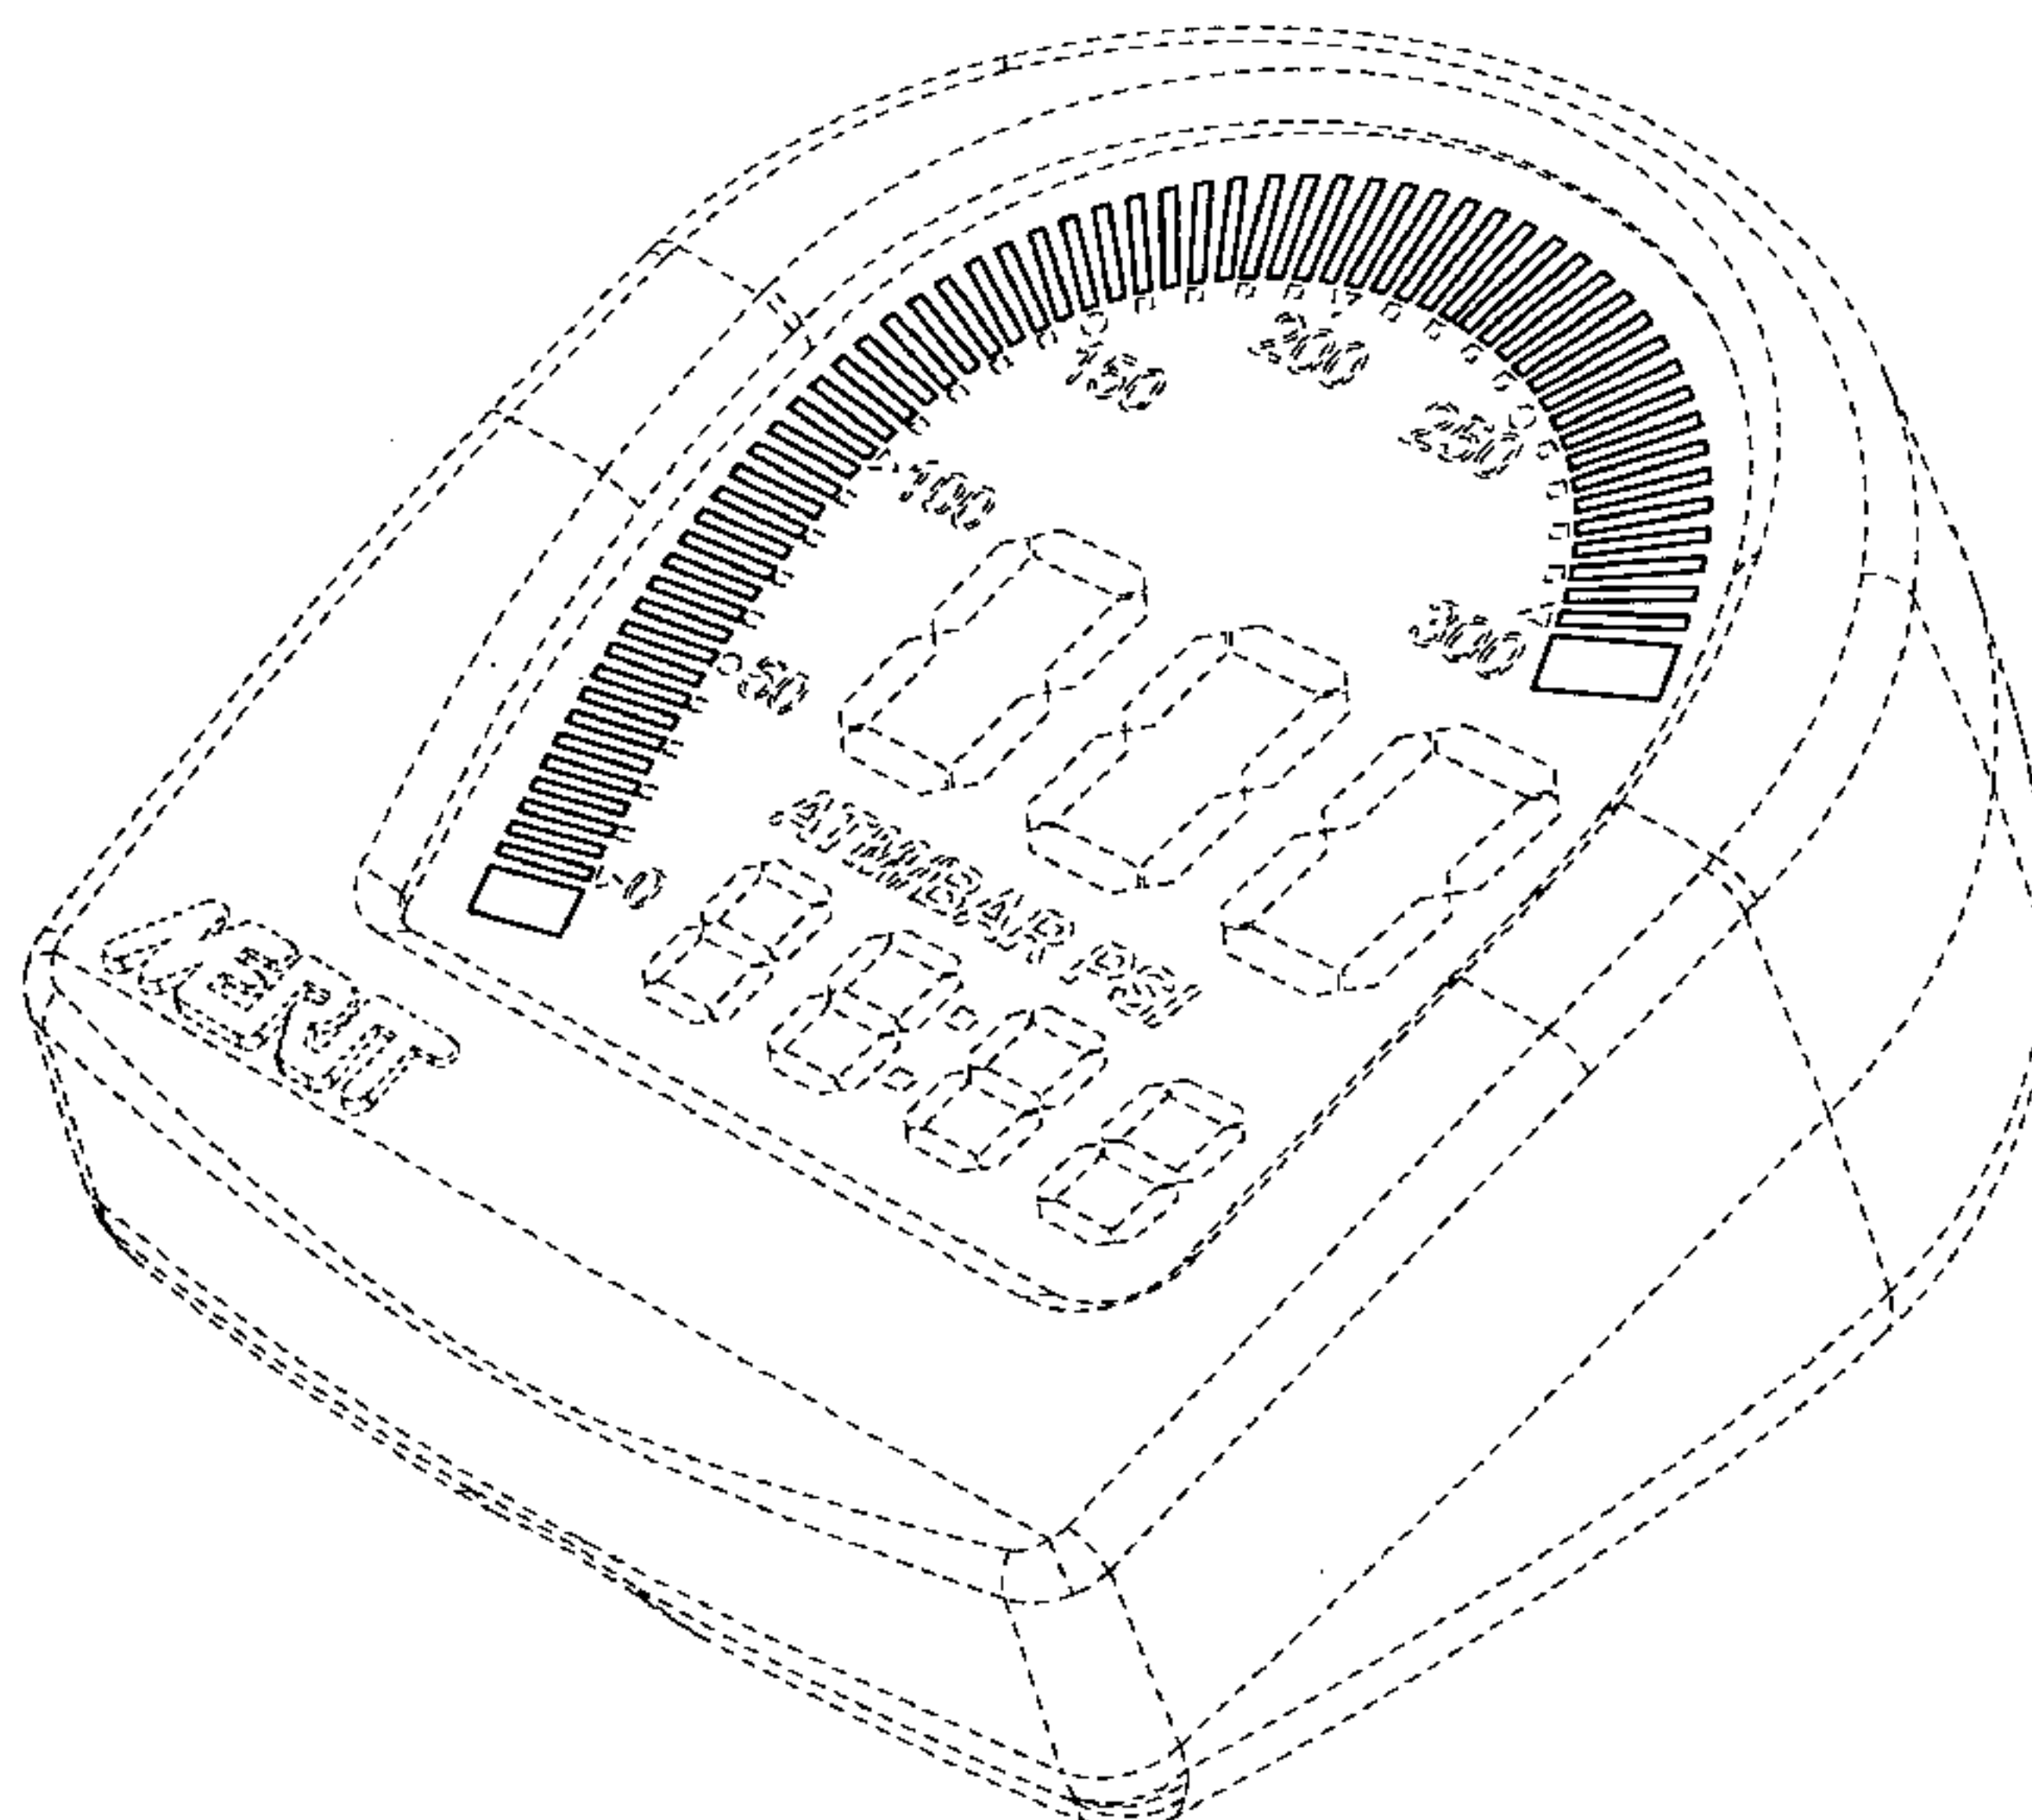

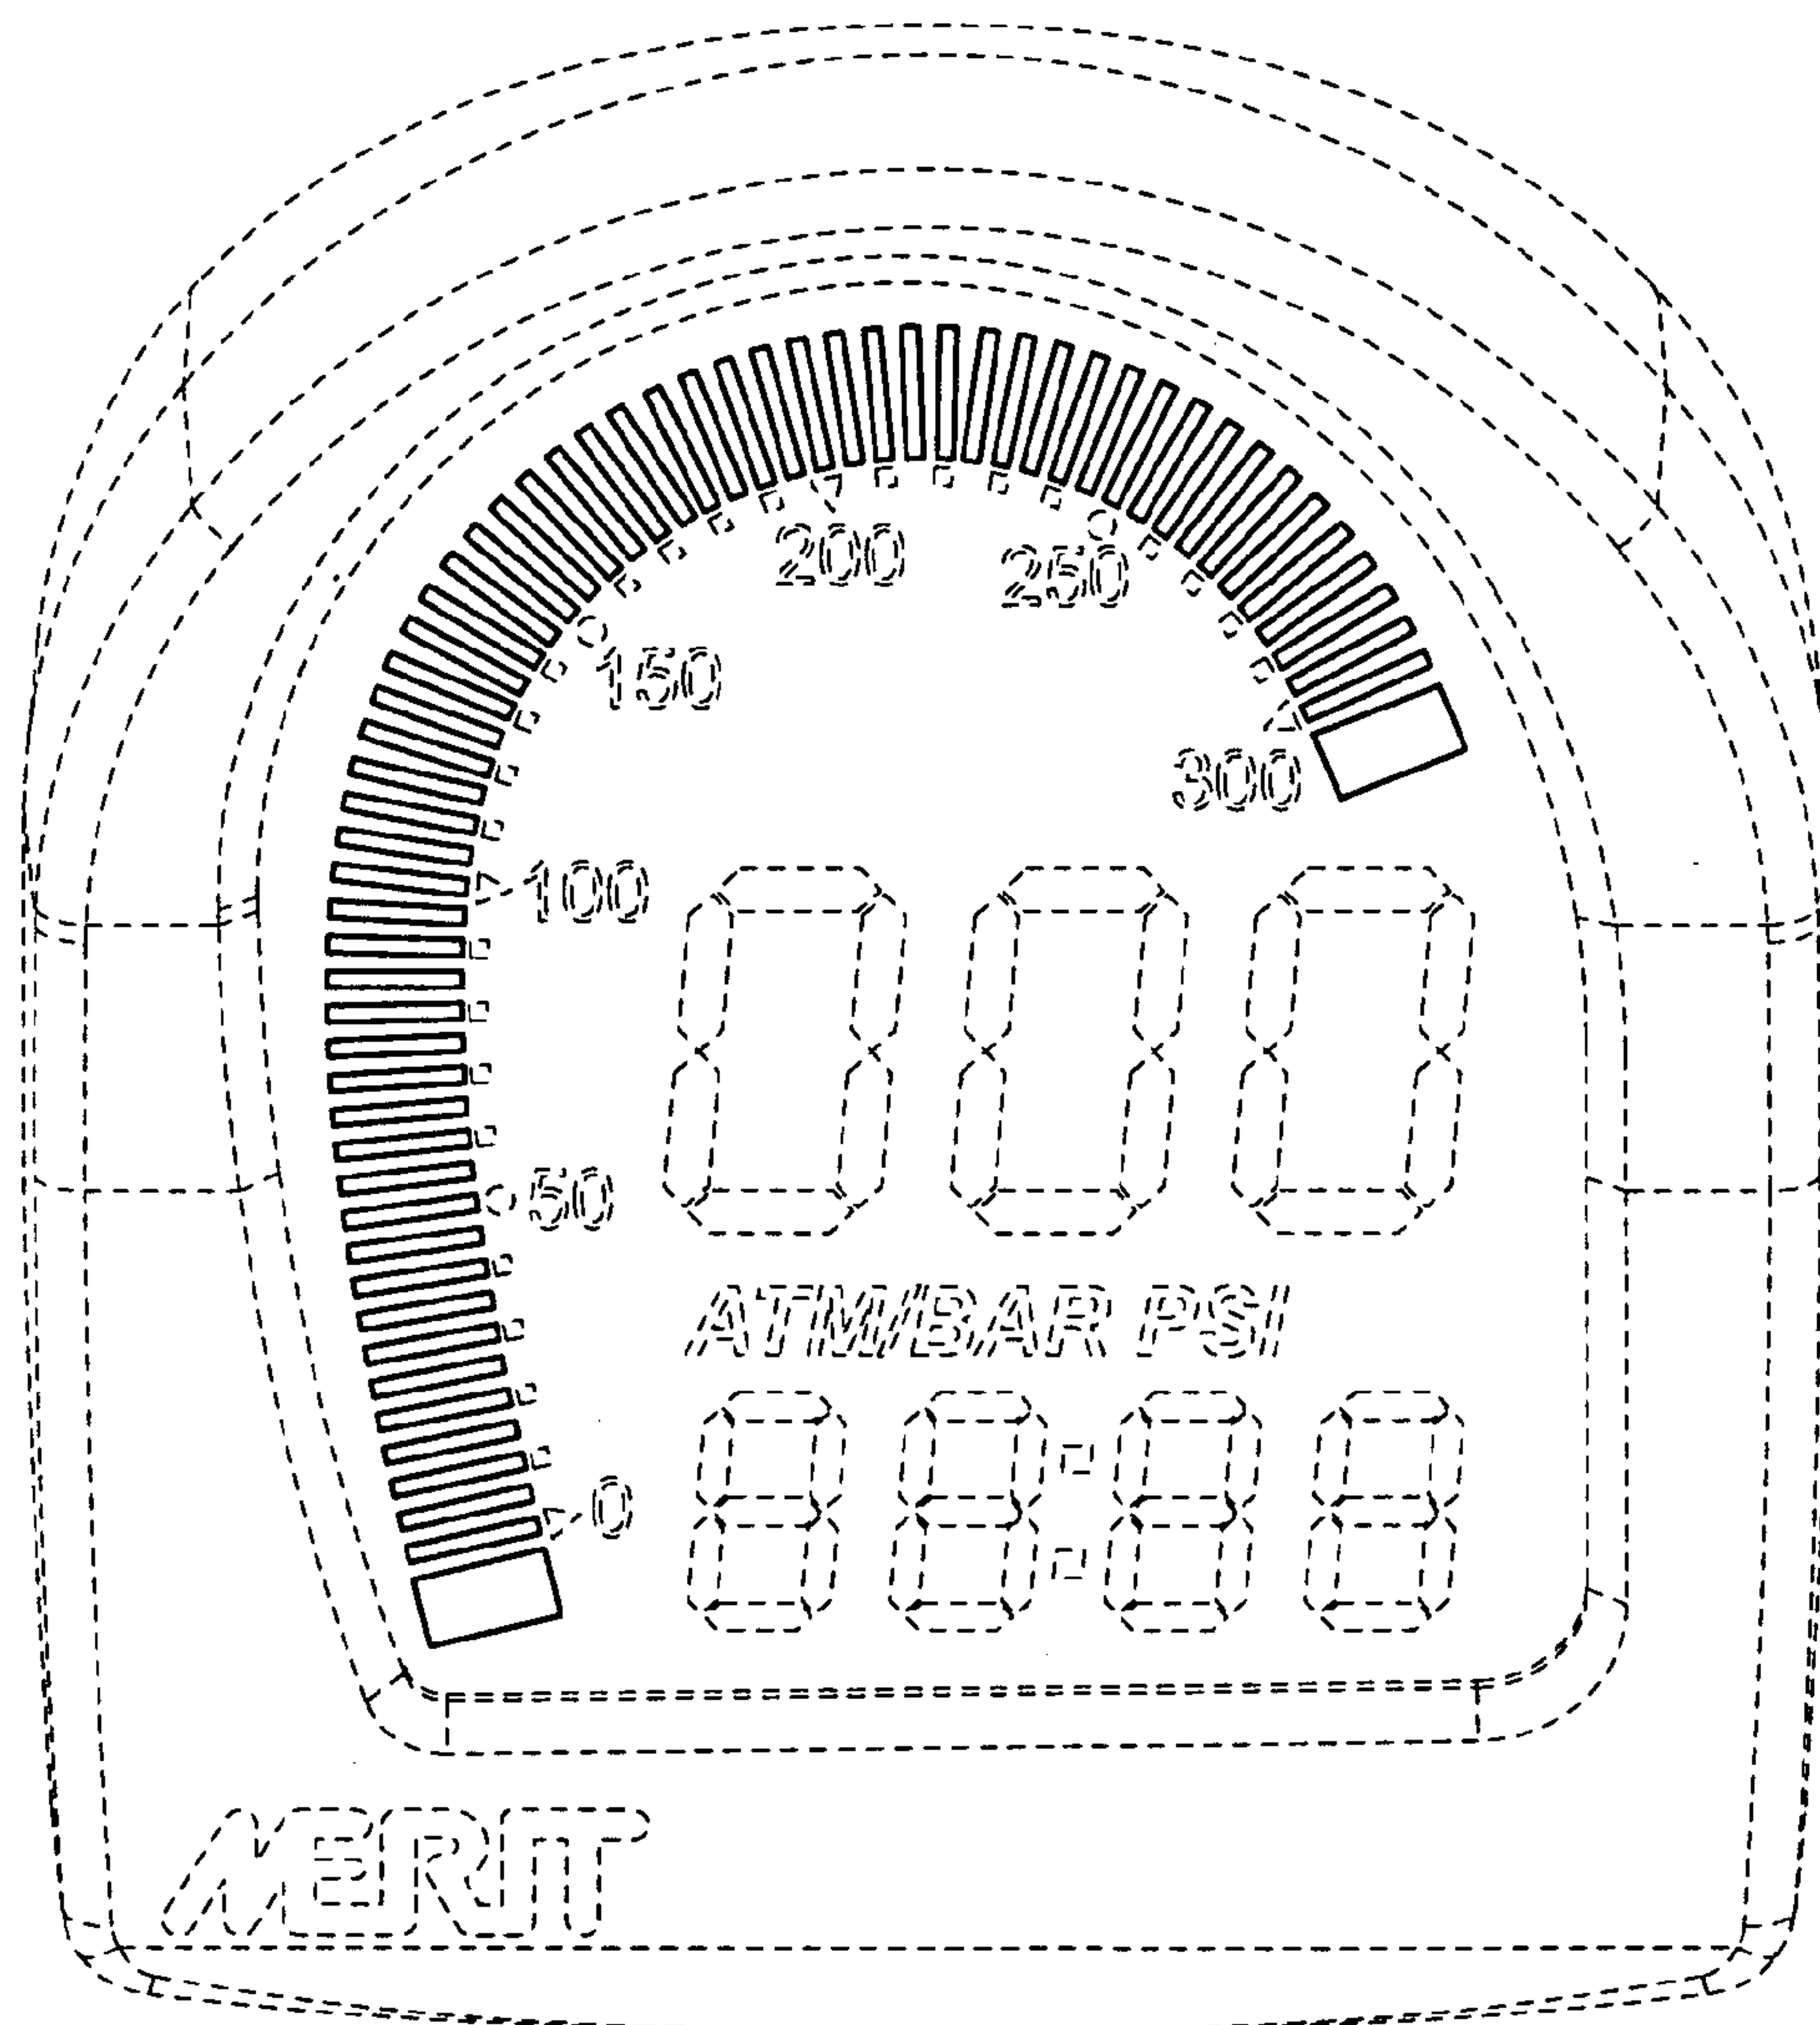
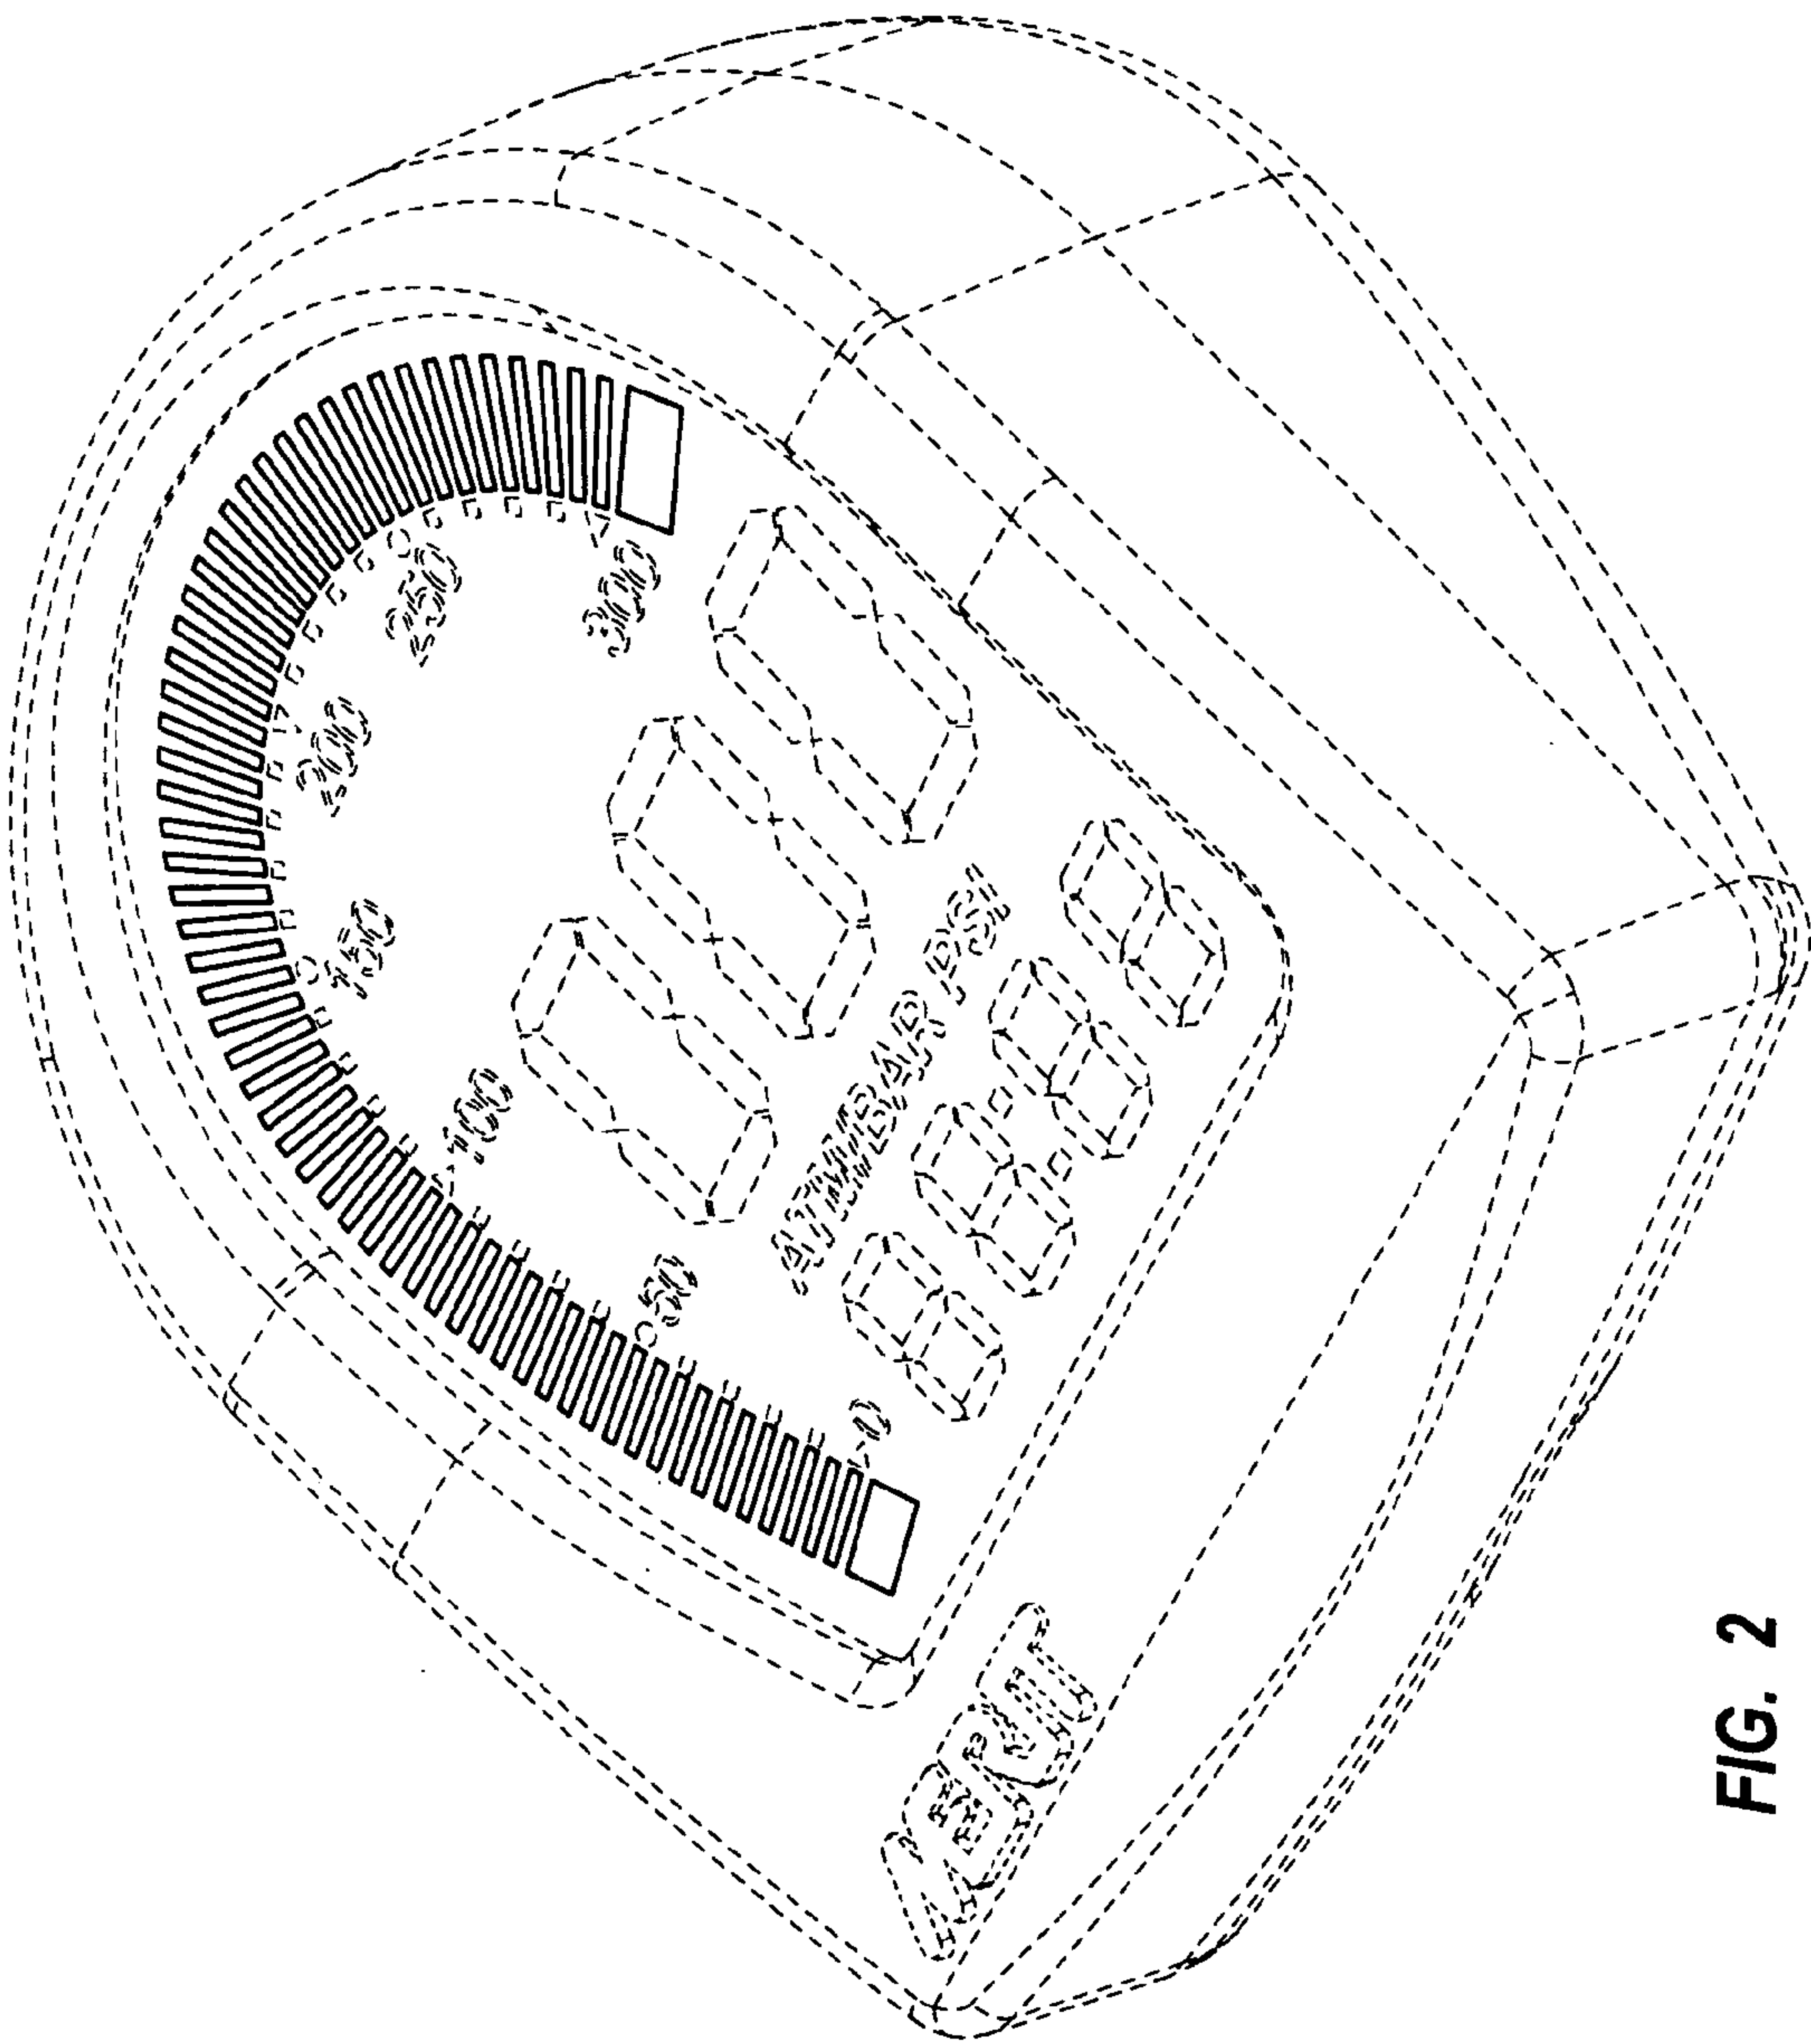


FIG. 1



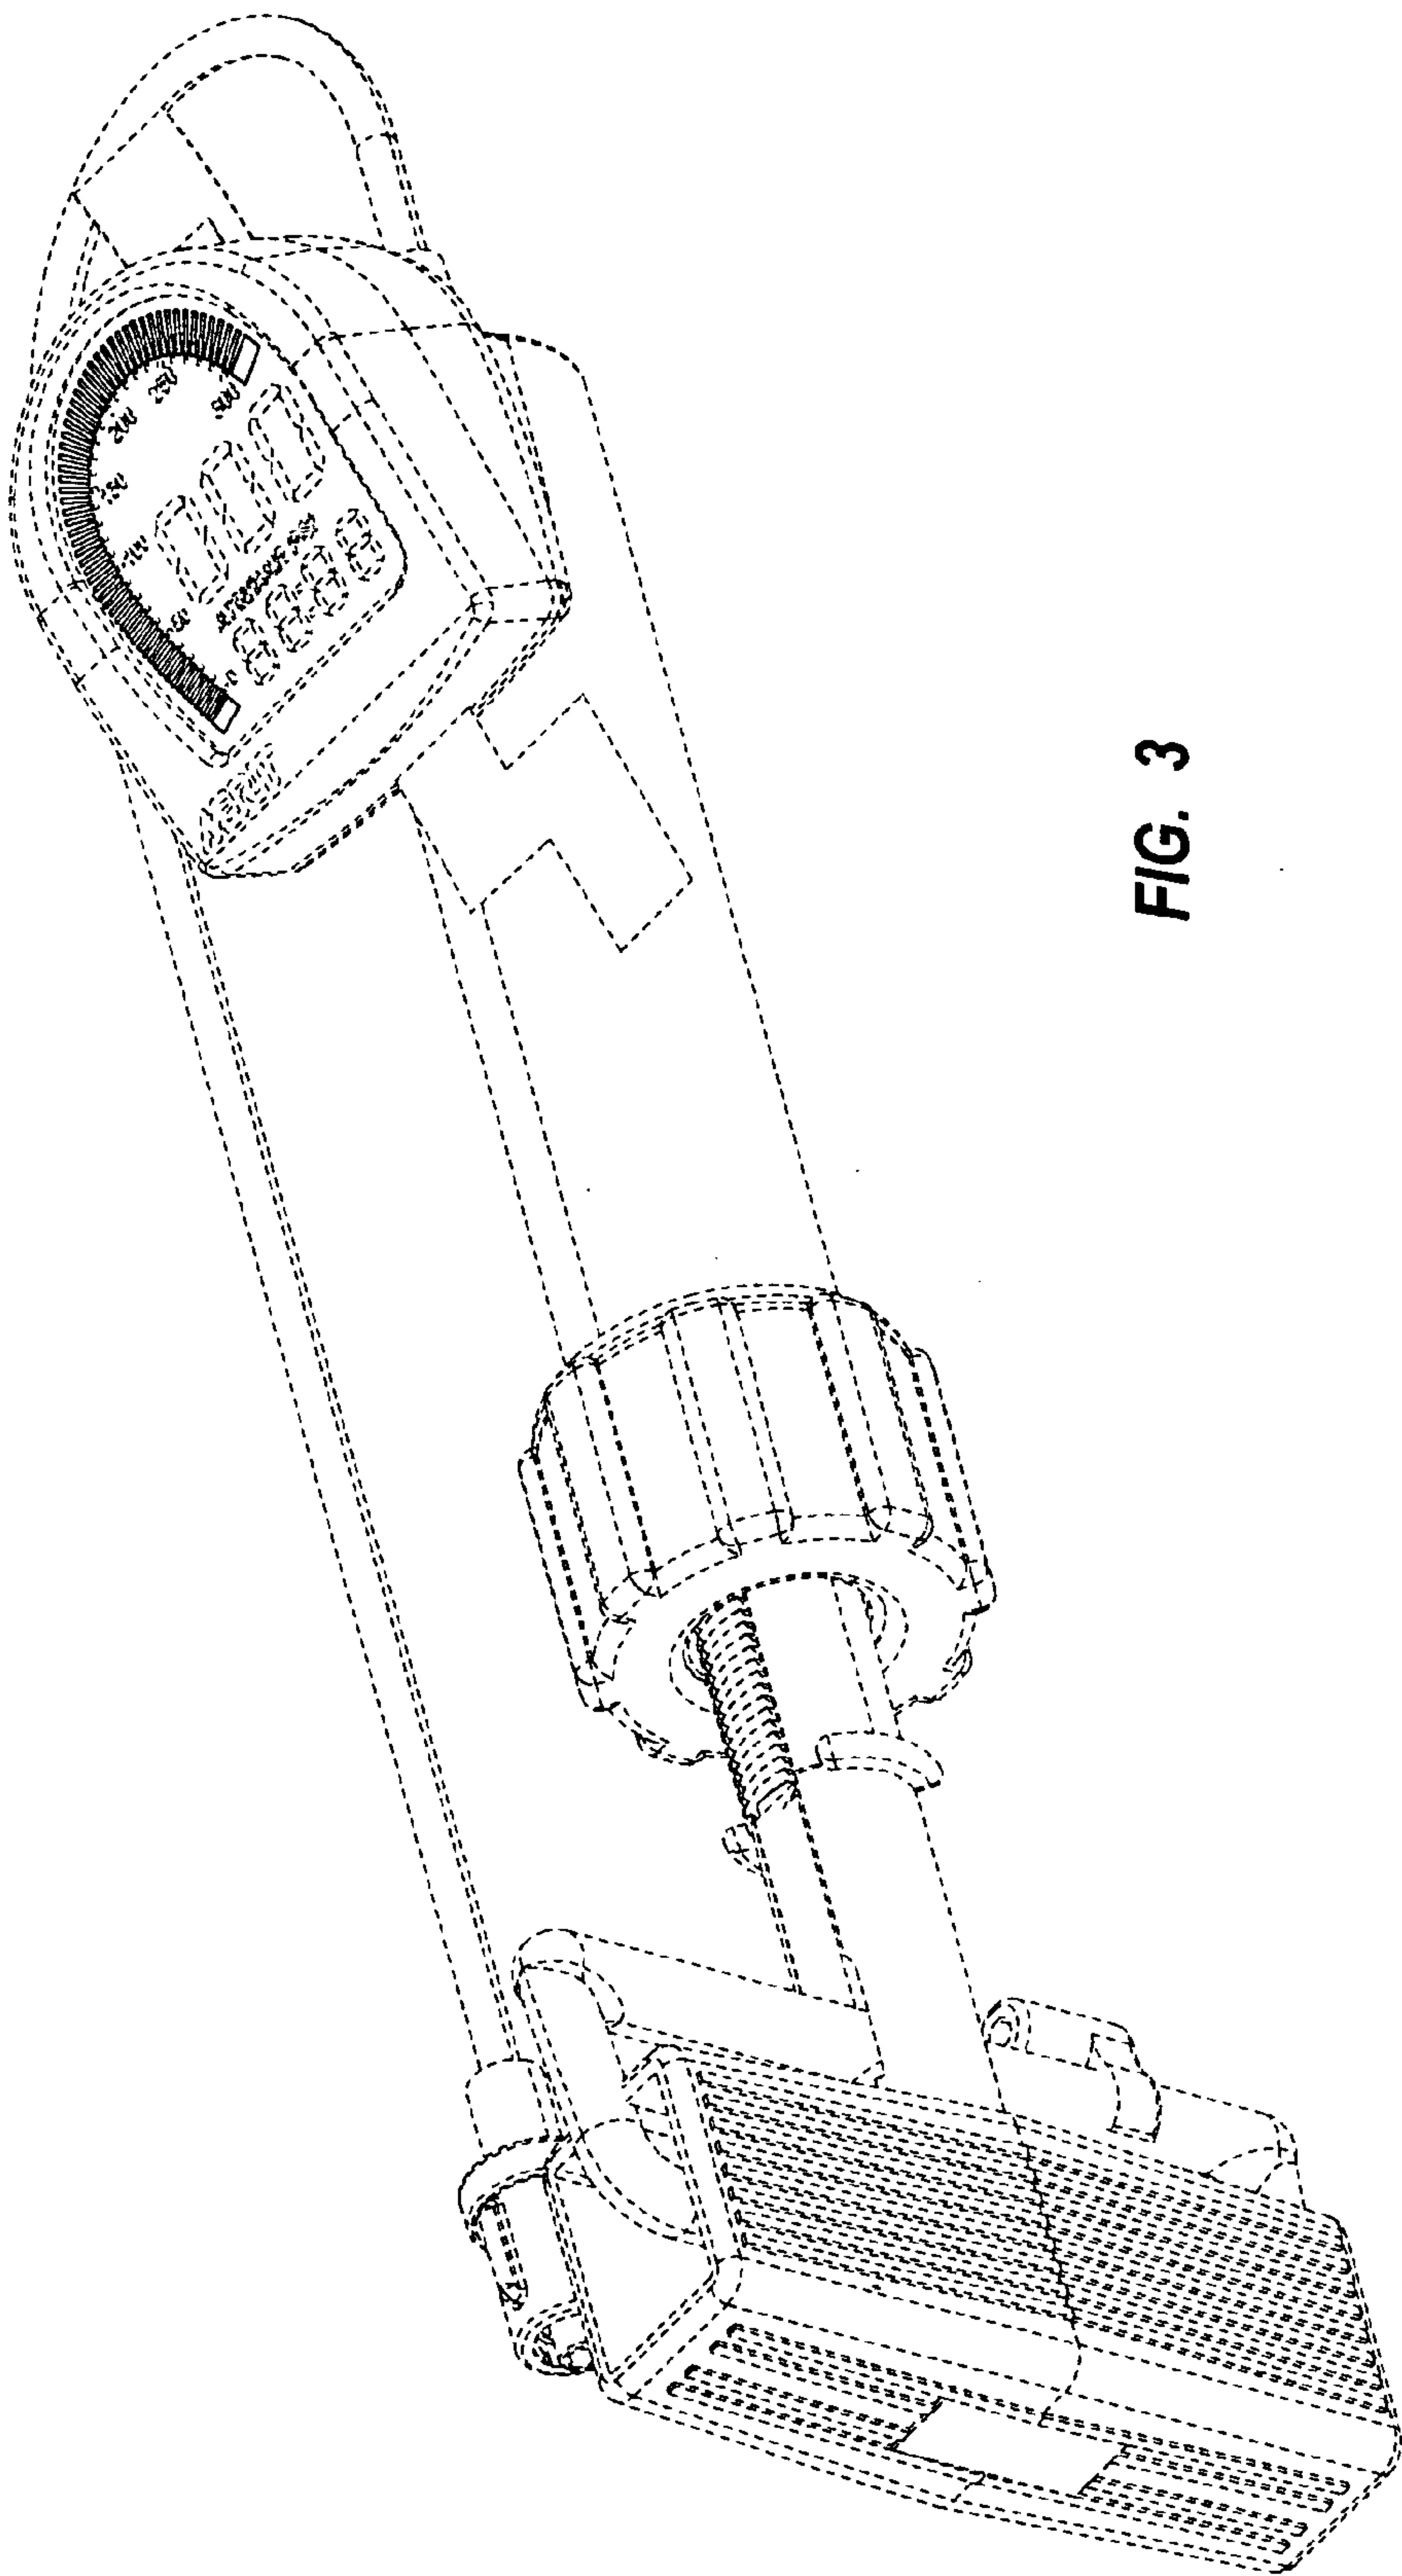


FIG. 3

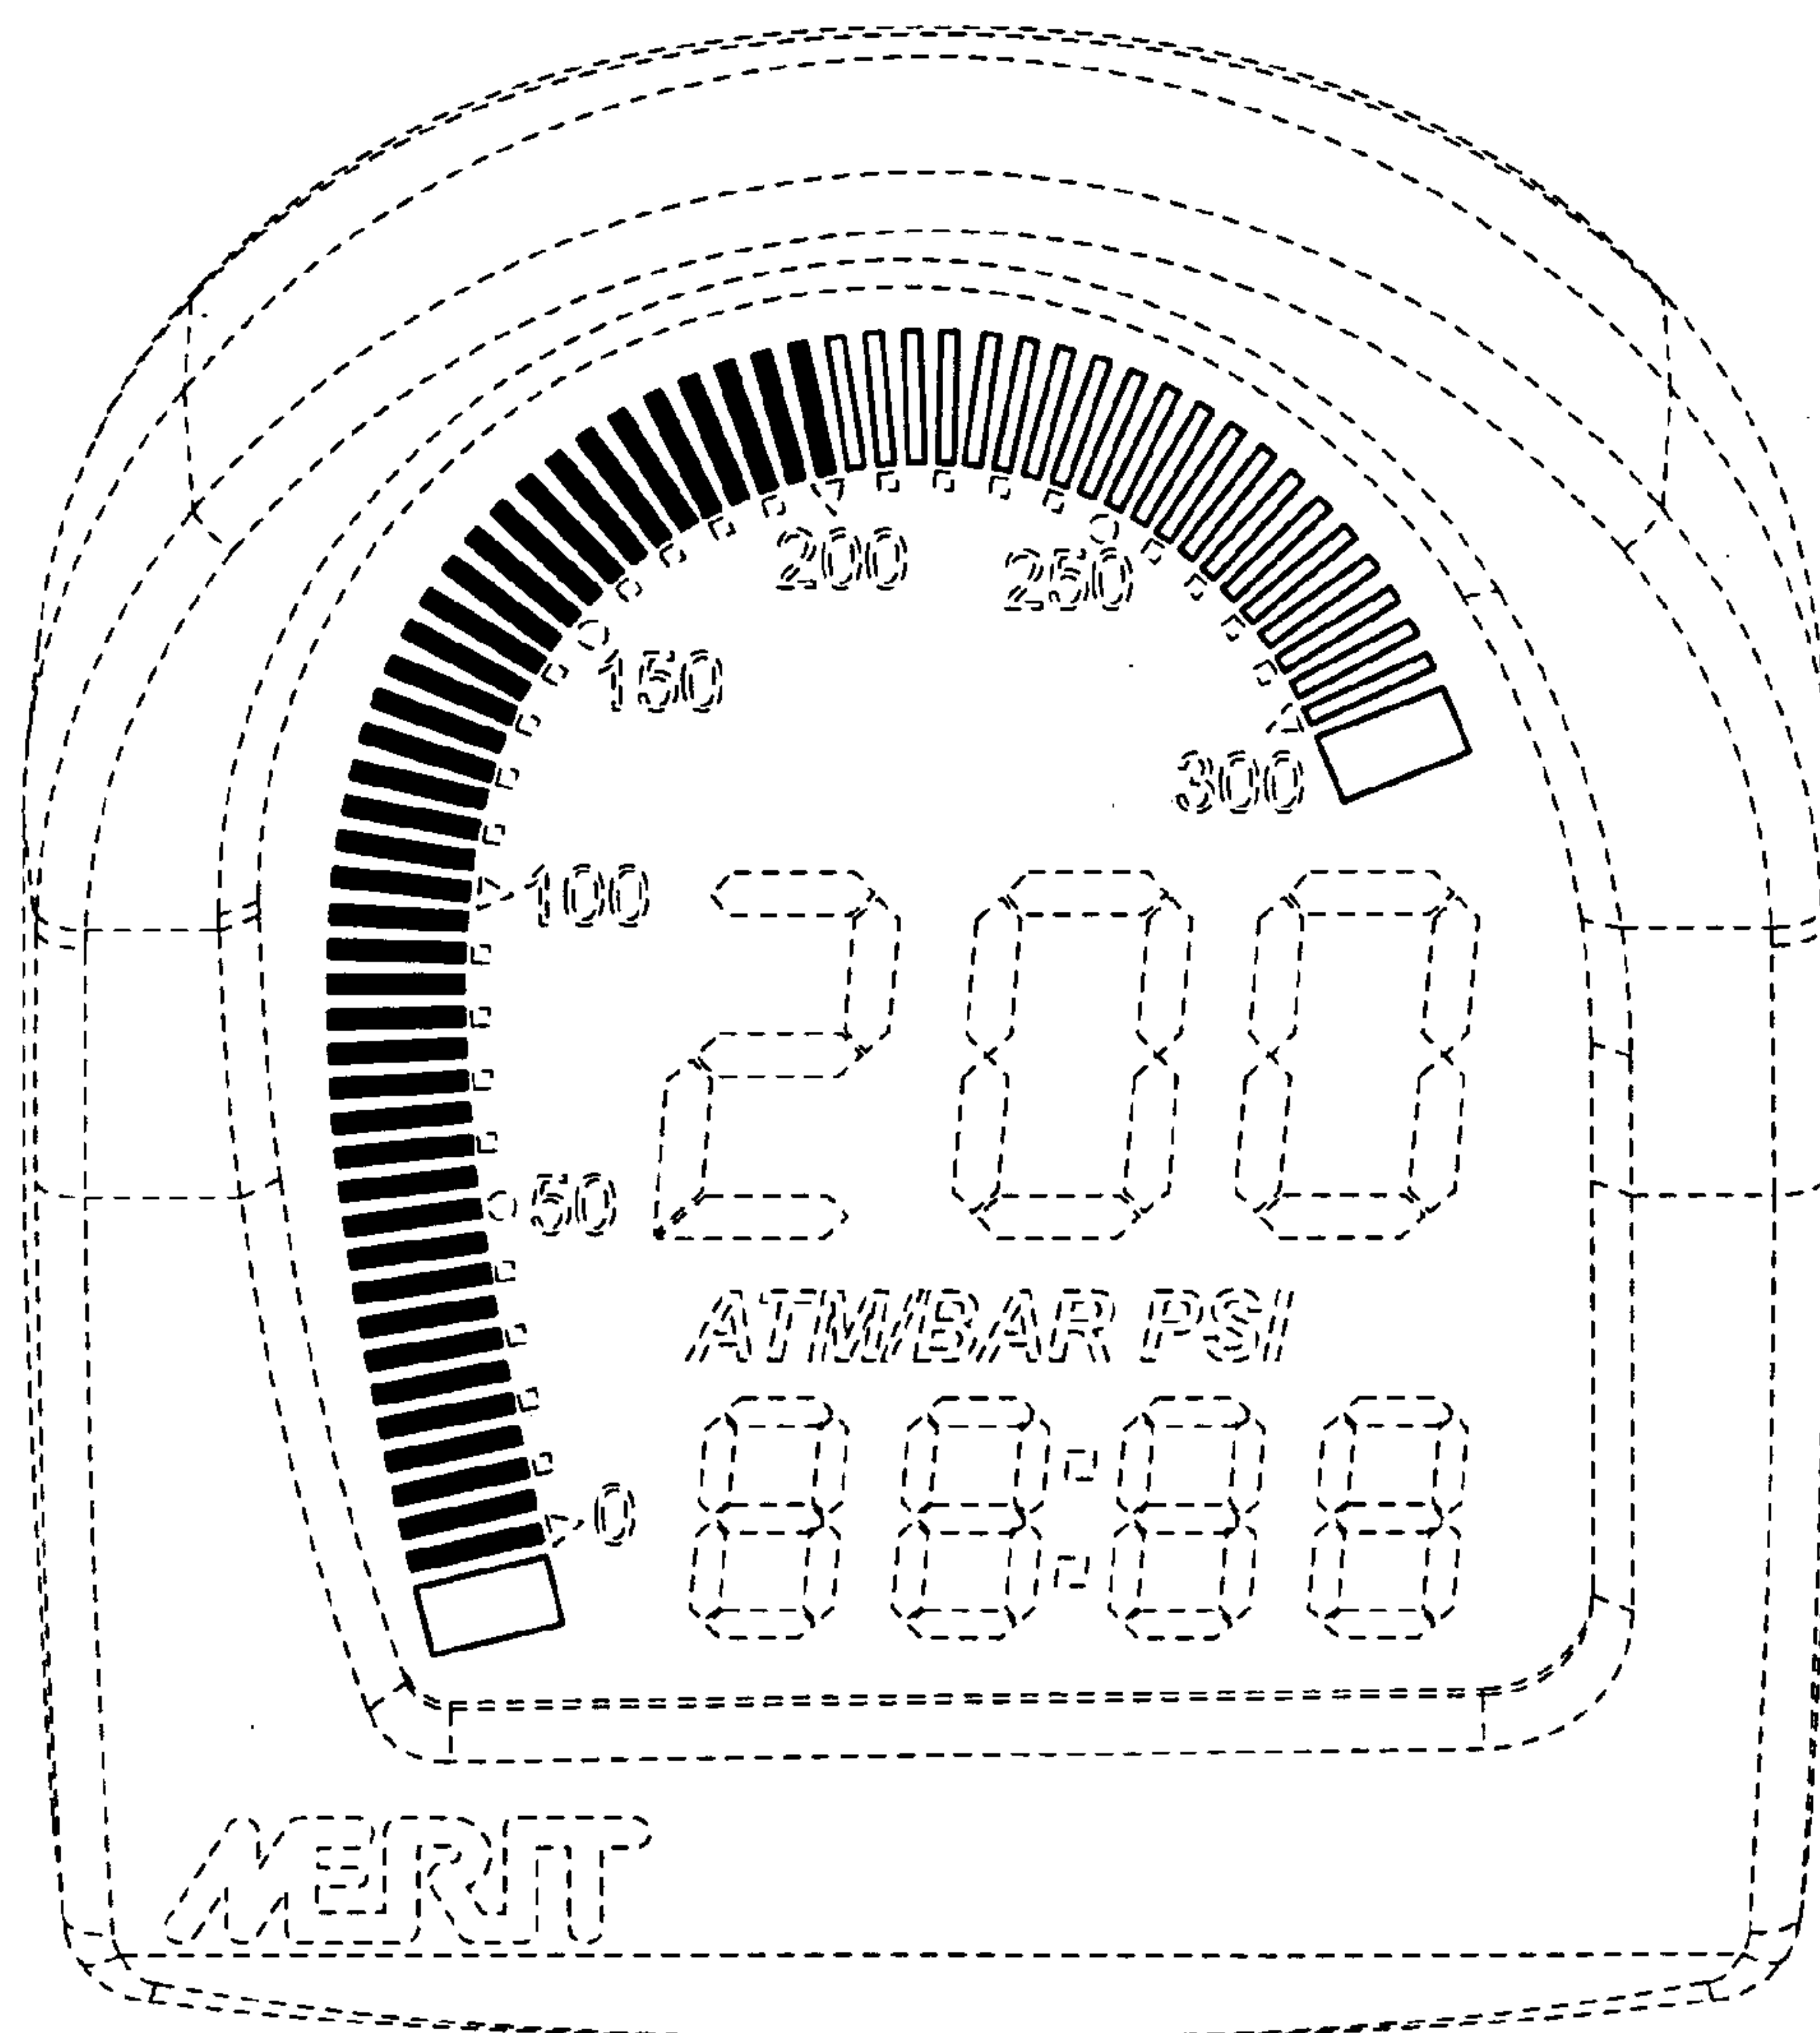


FIG. 4

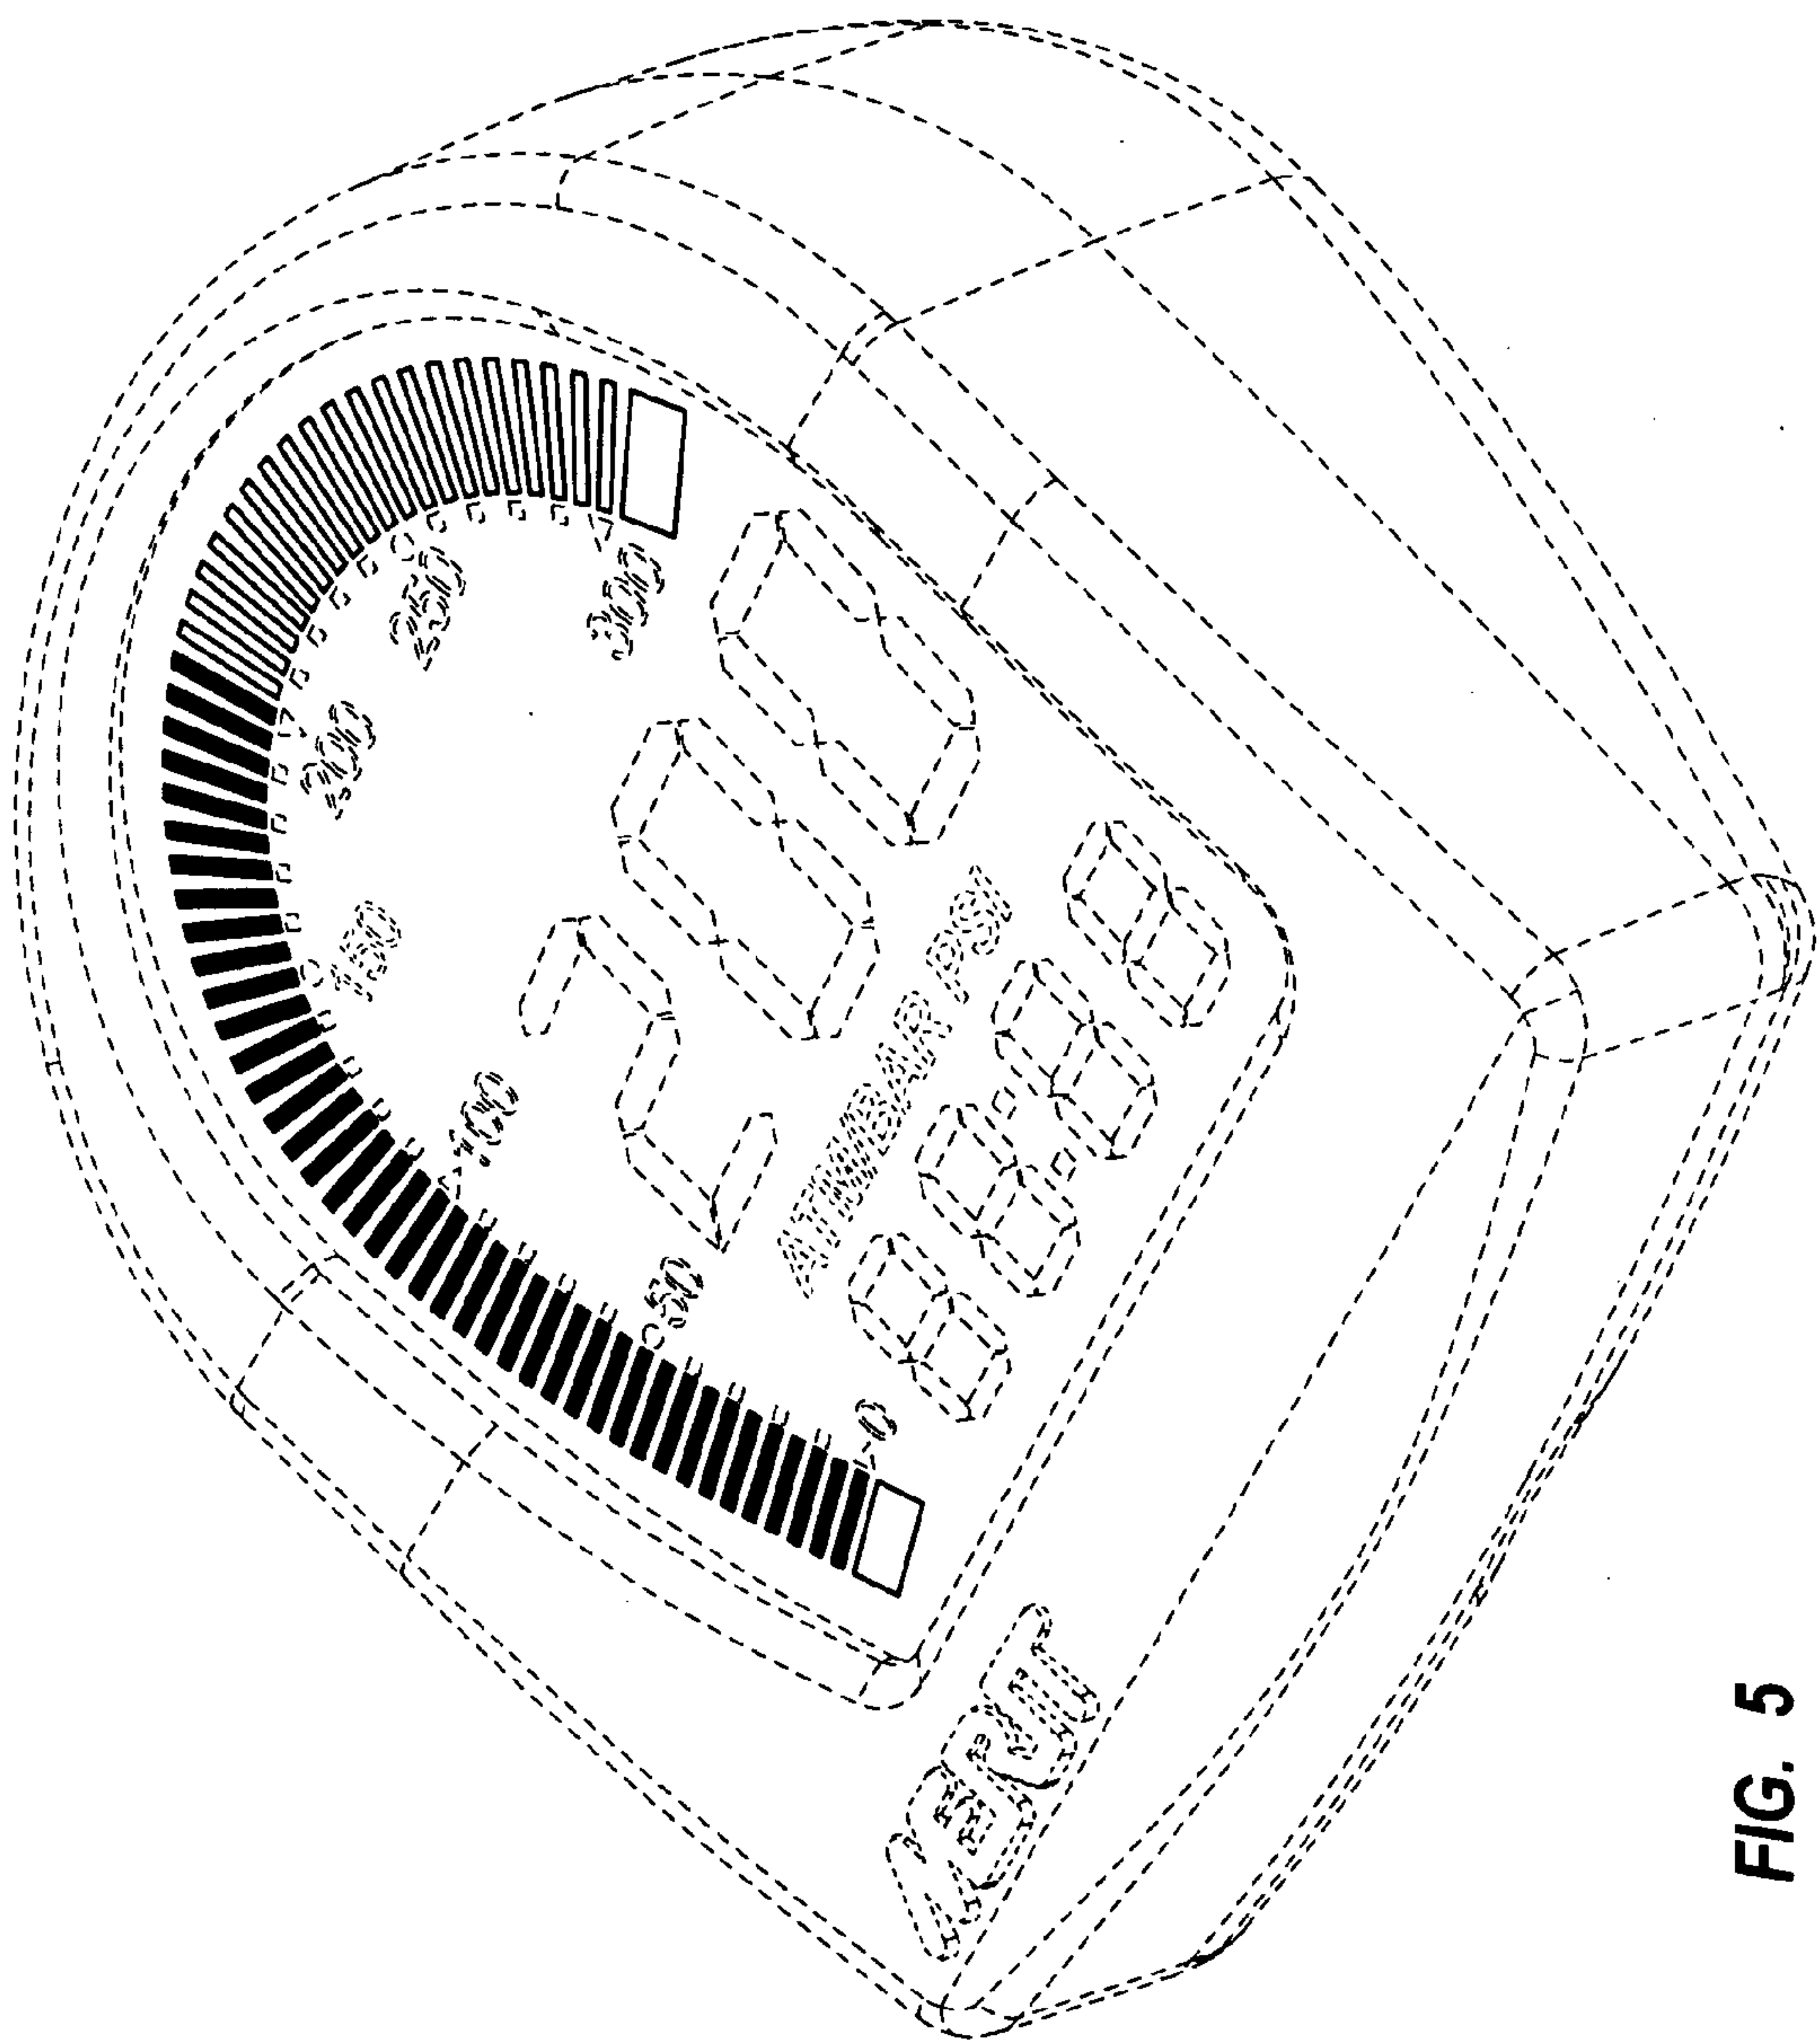


FIG. 5

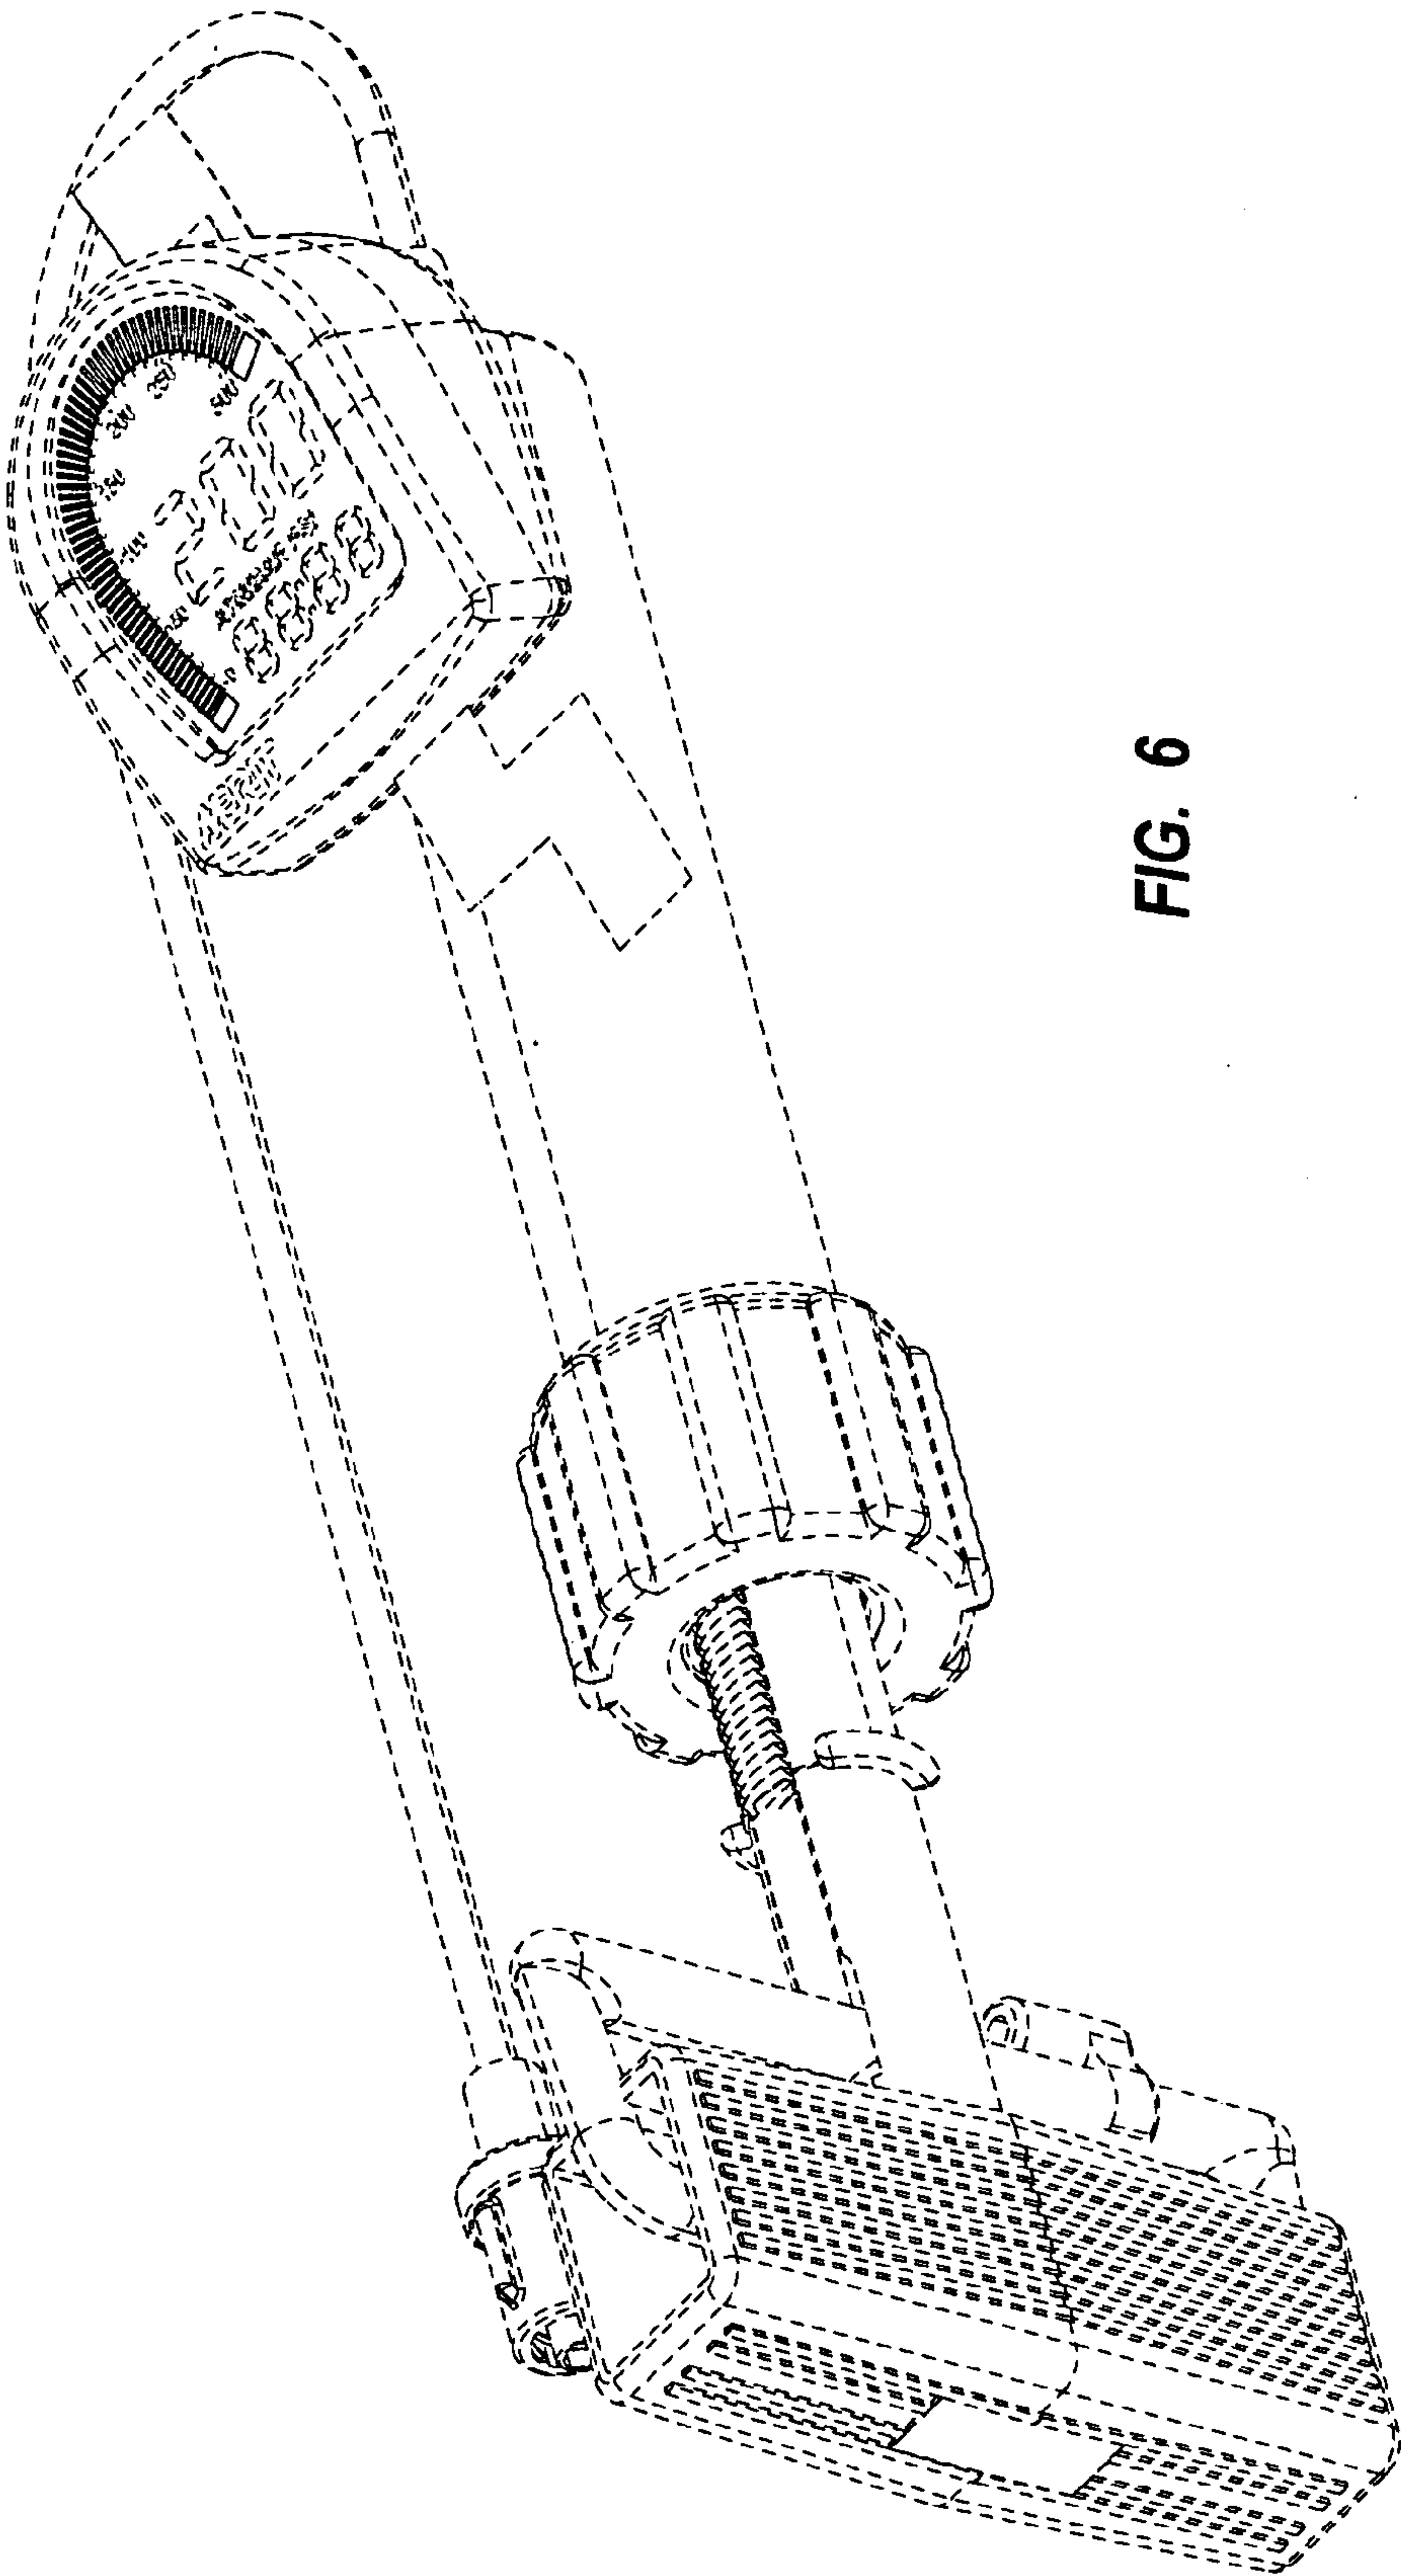


FIG. 6

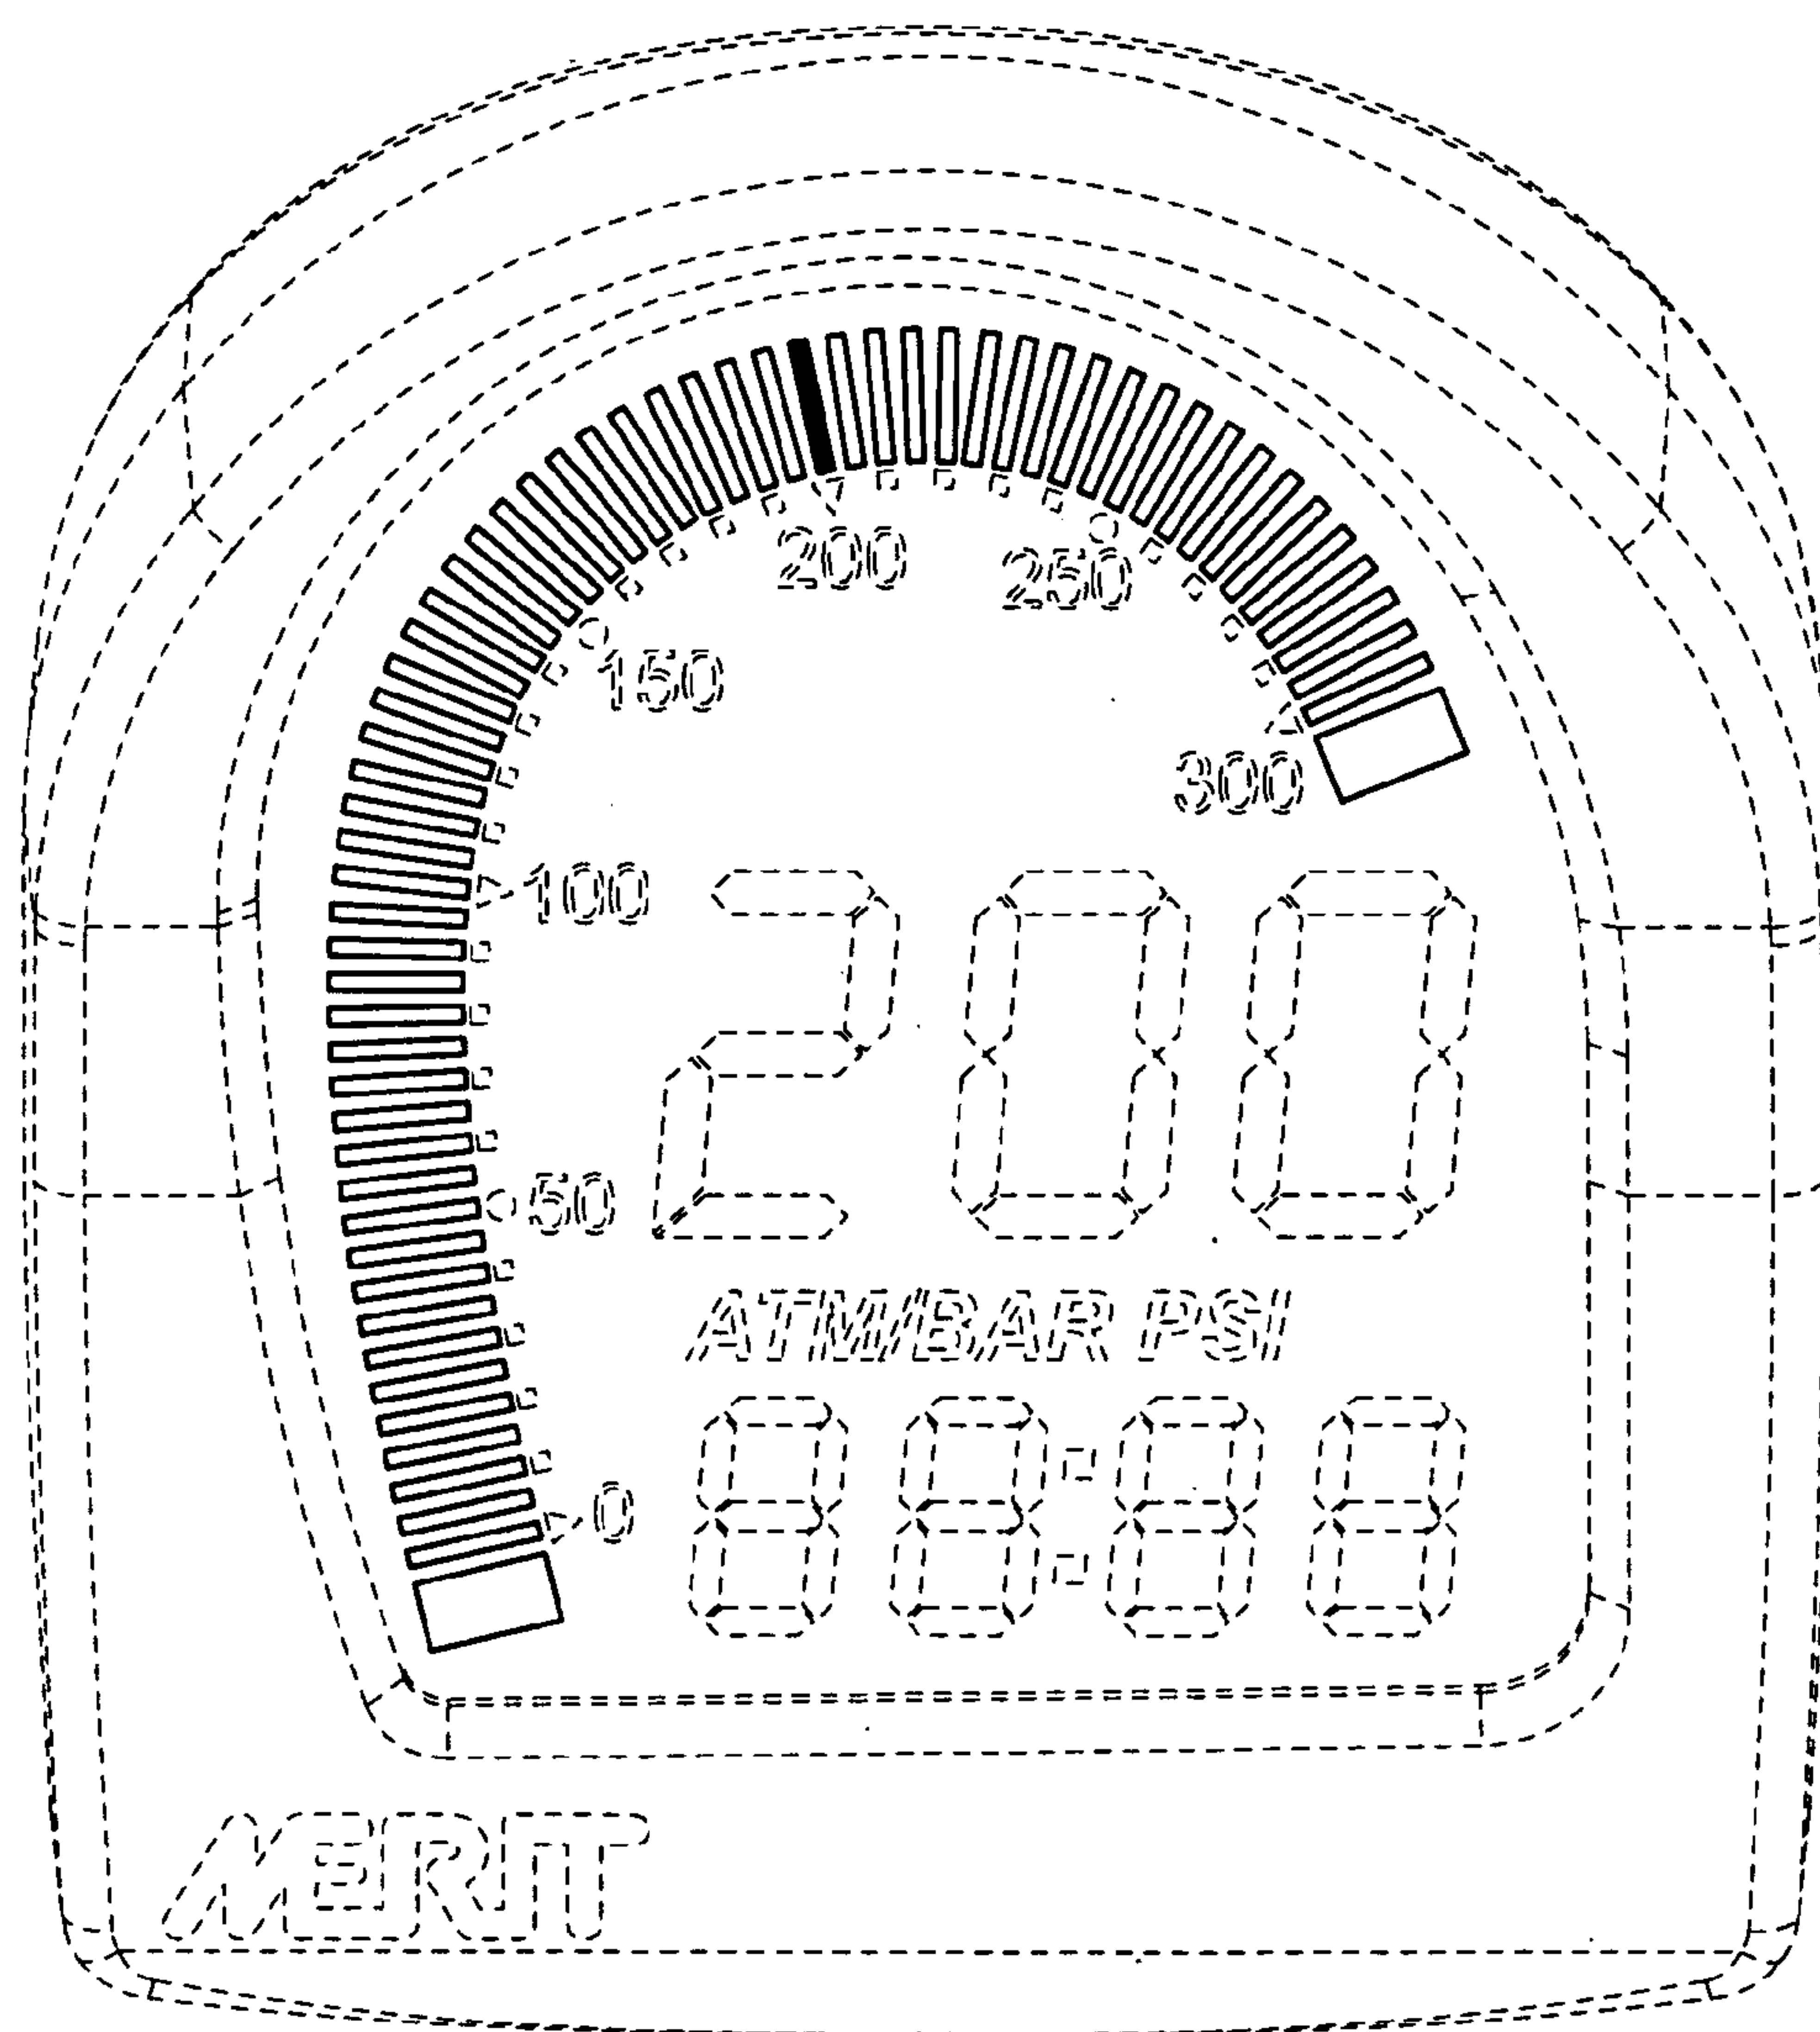


FIG. 7

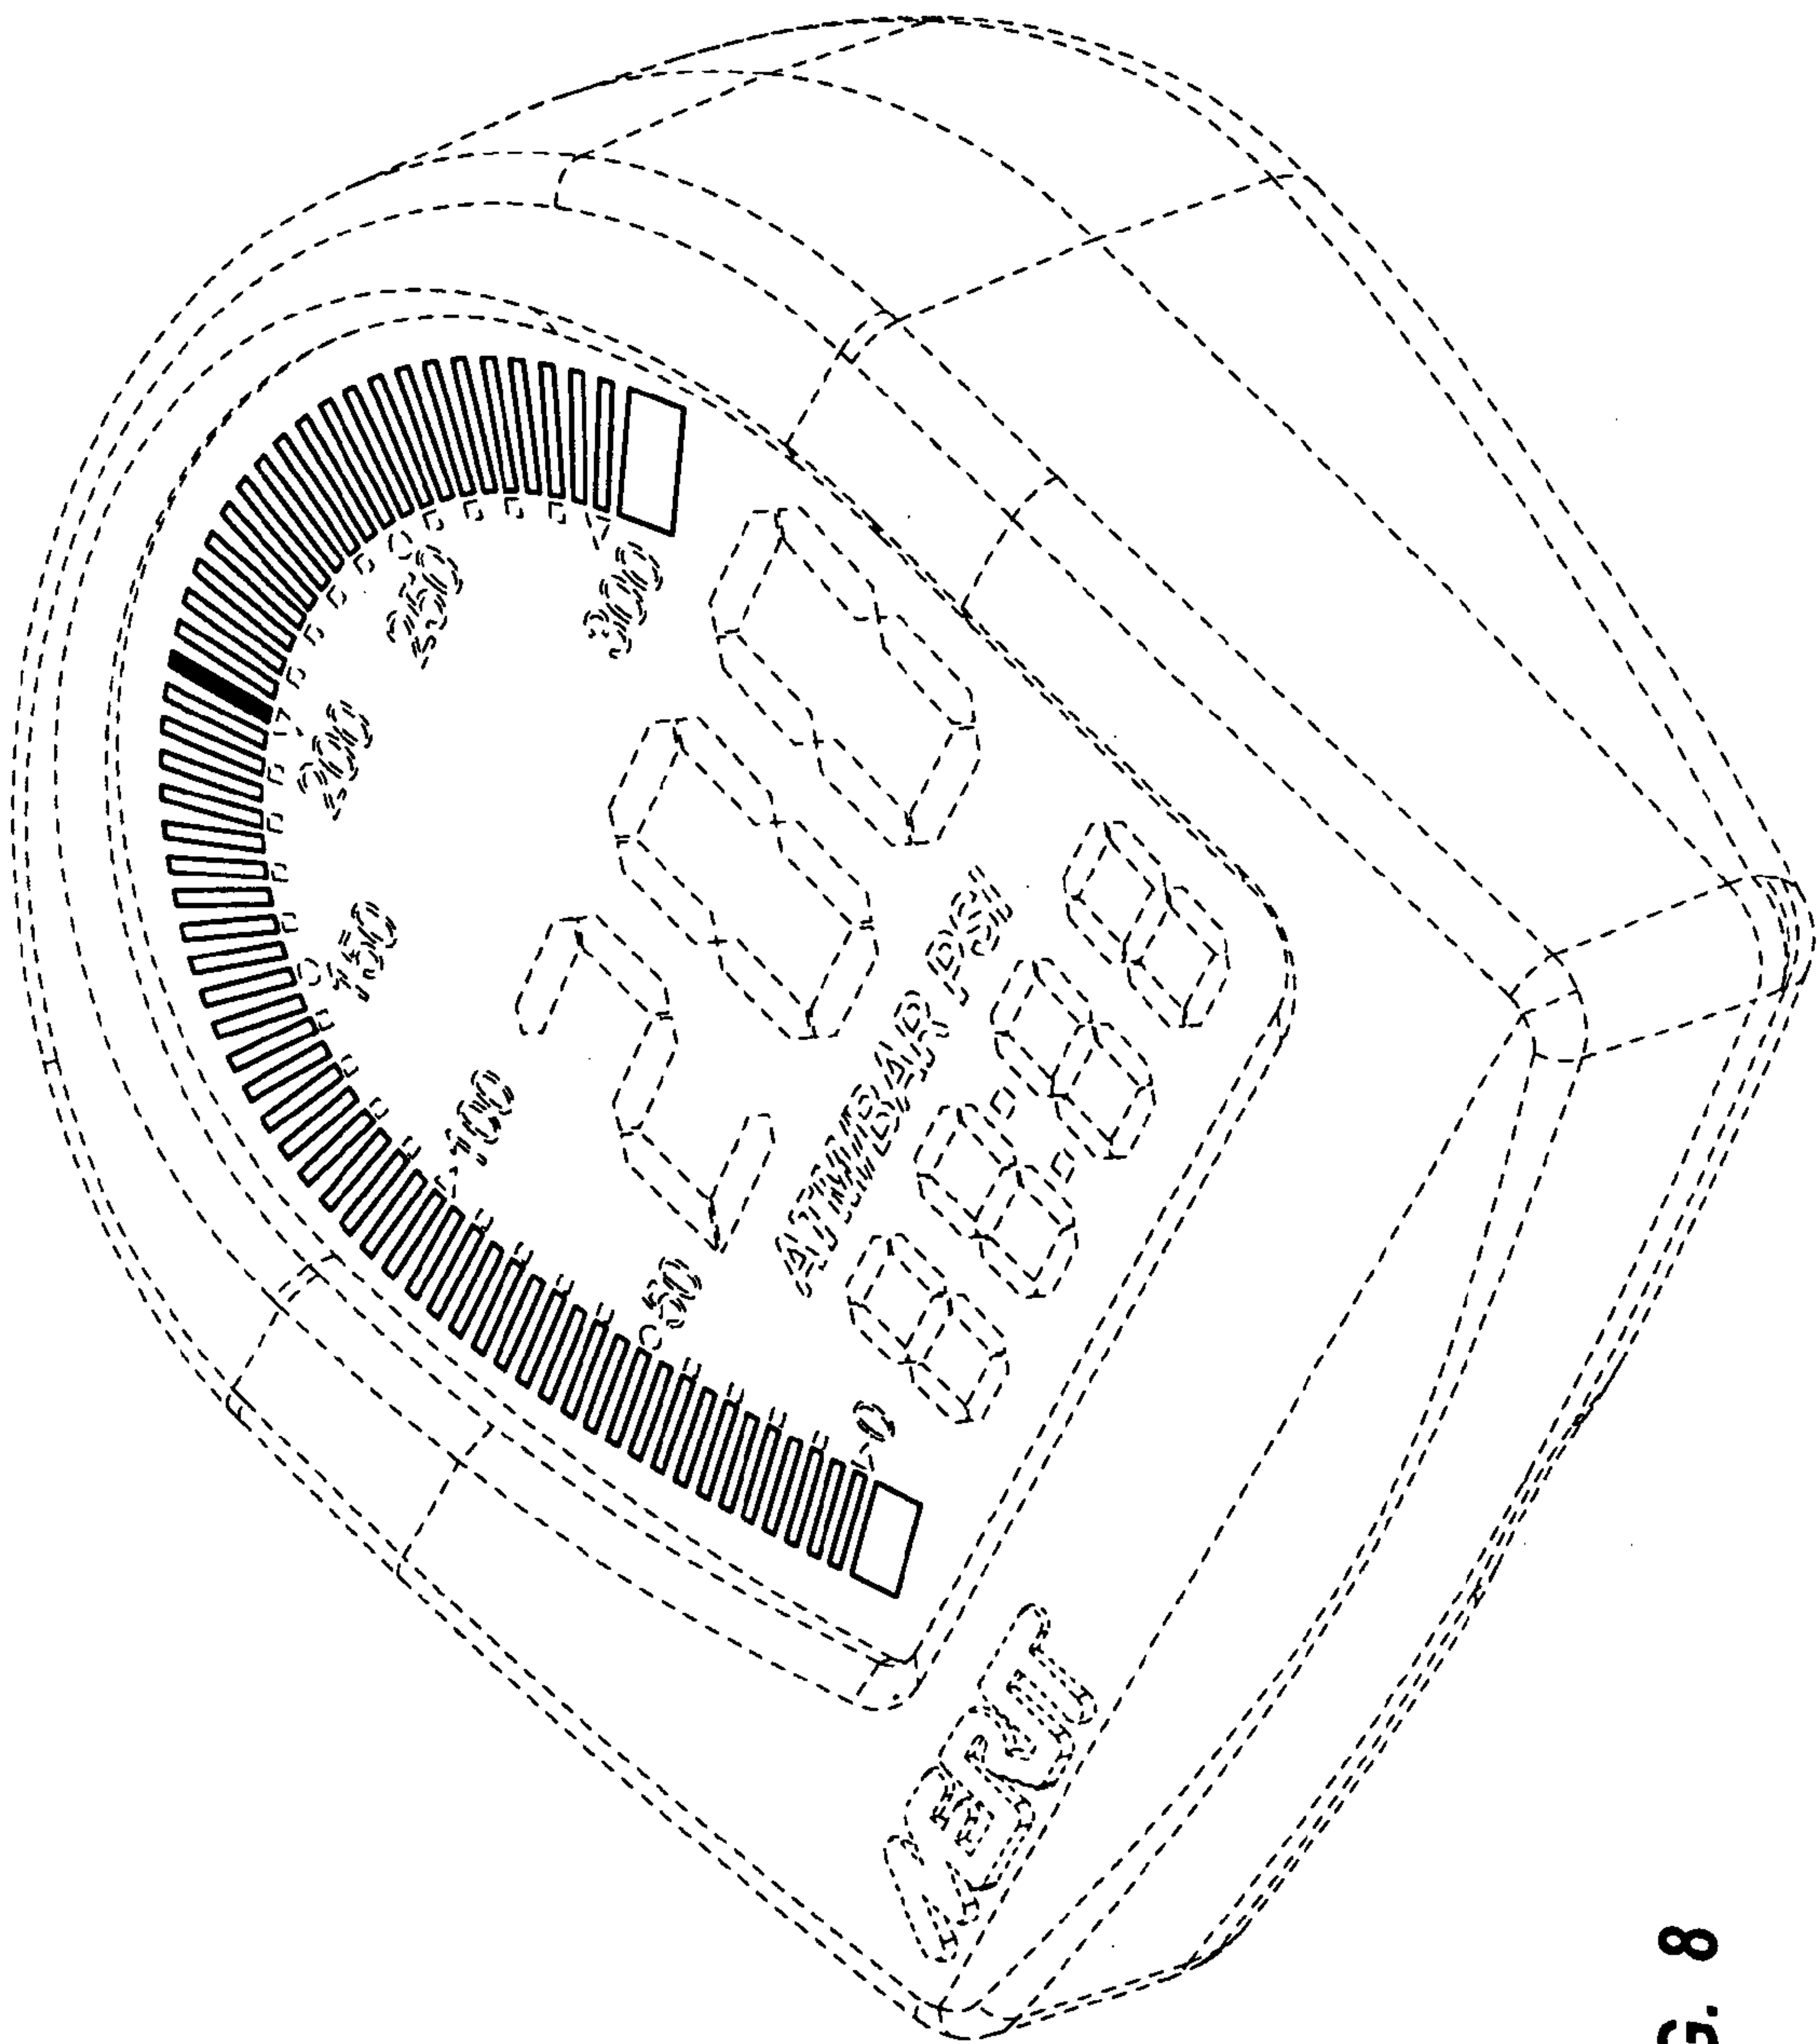


FIG. 8

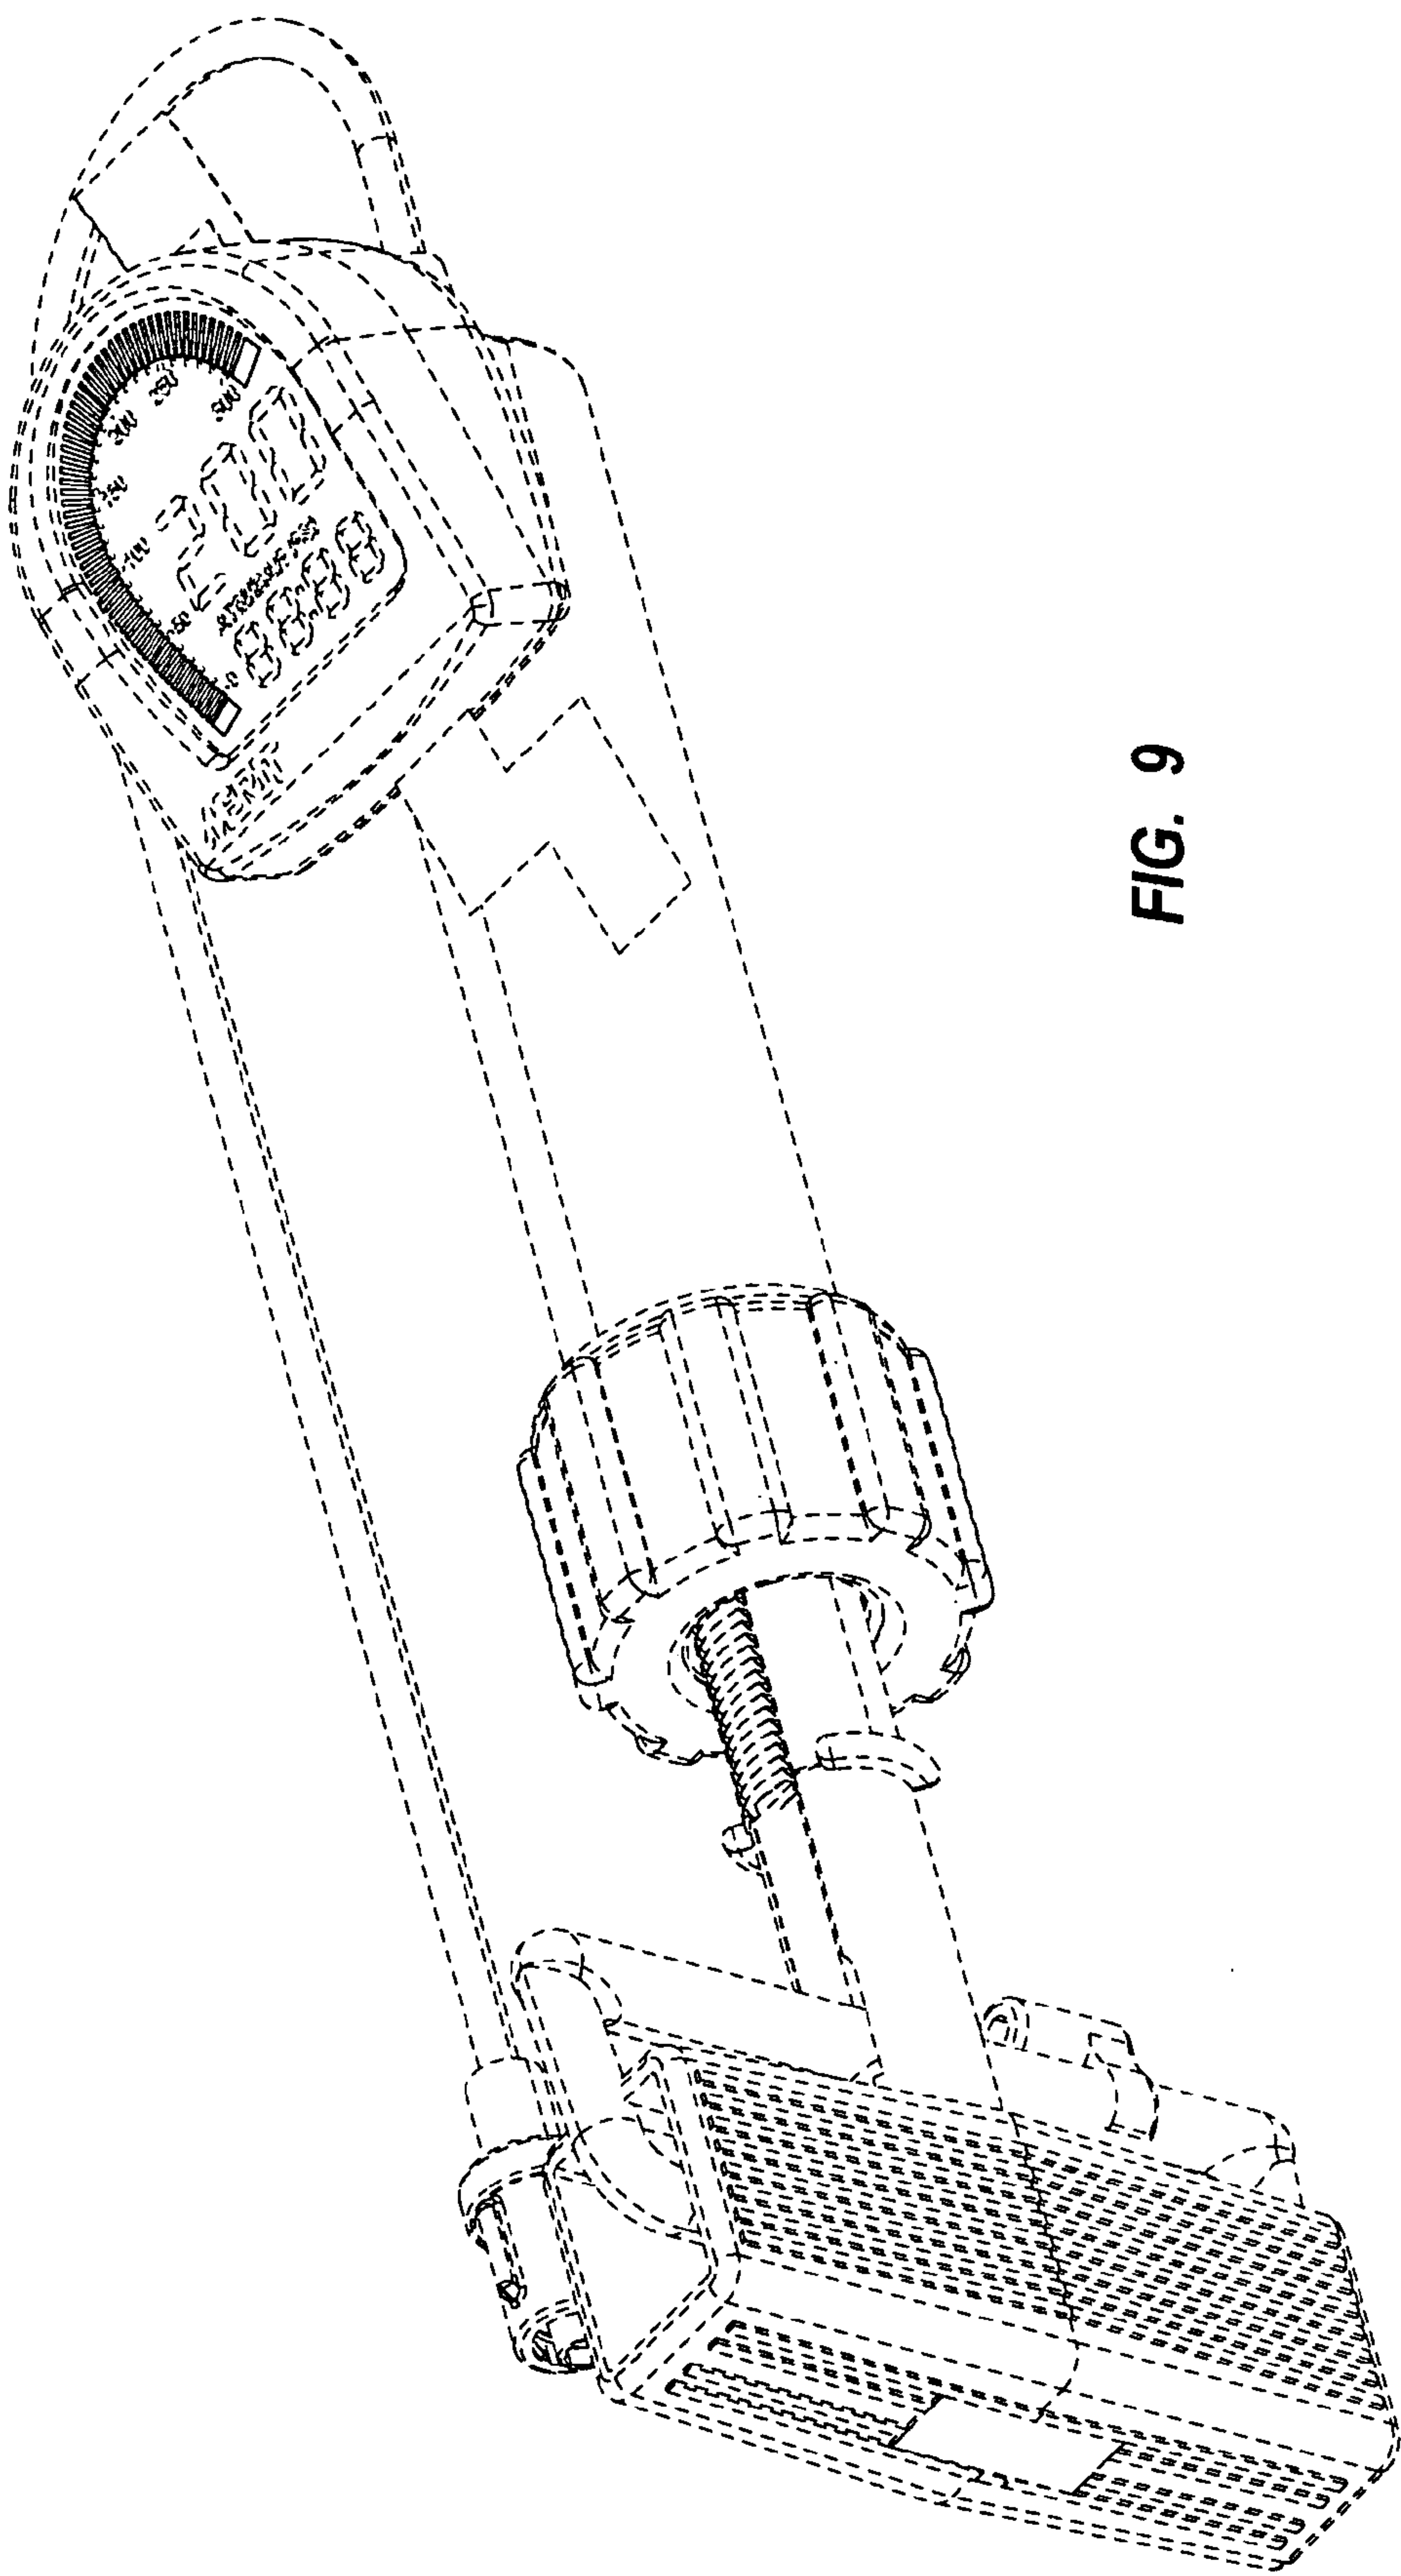


FIG. 9

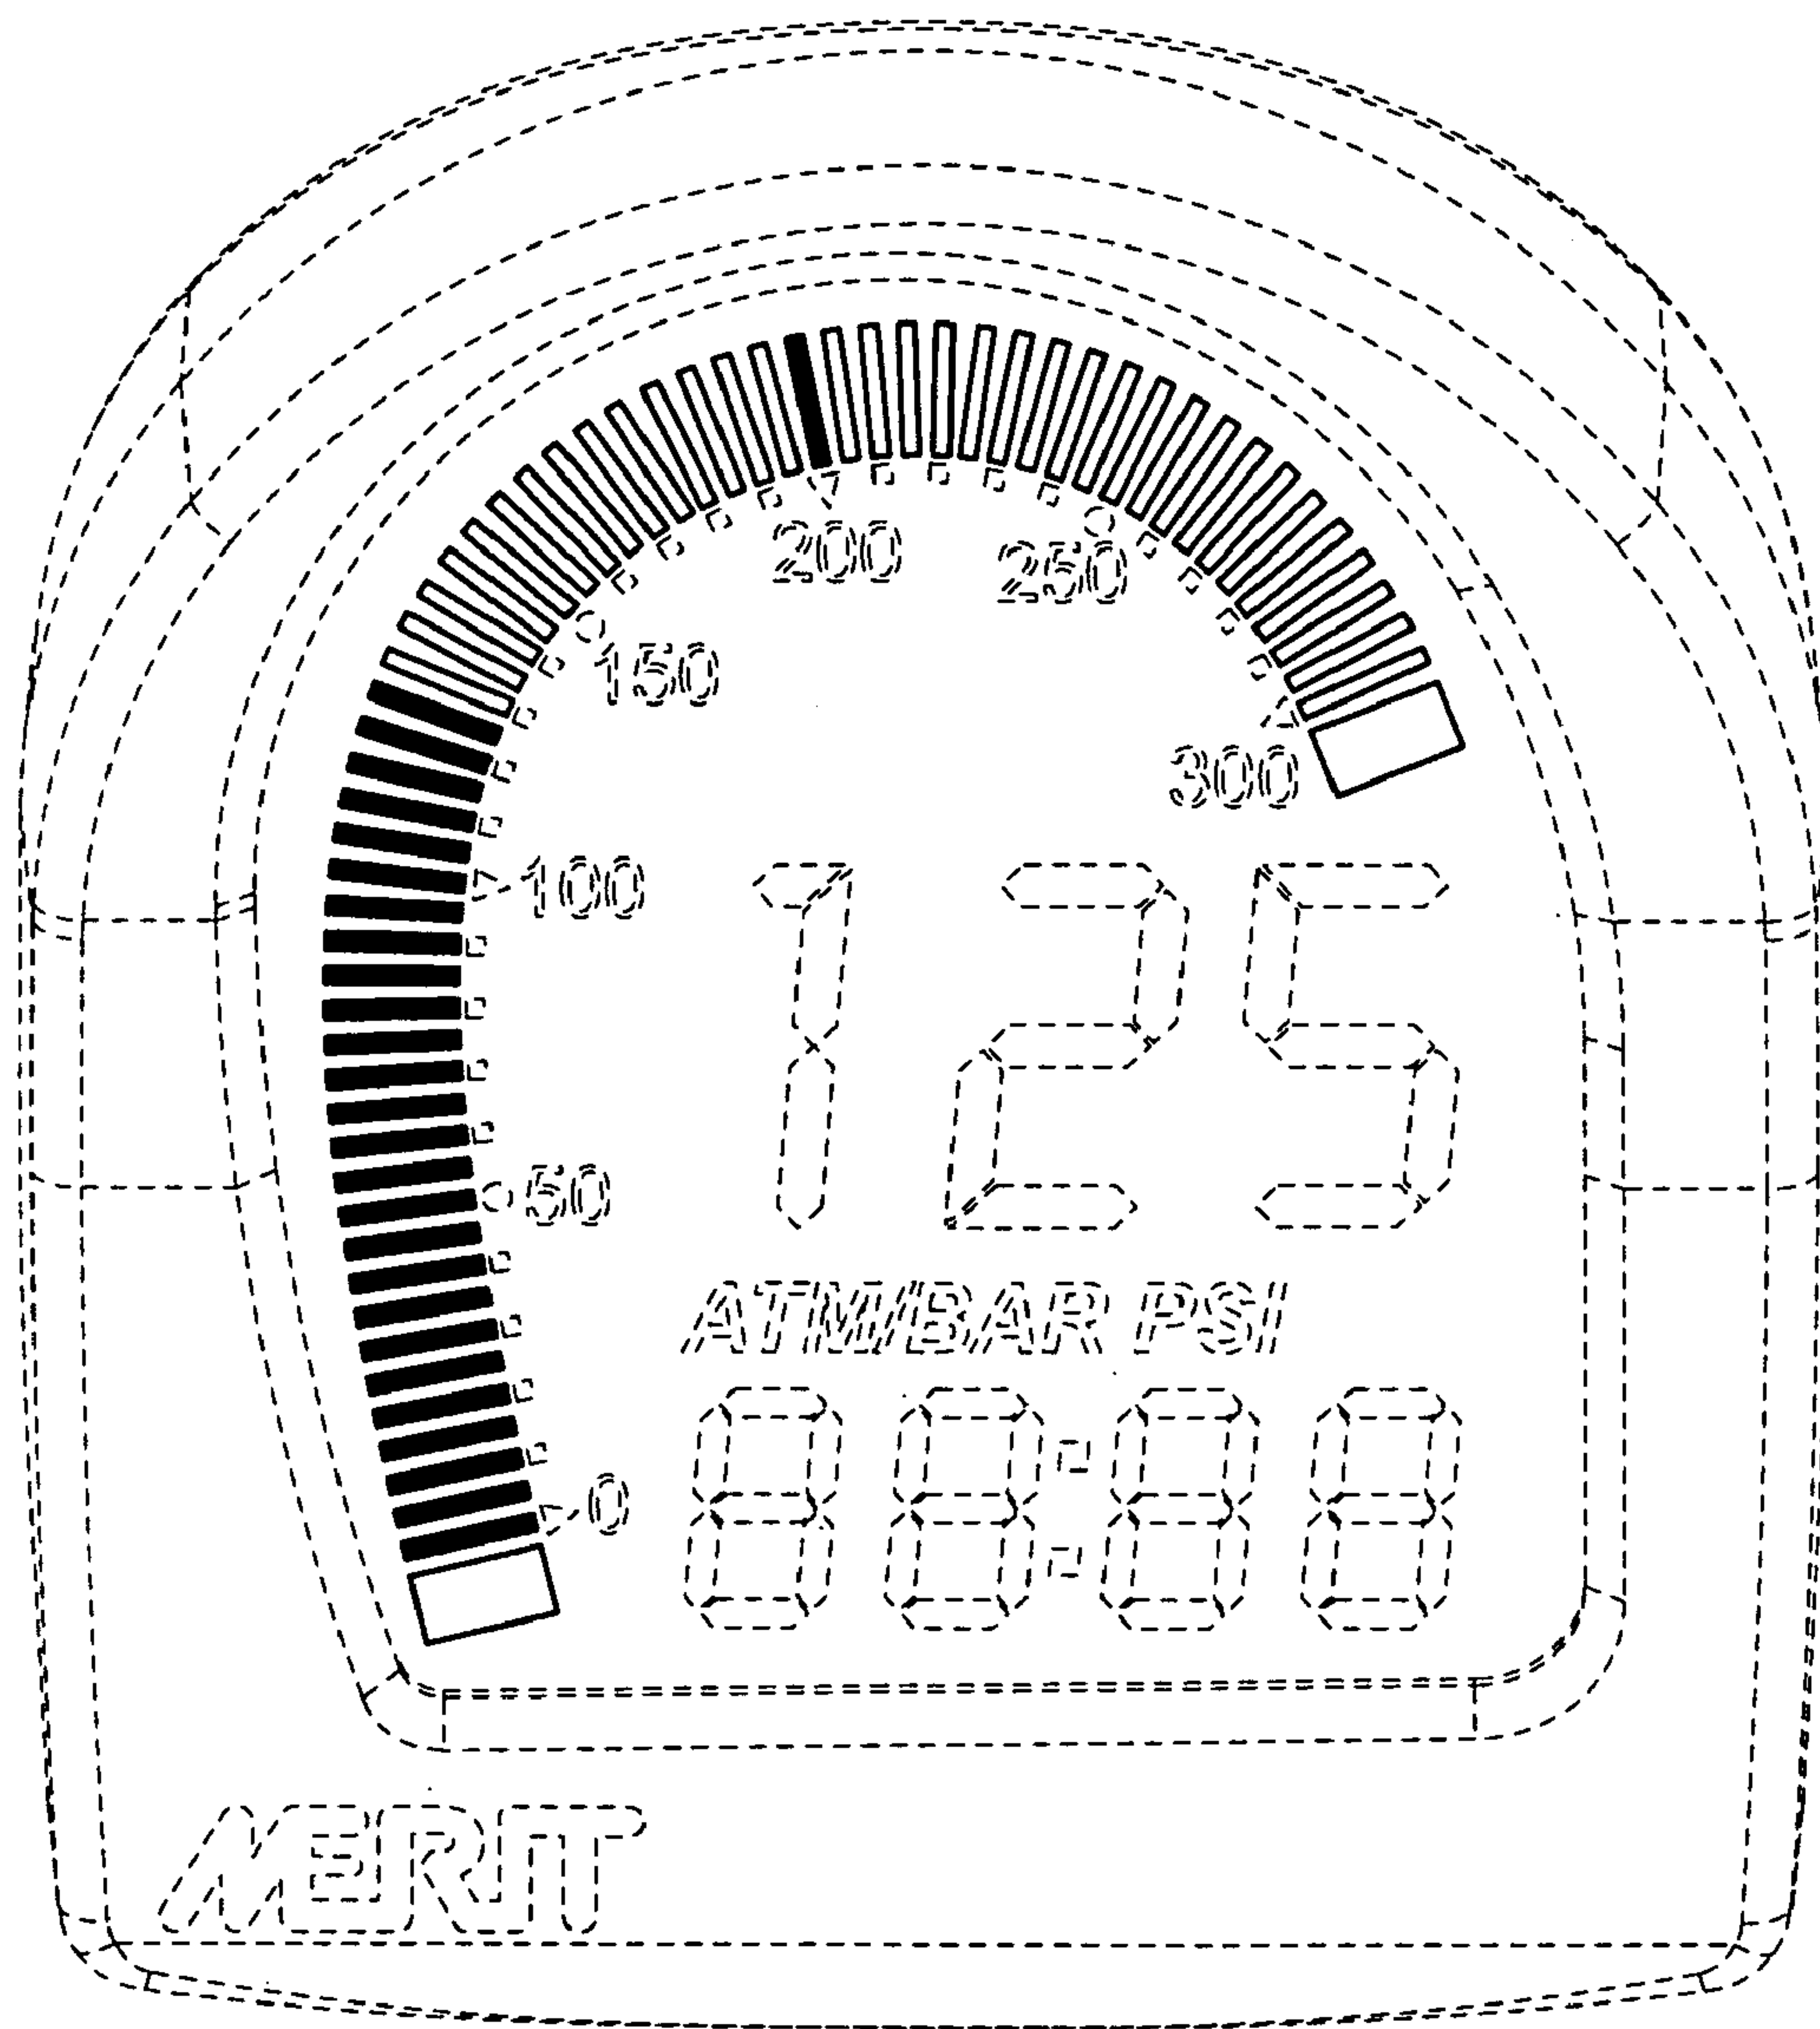


FIG. 10

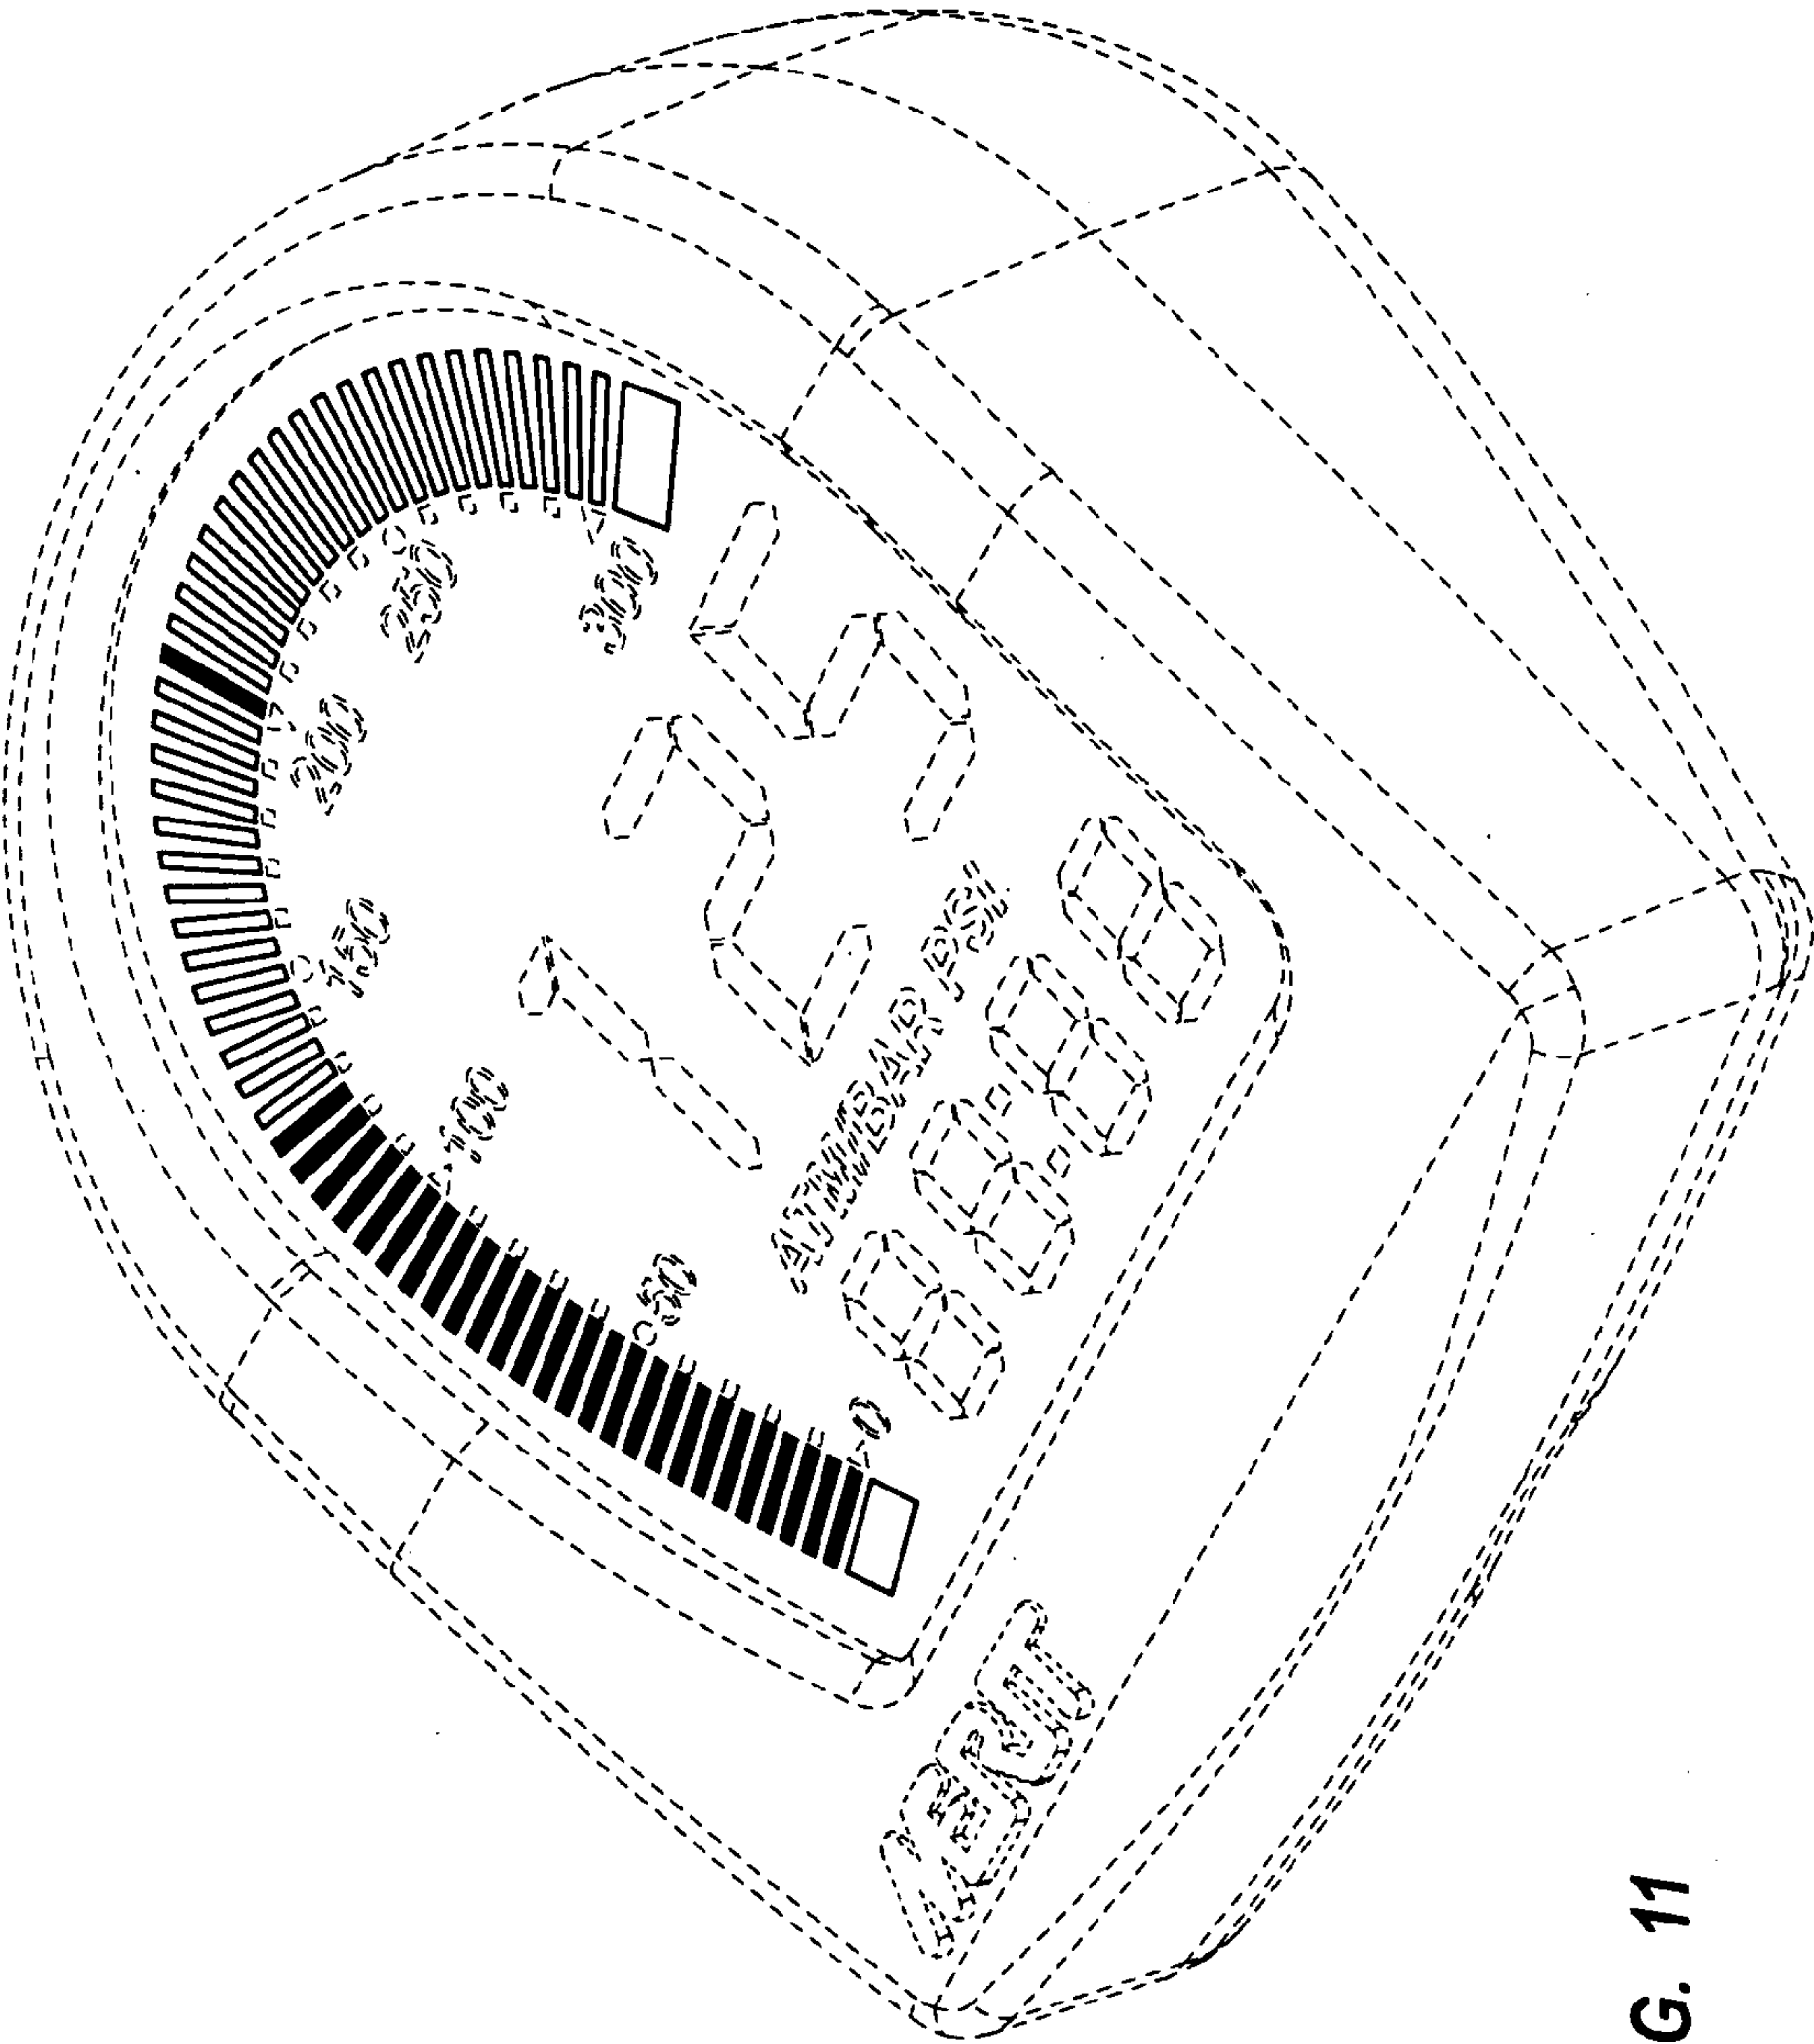


FIG. 11

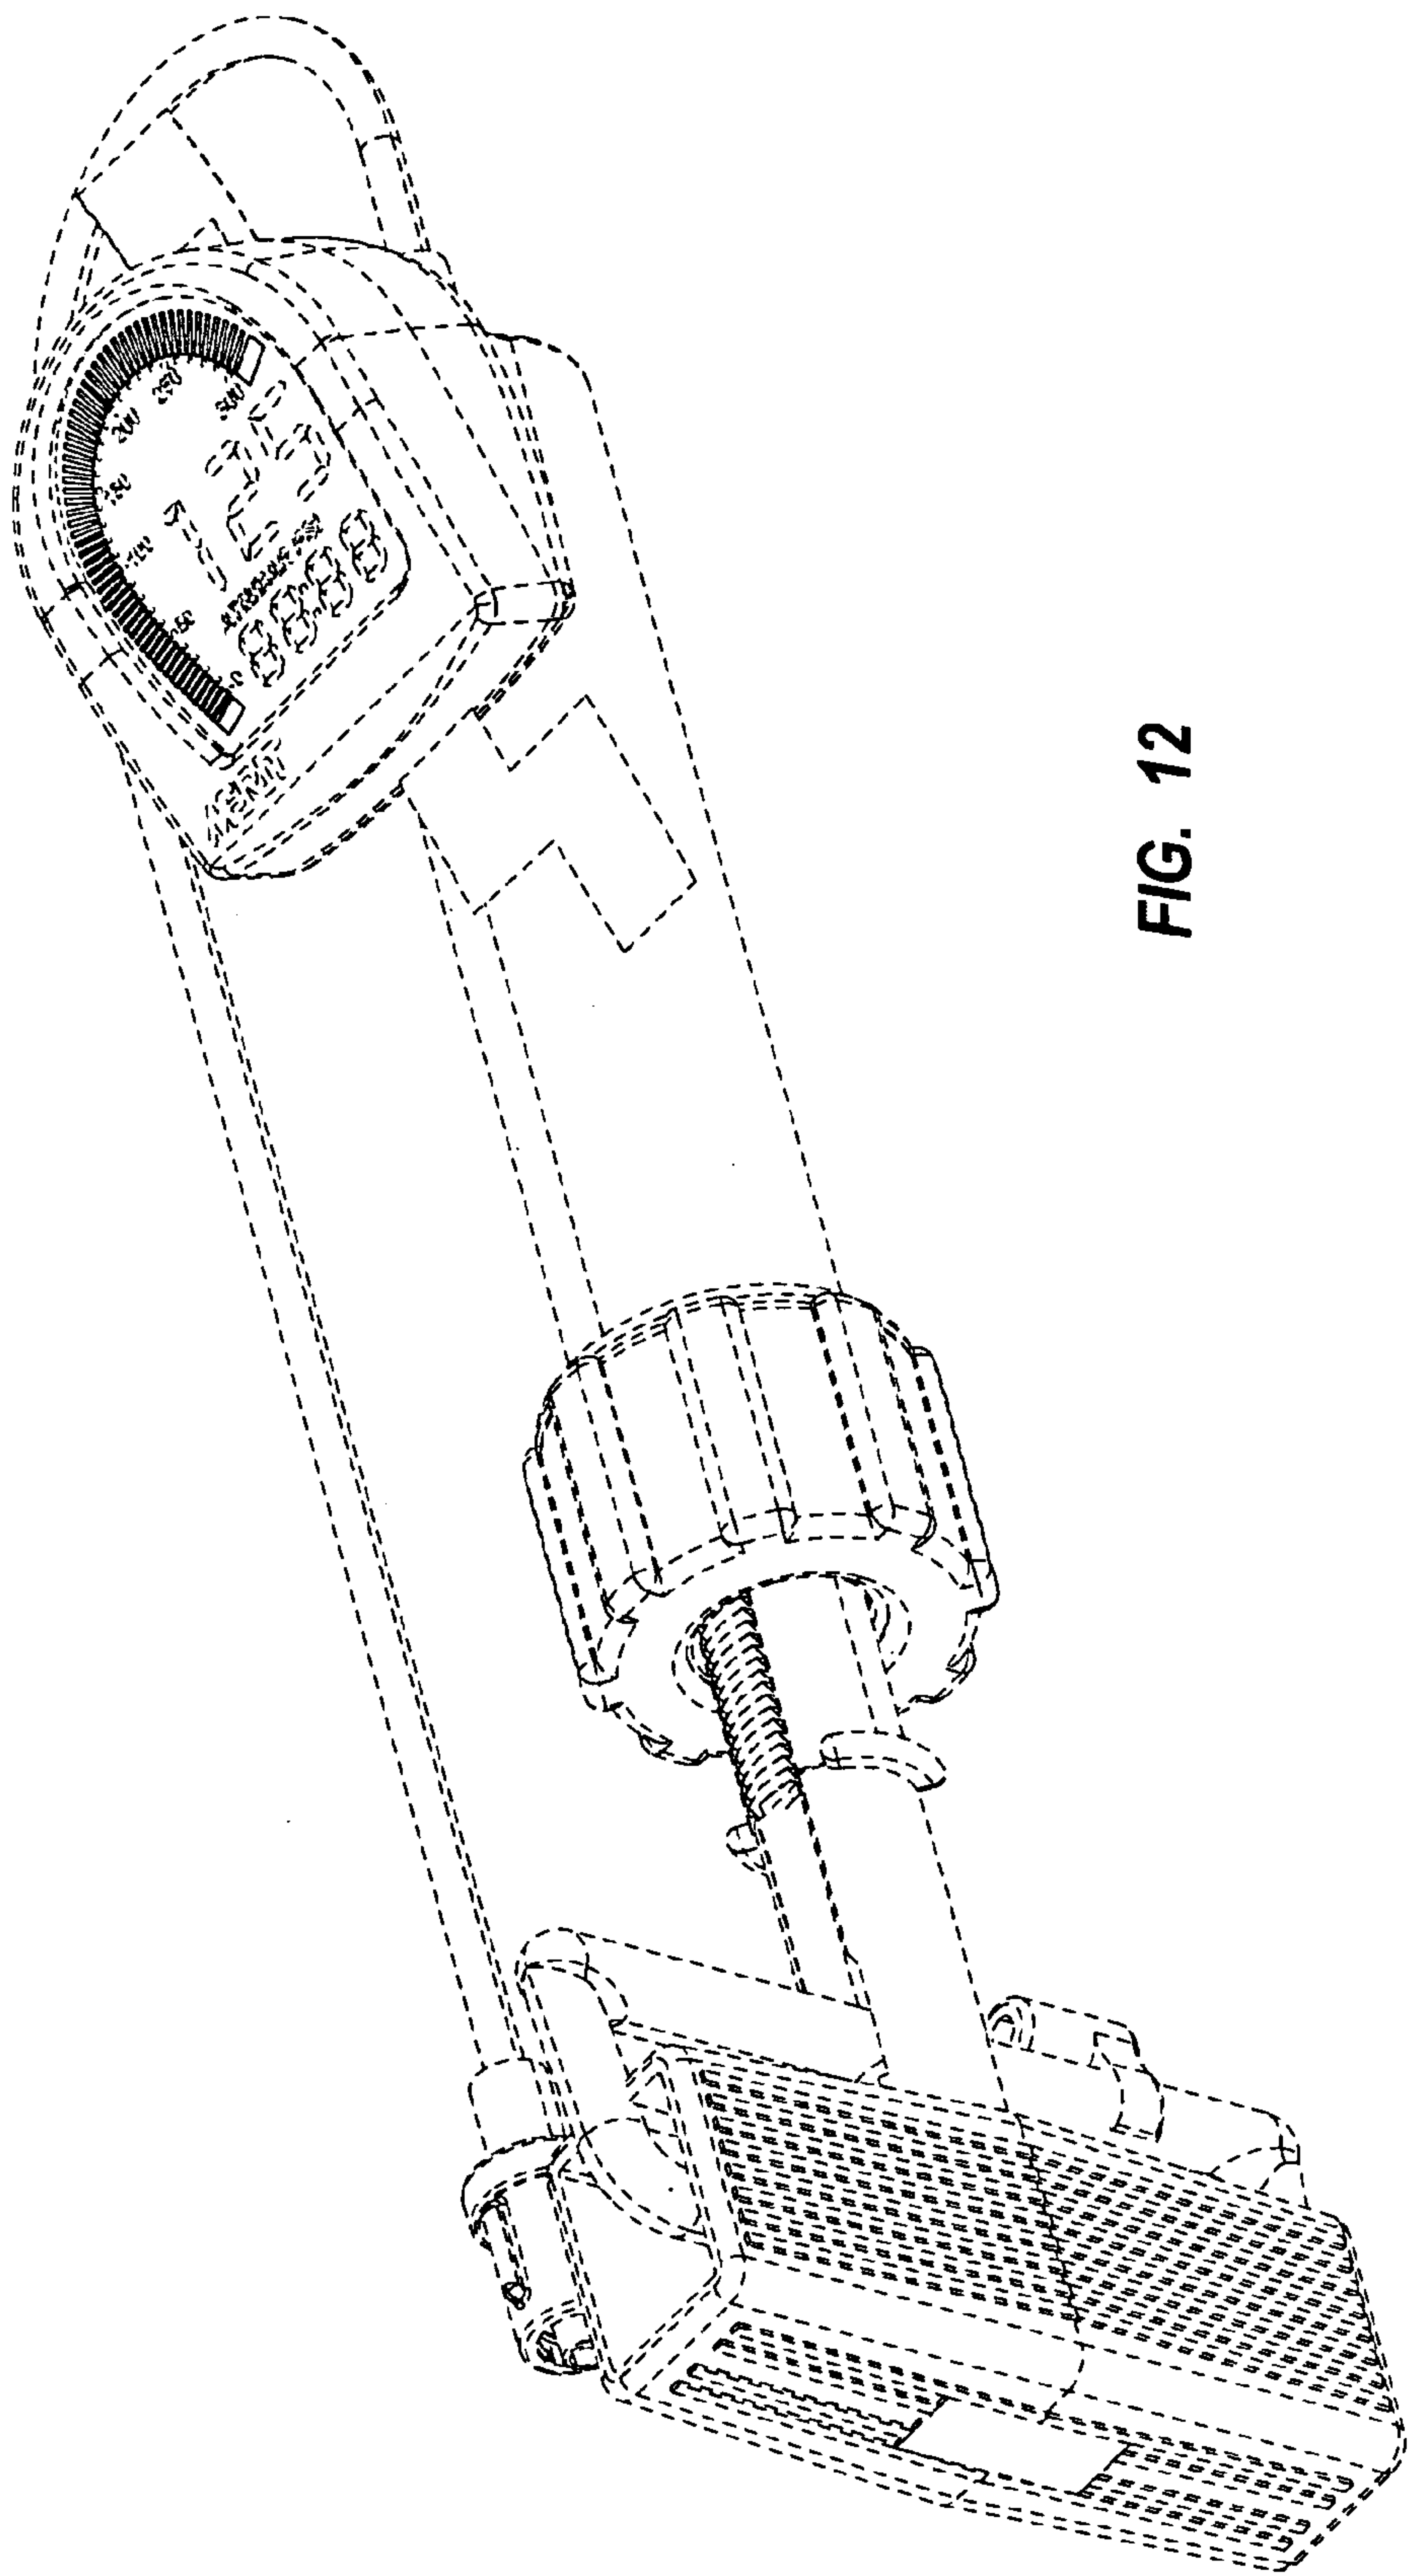


FIG. 12

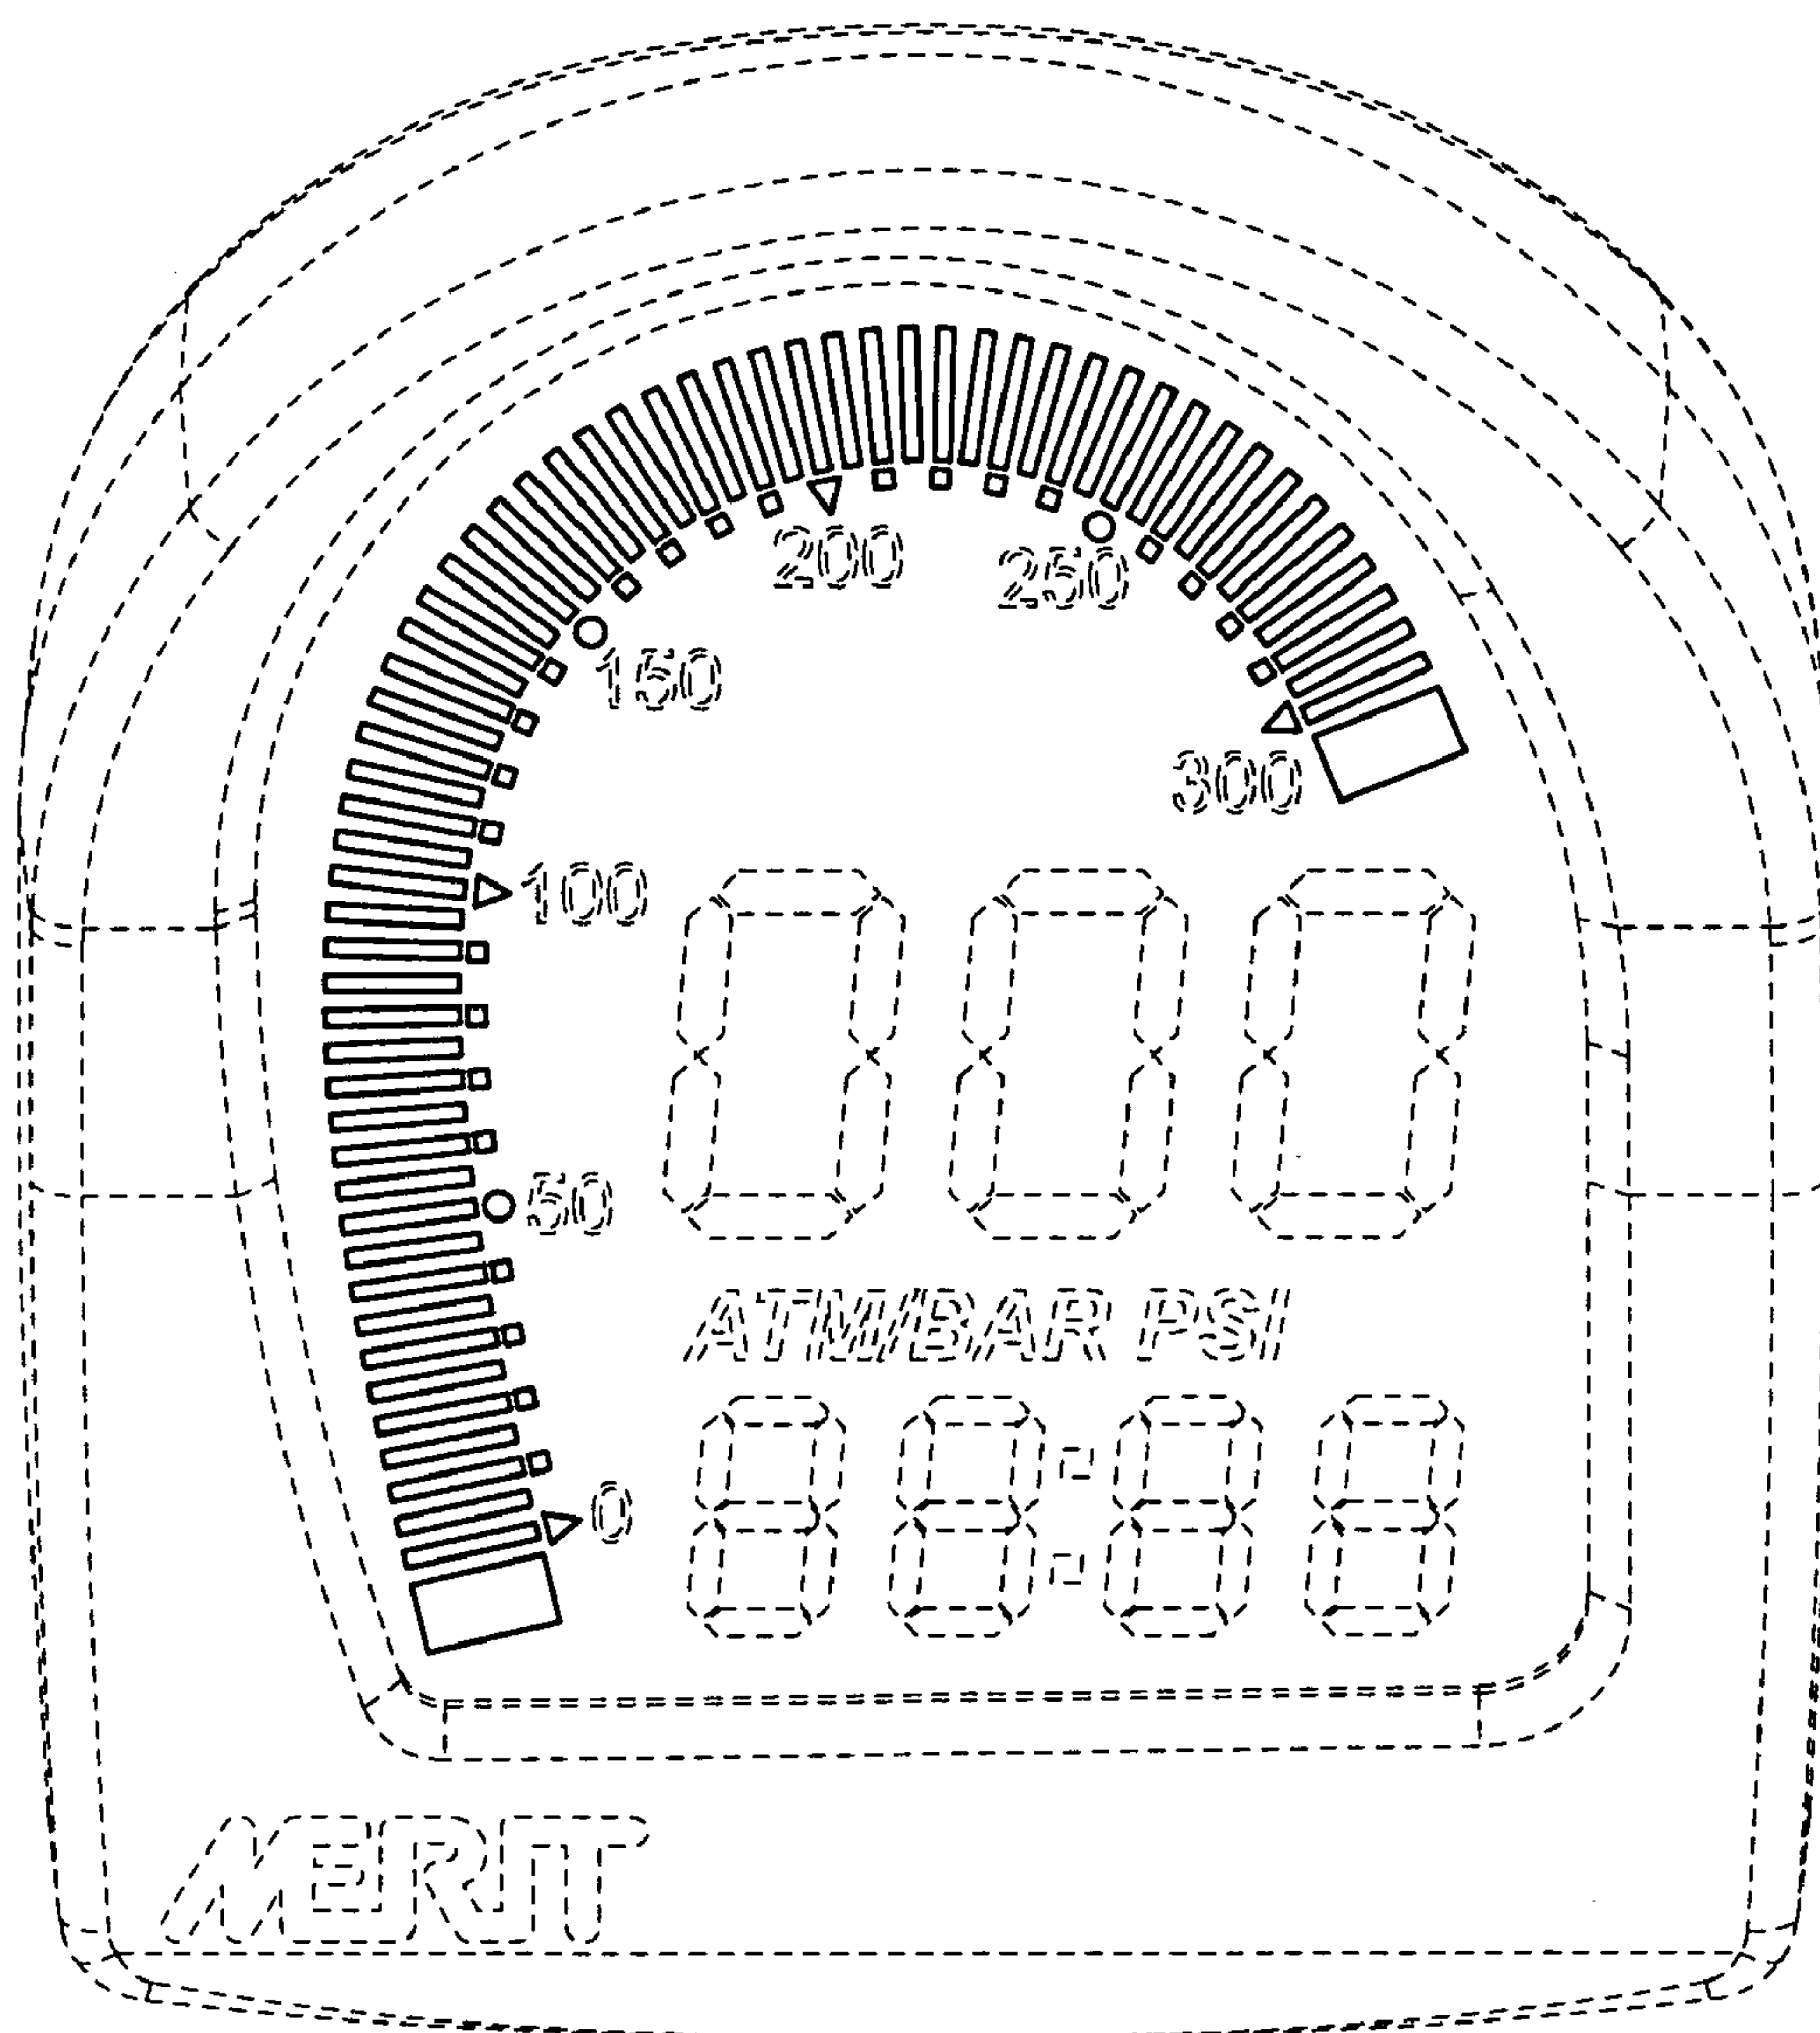


FIG. 13

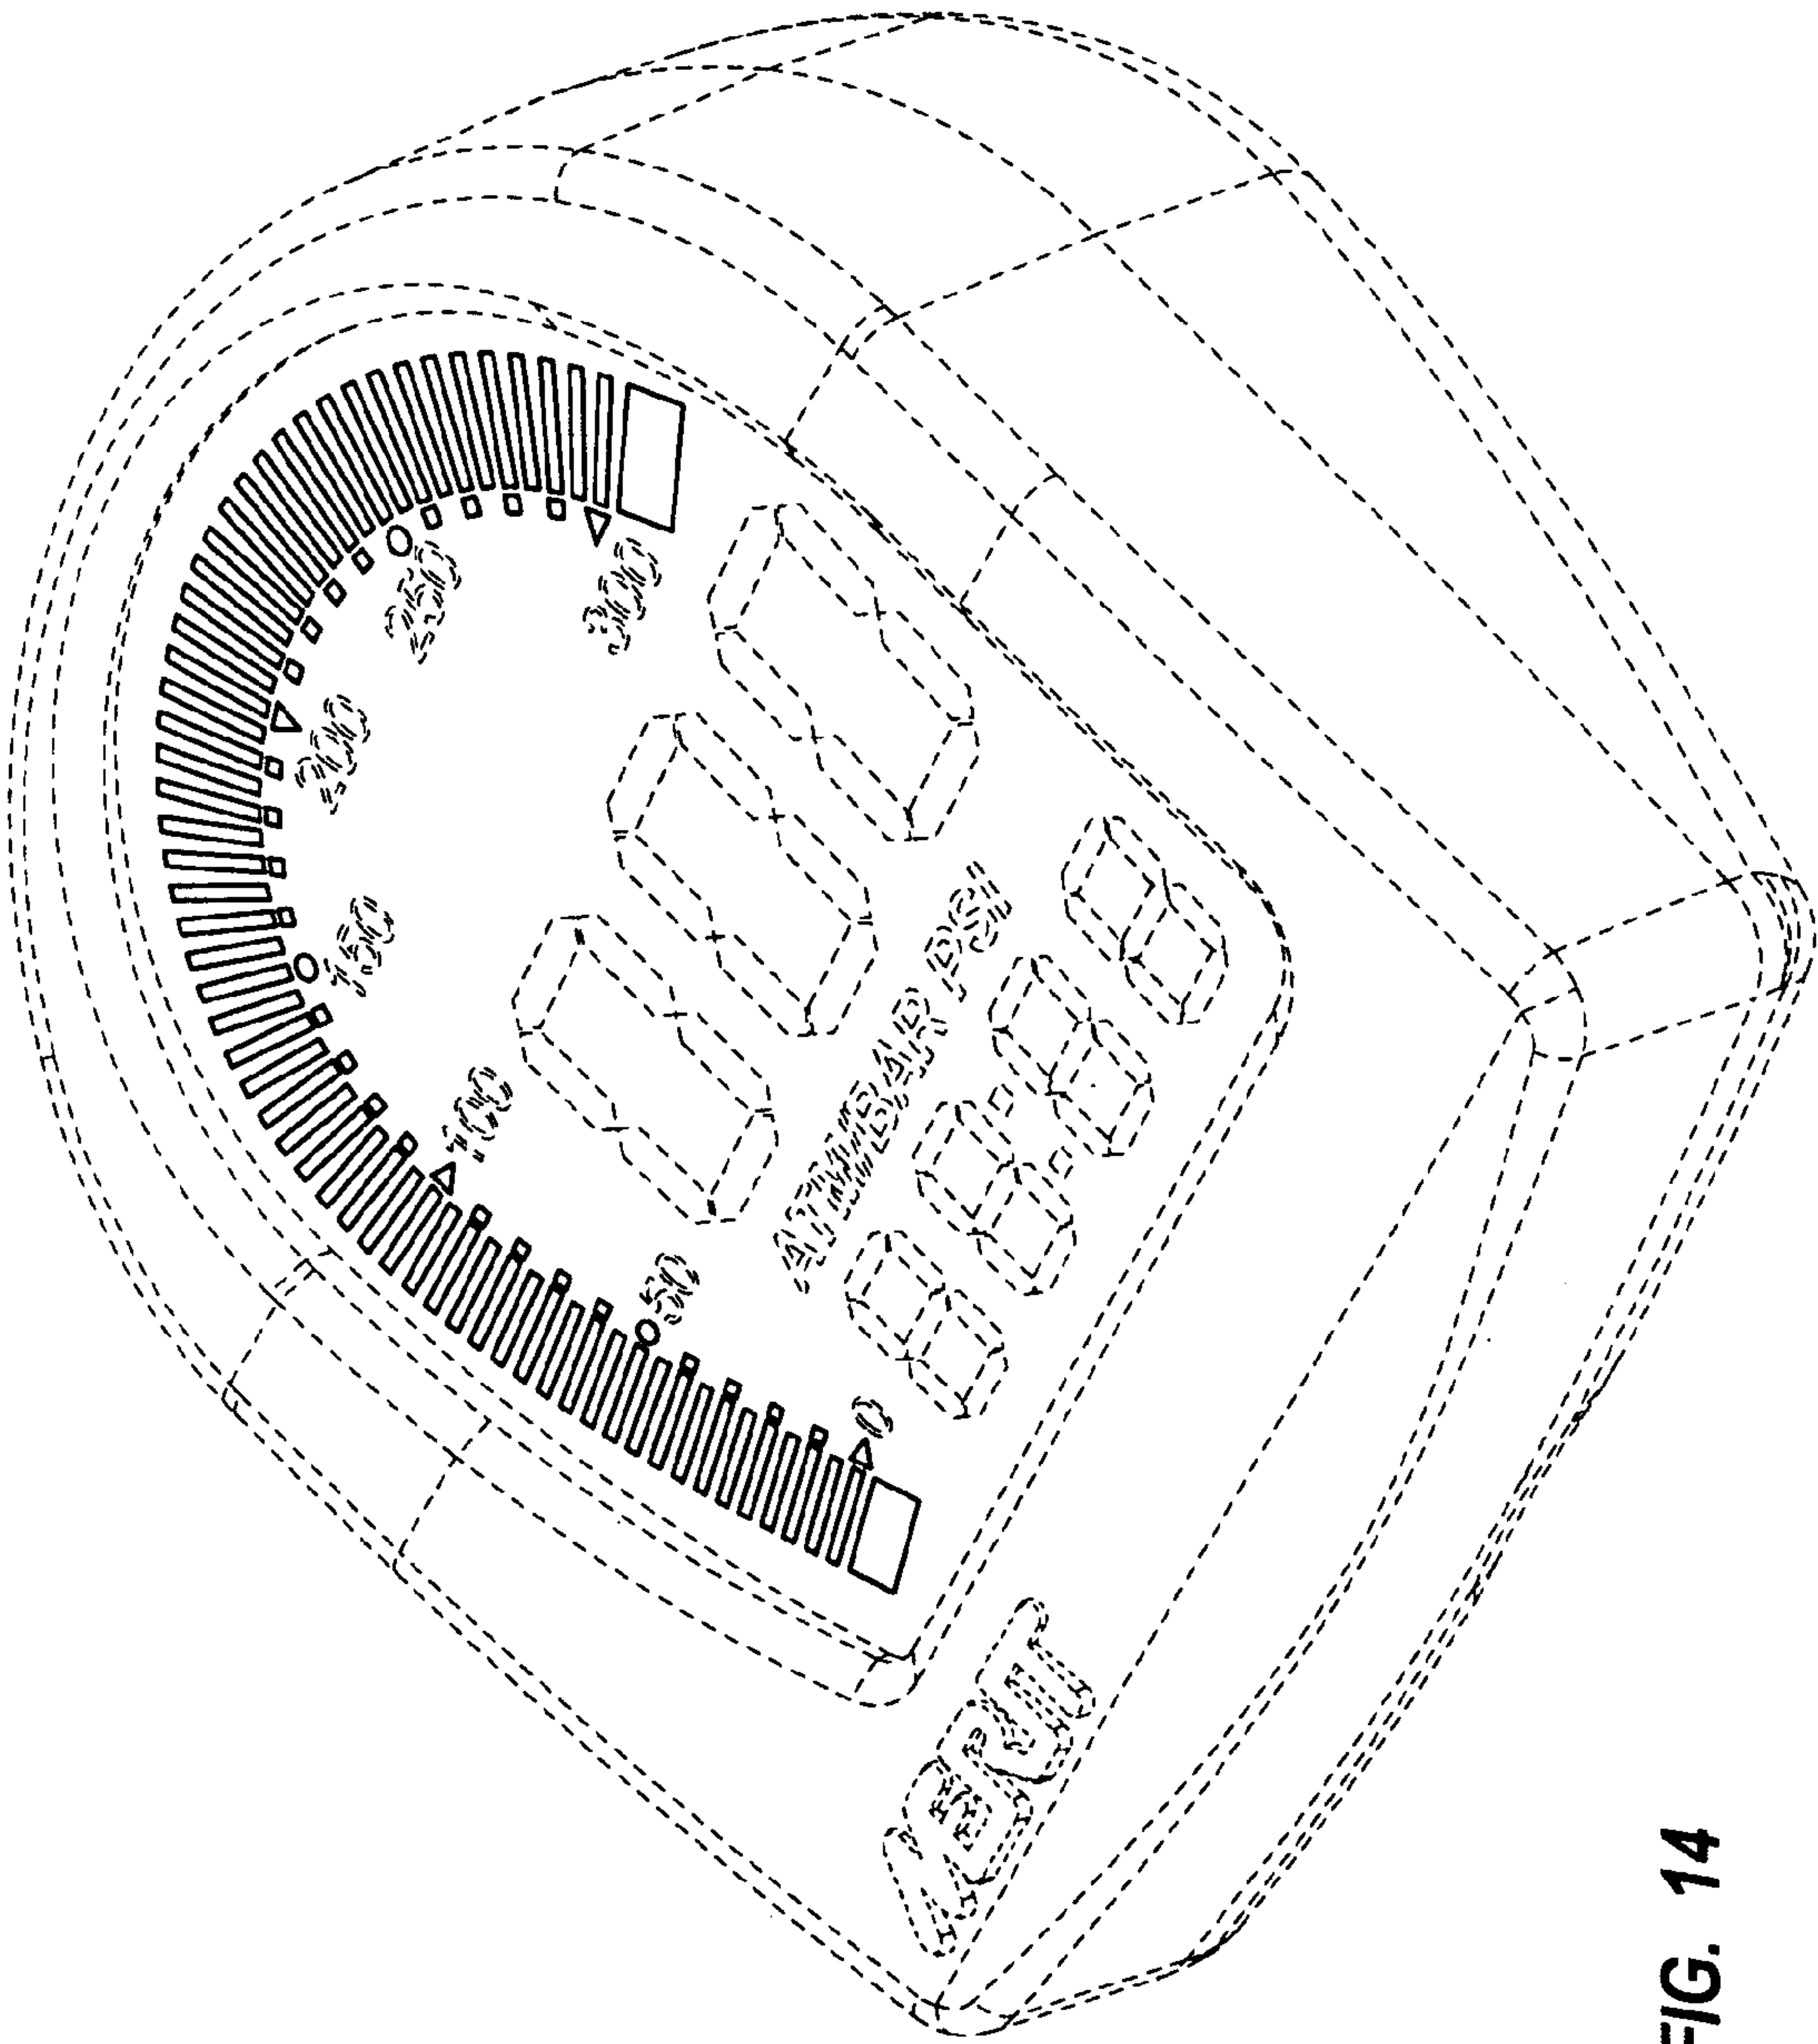


FIG. 14

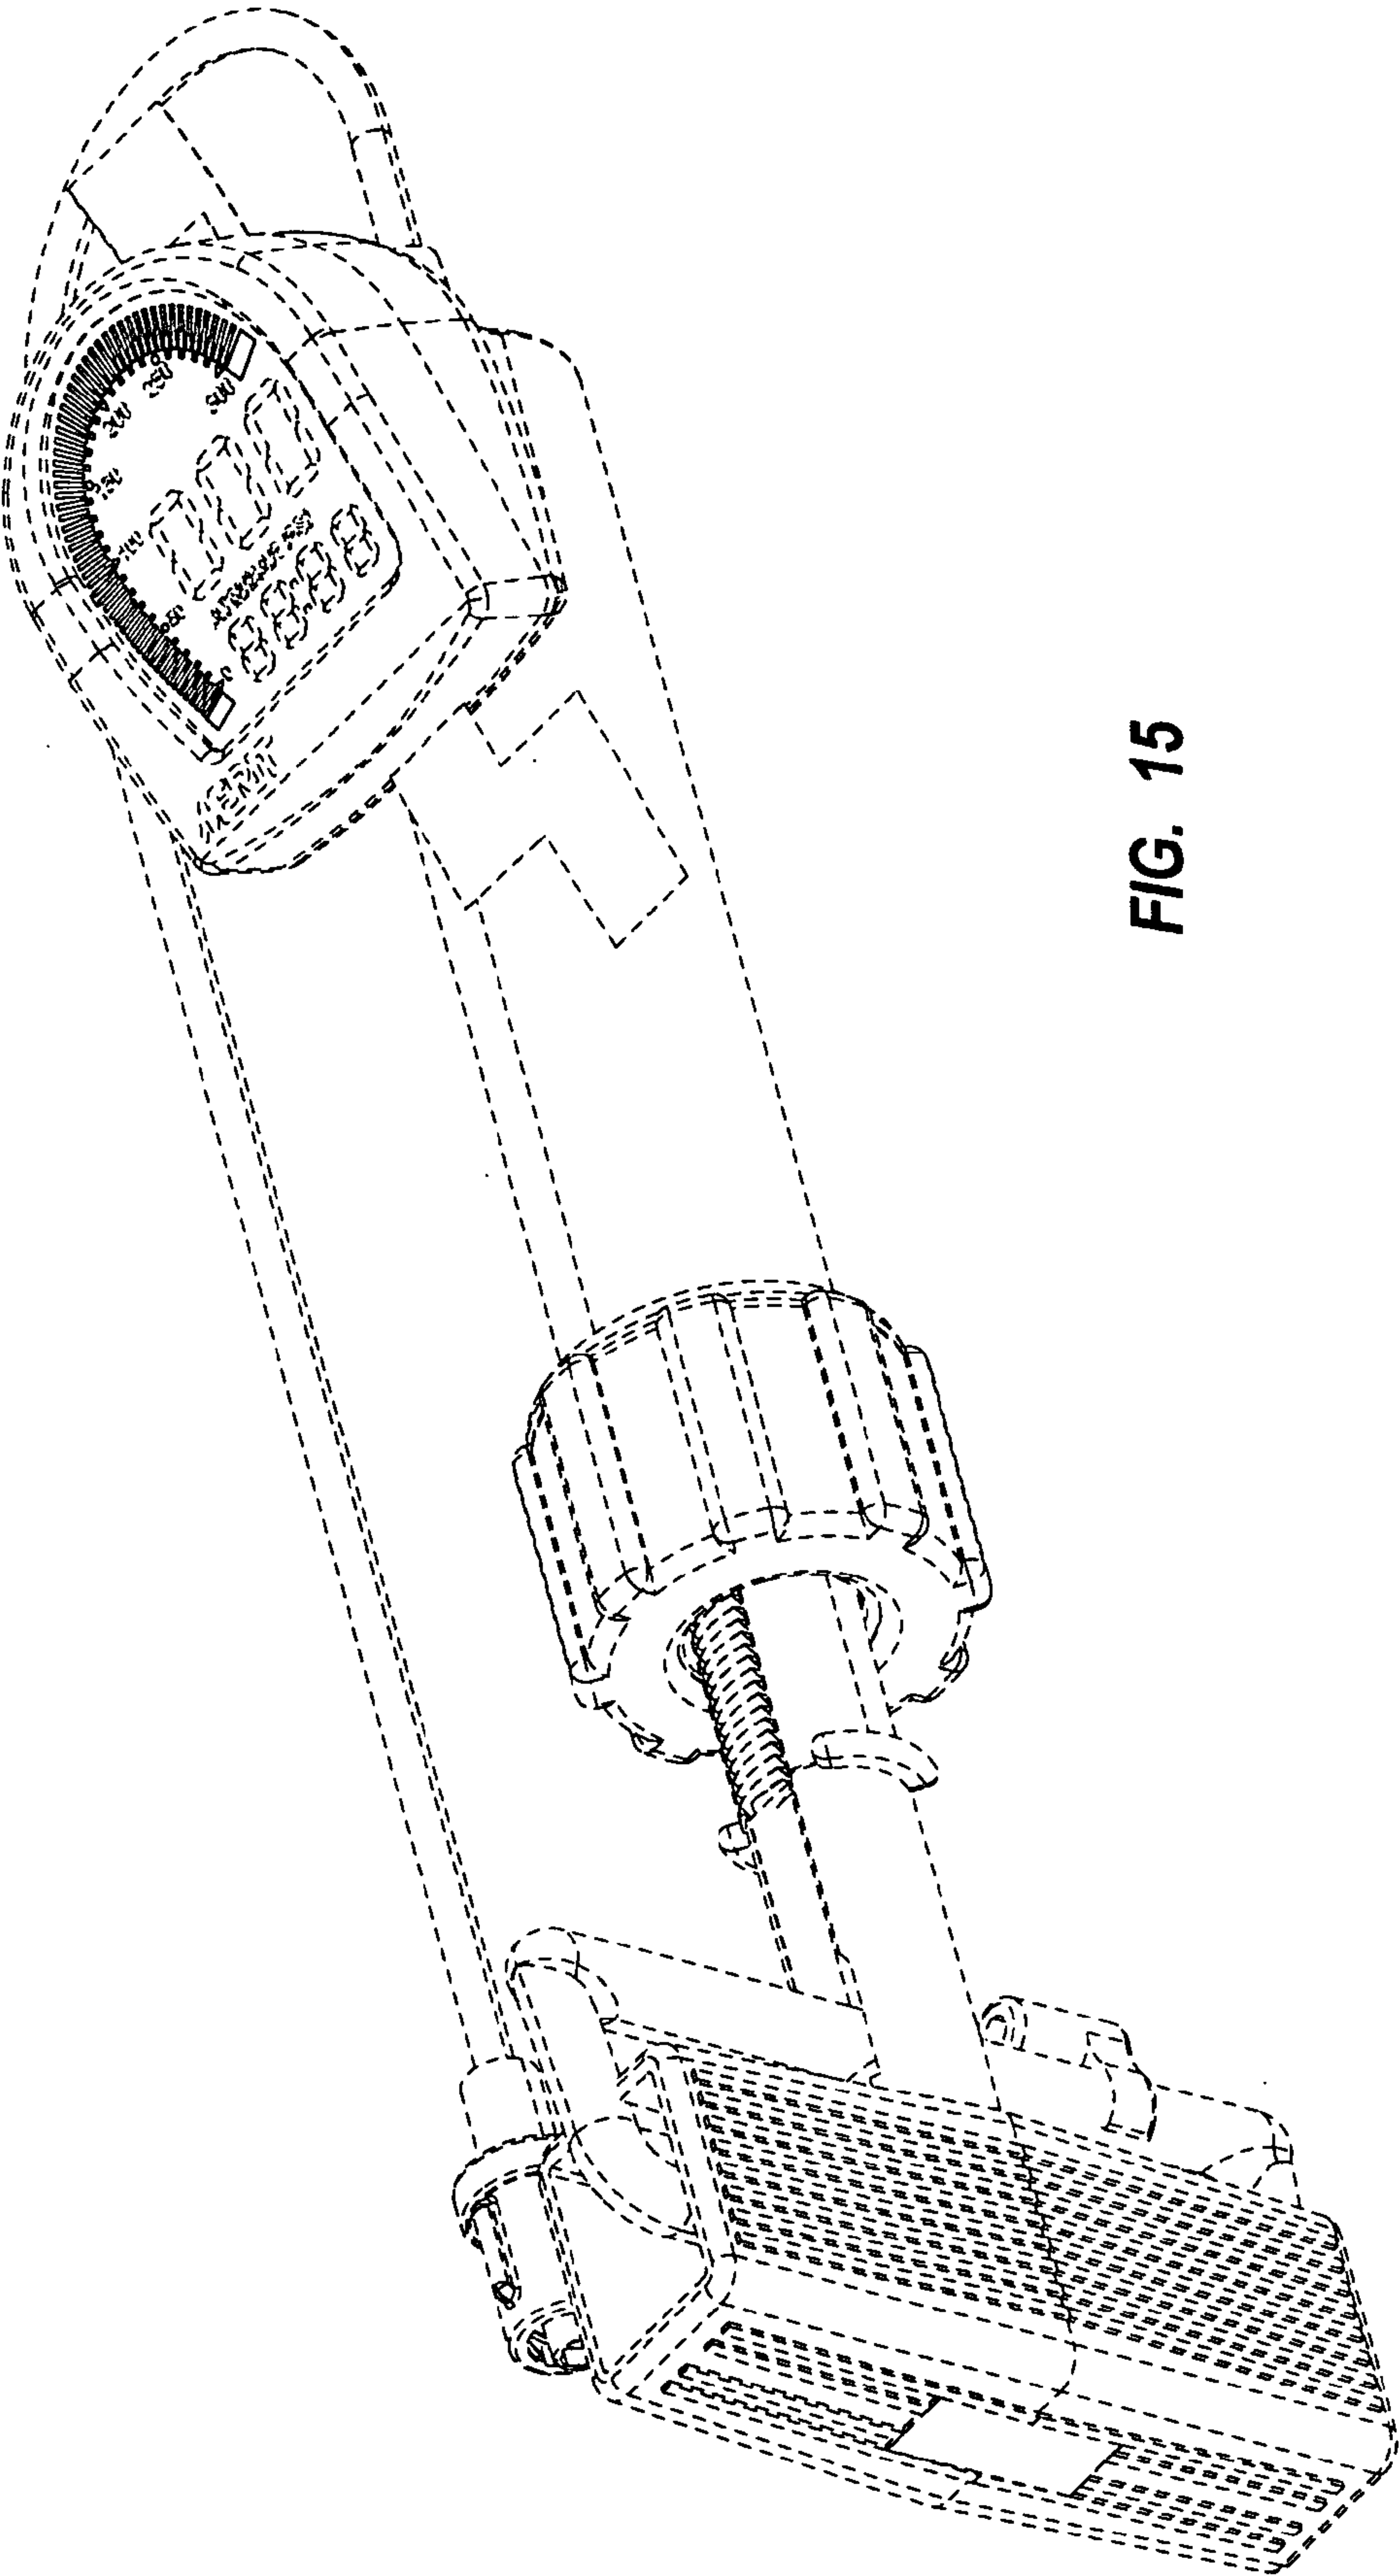


FIG. 15

UNITED STATES PATENT AND TRADEMARK OFFICE
Certificate

Patent No. D.597,037 S

Patented: July 28, 2009

On petition requesting issuance of a certificate for correction of inventorship pursuant to 35 U.S.C. 256, it has been found that the above identified patent, through error and without any deceptive intent, improperly sets forth the inventorship.

Accordingly, it is hereby certified that the correct inventorship of this patent is: Fred P. Lampropoulos, Salt Lake City, UT (US); Jim Mottola, Salt Lake City, UT (US); Steve Taylor, Salt Lake City, UT (US); Thomas Stout, Salt Lake City, UT (US); and Blaine Johnson, Riverton, UT (US).

Signed and Sealed this Thirtieth day of November 2010.

STELLA M. REID
Supervisory Patent Examiner
Art Unit 2912
Technology Center 2900