



US00D598114S

(12) **United States Design Patent**
Cryan

(10) **Patent No.:** **US D598,114 S**

(45) **Date of Patent:** **** Aug. 11, 2009**

(54) **BIOELECTRODE**

(75) Inventor: **Marc P. Cryan**, Maynard, MA (US)

(73) Assignee: **NeuroMetrix, Inc.**, Waltham, MA (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/322,851**

(22) Filed: **Aug. 13, 2008**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/187**

(58) **Field of Classification Search** D24/167-168,
D24/186-187, 232; D13/182; 600/372-384,
600/386, 388, 393; 607/62, 109, 121, 139
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | |
|-----------|------|---------|-----------------|-------|---------|
| 4,957,109 | A * | 9/1990 | Groeger et al. | | 600/391 |
| D425,203 | S * | 5/2000 | Sheehan et al. | | D24/187 |
| D443,063 | S * | 5/2001 | Pisani et al. | | D24/187 |
| 6,298,255 | B1 * | 10/2001 | Cordero et al. | | 600/372 |
| D475,138 | S * | 5/2003 | Baura et al. | | D24/187 |
| D492,782 | S * | 7/2004 | Faller et al. | | D24/167 |
| 6,847,836 | B1 * | 1/2005 | Sujdak | | 600/393 |
| D501,558 | S * | 2/2005 | Chastain et al. | | D24/187 |
| D505,206 | S * | 5/2005 | Chastain et al. | | D24/187 |
| D524,943 | S * | 7/2006 | Faller et al. | | D24/167 |
| D536,673 | S * | 2/2007 | Silber | | D13/182 |

| | | | | | |
|----------|-----|--------|-----------------|-------|---------|
| D541,421 | S * | 4/2007 | Metzger et al. | | D24/187 |
| D560,809 | S * | 1/2008 | Causevic et al. | | D24/187 |

* cited by examiner

Primary Examiner—Robert A. Delehanty

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Pandiscio & Pandiscio


(57) **CLAIM**

The ornamental design for a bioelectrode, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the bioelectrode;
 FIG. 2 is a front side view, in elevation, of the bioelectrode, taken from the frame of reference of FIG. 1;
 FIG. 3 is a rear side view, in elevation, of the bioelectrode, taken from the frame of reference of FIG. 1;
 FIG. 4 is a right end view, in elevation, of the bioelectrode, taken from the frame of reference of FIG. 1;
 FIG. 5 is a left end view, in elevation, of the bioelectrode, taken from the frame of reference of FIG. 1;
 FIG. 6 is a top face view of the bioelectrode, taken from the frame of reference of FIG. 1; and,
 FIG. 7 is a bottom face view of the bioelectrode, taken from the frame of reference of FIG. 1.

1 Claim, 4 Drawing Sheets

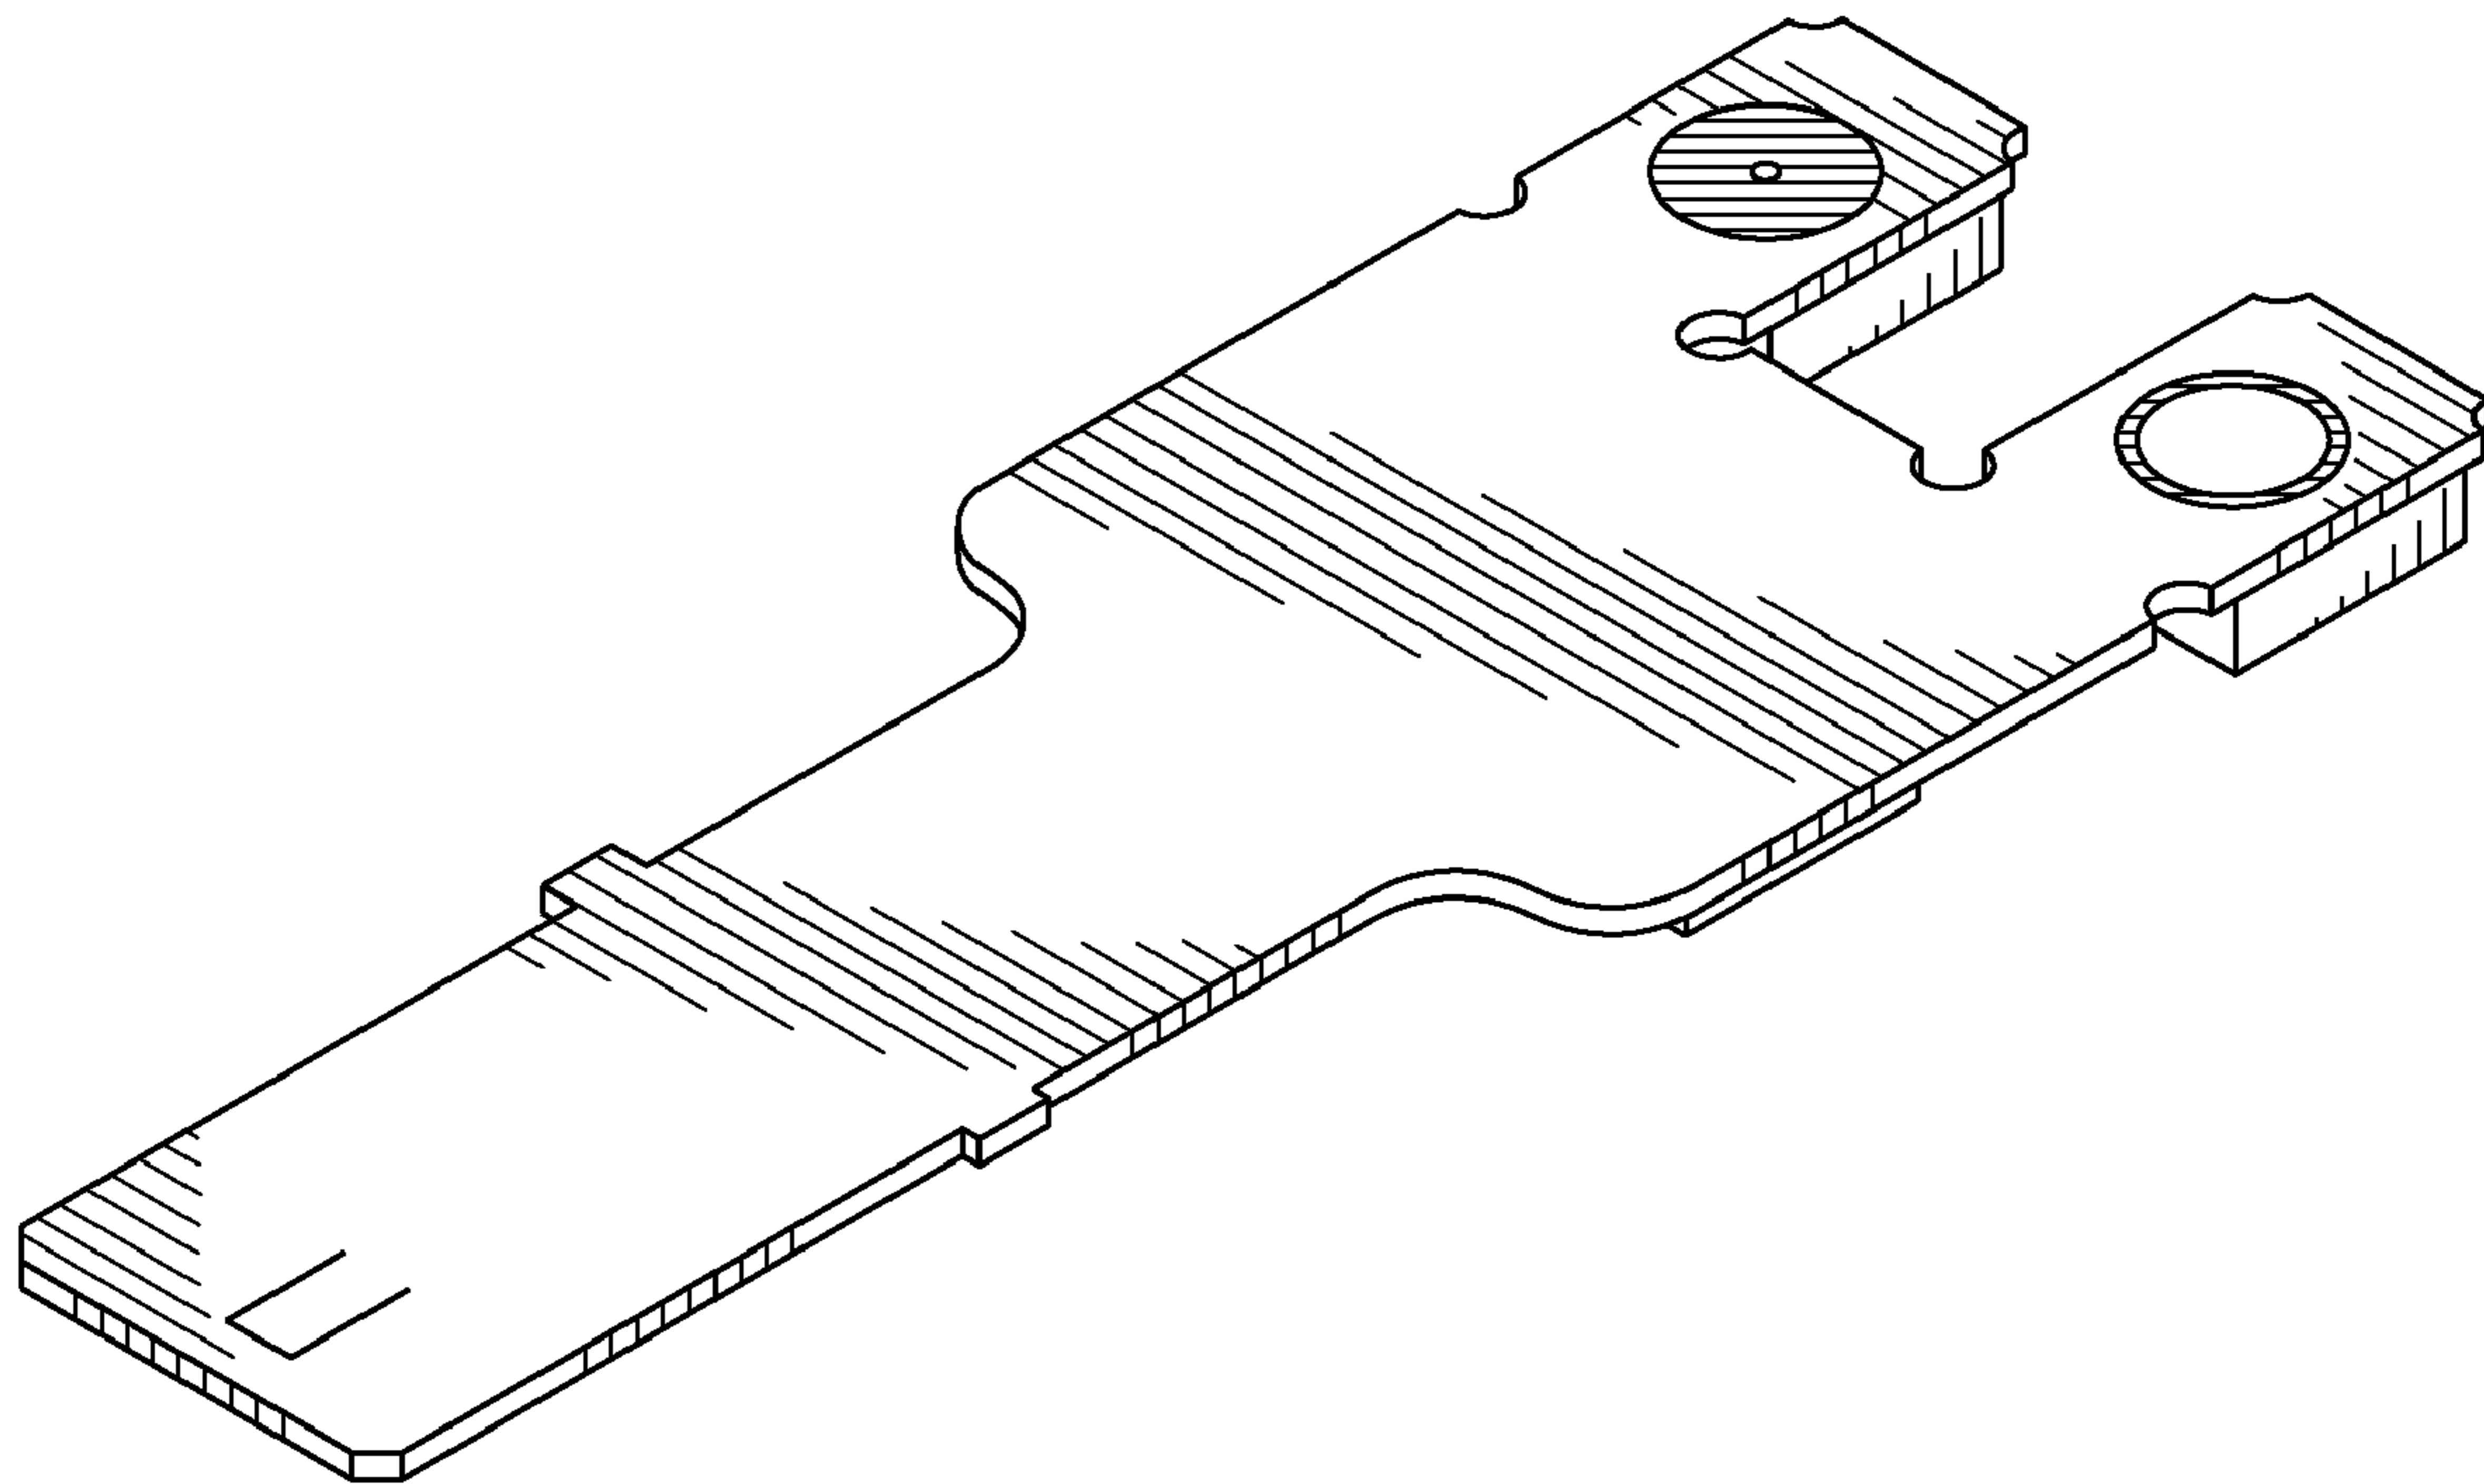

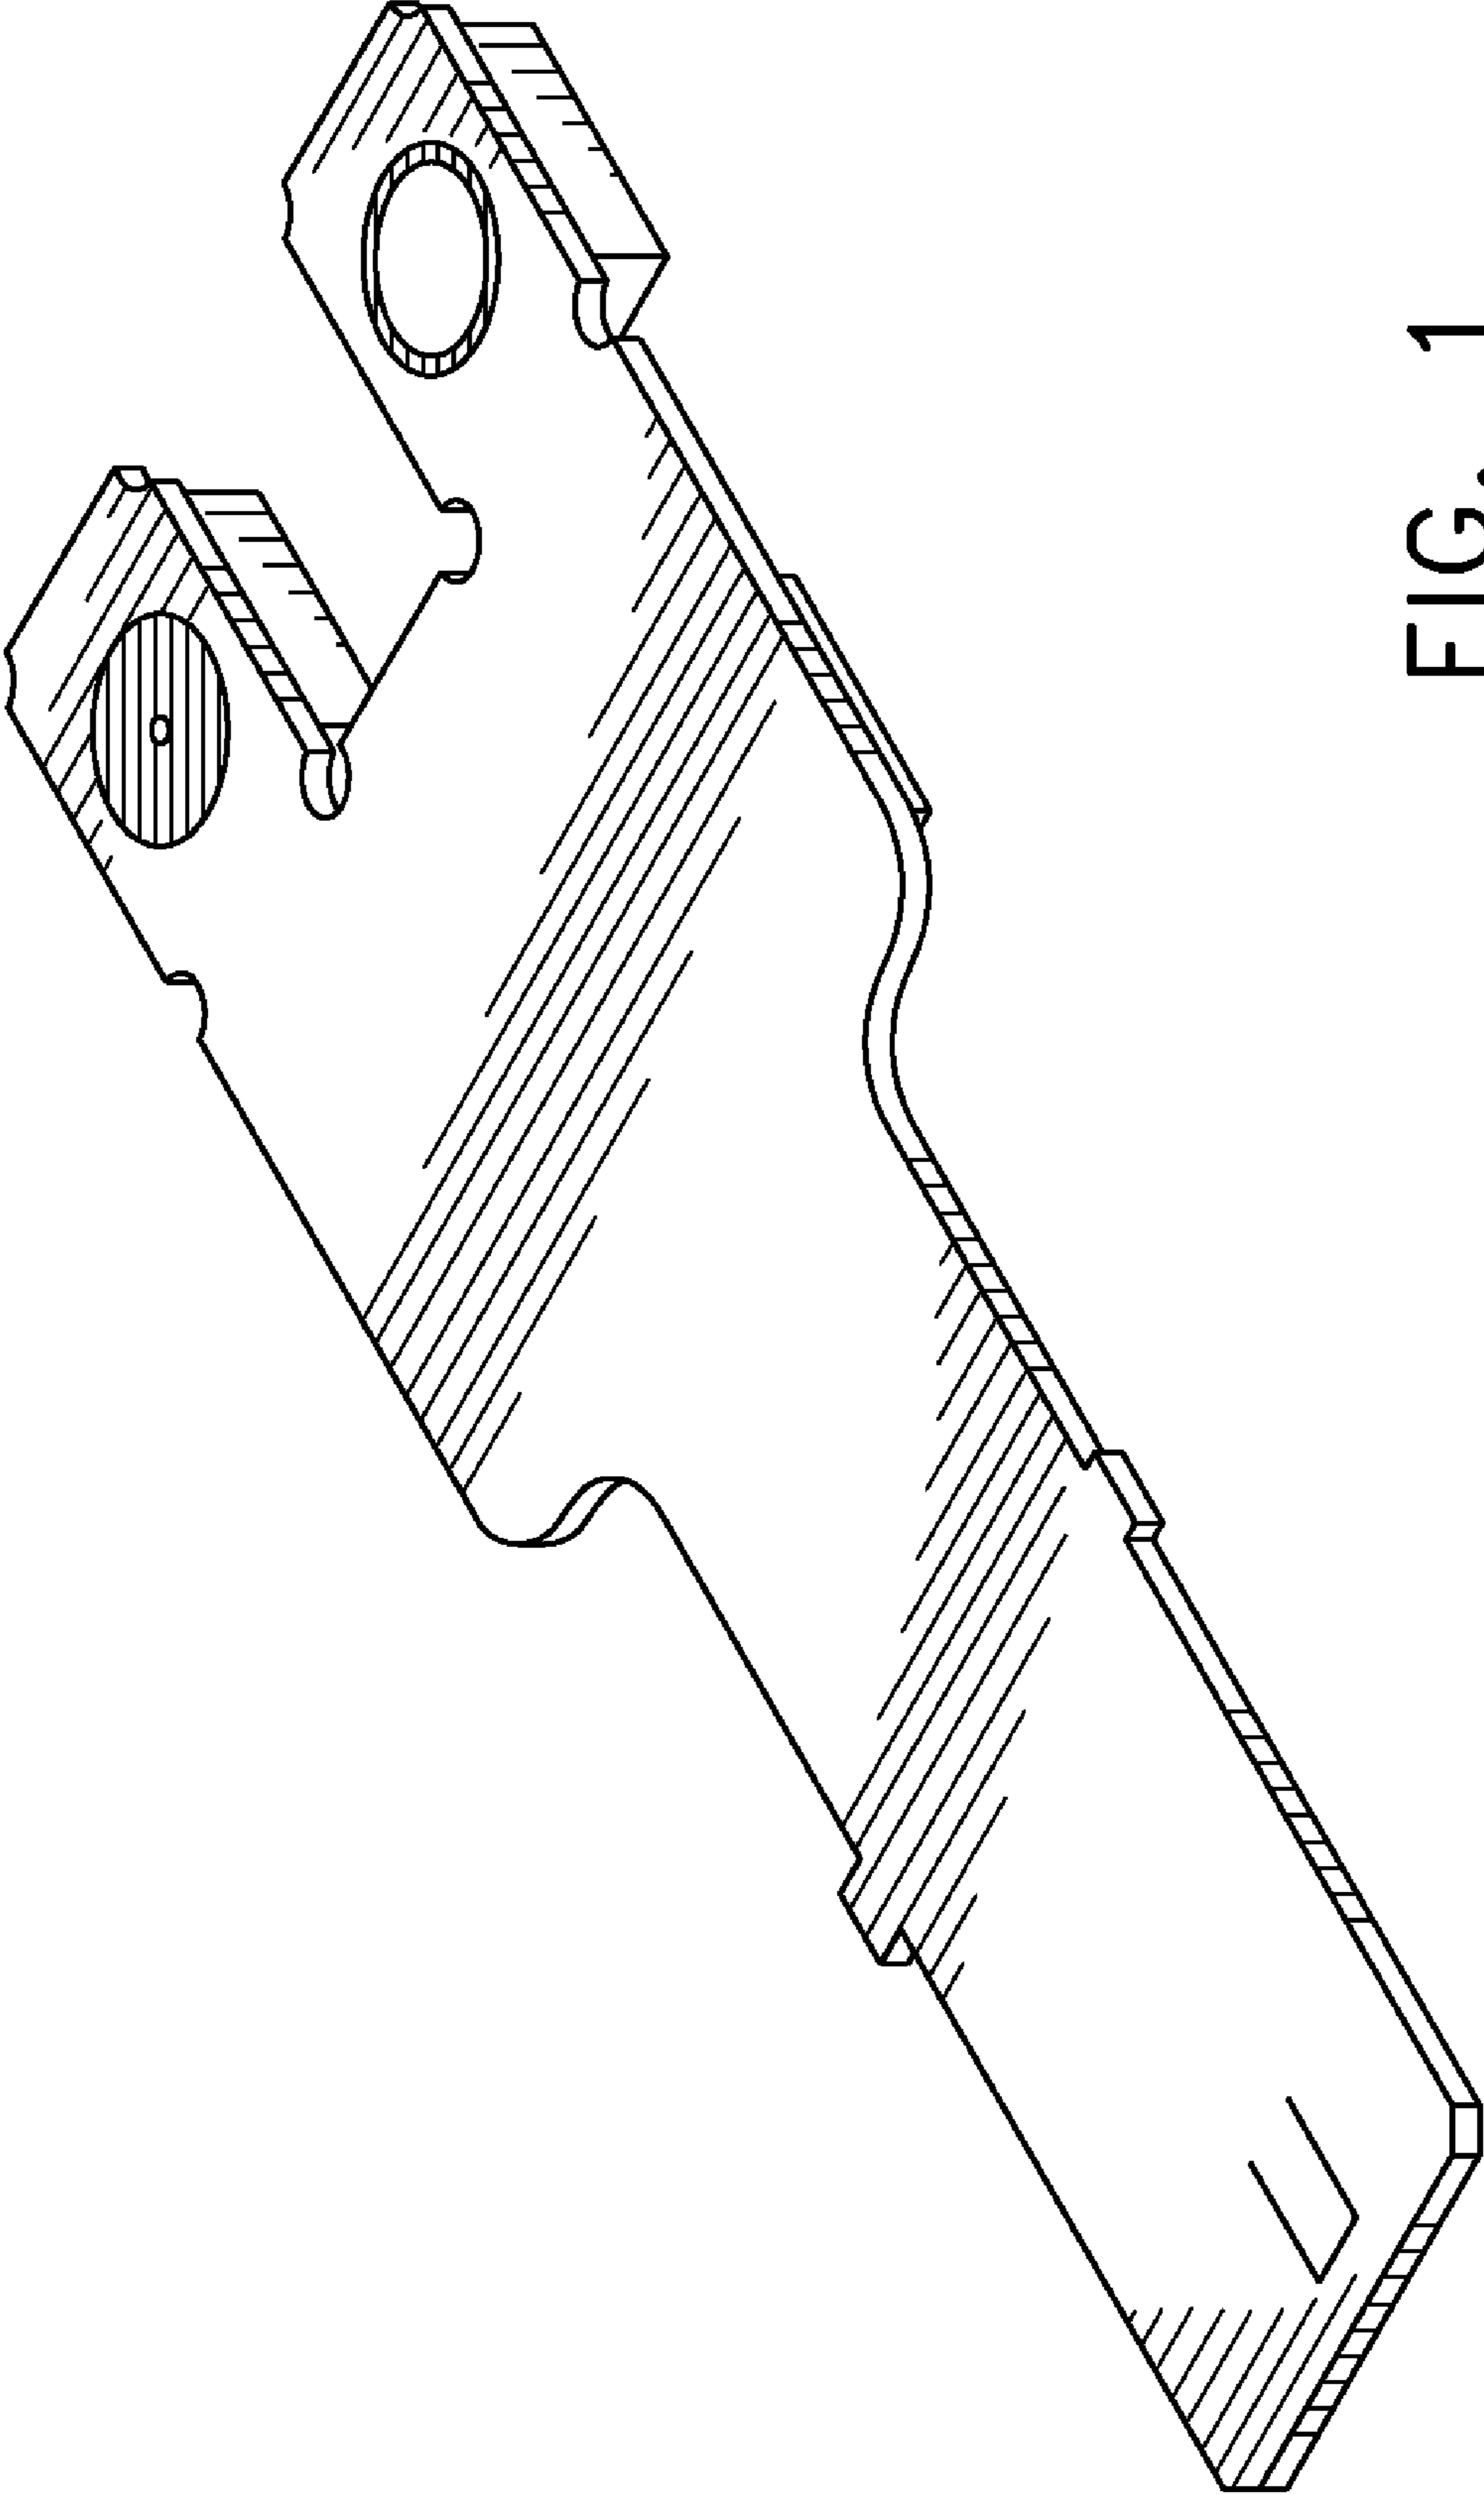


FIG. 1



FIG. 2




FIG. 3

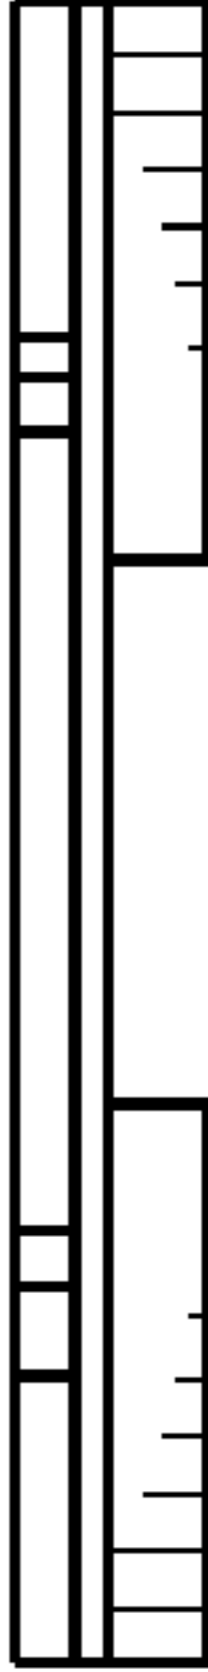


FIG. 4



FIG. 5

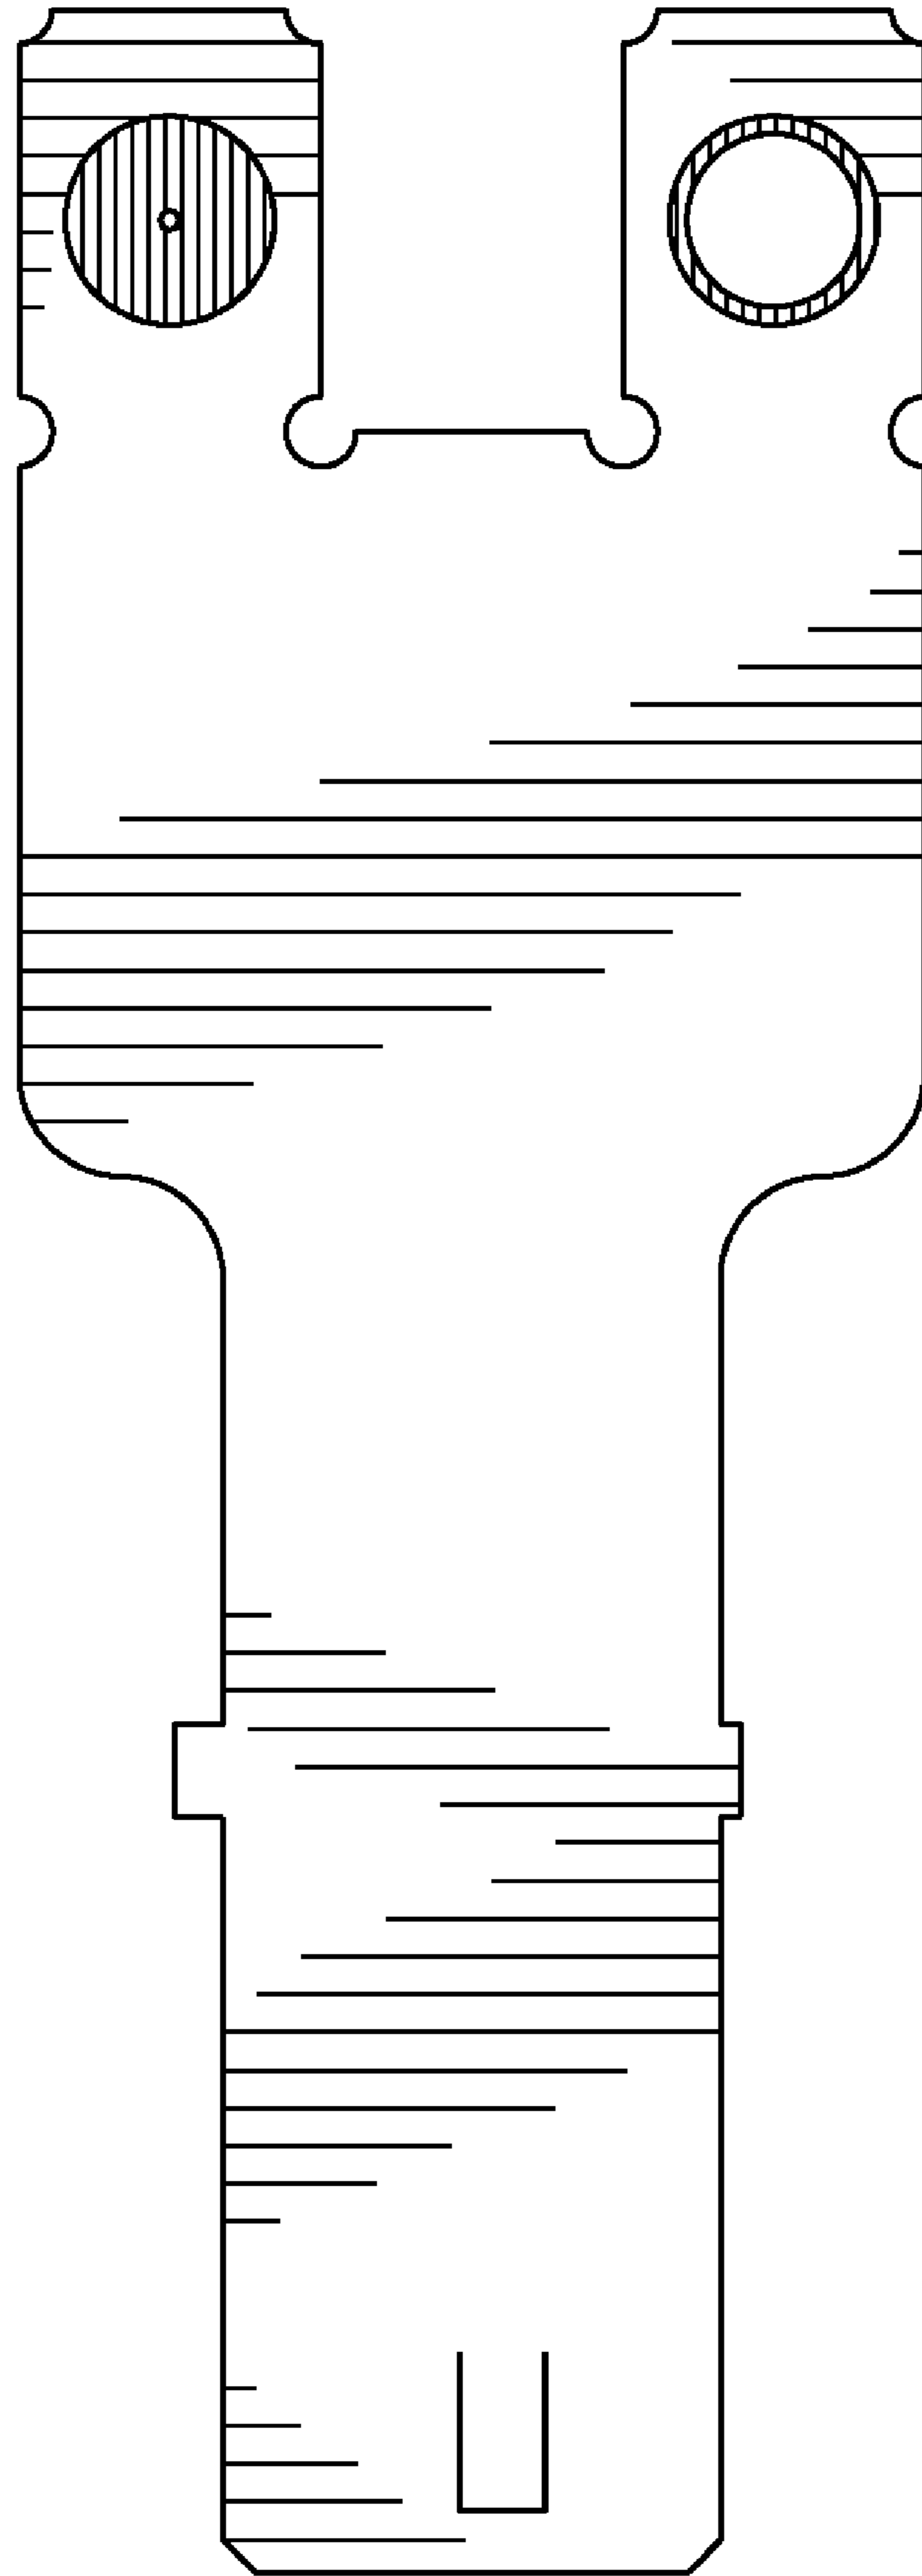


FIG. 6

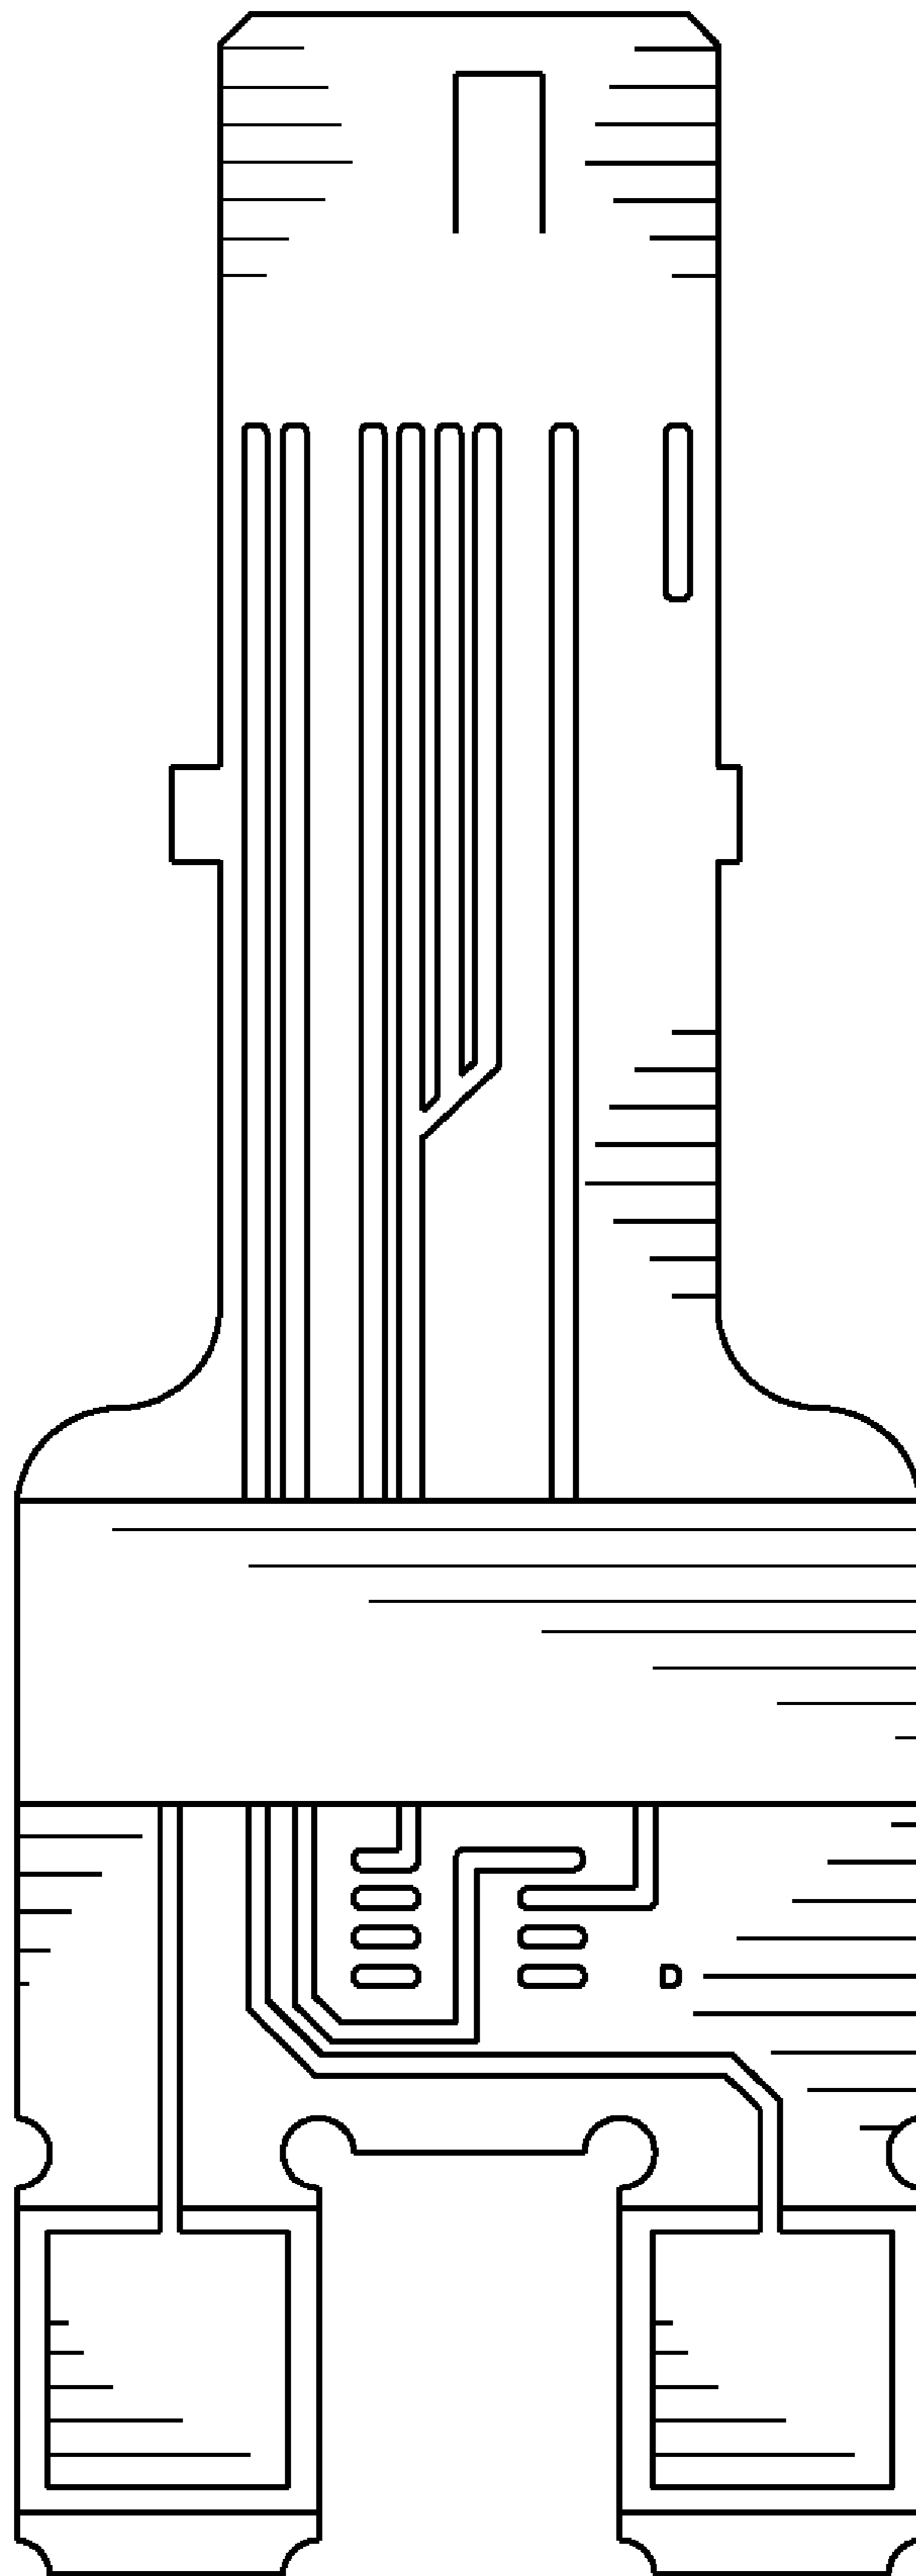


FIG. 7