

US00D601259S

(12) **United States Design Patent**
Guthrie et al.

(10) **Patent No.:** **US D601,259 S**
(45) **Date of Patent:** **** Sep. 29, 2009**

(54) **DOCKING CRADLE FOR A BLOOD
GLUCOSE METER**

(76) Inventors: **Brian Guthrie**, 48 Culduthel Mains
Crescent, Inverness (GB) IV2 6RG;
Allan Macrae, 20a Culcabock Avenue,
Inverness (GB) IV2 3RG; **Keith Lawrie**,
115 Towerhill Cres, Craddleshall,
Inverness (GB) IV2 5GZ; **Allan
Faulkner**, 9 High Street, Avoch,
Ross-Shire (GB) IV9 8PT

(**) Term: **14 Years**

(21) Appl. No.: **29/326,928**

(22) Filed: **Oct. 27, 2008**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Classification Search** D24/107,
D24/158, 165–169, 186, 232; D10/70, 78,
D10/81, 98, 104; D14/149, 151, 168, 253,
D14/341, 371, 374–375; 600/309, 316, 322,
600/365, 368; 422/56–58, 61, 68.1, 102,
422/104; 435/16; 436/168–169, 183; 455/404.1;
379/428.4, 441, 446, 454–455

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D275,482 S * 9/1984 Coons et al. D14/253
D286,437 S * 10/1986 Nishibori D24/165
D319,100 S * 8/1991 Umemoto et al. D24/169
D331,286 S * 11/1992 Cameron et al. D24/169
D348,265 S * 6/1994 Nagele D14/151
D361,129 S * 8/1995 Collins et al. D24/169

D381,748 S * 7/1997 Matsuda et al. D24/169
D393,314 S * 4/1998 Meisner et al. D24/169
6,088,605 A * 7/2000 Griffith et al. 600/316
D441,867 S * 5/2001 Belisle et al. D24/169
D445,190 S * 7/2001 Byler et al. D24/165
D446,306 S * 8/2001 Ochi et al. D24/186
D462,771 S * 9/2002 Weber D24/169
D496,732 S * 9/2004 Nagai et al. D24/169
D508,565 S * 8/2005 Nephin et al. D24/186
D533,279 S * 12/2006 Kobayashi et al. D24/165
D537,944 S * 3/2007 Eda et al. D24/165
D583,060 S * 12/2008 Kitamura et al. D24/165
D584,975 S * 1/2009 Haberstroh D10/81

* cited by examiner

Primary Examiner—Philip S Hyder

Assistant Examiner—Susan E Krakower

(57) **CLAIM**

We claim the ornamental design for an docking cradle for a blood glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is one perspective view of the docking cradle for a blood glucose meter, as viewed from a top position;

FIG. 2 is another perspective view of the docking cradle for a blood glucose meter, as viewed from a bottom position;

FIG. 3 is a top plan view thereof;

FIG. 4 is a front elevational view thereof;


FIG. 5 is a back elevational view thereof;

FIG. 6 is a bottom plan view thereof; and

FIG. 7 is a side elevational view thereof; and,

FIG. 8 is another side elevational view thereof.

1 Claim, 4 Drawing Sheets

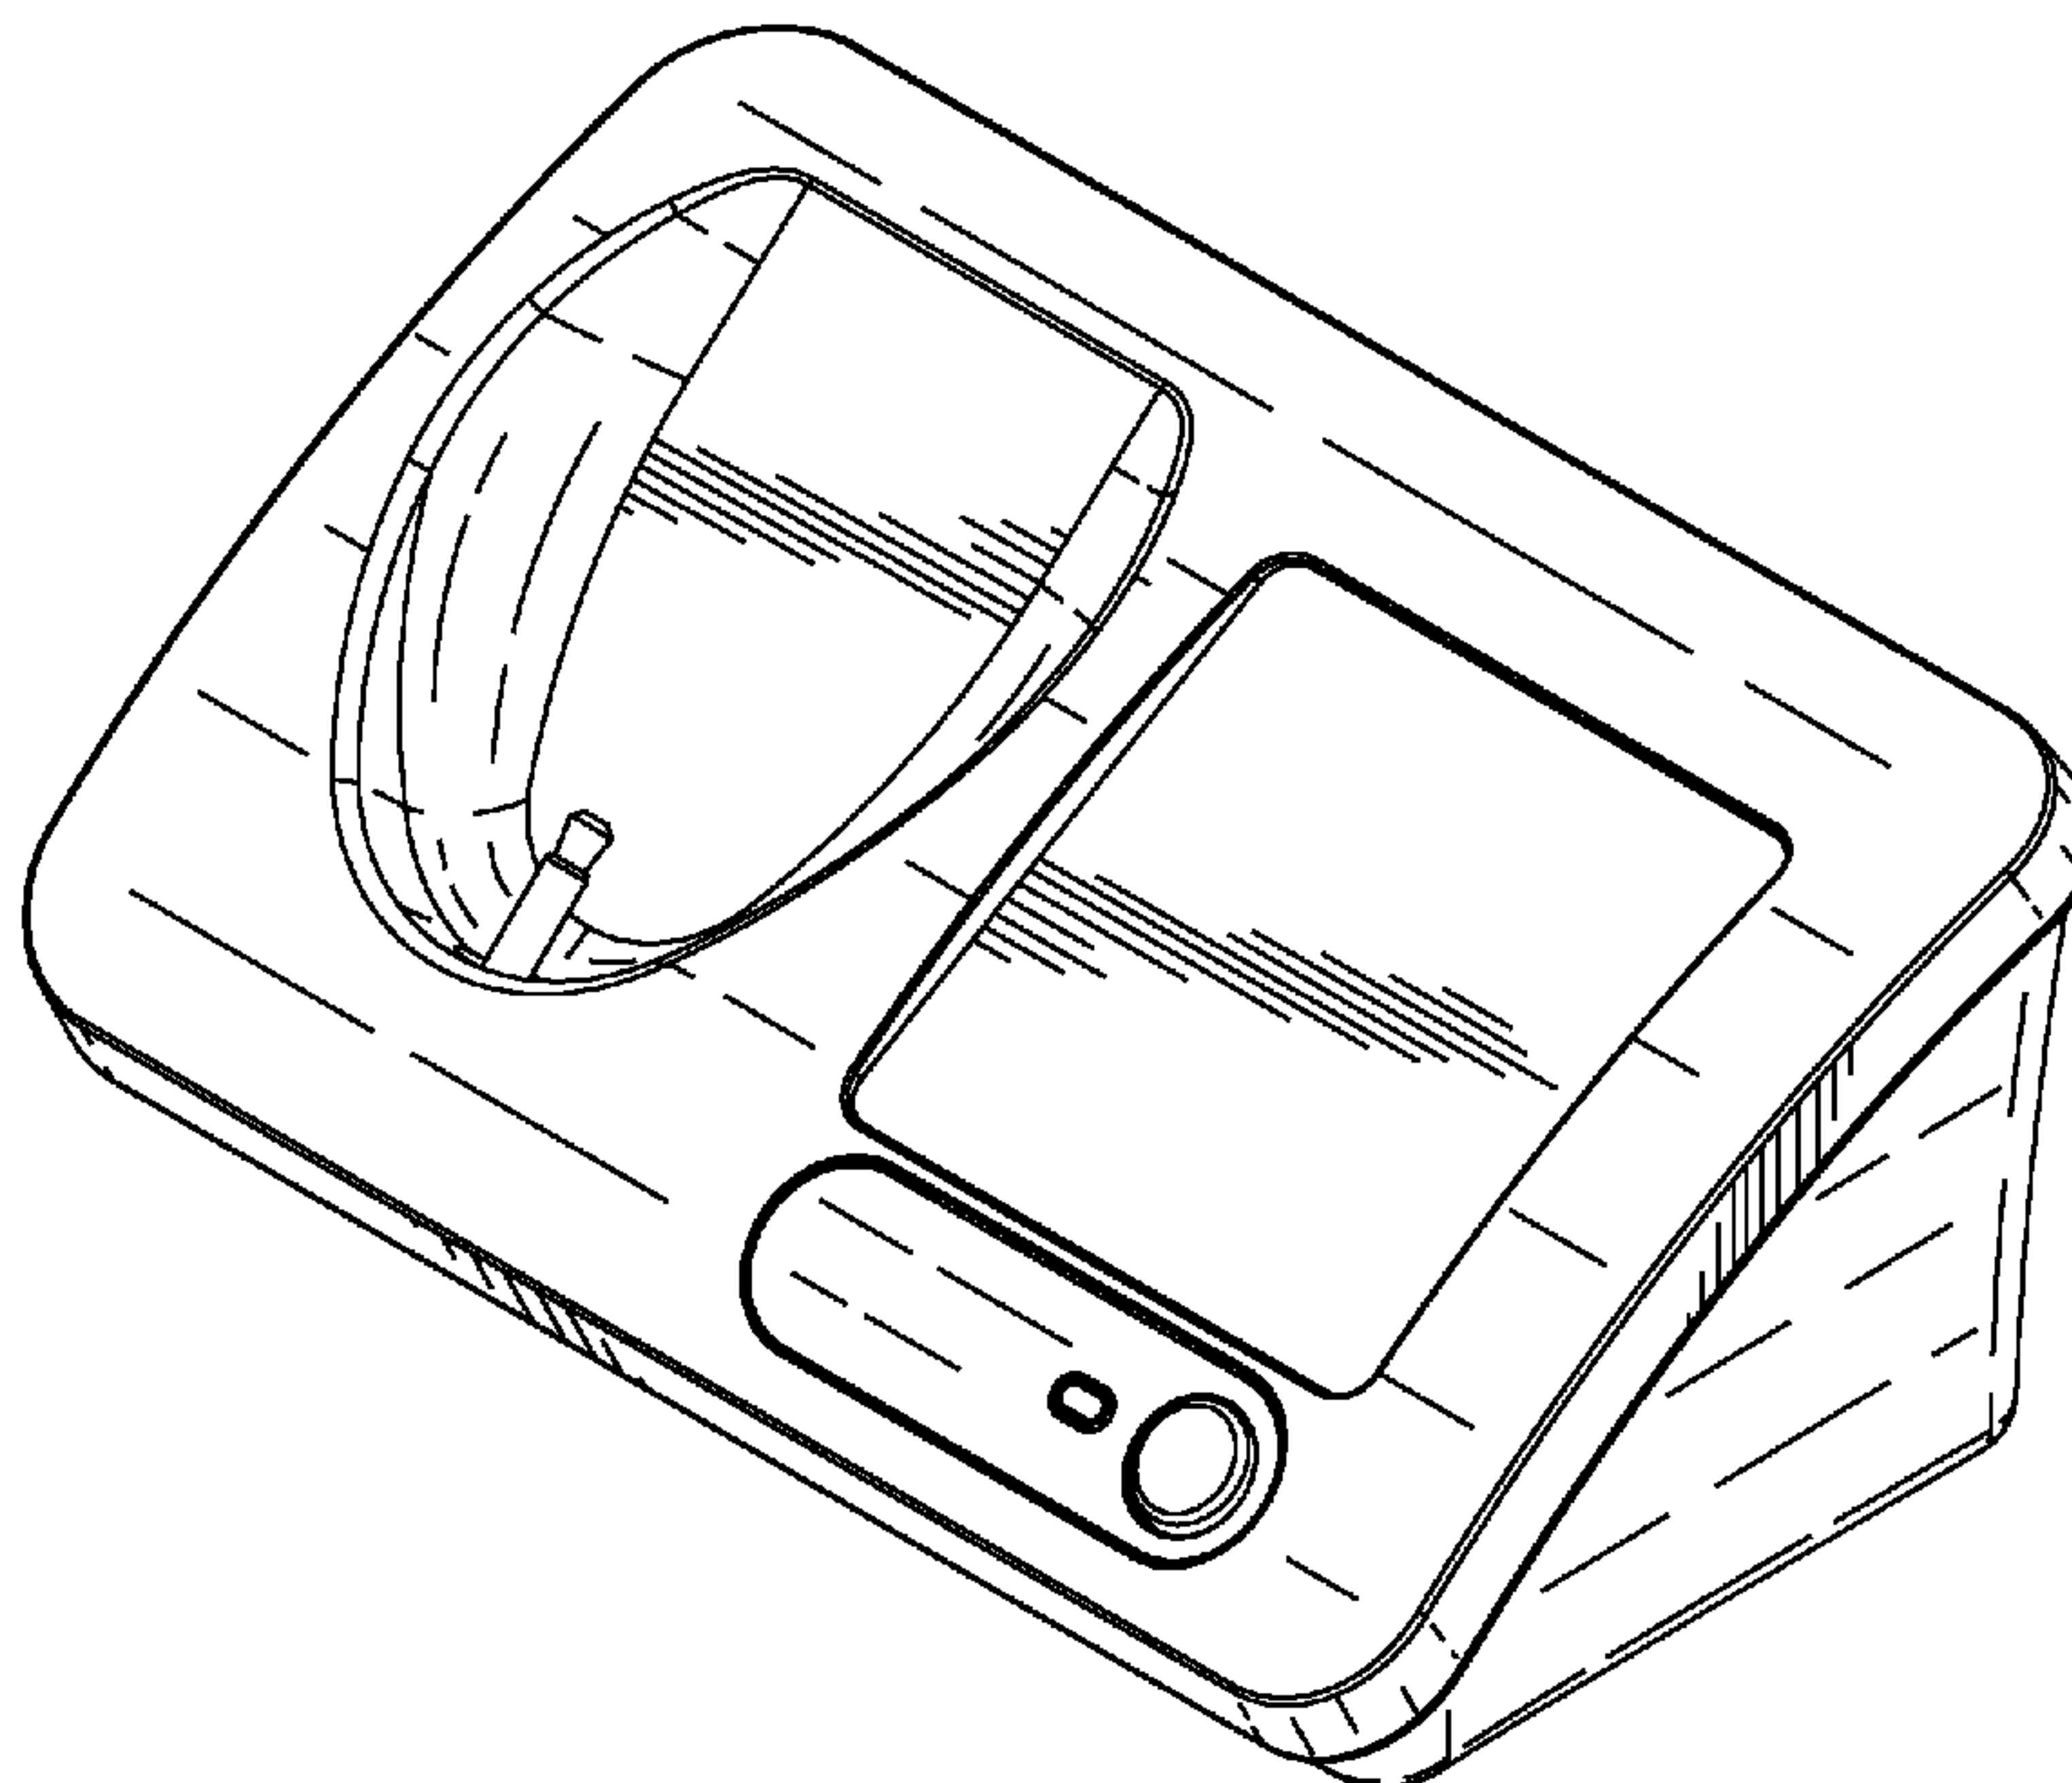

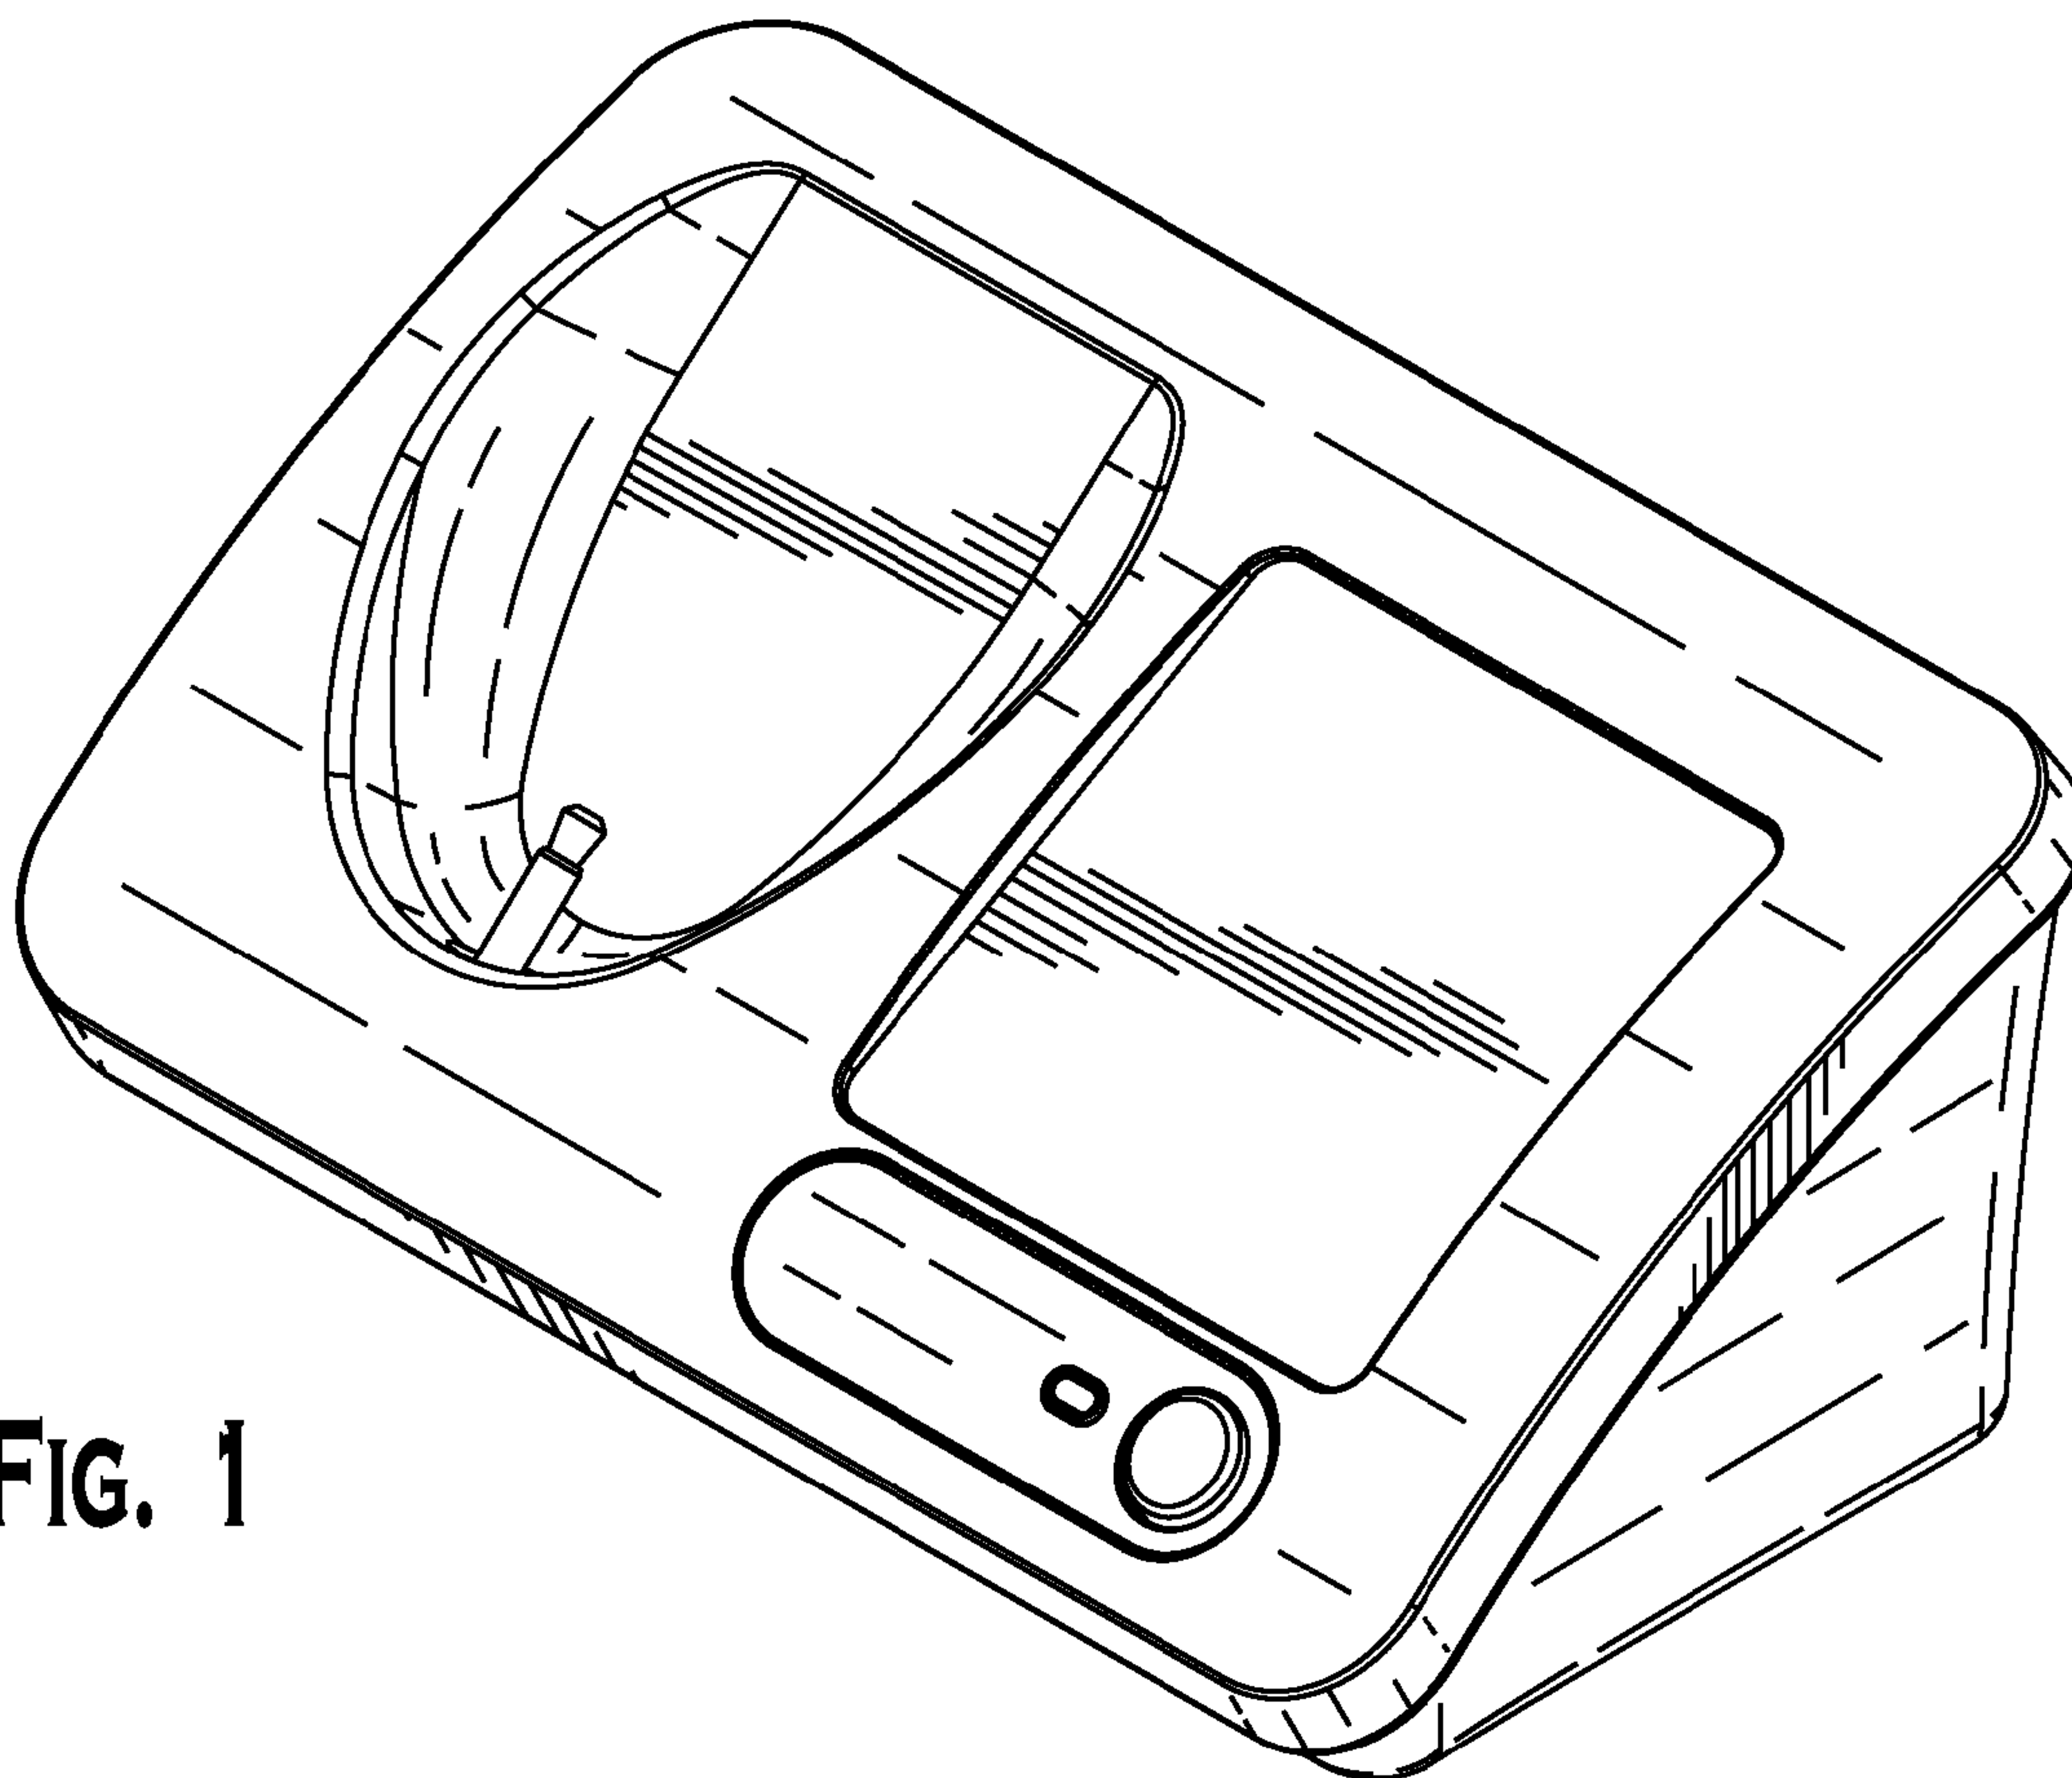


FIG. 1

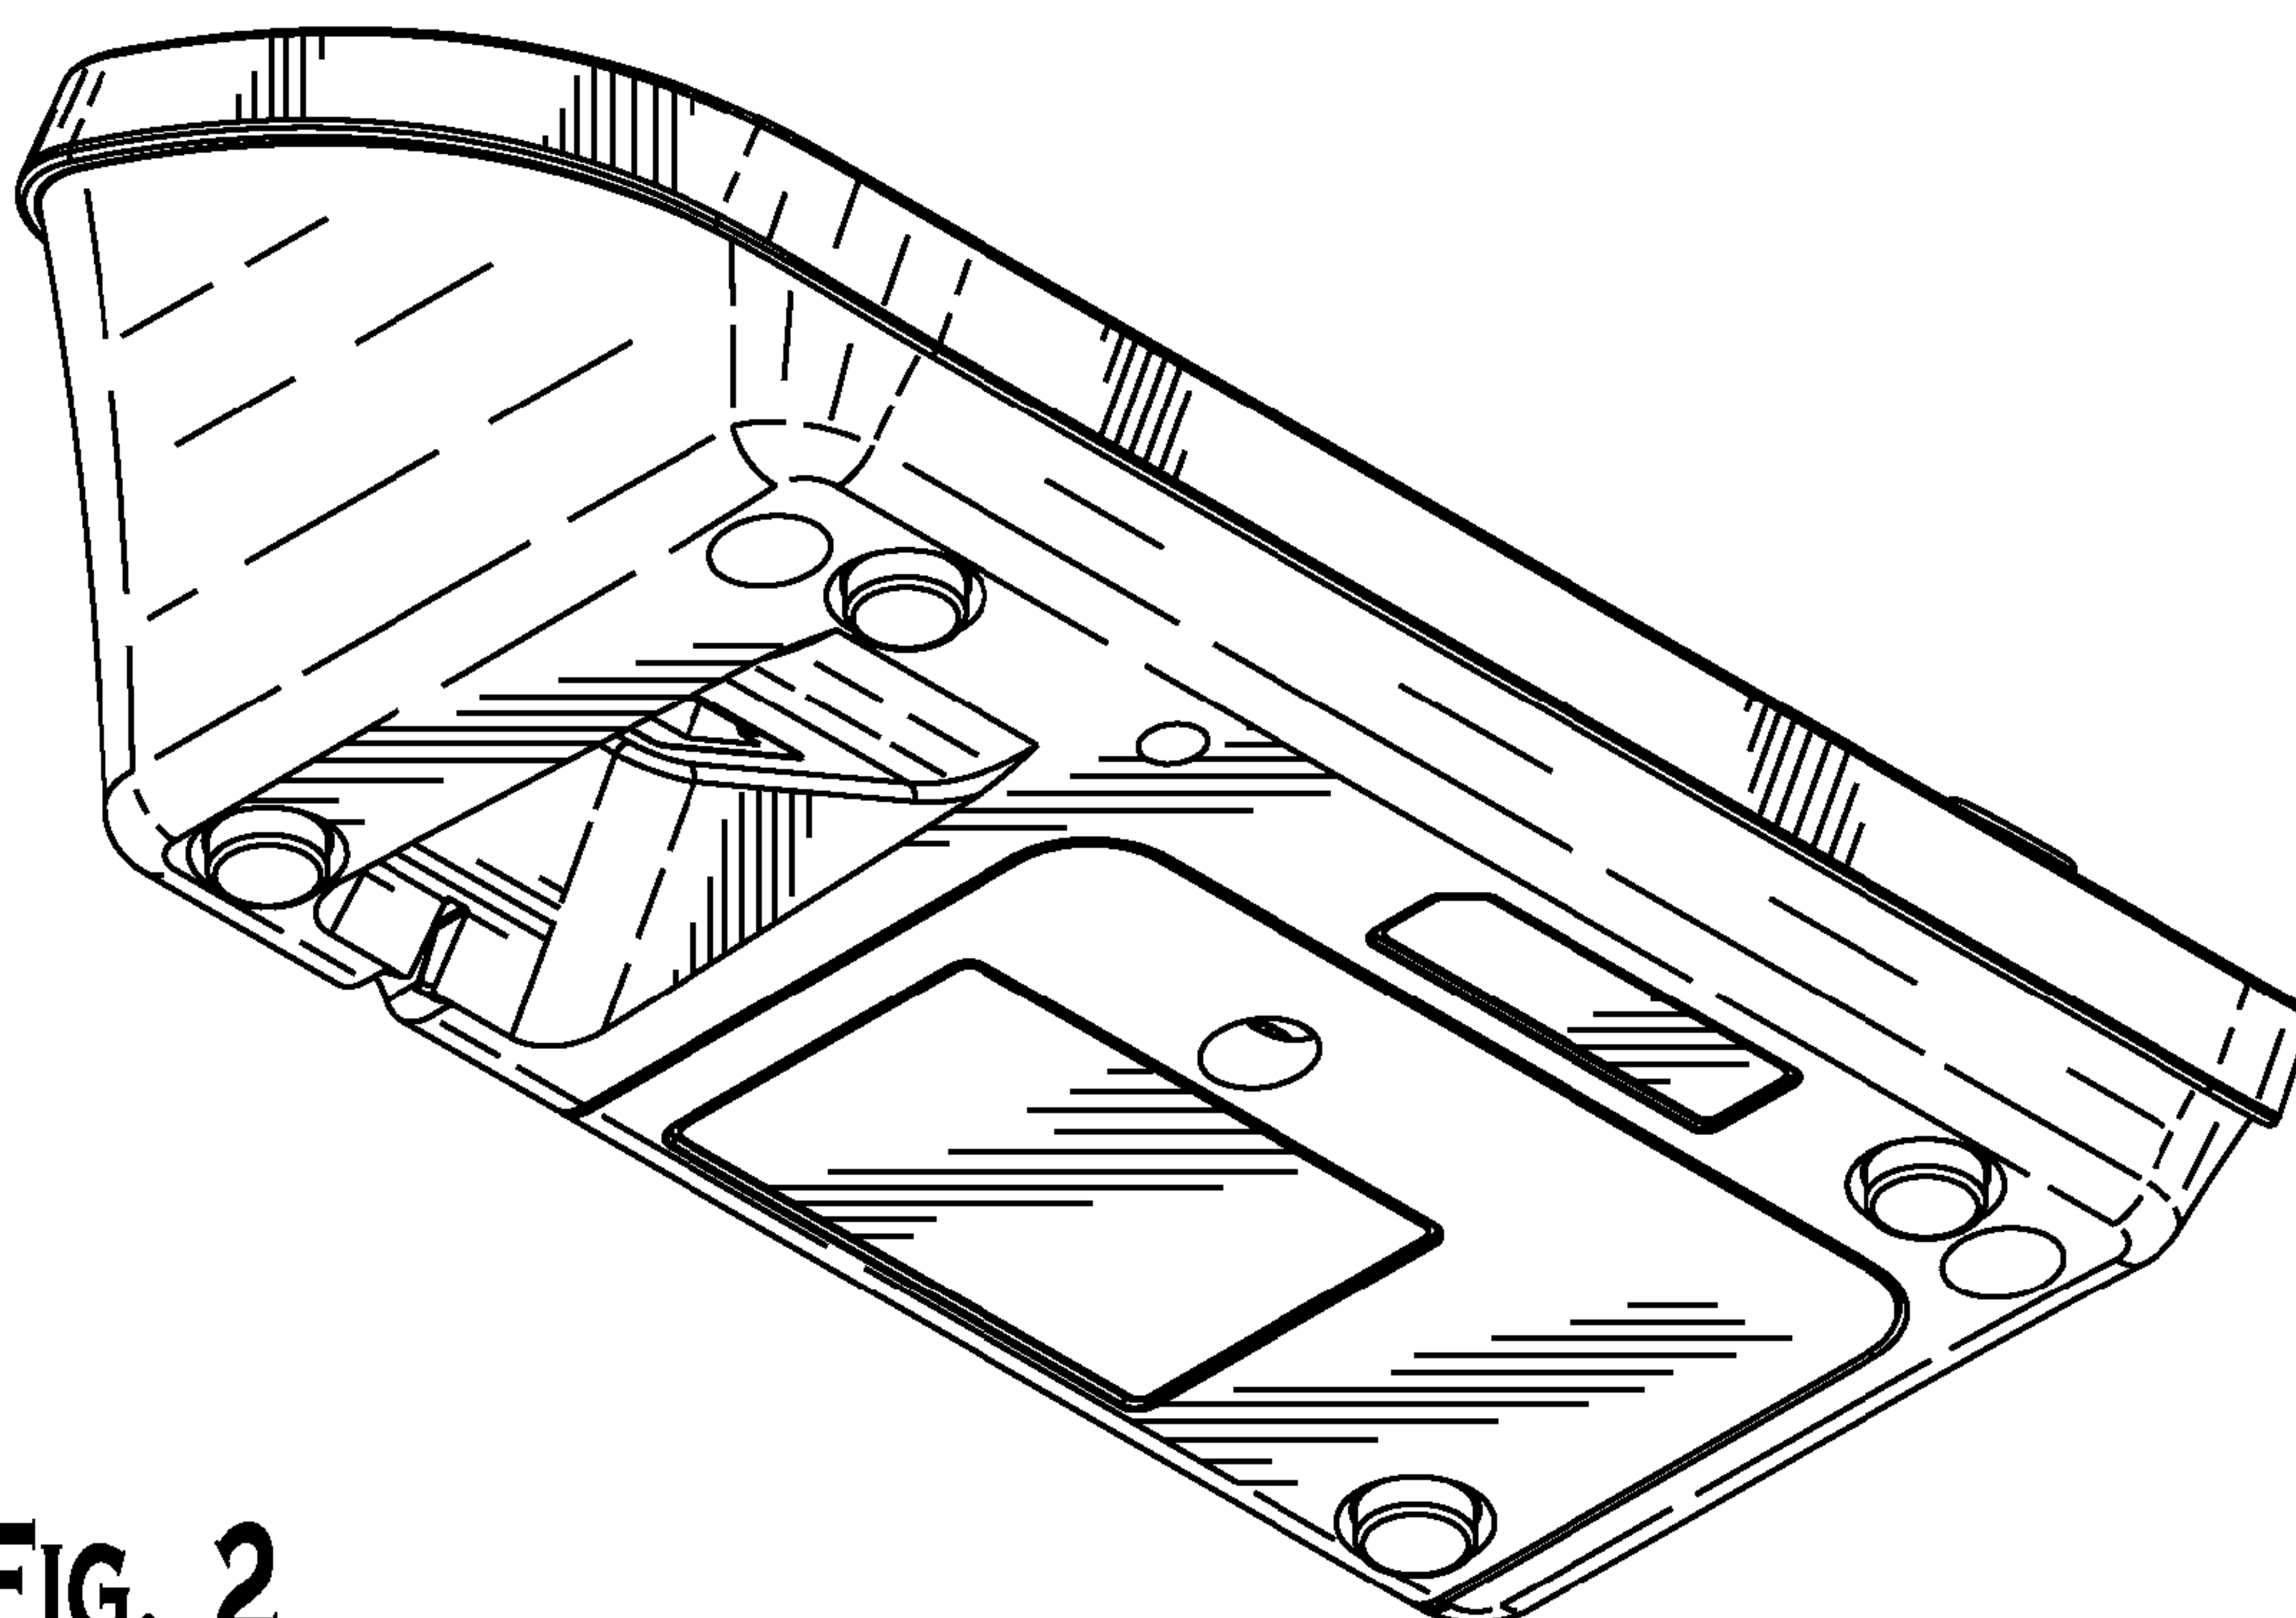


FIG. 2

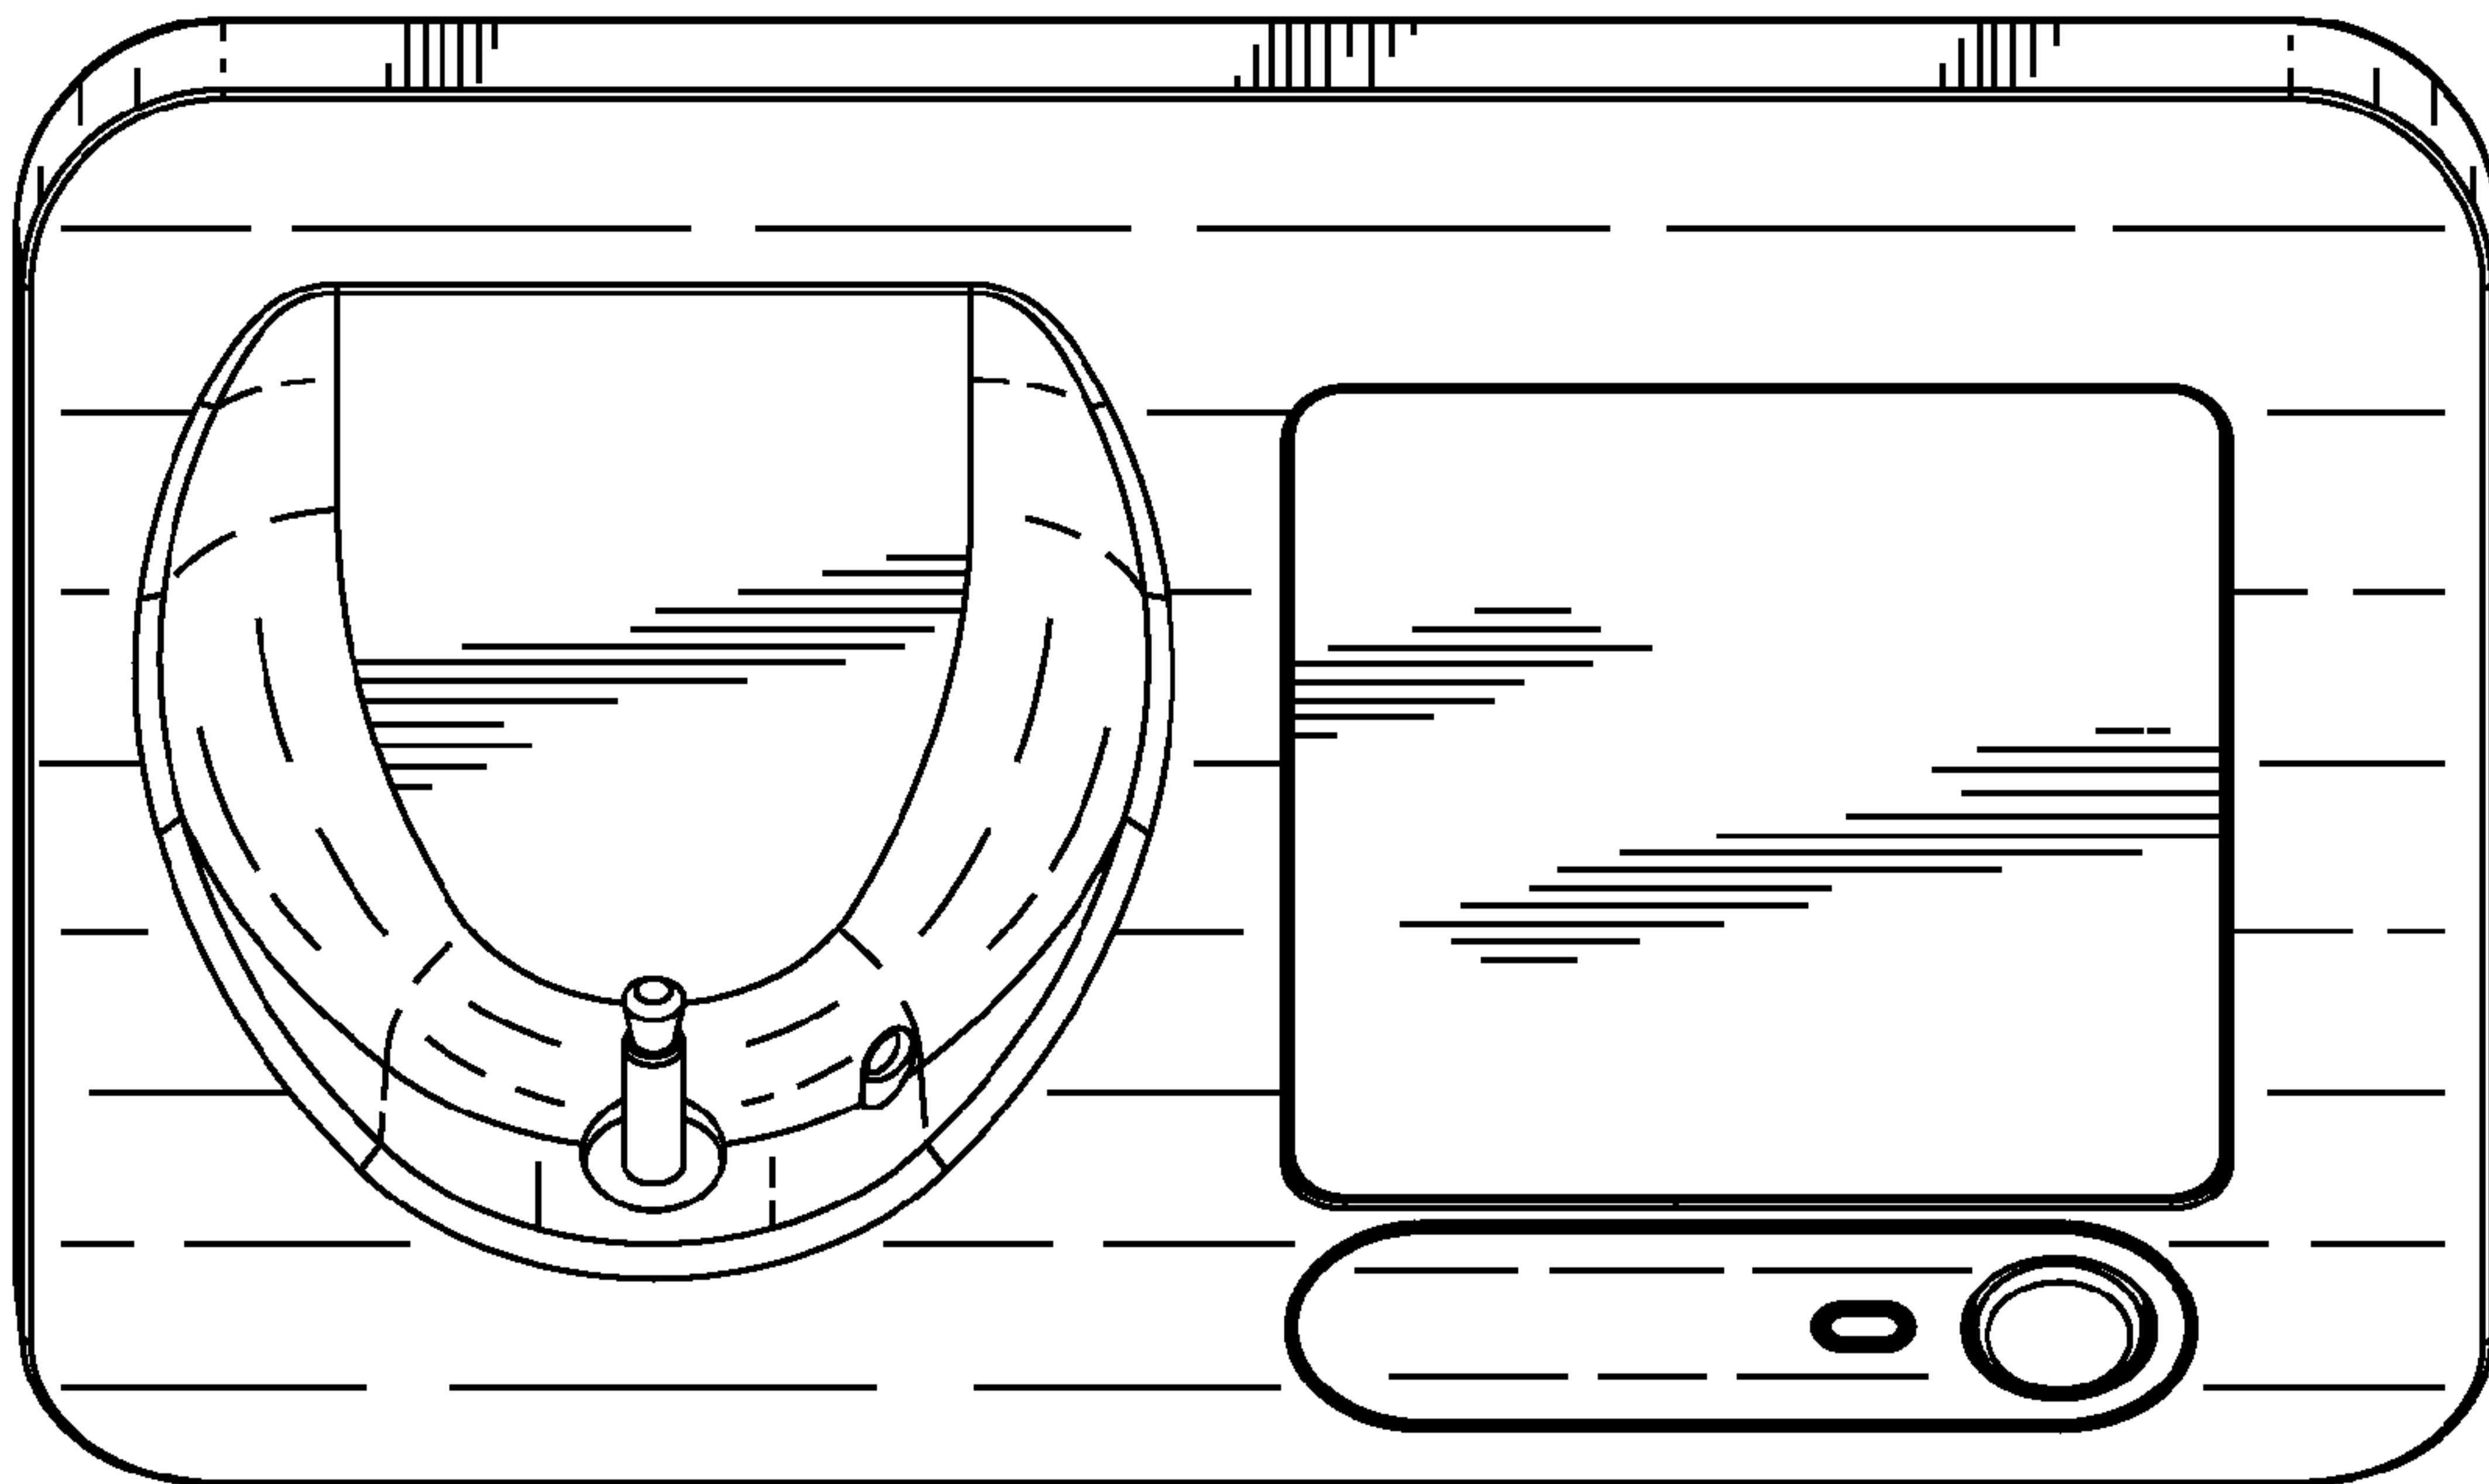


FIG. 3

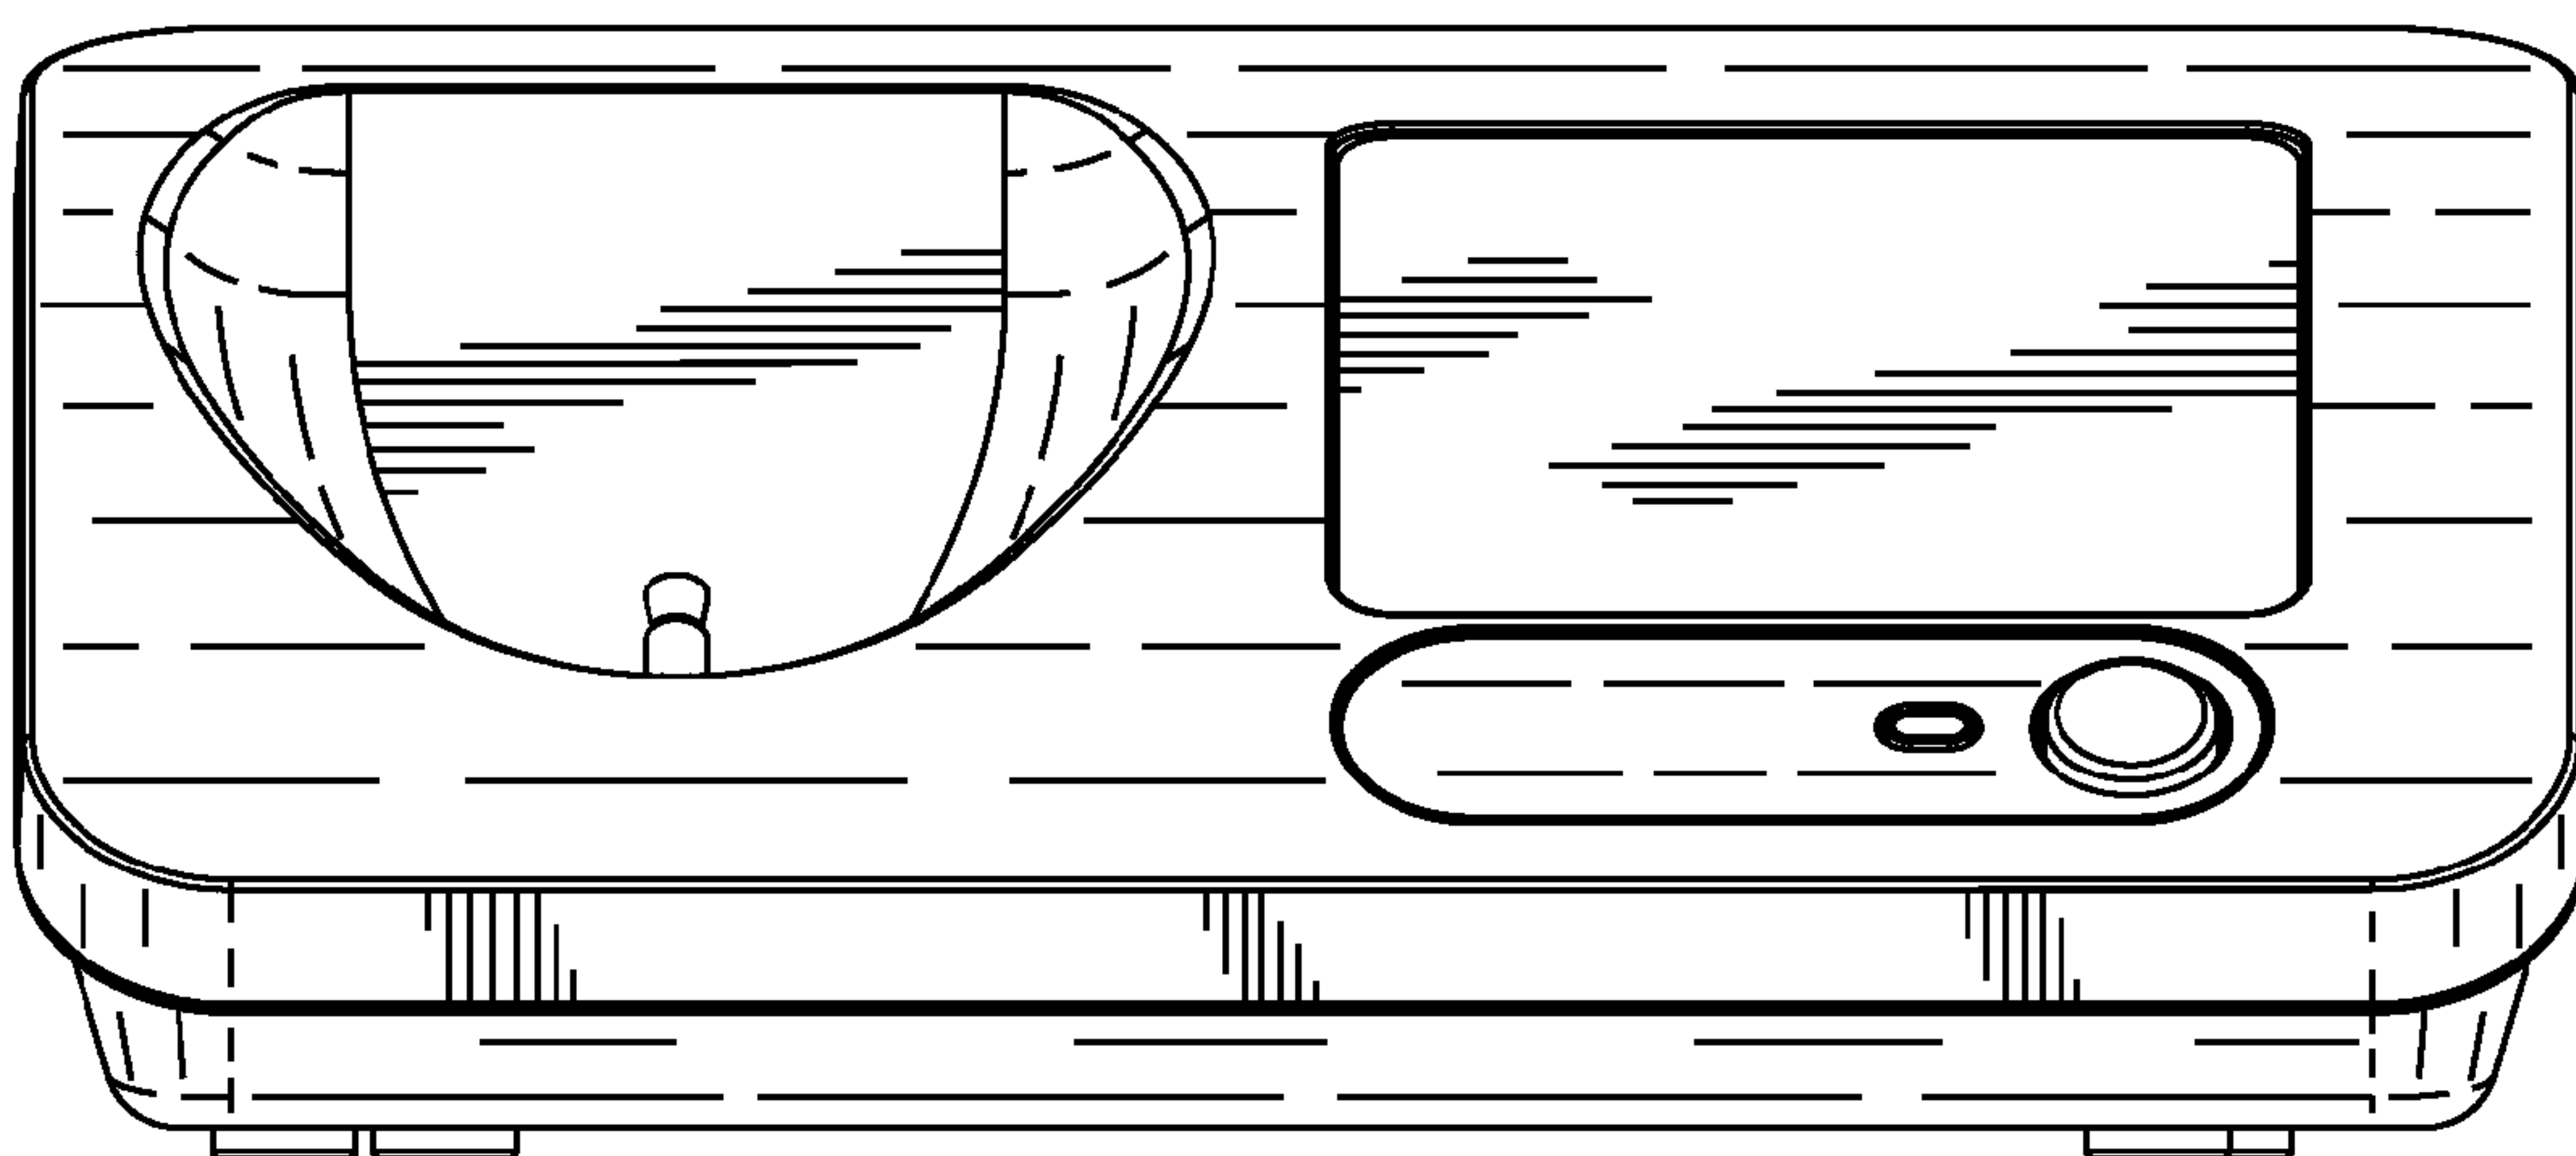


FIG. 4

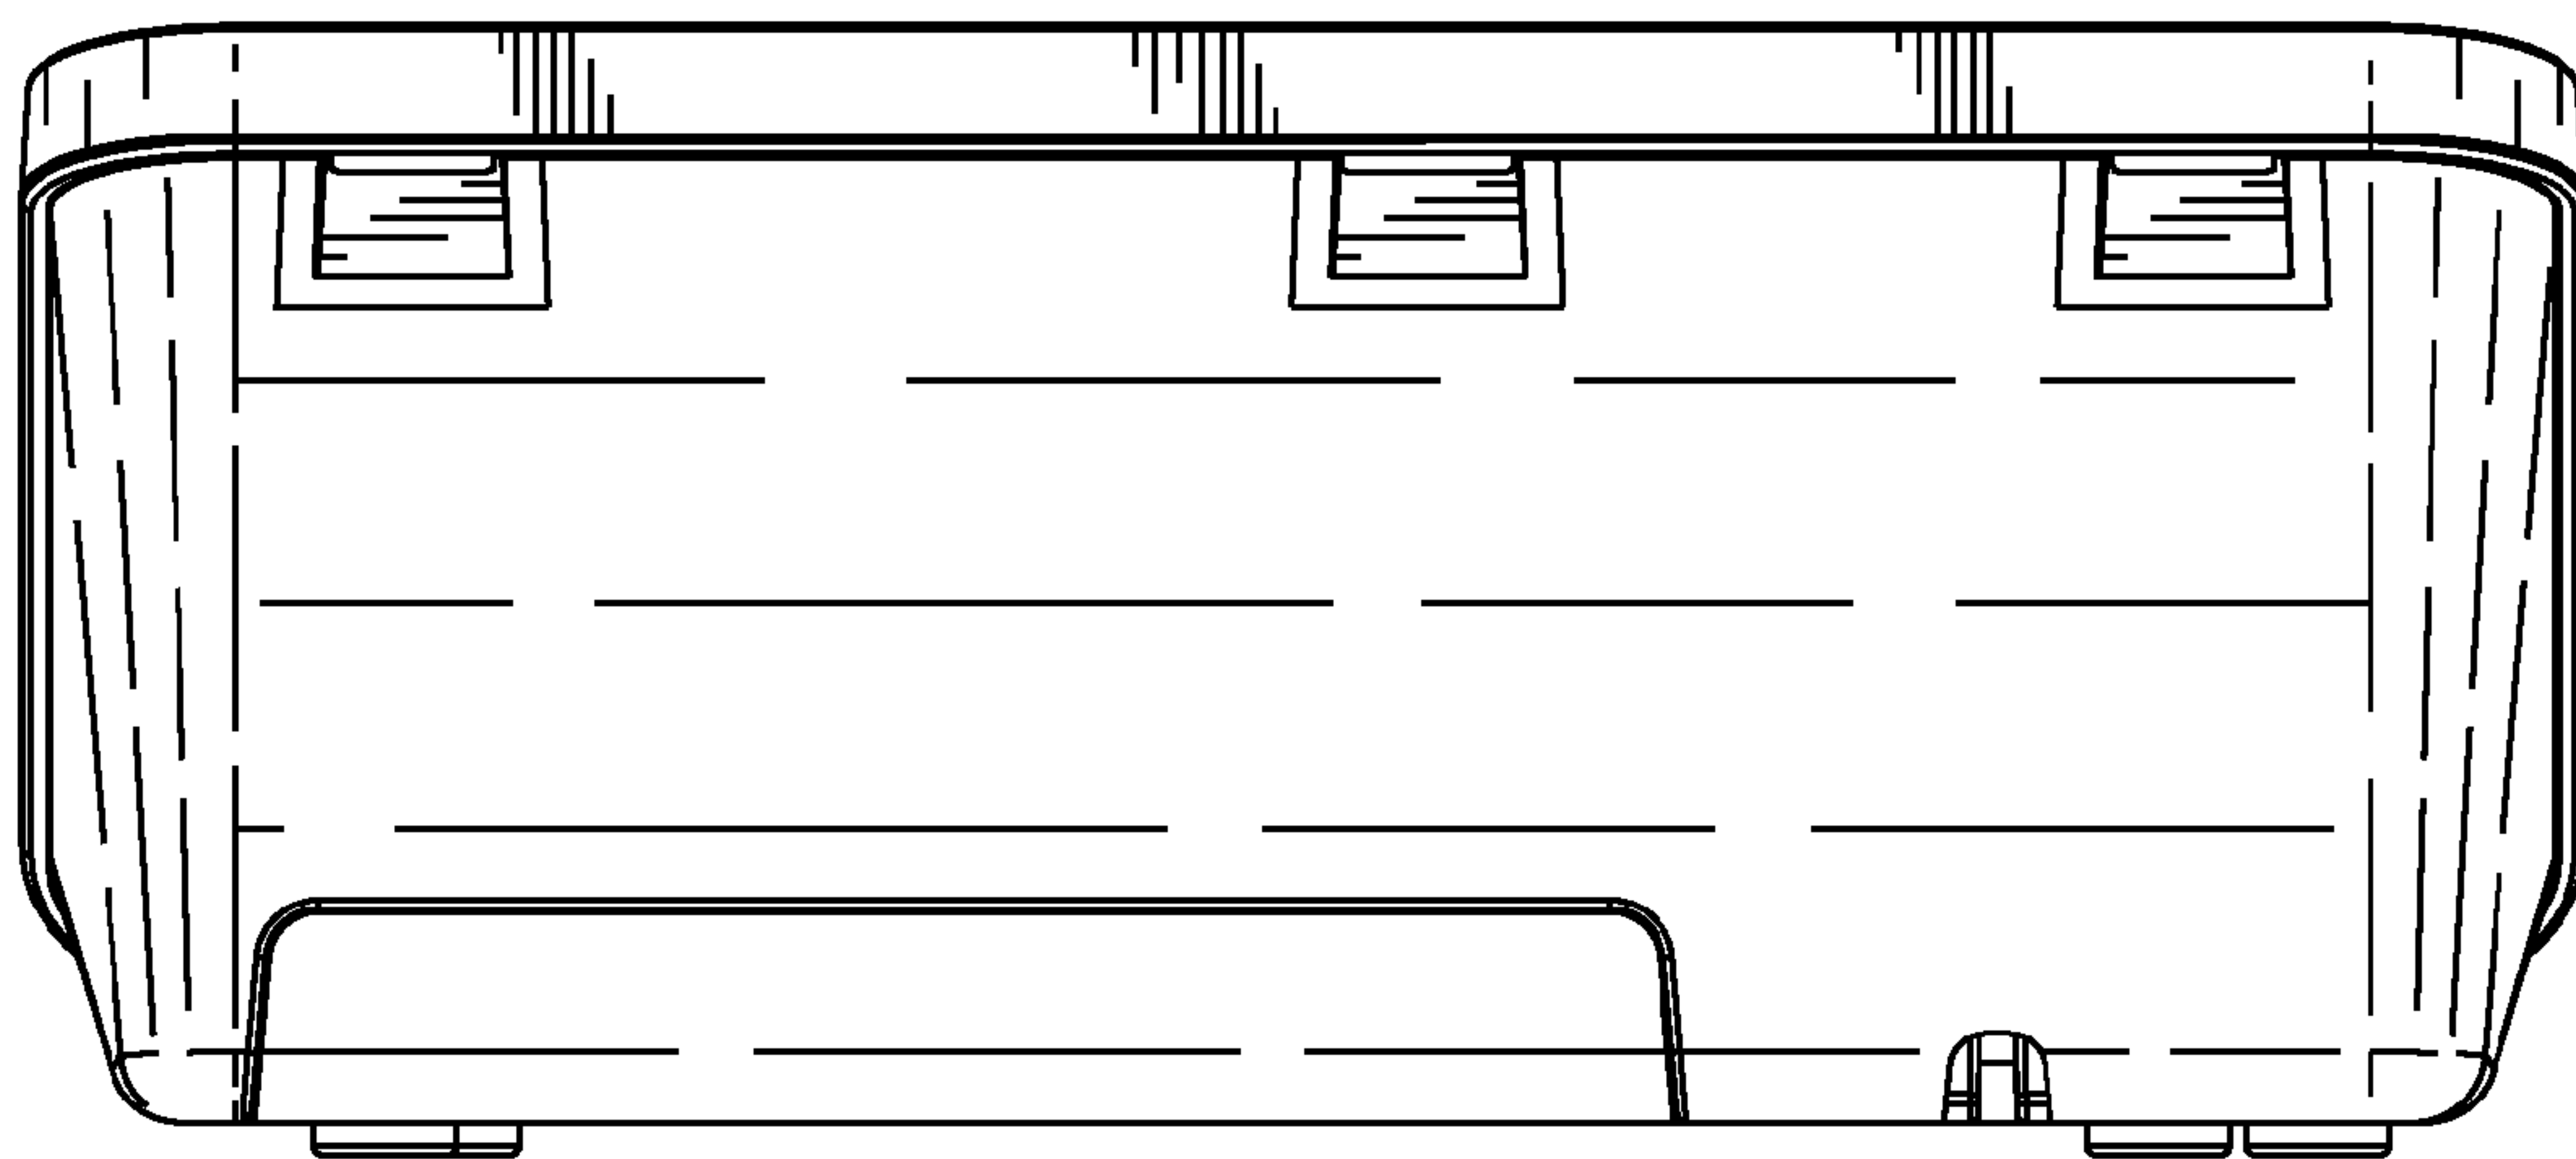


FIG. 5

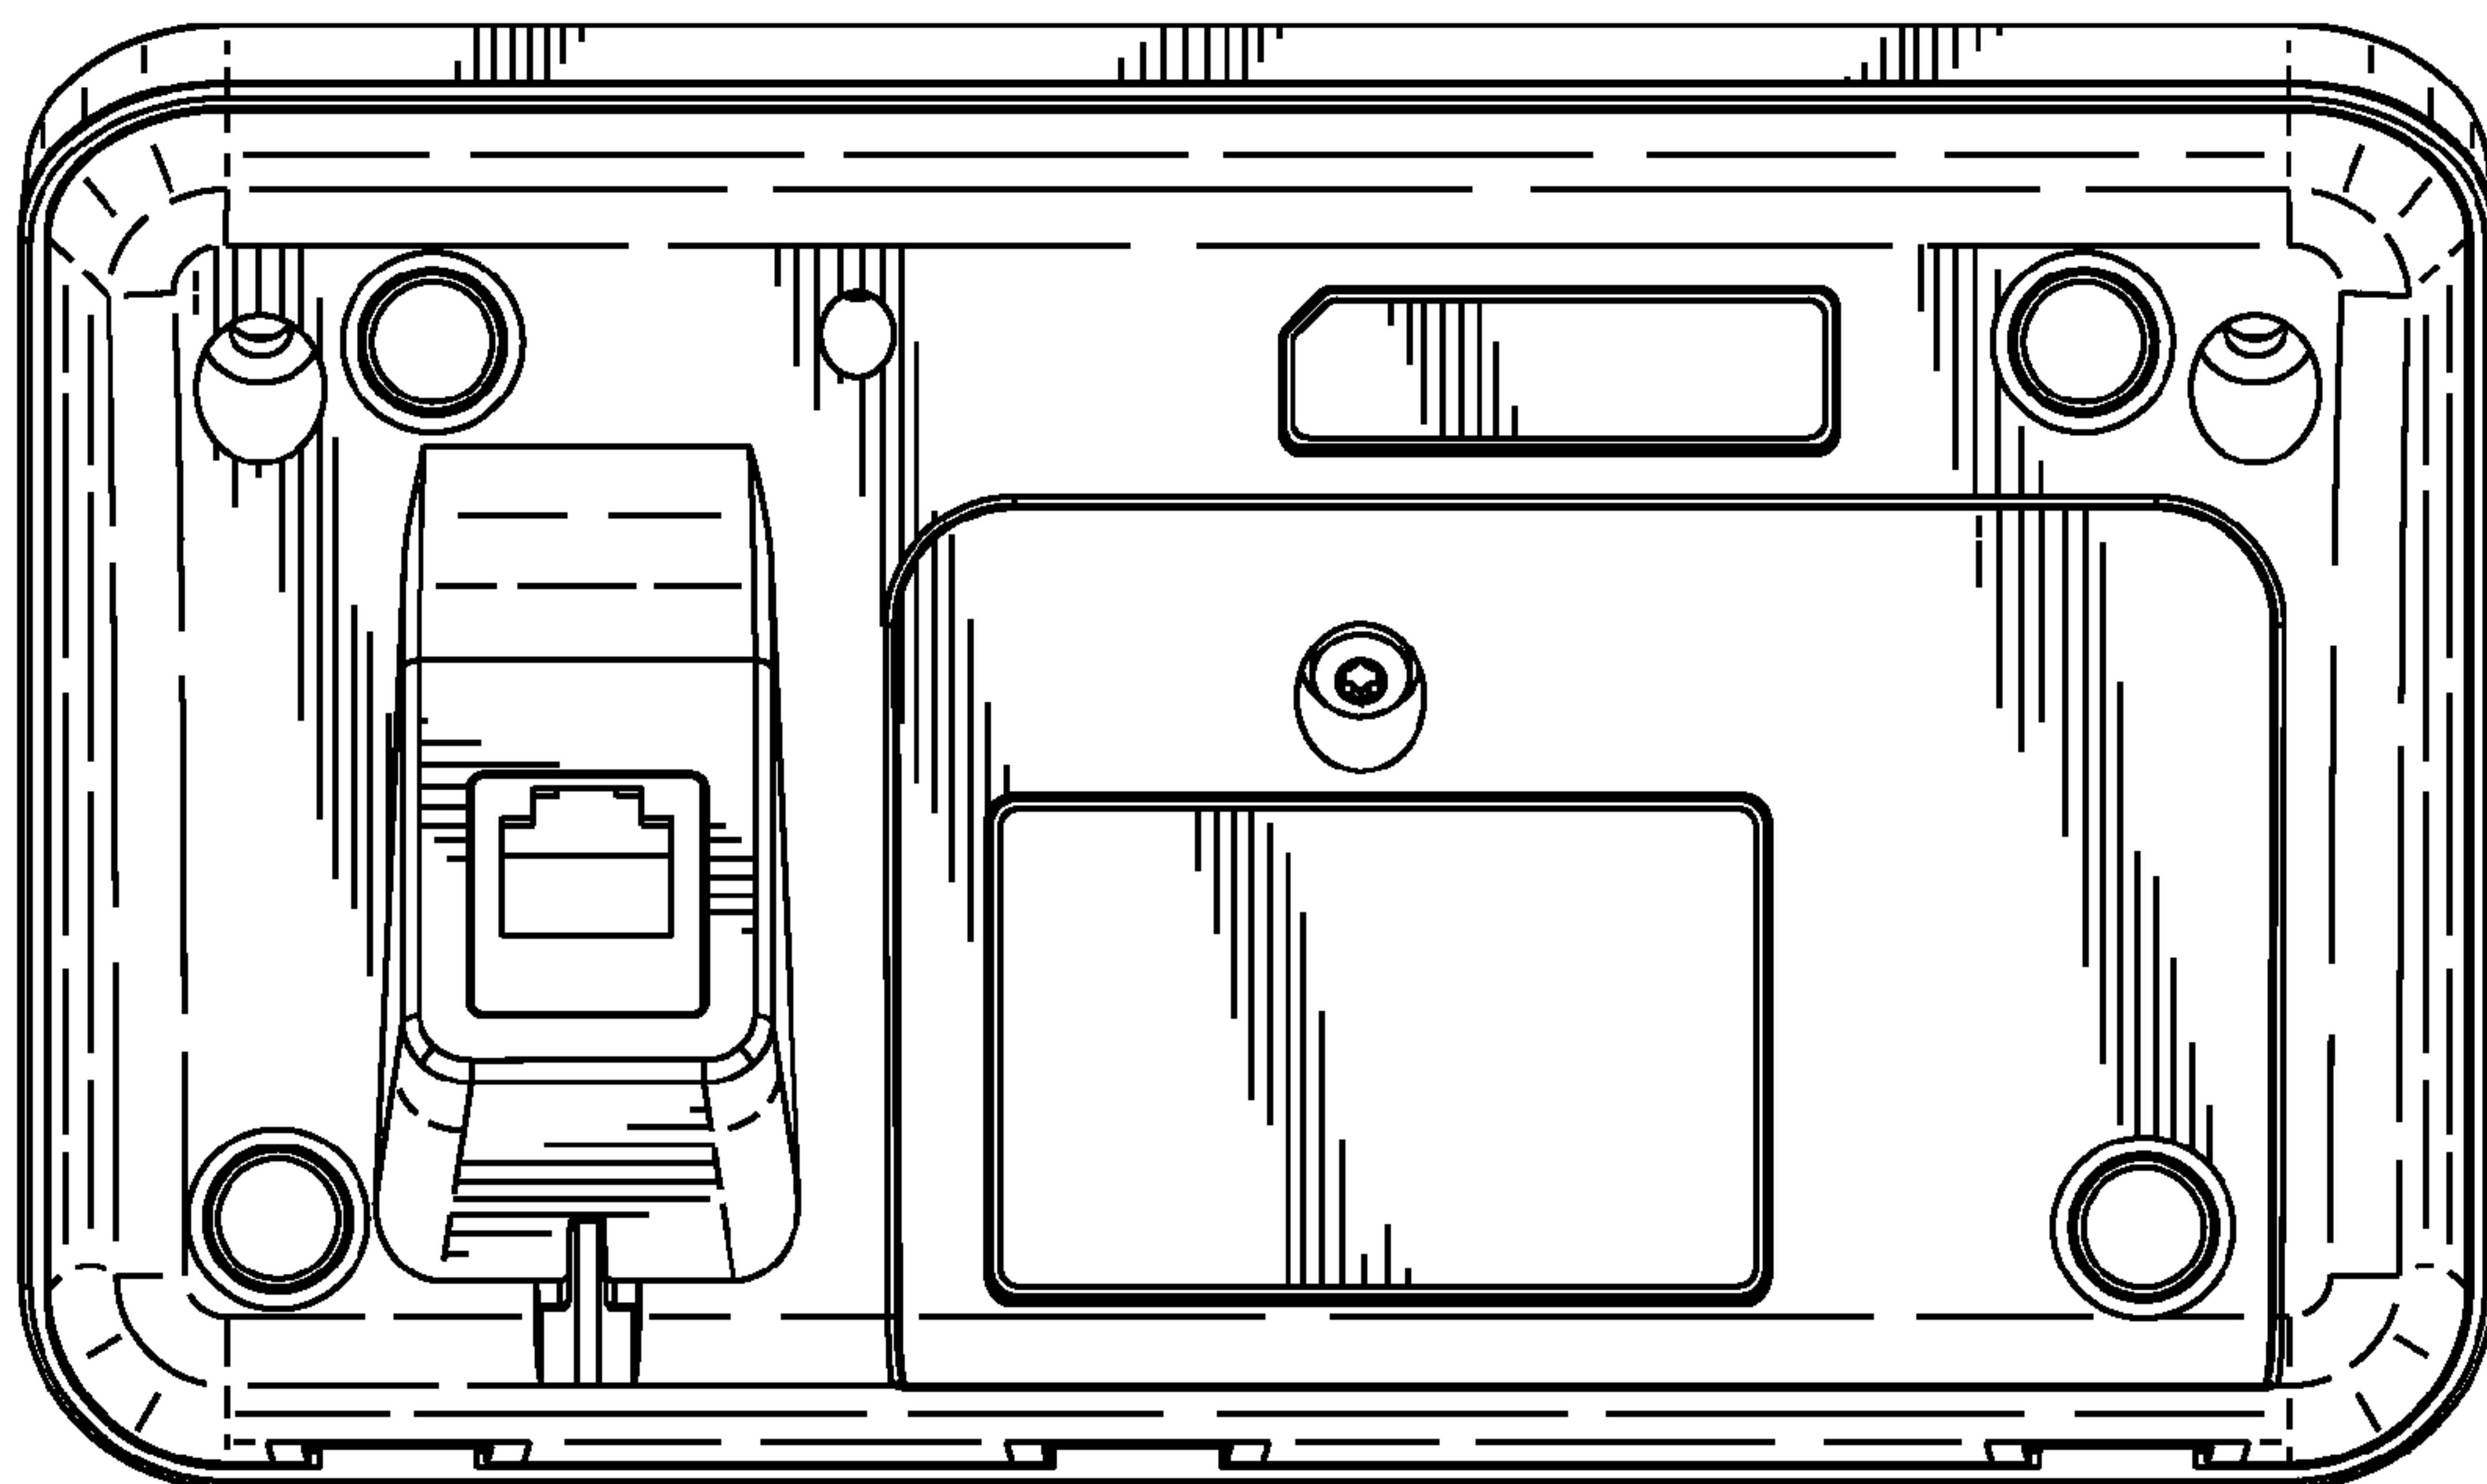


FIG. 6

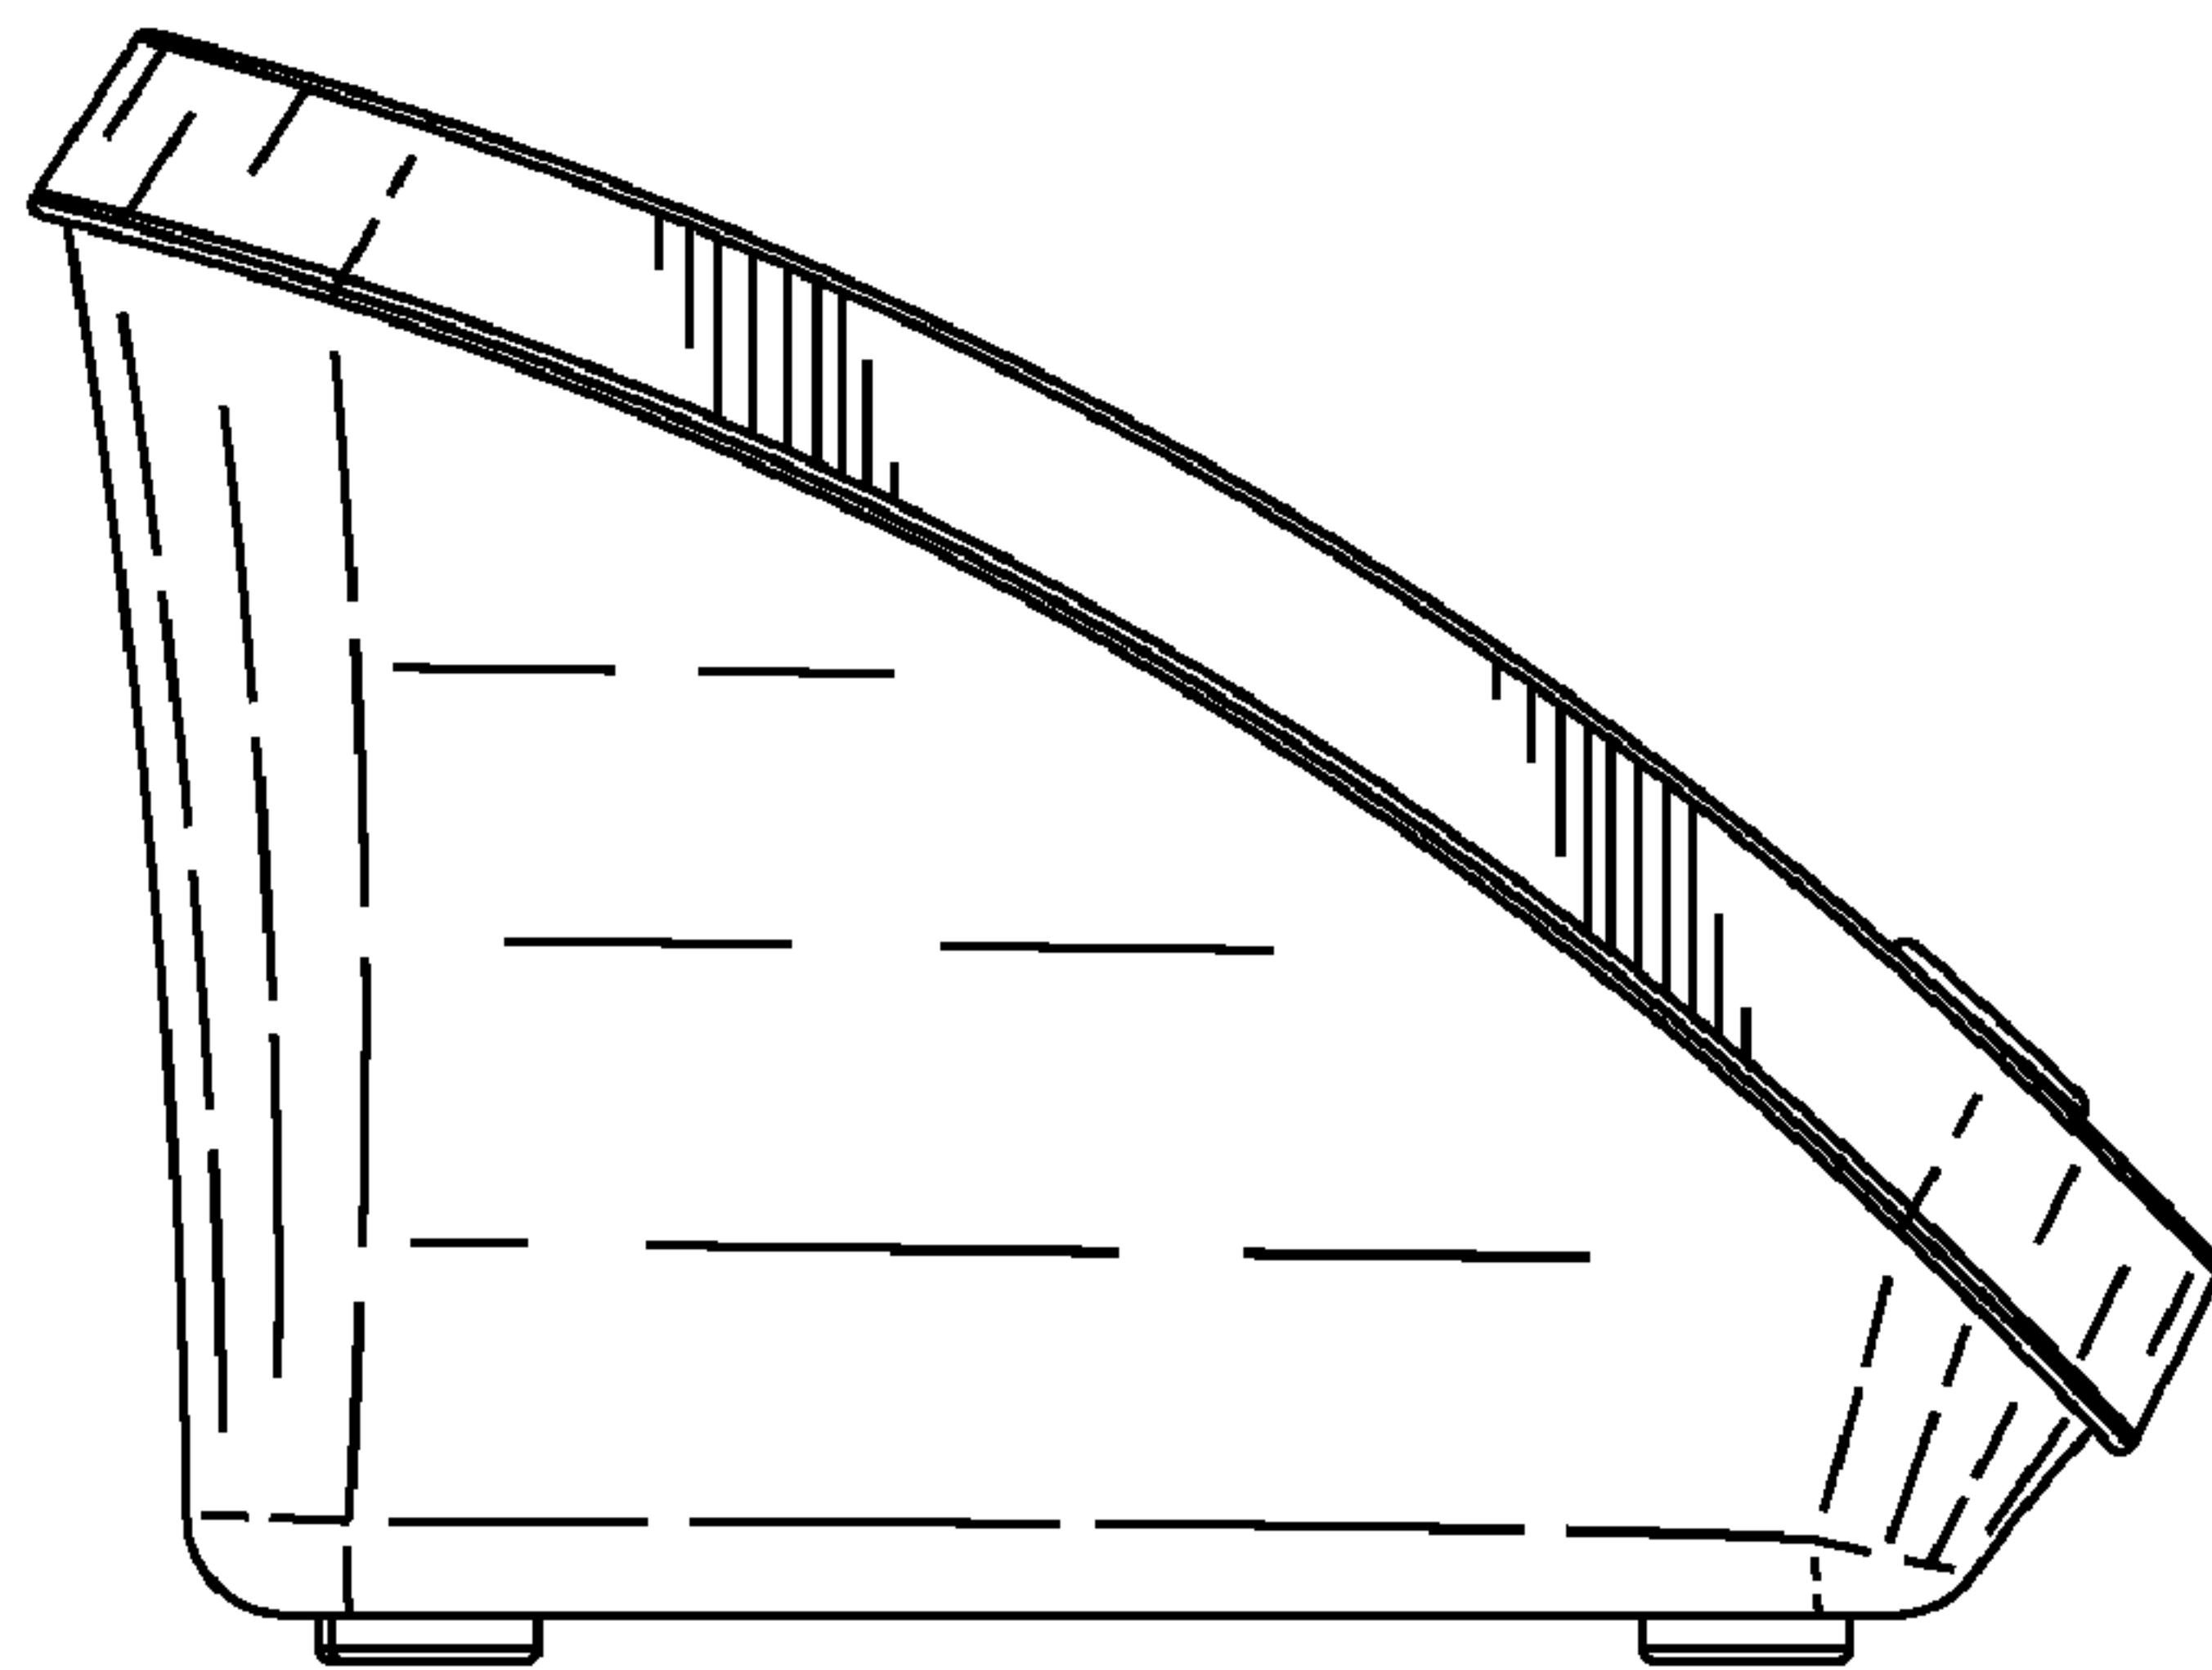


FIG. 7

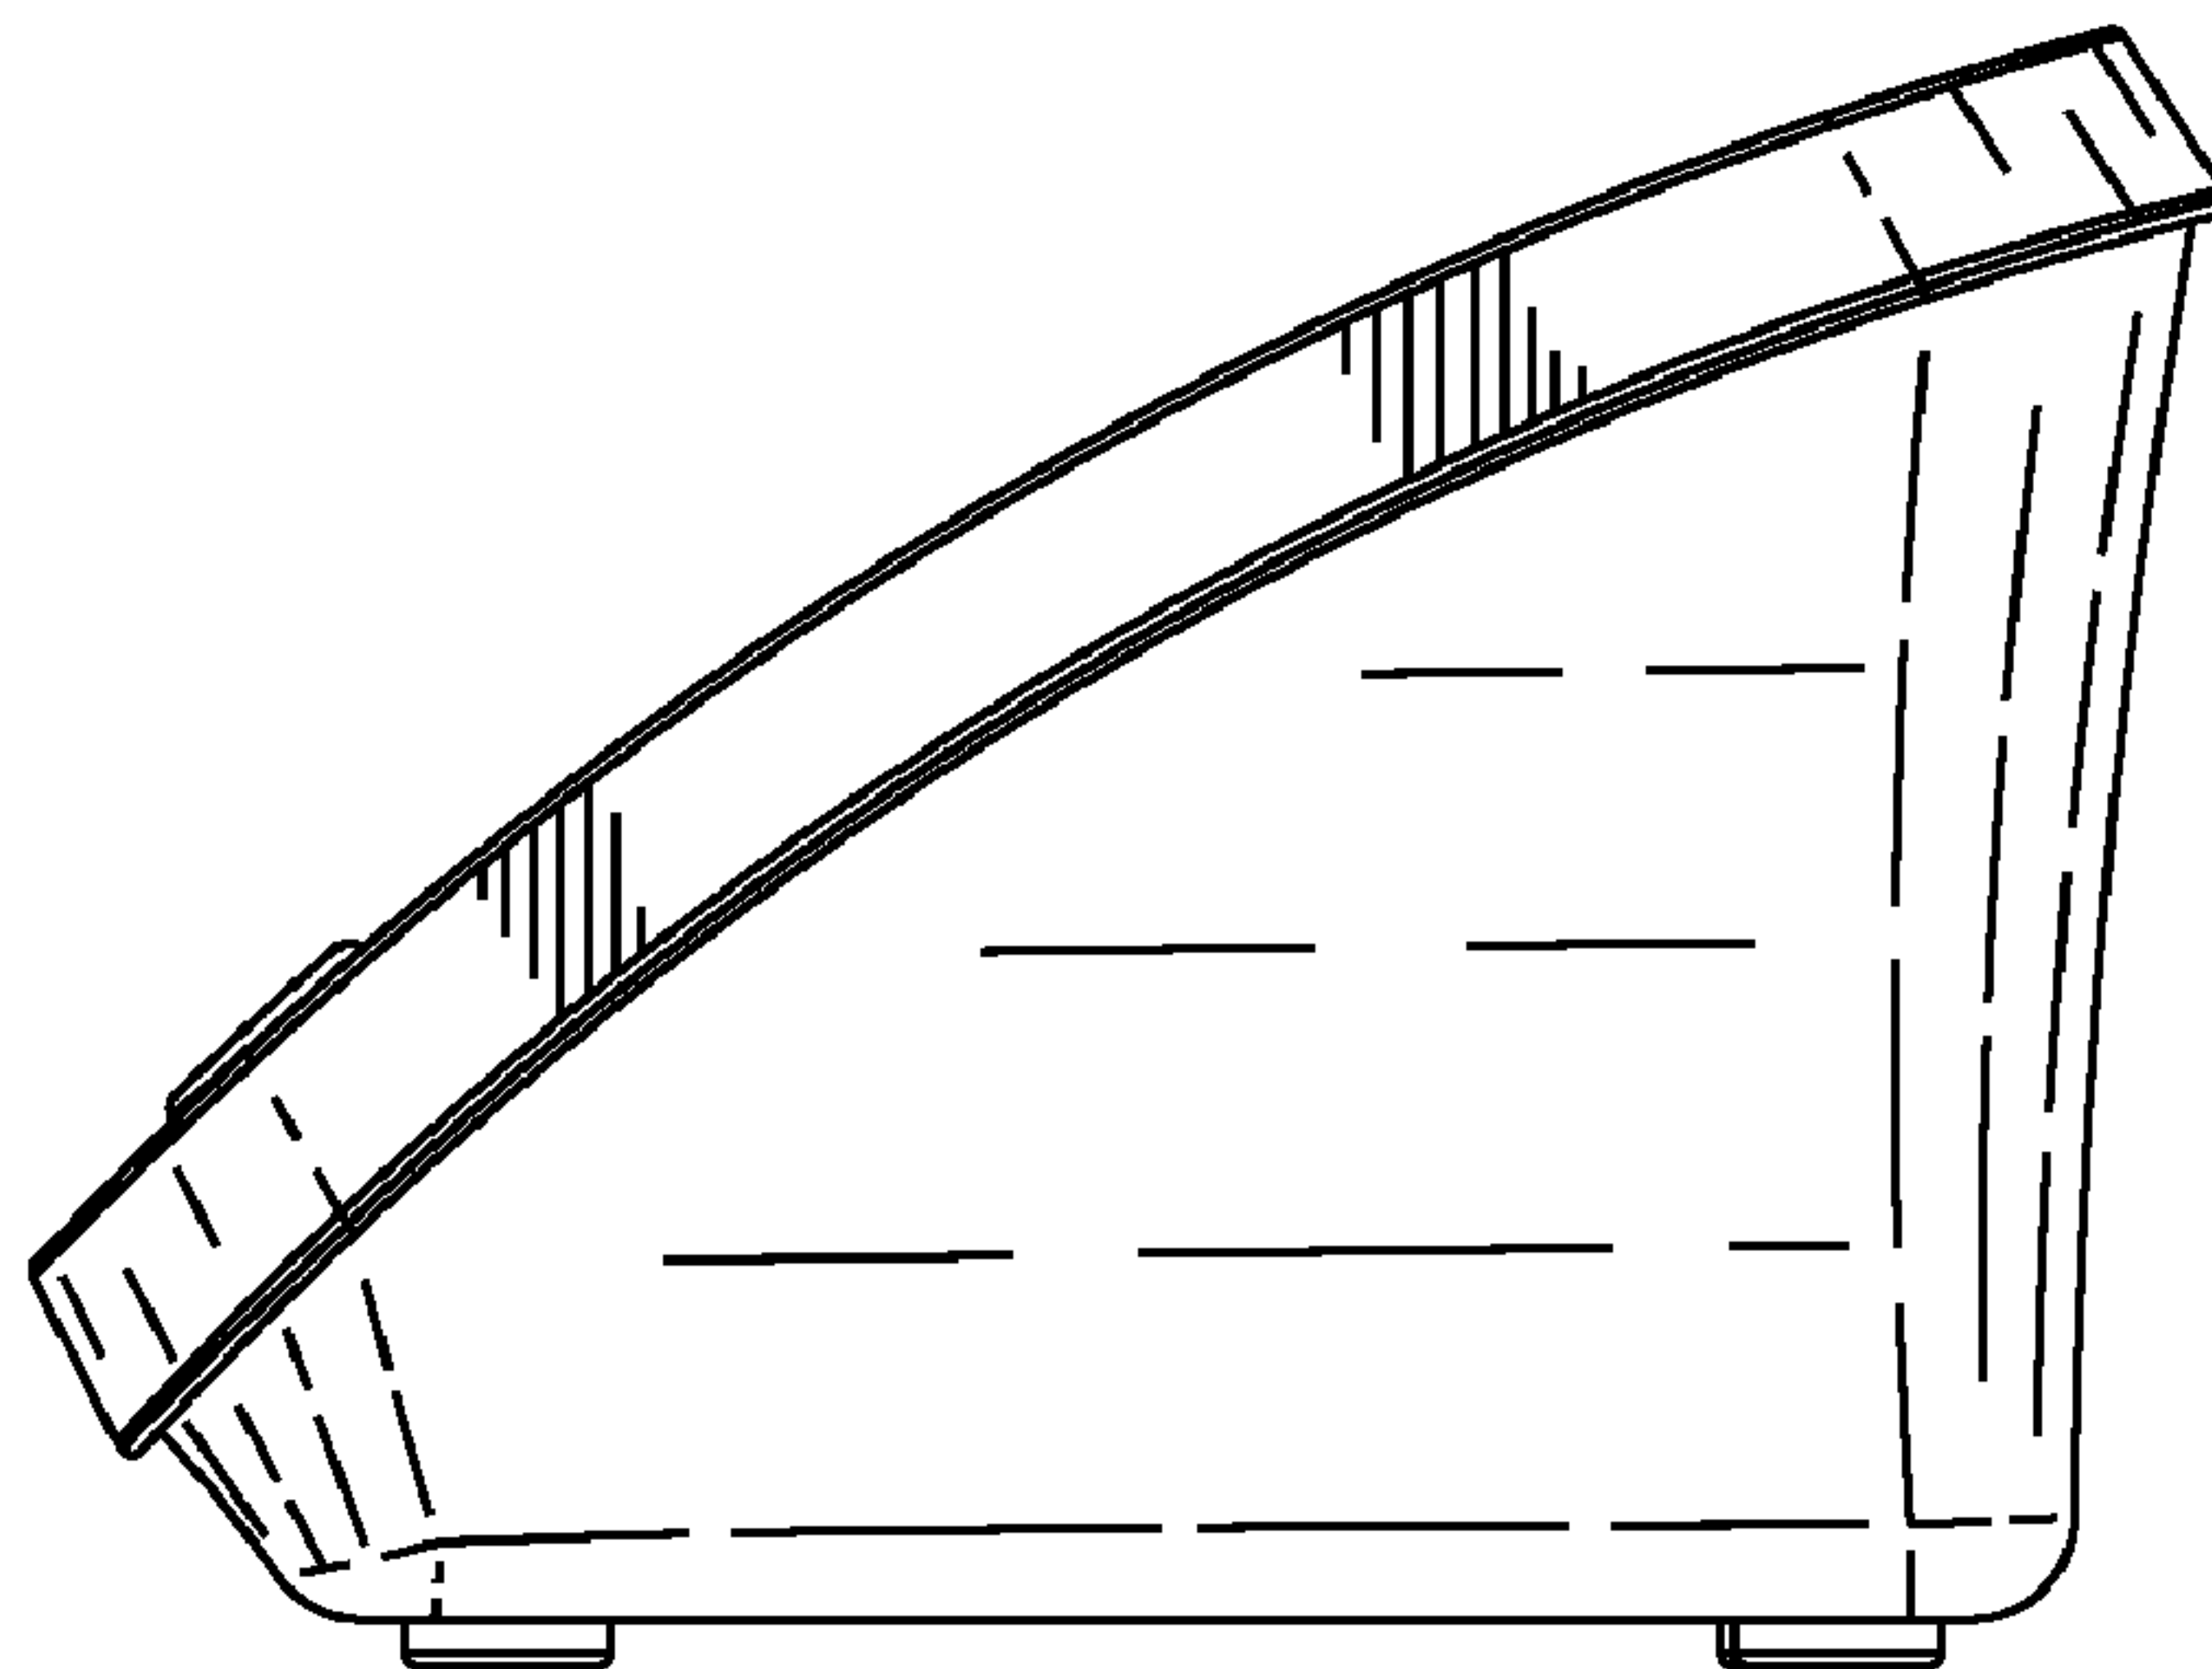


FIG. 8