



US00D602165S

(12) **United States Design Patent**
Dimmer et al.

(10) **Patent No.:** **US D602,165 S**
(45) **Date of Patent:** **** Oct. 13, 2009**

(54) **DIAGNOSTIC TEST STRIP**

(75) Inventors: **Stephen Dimmer**, Hampshire (GB); **Ian Thomas Hart**, Hampshire (GB); **James Anthony Michael Lees-Smith**, Hampshire (GB); **Ali Malone**, Hampshire (GB)

(73) Assignee: **Oxoid Limited**, Hampshire (GB)

(**) Term: **14 Years**

(21) Appl. No.: **29/306,598**

(22) Filed: **Apr. 11, 2008**

Related U.S. Application Data

(63) Continuation-in-part of application No. 29/283,335, filed on Aug. 10, 2007, now Pat. No. Des. 572,369.

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/225**

(58) **Field of Classification Search** D24/216-226,
D24/169; D10/81; 422/56, 58, 61, 63, 69,
422/99, 102; 436/65, 66
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D266,694	S *	10/1982	Boger et al.	D24/225
5,413,761	A	5/1995	Dulaney		
D381,591	S	7/1997	Rice et al.		
D392,391	S	3/1998	Douglas et al.		
6,268,210	B1 *	7/2001	Baier et al.	435/288.5
D450,854	S	11/2001	Lipman et al.		
D456,083	S	4/2002	Clark et al.		
D456,910	S	5/2002	Clark et al.		
D462,122	S	8/2002	Hutcheson et al.		
D477,670	S	7/2003	Jurik et al.		
6,720,143	B2 *	4/2004	Juncosa et al.	435/6
6,723,500	B2 *	4/2004	Yu	435/4

D501,560	S	2/2005	Whyte et al.		
6,855,561	B2	2/2005	Jerome et al.		
D512,512	S	12/2005	Bell et al.		
D566,849	S *	4/2008	Vermeiden	D24/225
D566,850	S *	4/2008	Vermeiden	D24/225
2004/0018115	A1 *	1/2004	Karp	422/58

* cited by examiner

Primary Examiner—T. Chase Nelson

Assistant Examiner—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Wood, Herron & Evans LLP

(57) **CLAIM**

The ornamental design for the diagnostic test strip, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a first embodiment of our new diagnostic test strip design;

FIG. 2 is an a front elevation view thereof;

FIG. 3 is a left-side elevation view thereof (the right-side elevation view being identical); and

FIG. 4 is a top plan view thereof (the bottom plan view being identical).

FIG. 5 is a perspective view of a second embodiment of our new diagnostic test strip design, wherein solid black surface shading represents contrasting color;


FIG. 6 is an a front elevation view thereof;

FIG. 7 is a left-side elevation view thereof (the right-side elevation view being identical); and,

FIG. 8 is a top plan view thereof (the bottom plan view being identical).

The broken lines in the drawing figures are included for the purpose of illustrating portions of the diagnostic test strip that form no part of the claimed design

1 Claim, 2 Drawing Sheets

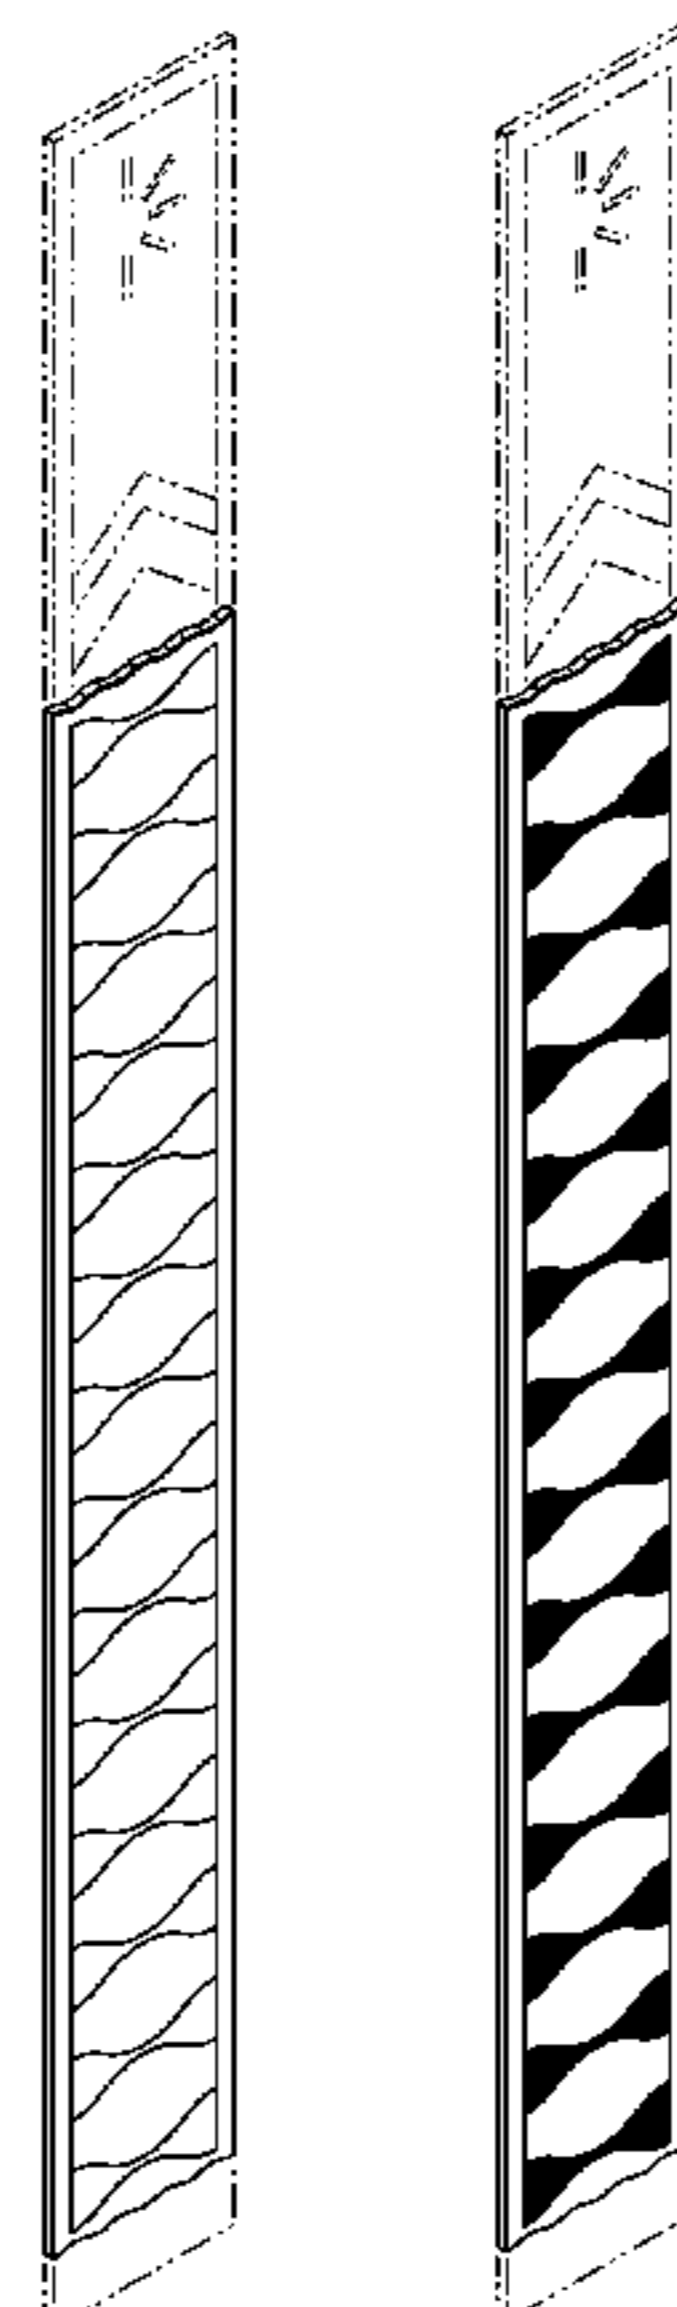

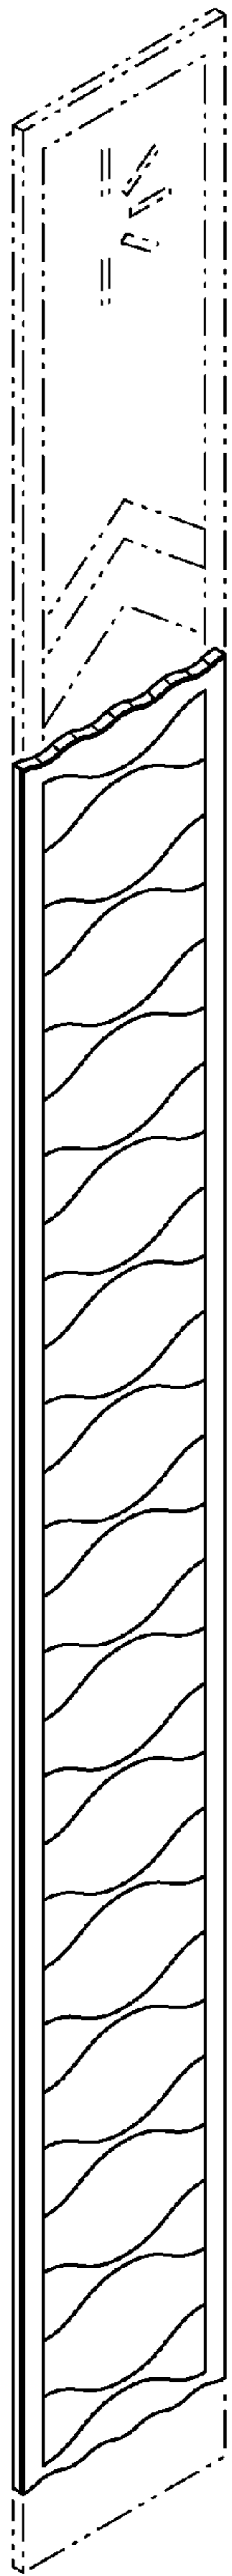


FIG. 1

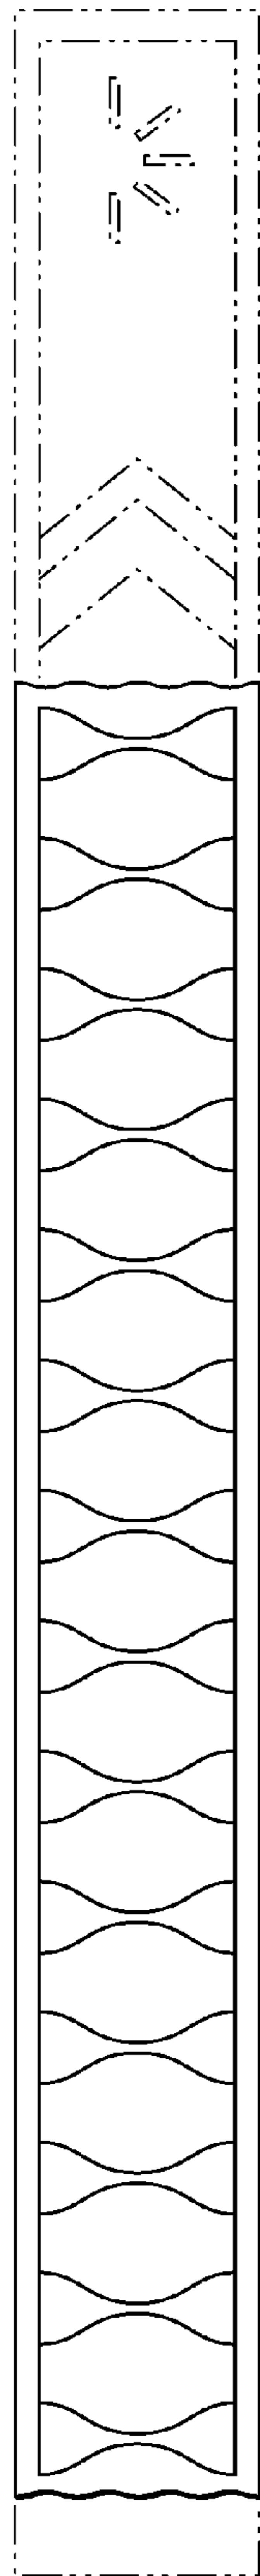


FIG. 2



FIG. 3



FIG. 4

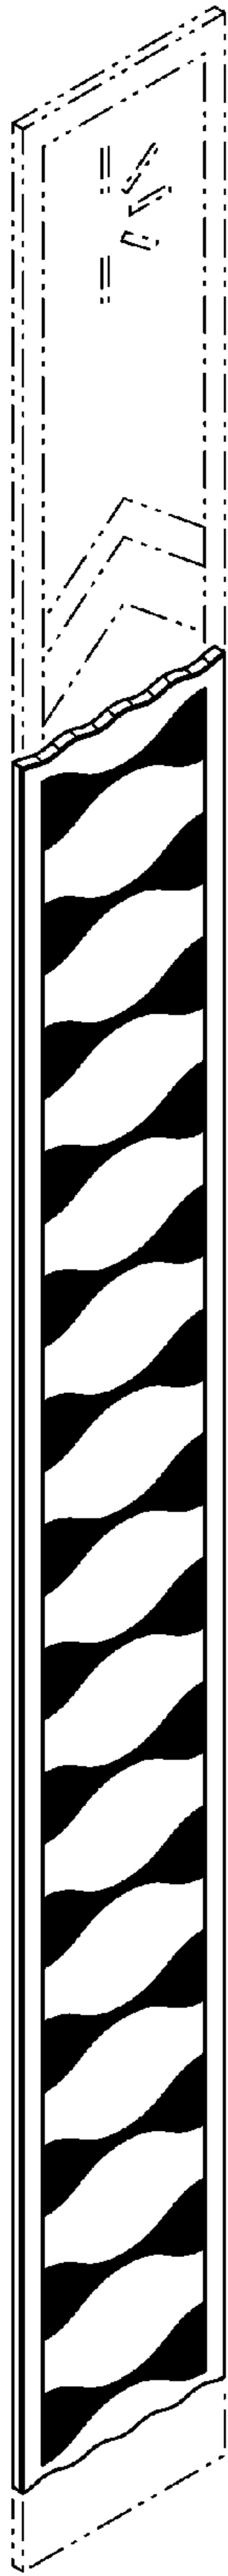


FIG. 5

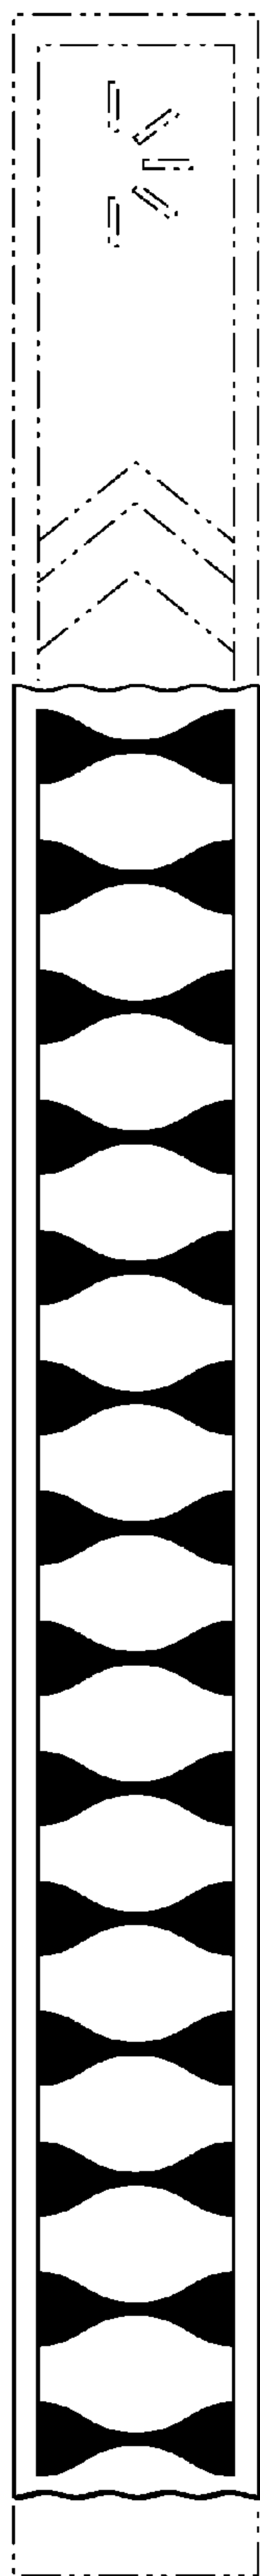


FIG. 6



FIG. 7




FIG. 8