



US00D603958S

(12) **United States Design Patent**  
**Schwartz et al.**

(10) **Patent No.:** **US D603,958 S**

(45) **Date of Patent:** **\*\* Nov. 10, 2009**

(54) **ENDOSCOPE INTUBATION DEVICE WITH A CONTROL GRIP AND A PIVOTABLE DISPLAY**

(75) Inventors: **John Schwartz**, Williamston, MI (US);  
**Richard Schwartz**, Evans, GA (US);  
**Harsha Setty**, Martinez, GA (US)

(73) Assignee: **AI Medical Devices, Inc.**, Williamston, MI (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/312,314**

(22) Filed: **Oct. 14, 2008**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/138**

(58) **Field of Classification Search** ..... D24/138,  
D24/133, 137, 140; 600/120, 109, 131, 160,  
600/179; 128/200.26, 207.14–207.17

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

4,742,819	A *	5/1988	George	.....	600/109
D410,286	S *	5/1999	Tamirisa	.....	D24/138
6,539,942	B2 *	4/2003	Schwartz et al.	.....	128/207.14
D533,939	S *	12/2006	Root et al.	.....	D24/138
D580,549	S *	11/2008	Schwartz et al.	.....	D24/133
7,458,375	B2 *	12/2008	Schwartz et al.	.....	128/207.14
2008/0208000	A1 *	8/2008	Schwartz et al.	.....	600/120
2008/0308098	A1 *	12/2008	Schwartz et al.	.....	128/200.26

\* cited by examiner

*Primary Examiner*—Ian Simmons  
*Assistant Examiner*—Christopher Lee  
(74) *Attorney, Agent, or Firm*—Ian C. McLeod

(57) **CLAIM**

The ornamental design for an endoscope intubation device with a control grip and a pivotable display, as shown and described.

**DESCRIPTION**

FIG. 1 is a right side view of an endoscope intubation device with a control grip and pivotable display showing our new design;

FIG. 2 is a front view thereof showing the display;

FIG. 3 is a left side view thereof. The broken lines in FIG. 3 are included for the purpose of illustrating a portion of the endoscope intubation device with a control grip and a pivotable display that forms no part of the claimed design.

FIG. 4 is a back view thereof showing the distal end of the tube. The broken lines in FIG. 4 are included for the purpose of illustrating a portion of the endoscope intubation device with a control grip and a pivotable display that forms no part of the claimed design.


FIG. 5 is a bottom side view thereof;

FIG. 6 is a top side view thereof; and,

FIG. 7 is a perspective view thereof.

The shaft portion in FIGS. 1, 3, 5, 6 and 7 is shown broken away to show indeterminate length and for ease of illustration.

**1 Claim, 7 Drawing Sheets**

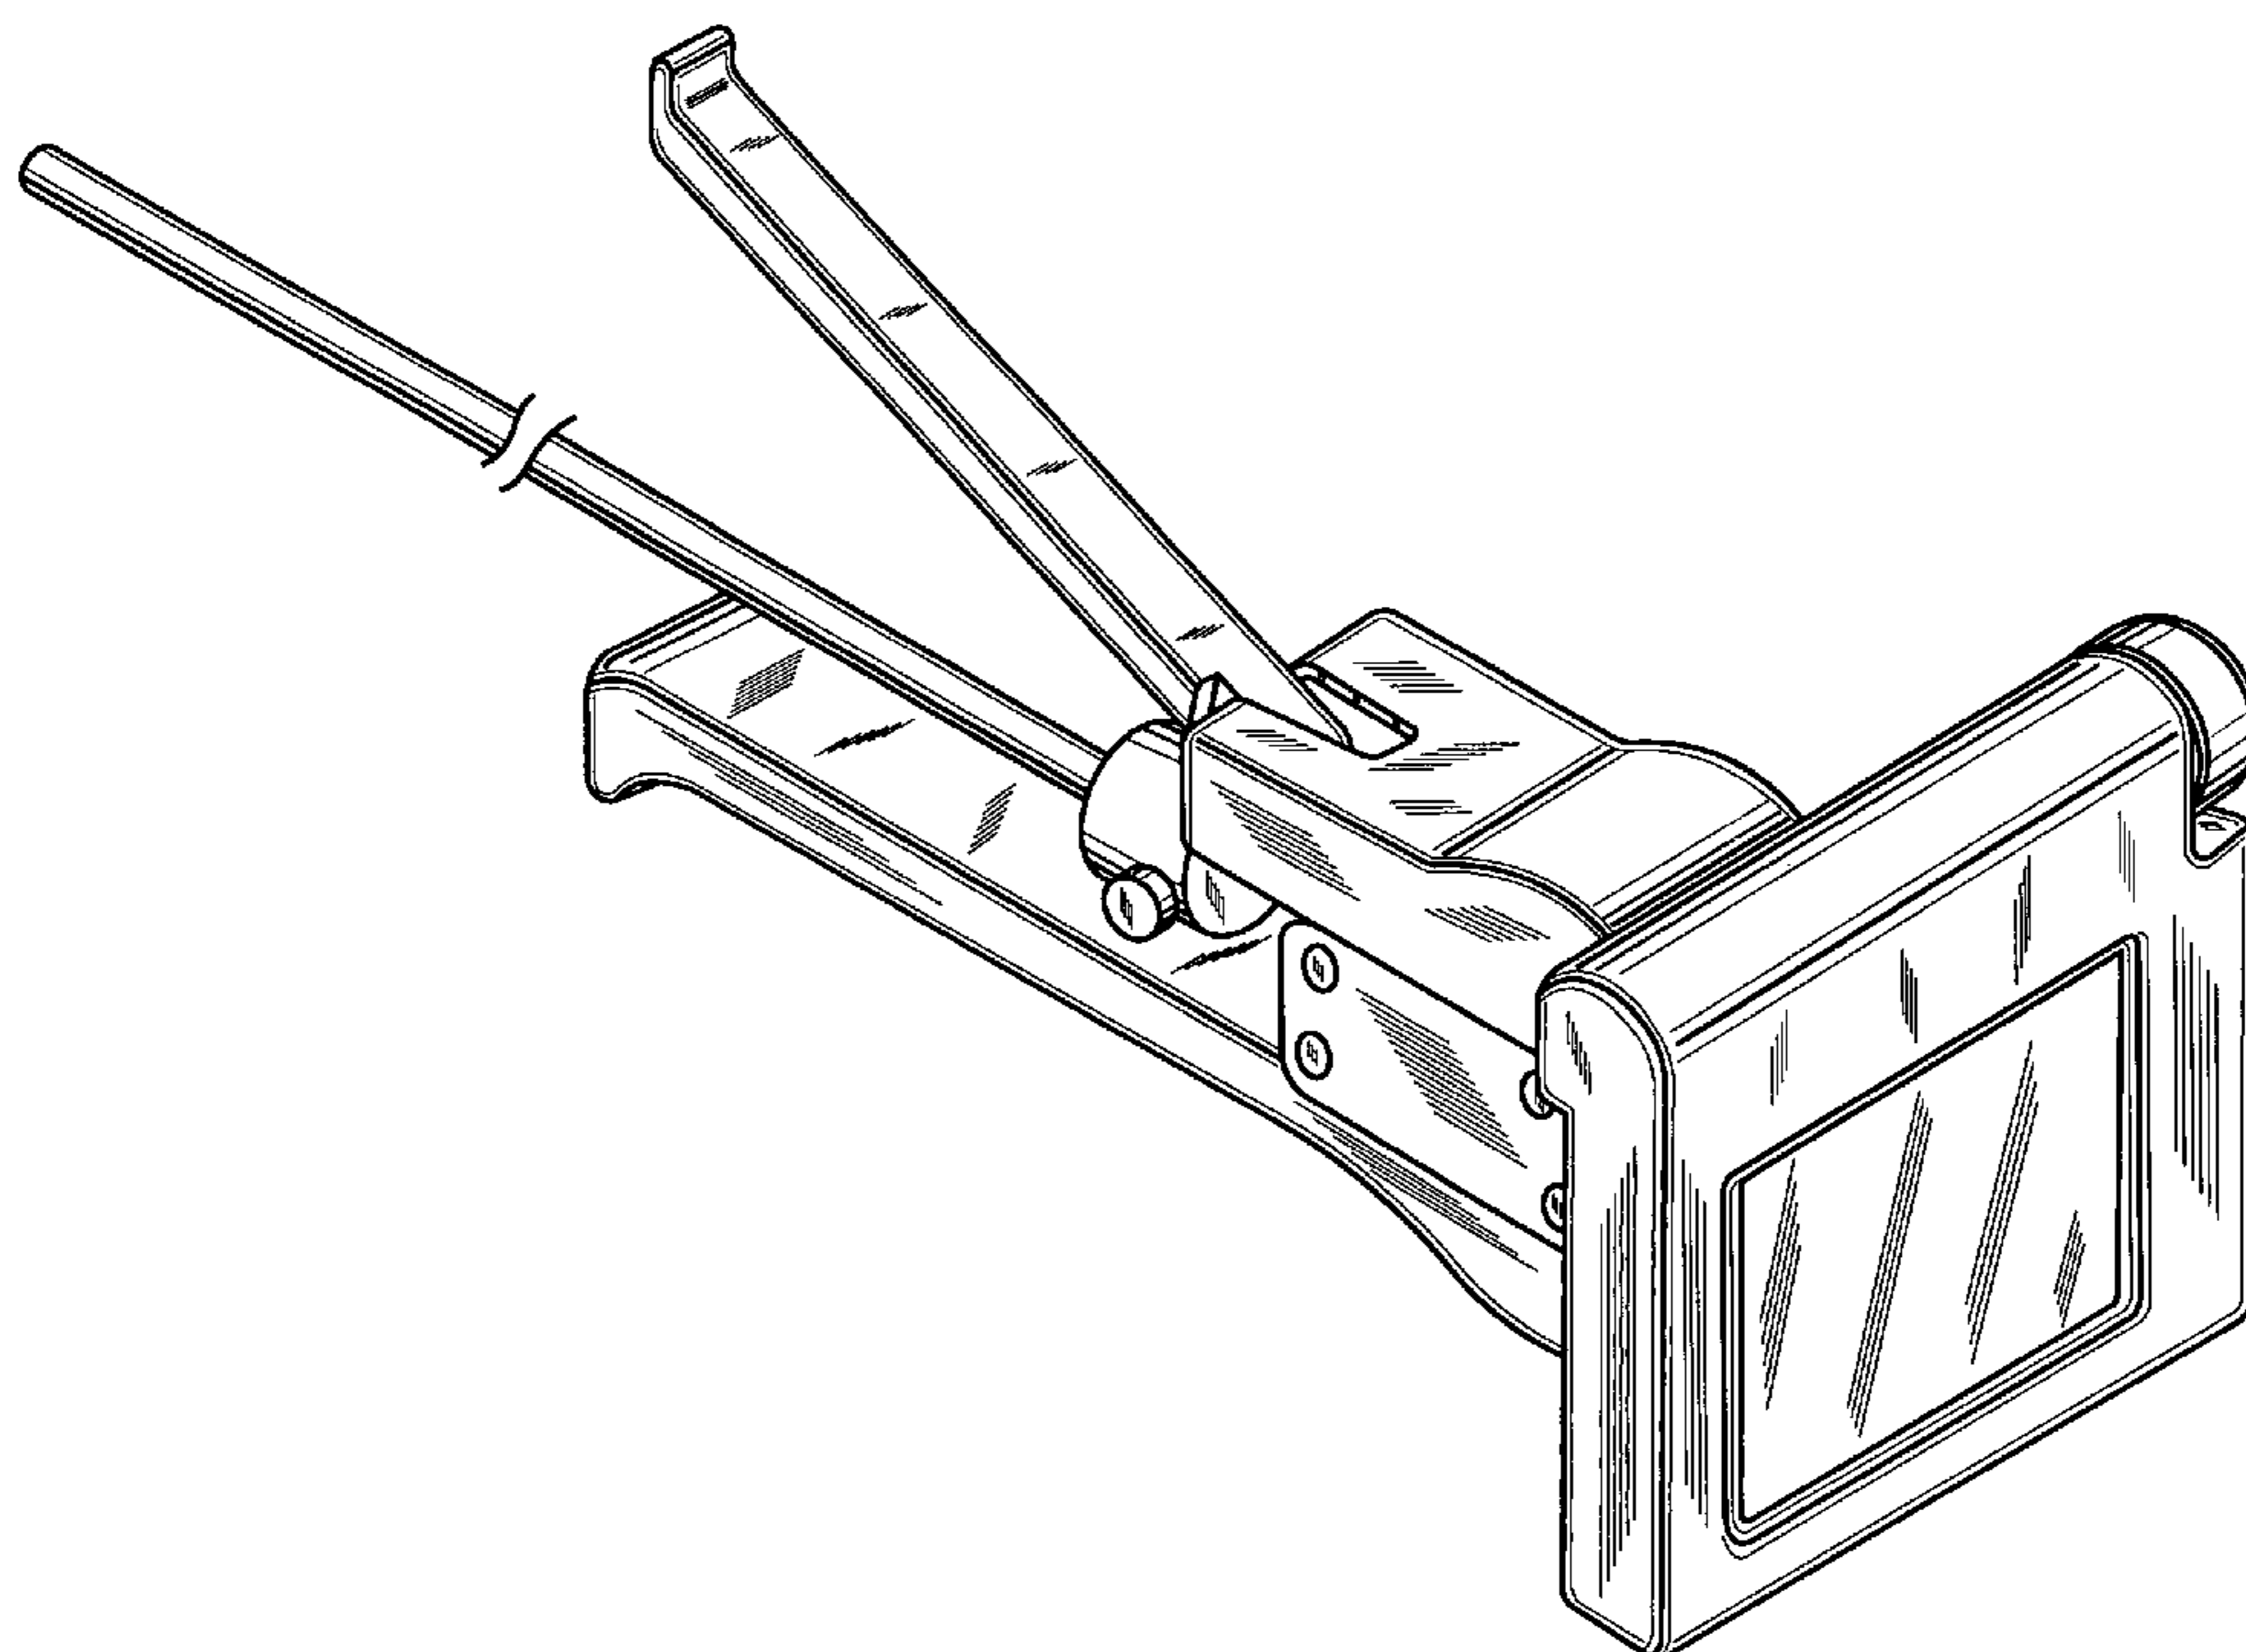

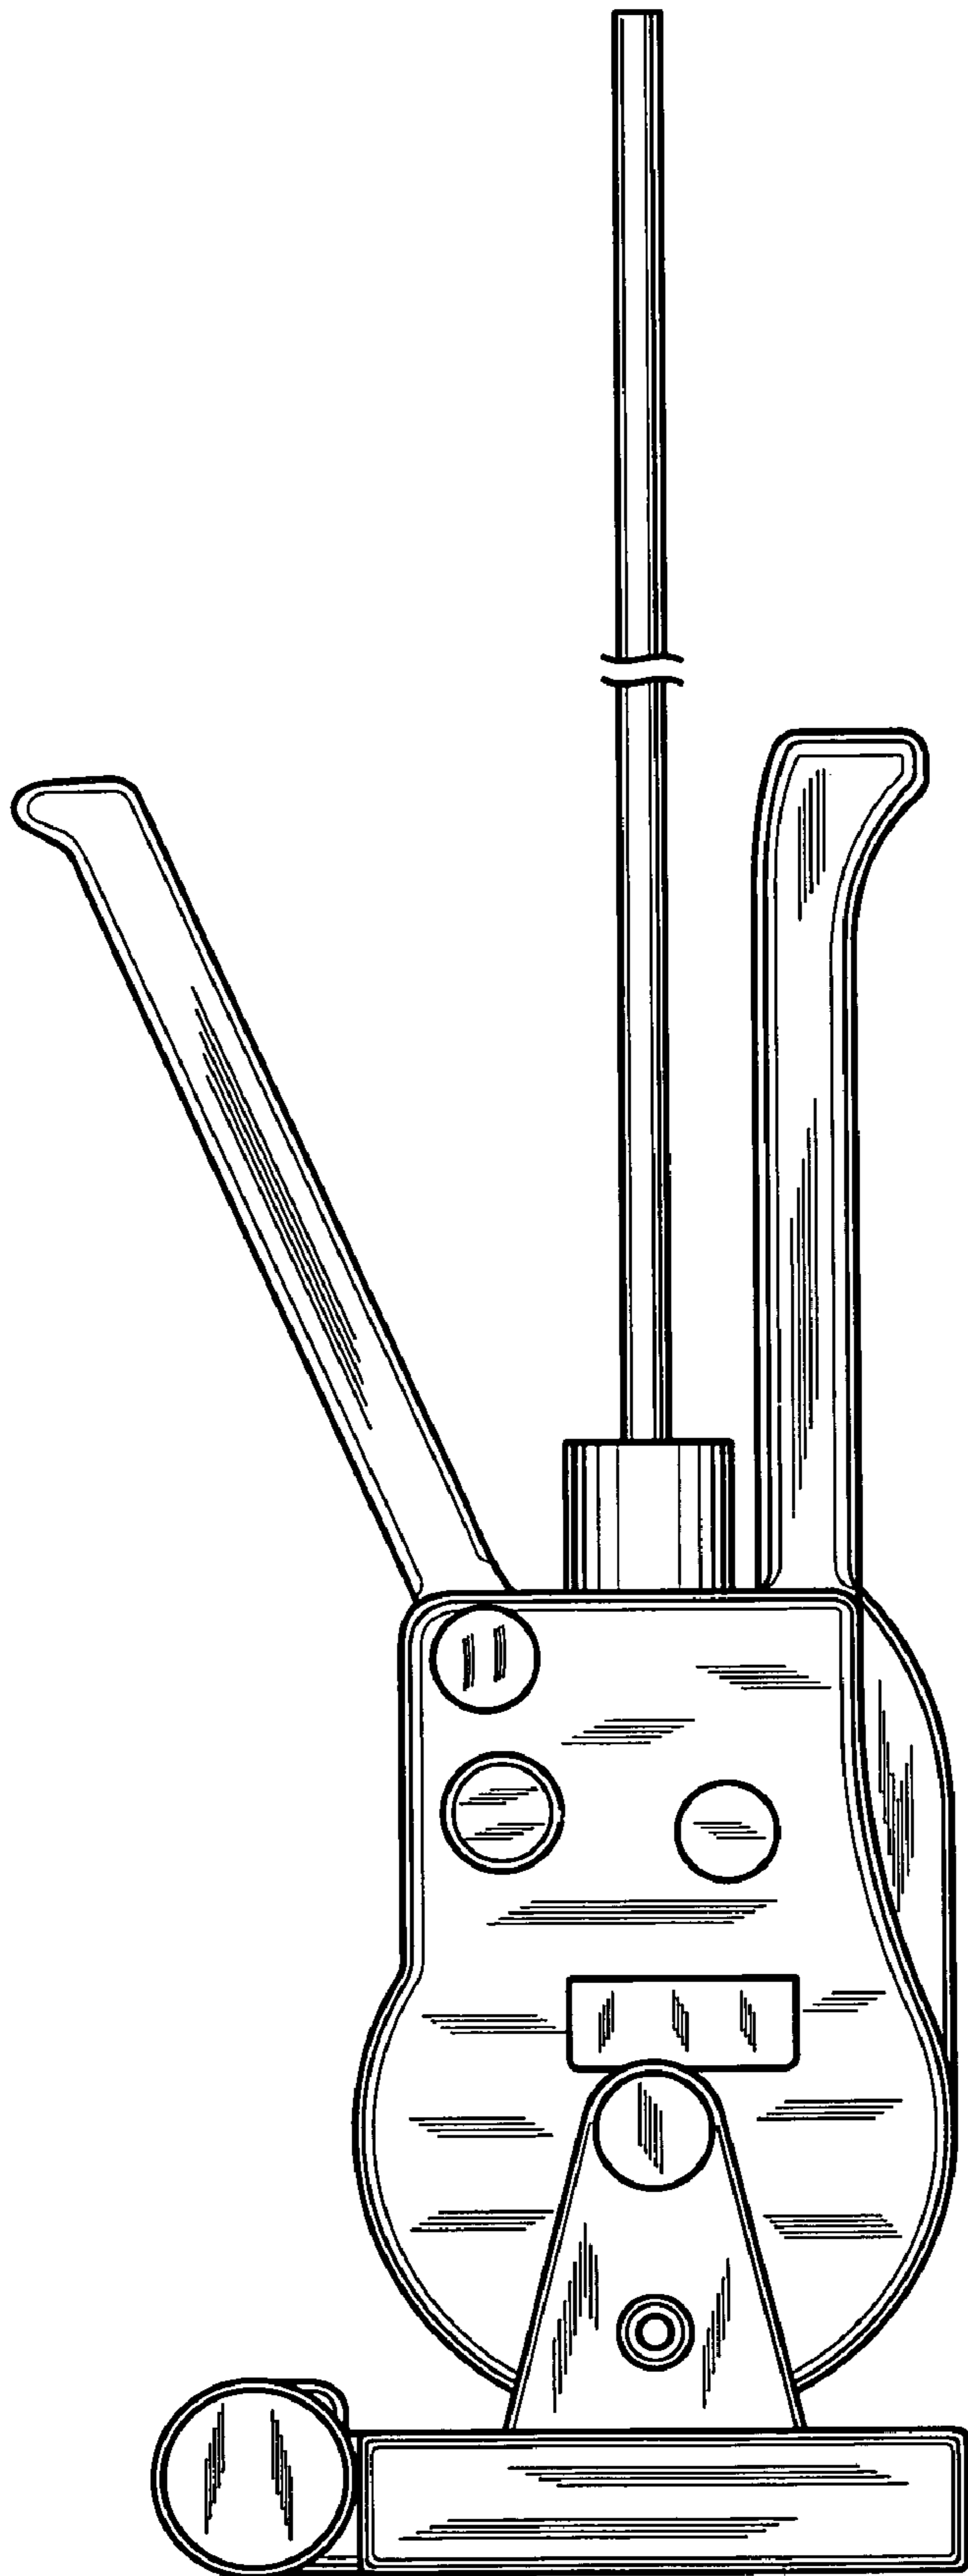


FIG. 1

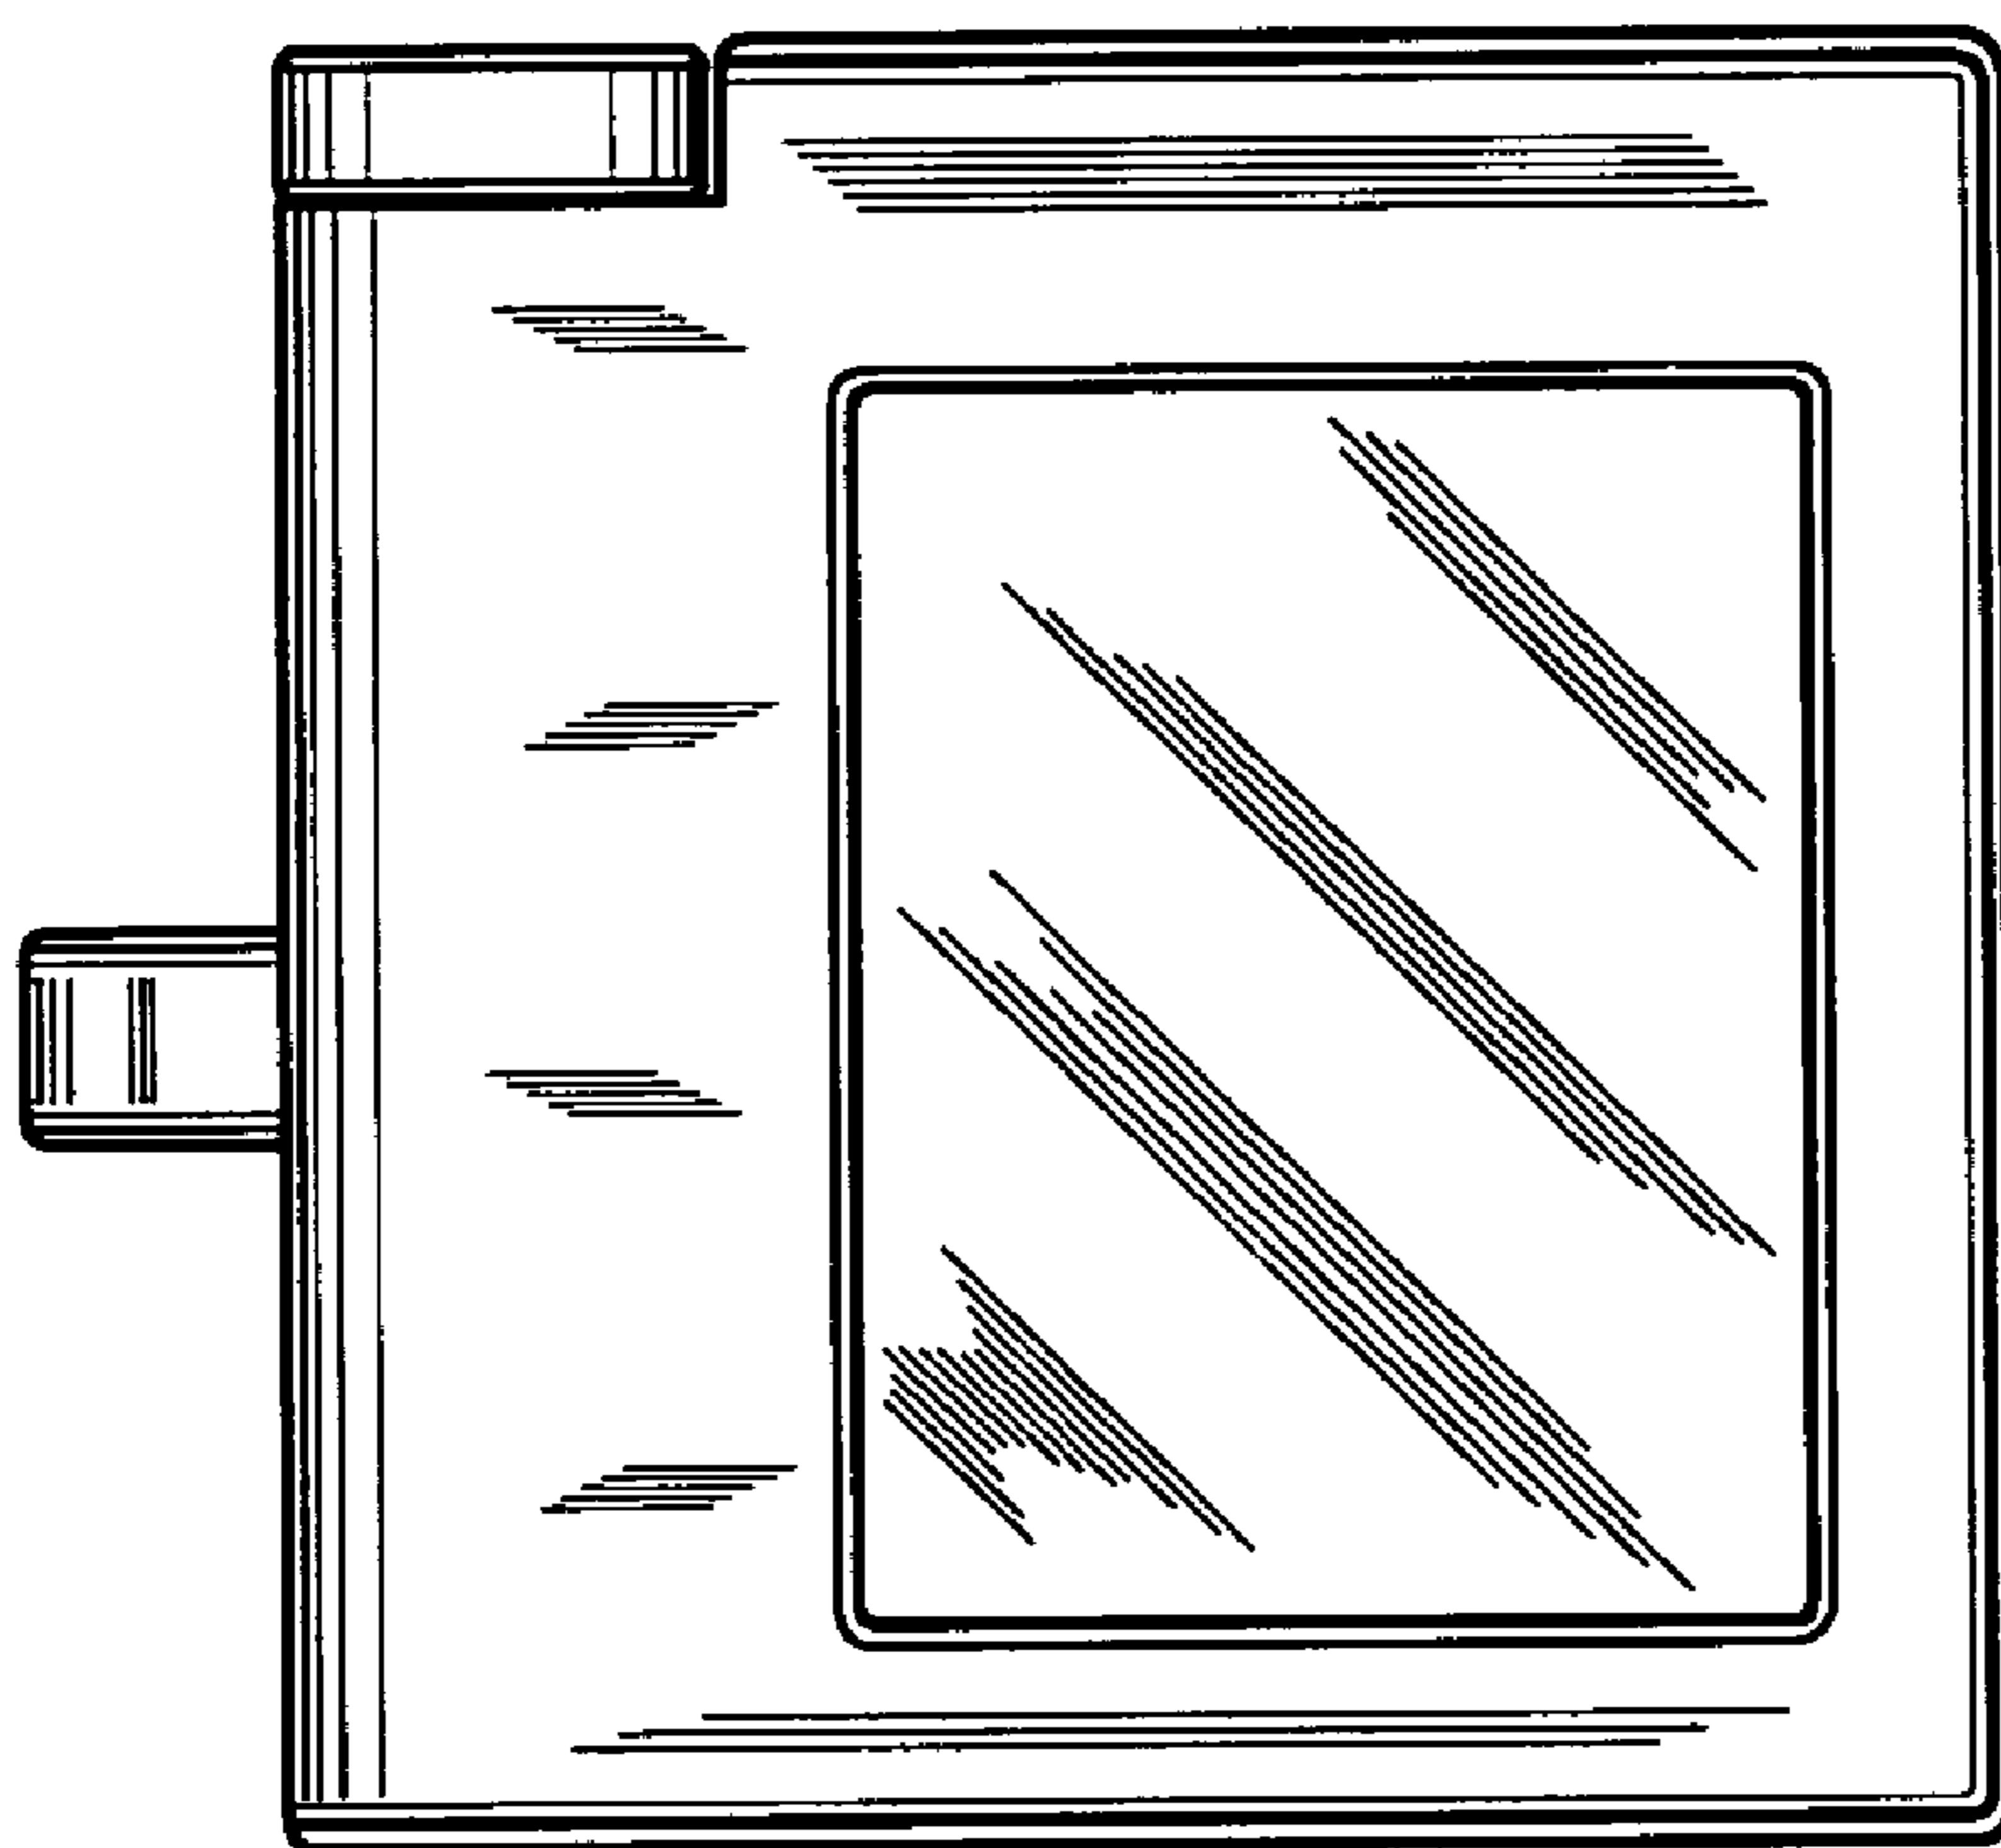


FIG. 2

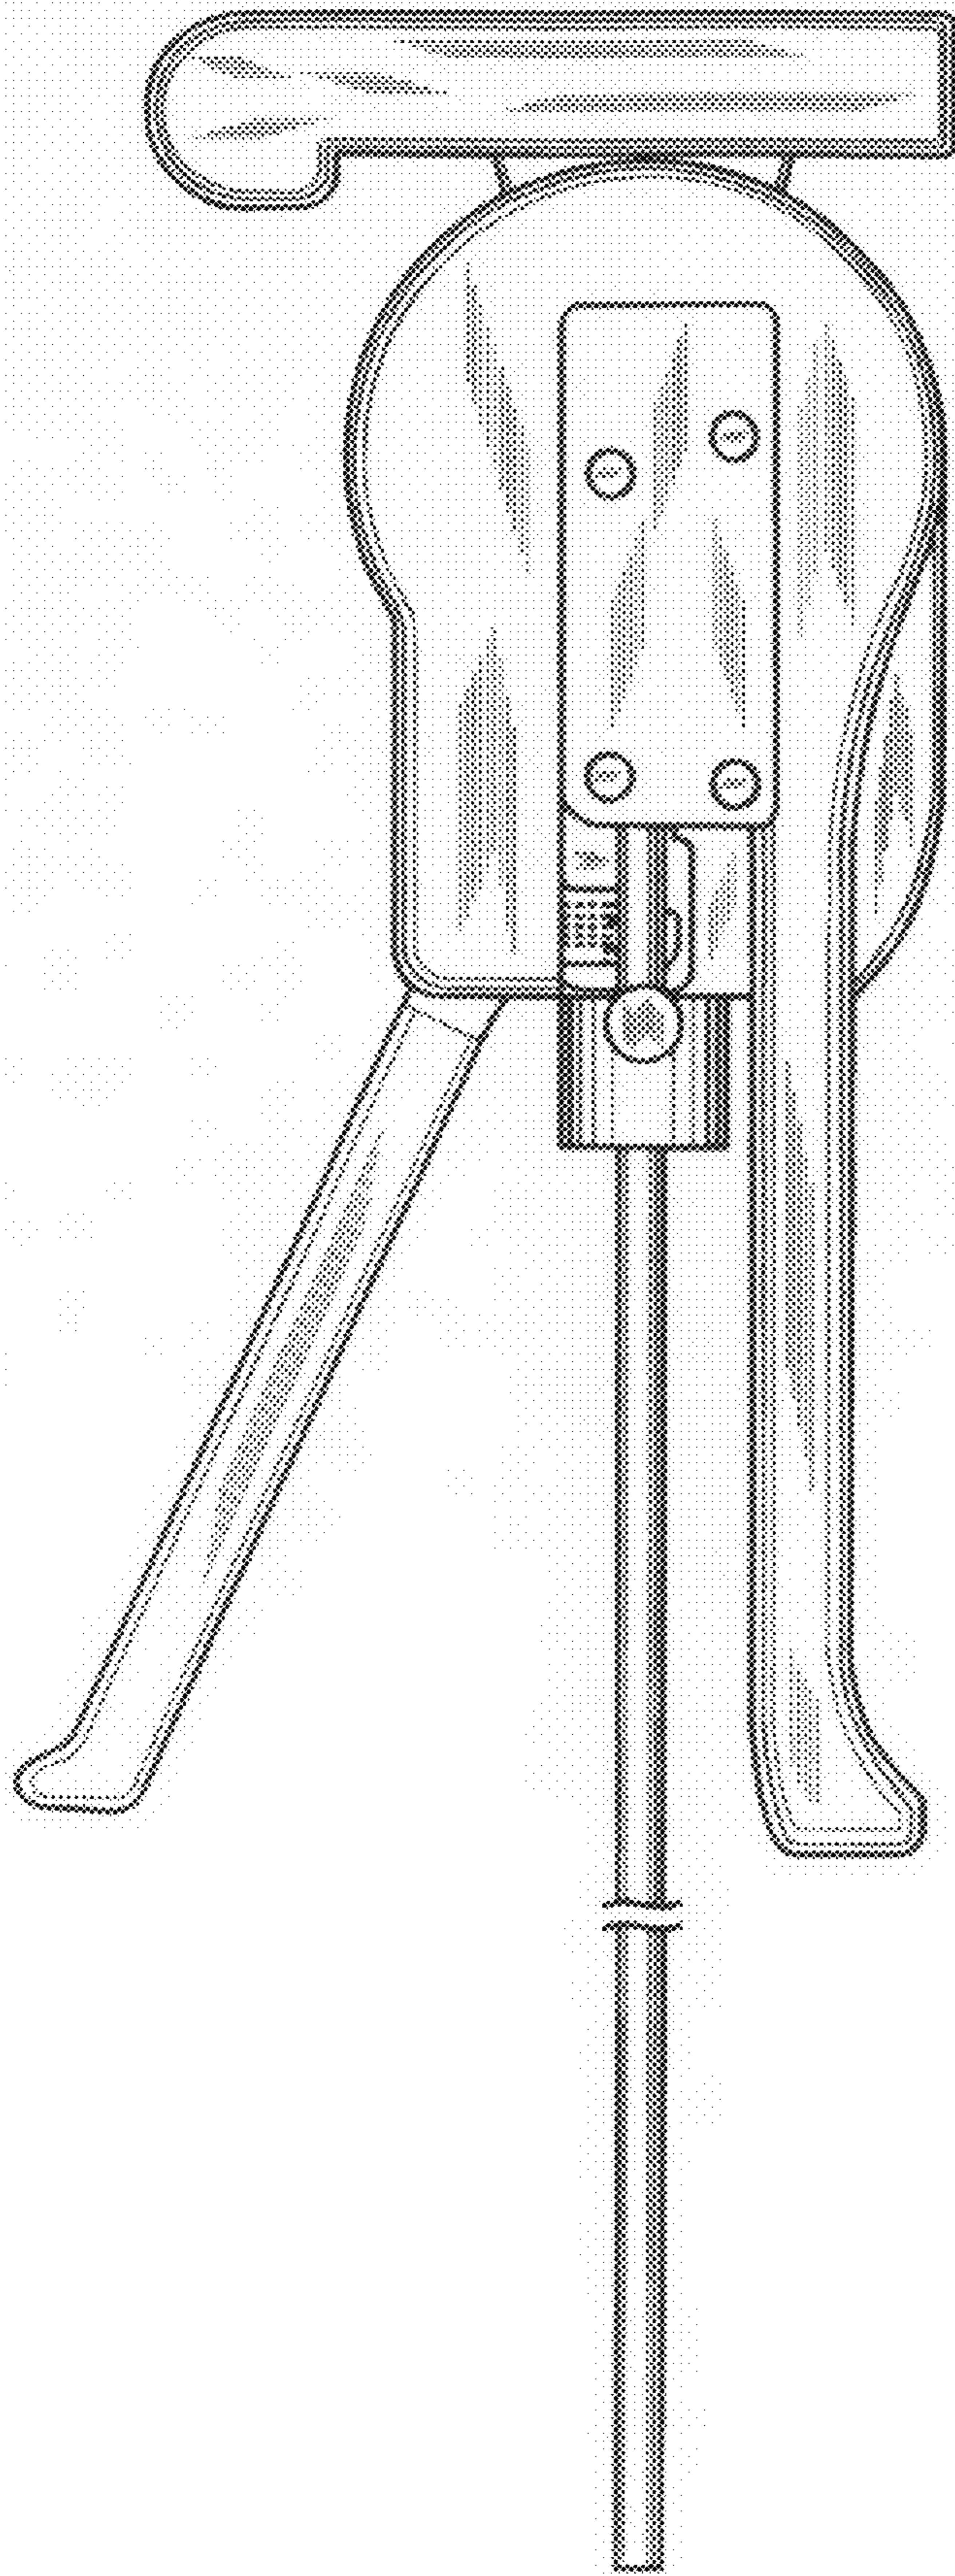


FIG. 3

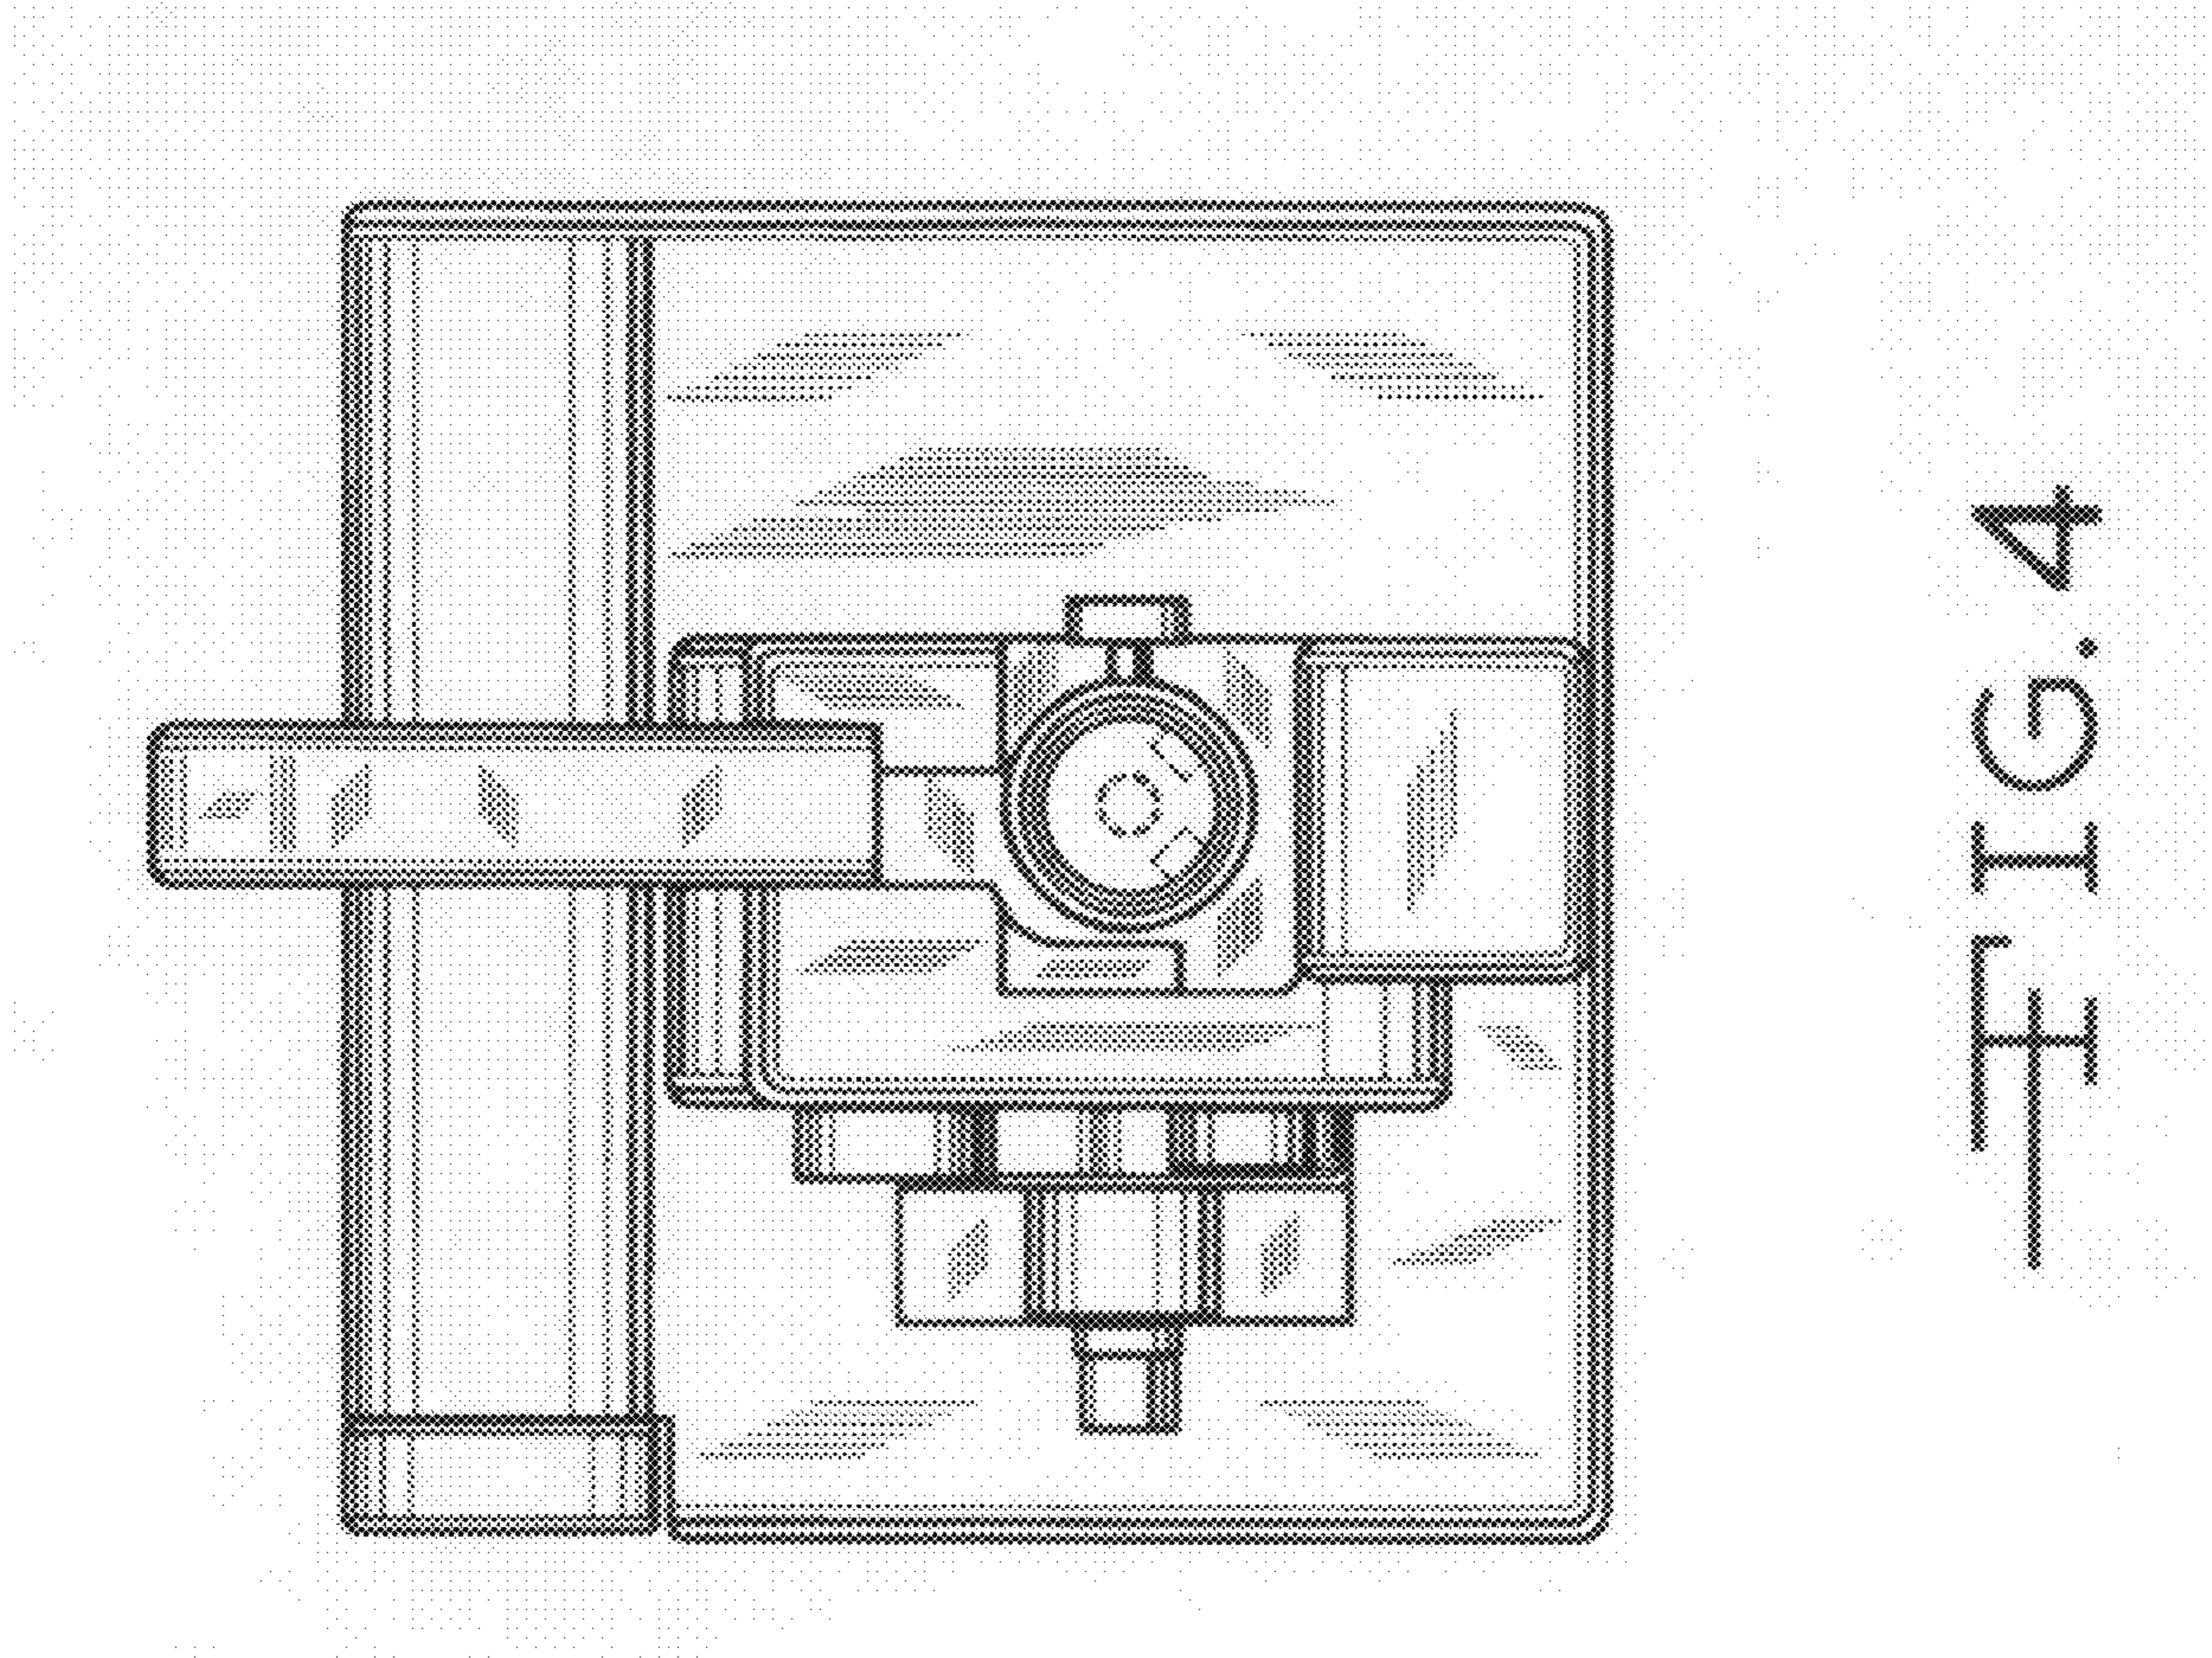


FIG. 4

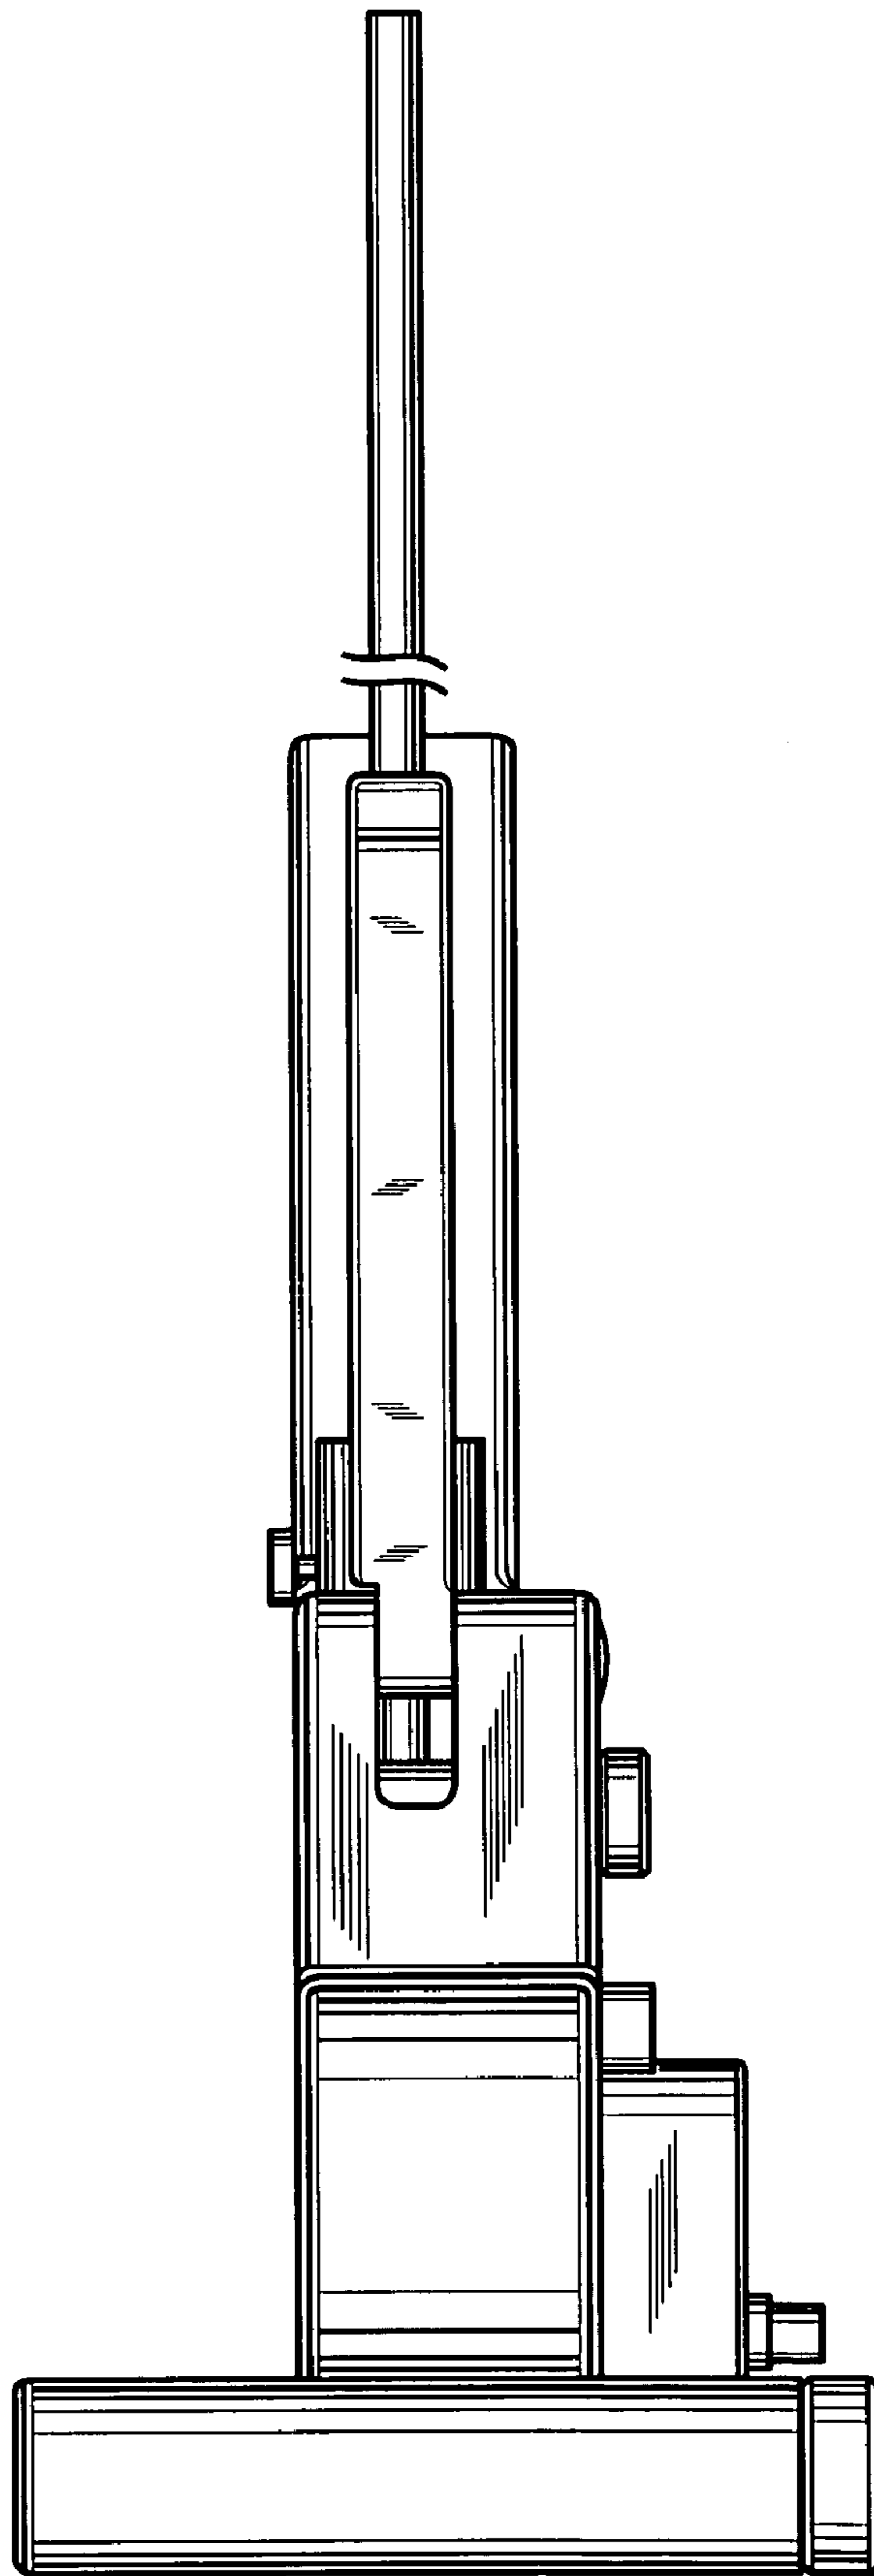


FIG. 5

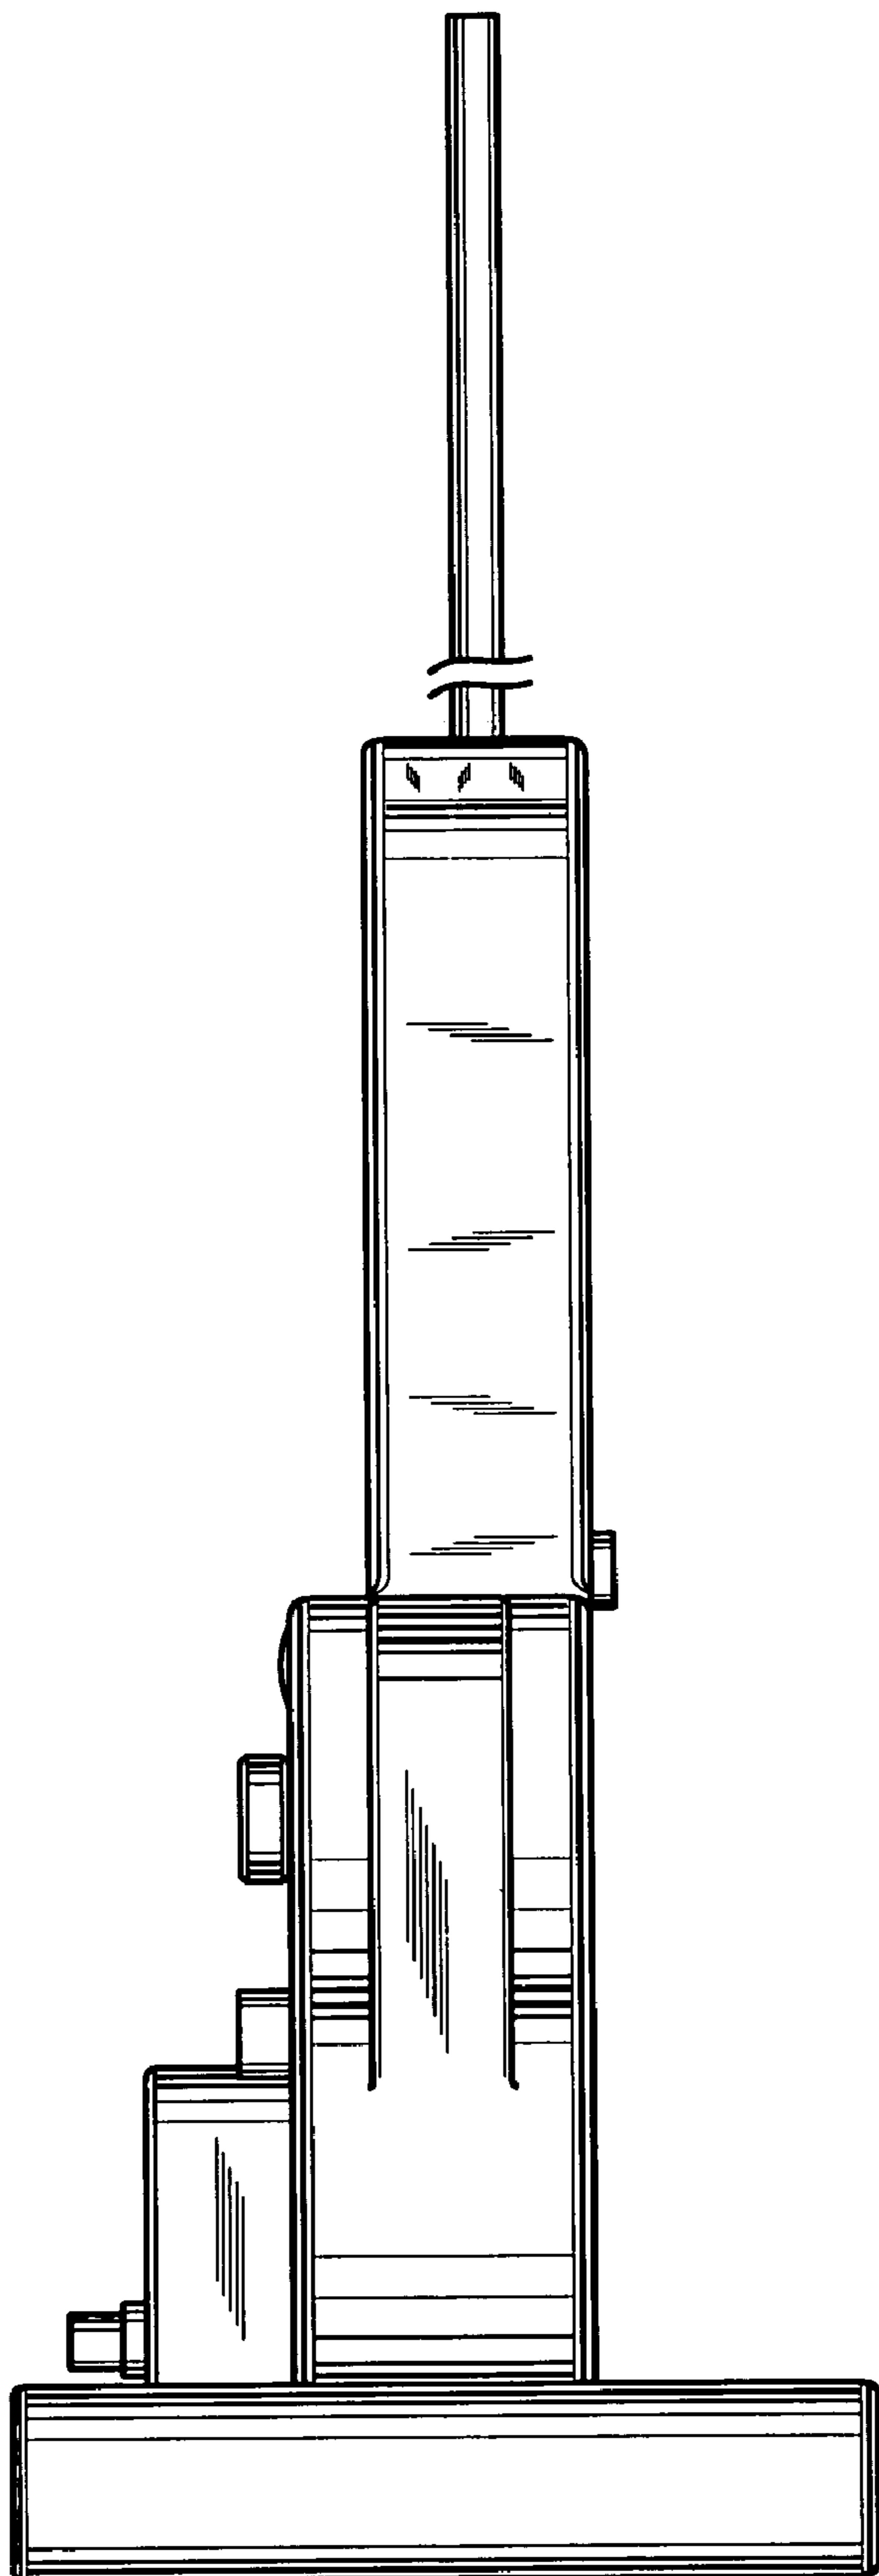


FIG. 6

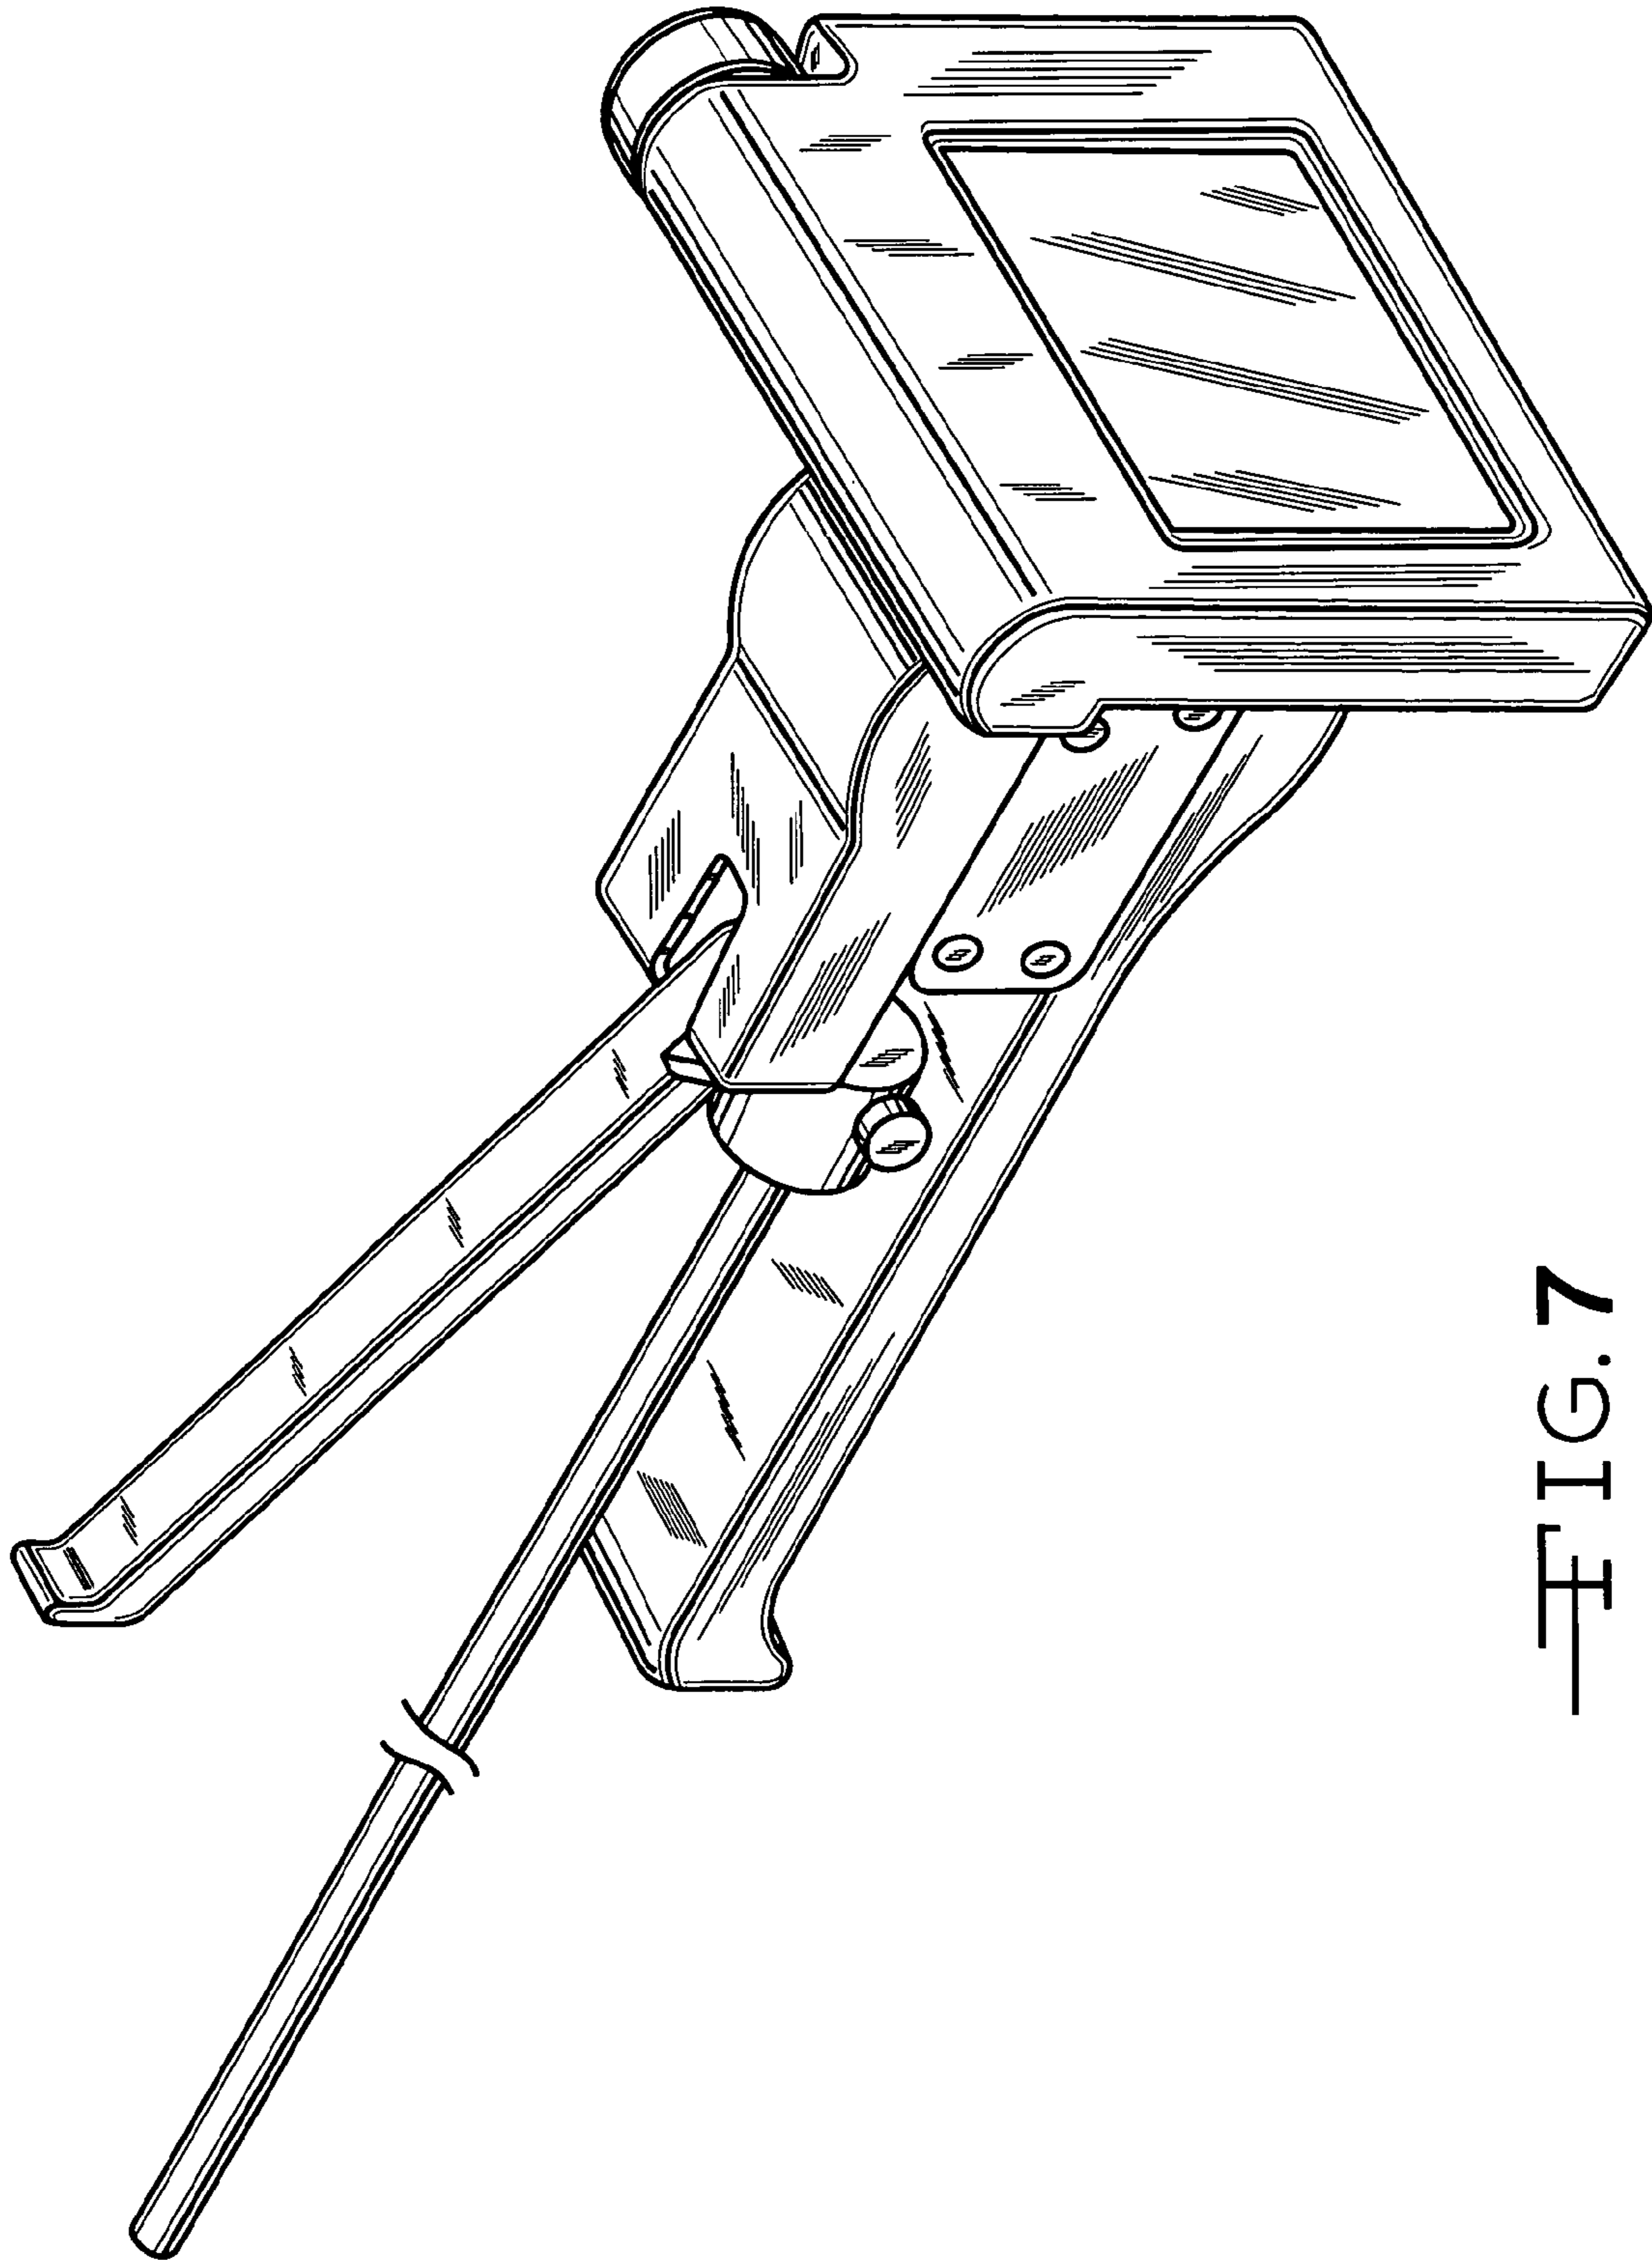


FIG. 7