

US00D604185S

(12) **United States Design Patent**
Watanabe et al.

(10) **Patent No.:** **US D604,185 S**
(45) **Date of Patent:** **** Nov. 17, 2009**

(54) **BIO-SENSOR**

(57) **CLAIM**

(75) Inventors: **Shigenori Watanabe**, Saitama (JP);
Shunichi Wakamatsu, Saitama (JP);
Hiroyuki Kukita, Saitama (JP); **Takeru**
Mutoh, Saitama (JP)

The ornamental design for a bio-sensor, as shown and described.

(73) Assignee: **Nihon Dempa Kogyo Co., Ltd.**, Tokyo
(JP)

DESCRIPTION

(**) Term: **14 Years**

(21) Appl. No.: **29/310,758**

(22) Filed: **Sep. 9, 2008**

(51) **LOC (9) Cl.** **10-04**

(52) **U.S. Cl.** **D10/46**

(58) **Field of Classification Search** D10/46;
73/24.06, 580, 778; 310/8.2, 8.9, 320, 344,
310/553, 361, 370; 324/715–719; 333/72;
204/403, 416, 418, 419; 435/288, 291, 817
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,387,328 A * 2/1995 Sohn 257/253
6,776,888 B2 * 8/2004 Yamamoto et al. 204/403.09
D575,169 S 8/2008 Wakamatsu et al.

OTHER PUBLICATIONS

U.S. Appl. No. 29/294,262, filed Dec. 31, 2007, Shunichi
Wakamatsu, et al.

* cited by examiner

Primary Examiner—Antoine D Davis

(74) *Attorney, Agent, or Firm*—Edwards Angell Palmer &
Dodge LLP; Scott D. Wofsy

FIG. 1 is a front view of a bio-sensor of a new design;

FIG. 2 is a back view thereof;

FIG. 3 is a left side view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a plan view thereof;

FIG. 6 is a bottom plan view thereof;

FIG. 7 is a front view of a crystal resonator, the bio-sensor
being eliminated for ease of illustration;

FIG. 8 is a back view of a crystal resonator, the bio-sensor
being eliminated for ease of illustration;

FIG. 9 is a left side view of a crystal resonator, the bio-sensor
being eliminated for ease of illustration;

FIG. 10 is a right side view of a crystal resonator, the bio-
sensor being eliminated for ease of illustration;


FIG. 11 is a plan view of a crystal resonator, the bio-sensor
being eliminated for ease of illustration;

FIG. 12 is a bottom plan view of a crystal resonator, the
bio-sensor being eliminated for ease of illustration; and,

FIG. 13 is a referential assembling drawing showing a con-
dition wherein the bio-sensor is incorporated in a sensing
apparatus.

The broken line showing of structural features are included
for the purpose of illustrating non-claimed subject matter and
forms no part of the claimed design.

1 Claim, 4 Drawing Sheets

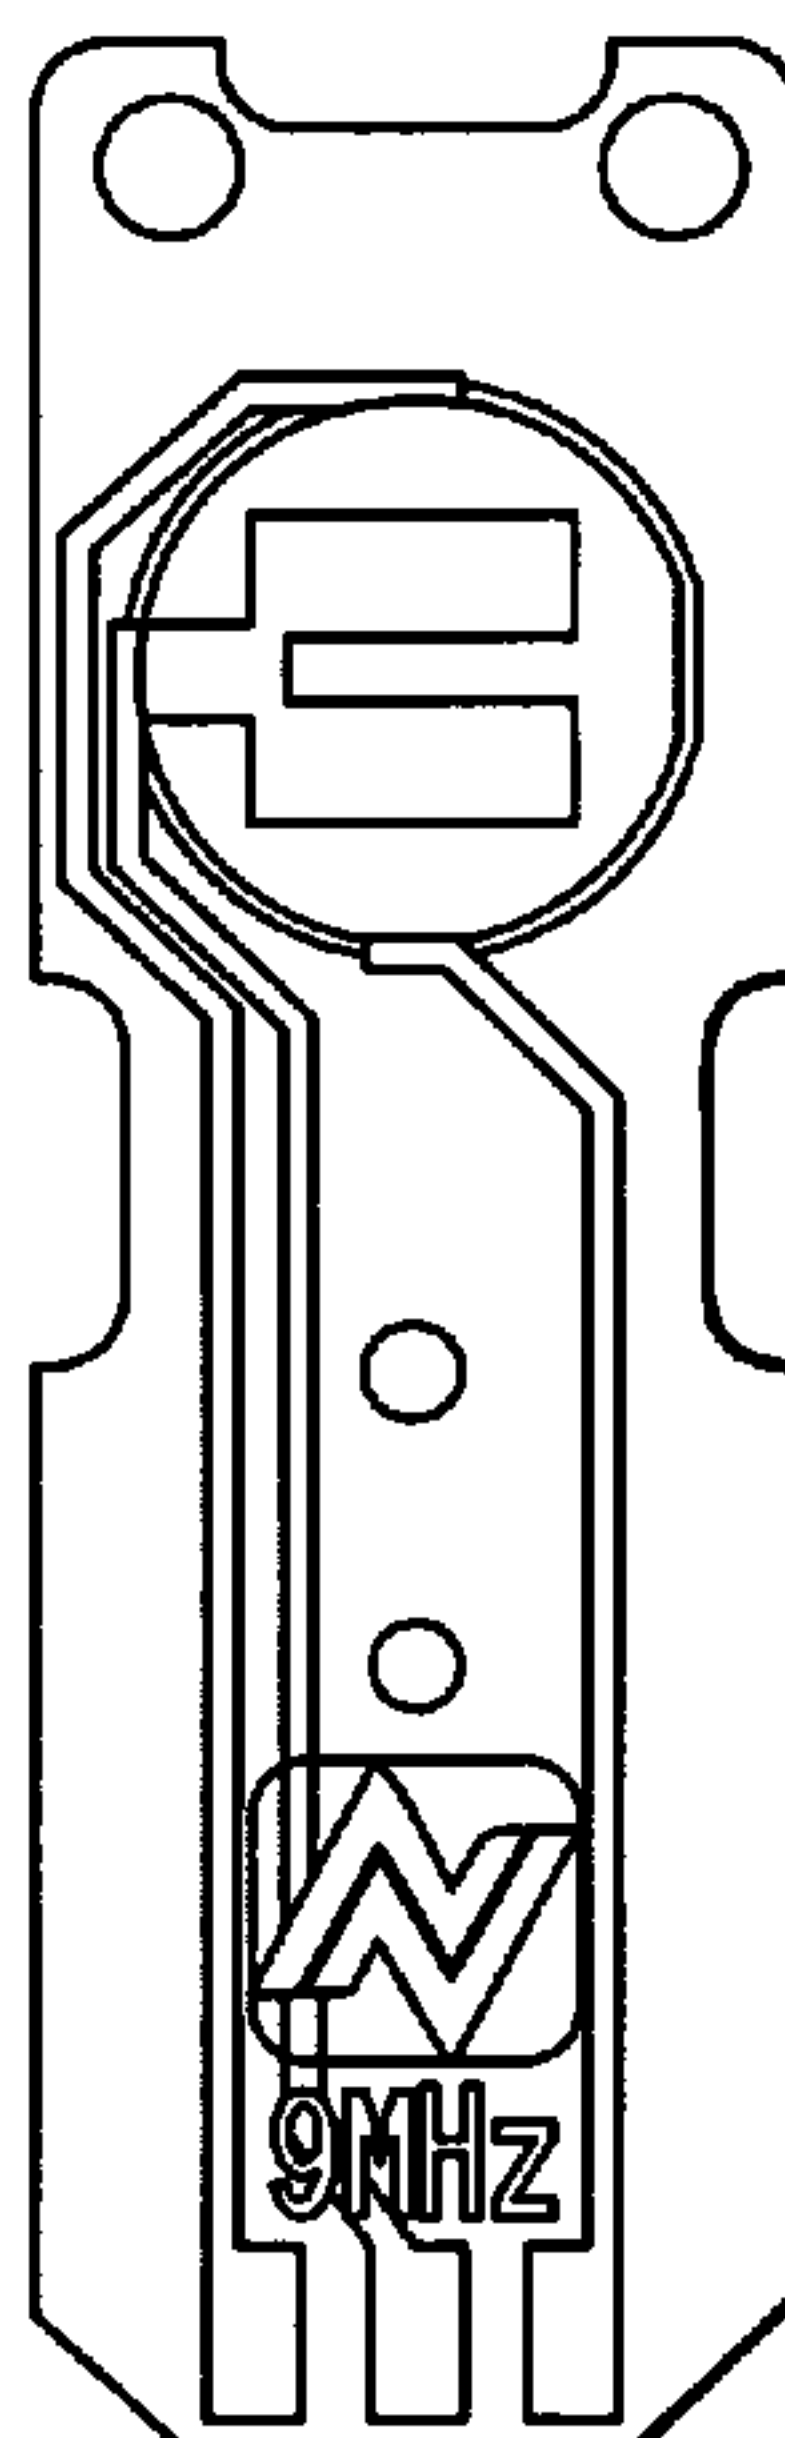

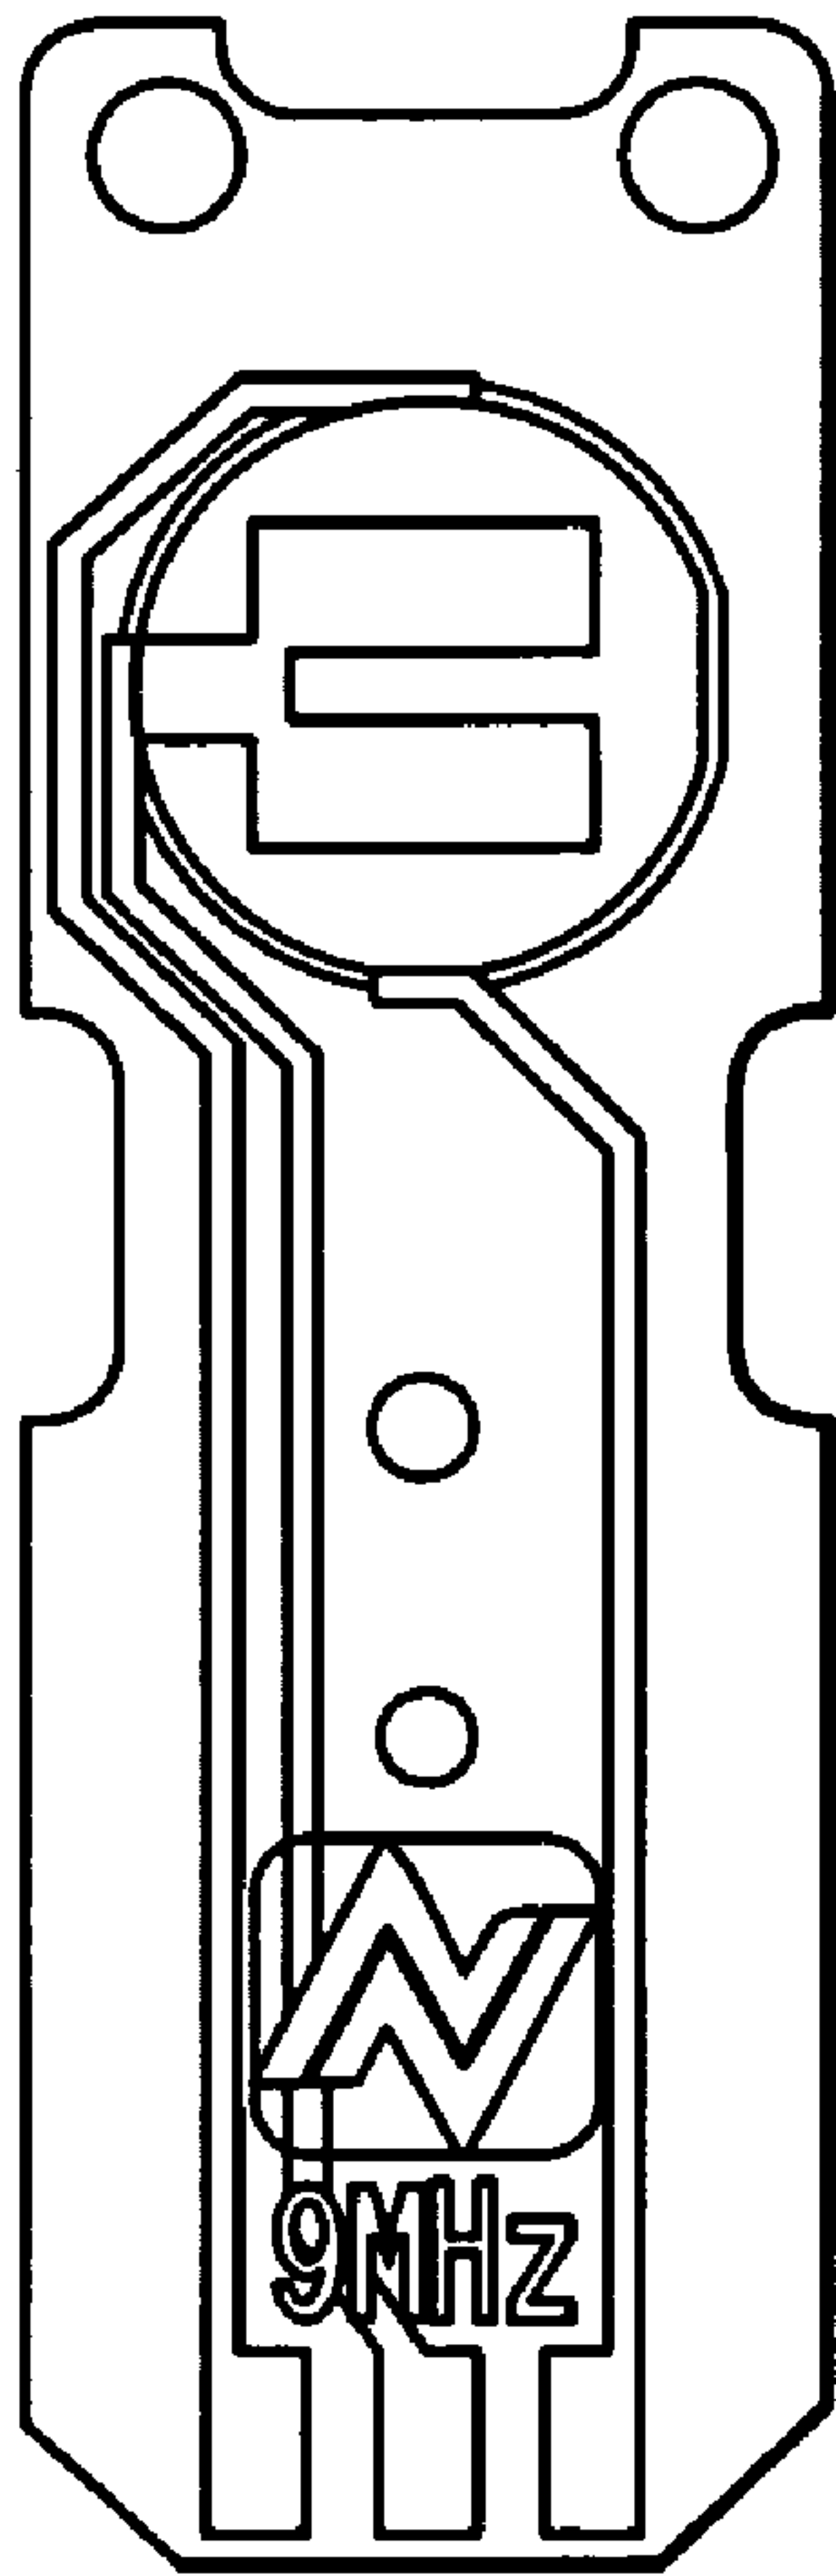


Fig. 1

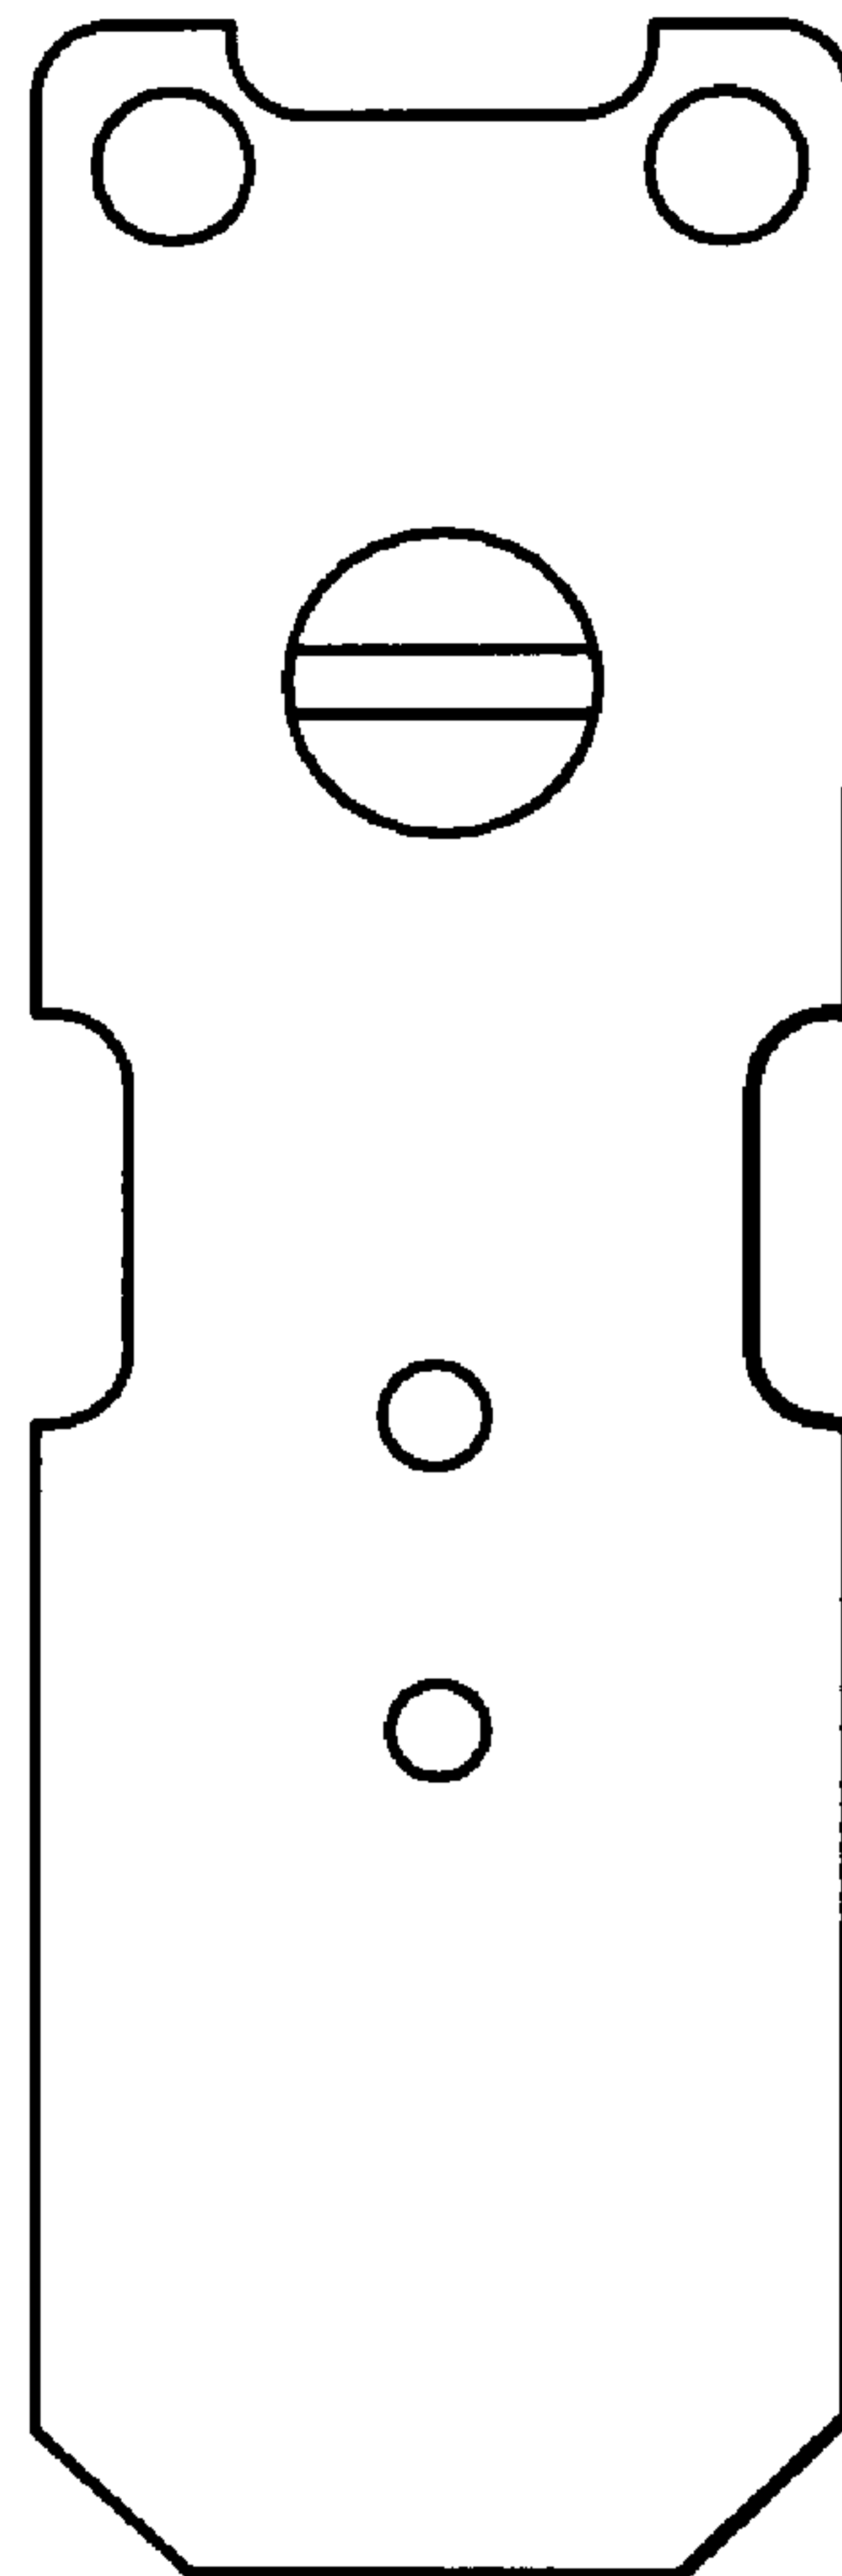


Fig. 2



Fig. 3




Fig. 4



Fig. 5



Fig. 6

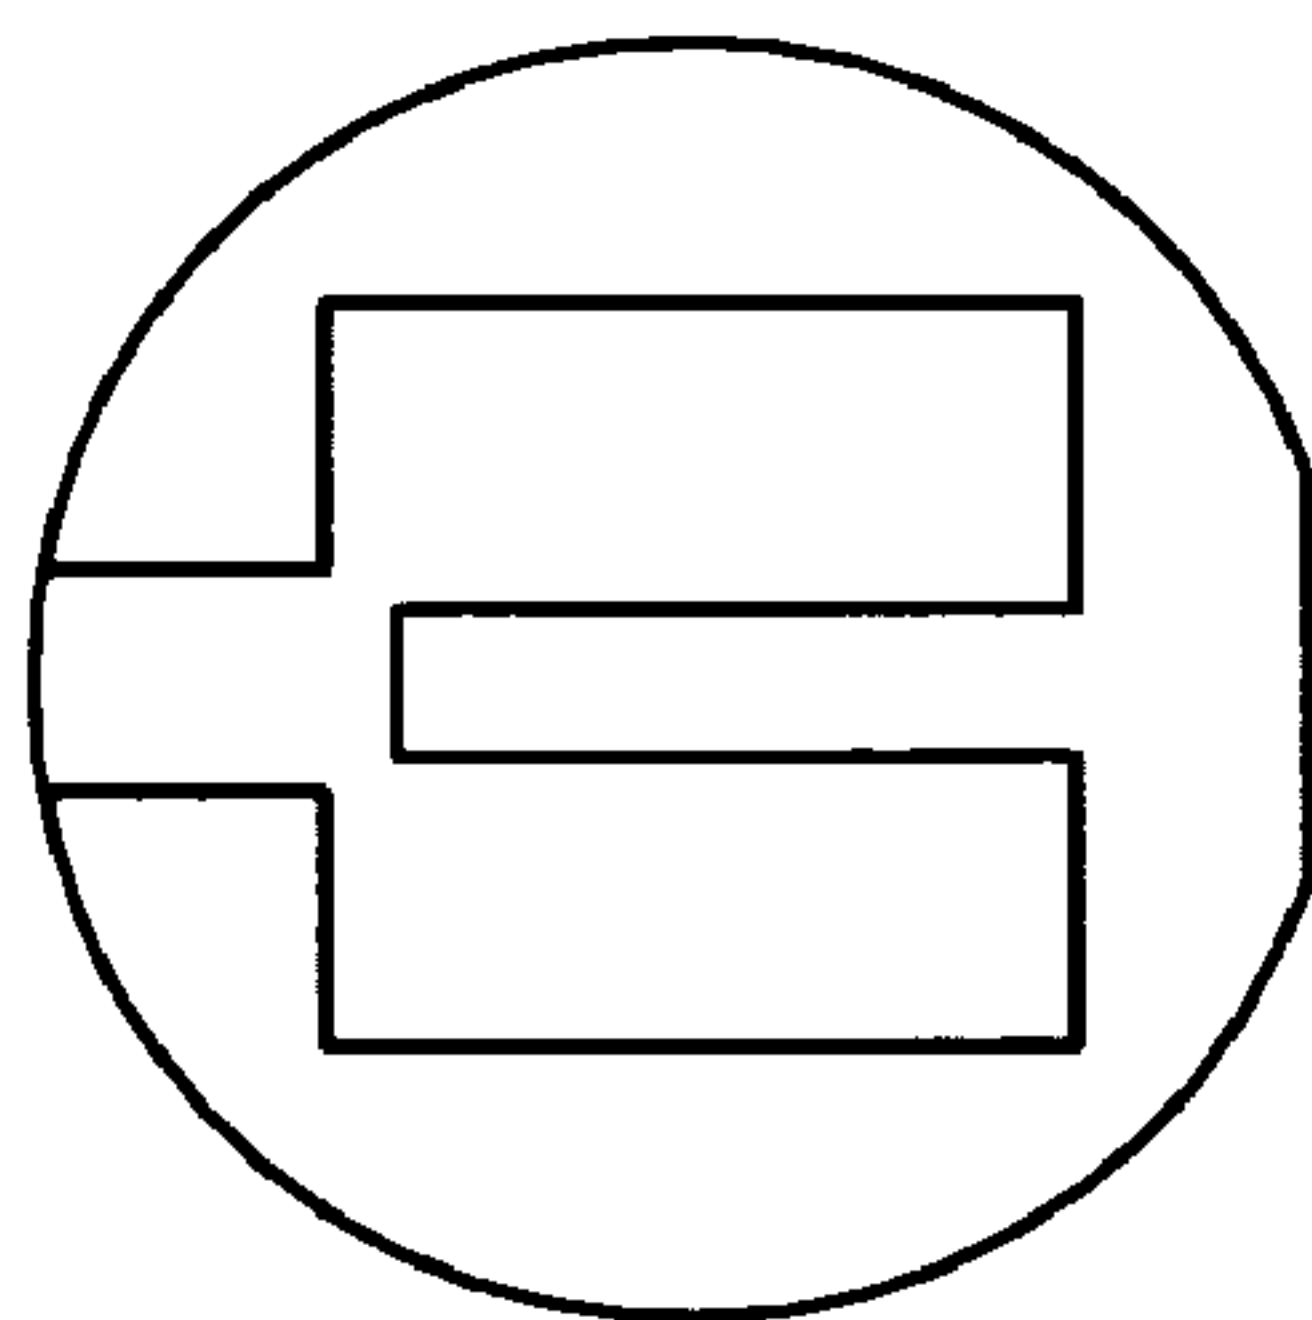


Fig. 7

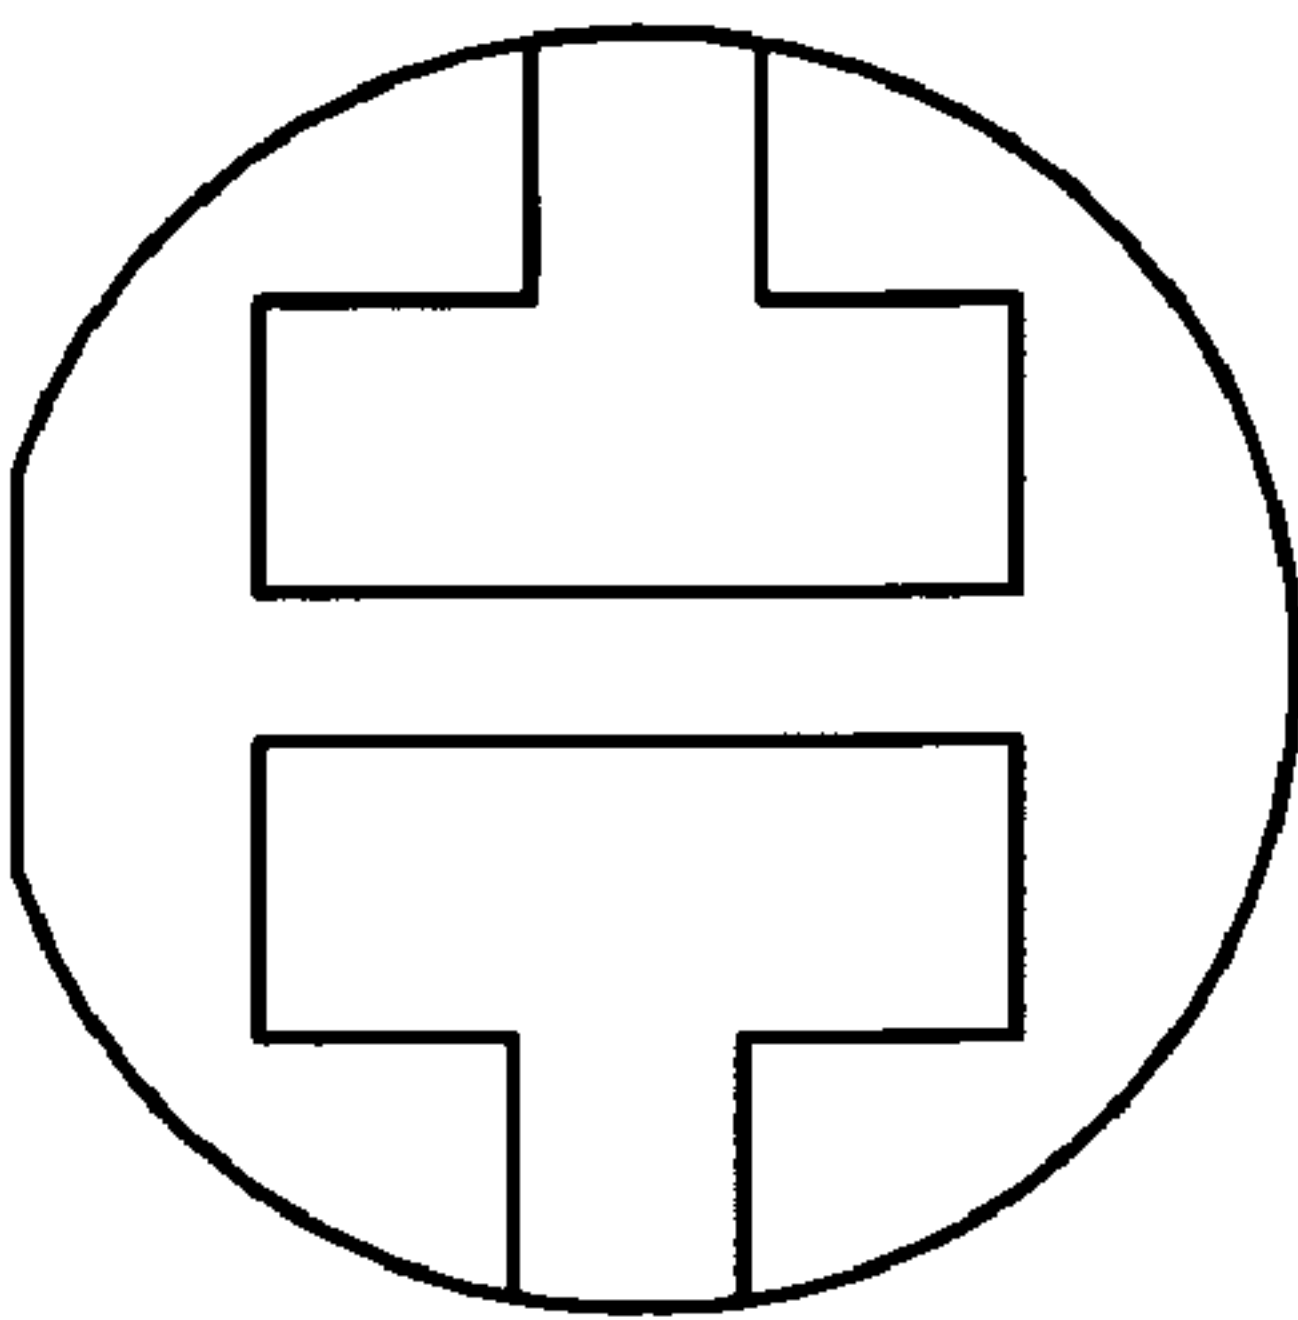


Fig. 8



Fig. 9



Fig. 10



Fig. 11



Fig. 12

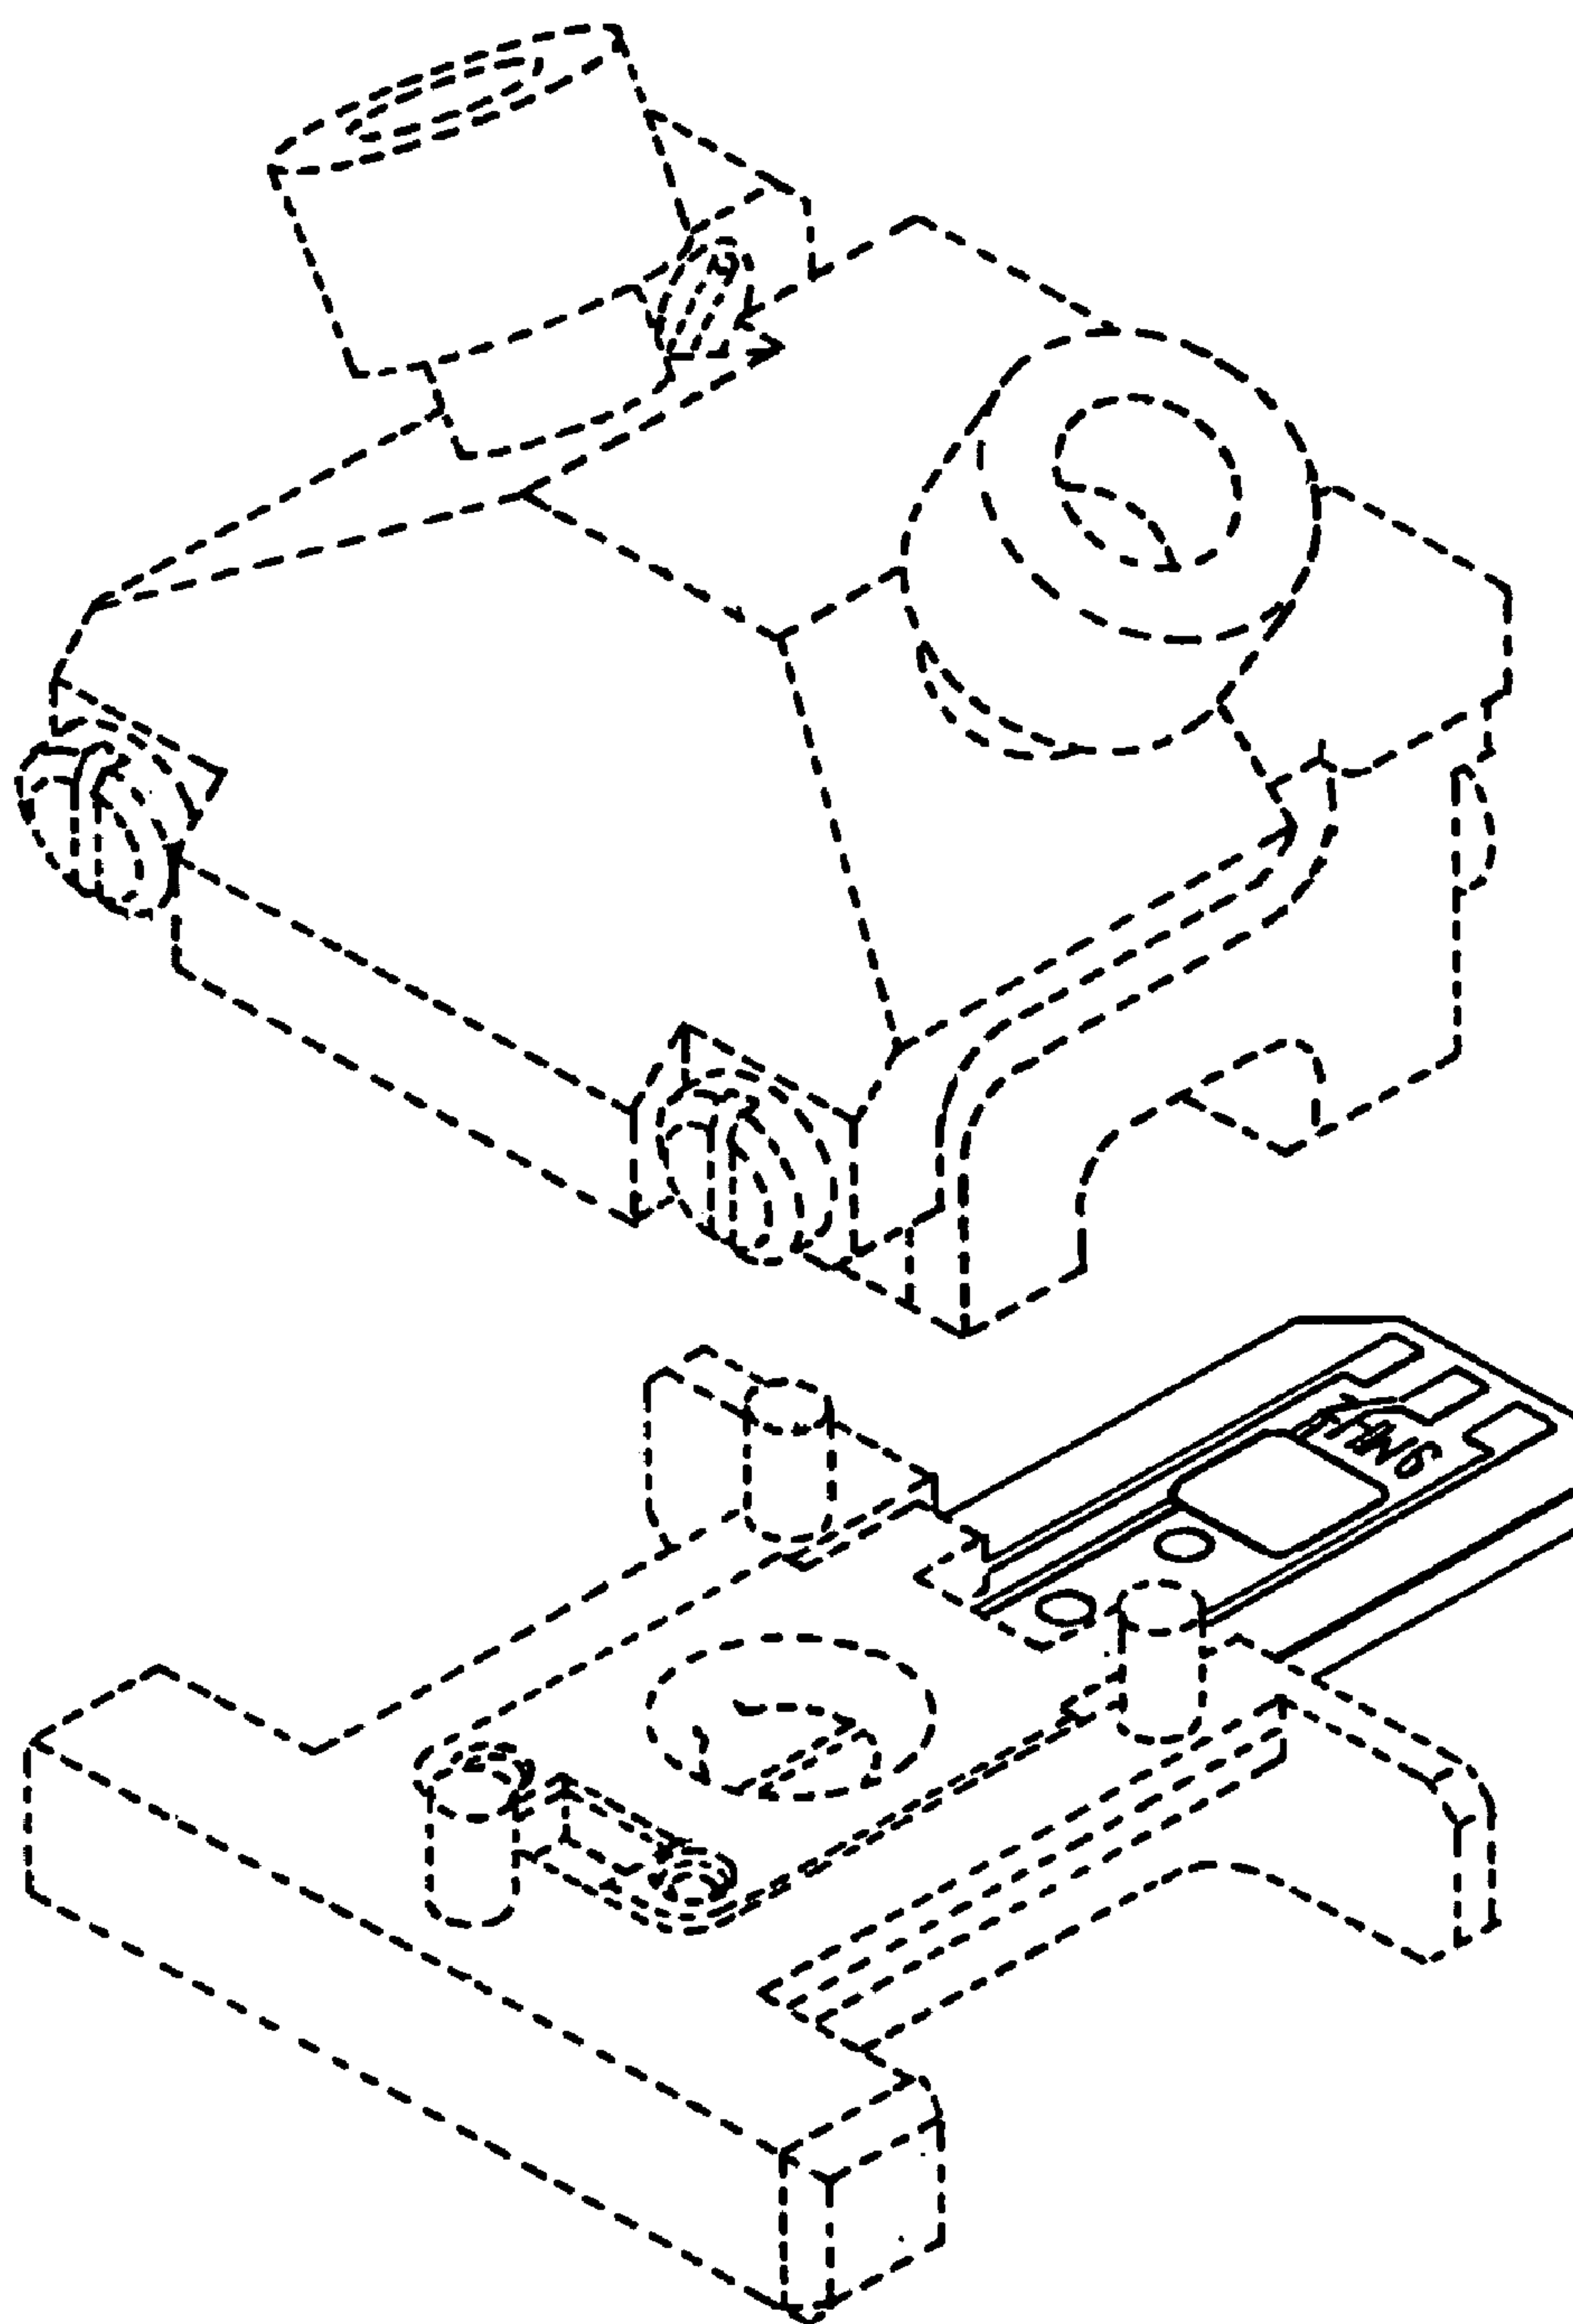


Fig. 13