



US00D606651S

(12) **United States Design Patent**  
**Bukoski et al.**

(10) **Patent No.:** **US D606,651 S**

(45) **Date of Patent:** **\*\* Dec. 22, 2009**

(54) **HANDLE PORTION OF A DENTAL SYRINGE**

(75) Inventors: **Timothy Daniel Bukoski**, Sherwood, OR (US); **Glenn A. Klecker**, Silverton, OR (US); **Jason Spencer**, Tega Cay, SC (US); **John Spencer**, Palm Desert, CA (US)

(73) Assignee: **Dental Components LLC**, Newberg, OR (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/335,761**

(22) Filed: **Apr. 21, 2009**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/113**

(58) **Field of Classification Search** ..... D24/112-114, D24/133, 186, 104, 130, 127, 152, 144; 606/181, 606/185, 205, 142; 604/232, 187, 158, 164.08, 604/192, 263, 163, 181, 184, 198, 227; 433/80; D4/131-135, 138; D32/51

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D220,185 S *	3/1971	Lake et al. ....	D24/113
D230,154 S *	1/1974	House .....	D24/113
D230,272 S	2/1974	Bueckle	
4,619,612 A	10/1986	Weber et al.	
4,907,968 A	3/1990	Eisner et al.	
D316,600 S	4/1991	Austin, Jr. et al.	
5,125,835 A	6/1992	Young	
5,199,871 A	4/1993	Young	
5,234,338 A	8/1993	Young	
5,489,205 A	2/1996	Davis et al.	
D377,716 S *	2/1997	Karon .....	D4/138
D396,957 S *	8/1998	Allende .....	D4/138
5,848,893 A	12/1998	Martin et al.	
D409,305 S	5/1999	Martin et al.	
6,293,792 B1	9/2001	Hanson	
D449,909 S *	10/2001	Randolph et al. ....	D4/138
D452,994 S *	1/2002	Mink et al. ....	D4/138

D458,761 S *	6/2002	Mason et al. ....	D4/135
D462,440 S *	9/2002	Formanek .....	D24/133
D578,773 S *	10/2008	Sherman et al. ....	D4/138
D580,658 S *	11/2008	Berti .....	D4/138
D586,562 S *	2/2009	Lui et al. ....	D4/138
D590,502 S *	4/2009	Geisser et al. ....	D24/133
D597,668 S *	8/2009	Woodruff et al. ....	D24/133

**OTHER PUBLICATIONS**

[http://www.carsondental.com/admin/uploads/safetips\\_medium.jpg](http://www.carsondental.com/admin/uploads/safetips_medium.jpg)  
(1 pg.) website visited Feb. 11, 2009.

(Continued)

*Primary Examiner*—T. Chase Nelson  
*Assistant Examiner*—David G Muller  
(74) *Attorney, Agent, or Firm*—Alston & Bird LLP

(57) **CLAIM**

The ornamental design for a handle portion of a dental syringe, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a handle portion of a dental syringe according to our new design;

FIG. 2 is a right side elevation view thereof;

FIG. 3 is a left side elevation view thereof;

FIG. 4 is a front elevation view thereof;


FIG. 5 is a rear elevation view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.


Broken lines shown herein which are illustrative of environmental structure of the upper portion, buttons, tip, bottom opening, and neck circumference of the dental syringe form no part of the claimed design. Broken lines shown herein which define the upper bounds of the handle portion of the dental syringe form no part of the claimed design.

**1 Claim, 6 Drawing Sheets**

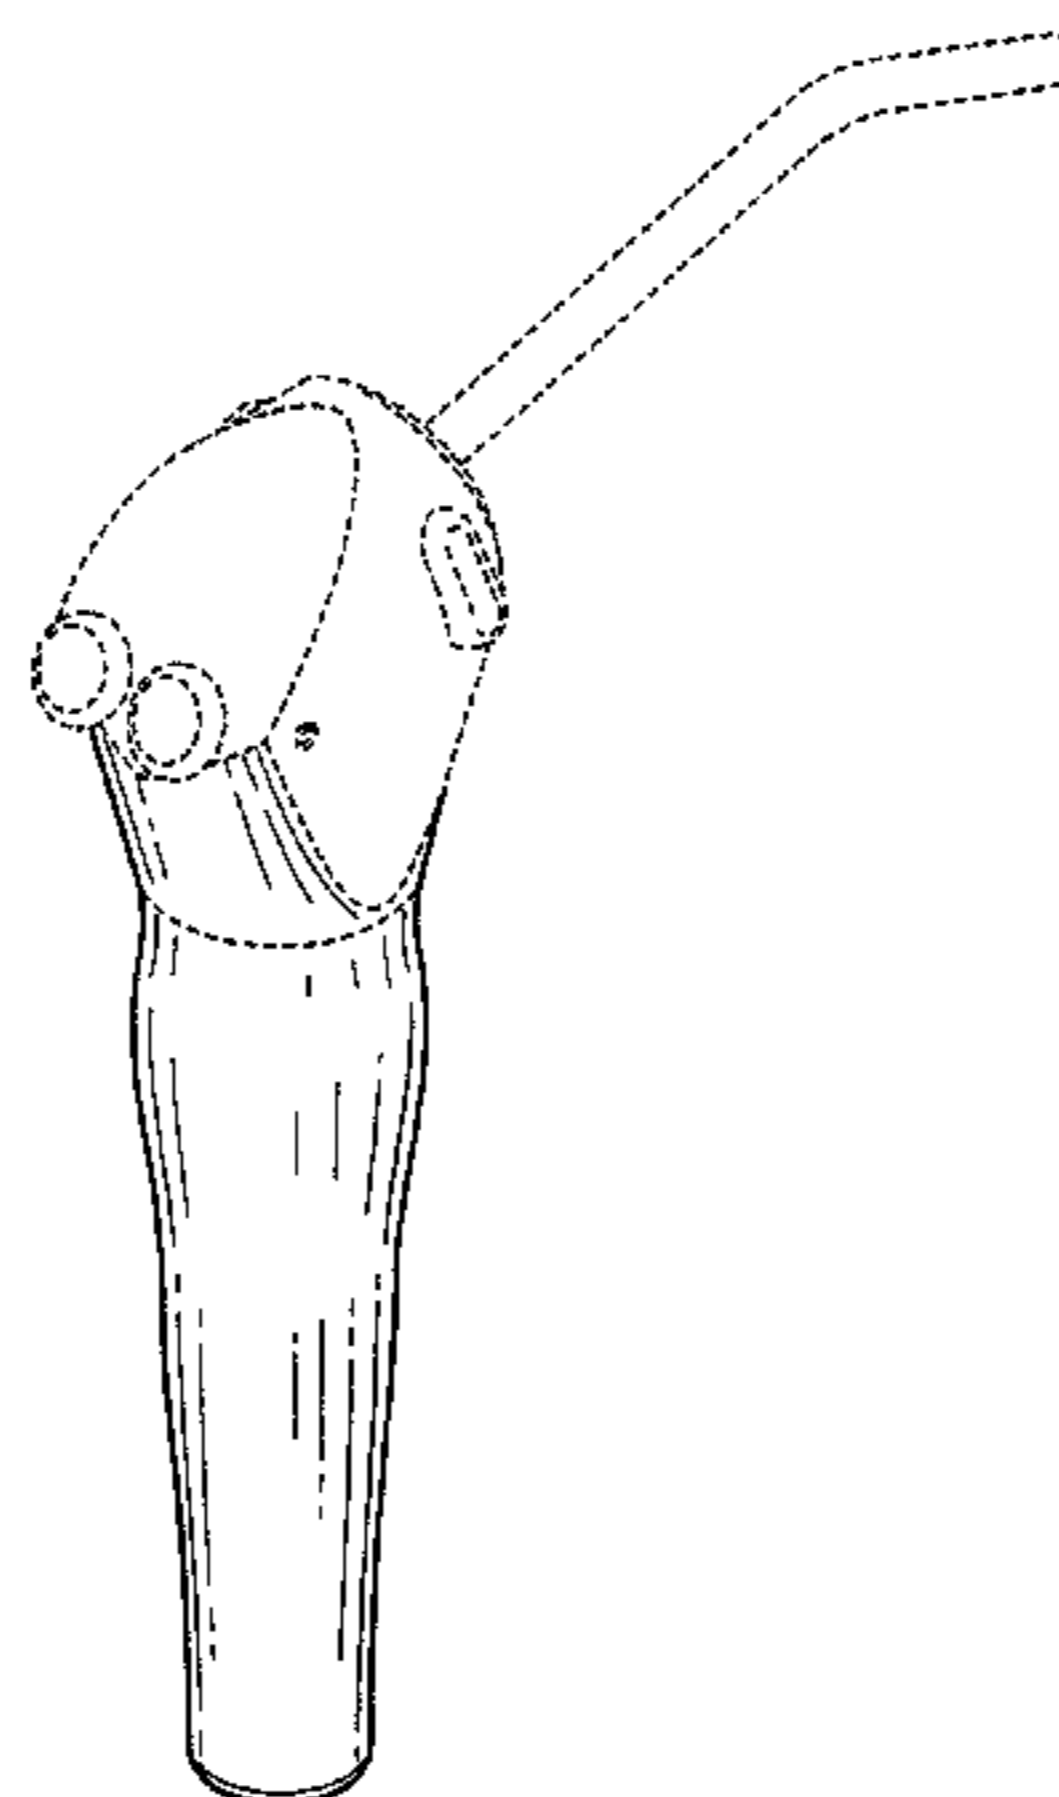

OTHER PUBLICATIONS

- <http://www.dcionline.com/PTIMG/3307b.jpg> (1 pg.) website visited Feb. 11, 2009.
- <http://www.dcionline.com/PTIMG/3369b.jpg> (1 pg.) website visited Feb. 11, 2009.
- <http://www.dcionline.com/PTIMG/3429b.jpg> (1 pg.) website visited Feb. 11, 2009.
- <http://www.dcionline.com/PTIMG/3430b.jpg> (1 pg.) website visited Feb. 11, 2009.
- <http://www.dcionline.com/PTIMG/3480b.jpg> (1 pg.) website visited Feb. 11, 2009.
- [http://dentalequipmentsparts.com/dental-service-parts/pinnacle\\_disposable\\_products/77200.jpg](http://dentalequipmentsparts.com/dental-service-parts/pinnacle_disposable_products/77200.jpg) (1 pgs.) website visited Feb. 11, 2009.
- [http://i7.ebayimg.com/03/i/000/36/c7/30ef\\_1\\_sb01.JPG](http://i7.ebayimg.com/03/i/000/36/c7/30ef_1_sb01.JPG) (1 pg.) website visited Feb. 11, 2009.
- <http://dirtydentistry.info/pictures/syringe.jpg> (1 pgs.) website visited Feb. 11, 2009.
- <http://www.nature.com/bdj/journal/v193/n8/images/4801601-15.jpg> (1 pg.) website visited Feb. 11, 2009.
- <https://www.net32.com/images/equipment/Air-Water-Syringes-metal-tip-quick-change.jpg> (1 pg.) website visited Feb. 11, 2009.
- \* cited by examiner

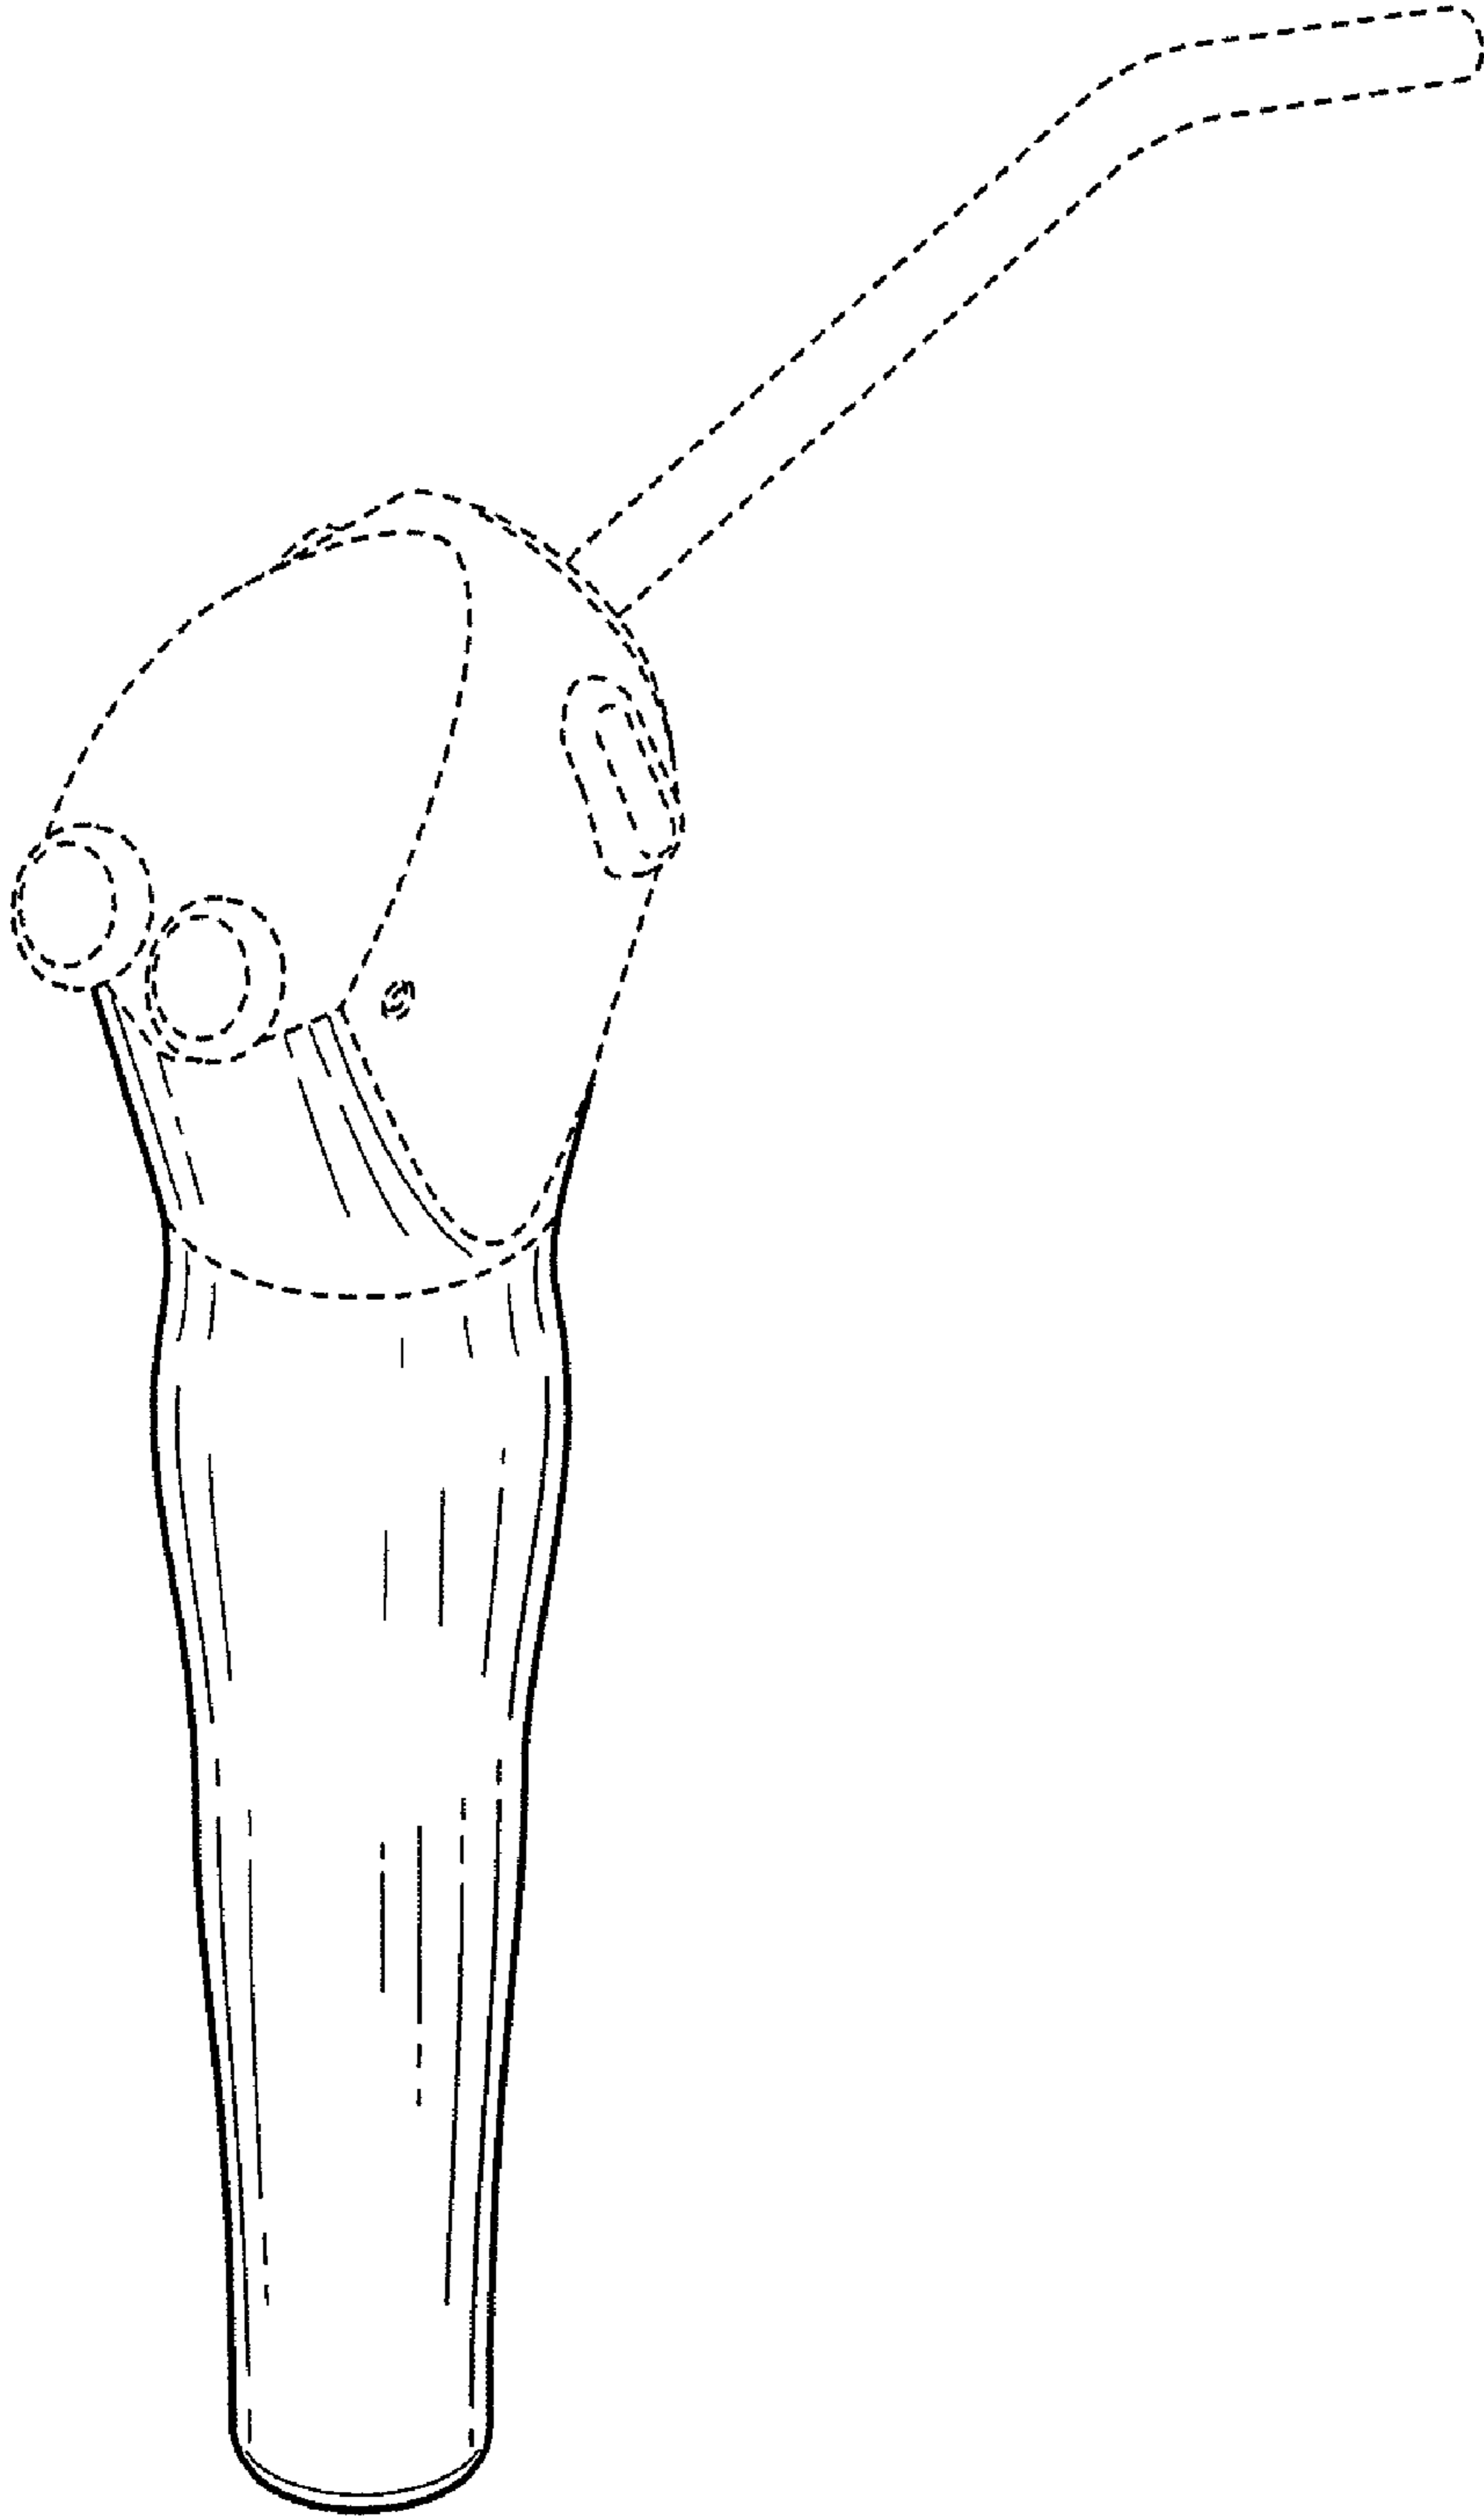

**FIG. 1**



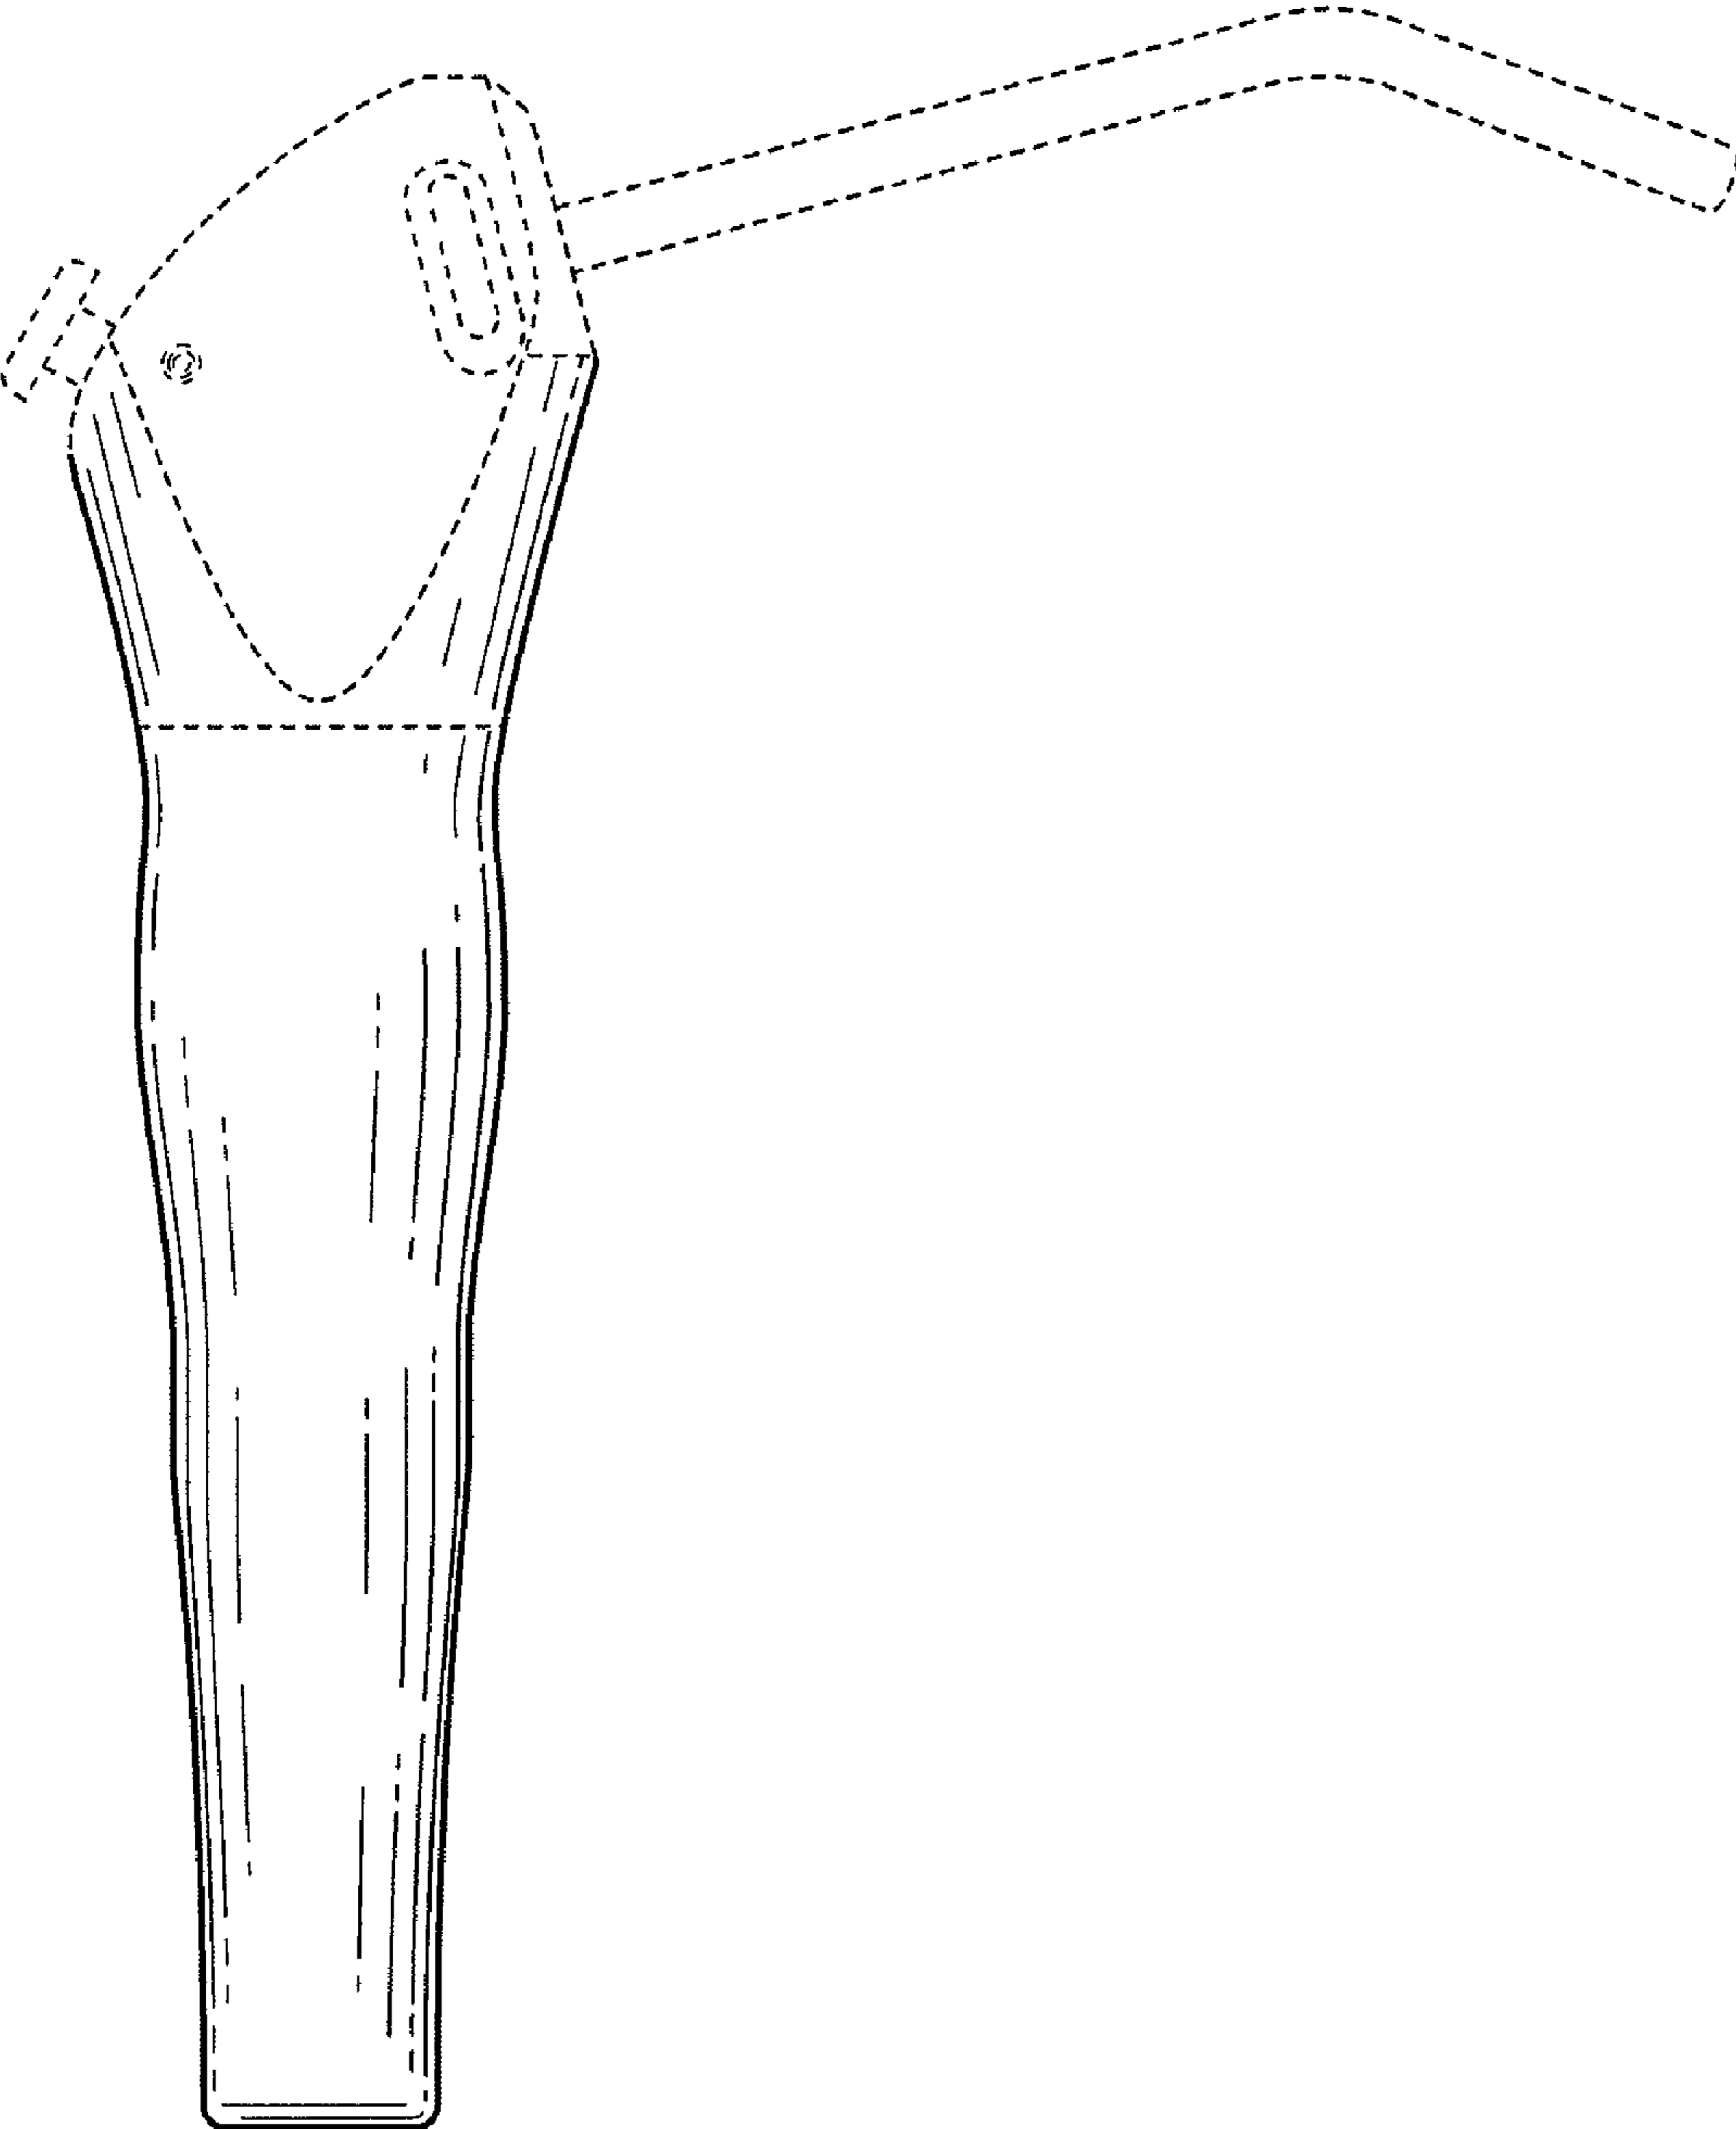



FIG. 2

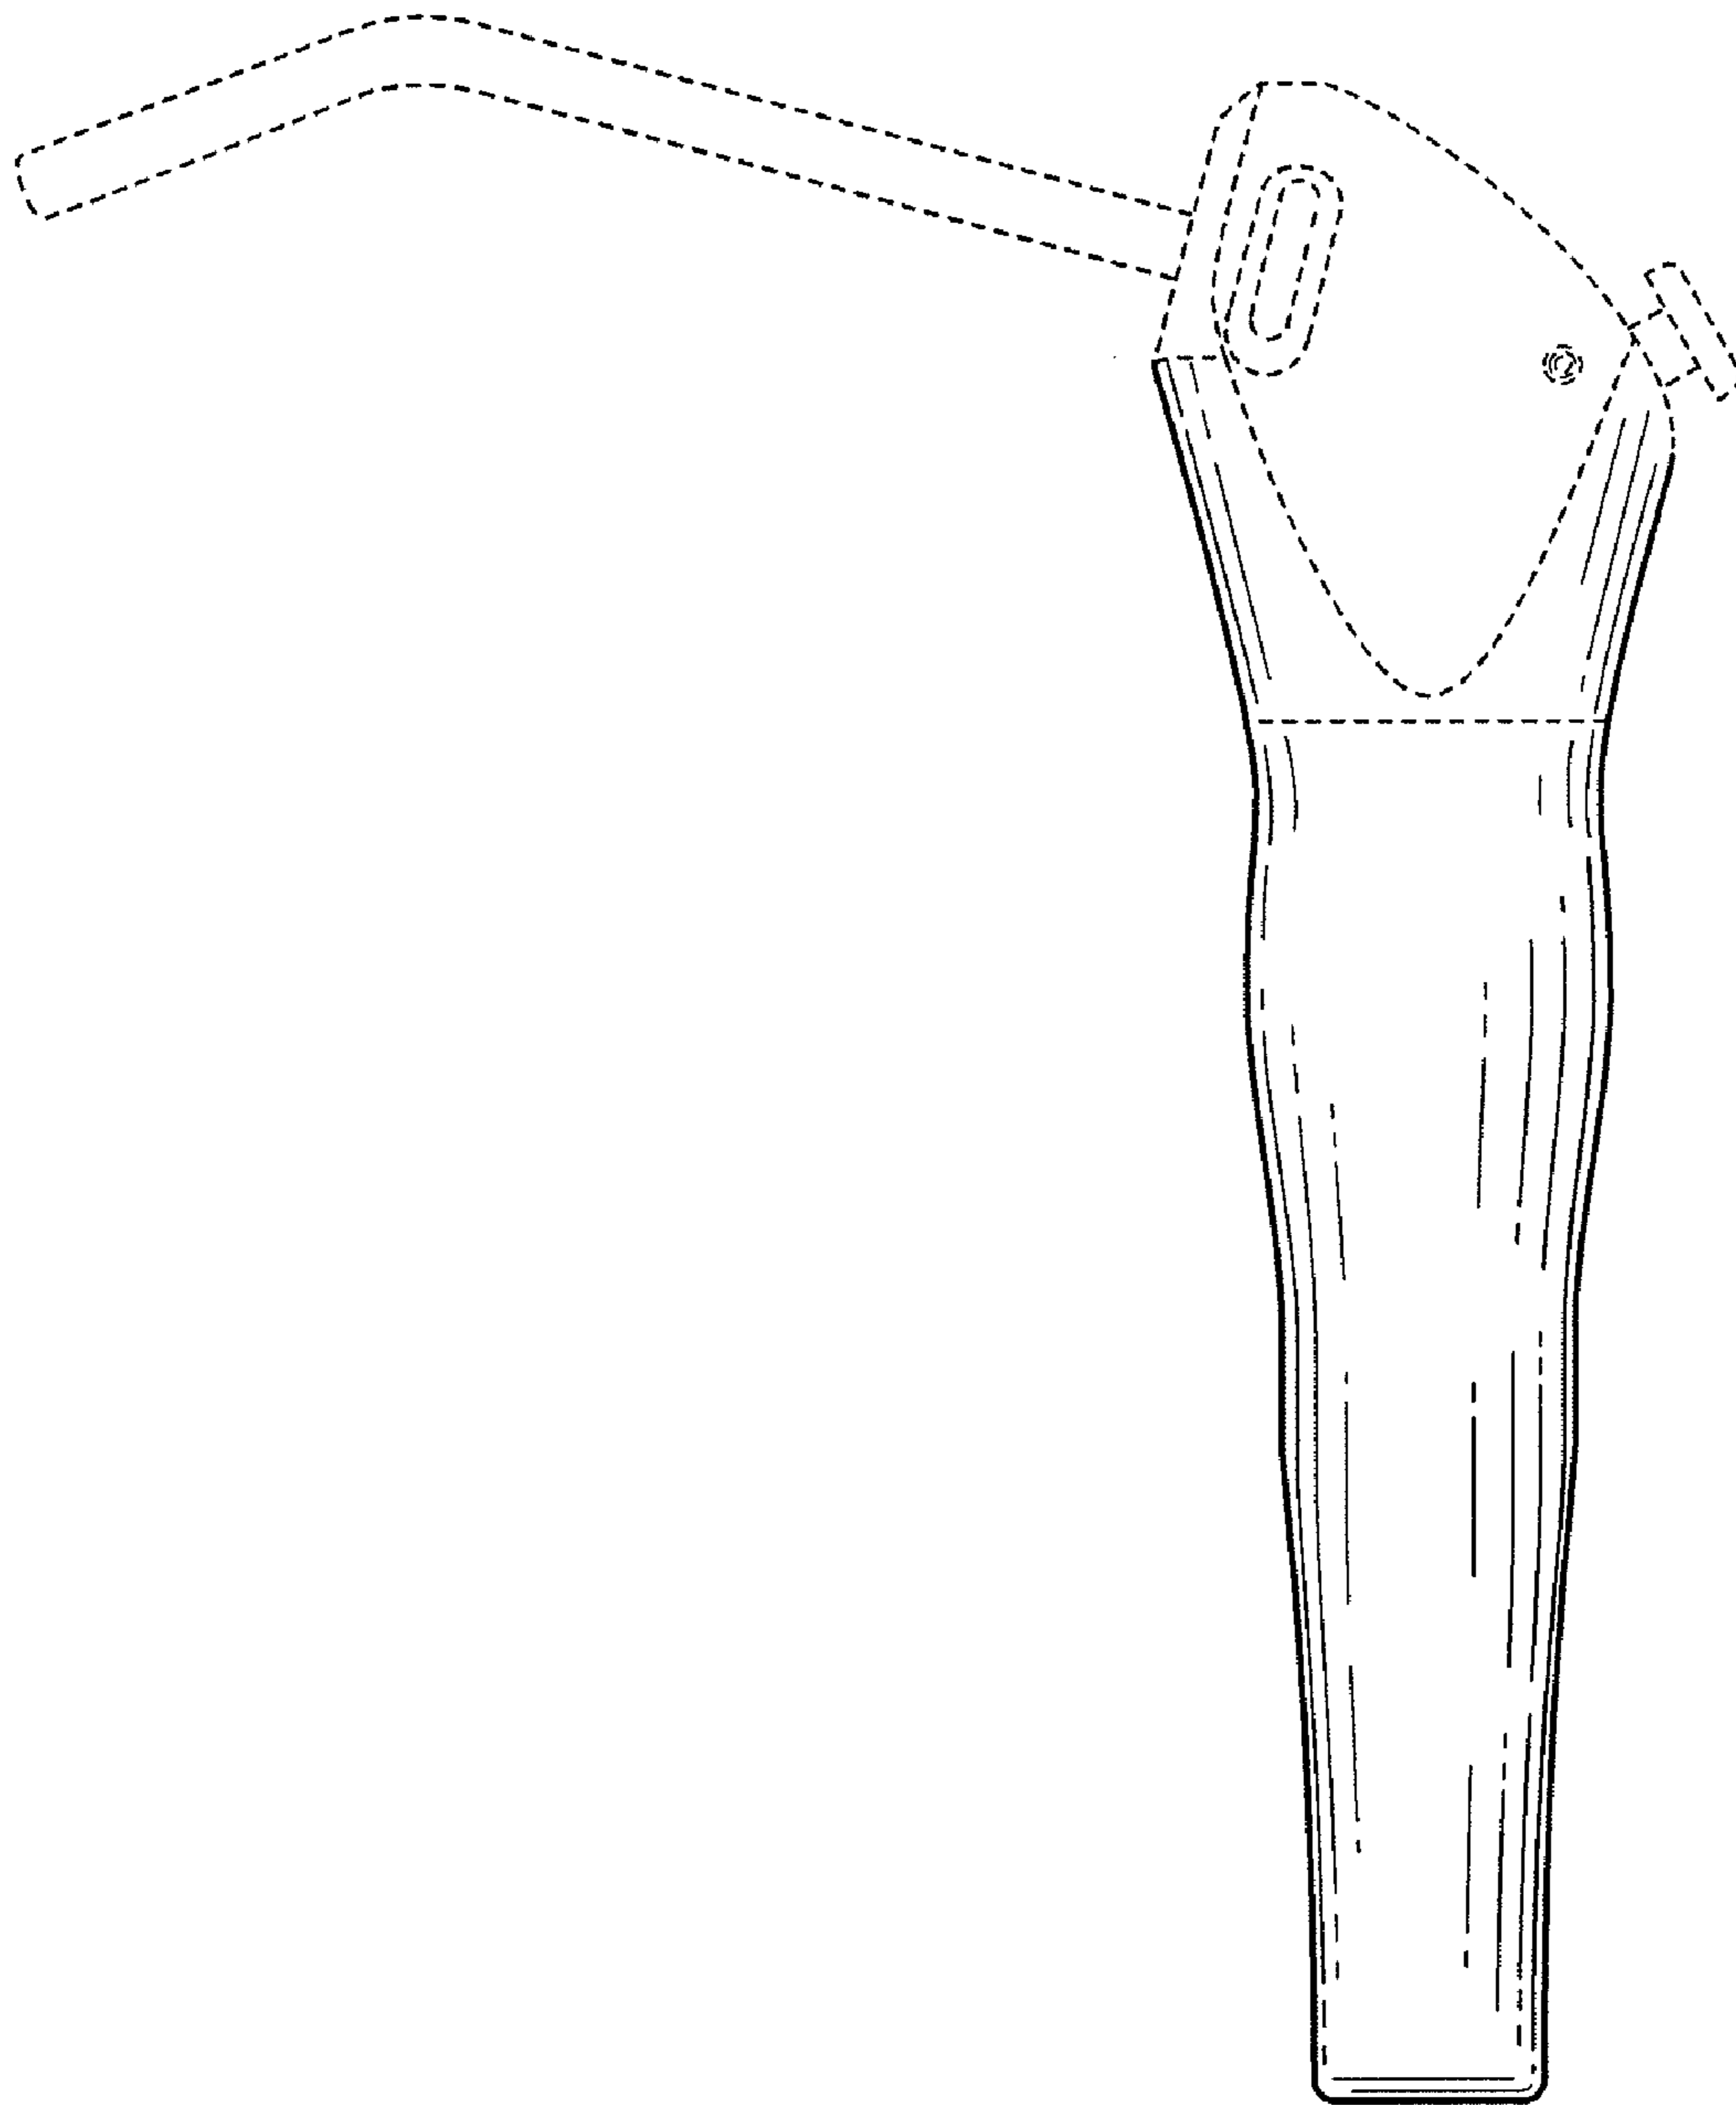


**FIG. 3**

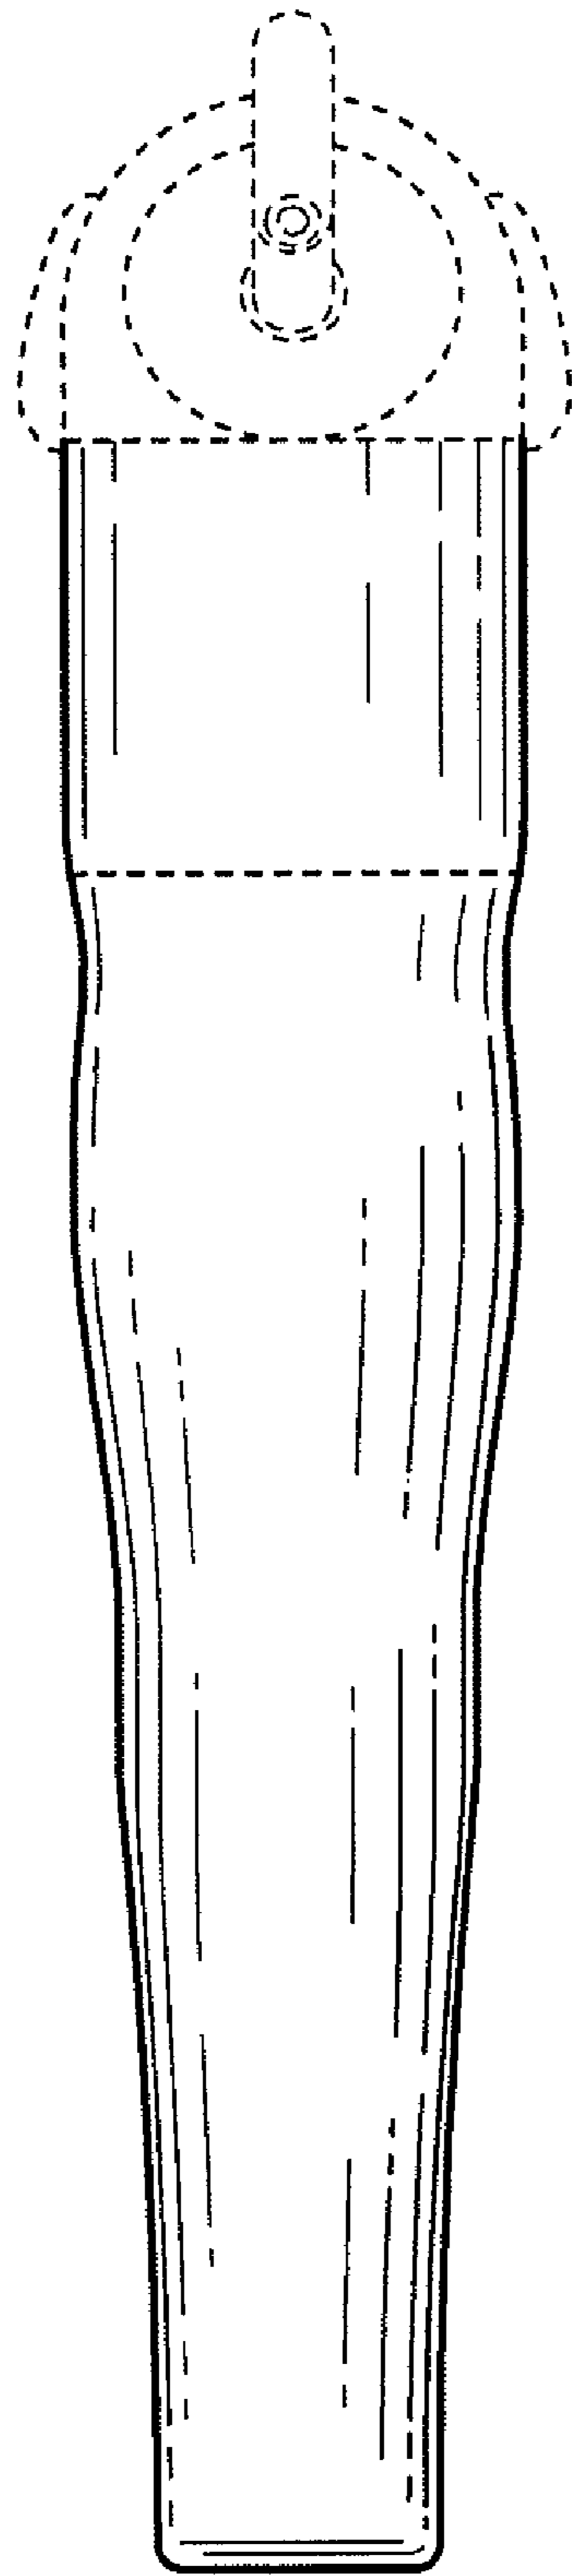


**FIG. 4**

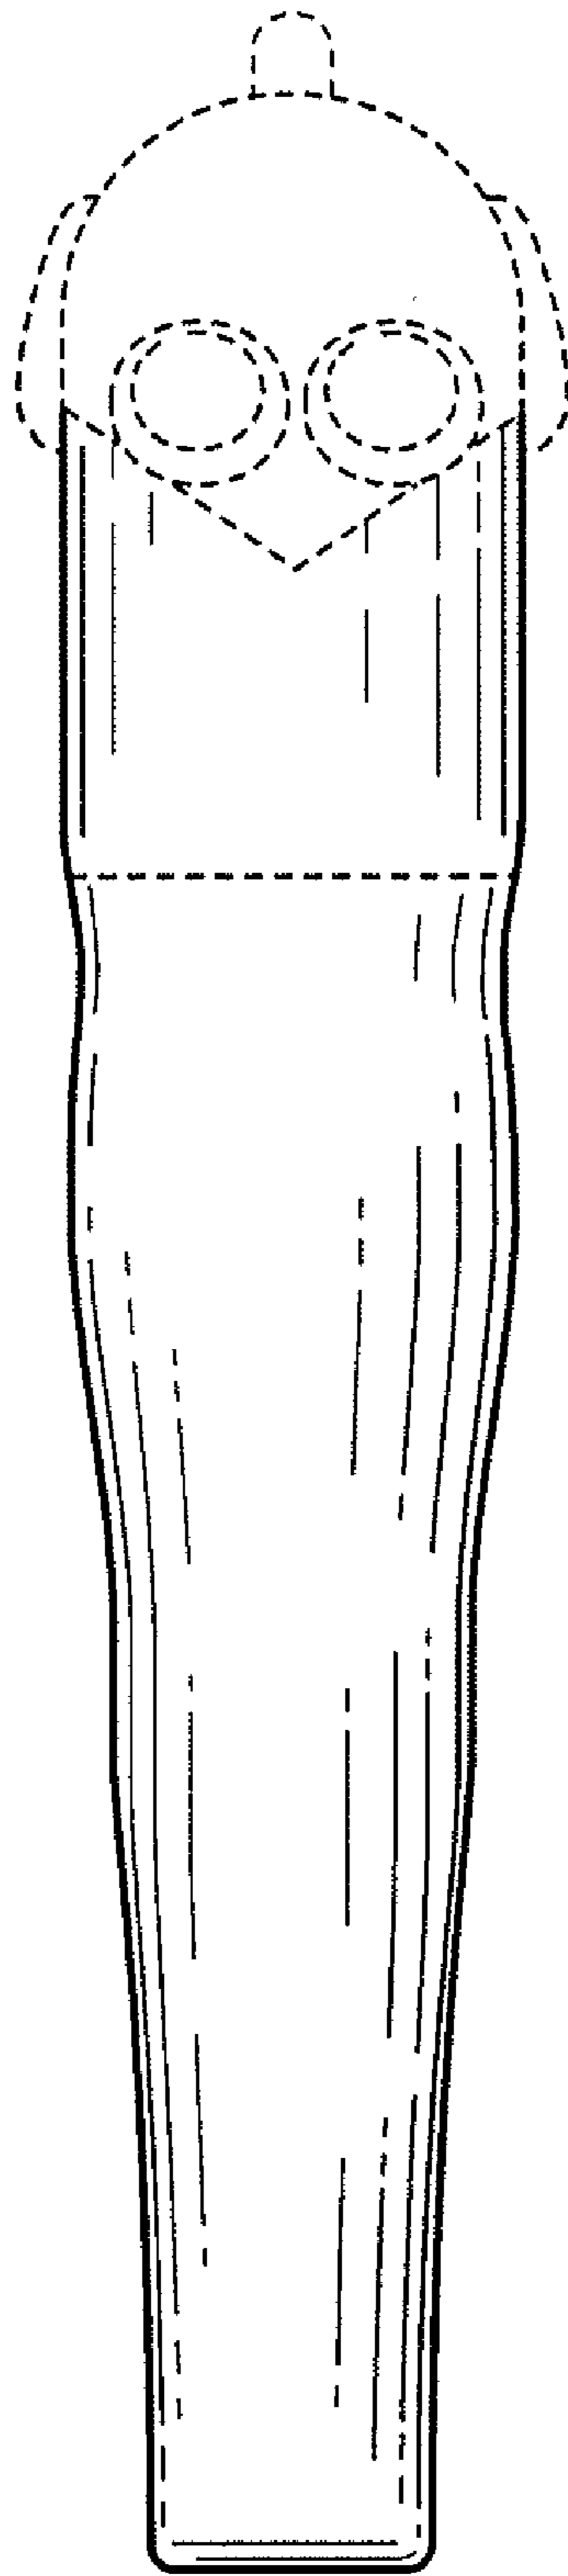

**FIG. 5**

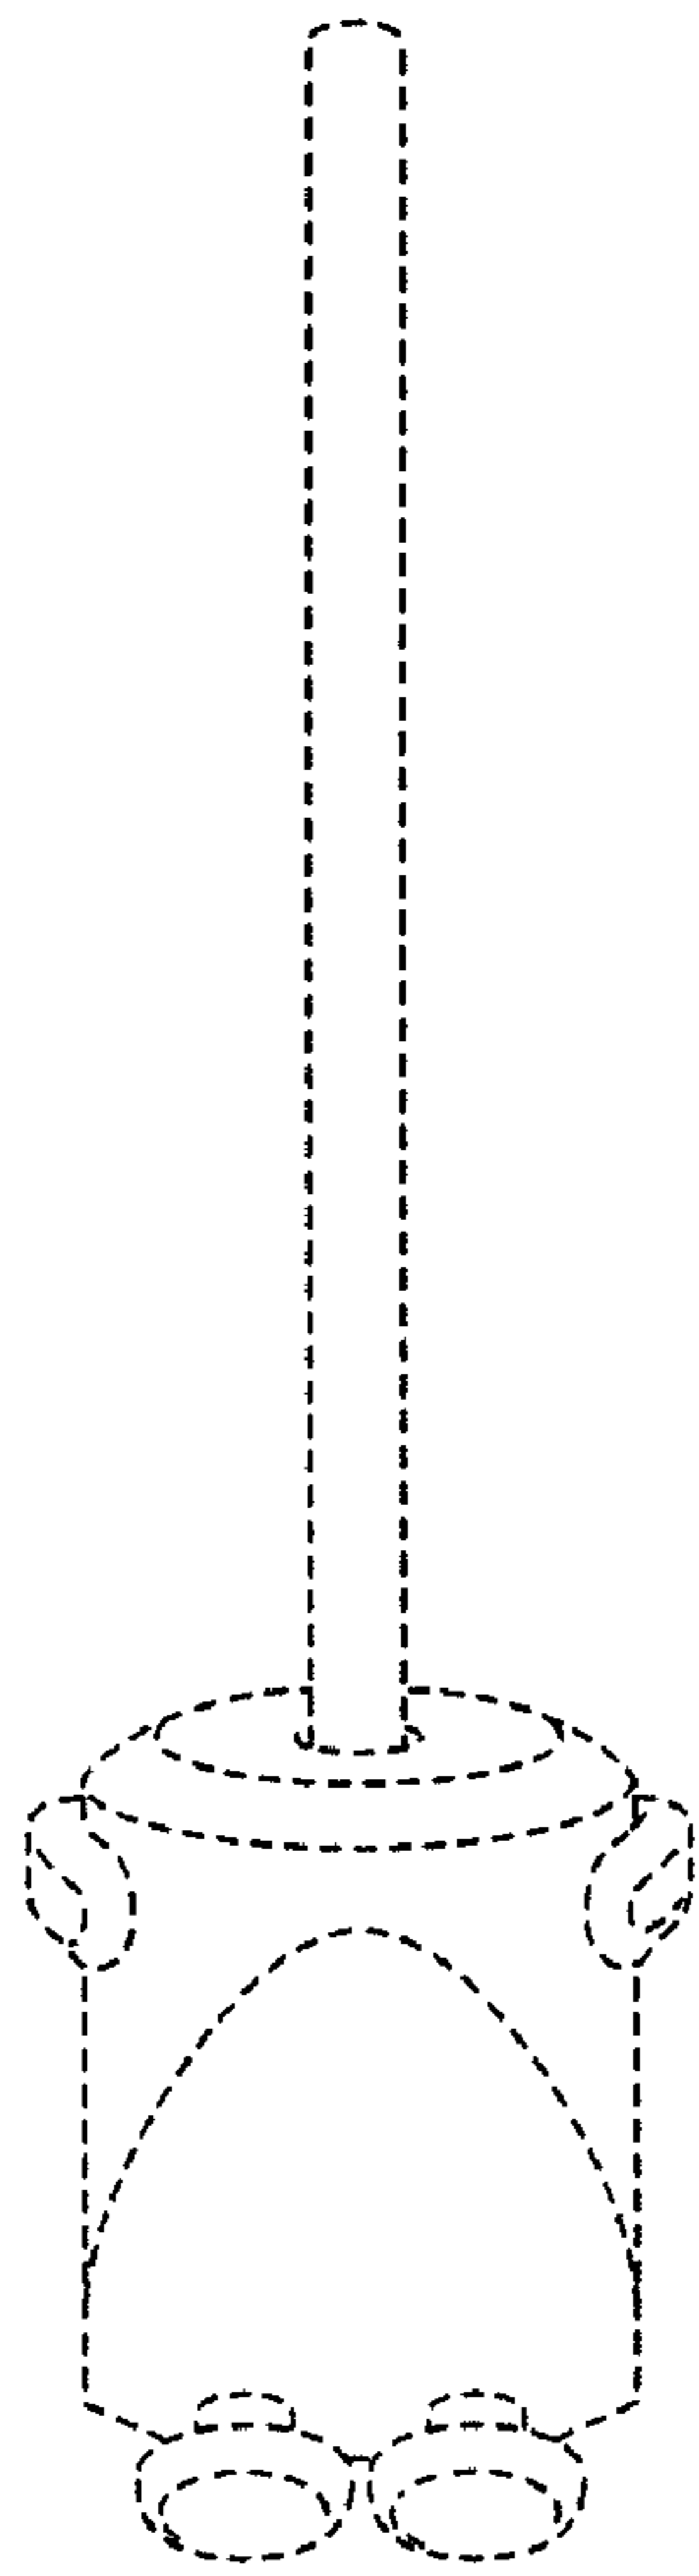

**FIG. 6**

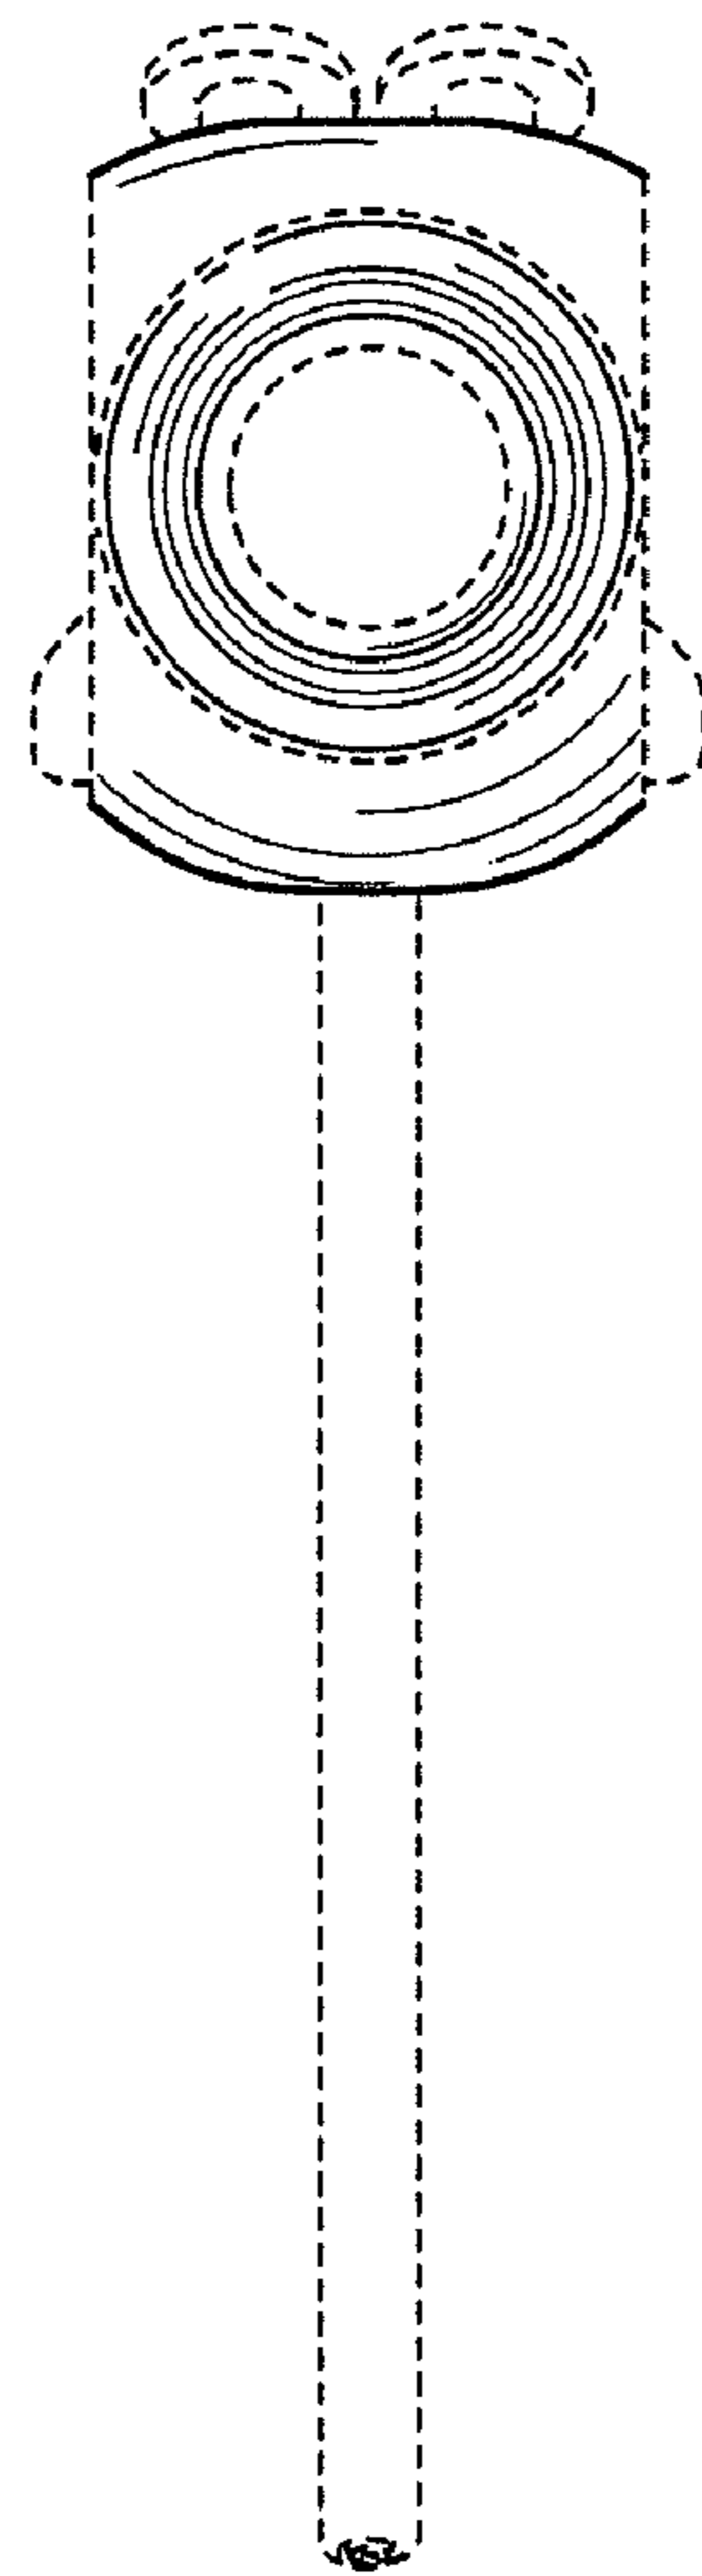

**FIG. 7**