



US00D608446S

(12) **United States Design Patent**  
**Shibata et al.**

(10) **Patent No.:** **US D608,446 S**  
(45) **Date of Patent:** **\*\* Jan. 19, 2010**

(54) **ARM PLATE FOR SPHYGMOMANOMETER**

6,714,814 B2 3/2004 Yamada et al.  
D489,113 S 4/2004 Peterson  
6,726,633 B2 4/2004 Kitagawa

(75) Inventors: **Fumie Shibata**, Tokyo (JP); **Yuki Shibata**, Tokyo (JP); **Tadashi Koike**, Kyoto (JP); **Tomohiro Kukita**, Kyoto (JP); **Masataka Yanagase**, Osaka (JP); **Yukiko Mitsunami**, Otsu (JP)

(Continued)

**FOREIGN PATENT DOCUMENTS**

(73) Assignee: **Omron Healthcare Co., Ltd.**, Kyoto (JP)

JP 1140559 5/2002

(Continued)

(\*\*) Term: **14 Years**

**OTHER PUBLICATIONS**

(21) Appl. No.: **29/318,610**

RD 000223979 0001-0006, Sphygmometers, Nov. 30, 2004.

(22) Filed: **May 22, 2008**

(Continued)

(30) **Foreign Application Priority Data**

Nov. 30, 2007 (JP) ..... 2007-032948

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Capitol City TechLaw

(51) **LOC (9) Cl.** ..... **24-02**

(57) **CLAIM**

(52) **U.S. Cl.** ..... **D24/165**

(58) **Field of Classification Search** ..... D24/164–169,  
D24/186, 183, 184; D10/98; 600/301, 481,  
600/483–485, 490, 493–495, 499, 500, 501;  
128/900; 5/646

The ornamental design for an arm plate for sphygmomanometer, as shown and described.

See application file for complete search history.

**DESCRIPTION**


(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D123,424 S \* 11/1940 Williams ..... D24/167  
3,935,984 A 2/1976 Lichowsky et al.  
D244,235 S 5/1977 Lichowsky  
4,058,117 A 11/1977 Kaspari et al.  
D254,629 S 4/1980 Yen  
D290,876 S 7/1987 Arduini et al.  
D321,562 S 11/1991 Ljungvall  
D341,658 S 11/1993 Kojima  
5,511,551 A 4/1996 Sano et al.  
D422,362 S \* 4/2000 Ames ..... D24/183  
D424,698 S \* 5/2000 Ames ..... D24/183  
D438,970 S \* 3/2001 TerMeer et al. .... D24/165  
6,213,953 B1 4/2001 Reeves  
D447,568 S 9/2001 Hall et al.

FIG. 1 is a front perspective view of an arm plate for sphygmomanometer showing our new design;  
FIG. 2 is a rear perspective view thereof;  
FIG. 3 is a front elevational view thereof;  
FIG. 4 is a rear elevational view thereof;  
FIG. 5 is a top plan view thereof;  
FIG. 6 is a bottom plan view thereof;  
FIG. 7 is a right side elevational view thereof;  
FIG. 8 is a left side elevational view thereof;  
FIG. 9 is a front perspective view thereof with a joint shown in a folded position; and,  
FIG. 10 is a rear perspective view thereof with the joint shown in a folded position.

**1 Claim, 4 Drawing Sheets**

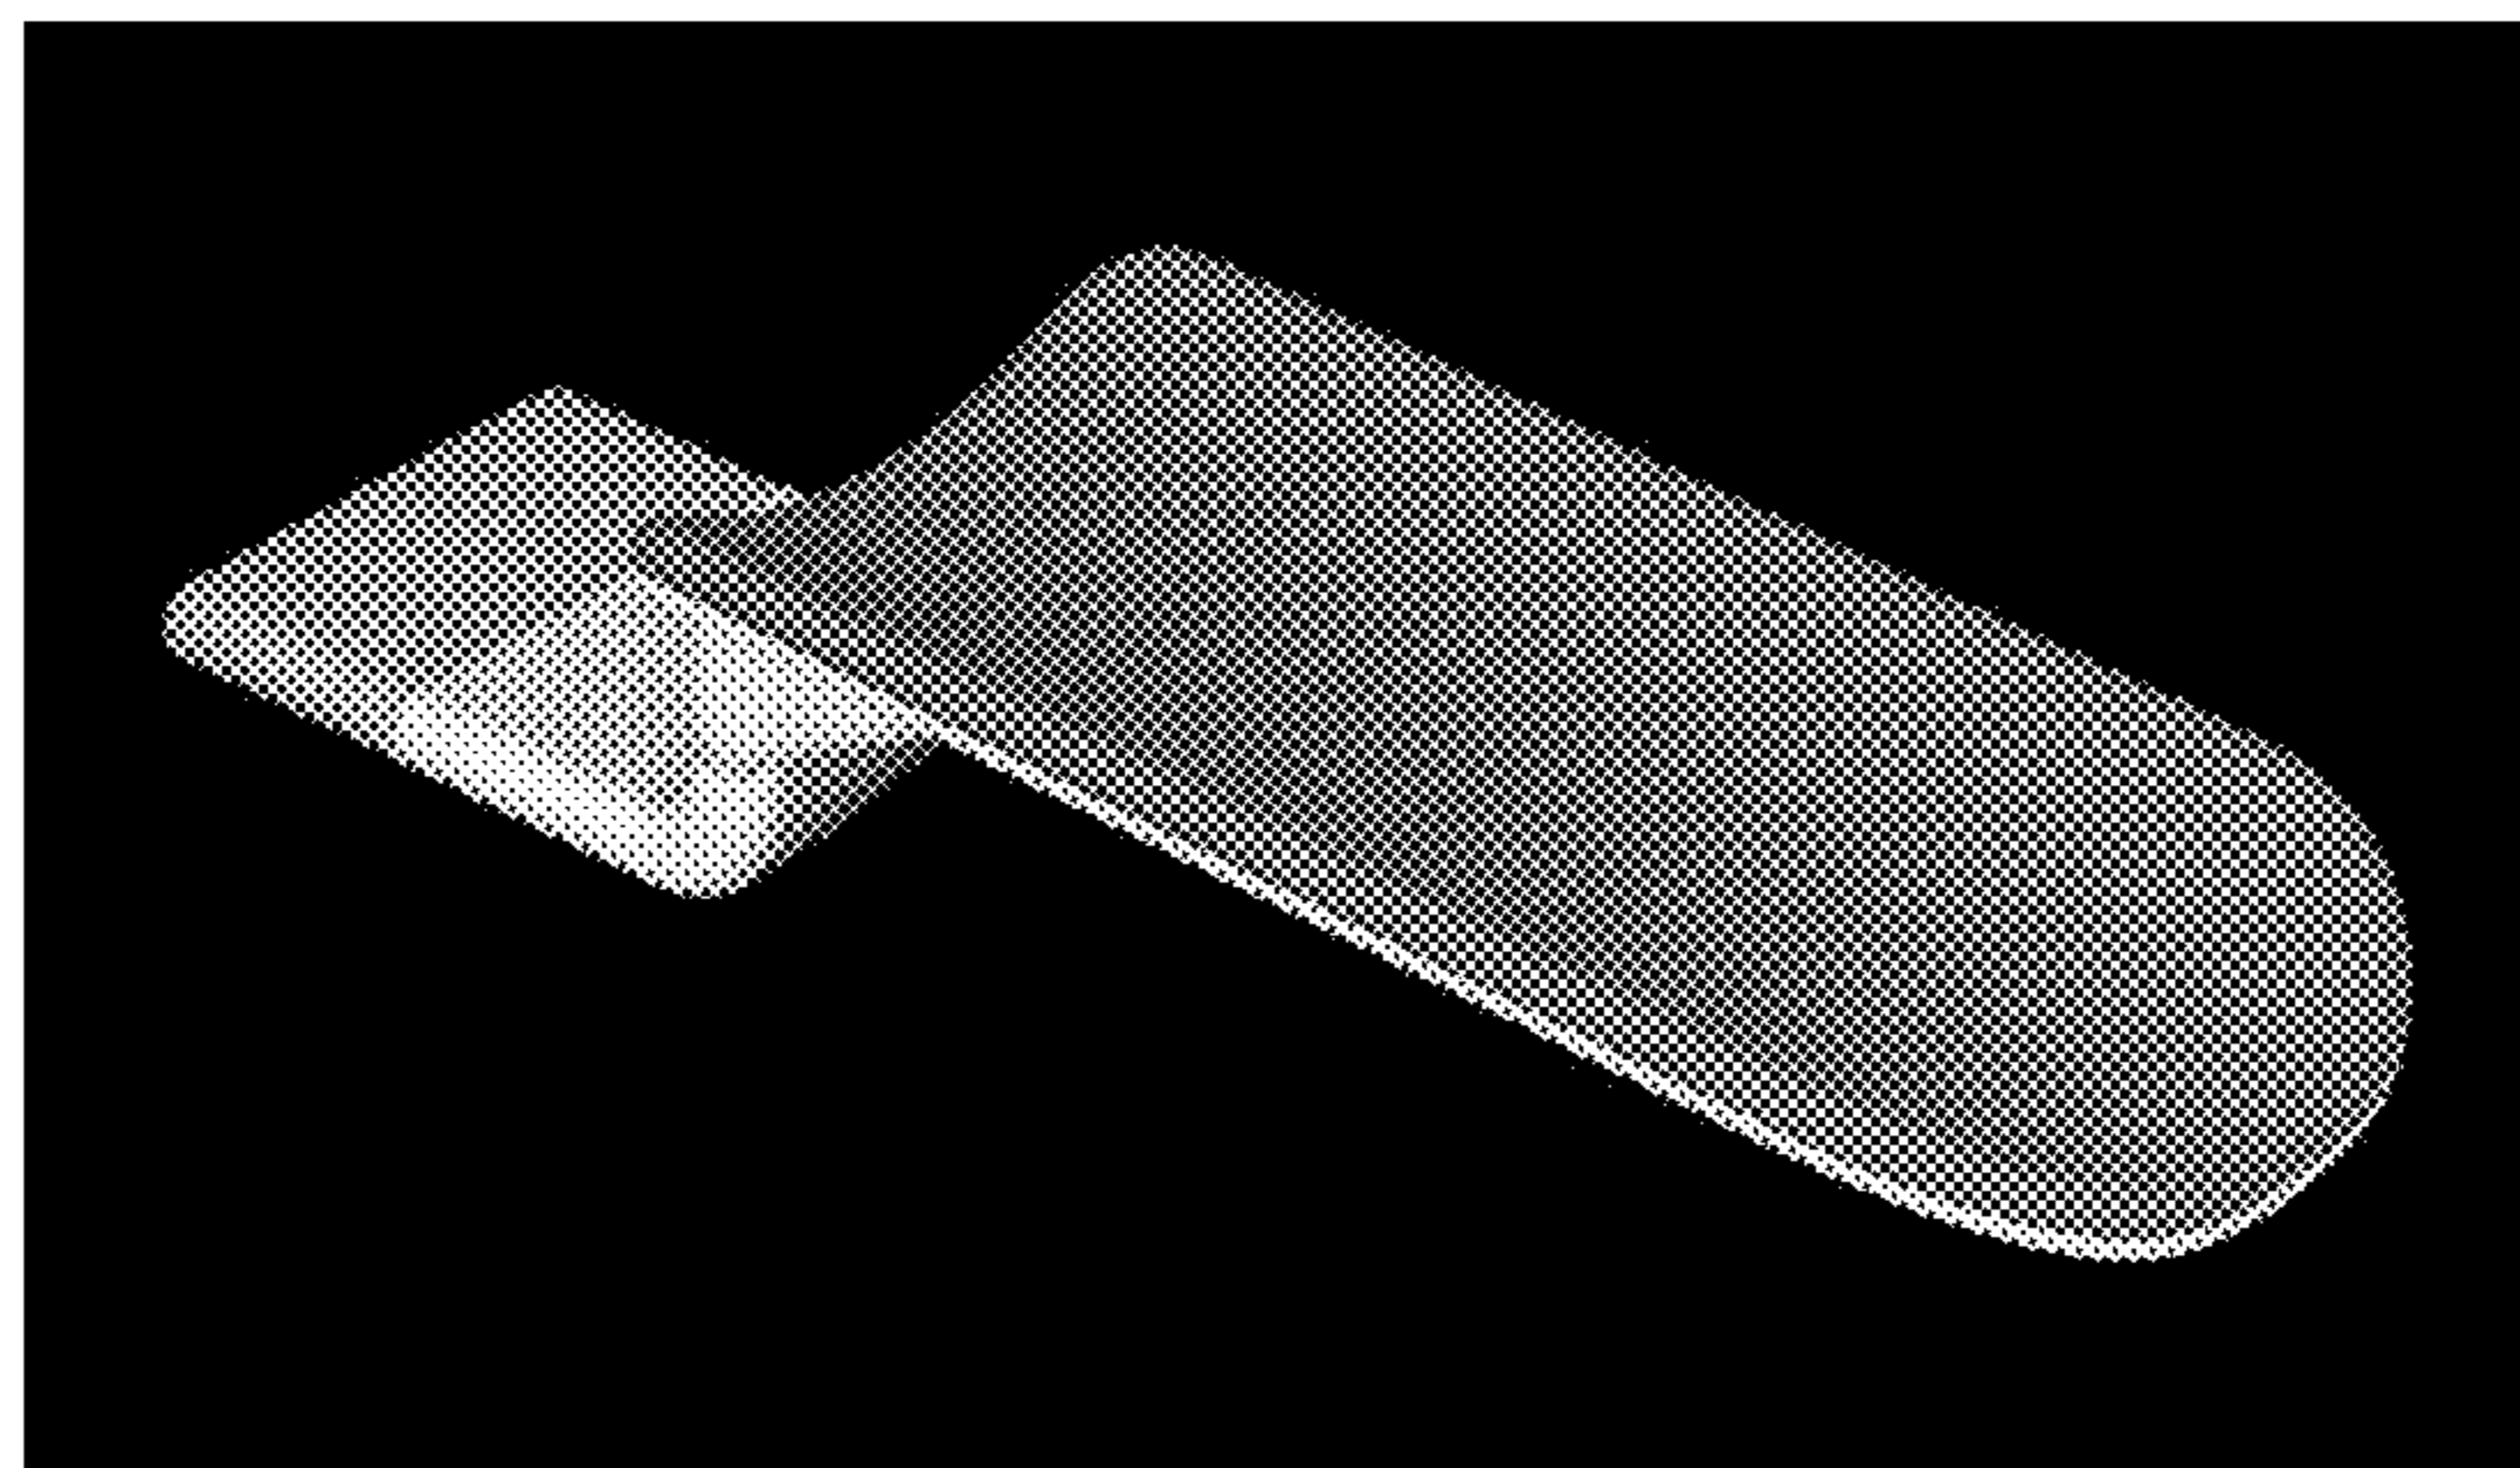

# US D608,446 S

Page 2

---

## U.S. PATENT DOCUMENTS

D518,894 S \* 4/2006 Kirn ..... D24/184  
D530,012 S 10/2006 Eda et al.  
7,232,413 B2 6/2007 Hashimoto et al.  
D560,279 S 1/2008 Eda et al.  
D561,339 S 2/2008 Eda et al.  
D569,000 S \* 5/2008 Itonaga et al. .... D24/186

## FOREIGN PATENT DOCUMENTS

JP 1200780 4/2004

JP 1216857 9/2004  
JP 1284981 10/2006

## OTHER PUBLICATIONS

Terumo Corporation, Brochure, Terumo Corporation, "Arm in® Plus", Electronic Sphygmomanometer, ES-P2000U, published Aug., 2005.

\* cited by examiner

Fig. 1

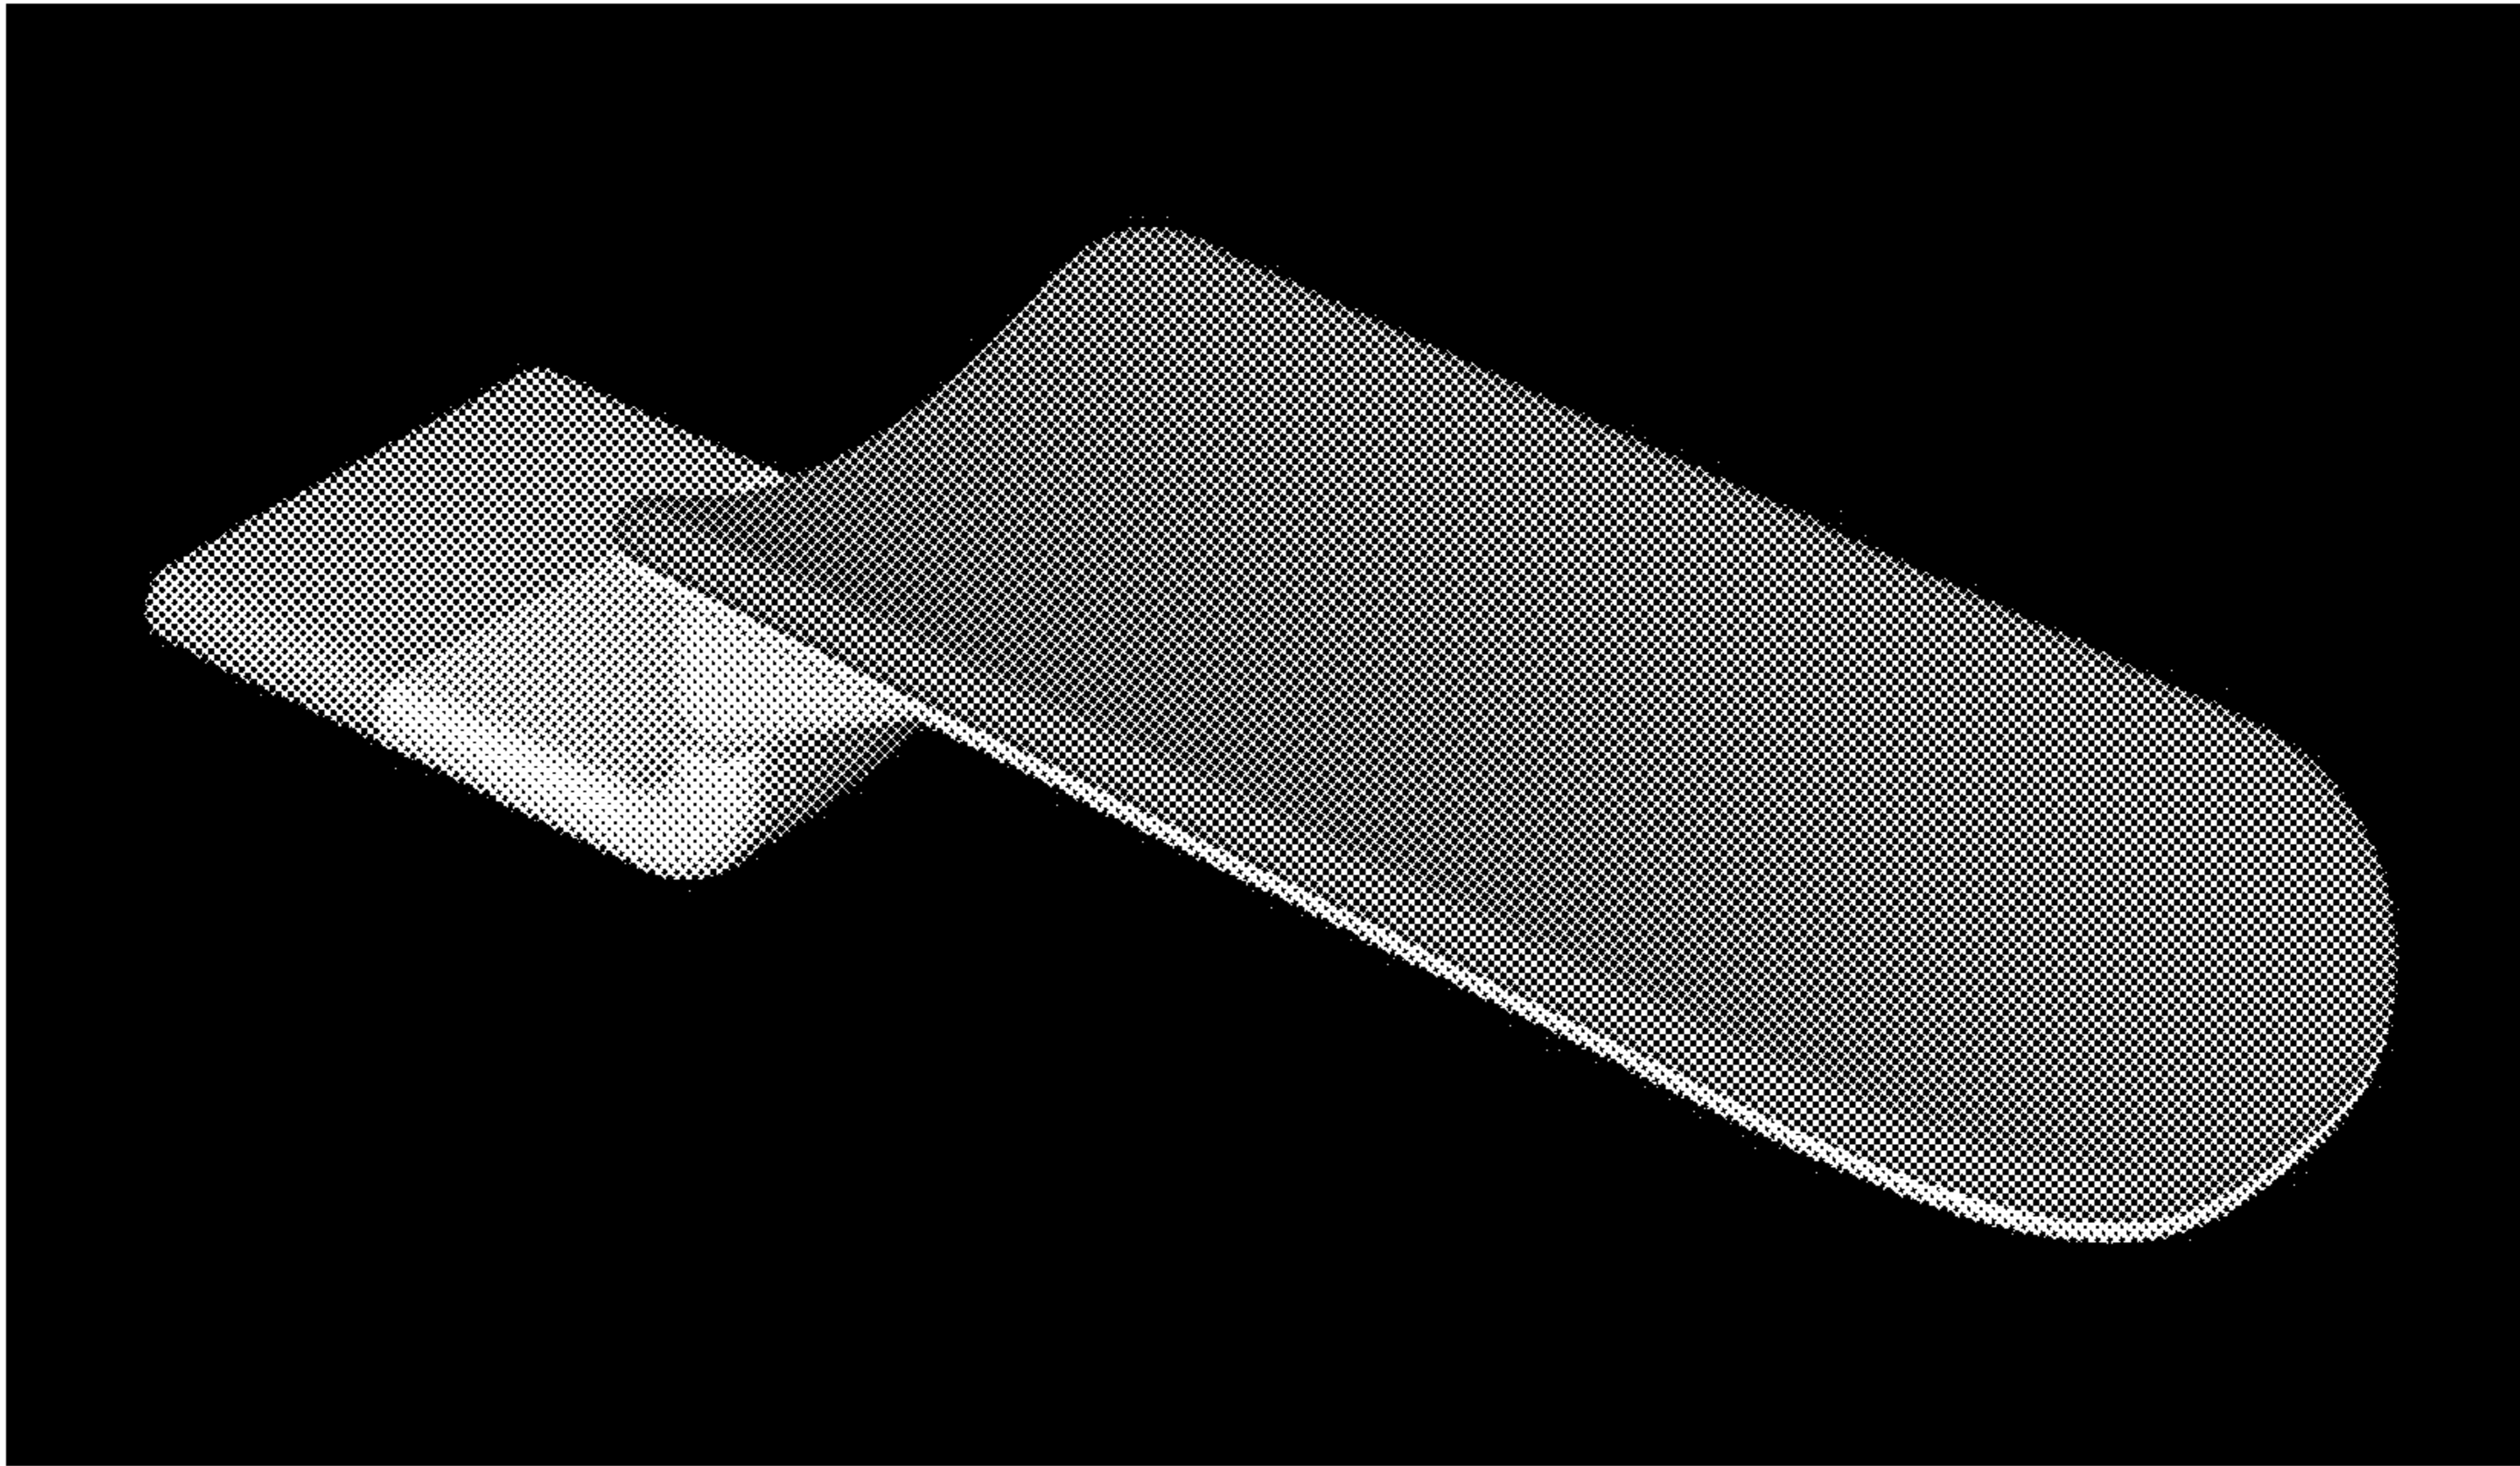


Fig. 2

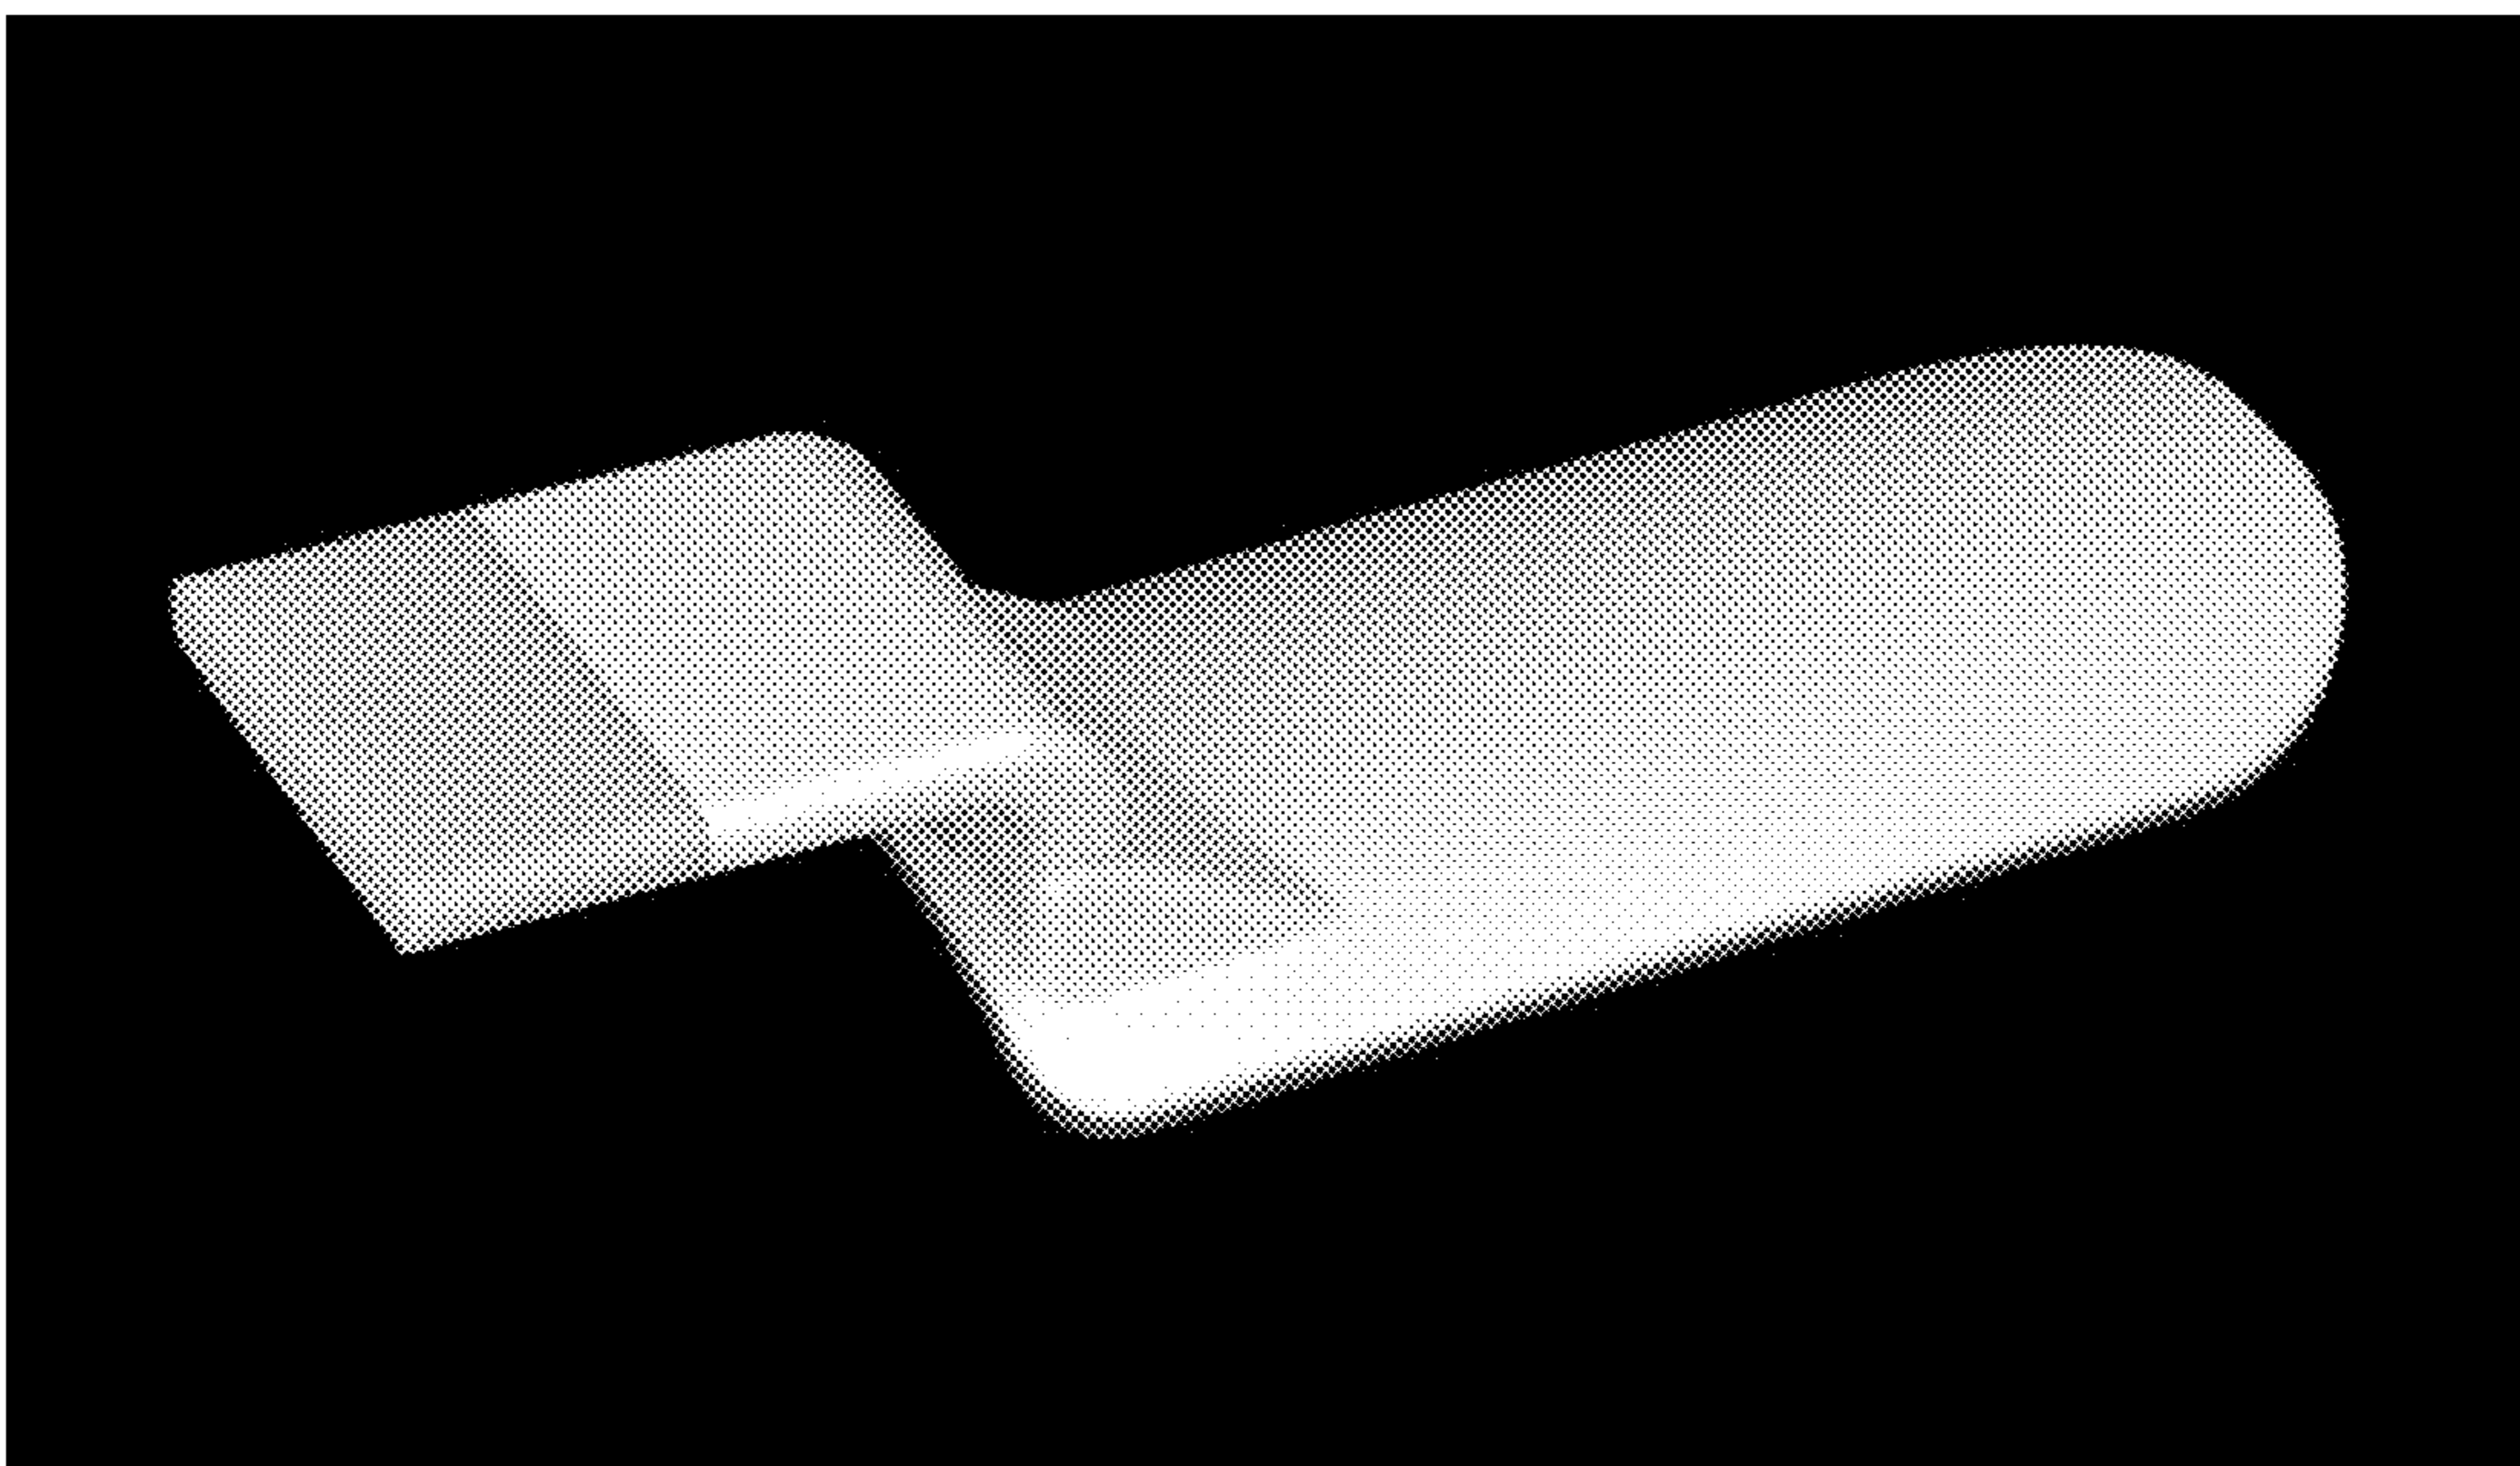




Fig. 3

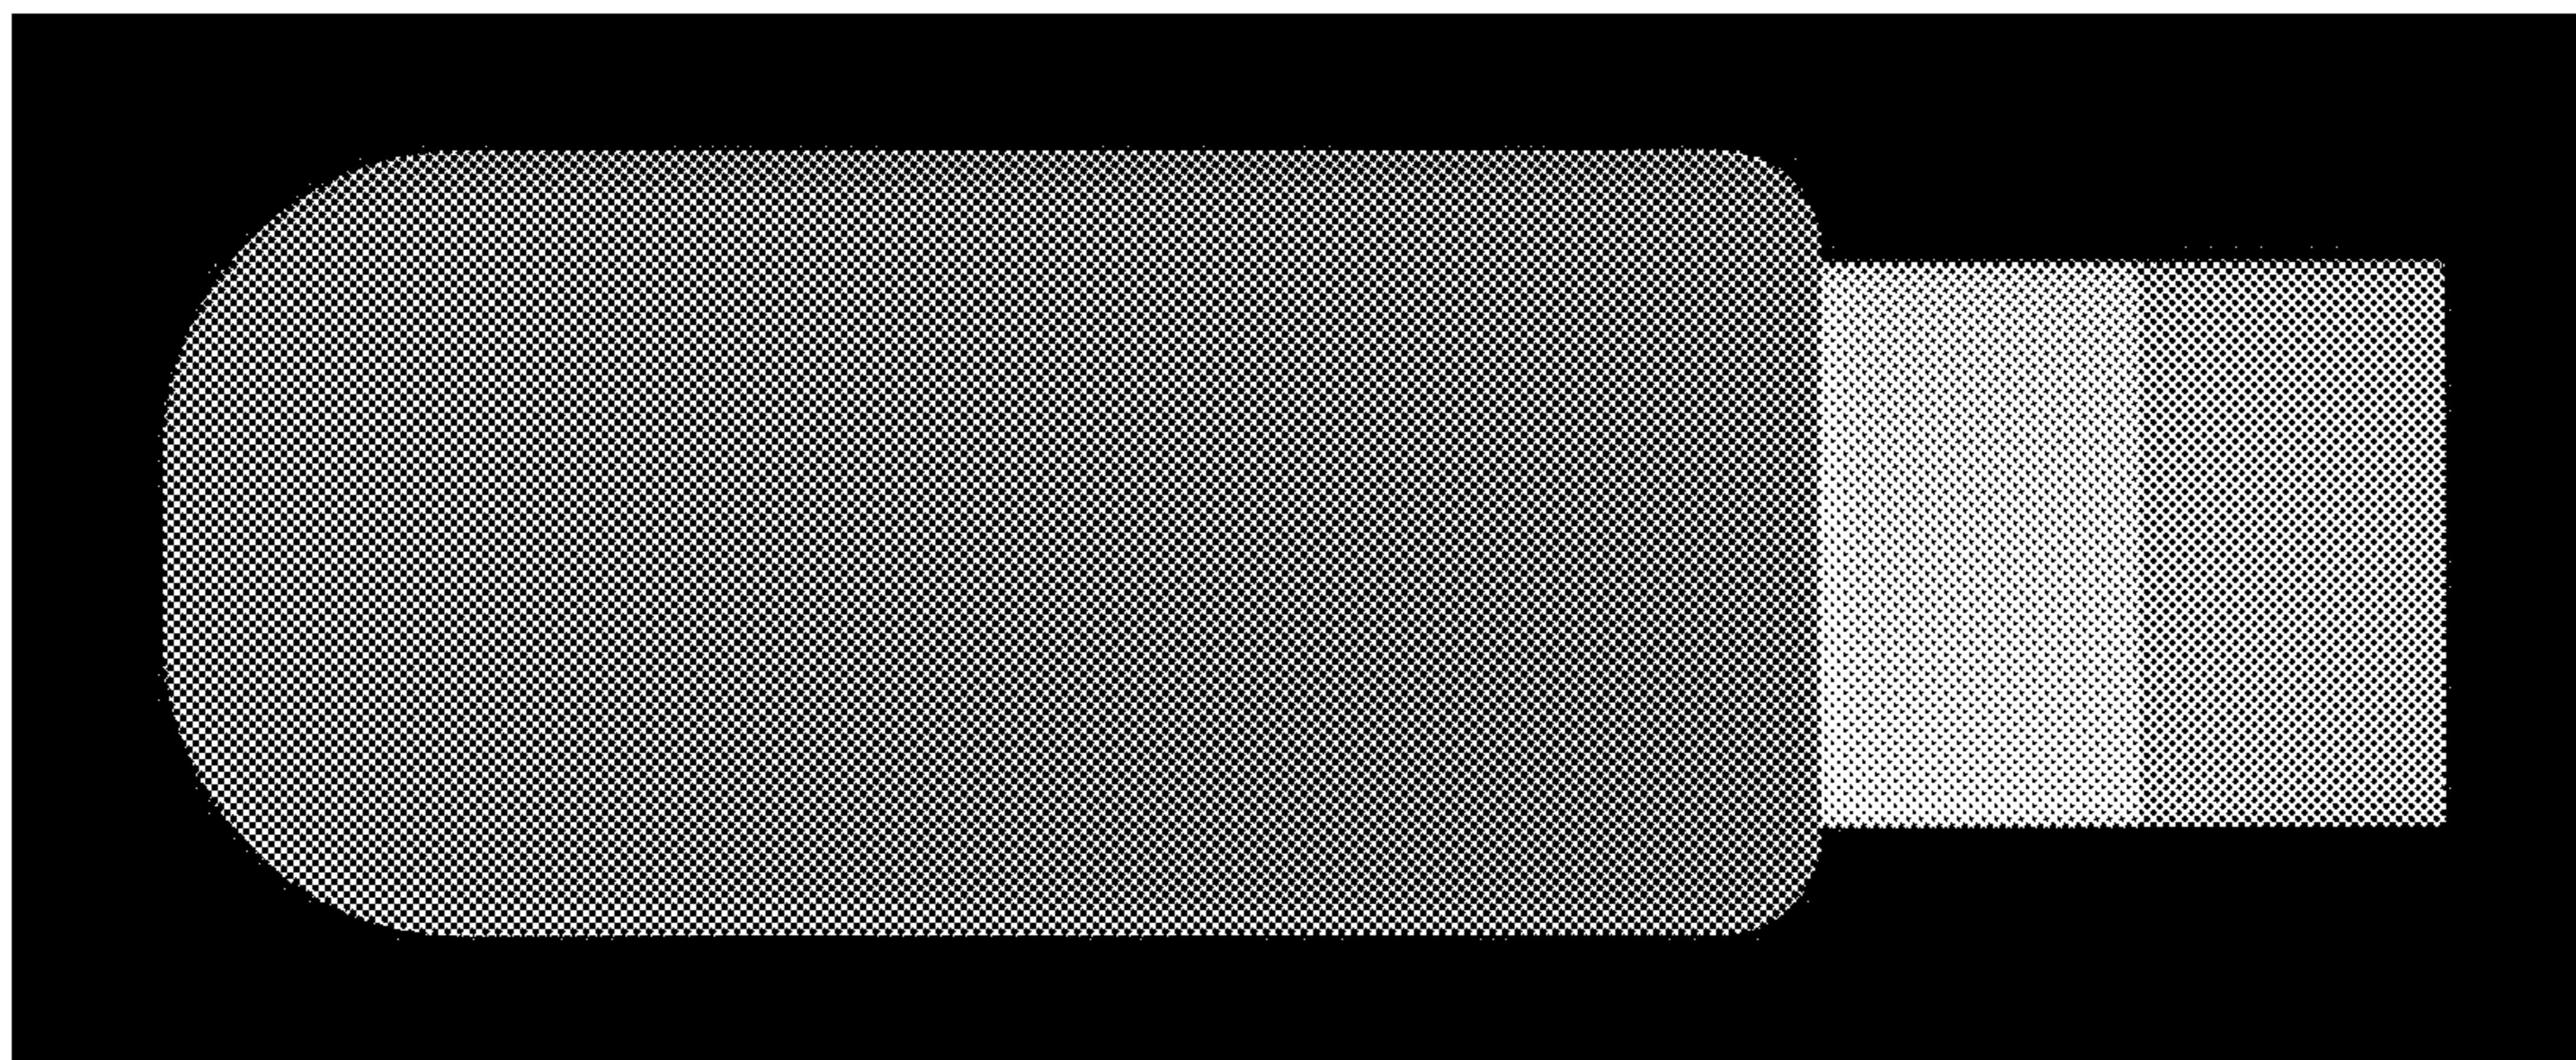


Fig. 4

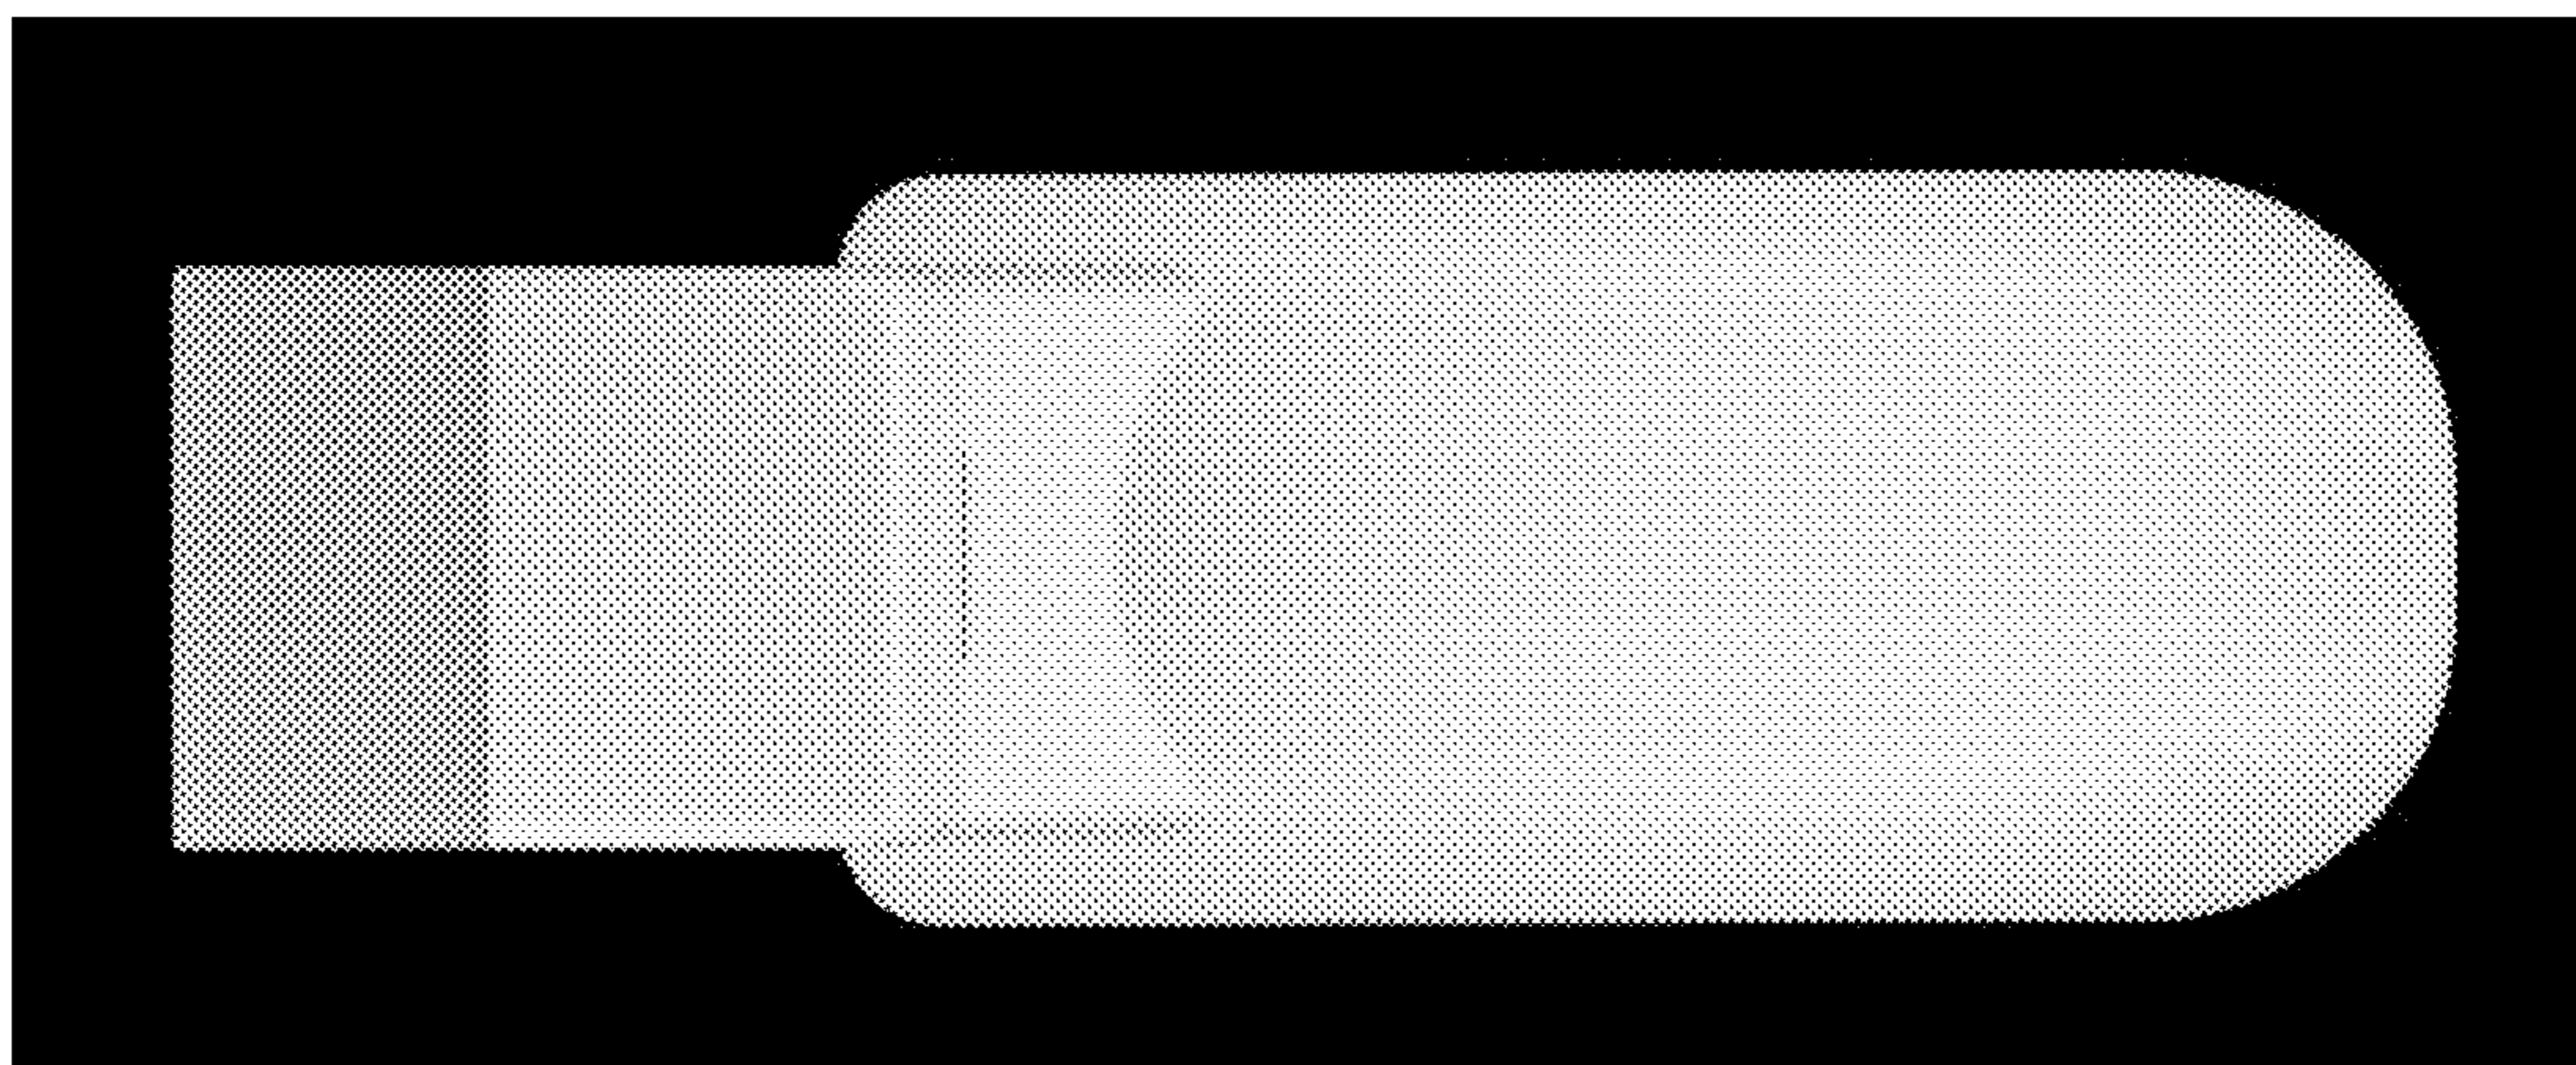


Fig. 5

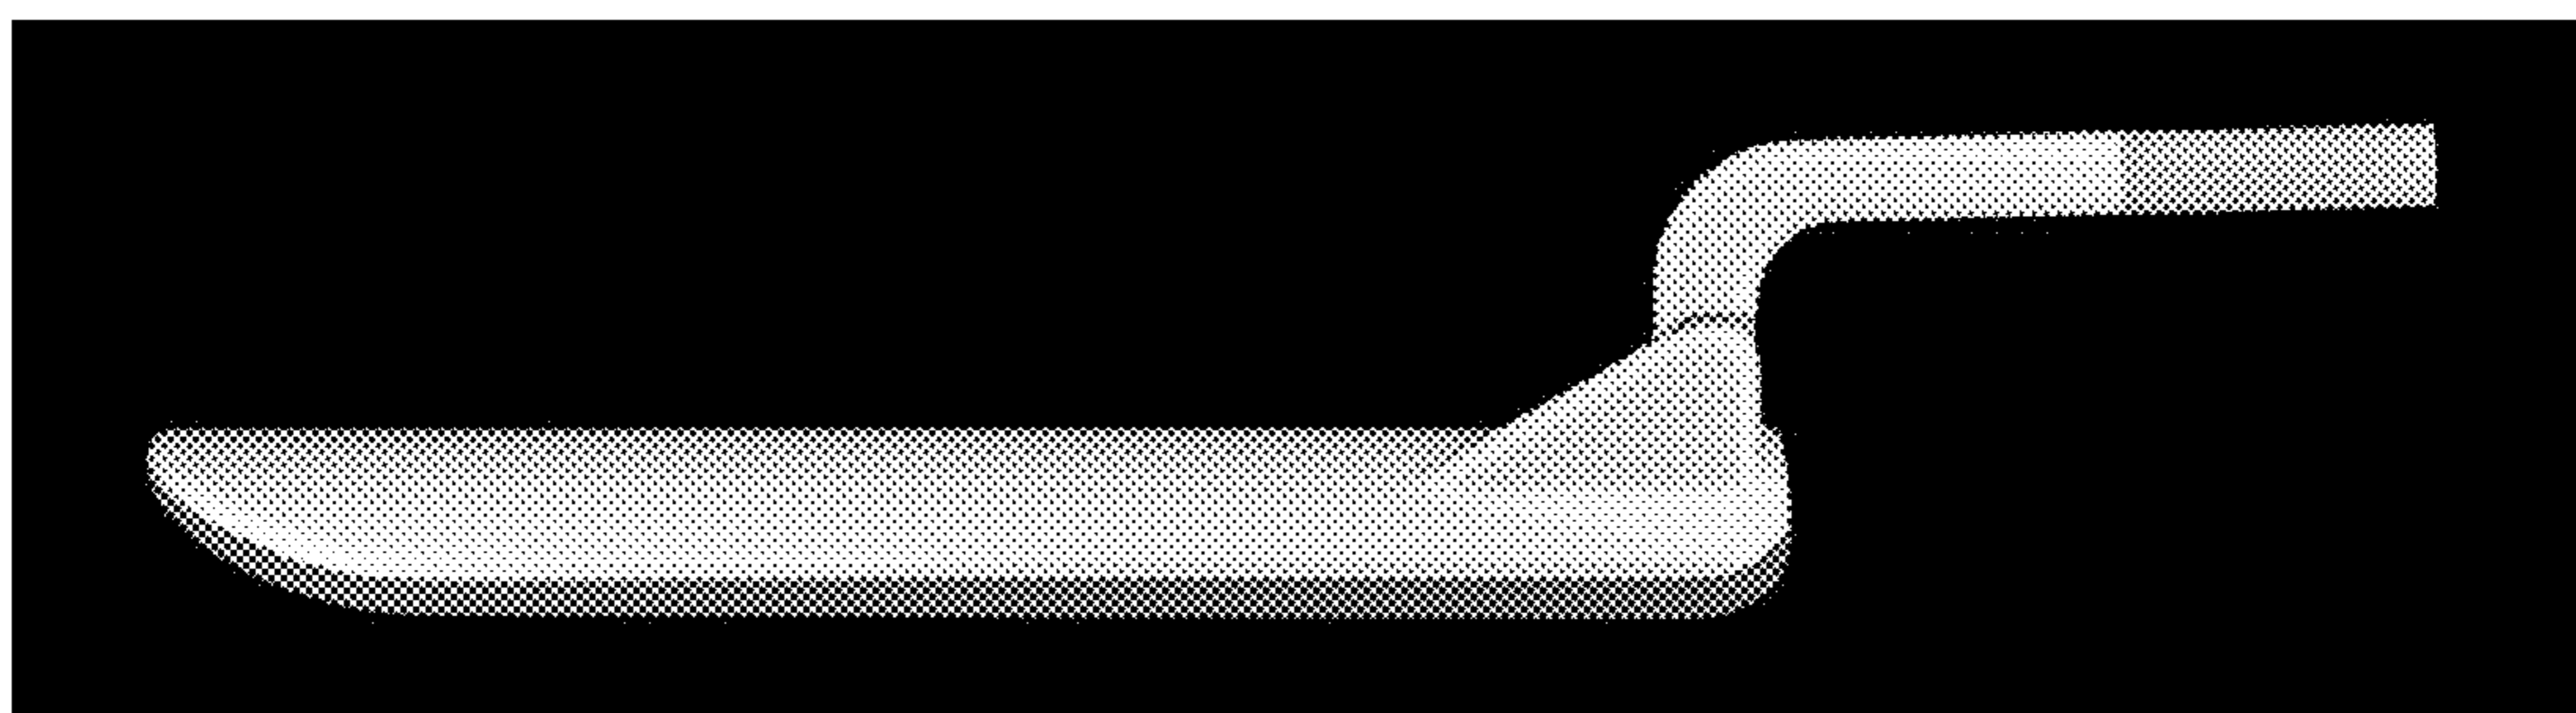


Fig. 6

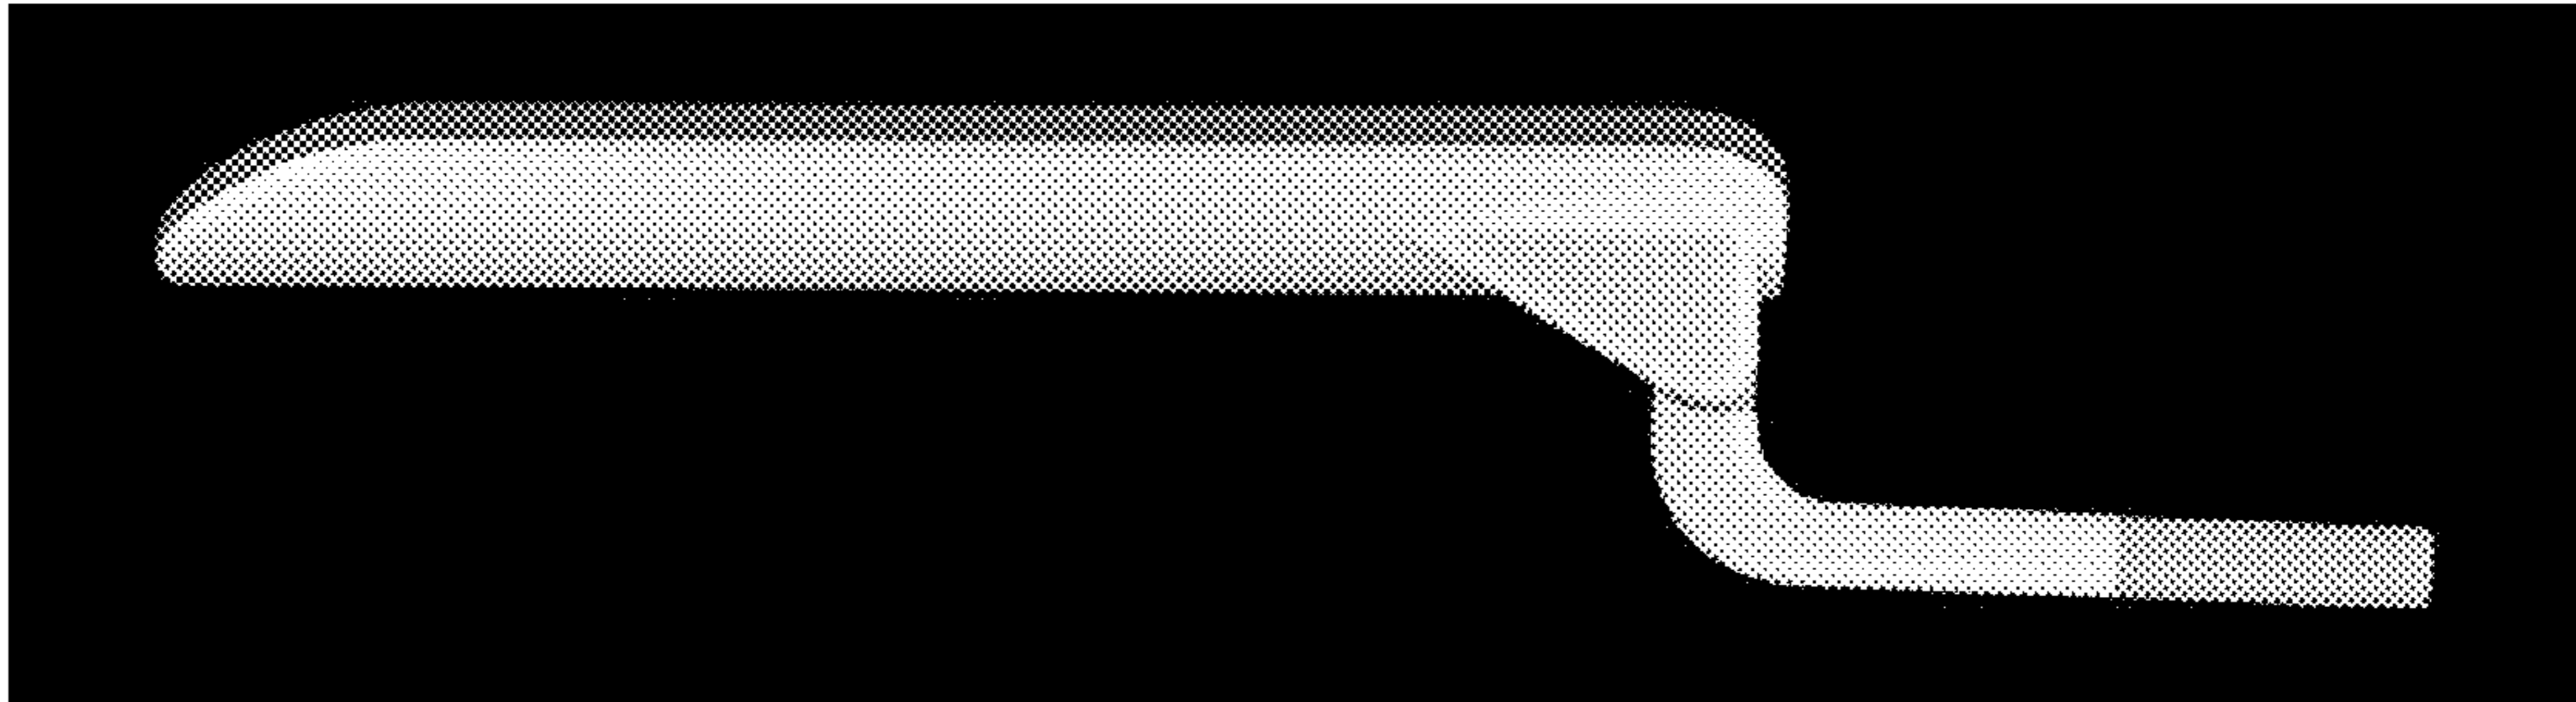


Fig. 7

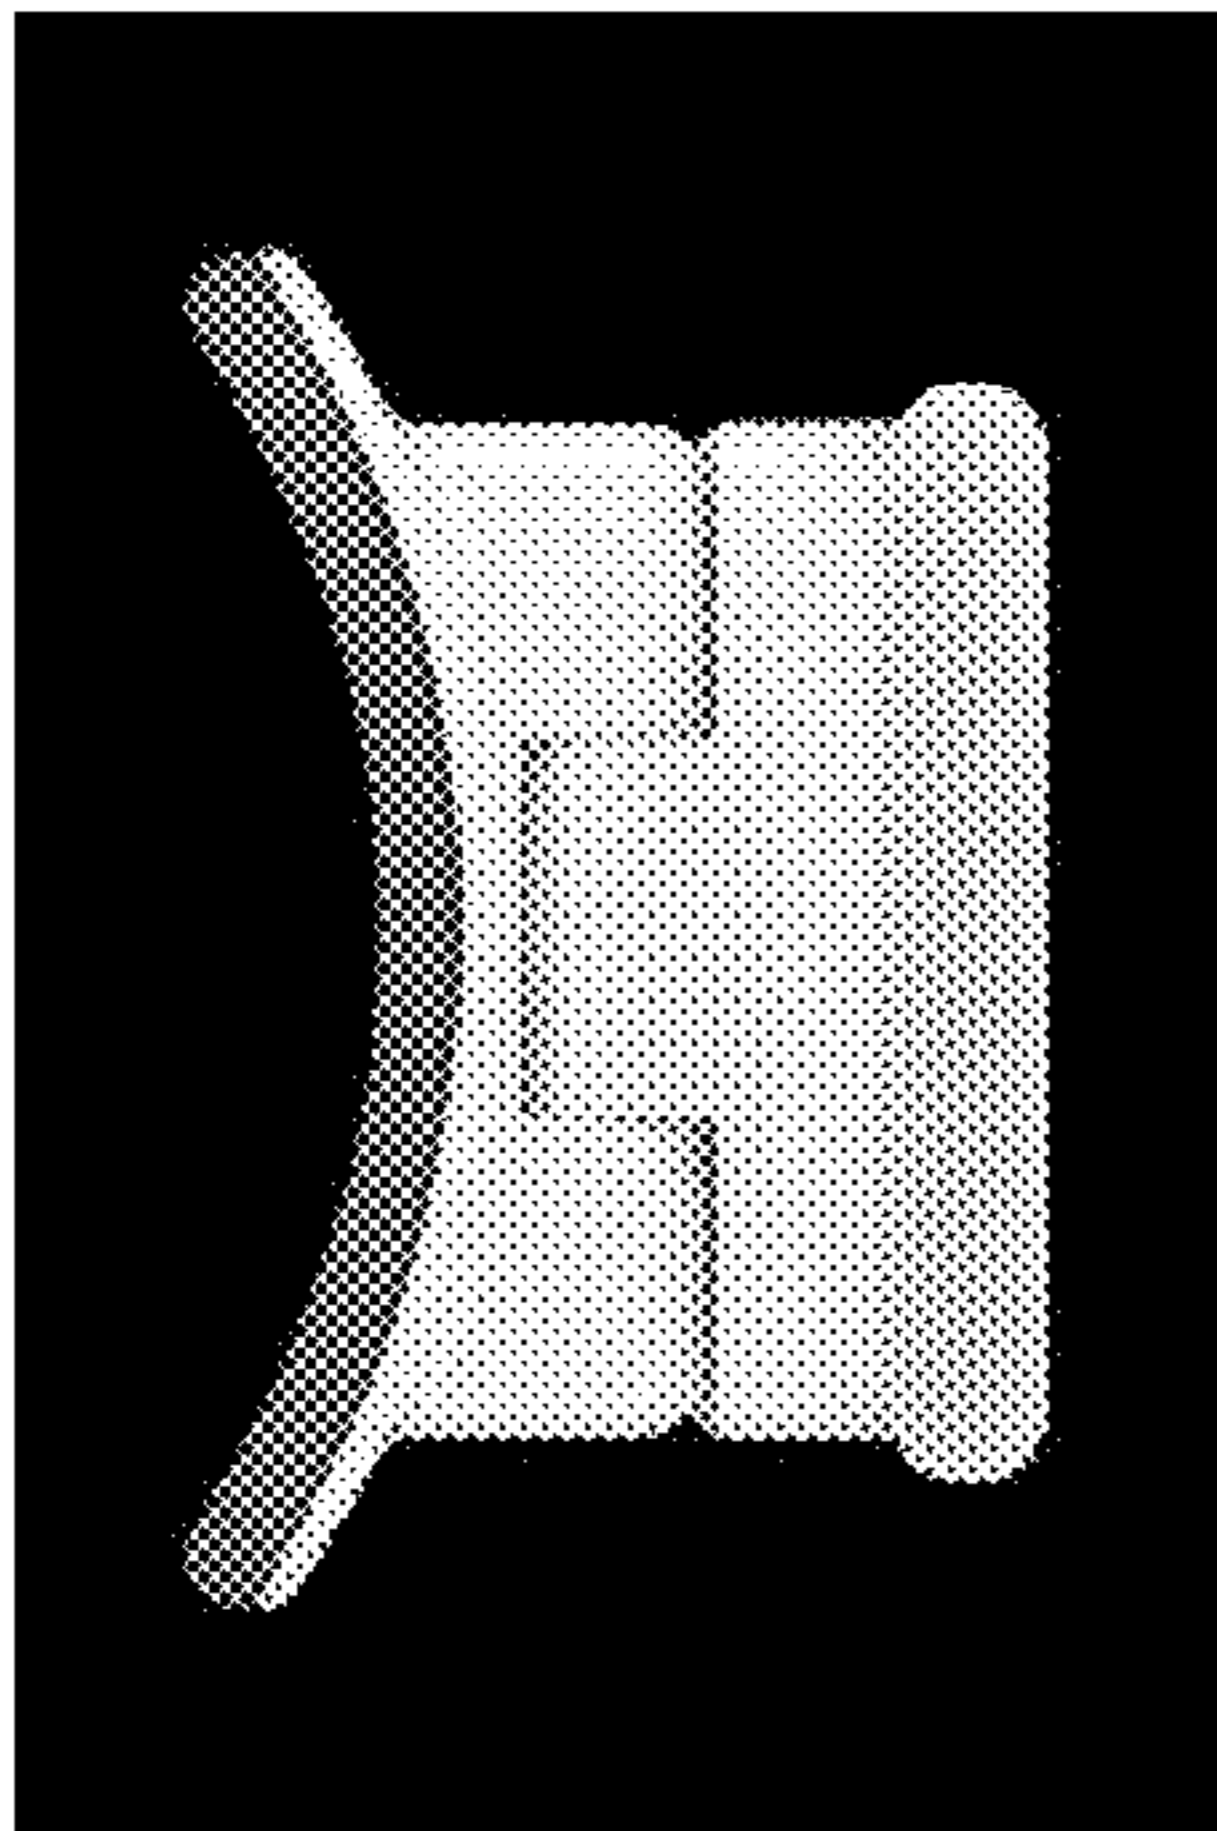


Fig. 8

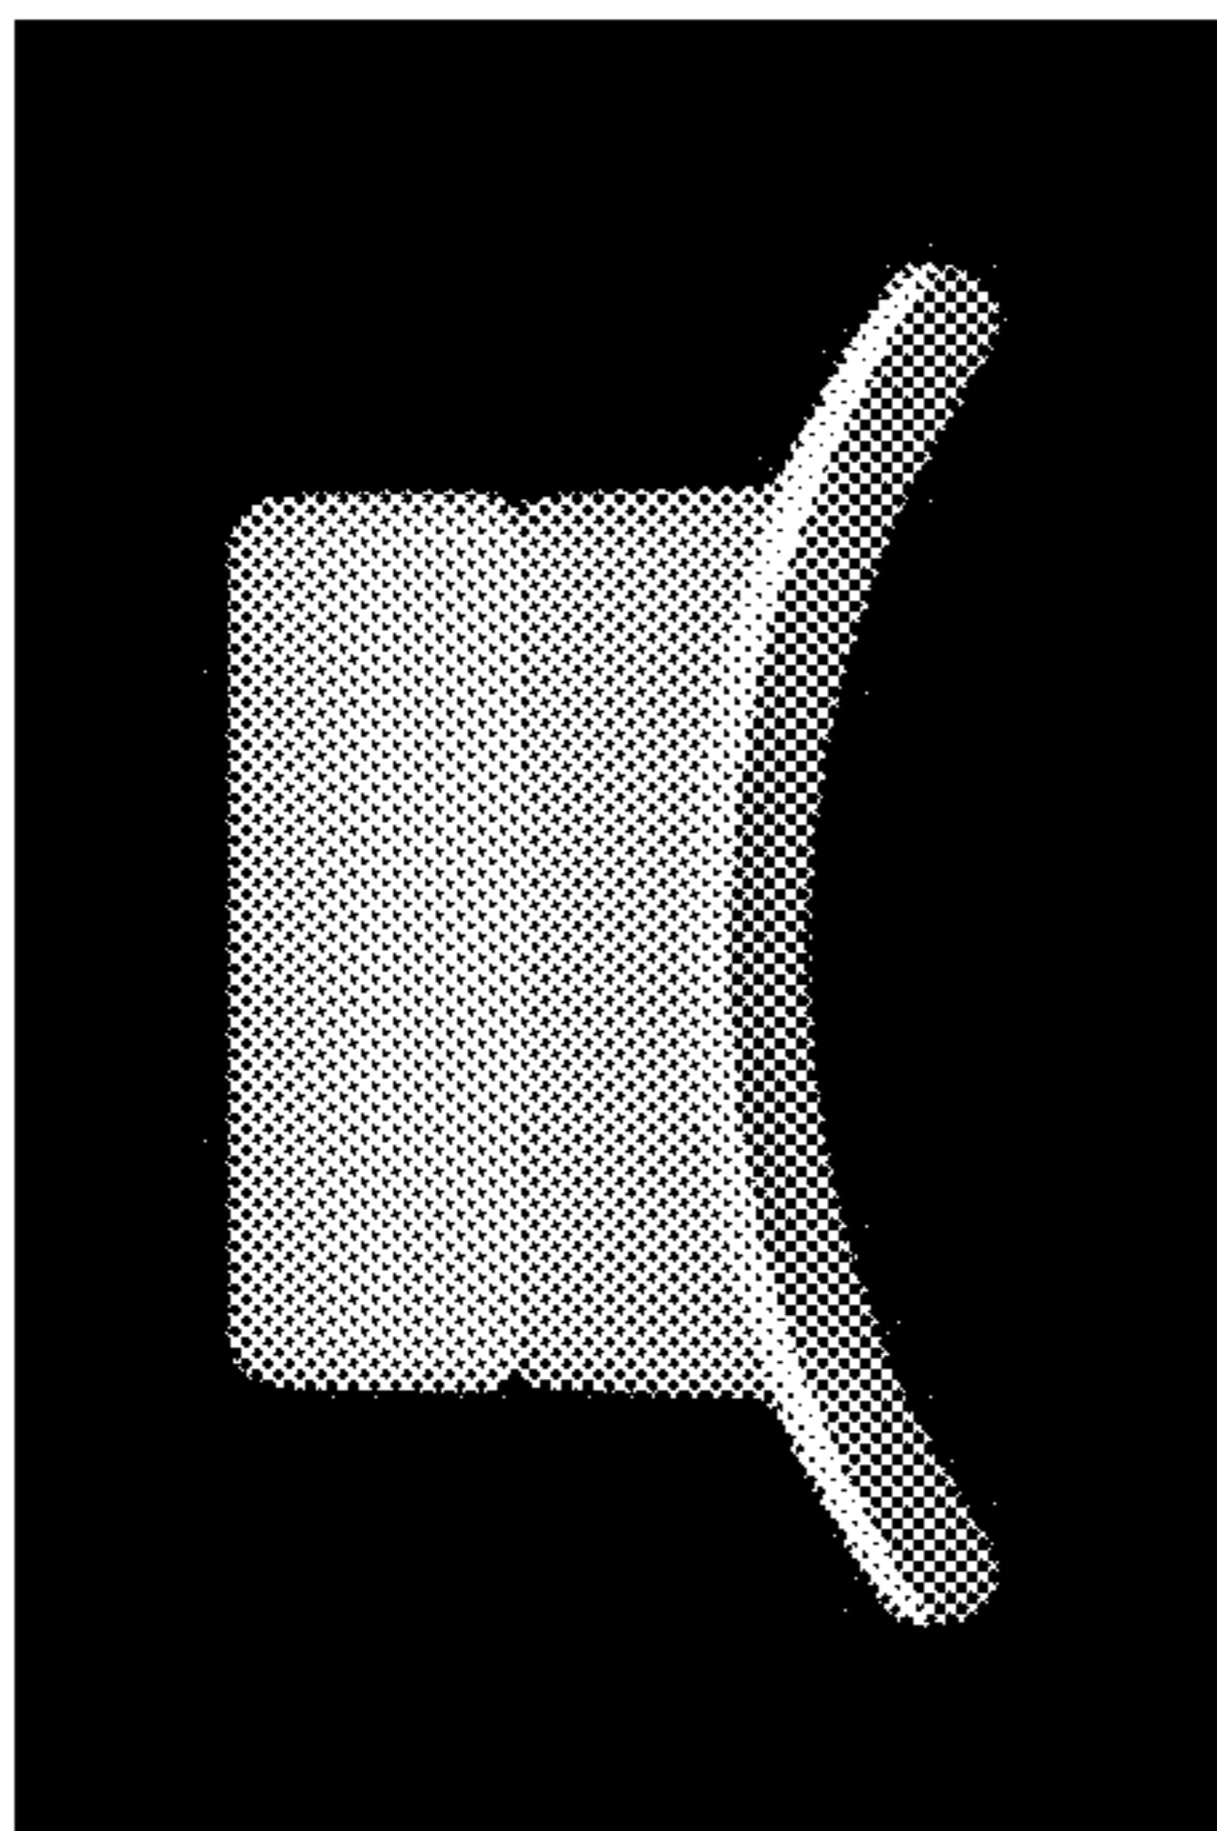




Fig. 9

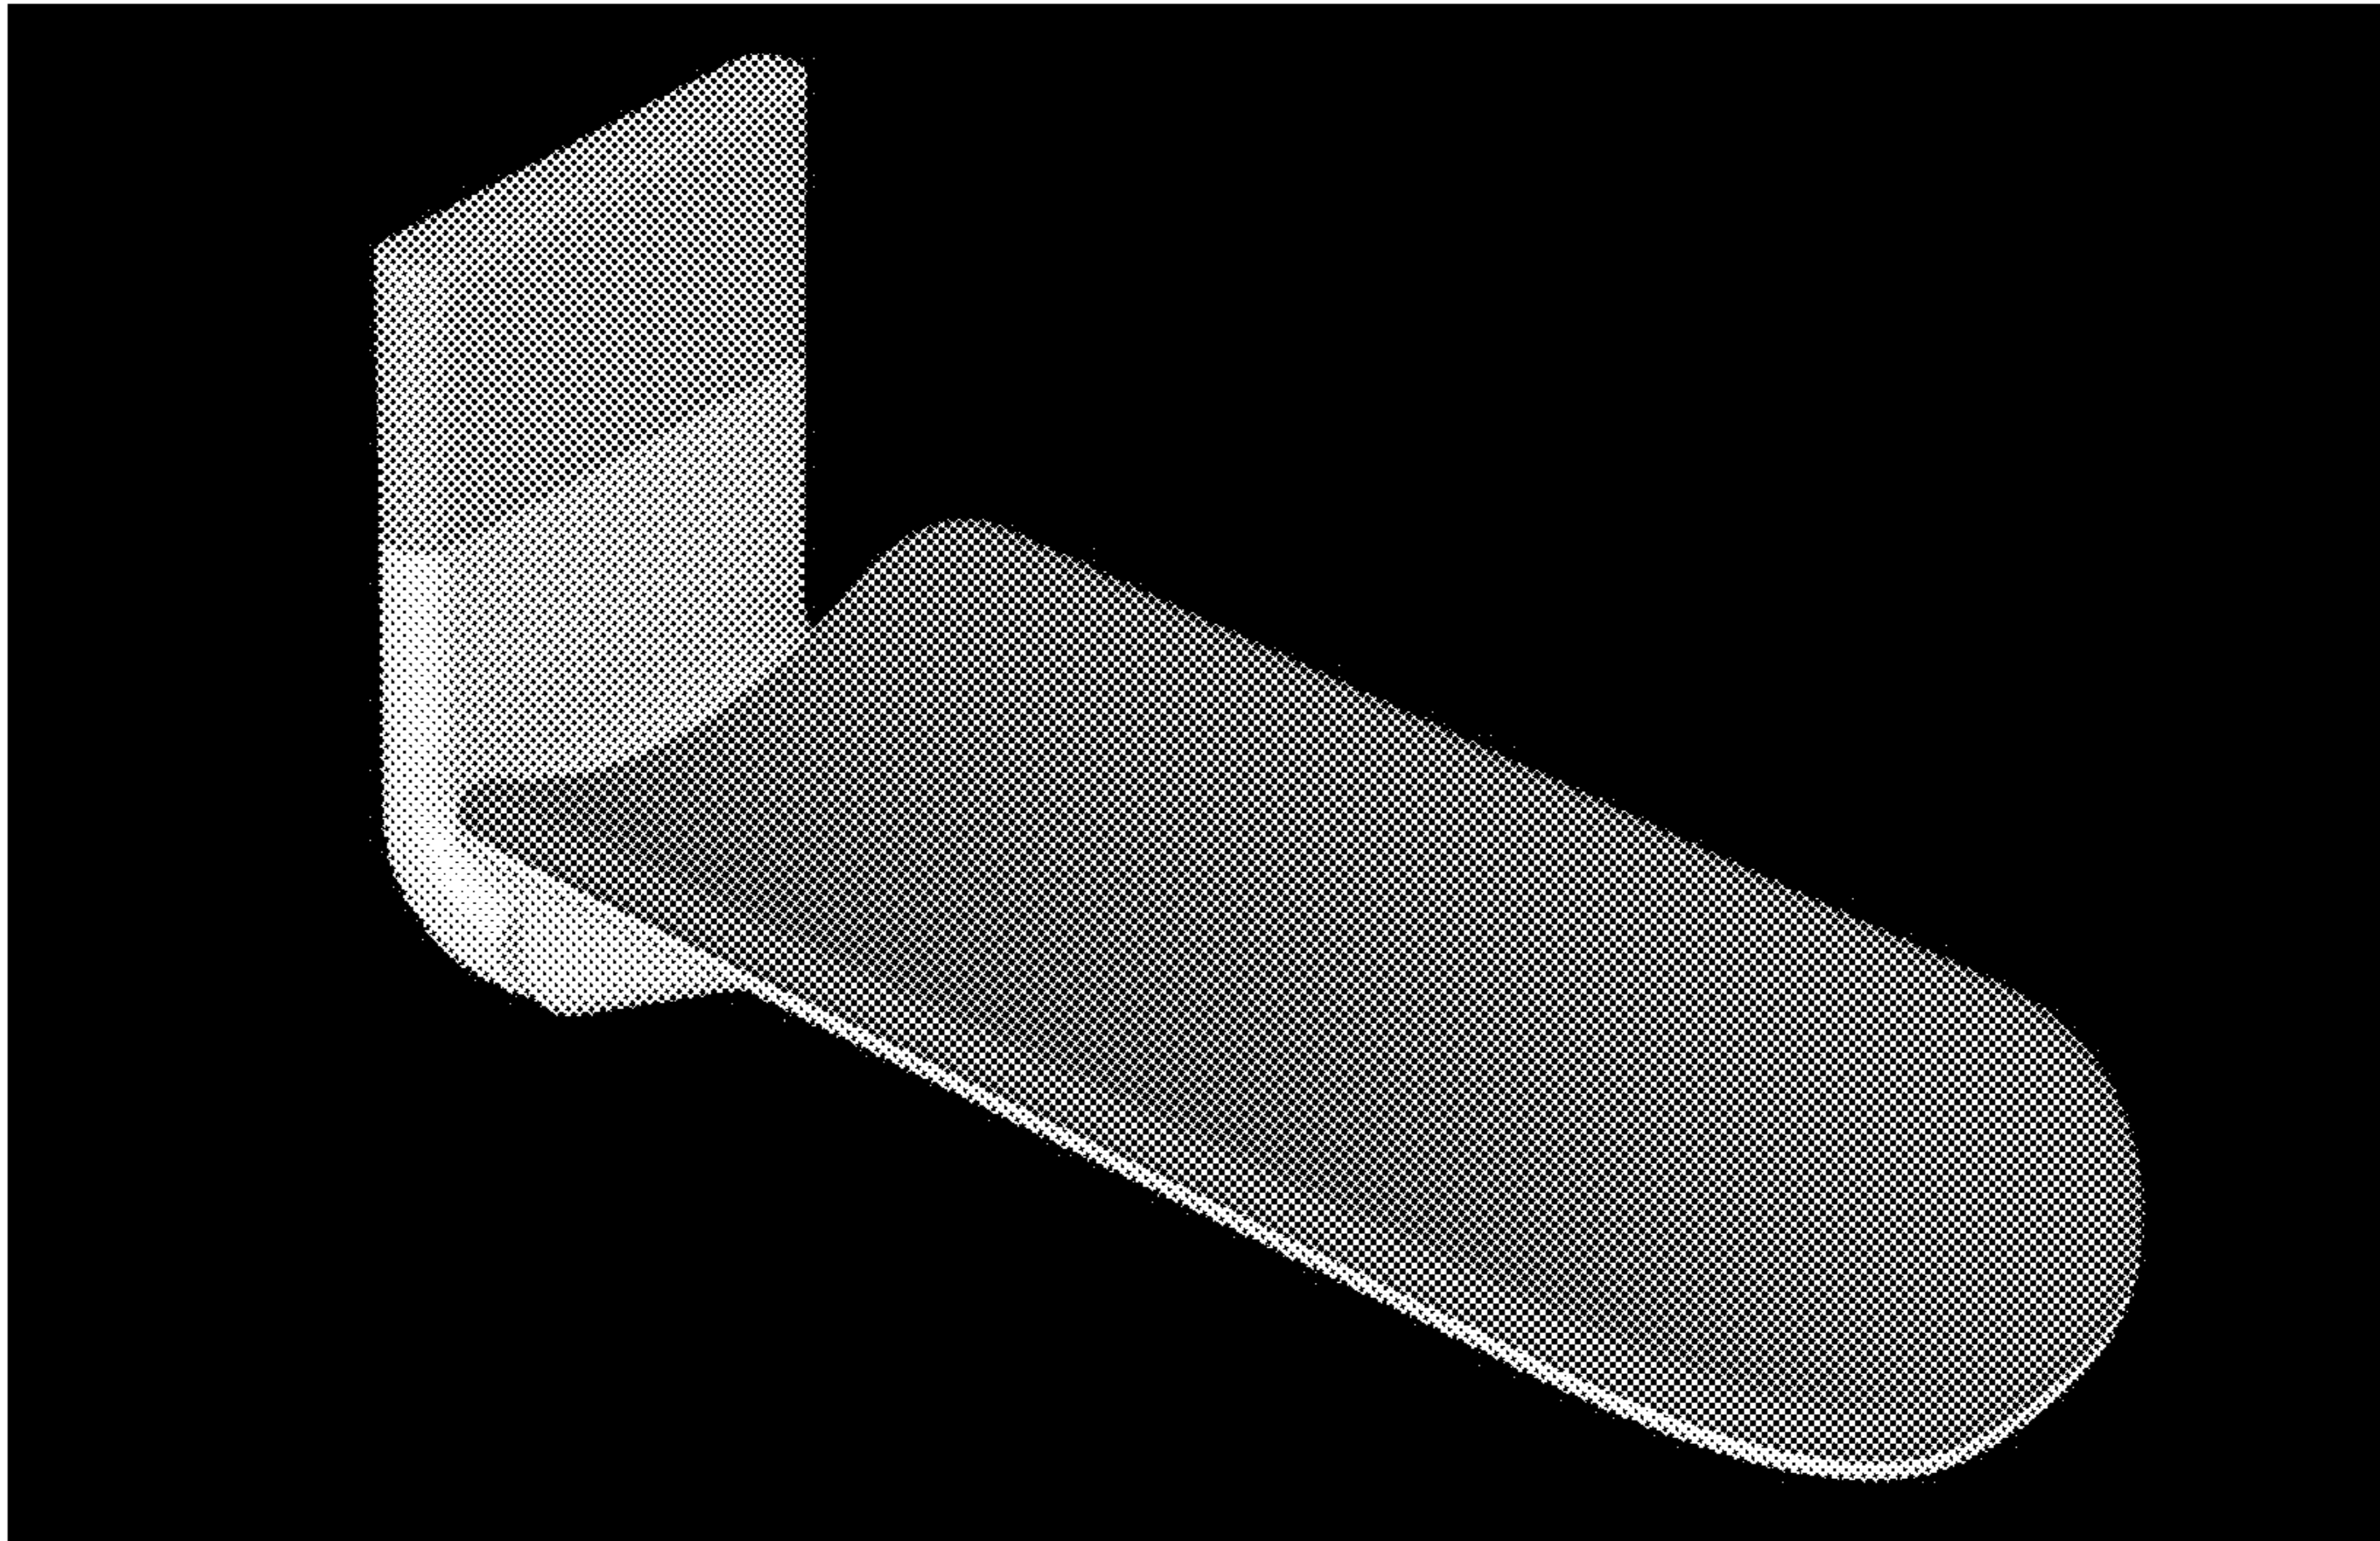


Fig. 10

