



US00D608892S

(12) **United States Design Patent**
Takano et al.

(10) **Patent No.:** **US D608,892 S**
(45) **Date of Patent:** **** Jan. 26, 2010**

(54) **GLUCOSE METER**

(75) Inventors: **Hiroshi Takano**, Toon (JP); **Masakazu Mori**, Toon (JP); **Michael Woolsey**, Tarrytown, NY (US); **Derek Lok**, Tarrytown, NY (US); **Gerald Shaffer**, Tarrytown, NY (US)

(73) Assignees: **Panasonic Corporation**, Kadoma-shi (JP); **Bayer Healthcare LLC**, Tarrytown, NY (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/327,937**

(22) Filed: **Nov. 14, 2008**

Related U.S. Application Data

(62) Division of application No. 29/280,788, filed on Jun. 7, 2007, now Pat. No. Des. 587,376.

(30) **Foreign Application Priority Data**

Dec. 7, 2006 (JP) 2006-033770
Dec. 7, 2006 (JP) 2006-033773

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Classification Search** D24/165-169,
D24/186; D10/78, 81; 600/309, 316, 322,
600/365, 368; 422/58, 61, 68.1

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D369,216 S 4/1996 Micinski
D369,864 S 5/1996 Petersen
D371,198 S 6/1996 Savage
D371,440 S 7/1996 Petersen
5,605,837 A 2/1997 Karimi
5,989,917 A * 11/1999 McAleer et al. 436/46
D424,696 S * 5/2000 Ray et al. D24/169
D429,527 S 8/2000 Bolam

D440,312 S 4/2001 Bertrand
D452,564 S 12/2001 Micinski
D456,514 S 4/2002 Brown
D460,823 S 7/2002 Steinberg
6,458,326 B1 10/2002 Modzelewski
D468,714 S 1/2003 Maruska
D469,107 S 1/2003 Miller
D472,834 S 4/2003 Ueda
D473,310 S 4/2003 Schlagheck
D484,600 S 12/2003 Kaar
D495,418 S 8/2004 Rounds
D496,461 S 9/2004 Neel
D502,654 S 3/2005 Nishiura
D522,656 S 6/2006 Orr

(Continued)

FOREIGN PATENT DOCUMENTS

JP 986576 S 8/1997

(Continued)

Primary Examiner—T. Chase Nelson

Assistant Examiner—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Christensen O'Connor Johnson Kindness PLLC

(57) **CLAIM**

The ornamental design for a glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the front, right side and bottom of a glucose meter showing our new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;


FIG. 4 is a left side view thereof;

FIG. 5 is a right side view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom view thereof.

1 Claim, 4 Drawing Sheets

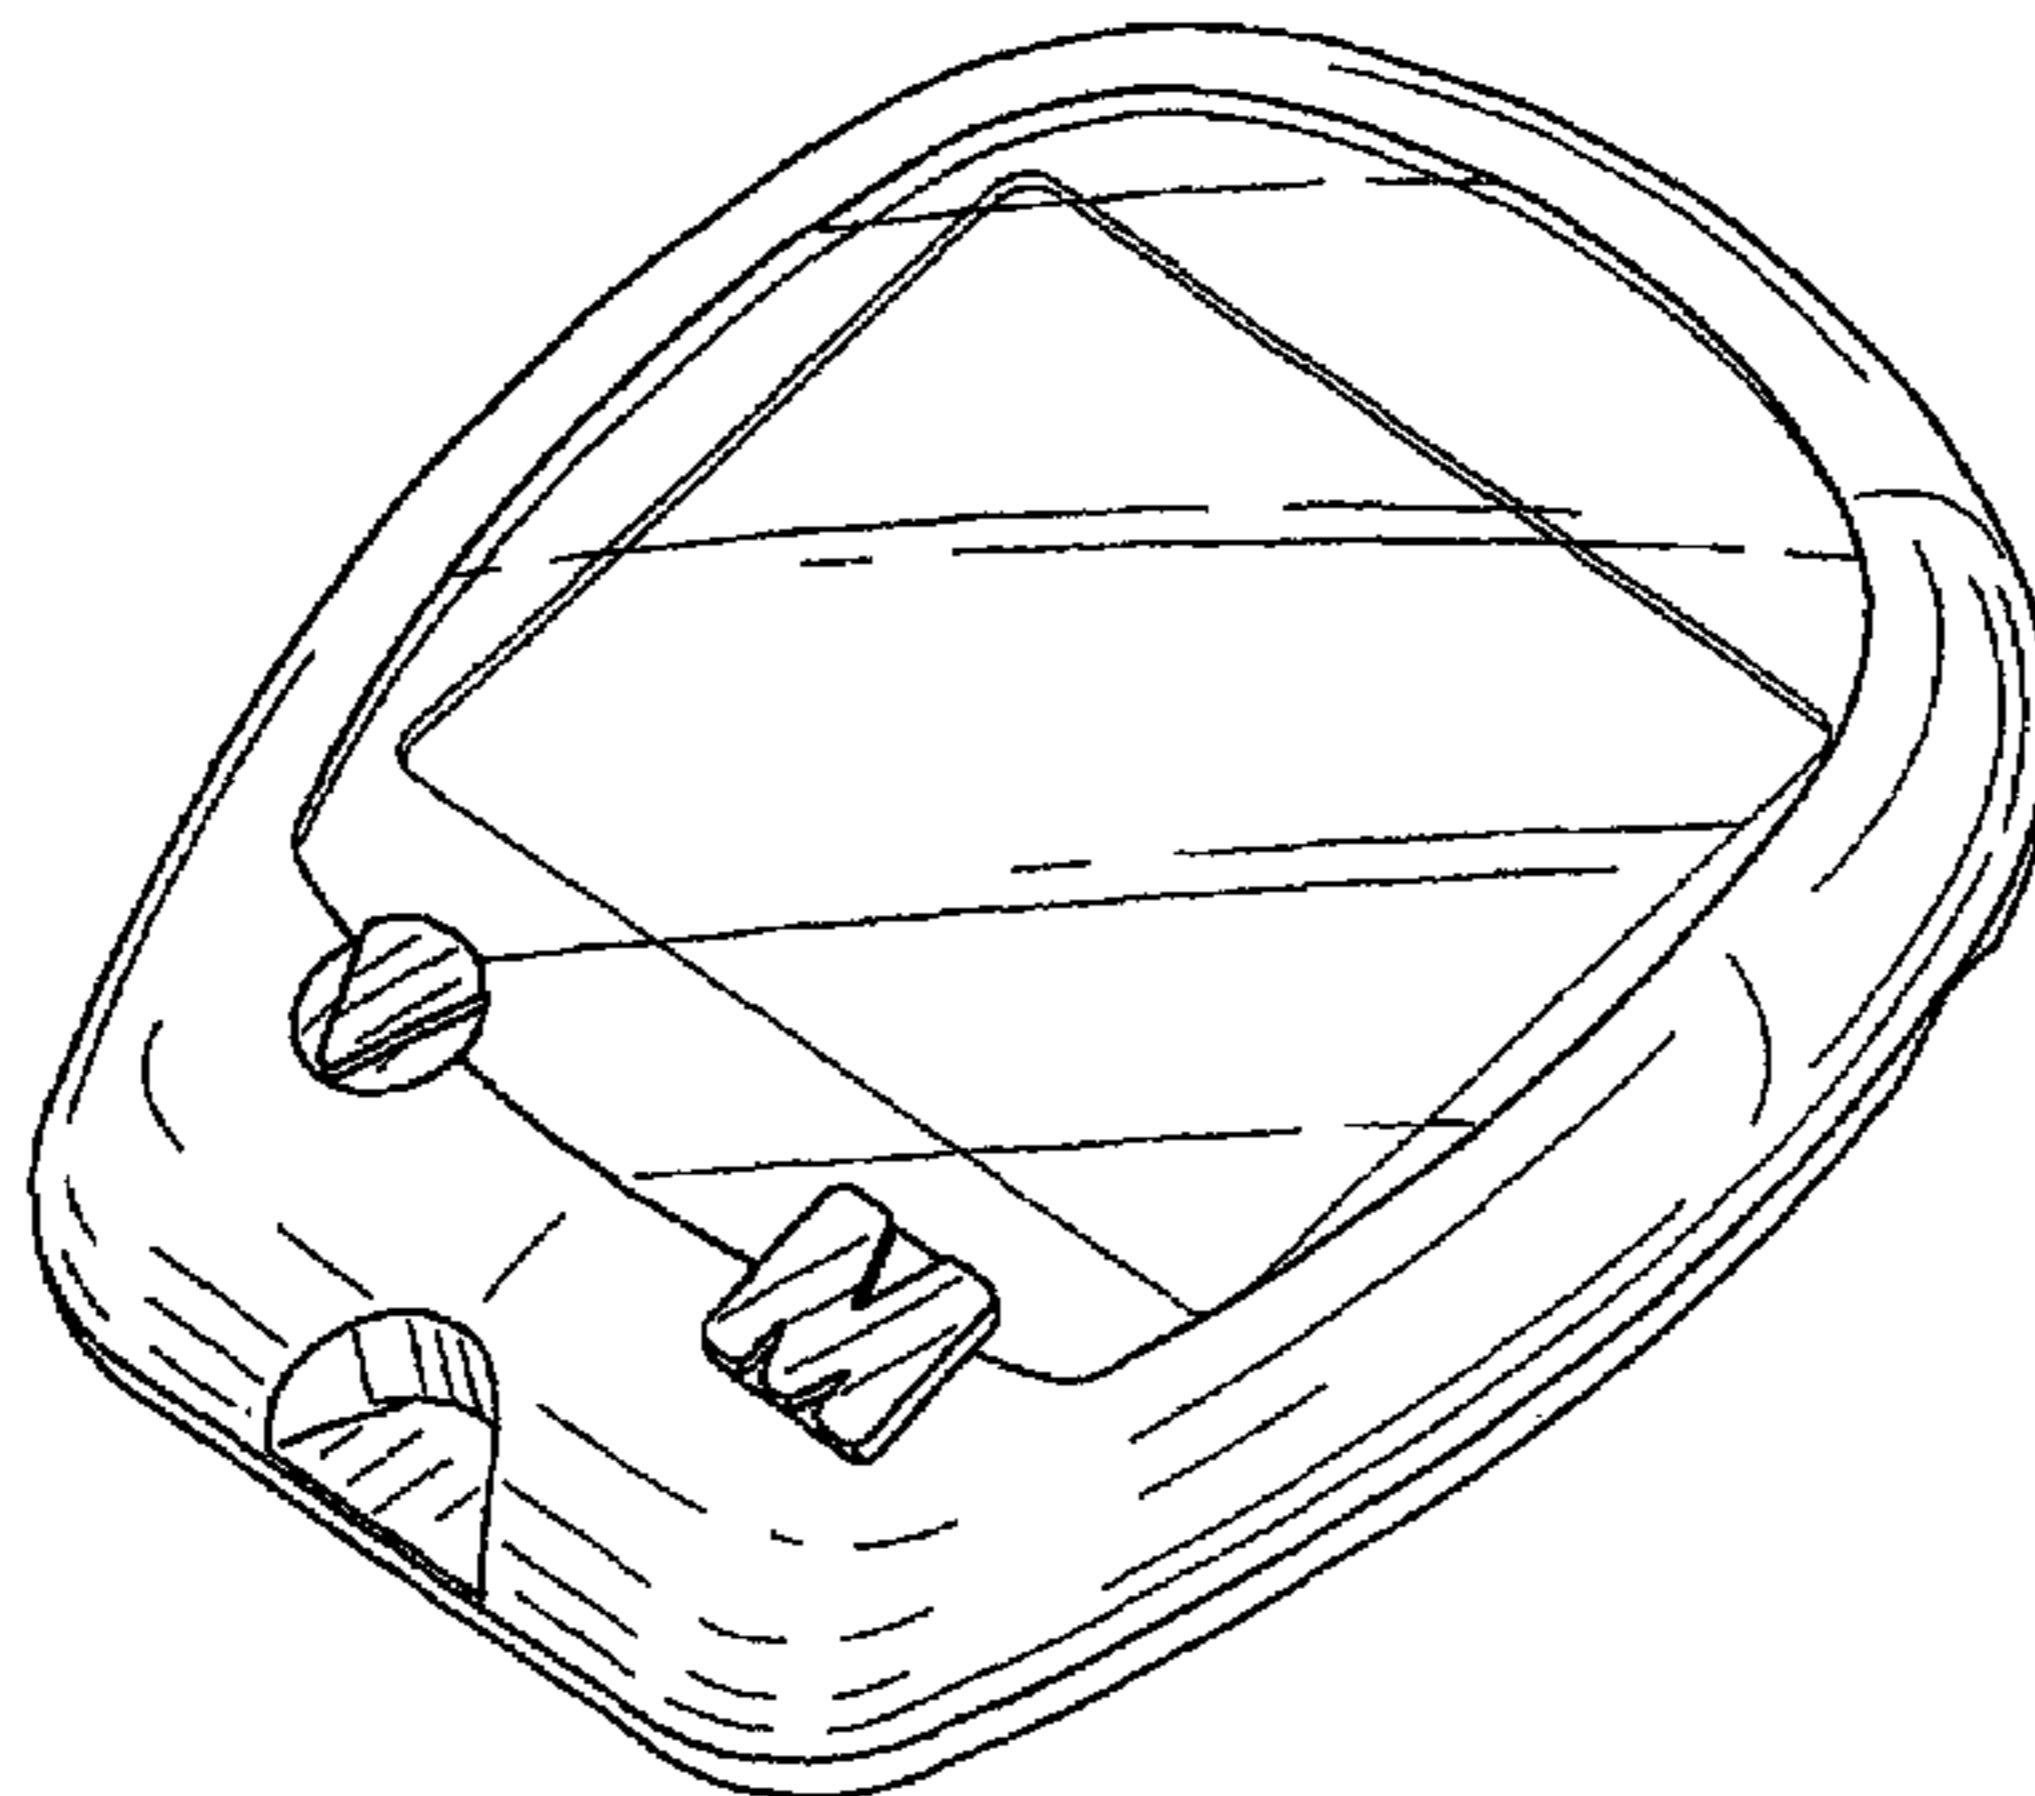

US D608,892 S

Page 2

U.S. PATENT DOCUMENTS					
			JP	D1192909 S	12/2003
			JP	D1192910 S	12/2003
7,181,350	B2	2/2007 Oberding	JP	D1192911 S	12/2003
D546,456	S	7/2007 May	JP	D1192912 S	12/2003
D546,457	S *	7/2007 Hannant et al. D24/186	JP	D1192913 S	12/2003
7,241,265	B2	7/2007 Cummings	JP	D1192914 S	12/2003
D548,347	S	8/2007 Ichino	JP	D1193467 S	1/2004
D549,343	S *	8/2007 Schlagheck et al. D24/169	JP	D1224545 S	12/2004
D555,021	S	11/2007 Rounds	JP	D1255662 S	11/2005
2003/0223906	A1	12/2003 McAllister	JP	D1256776 S	11/2005
2006/0182658	A1	8/2006 Wu	JP	D1269215 S	4/2006
			JP	D1292283 S	1/2007
FOREIGN PATENT DOCUMENTS			JP	D1206918 S	5/2007
JP	987768	S 8/1997	JP	D1206919 S	5/2007
JP	D1060640	S 2/2000	JP	D1206920 S	5/2007
JP	D1060644	S 2/2000	JP	D1206921 S	5/2007
JP	D1109739	S 5/2001	JP	D1206922 S	5/2007
JP	D1111904	S 6/2001	JP	D1206923 S	5/2007
JP	D1145566	S 7/2002	JP	D1301304 S	5/2007
JP	D1145580	S 7/2002	JP	D1301943 S	5/2007
JP	D1145581	S 7/2002	JP	D1312669 S	10/2007
JP	D1171179	S 4/2003	JP	D1316848 S	12/2007
JP	D1171182	S 4/2003	JP	D1316849 S	12/2007
JP	D1171284	S 4/2003			
JP	D1191803	S 12/2003			

* cited by examiner

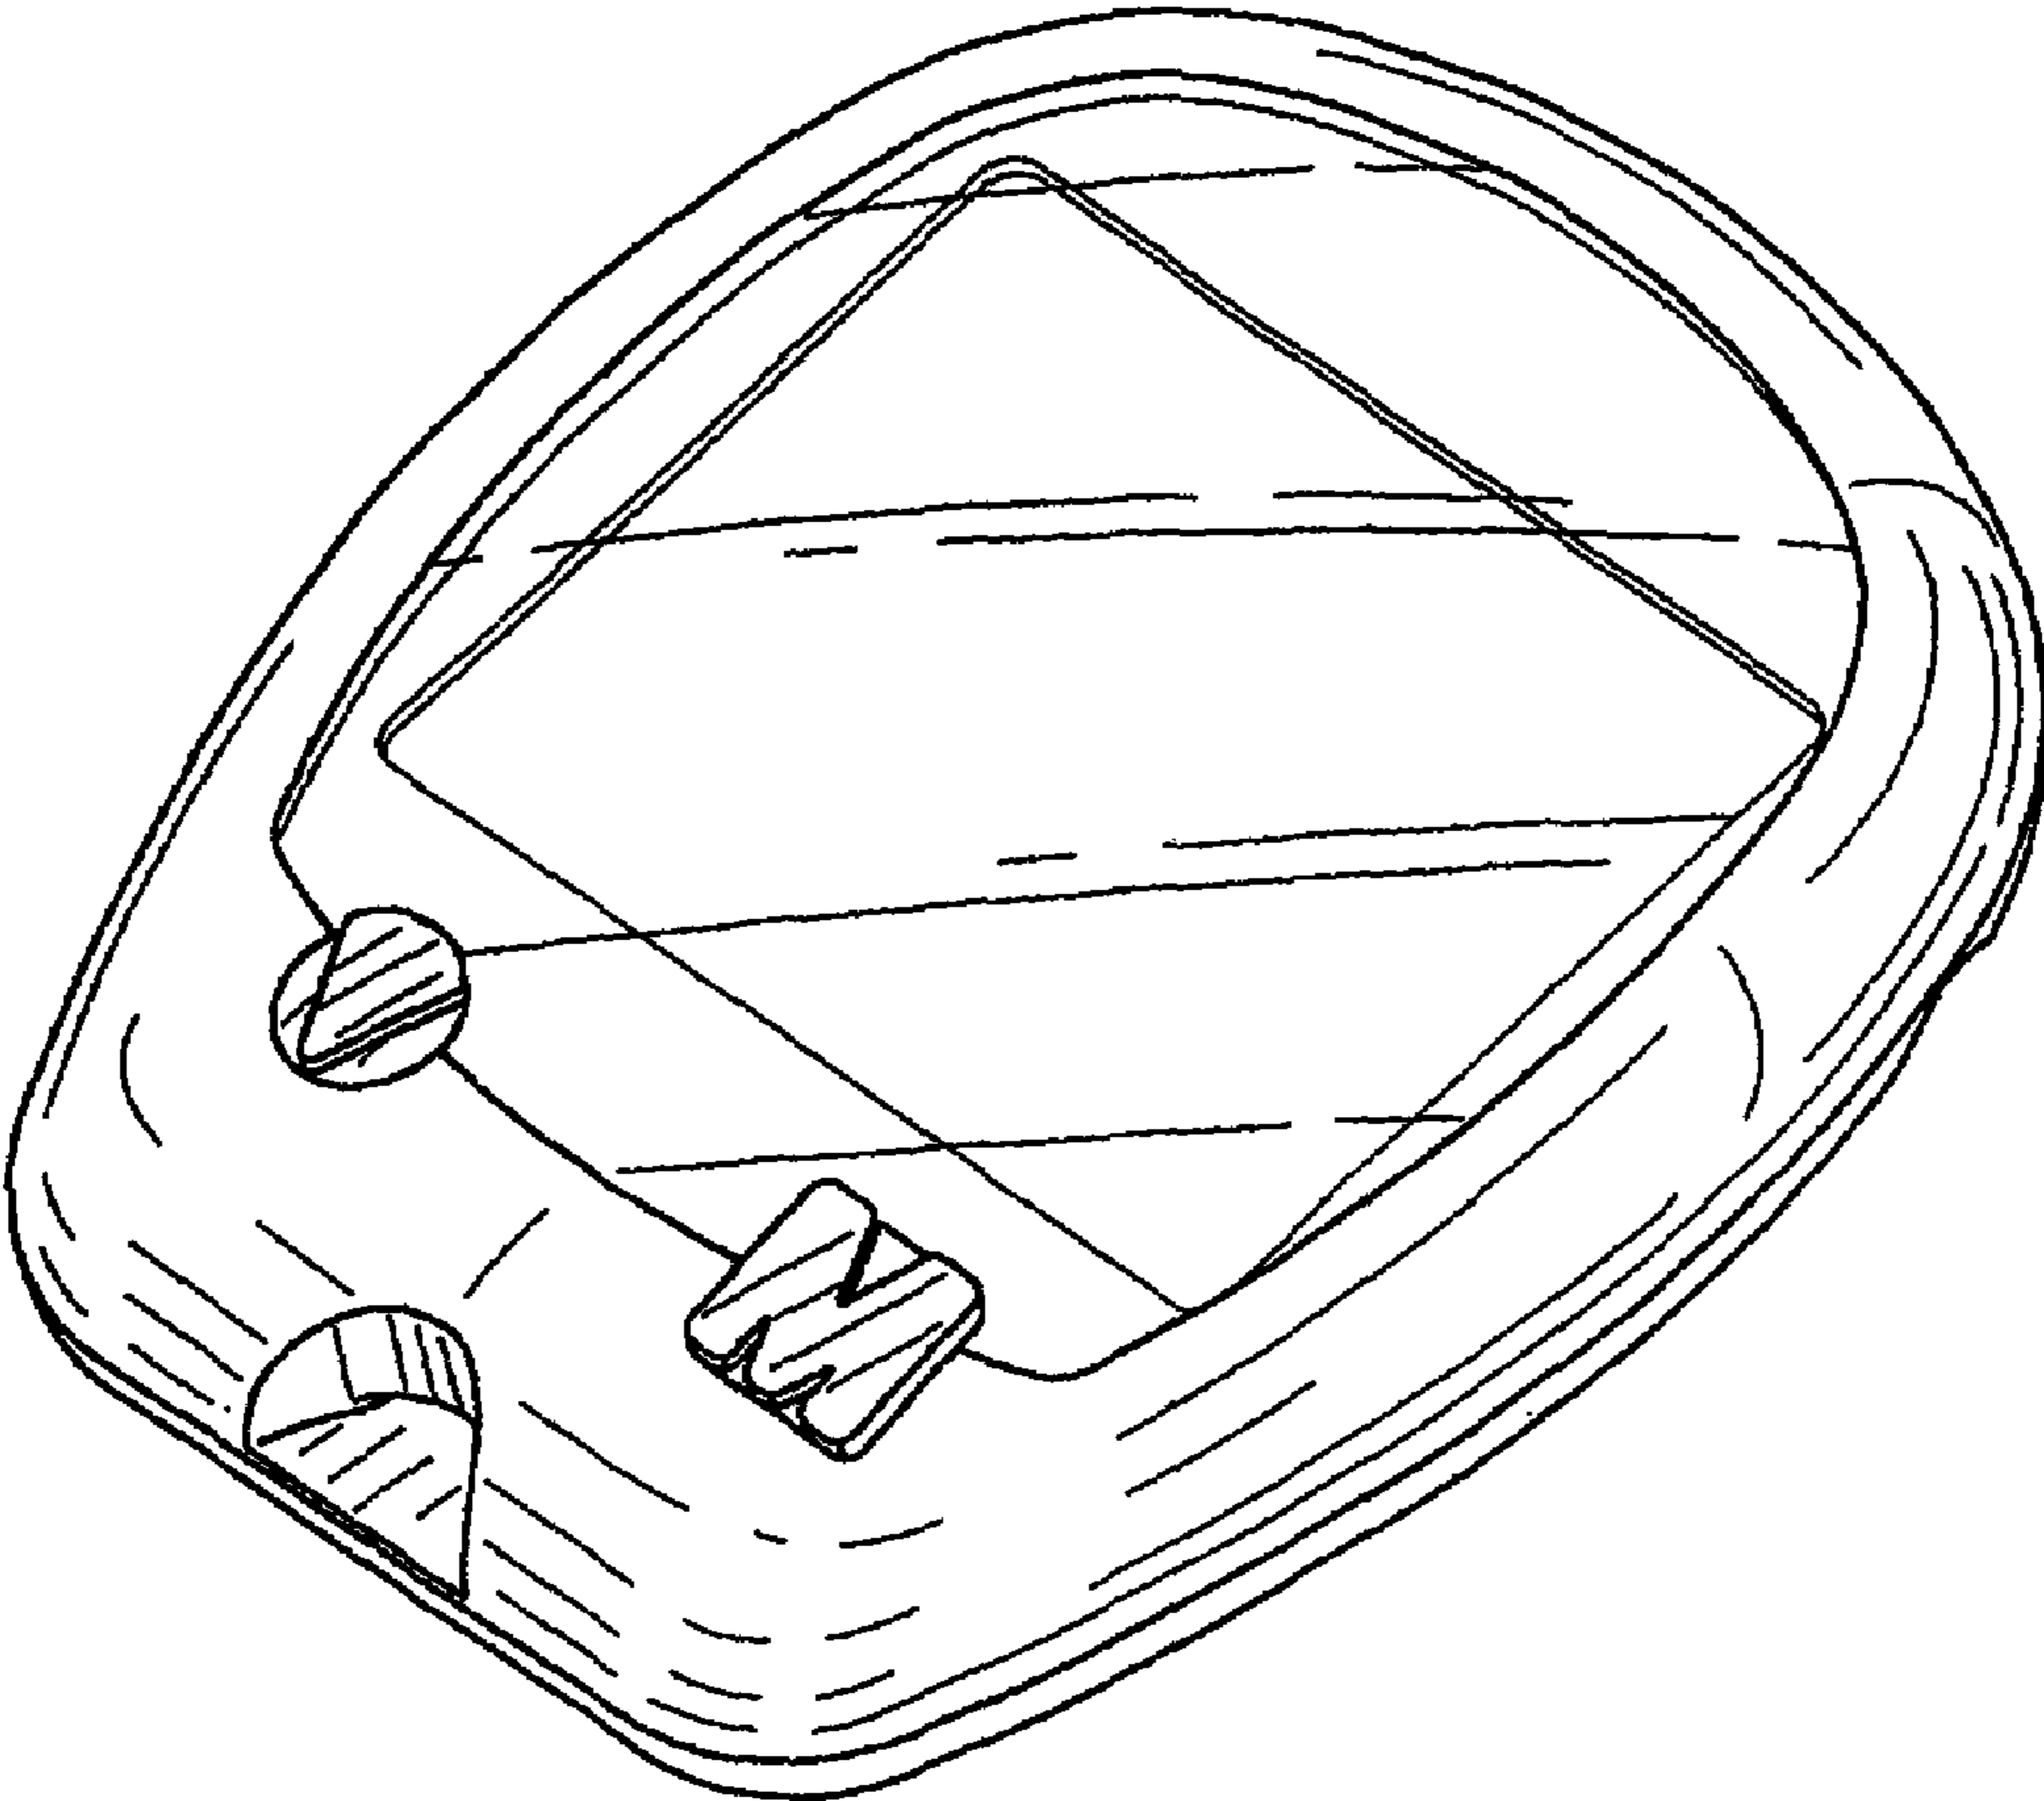


FIG. 1

FIG. 2

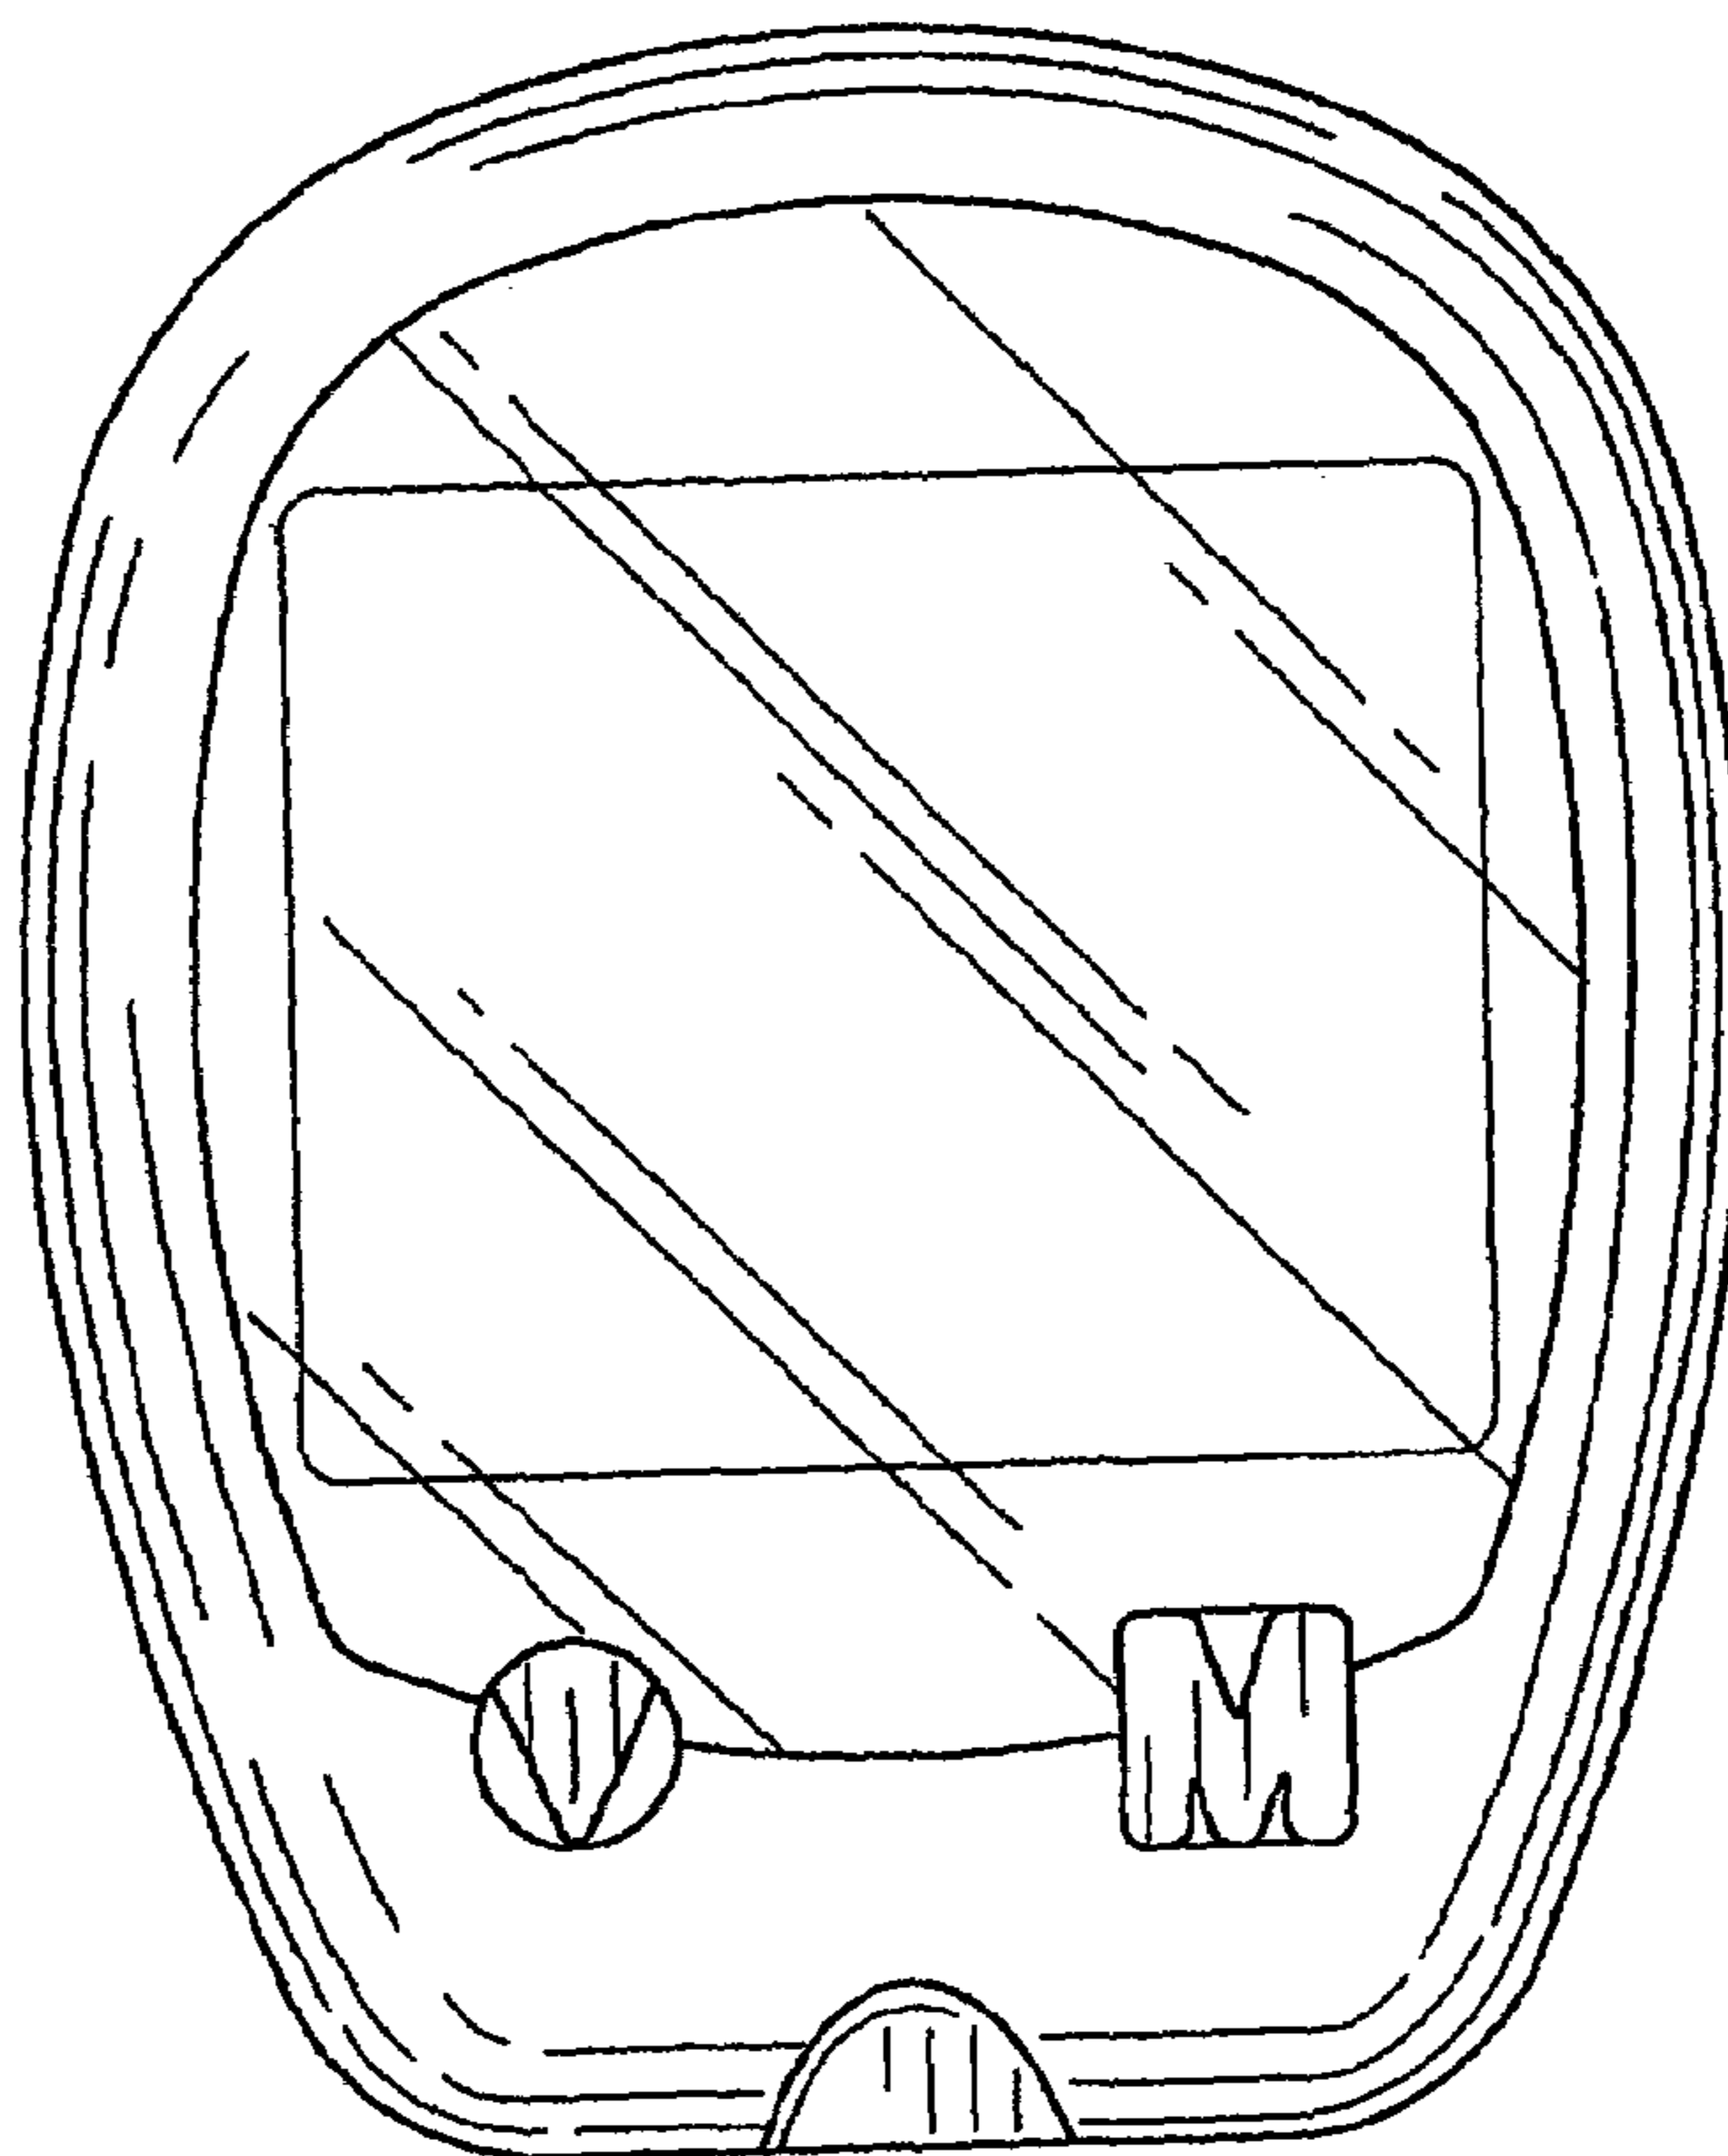
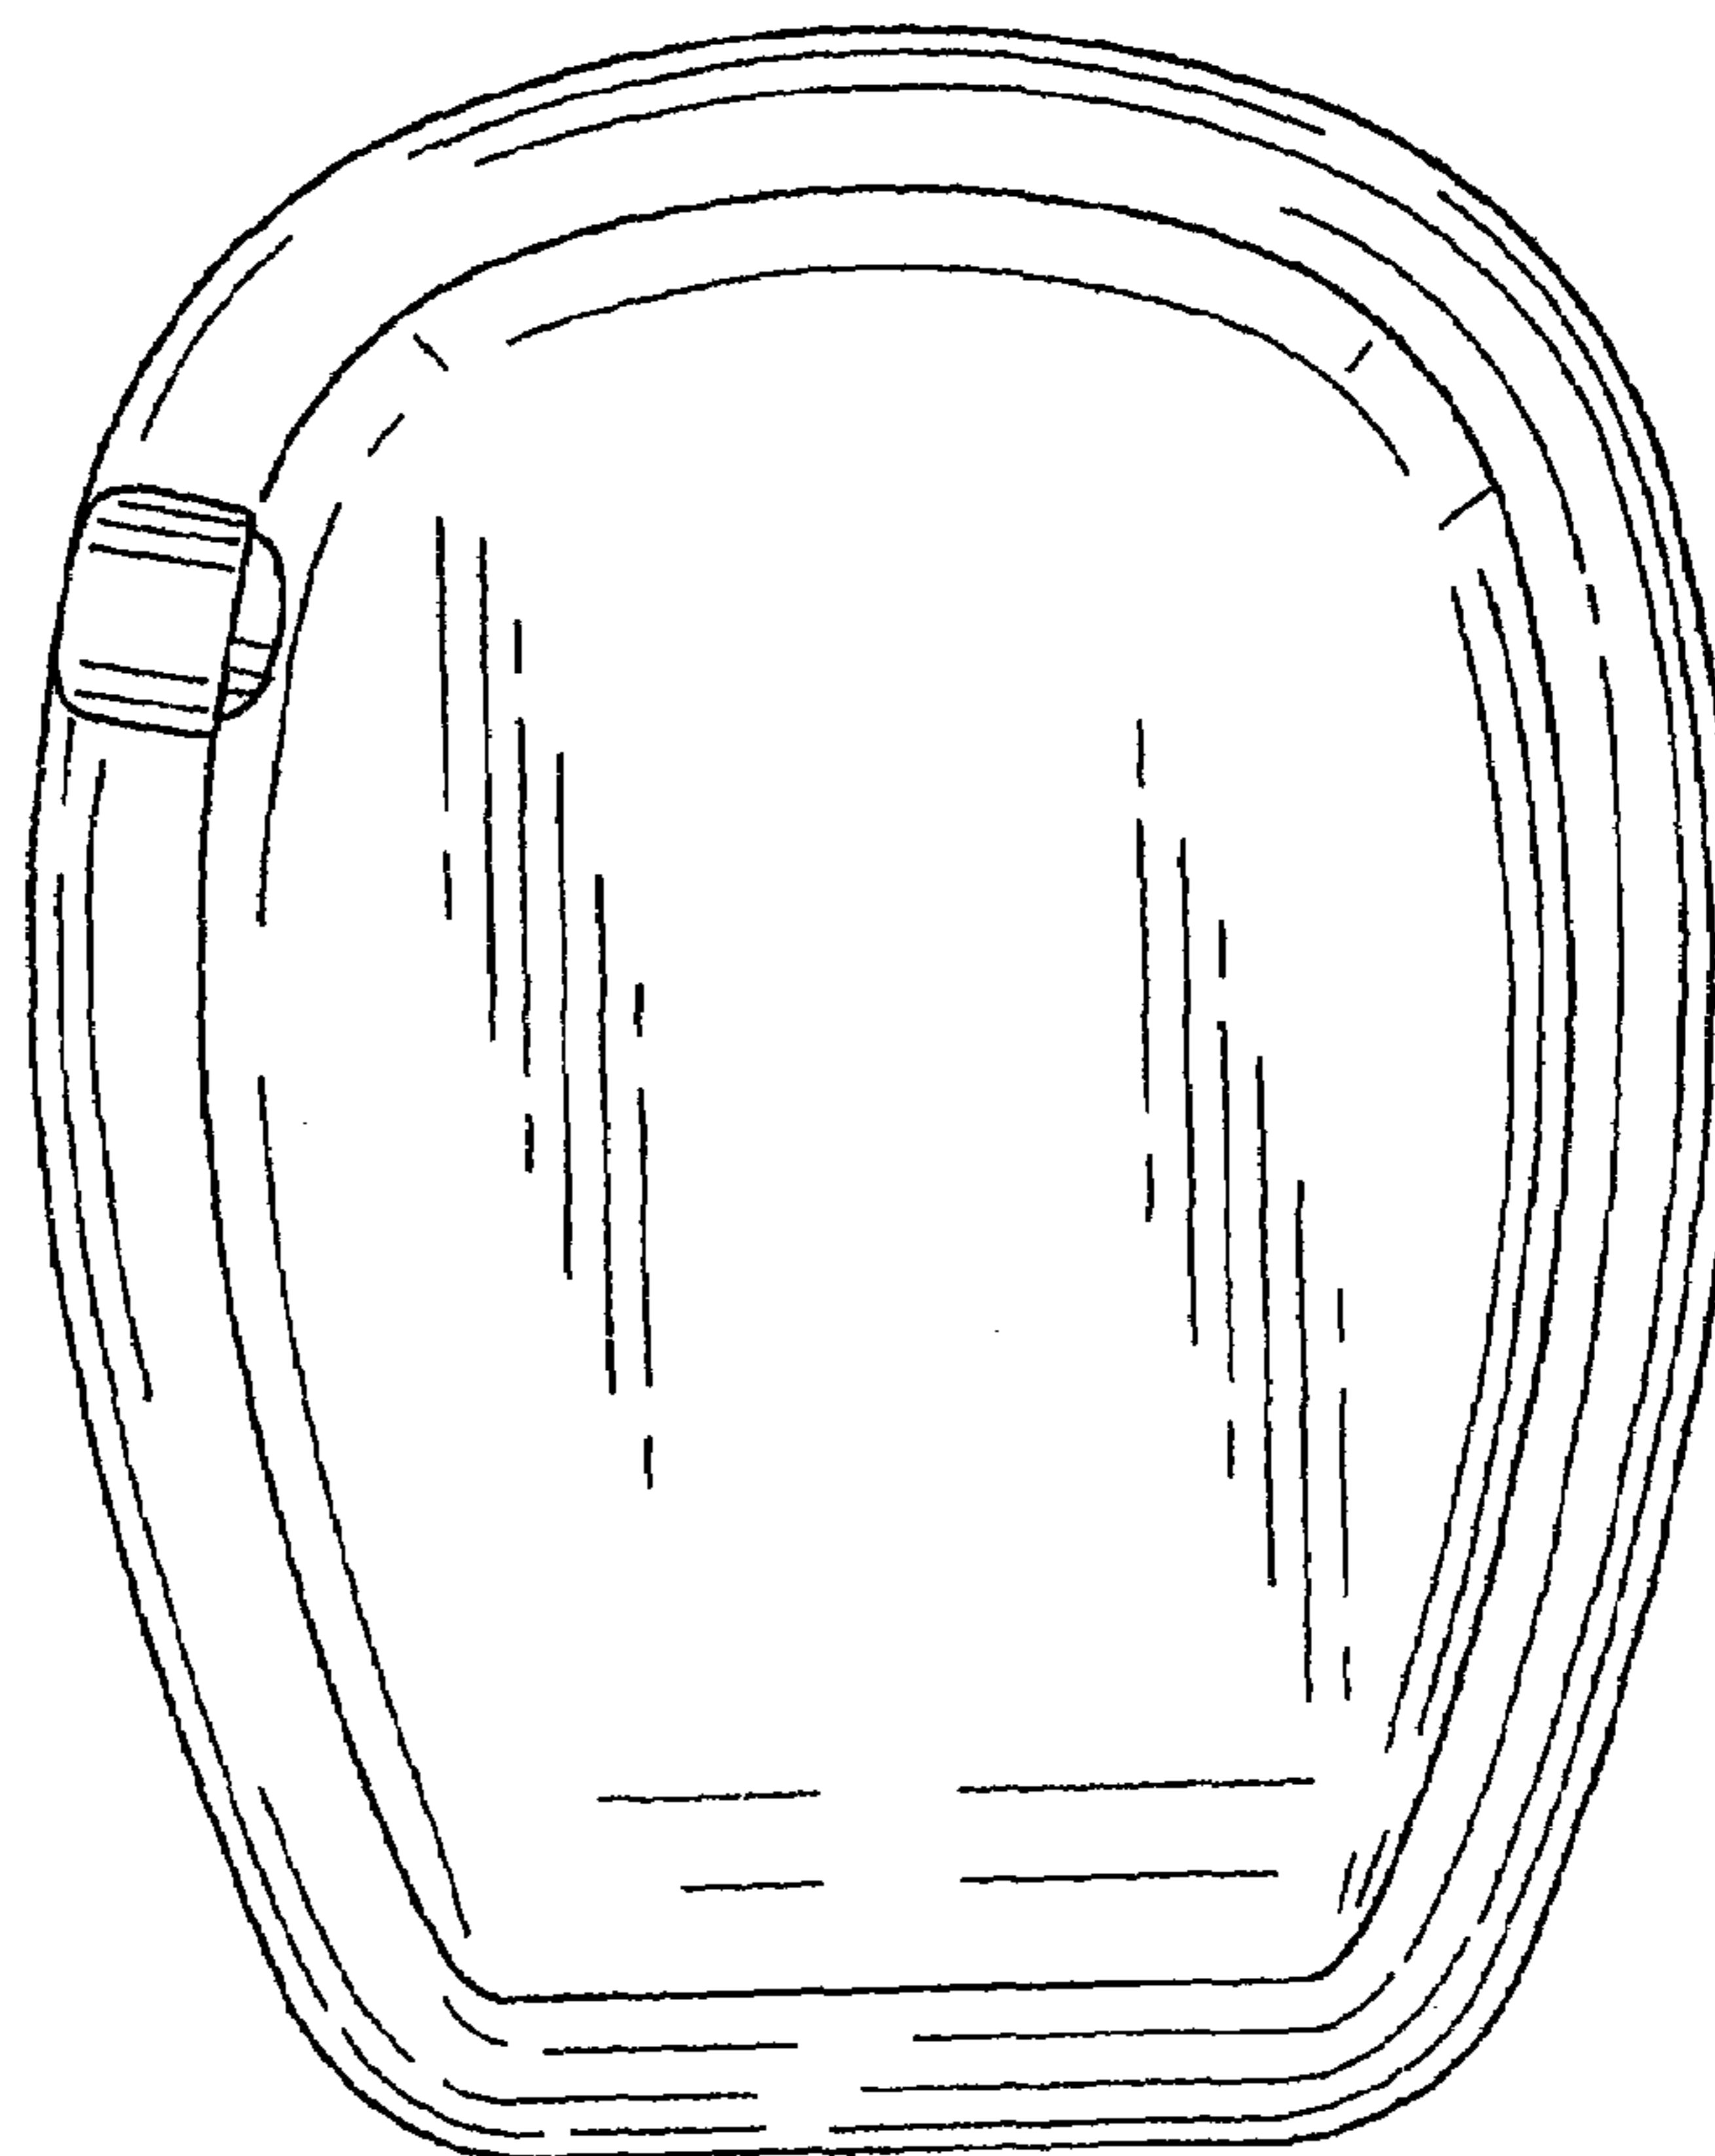


FIG. 3



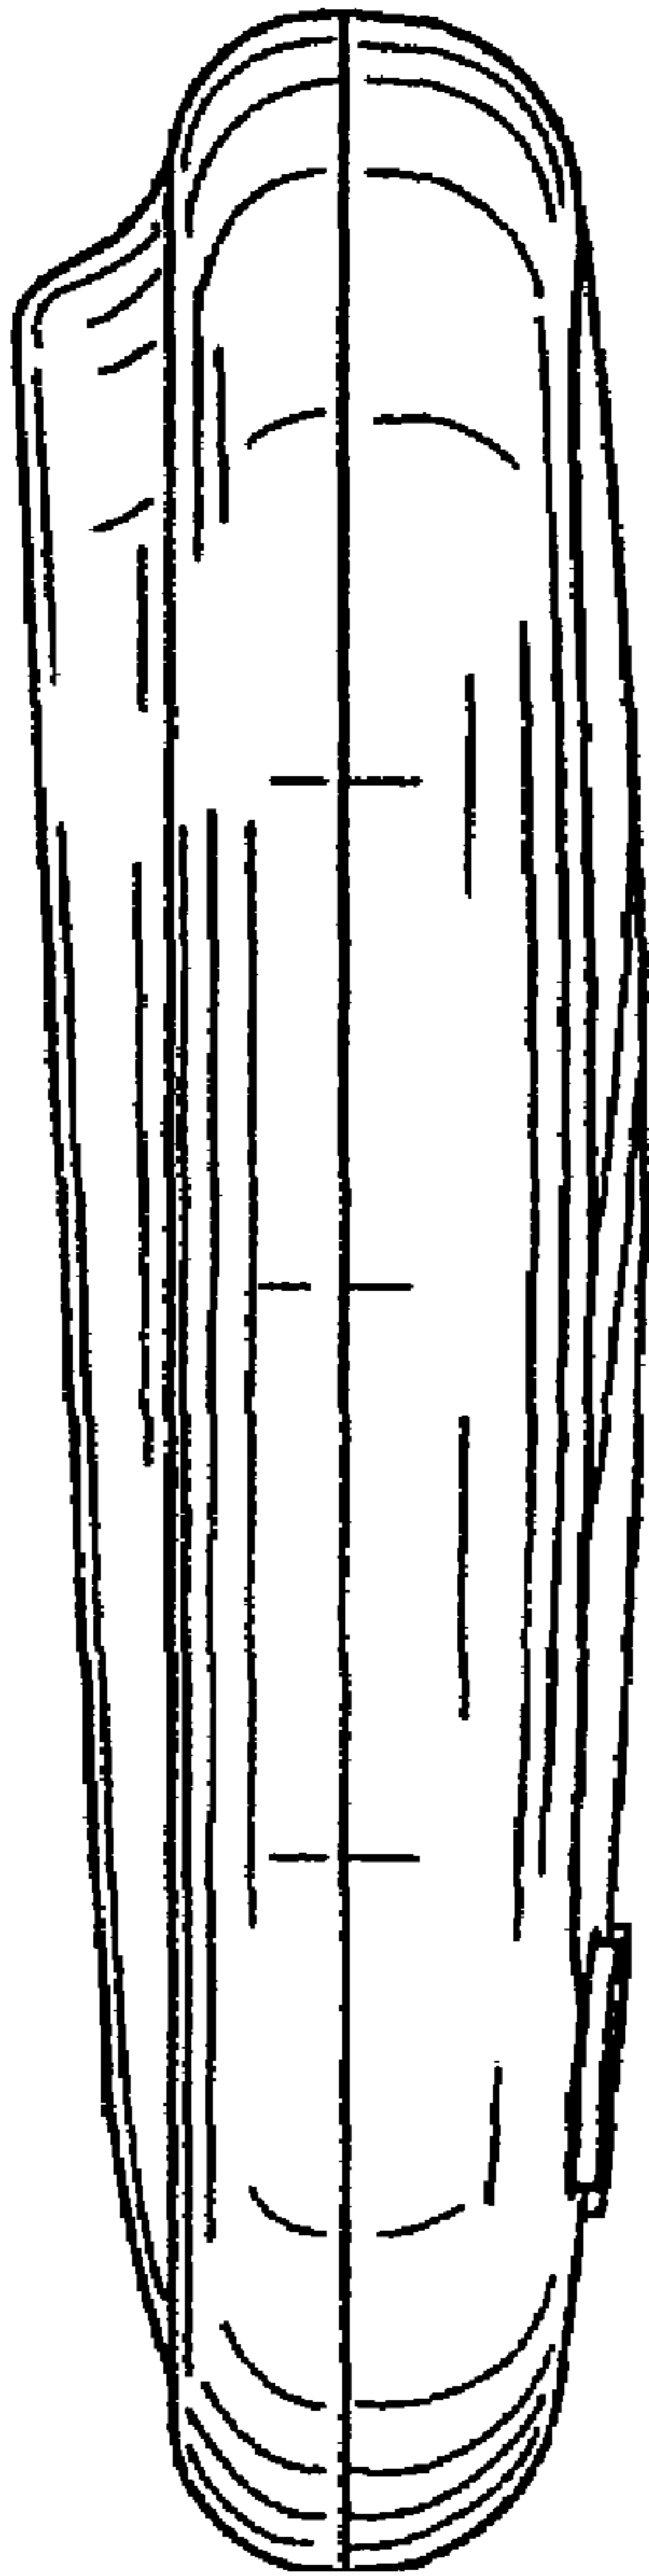


FIG. 4

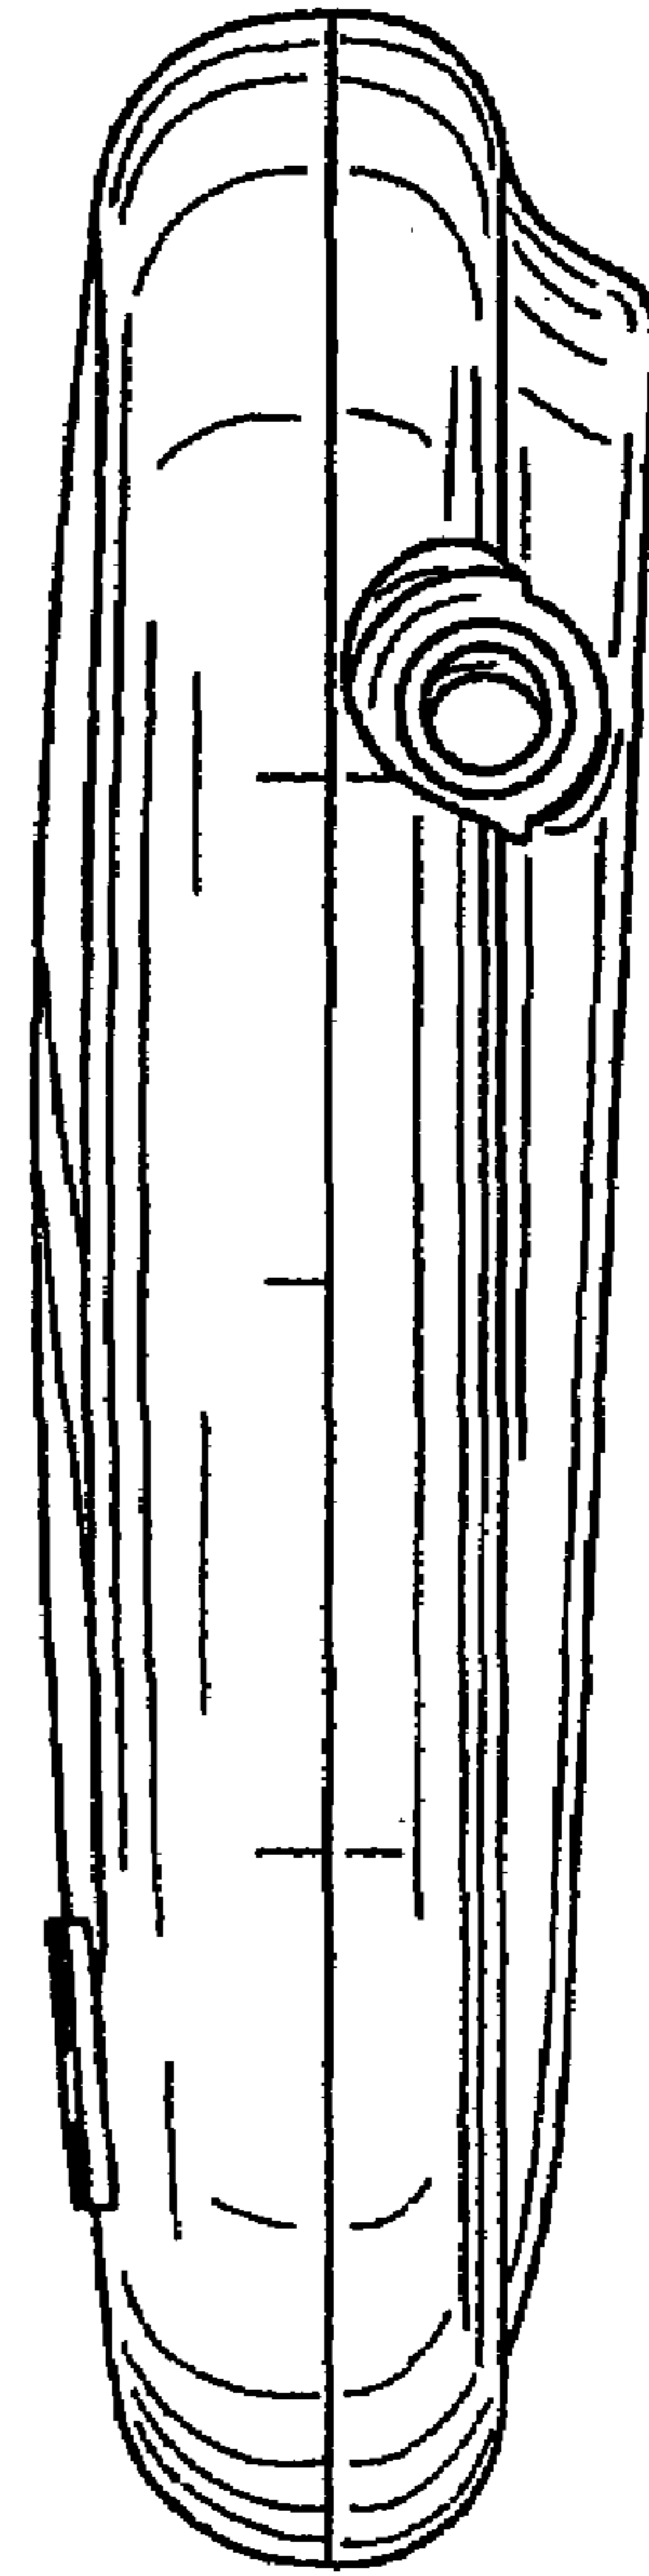


FIG. 5

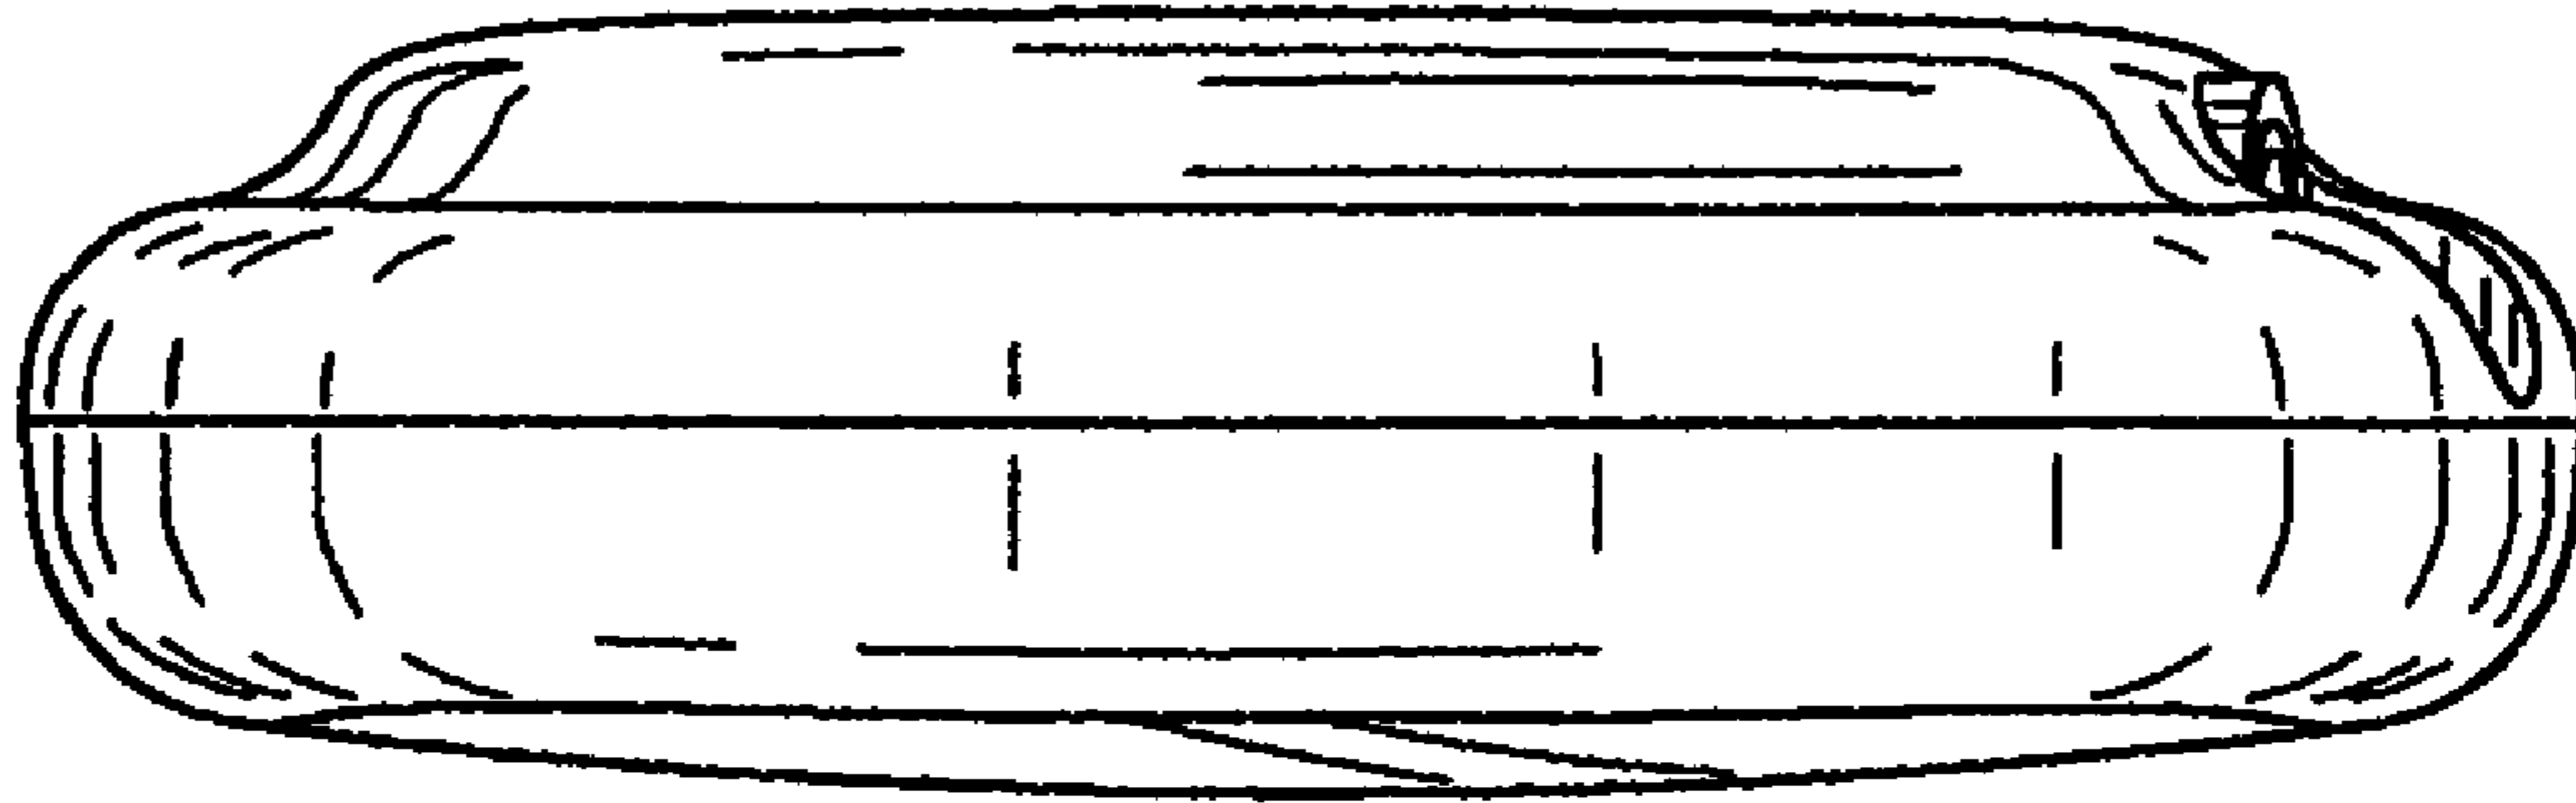


FIG. 6

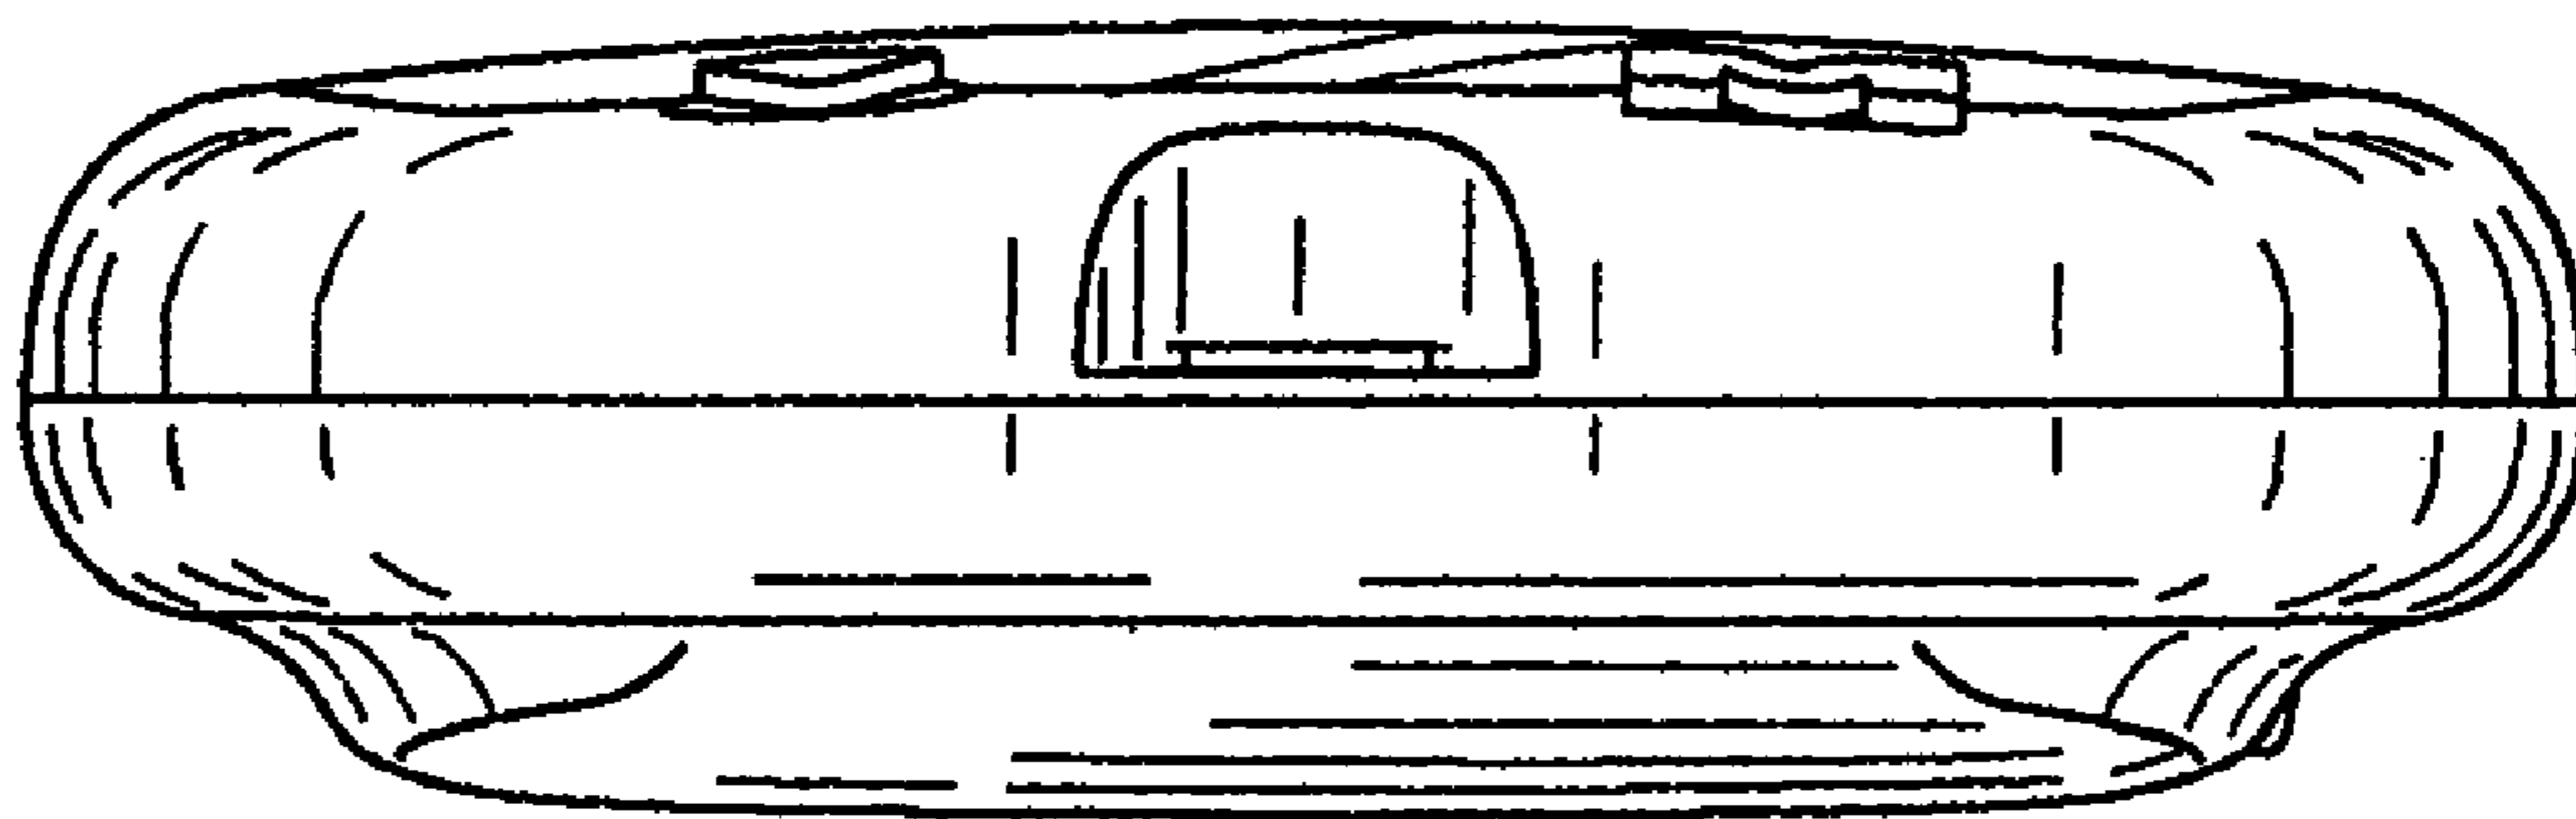


FIG. 7