



US00D609335S

(12) **United States Design Patent**
Cuevas et al.

(10) **Patent No.:** **US D609,335 S**
(45) **Date of Patent:** **** Feb. 2, 2010**

(54) **STOMA PAD**

(75) Inventors: **Brian J. Cuevas**, Cumming, GA (US);
Joseph A. Cesa, Cumming, GA (US);
Michael Sleva, Atlanta, GA (US); **Sam**
C. Chan, Atlanta, GA (US); **Marjory J.**
Greenhalgh, Decatur, GA (US)

(73) Assignee: **Kimberly-Clark Worldwide, Inc.**,
Neenah, WI (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/320,500**

(22) Filed: **Jun. 27, 2008**

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/128**

(58) **Field of Classification Search** D24/112,
D24/124, 128; 128/207.14–207.17, 200.26,
128/205.24, 207.29; 604/158, 165
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 3,338,992 A 8/1967 Kinney
- 3,341,394 A 9/1967 Kinney
- 3,502,763 A 3/1970 Hartmann
- 3,542,615 A 11/1970 Dobo et al.
- 3,688,774 A * 9/1972 Akiyama et al. 128/200.26
- 3,692,618 A 9/1972 Dorschner et al.
- 3,802,817 A 4/1974 Matsuki et al.
- 3,849,241 A 11/1974 Butin et al.
- 4,033,353 A 7/1977 La Rosa
- 4,041,203 A 8/1977 Brock et al.
- 4,085,752 A * 4/1978 Canale 604/370
- 4,100,324 A 7/1978 Anderson et al.
- 4,235,229 A 11/1980 Ranford et al.
- 4,340,563 A 7/1982 Appel et al.
- 4,470,176 A 9/1984 Vermeulen et al.
- 4,817,598 A * 4/1989 LaBombard 128/207.14
- 4,818,464 A 4/1989 Lau
- D304,080 S * 10/1989 Lee et al. D24/129
- 5,058,579 A * 10/1991 Terry et al. 128/207.14

- 5,145,727 A 9/1992 Potts et al.
- 5,169,706 A 12/1992 Collier, IV et al.
- 5,178,931 A 1/1993 Perkins et al.
- 5,188,885 A 2/1993 Timmons et al.
- D336,548 S * 6/1993 Zeller D29/121.1
- 5,237,988 A 8/1993 McNeese

(Continued)

FOREIGN PATENT DOCUMENTS

GB 1431761 A 4/1976

(Continued)

OTHER PUBLICATIONS

ASTM Designation: D 2240-05, Standard Test Method for Rubber Property—Durometer Hardness, Published Sep. 2005, pp. 1-13.

Primary Examiner—T. Chase Nelson
Assistant Examiner—Eric L Goodman
(74) *Attorney, Agent, or Firm*—James B Robinson

(57) **CLAIM**


We claim the ornamental design for a stoma pad, as shown and described.

DESCRIPTION

The single view is a top view of the stoma pad. The broken lines represent lines of weakness along which the pad may be torn.

The broken lines represent lines of weakness along which the pad may be torn and forms a part of the claimed design. The stoma pad is flat and without contour.

1 Claim, 1 Drawing Sheet

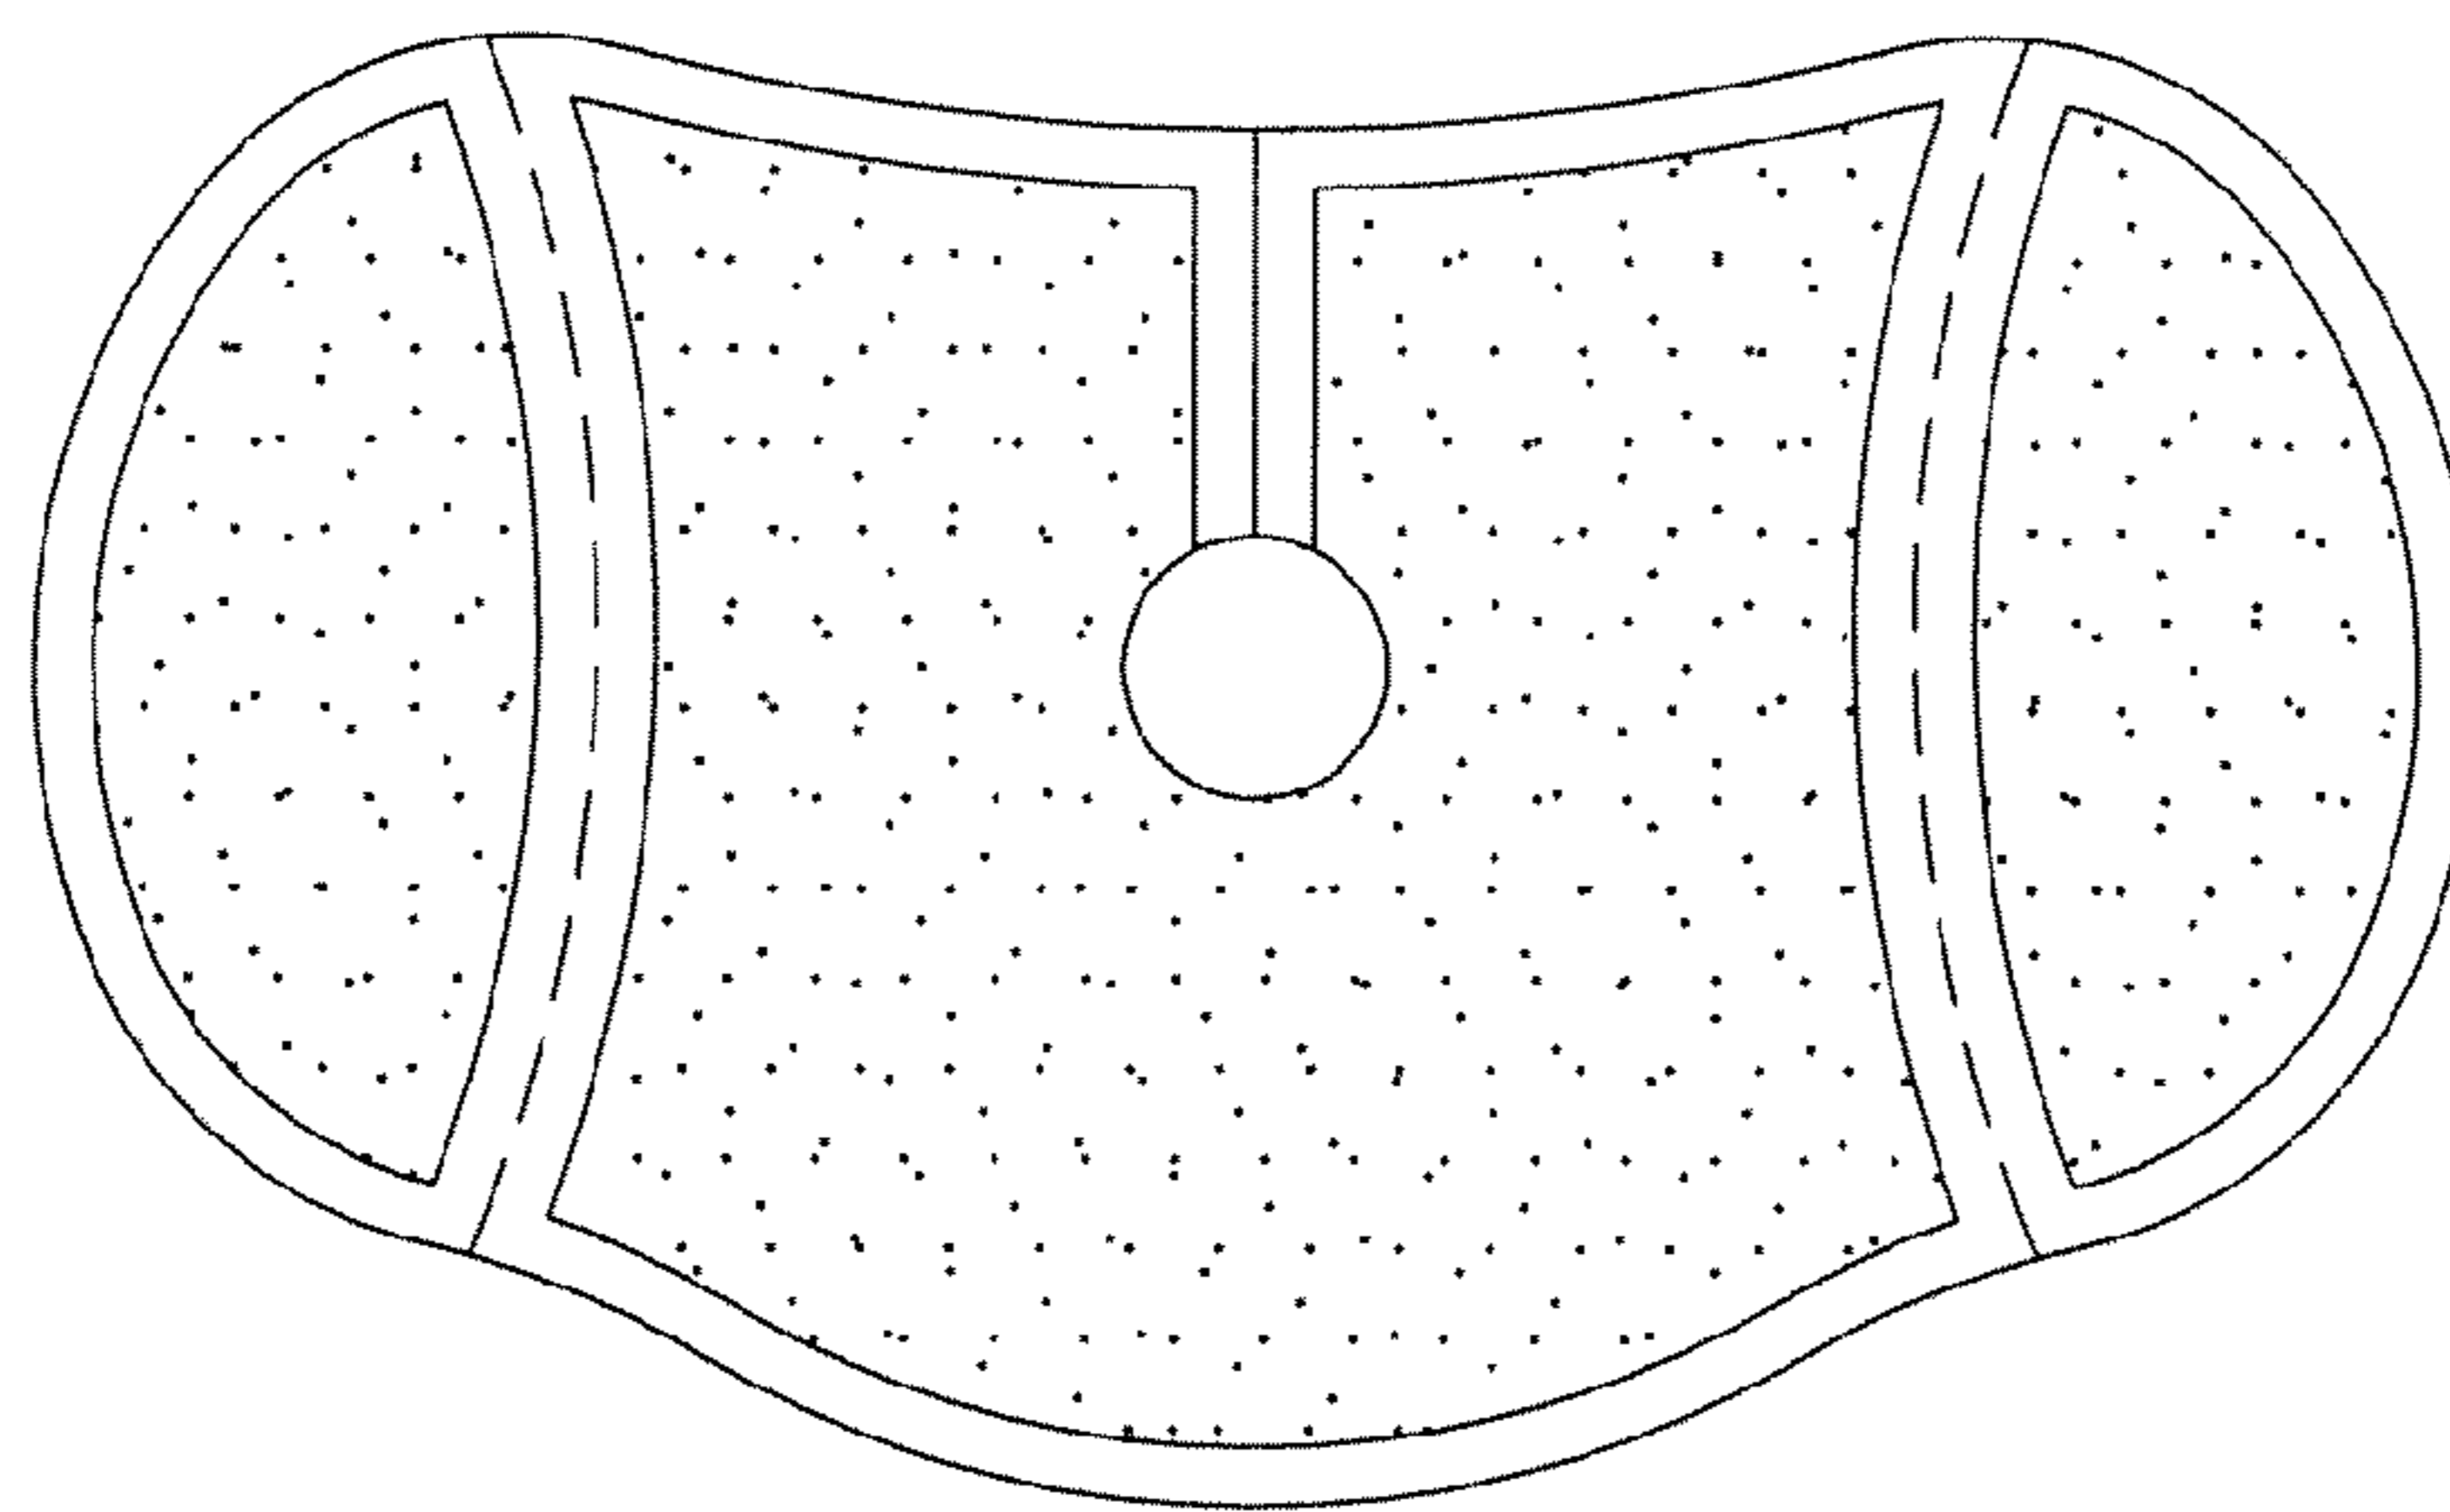

US D609,335 S

Page 2

U.S. PATENT DOCUMENTS

5,251,616 A 10/1993 Desch
5,819,734 A 10/1998 Deily et al.
5,839,437 A 11/1998 Briggs, III
6,105,577 A * 8/2000 Varner 128/207.17
D492,411 S * 6/2004 Bierman D24/128
D503,977 S * 4/2005 Bierman D24/128
7,093,598 B1 8/2006 Hanneman et al.
D528,206 S * 9/2006 Bierman D24/128
2005/0081860 A1 4/2005 Gonzales
2005/0166924 A1 8/2005 Thomas et al.

2006/0124134 A1 6/2006 Wood
2007/0068533 A1 * 3/2007 Bierman et al. 128/207.17
2008/0078402 A1 * 4/2008 Mongeon 128/207.15
2009/0032018 A1 * 2/2009 Eaton et al. 128/201.22

FOREIGN PATENT DOCUMENTS

GB 2102490 A 2/1983
WO WO 2006/087512 8/2006
WO WO 2006/087513 8/2006

* cited by examiner

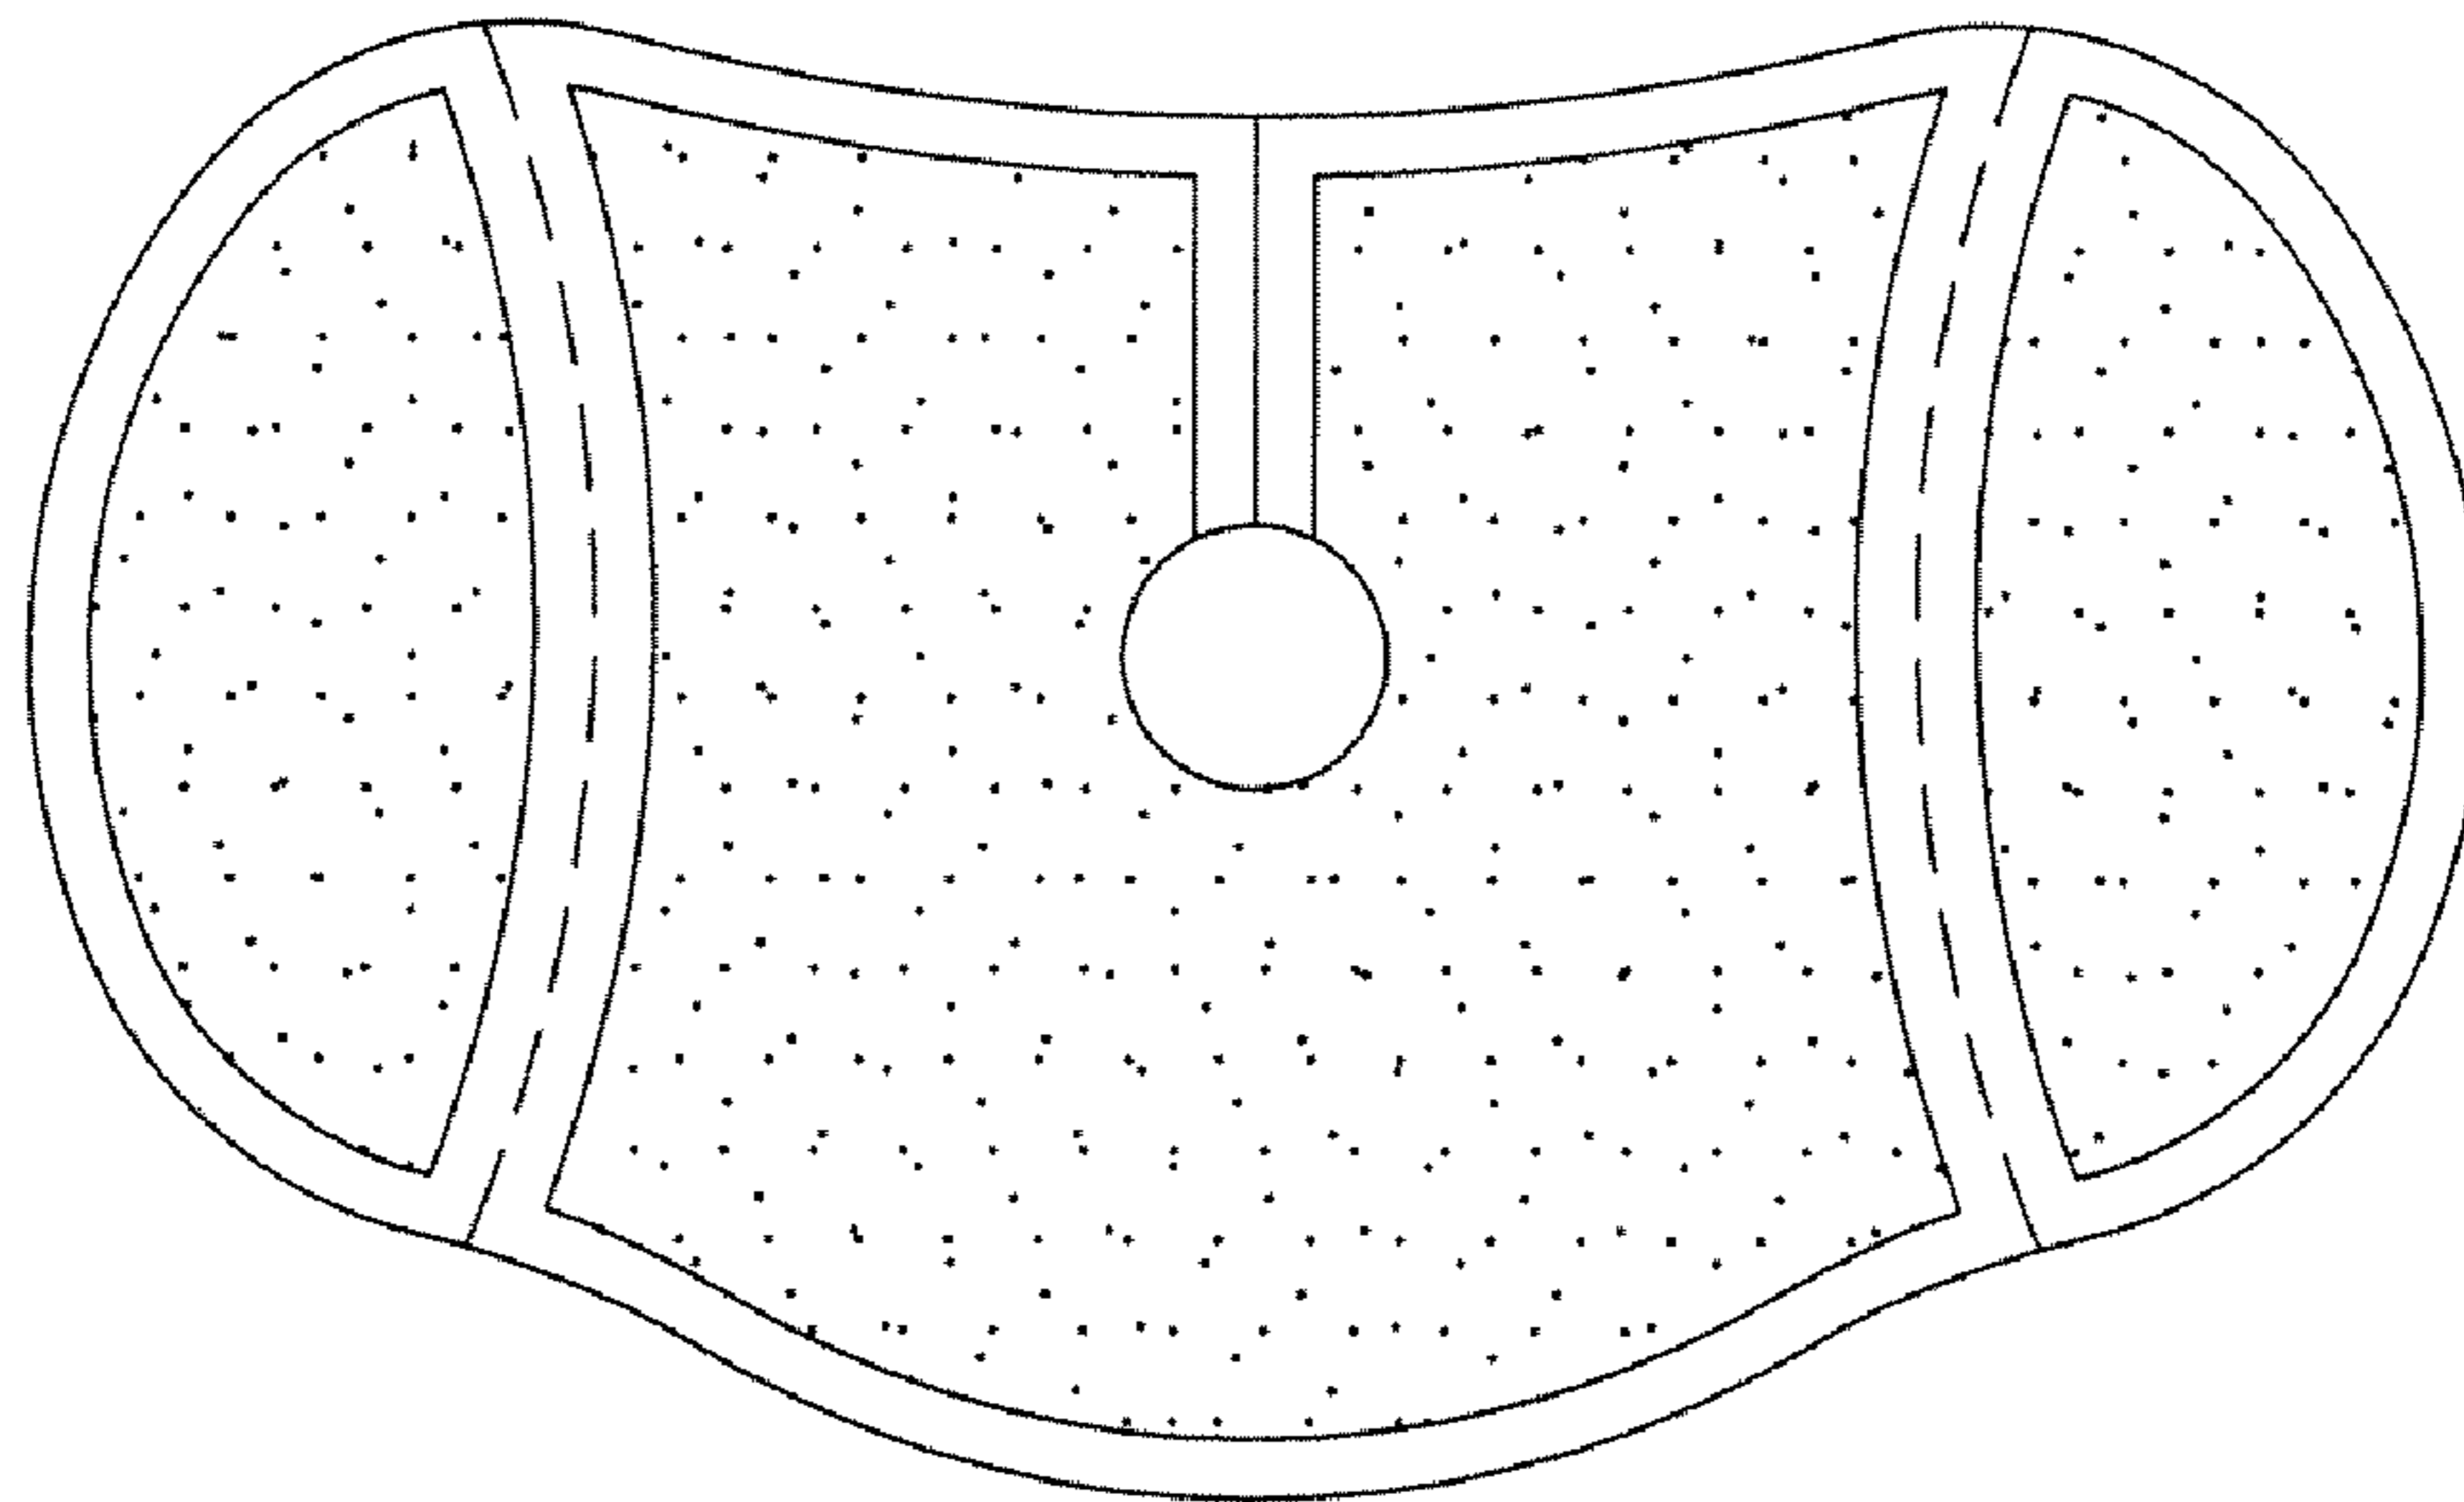


FIG. 1