

US00D609351S

(12) **United States Design Patent**
Wagener et al.

(10) **Patent No.:** **US D609,351 S**
(45) **Date of Patent:** **** Feb. 2, 2010**

(54) **MEDICAL MONITOR**

(75) Inventors: **Morten Wagener**, San Francisco, CA
(US); **David F. Gustafson**, Sacramento,
CA (US); **Ian Edwards**, Skaneateles,
NY (US); **Ah Leen Neo**, Singapore
(SG); **Bobby Gee Han Png**, Singapore
(SG)

(73) Assignee: **Welch Allyn, Inc.**, Skaneateles Falls, NY
(US)

(**) Term: **14 Years**

(21) Appl. No.: **29/334,317**

(22) Filed: **Mar. 24, 2009**

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/107,
D24/137-138, 158, 164-165, 167, 169-170,
D24/186-187, 231, 232; D10/78, 81, 104;
600/300-301, 368, 372, 481, 529, 544, 554,
600/561; 422/1, 61, 68.1, 99-104, 129; 128/903,
128/671

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D299,861 S * 2/1989 Hunsdale et al. D24/186
D390,666 S * 2/1998 Lagerlof D24/186
D392,043 S 3/1998 Cooper et al.
D414,870 S * 10/1999 Saltzstein et al. D24/186
D447,569 S * 9/2001 Baily et al. D24/186
D460,559 S 7/2002 Knieriem et al.
D512,151 S 11/2005 Ward et al.
D516,026 S 2/2006 Barrett et al.
D535,031 S 1/2007 Barrett et al.
D536,794 S 2/2007 Knieriem et al.

D536,795 S 2/2007 Knieriem et al.
D547,454 S * 7/2007 Hsieh D24/186
D549,831 S 8/2007 Ward et al.
D551,769 S * 9/2007 Skwarek et al. D24/186
D554,266 S * 10/2007 Striepe et al. D24/186
D569,001 S * 5/2008 Omaki D24/186
D569,521 S * 5/2008 Omaki D24/186
7,515,043 B2 4/2009 Welch et al.
D592,754 S * 5/2009 Koike et al. D24/186
D598,551 S * 8/2009 Miwa et al. D24/186

OTHER PUBLICATIONS

U.S. Appl. No. 29/323,125, Lathrop et al.
U.S. Appl. No. 29/323,129, Lathrop et al.
U.S. Appl. No. 29/323,133, Lathrop et al.

* cited by examiner

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Hiscock & Barclay, LLP

(57) **CLAIM**

The ornamental design for a medical monitor, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a medical monitor, illustrating my new design;

FIG. 2 is a bottom perspective view thereof;

FIG. 3 is a top plan view thereof;

FIG. 4 is a left side view thereof;



FIG. 5 is a right side view thereof;

FIG. 6 is a front end view thereof;

FIG. 7 is a rear end view thereof; and,

FIG. 8 is a bottom view thereof.

1 Claim, 3 Drawing Sheets

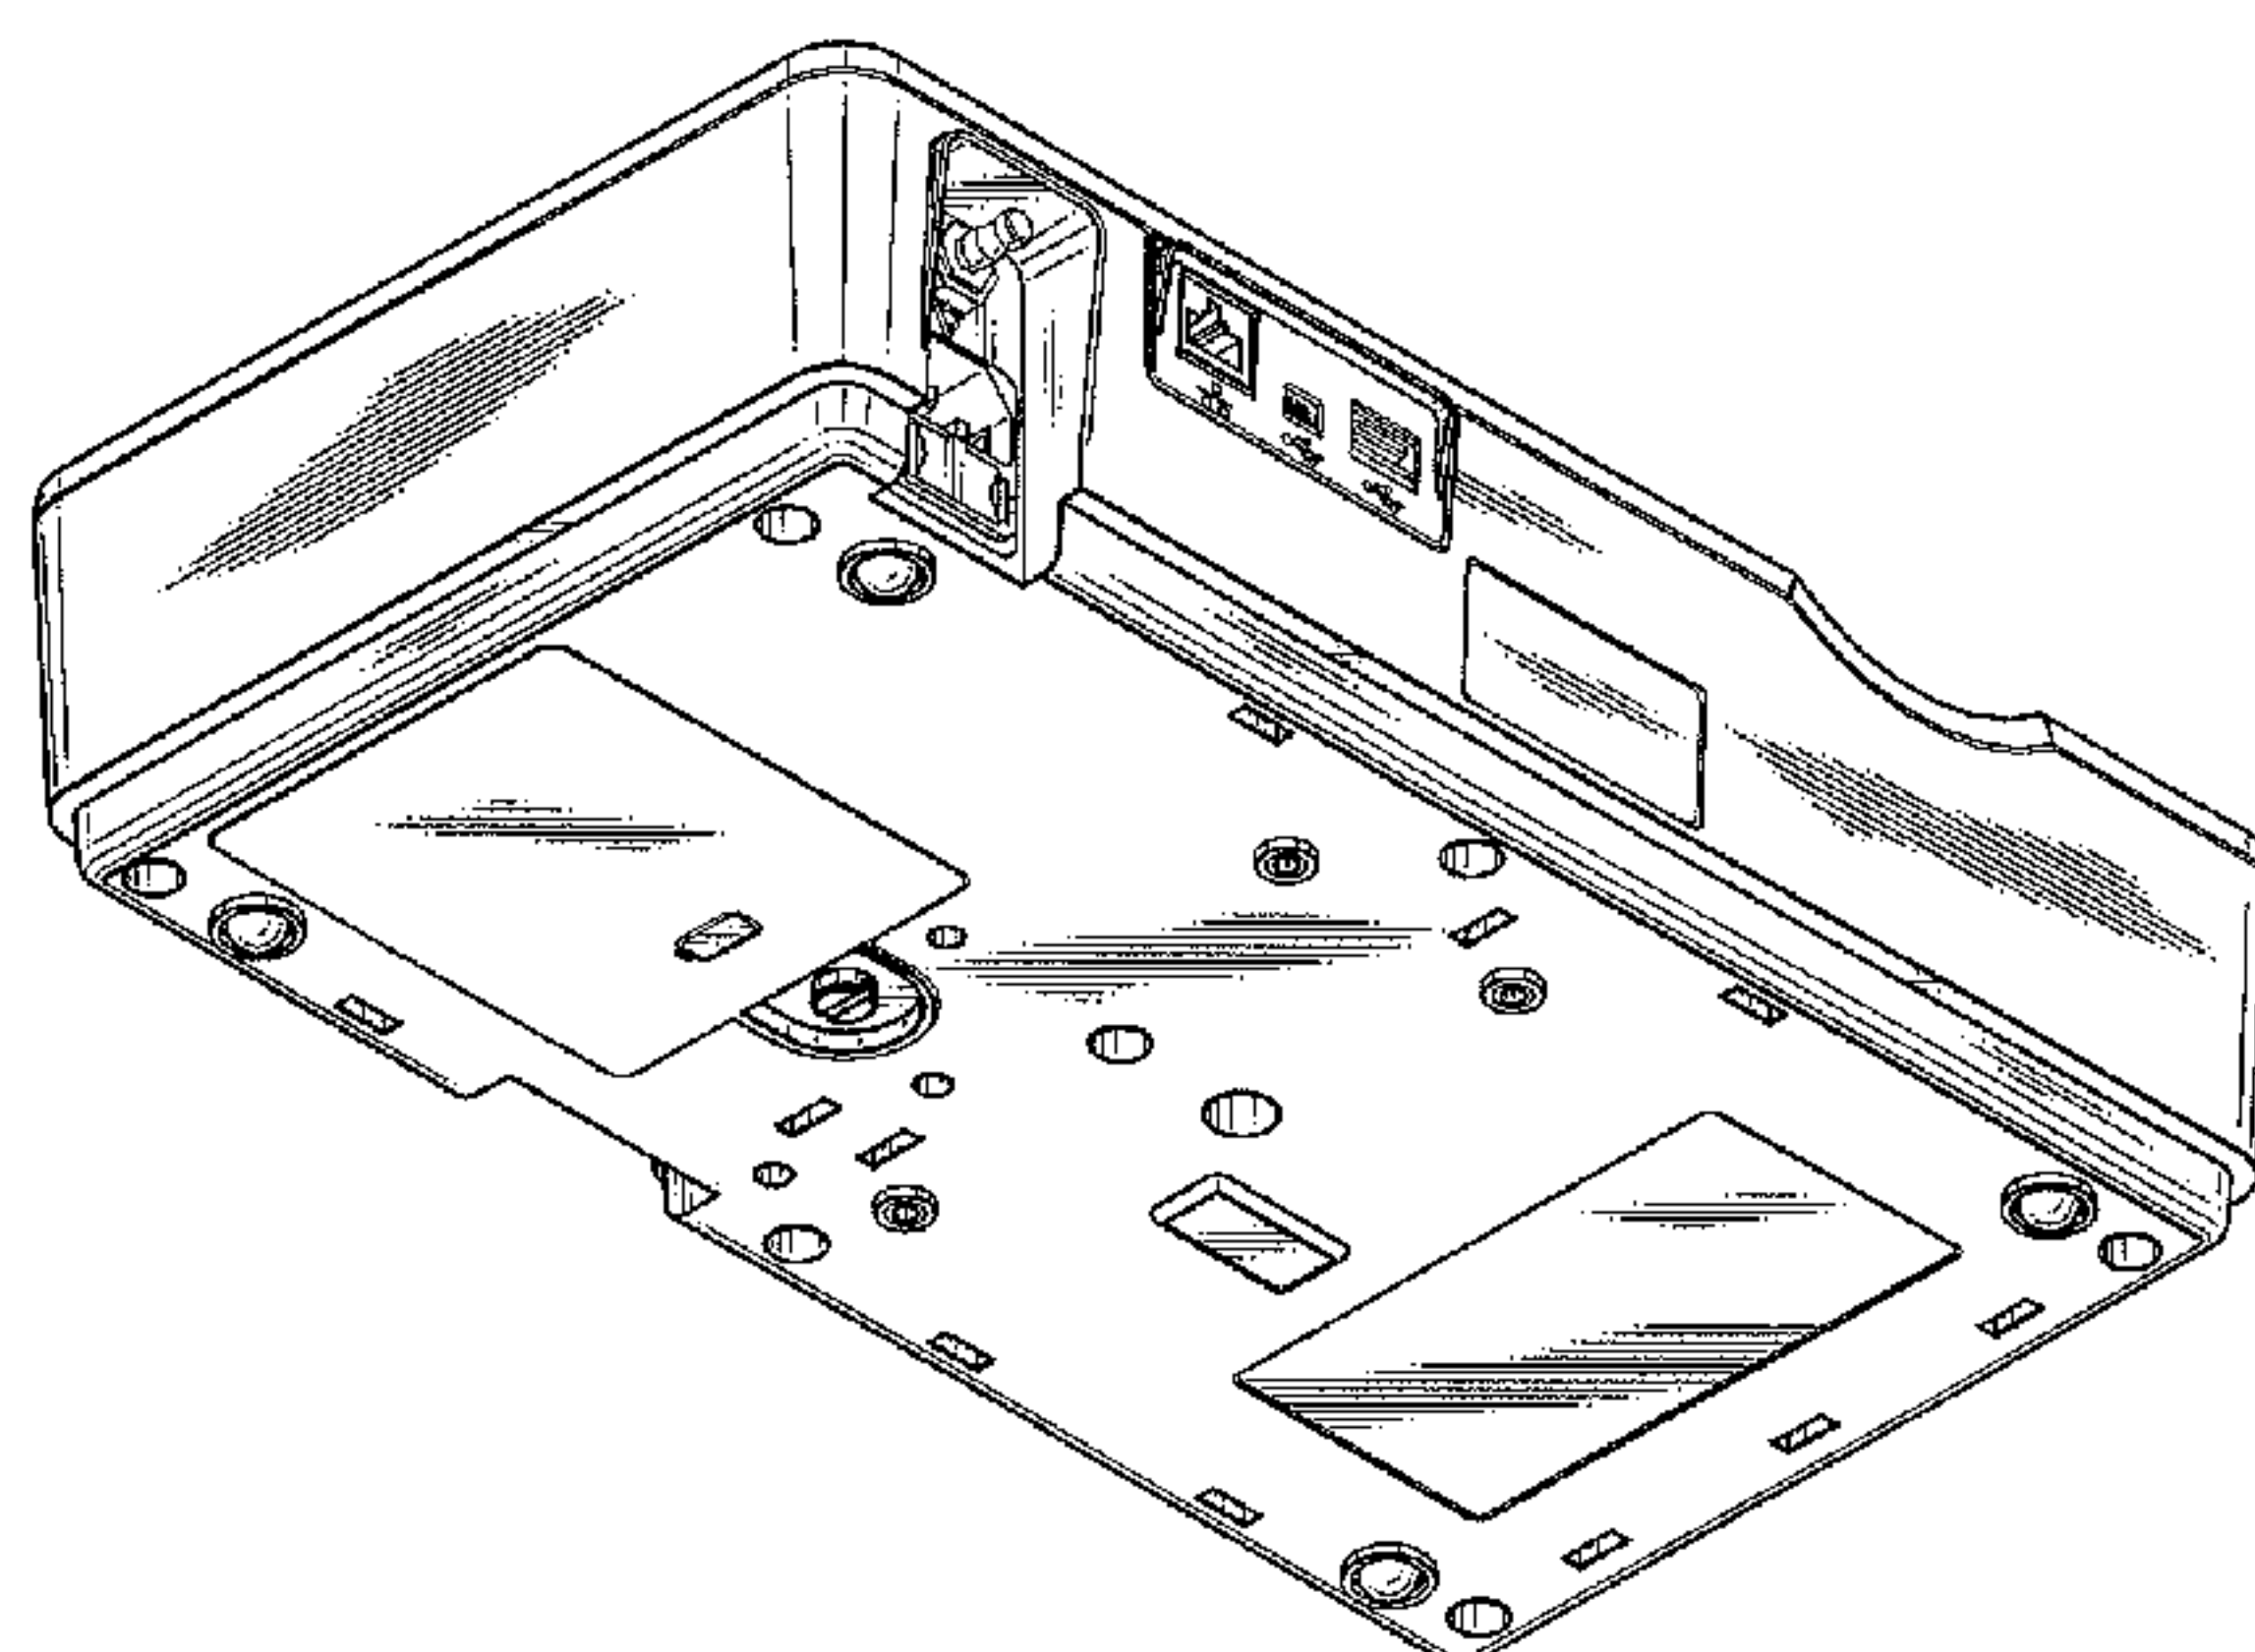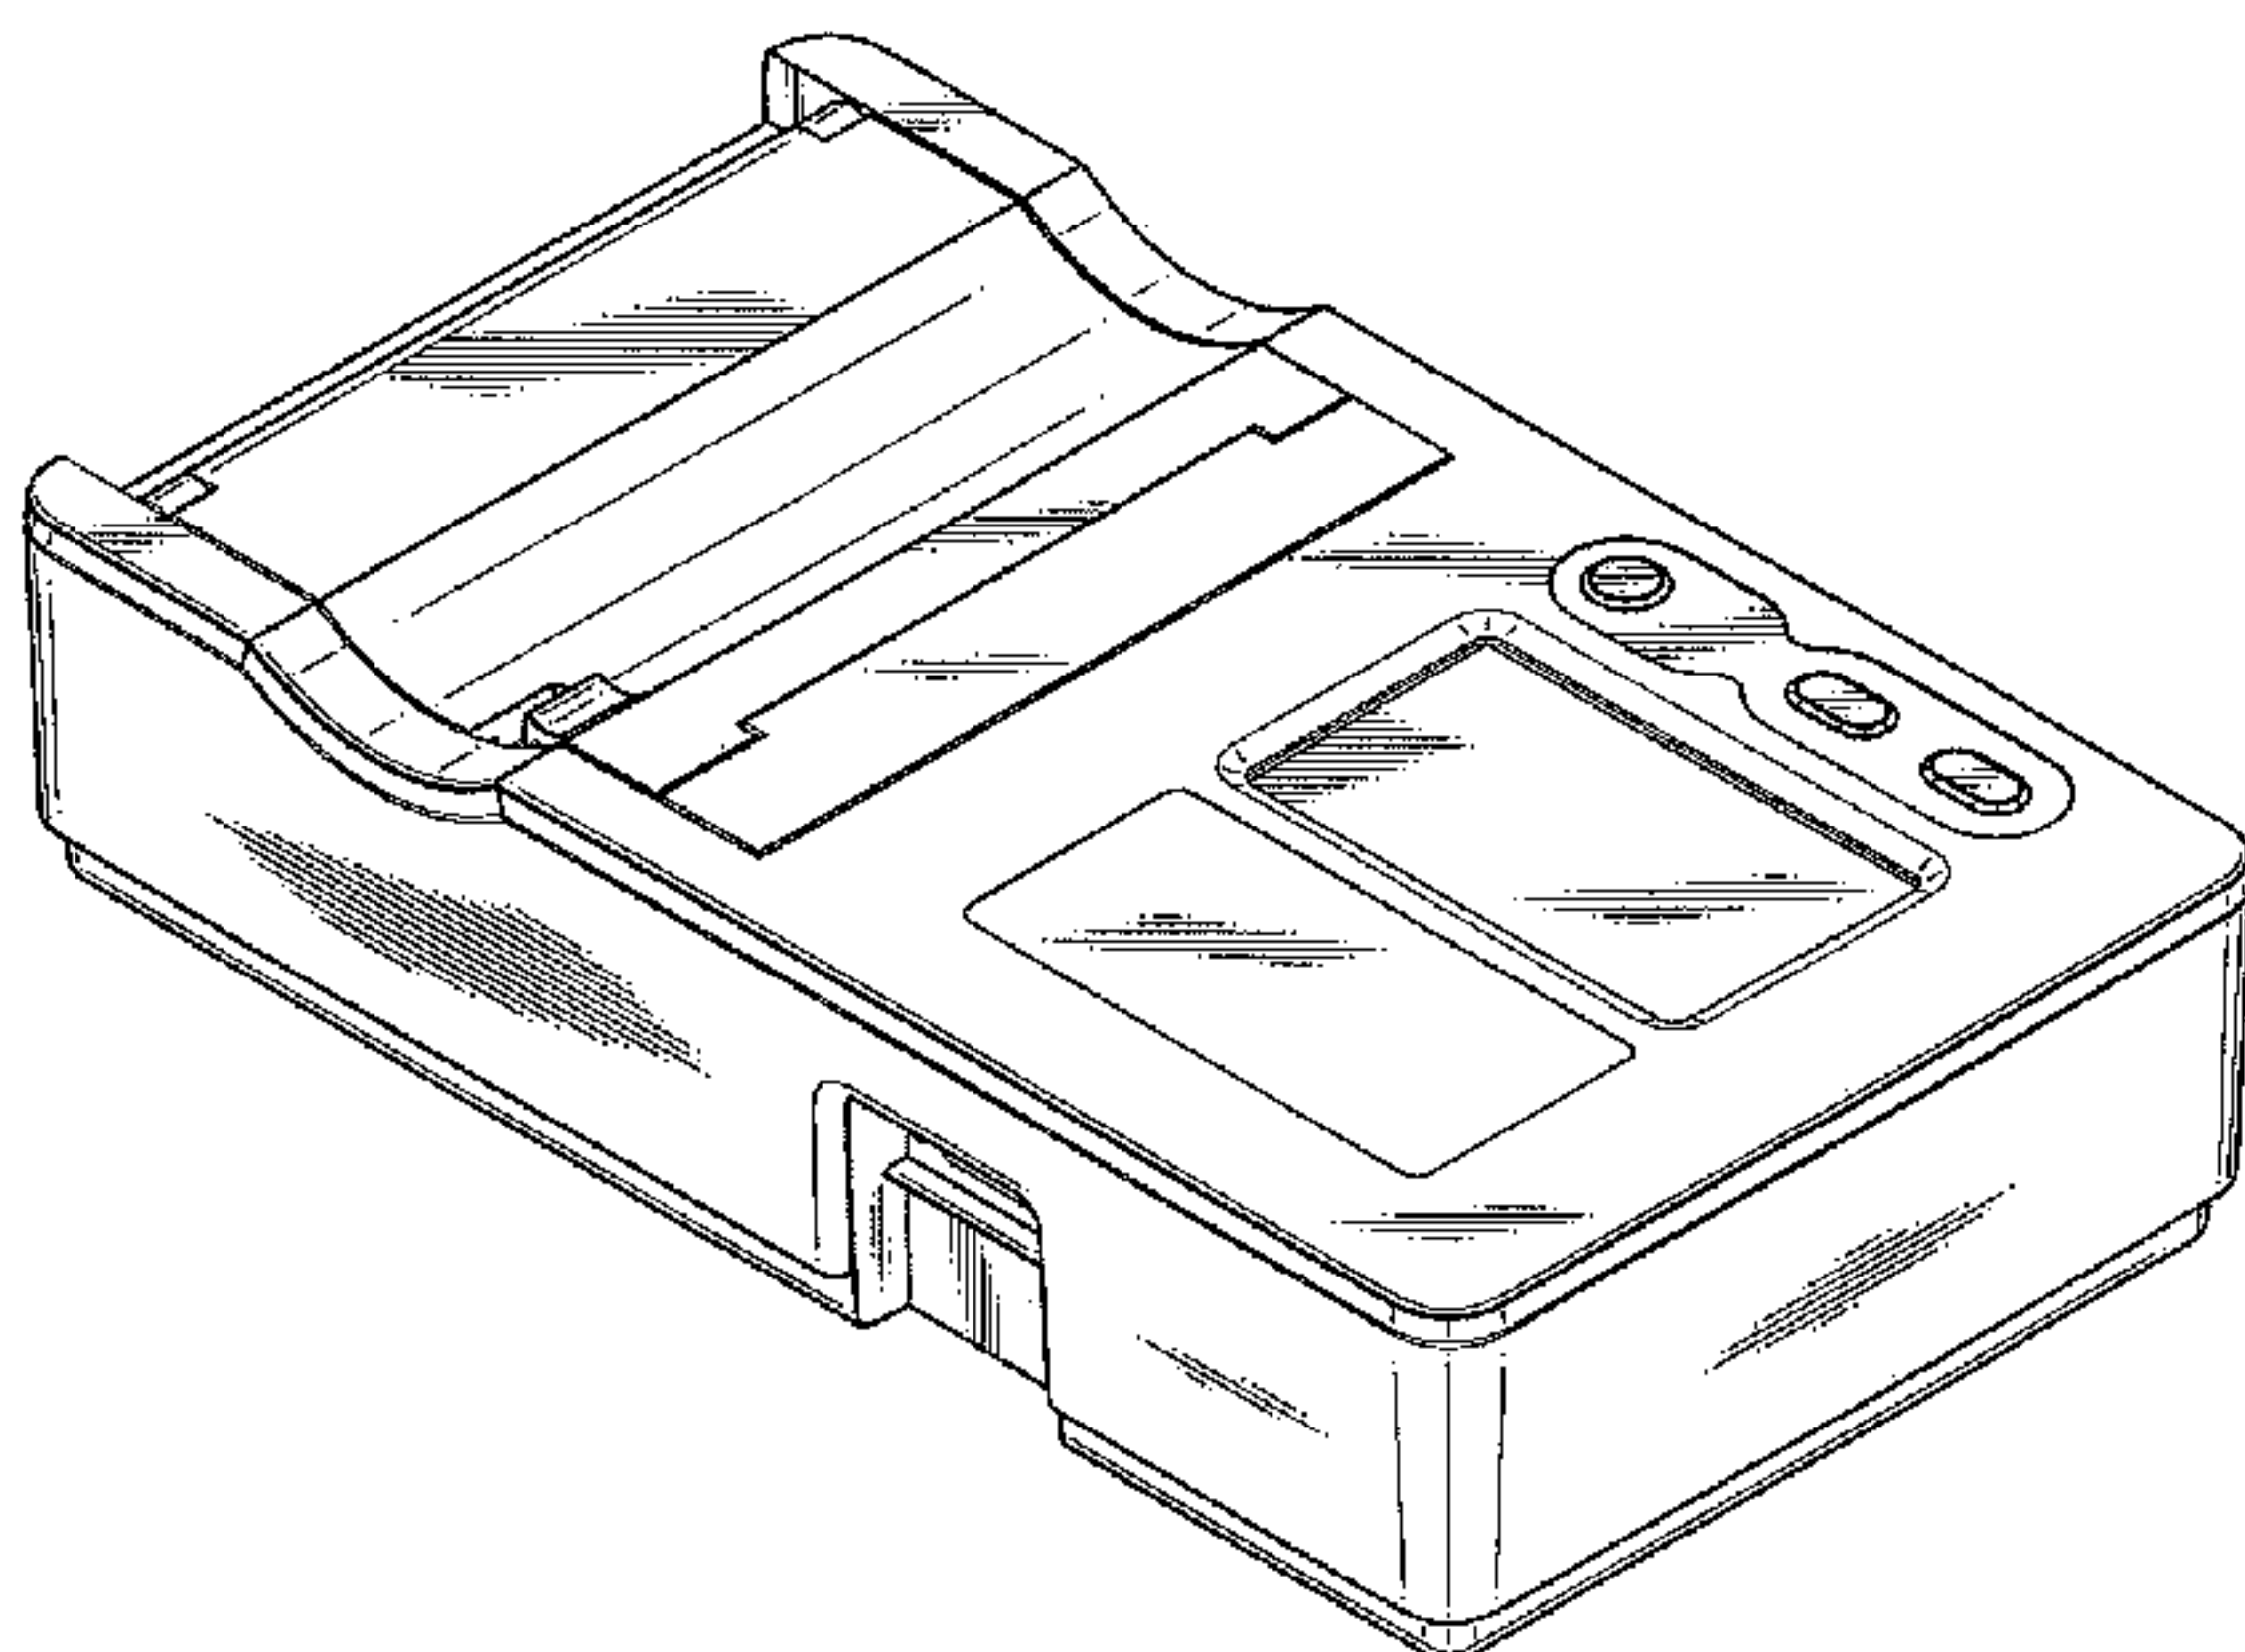

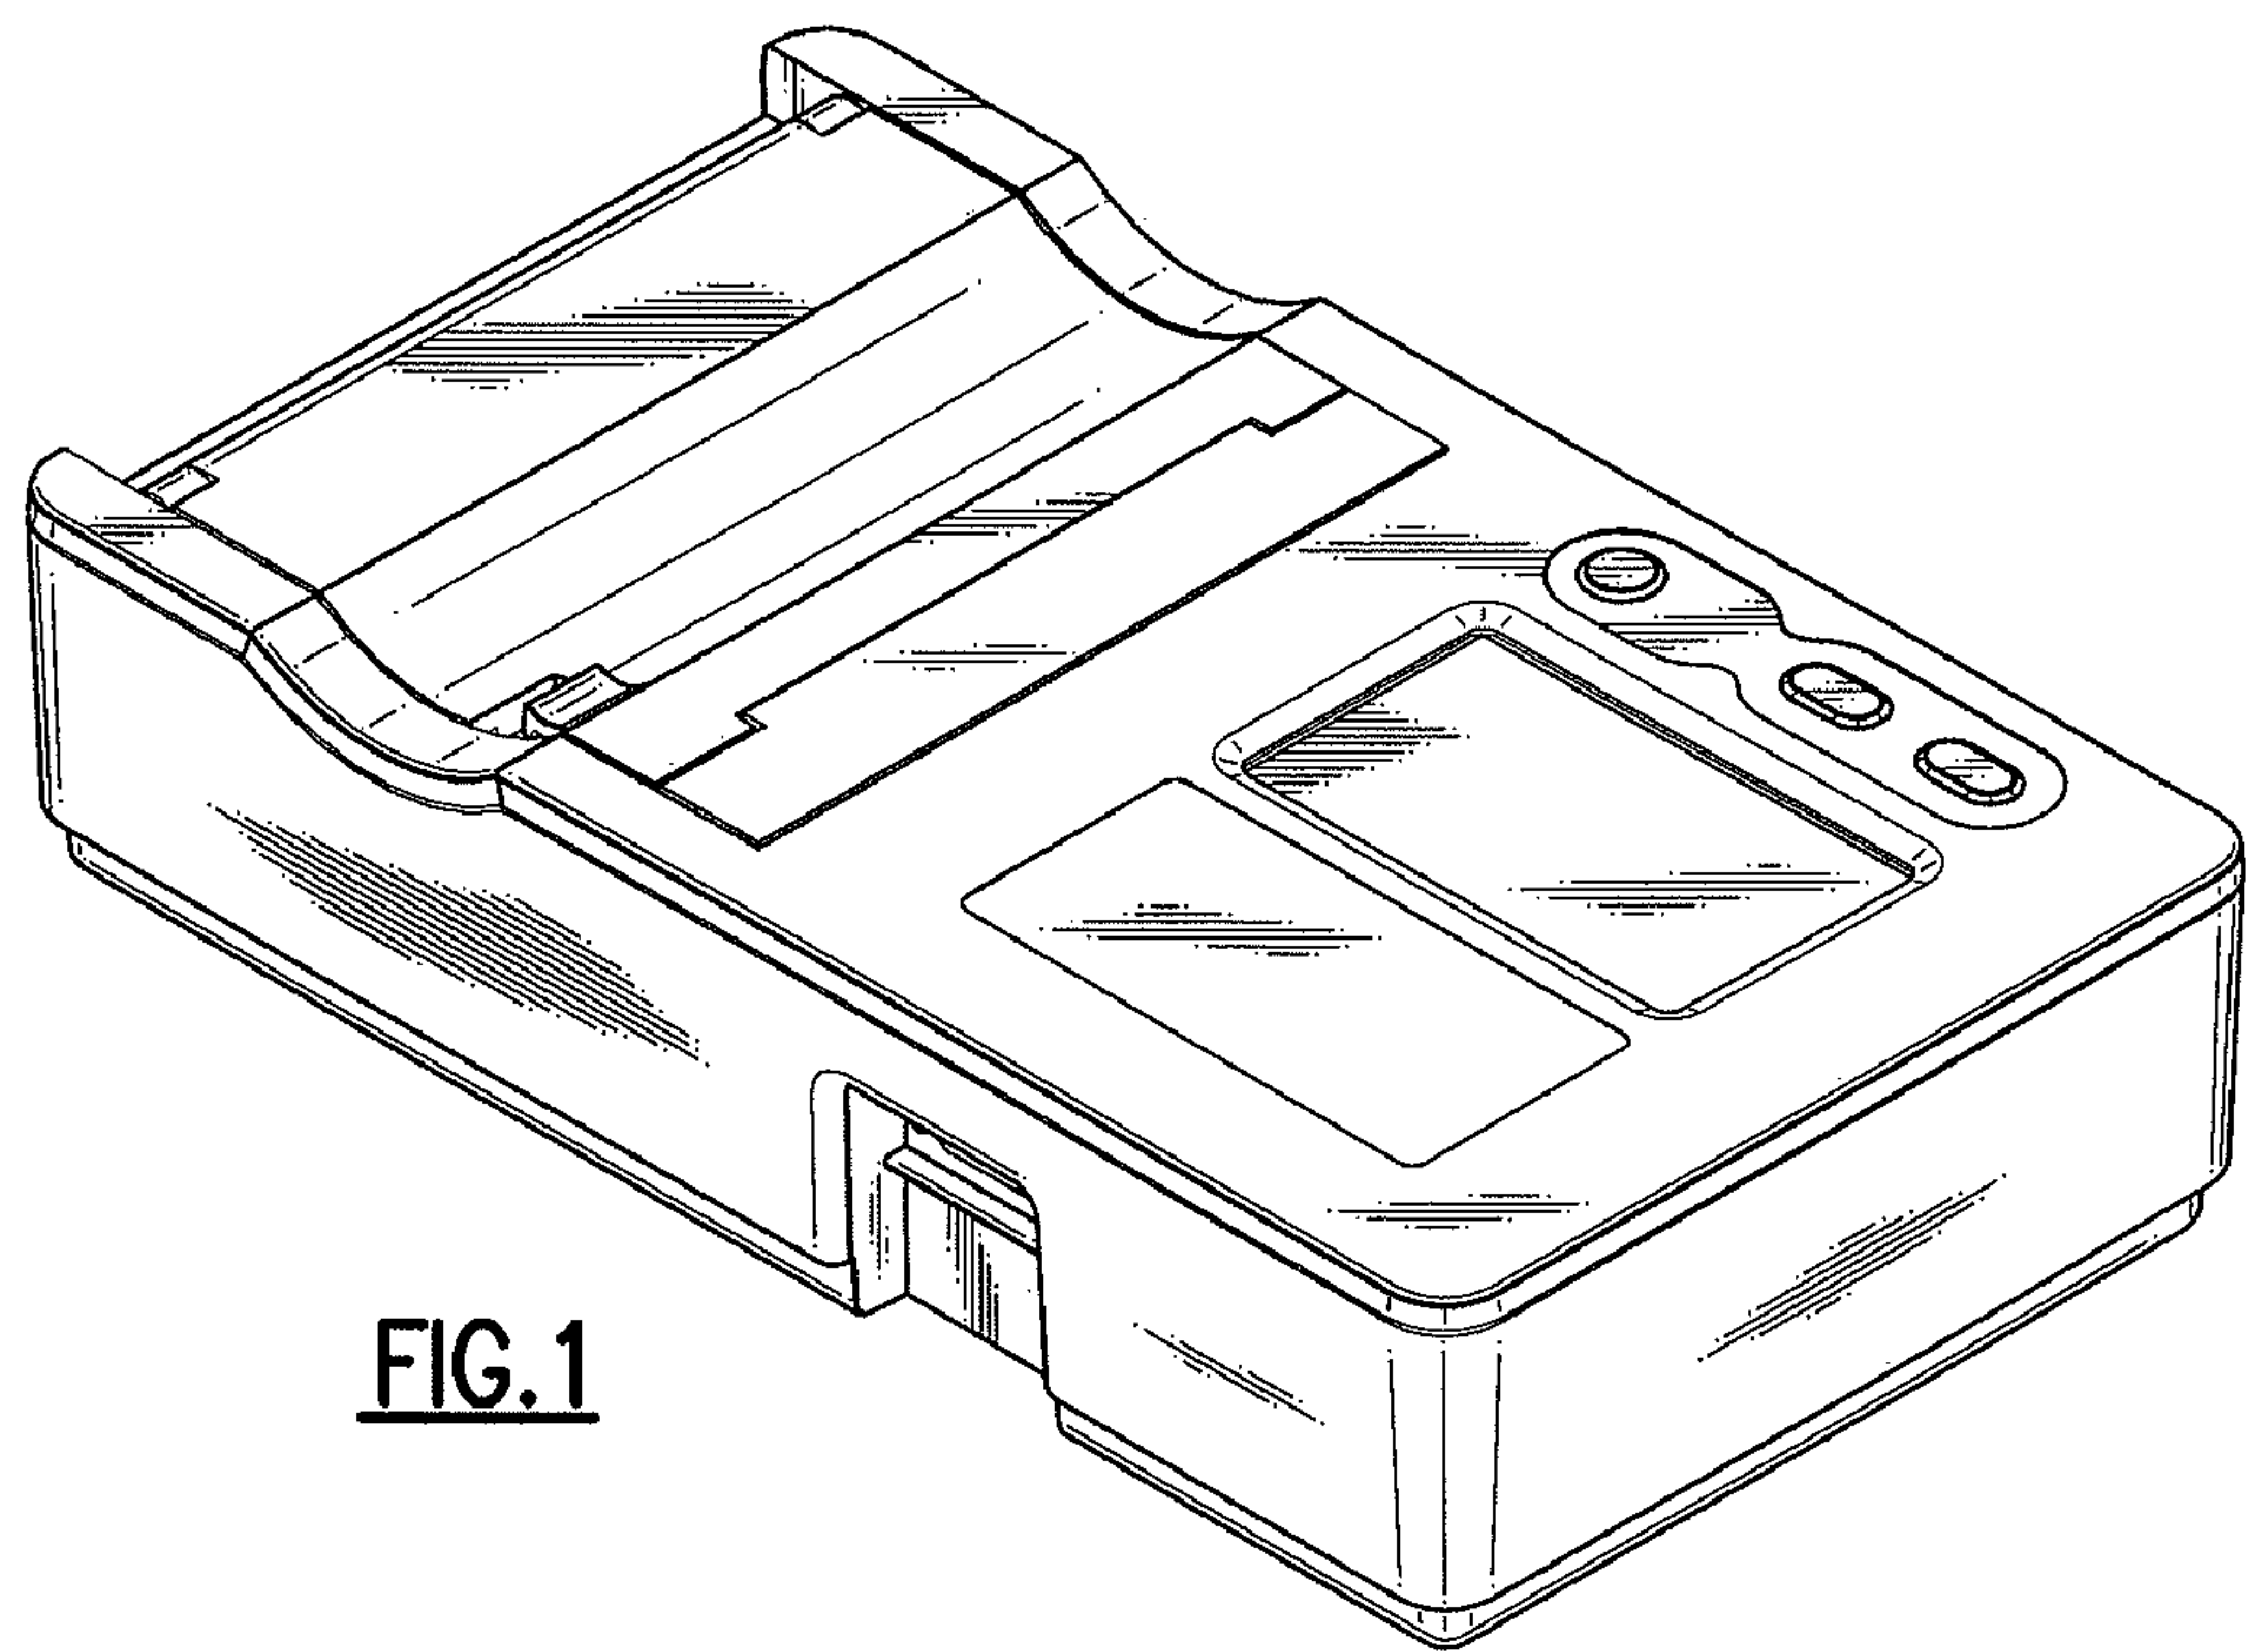


FIG. 1

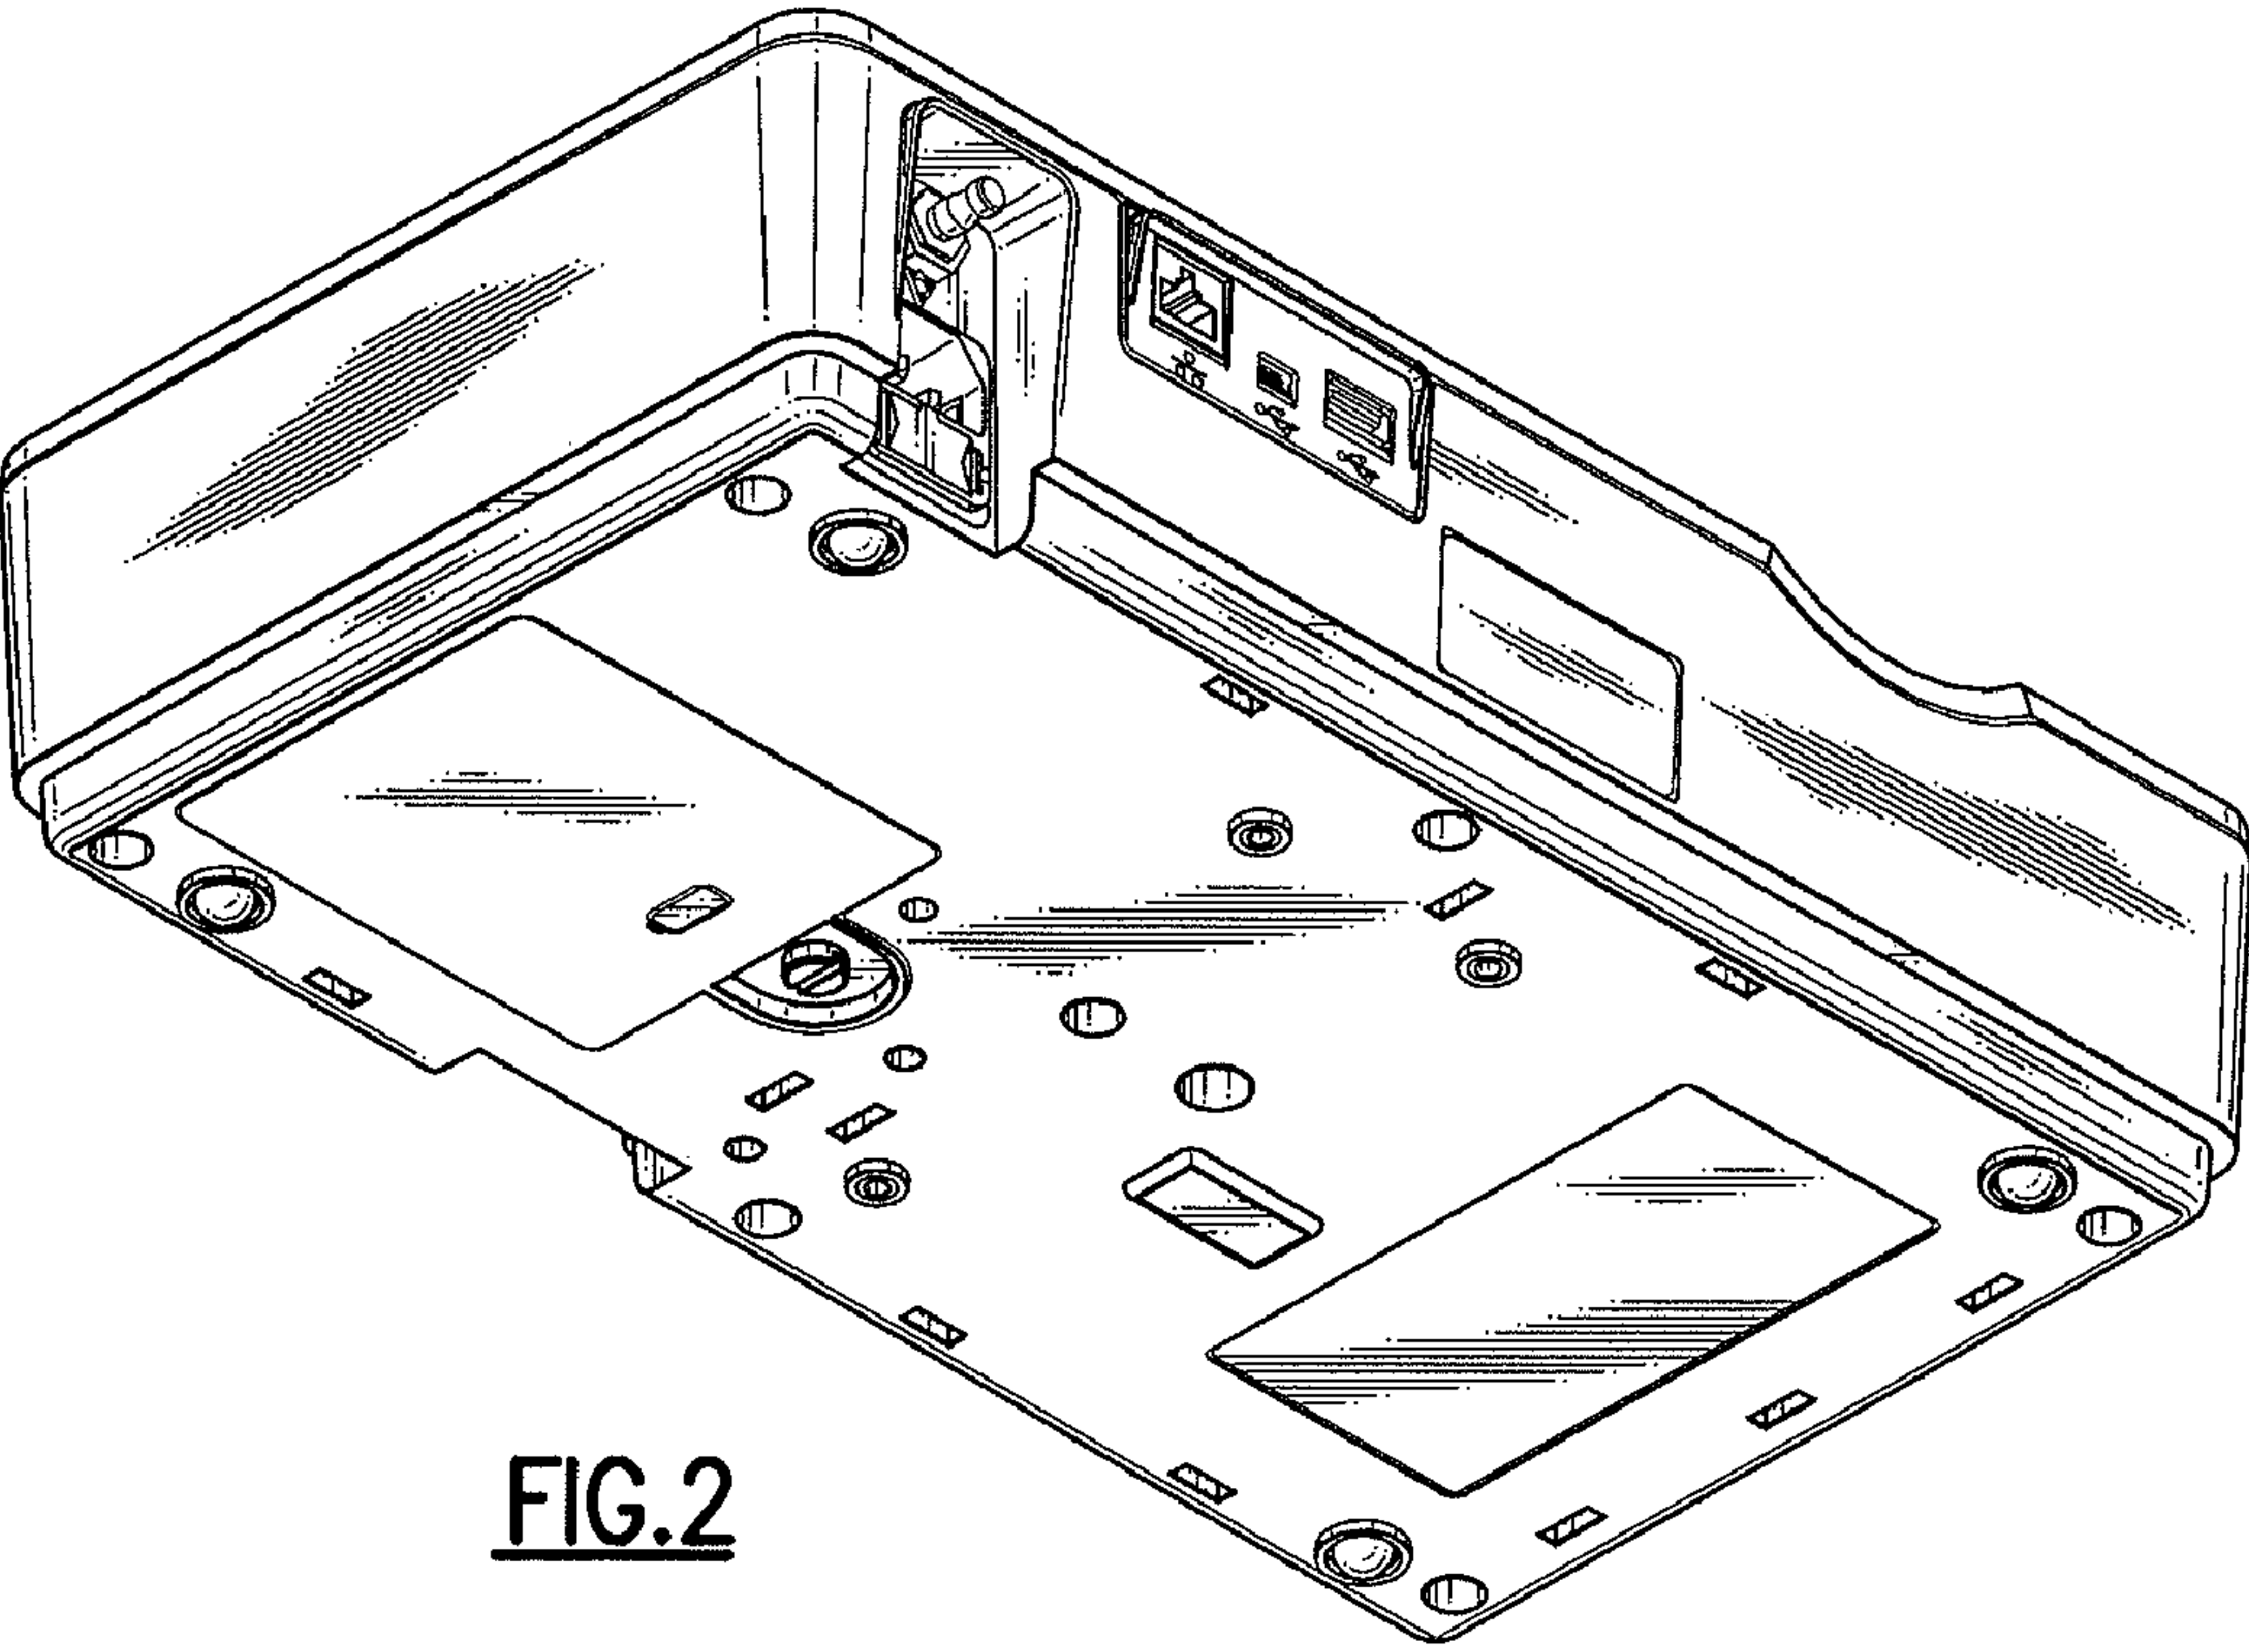


FIG. 2

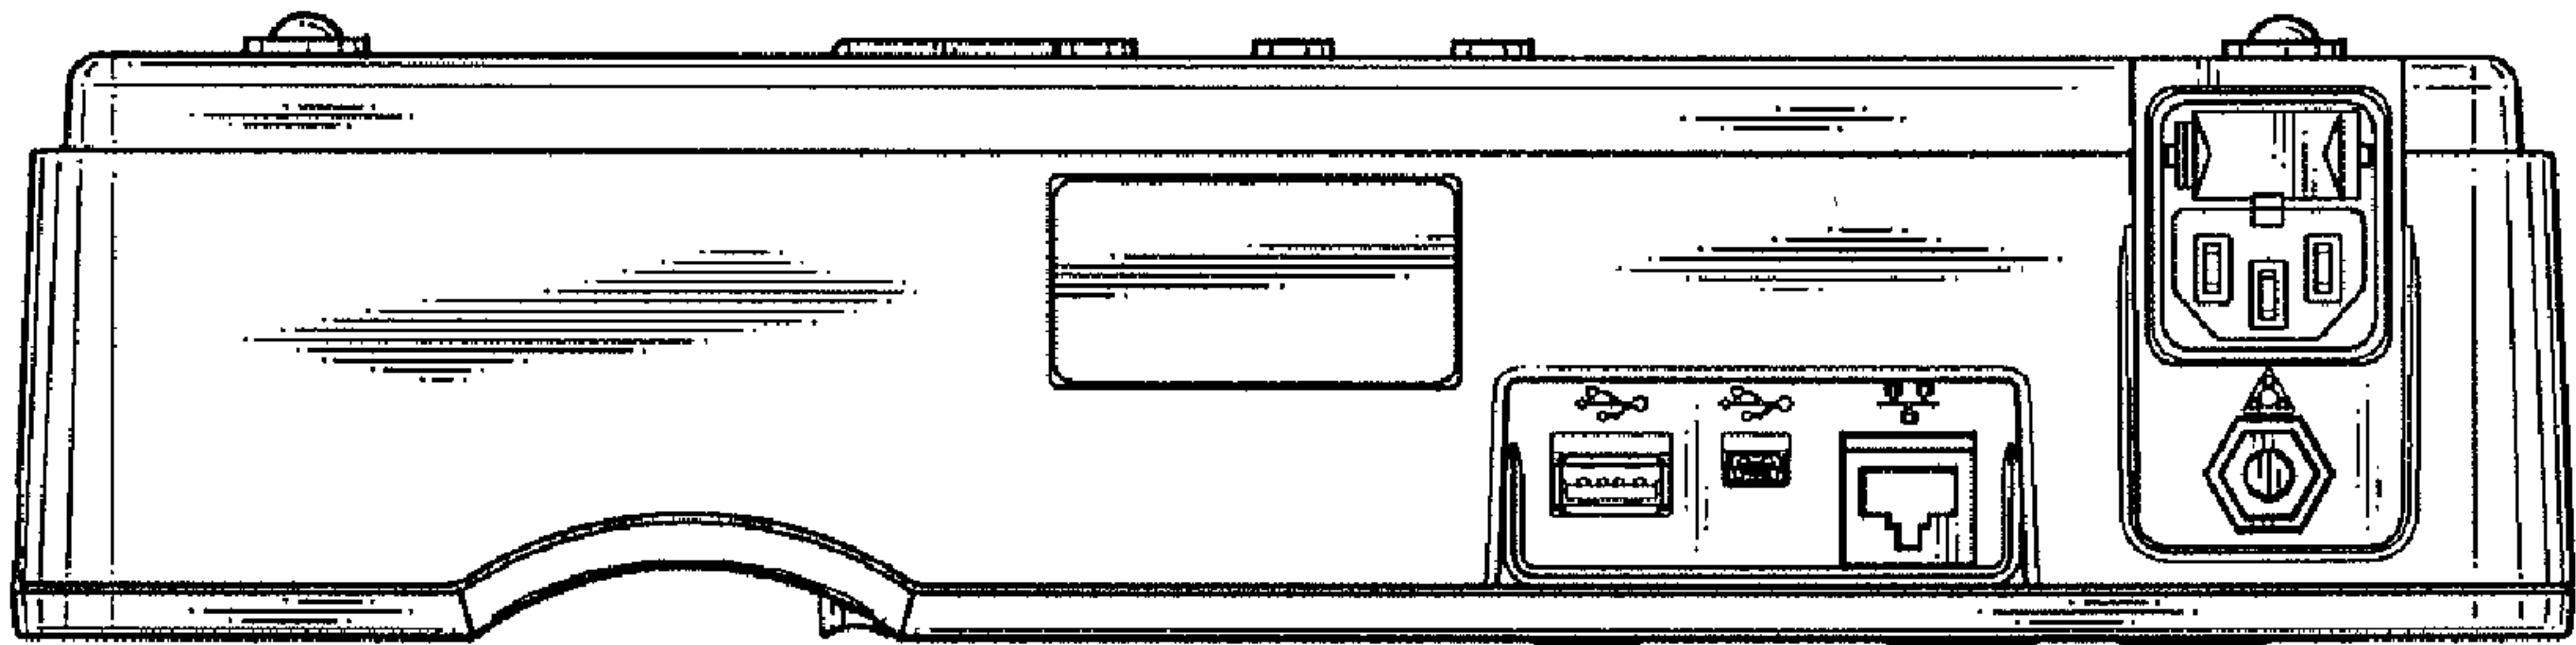


FIG. 5

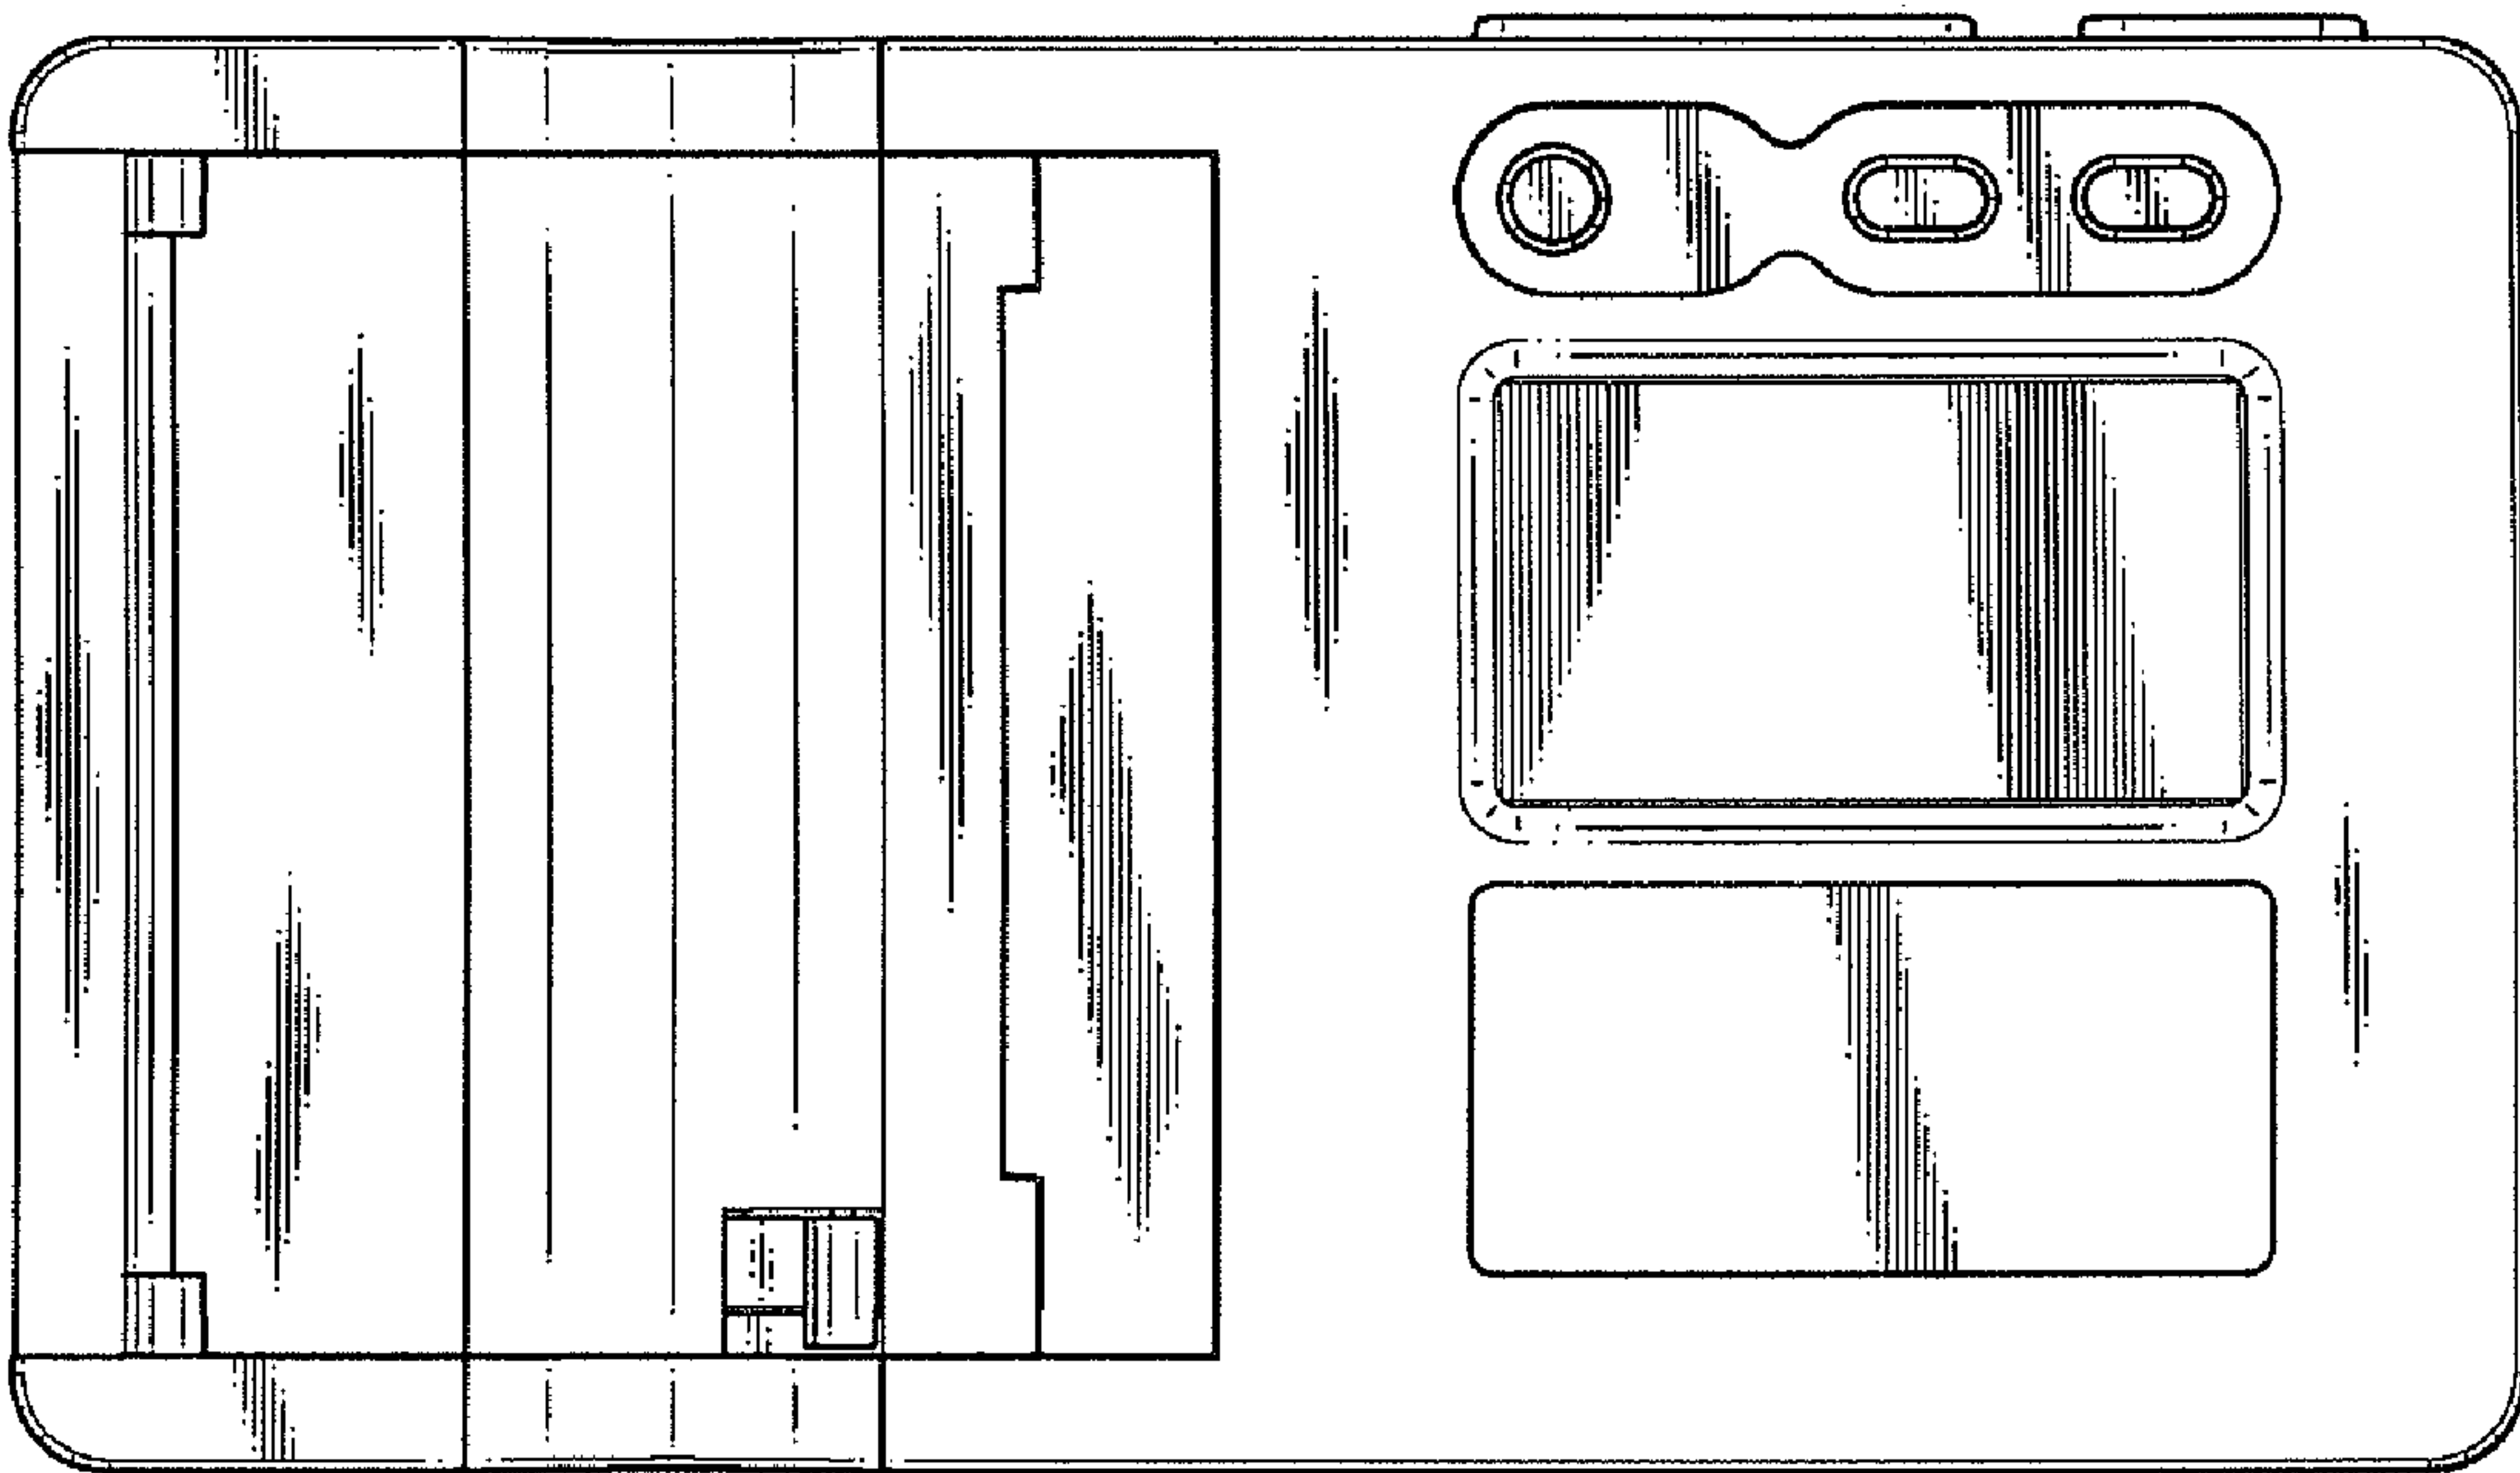


FIG. 3

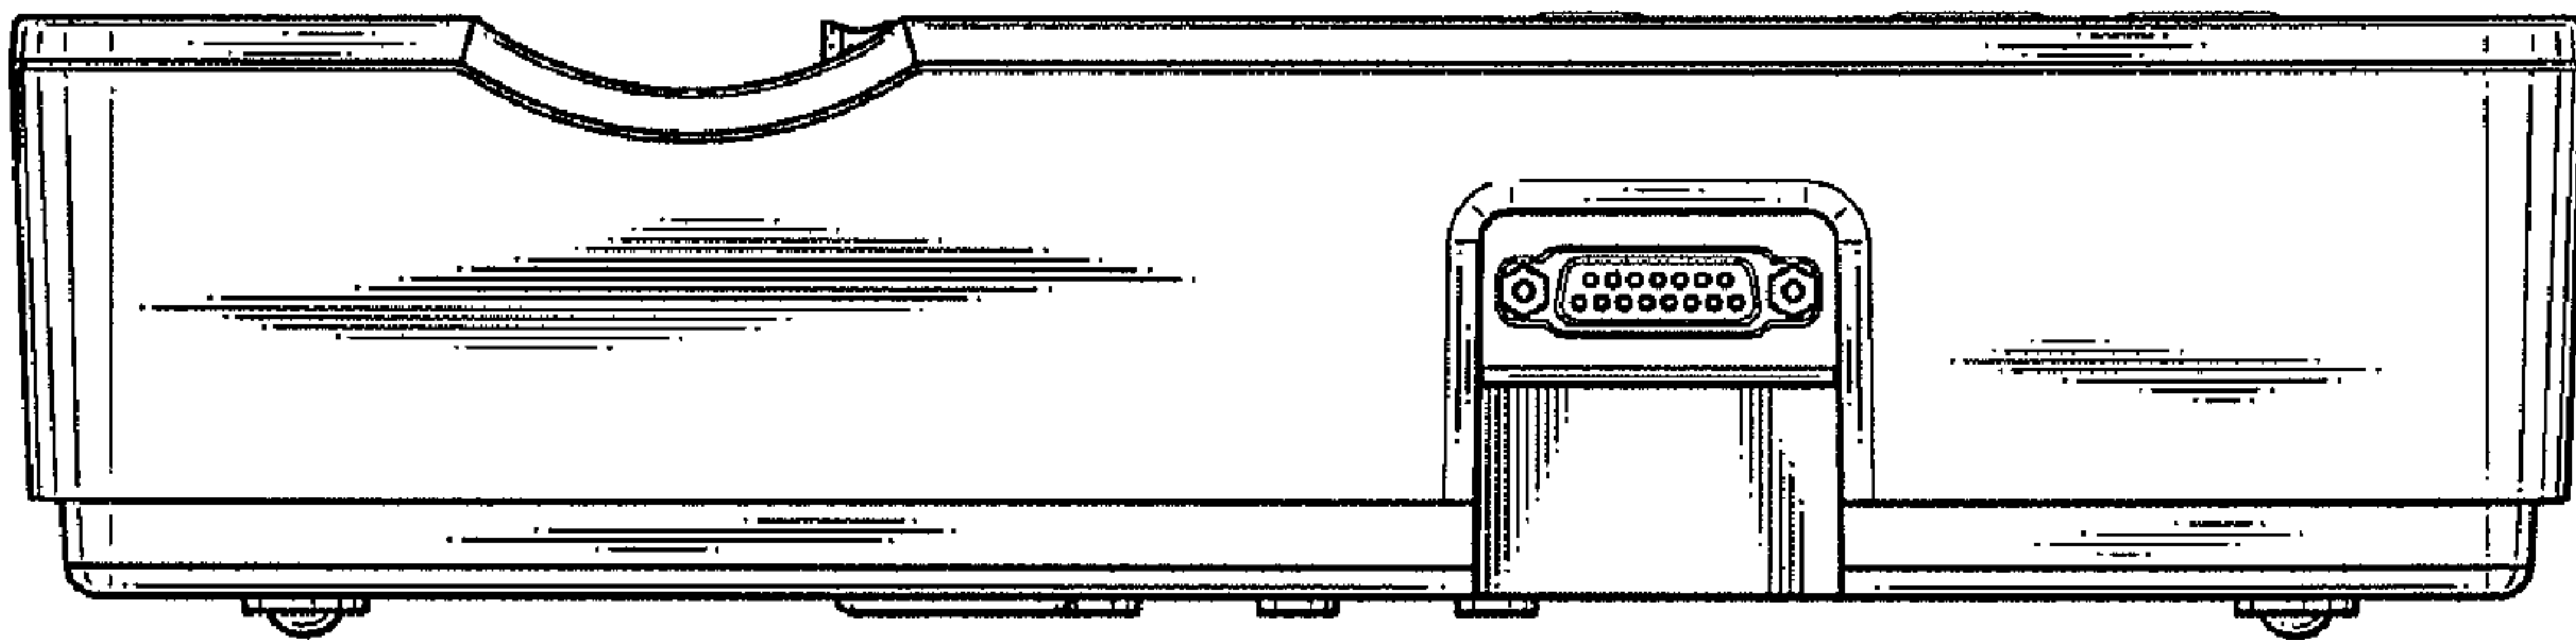


FIG. 4

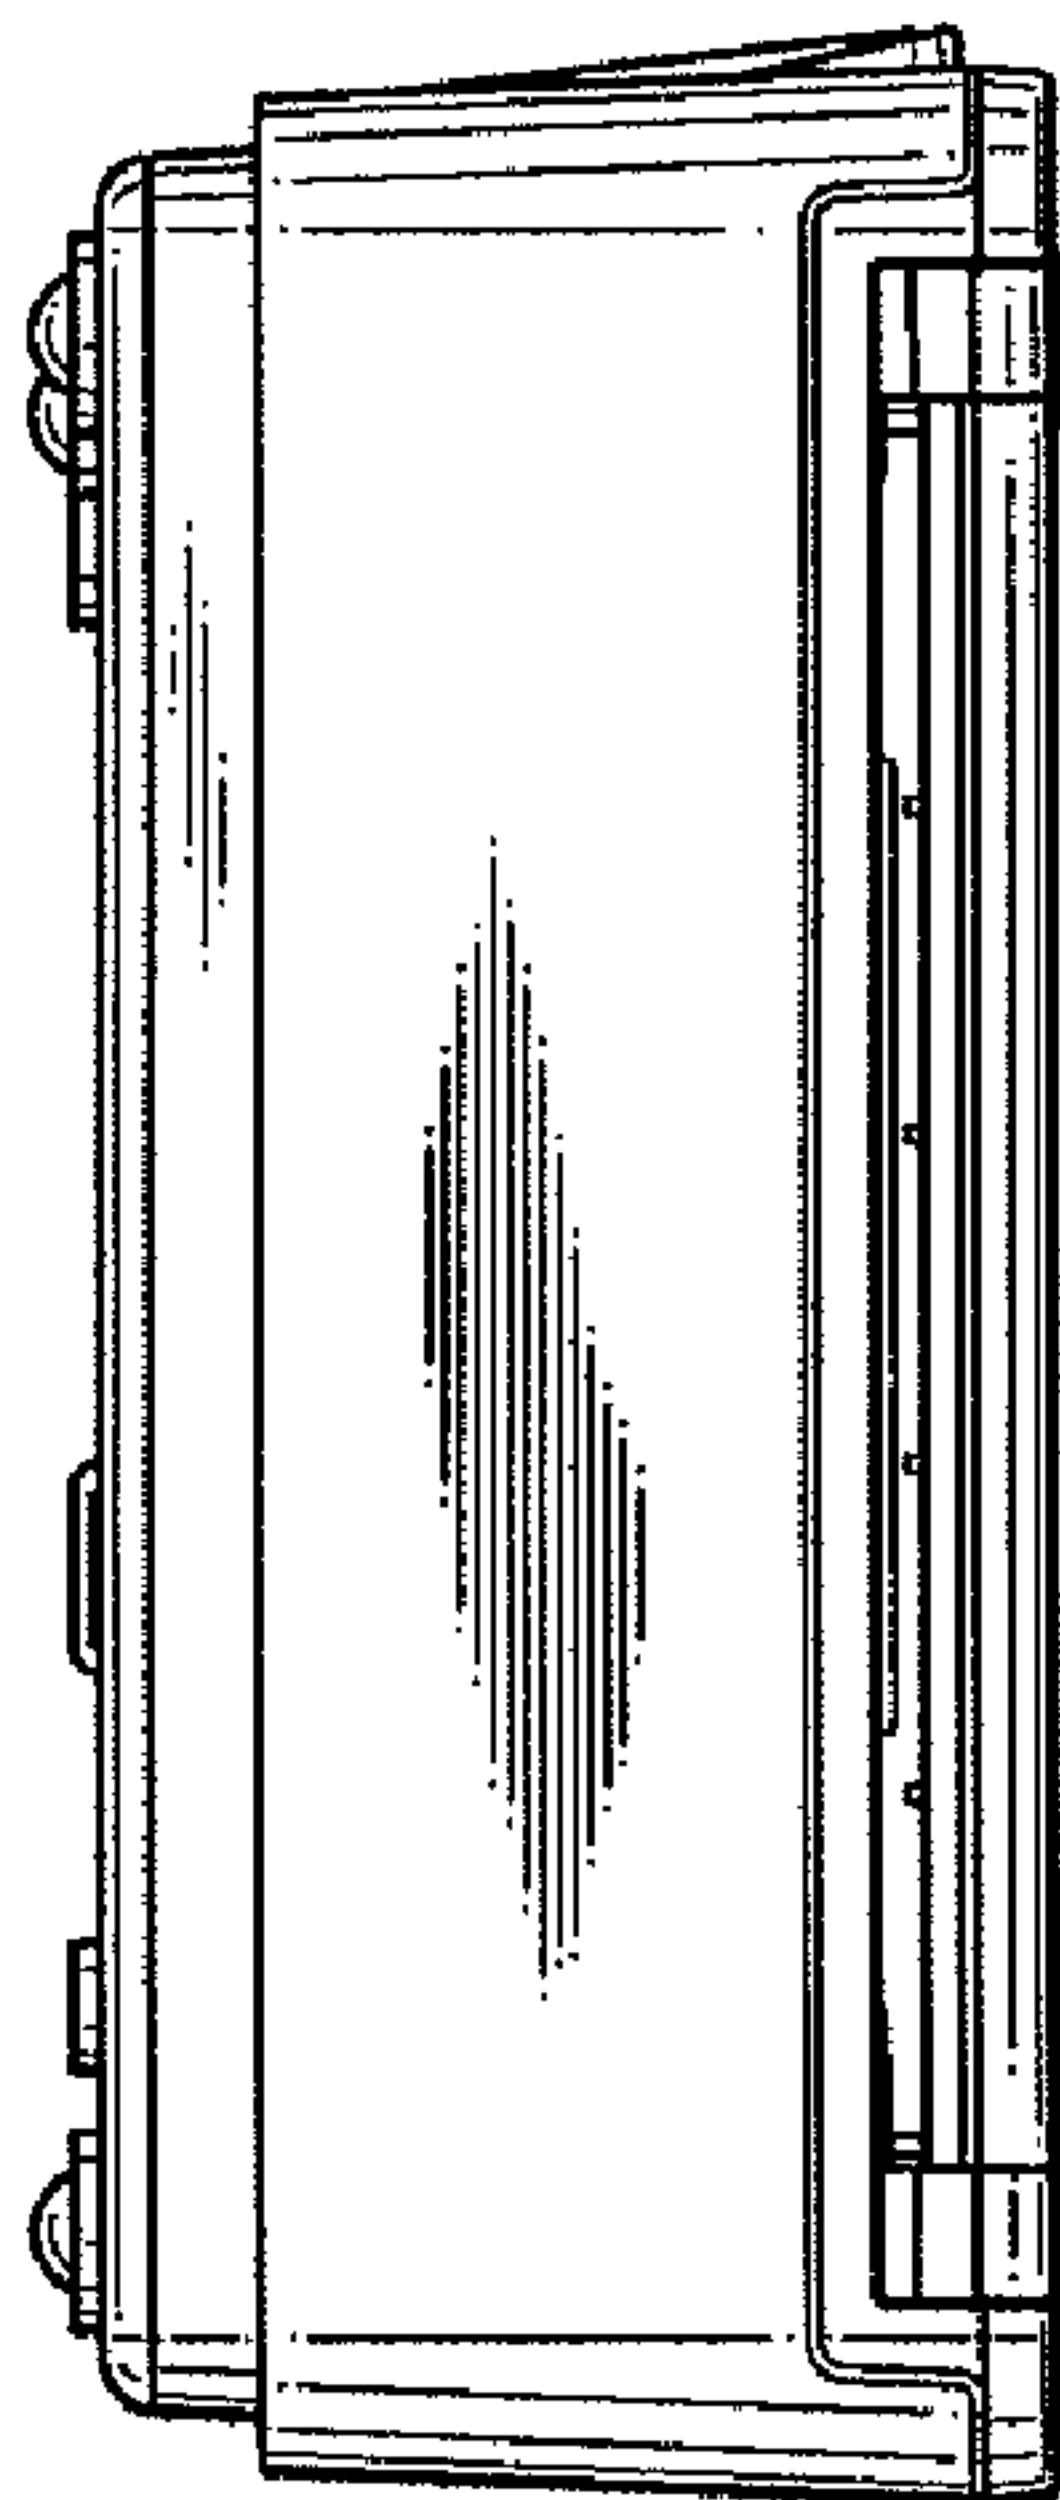


FIG.6

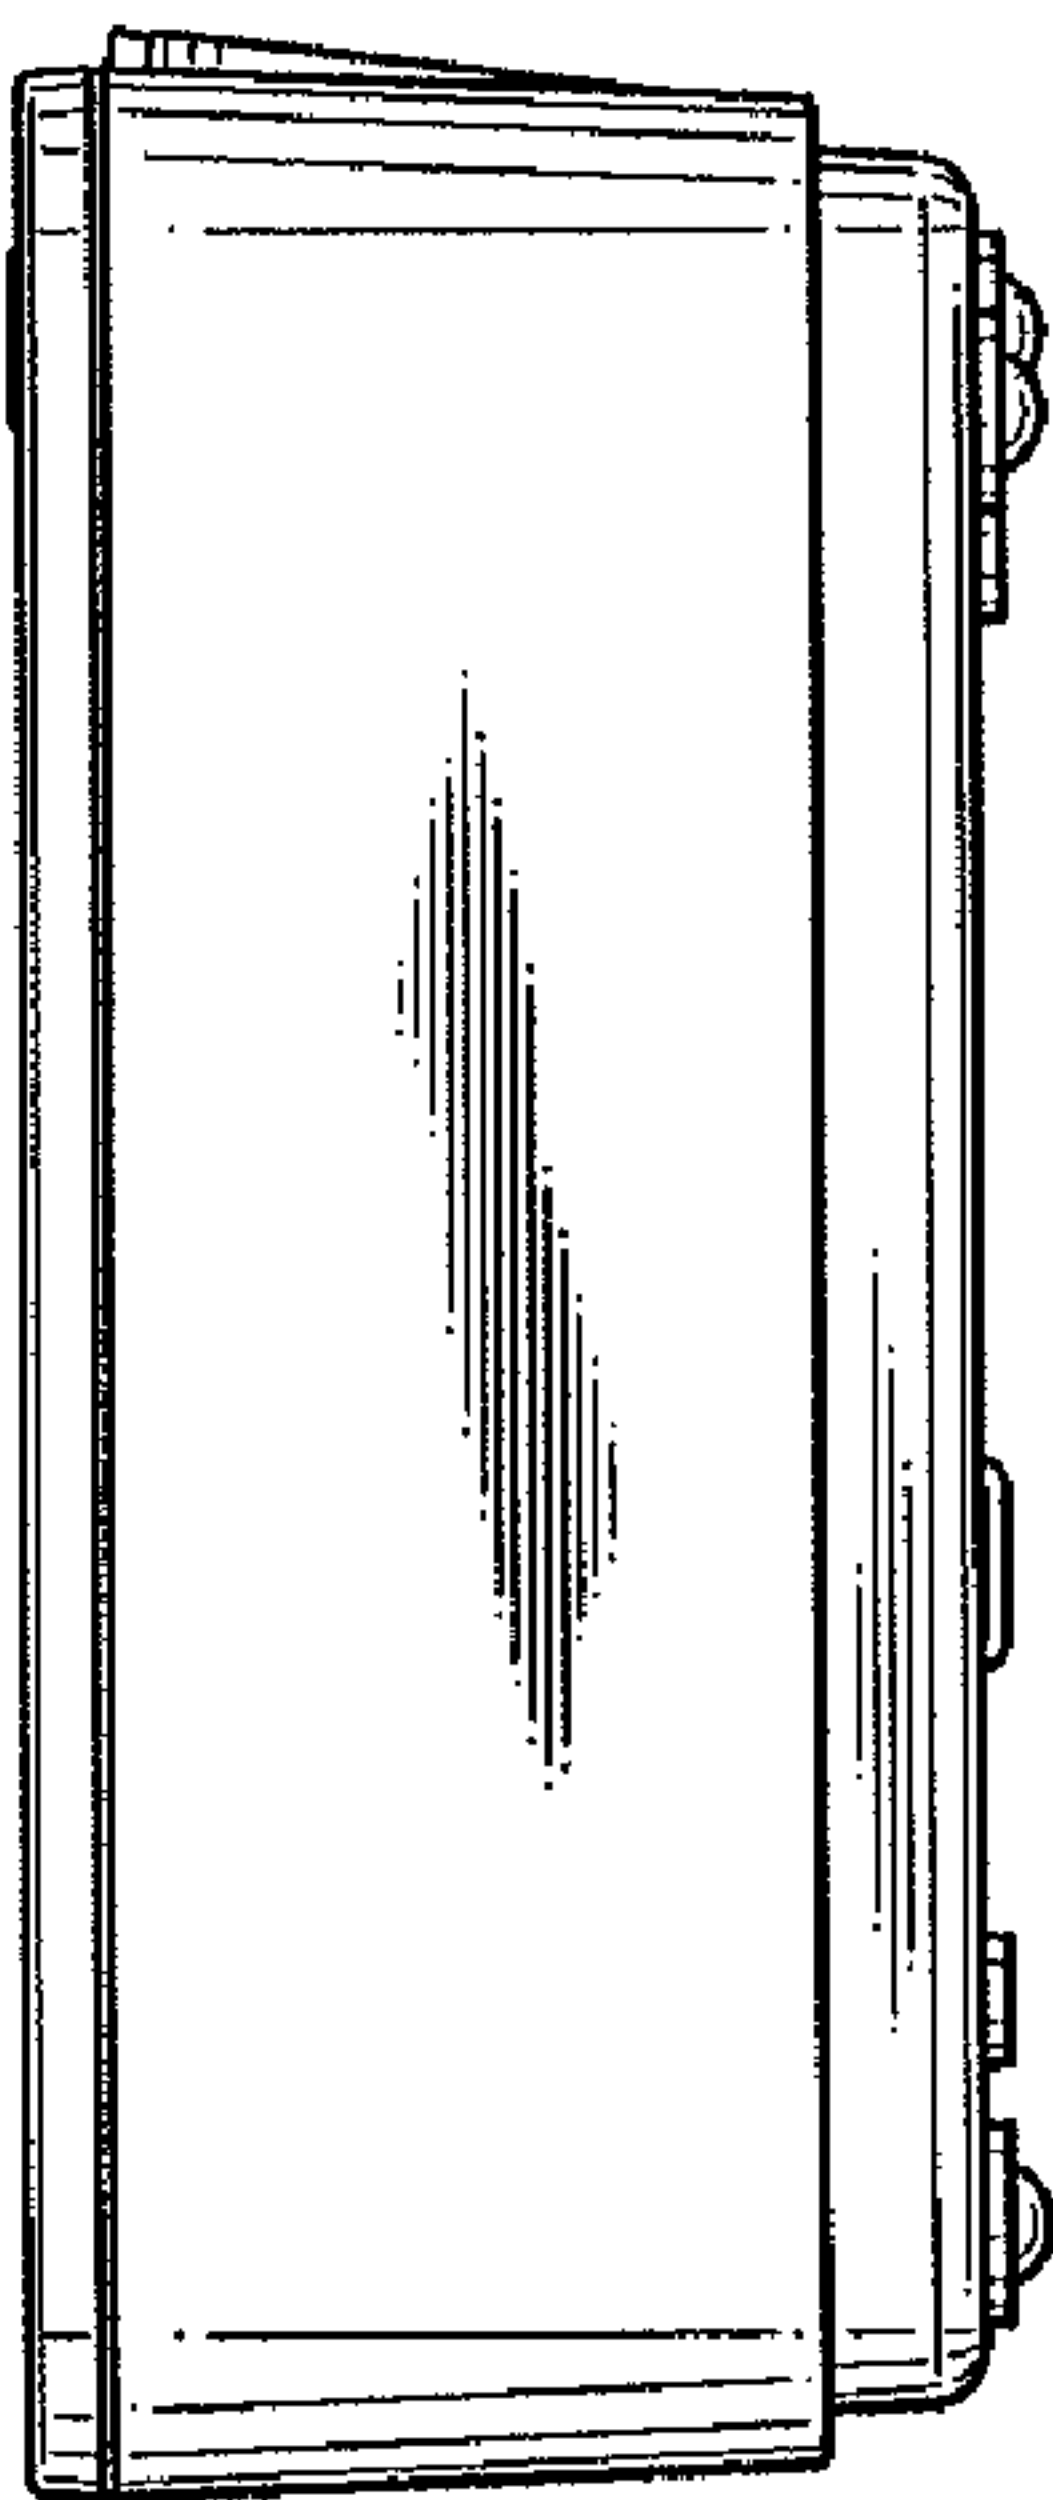


FIG.7

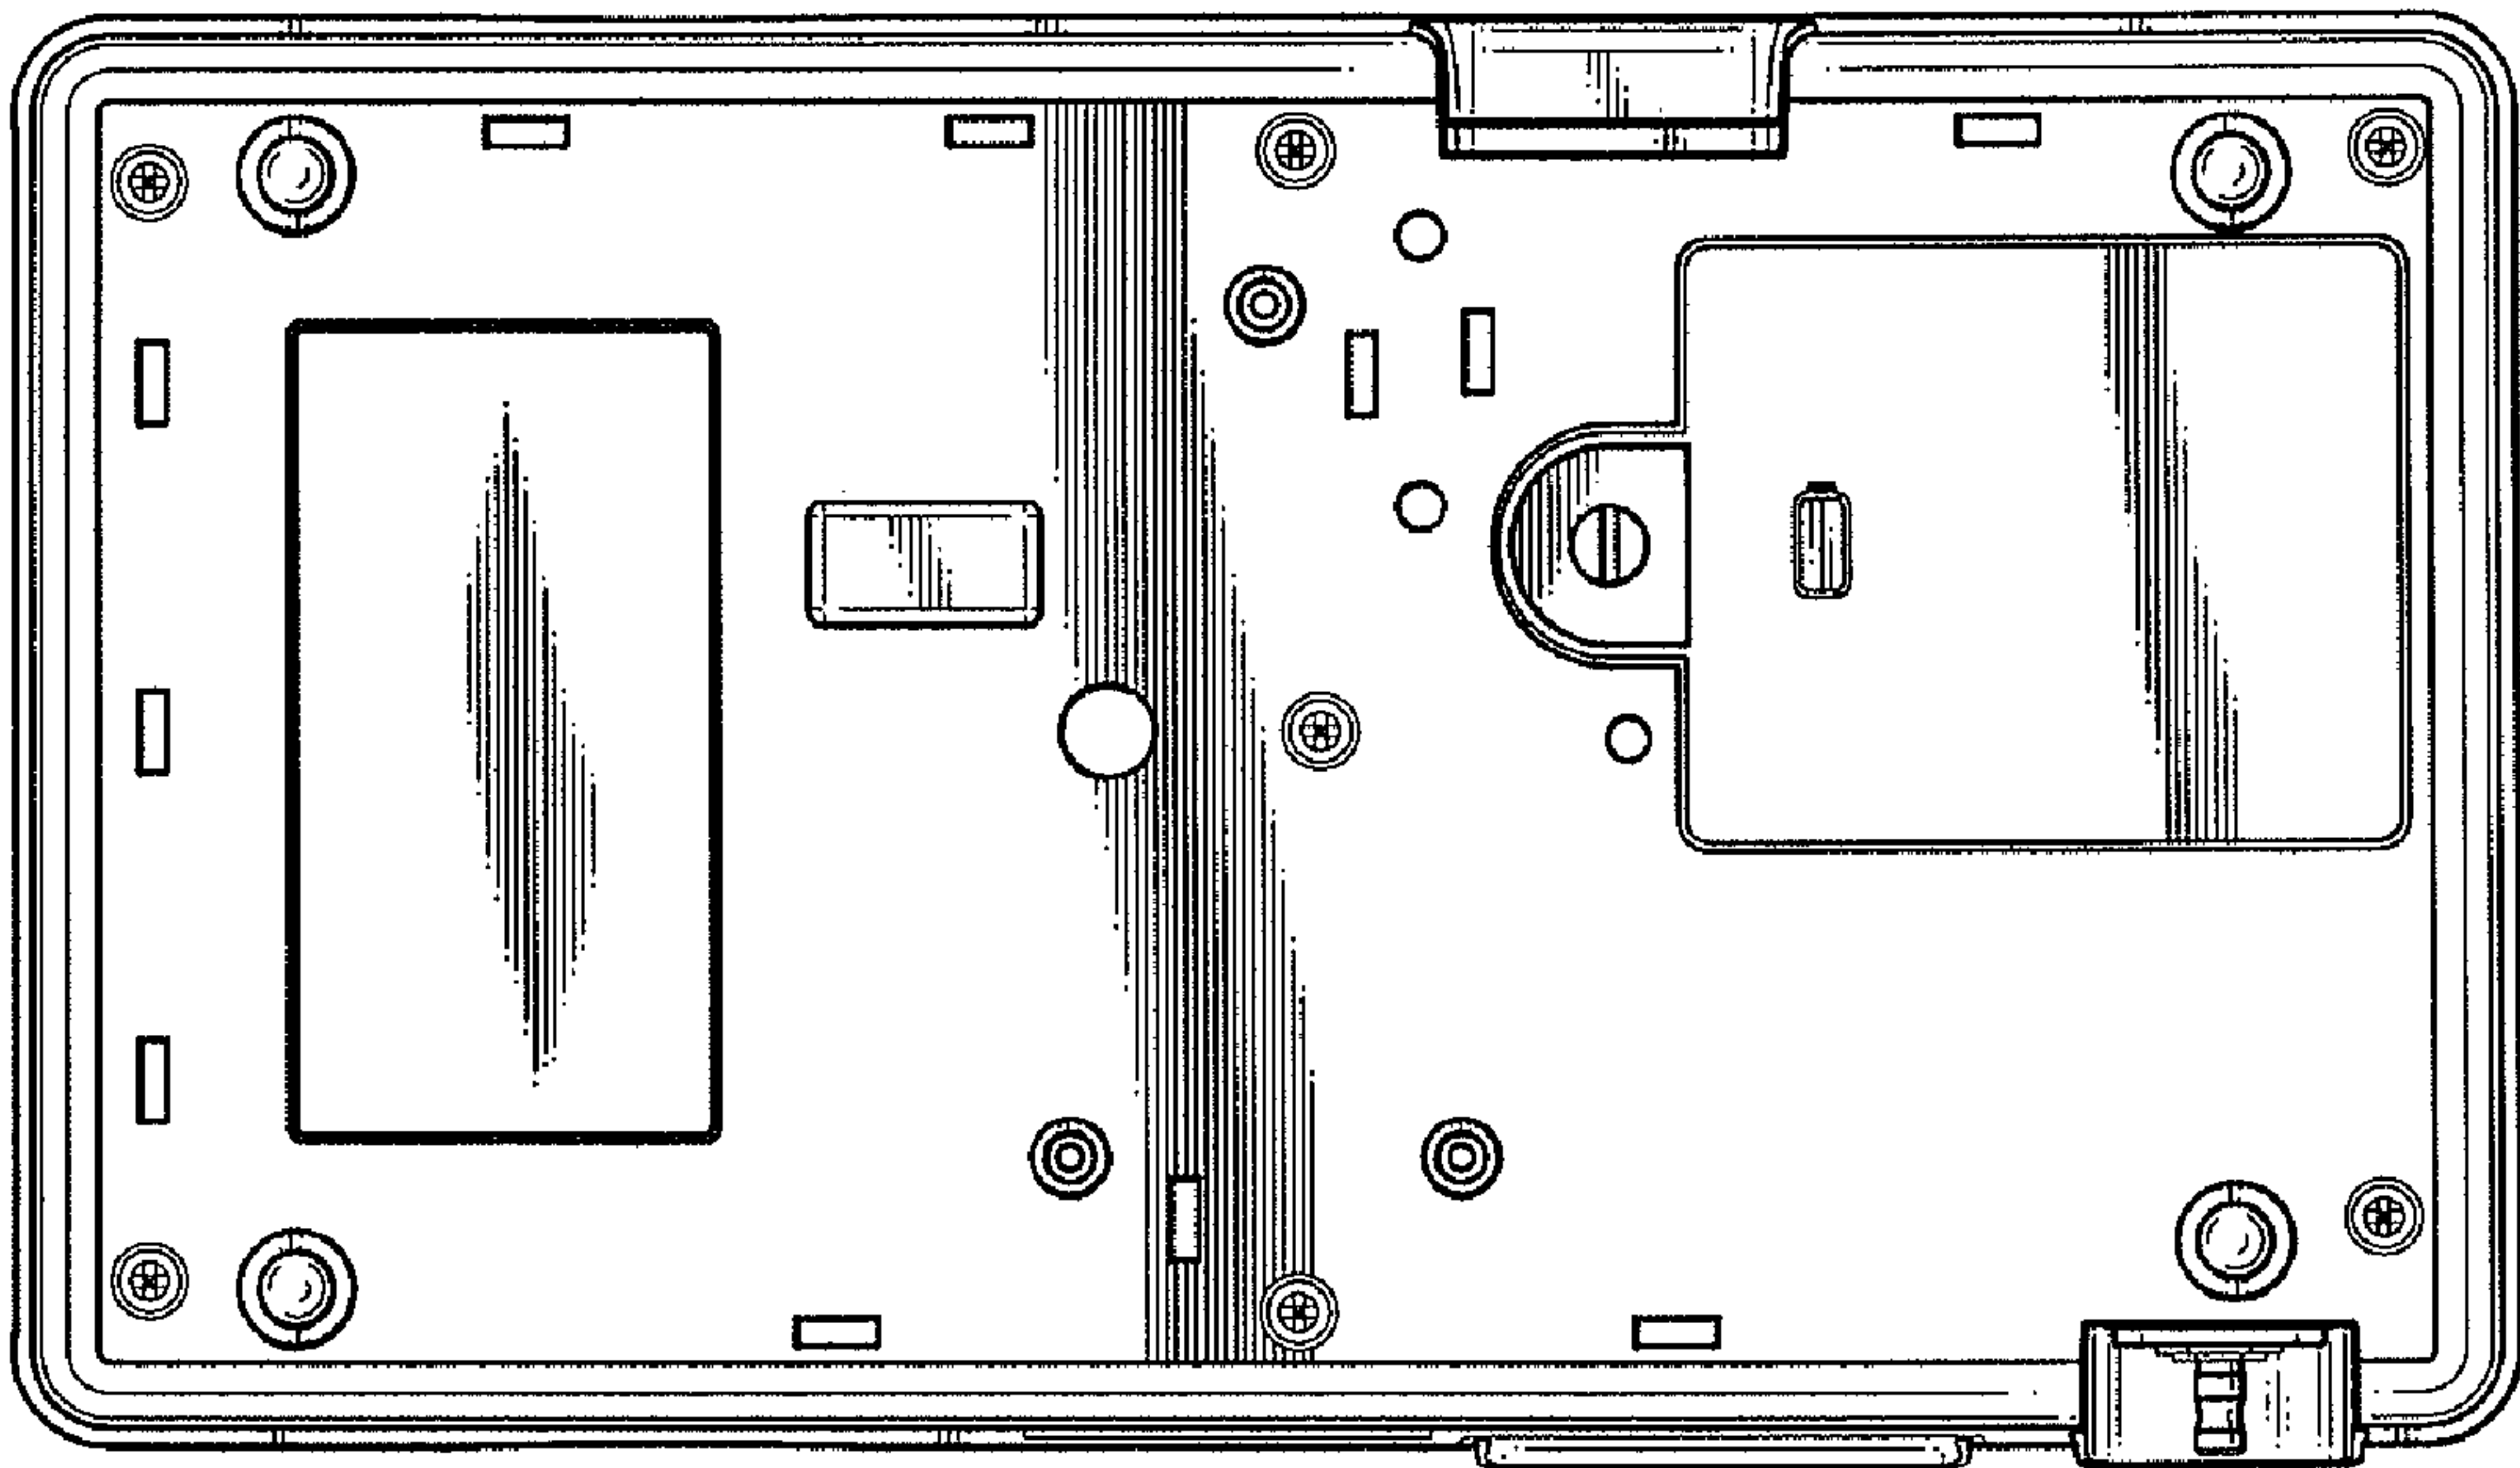


FIG.8