



US00D609812S

(12) **United States Design Patent**  
**Shibata et al.**

(10) **Patent No.:** **US D609,812 S**

(45) **Date of Patent:** **\*\* Feb. 9, 2010**

(54) **SPHYGMOMANOMETER**

(75) Inventors: **Fumie Shibata**, Tokyo (JP); **Yuki Shibata**, Tokyo (JP); **Tadashi Koike**, Kyoto (JP); **Tomohiro Kukita**, Kyoto (JP); **Masataka Yanagase**, Osaka (JP); **Yukiko Mitsunami**, Otsu (JP)

(73) Assignee: **Omron Healthcare Co., Ltd.**, Kyoto (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/318,599**

(22) Filed: **May 22, 2008**

(30) **Foreign Application Priority Data**

Nov. 30, 2007	(JP)	.....	2007-032943
Nov. 30, 2007	(JP)	.....	2007-032944
Nov. 30, 2007	(JP)	.....	2007-032945
Nov. 30, 2007	(JP)	.....	2007-032946
Nov. 30, 2007	(JP)	.....	2007-032947

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/165**

(58) **Field of Classification Search** ..... D24/164-169, D24/186; D10/98; 600/301, 481, 483-485, 600/490, 493-495, 499, 500, 501; 128/900  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,935,984 A 2/1976 Lichowsky et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

JP 1140559 5/2002

(Continued)

**OTHER PUBLICATIONS**

RD 000223979 0001-0006, Sphygmometers, Nov. 30, 2004.

(Continued)

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Capitol City TechLaw

(57) **CLAIM**

The ornamental design for a sphygmomanometer, as shown and described.

**DESCRIPTION**

FIG. 1 is a front perspective view of a first embodiment of a sphygmomanometer showing our new design;

FIG. 2 is a rear perspective view thereof;

FIG. 3 is a front elevational view thereof;

FIG. 4 is a rear elevational view thereof;

FIG. 5 is a top plan view thereof;

FIG. 6 is a bottom plan view thereof;

FIG. 7 is a right side elevational view thereof;

FIG. 8 is a left side elevational view thereof;

FIG. 9 is a front perspective view thereof with an armband shown in an opened position;

FIG. 10 is a rear perspective view thereof with the armband shown in an opened position;

FIG. 11 is a front elevational view thereof with the armband shown in an opened position;

FIG. 12 is a rear elevational view thereof with the armband shown in an opened position;


FIG. 13 is a top plan view thereof with the armband shown in an opened position;

FIG. 14 is a bottom plan view thereof with the armband shown in an opened position;

FIG. 15 is a right side elevational view thereof with the armband shown in an opened position; and

FIG. 16 is a left side elevational view thereof with the armband shown in an opened position.

**1 Claim, 8 Drawing Sheets**

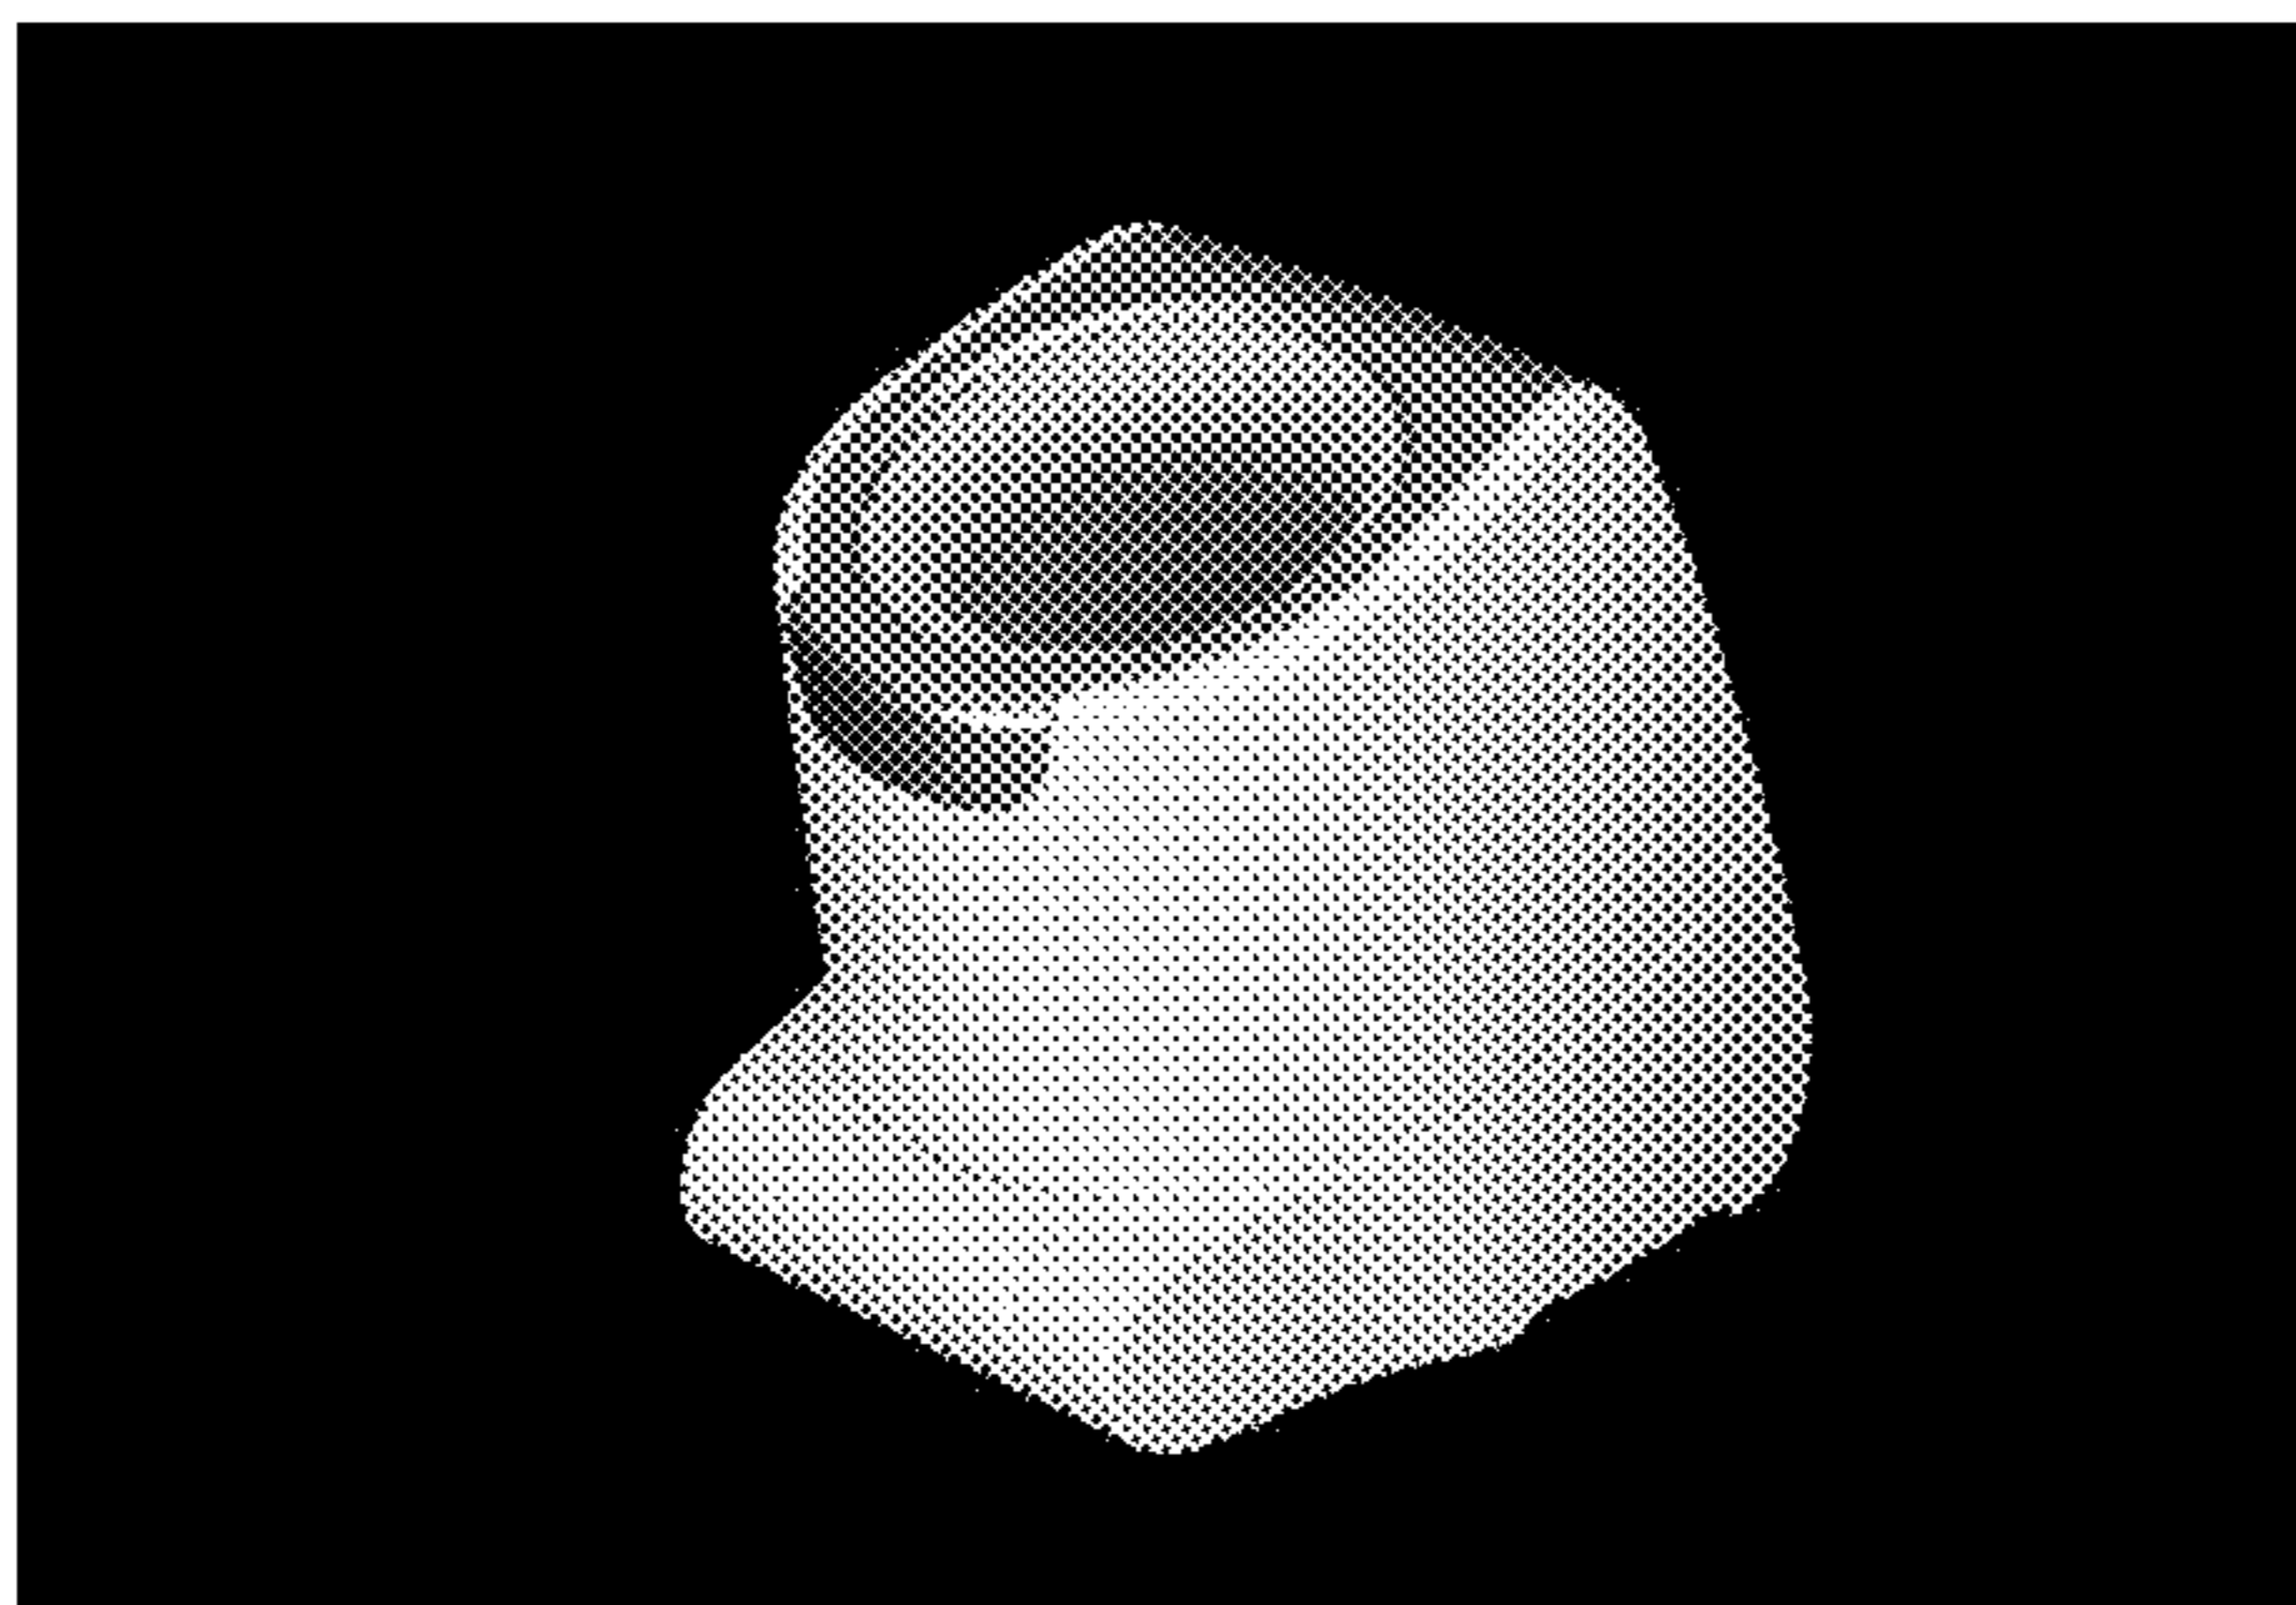

# US D609,812 S

Page 2

---

## U.S. PATENT DOCUMENTS

D244,235 S 5/1977 Lichowsky  
4,058,117 A 11/1977 Kaspari et al.  
D254,629 S 4/1980 Yen  
D290,876 S 7/1987 Arduini et al.  
D321,562 S 11/1991 Ljungvall  
D341,658 S 11/1993 Kojima  
5,511,551 A 4/1996 Sano et al.  
6,213,953 B1 4/2001 Reeves  
D445,900 S \* 7/2001 Nalbandian et al. .... D24/165  
D447,568 S 9/2001 Hall et al.  
6,714,814 B2 3/2004 Yamada et al.  
D489,113 S 4/2004 Peterson  
6,726,633 B2 4/2004 Kitagawa  
D530,012 S 10/2006 Eda et al.

7,232,413 B2 6/2007 Hashimoto et al.  
D560,279 S 1/2008 Eda et al.  
D561,339 S 2/2008 Eda et al.  
D590,506 S \* 4/2009 Krishnan ..... D24/186

## FOREIGN PATENT DOCUMENTS

JP 1200780 4/2004  
JP 1216857 9/2004  
JP 1284981 10/2006

## OTHER PUBLICATIONS

Terumo Corporation, Brochure, Terumo Corporation, "Arm In® Plus", Electronic Sphygmomanometer, ES-P2000U, published Aug. 2005.

\* cited by examiner

FIG. 1

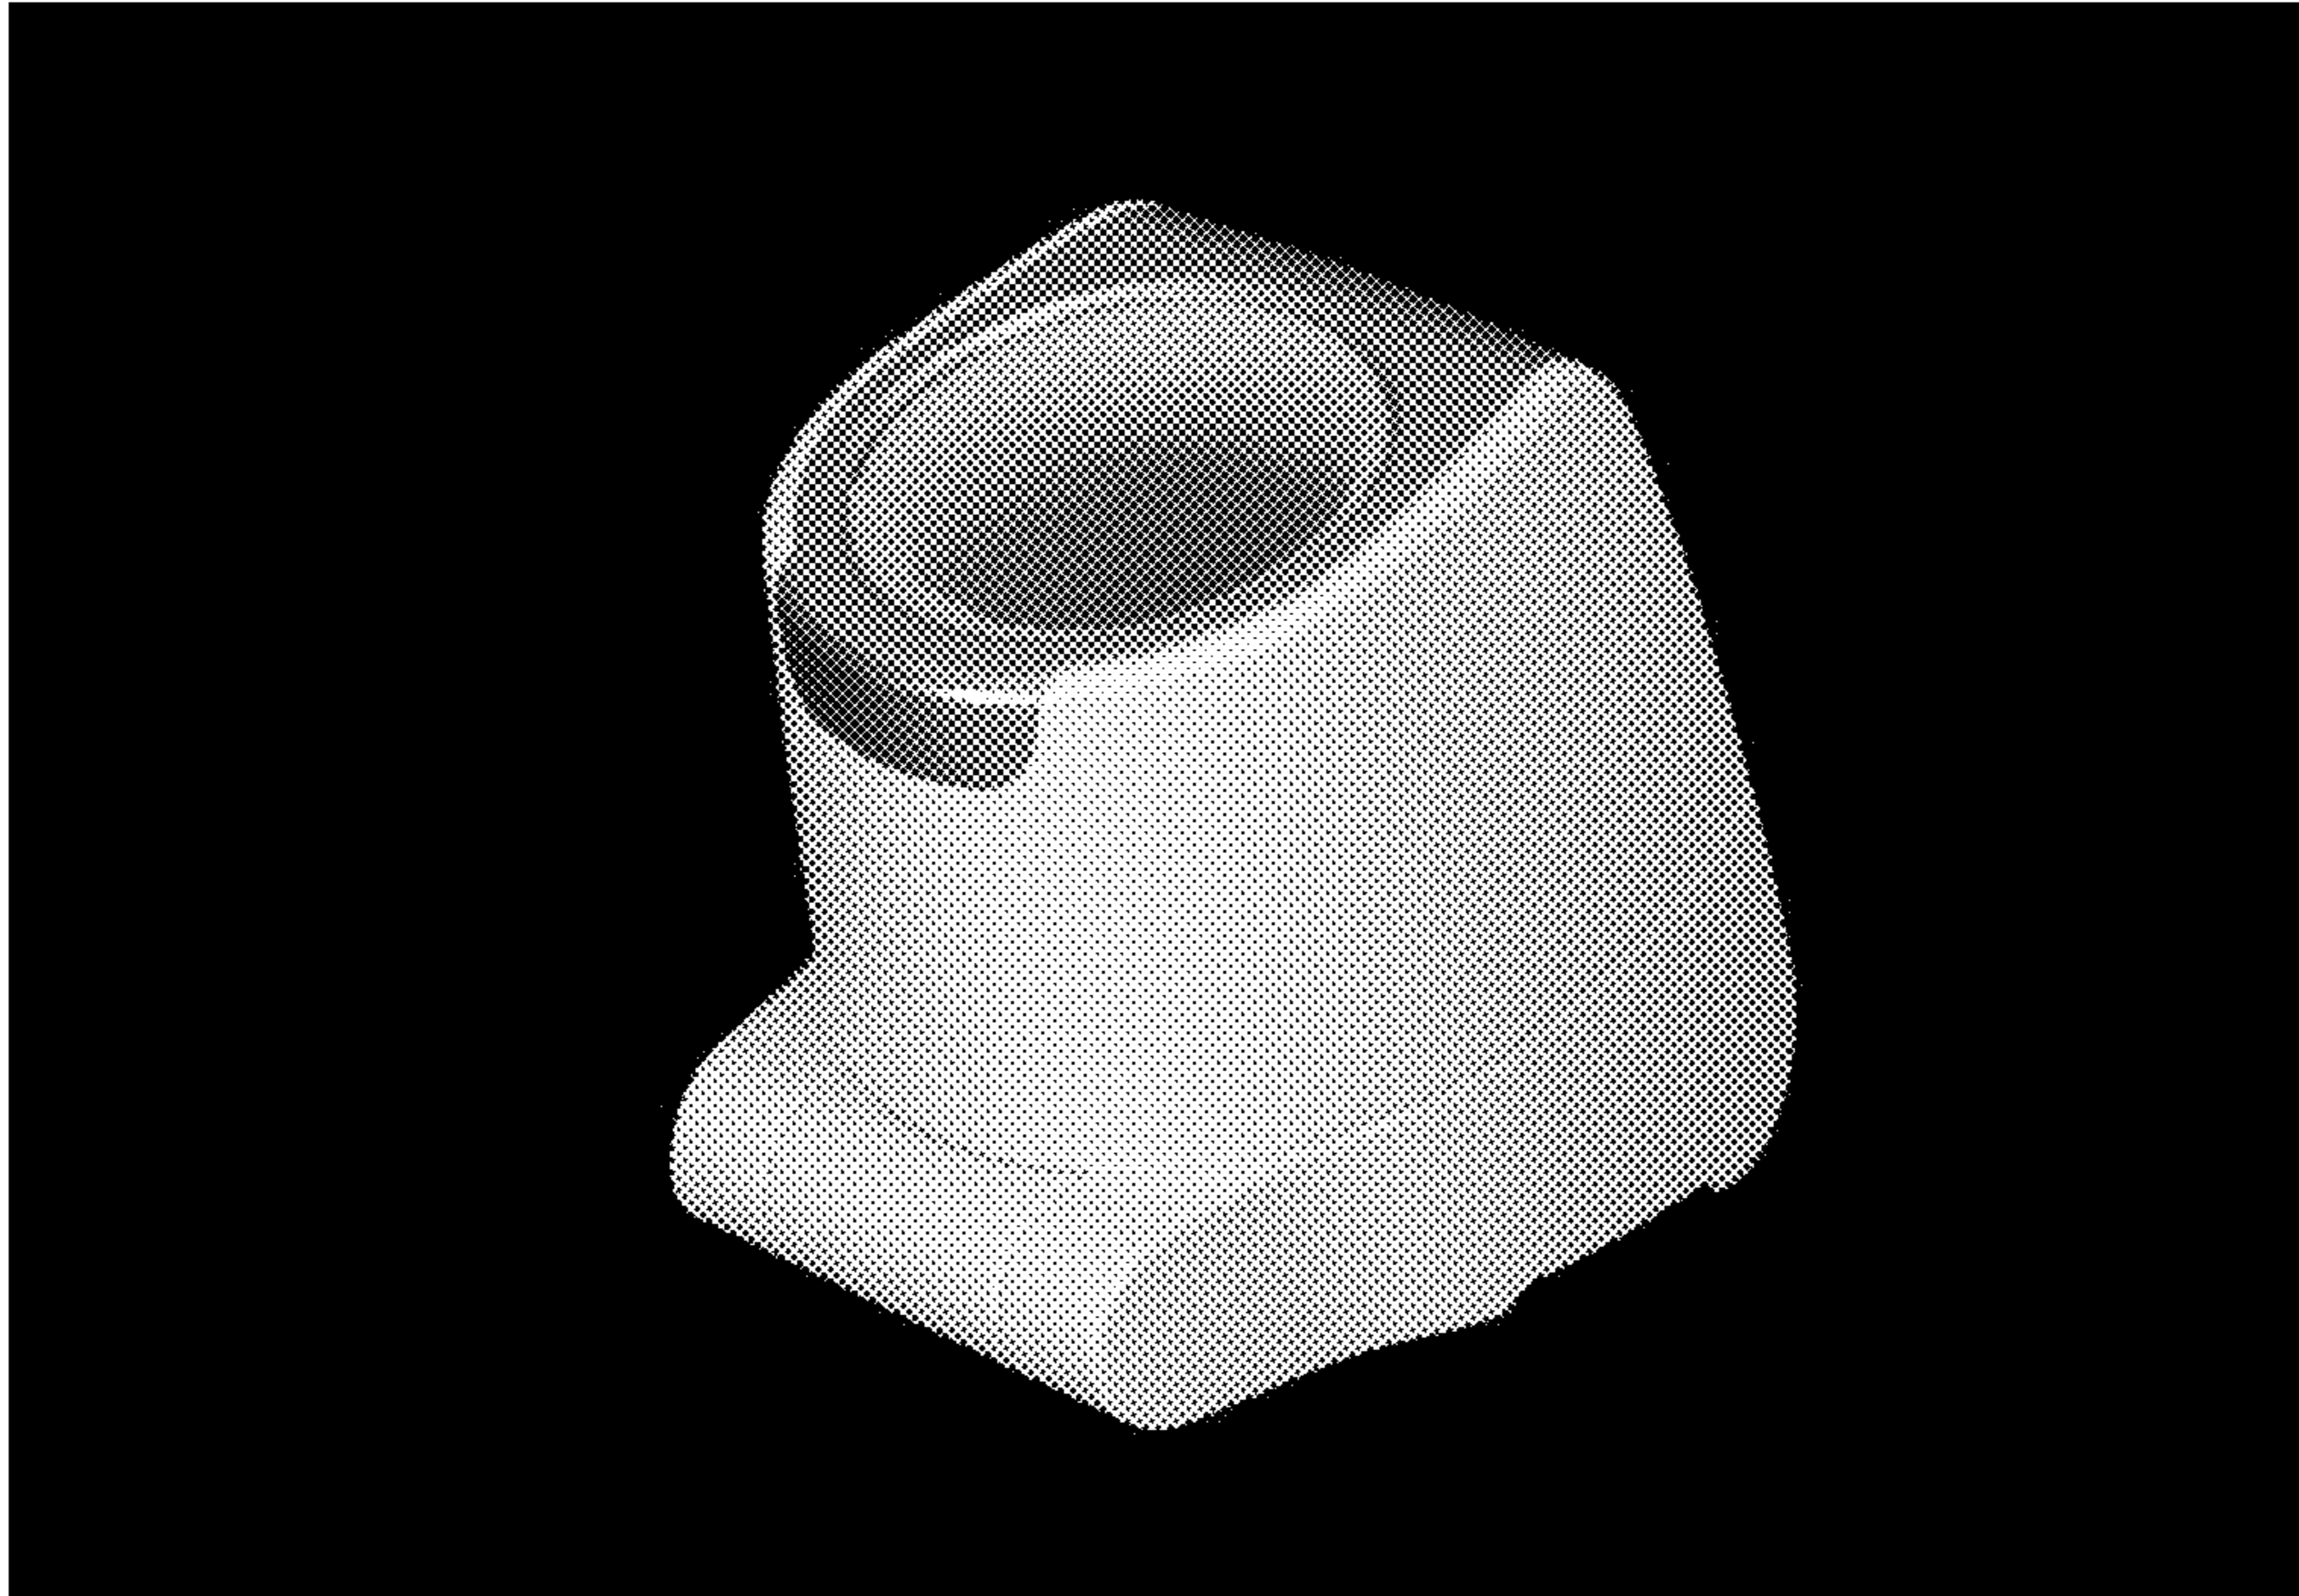


FIG. 2





FIG. 3

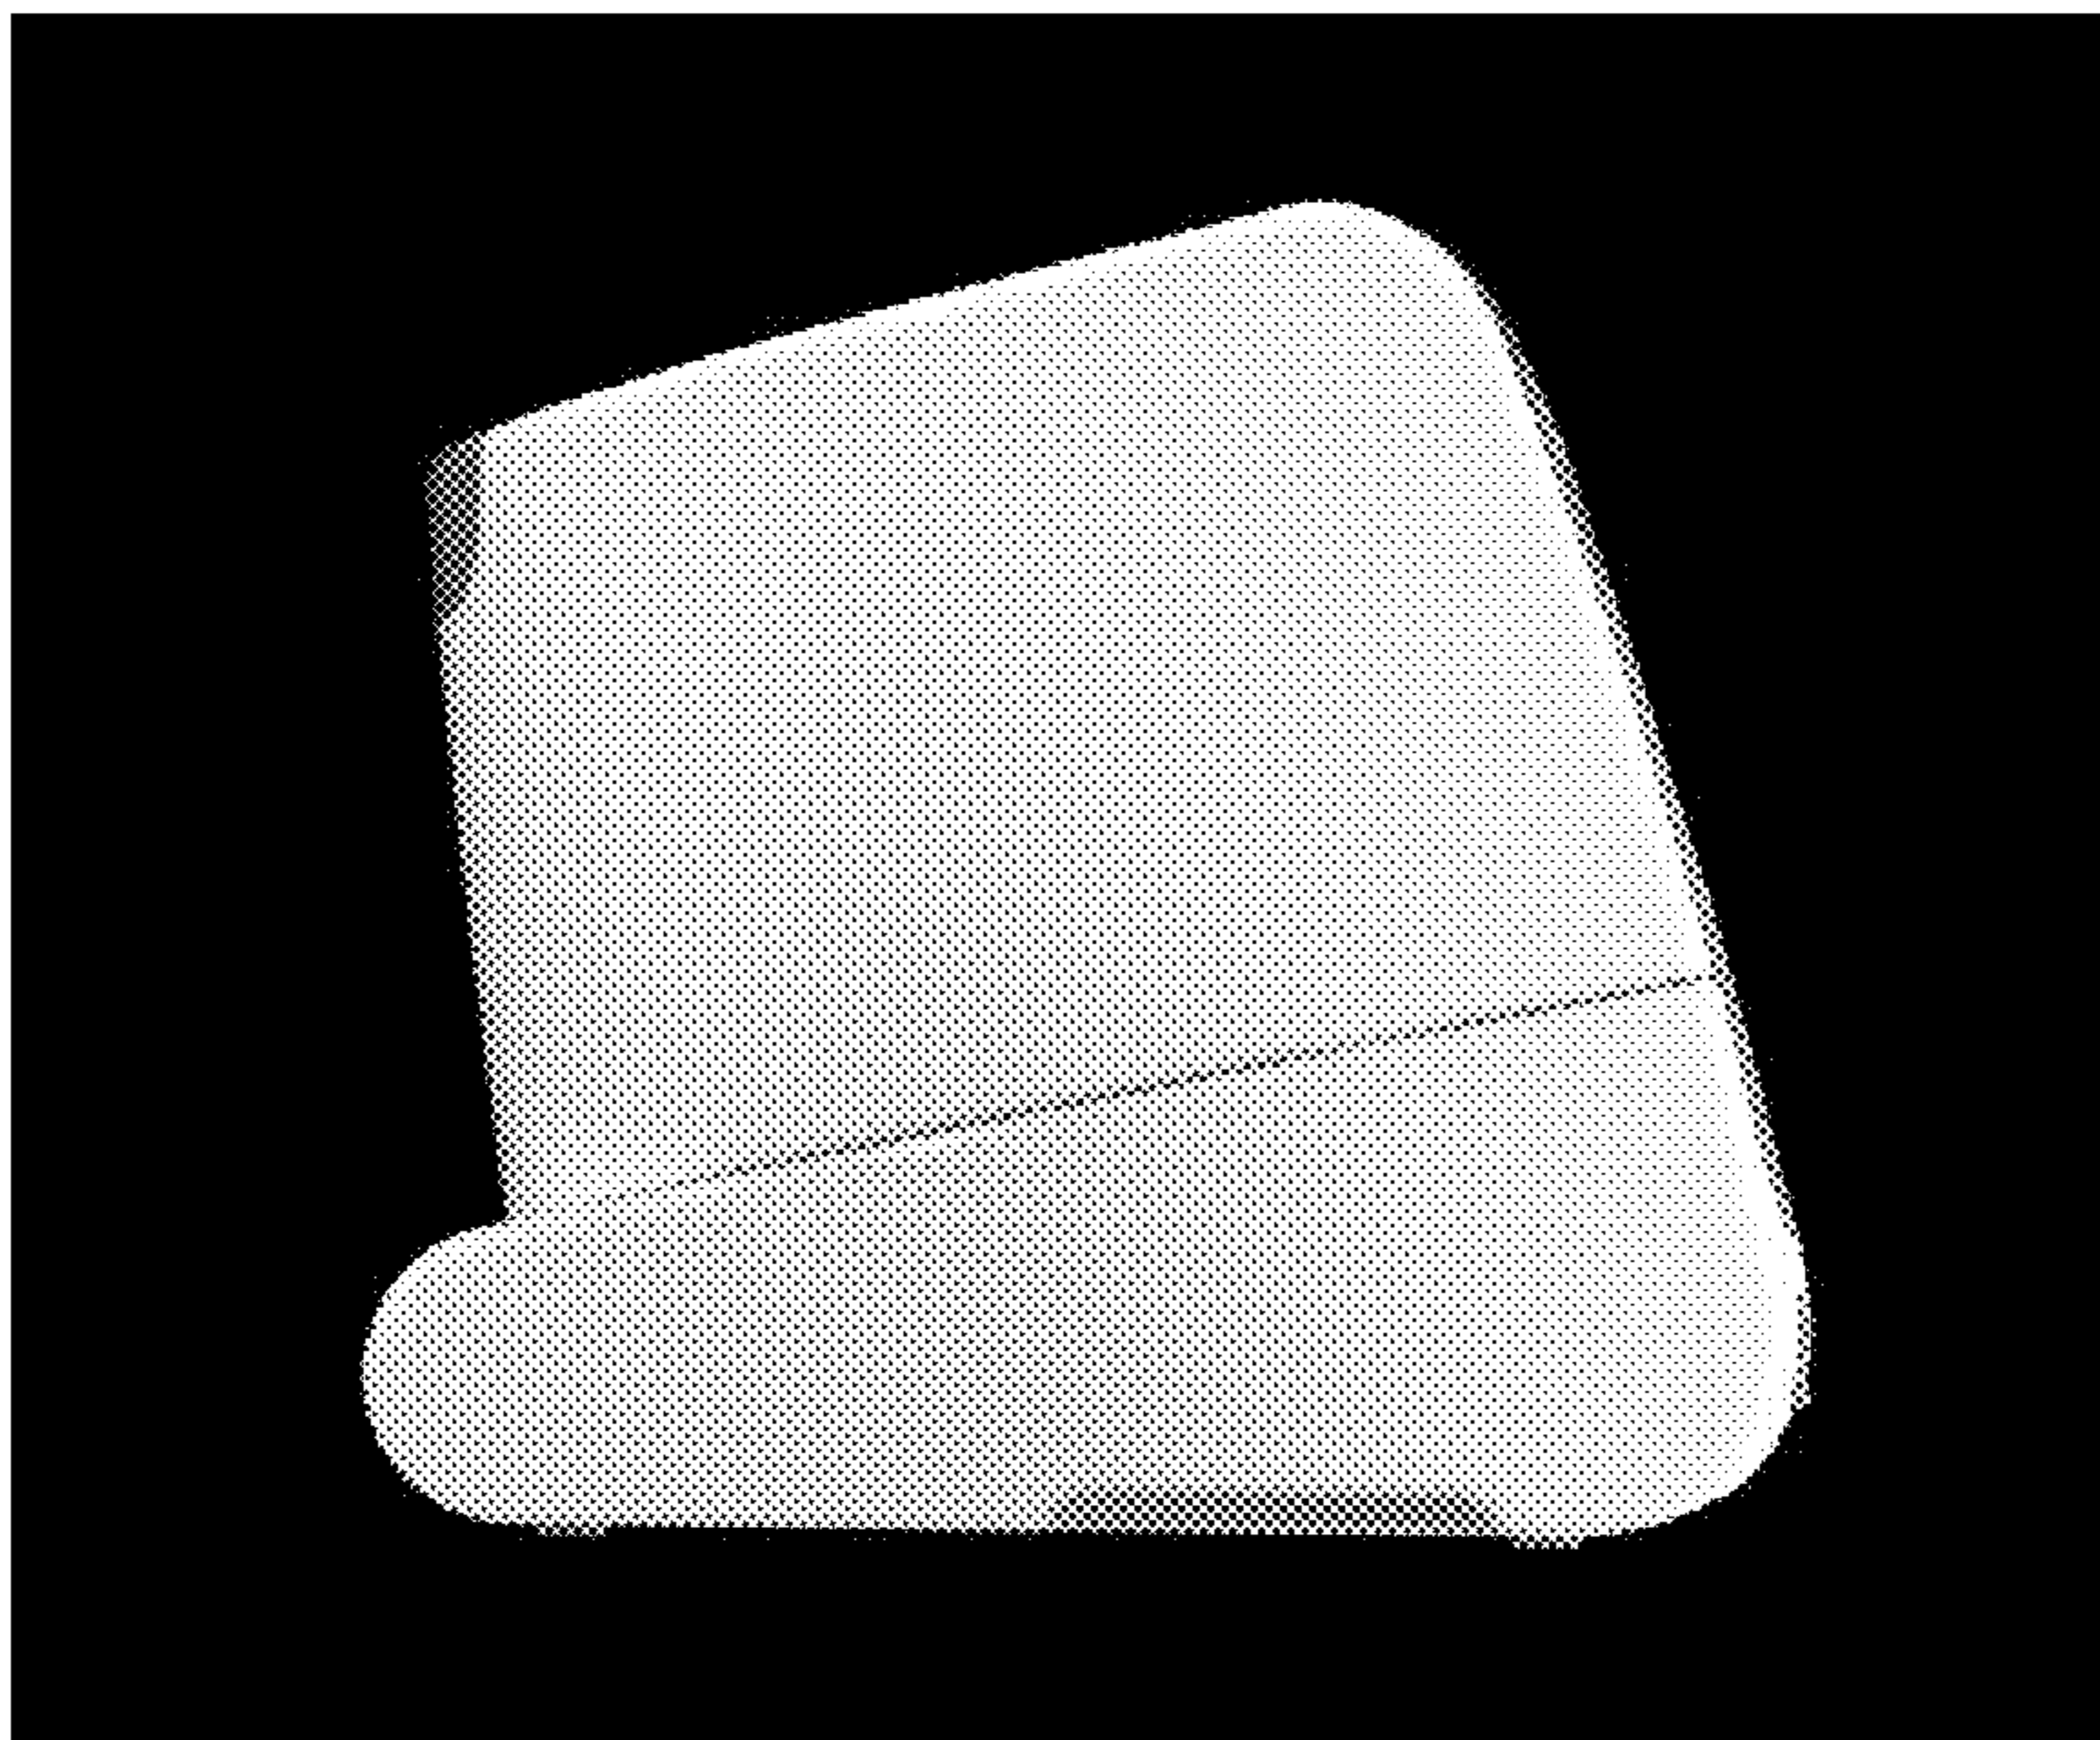


FIG. 4

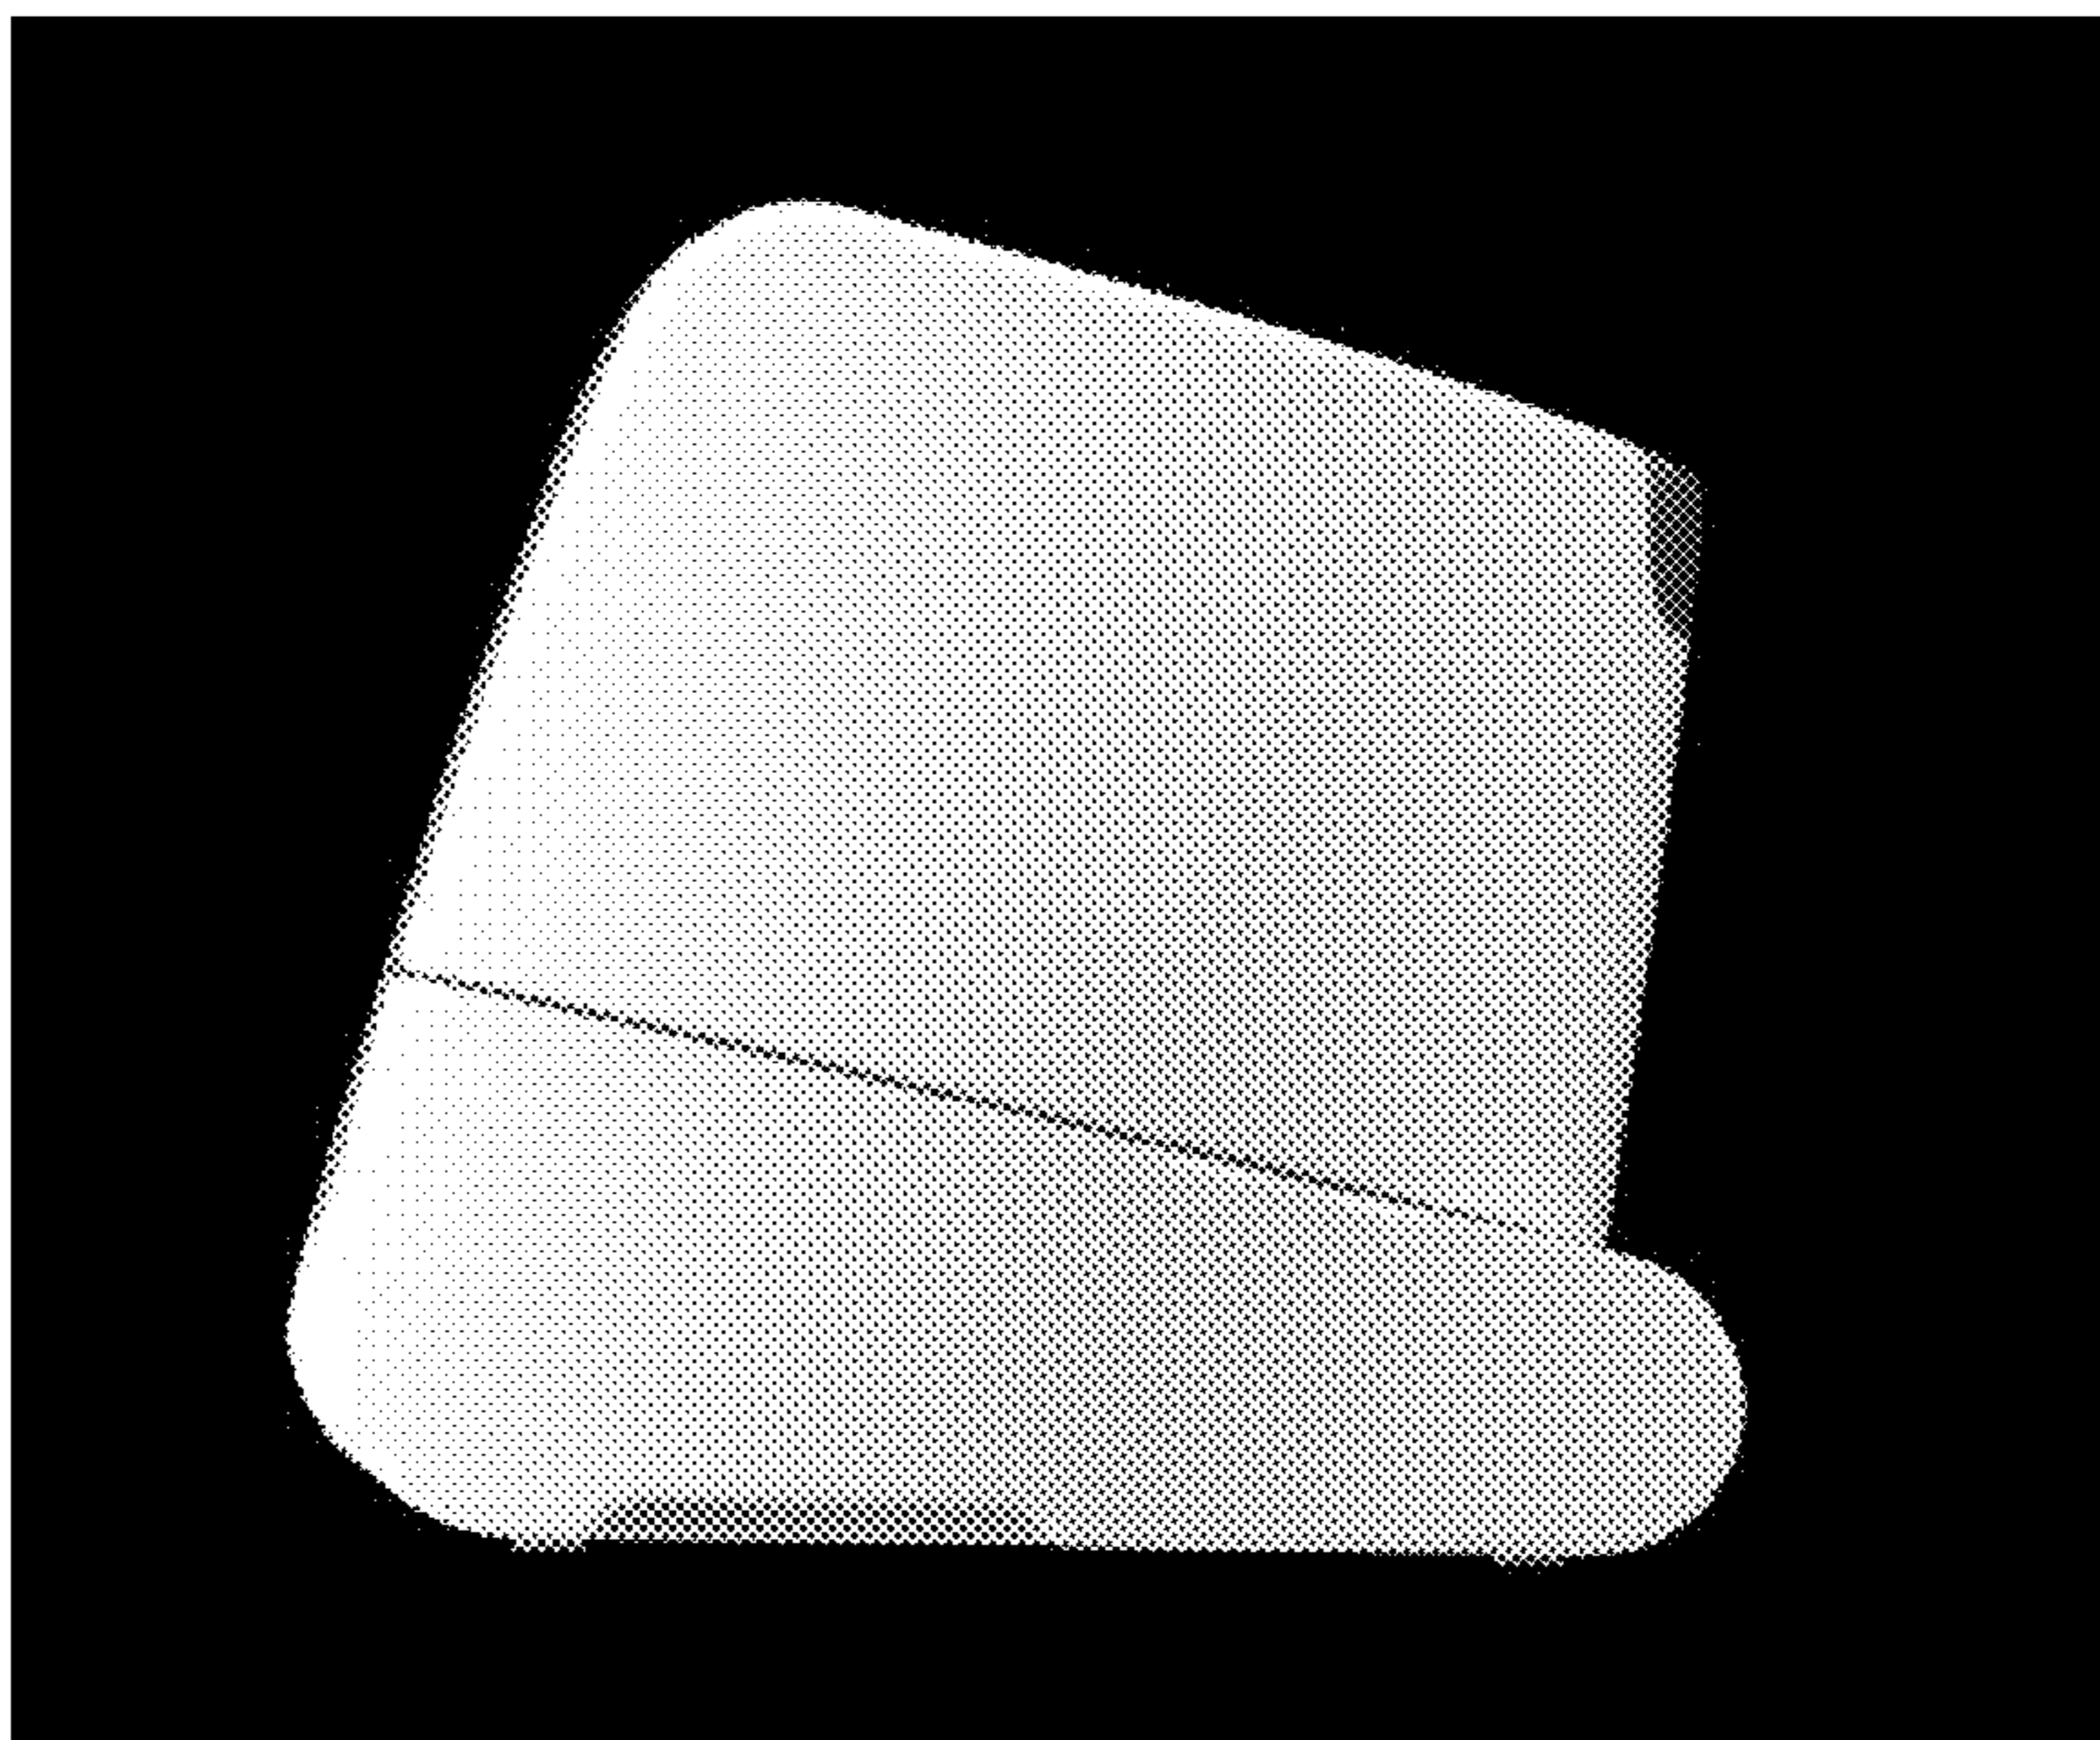


FIG. 5

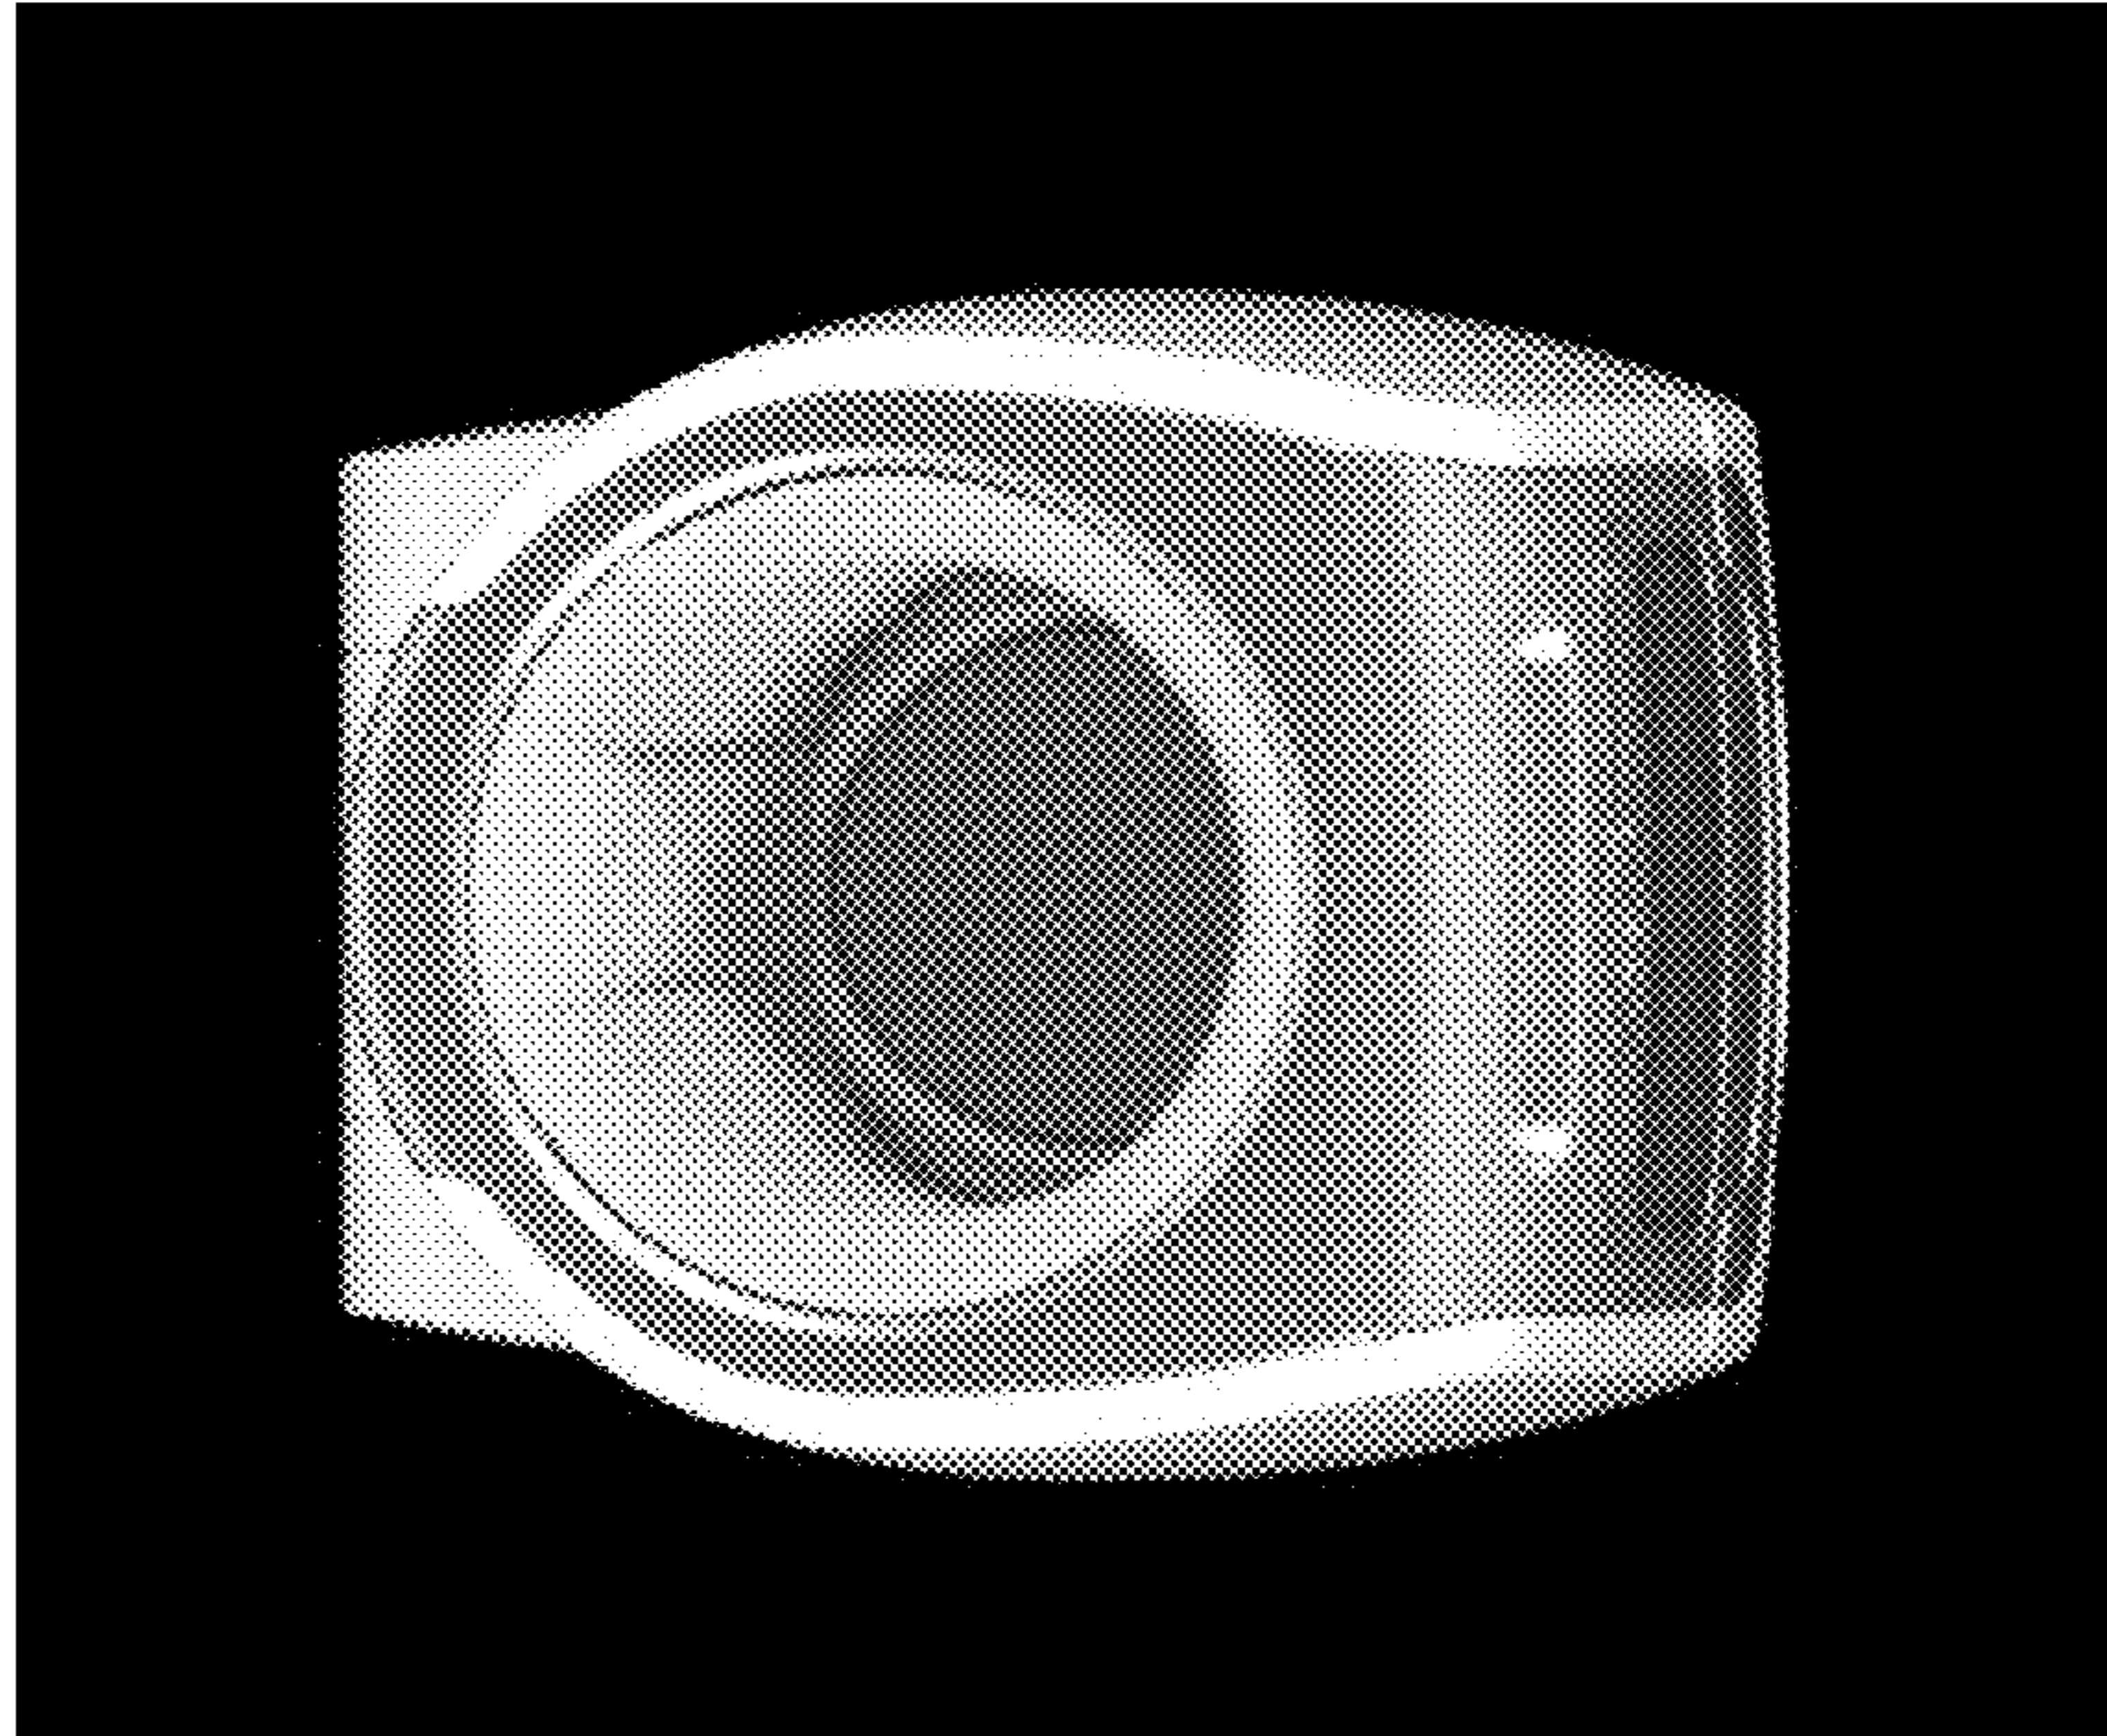


FIG. 6

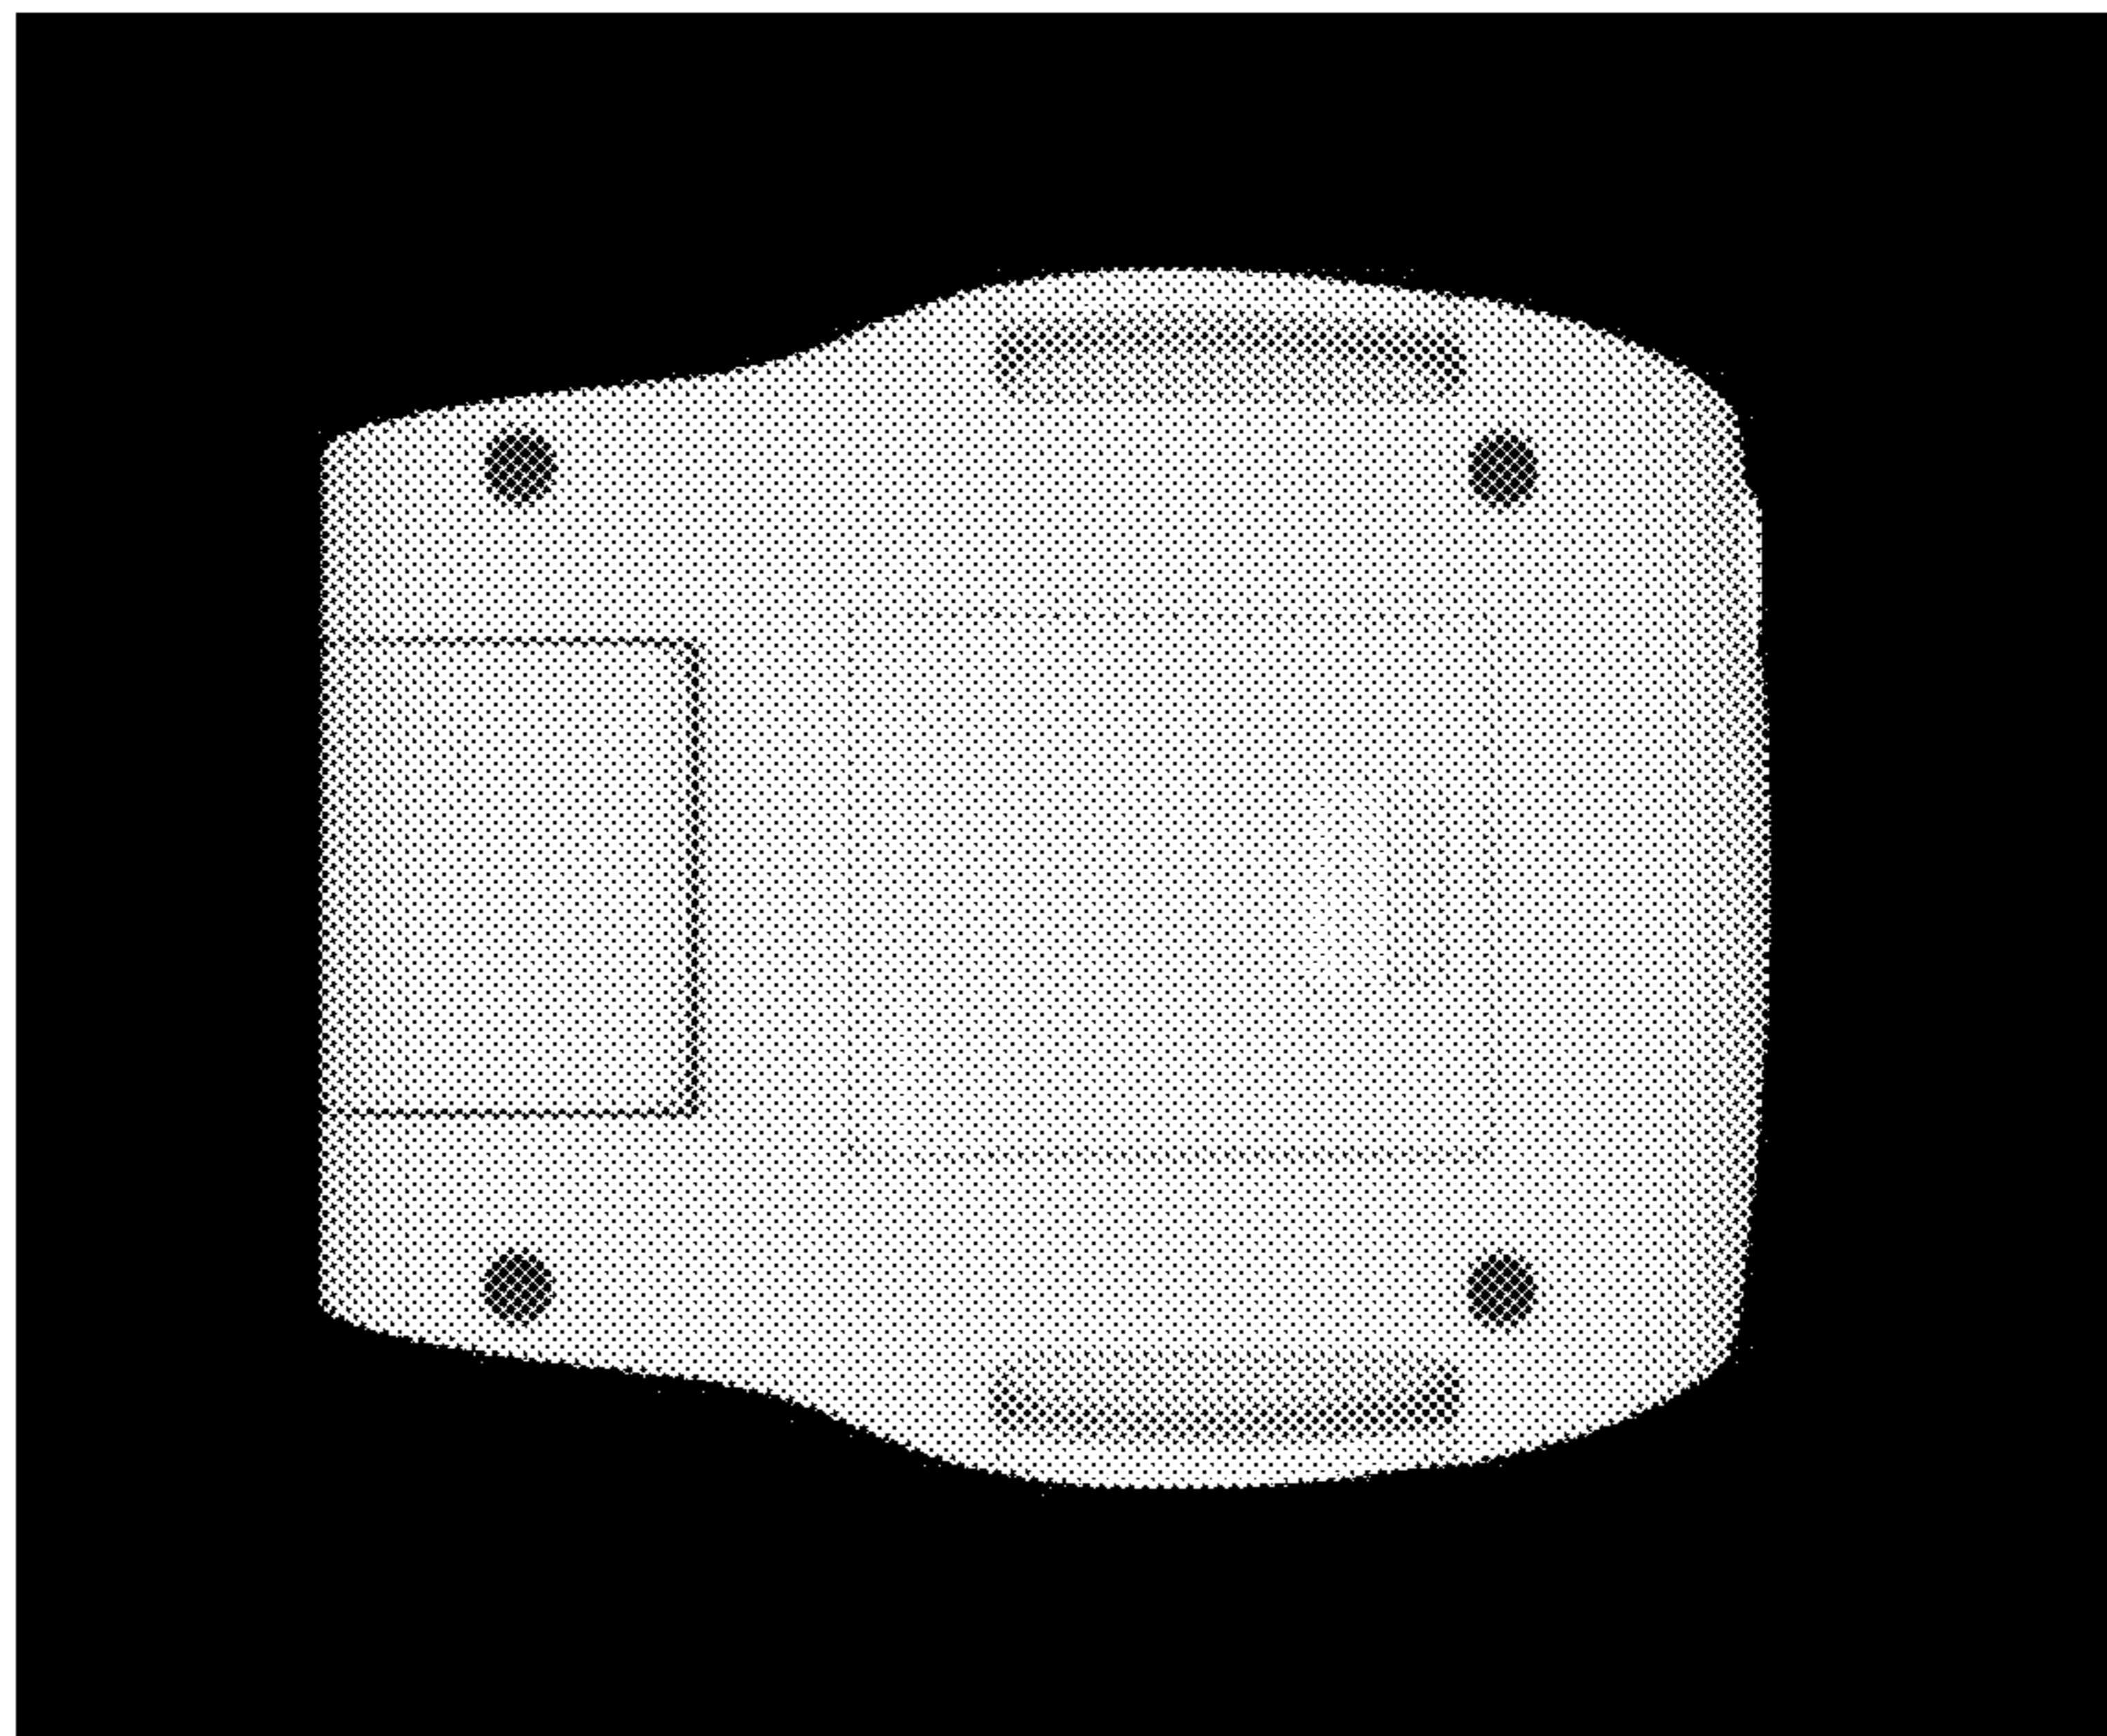




FIG. 7

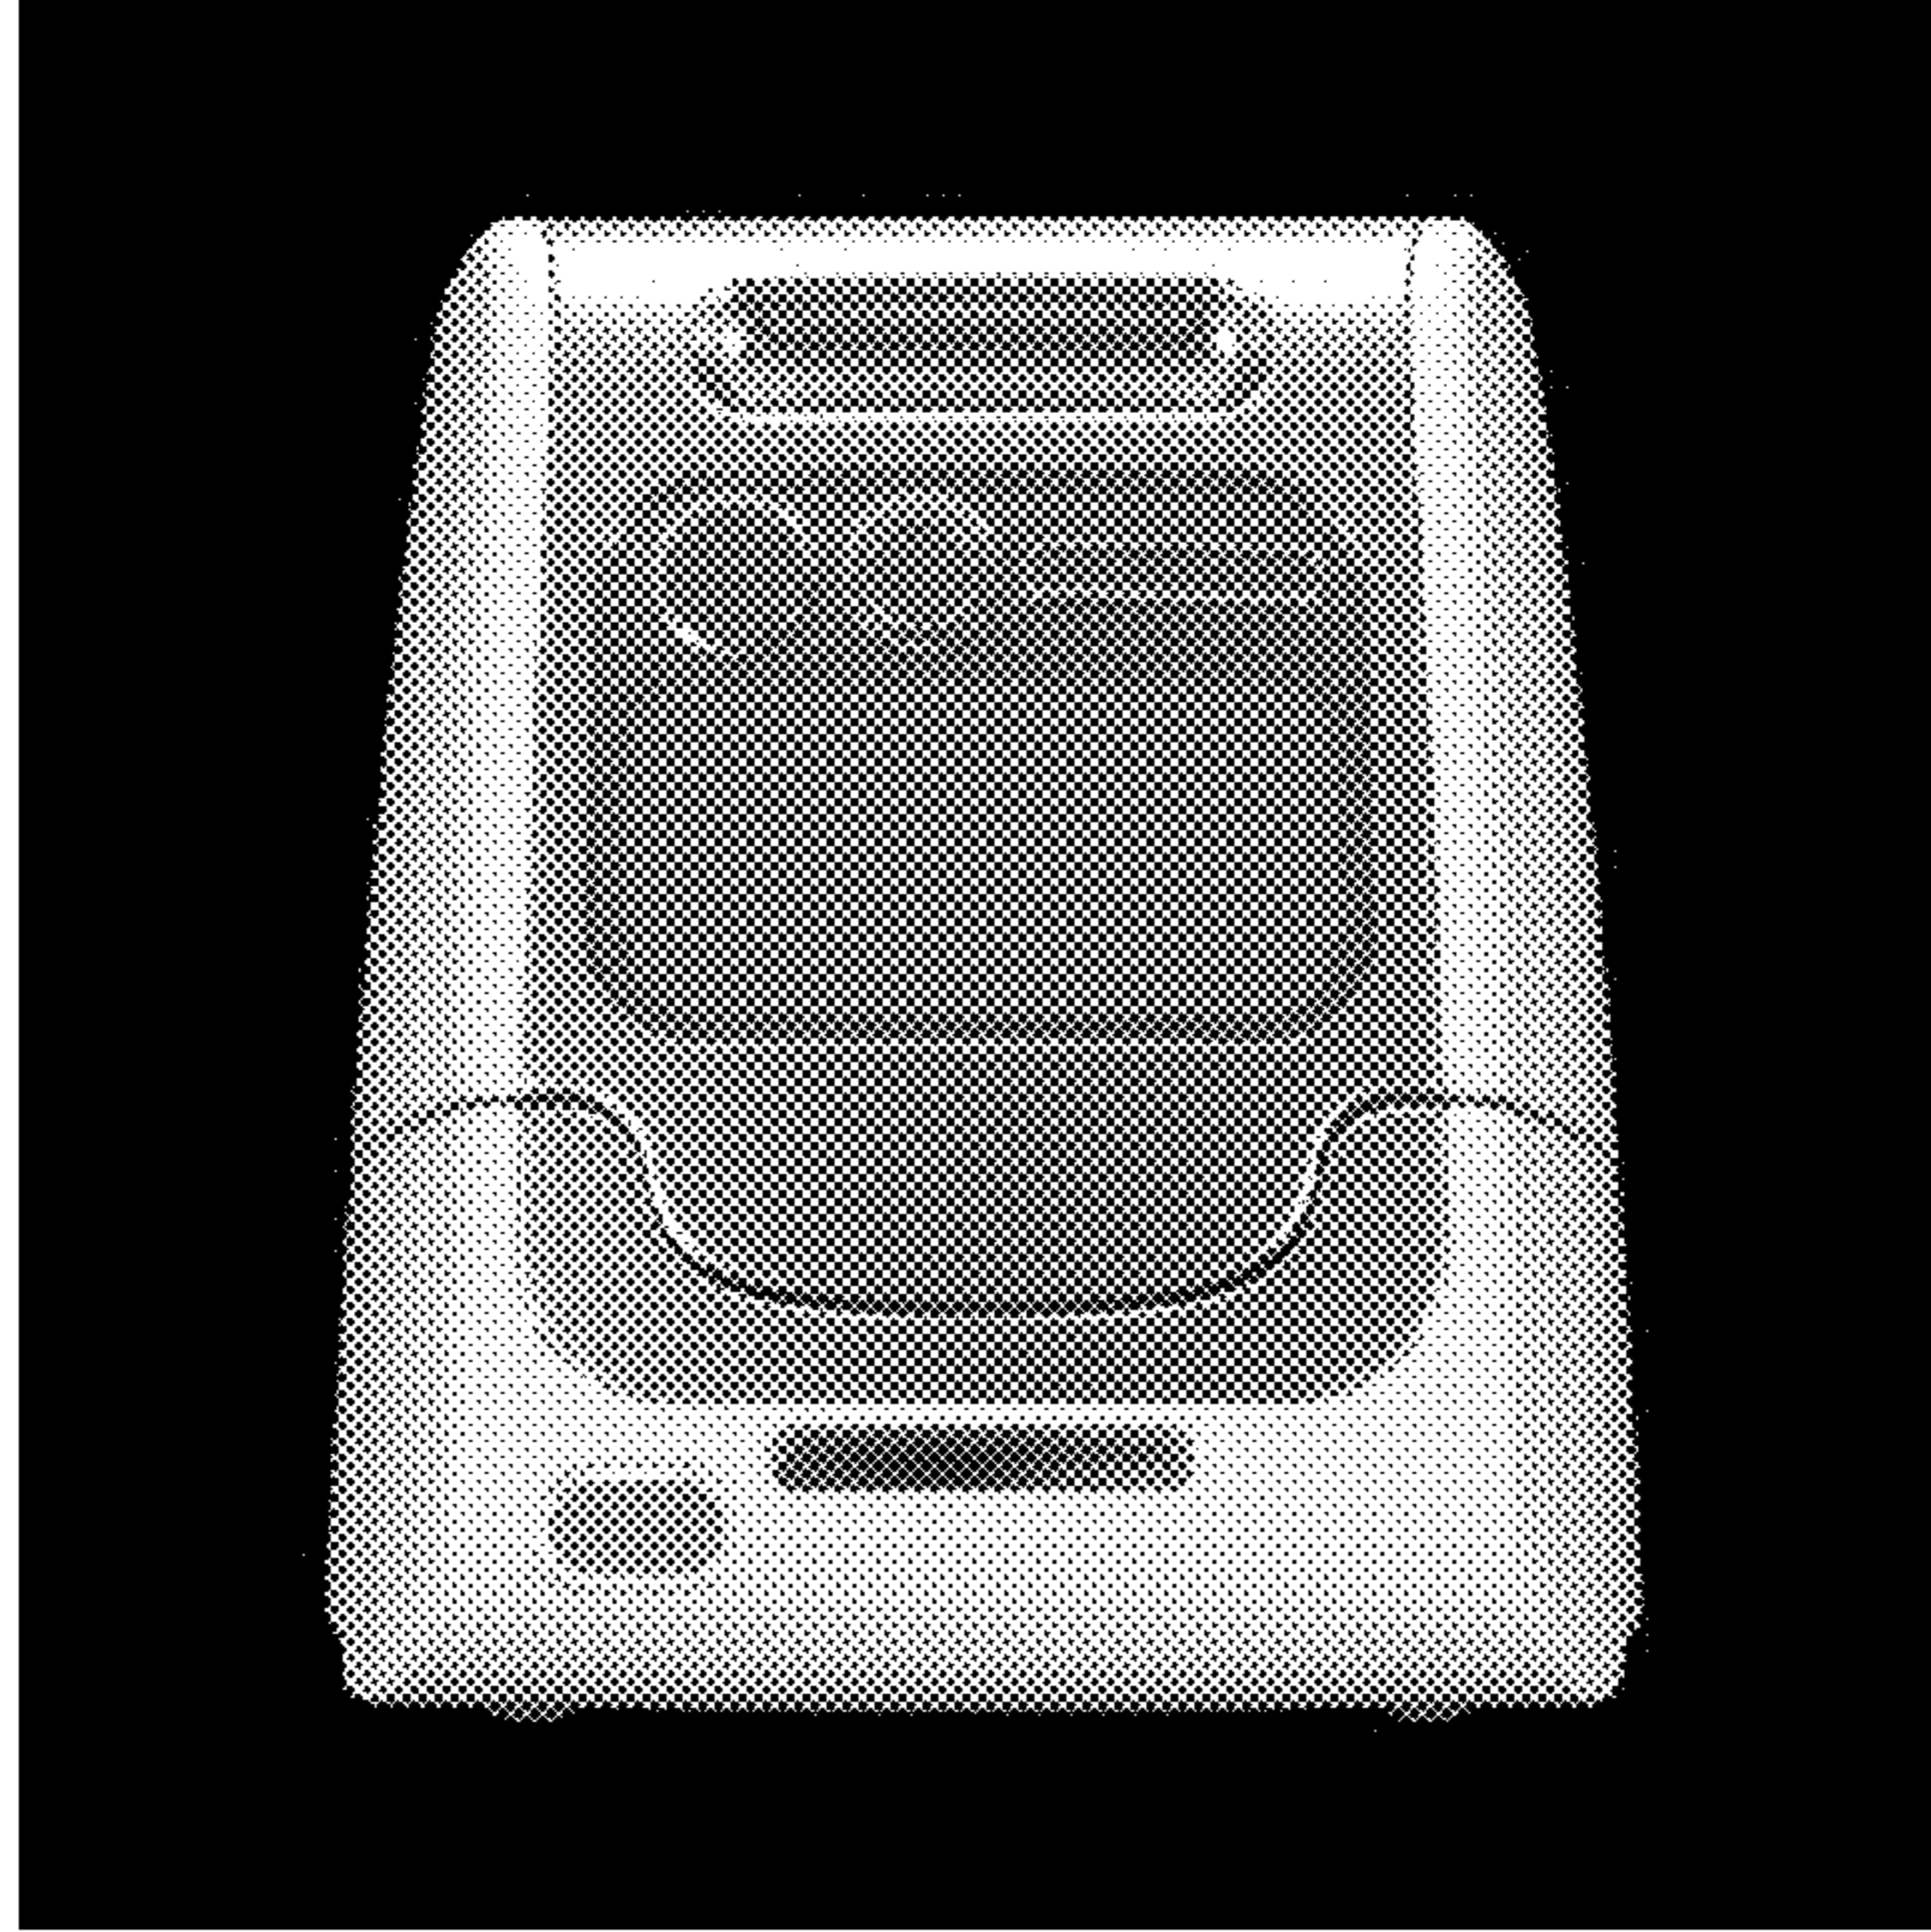


FIG. 8

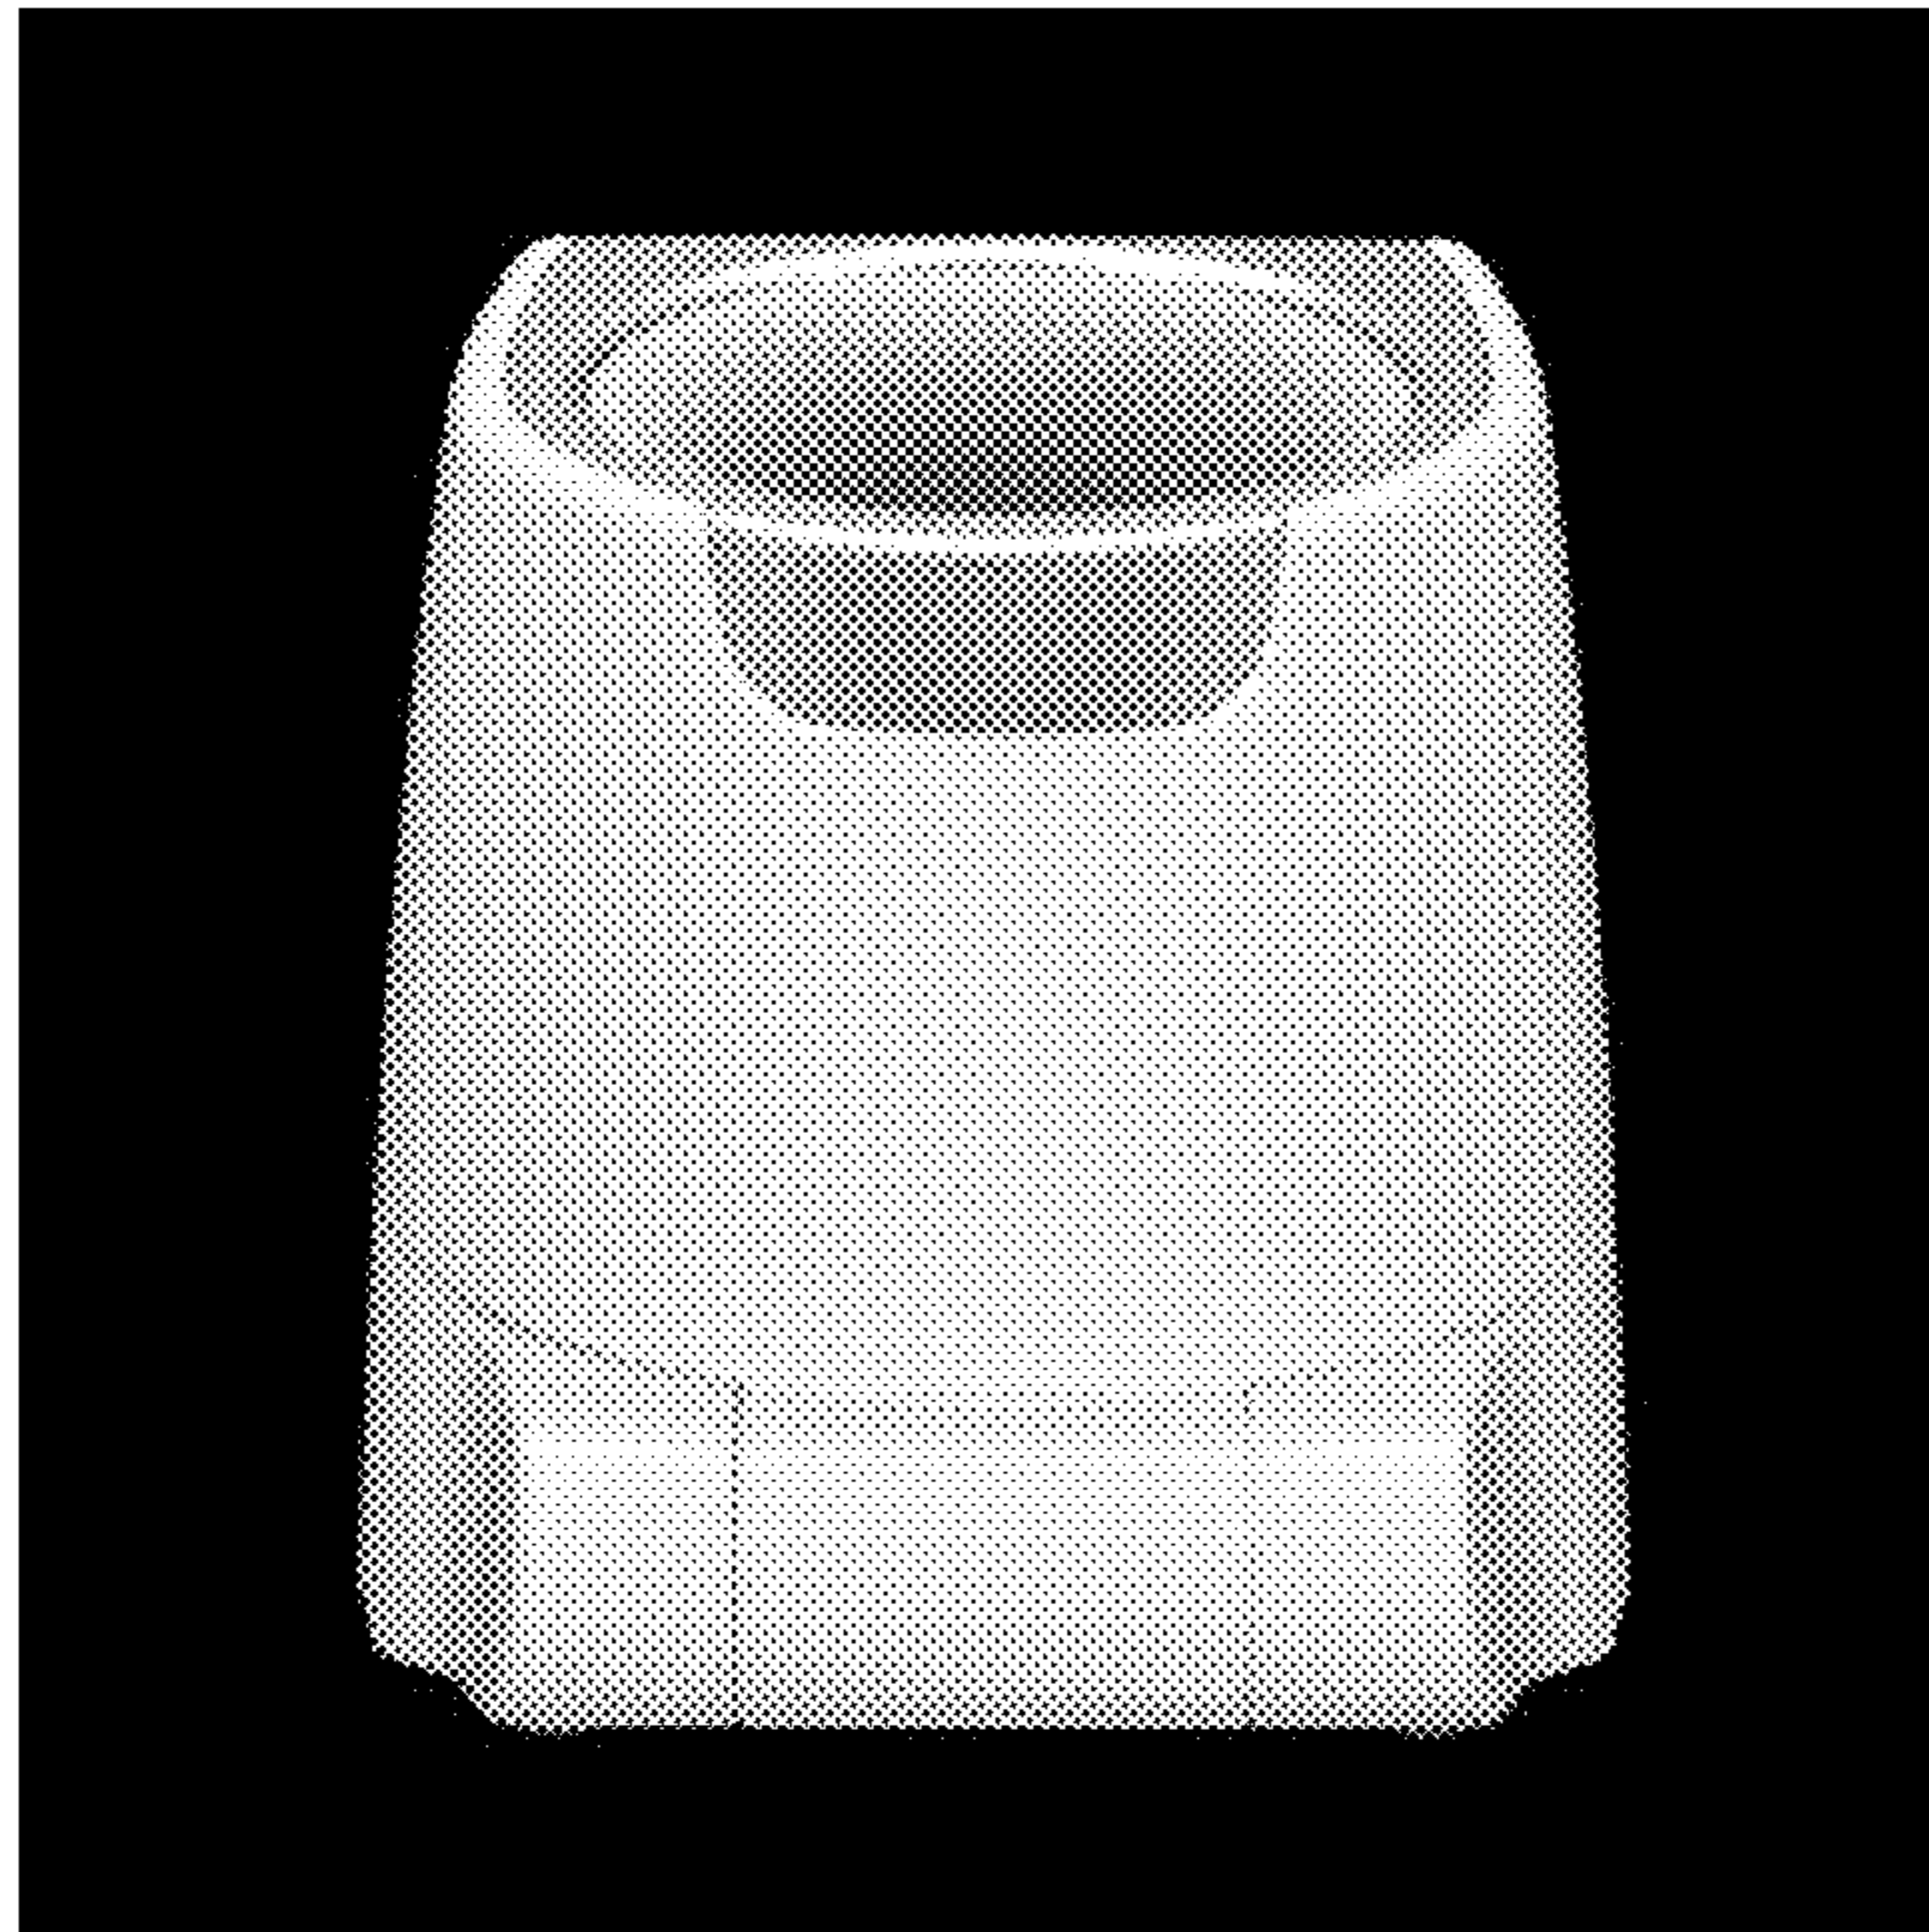


FIG. 9

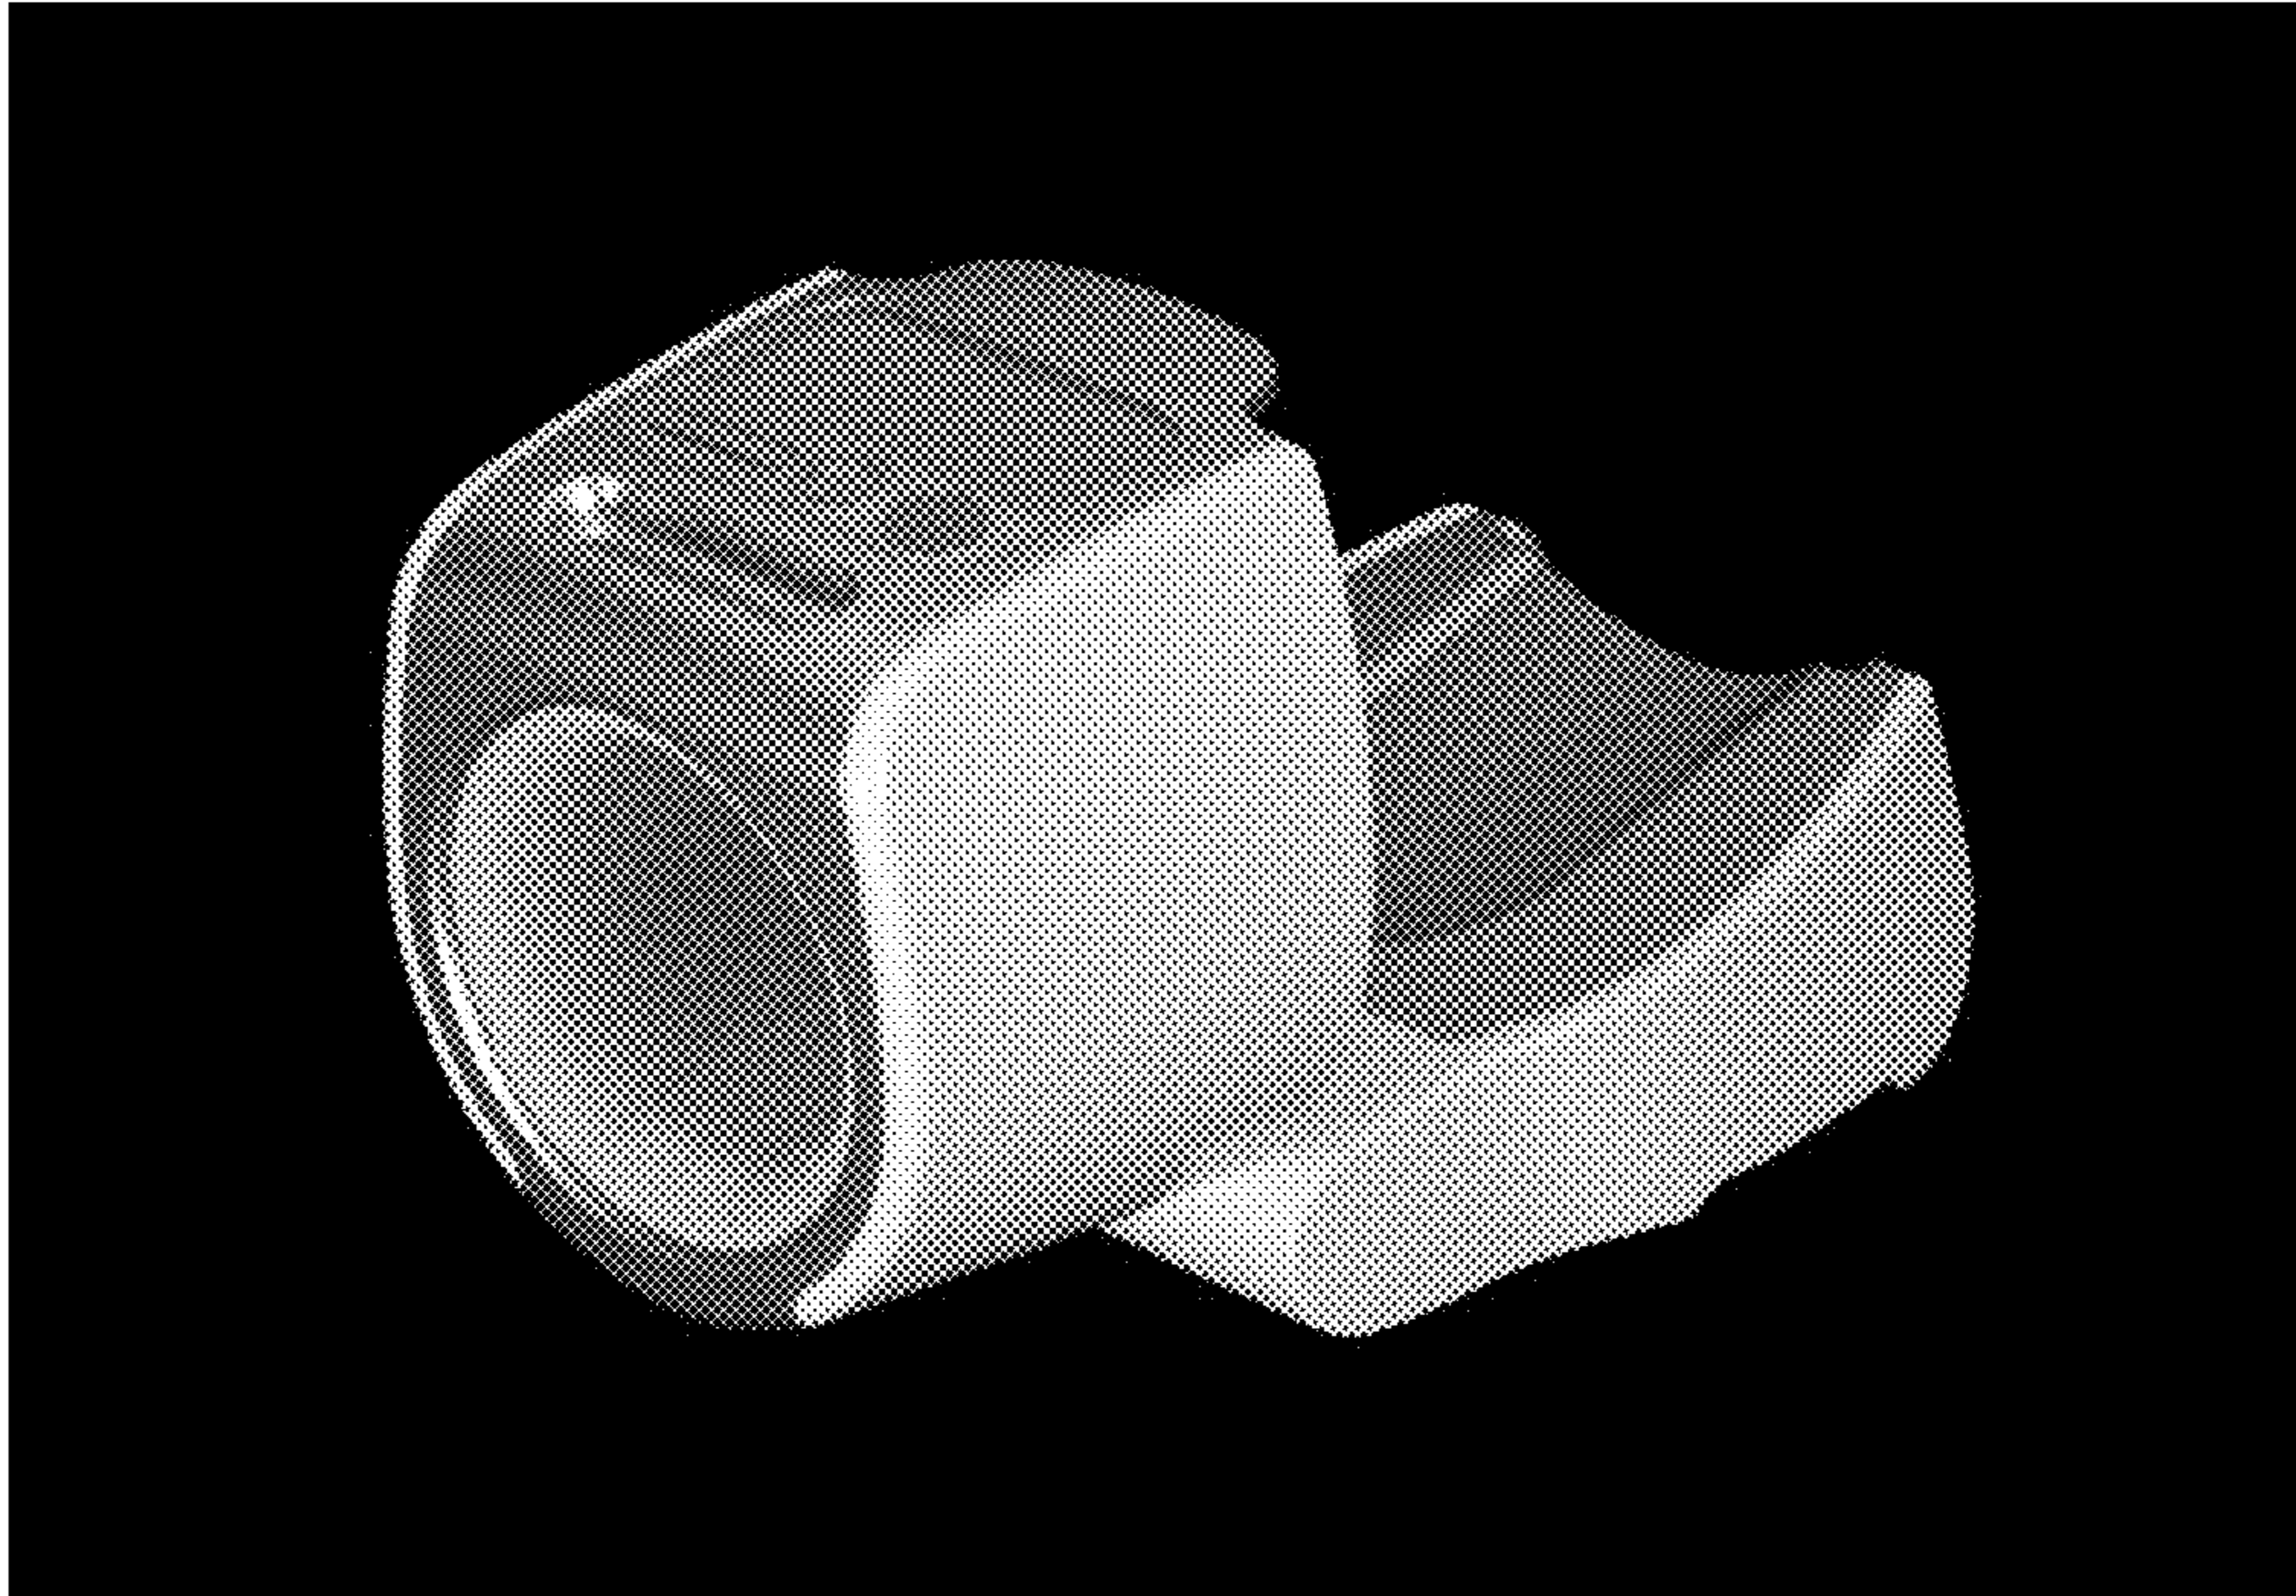


FIG. 10





FIG. 11

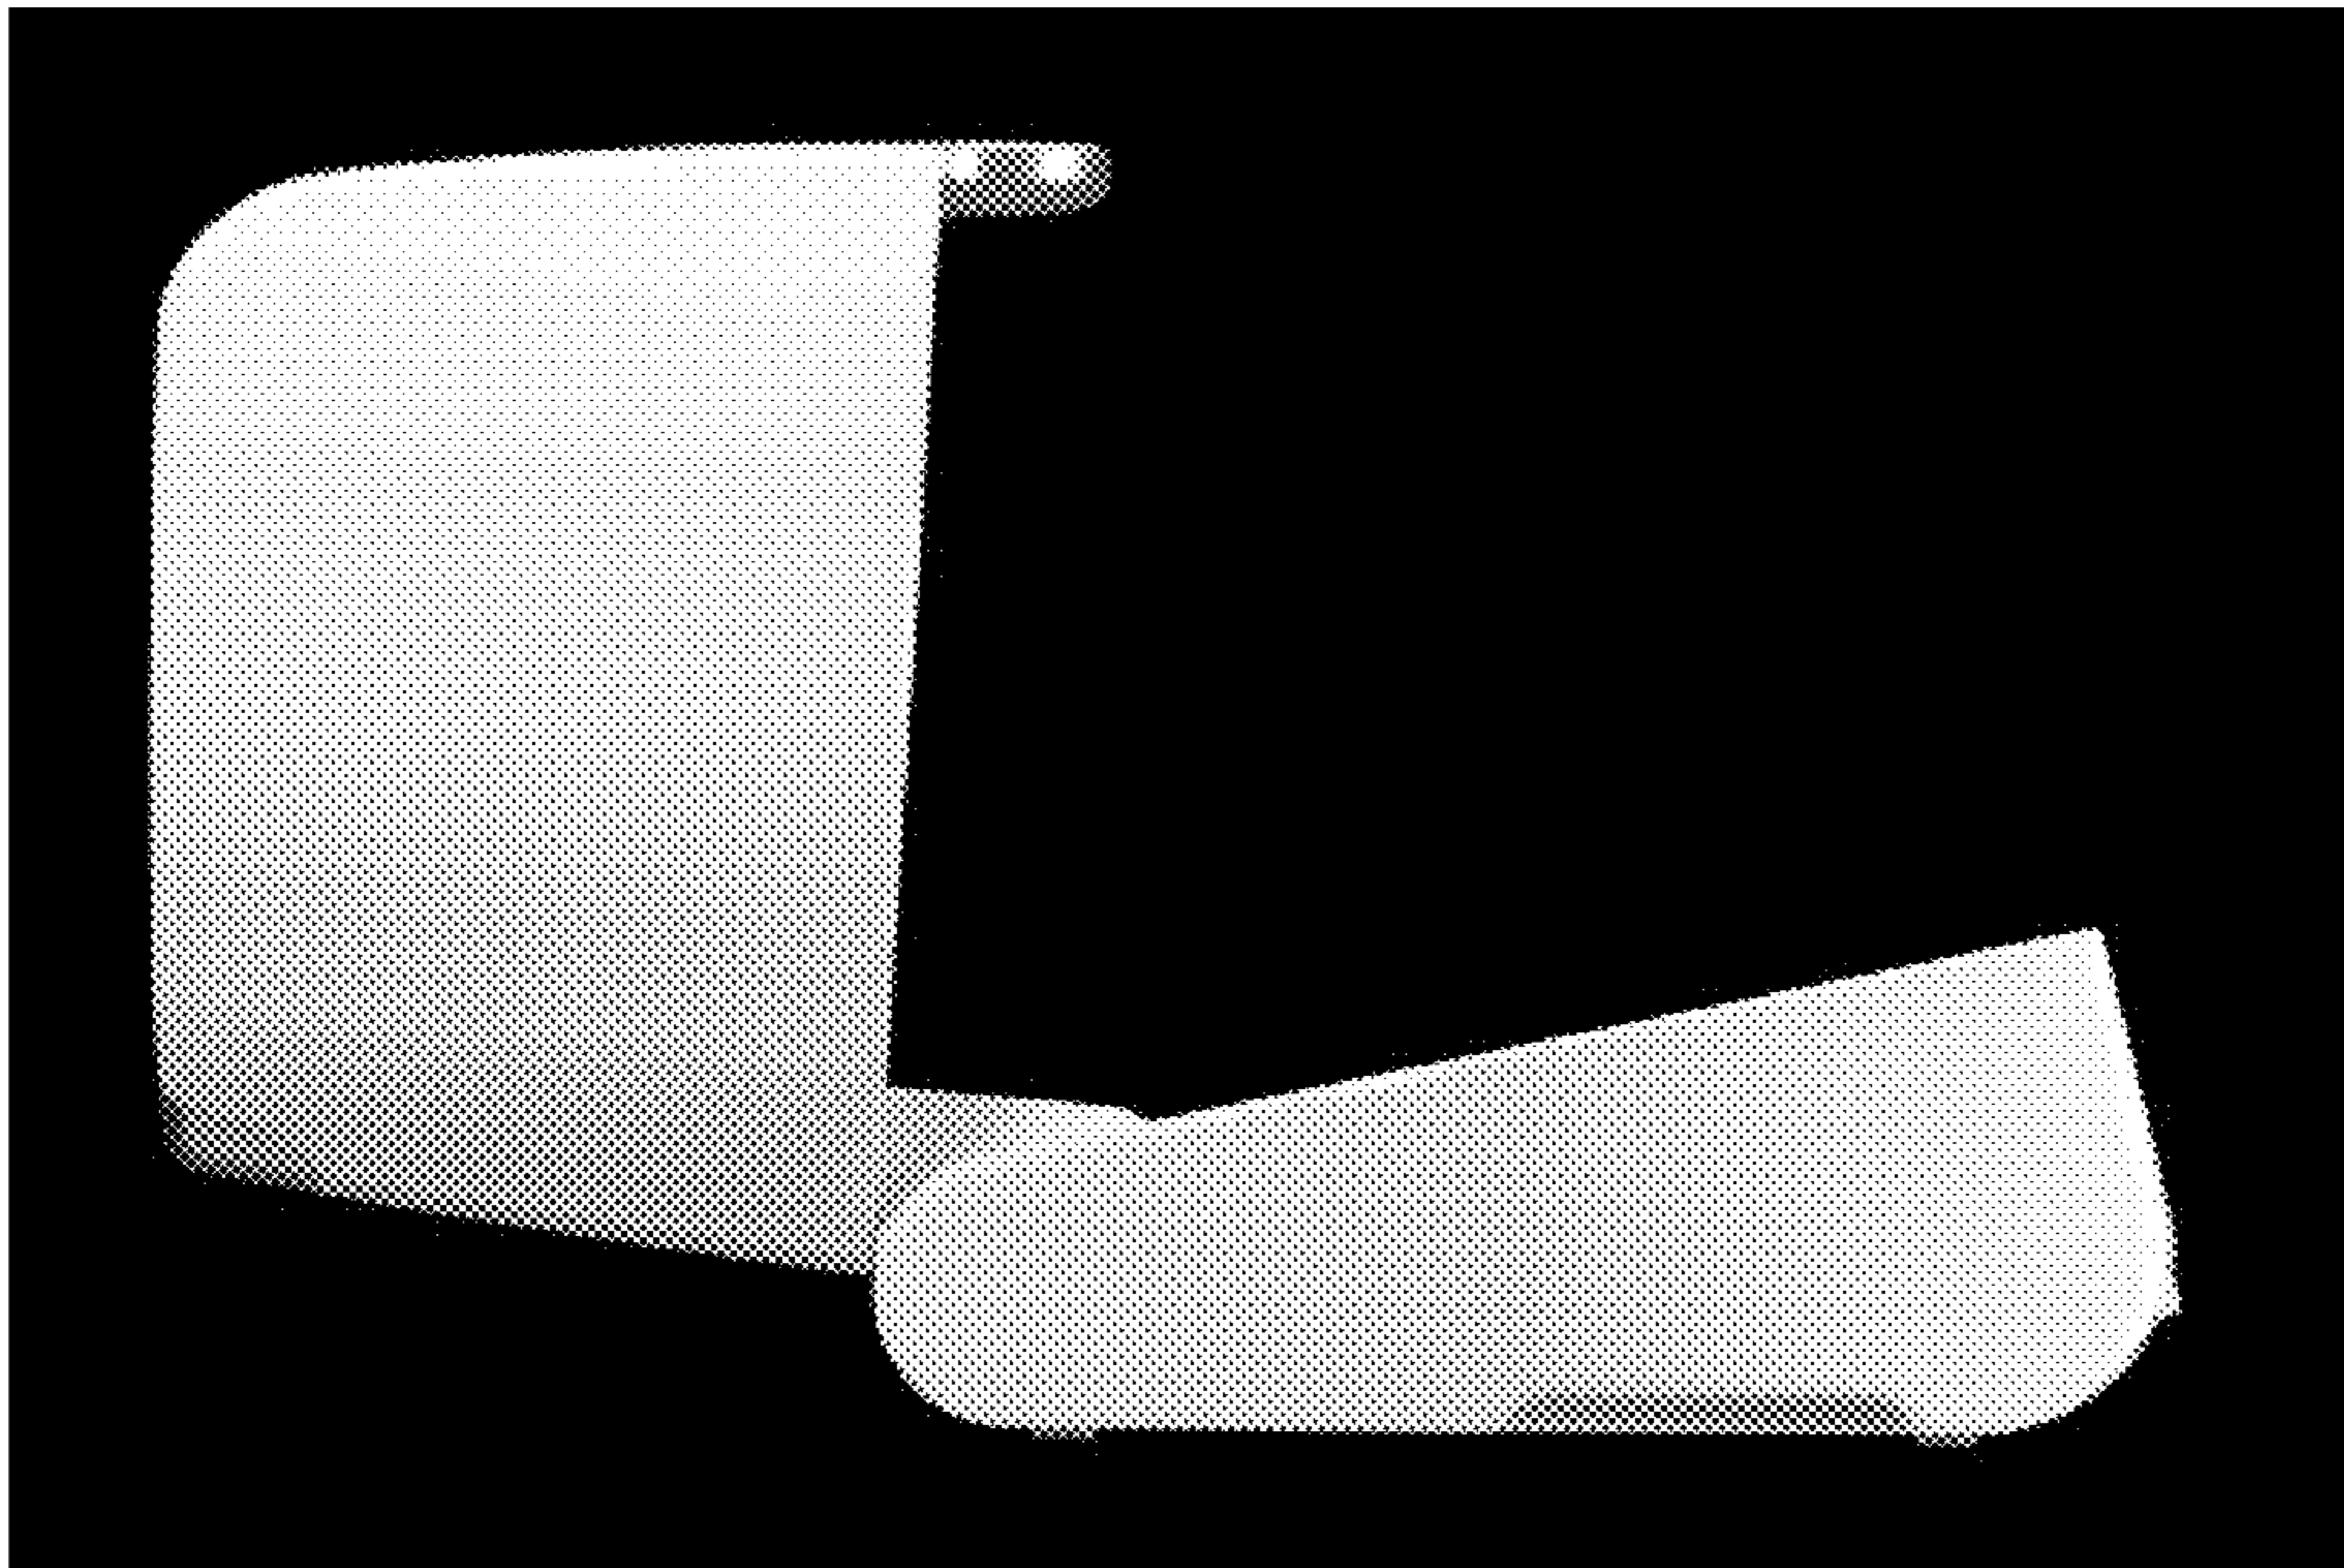


FIG. 12

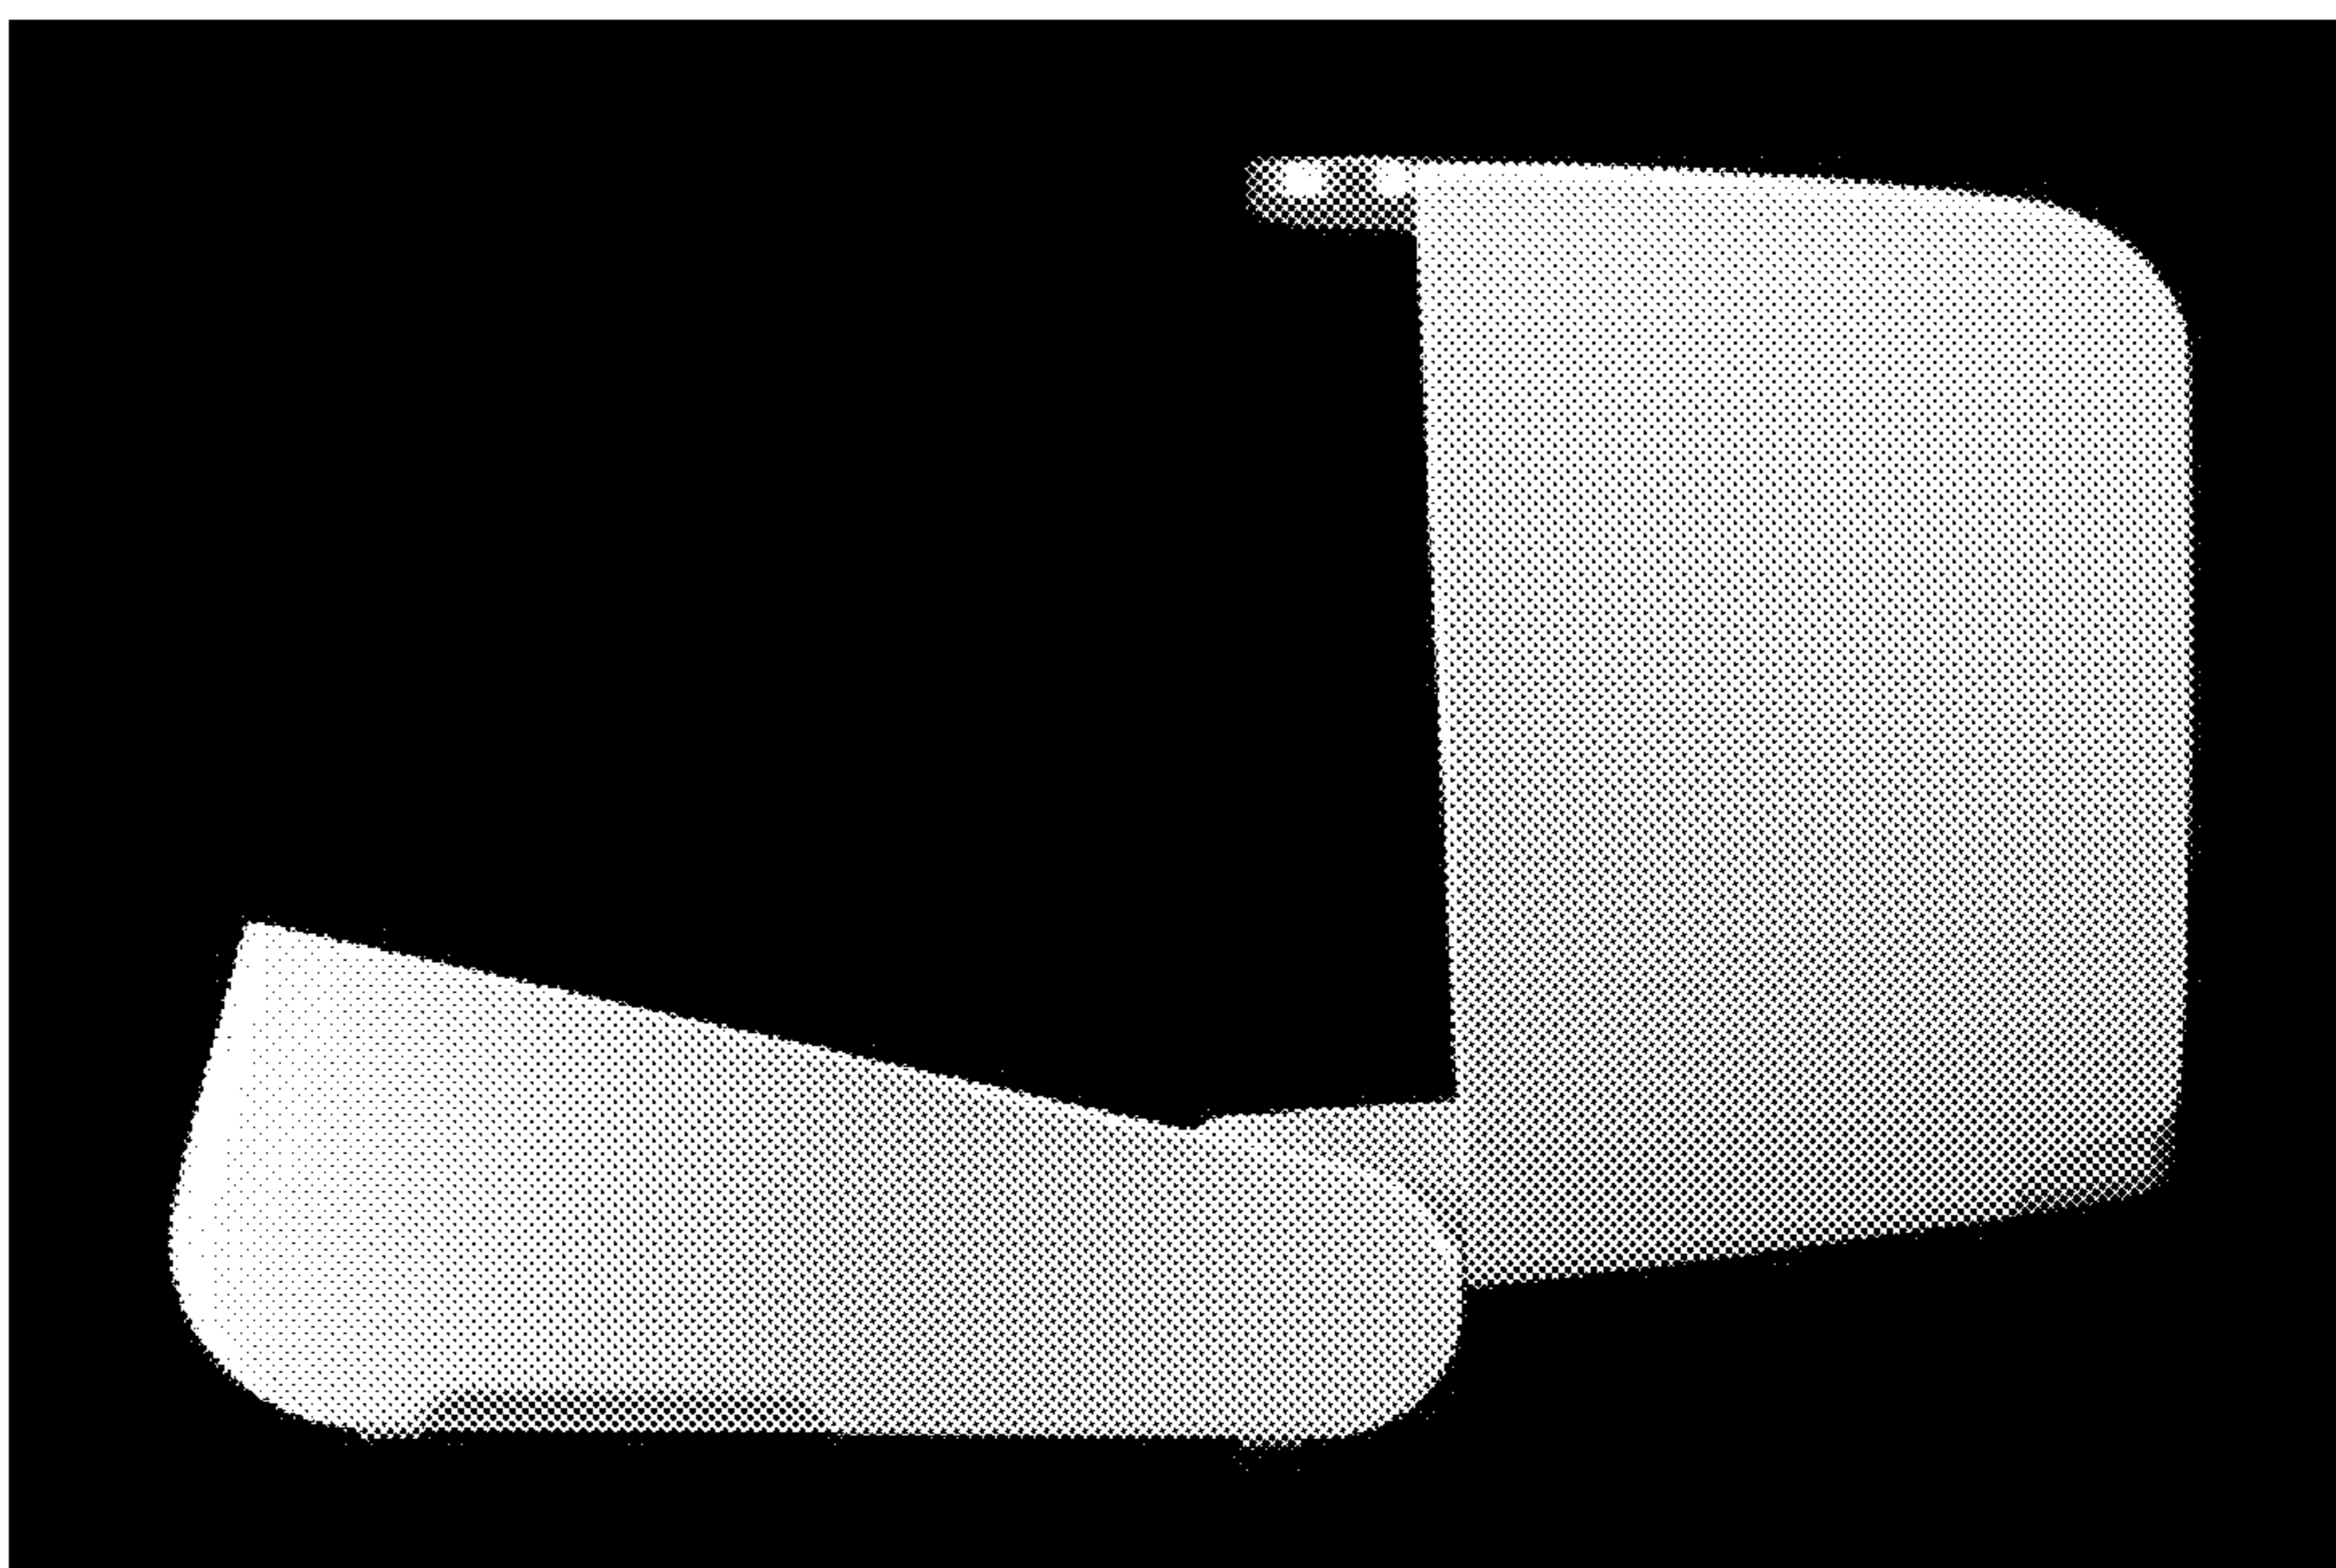




FIG. 13

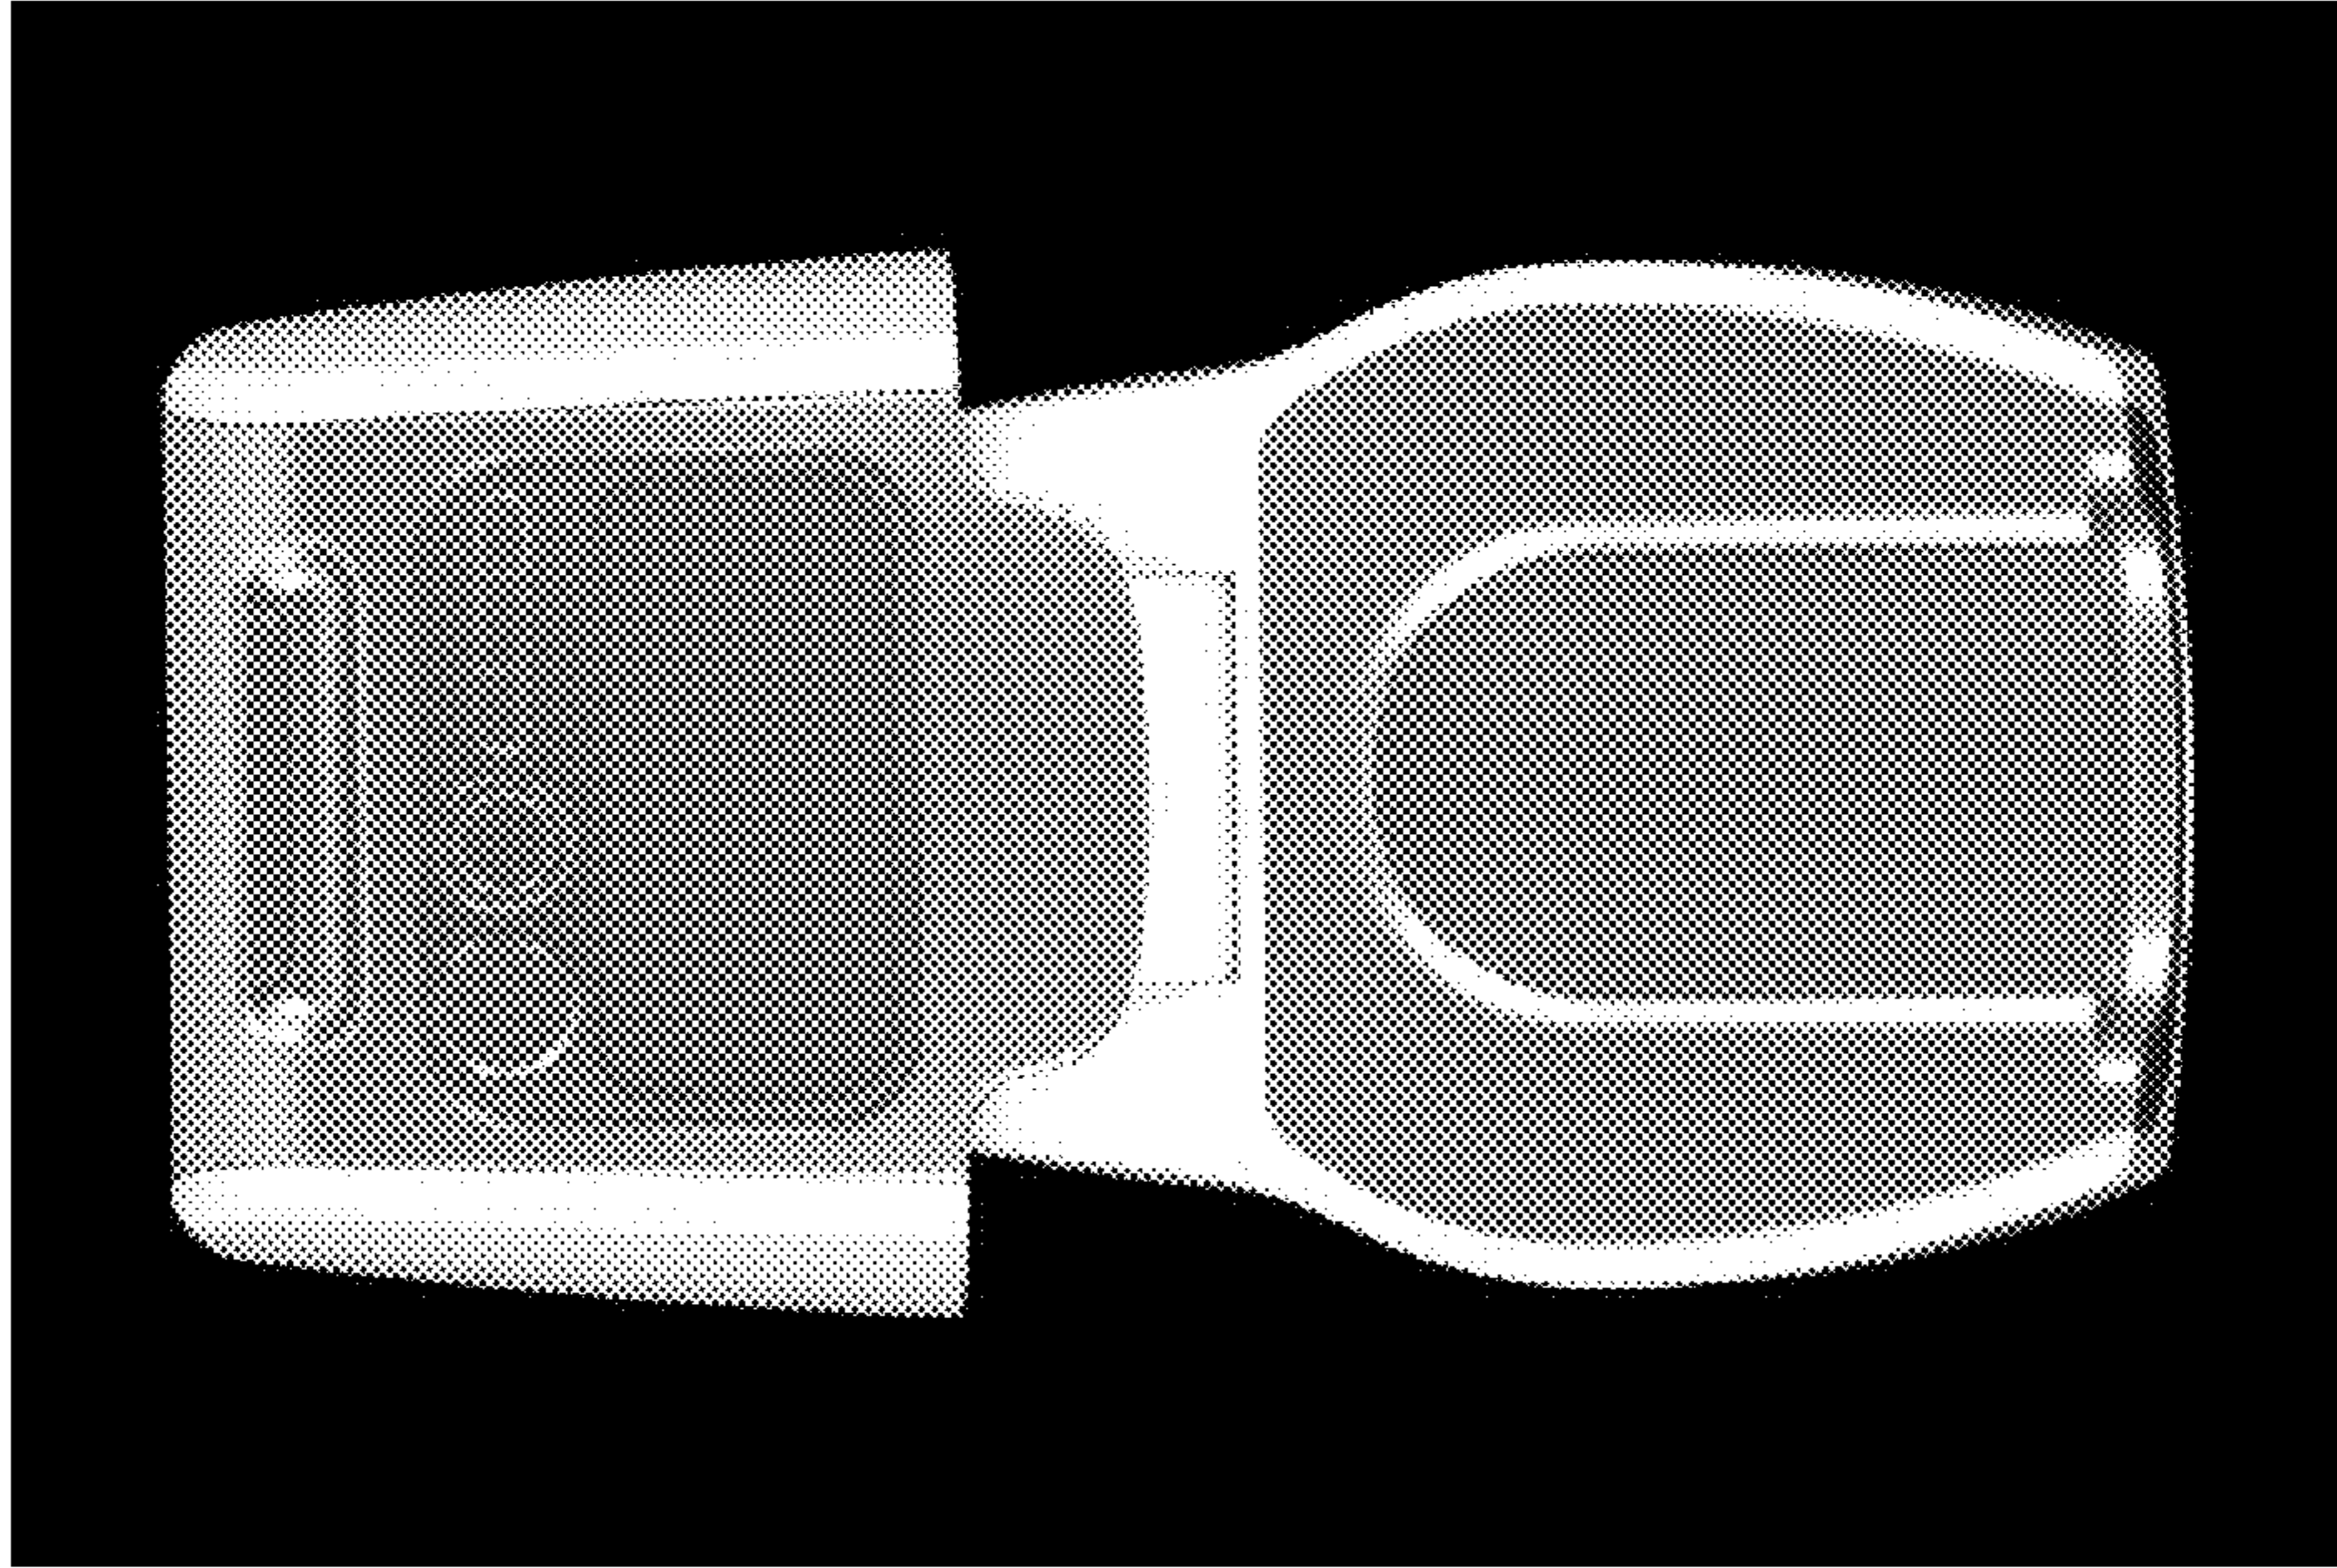


FIG. 14

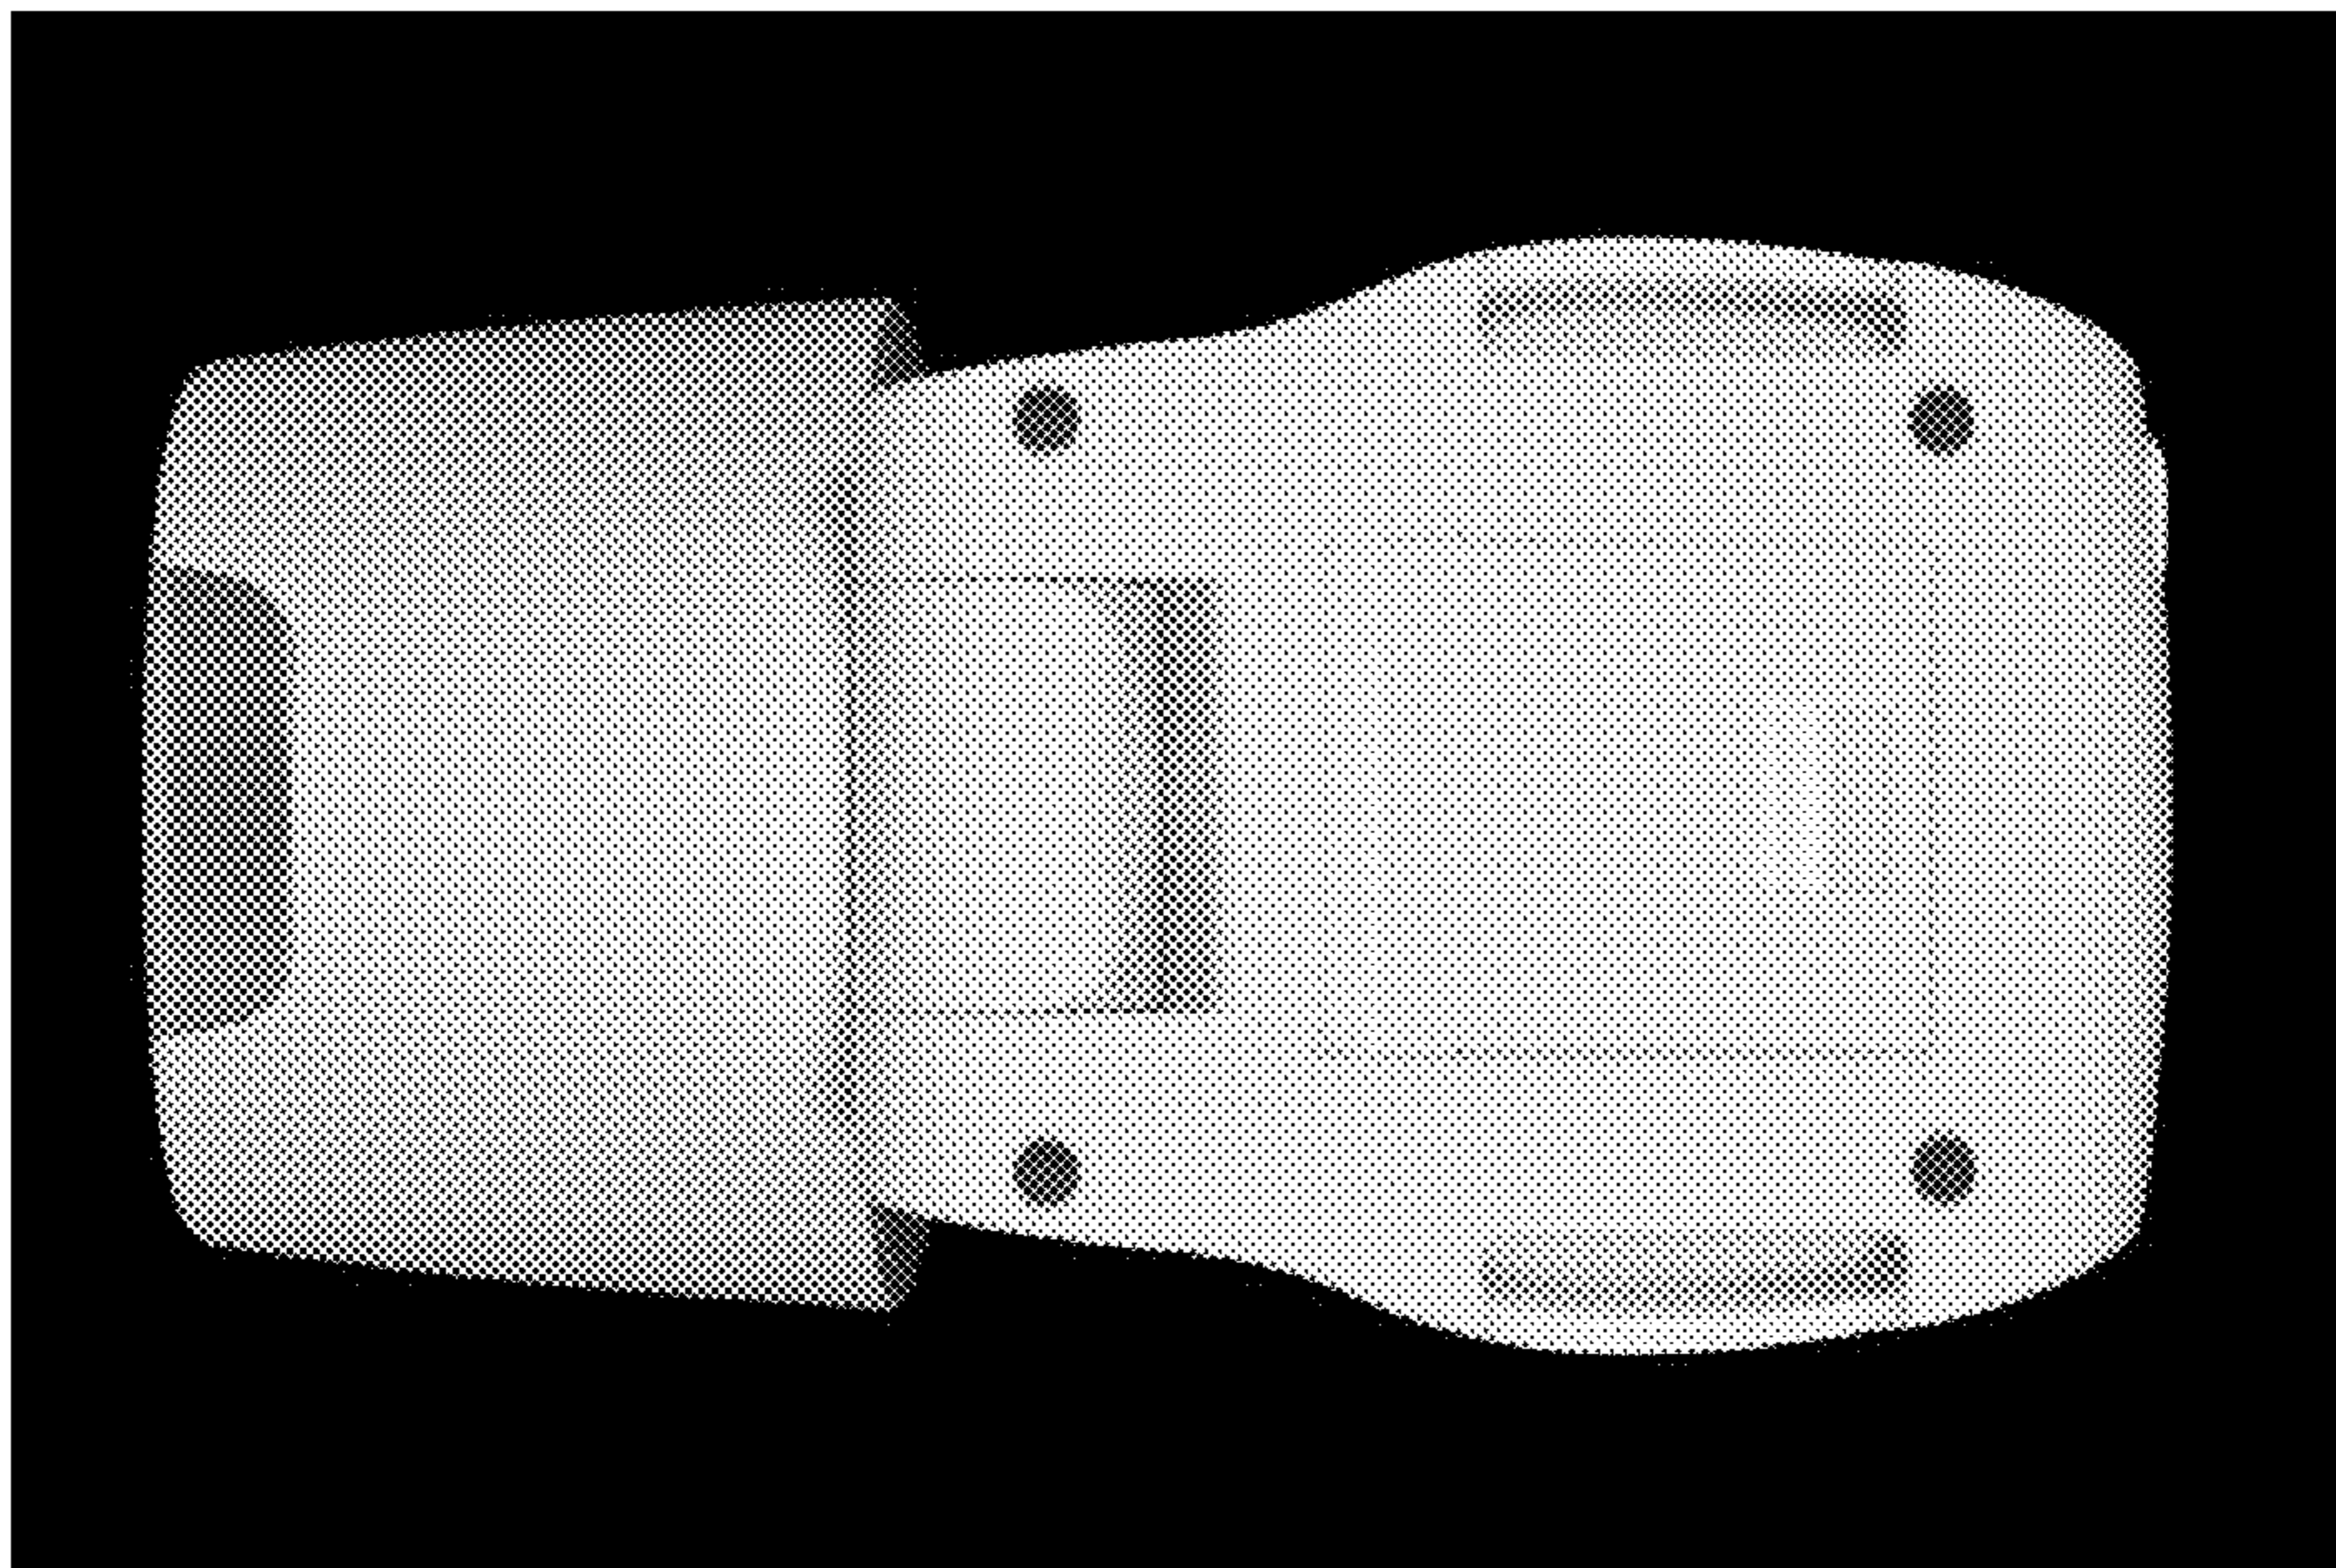


FIG. 15

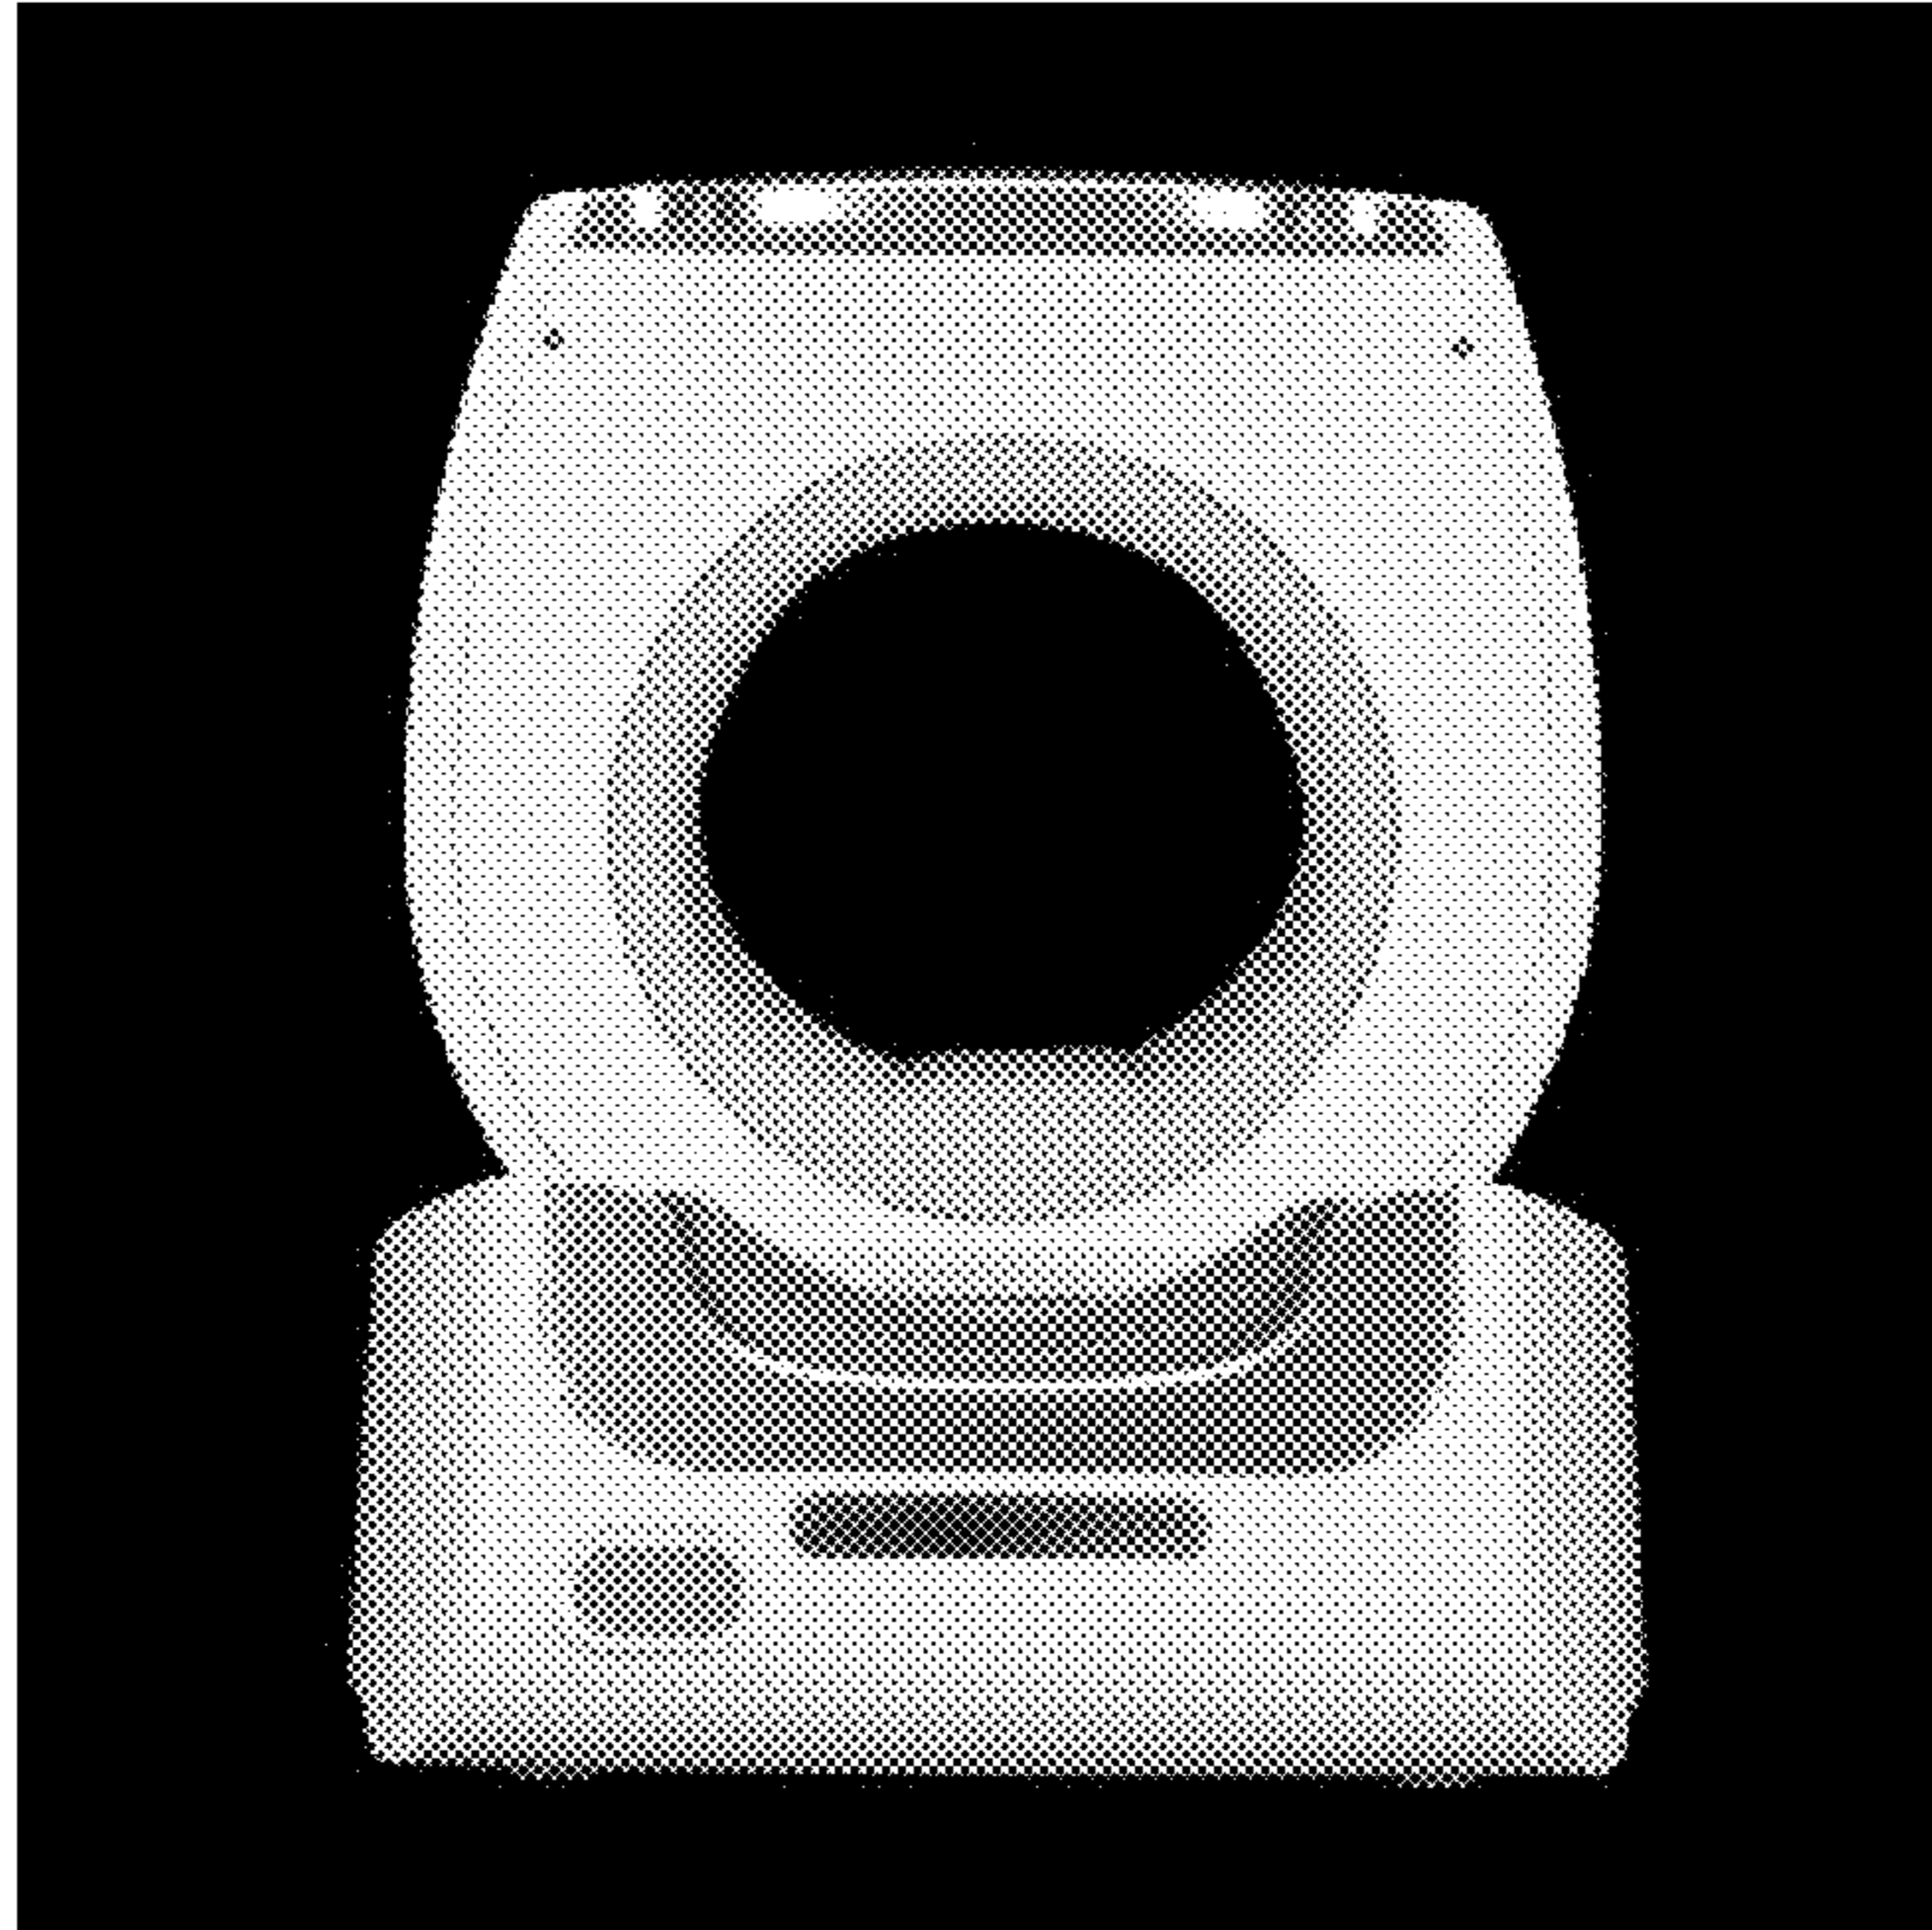


FIG. 16

