



US00D610261S

(12) **United States Design Patent**  
**Strother et al.**

(10) **Patent No.:** **US D610,261 S**  
(45) **Date of Patent:** **\*\* Feb. 16, 2010**

(54) **IMPLANTABLE PULSE GENERATOR**

(75) Inventors: **Robert B. Strother**, Willoughby Hills, OH (US); **Joseph J. Mrva**, Euclid, OH (US); **Geoffrey B. Thrope**, Shaker Heights, OH (US)

(73) Assignee: **Medtronic Urinary Solutions, Inc.**, Minneapolis, MN (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/291,647**

(22) Filed: **Sep. 7, 2007**

**Related U.S. Application Data**

(63) Continuation of application No. 11/517,056, filed on Sep. 7, 2006.

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/186; D24/155**

(58) **Field of Classification Search** ..... D24/144, D24/158, 164, 167, 168, 170, 187, 200, 231; 600/300, 301, 368, 372, 481, 529, 544, 554, 600/561; 607/4, 5, 9, 30  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D250,719 S \* 1/1979 Jacobson et al. .... D24/167  
D269,205 S \* 5/1983 Langer et al. .... D24/167  
D280,930 S \* 10/1985 Speicher et al. .... D24/167  
D316,145 S \* 4/1991 Ware ..... D24/167

5,107,836 A \* 4/1992 Fenster ..... 607/36  
5,144,946 A \* 9/1992 Weinberg et al. .... 607/2  
D337,820 S \* 7/1993 Hooper et al. .... D24/155  
D338,731 S \* 8/1993 Byland et al. .... D24/155  
D343,901 S \* 2/1994 Anderson ..... D24/155  
D478,990 S \* 8/2003 Kroll ..... D24/167  
D523,144 S \* 6/2006 Wenger et al. .... D24/155  
D559,987 S \* 1/2008 Strother et al. .... D24/187

\* cited by examiner

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Shumaker & Sieffert, P.A.

(57) **CLAIM**

The ornamental design for an implantable pulse generator, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an implantable pulse generator showing our new design;

FIG. 2 is a top plan view thereof;

FIG. 3 is a bottom plan view thereof;

FIG. 4 is a left side elevation view thereof;


FIG. 5 is a right side elevation view thereof;

FIG. 6 is a rear elevation view thereof; and,

FIG. 7 is a front elevation view thereof.

The broken lines are included for the purposes of illustrating a portion of the implantable pulse generator that forms no part of the claimed design.

**1 Claim, 1 Drawing Sheet**

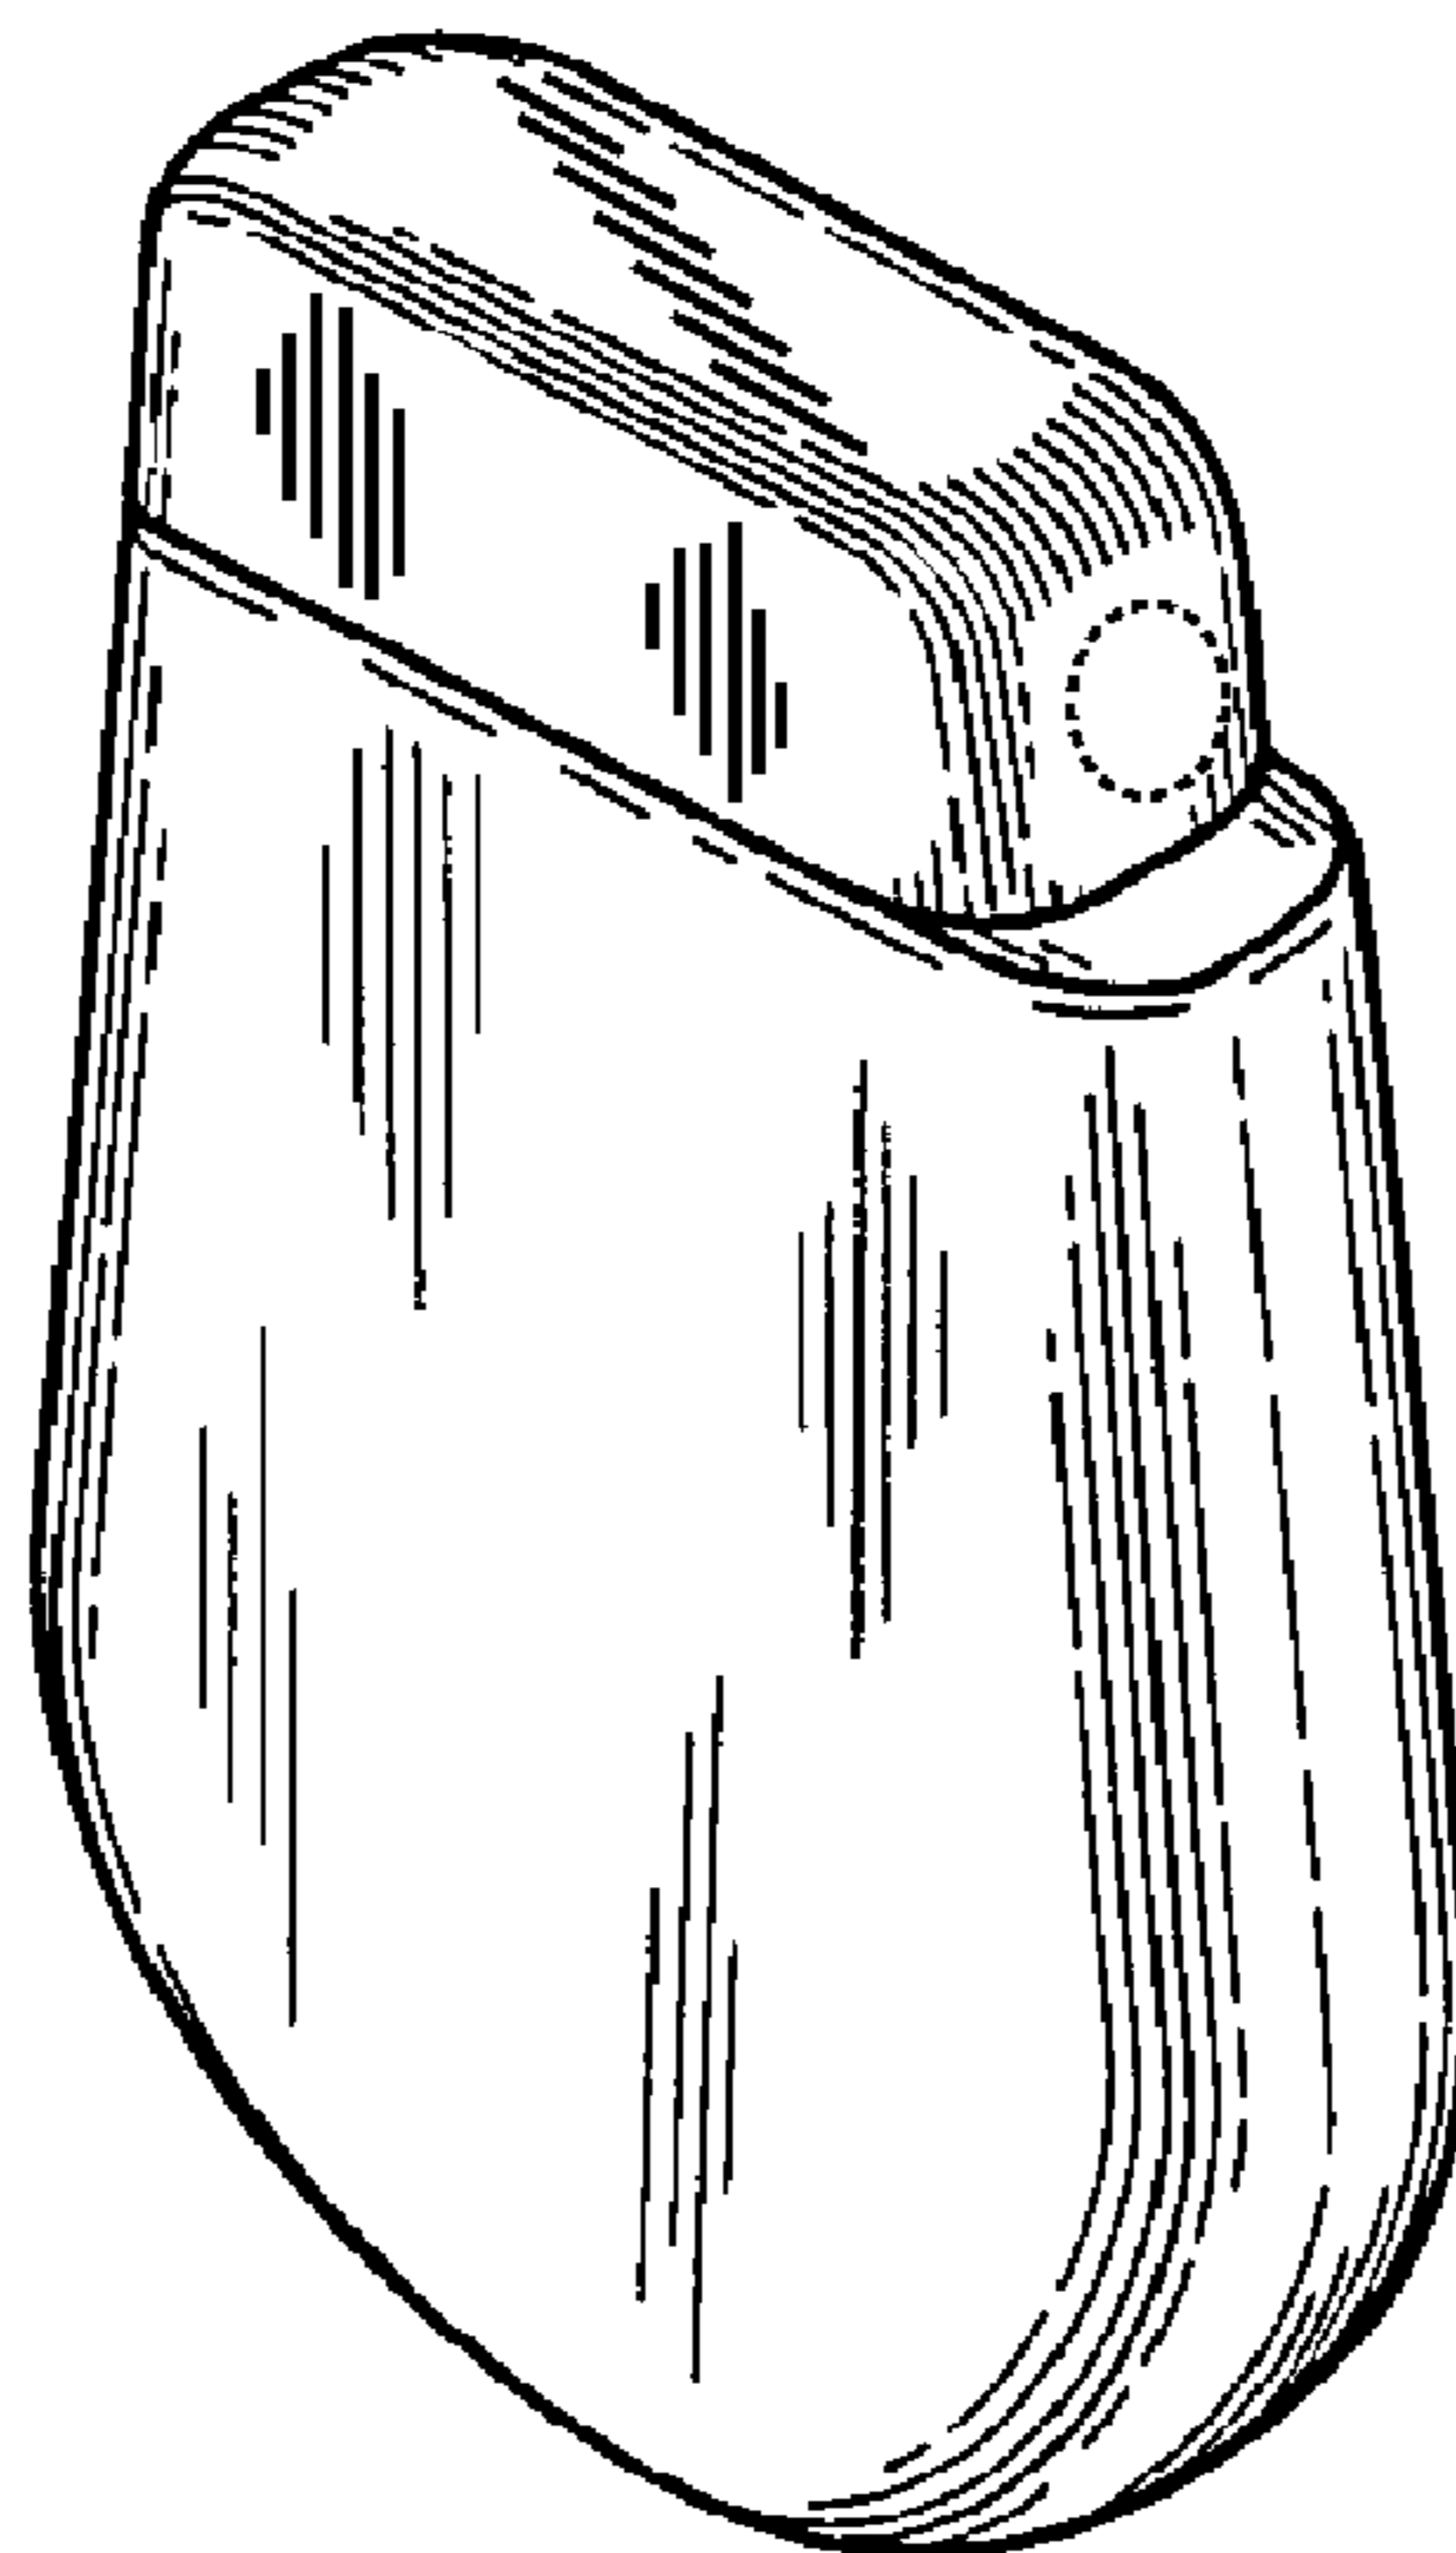

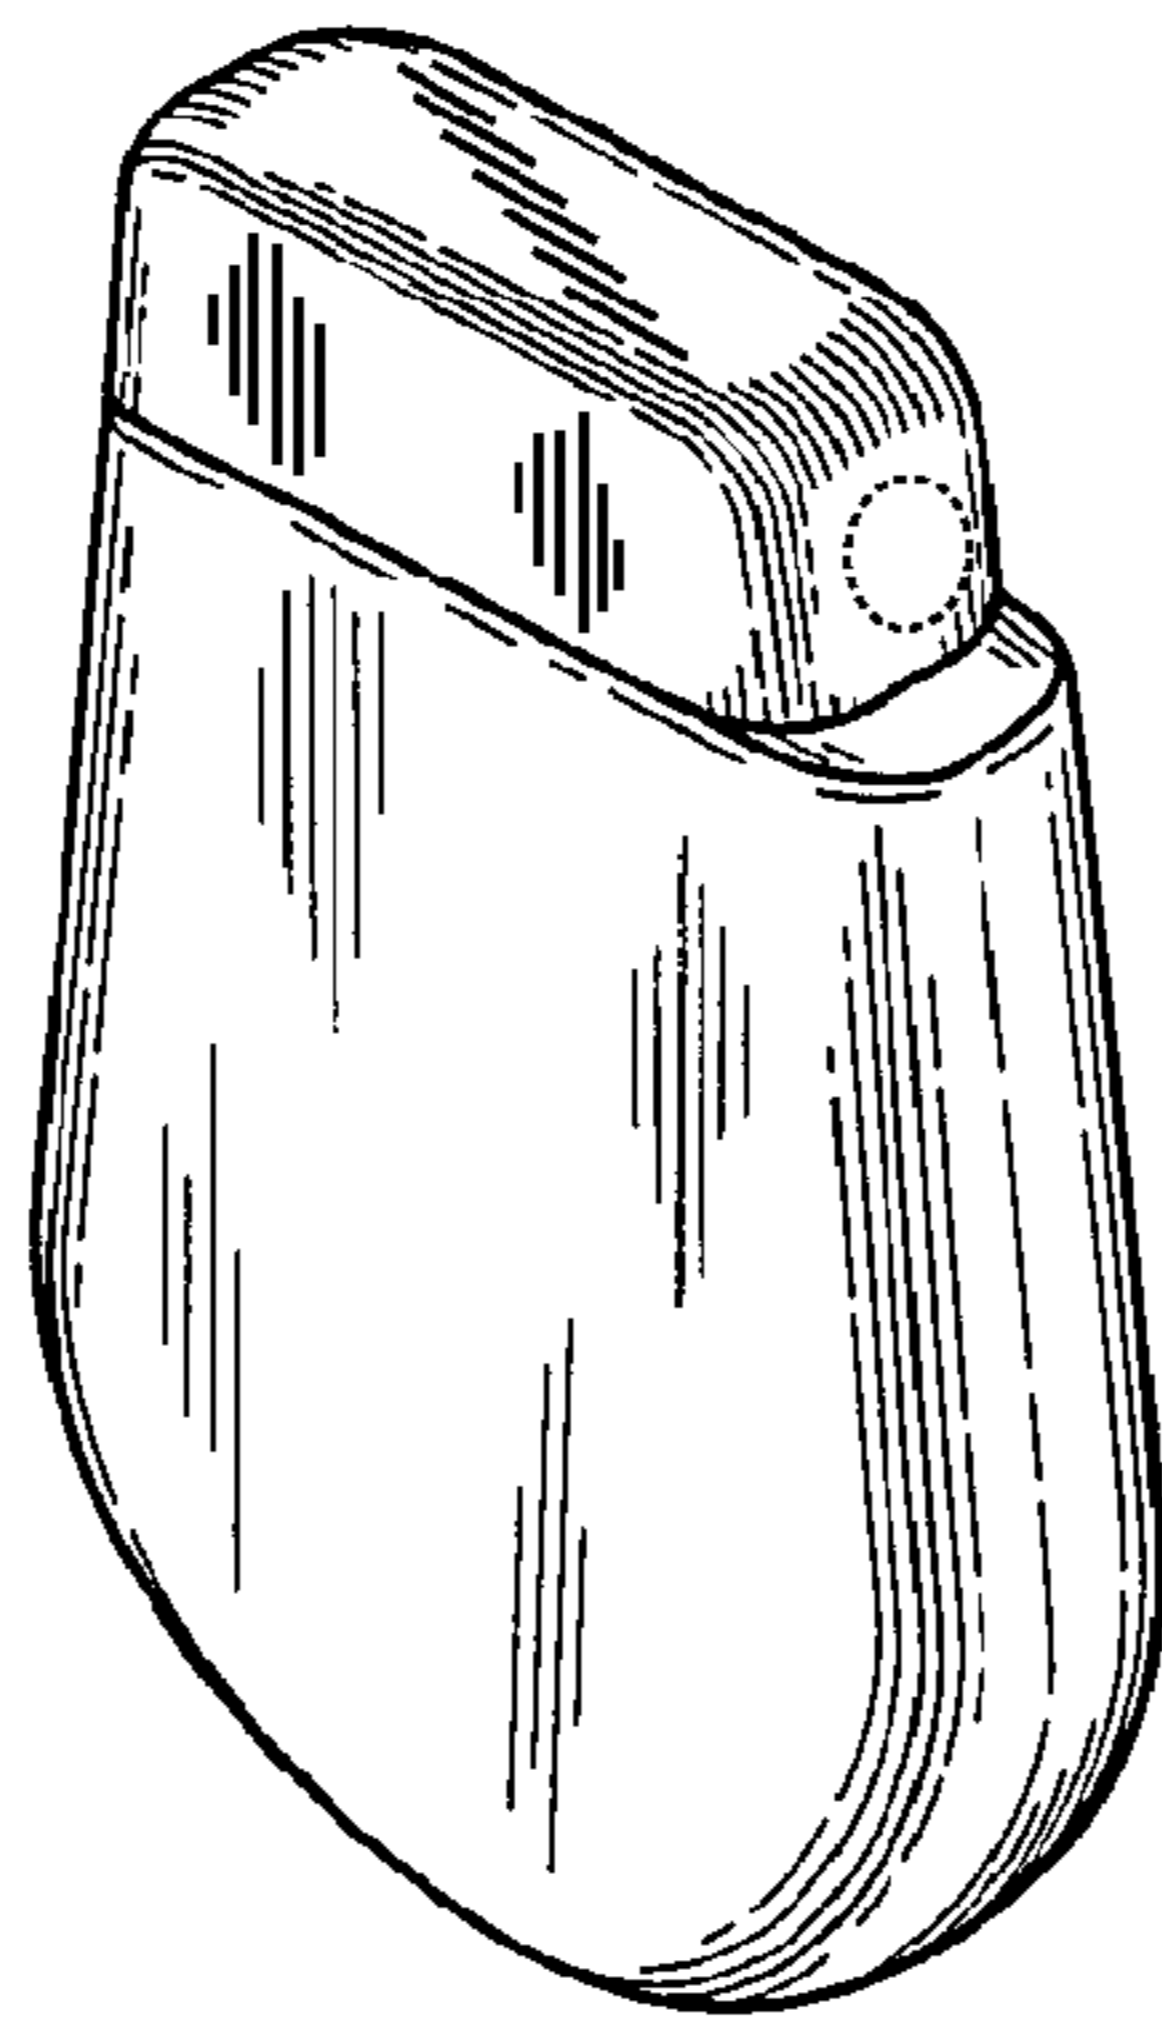


Fig. 1

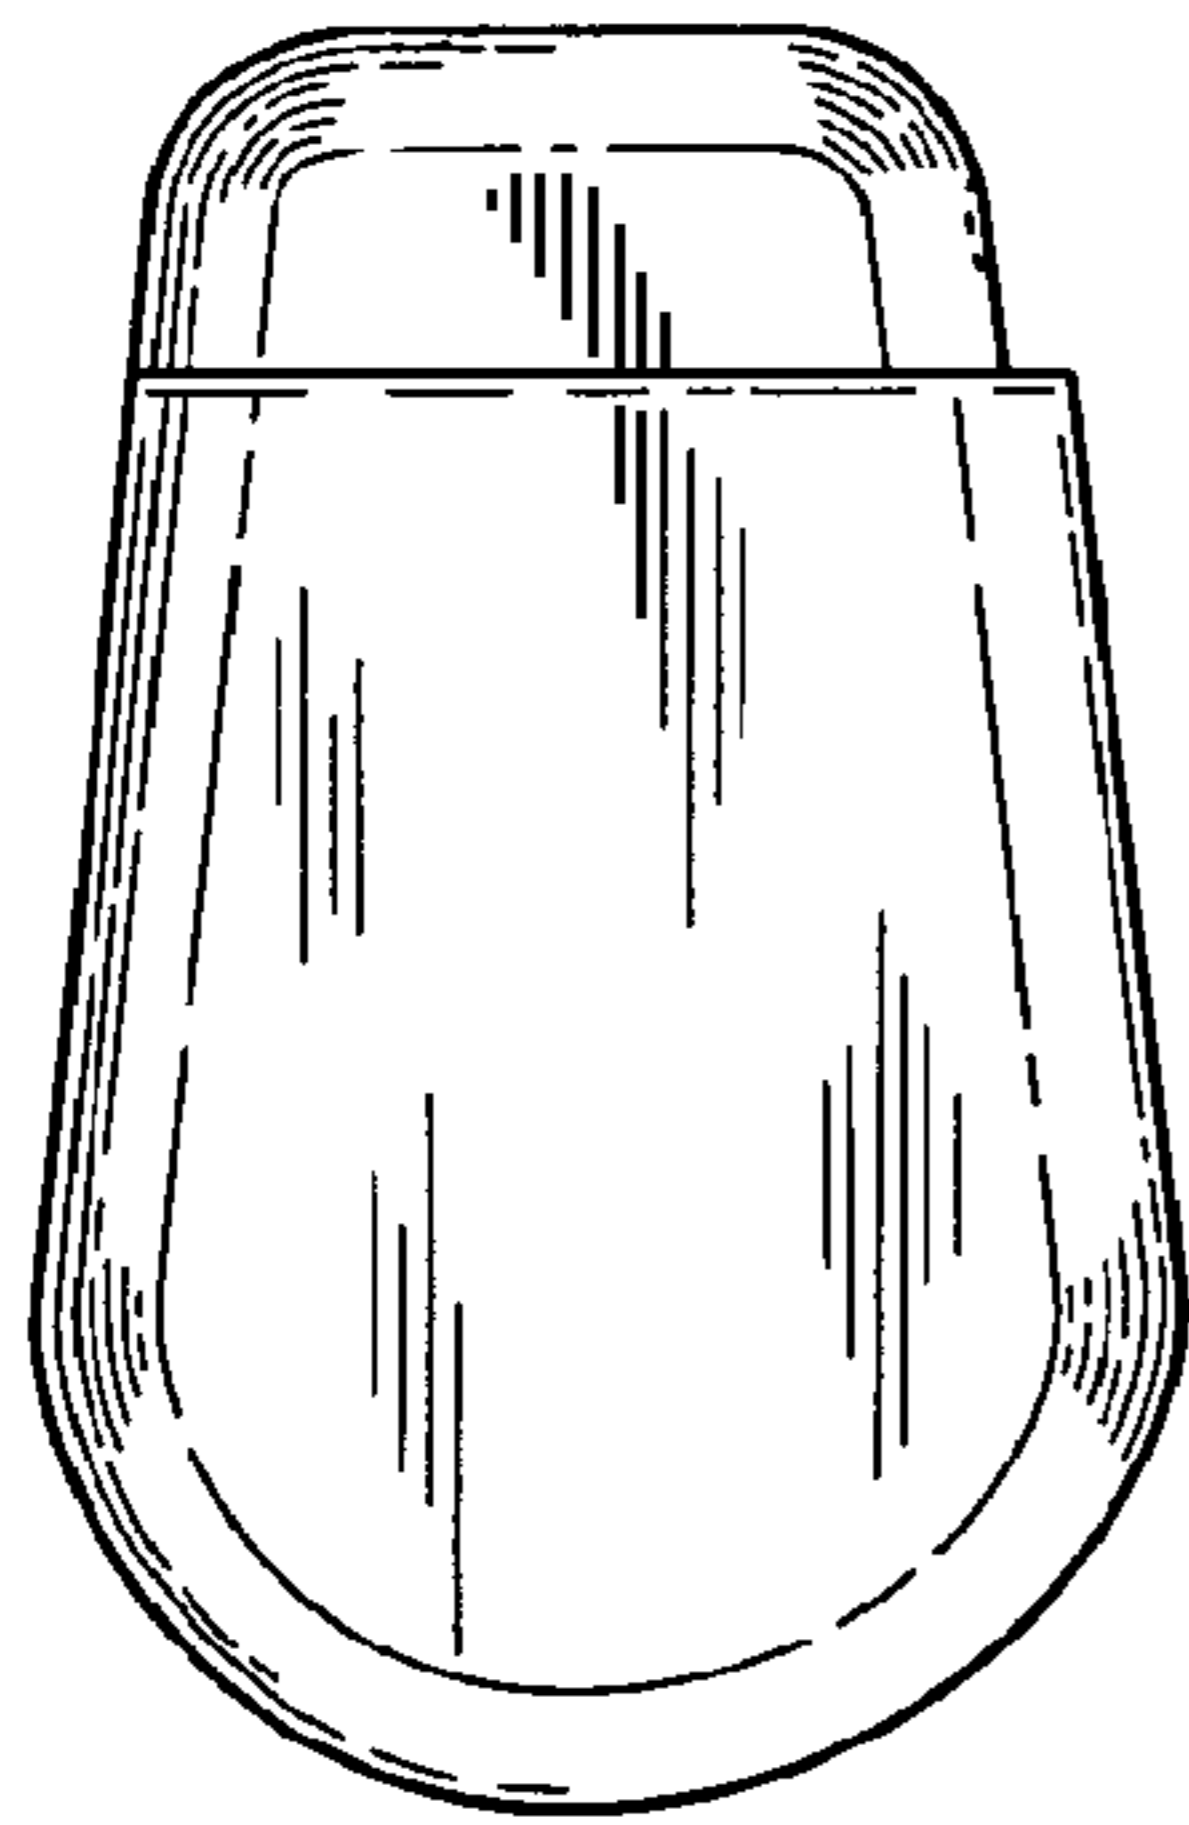


Fig. 2

Fig. 3

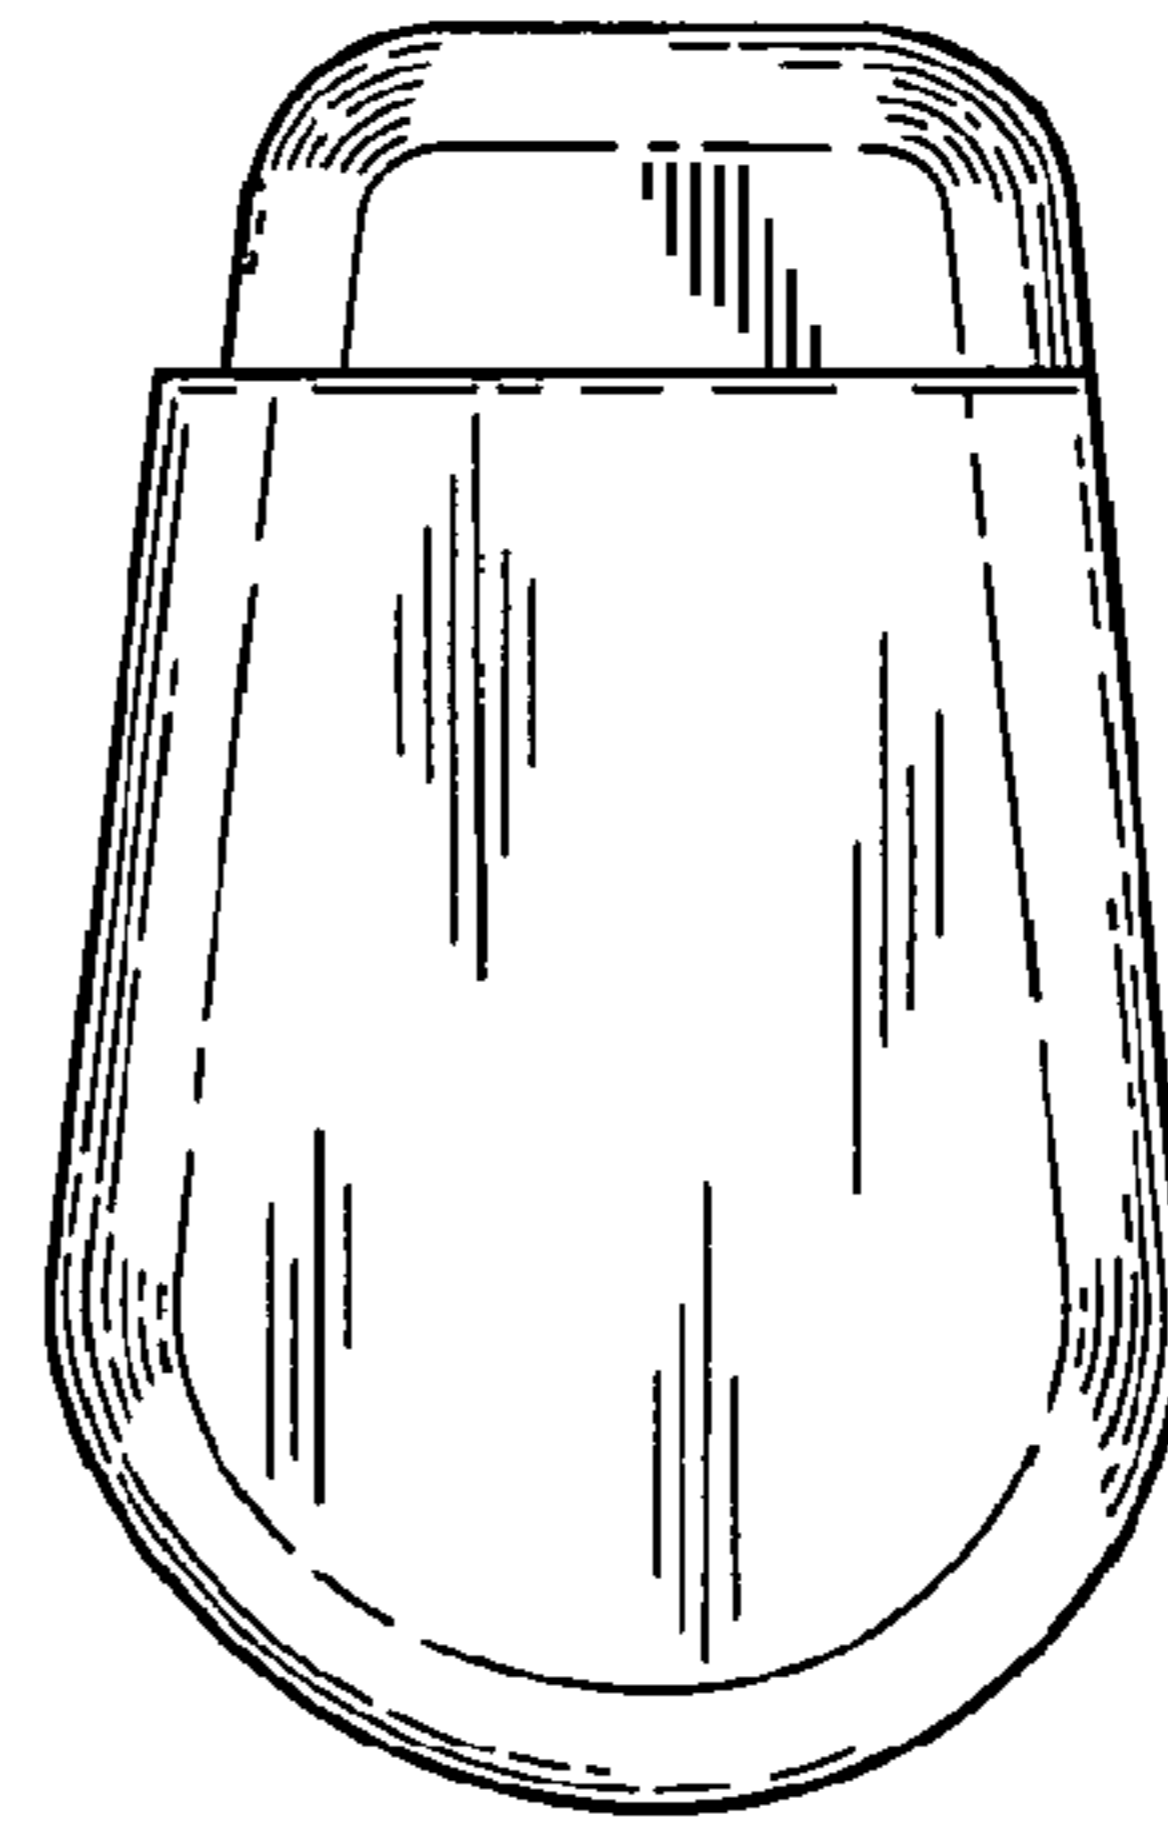


Fig. 4

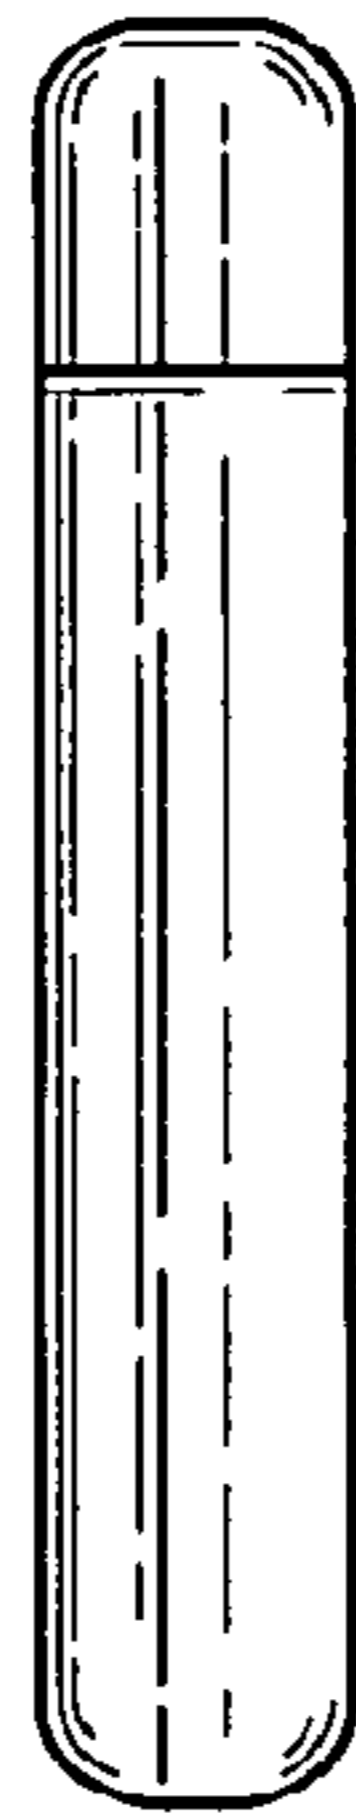


Fig. 5

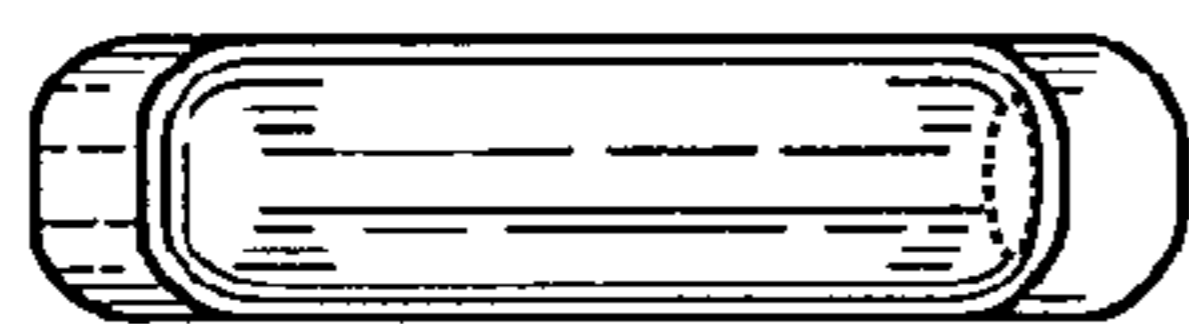
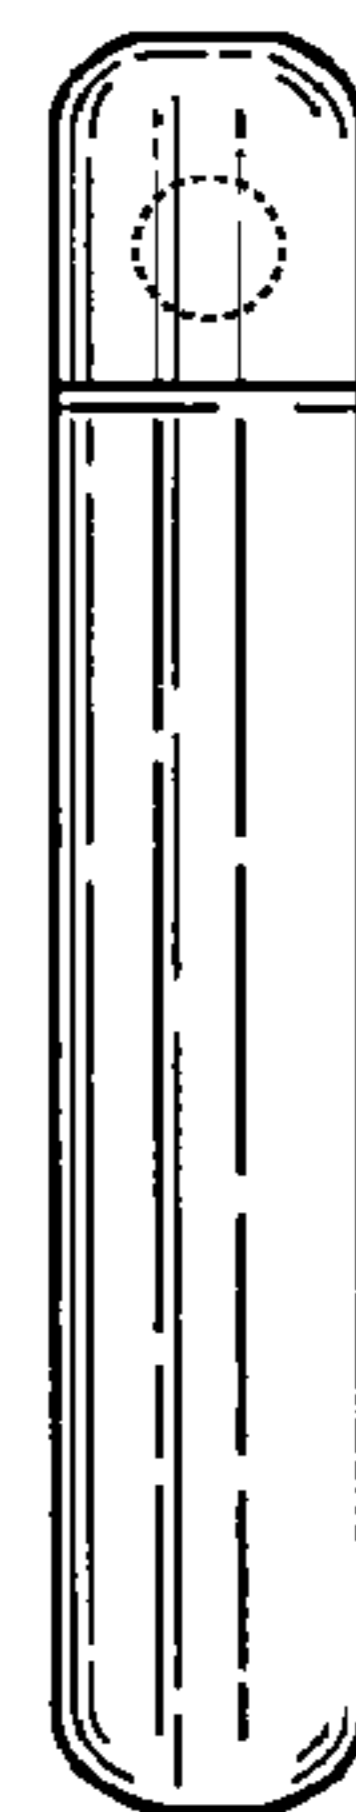


Fig. 6

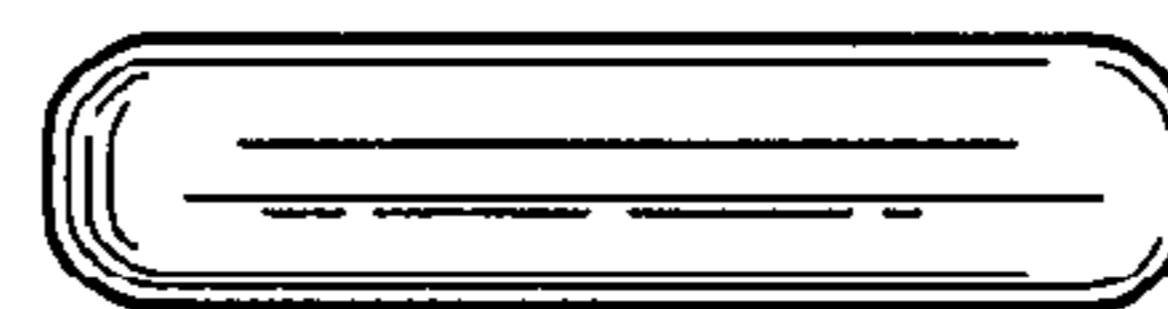


Fig. 7