



US00D611596S

(12) **United States Design Patent**  
**Kousai et al.**

(10) **Patent No.:** **US D611,596 S**  
(45) **Date of Patent:** **\*\* Mar. 9, 2010**

(54) **GUIDE WIRE FOR CATHETER**

(75) Inventors: **Tadashi Kousai**, Shizuoka-ken (JP);  
**Junichi Kobayashi**, Shizuoka-ken (JP);  
**Yasushi Kinoshita**, Shizuoka-ken (JP)

(73) Assignee: **Terumo Kabushiki Kaisha**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/309,714**

(22) Filed: **Sep. 29, 2008**

(30) **Foreign Application Priority Data**

Mar. 27, 2008	(JP)	.....	2008-007637
Mar. 27, 2008	(JP)	.....	2008-007638
Mar. 27, 2008	(JP)	.....	2008-007639
Mar. 27, 2008	(JP)	.....	2008-007640

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/130**

(58) **Field of Classification Search** ..... D24/112,  
D24/130; 604/164.01, 164.05, 165.3, 167,  
604/160, 161, 523, 264, 167.02, 272, 533,  
604/525, 905, 912, 177, 83, 921, 539  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

5,247,942 A \* 9/1993 Prather et al. .... 600/585

(Continued)

**OTHER PUBLICATIONS**

“Cheer Leader” Tri-Med Corporation issued before Mar. 27, 2008.

(Continued)

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Jean C. Edwards, Esq.;  
Akerman Senterfitt

(57) **CLAIM**

The ornamental design for a guide wire for catheter, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the front, left and top of a guide wire for catheter according to one embodiment showing our new design;

FIG. 2 is a front view thereof;

FIG. 3 is rear view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a bottom view thereof;

FIG. 6 is a left side view thereof;

FIG. 7 is a right side view thereof;

FIG. 8 is an enlarged left side view thereof;

FIG. 9 is an enlarged right side view thereof;

FIG. 10 is a partially enlarged view at 10—10 shown in FIG. 2 thereof;

FIG. 11 is a partially enlarged view at 11—11 shown in FIG. 2 thereof;

FIG. 12 is a partially enlarged view at 12—12 shown in FIG. 2 thereof;

FIG. 13 is a partially enlarged view at 13—13 shown in FIG. 2 thereof;

FIG. 14 is a partially enlarged view at 14—14 shown in FIG. 4 thereof;


FIG. 15 is a partially enlarged view at 15—15 shown in FIG. 4 thereof;

FIG. 16 is a partially enlarged view at 16—16 shown in FIG. 4 thereof; and,

FIG. 17 is a partially enlarged view at 17—17 shown in FIG. 4 thereof.

The elements shown in broken lines are for illustrative purposes only and form no part of the claimed design.

**1 Claim, 5 Drawing Sheets**

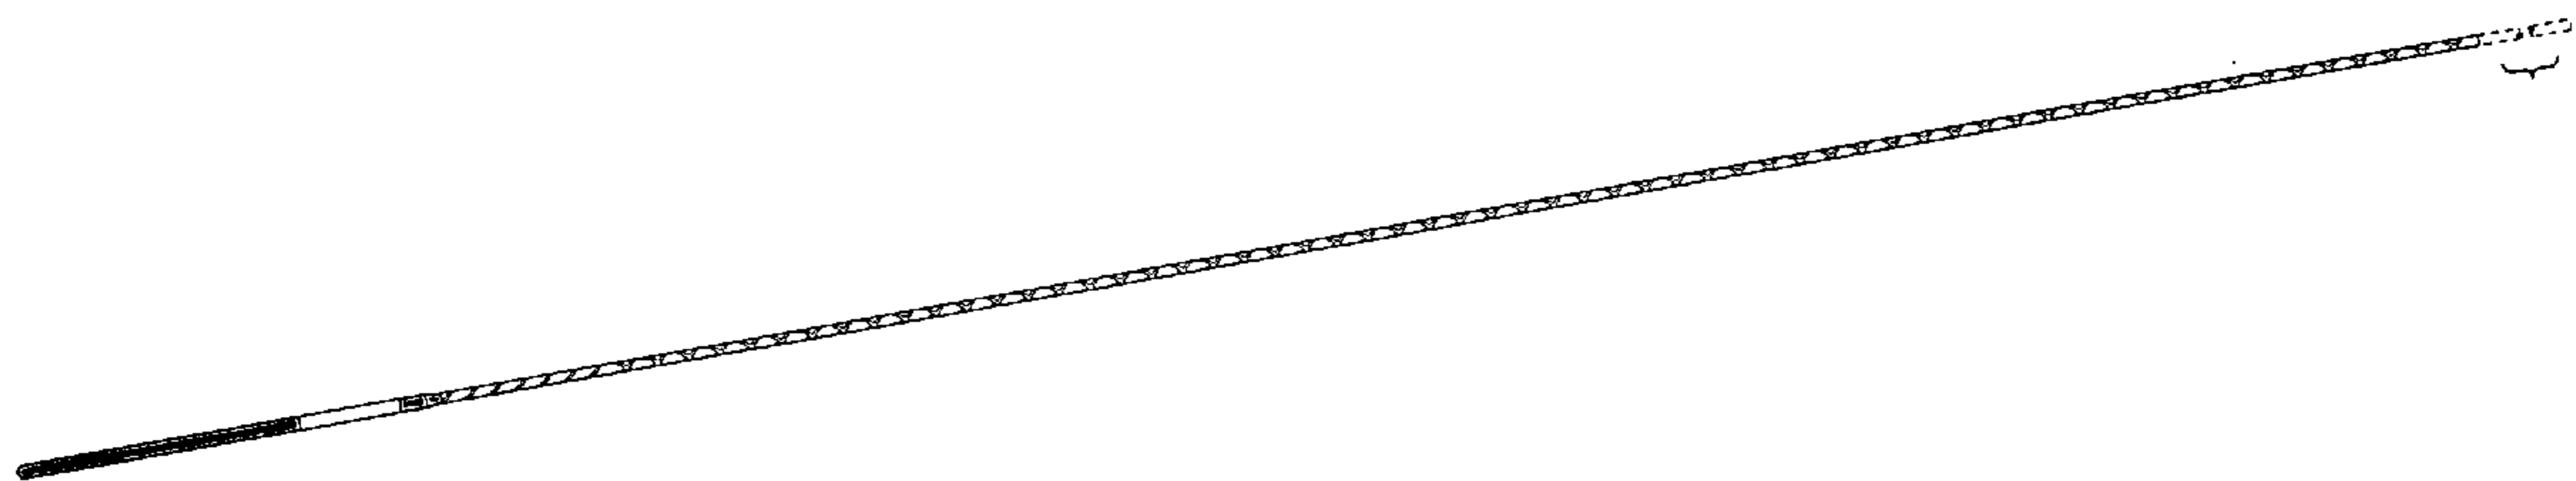

# US D611,596 S

Page 2

---

## U.S. PATENT DOCUMENTS

5,379,779 A 1/1995 Rowland et al.  
D363,544 S \* 10/1995 Rowland et al. .... D24/140  
D363,776 S \* 10/1995 Rowland et al. .... D24/140  
D392,037 S \* 3/1998 Musgrave et al. .... D24/112  
6,143,013 A \* 11/2000 Samson et al. .... 606/192  
6,368,316 B1 \* 4/2002 Jansen et al. .... 604/526  
D496,728 S \* 9/2004 Holsinger ..... D24/130  
6,811,958 B2 11/2004 Iwami et al.  
7,104,979 B2 \* 9/2006 Jansen et al. .... 604/525  
7,278,973 B2 10/2007 Iwami et al.

2004/0024435 A1 \* 2/2004 Leckrone et al. .... 607/101  
2007/0060944 A1 \* 3/2007 Boldenow et al. .... 606/200  
2009/0157162 A1 \* 6/2009 Chow et al. .... 623/1.11

## OTHER PUBLICATIONS

“Hydra Jagwire High Performance guidewire” Boston Scientific Japan Corporation issued before Mar. 27, 2008.  
“Tracer Metro Direct Wire Guide with Aqua Coat Tip” Wilson-Cook Medical Incorporation issued in 2002.

\* cited by examiner

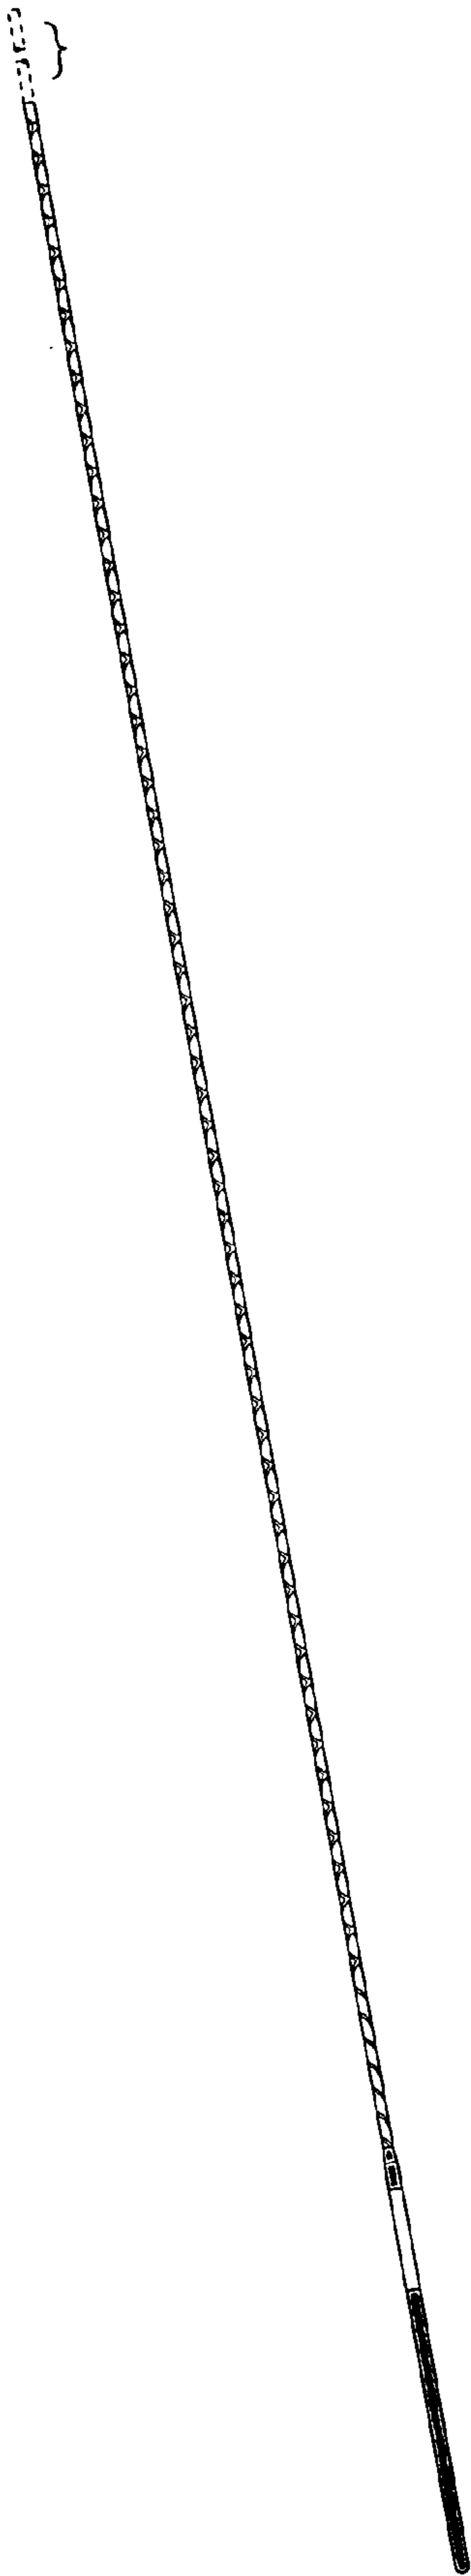


FIG. 1

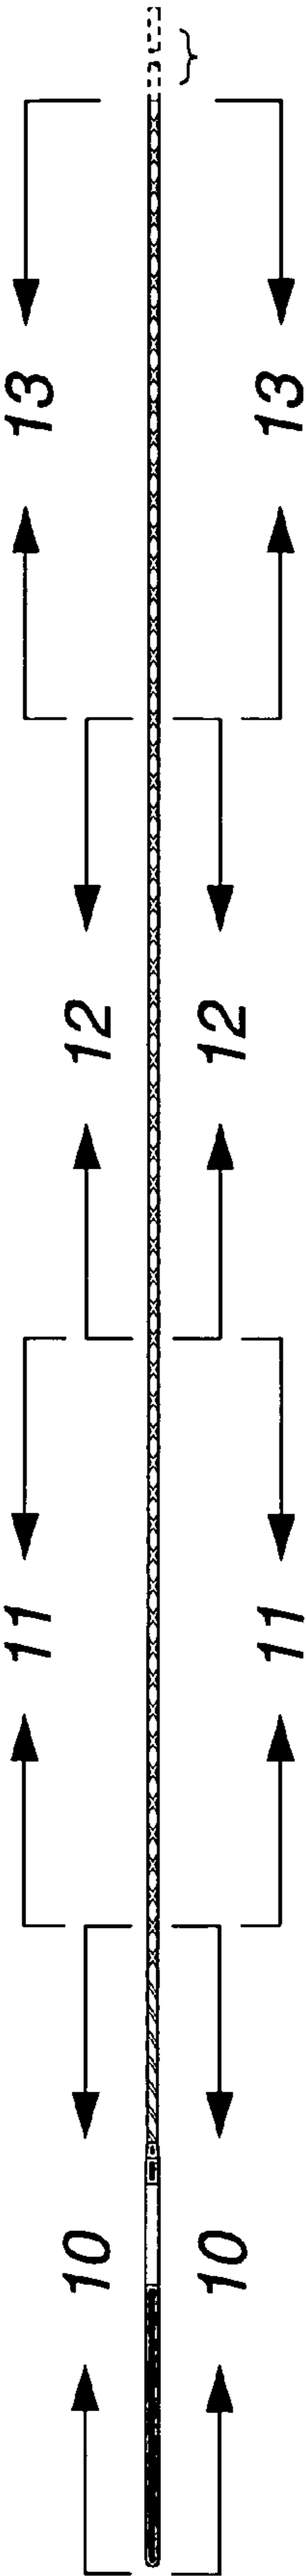


FIG. 2



FIG. 3

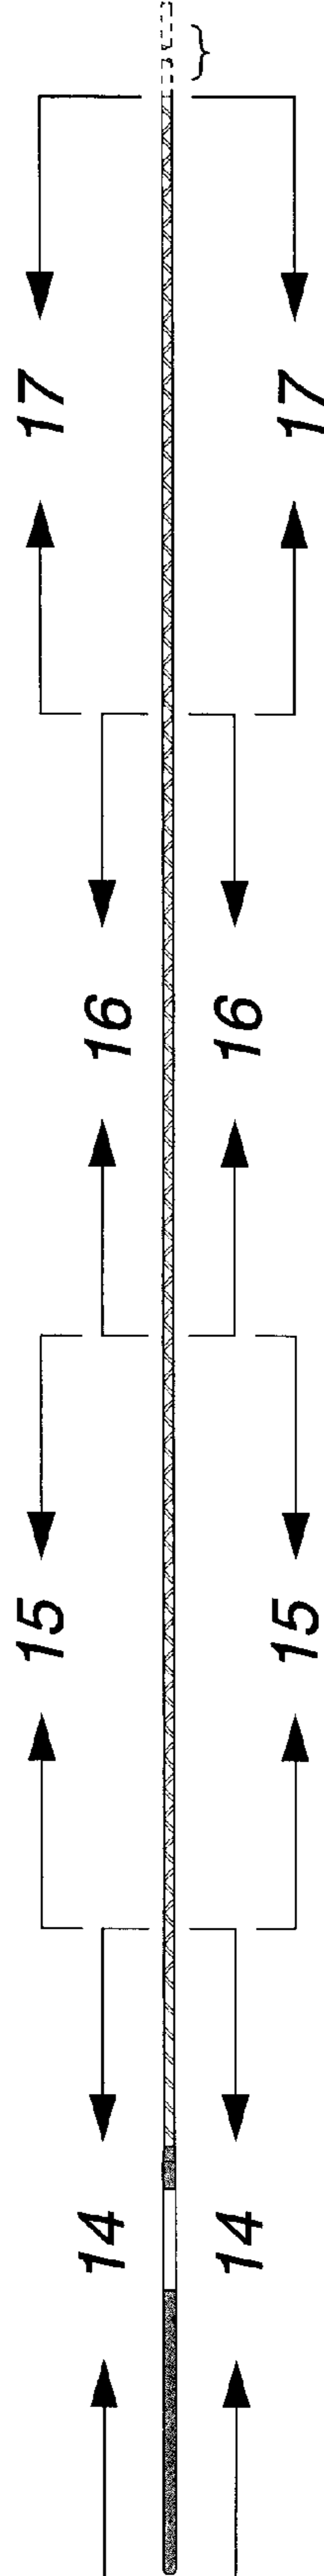


FIG. 4

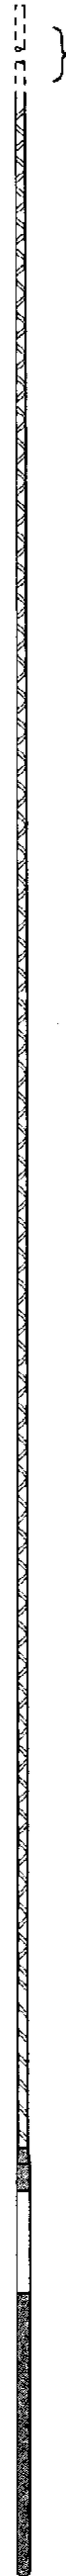



FIG. 5

◉


*FIG. 6*

◉

*FIG. 7*

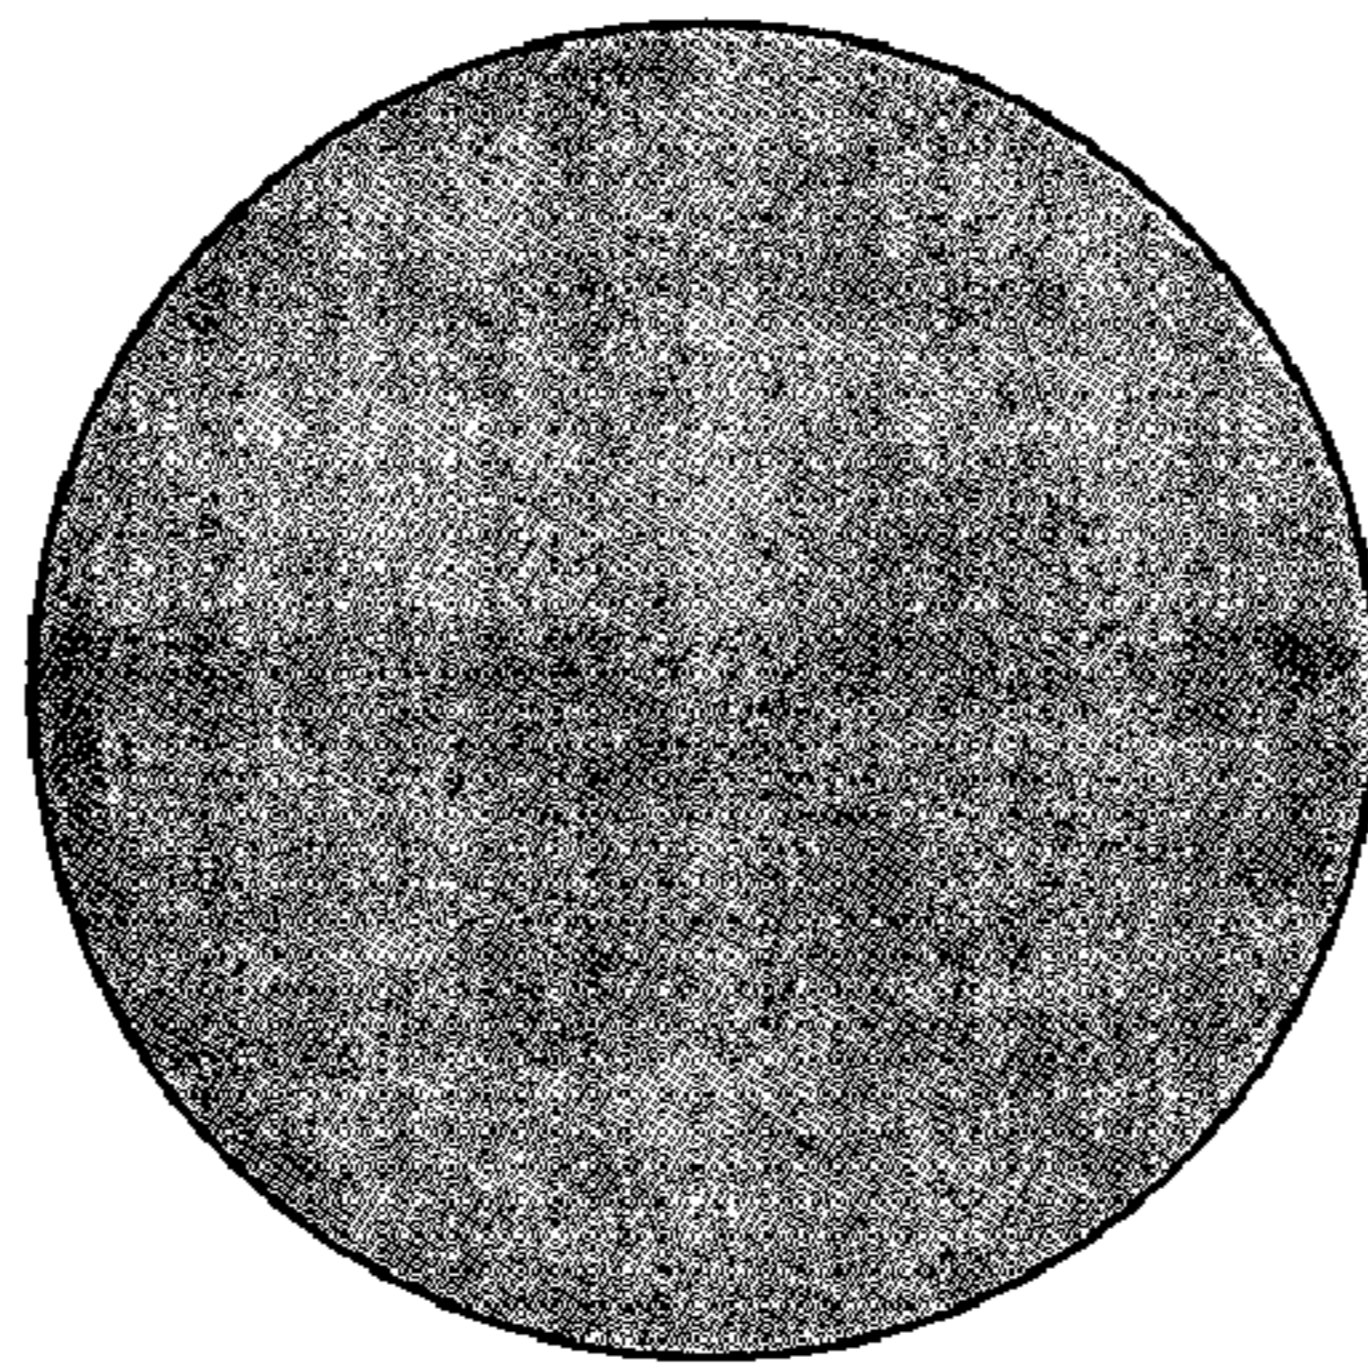

*FIG. 8*

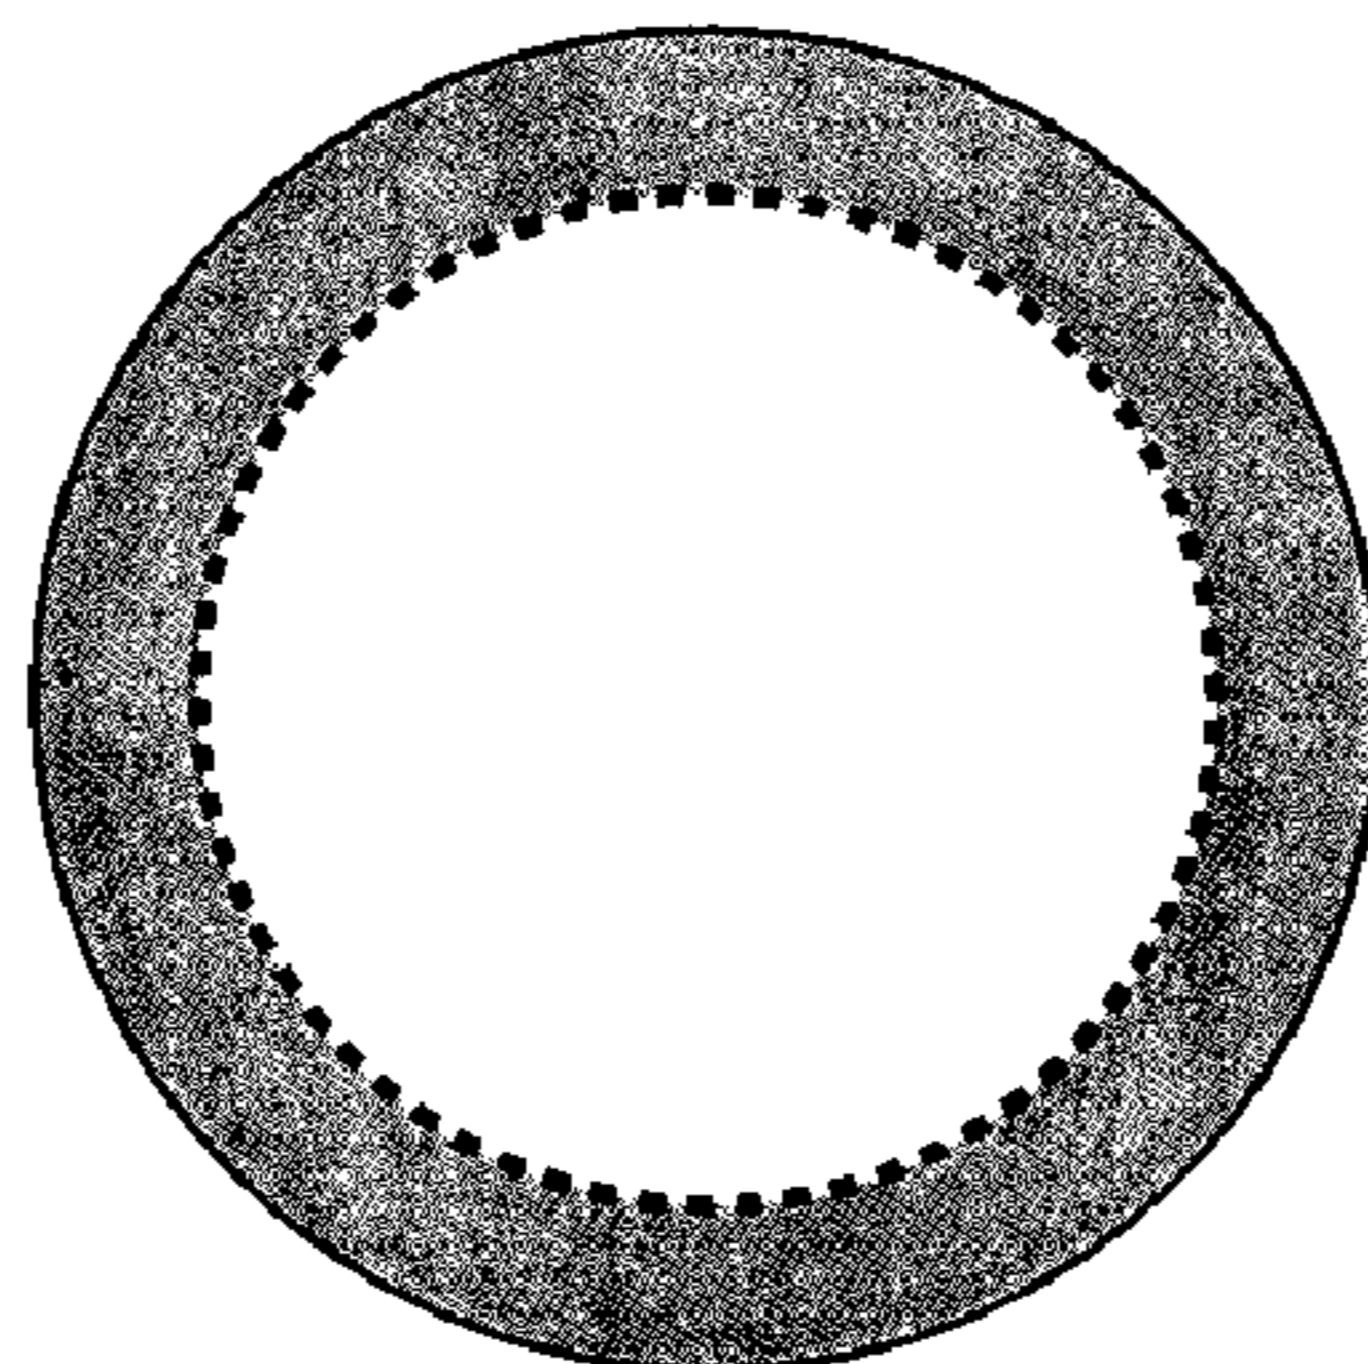

*FIG. 9*



FIG. 10



FIG. 11



FIG. 12



FIG. 13



FIG. 14



FIG. 15



FIG. 16



FIG. 17