



US00D613397S

(12) **United States Design Patent**  
**Nakao et al.**

(10) **Patent No.:** **US D613,397 S**  
(45) **Date of Patent:** **\*\* Apr. 6, 2010**

(54) **INHALER**

(75) Inventors: **Takaaki Nakao**, Tokushima (JP);  
**Shintaro Adachi**, Tokushima (JP);  
**Tetsuya Sato**, Osaka (JP); **Toru**  
**Nishibayashi**, Osaka (JP)

(73) Assignees: **Otsuka Pharmaceutical Co., Ltd.** (JP);  
**Otsuka Techno Corporation** (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/328,401**

(22) Filed: **Nov. 24, 2008**

(30) **Foreign Application Priority Data**

May 23, 2008 (JP) ..... 2008-013034

(51) **LOC (9) Cl.** ..... **29-02**

(52) **U.S. Cl.** ..... **D24/110**

(58) **Field of Classification Search** ..... D24/110;  
D9/529, 551, 682; 128/200.23, 200.12, 200.14,  
128/200.21, 205.23, 203.12, 203.15, 203.13  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D355,029 S \* 1/1995 Kinneir et al. .... D24/110  
D452,910 S \* 1/2002 Braithwaite et al. .... D24/110  
D499,802 S \* 12/2004 Pinon et al. .... D24/110  
D518,170 S \* 3/2006 Clarke et al. .... D24/110  
D527,815 S \* 9/2006 Nishibayashi et al. .... D24/110  
D528,654 S \* 9/2006 Nishibayashi et al. .... D24/110  
D560,793 S \* 1/2008 Pearl et al. .... D24/110  
2009/0205656 A1 \* 8/2009 Nishibayashi et al. .. 128/203.15

**FOREIGN PATENT DOCUMENTS**

KR 30-0454447 6/2007  
TW 381870 2/2000

TW D103463 3/2005  
TW D103464 3/2005  
TW D119776 11/2007

\* cited by examiner

*Primary Examiner*—Ian Simmons  
*Assistant Examiner*—Christopher Lee

(74) *Attorney, Agent, or Firm*—SAIDMAN DesignLaw  
Group

(57) **CLAIM**

The ornamental design for an inhaler, as shown and  
described.

**DESCRIPTION**

FIG. 1 is a front perspective view of an inhaler showing our  
new design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a left side view thereof;

FIG. 6 is a top view thereof;

FIG. 7 is a bottom view thereof;

FIG. 8 is a front perspective view with the inhaler in an open  
position;

FIG. 9 is a front view thereof;

FIG. 10 is a rear view thereof;

FIG. 11 is a right side view thereof;


FIG. 12 is a left side view thereof;


FIG. 13 is a top view thereof; and,

FIG. 14 is a bottom view thereof.


The broken lines are environmental and form no part of the  
claimed design.

**1 Claim, 8 Drawing Sheets**

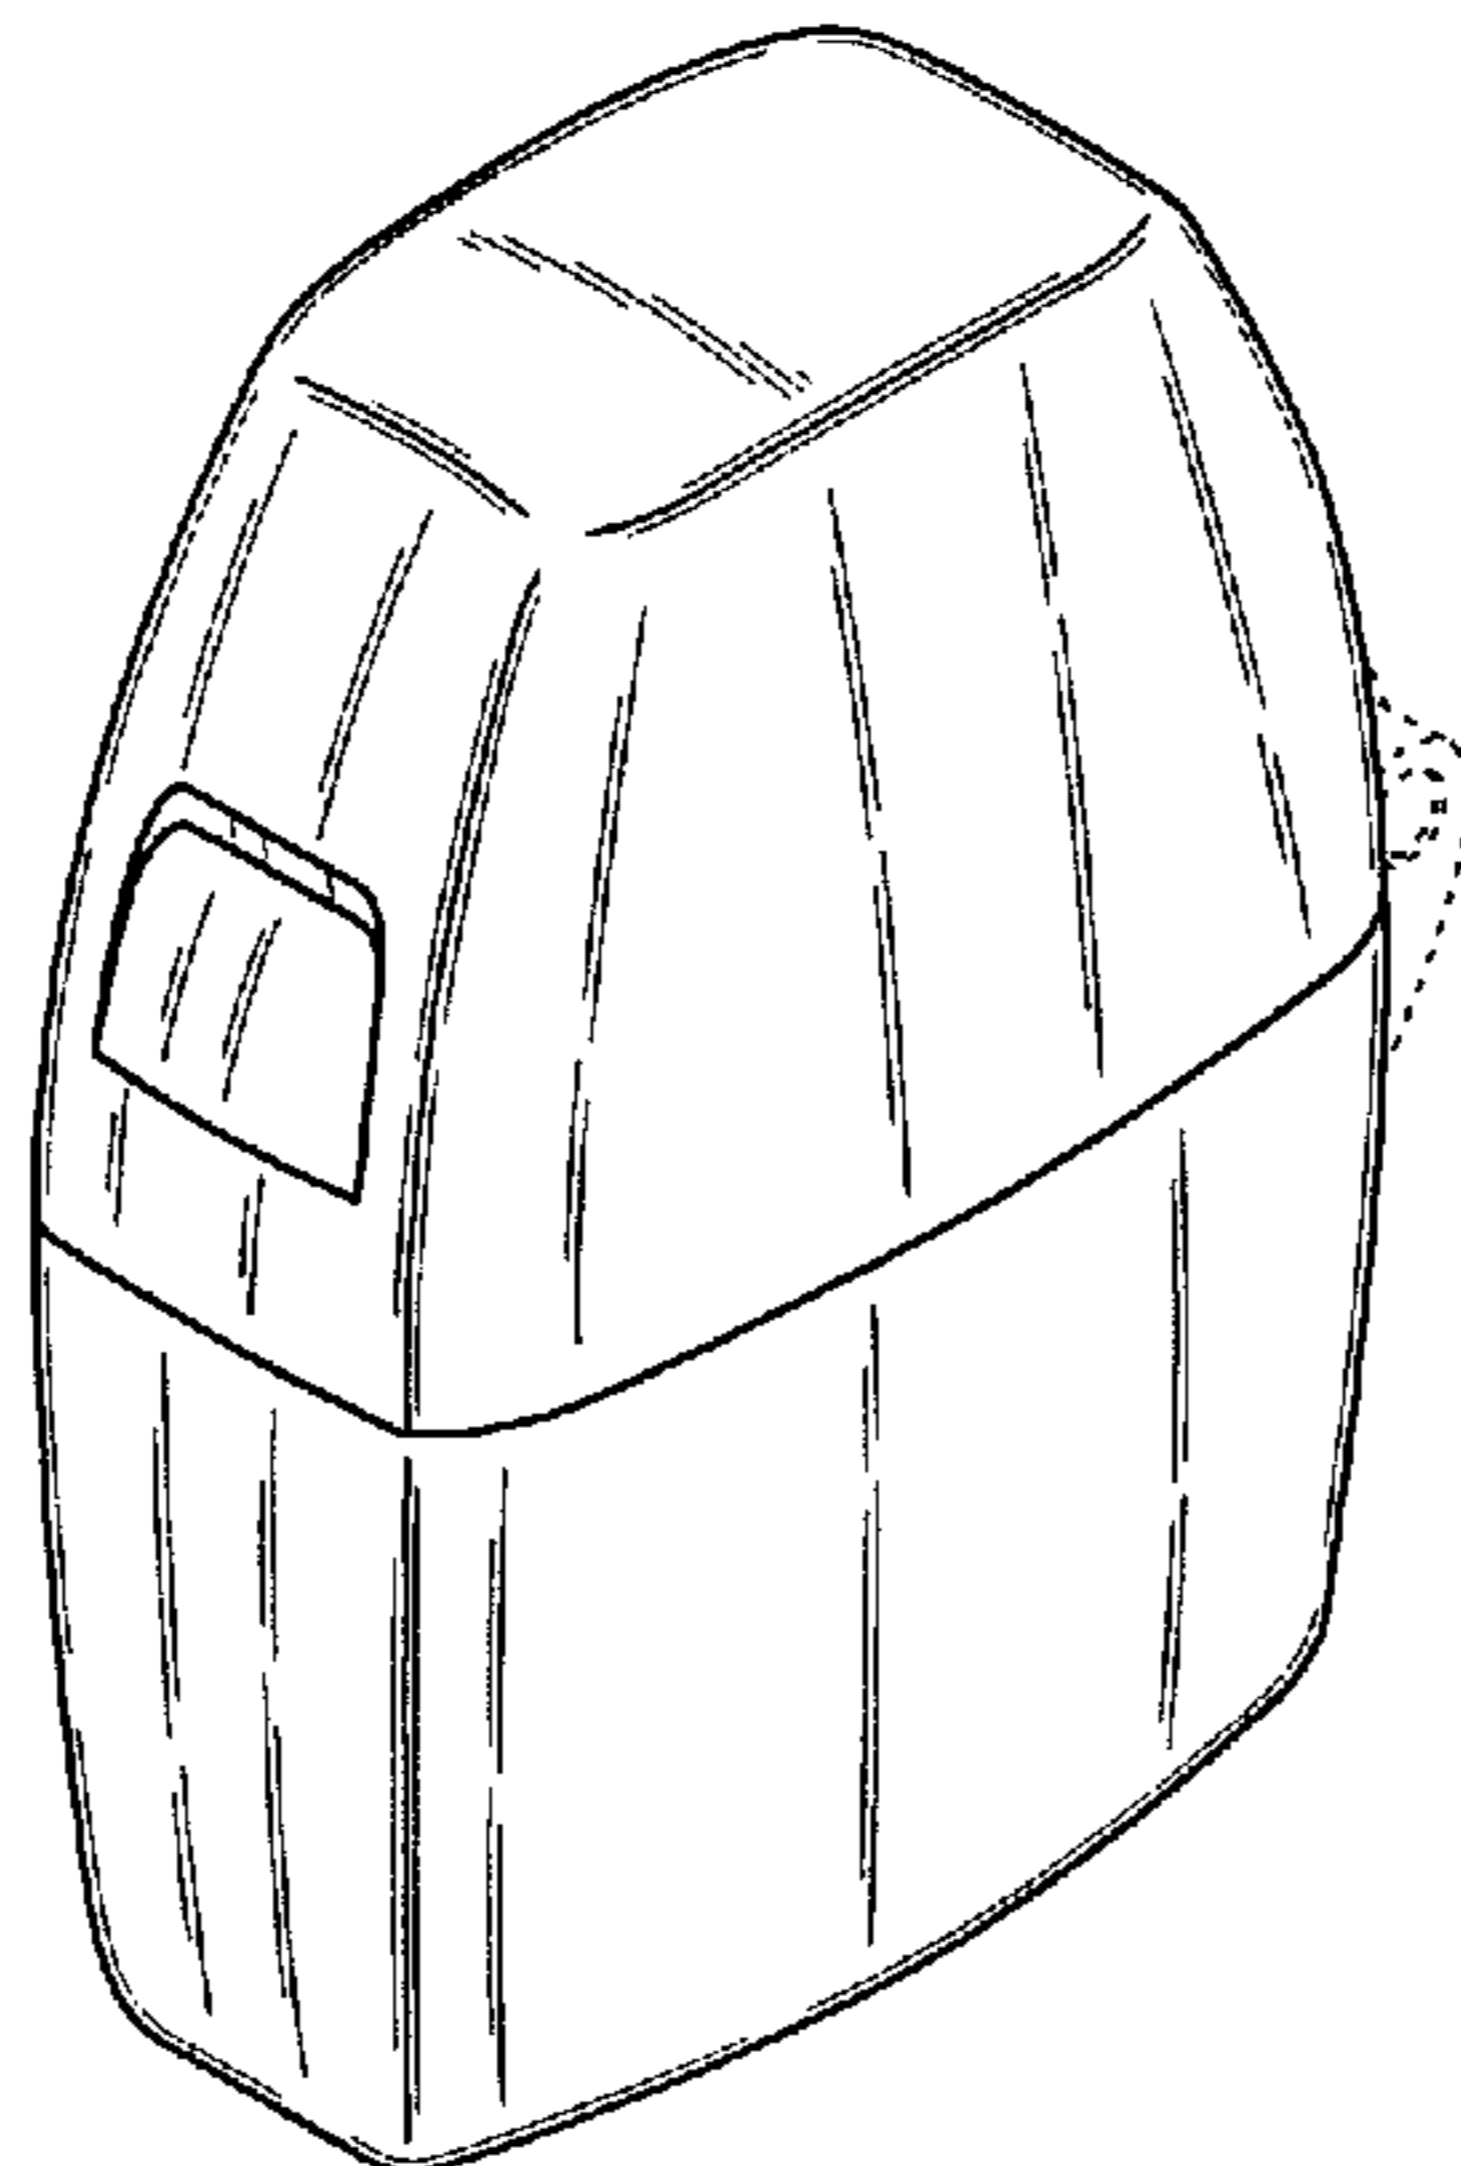


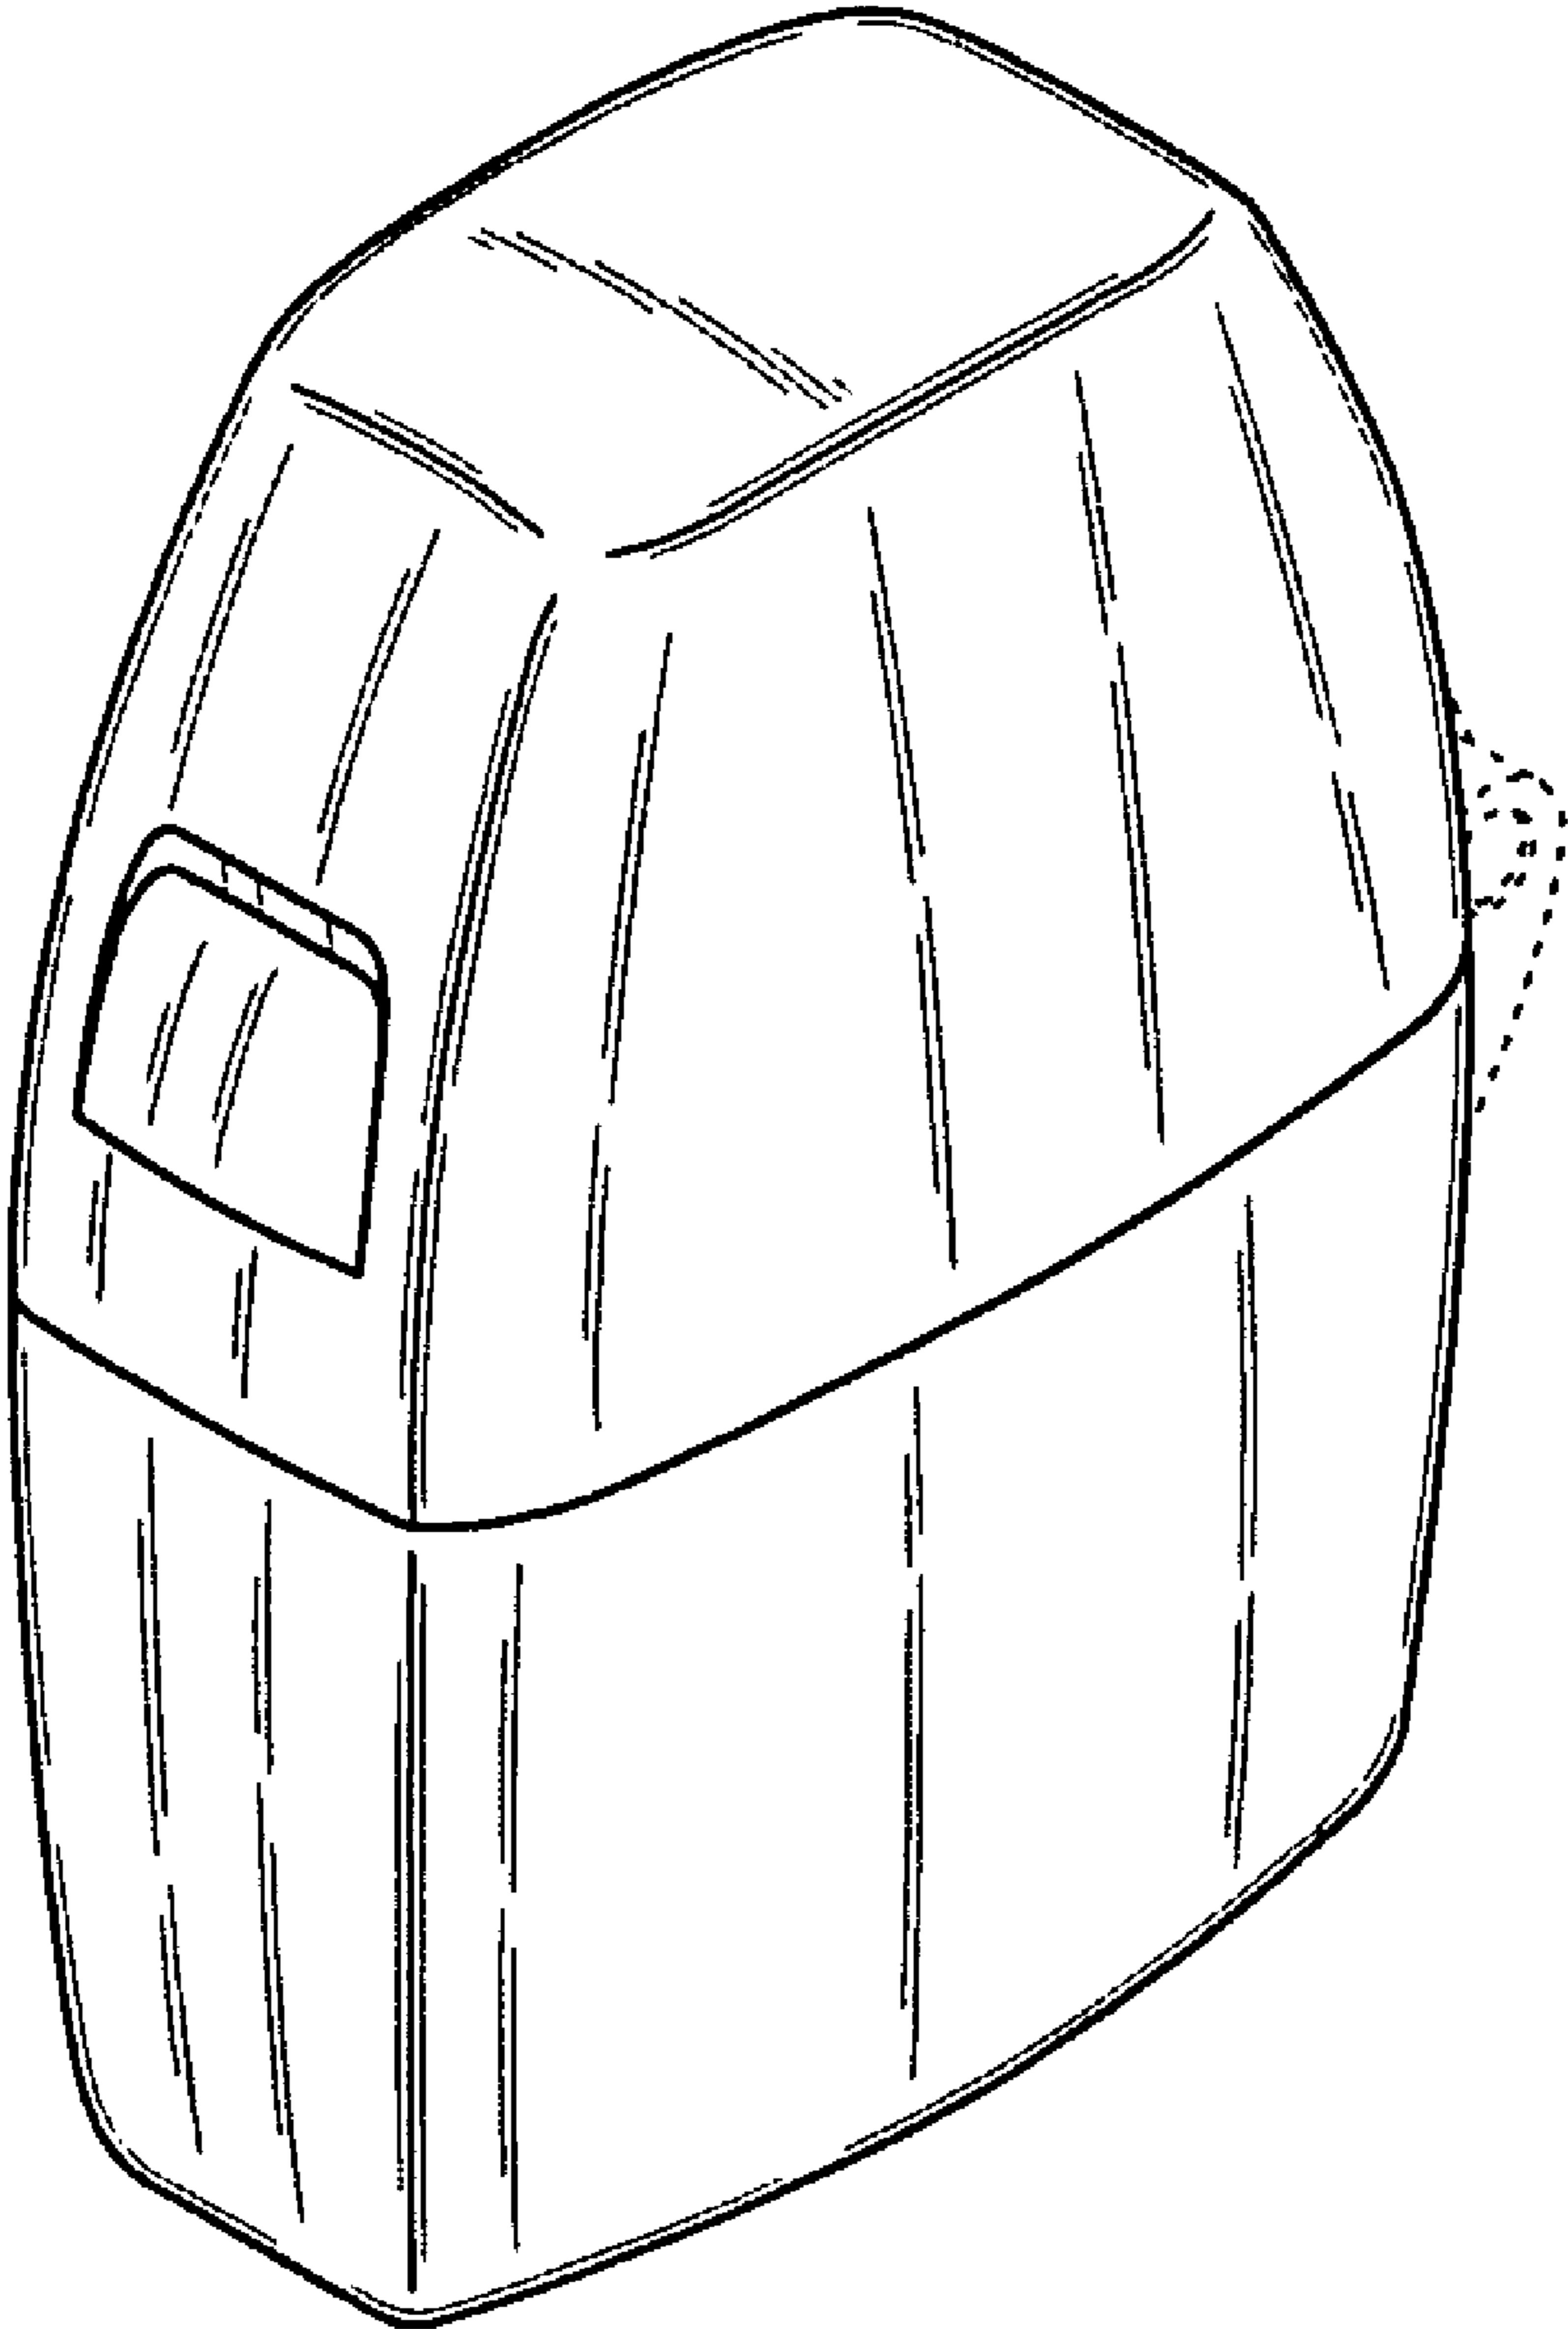


**Fig. 1**

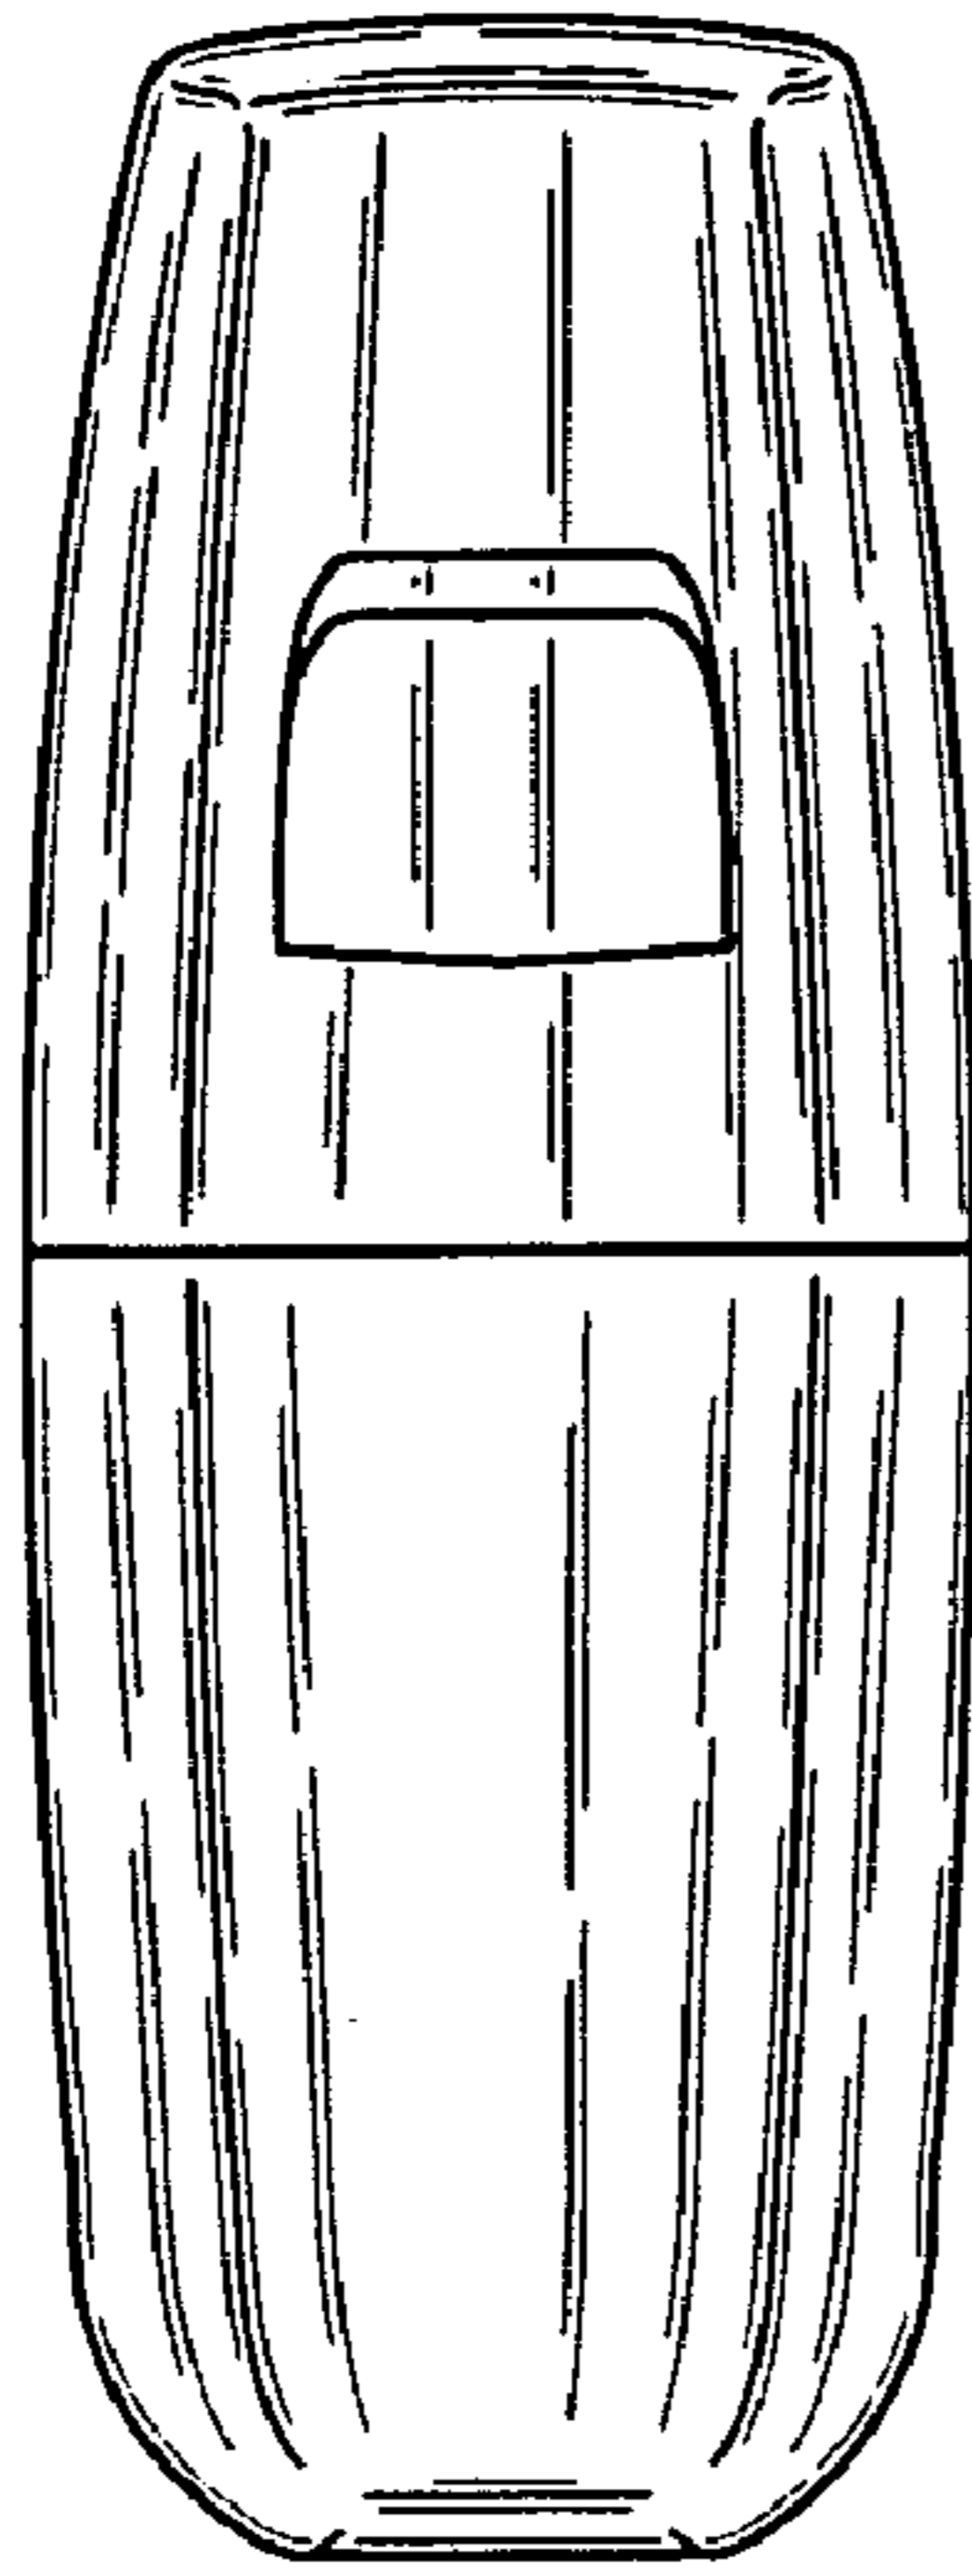


**Fig. 2**

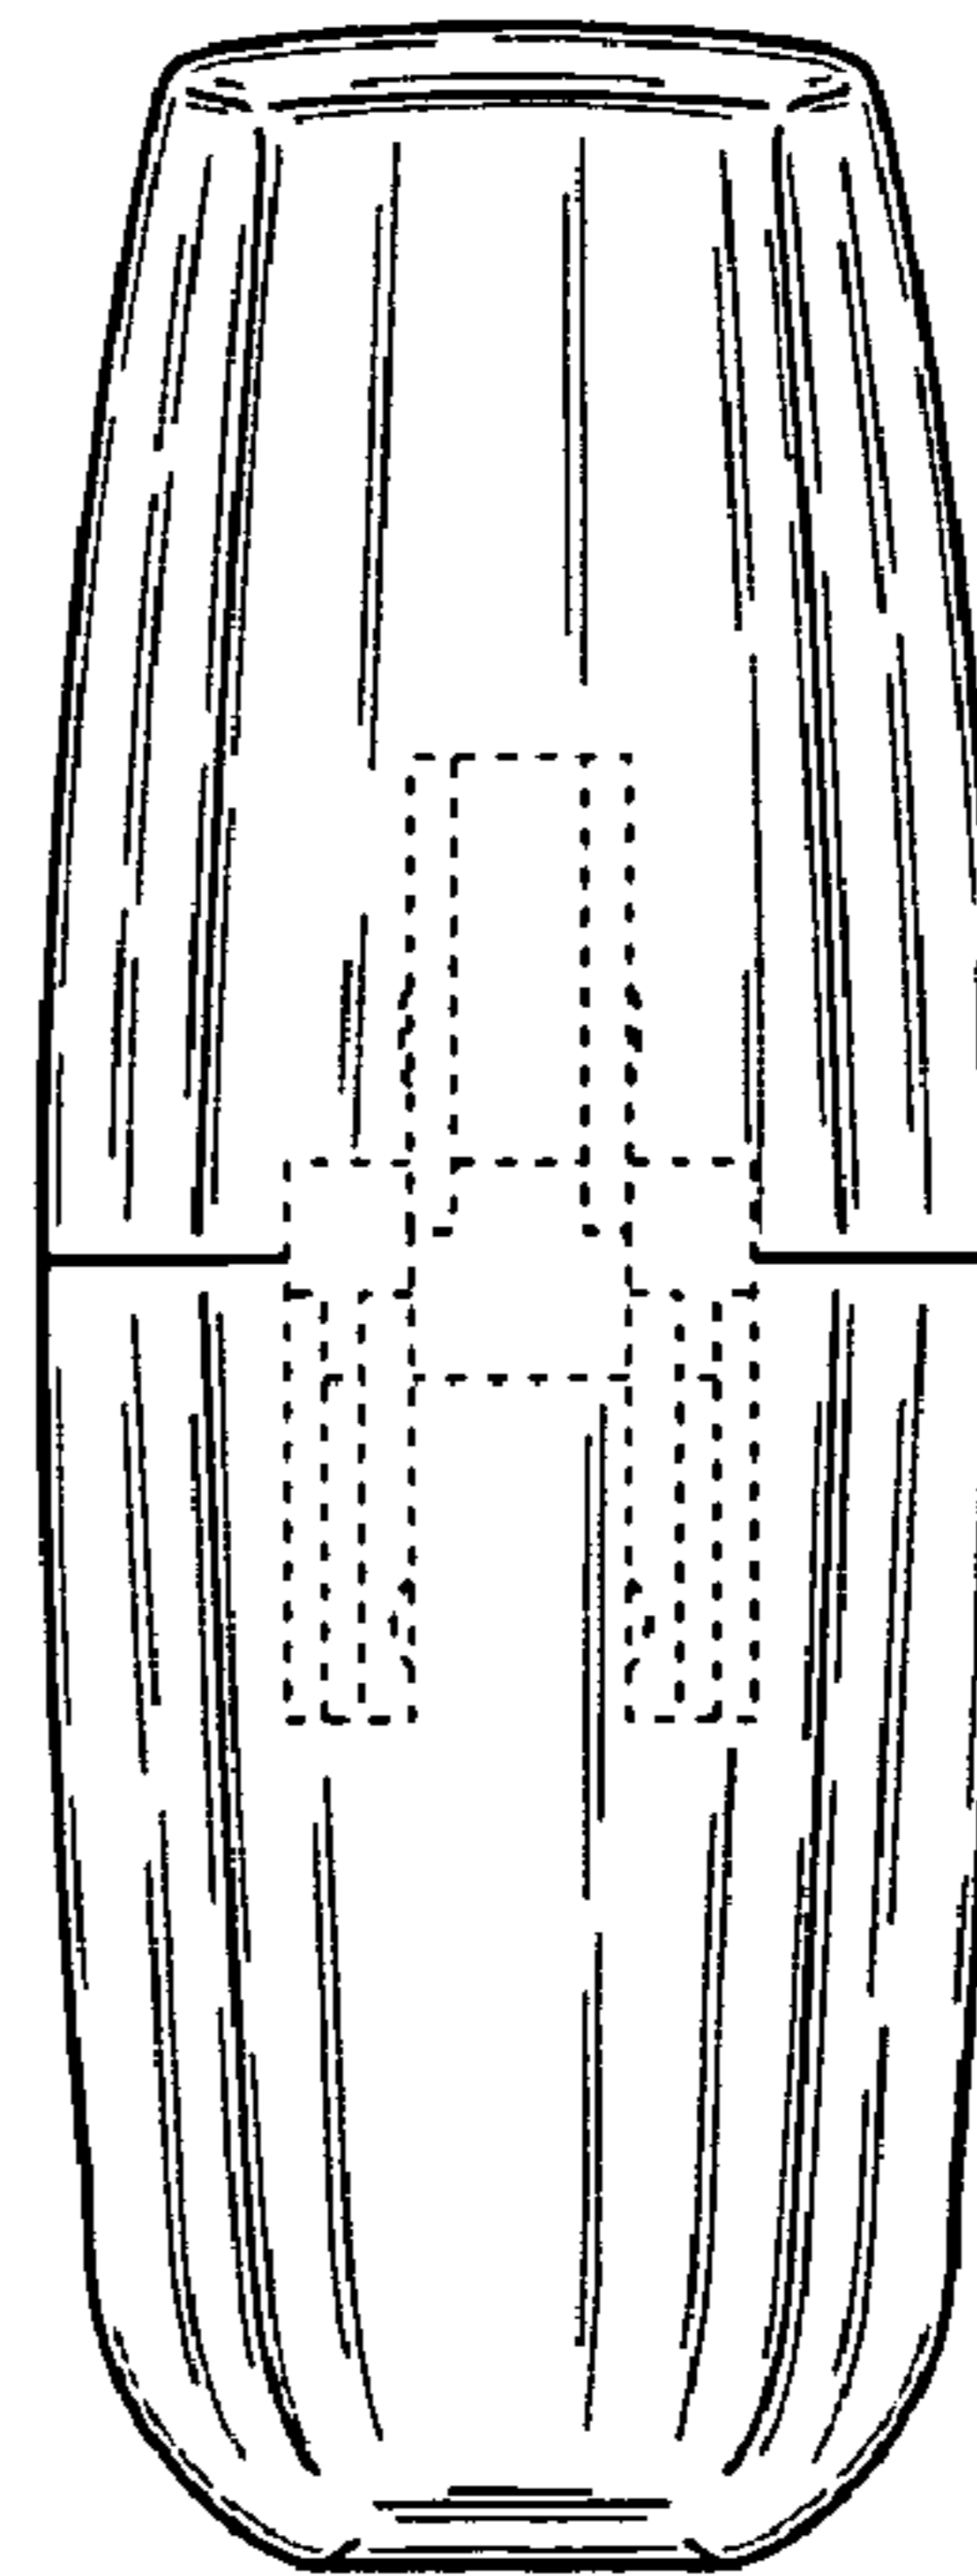


**Fig. 3**

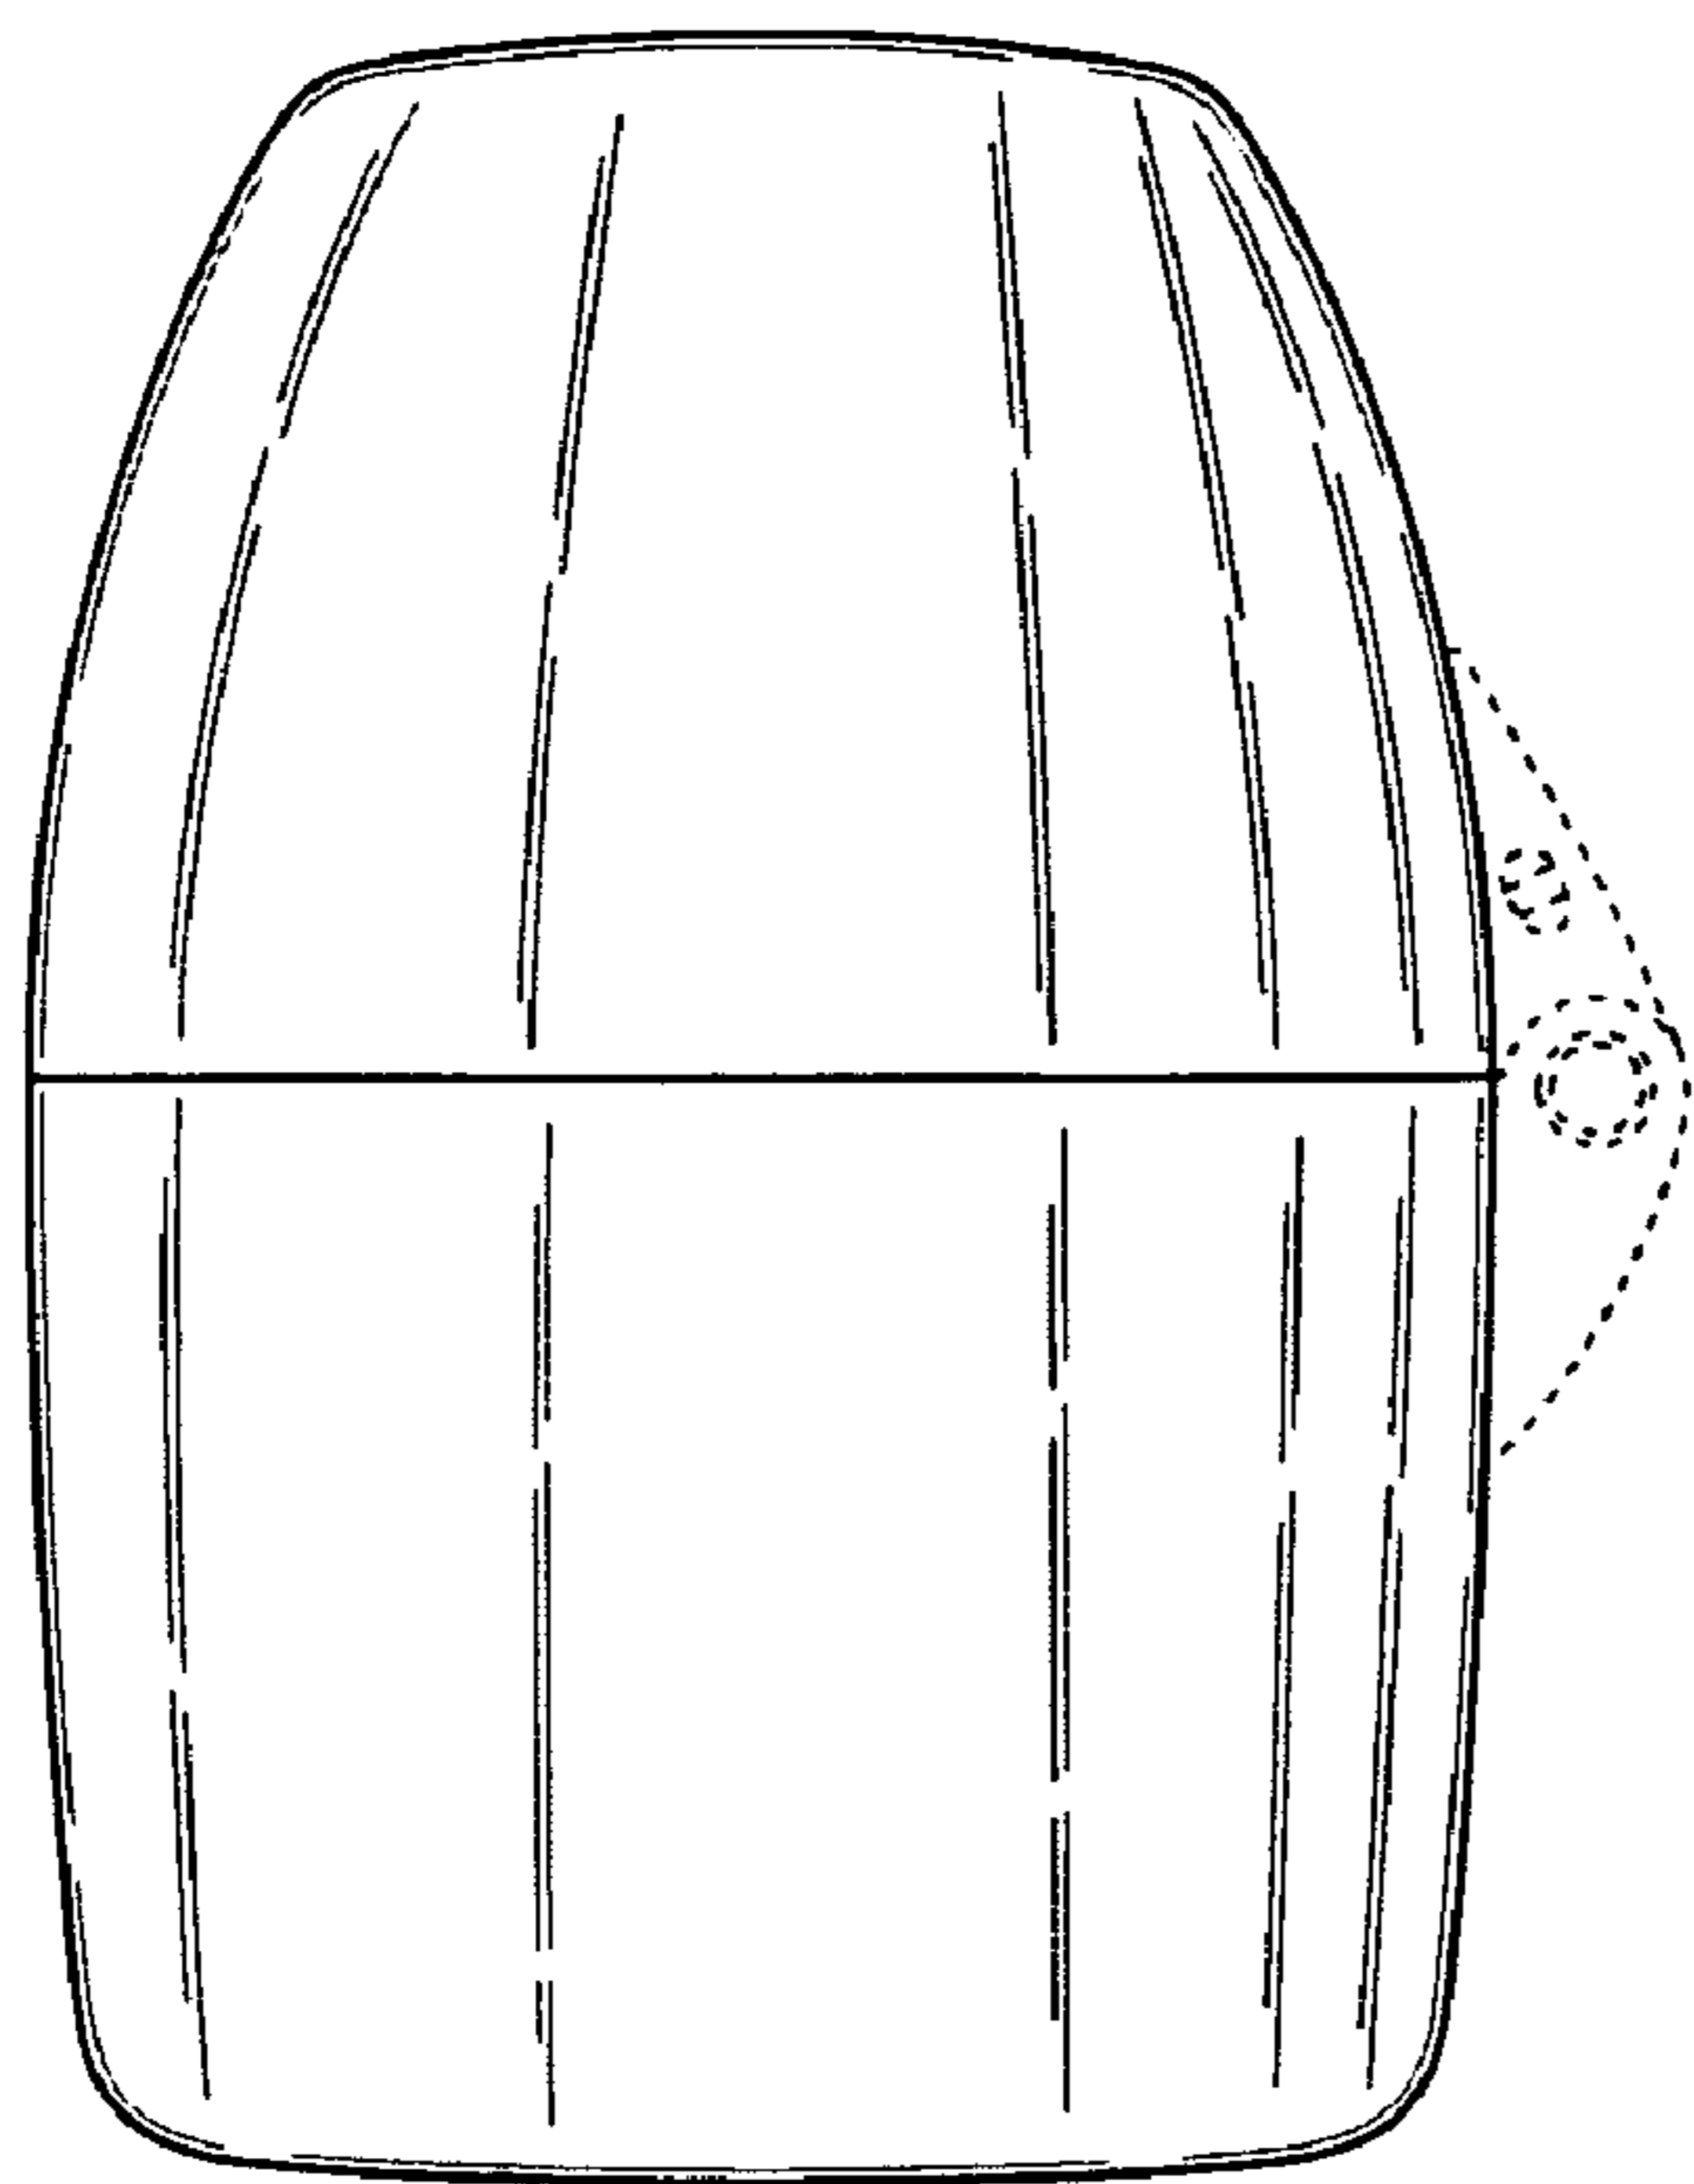


**Fig. 4**

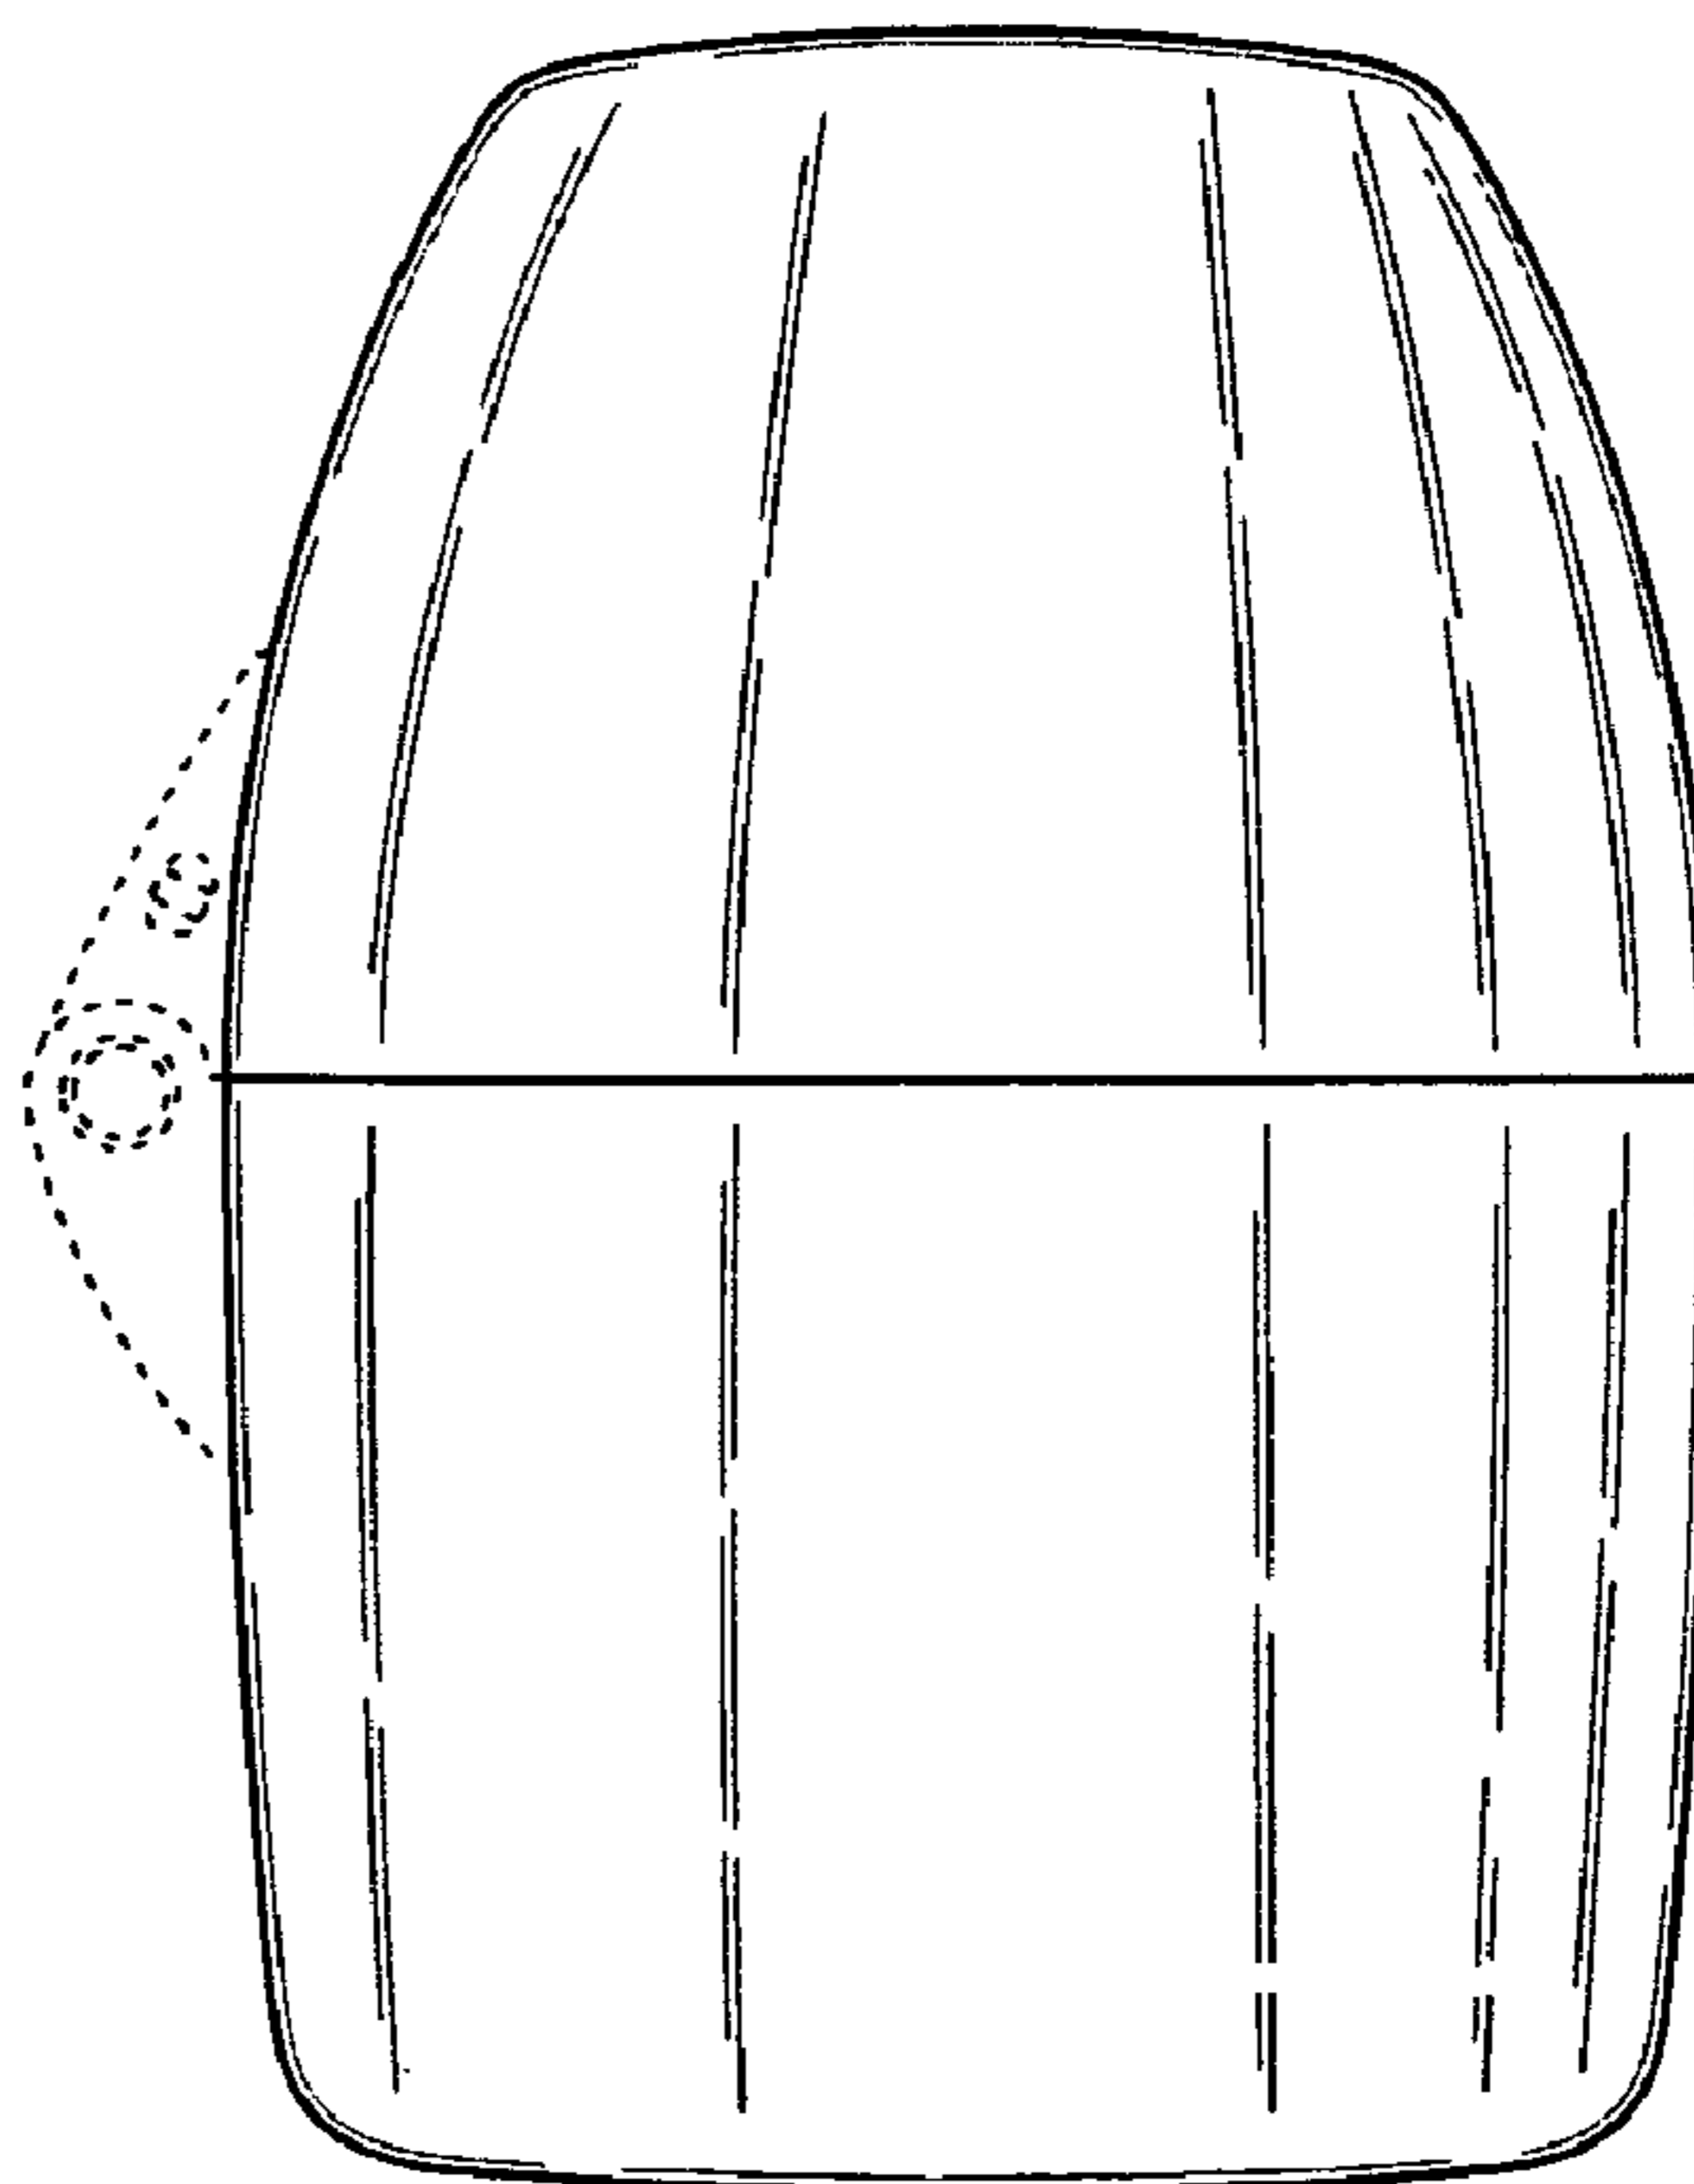


**Fig. 5**

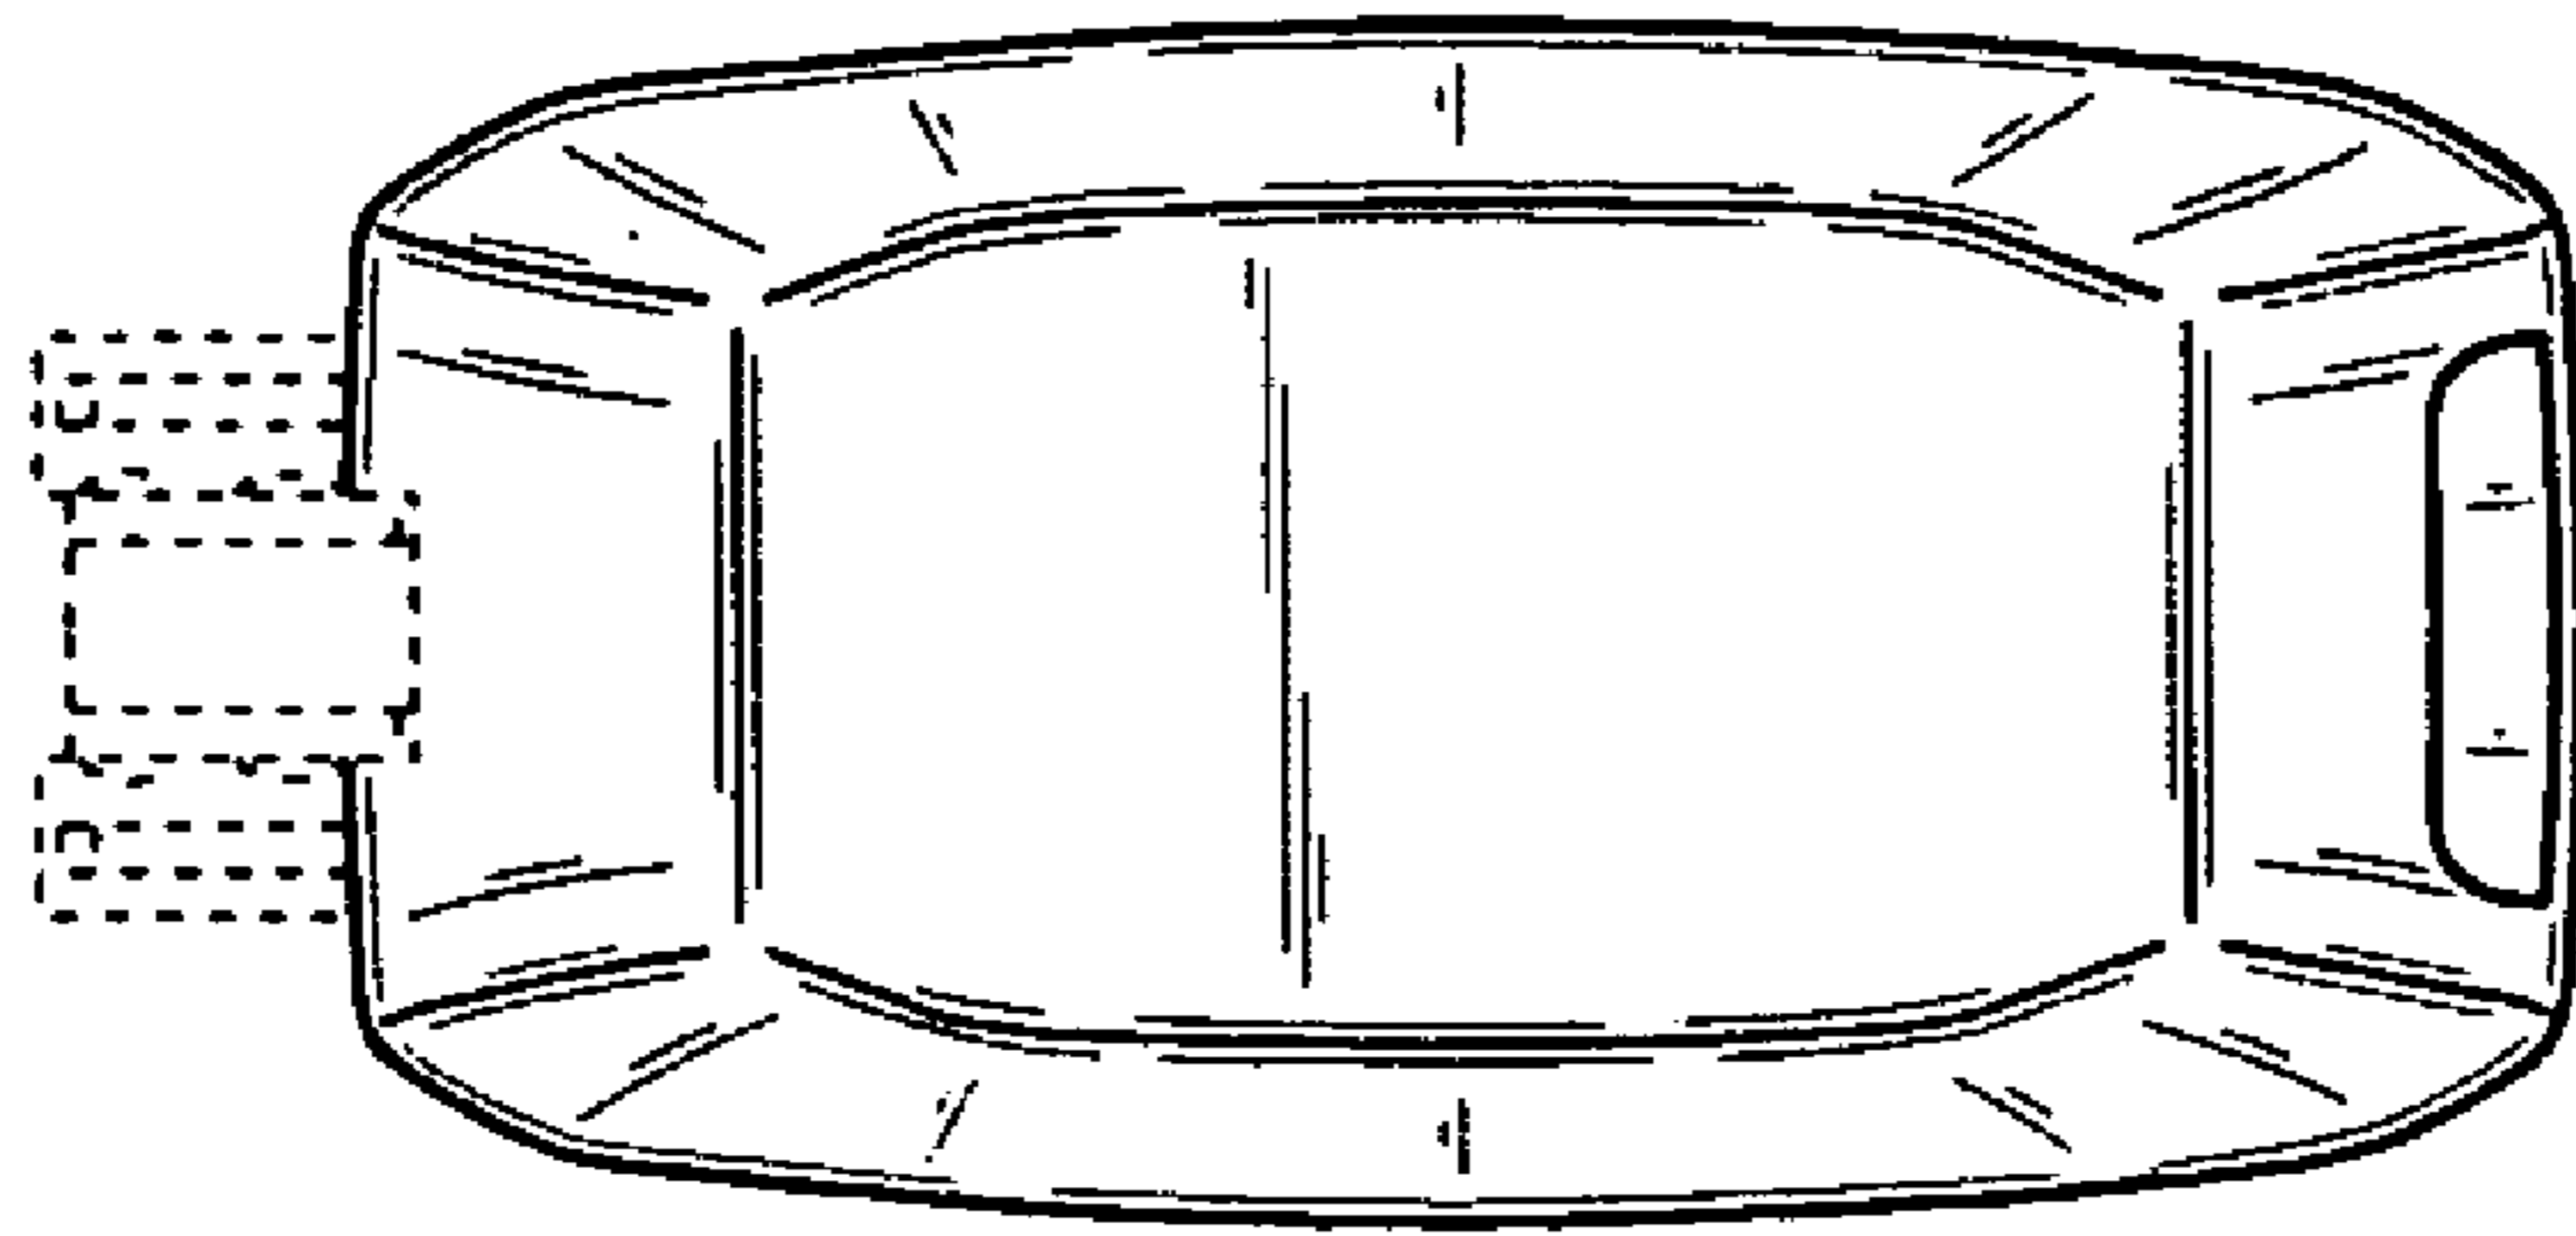


**Fig. 6**

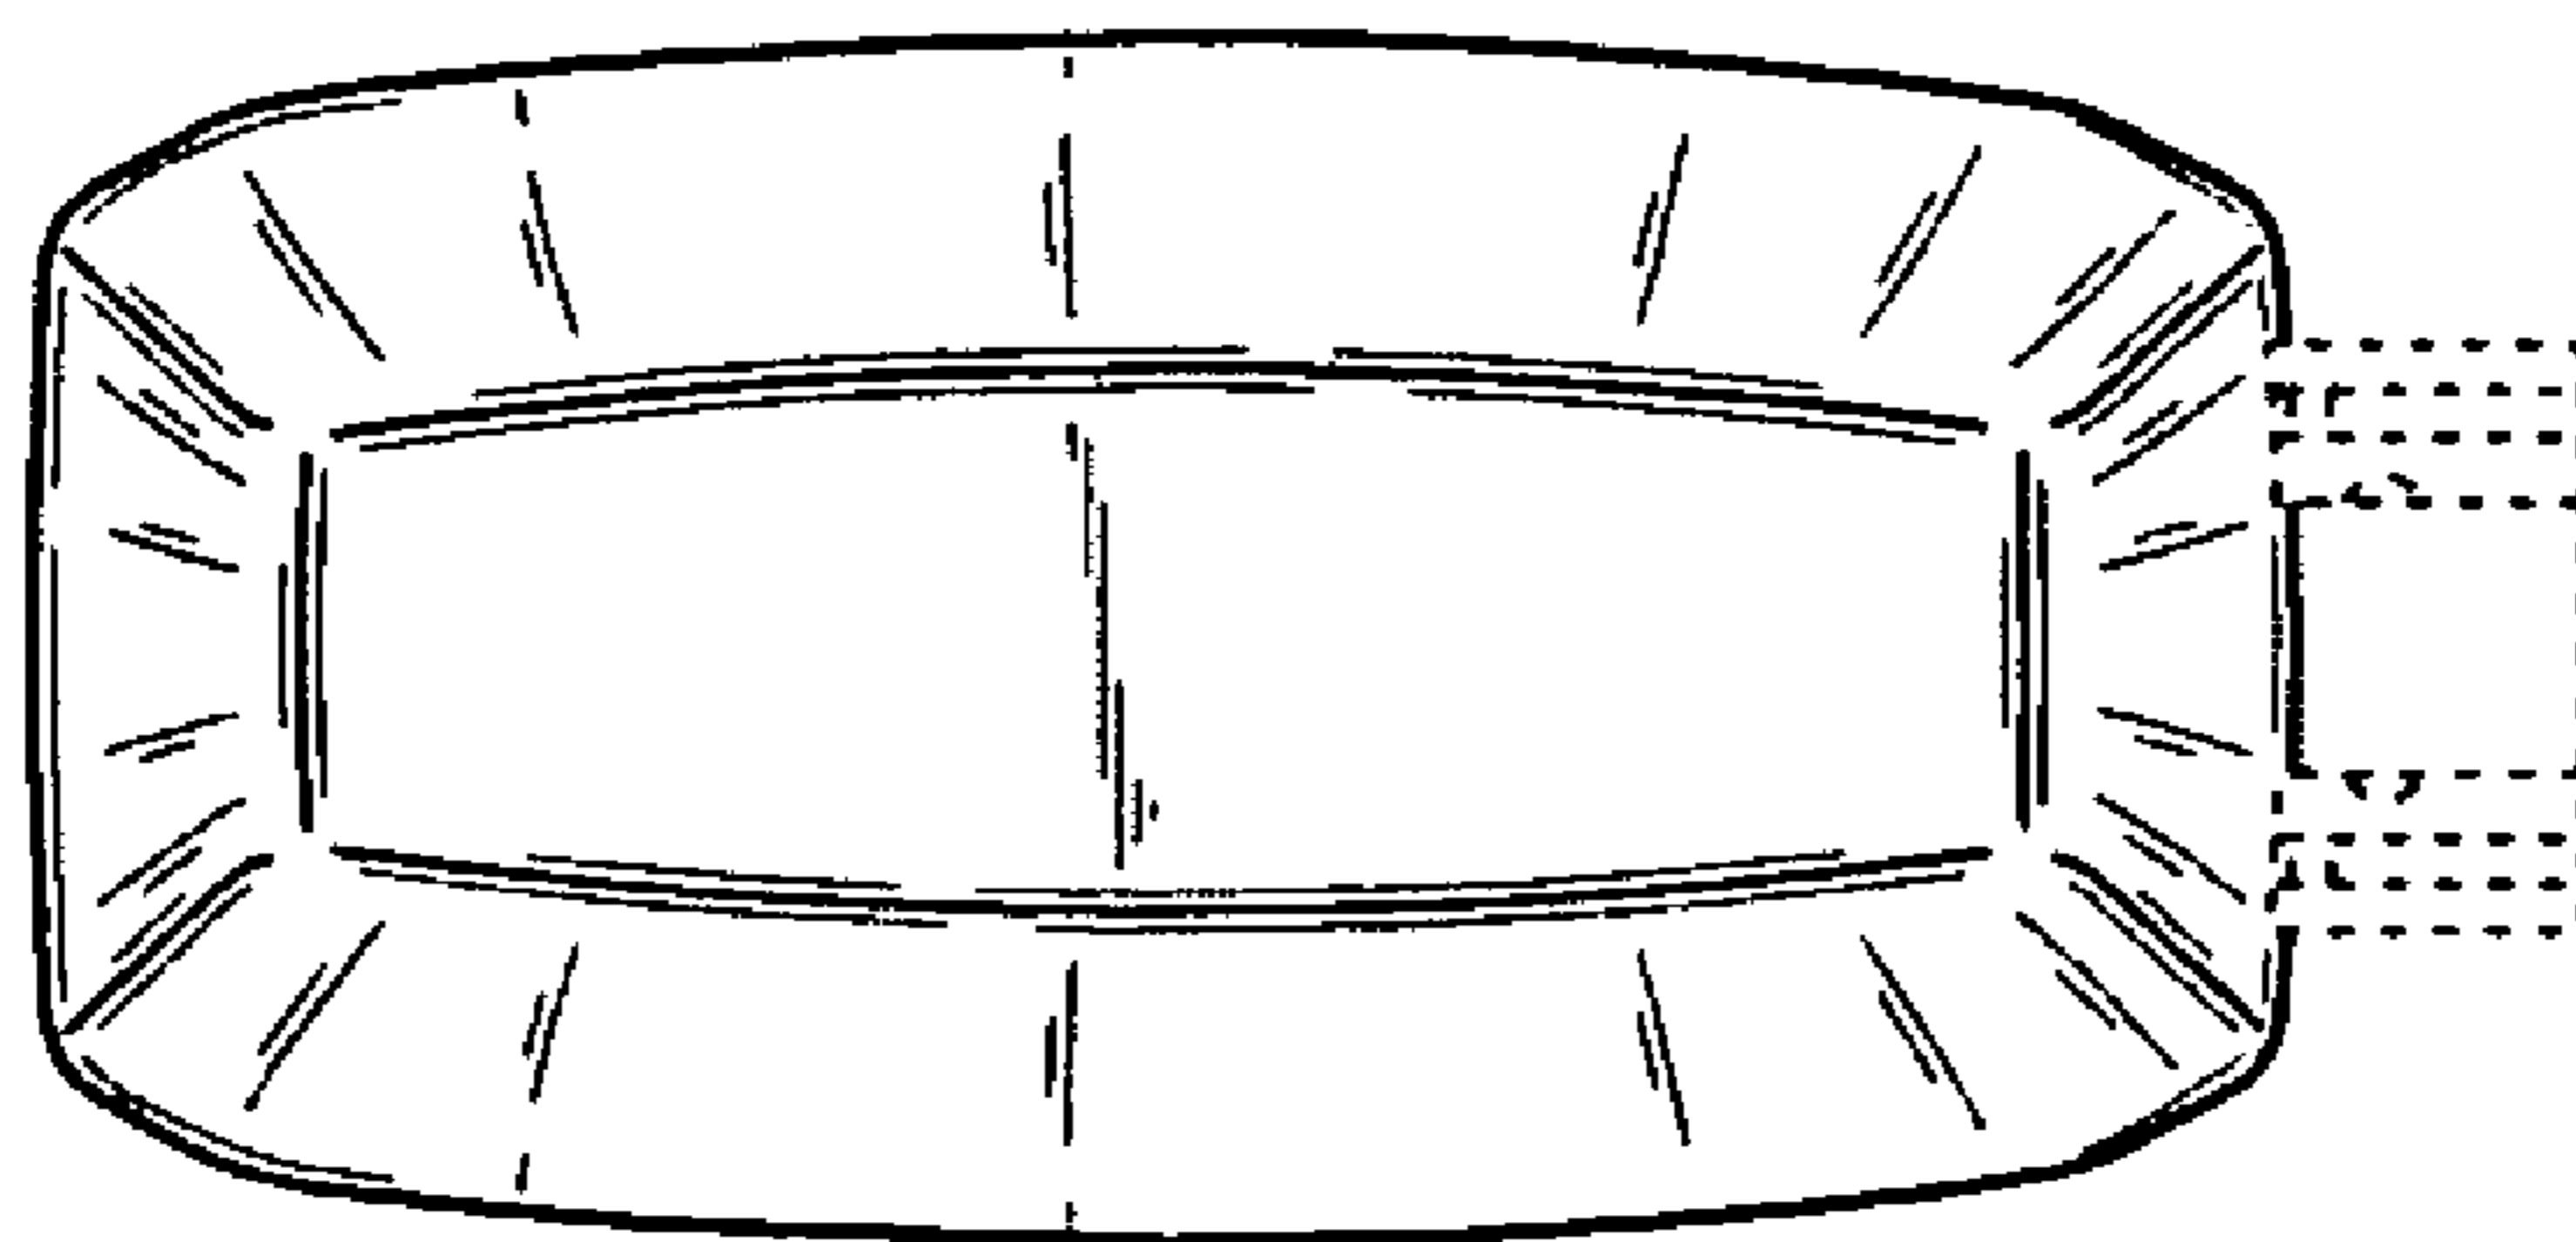


**Fig. 7**

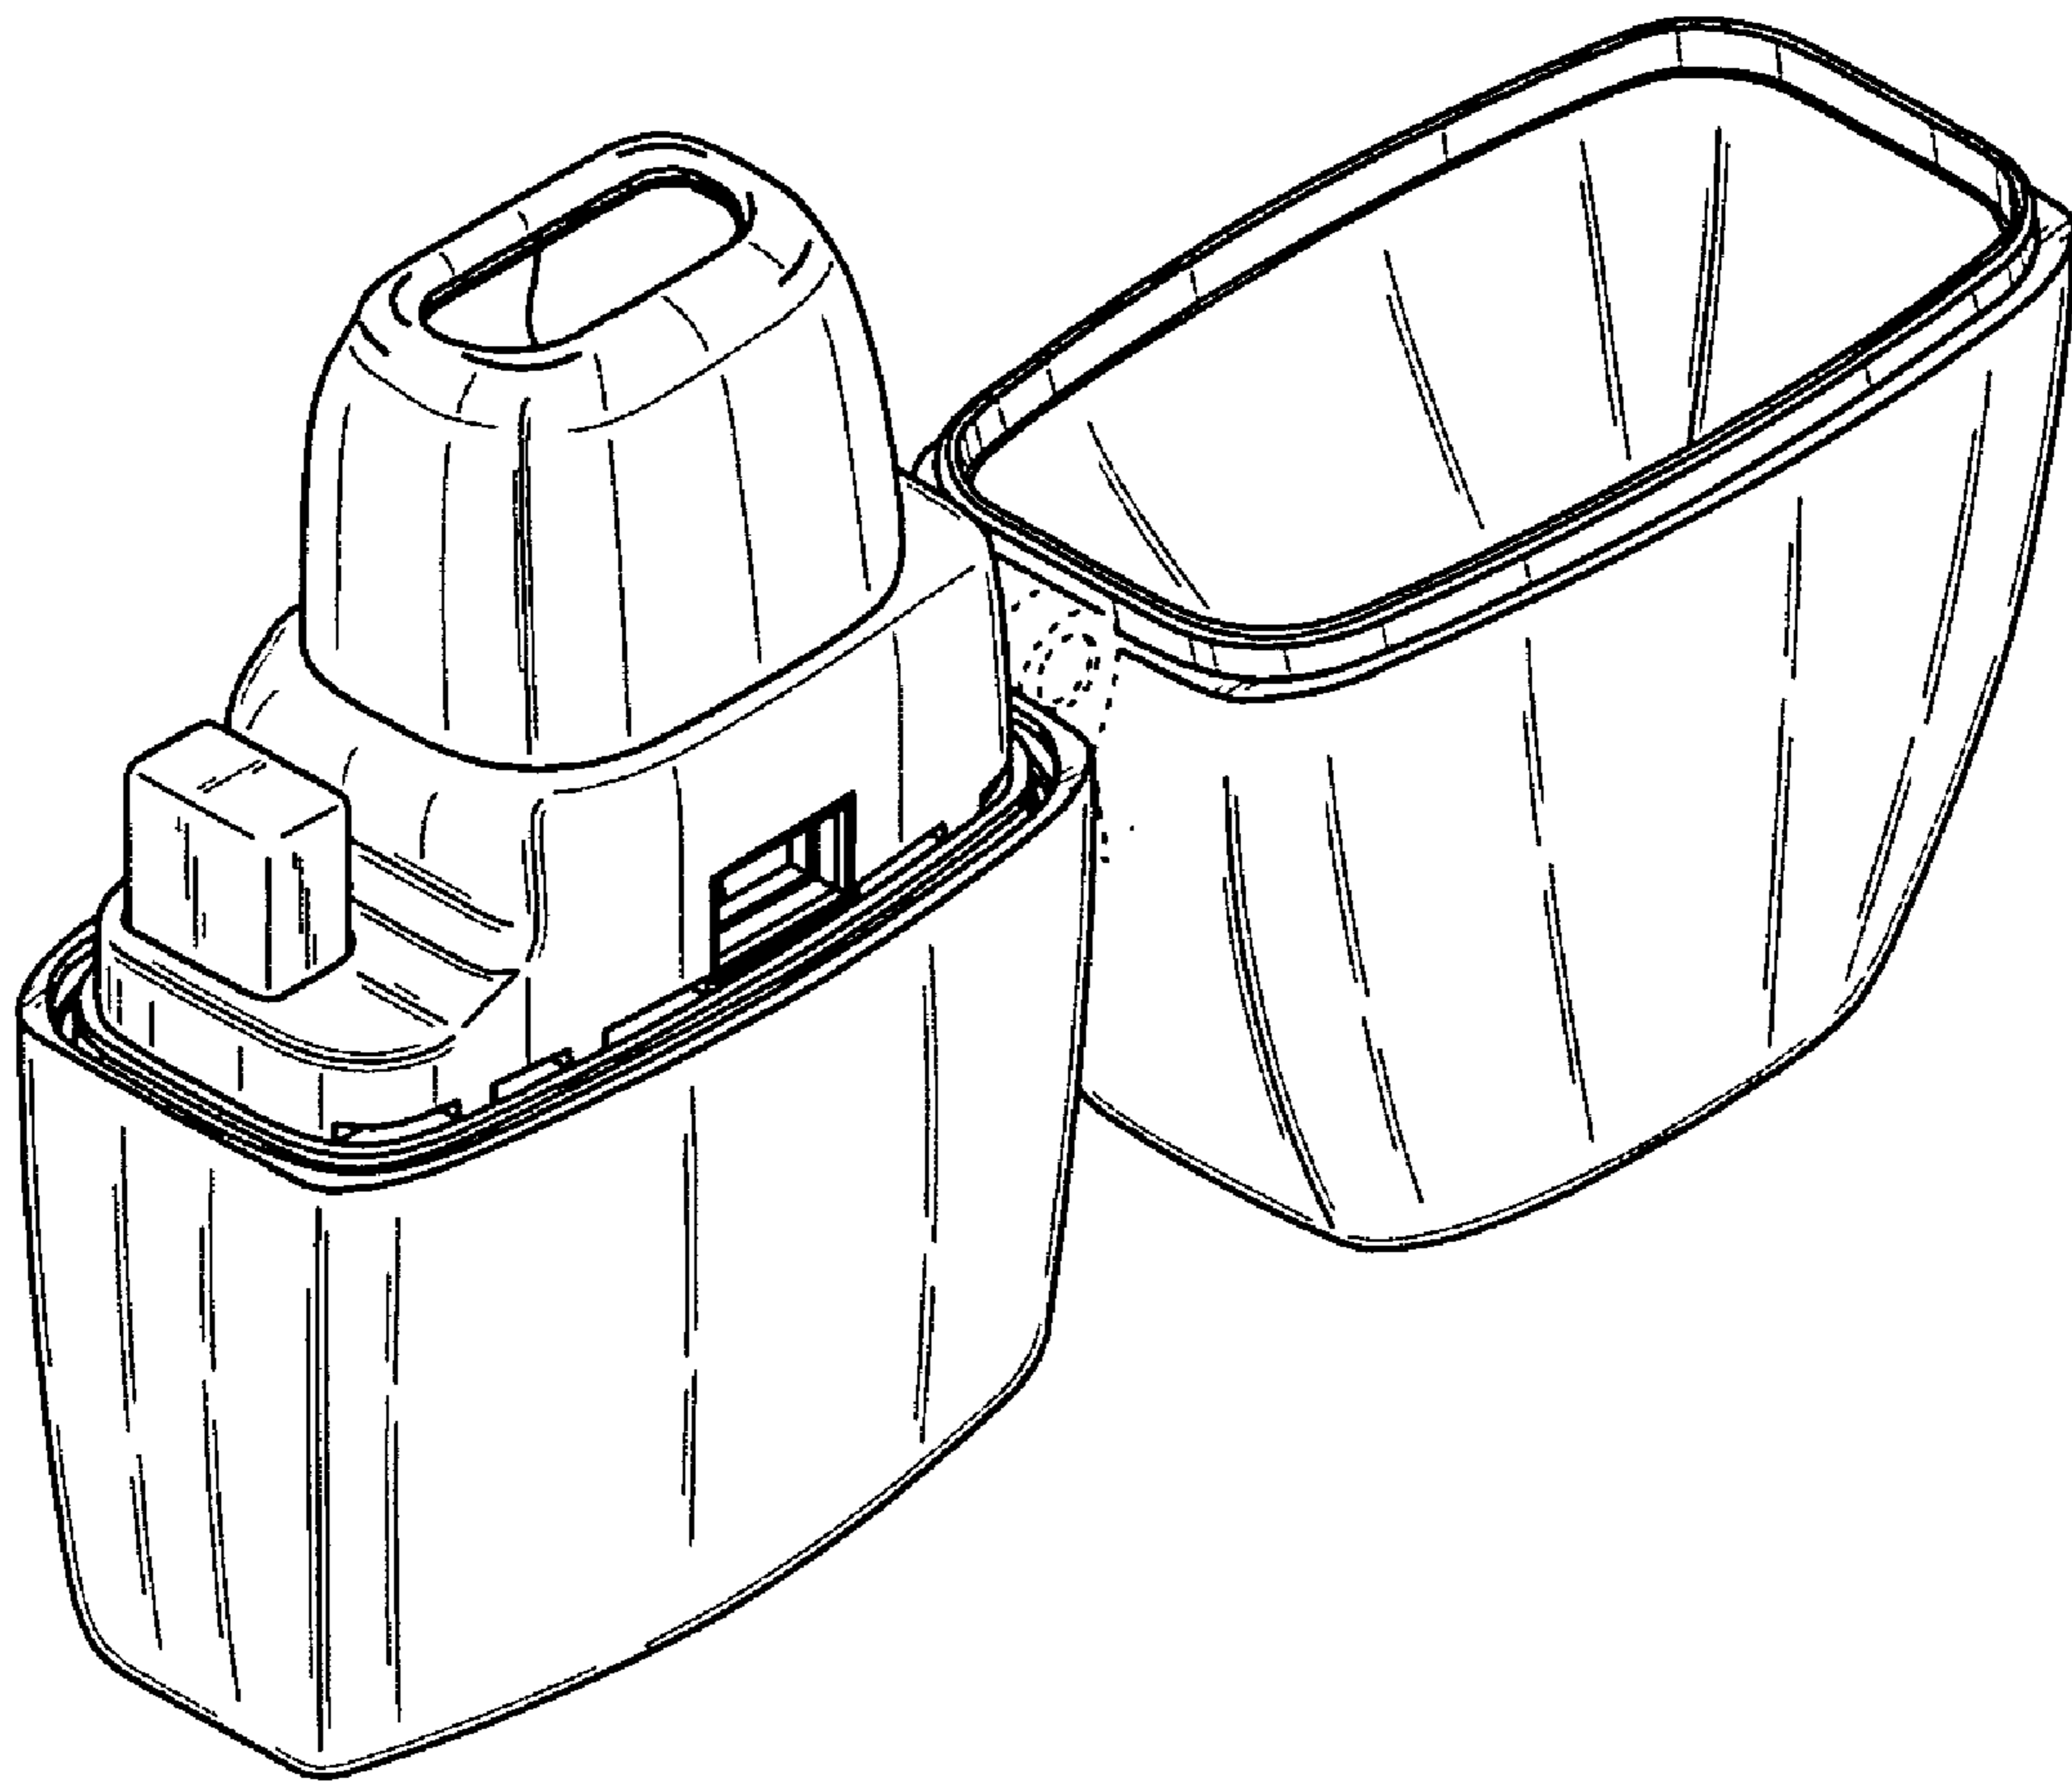


**Fig. 8**

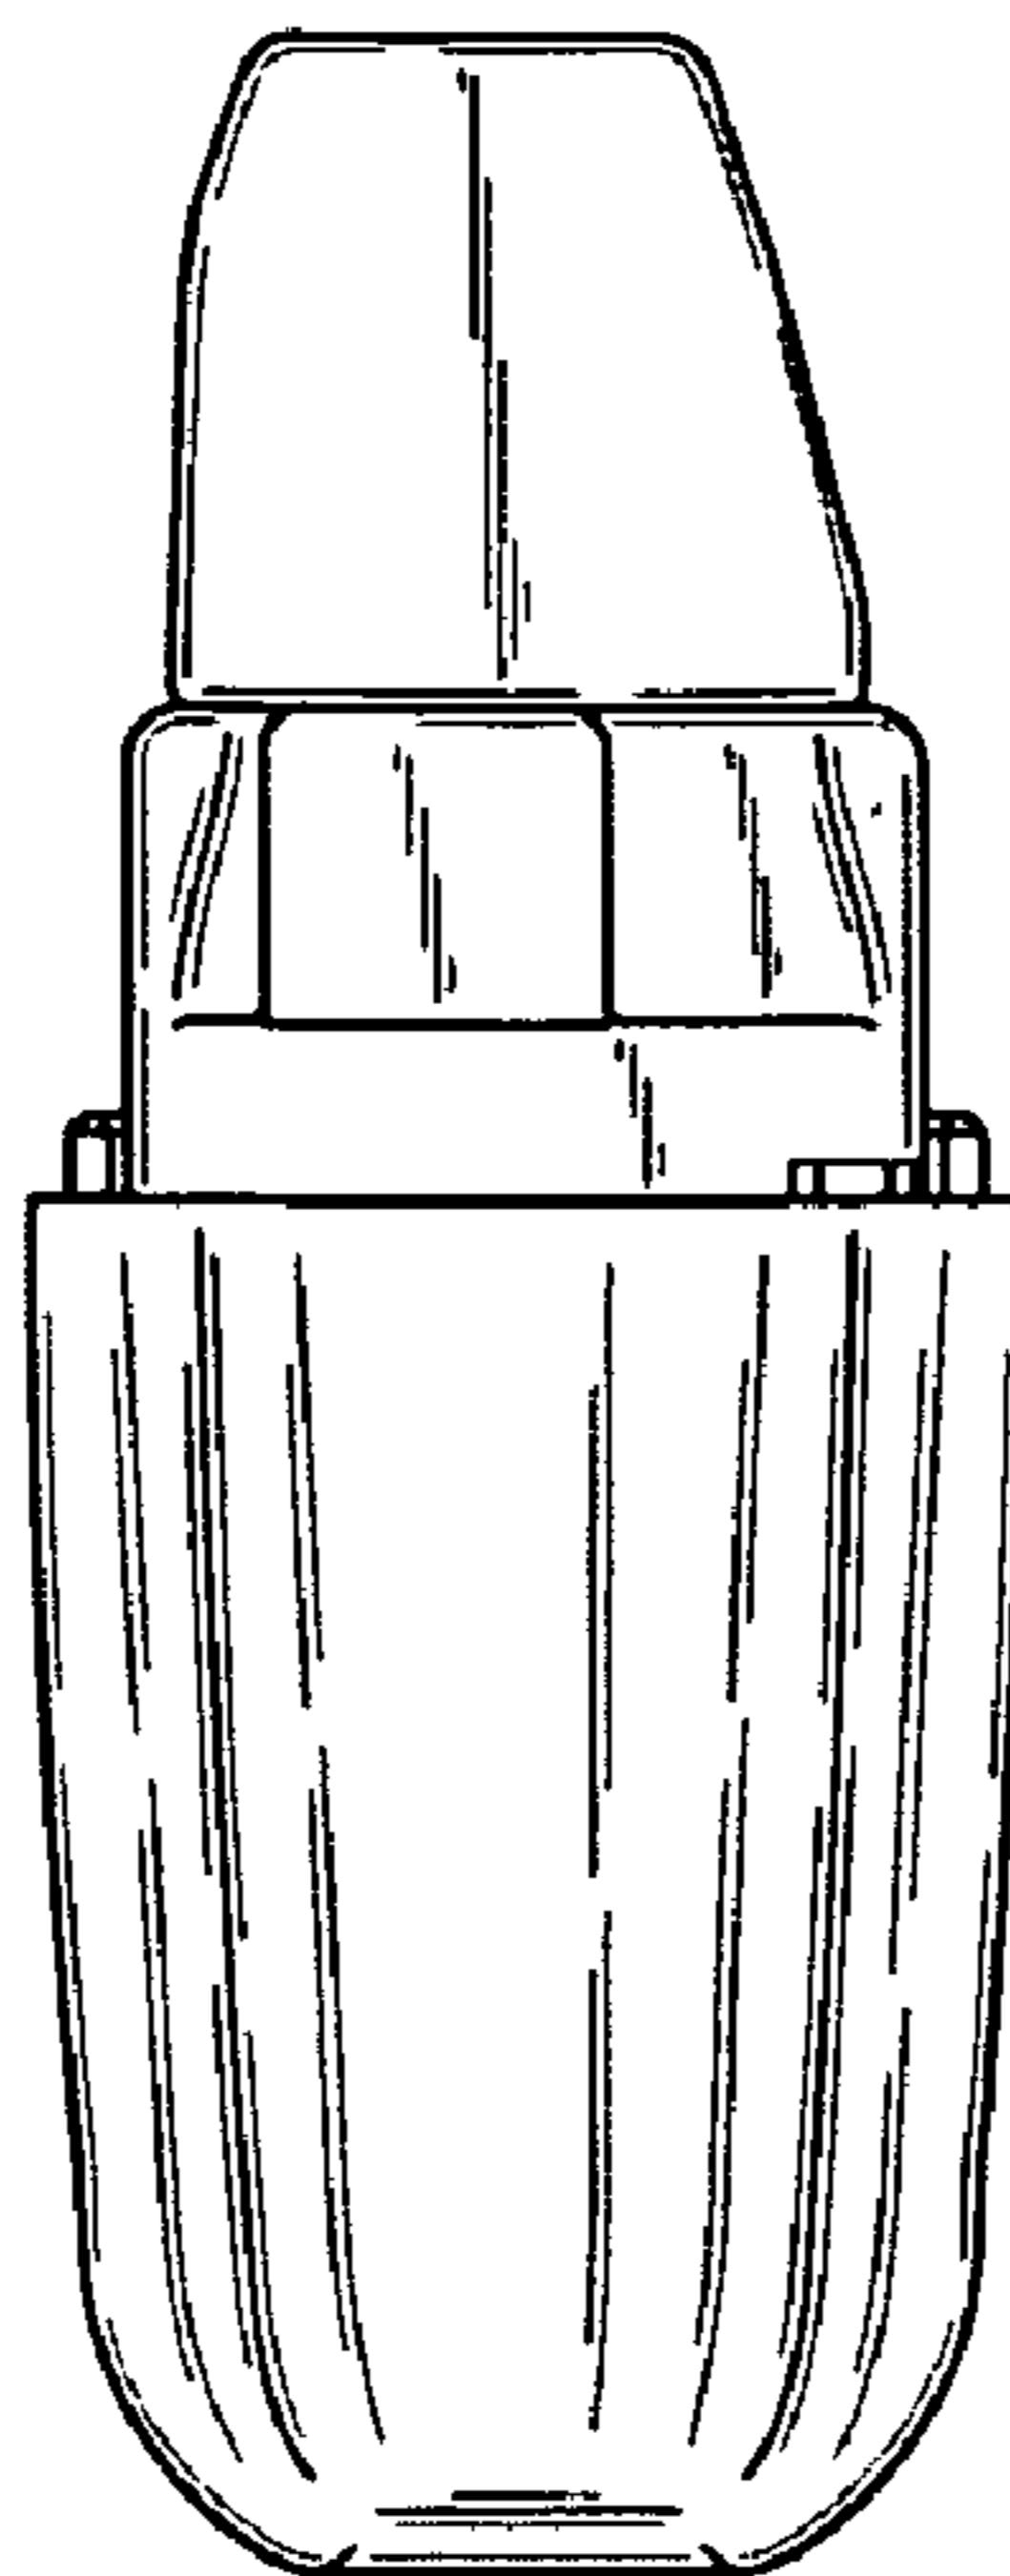


**Fig. 9**

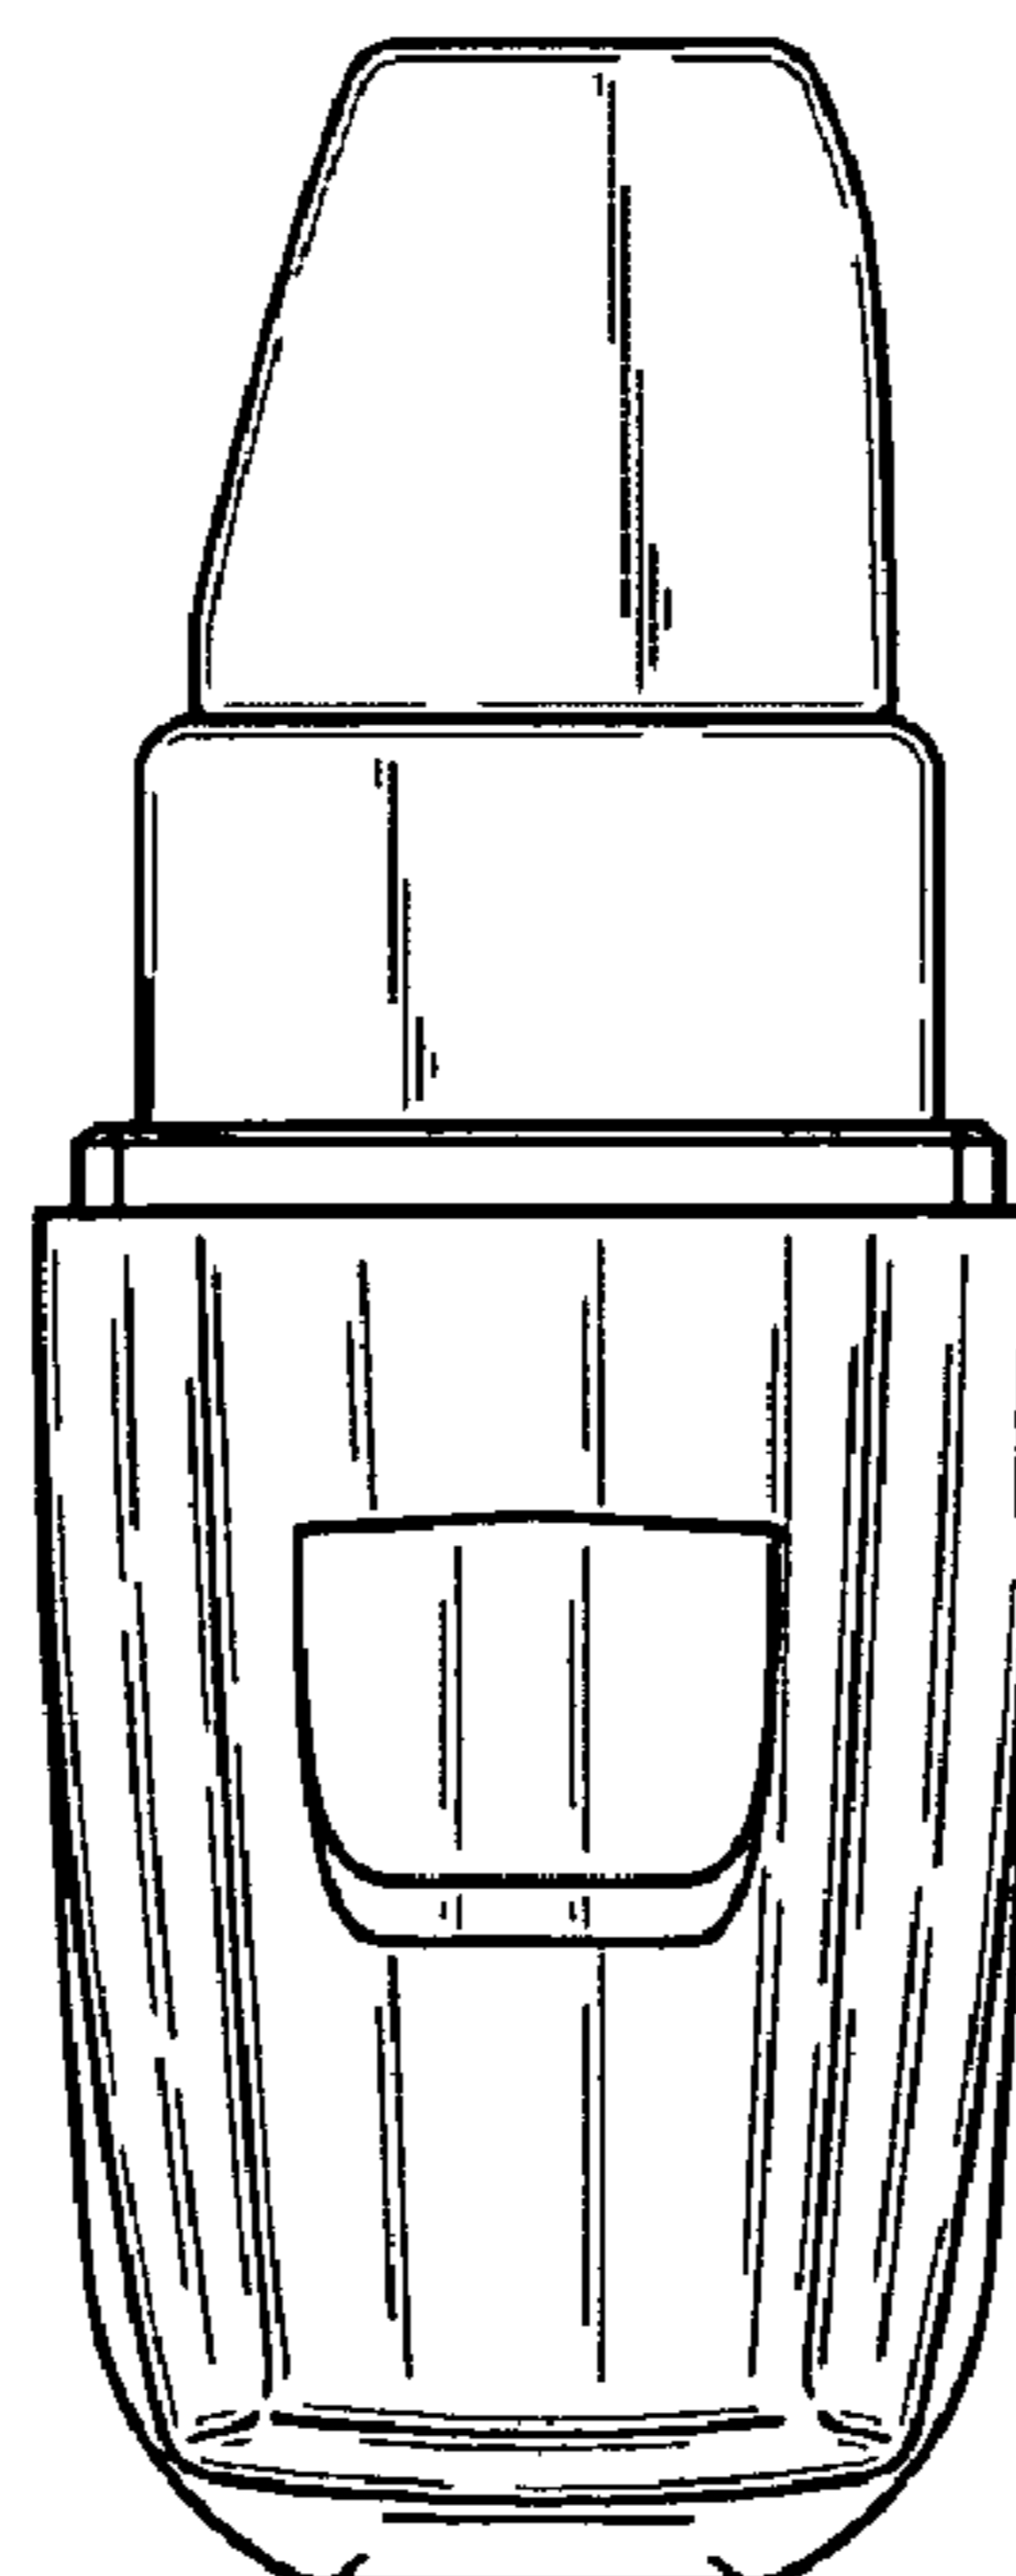

**Fig. 10**

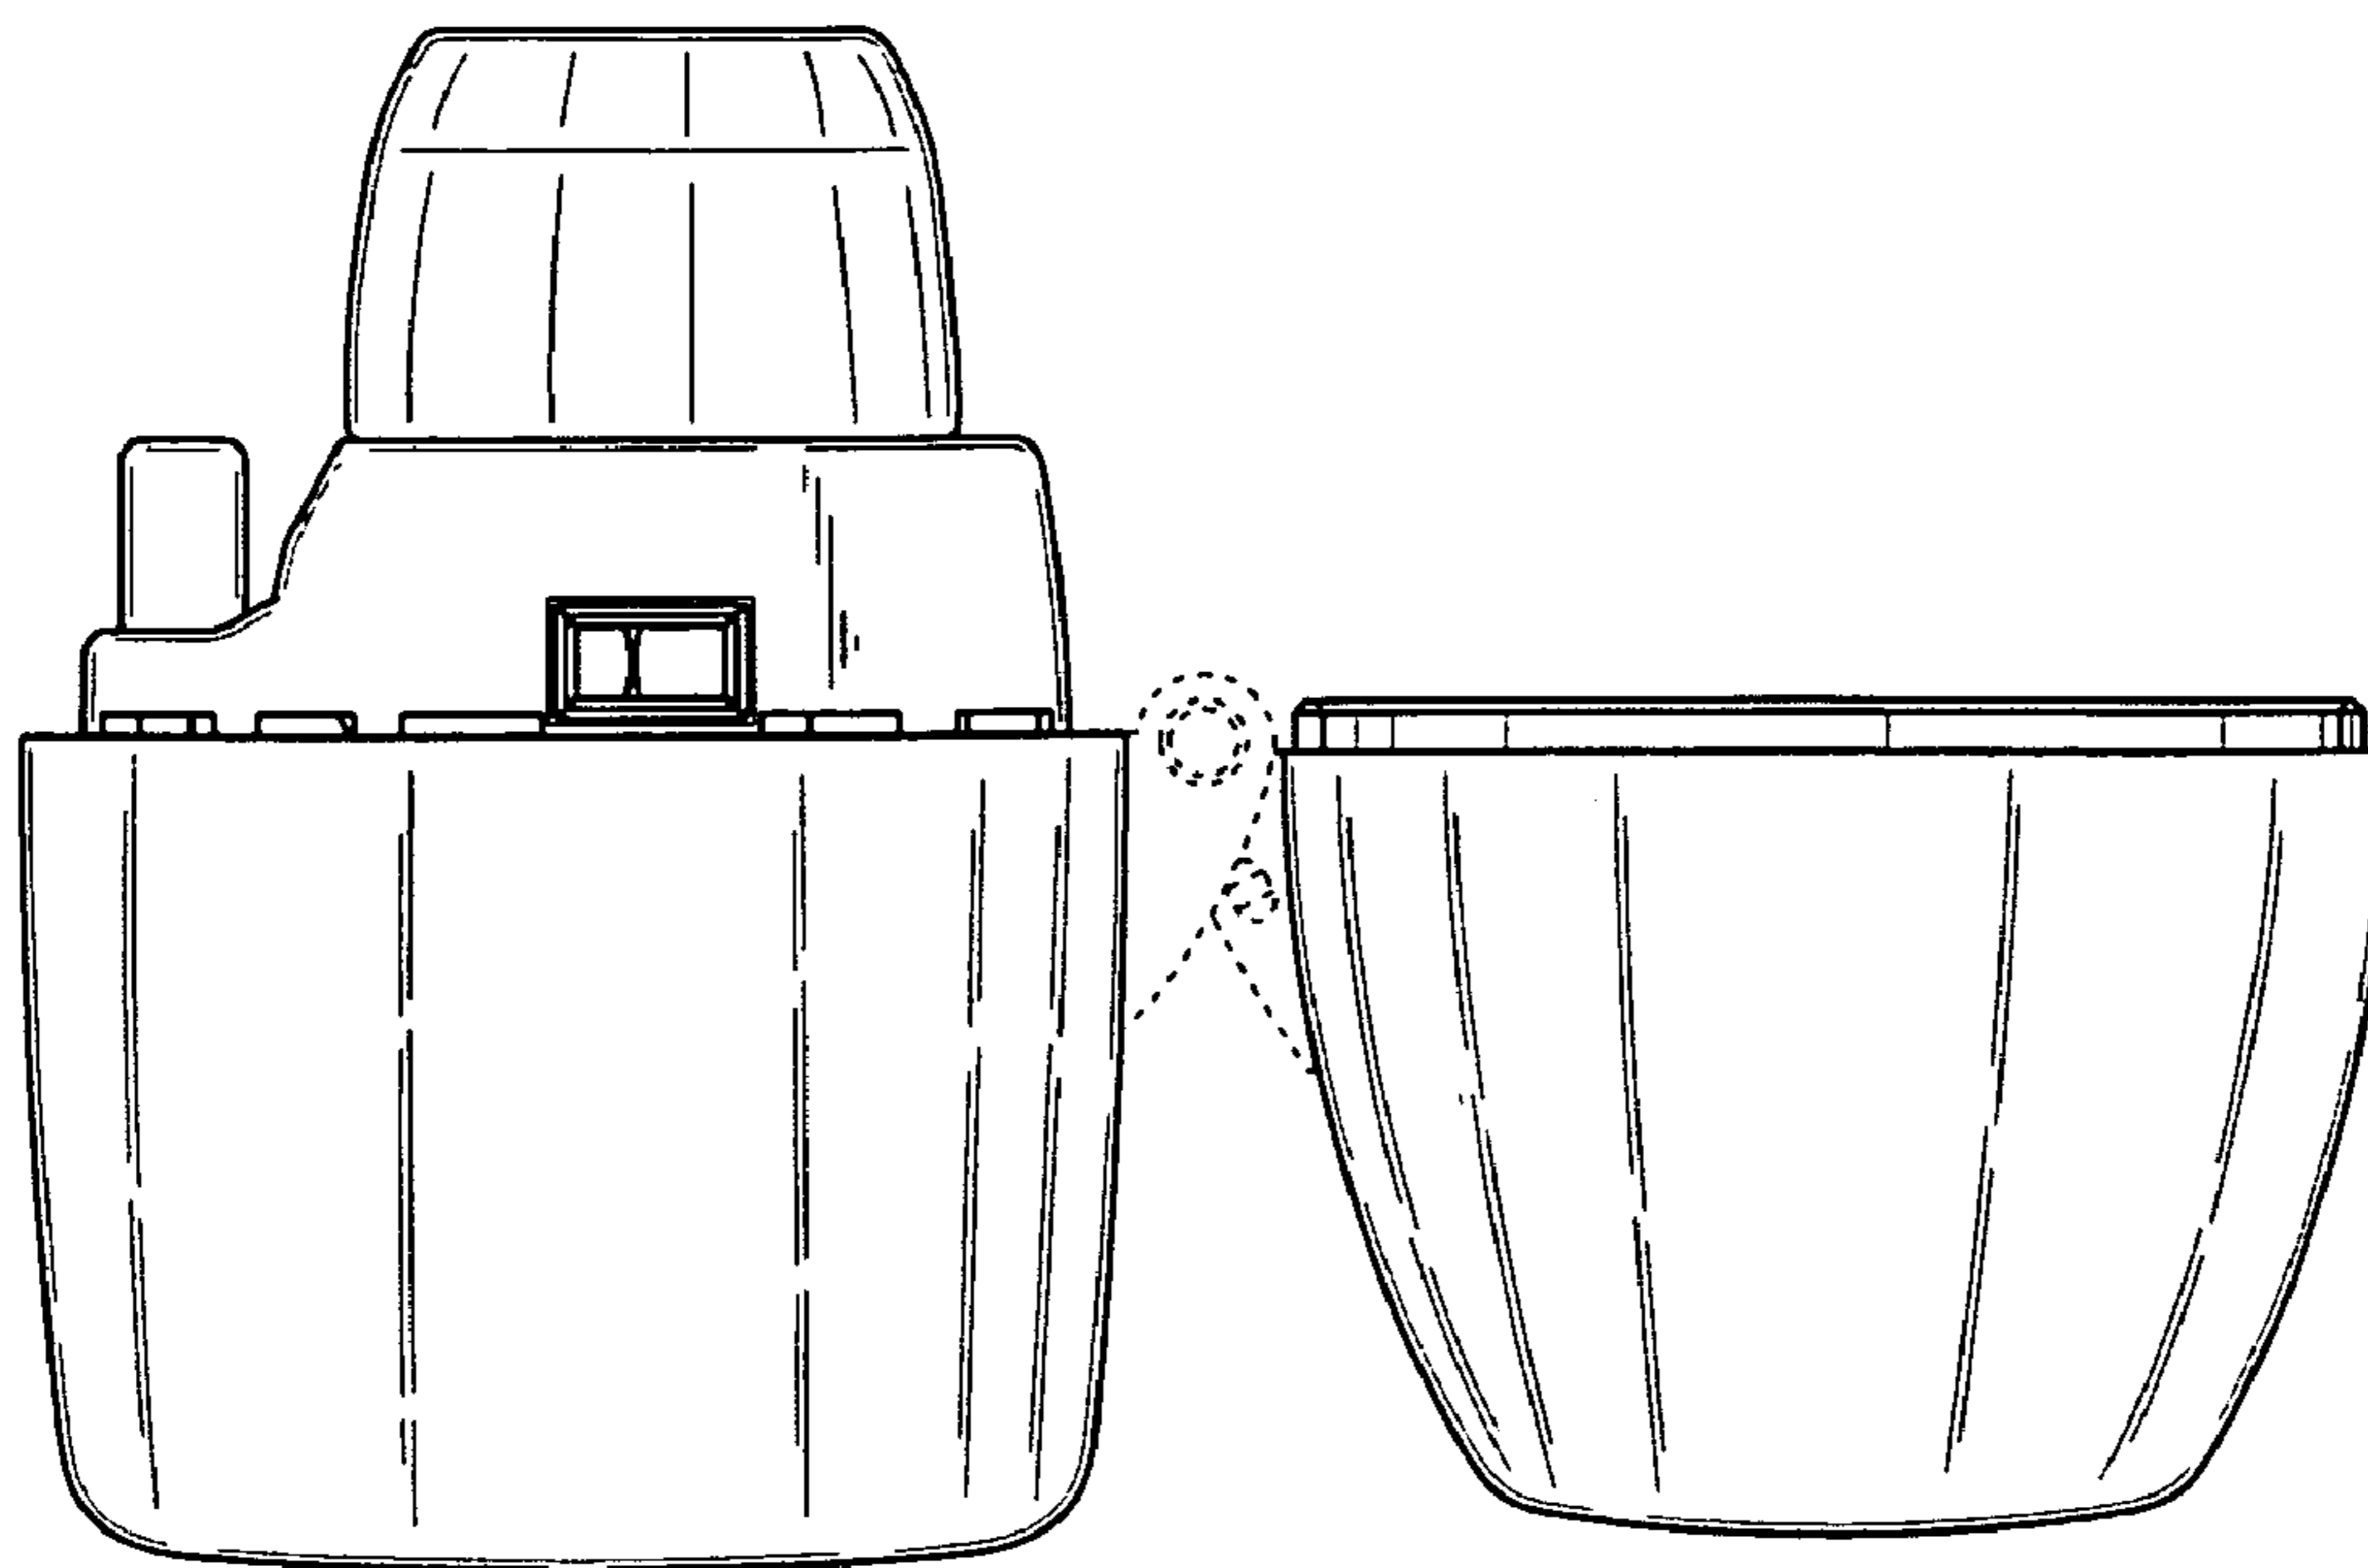


**Fig. 11**

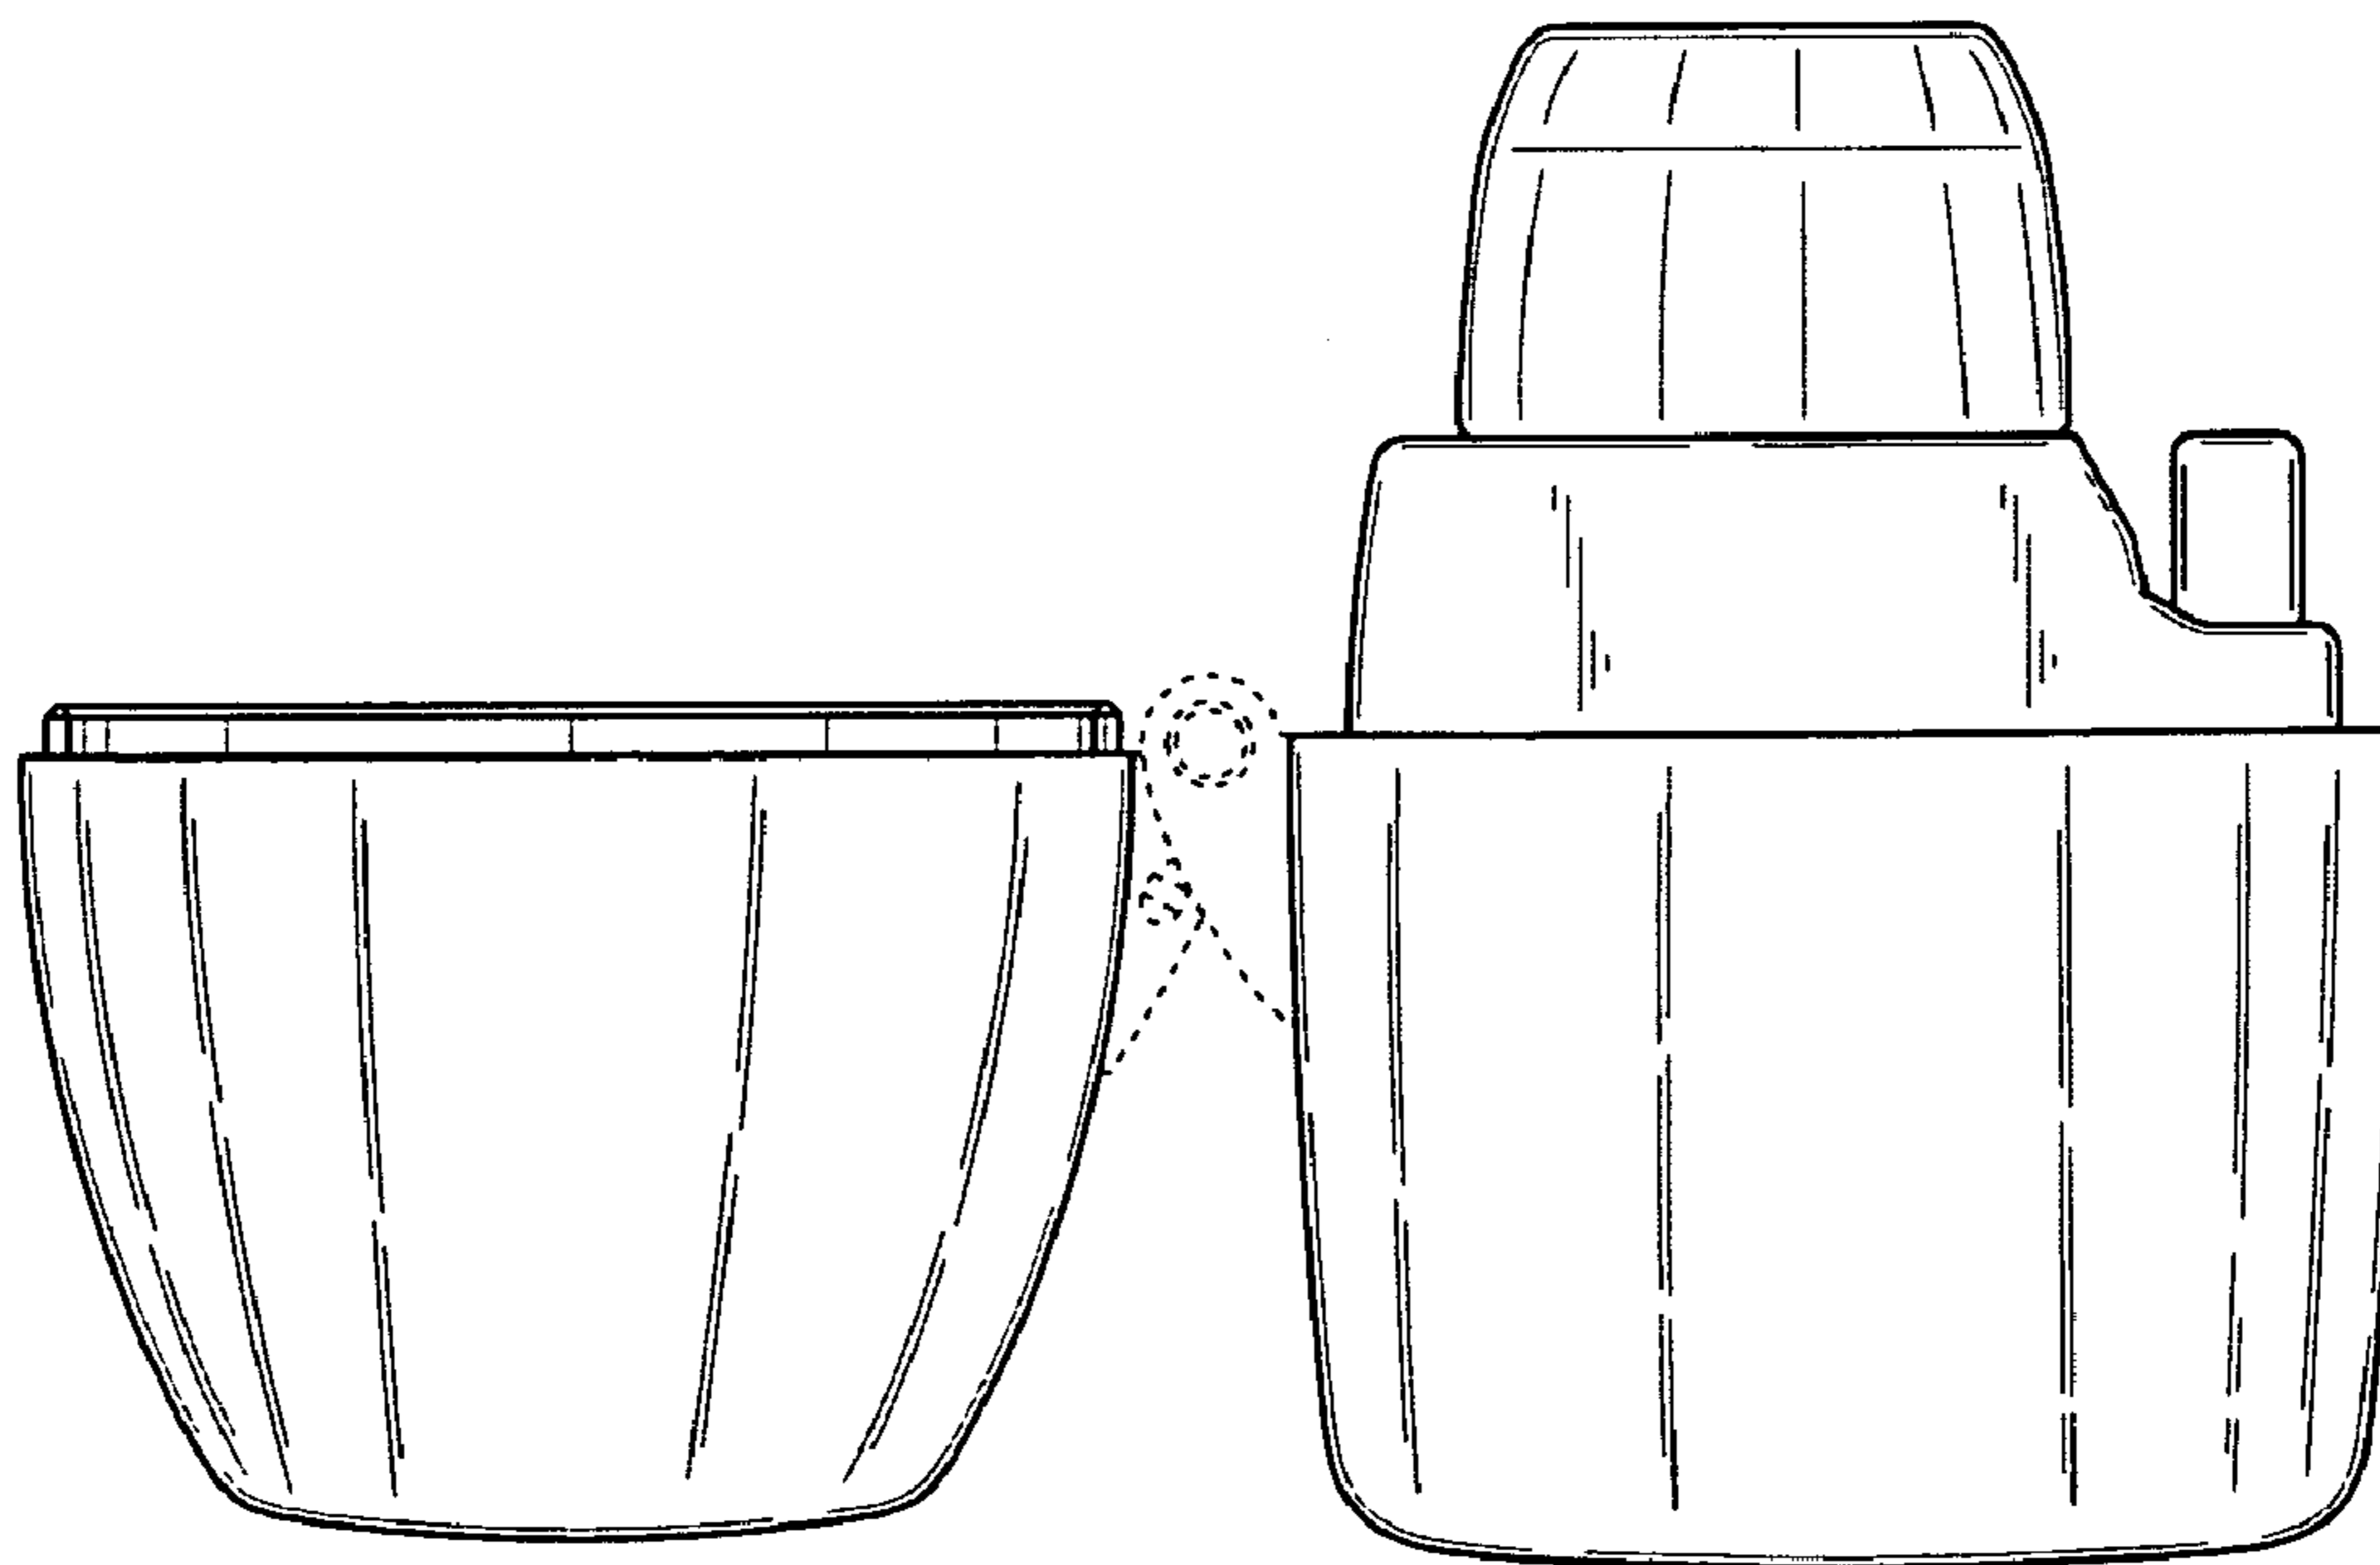


**Fig. 12**



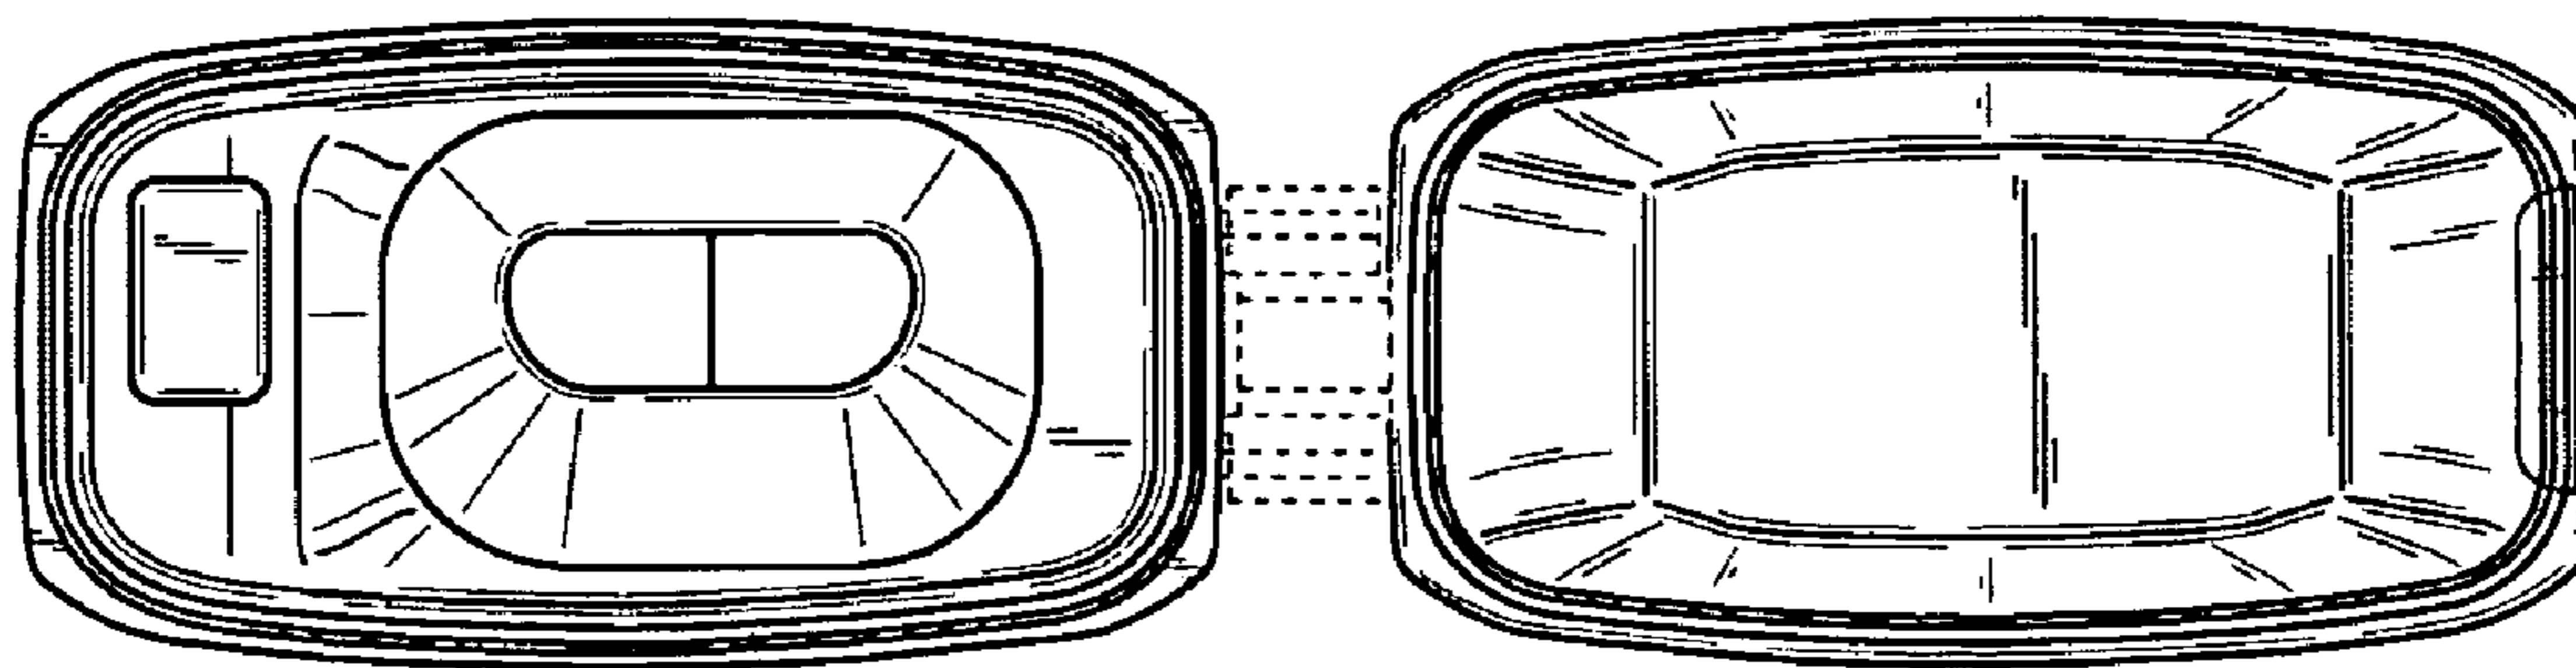

**Fig. 13**

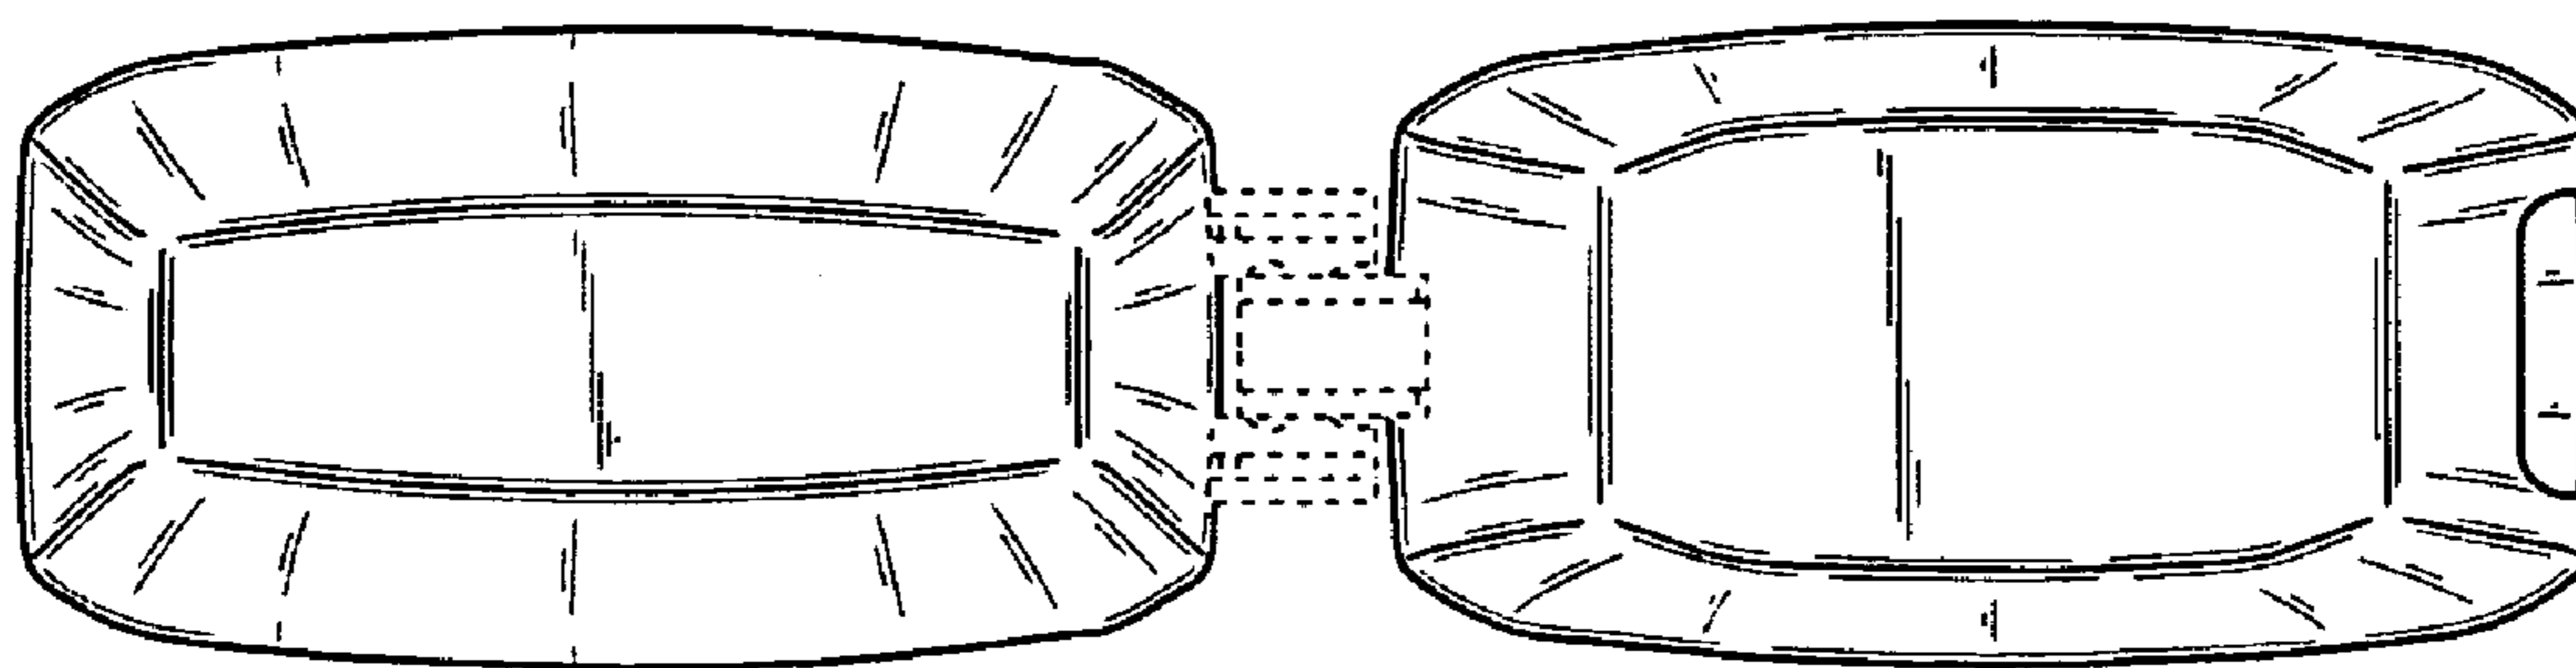

**Fig. 14**