



US00D614587S

(12) **United States Design Patent**
Yodfat et al.

(10) **Patent No.:** **US D614,587 S**
(45) **Date of Patent:** **** Apr. 27, 2010**

(54) **REMOTE CONTROL FOR DRUG INFUSION PUMP**

(75) Inventors: **Ofer Yodfat**, Maccabim-Reut (IL);
Avraham Neta, Misgav (IL); **Daphne Haim-Langford**, Zichron Yaakov (IL)

(73) Assignee: **Medingo, Ltd.**, Yoqneam (IL)

(**) Term: **14 Years**

(21) Appl. No.: **29/285,862**

(22) Filed: **Apr. 13, 2007**

(51) **LOC (9) Cl.** **14-03**

(52) **U.S. Cl.** **D13/168**

(58) **Field of Classification Search** D13/168,
D13/164, 171; D14/218, 100, 106, 113–115;
D10/104, 106, 108; 128/200.14; 340/425.5,
340/426, 825.31, 825.69, 825.72, 713, 990,
340/995; 604/19, 48, 65, 67, 207, 151; D24/133,
D24/138, 169, 184–185; 342/451, 419, 457;
343/357, 113

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D342,260	S	*	12/1993	Sakata	D14/218
D351,173	S	*	10/1994	Yeh	D14/218
D357,919	S	*	5/1995	Tsui	D14/218
D364,850	S	*	12/1995	Estrada et al.	D14/346
5,861,821	A	*	1/1999	Kato et al.	341/22
D411,539	S	*	6/1999	Nagai et al.	D14/218
D424,060	S	*	5/2000	Baker et al.	D14/218
D460,053	S	*	7/2002	Choi	D13/168
D469,708	S	*	2/2003	To et al.	D10/104
6,572,585	B2	*	6/2003	Choi	604/131
D476,973	S	*	7/2003	Yamagishi	D14/218
D477,591	S	*	7/2003	Hung	D14/218
6,656,159	B2	*	12/2003	Flaherty	604/131
6,689,091	B2	*	2/2004	Bui et al.	604/67
6,704,005	B2	*	3/2004	Kato et al.	345/173
D494,145	S	*	8/2004	Klimas	D13/168

D531,137	S	*	10/2006	Wu	D13/168
7,271,734	B2	*	9/2007	Sata et al.	340/825.72
2003/0167036	A1	*	9/2003	Flaherty	604/67
2004/0087894	A1	*	5/2004	Flaherty	604/65
2007/0255250	A1	*	11/2007	Moberg et al.	604/503
2009/0247931	A1	*	10/2009	Damgaard-Sorensen	604/19
2009/0254037	A1	*	10/2009	Bryant et al.	604/151

* cited by examiner

Primary Examiner—T. Chase Nelson
Assistant Examiner—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Mintz, Levin, Cohn, Ferris, Glovsky and Popeo PC

(57) **CLAIM**

The ornamental design of a remote control for drug infusion pump, as shown and described.

DESCRIPTION

FIG. 1 is a right side view of a remote control for drug infusion pump;

FIG. 2 is a left side view of a remote control for drug infusion pump;

FIG. 3 is a front side view of a remote control for drug infusion pump;

FIG. 4 is a rear view of a remote control for drug infusion pump;

FIG. 5 is a top view of a remote control for drug infusion pump;


FIG. 6 is a bottom view of a remote control for drug infusion pump;

FIG. 7 is a first isometric view of a remote control for drug infusion pump;

FIG. 8 is a second isometric view of a remote control for drug infusion pump; and,

FIG. 9 is a third isometric view of a remote control for drug infusion pump.

1 Claim, 7 Drawing Sheets

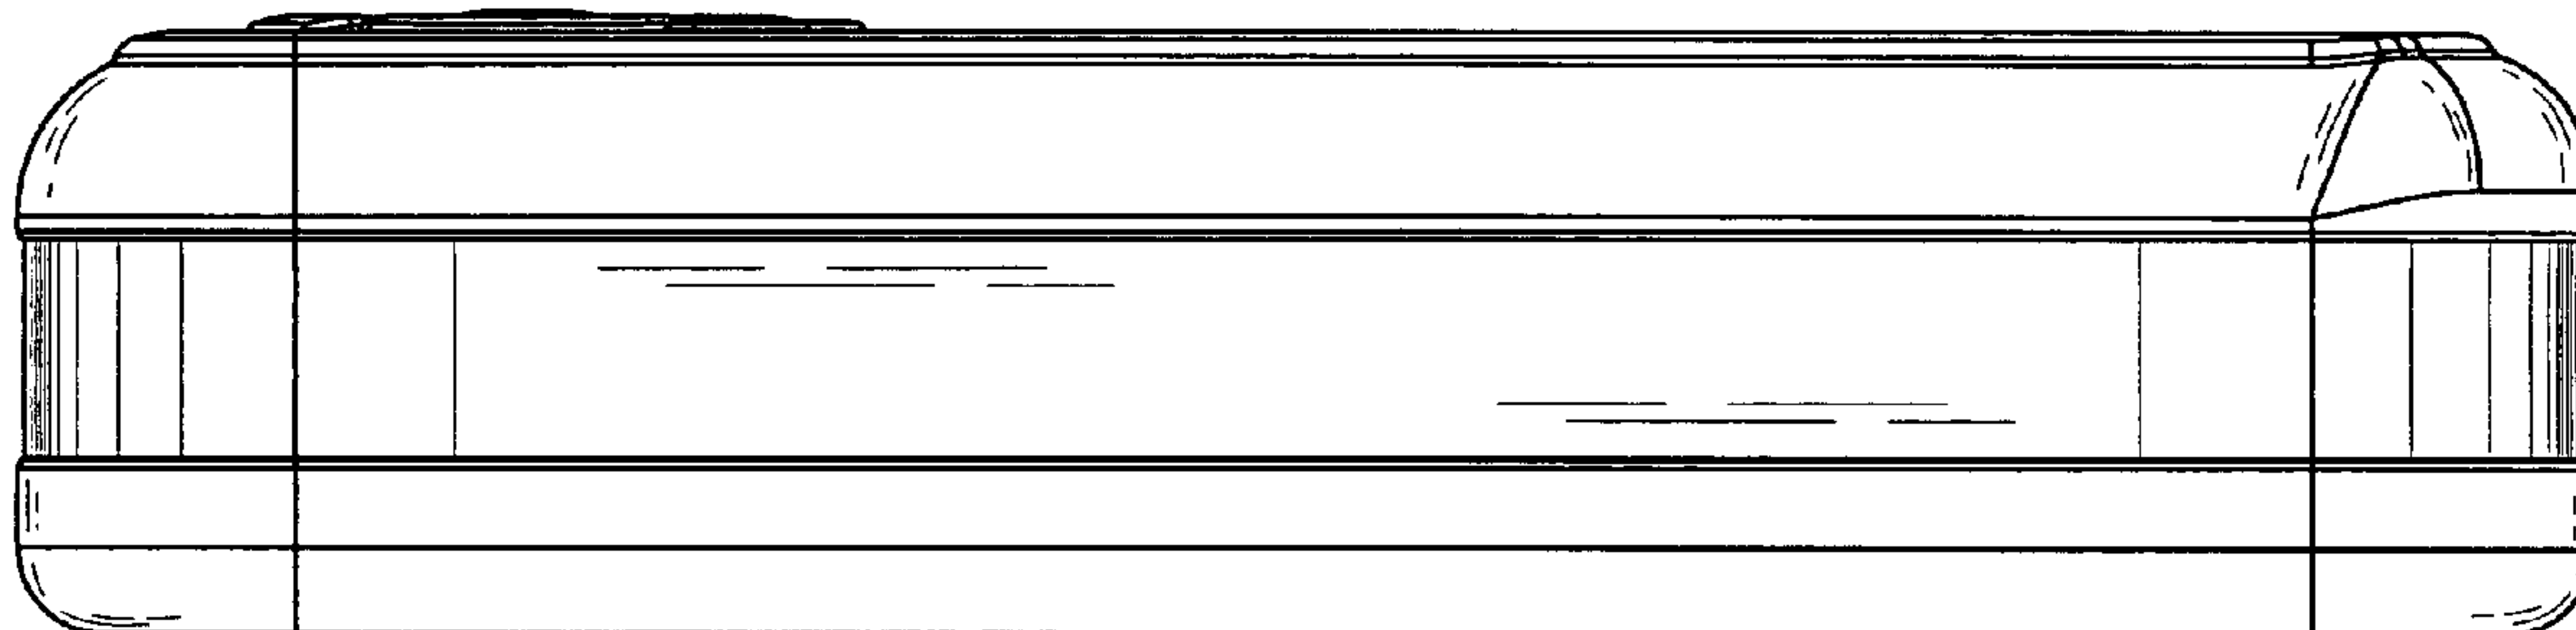

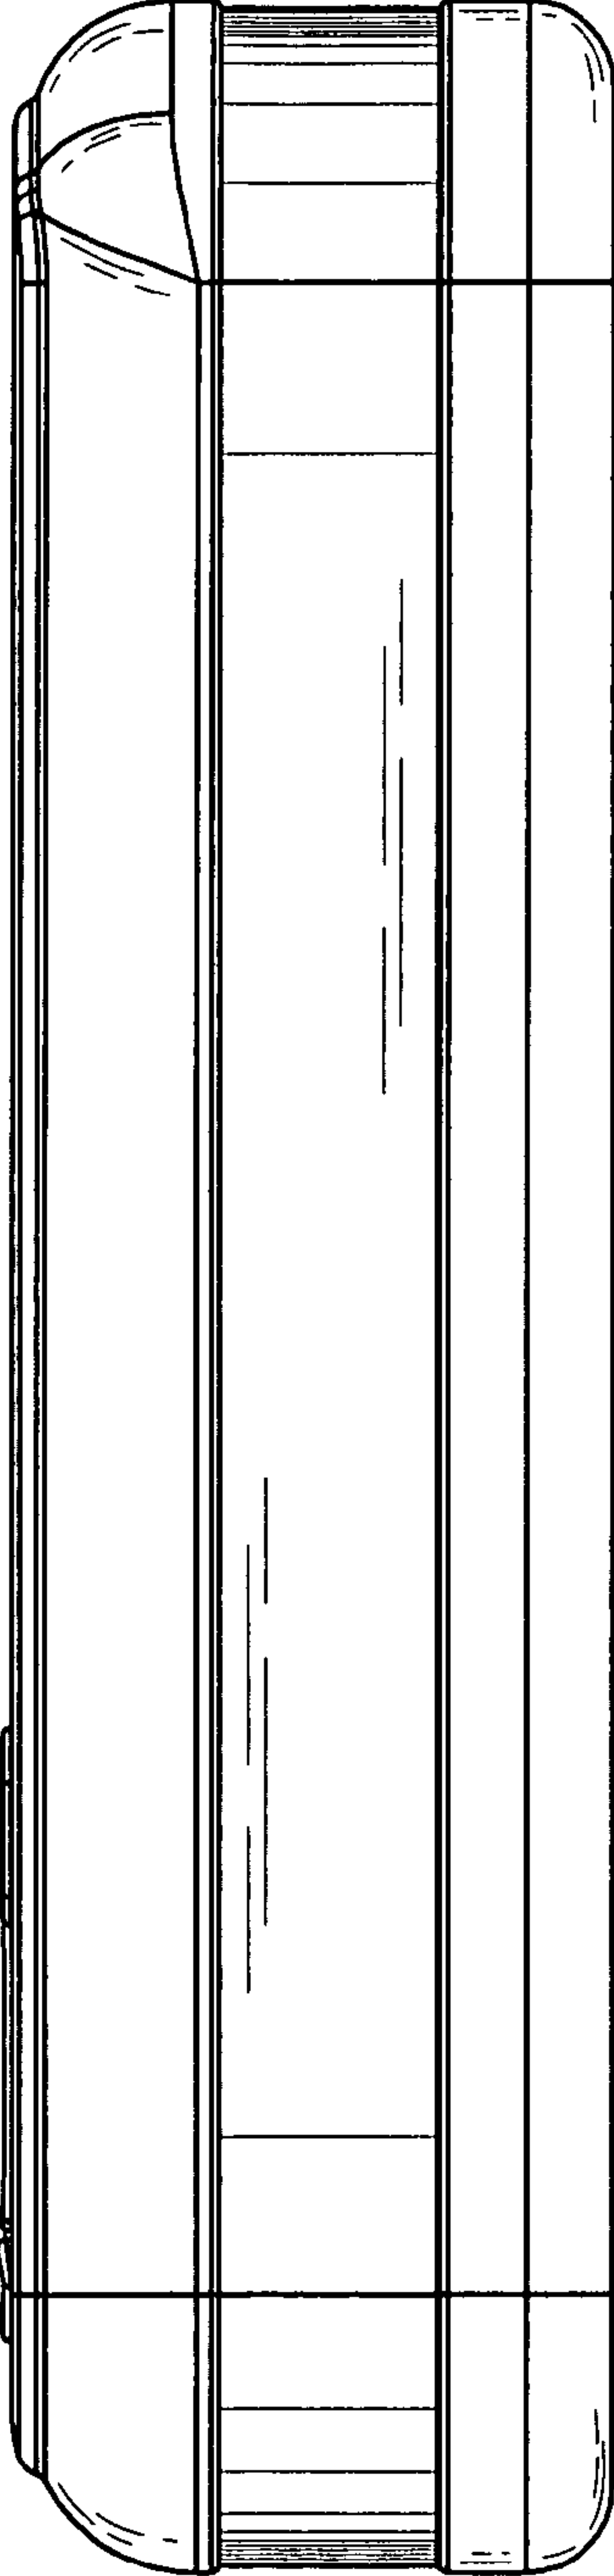


Fig. 1

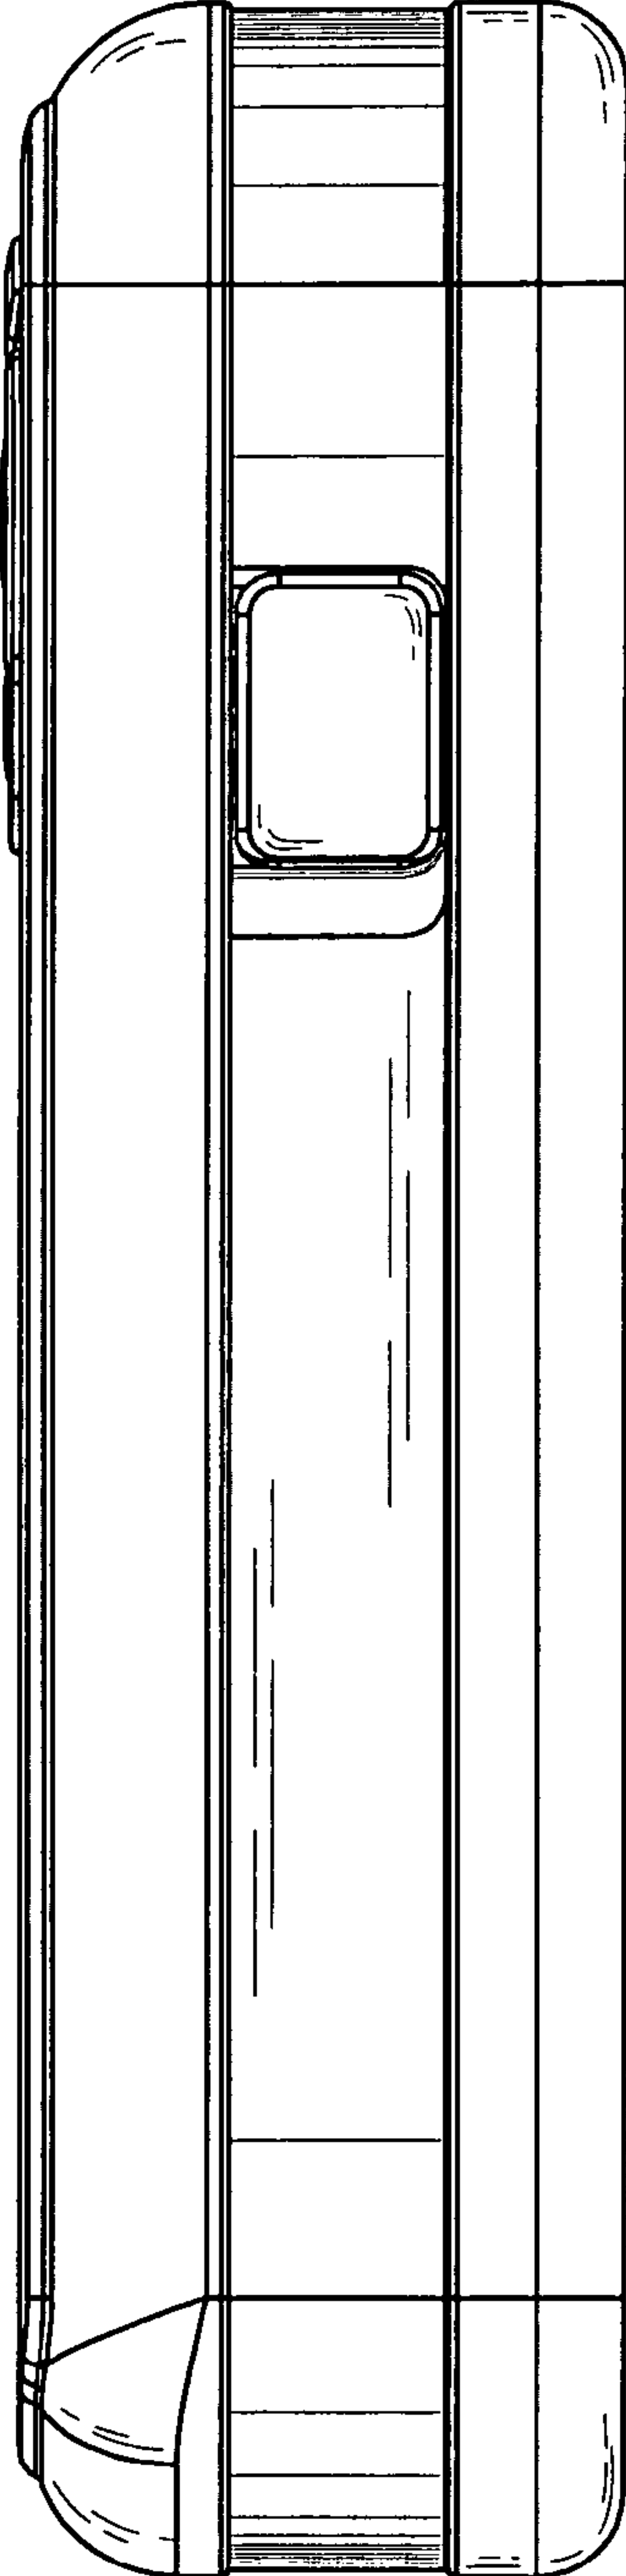


Fig. 2

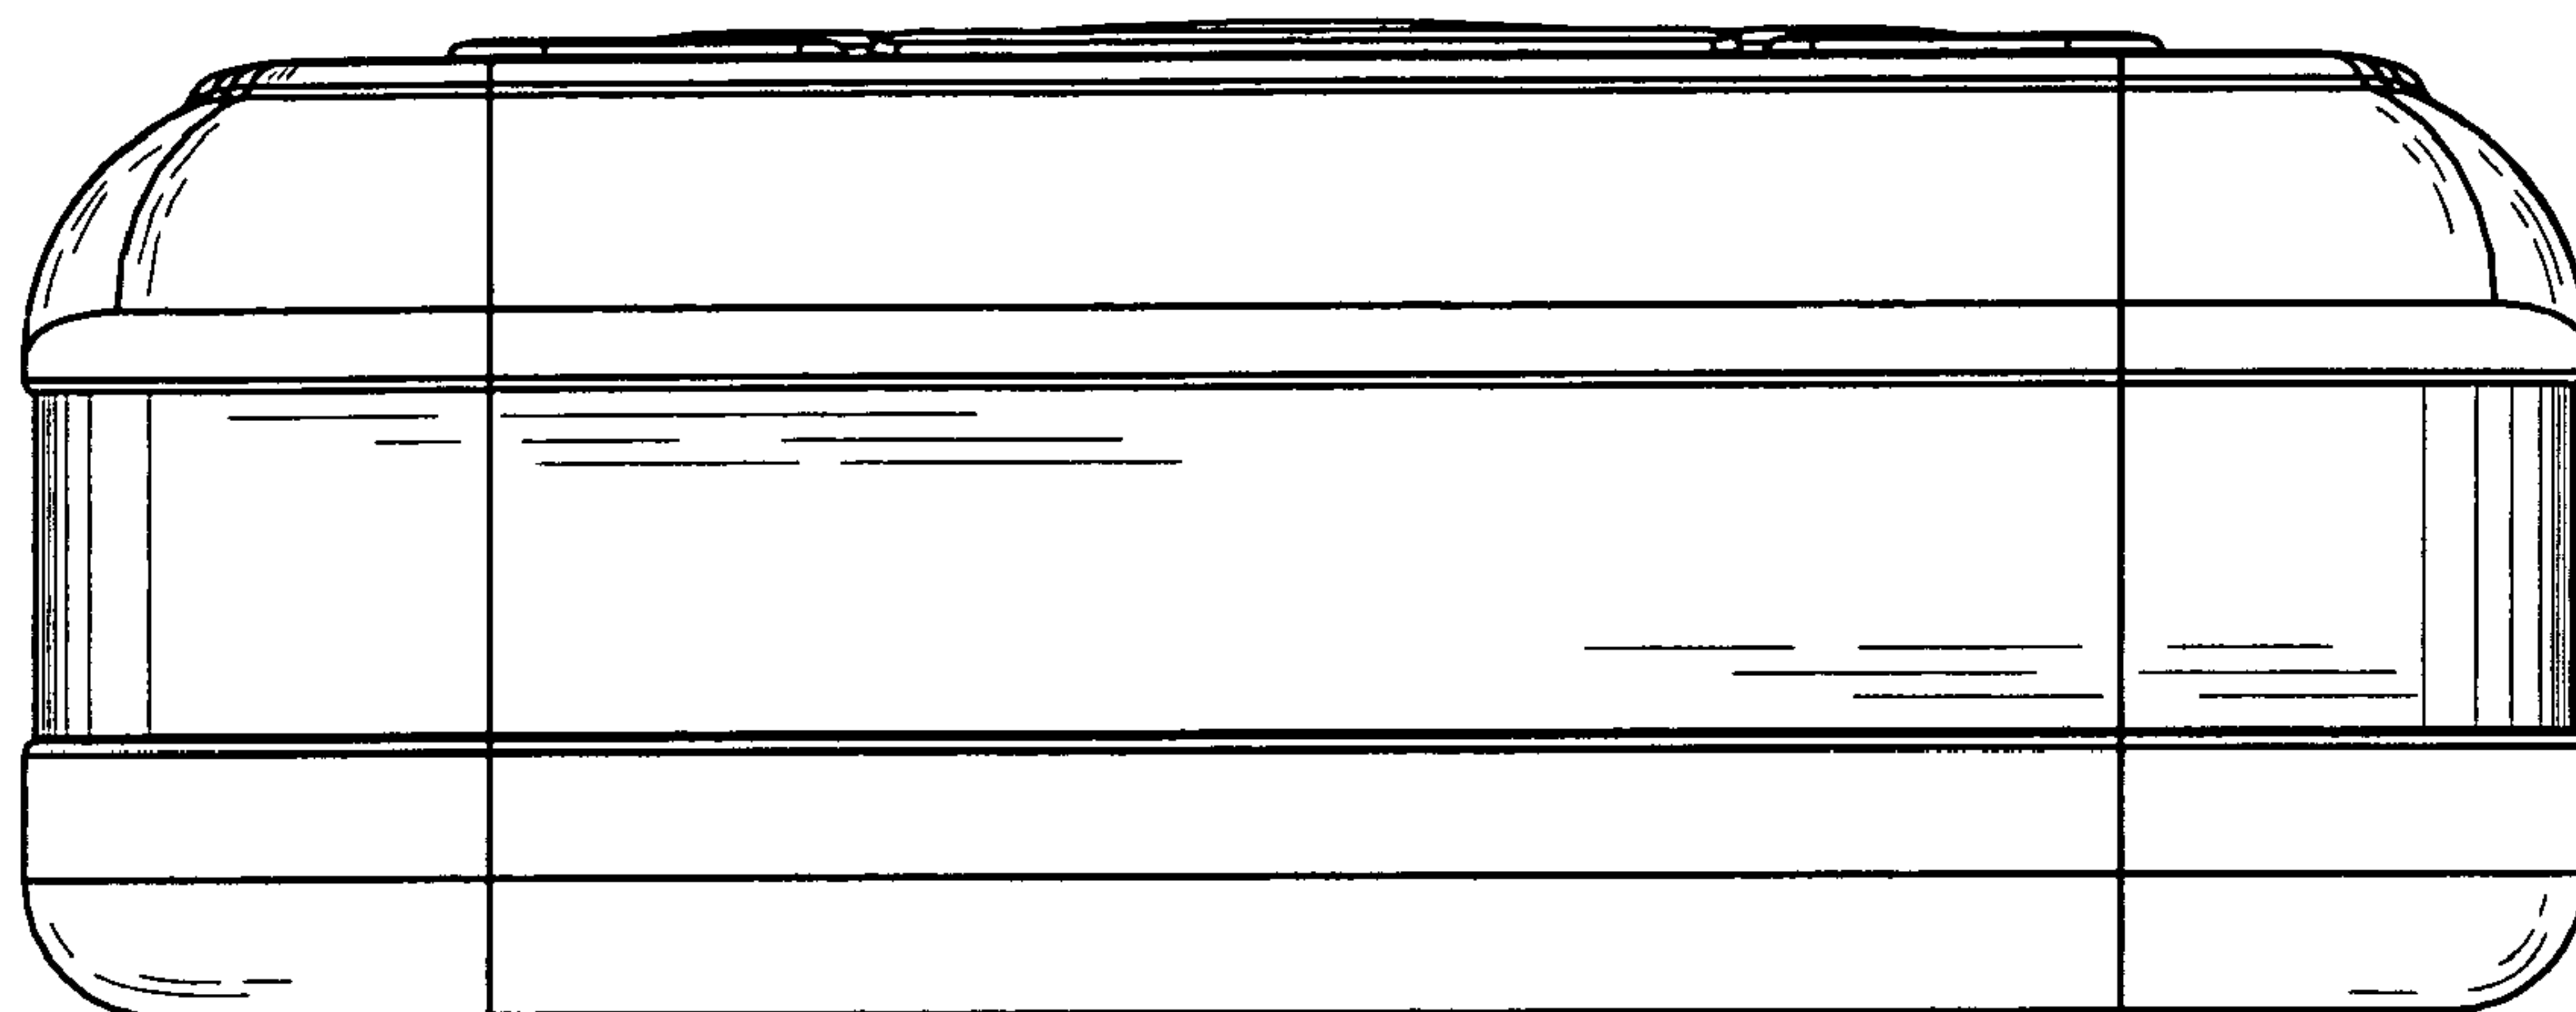


Fig. 3

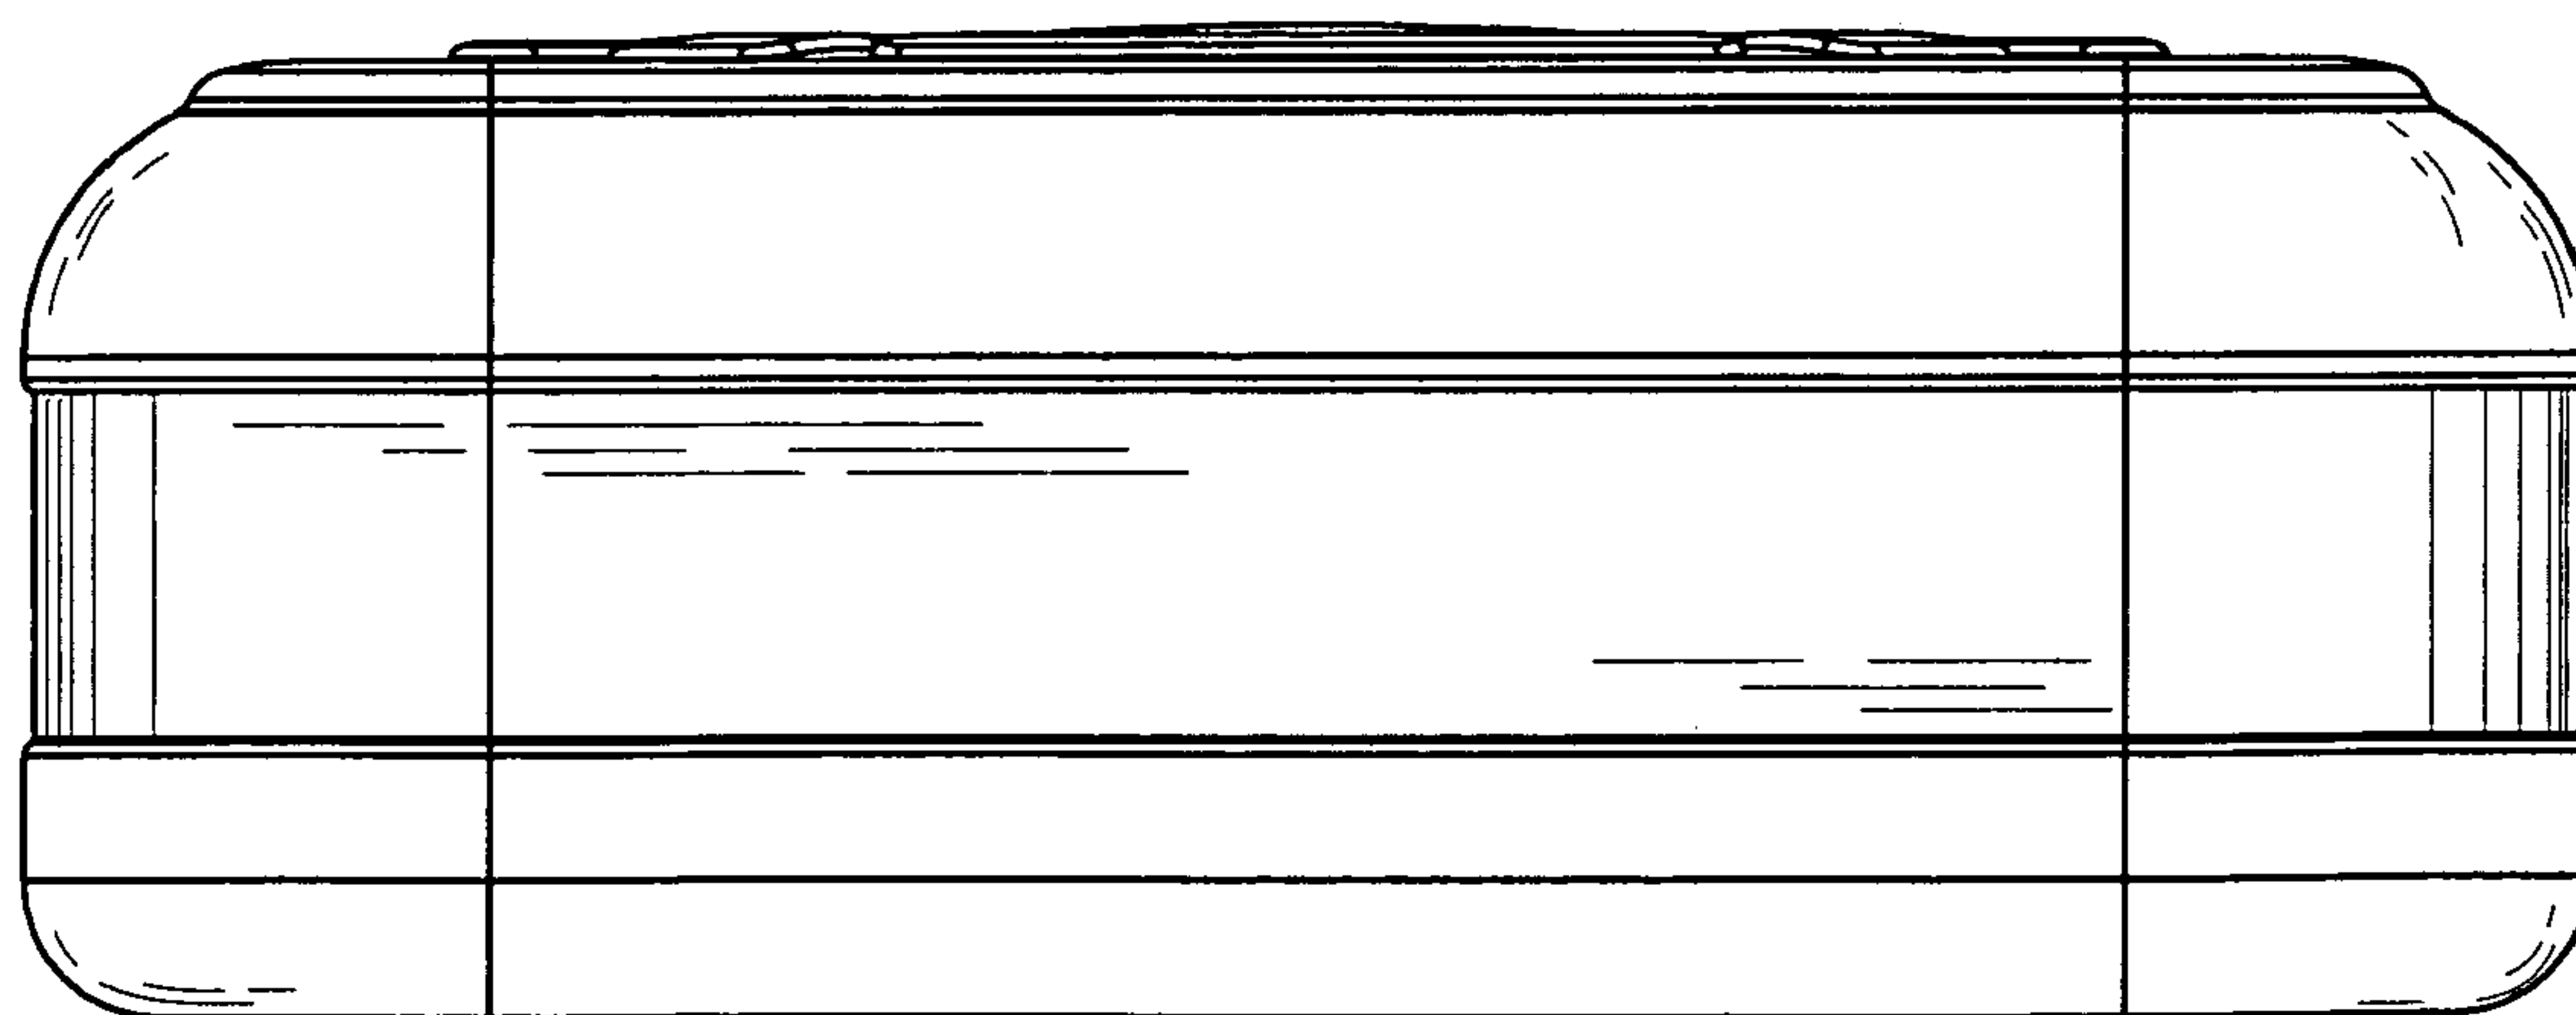


Fig. 4

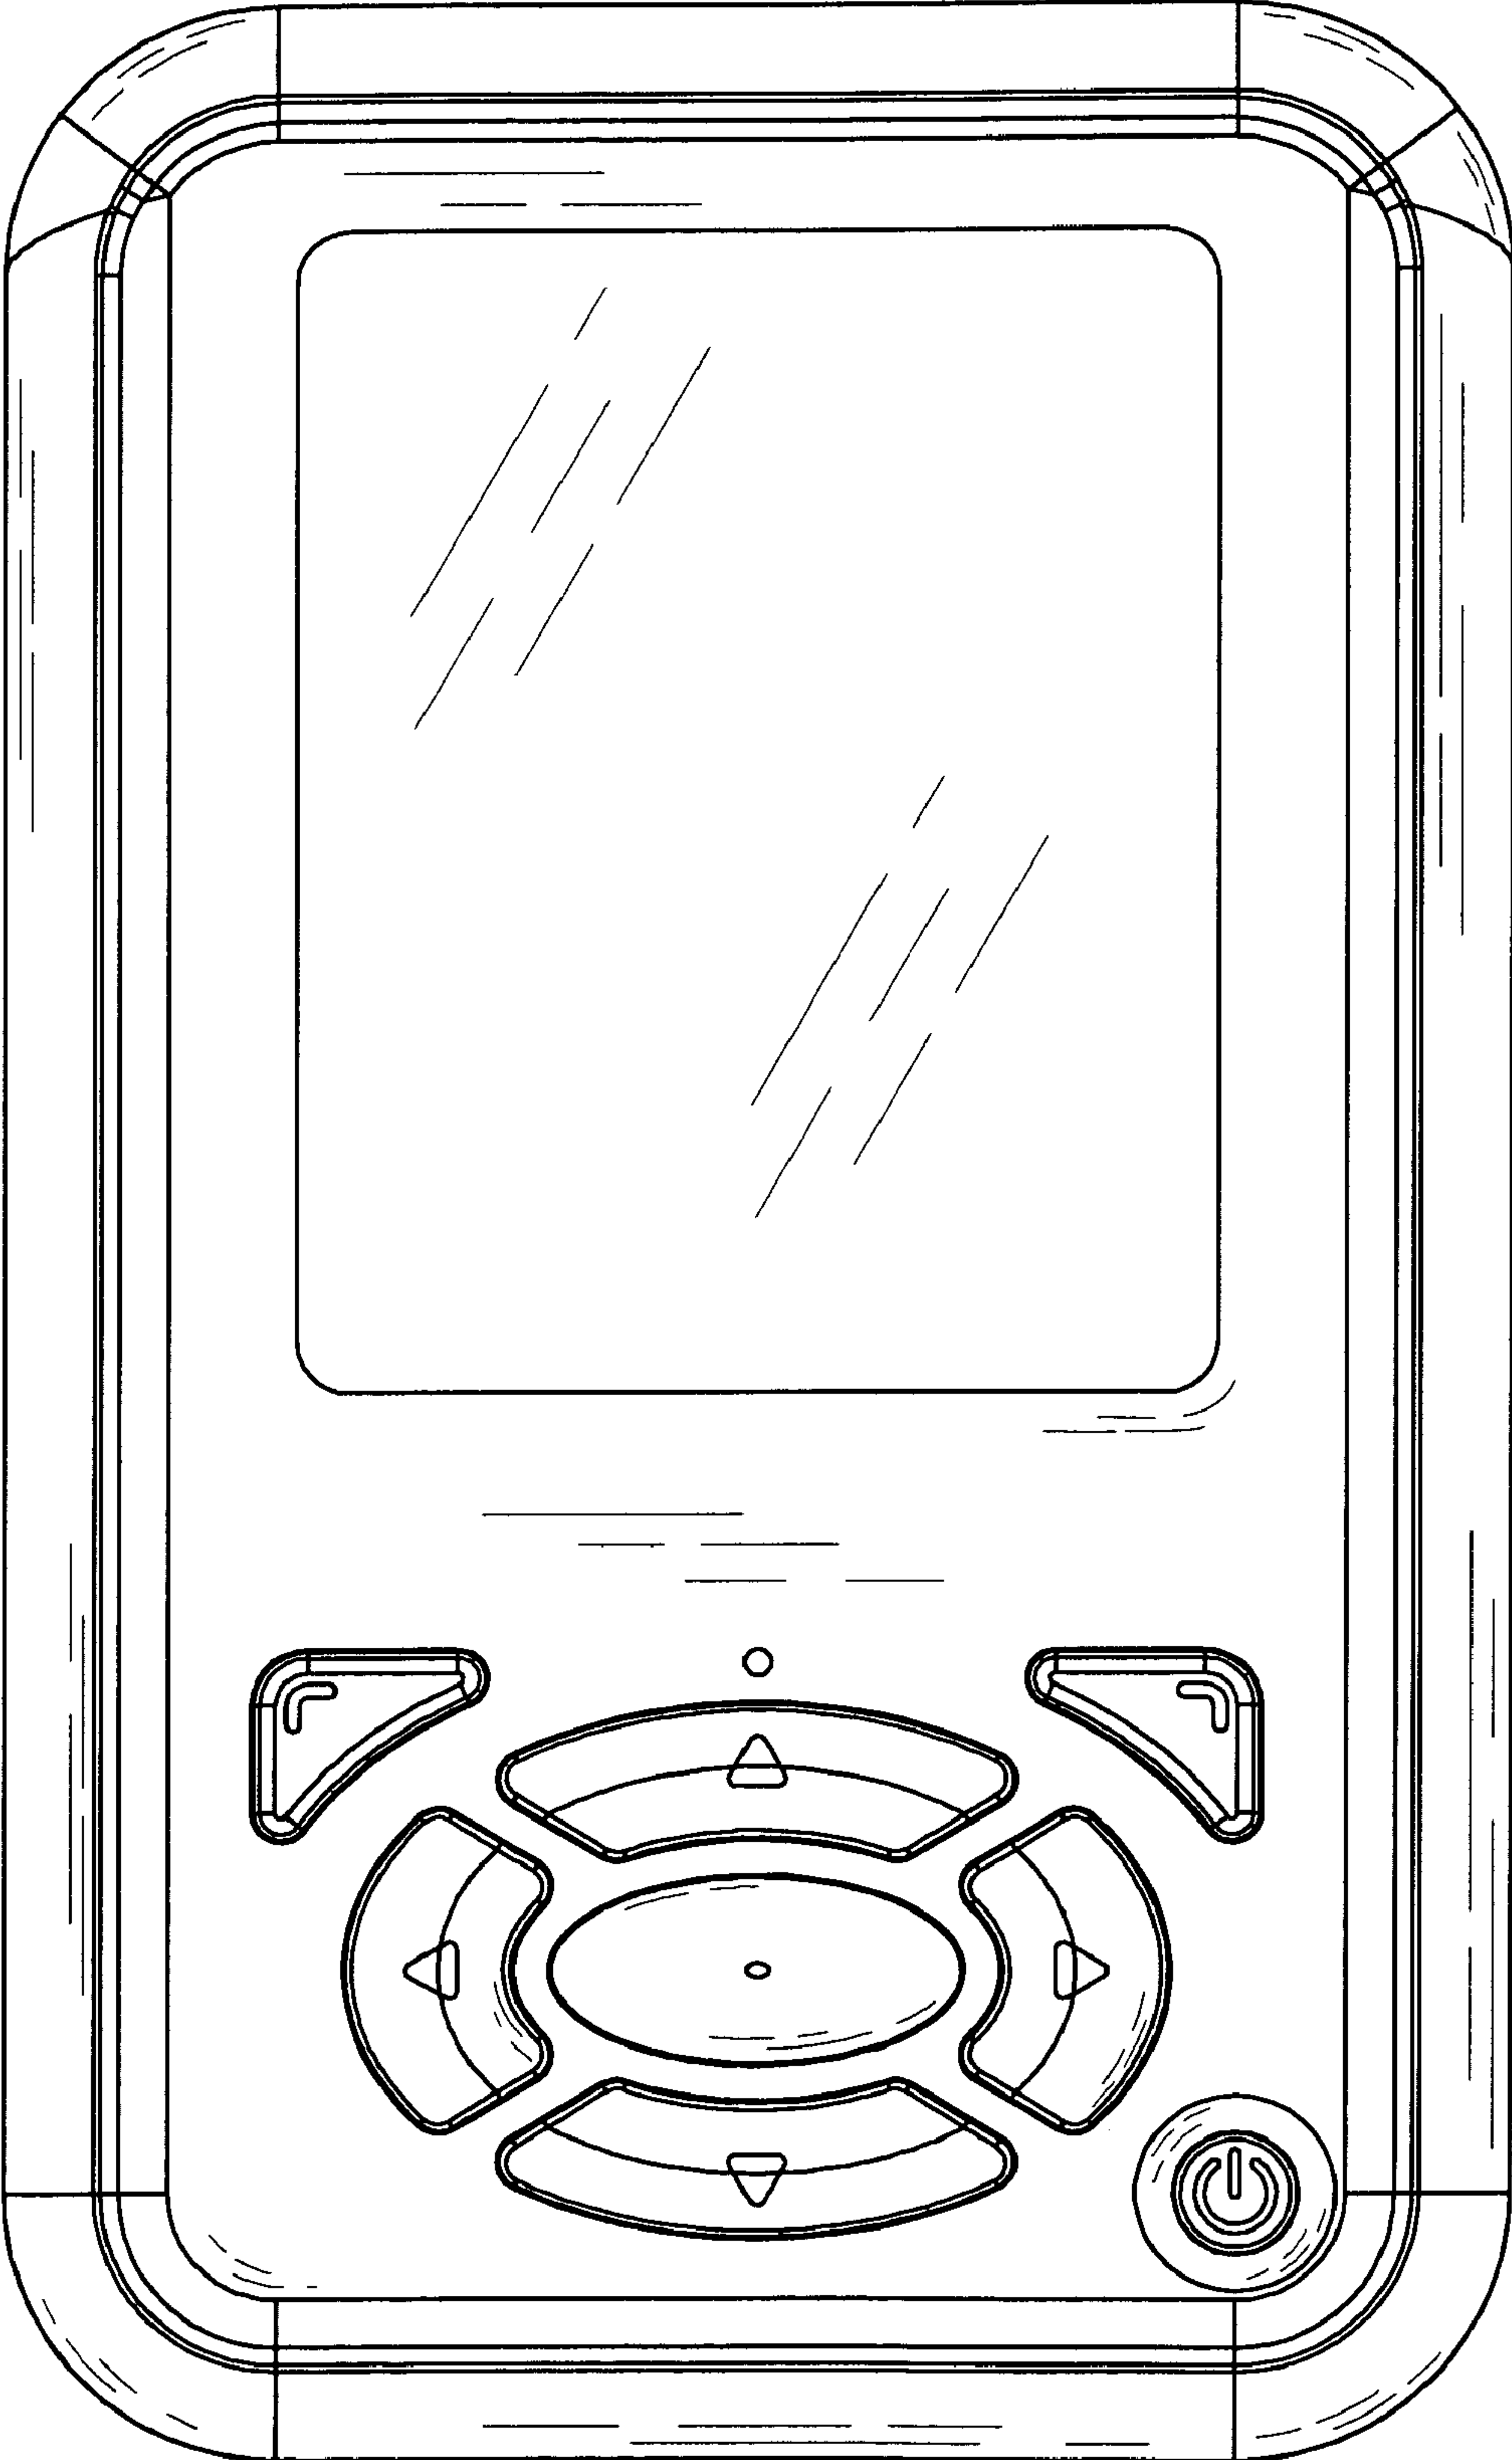


Fig. 5

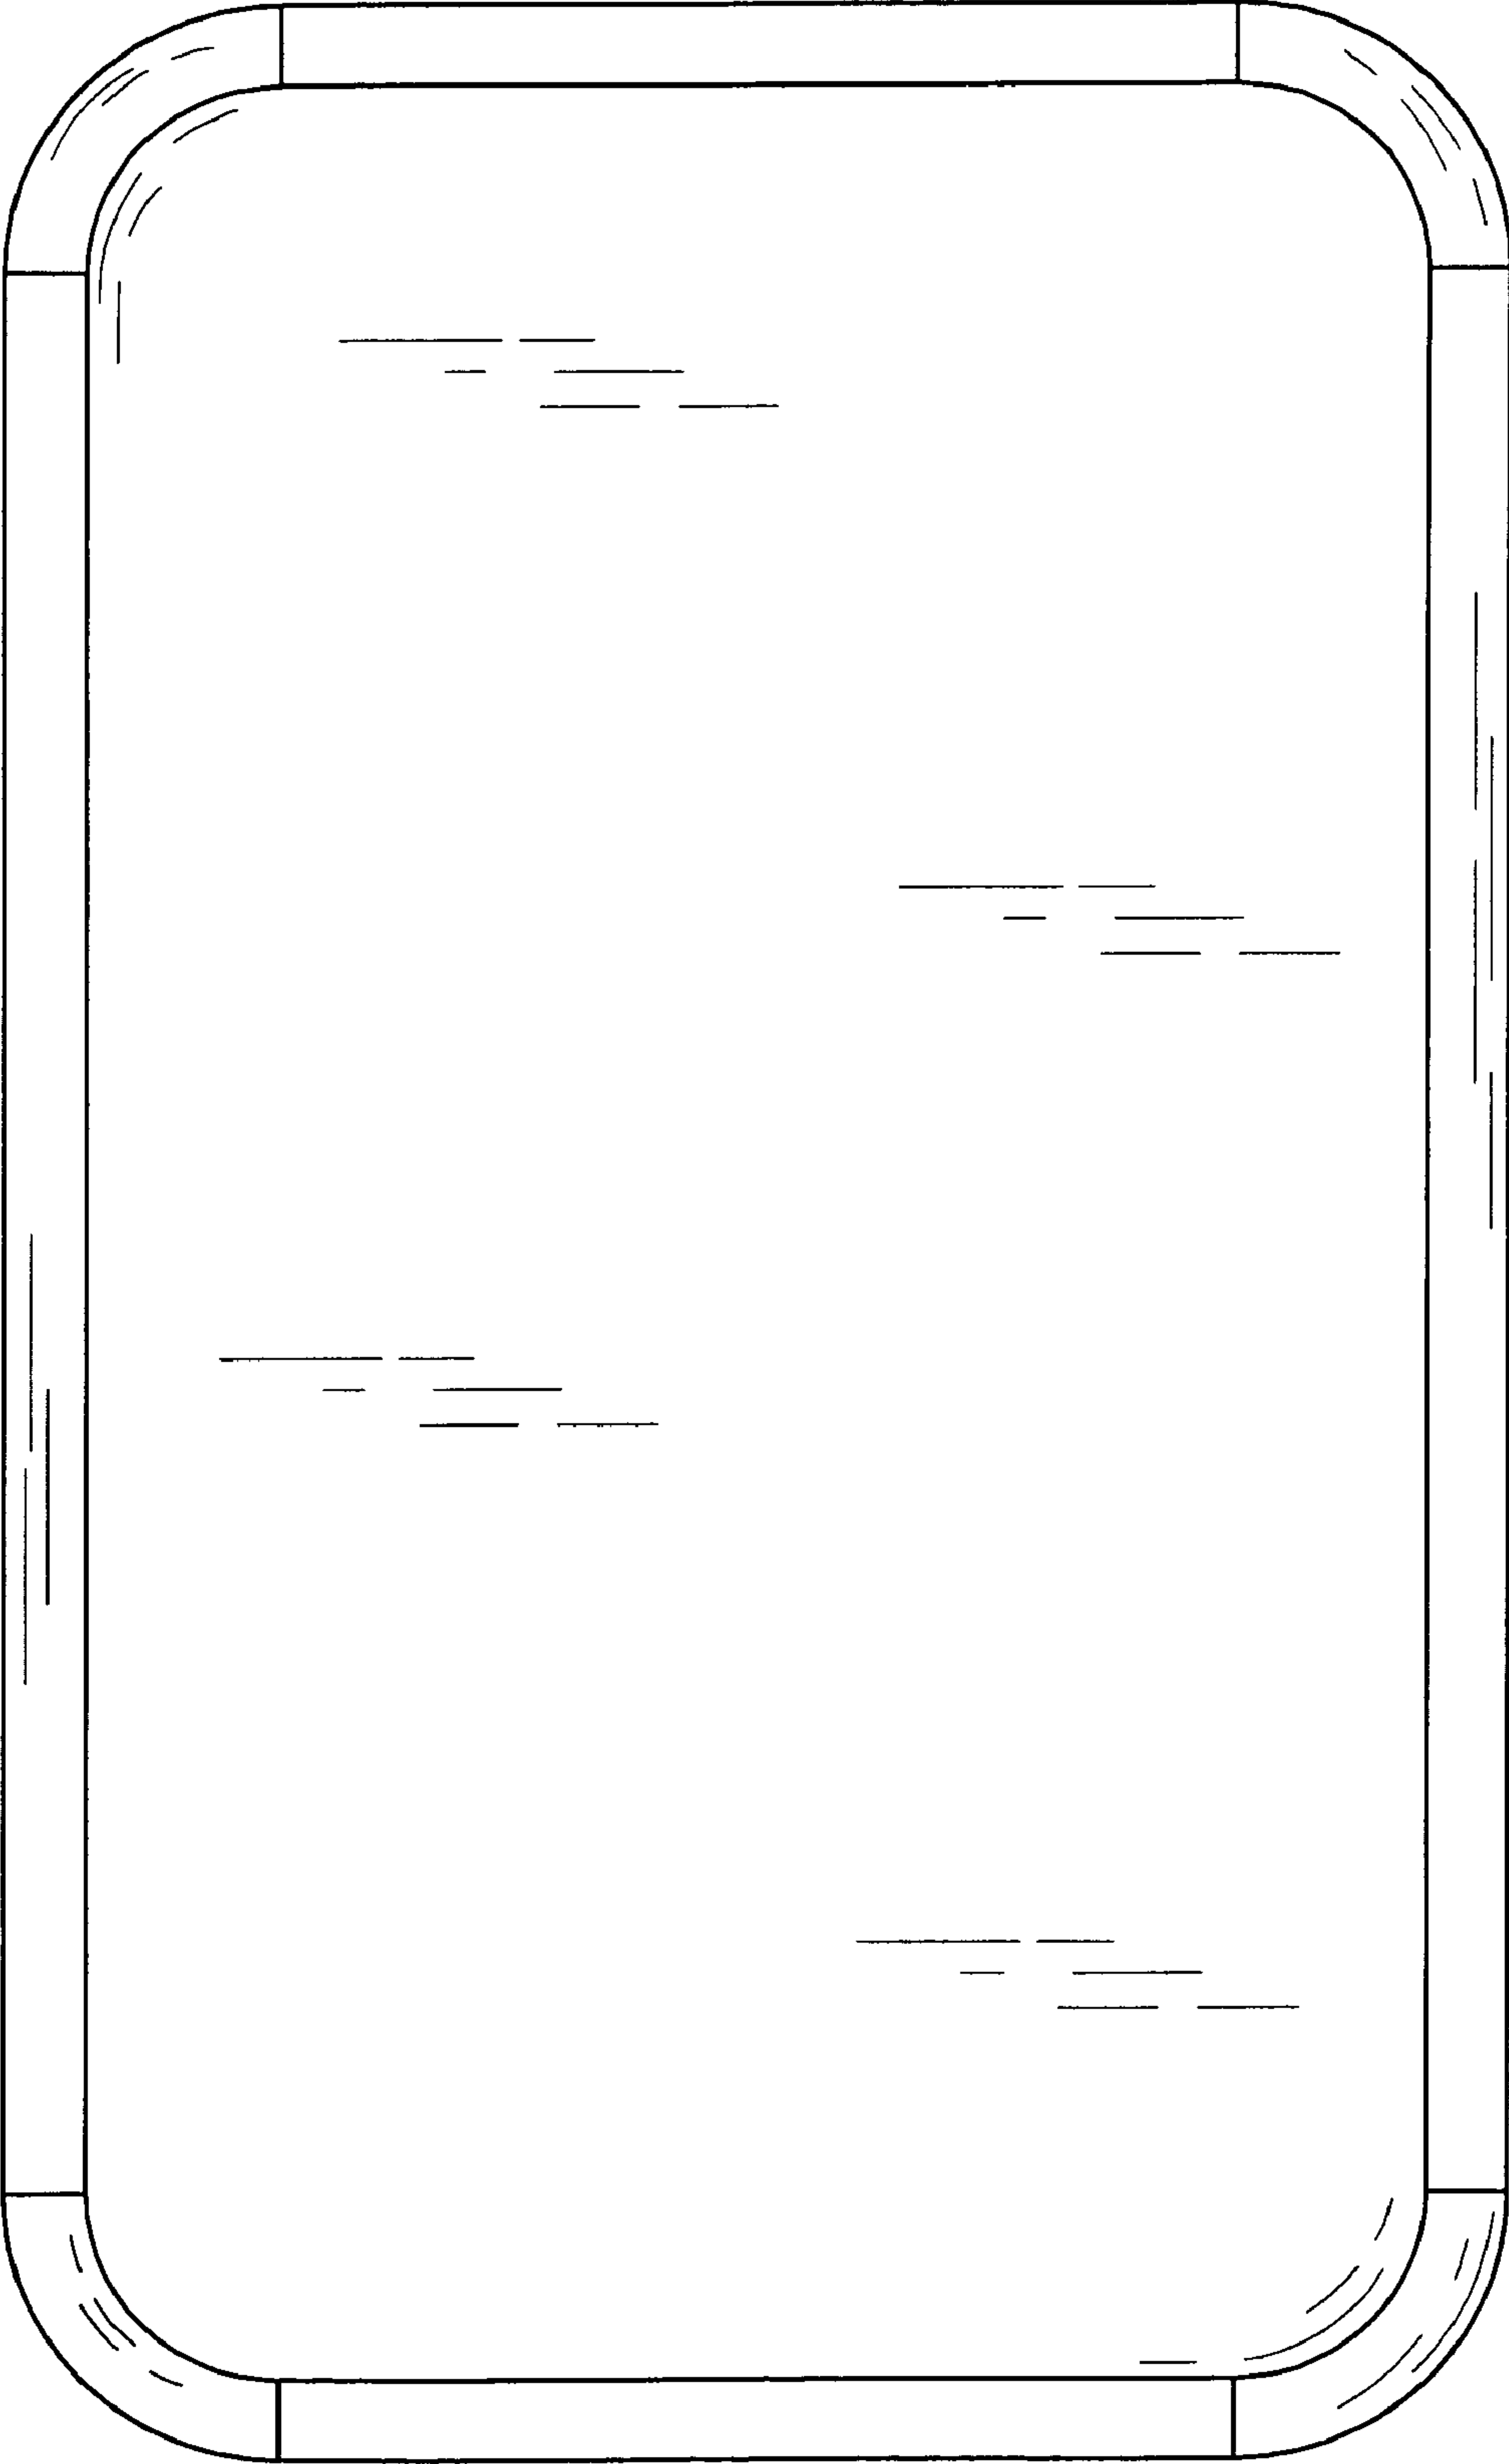


Fig. 6

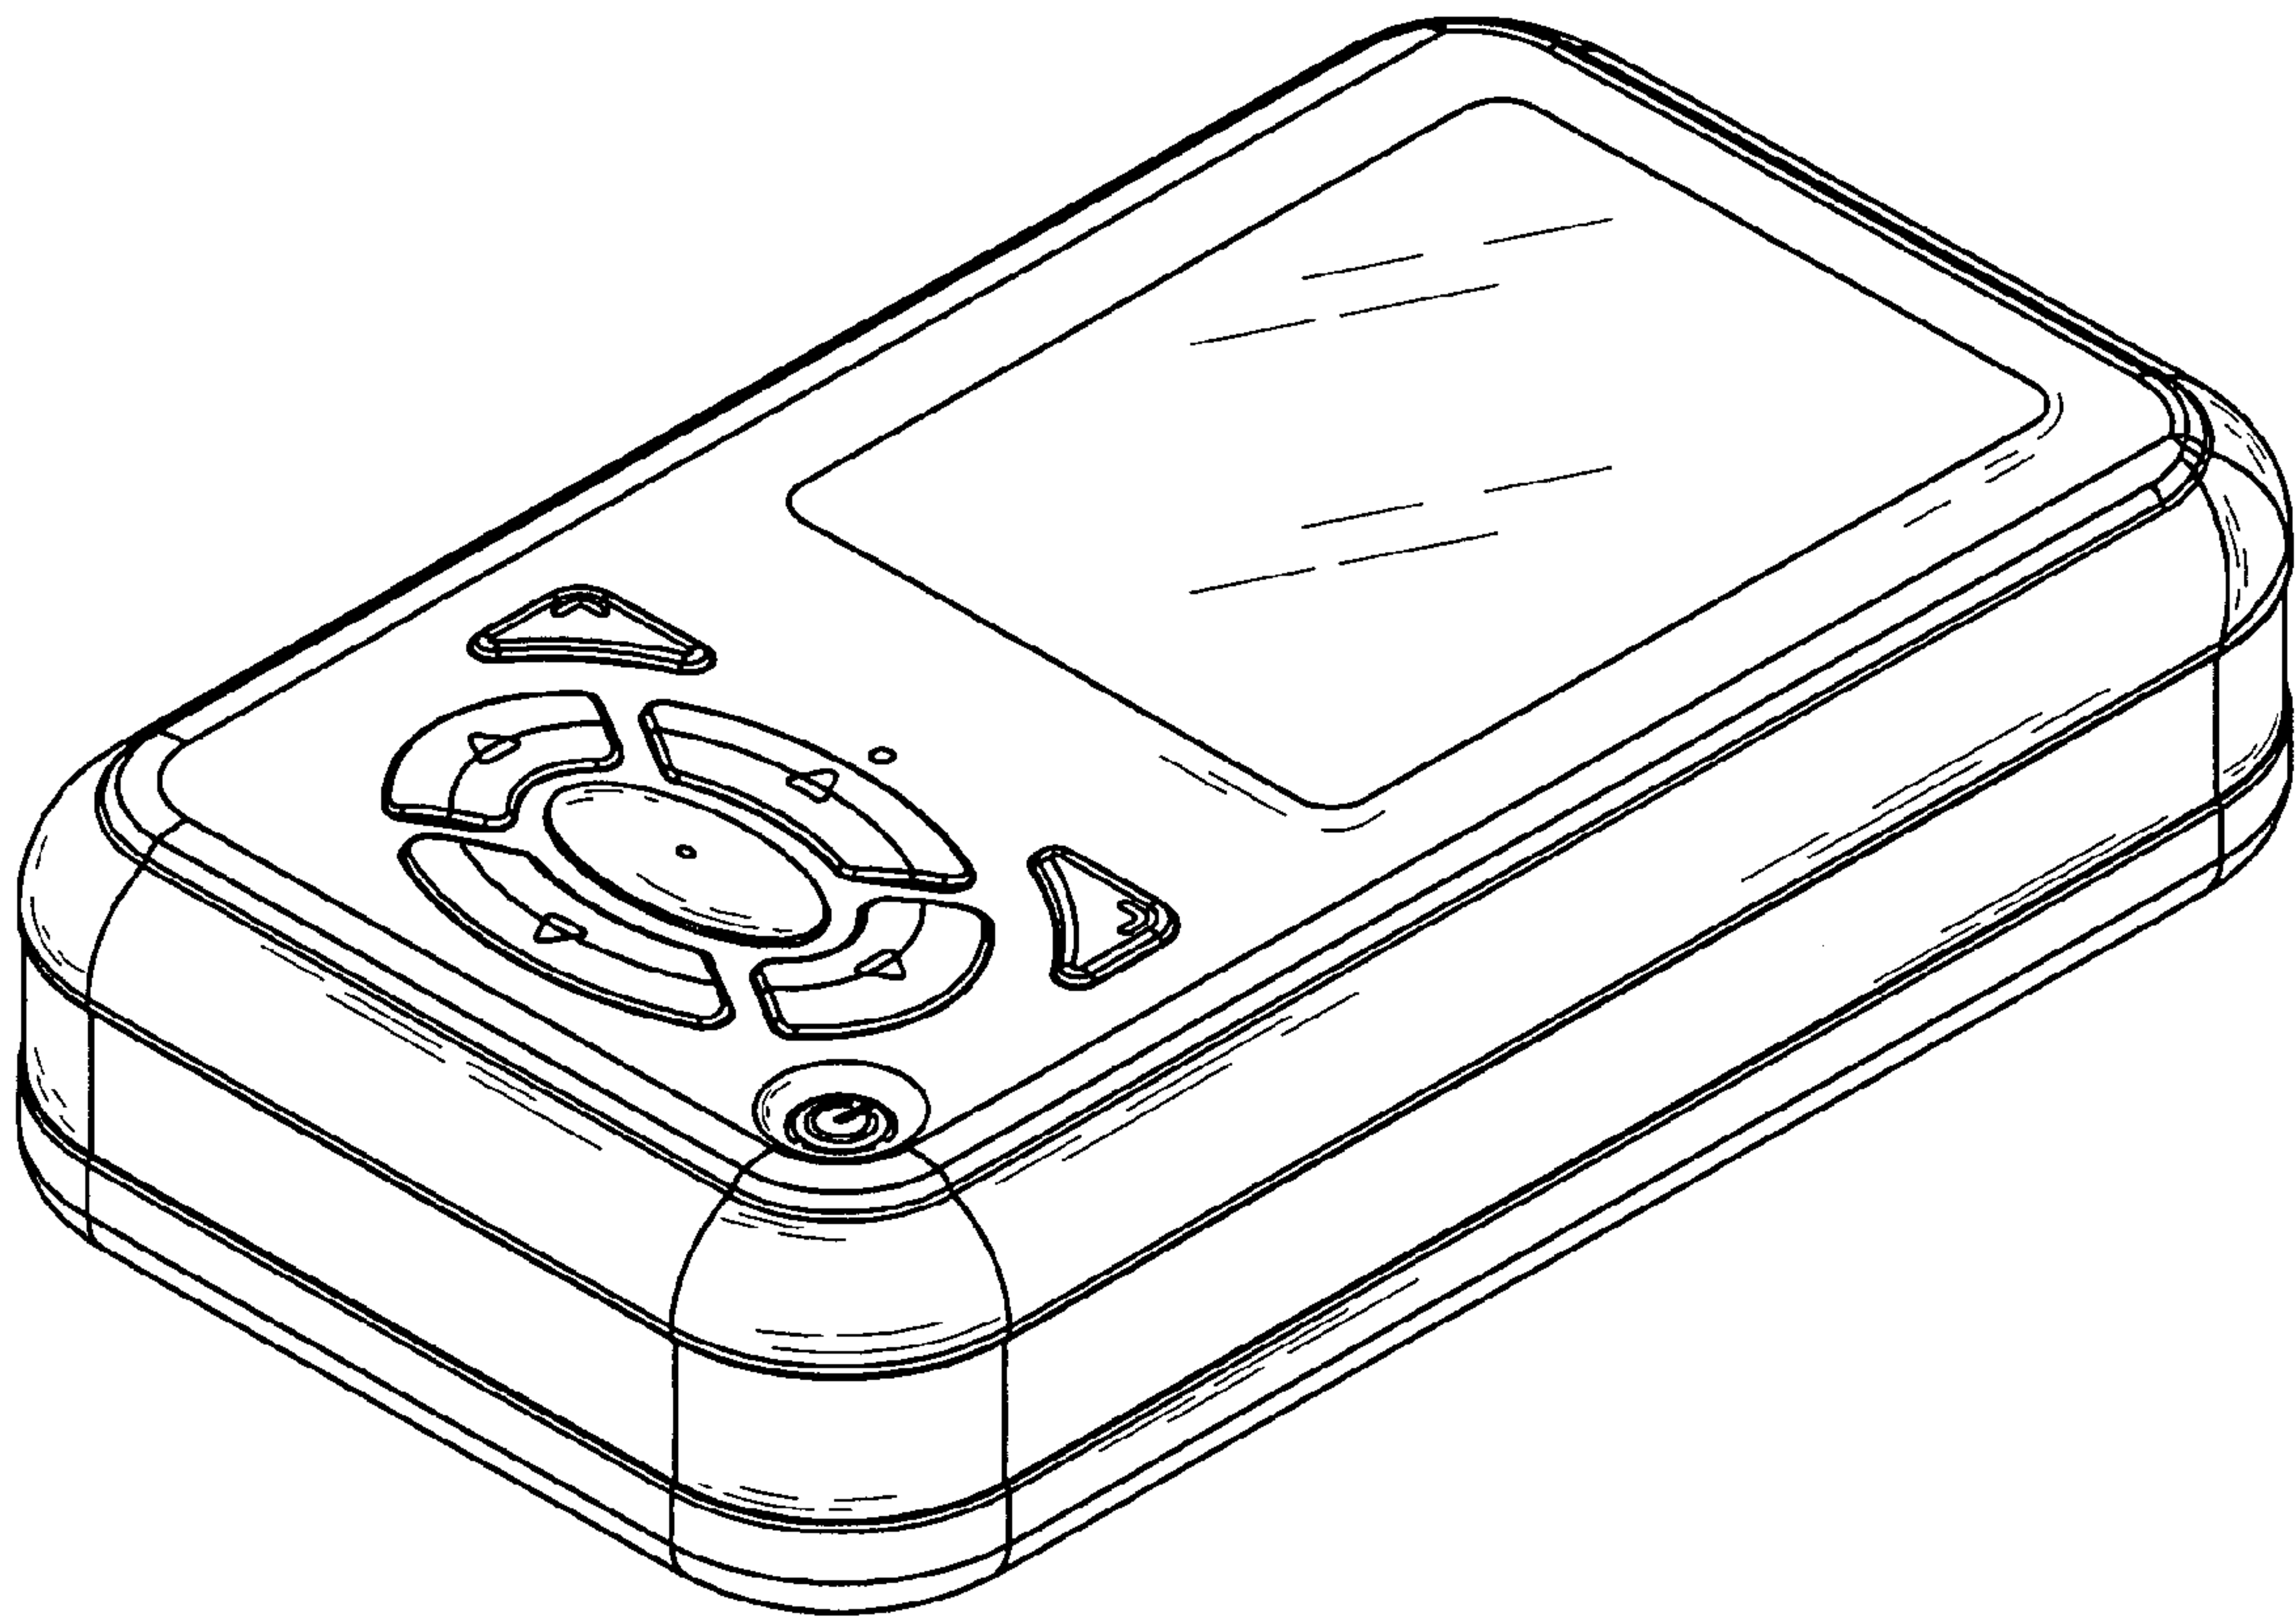


Fig. 7

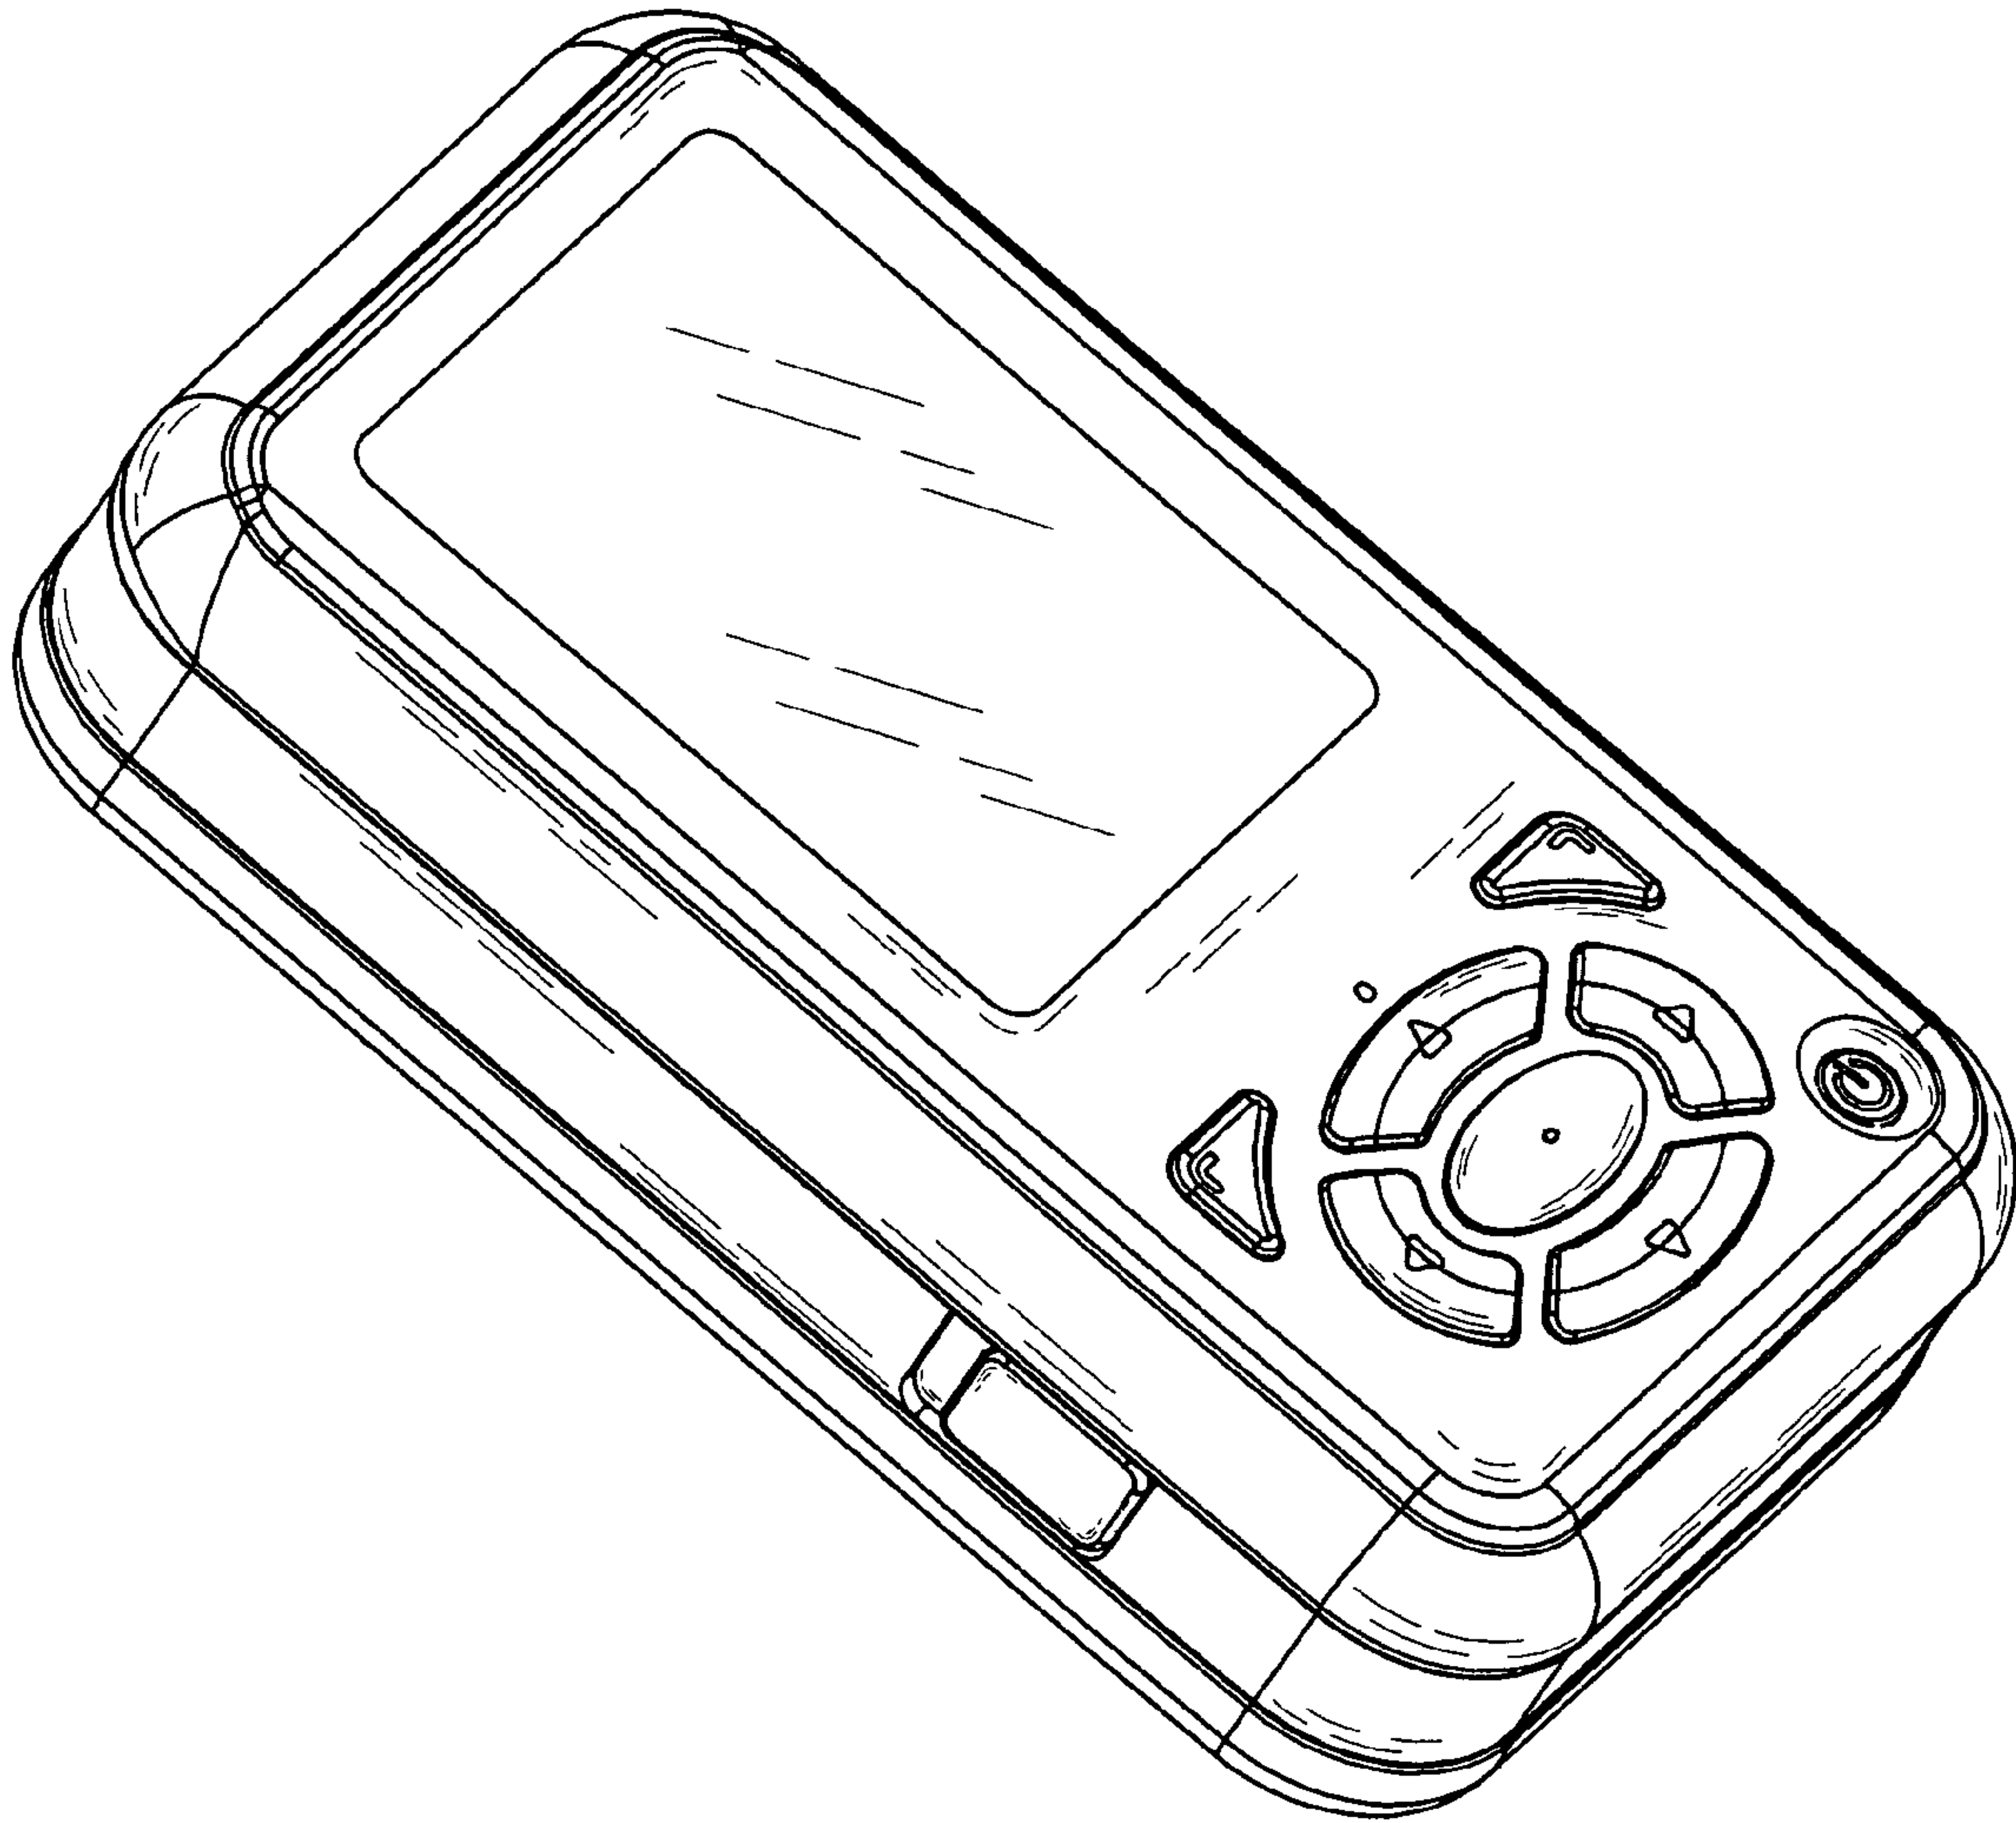


Fig. 8

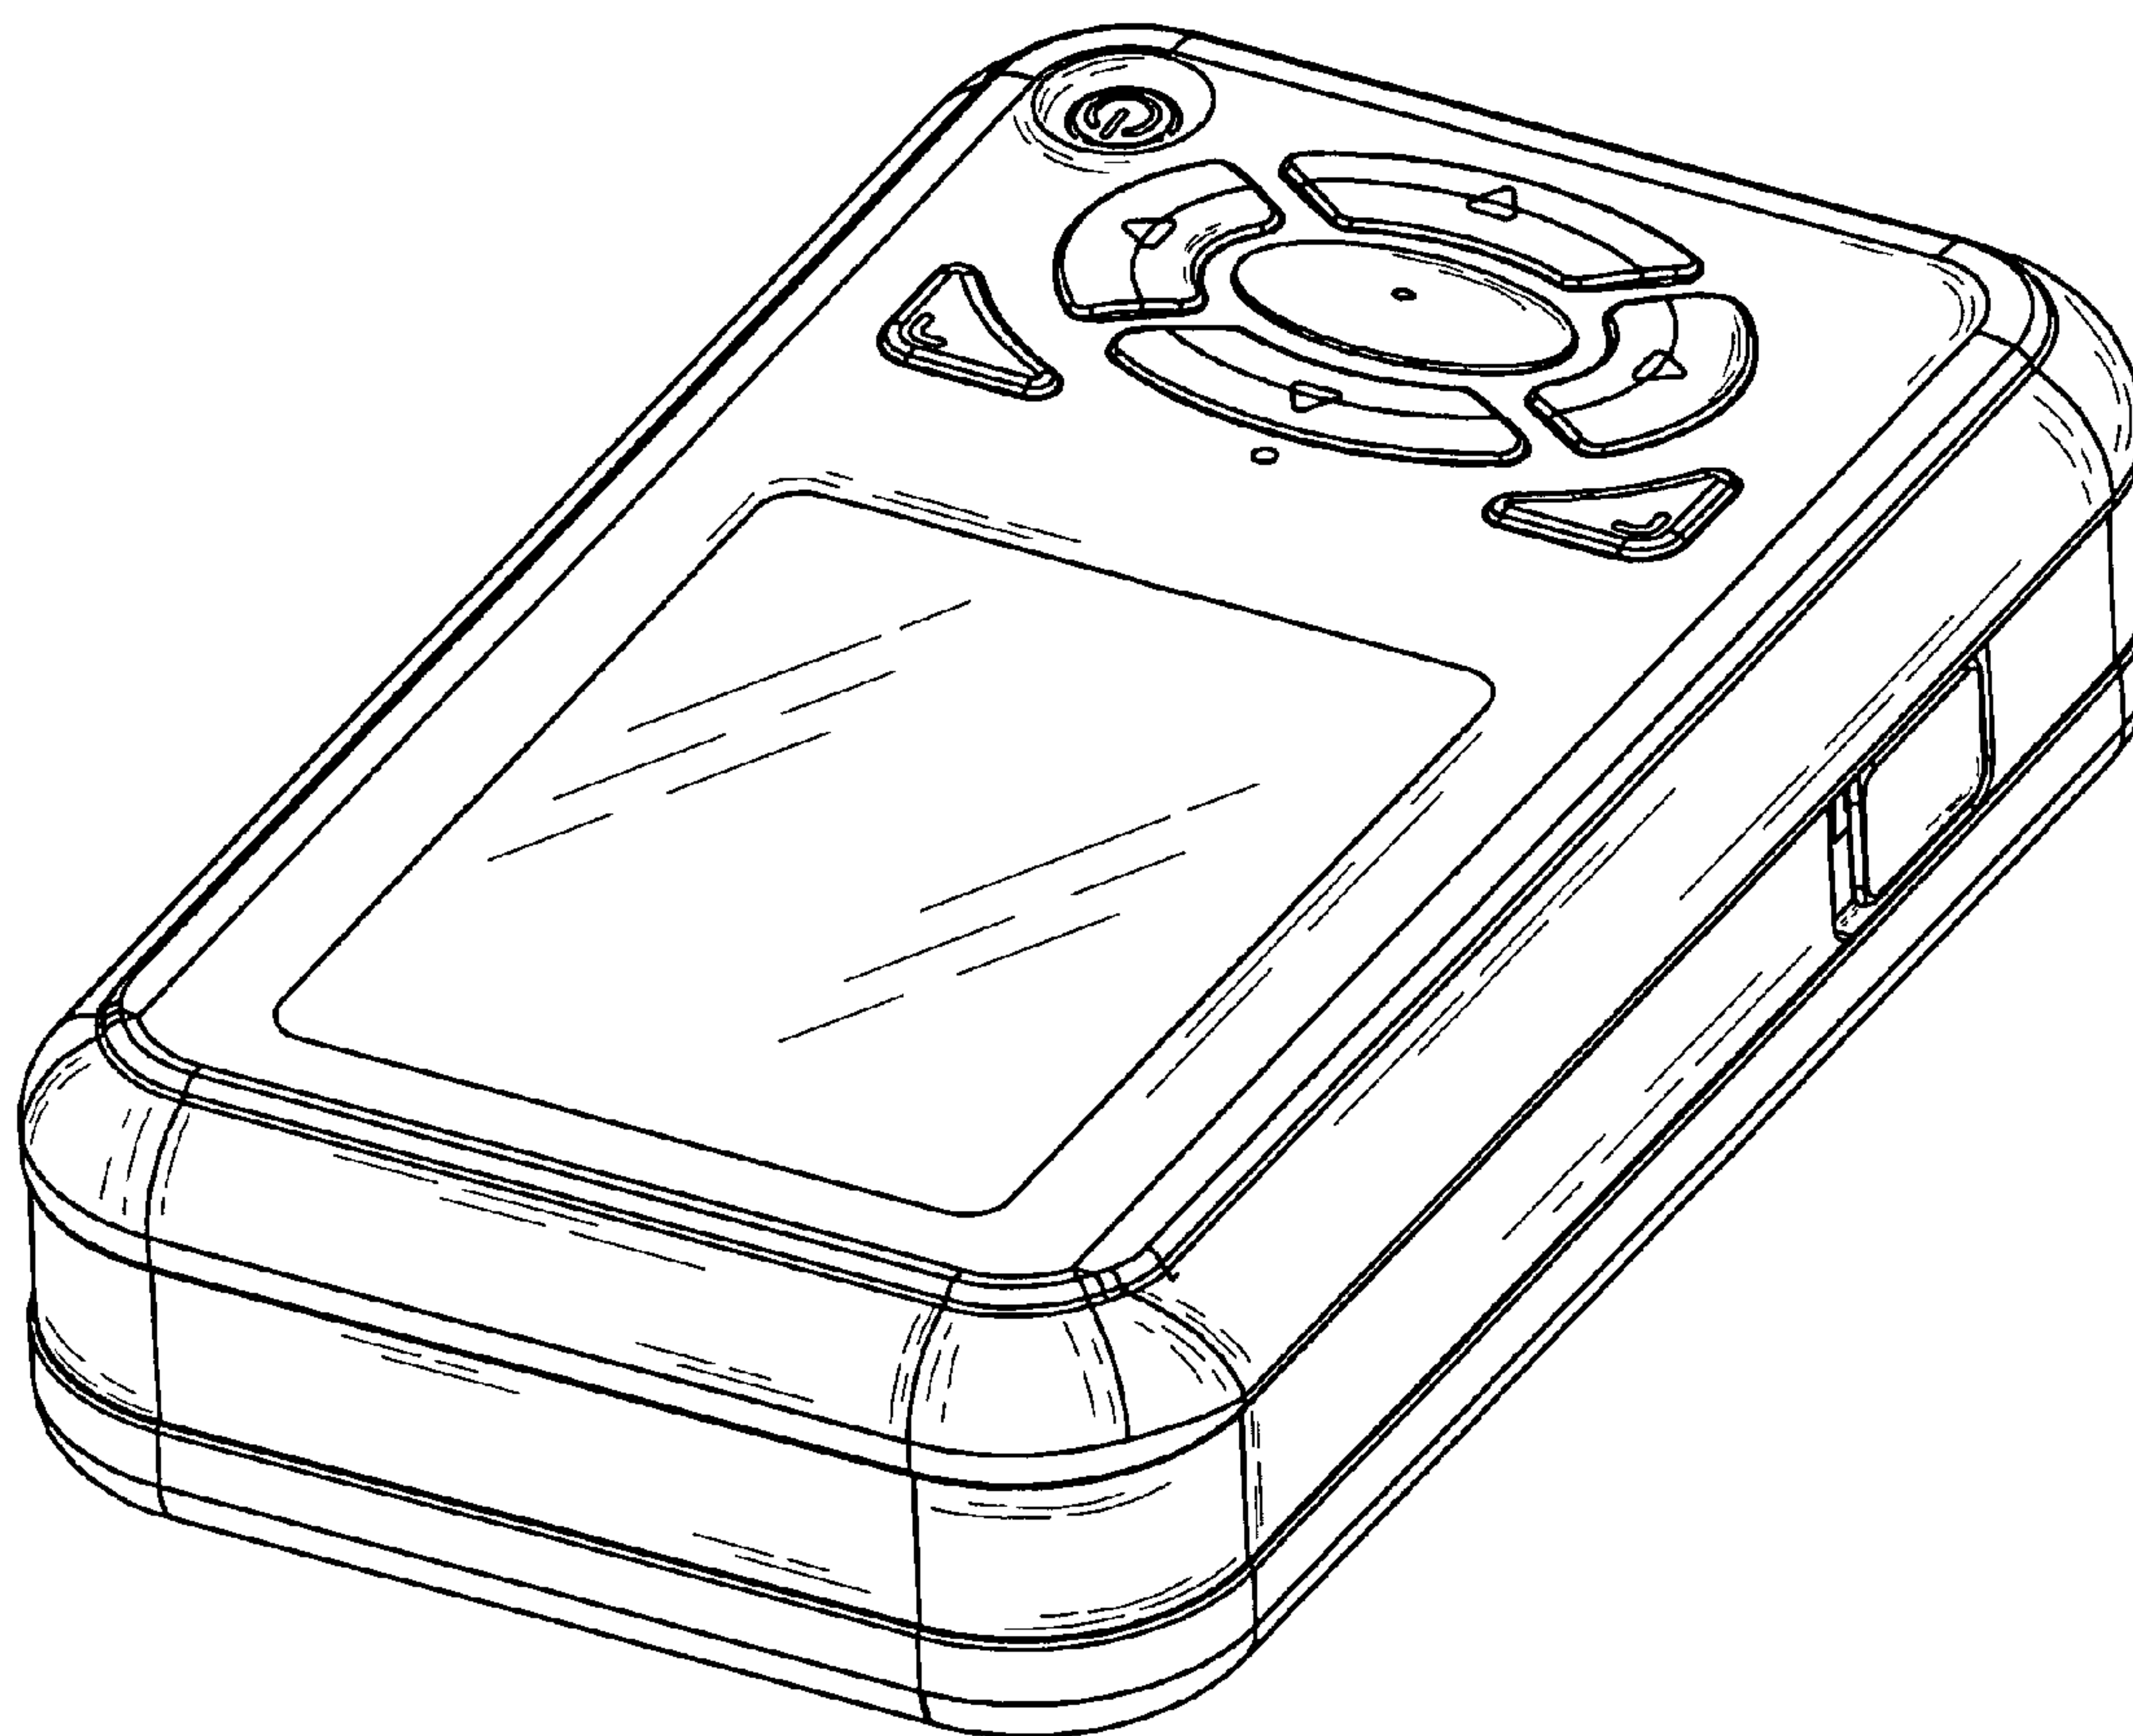


Fig. 9