



US00D616983S

(12) **United States Design Patent**  
**Kyvik et al.**

(10) **Patent No.:** **US D616,983 S**  
(45) **Date of Patent:** **\*\* Jun. 1, 2010**

(54) **CATHETER ANCHOR PAD WITH RELEASE LAYER**

(76) Inventors: **Kurt Kyvik**, 5350 SW. First La., Ocala, FL (US) 34474; **Scott Ryan**, 5350 SW. First La., Ocala, FL (US) 34474

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/316,039**

(22) Filed: **Aug. 18, 2009**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/128**

(58) **Field of Classification Search** ..... D24/127-130,  
D24/189; 604/179-180, 187, 227; 602/58-59;  
128/DIG. 26

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,693,032	A *	12/1997	Bierman	604/180
D492,411	S *	6/2004	Bierman	D24/128
D503,977	S *	4/2005	Bierman	D24/128
D528,206	S *	9/2006	Bierman	D24/128
D552,732	S *	10/2007	Bierman et al.	D24/128
7,563,251	B2 *	7/2009	Bierman et al.	604/174
D608,444	S *	1/2010	Kyvik et al.	D24/130
D608,887	S *	1/2010	Kyvik et al.	D24/130
2009/0137961	A1 *	5/2009	Bracken	604/177
2009/0187130	A1 *	7/2009	Asmus et al.	602/57
2010/0022962	A1 *	1/2010	Bierman et al.	604/180

\* cited by examiner

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Eric L Goodman

(74) *Attorney, Agent, or Firm*—Thomas C. Saitta

(57) **CLAIM**

The ornamental design for a catheter anchor pad with release layer, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the catheter anchor pad with release layer, shown in an open position.

FIG. 2 is a top view of the catheter anchor pad with release layer, shown in the closed position.

FIG. 3 is a bottom view of the catheter anchor pad with release layer, shown in the closed position.

FIG. 4 is a right side view of the catheter anchor pad with release layer, shown in the closed position.

FIG. 5 is a left side view of the catheter anchor pad with release layer, shown in the closed position.

FIG. 6 is a front view of the catheter anchor pad with release layer, shown in the closed position., the rear view being a mirror image.

FIG. 7 is a top view of the catheter anchor pad with the release layer removed, shown in the closed position.

FIG. 8 is a bottom view of the catheter anchor pad with release layer removed, shown in the closed position.


FIG. 9 is a right side view of the catheter anchor pad with release layer removed, shown in the closed position.


FIG. 10 is a left side view of the catheter anchor pad with release layer removed, shown in the closed position; and,

FIG. 11 is a front view of the catheter anchor pad with release layer removed, shown in the closed position, the rear view being a mirror image.


The broken line showing in FIGS. 1 and 2 represents perforation lines and forms a part of the claimed design.

**1 Claim, 5 Drawing Sheets**

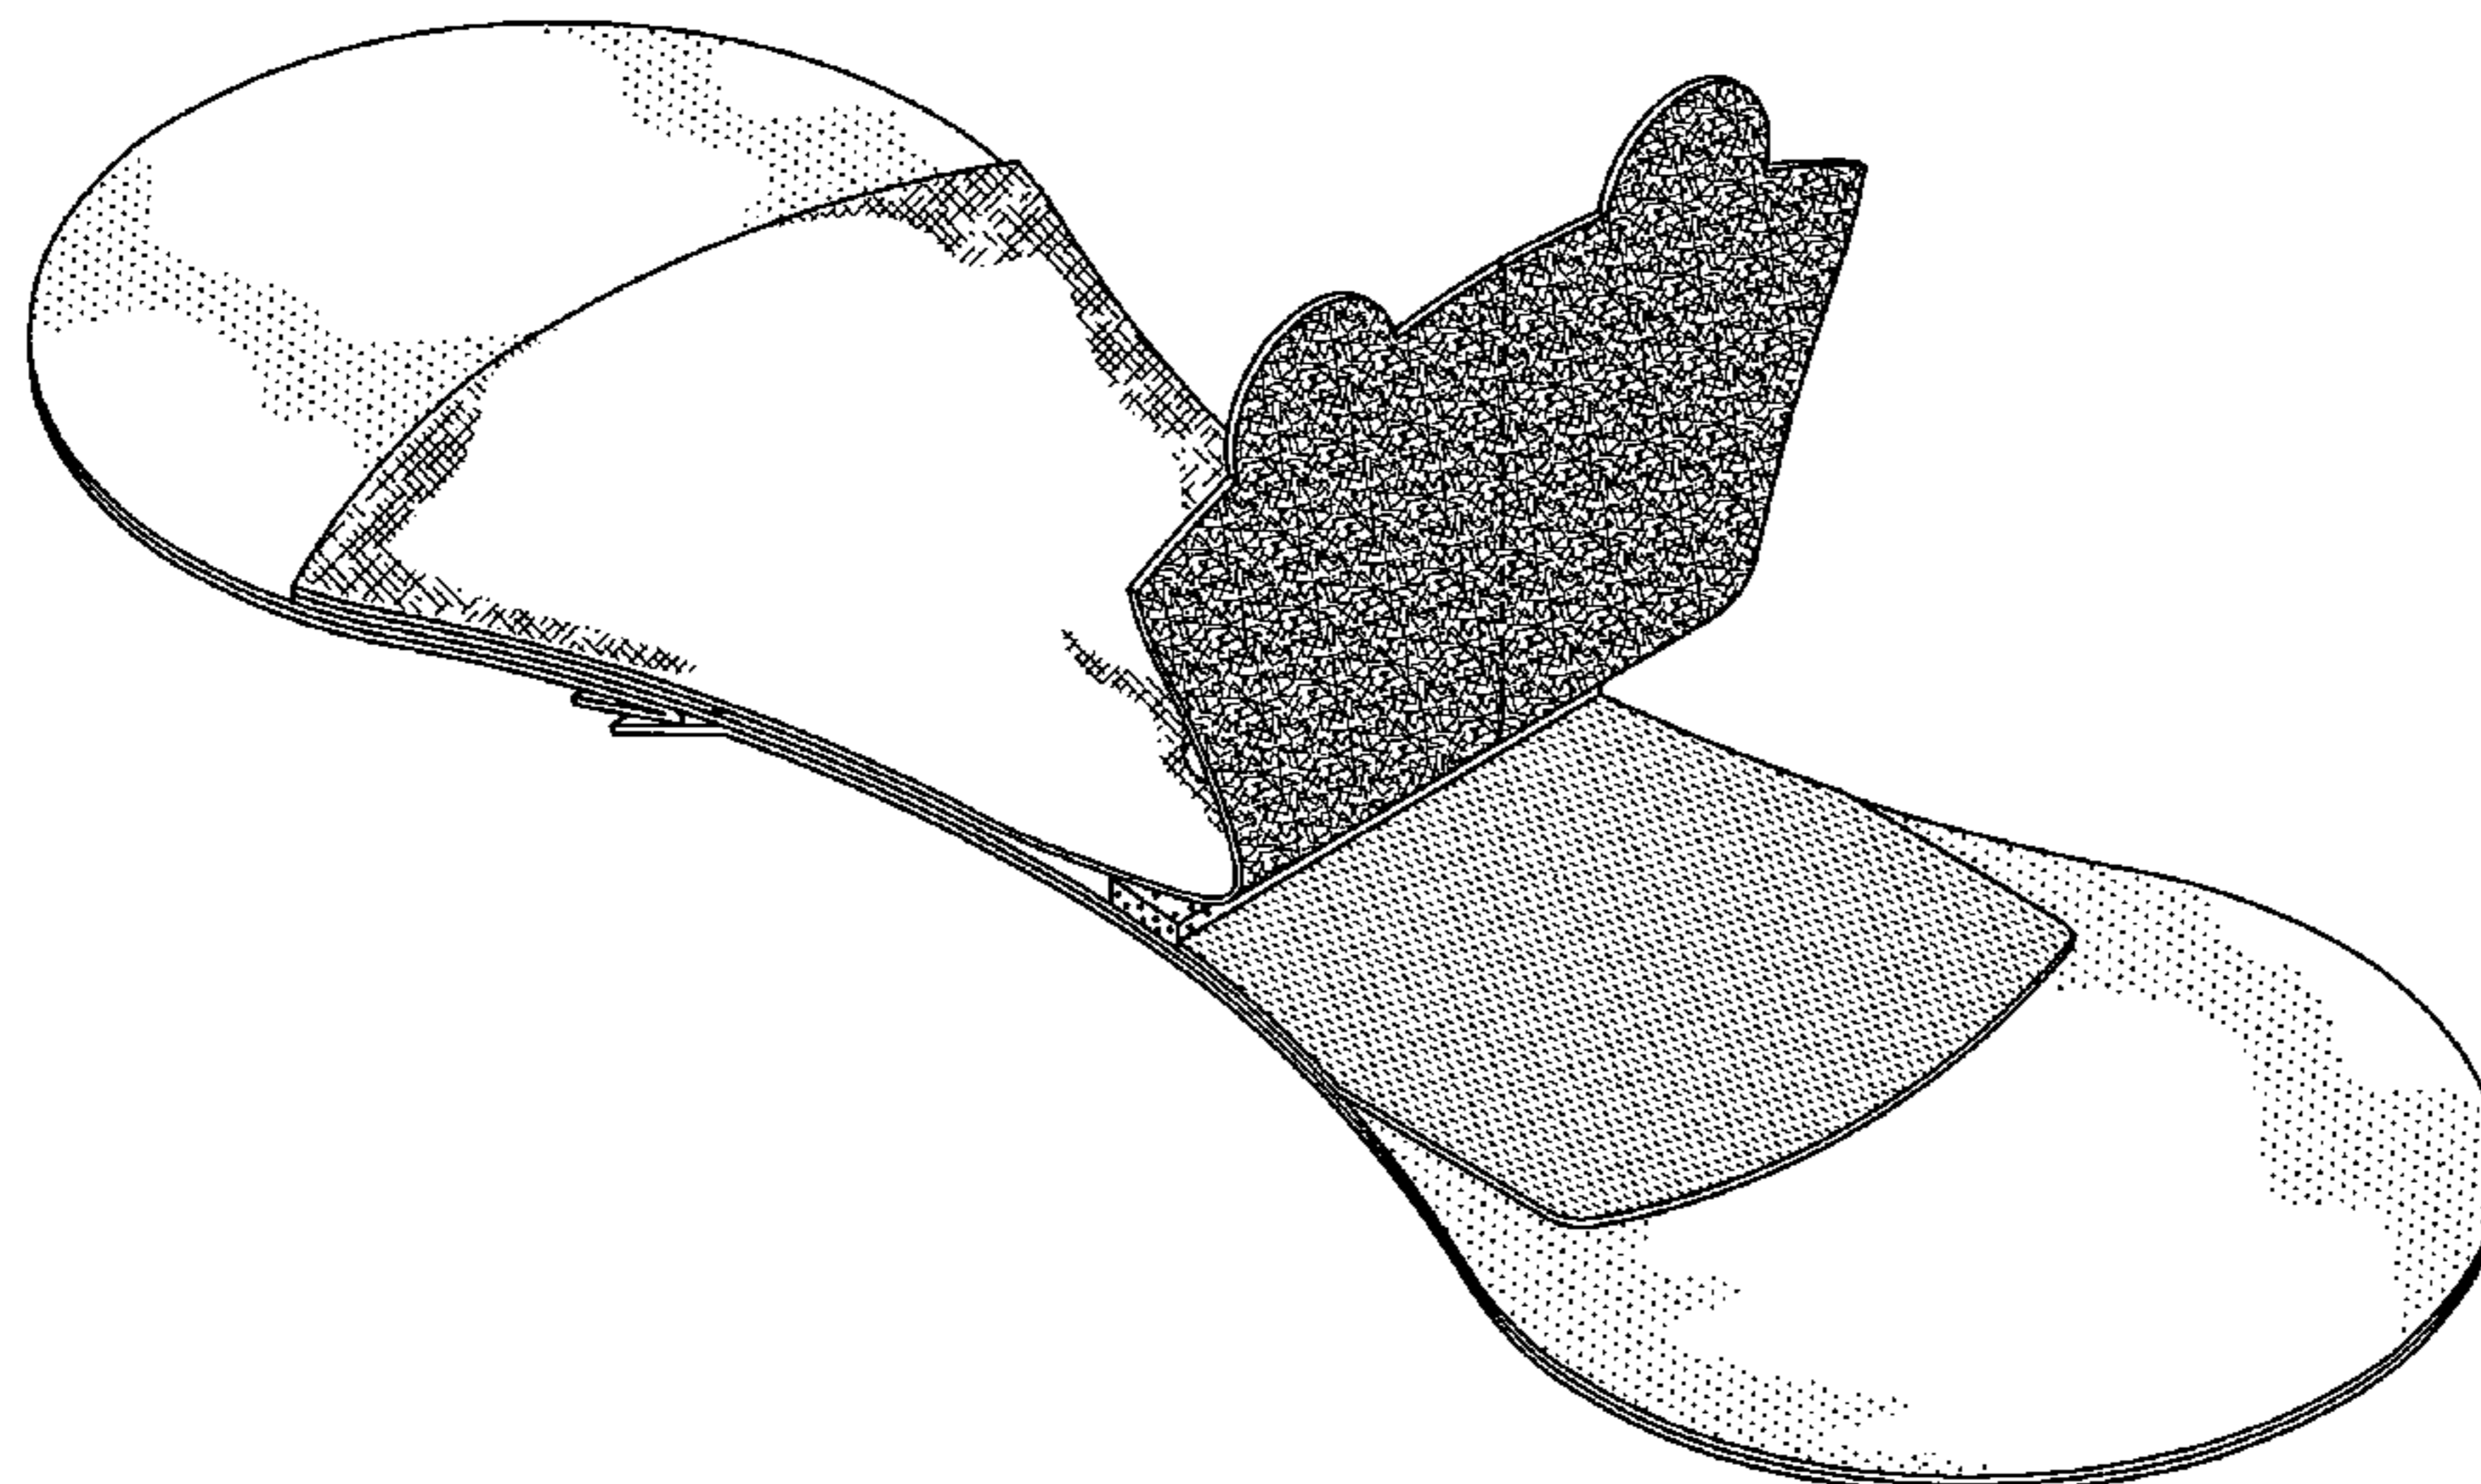


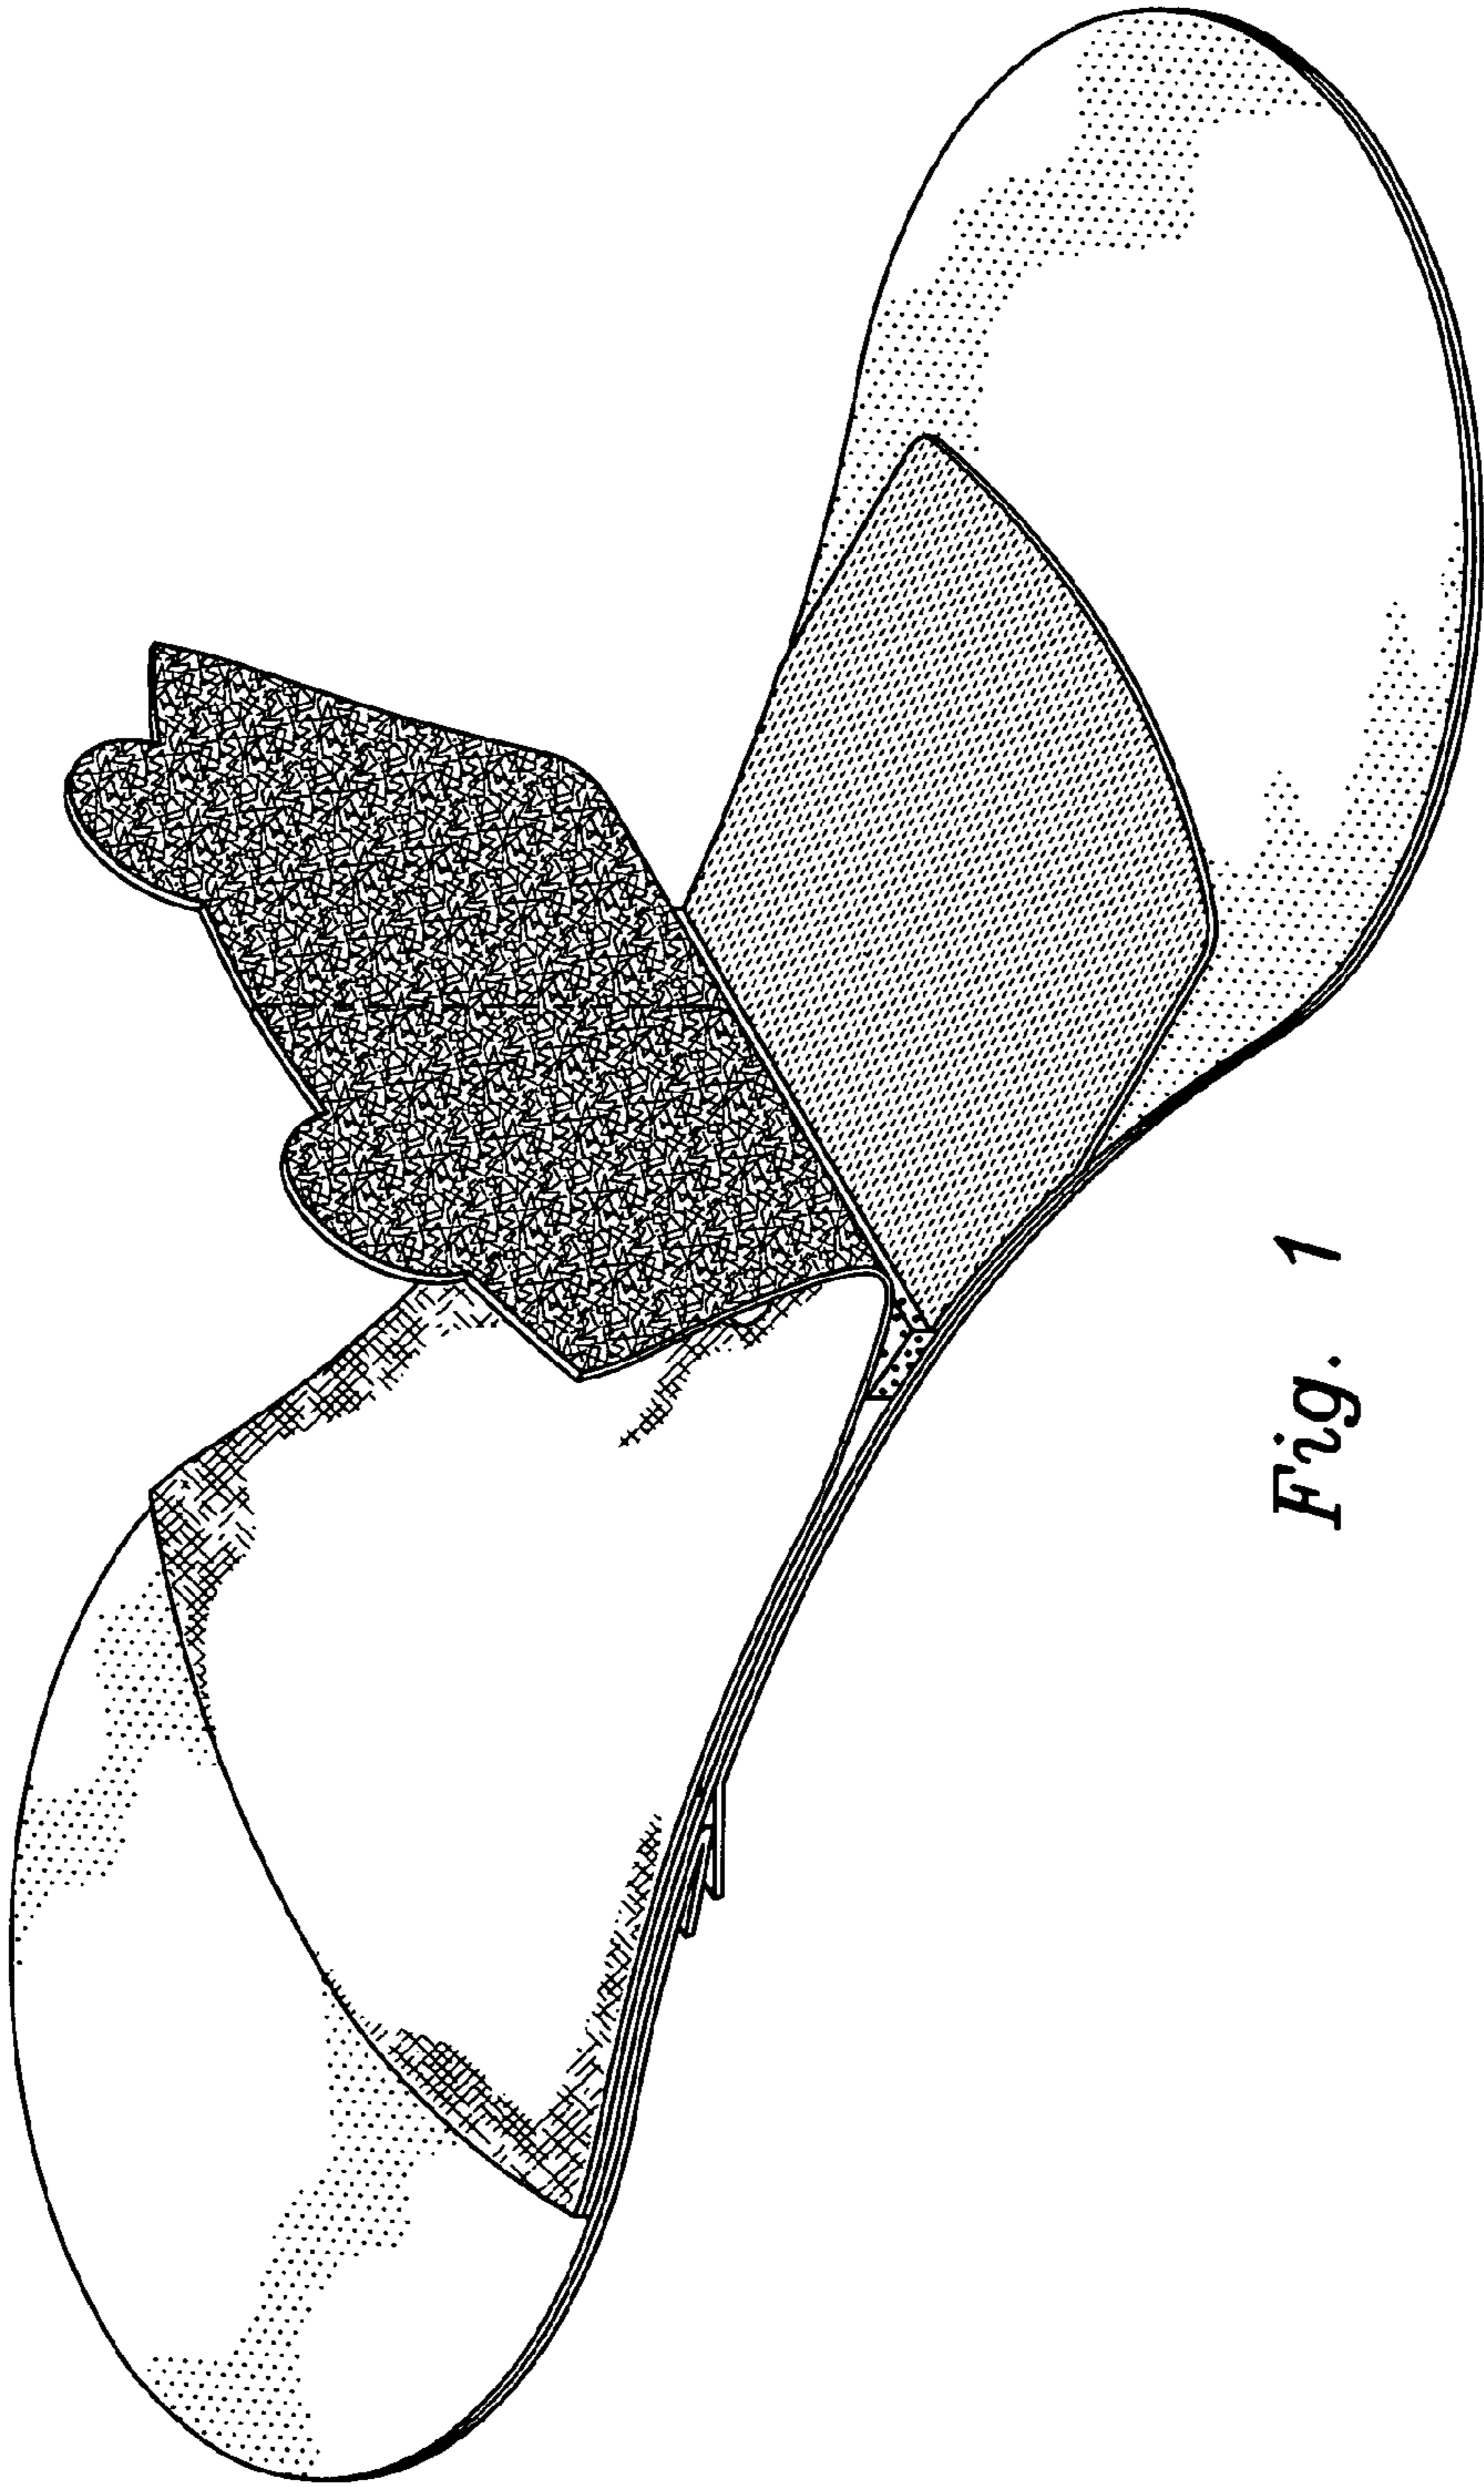

*Fig. 1*

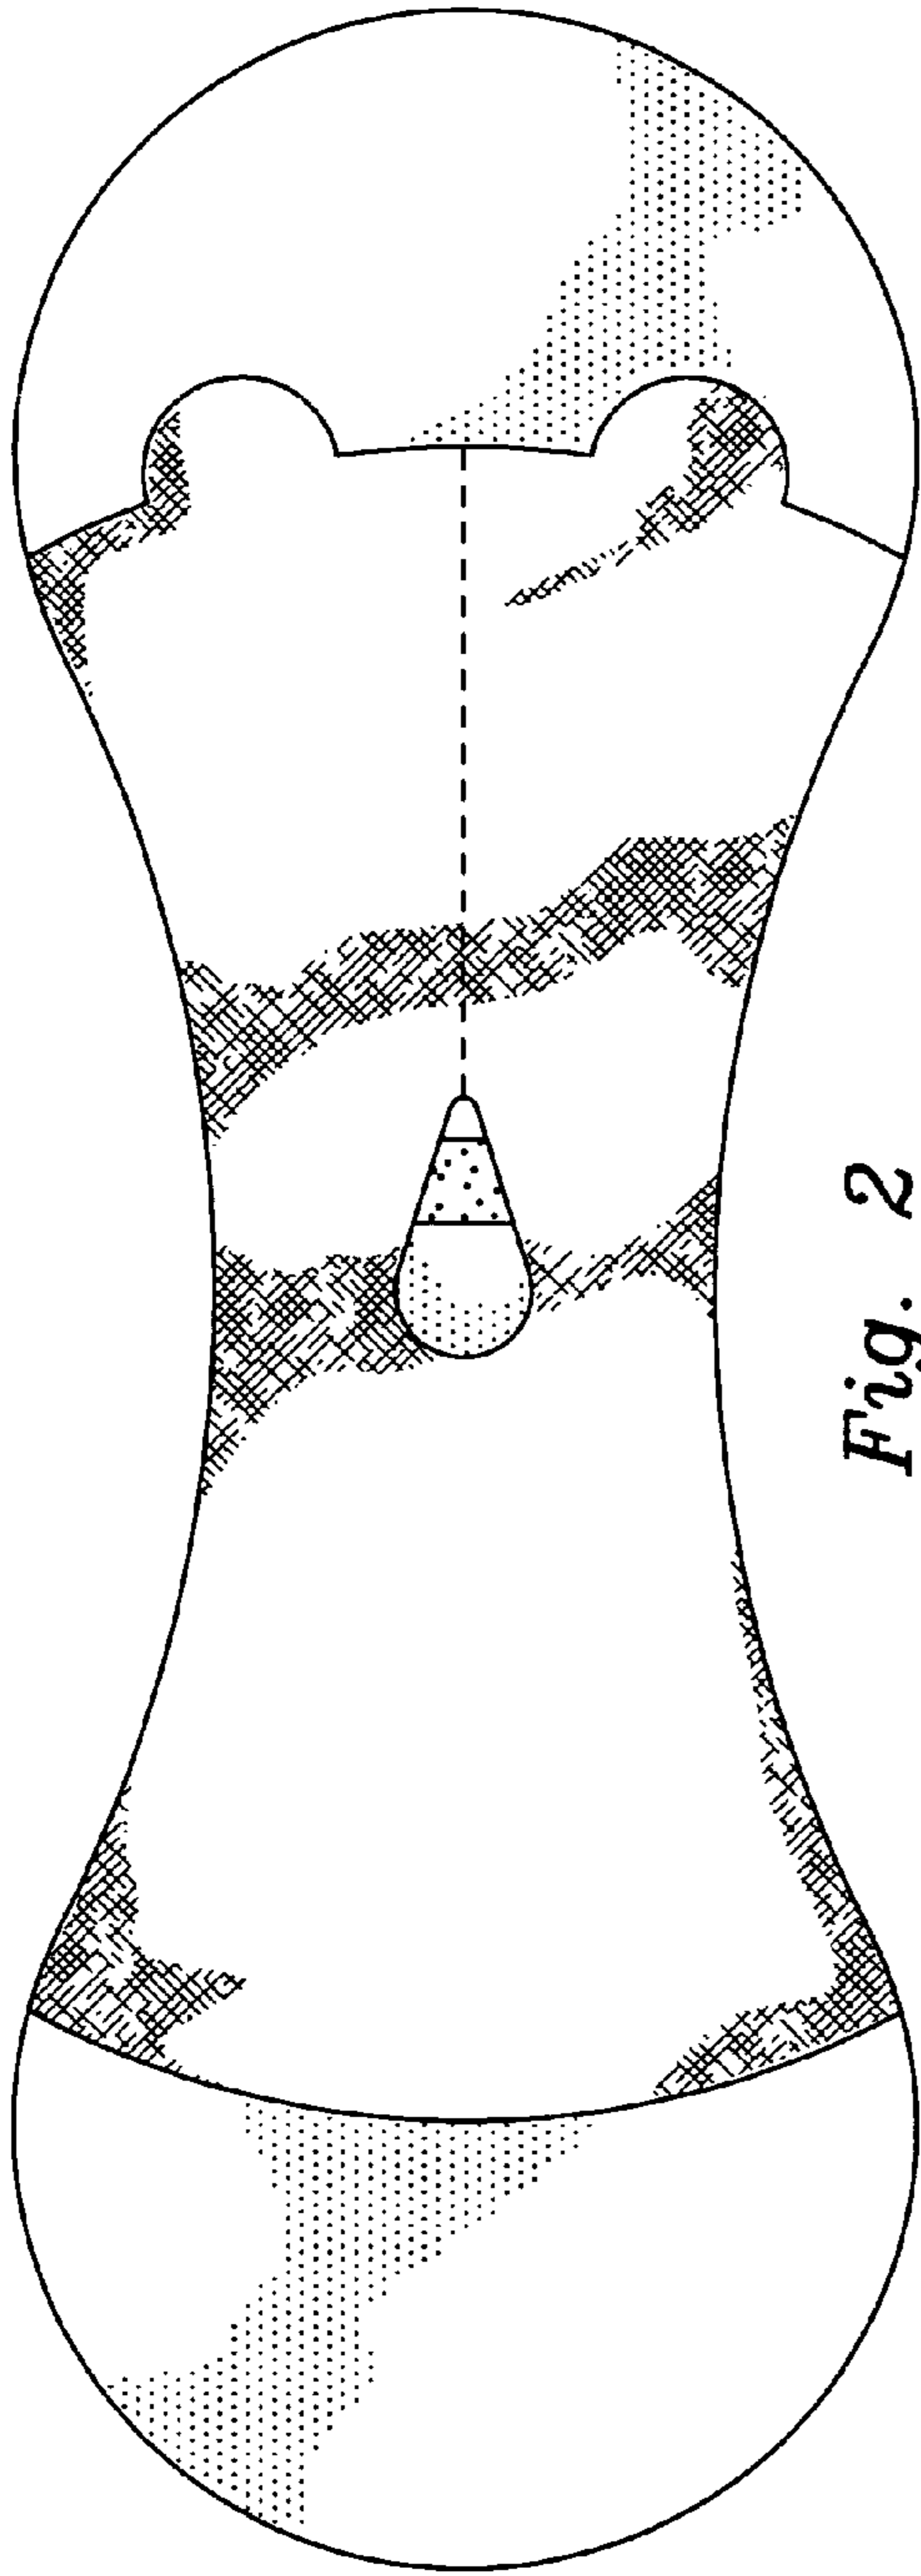

*Fig. 2*

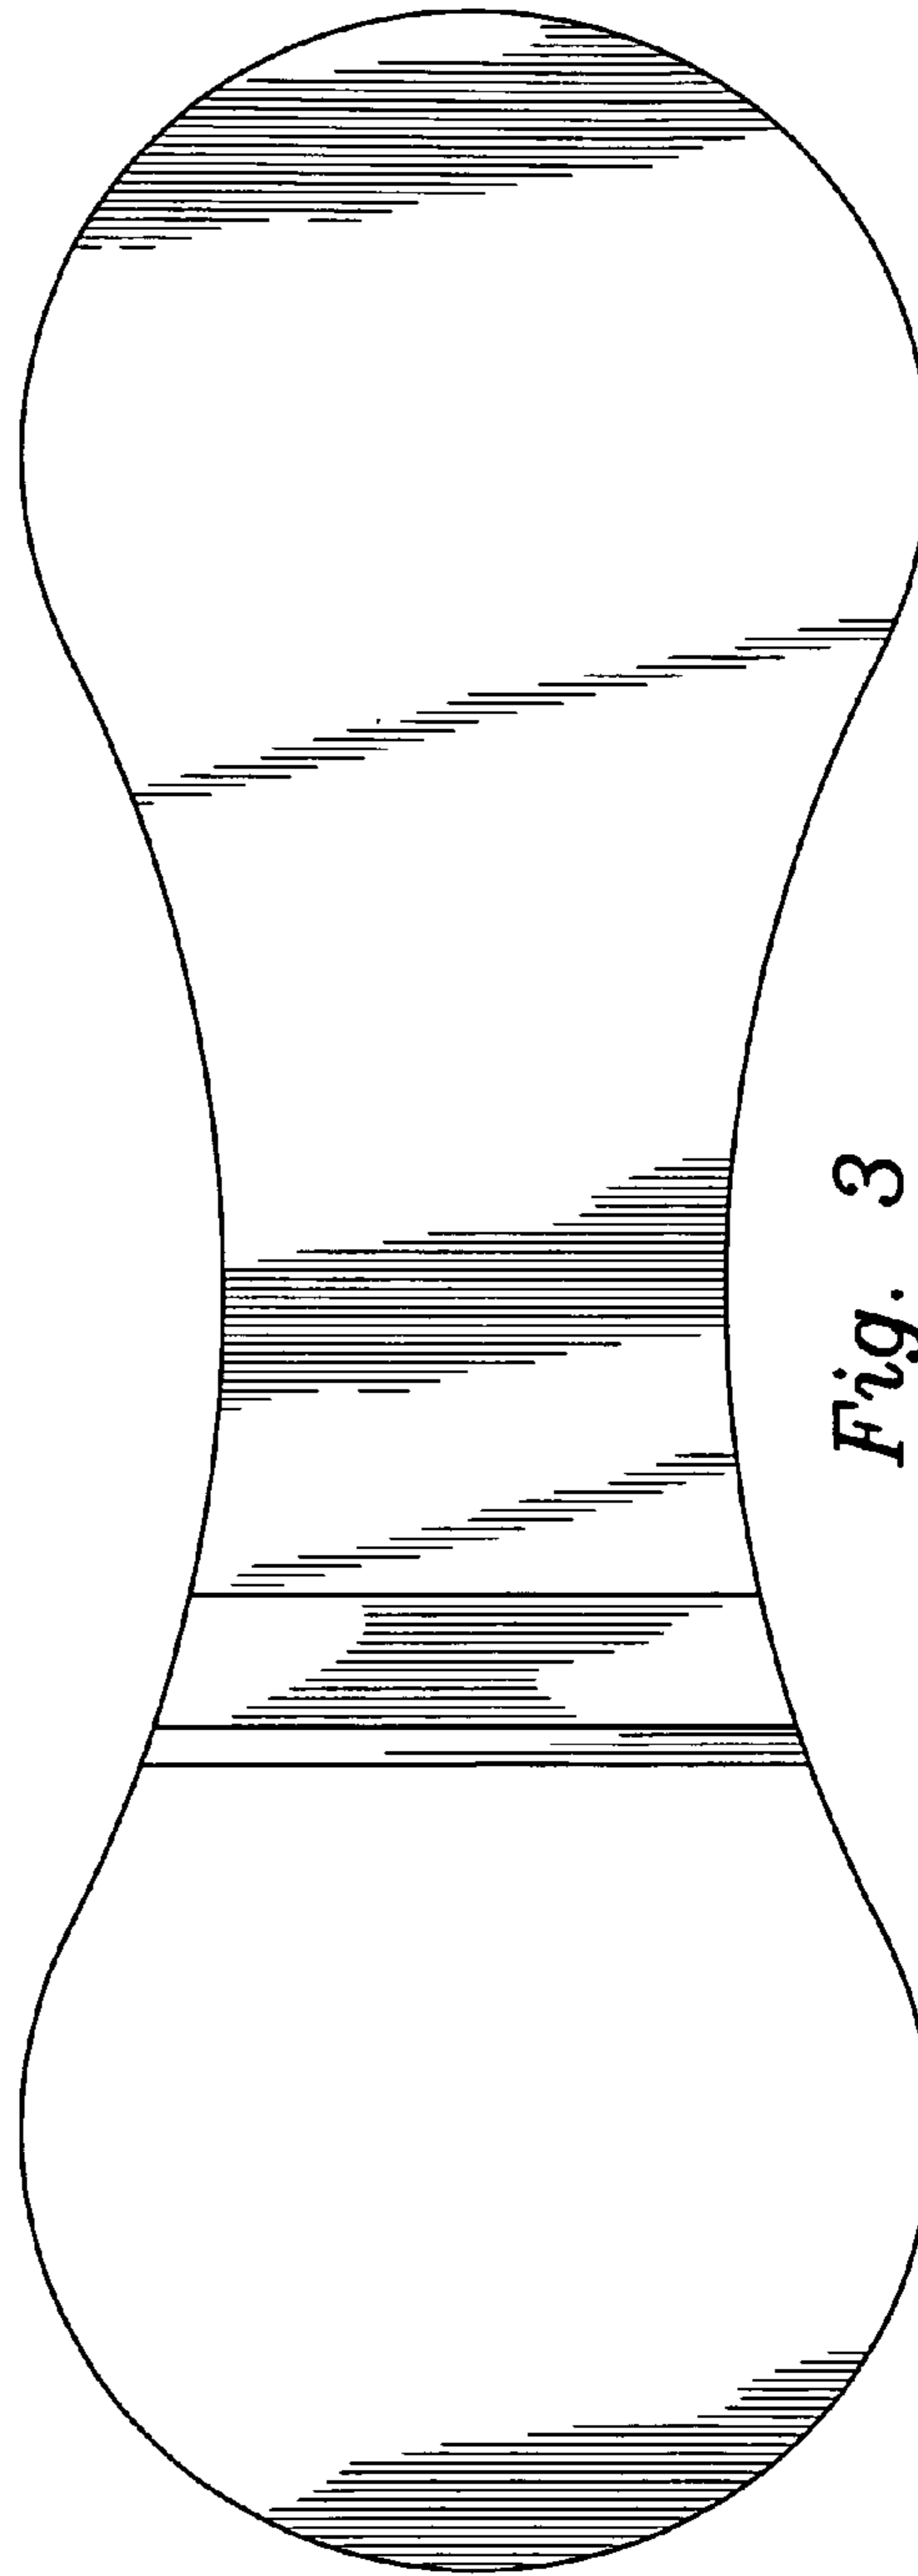


*Fig. 3*




*Fig. 4*




*Fig. 5*

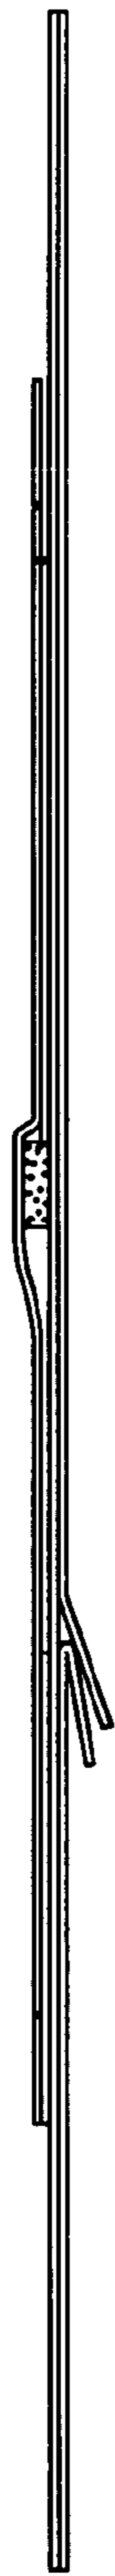

*Fig. 6*

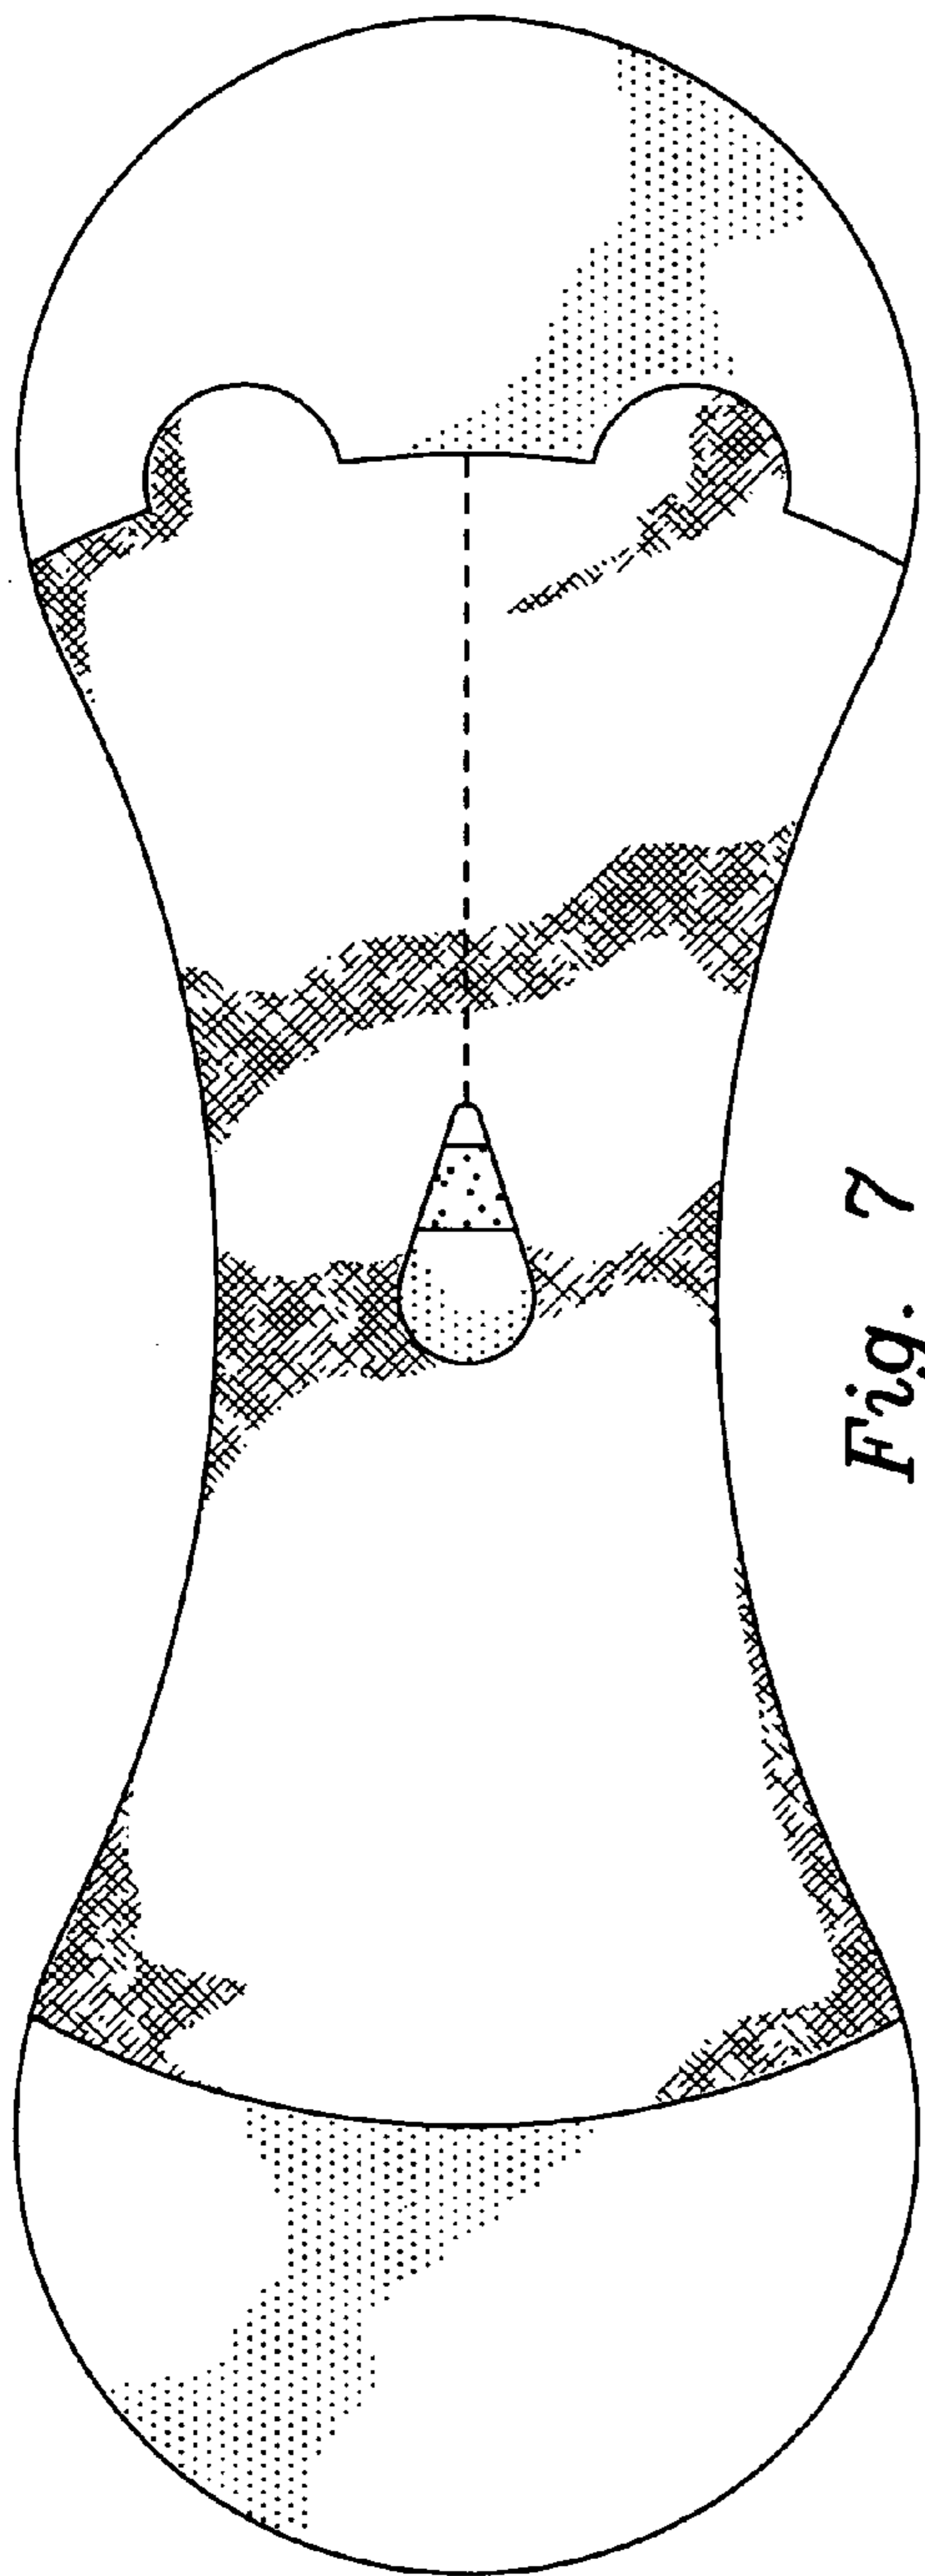

*Fig. 7*

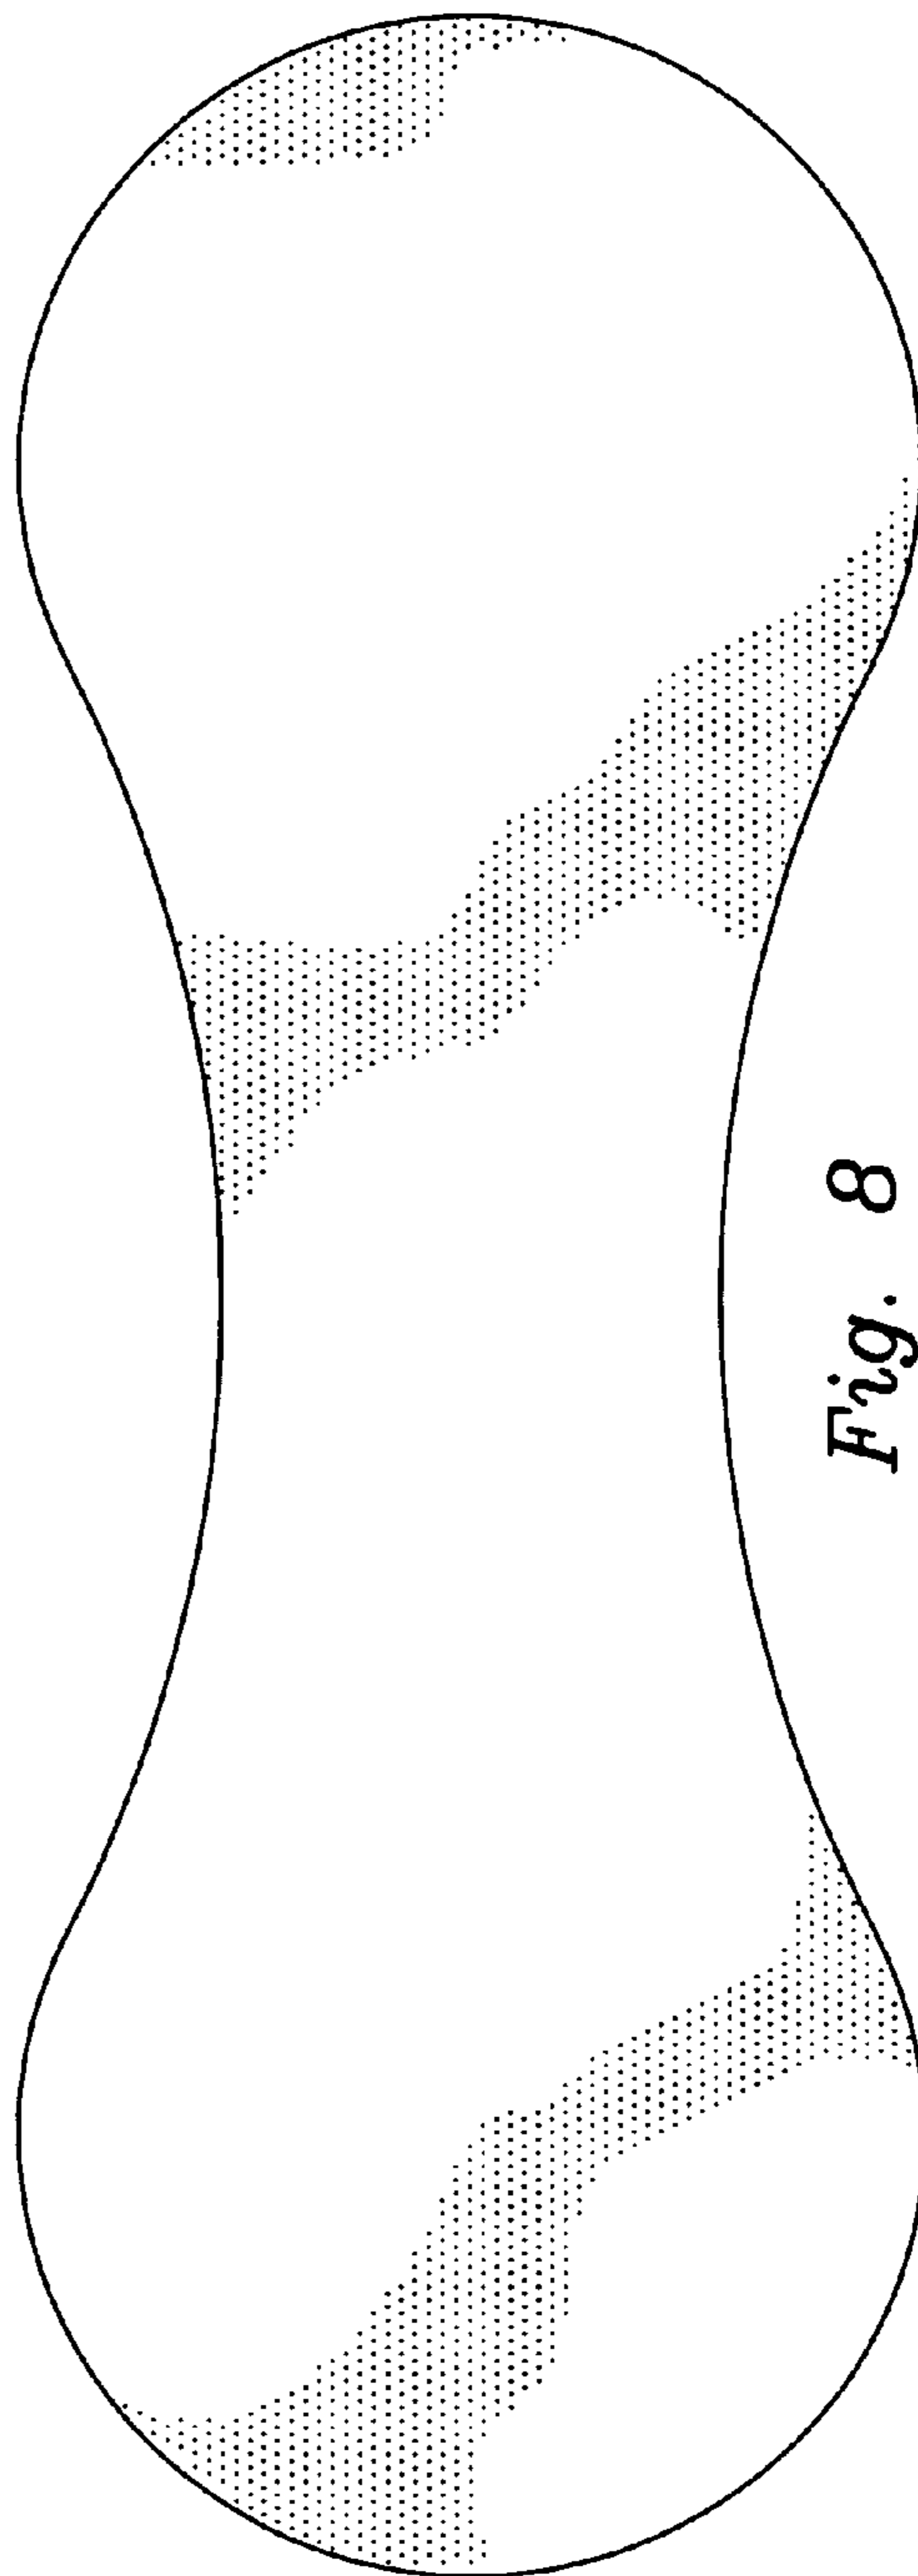

*Fig. 8*



*Fig. 9*



*Fig. 10*



*Fig. 11*