



US00D616990S

(12) **United States Design Patent**
Suzuki

(10) **Patent No.:** **US D616,990 S**
(45) **Date of Patent:** **** Jun. 1, 2010**

(54) **PROBE FOR AN ULTRASONIC DIAGNOSIS APPARATUS**

D545,433 S * 6/2007 Messerly et al. D24/158
D546,460 S * 7/2007 Hasegawa D24/186
D589,515 S * 3/2009 Brunner et al. D14/412
D596,300 S * 7/2009 Han et al. D24/186

(75) Inventor: **Shogo Suzuki**, Kawasaki (JP)

FOREIGN PATENT DOCUMENTS

(73) Assignees: **Kabushiki Kaisha Toshiba** (JP);
Toshiba Medical Systems Corporation
(JP)

JP 857709 1/1993
JP 892760 3/1994
JP 1267931 4/2006

(**) Term: **14 Years**

* cited by examiner

(21) Appl. No.: **29/279,803**

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(22) Filed: **May 8, 2007**

(74) *Attorney, Agent, or Firm*—Banner & Witcoff, Ltd.

(30) **Foreign Application Priority Data**

(57) **CLAIM**

Mar. 7, 2007 (JP) 2007-005928

The ornamental design for a probe for an ultrasonic diagnosis apparatus, as shown and described.

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/107,
D24/138, 141, 158, 164, 165, 167, 170, 186–187,
D24/231; D10/57, 60, 78, 80; 600/407,
600/461, 459, 447; 378/98.7, 98.8, 189;
D14/412

DESCRIPTION

FIG. 1 is a front, bottom and left side perspective view of a probe for an ultrasonic diagnosis apparatus, showing my new design;

See application file for complete search history.

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

(56) **References Cited**

U.S. PATENT DOCUMENTS

D245,513 S * 8/1977 Kopel D24/187
4,796,632 A * 1/1989 Boyd et al. 600/459
D319,793 S * 9/1991 Dubut D10/60
D320,078 S * 9/1991 Terwilliger et al. D24/138
D389,919 S * 1/1998 Ninomiya et al. D24/186
5,839,442 A * 11/1998 Chiang et al. 600/447
5,897,503 A * 4/1999 Lyon et al. 600/459
D544,606 S * 6/2007 Hasegawa et al. D24/186

FIG. 4 is a top plan view thereof;


FIG. 5 is a bottom plan view thereof;

FIG. 6 is a left side elevational view thereof; and,

FIG. 7 is a right side elevational view thereof.

The broken line showing of the remainder of the probe for an ultrasonic diagnosis apparatus is for illustrative purposes only and forms no part of the claimed design.

1 Claim, 2 Drawing Sheets

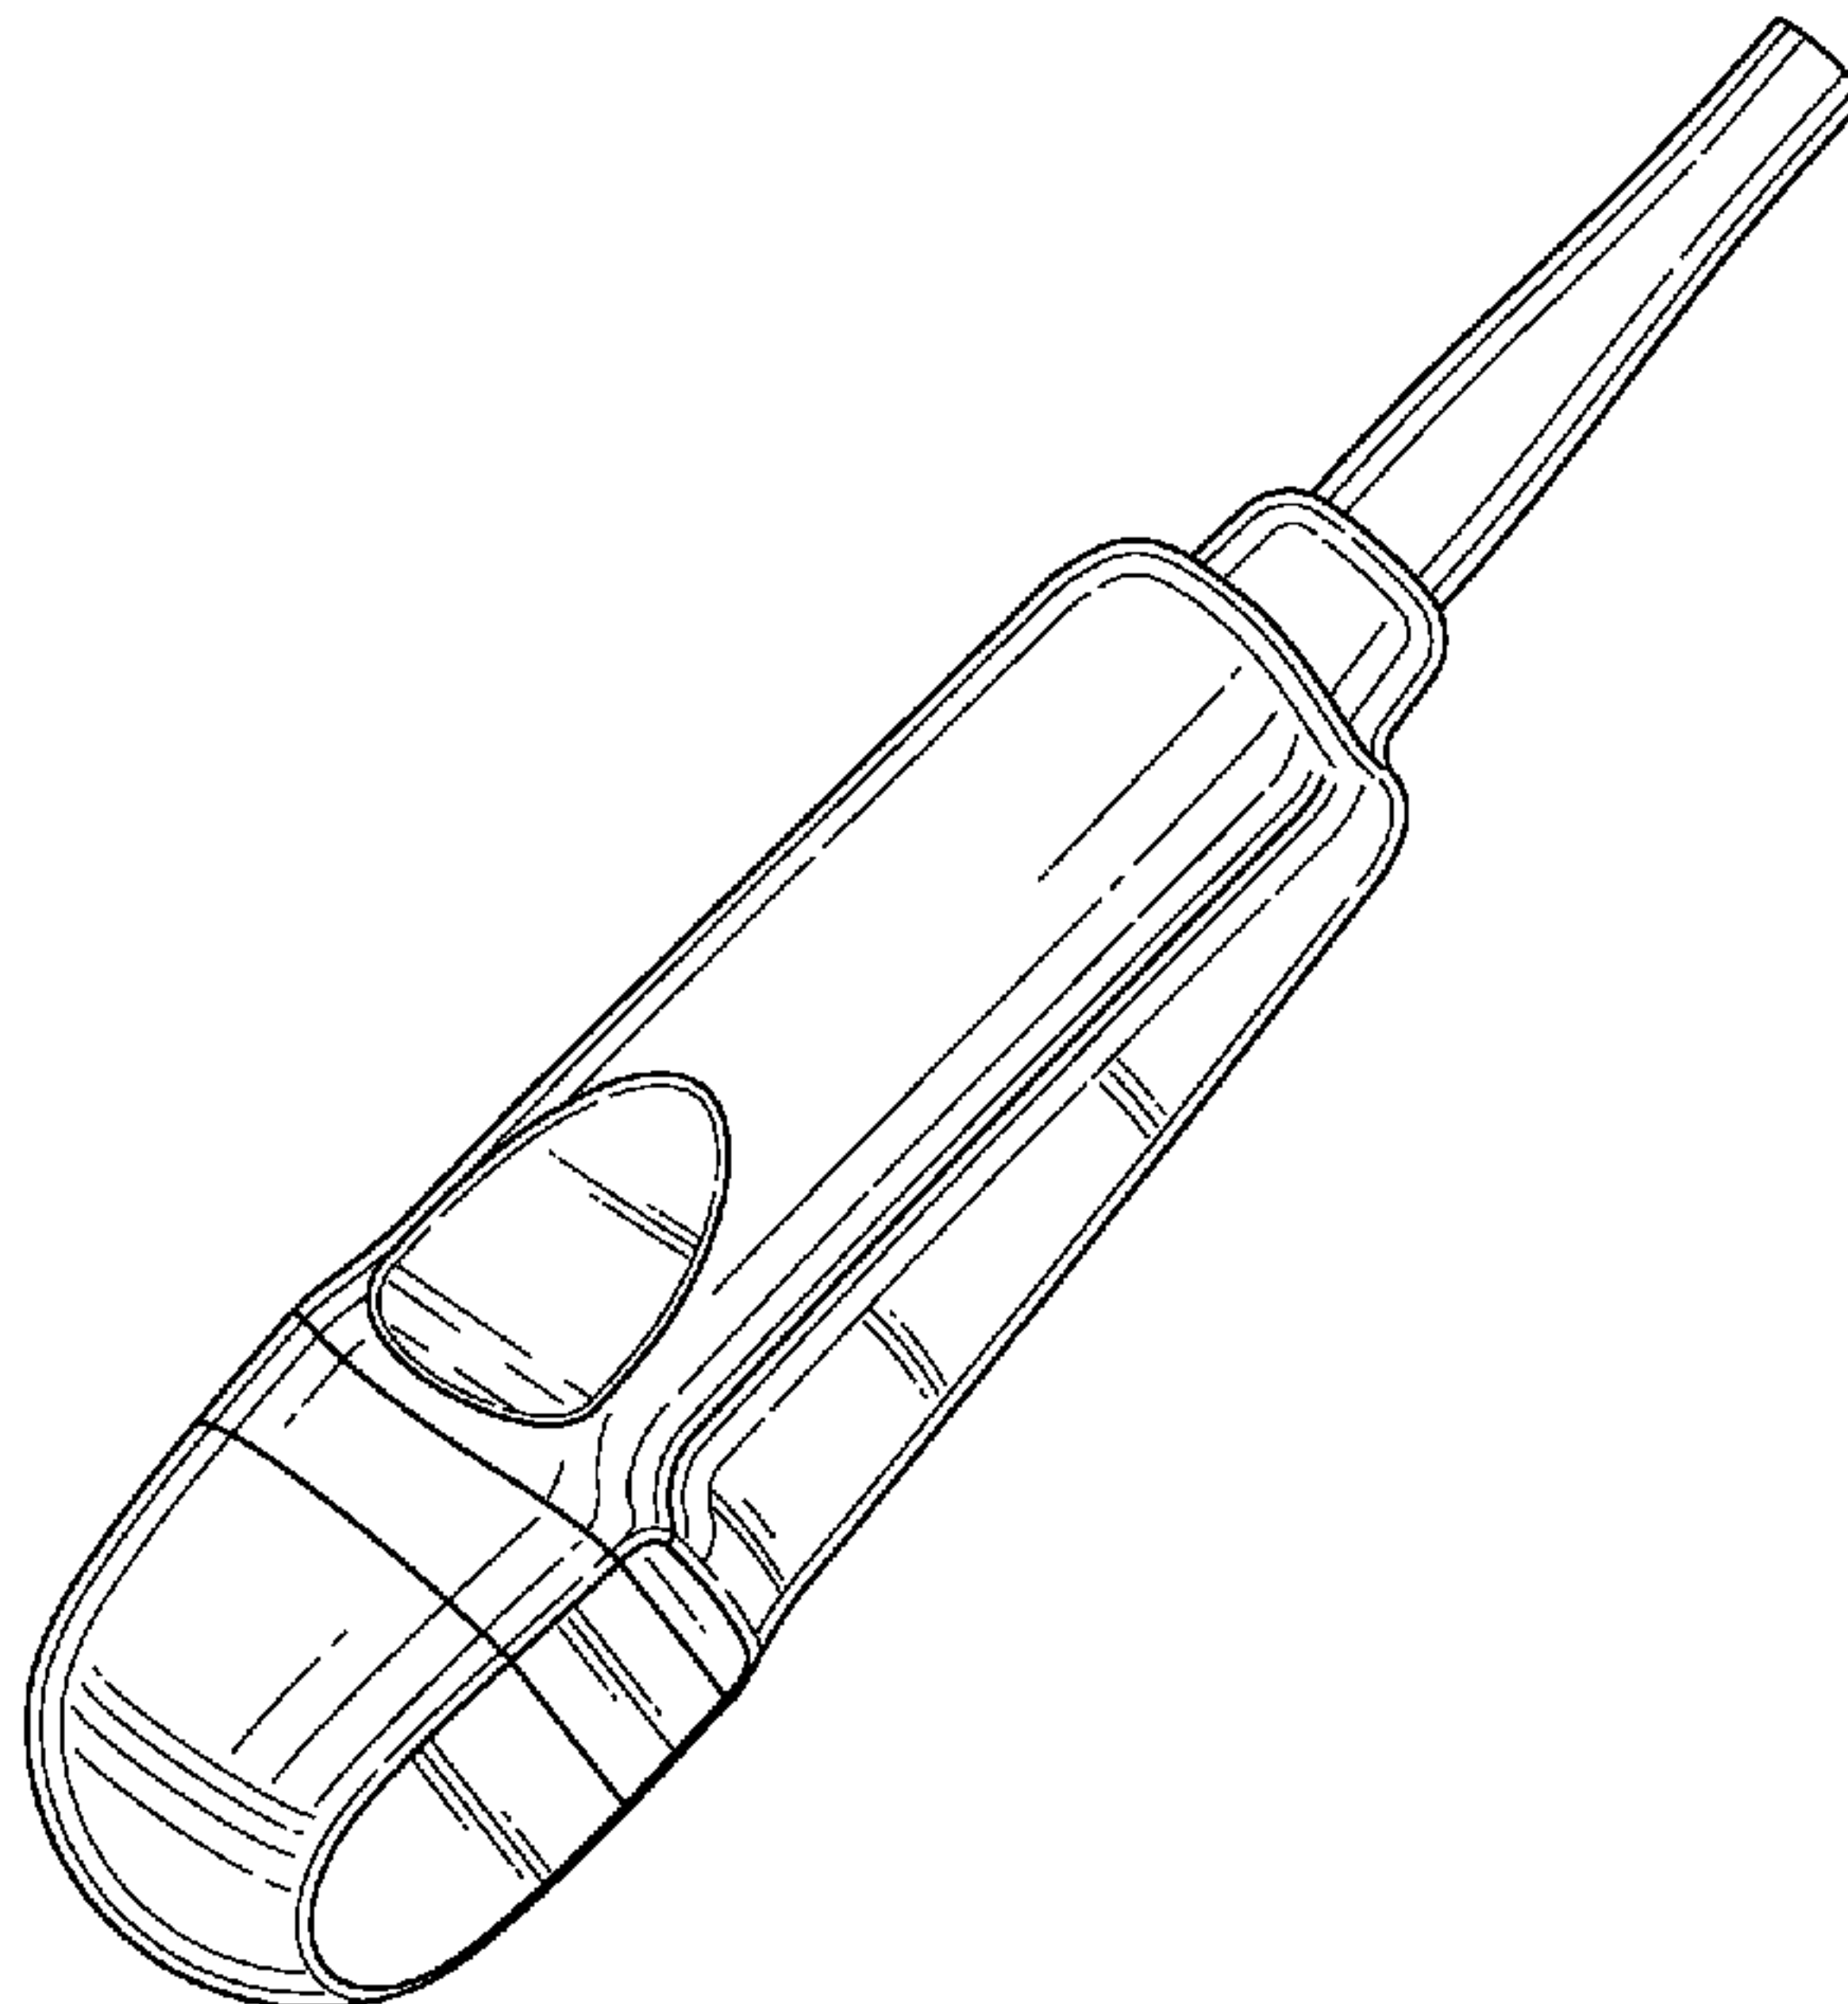

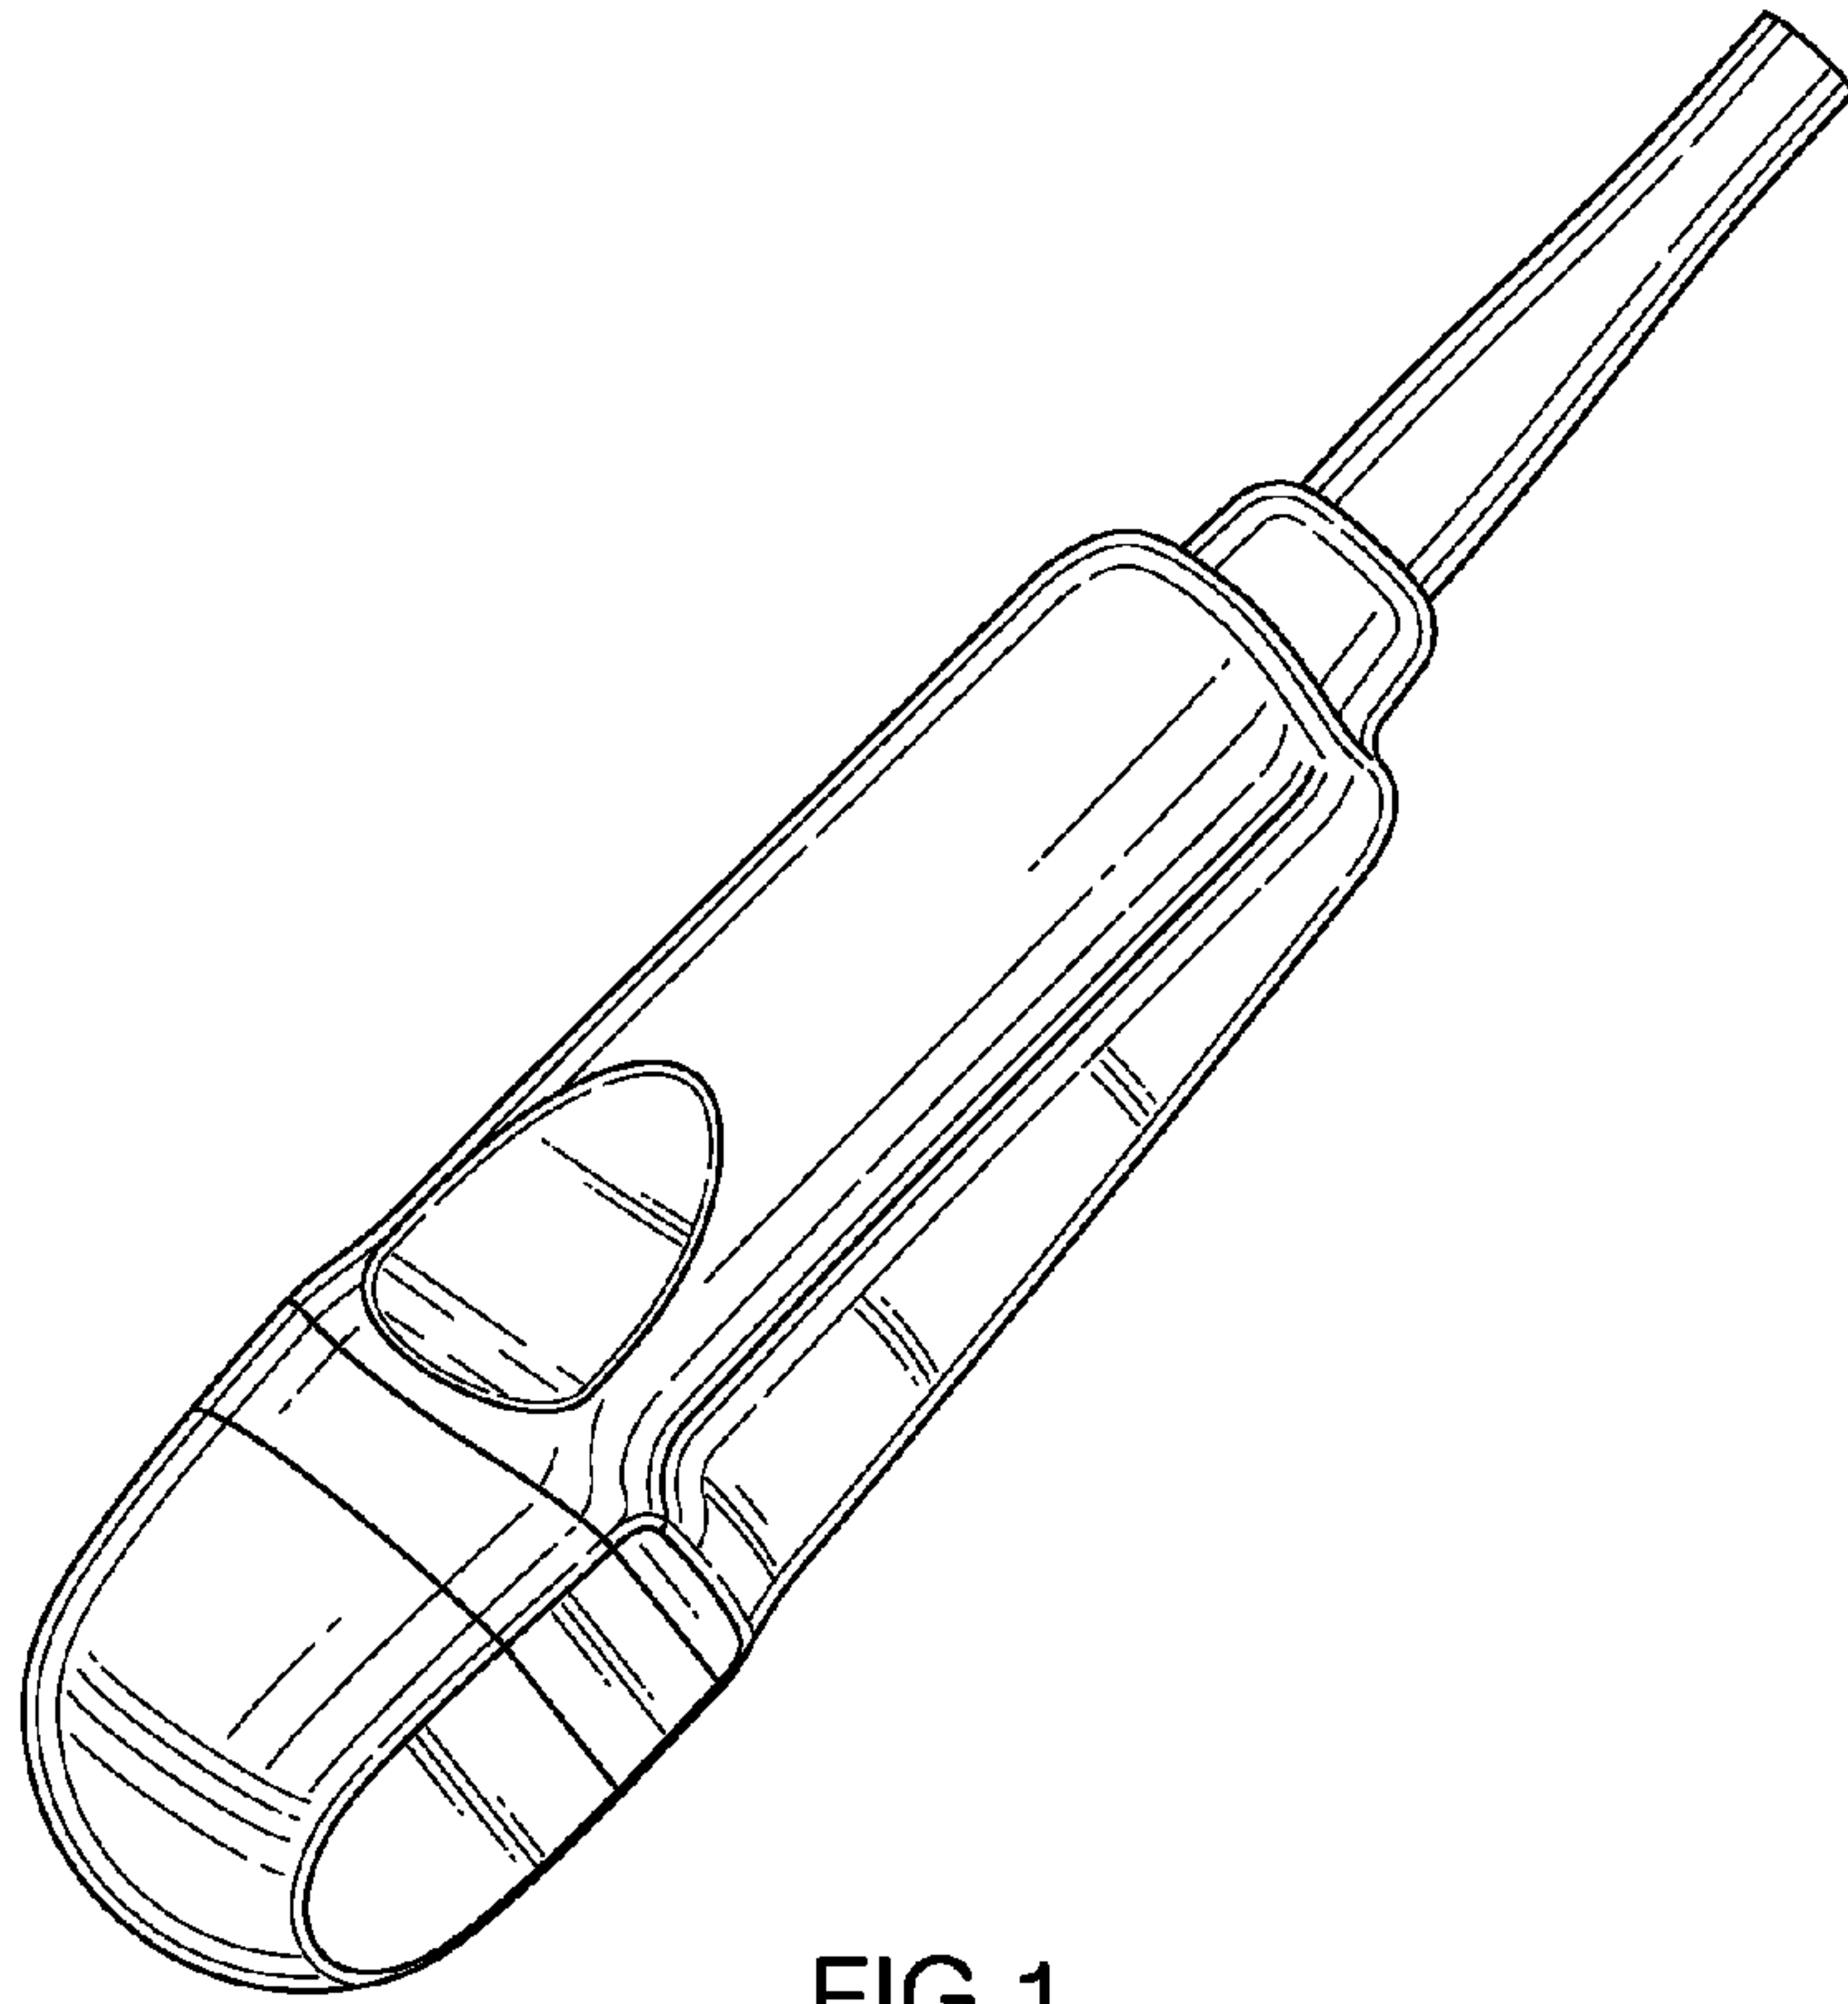


FIG.1

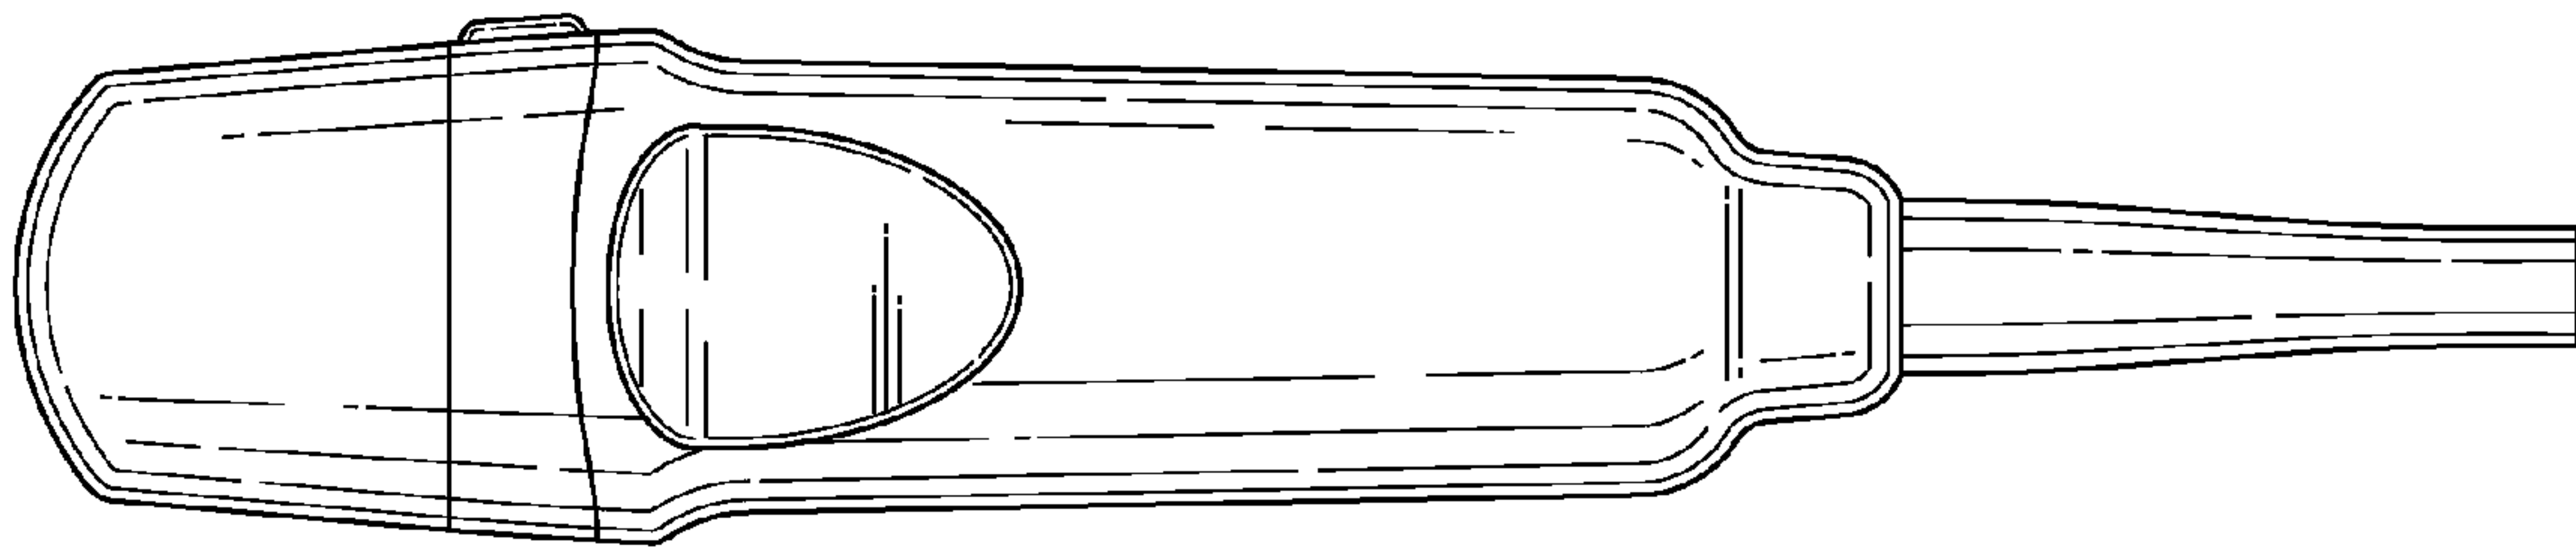


FIG.2

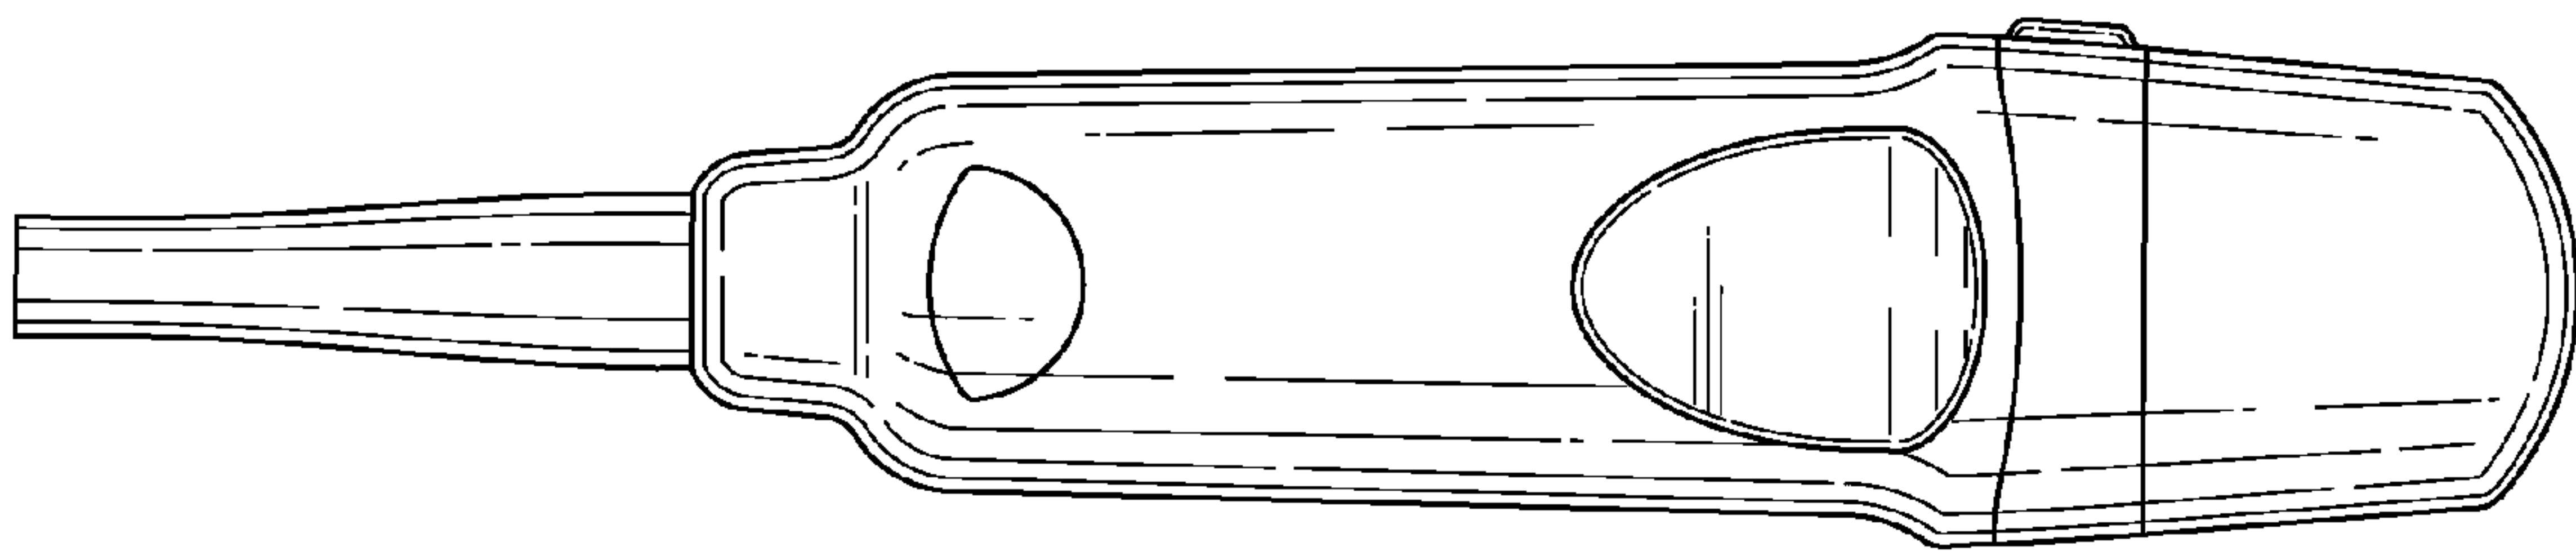


FIG.3

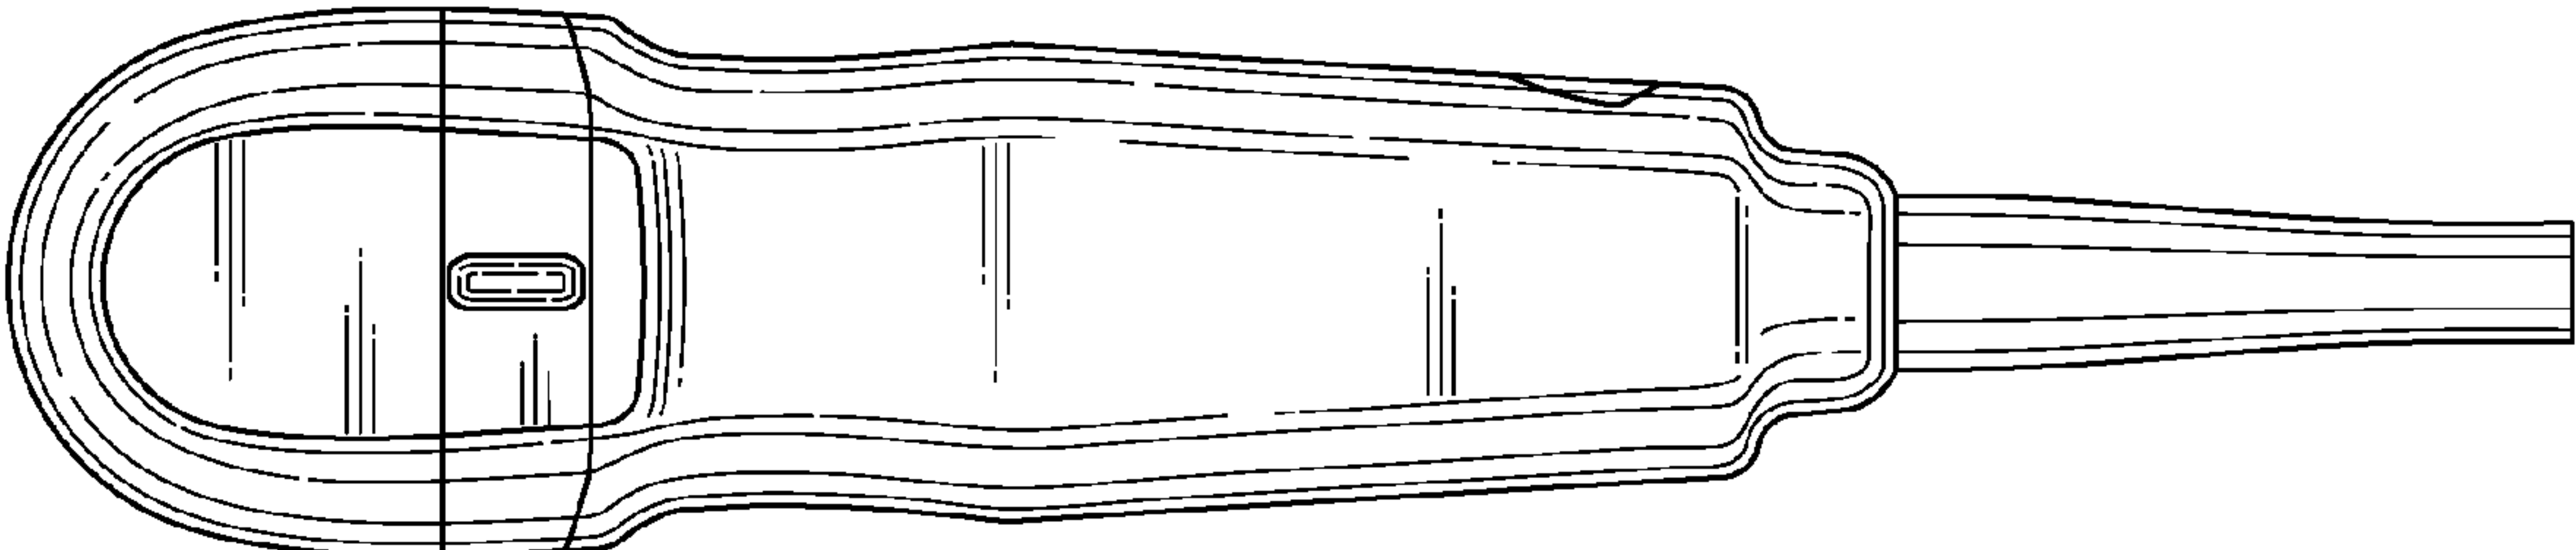


FIG.4

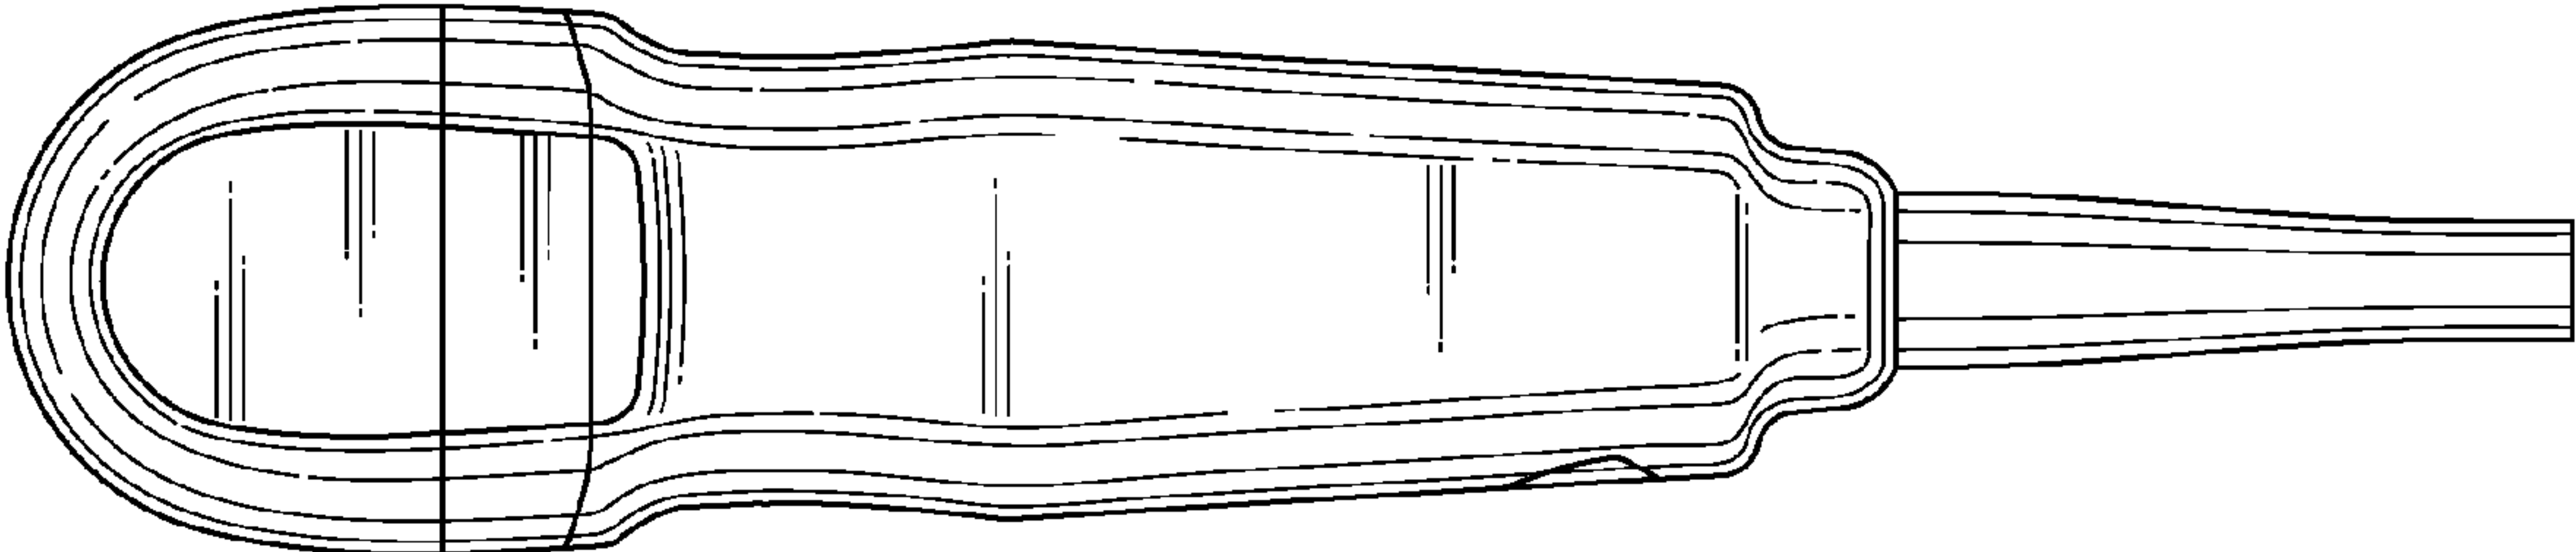


FIG.5

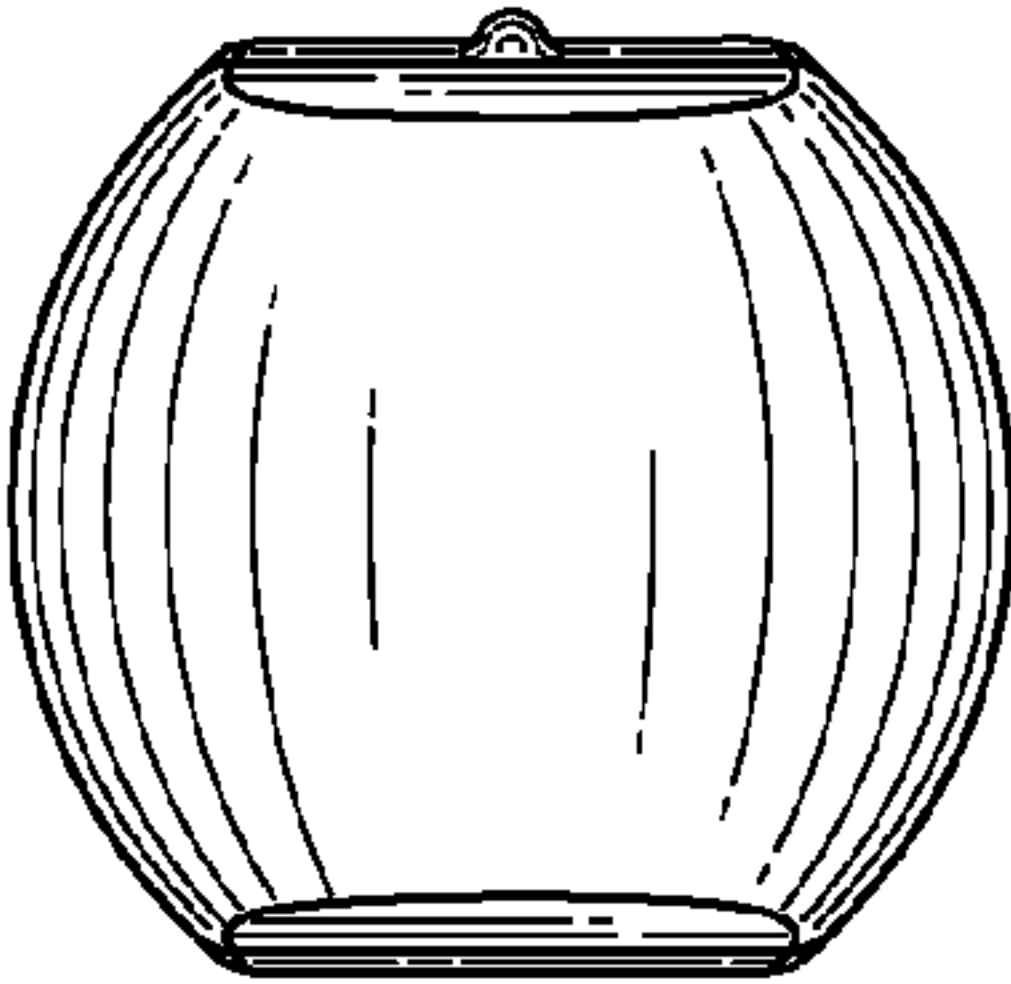


FIG.6

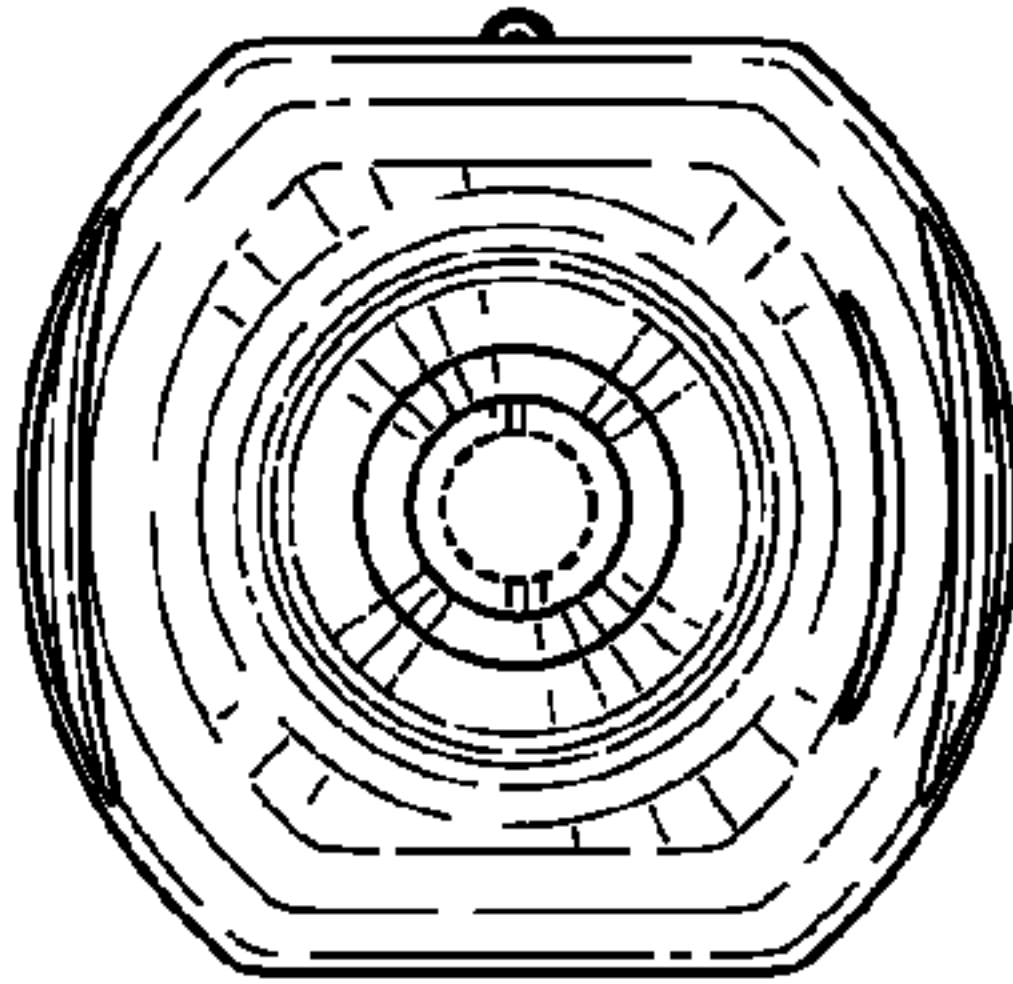


FIG.7