



US00D616994S

(12) **United States Design Patent**
Cummings et al.

(10) **Patent No.:** **US D616,994 S**
(45) **Date of Patent:** **** Jun. 1, 2010**

(54) **BIOMEDICAL ELECTRODE**

(75) Inventors: **Edward A. Cummings**, Armagh (GB);
James E. Southwell, Brockworth (GB);
Alun Wilcox, Richmond (GB); **Michael James**, Tooting (GB); **Morton Watkins**,
Stroud (GB)

(73) Assignee: **Unomedical Limited**, Worcestershire
(GB)

(**) Term: **14 Years**

(21) Appl. No.: **29/257,537**

(22) Filed: **Apr. 4, 2006**

(30) **Foreign Application Priority Data**

Oct. 4, 2005 (EM) 000420807

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/187**

(58) **Field of Classification Search** D24/144,
D24/164, 167, 168, 170, 187, 231; 600/300,
600/301, 368, 372, 481, 529, 544, 554, 561;
607/4, 5, 9, 30, 129

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D297,460 S * 8/1988 Inoue et al. D24/187
D297,461 S * 8/1988 Inoue et al. D24/168
5,354,328 A * 10/1994 Doan et al. 607/129
D369,667 S * 5/1996 Vincents et al. D24/187
D378,614 S * 3/1997 Jensen D24/187
D385,037 S * 10/1997 Jensen D24/187
D423,674 S * 4/2000 Bassøe D24/187
D429,337 S * 8/2000 Sanfilippo D24/187

D457,634 S * 5/2002 Rouns et al. D24/168
D458,376 S * 6/2002 Rouns et al. D24/168
D477,085 S * 7/2003 Sanfilippo D24/187
D478,173 S * 8/2003 Nielsen D24/187
D478,668 S * 8/2003 Epstein D24/187
D522,374 S * 6/2006 Nova et al. D24/187
D567,949 S * 4/2008 Lash et al. D24/168
D584,414 S * 1/2009 Lash et al. D24/187
D590,342 S * 4/2009 Davila et al. D24/187

* cited by examiner

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Klein, O’Neill & Singh, LLP

(57) **CLAIM**

The ornamental design of a biomedical electrode, as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of a biomedical electrode showing our new design with the conductive flap in a raised position;


FIG. 2 is a bottom perspective view of the biomedical electrode of FIG. 1, showing the conductive flap in a raised position;

FIG. 3 is a top perspective view of the biomedical electrode of FIG. 1, showing the conductive flap in a lowered position; and,

FIG. 4 is a bottom perspective view of the biomedical electrode in FIG. 1, showing the conductive flap in a lowered position.

The broken lines shown FIG. 3 are a fold line and forms part of the claimed design.

1 Claim, 2 Drawing Sheets

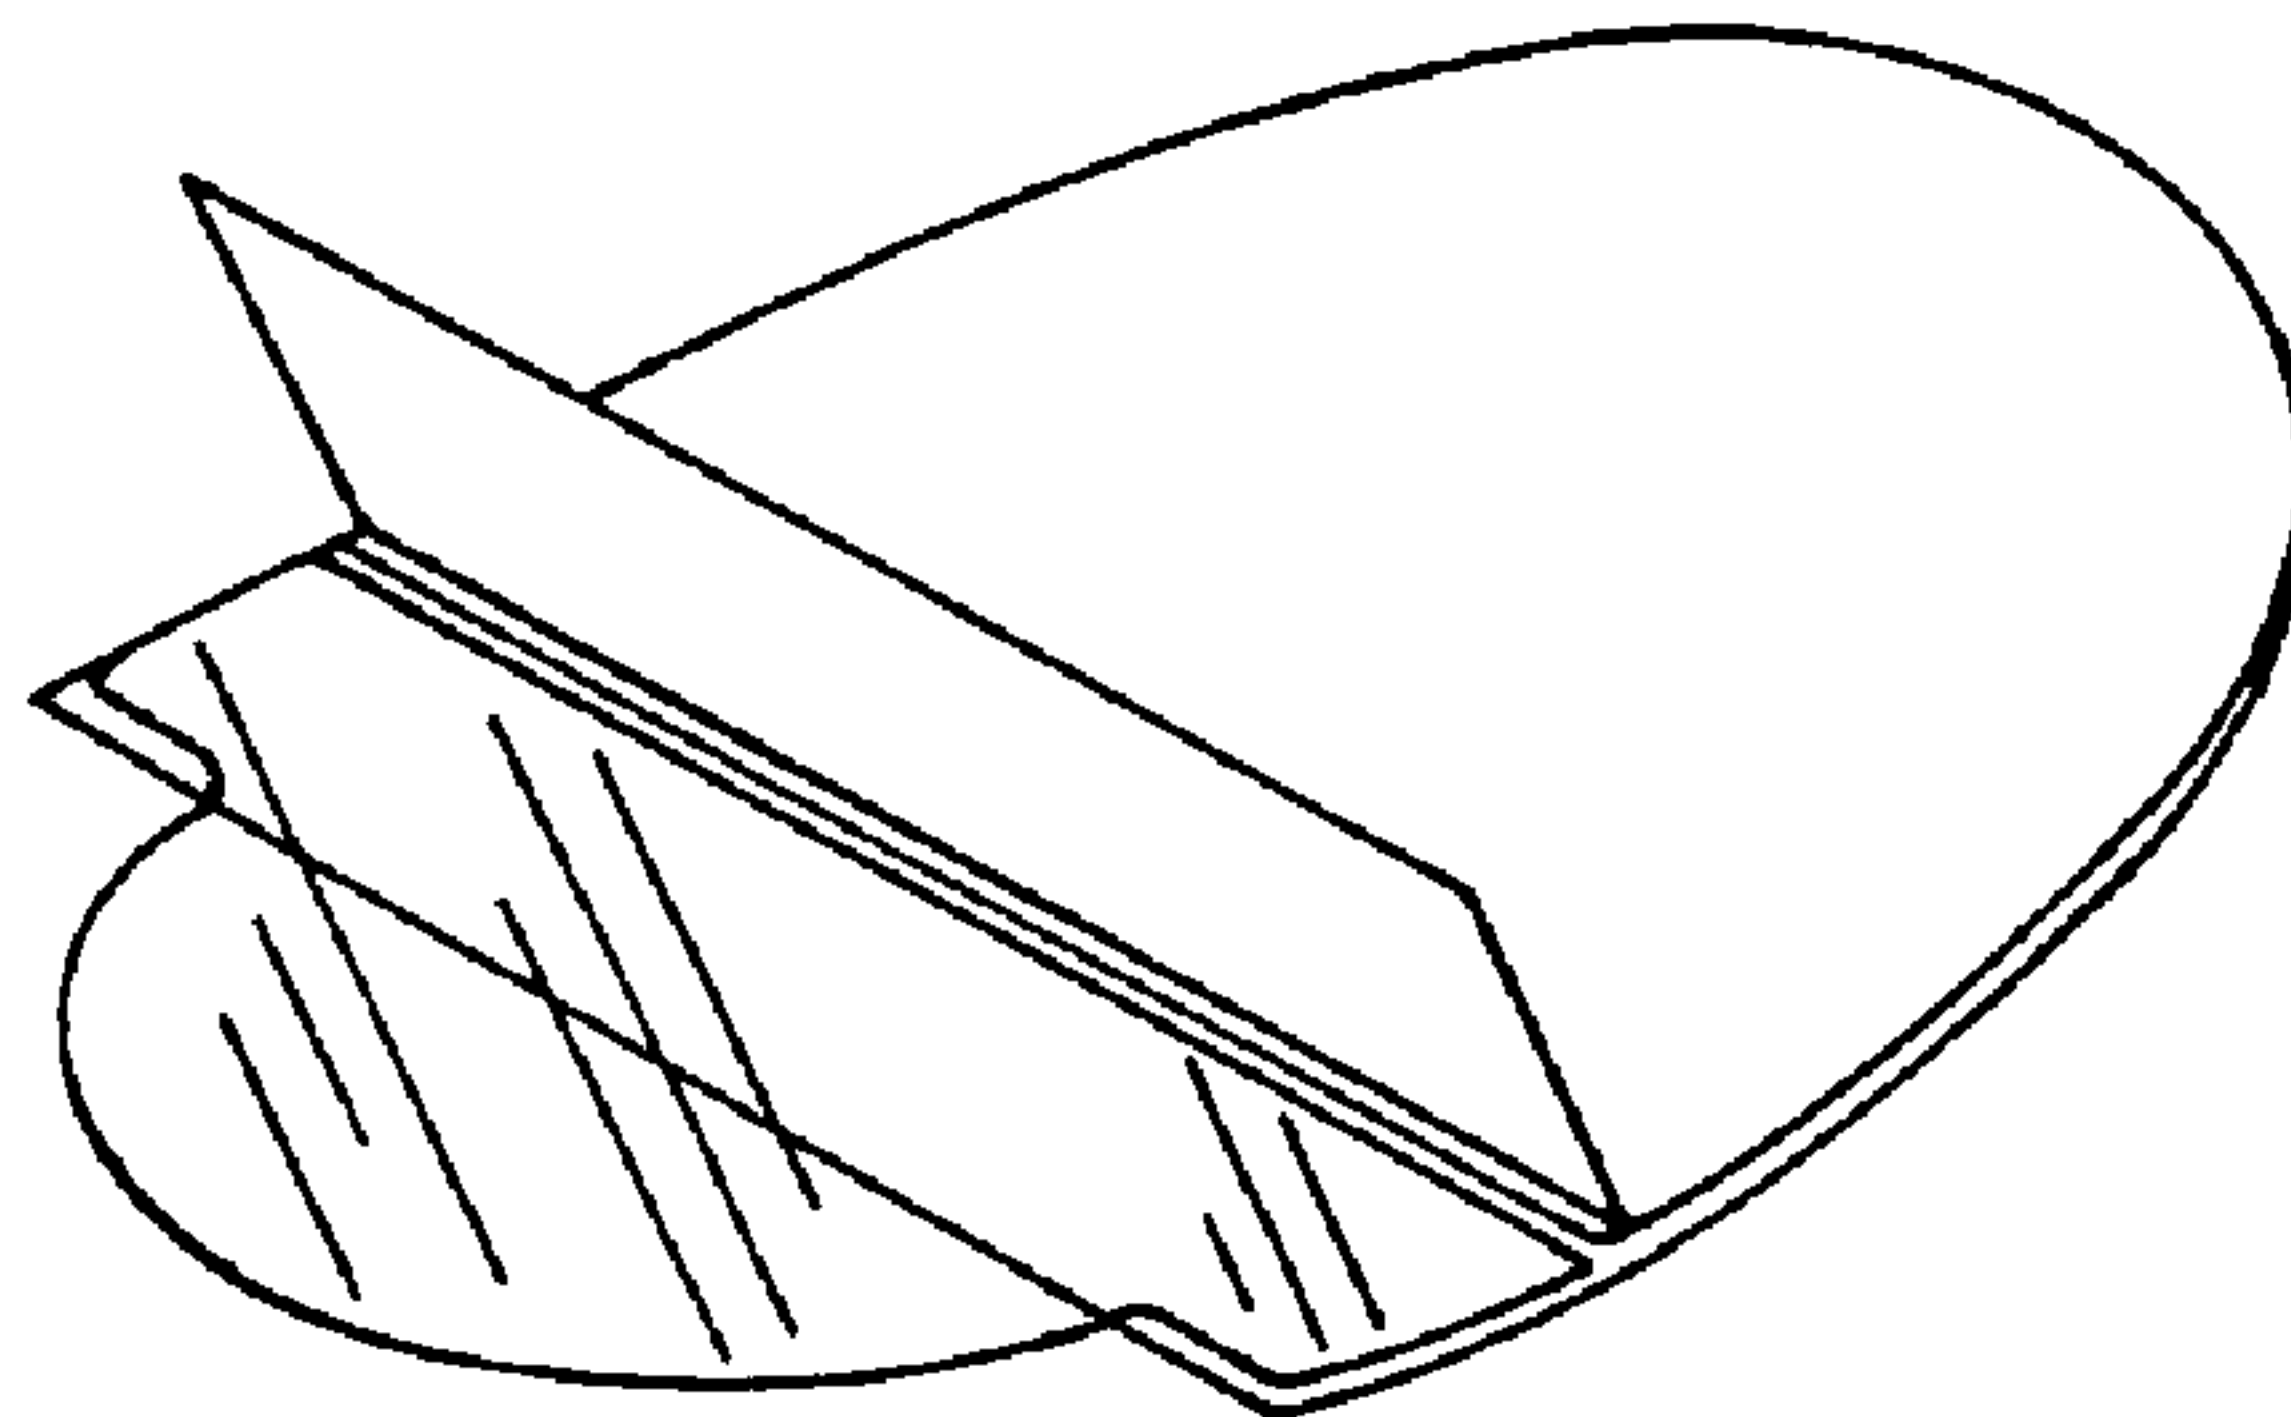

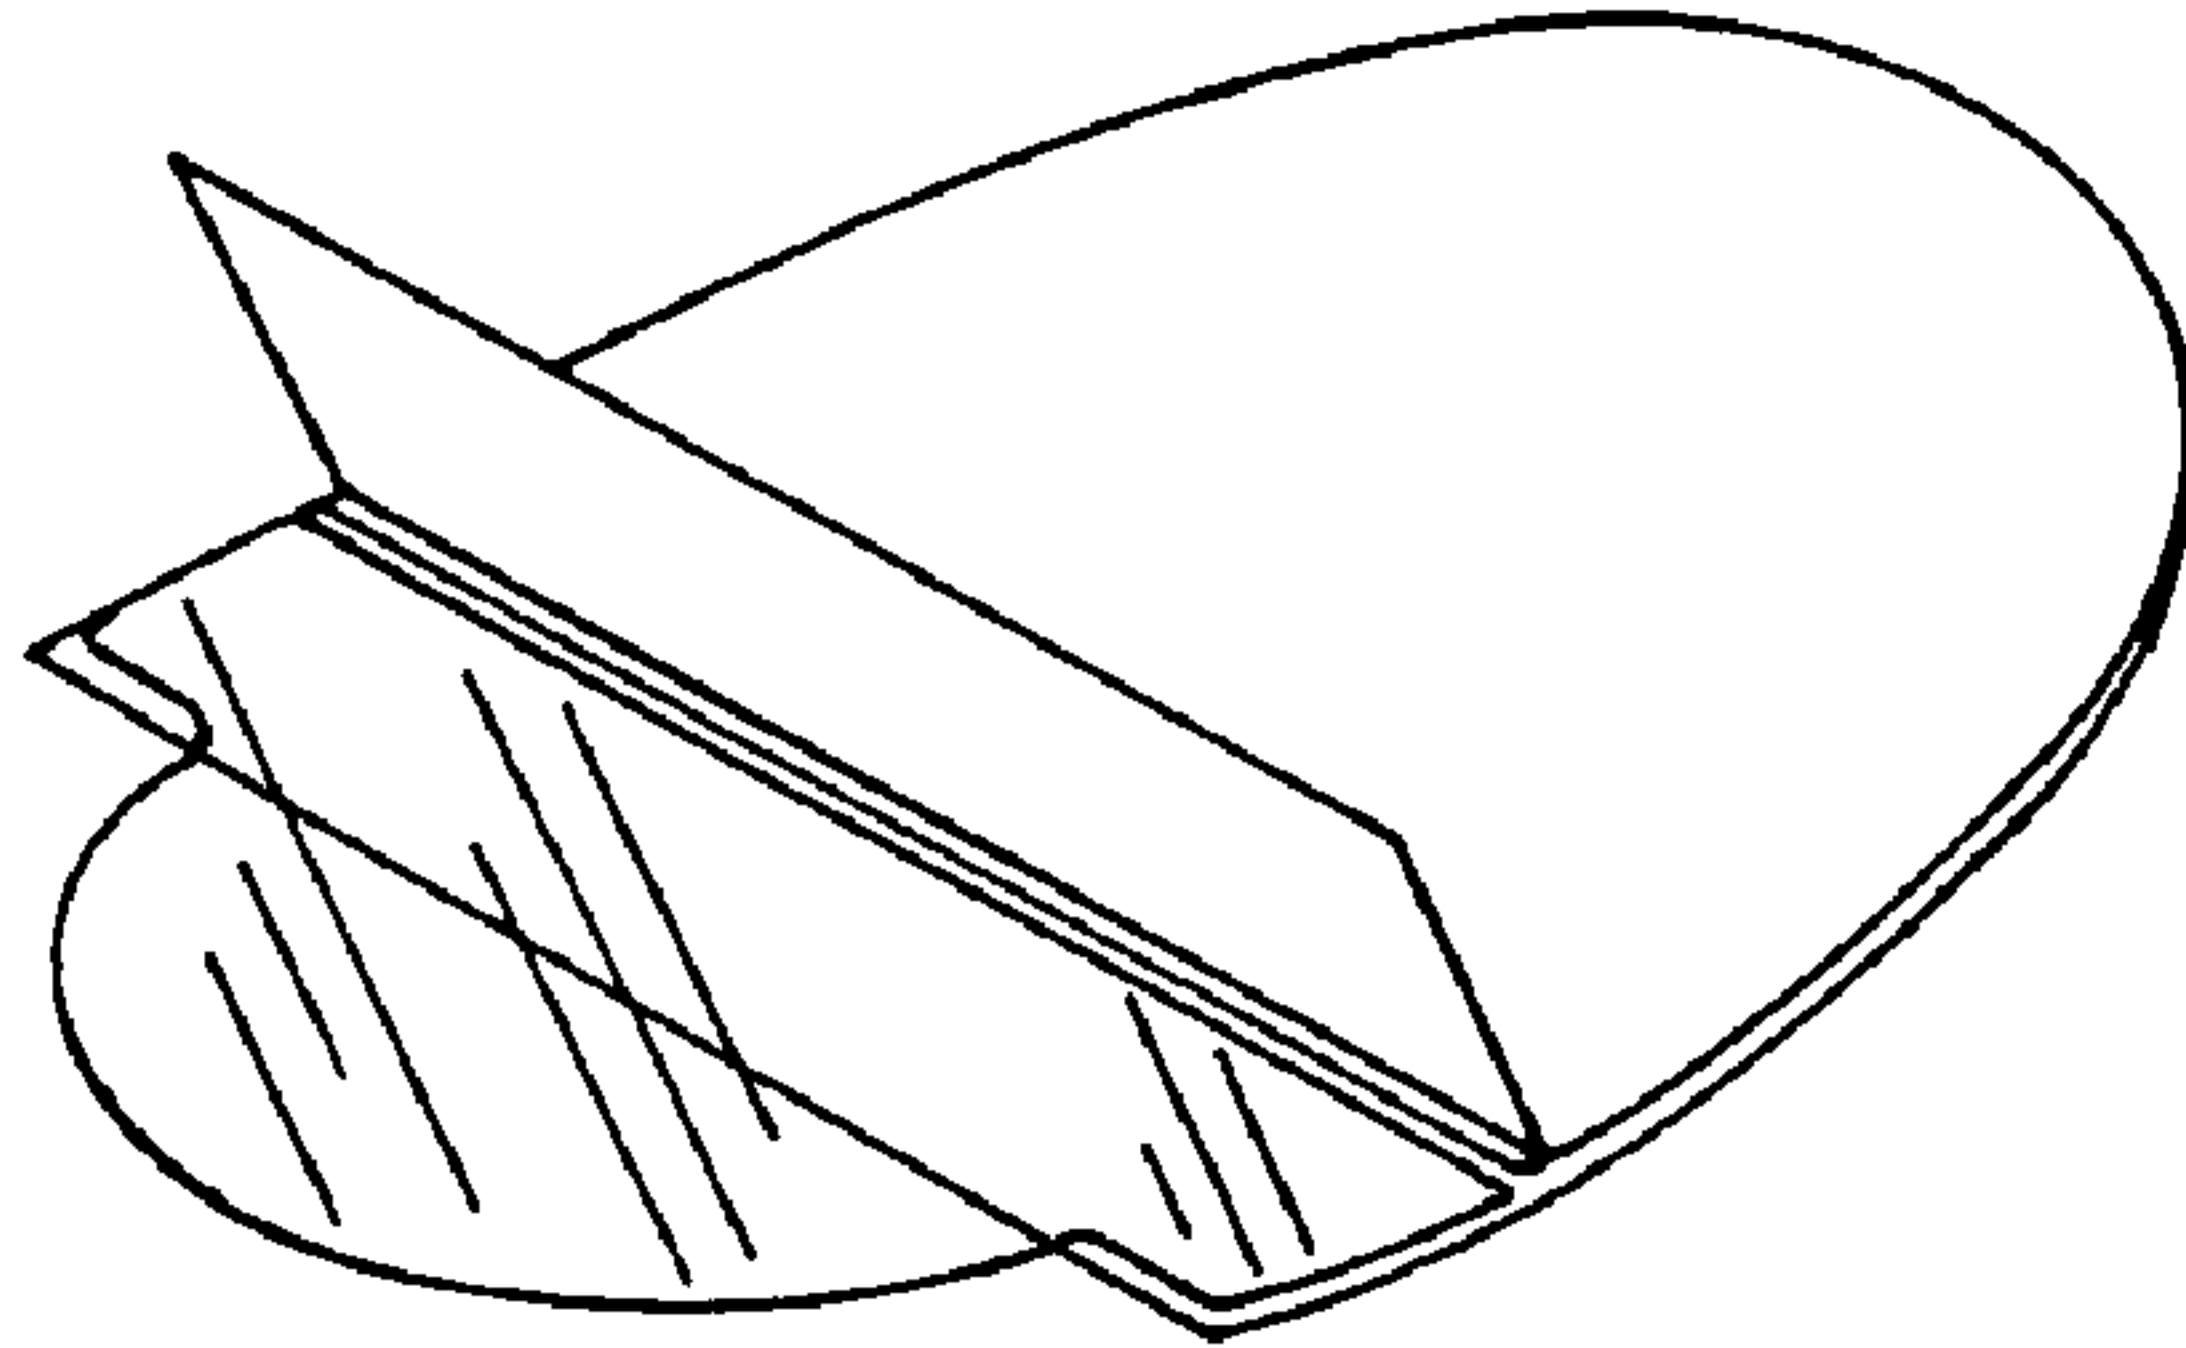


FIG. 1

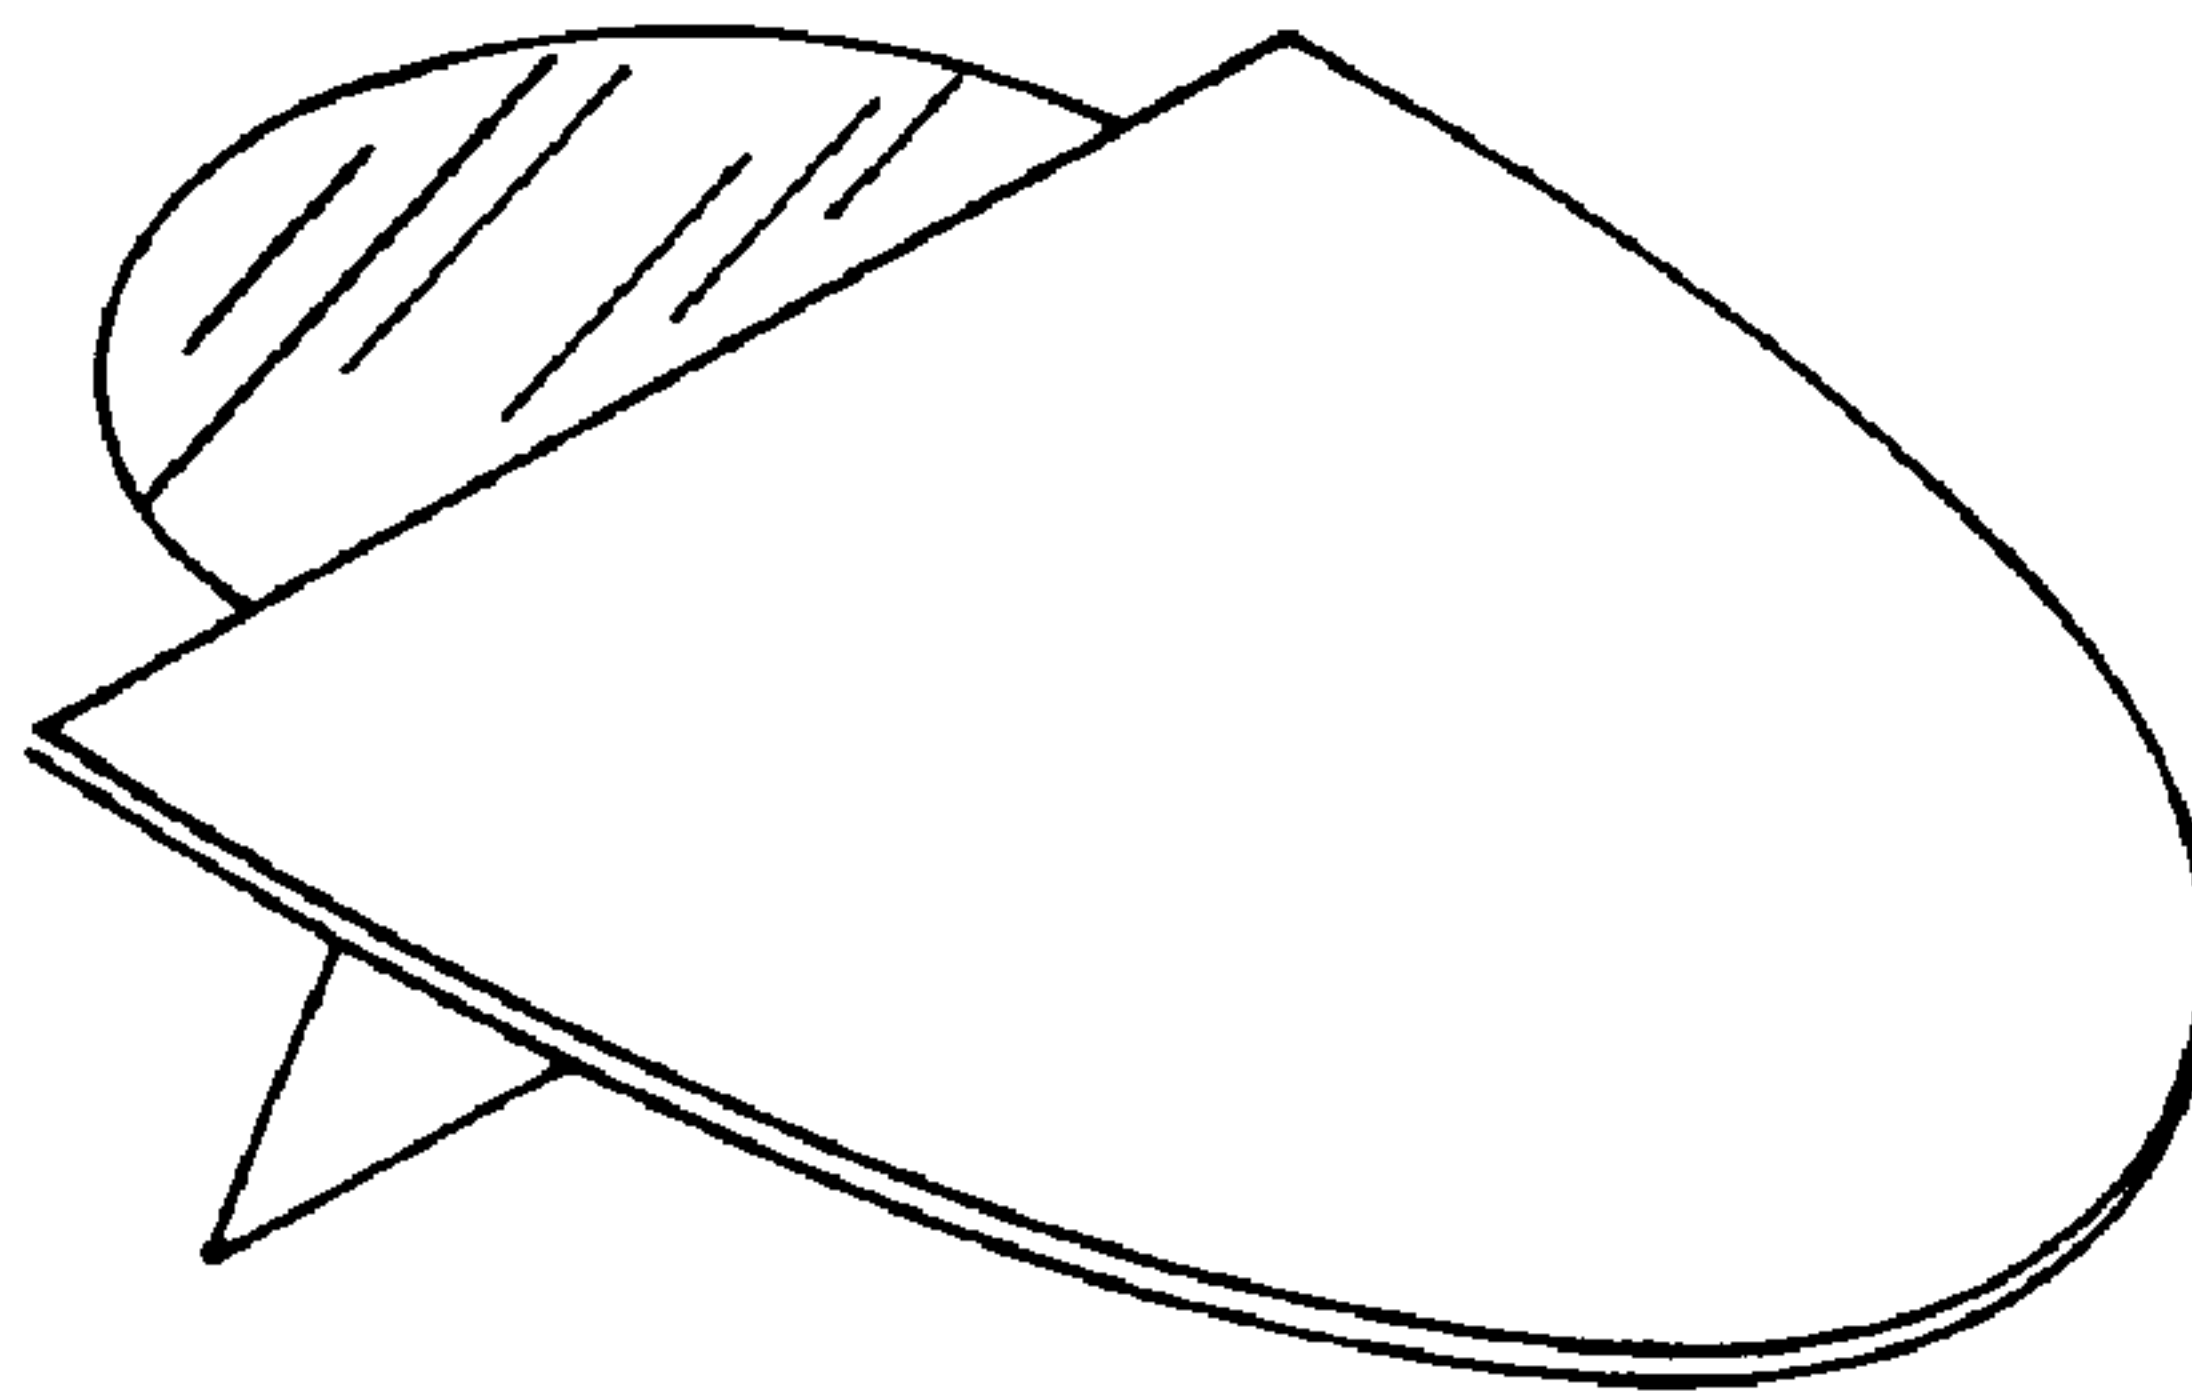


FIG. 2

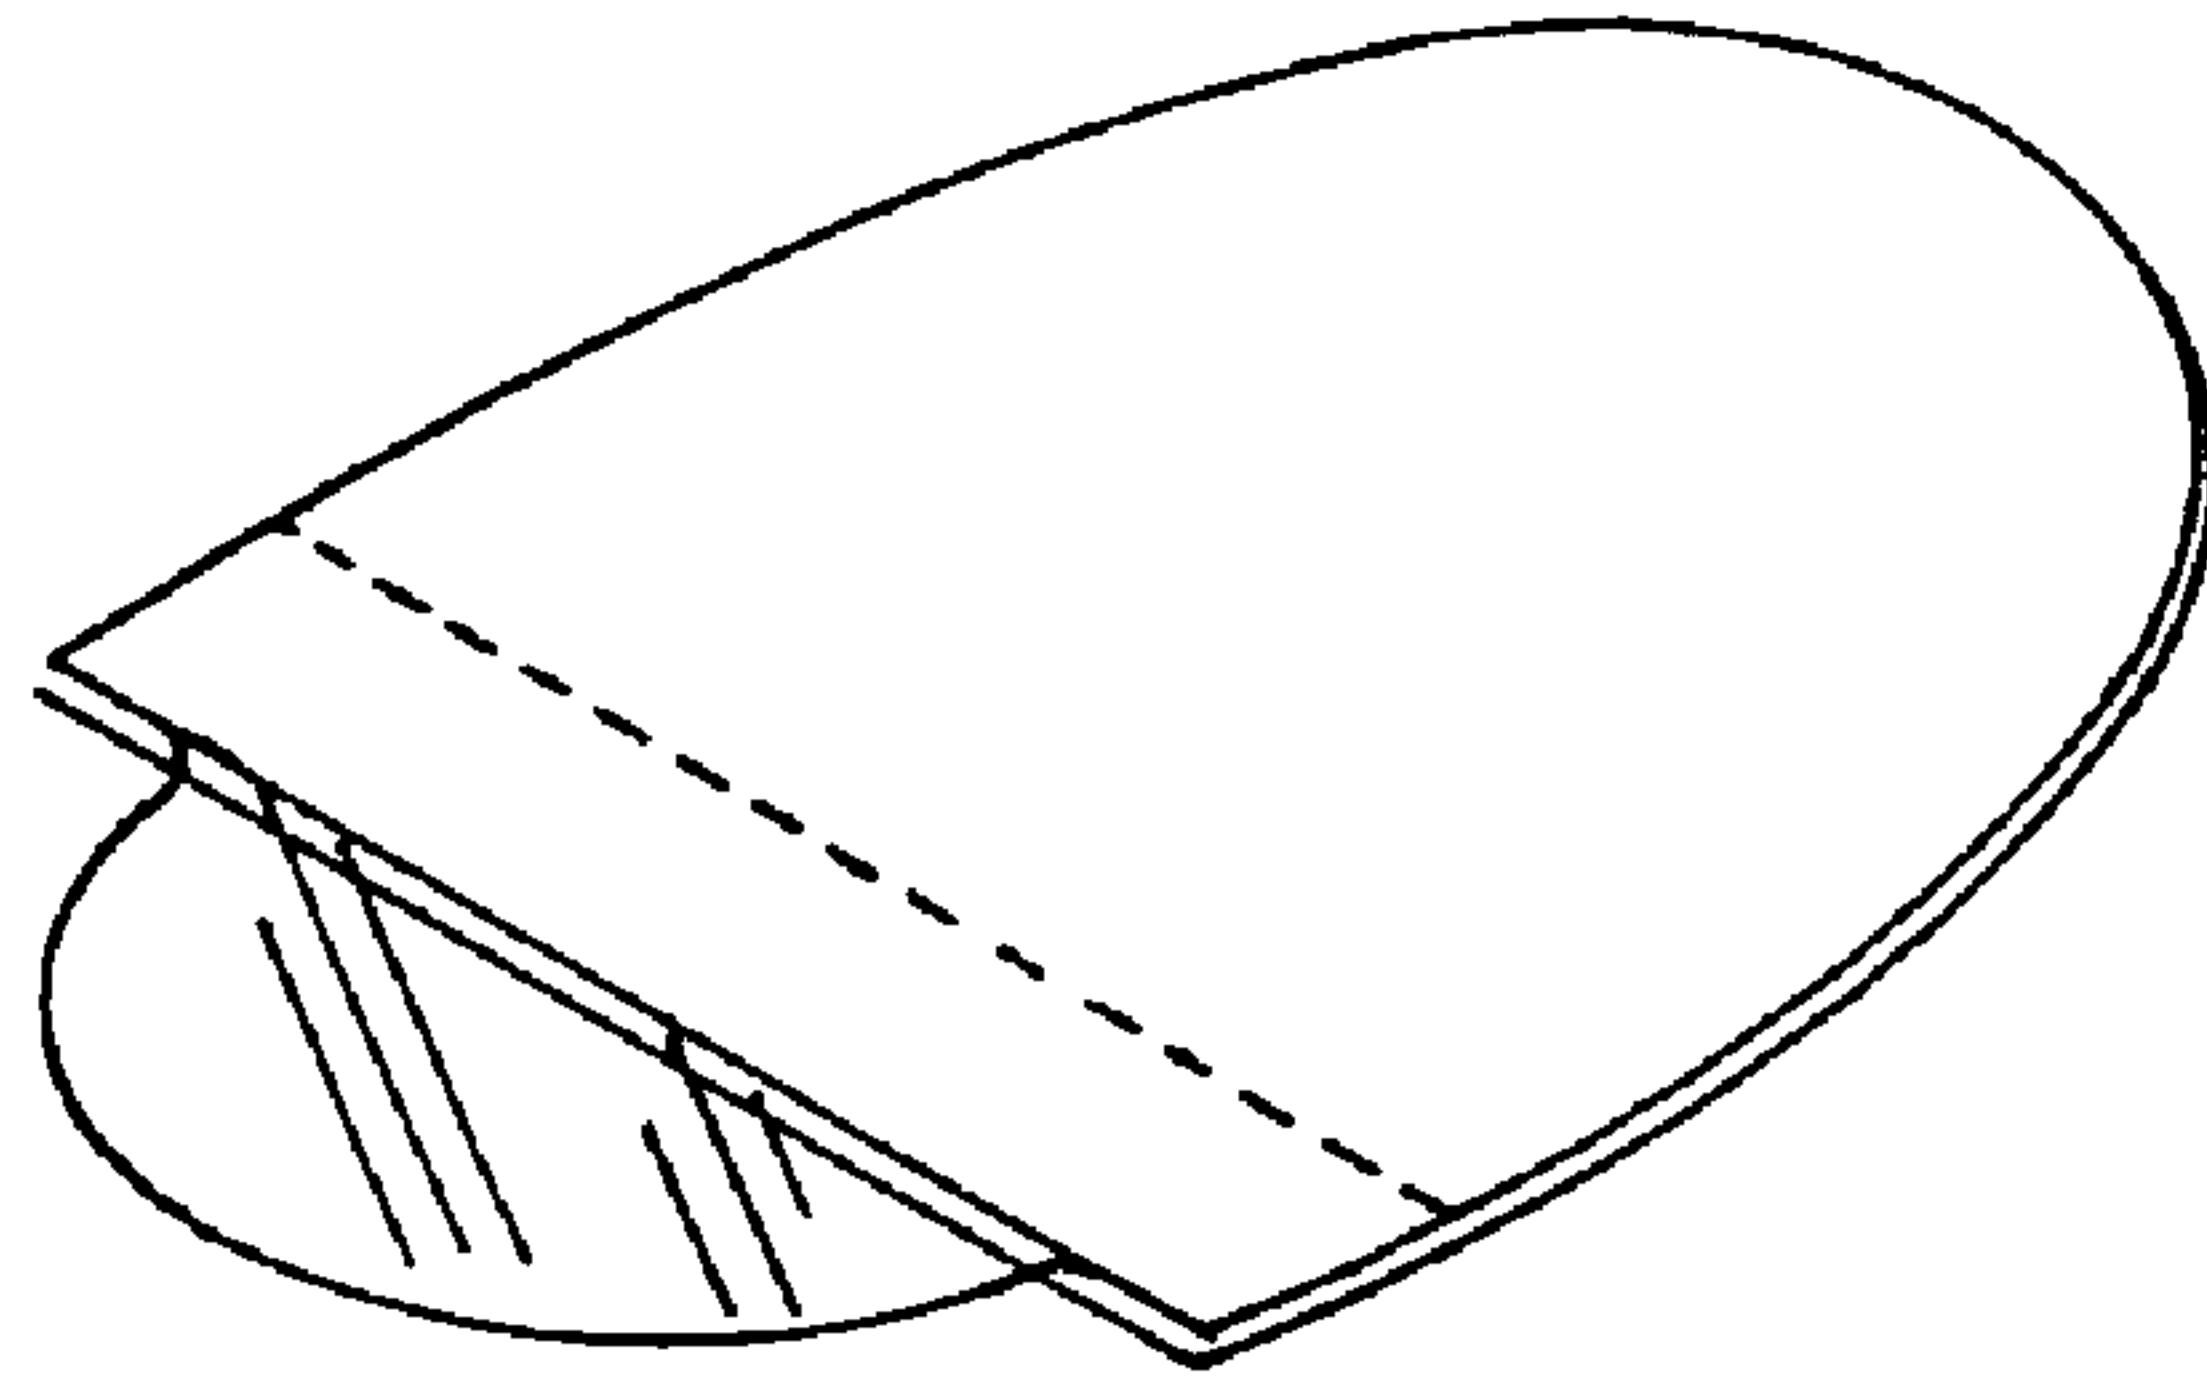


FIG. 3

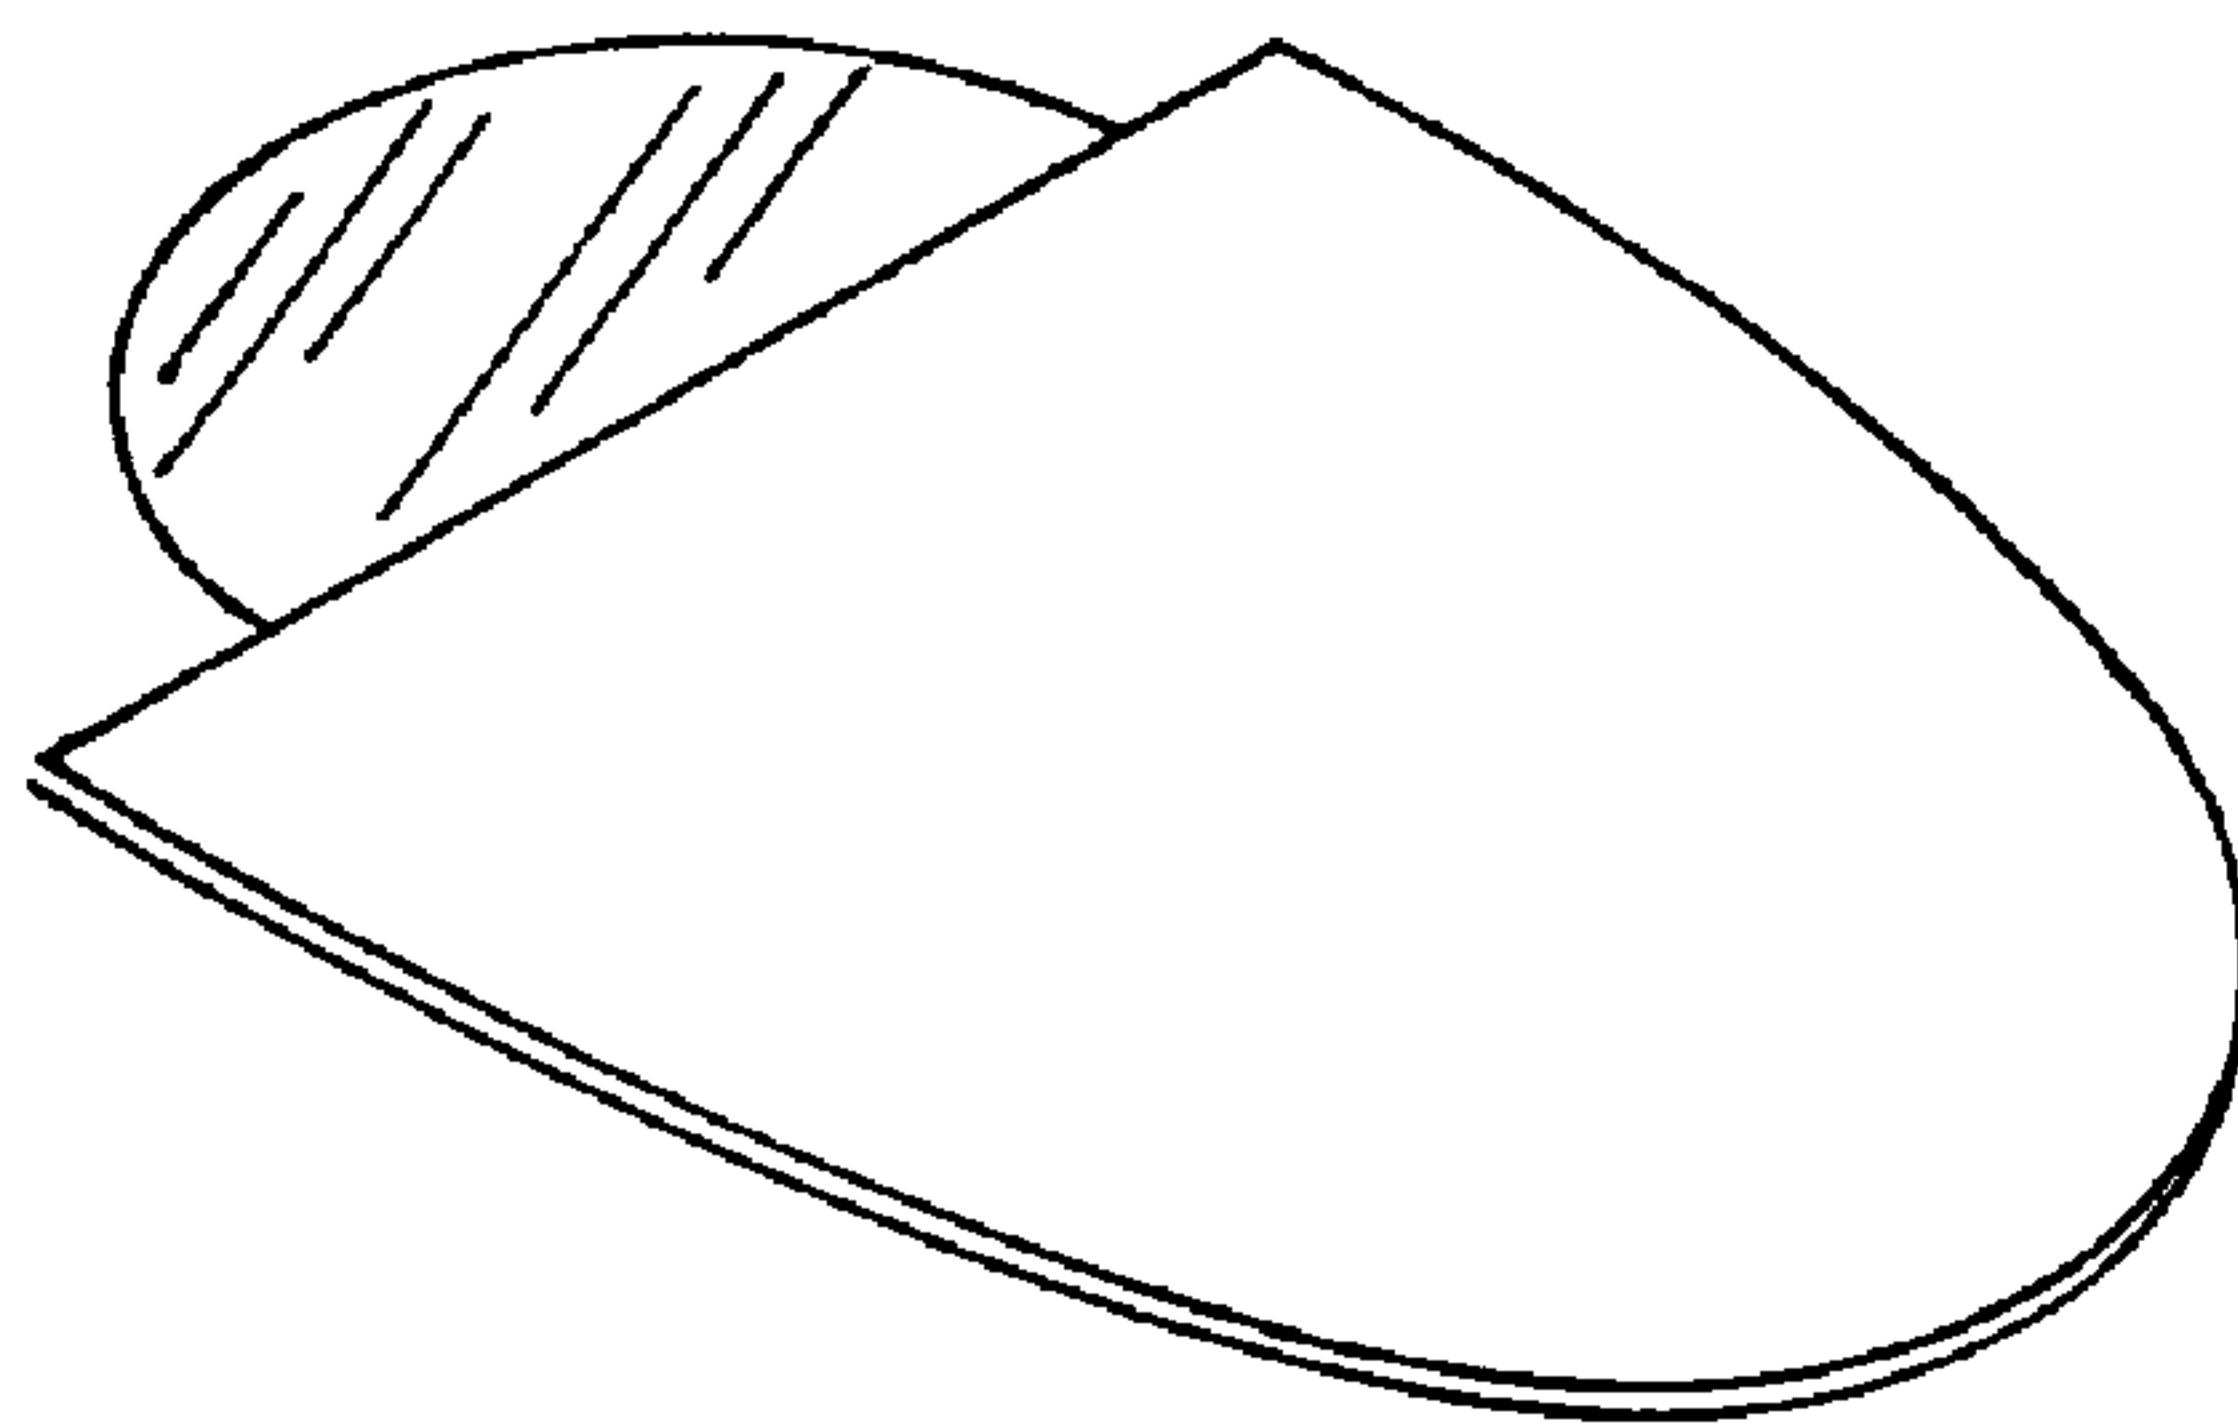


FIG. 4