



US00D620606S

(12) **United States Design Patent**  
**Wilson et al.**

(10) **Patent No.:** **US D620,606 S**  
(45) **Date of Patent:** **\*\* Jul. 27, 2010**

(54) **RACK FOR SUPPORTING LABORATORY APPARATUS**

(75) Inventors: **Stuart Mark Wilson**, London (GB);  
**Roger John Rosedale**, London (GB)

(73) Assignee: **Microsens Medtech Limited**, London (GB)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/343,690**

(22) Filed: **Sep. 17, 2009**

(30) **Foreign Application Priority Data**

Mar. 18, 2009 (EP) ..... 001107858

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/230**

(58) **Field of Classification Search** ..... D24/108,  
D24/127-130, 216, 224, 226-232, 221; 422/63-64,  
422/99-104, 250, 266, 297, 300, 476; 211/74,  
211/71.01

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D237,315 S \* 10/1975 Kowakowski et al. .... D24/226
- D276,462 S \* 11/1984 Villarreal ..... D24/229
- D280,663 S \* 9/1985 Albon et al. .... D24/226
- D300,245 S \* 3/1989 Navarro et al. .... D24/229
- D318,729 S \* 7/1991 Zachry ..... D24/227
- D332,834 S \* 1/1993 Hanna et al. .... D24/230
- D334,973 S \* 4/1993 Valentine et al. .... D24/227
- D337,830 S \* 7/1993 Coyne et al. .... D24/229
- D402,767 S \* 12/1998 Davis et al. .... D24/229
- D438,634 S \* 3/2001 Merry ..... D24/227
- D444,567 S \* 7/2001 Tang ..... D24/230
- D461,554 S \* 8/2002 Lafond et al. .... D24/227
- D466,219 S \* 11/2002 Wynschek et al. .... D24/227

- D484,989 S \* 1/2004 Gebrian ..... D24/230
- D486,580 S \* 2/2004 Abdel-Model ..... D24/229
- D595,423 S \* 6/2009 Johansson et al. .... D24/229
- D596,311 S \* 7/2009 Antons ..... D24/227
- D596,312 S \* 7/2009 Giraud et al. .... D24/230
- D596,758 S \* 7/2009 Constable ..... D24/230
- D598,566 S \* 8/2009 Allaer ..... D24/230

\* cited by examiner

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Pillsbury Winthrop Shaw Pittman LLP

(57) **CLAIM**

The ornamental design for a rack for supporting laboratory apparatus, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a rack for supporting laboratory apparatus showing our new design;

FIG. 2 is a front view of a rack for supporting laboratory apparatus shown in FIG. 1;

FIG. 3 is a back view of a rack for supporting laboratory apparatus shown in FIG. 1

FIG. 4 is a side elevation of one end of a rack for supporting laboratory apparatus shown in FIG. 1


FIG. 5 is a side elevation of the other end of a rack for supporting laboratory apparatus shown in FIG. 1

FIG. 6 is a top view of a rack for supporting laboratory apparatus shown in FIG. 1; and,

FIG. 7 is a bottom view of a rack for supporting laboratory apparatus shown in FIG. 1.

The broken lines shown are included for the purpose of illustrating a portion of the rack for supporting laboratory apparatus that forms no part of the claimed design.

**1 Claim, 3 Drawing Sheets**

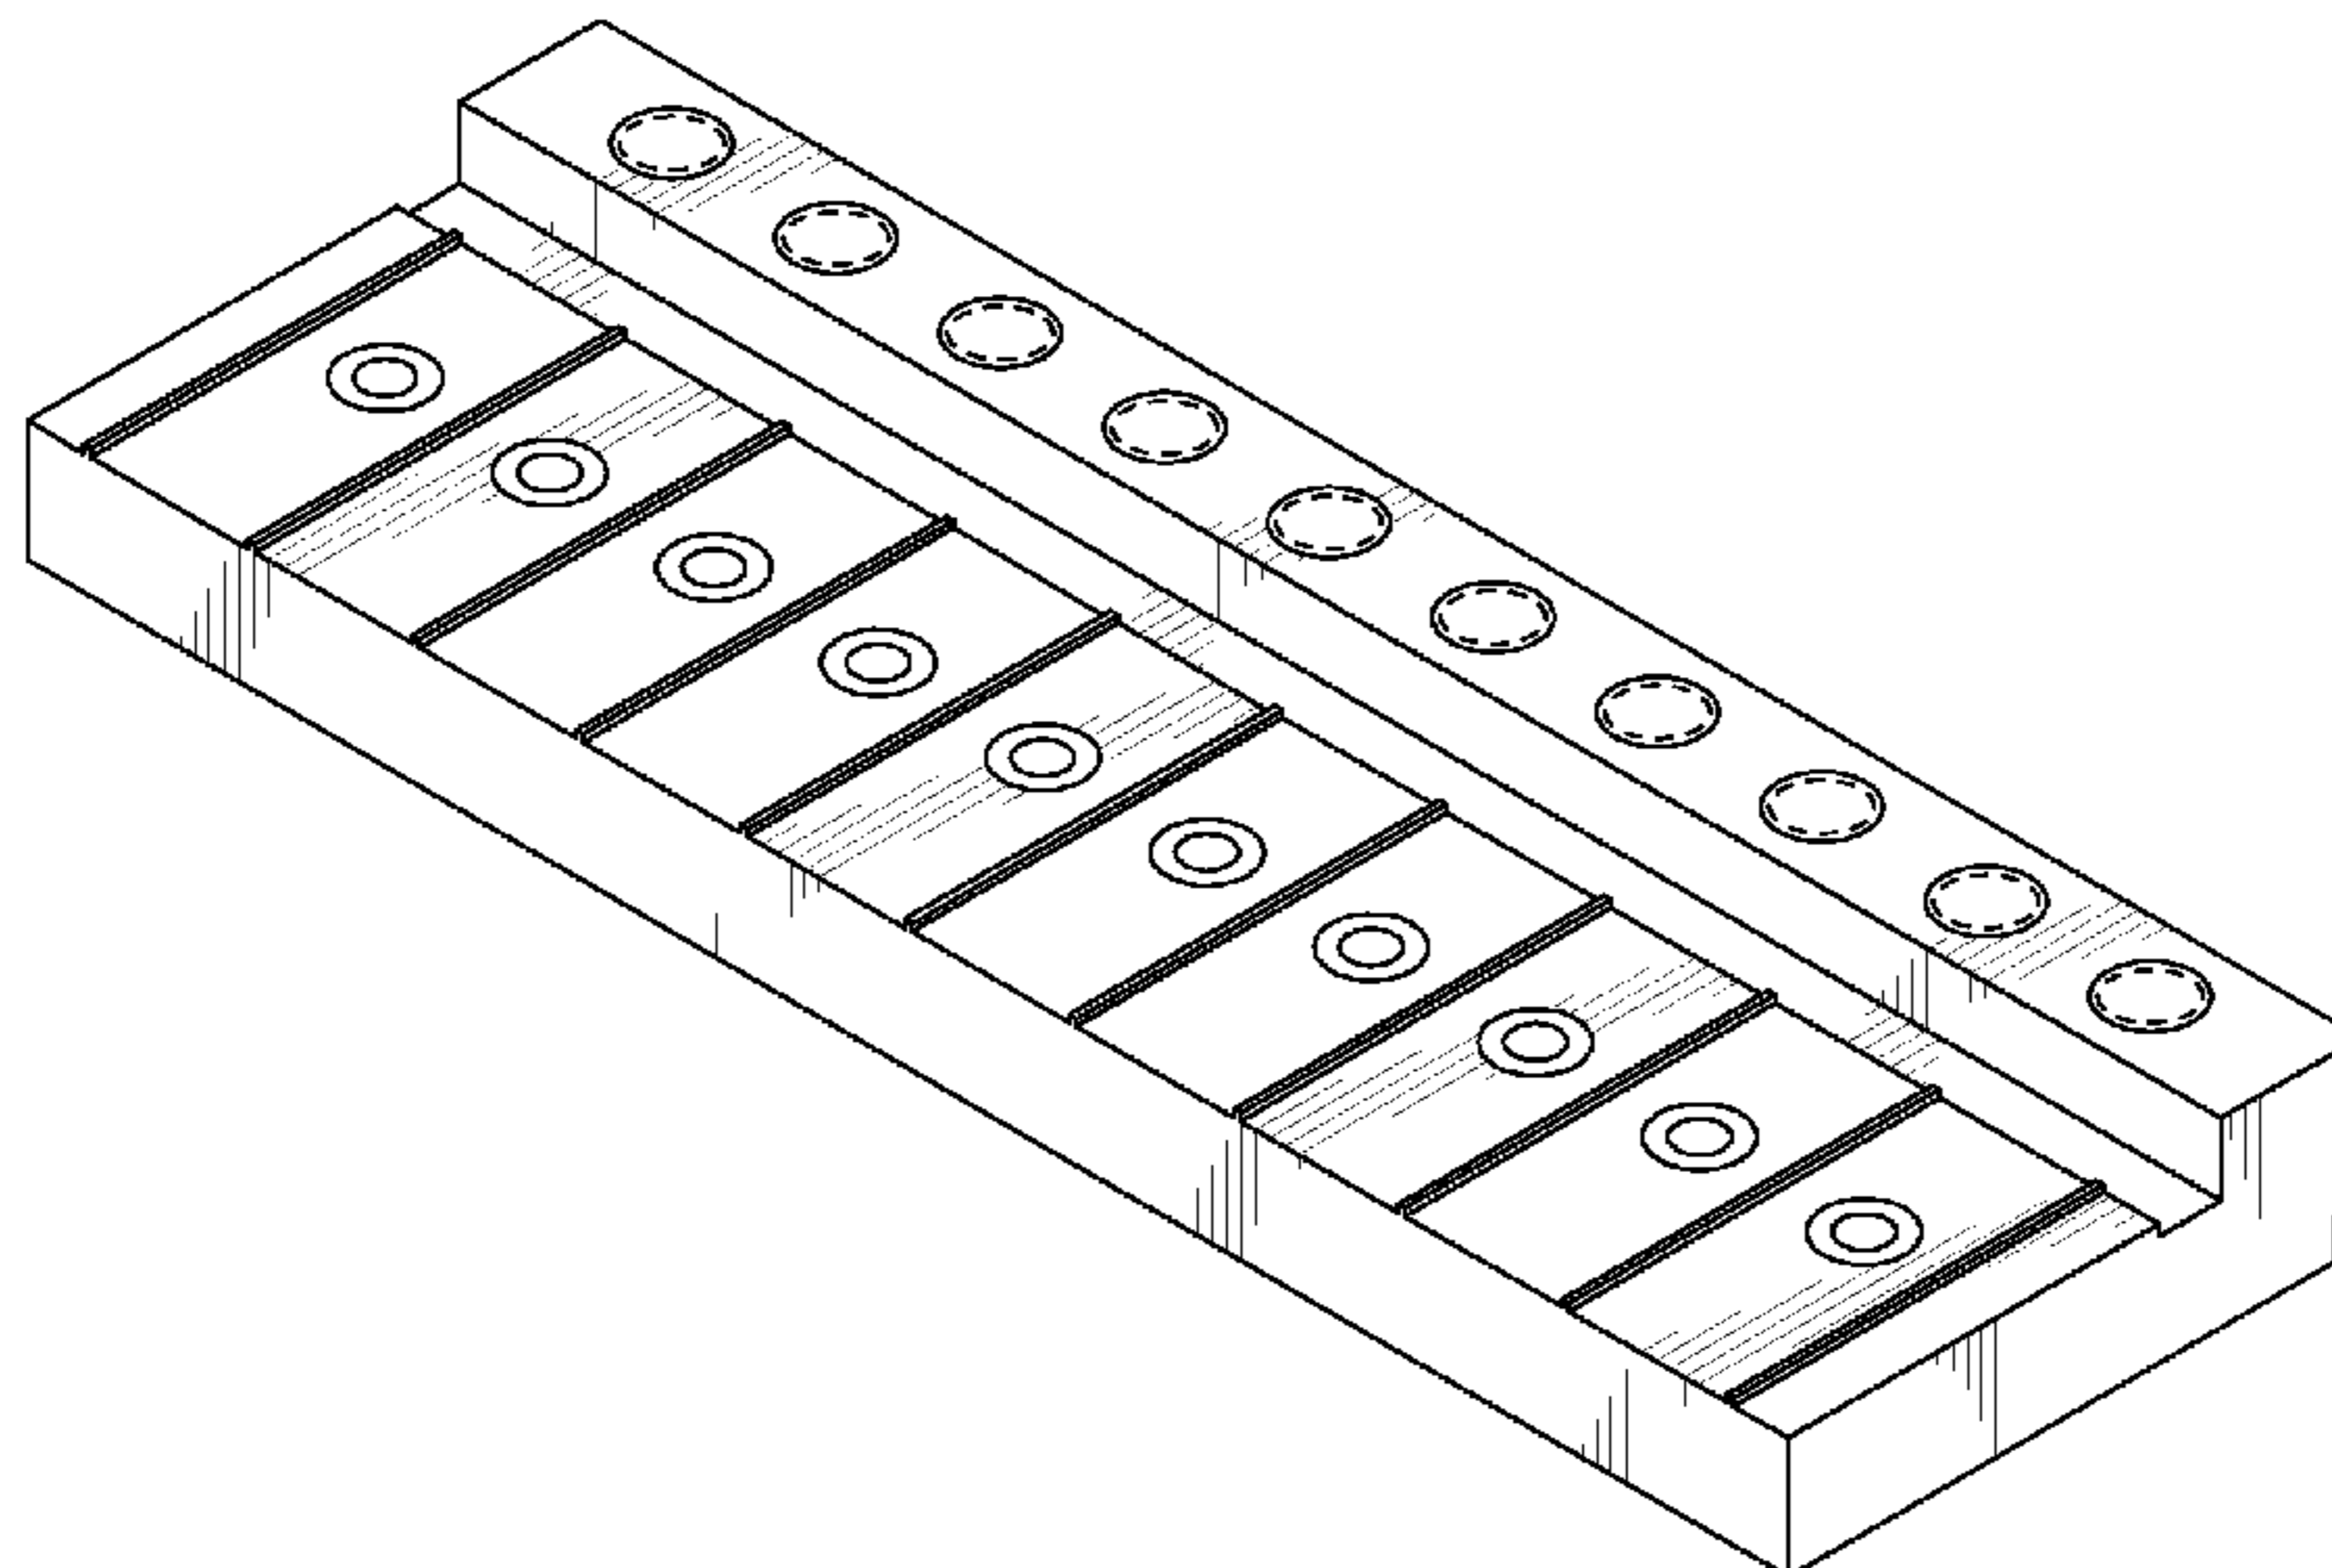

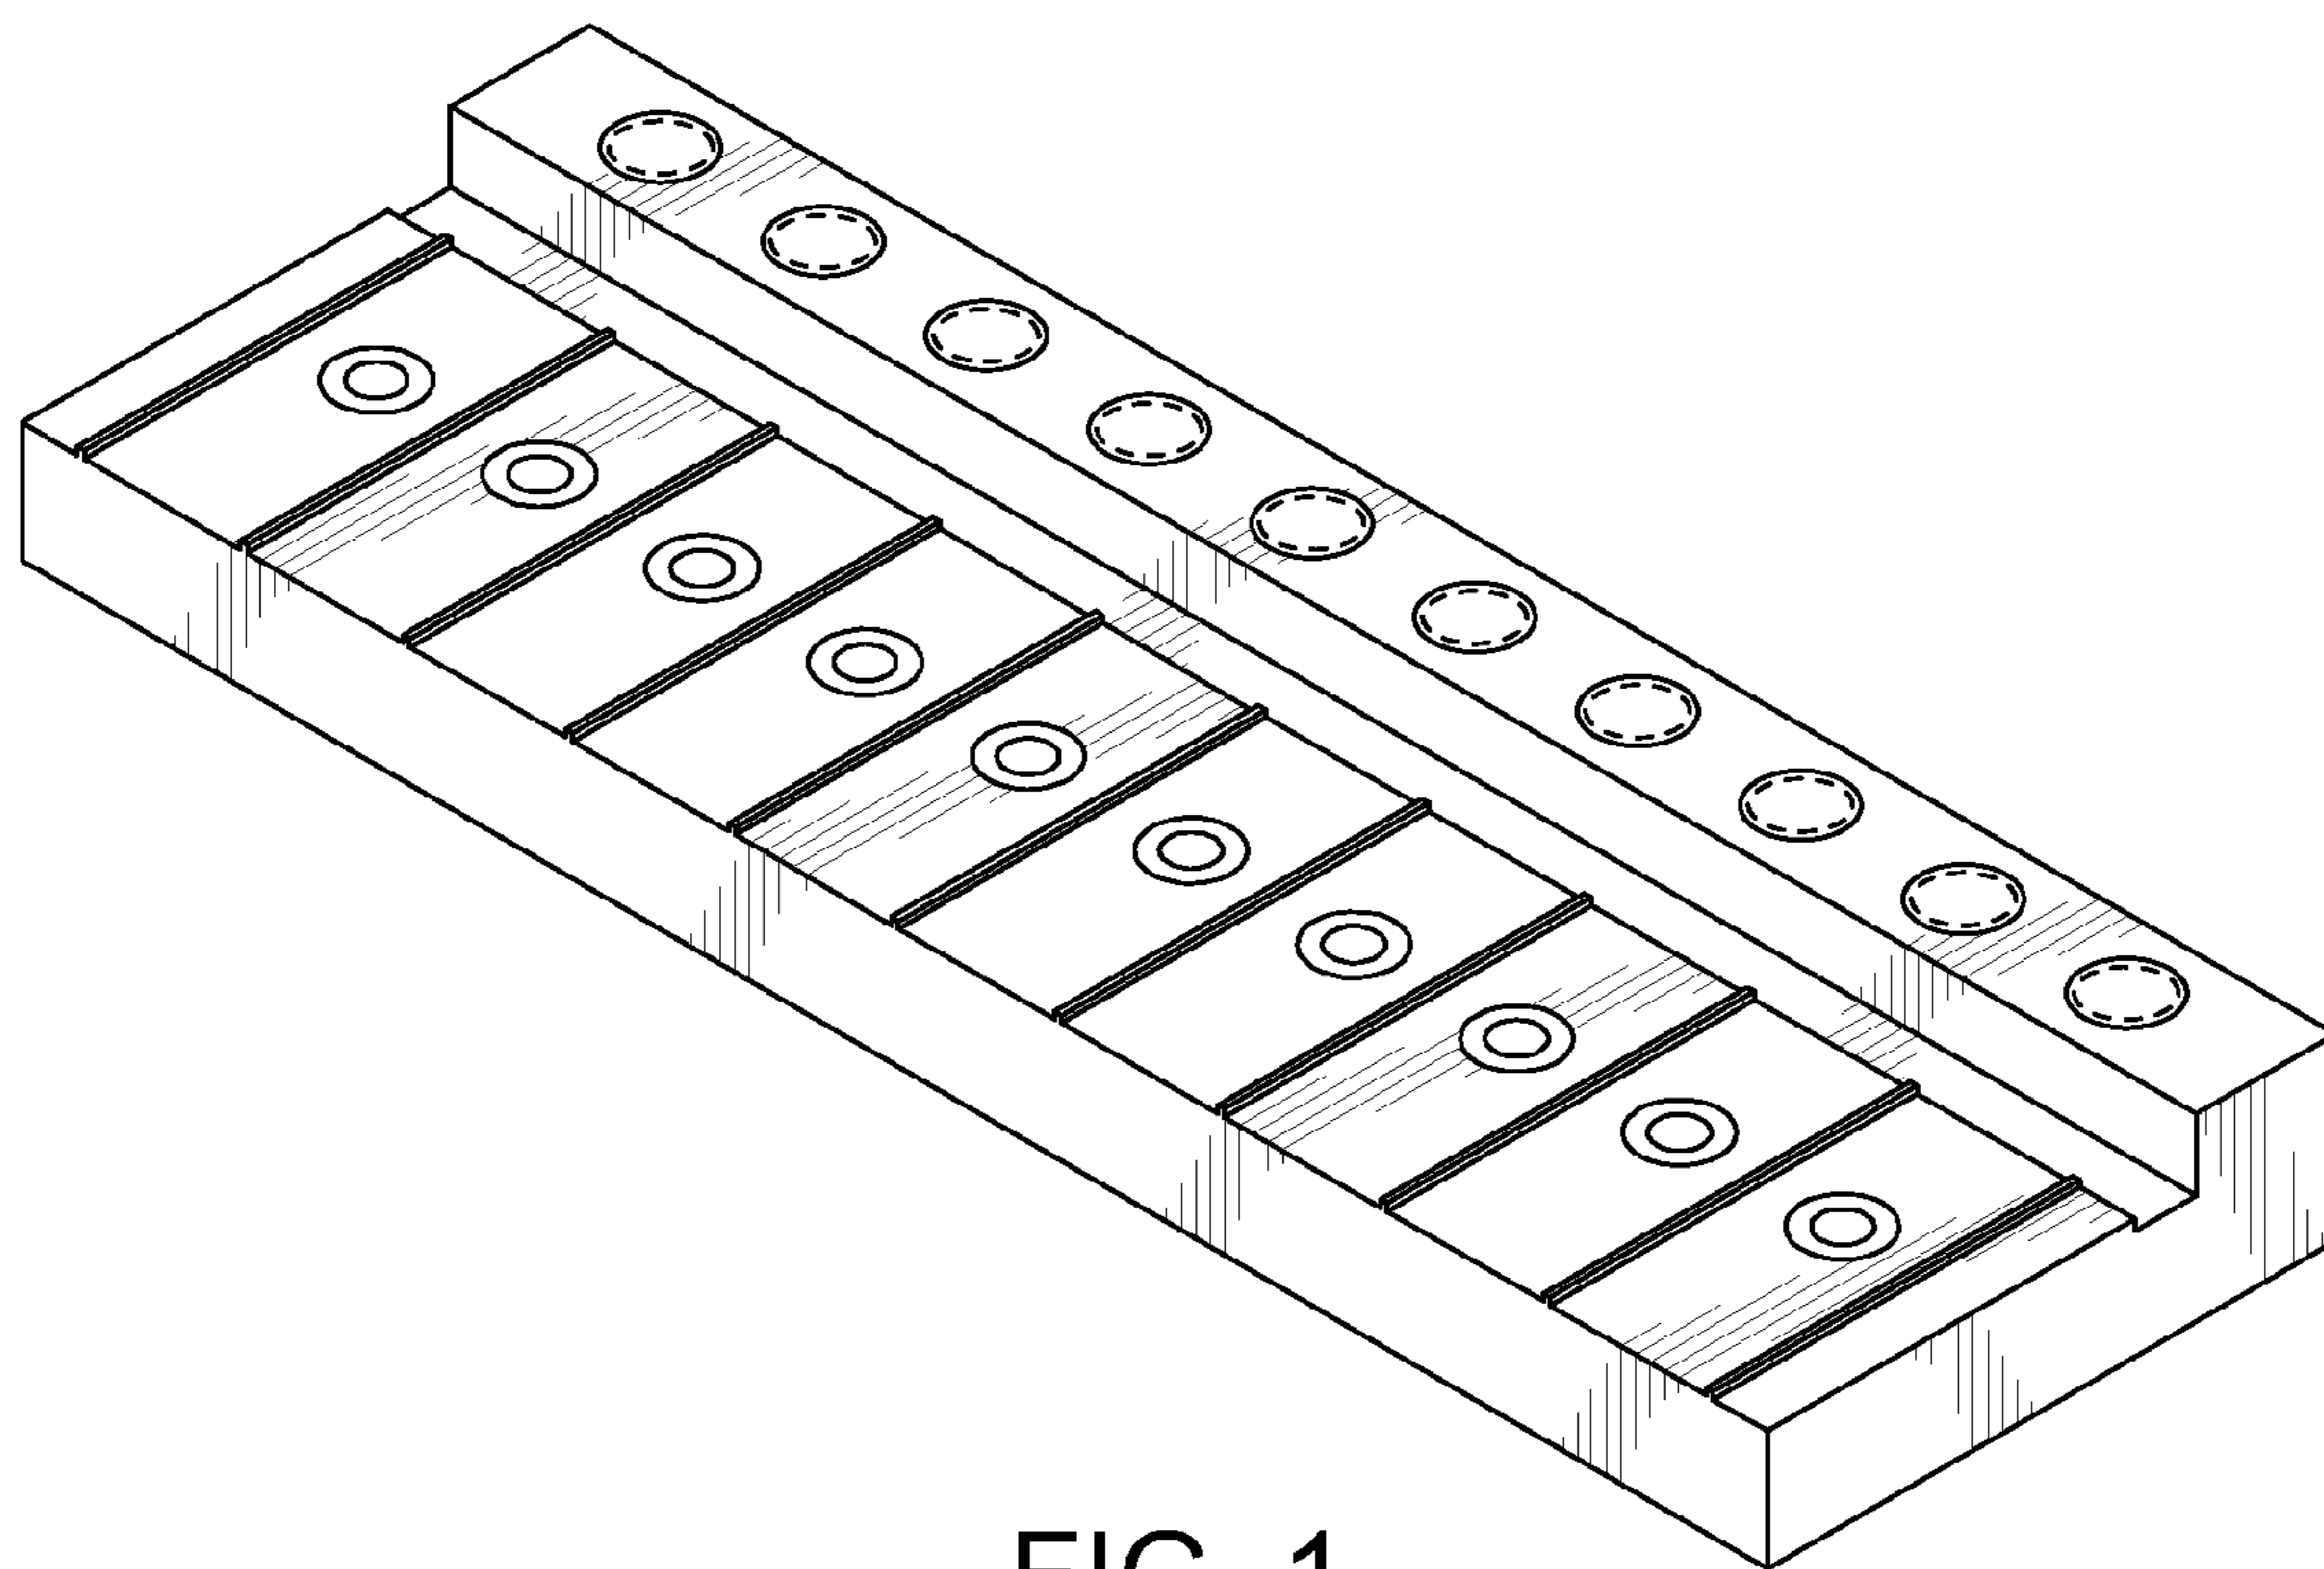


FIG. 1

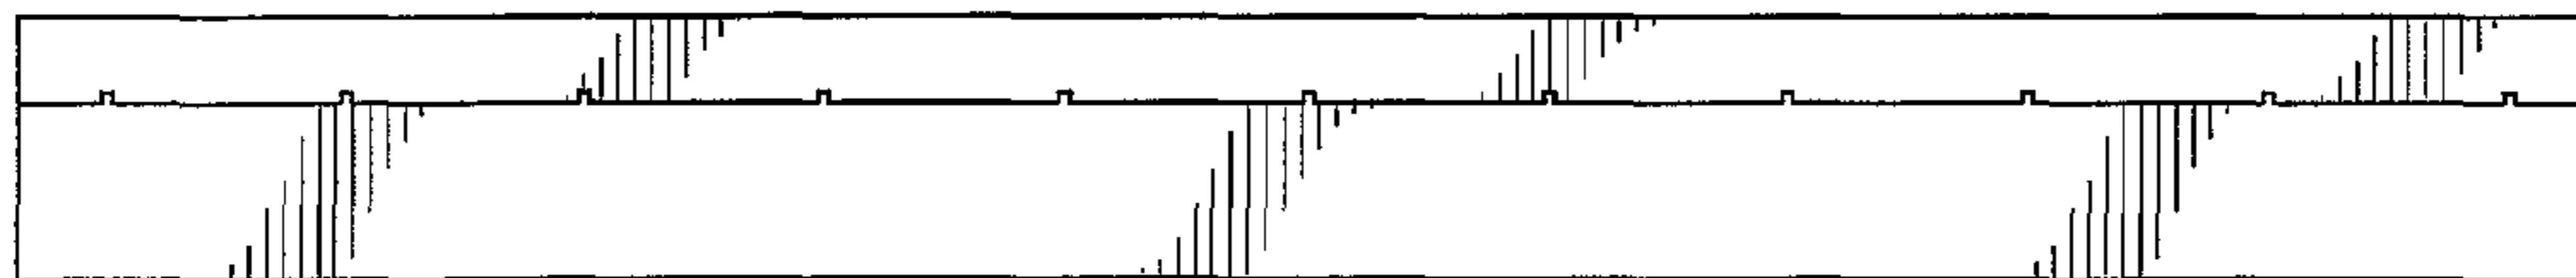


FIG. 2

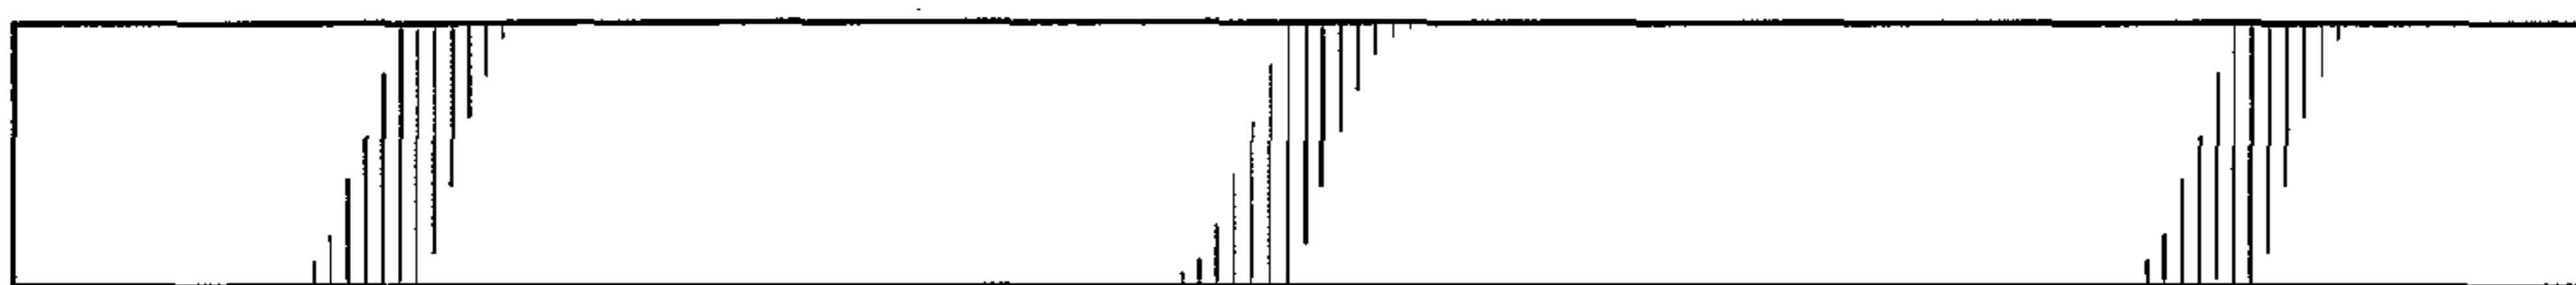


FIG. 3

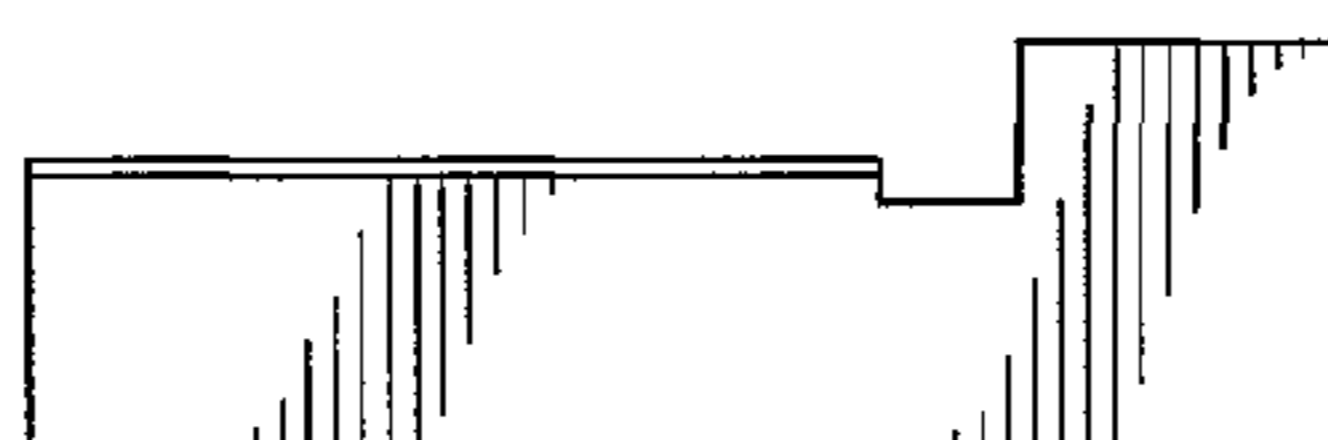


FIG. 4

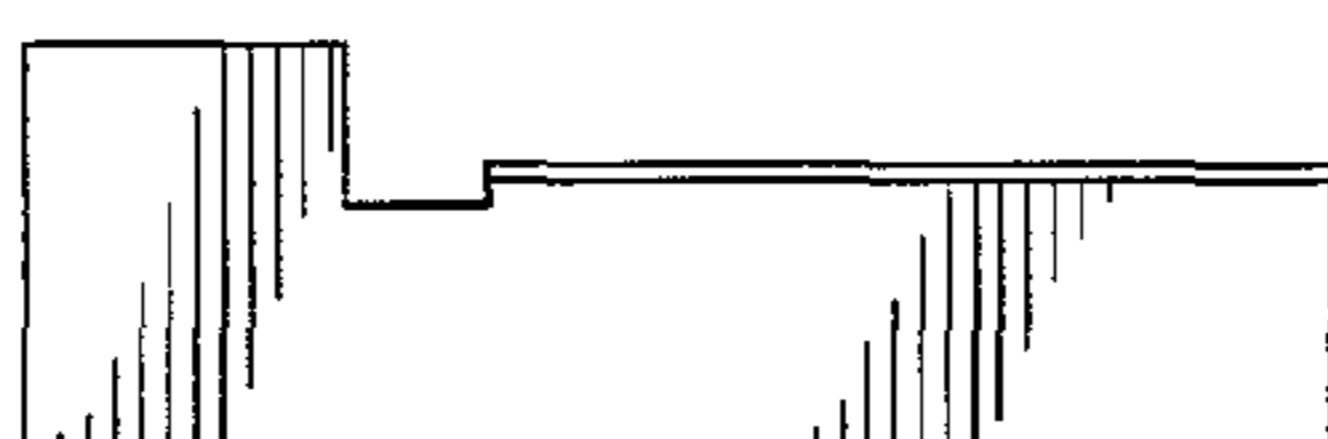


FIG. 5

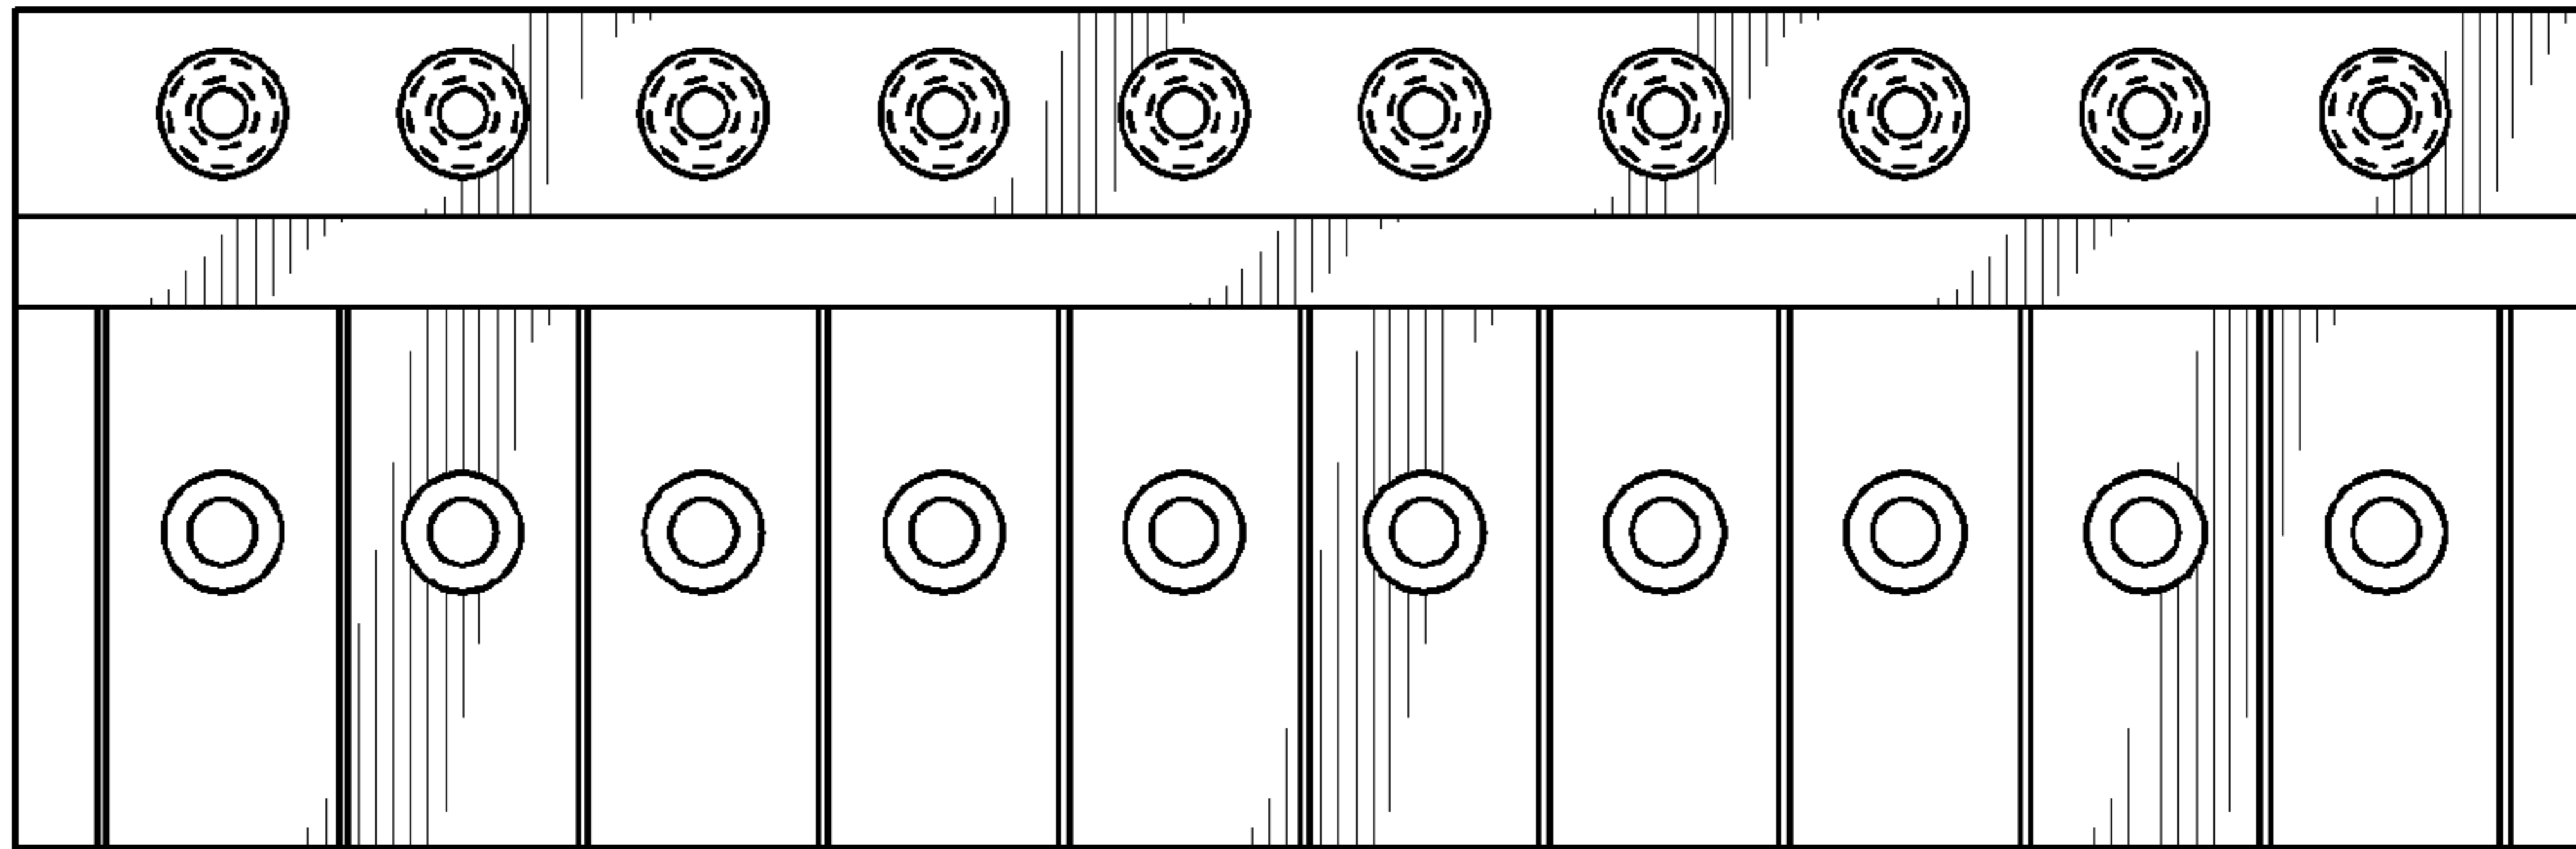


FIG. 6

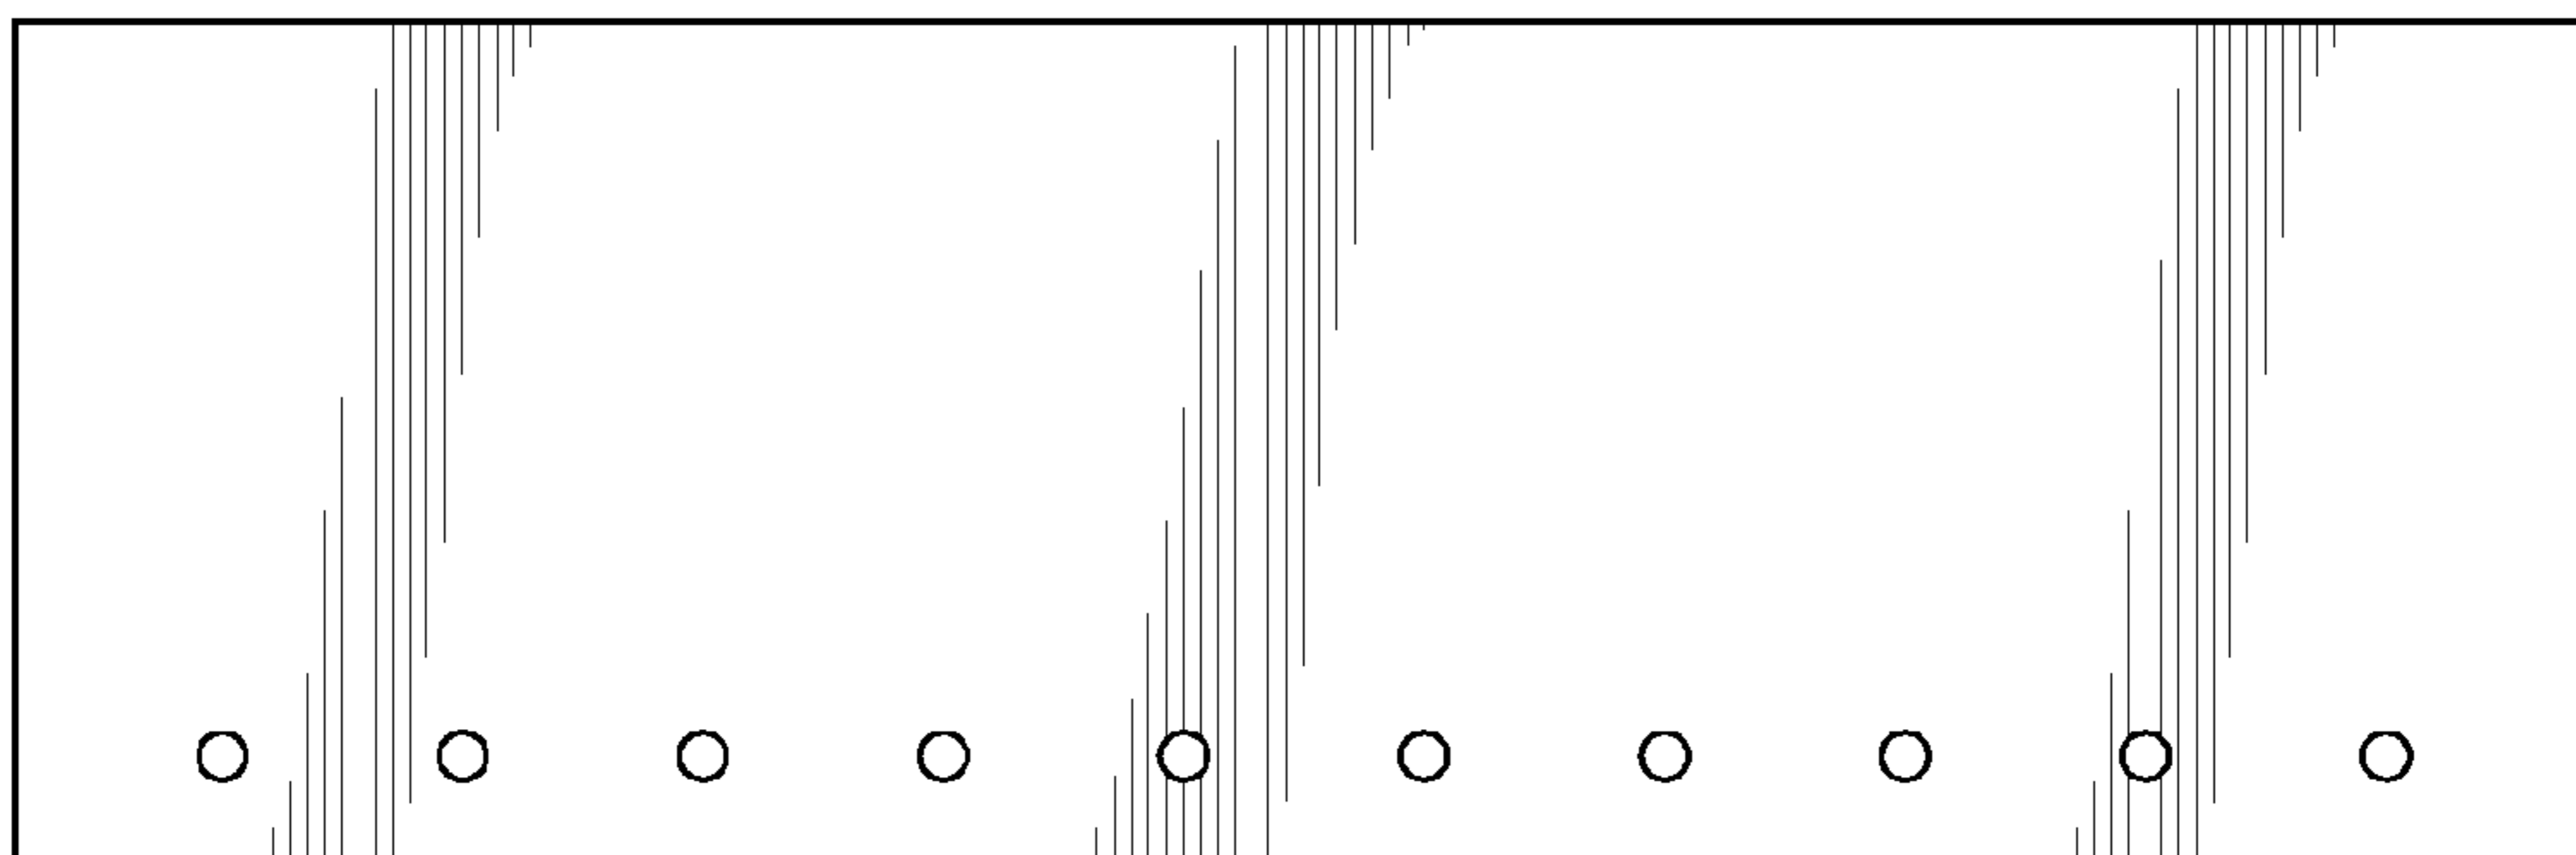


FIG. 7