



US00D621049S

(12) **United States Design Patent**
Takano et al.

(10) **Patent No.:** **US D621,049 S**

(45) **Date of Patent:** **** Aug. 3, 2010**

(54) **GLUCOSE METER**

(75) Inventors: **Hiroshi Takano**, Ehime (JP); **Noriyuki Shinohara**, Ehime (JP); **Carol Reno**, Essex Fells, NJ (US); **Art Oliveira**, Rockaway, NJ (US); **Gerald Shaffer**, Elkhart, IN (US); **Raymond Yao**, Tarrytown, NY (US)

6,458,326 B1 10/2002 Modzelewski
D468,714 S 1/2003 Maruska
D469,107 S 1/2003 Miller
D472,834 S 4/2003 Ueda
D473,310 S 4/2003 Schlagheck
D484,600 S 12/2003 Kaar
D495,418 S 8/2004 Rounds

(Continued)

(73) Assignees: **Panasonic Corporation**, Kadoma-shi (JP); **Bayer Healthcare LLC**, Tarrytown, NY (US)

FOREIGN PATENT DOCUMENTS

JP 986576 S 8/1997

(Continued)

(**) Term: **14 Years**

(21) Appl. No.: **29/320,460**

(22) Filed: **Jun. 27, 2008**

(30) **Foreign Application Priority Data**

Dec. 27, 2007 (JP) 2007-035850

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/169**

(58) **Field of Classification Search** D24/169,
D24/186, 216, 223; D10/81; 600/309, 316,
600/322, 365, 368

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D369,216 S 4/1996 Micinski
D369,864 S 5/1996 Petersen
D371,198 S 6/1996 Savage
D371,440 S 7/1996 Petersen
5,605,837 A 2/1997 Karimi
D406,895 S * 3/1999 Byrd et al. D24/169
D424,696 S * 5/2000 Ray et al. D24/169
D429,527 S 8/2000 Bolam
D440,312 S 4/2001 Bertrand
D452,564 S 12/2001 Micinski
D456,514 S 4/2002 Brown
D460,557 S 7/2002 Steinberg
D460,823 S 7/2002 Steinberg

OTHER PUBLICATIONS

Official Action (Enquiry) from the Patent Office of The Russian Federation dated Jul. 6, 2008, issued in corresponding Russian Application No. 2007502010, filed Jul. 6, 2007.

Primary Examiner—T. Chase Nelson

Assistant Examiner—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Christensen O'Connor Johnson Kindness PLLC

(57) **CLAIM**

The ornamental design for a glucose meter, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the front, right side and bottom of a glucose meter showing our new design;

FIG. 2 is a perspective view of the rear, left side and top thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a rear view thereof;


FIG. 5 is a left side view thereof;

FIG. 6 is a right side view thereof;

FIG. 7 is a top plan view thereof; and,

FIG. 8 is a bottom view thereof.

1 Claim, 3 Drawing Sheets

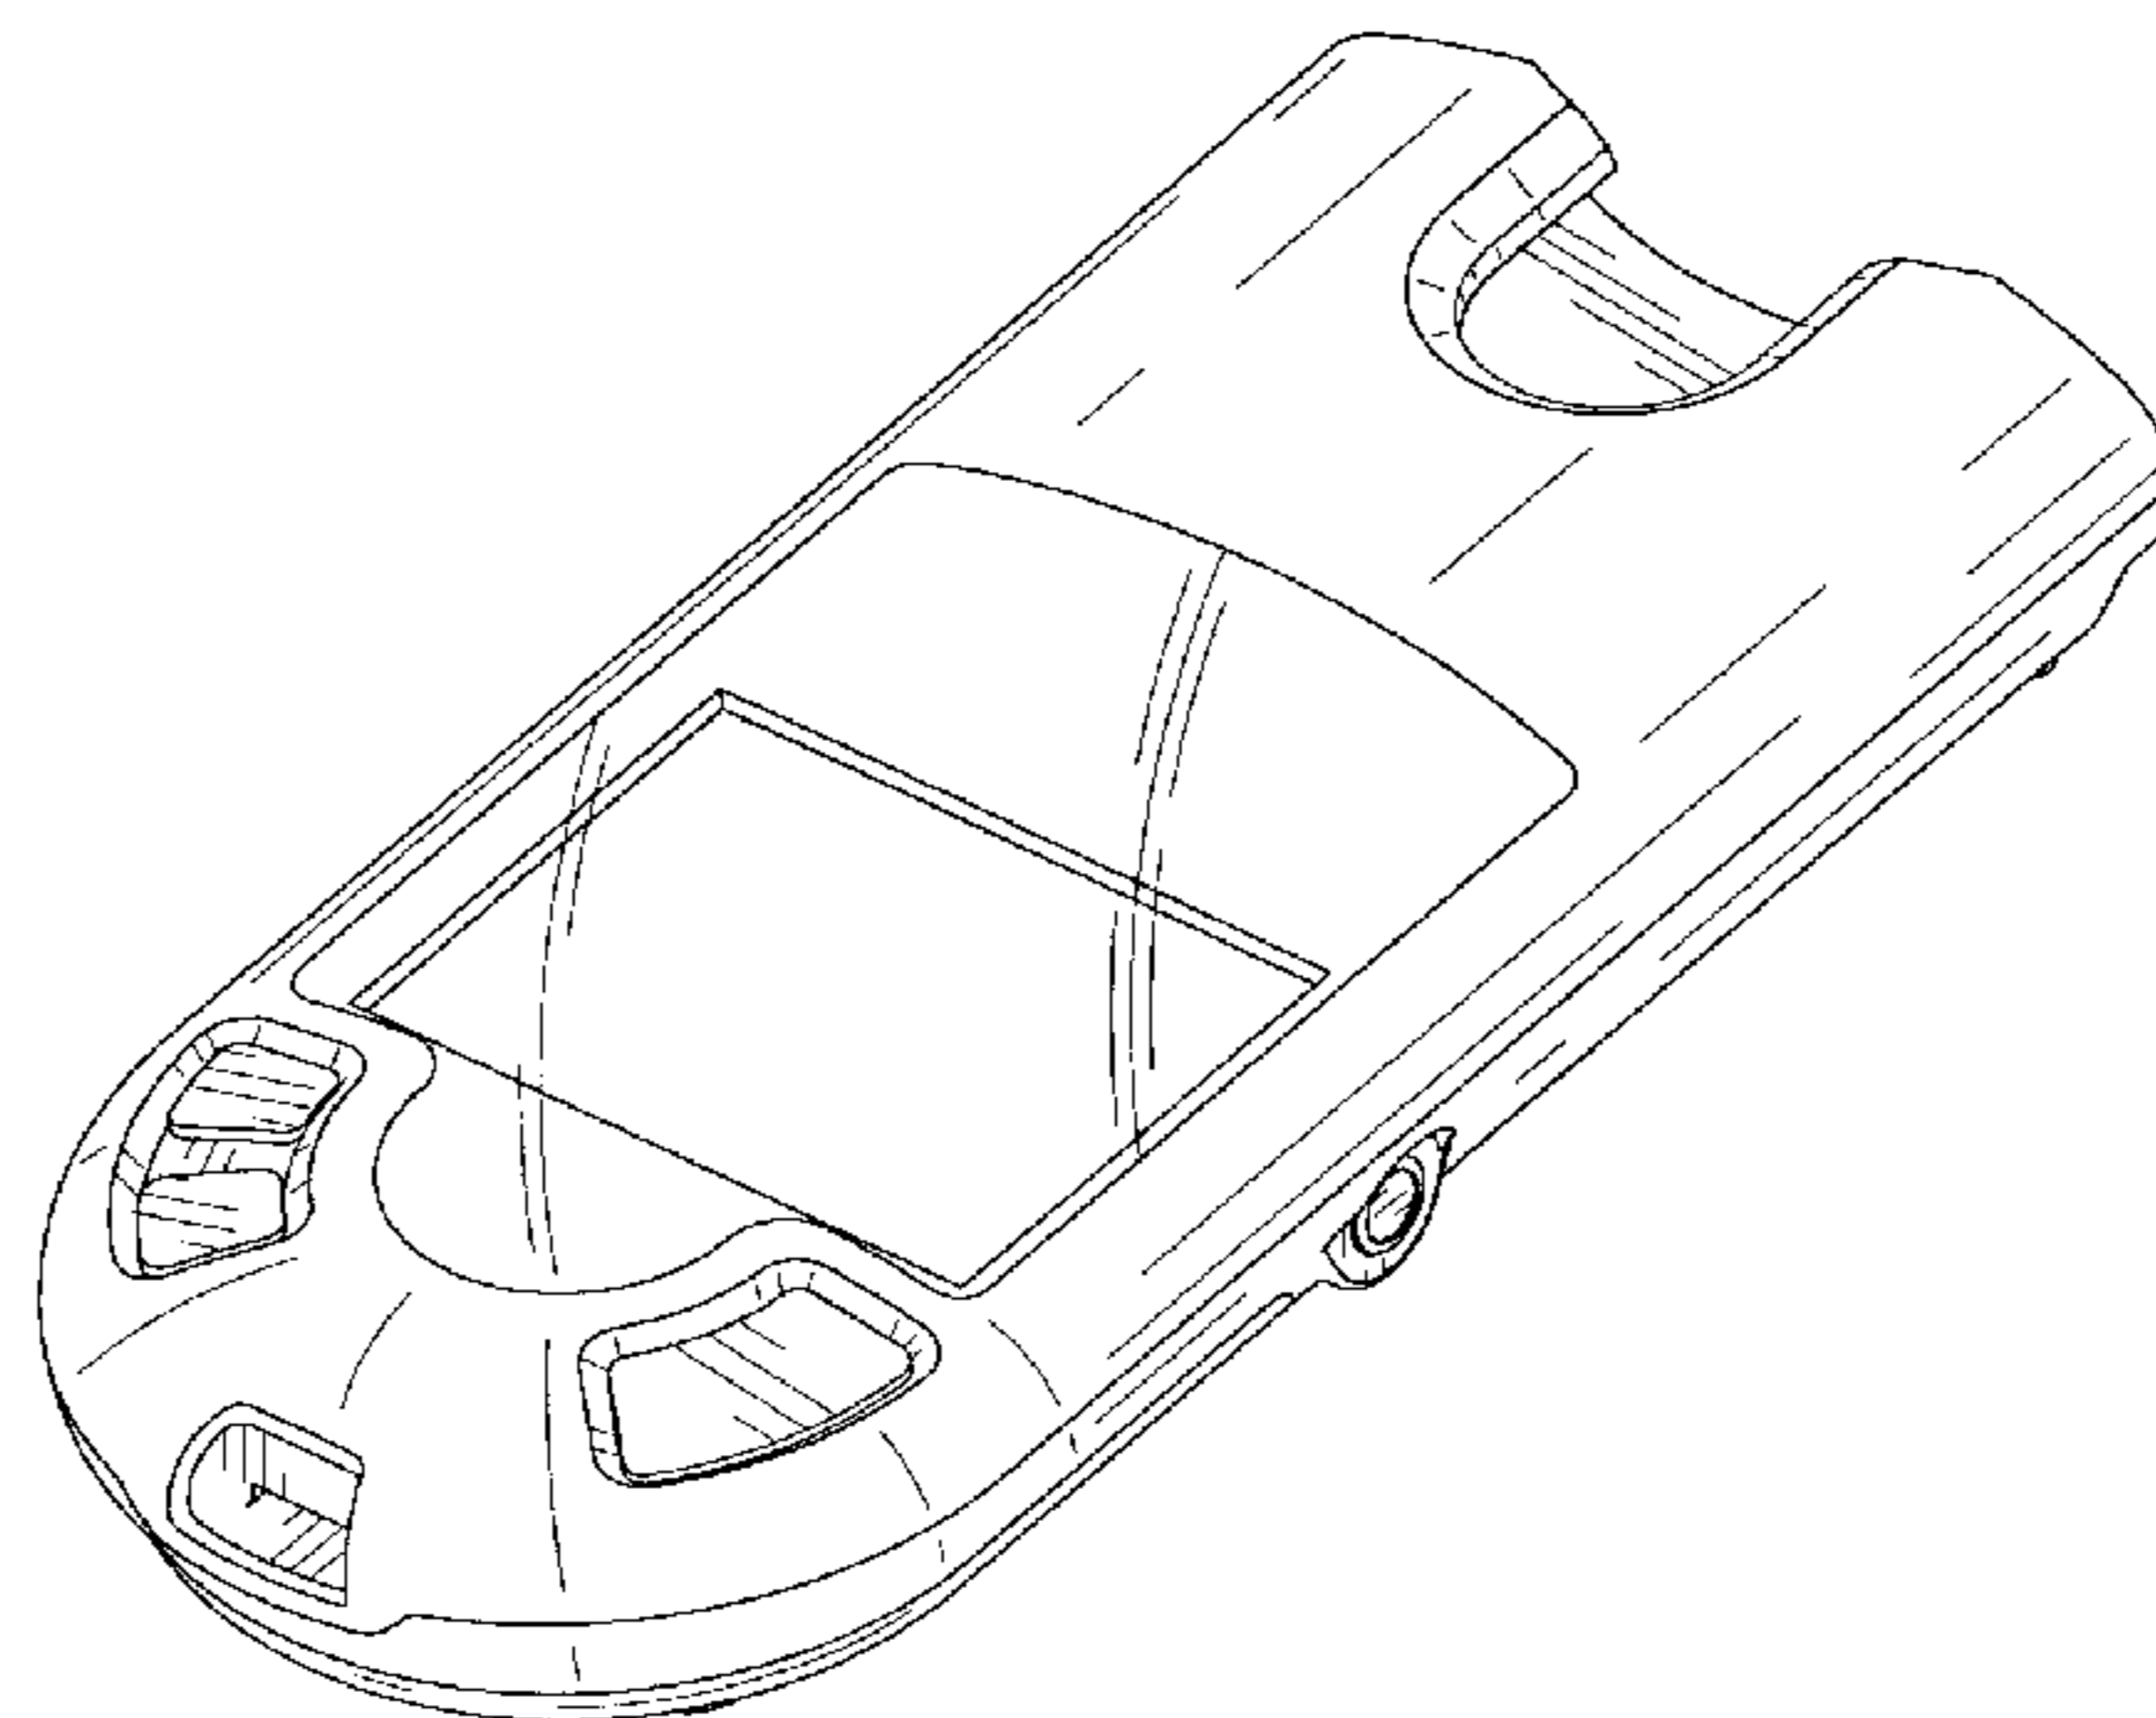

US D621,049 S

Page 2

U.S. PATENT DOCUMENTS

D496,461 S 9/2004 Neel
D502,654 S 3/2005 Nishiura
D522,656 S 6/2006 Orr
D534,444 S * 1/2007 Wallace D10/78
7,181,350 B2 2/2007 Oberding
D545,436 S * 6/2007 Padain D24/169
D546,456 S 7/2007 May
7,241,265 B2 7/2007 Cummings
D548,347 S 8/2007 Ichino
D551,350 S * 9/2007 Lorimer et al. D24/186
D555,021 S 11/2007 Rounds
D562,458 S * 2/2008 Padain D24/169
2003/0223906 A1 12/2003 McAllister
2006/0182658 A1 8/2006 Wu

FOREIGN PATENT DOCUMENTS

JP 987768 S 8/1997
JP 1060640 S 2/2000
JP 1060644 S 2/2000
JP 1109739 S 5/2001
JP 1111904 S 6/2001
JP D1145580 S 7/2002
JP D1145581 S 7/2002
JP 1171179 S 4/2003
JP 1171182 S 4/2003

JP 1171284 S 4/2003
JP 1191803 S 12/2003
JP D1192909 S 12/2003
JP D1192910 S 12/2003
JP D1192911 S 12/2003
JP D1192912 S 12/2003
JP D1192913 S 12/2003
JP D1192914 S 12/2003
JP 1193467 S 1/2004
JP 1224545 S 12/2004
JP 1255662 S 11/2005
JP 1256776 S 11/2005
JP 1269215 S 4/2006
JP 1292283 S 1/2007
JP 1301304 S 5/2007
JP 1301943 S 5/2007
JP D1206918 S 5/2007
JP D1206919 S 5/2007
JP D1206920 S 5/2007
JP D1206921 S 5/2007
JP D1206922 S 5/2007
JP D1206923 S 5/2007
JP D1145566 S 7/2007
JP 1312669 S 10/2007
JP D1316848 S 12/2007
JP D1316849 S 12/2007

* cited by examiner

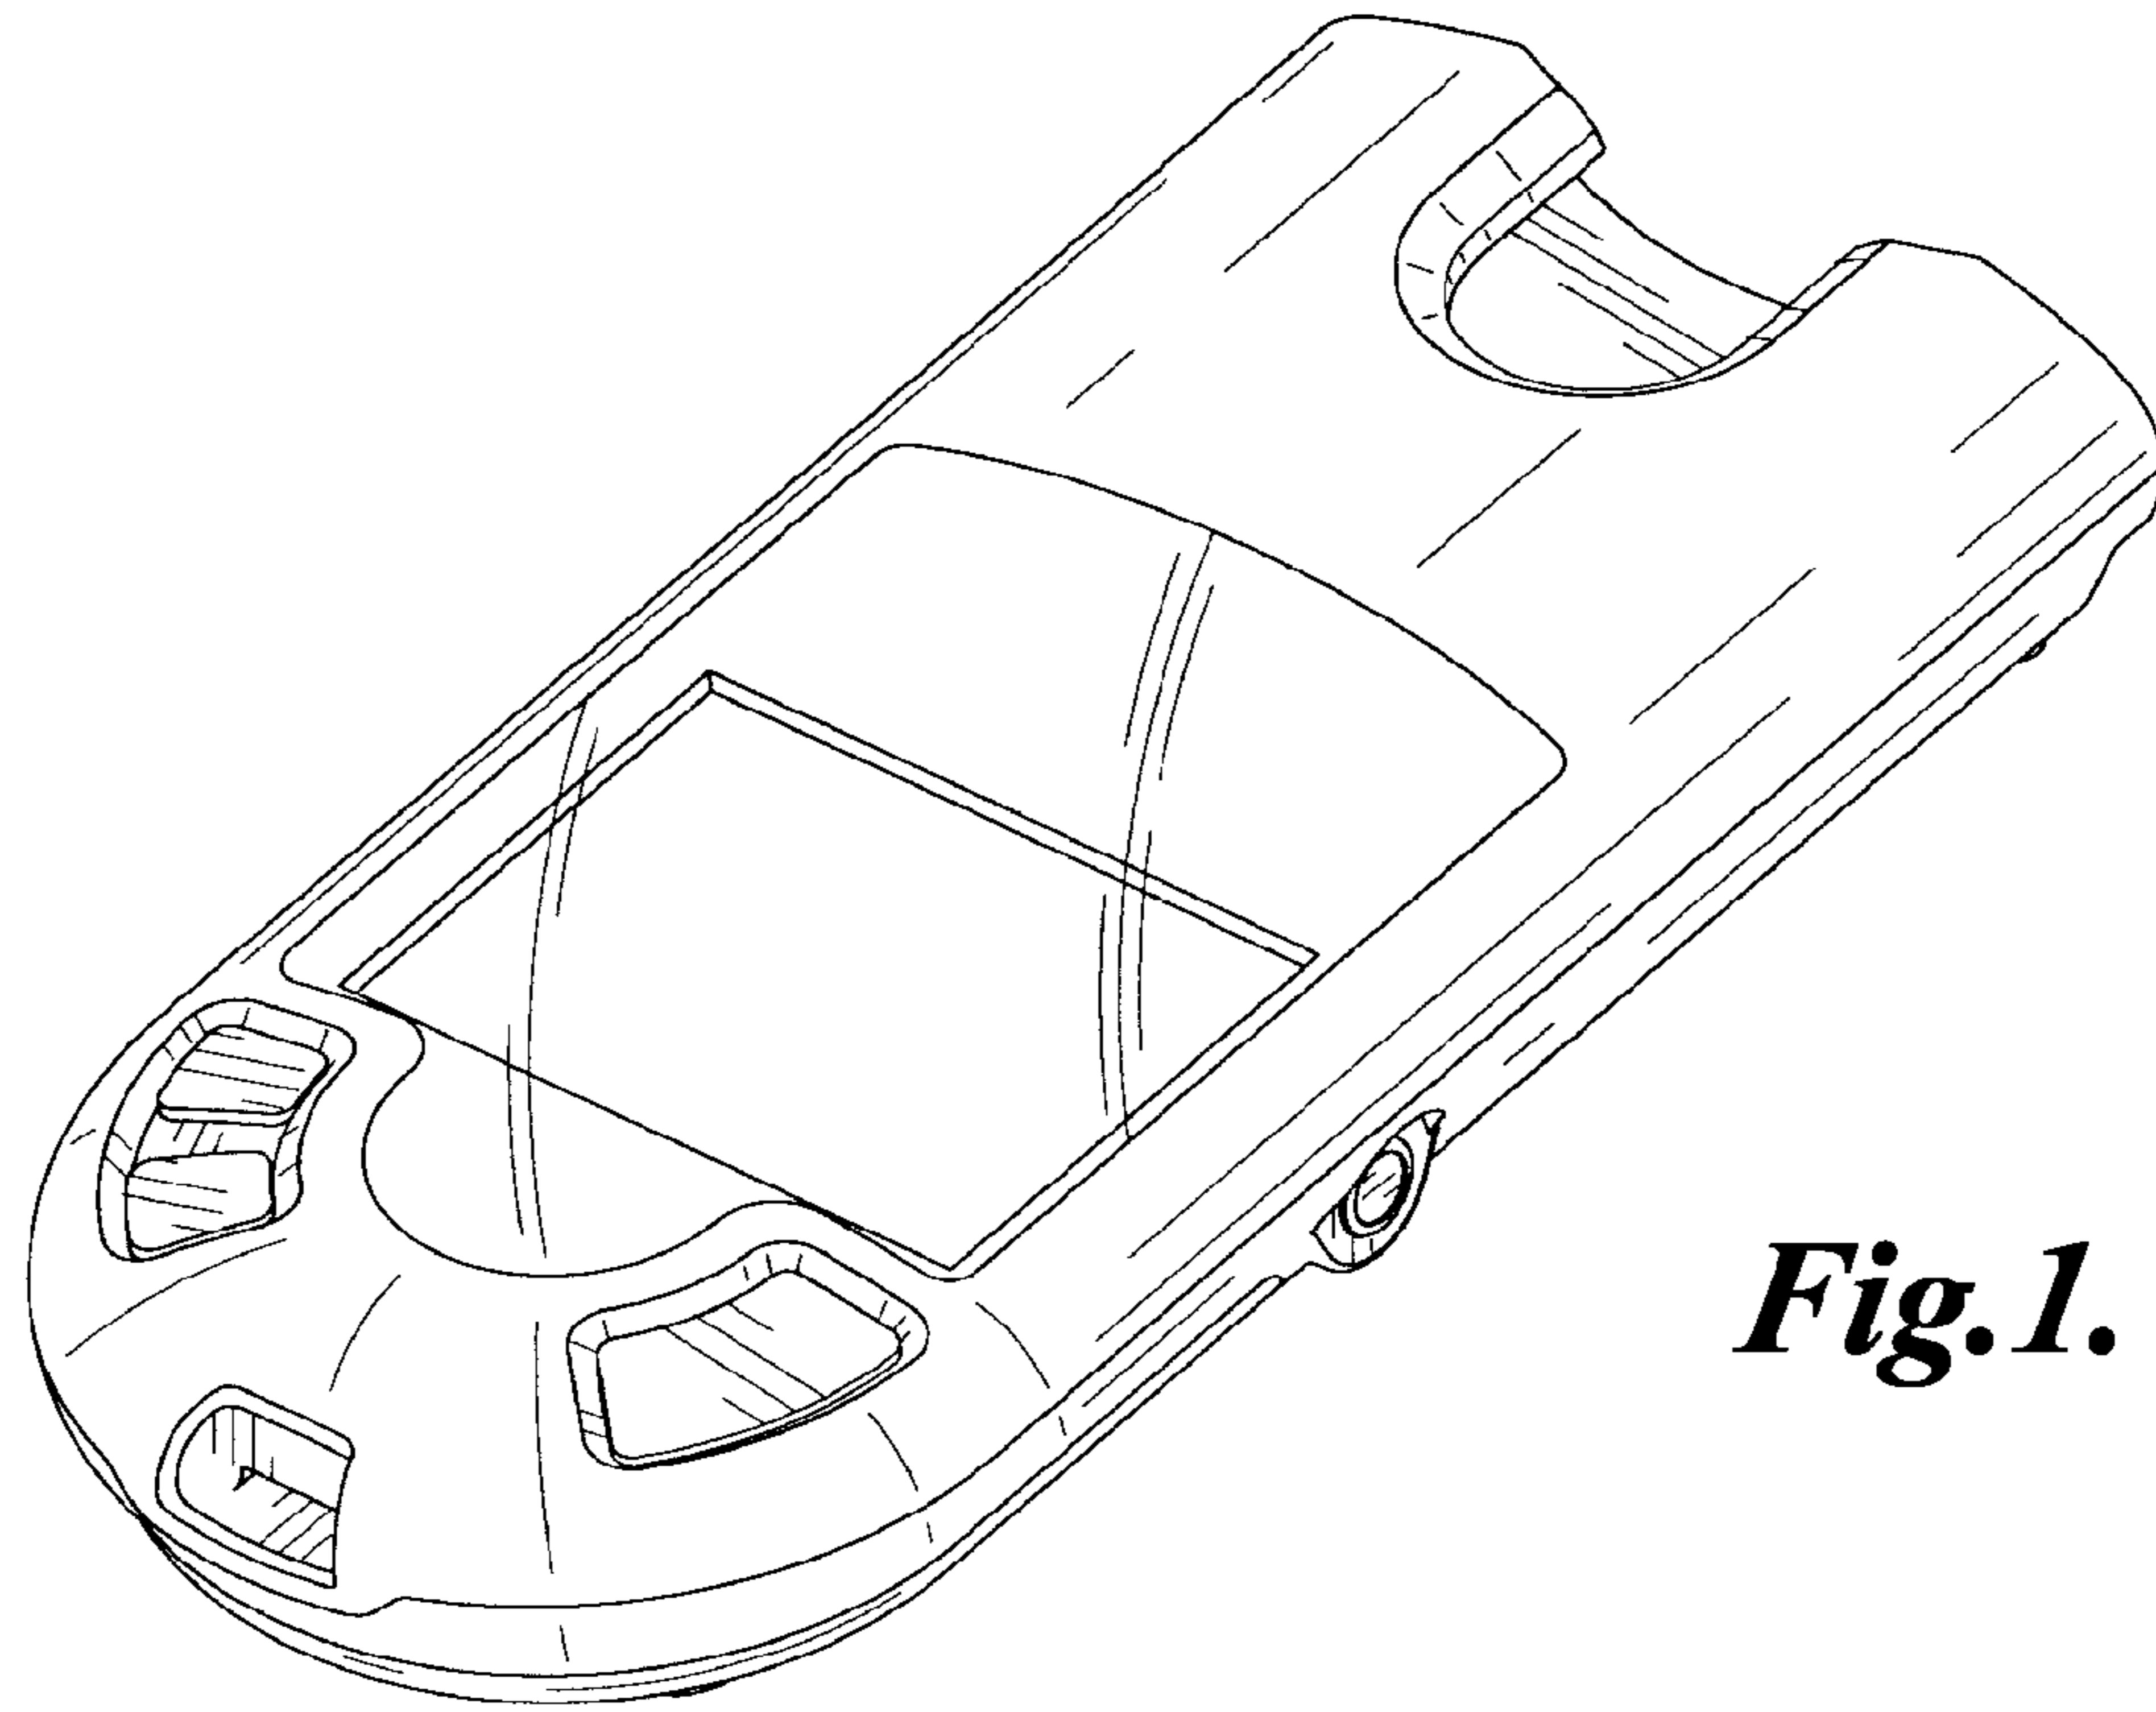


Fig. 1.

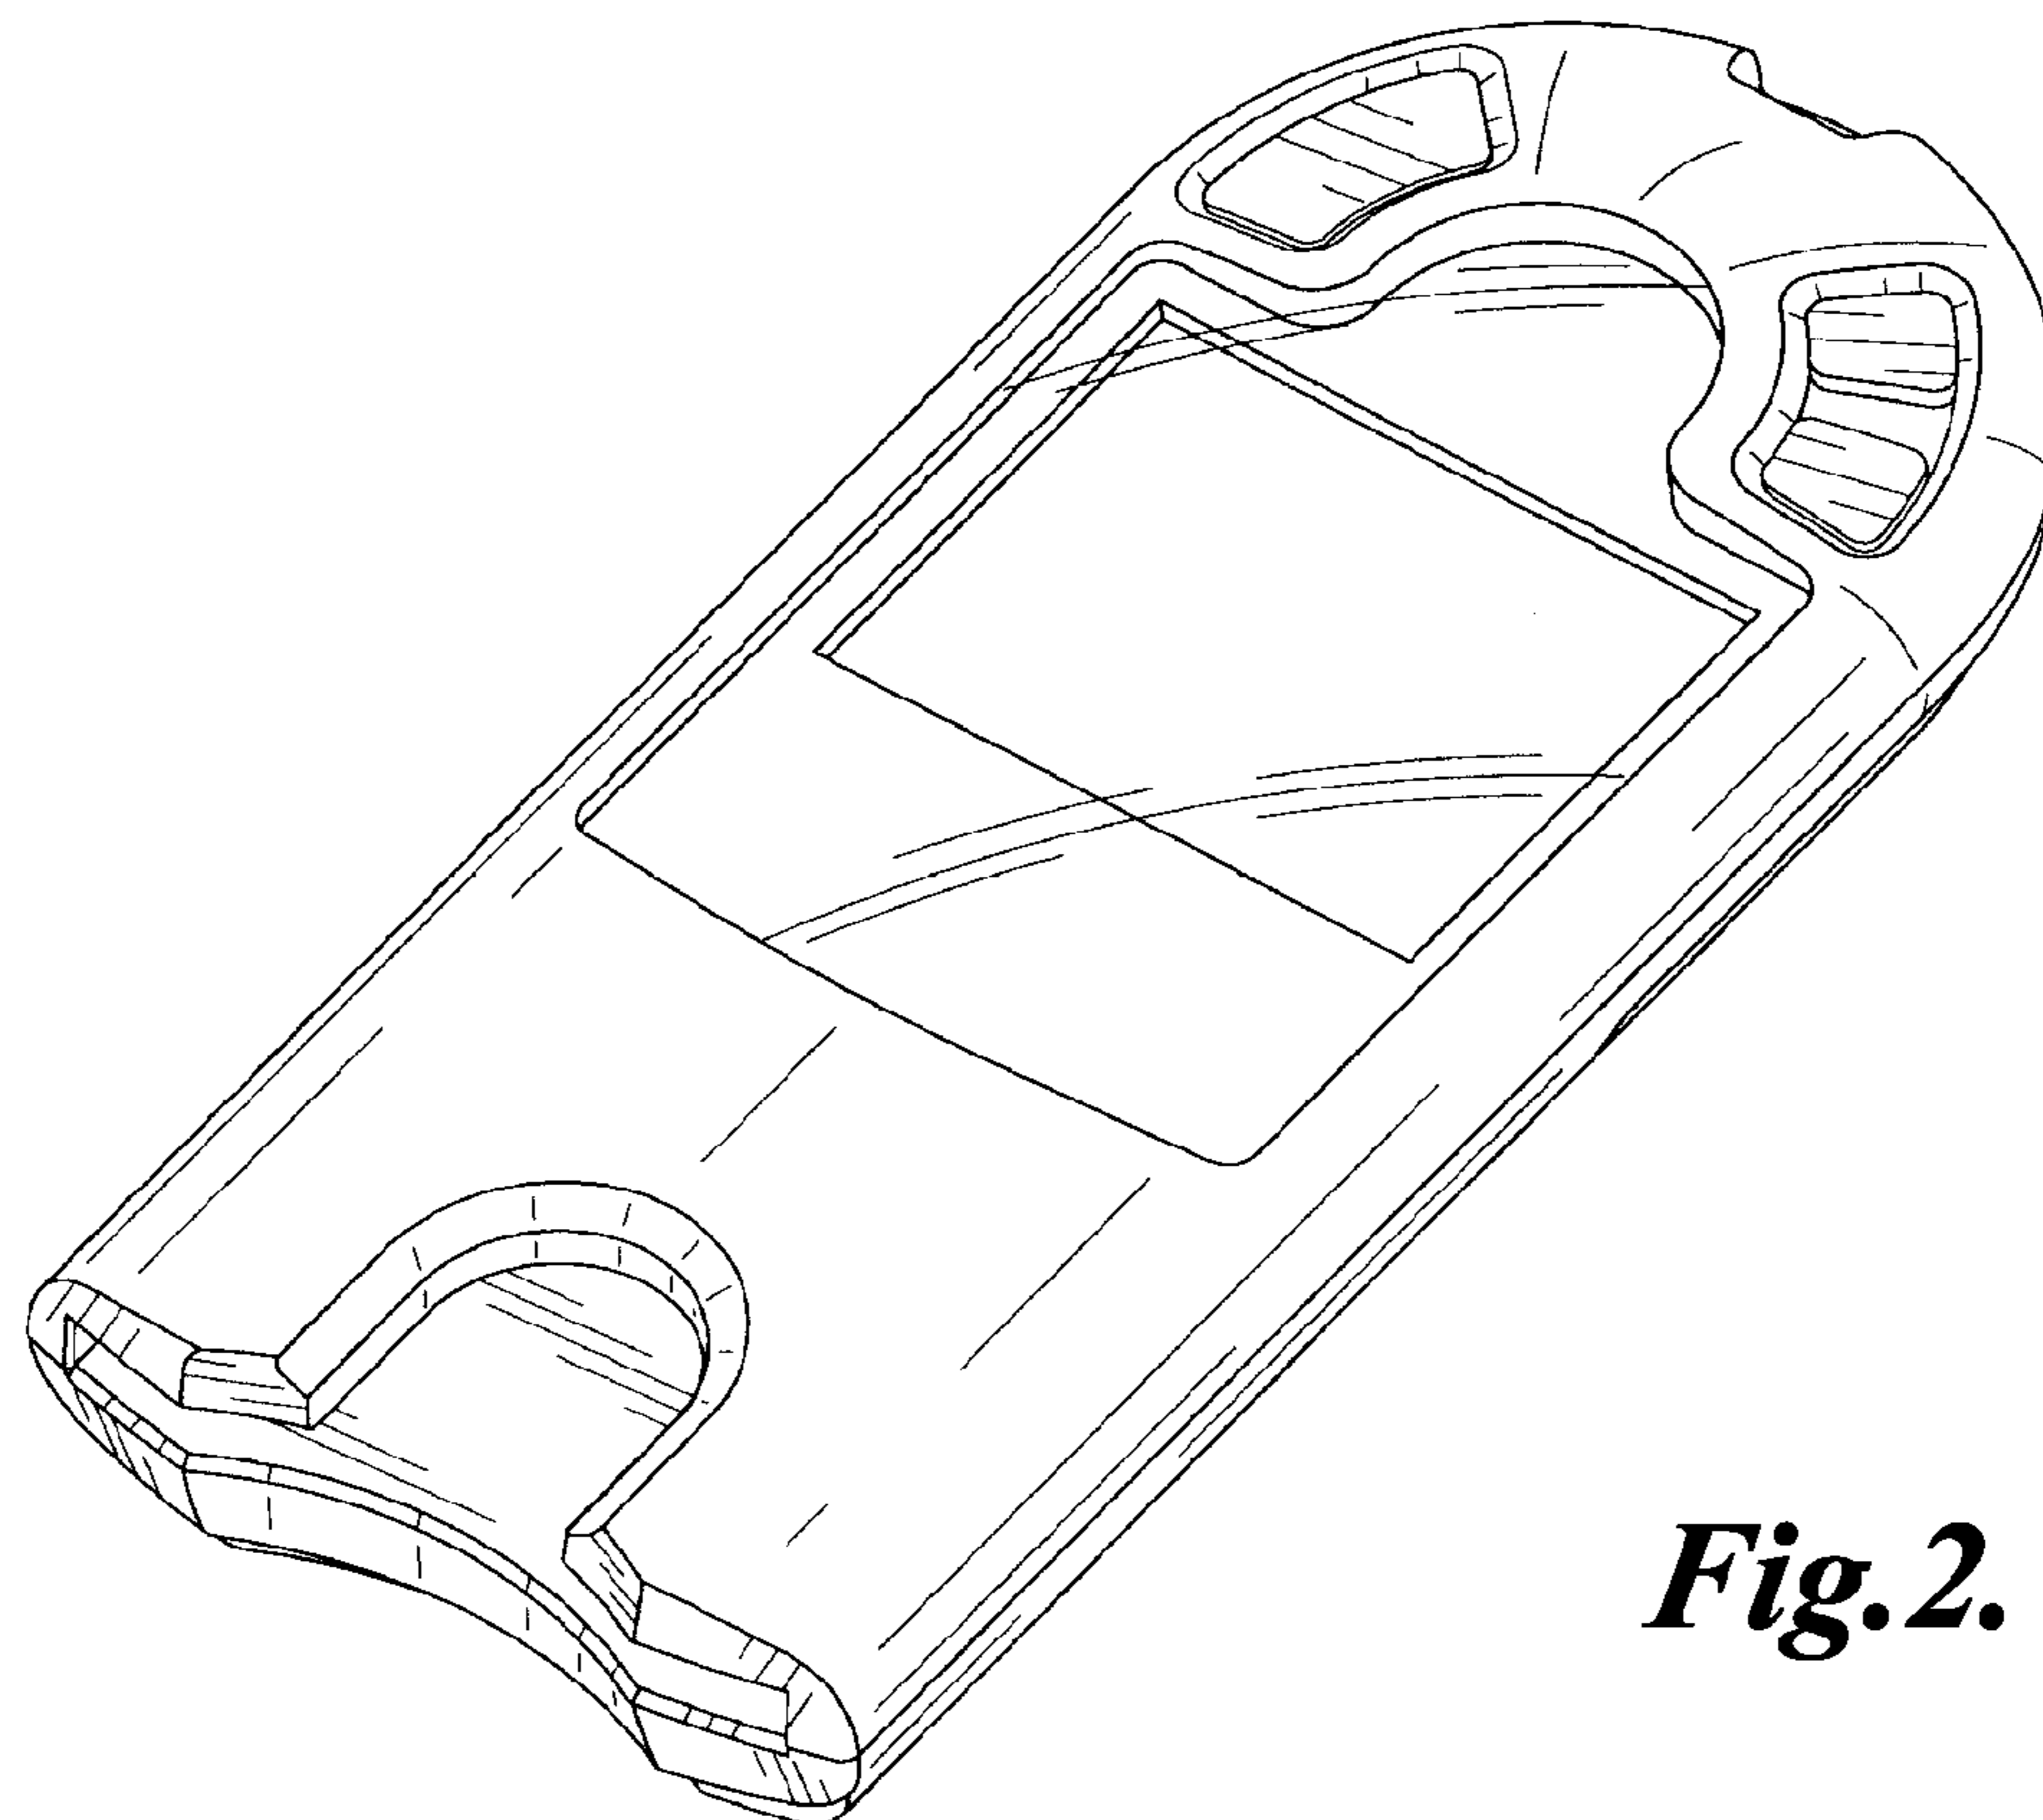


Fig. 2.

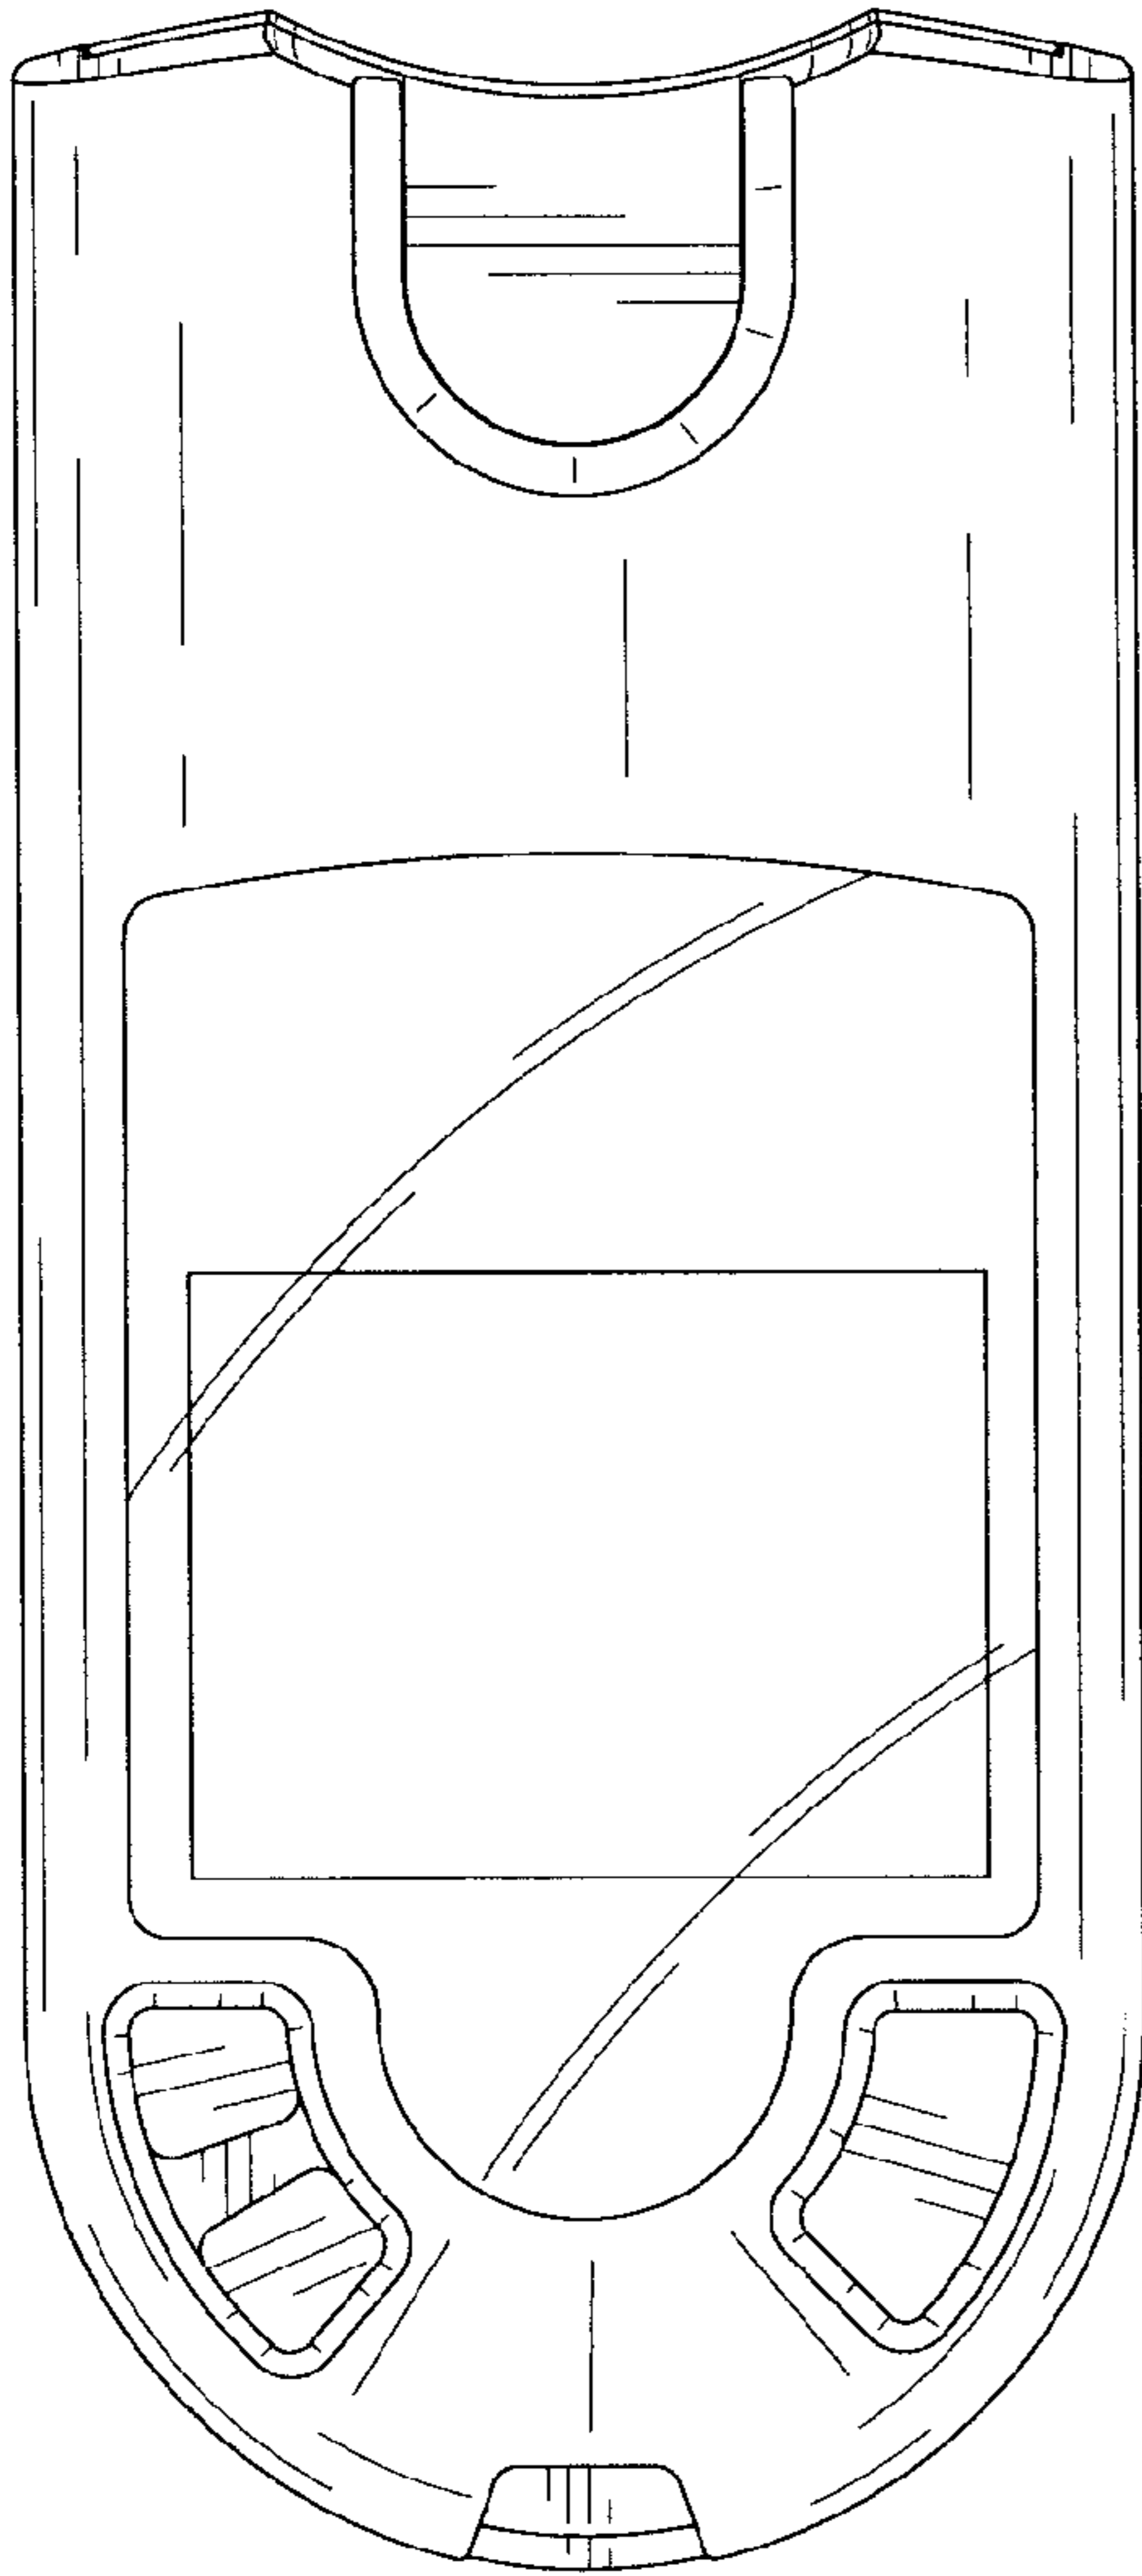


Fig.3.

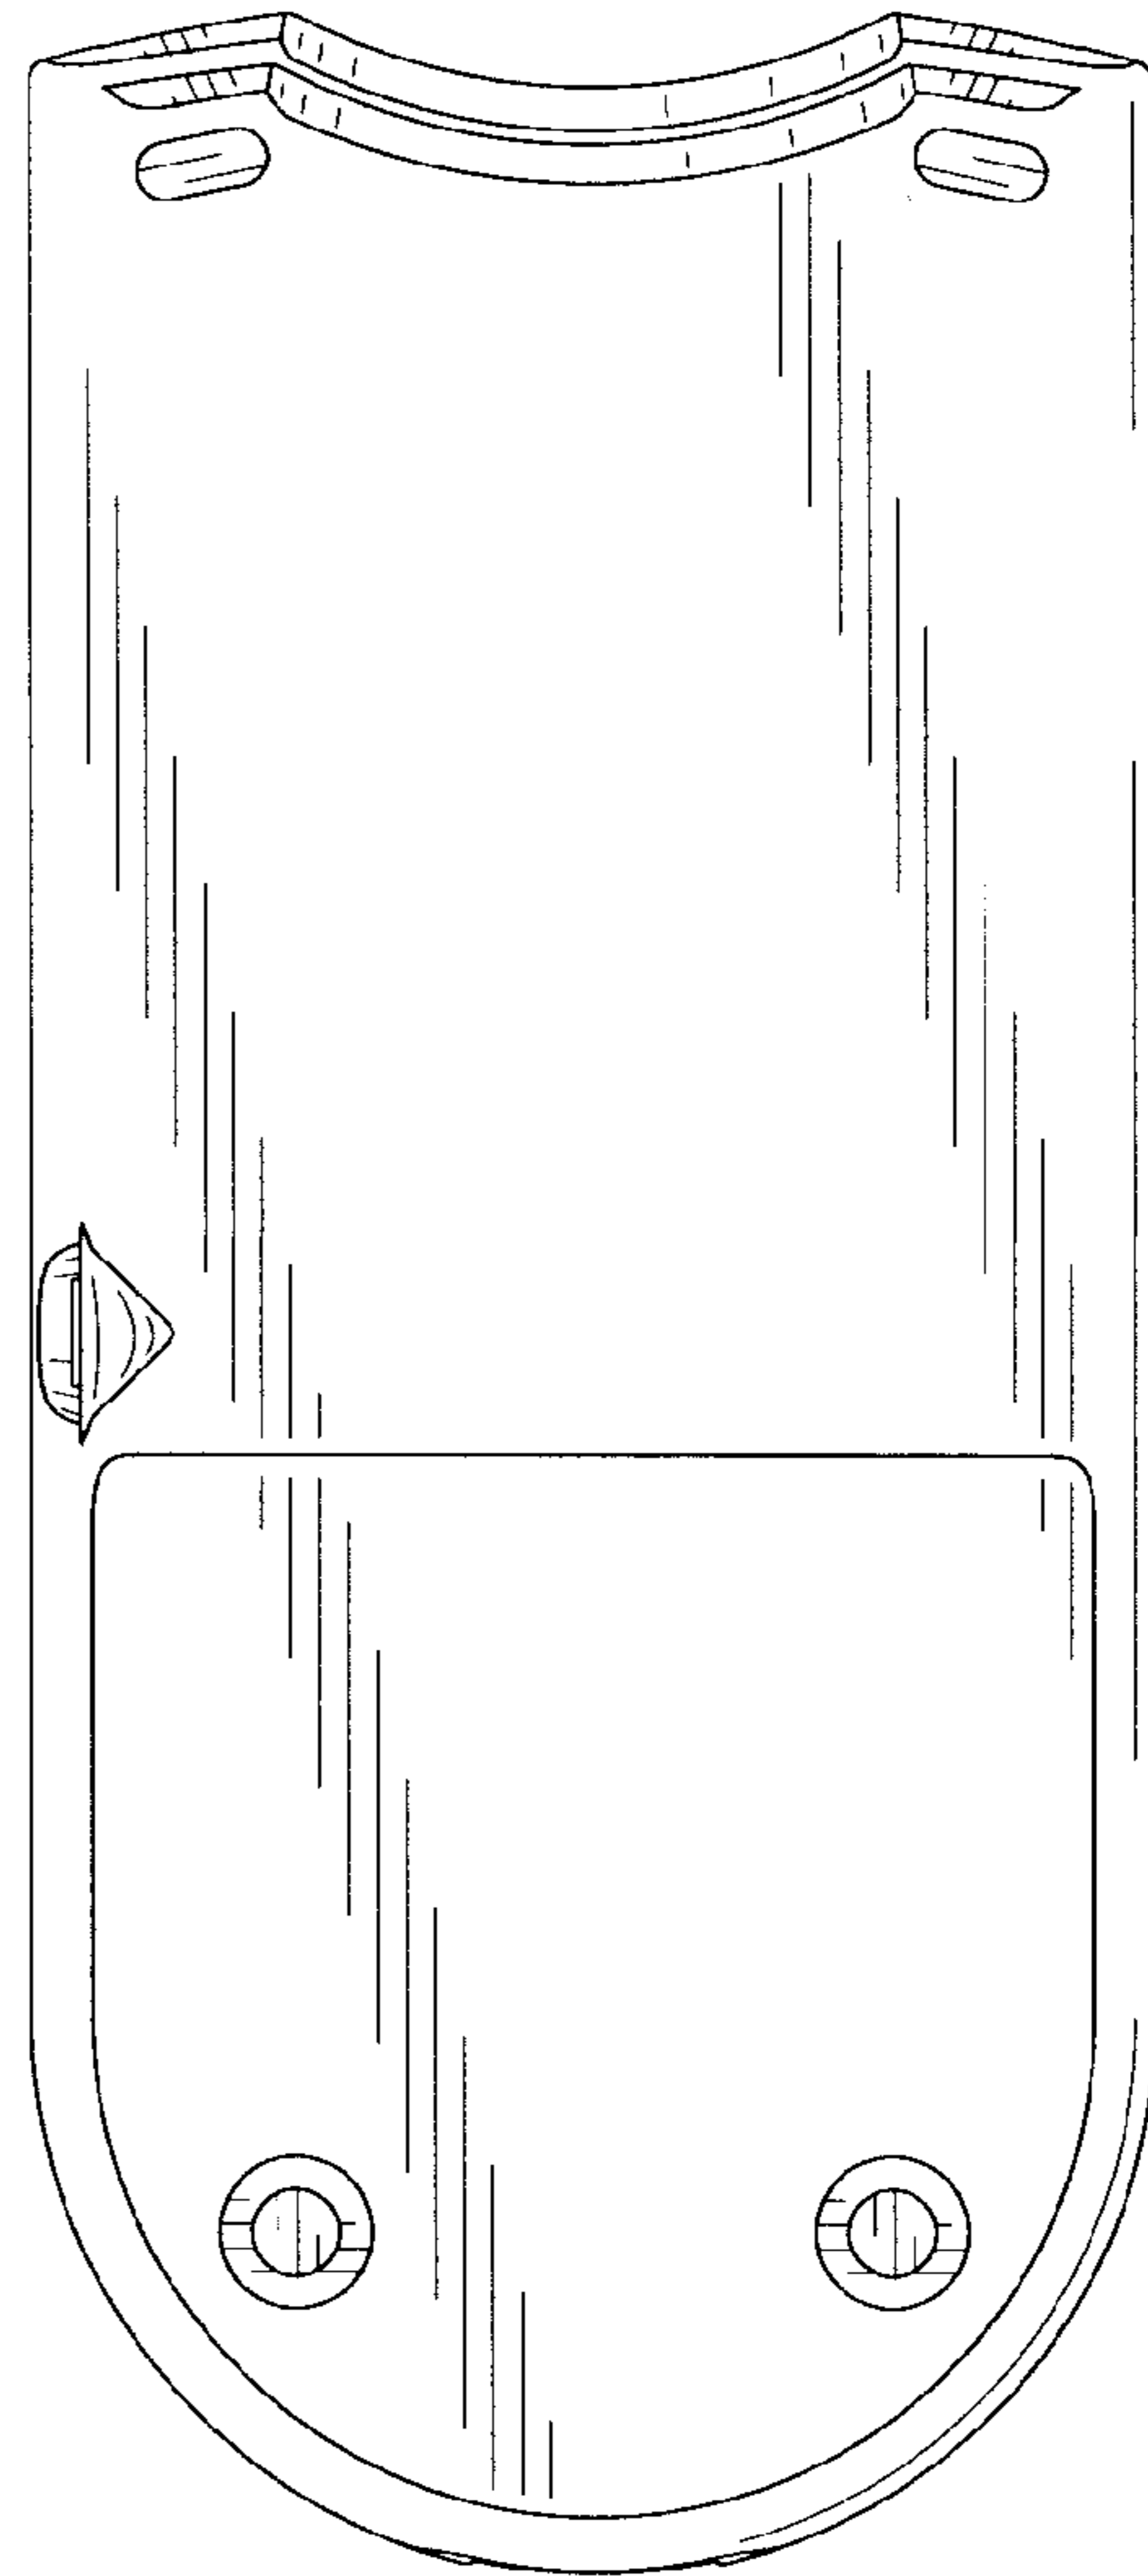


Fig.4.

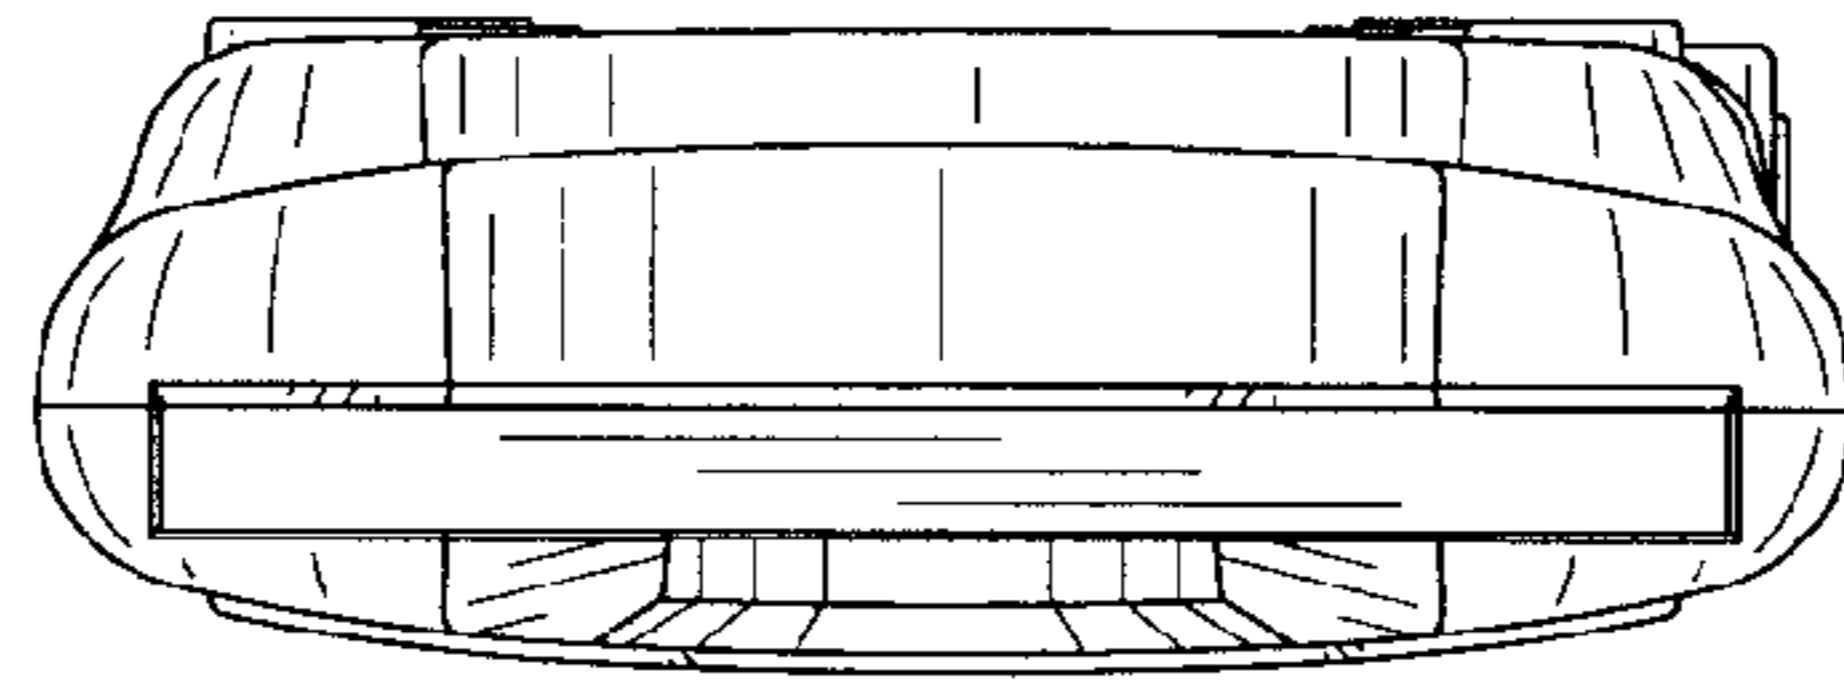


Fig. 7.

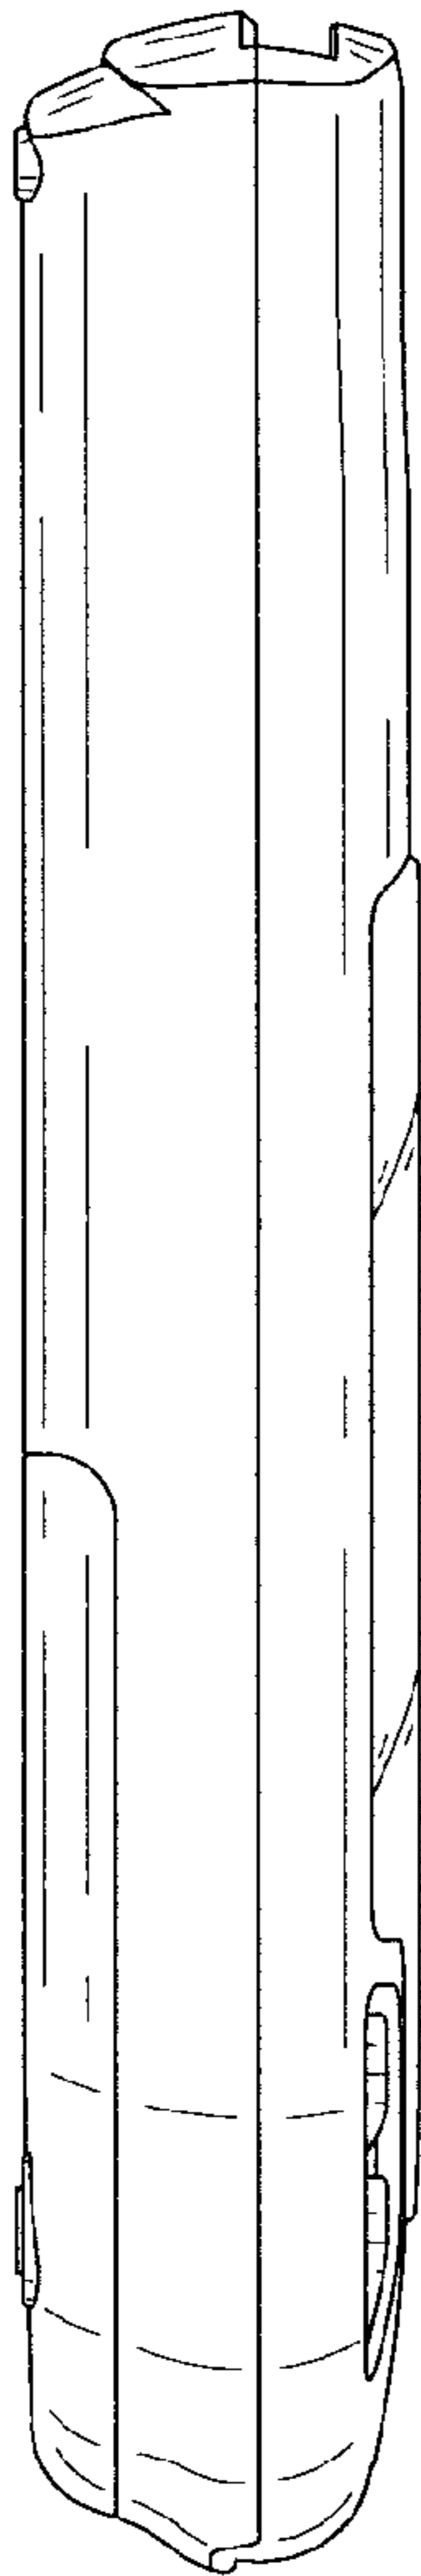


Fig. 5.

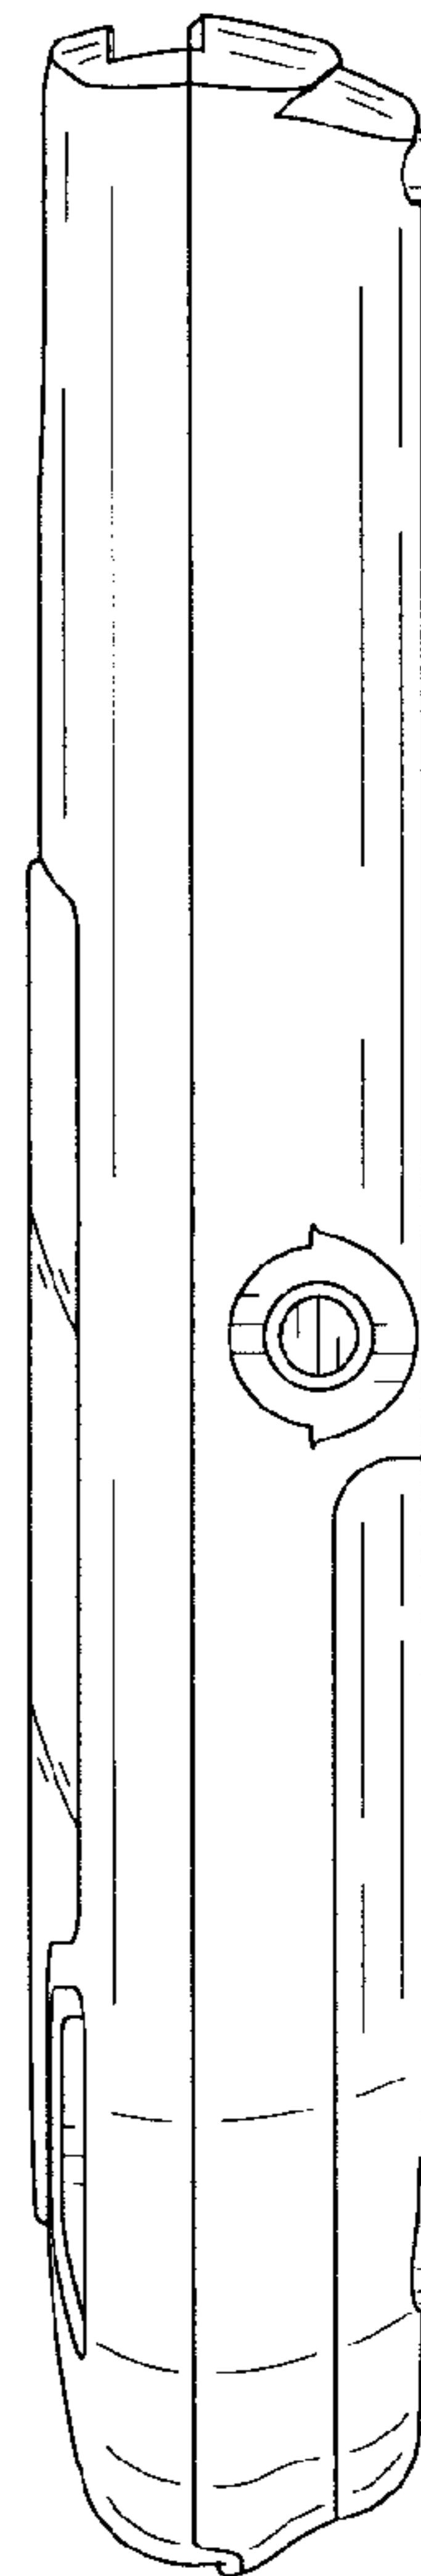


Fig. 6.

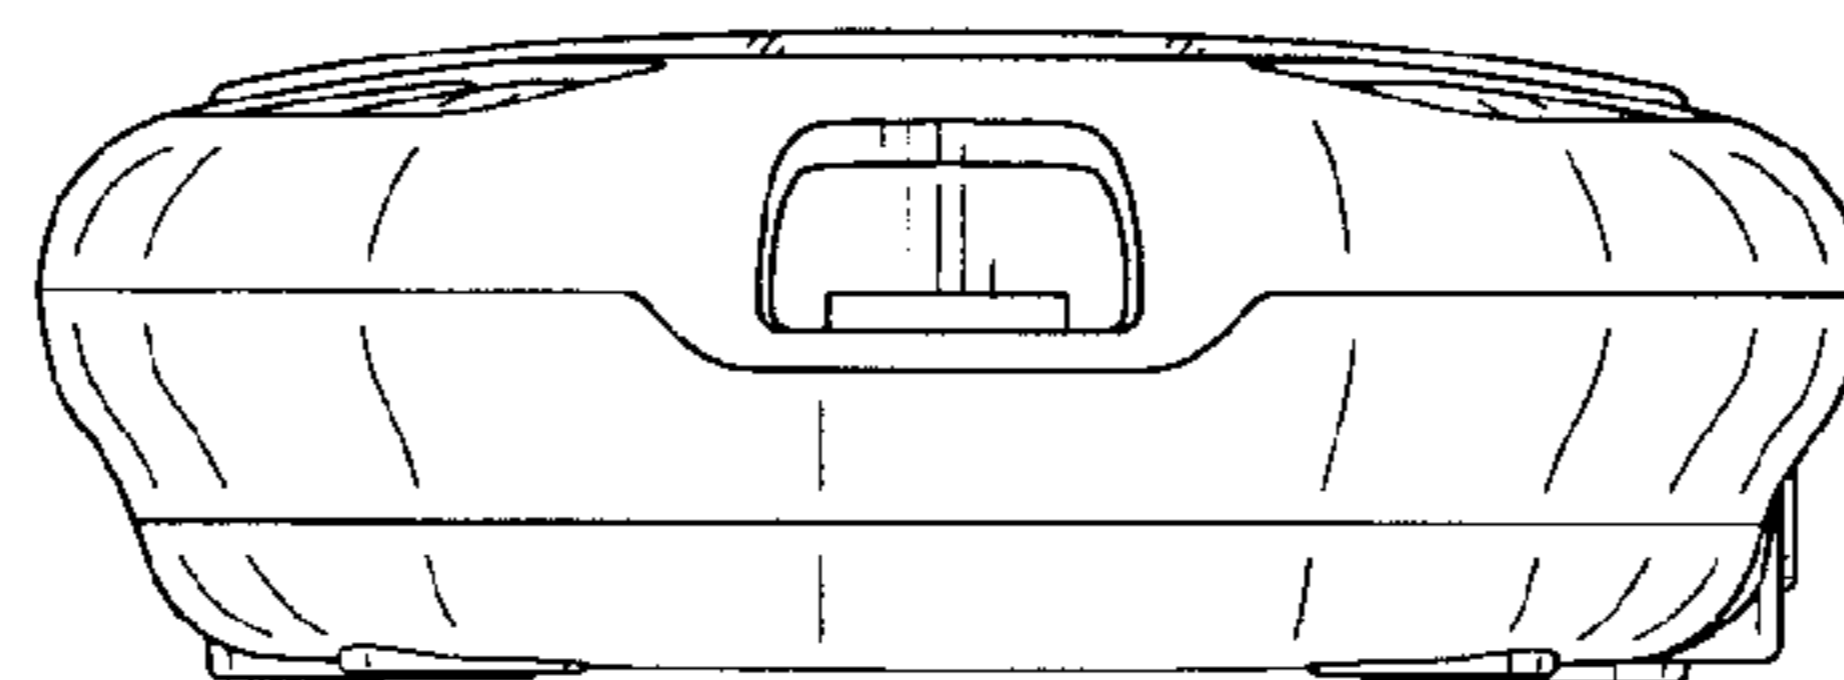


Fig. 8.