

US00D621050S

(12) **United States Design Patent**  
**Jamison et al.**

(10) **Patent No.:** **US D621,050 S**  
(45) **Date of Patent:** **\*\* Aug. 3, 2010**

(54) **OPHTHALMOLOGICAL INSTRUMENT  
STAND**

(75) Inventors: **Chris Mark Jamison**, West Chester, OH  
(US); **Scott Allen Armacost**, Hamilton,  
OH (US); **David E. Burbrink**, Cold  
Spring, KY (US)

(73) Assignee: **Reliance Medical Products, Inc.**,  
Mason, OH (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/332,033**

(22) Filed: **Feb. 6, 2009**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/177**

(58) **Field of Classification Search** ..... D24/176,  
D24/177, 179; 433/26, 29, 203.1, 215; 356/402,  
356/405, 406, 408; 364/413.28; 351/245;  
248/127

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

|              |         |                    |       |         |
|--------------|---------|--------------------|-------|---------|
| D235,274 S * | 6/1975  | Armbruster         | ..... | D24/172 |
| D292,526 S * | 10/1987 | Nakayama           | ..... | D24/172 |
| 4,910,386 A  | 3/1990  | Johnson            |       |         |
| D352,106 S * | 11/1994 | Fanney et al.      | ..... | D24/185 |
| D353,201 S   | 12/1994 | Crook et al.       |       |         |
| D354,176 S   | 1/1995  | Schwaegerle et al. |       |         |
| D354,177 S   | 1/1995  | Schwaegerle et al. |       |         |
| 5,399,007 A  | 3/1995  | Marconet           |       |         |
| 5,461,965 A  | 10/1995 | Schwaegerle        |       |         |
| 5,467,002 A  | 11/1995 | Brooks             |       |         |
| 5,480,212 A  | 1/1996  | Marconet           |       |         |
| D378,315 S   | 3/1997  | Schwaegerle et al. |       |         |
| D379,409 S   | 5/1997  | Schwaegerle et al. |       |         |
| 5,696,574 A  | 12/1997 | Schwaegerle        |       |         |
| 5,717,480 A  | 2/1998  | Brooks et al.      |       |         |
| D407,379 S   | 3/1999  | Schwaegerle        |       |         |
| 5,907,387 A  | 5/1999  | Schwaegerle        |       |         |
| D412,621 S   | 8/1999  | Smith et al.       |       |         |

D412,801 S 8/1999 Smith et al.

D418,339 S 1/2000 Smith et al.

D418,686 S 1/2000 Smith et al.

D419,343 S 1/2000 Smith et al.

D420,233 S 2/2000 Smith et al.

(Continued)

*Primary Examiner*—Ian Simmons

*Assistant Examiner*—Charles D Hanson

(74) *Attorney, Agent, or Firm*—Wood, Herron & Evans, LLP

(57) **CLAIM**

The ornamental design for an ophthalmological instrument stand, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an ophthalmological instrument stand with broken lines depicting environmental aspects showing my new design;

FIG. 2 is a perspective view similar to FIG. 1 in which environmental aspects have been removed;

FIG. 3 is a front view of the ophthalmological instrument stand;

FIG. 4 is a left side view of the ophthalmological instrument stand;

FIG. 5 is a rear side view of the ophthalmological instrument stand;


FIG. 6 is a right side view of the ophthalmological instrument stand;

FIG. 7 is a top view of the ophthalmological instrument stand; and,

FIG. 8 is a bottom view of the ophthalmological instrument stand.

The elements shown in broken lines in FIG. 1 are for illustrative purposes only, form no part of the claimed invention, and are instead included to show environmental aspects of the claimed invention.

**1 Claim, 7 Drawing Sheets**

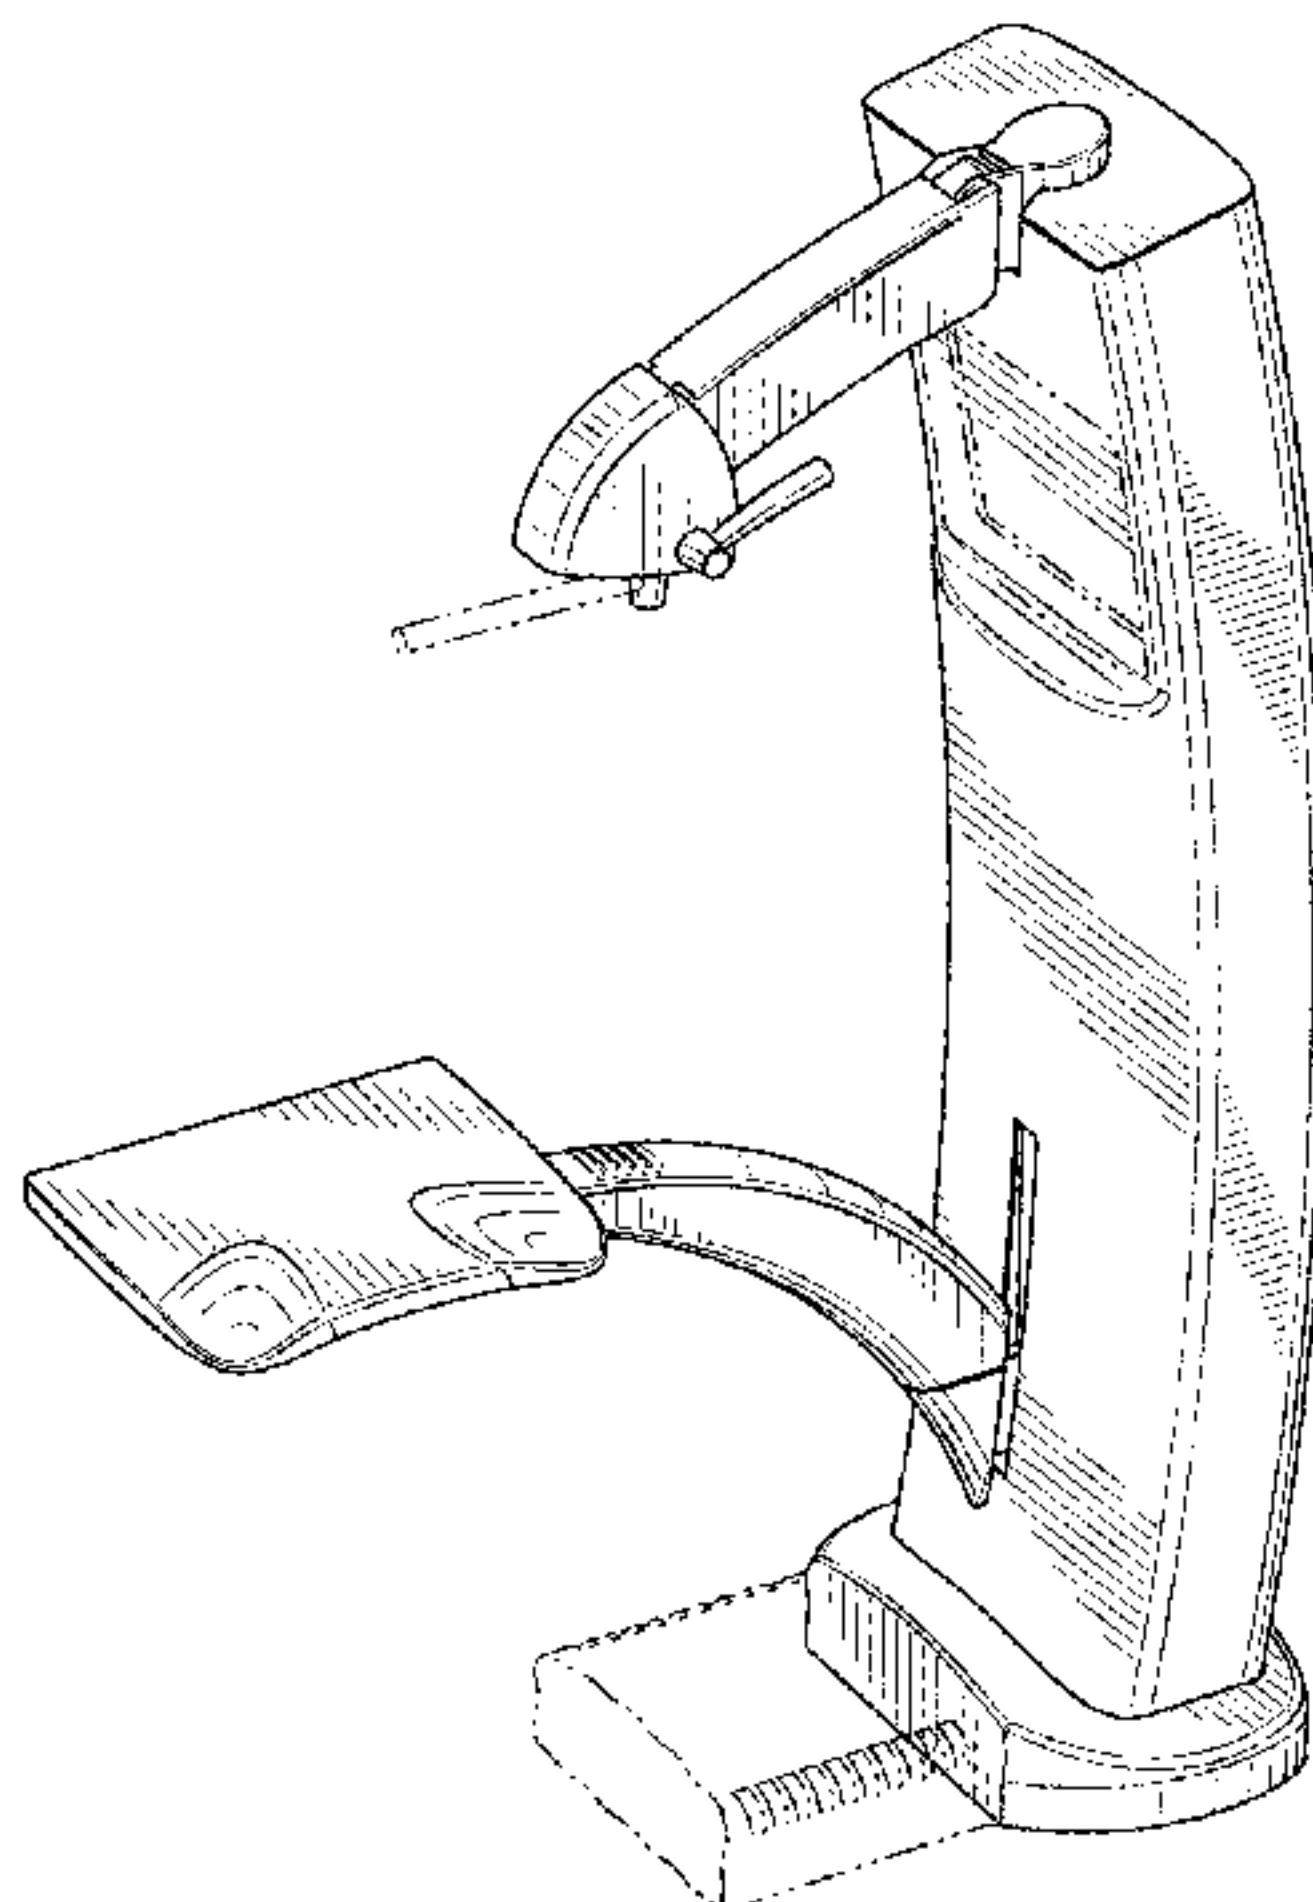

| U.S. PATENT DOCUMENTS |         |                        |                |         |                             |
|-----------------------|---------|------------------------|----------------|---------|-----------------------------|
| D423,262 S            | 4/2000  | Smith et al.           | 6,382,725 B1   | 5/2002  | Carroll                     |
| D424,200 S            | 5/2000  | Smith                  | D458,378 S *   | 6/2002  | Bevington ..... D24/177     |
| D424,337 S            | 5/2000  | Smith et al.           | 6,575,575 B2 * | 6/2003  | O'Brien et al. .... 351/245 |
| D425,341 S            | 5/2000  | Smith et al.           | 6,721,976 B2   | 4/2004  | Schwaegerle                 |
| D425,735 S            | 5/2000  | Smith et al.           | D503,233 S     | 3/2005  | Smith                       |
| D425,991 S            | 5/2000  | Smith et al.           | D504,515 S     | 4/2005  | Smith                       |
| D426,715 S            | 6/2000  | Smith et al.           | 6,886,199 B1   | 5/2005  | Schwaegerle                 |
| 6,095,649 A           | 8/2000  | Brooks et al.          | D506,257 S     | 6/2005  | Smith                       |
| 6,106,065 A           | 8/2000  | Carroll                | 6,928,676 B1   | 8/2005  | Schwaegerle                 |
| D433,588 S            | 11/2000 | Smith et al.           | D512,507 S     | 12/2005 | Smith                       |
| 6,264,329 B1          | 7/2001  | Brooks et al.          | D514,701 S     | 2/2006  | Smith                       |
| D456,080 S *          | 4/2002  | Karlsson ..... D24/185 | 7,401,921 B2 * | 7/2008  | Baker et al. .... 351/245   |
|                       |         |                        | 7,467,871 B2   | 12/2008 | Lawhorn et al.              |
|                       |         |                        |                |         | * cited by examiner         |

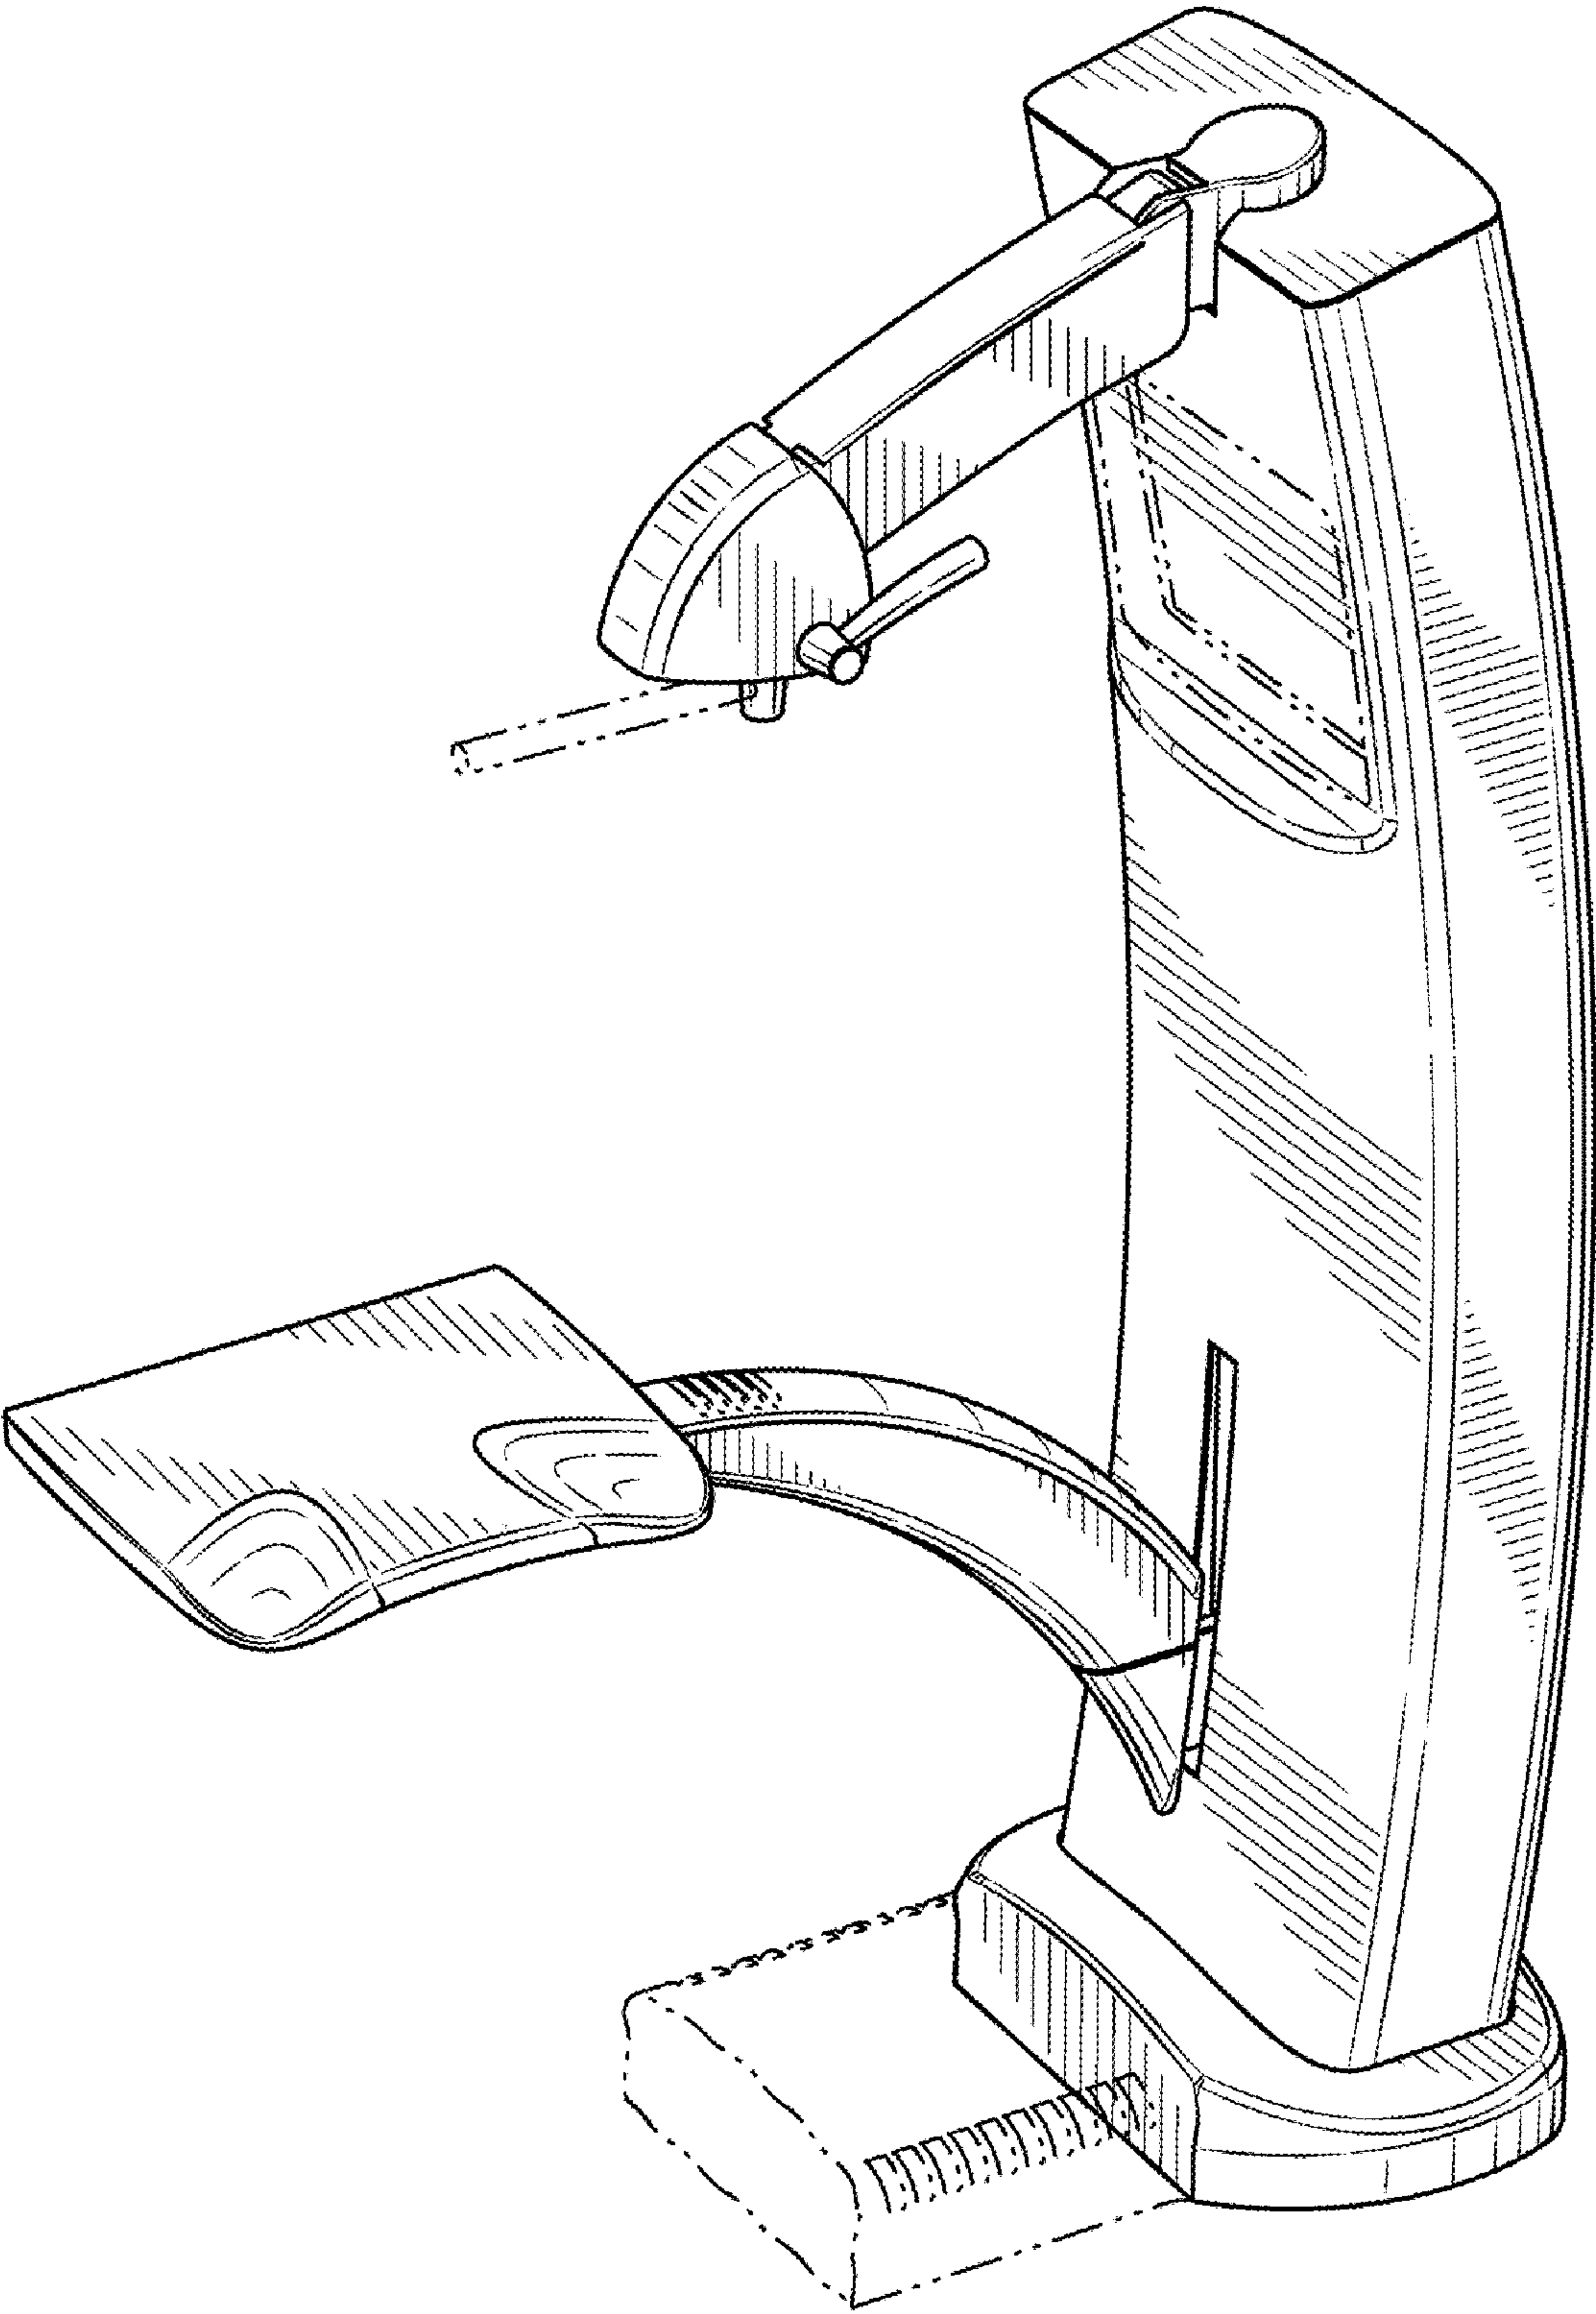


FIG. 1

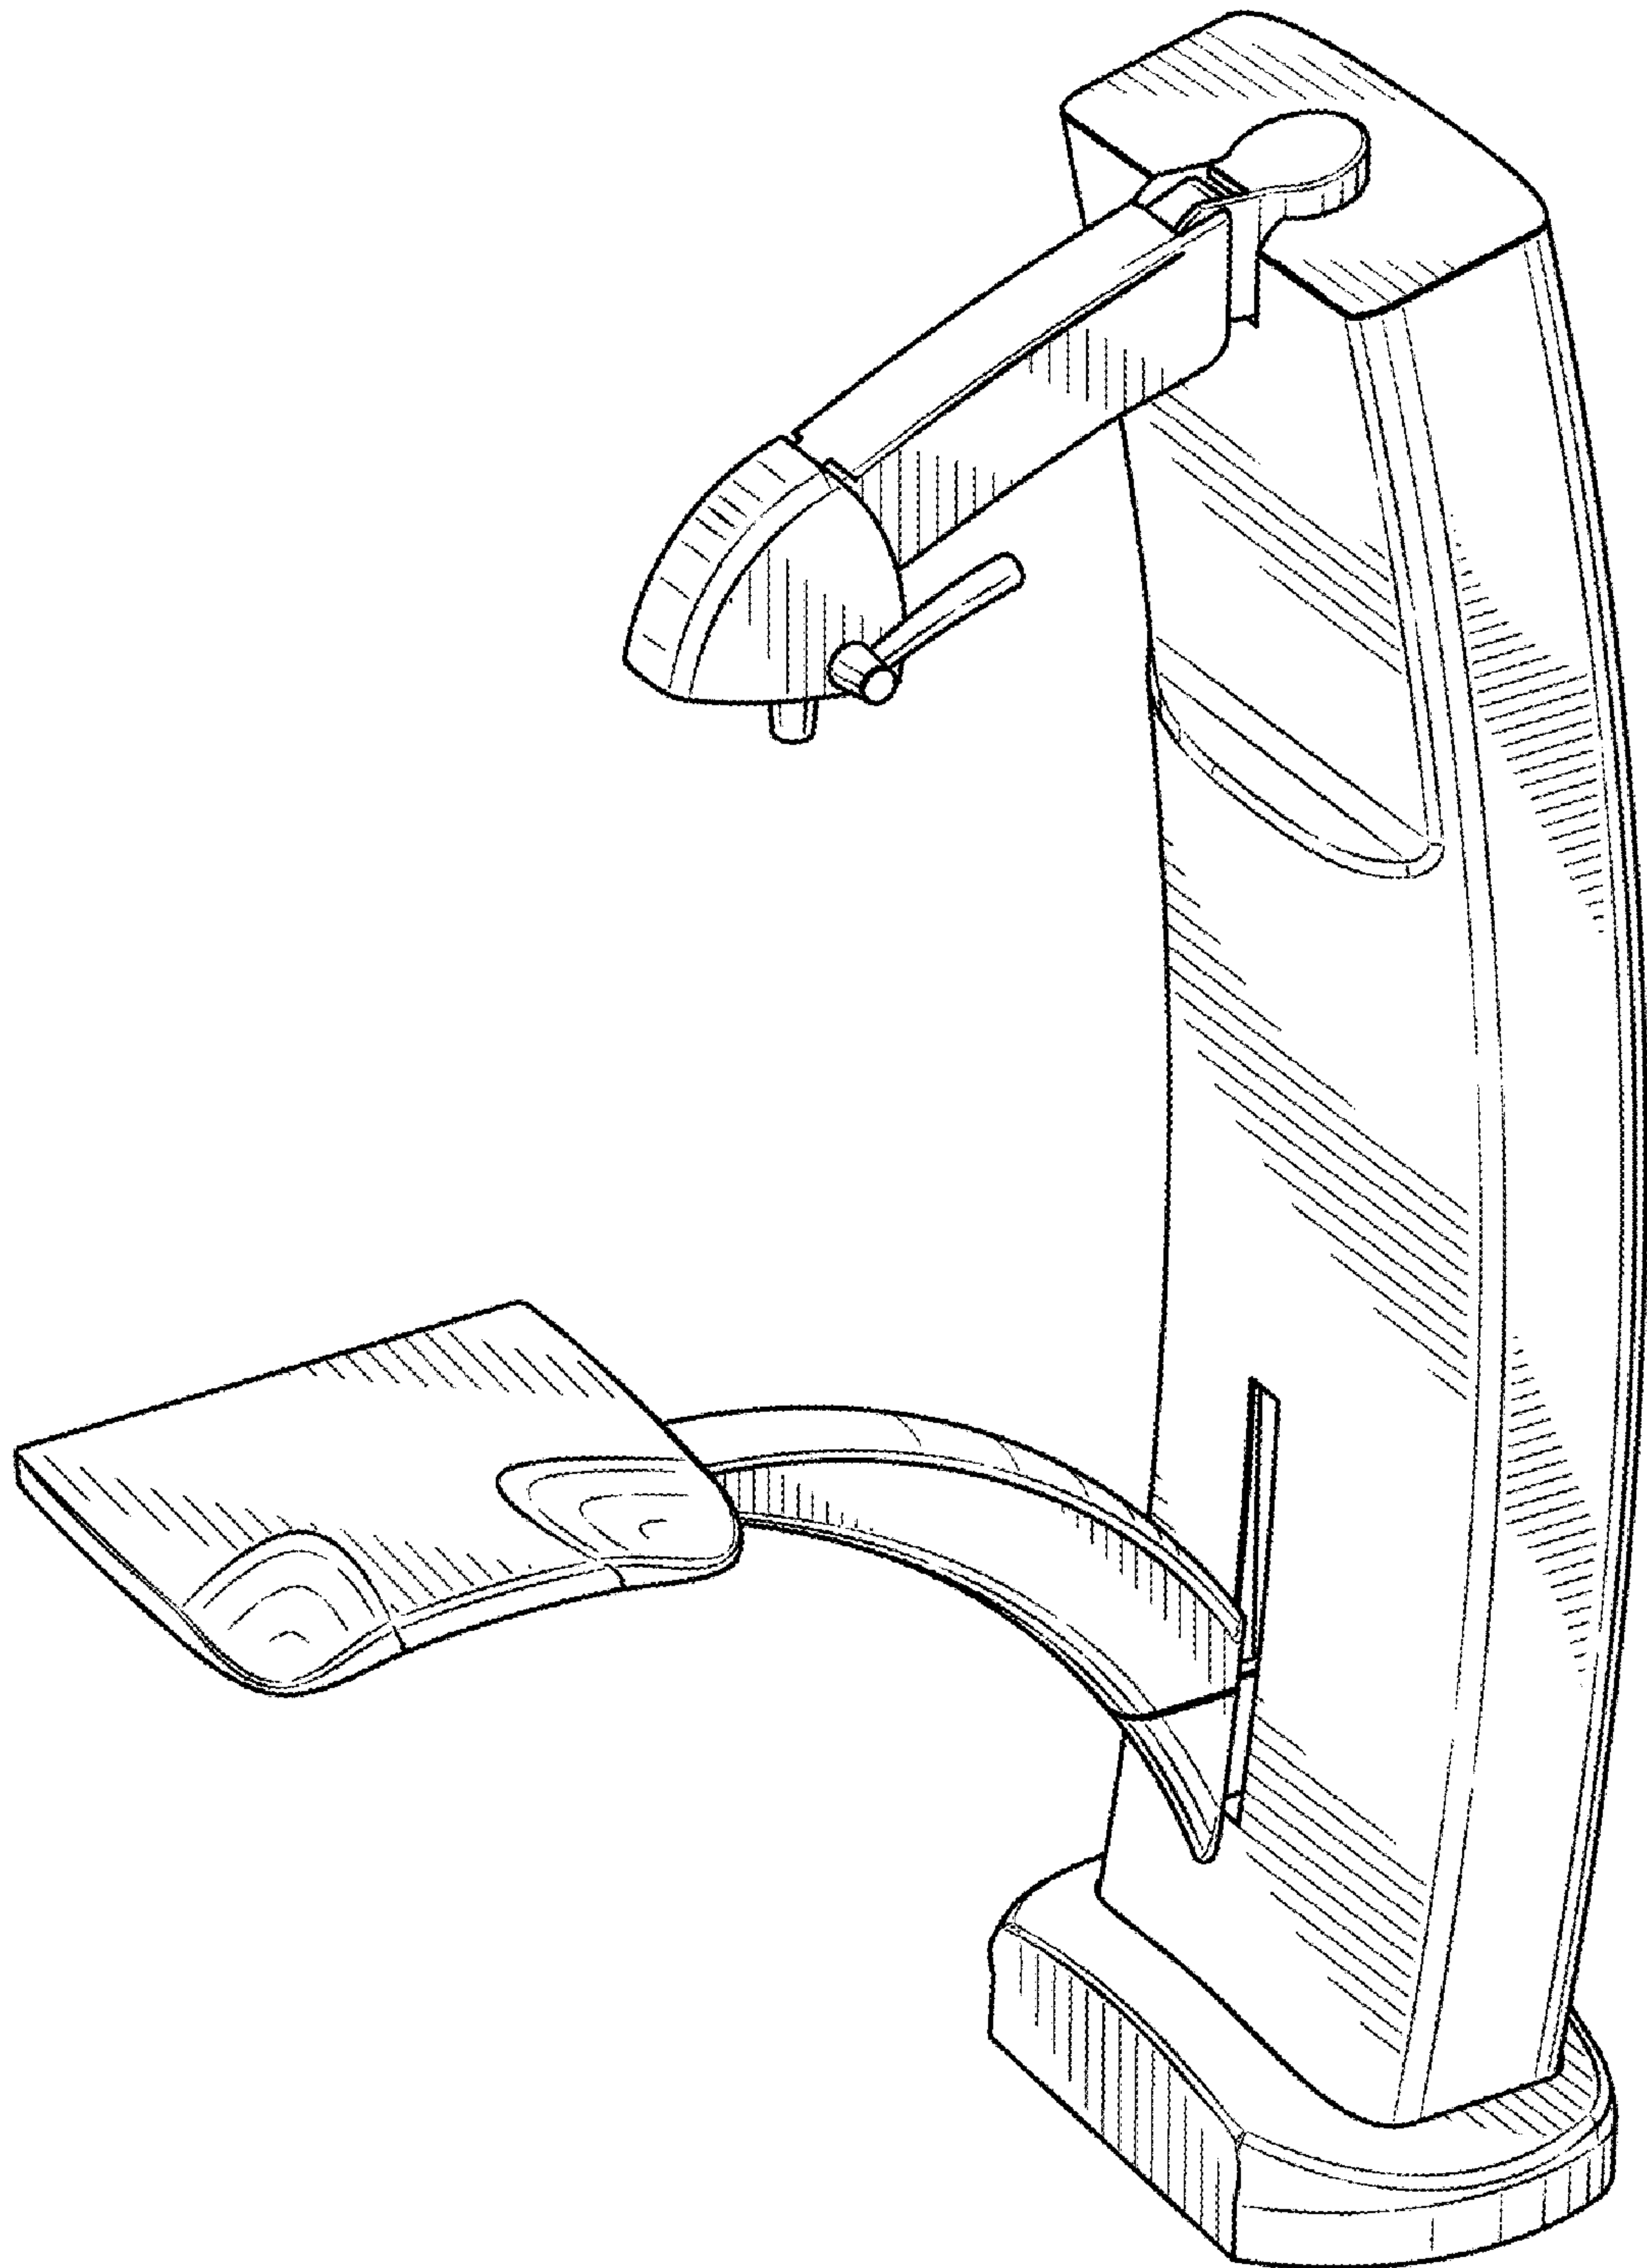


FIG. 2

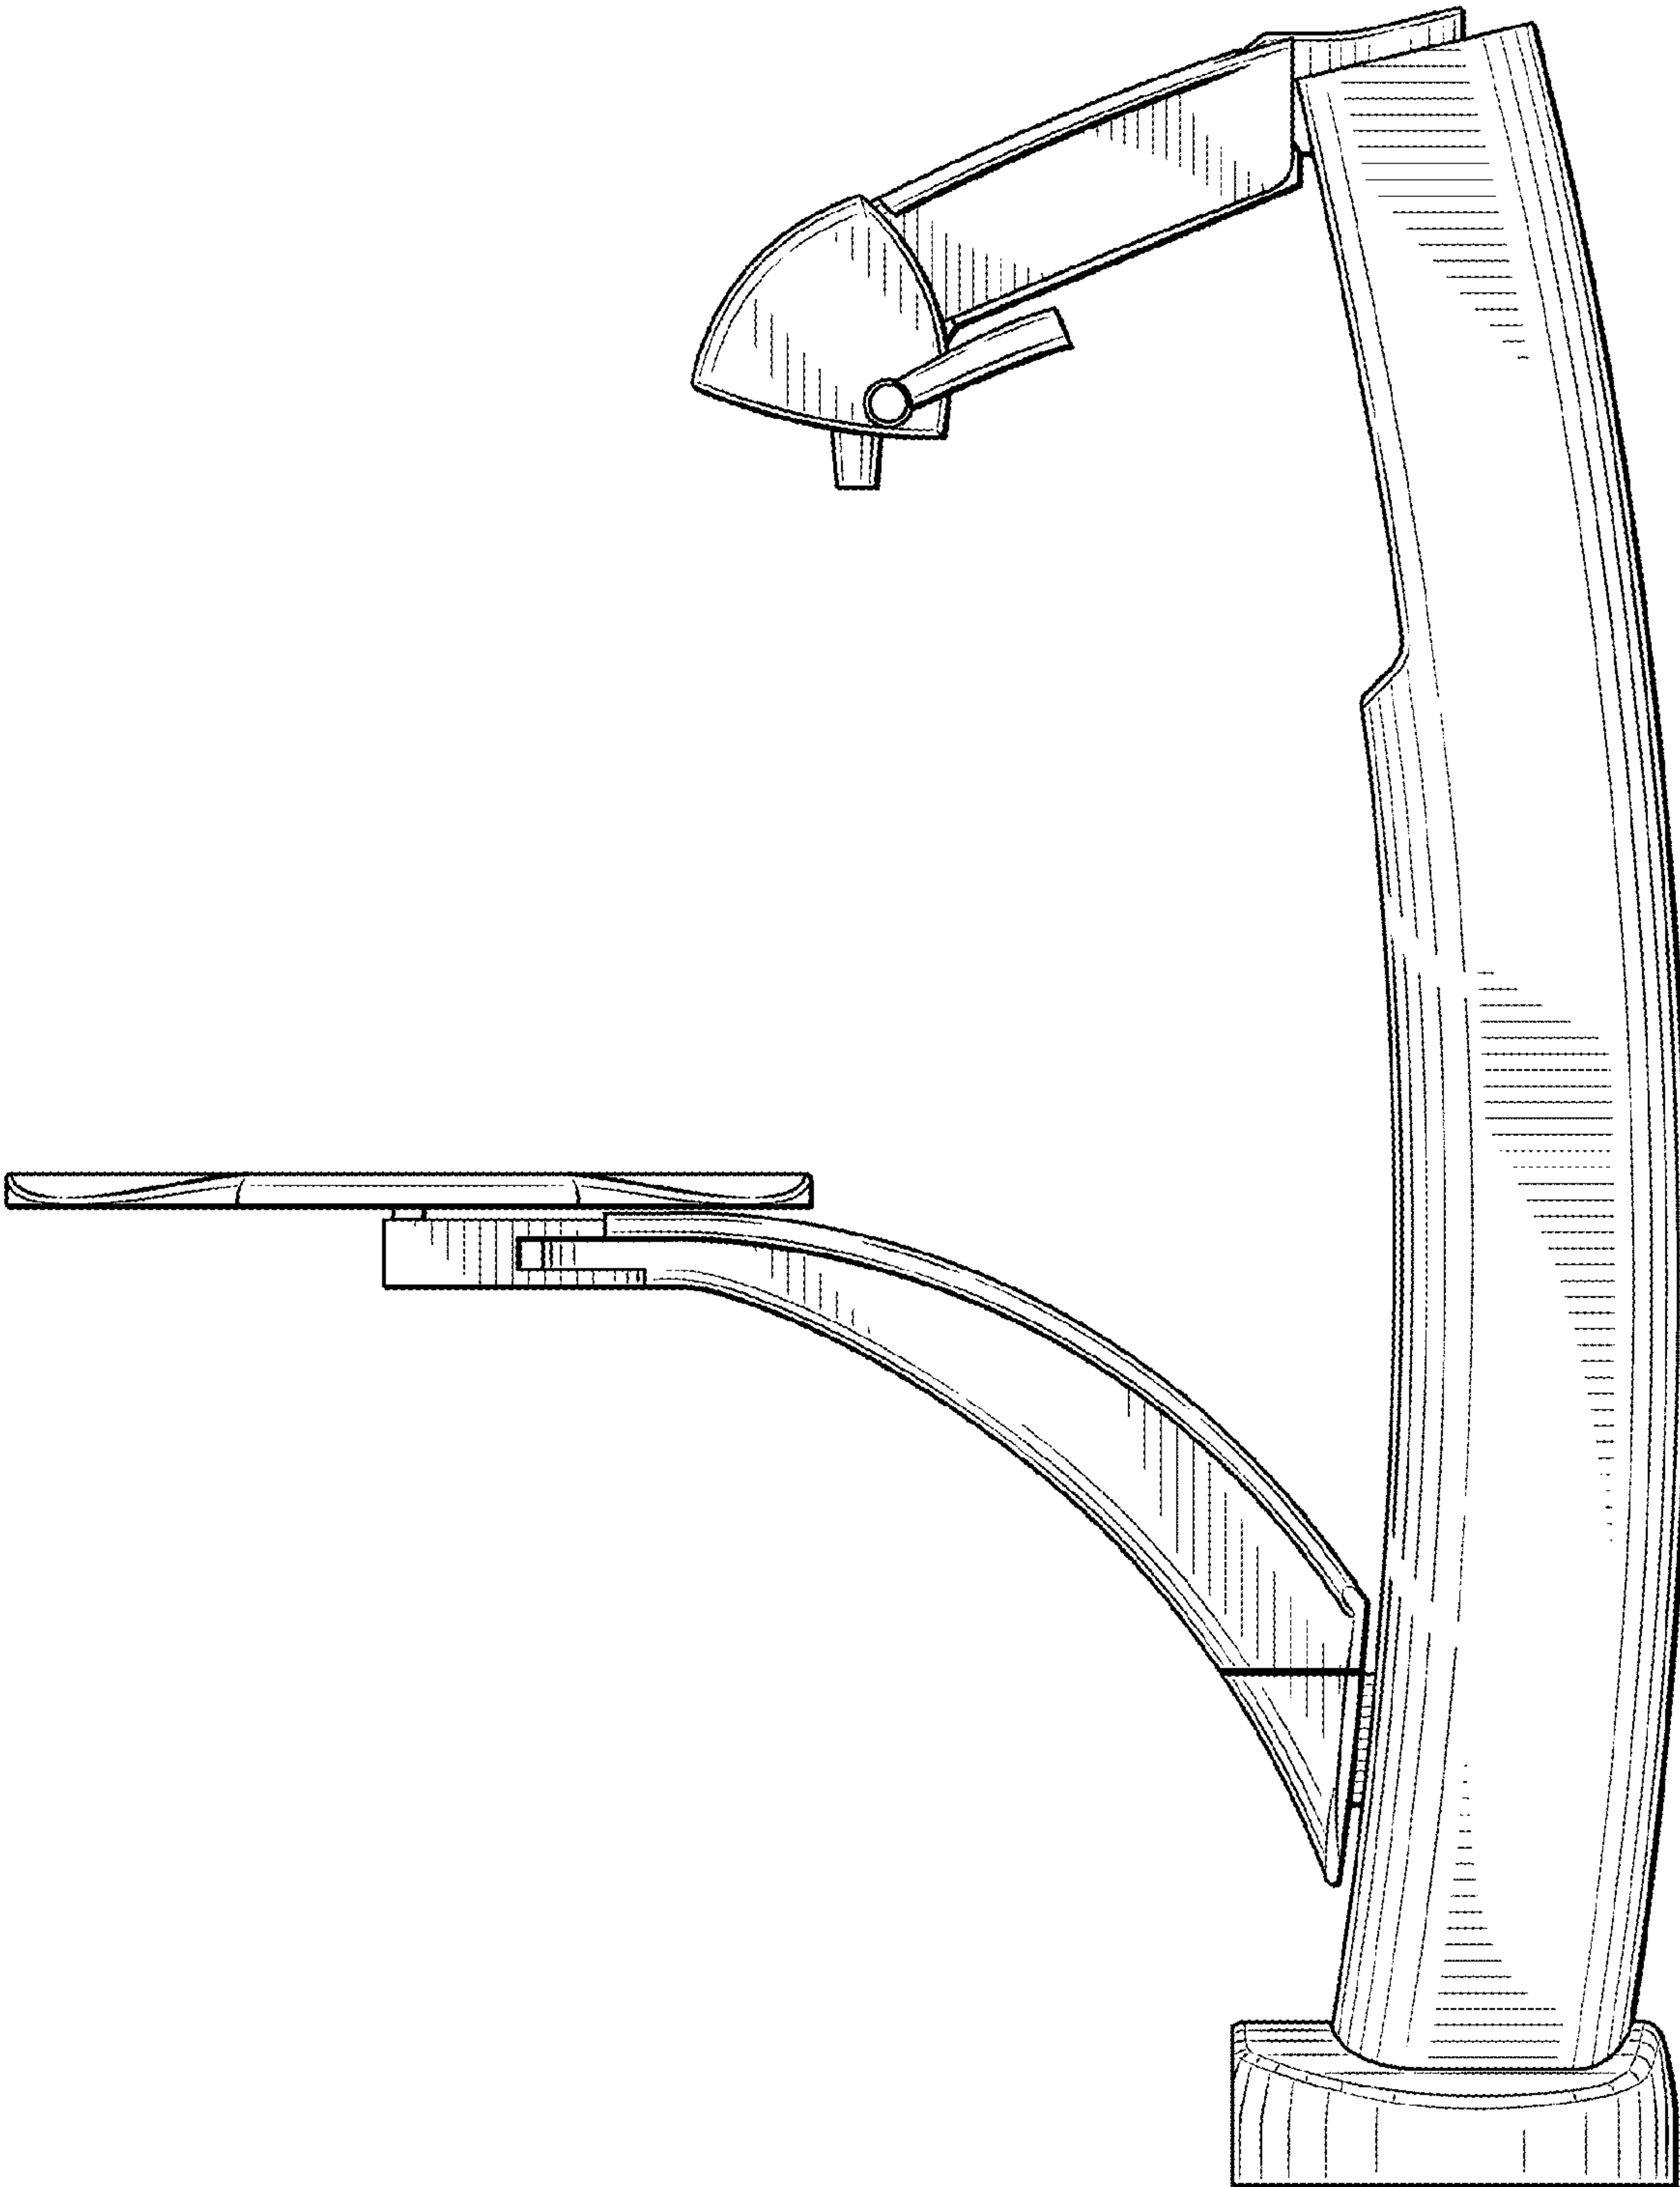


FIG. 3

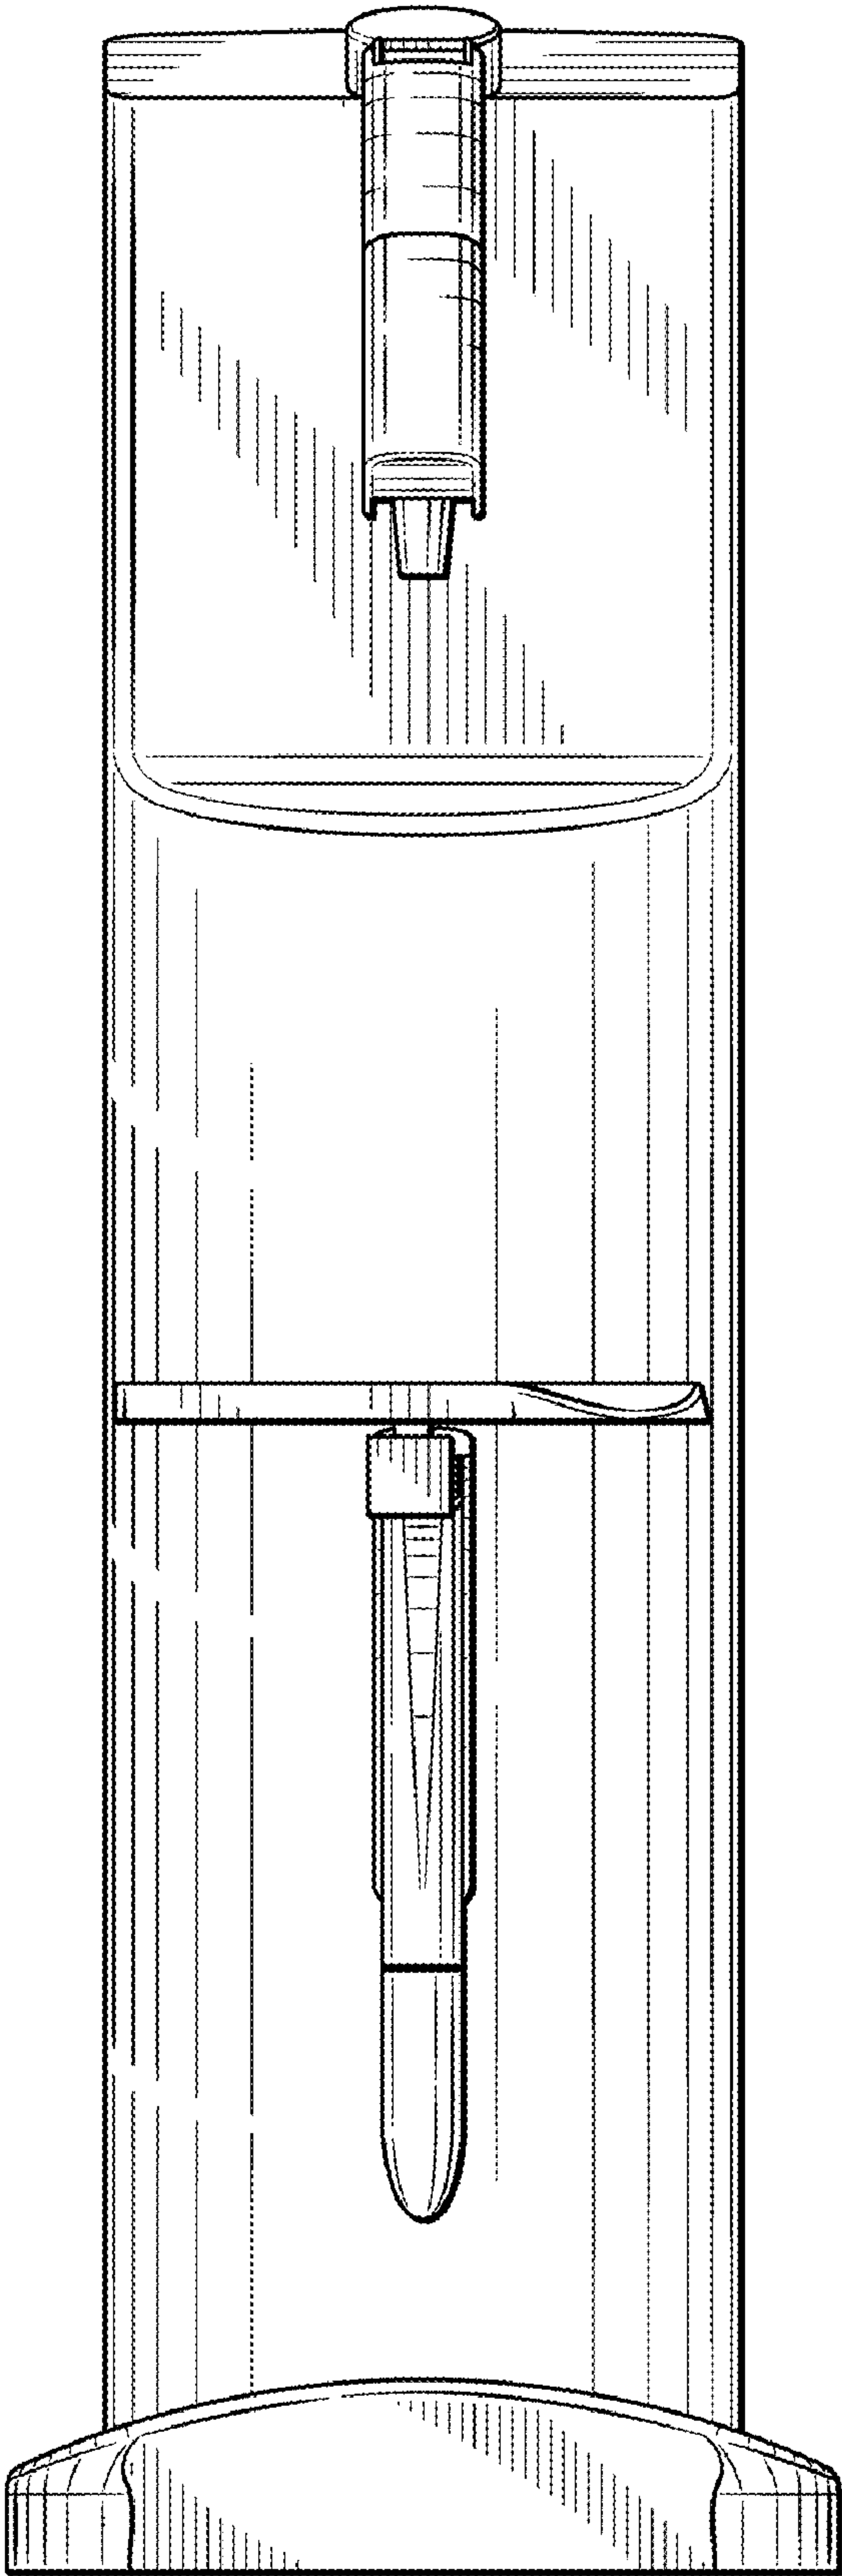


FIG. 4

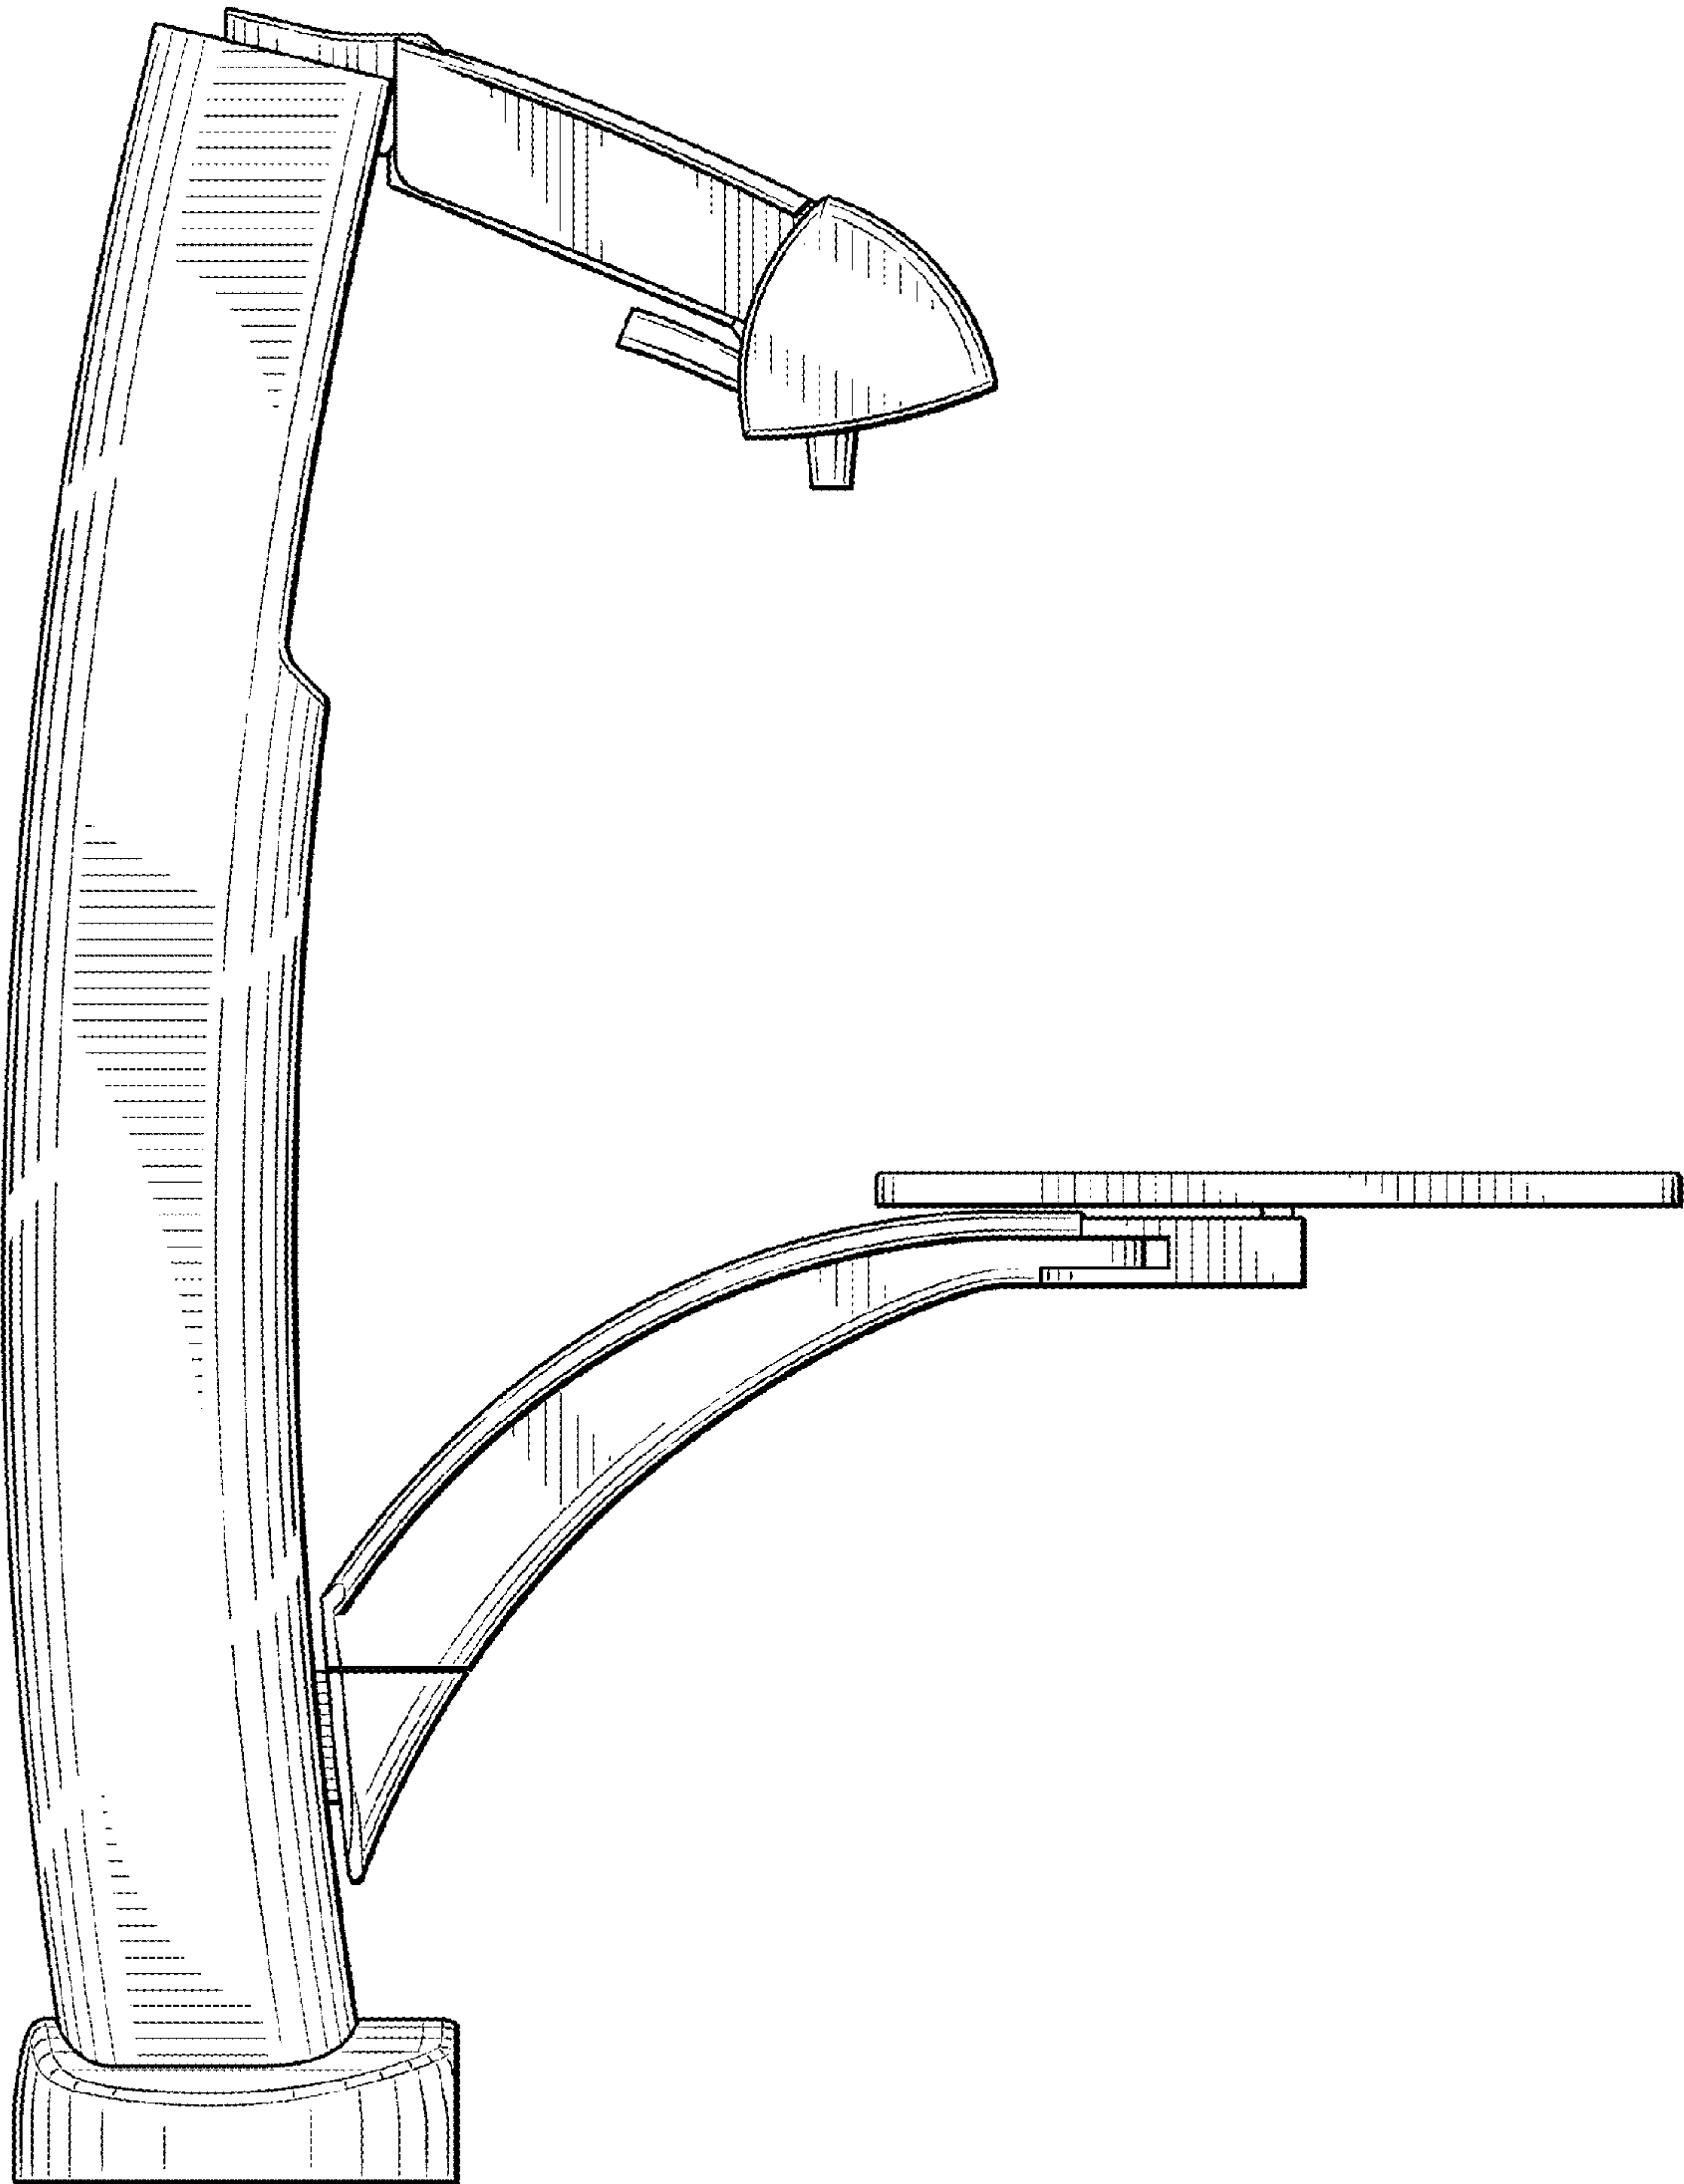


FIG. 5

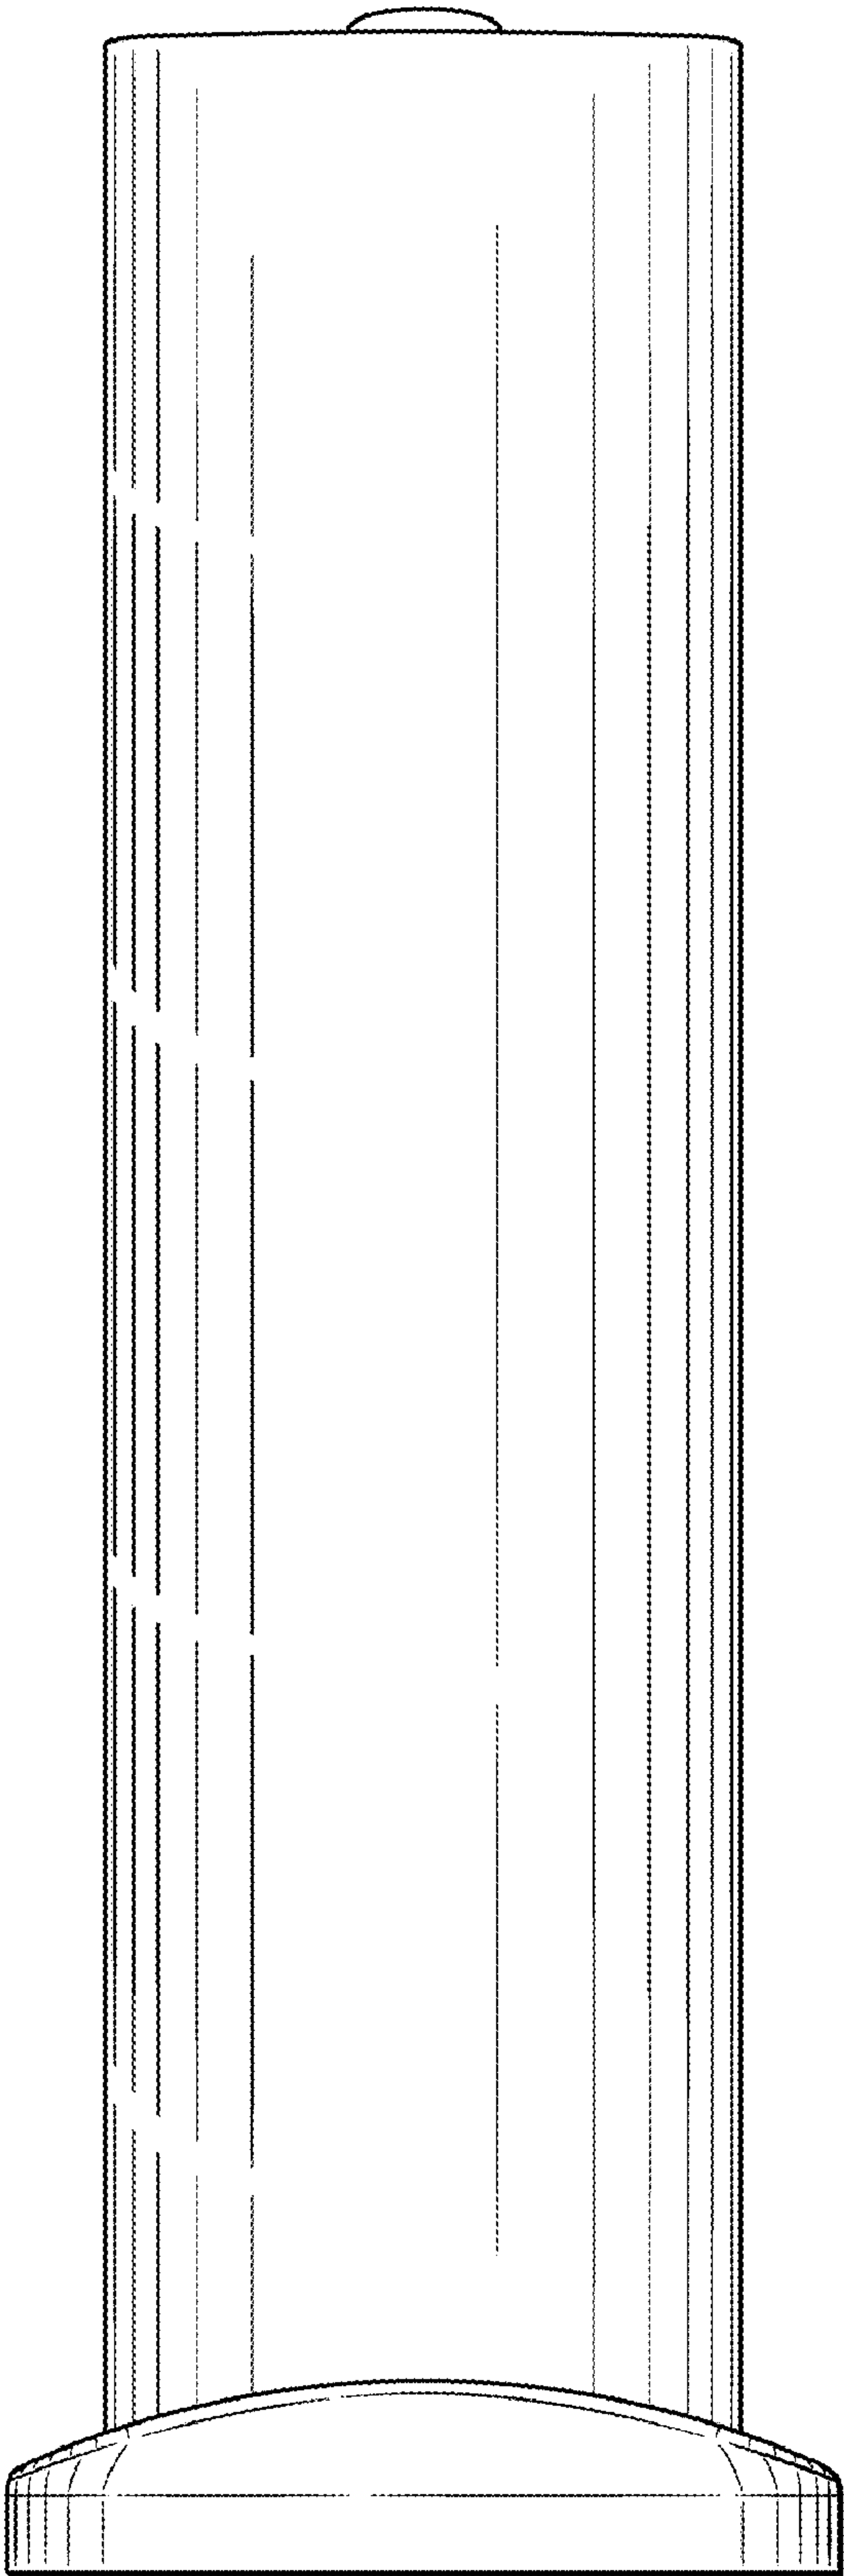


FIG. 6

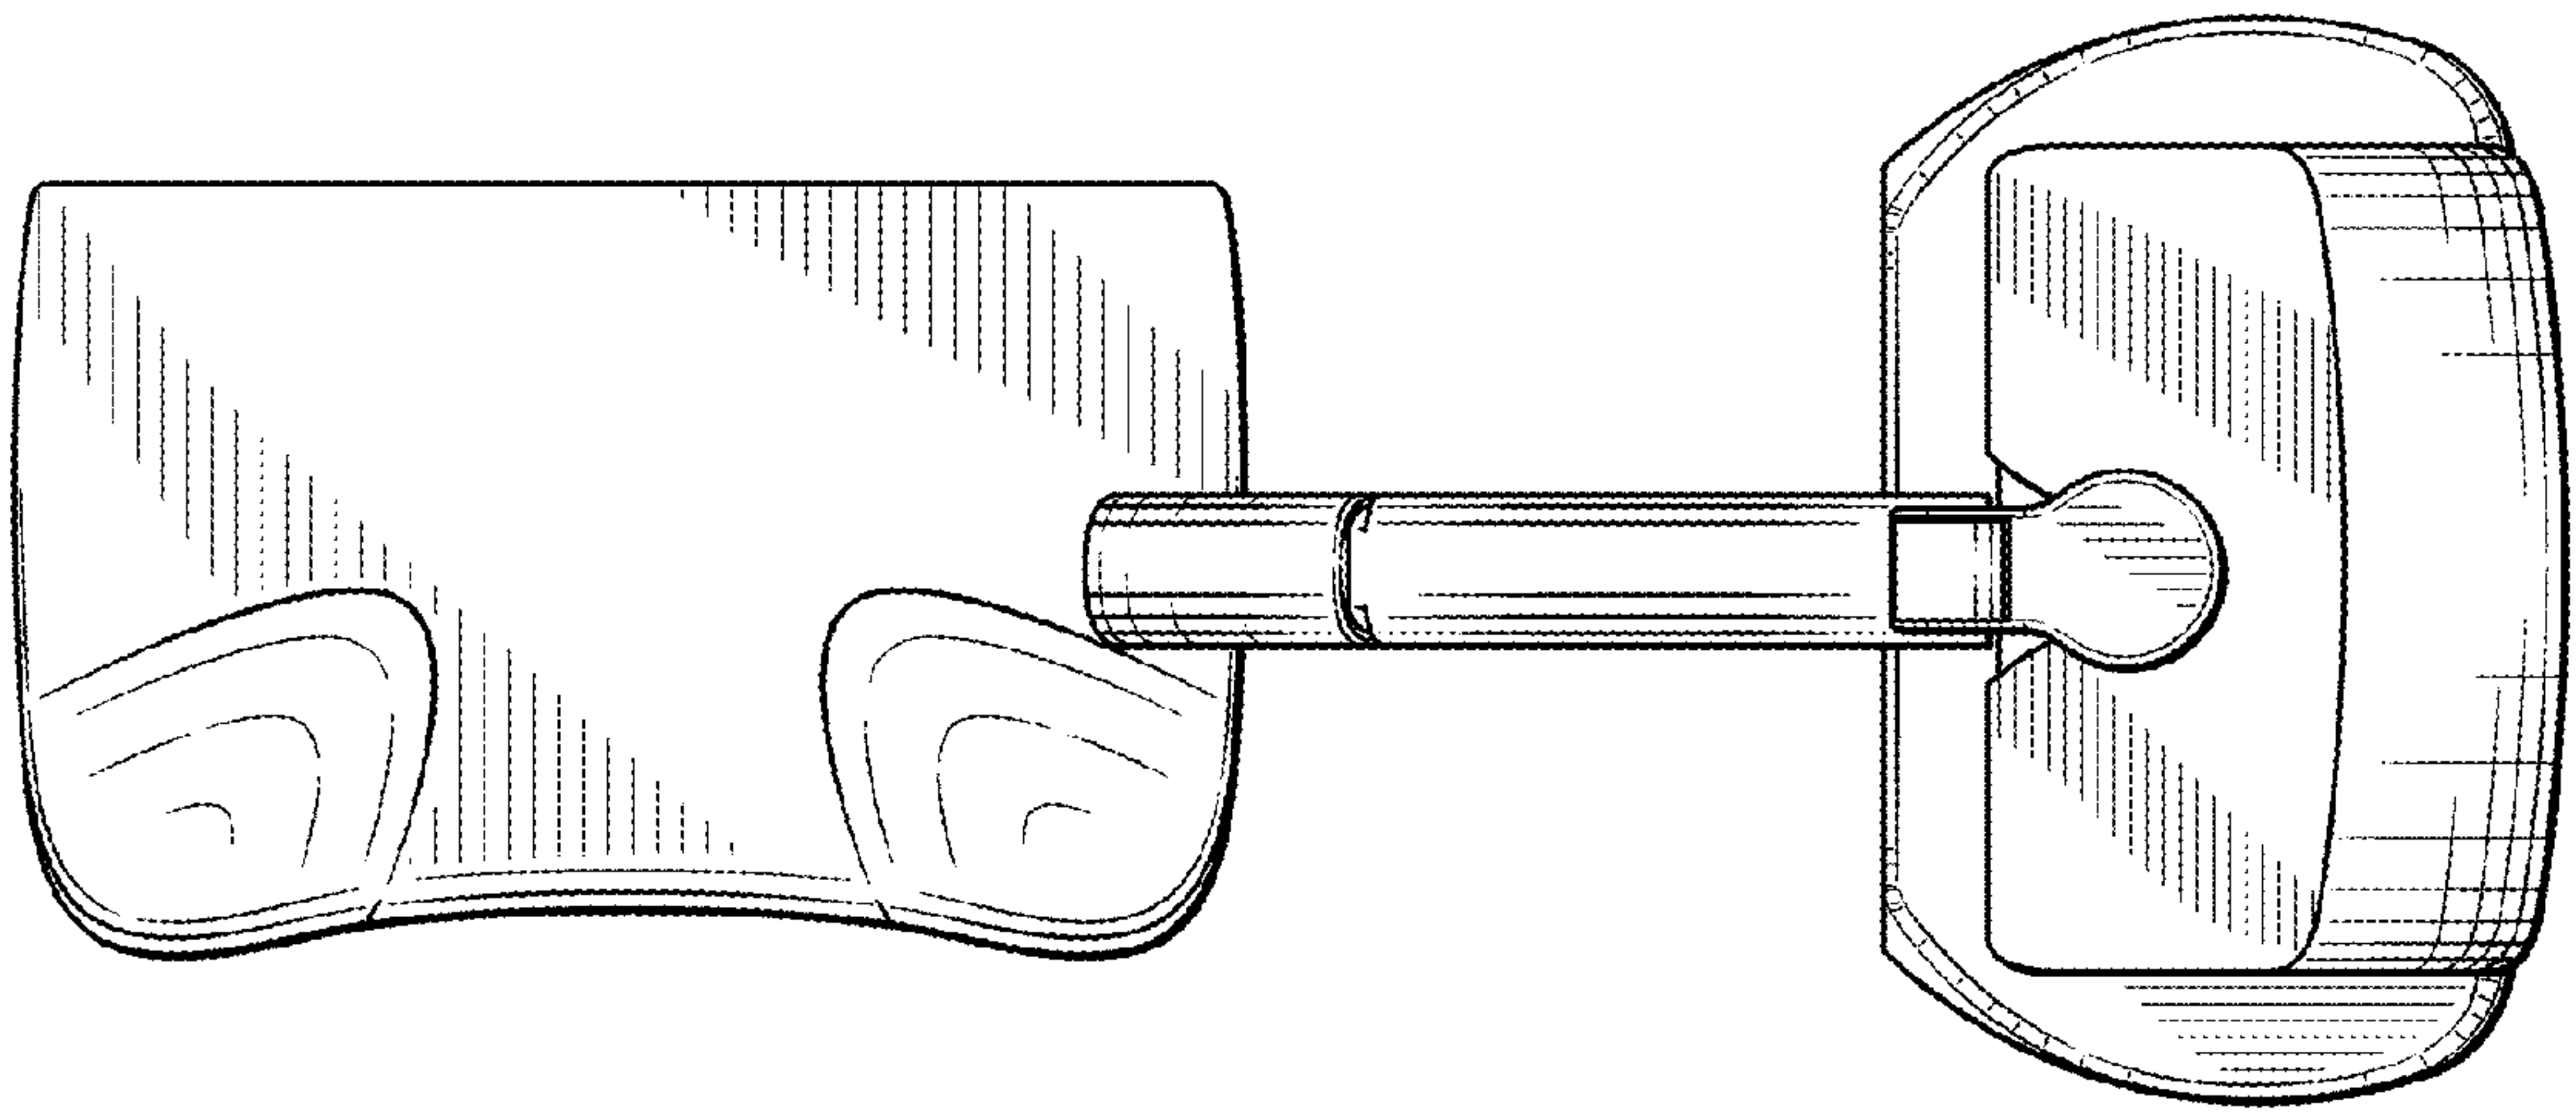


FIG. 7

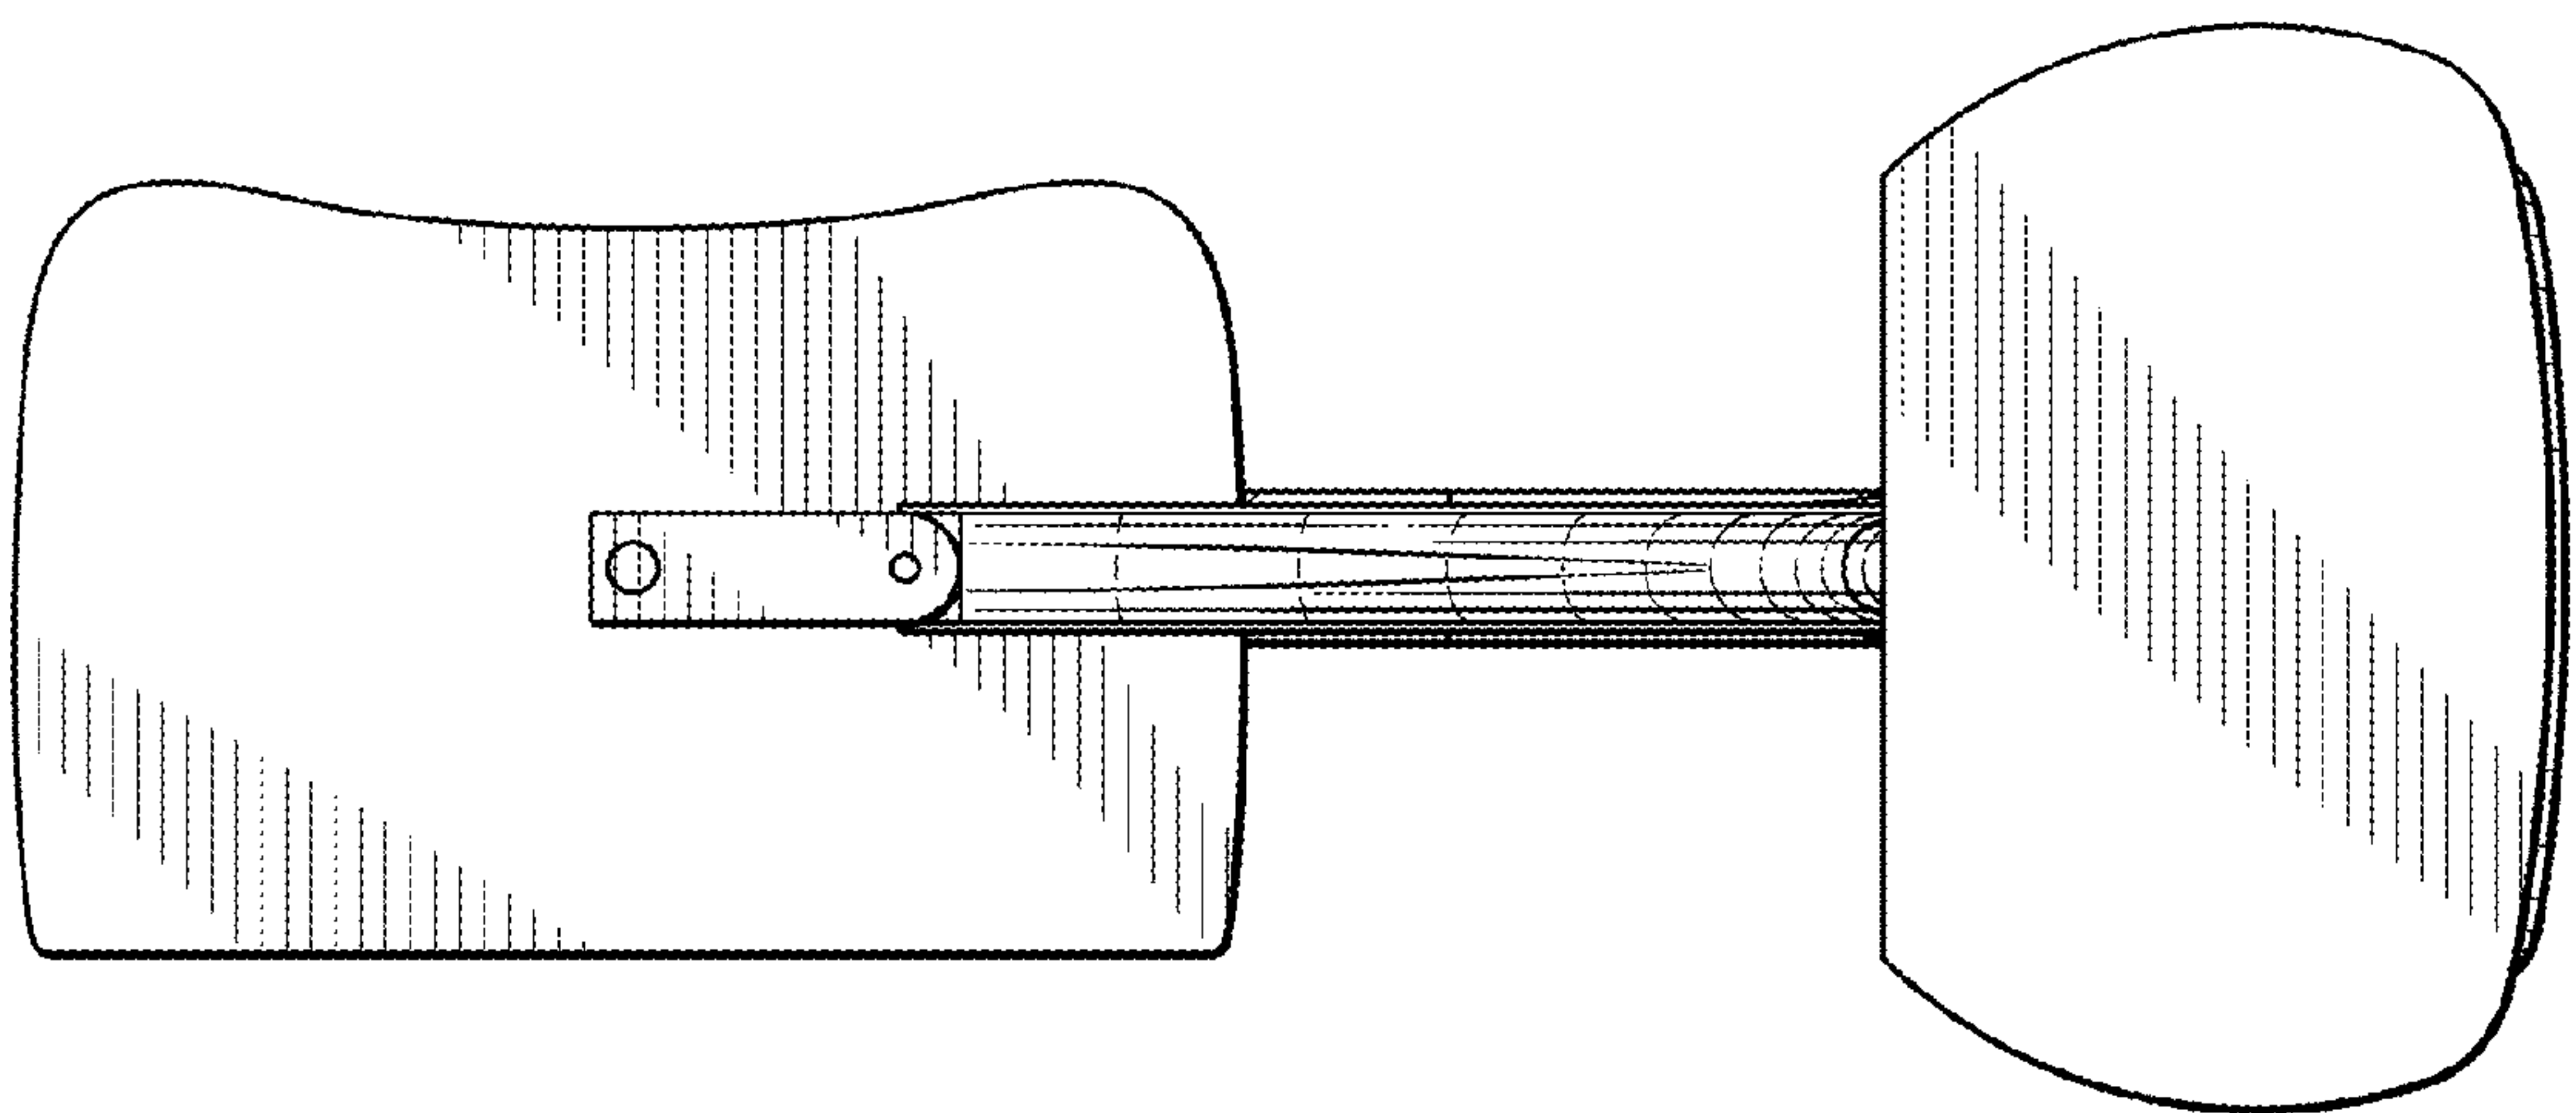


FIG. 8