



US00D621293S

(12) **United States Design Patent**  
**Lawrence**

(10) **Patent No.:** **US D621,293 S**

(45) **Date of Patent:** **\*\* Aug. 10, 2010**

(54) **GASTRIC BYPASS MEDICAL ALERT  
DEVICE**

D562,717 S \* 2/2008 Gonzales ..... D11/3  
D575,663 S \* 8/2008 Hayden ..... D11/79

\* cited by examiner

(76) Inventor: **Nadine Lawrence**, 2093 Creek Run Dr.,  
Brunswick, OH (US) 44212

*Primary Examiner*—Ralf Seifert

(74) *Attorney, Agent, or Firm*—Howard M. Cohn

(\*\*) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/352,027**

I claim the ornamental design of a gastric bypass medical alert device, as shown and described.

(22) Filed: **Dec. 15, 2009**

**DESCRIPTION**

(51) **LOC (9) Cl.** ..... **11-03**

FIG. 1 is a perspective view showing my gastric bypass medical alert device.

(52) **U.S. Cl.** ..... **D11/102; D11/116**

FIG. 2 is a front elevation view showing my gastric bypass medical alert device.

(58) **Field of Classification Search** ..... D11/1–2,  
D11/40–41, 43–50, 53, 56, 60, 63, 65, 67,  
D11/75–78.1, 86, 89, 95–105, 108–109, 115–116,  
D11/81, 54, 61, 79; 63/1.11, 1.12, 1.13,  
63/1.14, 1.16, 1.18, 13, 14.1, 35, 38, 39  
See application file for complete search history.

FIG. 3 is a top plan view showing my gastric bypass medical alert device.

FIG. 4 is a left side elevation view showing the left side portion of my gastric bypass medical alert device.

(56) **References Cited**

FIG. 5 is a rear elevation view showing my gastric bypass medical alert device.

**U.S. PATENT DOCUMENTS**

FIG. 6 is a right elevation view showing my gastric bypass medical alert device; and,


- D252,196 S \* 6/1979 Gehrke ..... D11/115
- D291,977 S \* 9/1987 Sebring ..... D11/54
- D301,558 S \* 6/1989 Fontana ..... D10/126
- D302,533 S \* 8/1989 Hagee ..... D11/104
- D406,784 S \* 3/1999 Thompson ..... D11/3
- D463,994 S \* 10/2002 Eisen ..... D11/96

FIG. 7 is a bottom plan view showing my gastric bypass medical alert device.

In the drawings, the surface shading represents the surface of the gastric bypass medical alert device.

**1 Claim, 2 Drawing Sheets**



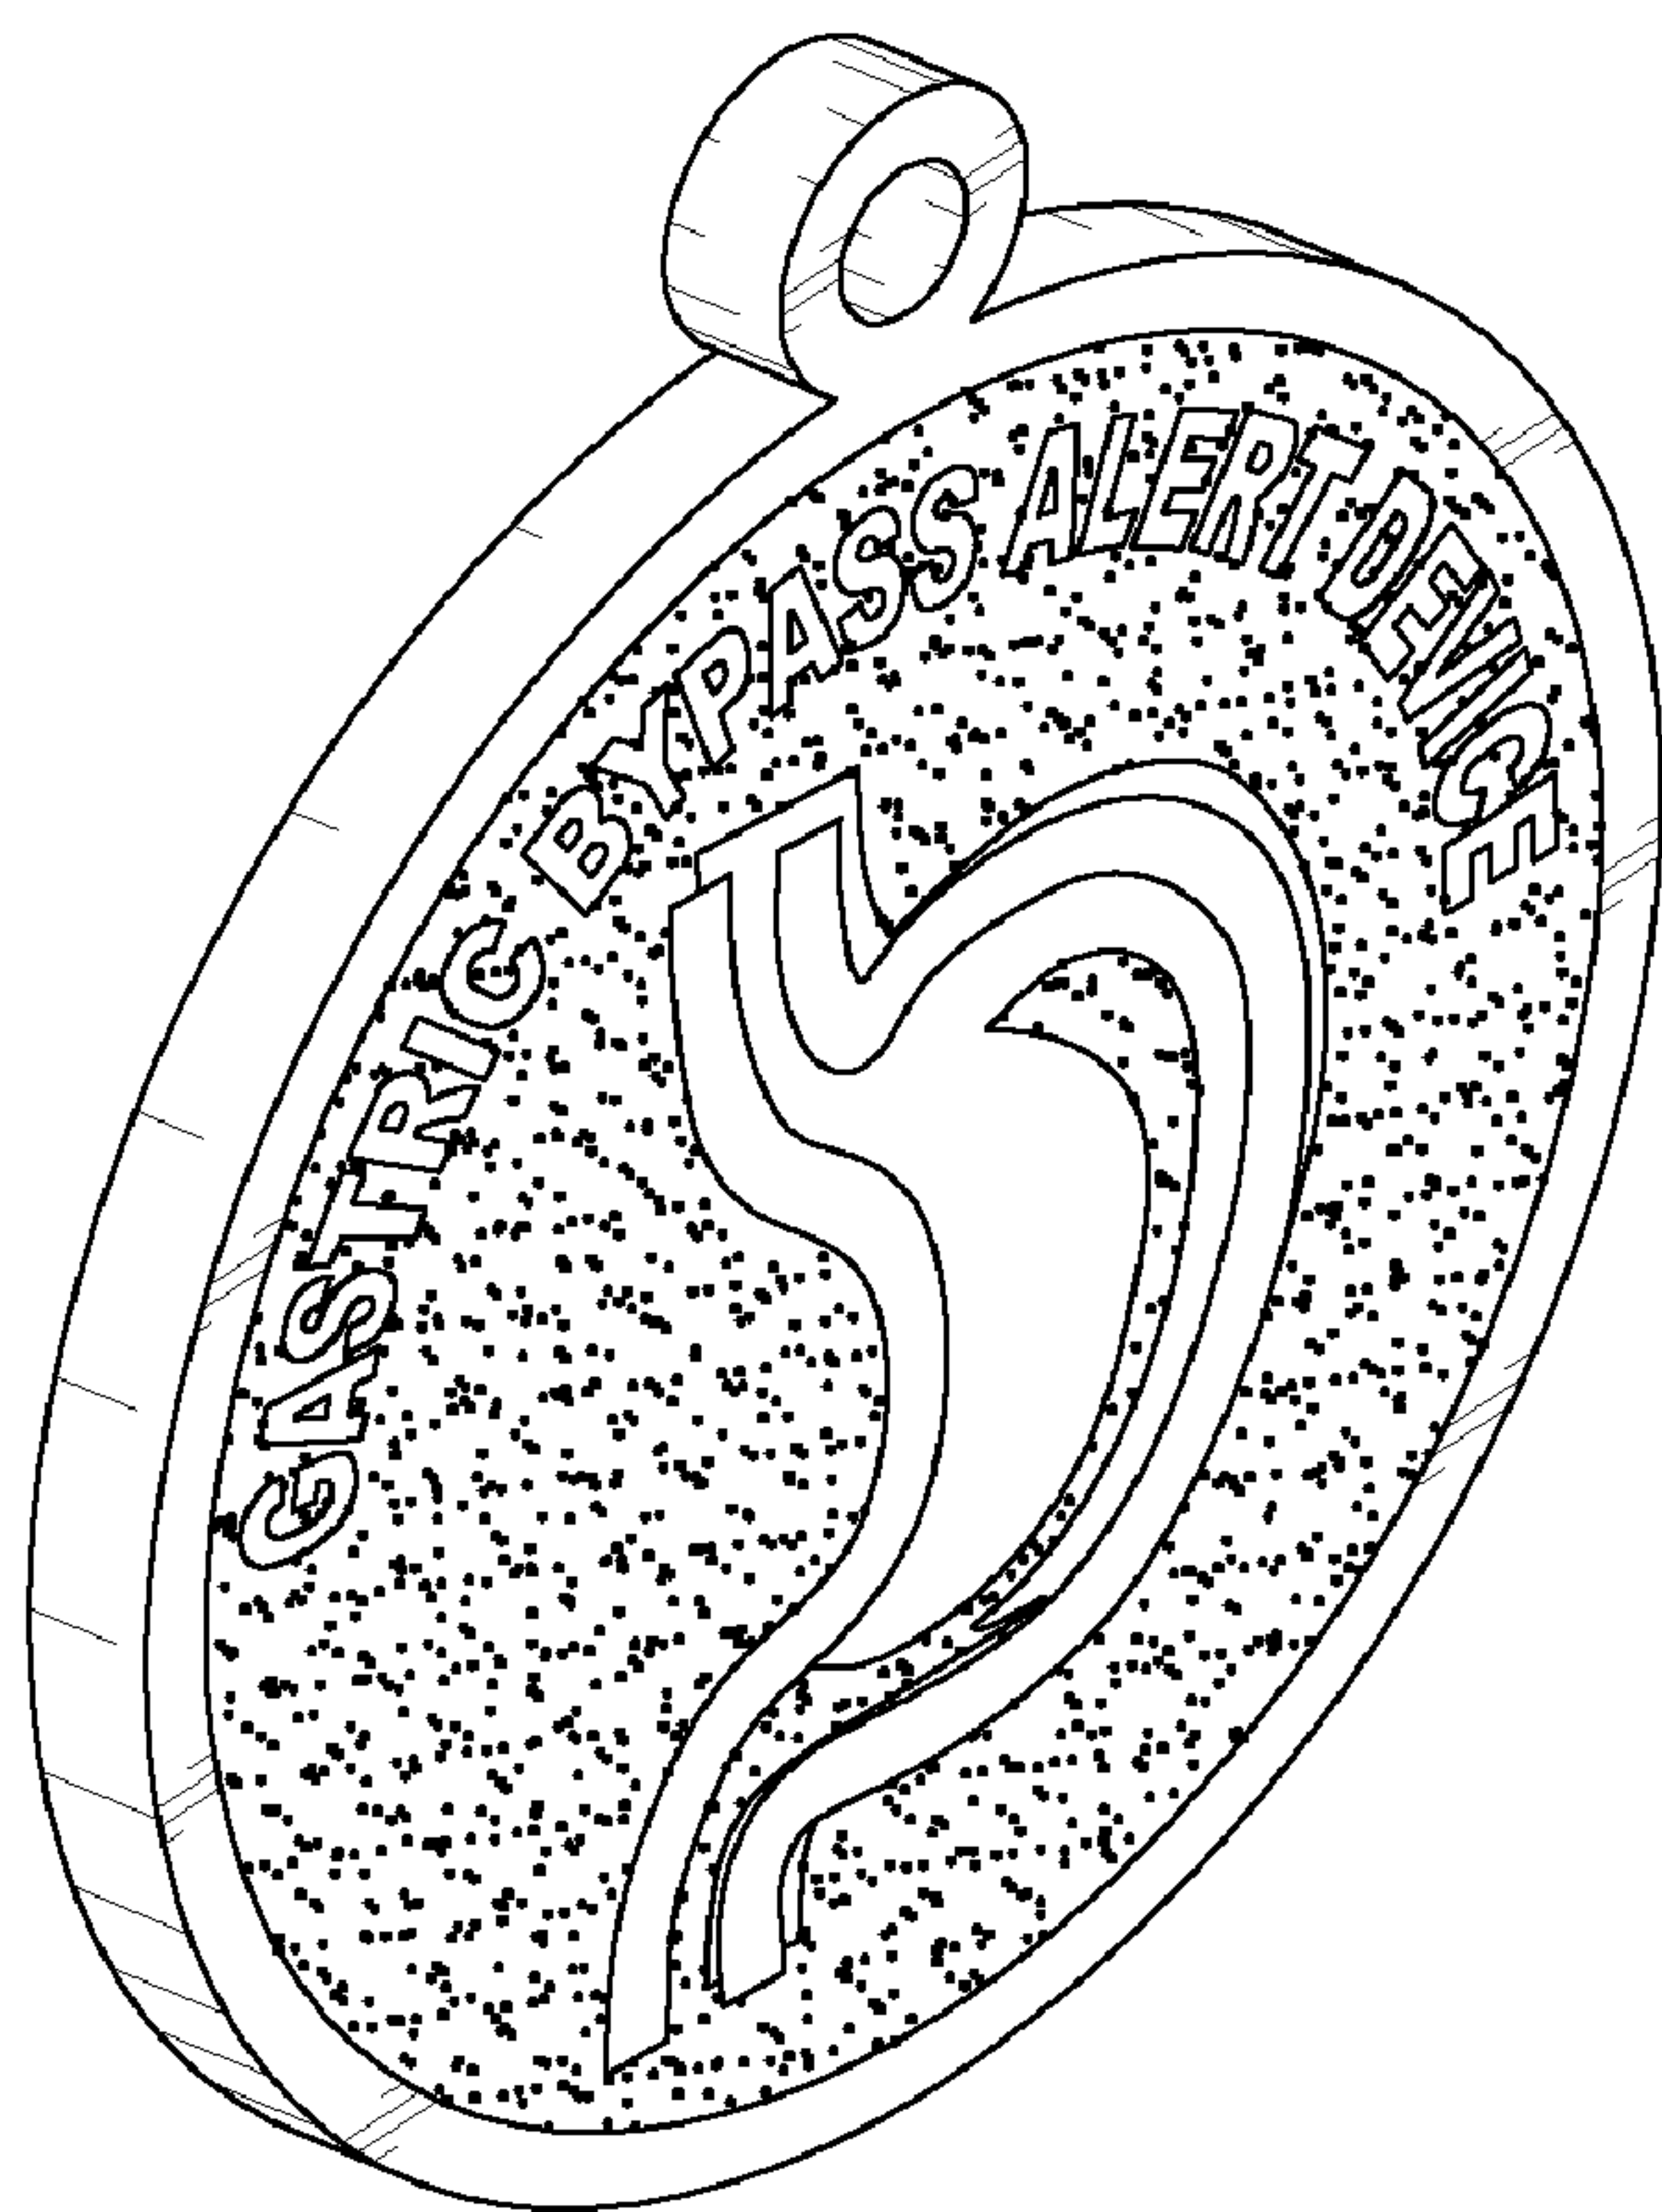

**FIG. 1**



**FIG. 2**



**FIG. 3**



**FIG. 4**

**FIG. 5**

**FIG. 6**



**FIG. 7**