

US00D621935S

(12) **United States Design Patent**  
**Cole et al.**

(10) **Patent No.:** **US D621,935 S**  
(45) **Date of Patent:** **\*\* Aug. 17, 2010**

(54) **STETHOSCOPE CLEANING ASSEMBLY**

D445,185 S \* 7/2001 Najmi ..... D24/134  
6,484,918 B1 \* 11/2002 Lefebvre ..... 224/670  
6,575,917 B2 6/2003 Giroux et al.  
7,258,125 B2 8/2007 Holbrook  
7,282,186 B2 10/2007 Lake, Jr. et al.  
7,406,973 B1 8/2008 Perlman et al.

(76) Inventors: **Michael R. Cole**, 10 Wedgewood Dr.,  
Stratham, NH (US) 03885; **Mathew**  
**Cardinali**, 28A Dearborn St.,  
Portsmouth, NH (US) 03801; **James M.**  
**Sellers**, 83 Garrison Dr., Eliot, ME (US)  
03903; **Michael Perlman**, 2210 SW.  
102nd Dr, Davie, FL (US) 33324; **Keith**  
**Rubin**, 2100 N. Ocean Blvd., Unit #501,  
Fort Lauderdale, FL (US) 33305

(Continued)

**FOREIGN PATENT DOCUMENTS**

WO WO 02/094326 A1 11/2002

(\*\*) Term: **14 Years**

(Continued)

(21) Appl. No.: **29/310,257**

**OTHER PUBLICATIONS**

(22) Filed: **Aug. 5, 2008**

Dix, et al., "Environmental Surface Cleaning First Defense Against  
Infectious Agents." [http://www.vpico.com/articlemanager/  
printerfriendly.aspx?article=60960](http://www.vpico.com/articlemanager/printerfriendly.aspx?article=60960); Dec. 2, 2006; 7pg.

**Related U.S. Application Data**

(Continued)

(63) Continuation-in-part of application No. 12/079,077,  
filed on Mar. 24, 2008, now Pat. No. 7,503,335, which  
is a continuation-in-part of application No. 11/728,  
207, filed on Mar. 23, 2007, now Pat. No. 7,406,973.

*Primary Examiner*—Ian Simmons  
*Assistant Examiner*—Christopher Lee  
(74) *Attorney, Agent, or Firm*—Malloy & Malloy, P.A.

(51) **LOC (9) Cl.** ..... **24-02**

(57) **CLAIM**

(52) **U.S. Cl.** ..... **D24/134**

(58) **Field of Classification Search** ..... D24/134,  
D24/135, 165, 140; D6/567; 181/131–137;  
600/528

The ornamental design for a stethoscope cleaning assembly,  
as shown and described.

See application file for complete search history.

**DESCRIPTION**


(56) **References Cited**

FIG. 1 is a front perspective view illustrating my design for a  
stethoscope cleaning assembly;  
FIG. 2 is a front view thereof;  
FIG. 3 is a left side view thereof;  
FIG. 4 is a top view thereof view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a bottom view thereof; and  
FIG. 7 is a rear view thereof; and,  
FIG. 8 is a rear perspective thereof.

**U.S. PATENT DOCUMENTS**

4,449,976 A 5/1984 Kamen  
5,048,549 A 9/1991 Hethcoat  
5,114,670 A 5/1992 Duffey  
5,185,532 A 2/1993 Zabsky et al.  
D375,161 S \* 10/1996 Hart ..... D24/134  
5,641,464 A 6/1997 Briggs, III et al.  
5,692,657 A \* 12/1997 Kilo et al. .... 224/269  
5,865,551 A 2/1999 Lalli et al.  
5,892,233 A 4/1999 Clement  
6,018,835 A 2/2000 Schonfeld  
D425,353 S \* 5/2000 Foy ..... D6/567

**1 Claim, 6 Drawing Sheets**

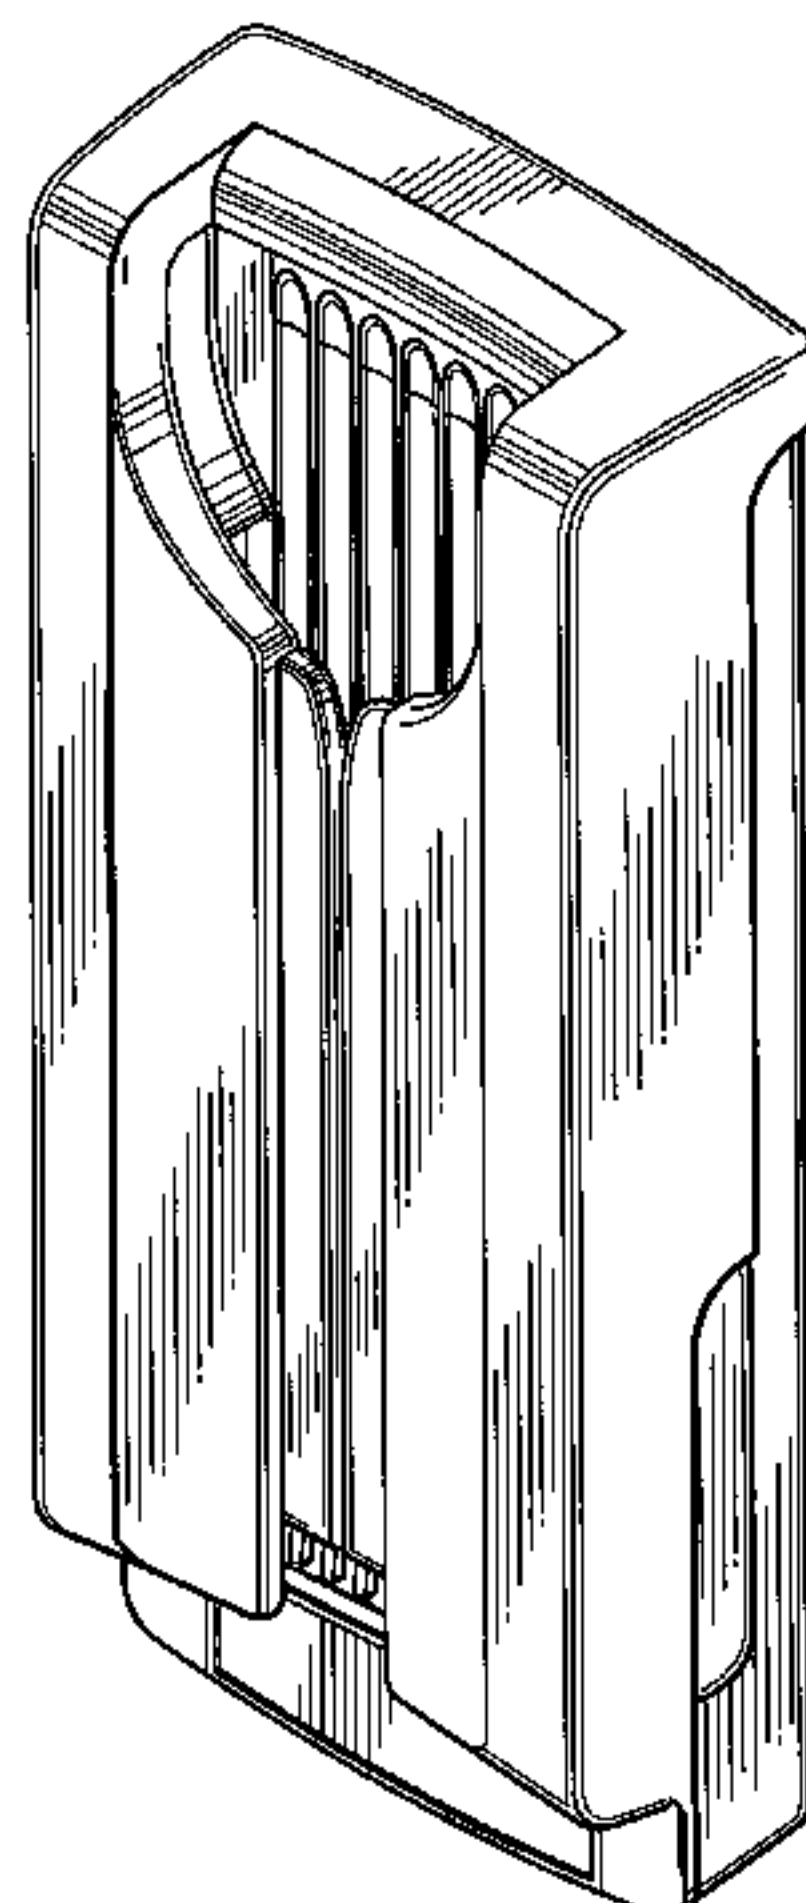

U.S. PATENT DOCUMENTS

7,503,335 B2 3/2009 Perlman et al.  
2002/0146343 A1 10/2002 Jenkins et al.  
2002/0198564 A1 12/2002 Pichon et al.  
2004/0258560 A1 12/2004 Lake, Jr. et al.  
2005/0214185 A1 9/2005 Castaneda  
2005/0236579 A1 10/2005 Jenkins et al.  
2005/0254992 A1 11/2005 Jenkins et al.  
2007/0080017 A1 4/2007 Stickley  
2007/0256753 A1 11/2007 Riley  
2008/0019889 A1 1/2008 Rogers et al.  
2009/0144918 A1 6/2009 Perlman et al.

FOREIGN PATENT DOCUMENTS

WO WO 2008/118311 A2 10/2008  
WO WO 2008/118401 A2 10/2008

OTHER PUBLICATIONS

Virgo Publishing., "A Clean Sweep: Surface Cleaning in the Healthcare Environment." <http://www.vpico.com/articlemanager/printerfriendly.aspx?article=60253>; Dec. 1, 2004; 3 pg.

McCaughey., "Coming Clean—New York Times." <http://www.nytimes.com/2005/06/06/opinion/06mccaughey.html?ei=5088&en=d591e517f...>; Dec. 2, 2006; 1 pg.  
Sharmila et al., "Stethoscope and Nosocomial Infection," *Indian Journal of Pediatrics*, 2000; 67 (3): 197-199.  
Marinella, et al., "The Stethoscopy: A Potential Source of Nosocomial Infection?," vol. 157(7), Apr. 14, 1997, pp. 786-790, Mar. 30, 2006.  
Jones, et al., "Stethoscopes: A Potential Vector of Infection?" *Annals of Emergency Medicine*. 26:3 Sep. 1995; 296-299.  
CDC, "Contact Precautions from the Guidelines for Isolation Precautions in Hospitals (Jan. 1996)." [http://www.cdc.gov/ncidod/dhqp/gl\\_isolation\\_contact.html](http://www.cdc.gov/ncidod/dhqp/gl_isolation_contact.html); Dec. 2, 2006; 2 pg.  
CDC, "Standard Precautions from the Guidelines for Isolation Precautions in Hospitals (Jan. 1996)." [http://www.cdc.gov/ncidod/dhqp/gl\\_isolation\\_standar.html](http://www.cdc.gov/ncidod/dhqp/gl_isolation_standar.html); Dec. 2, 2006; 2 pg.  
Schneider, "Report of the Council on Science and Public Health—CSAPH's Sunet Review of 1996 House Policies".  
"American Medical Association Proceedings of the House of Delegates," 50th Interim Meeting, Dec. 8-11, 1996. Resolution 501. Policy H-440. 908.

\* cited by examiner

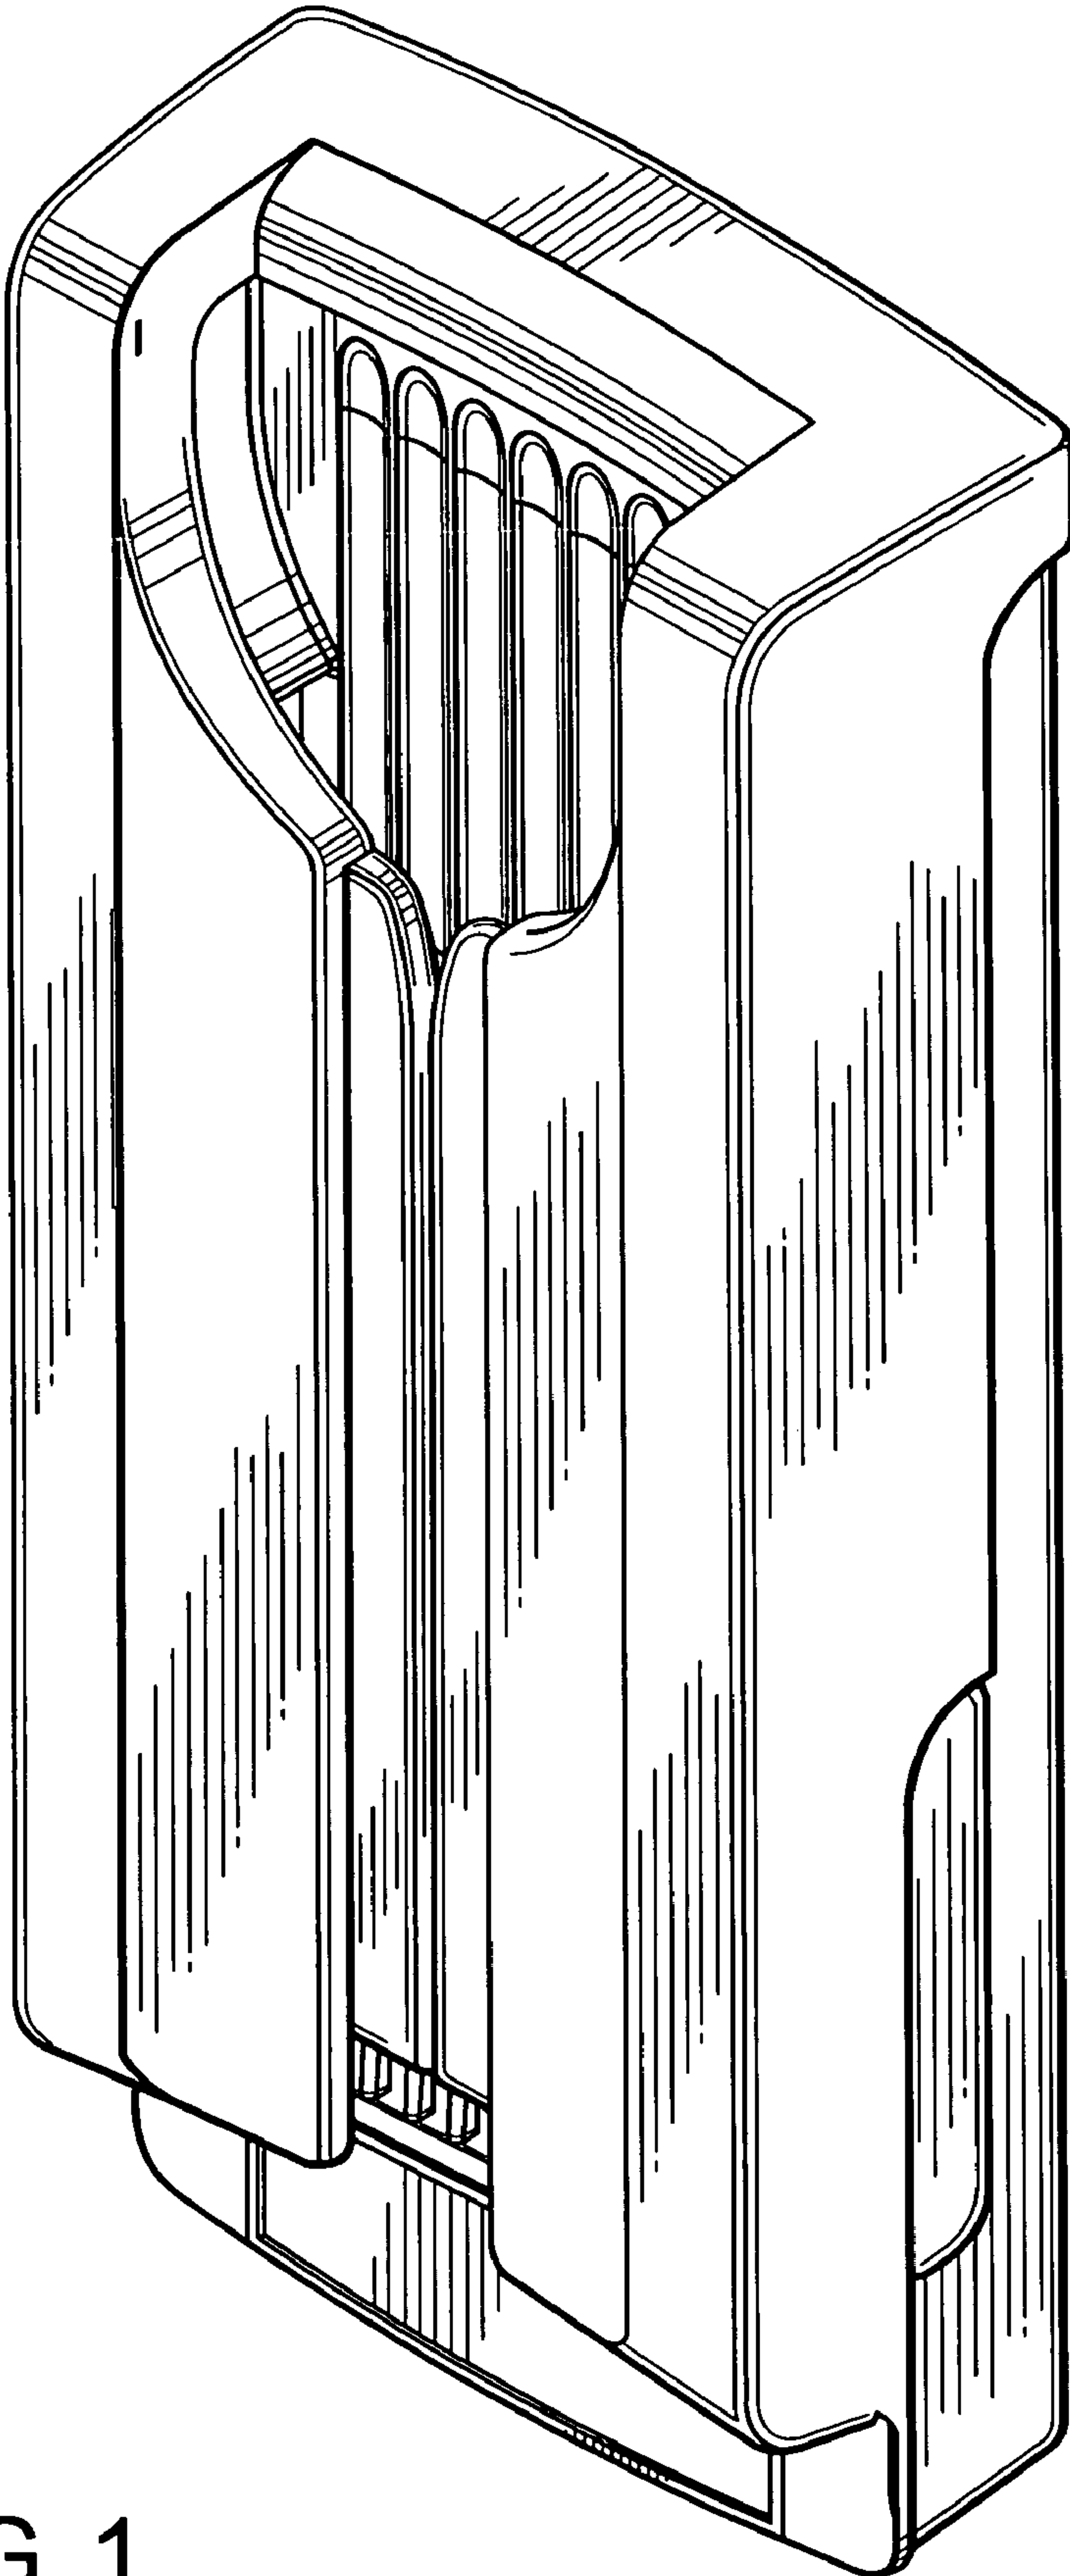


FIG. 1

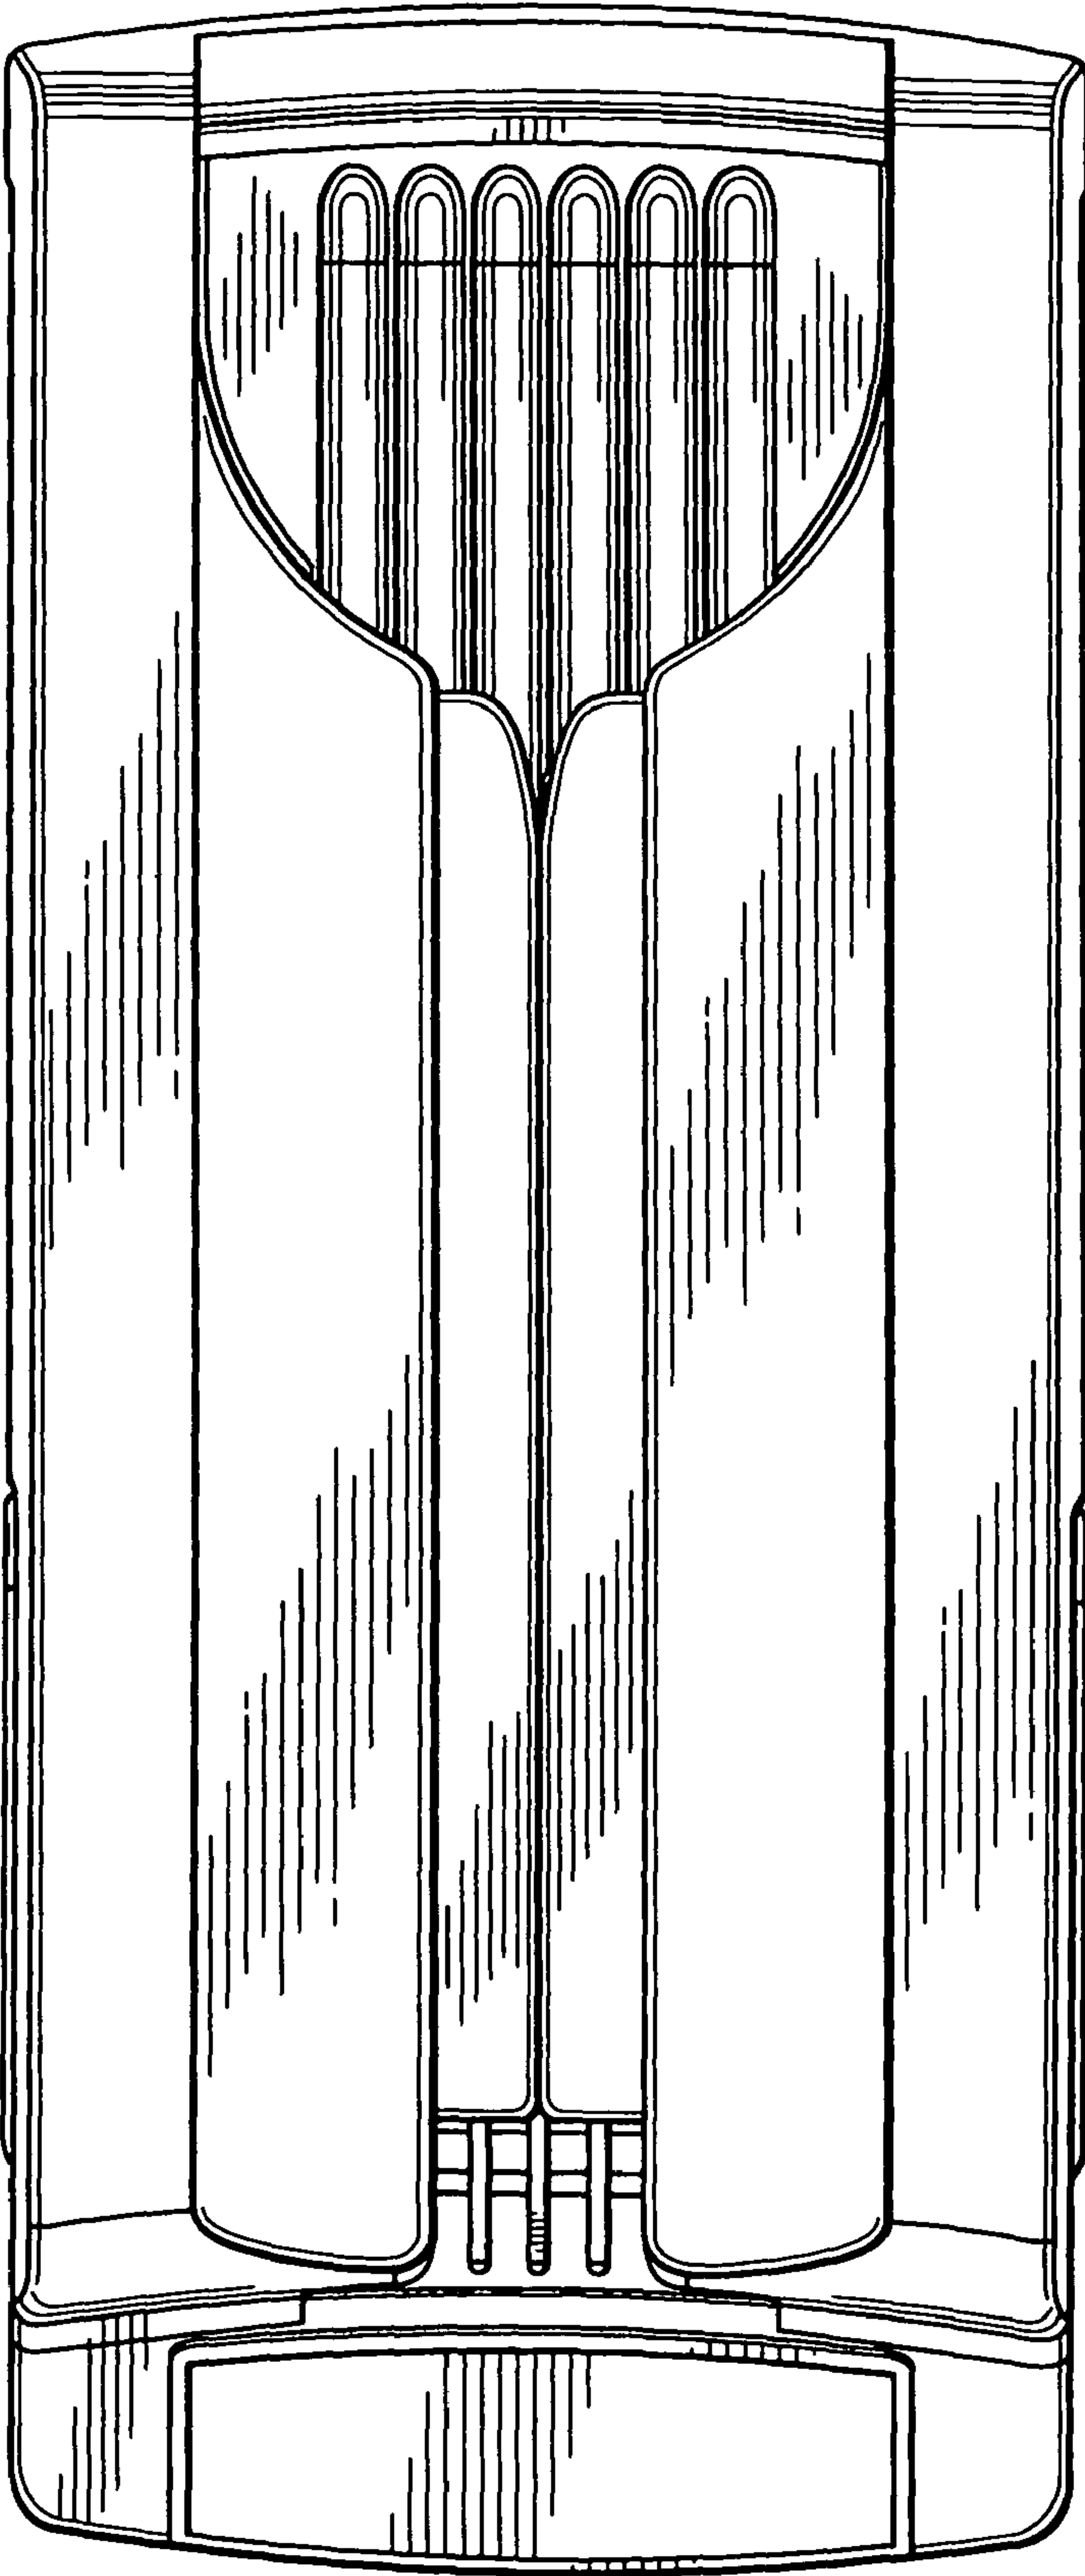


FIG. 2

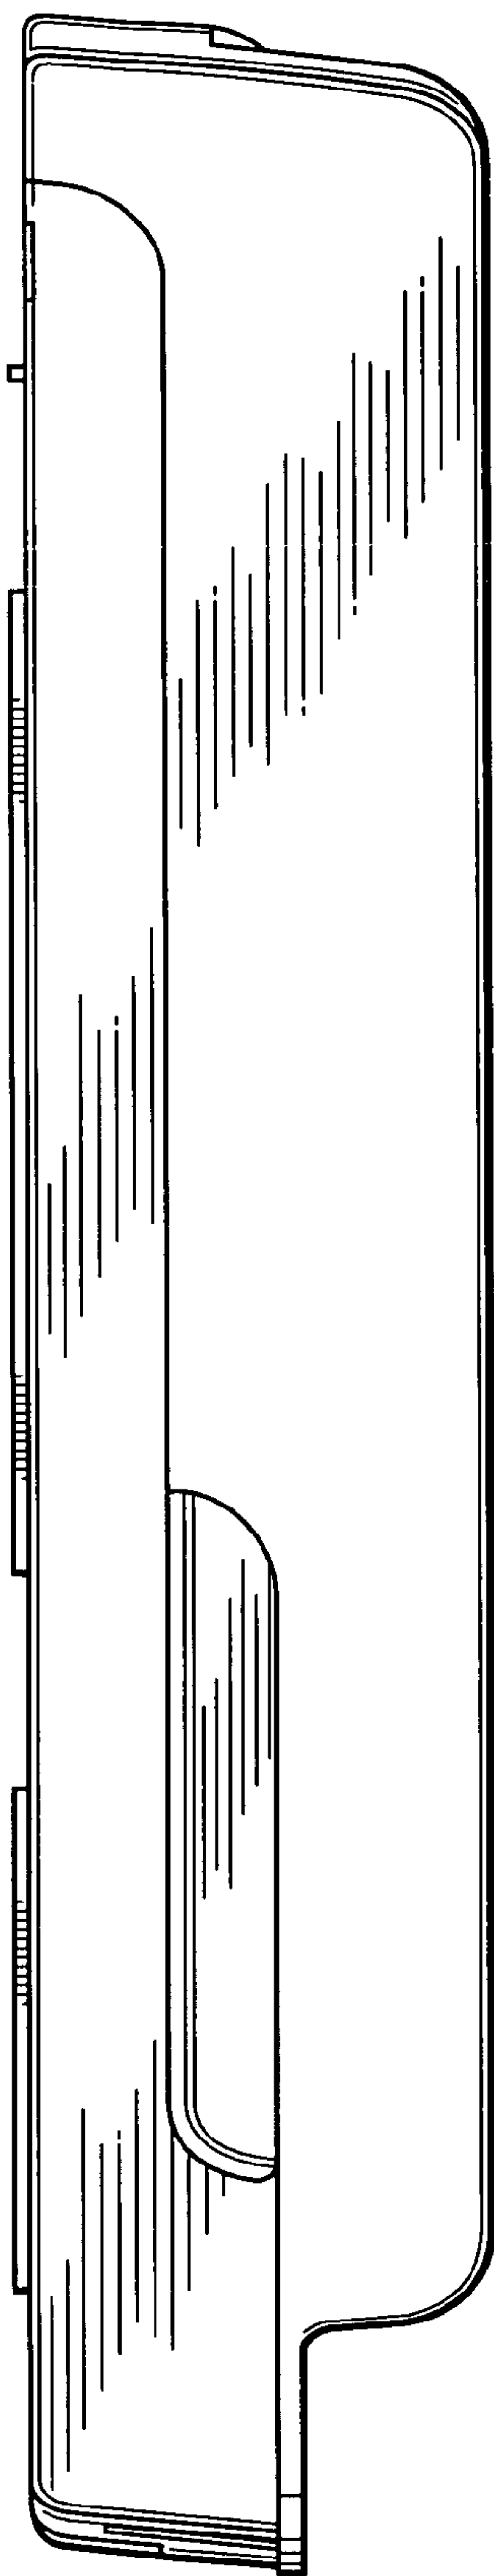


FIG. 3

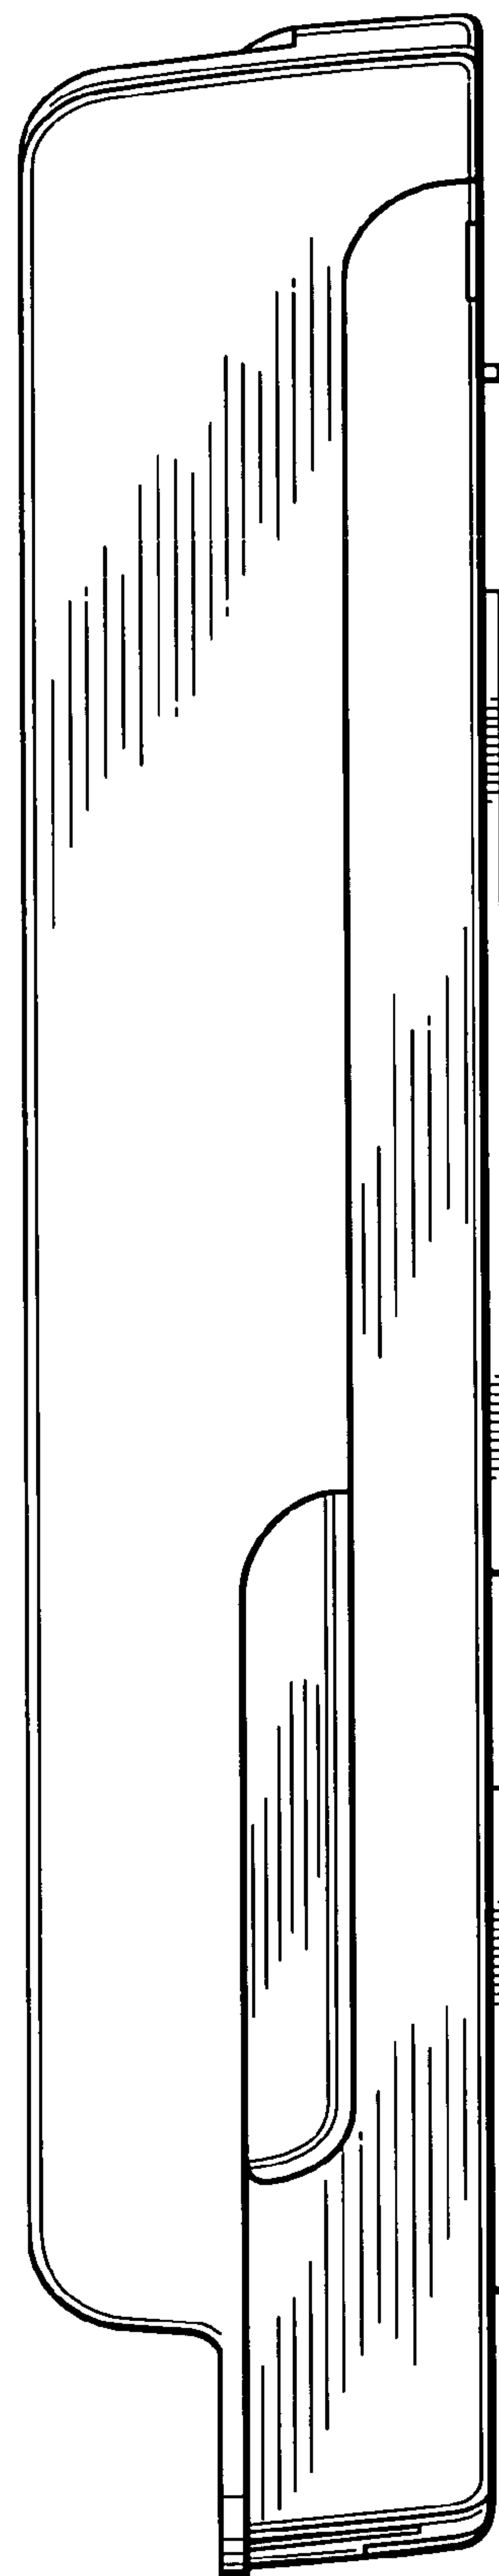


FIG. 5



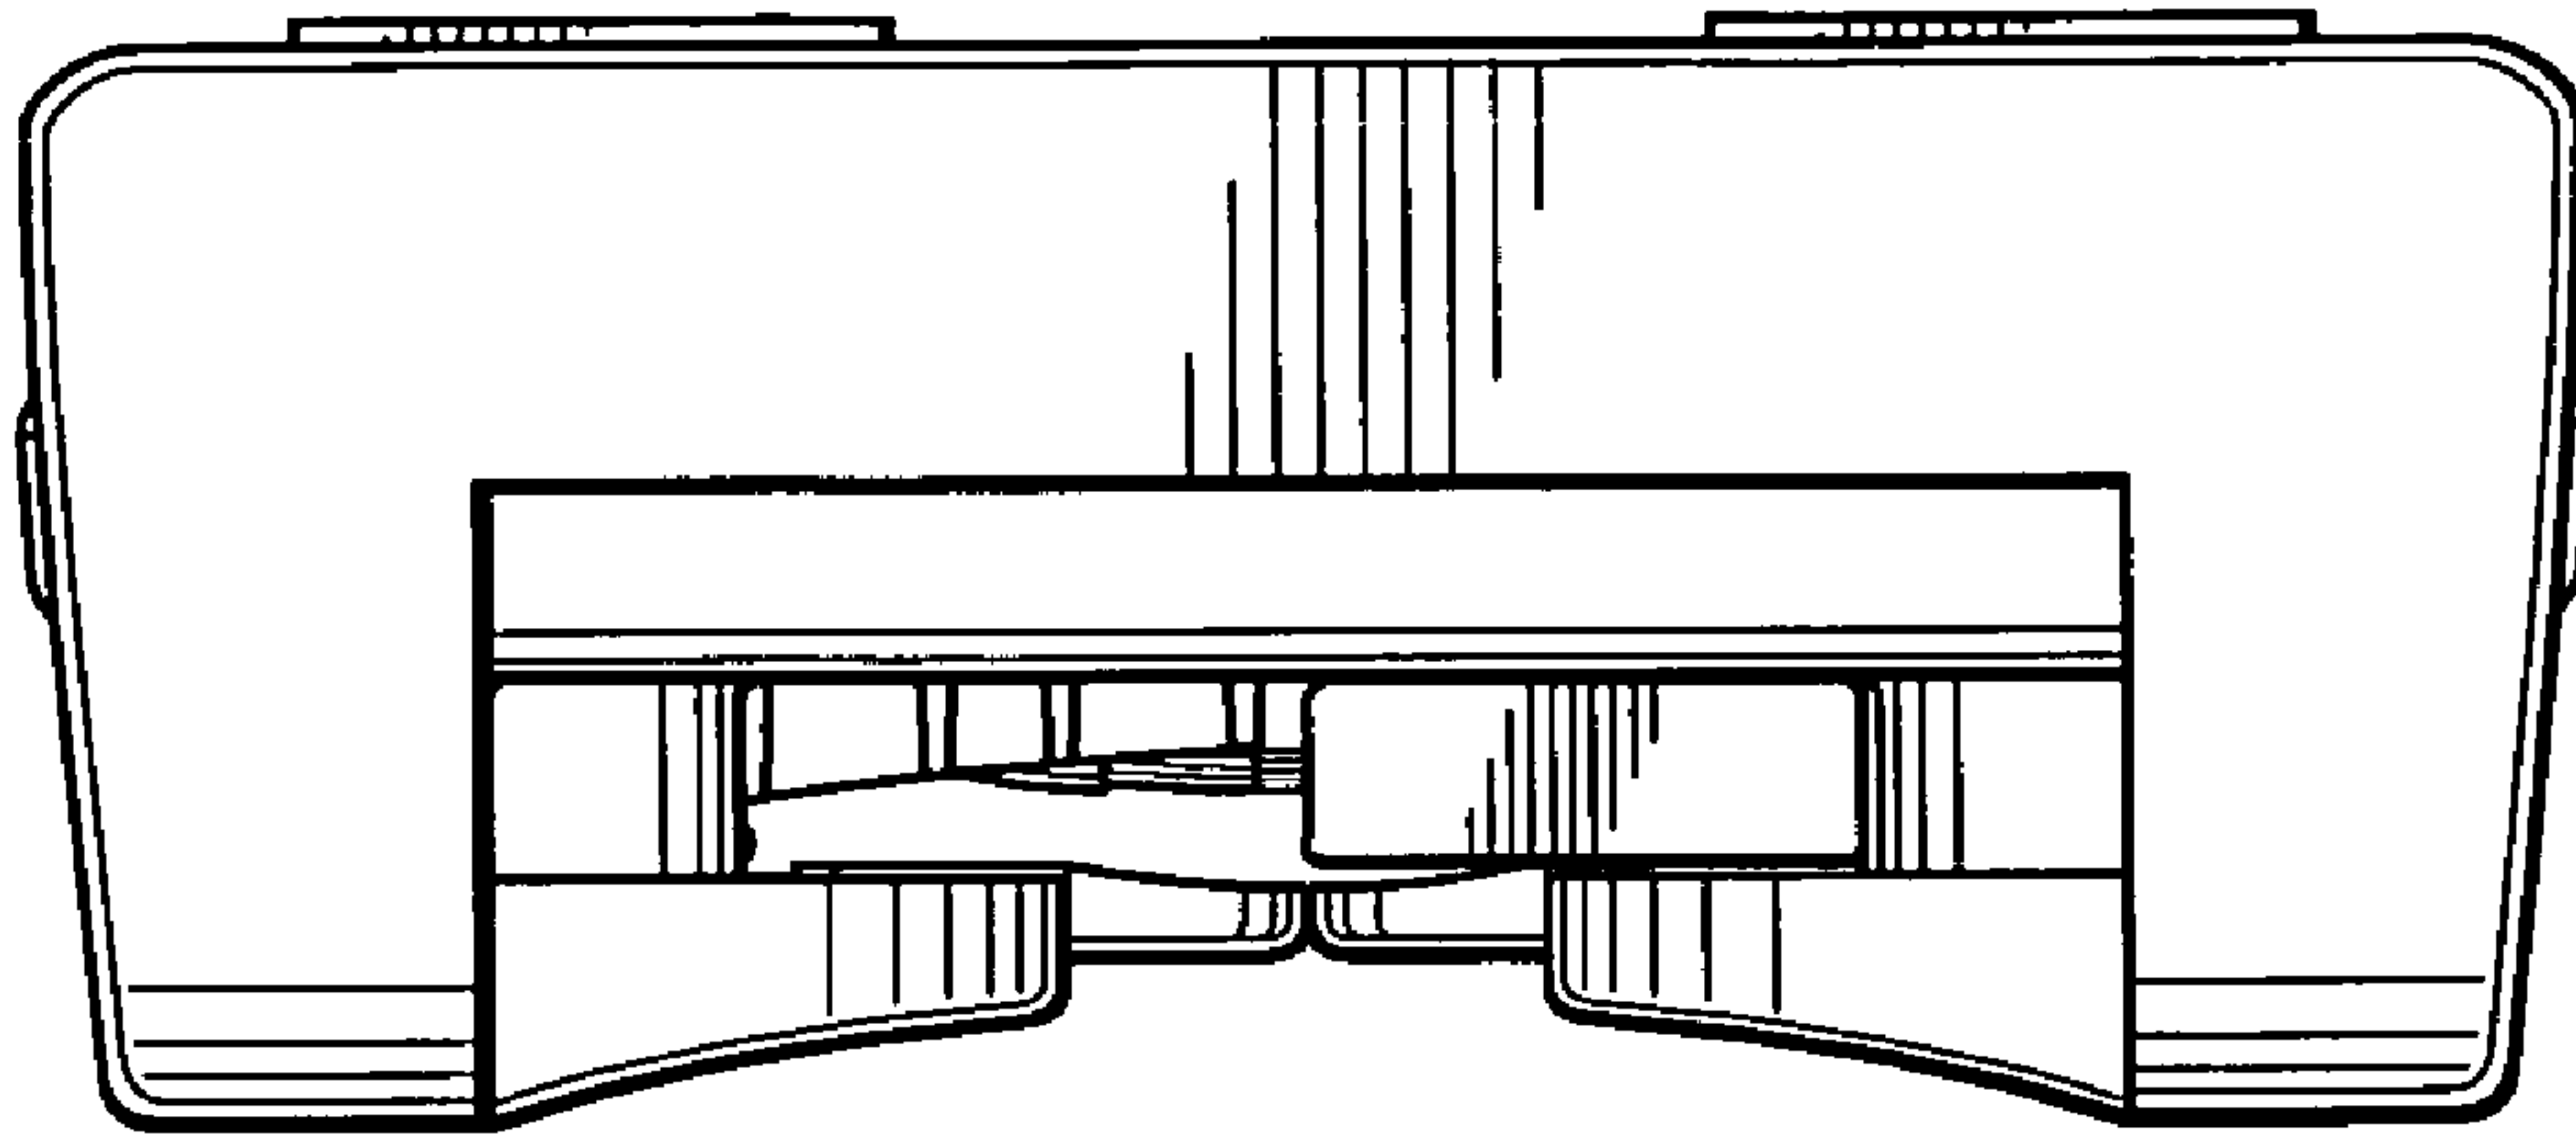


FIG. 4

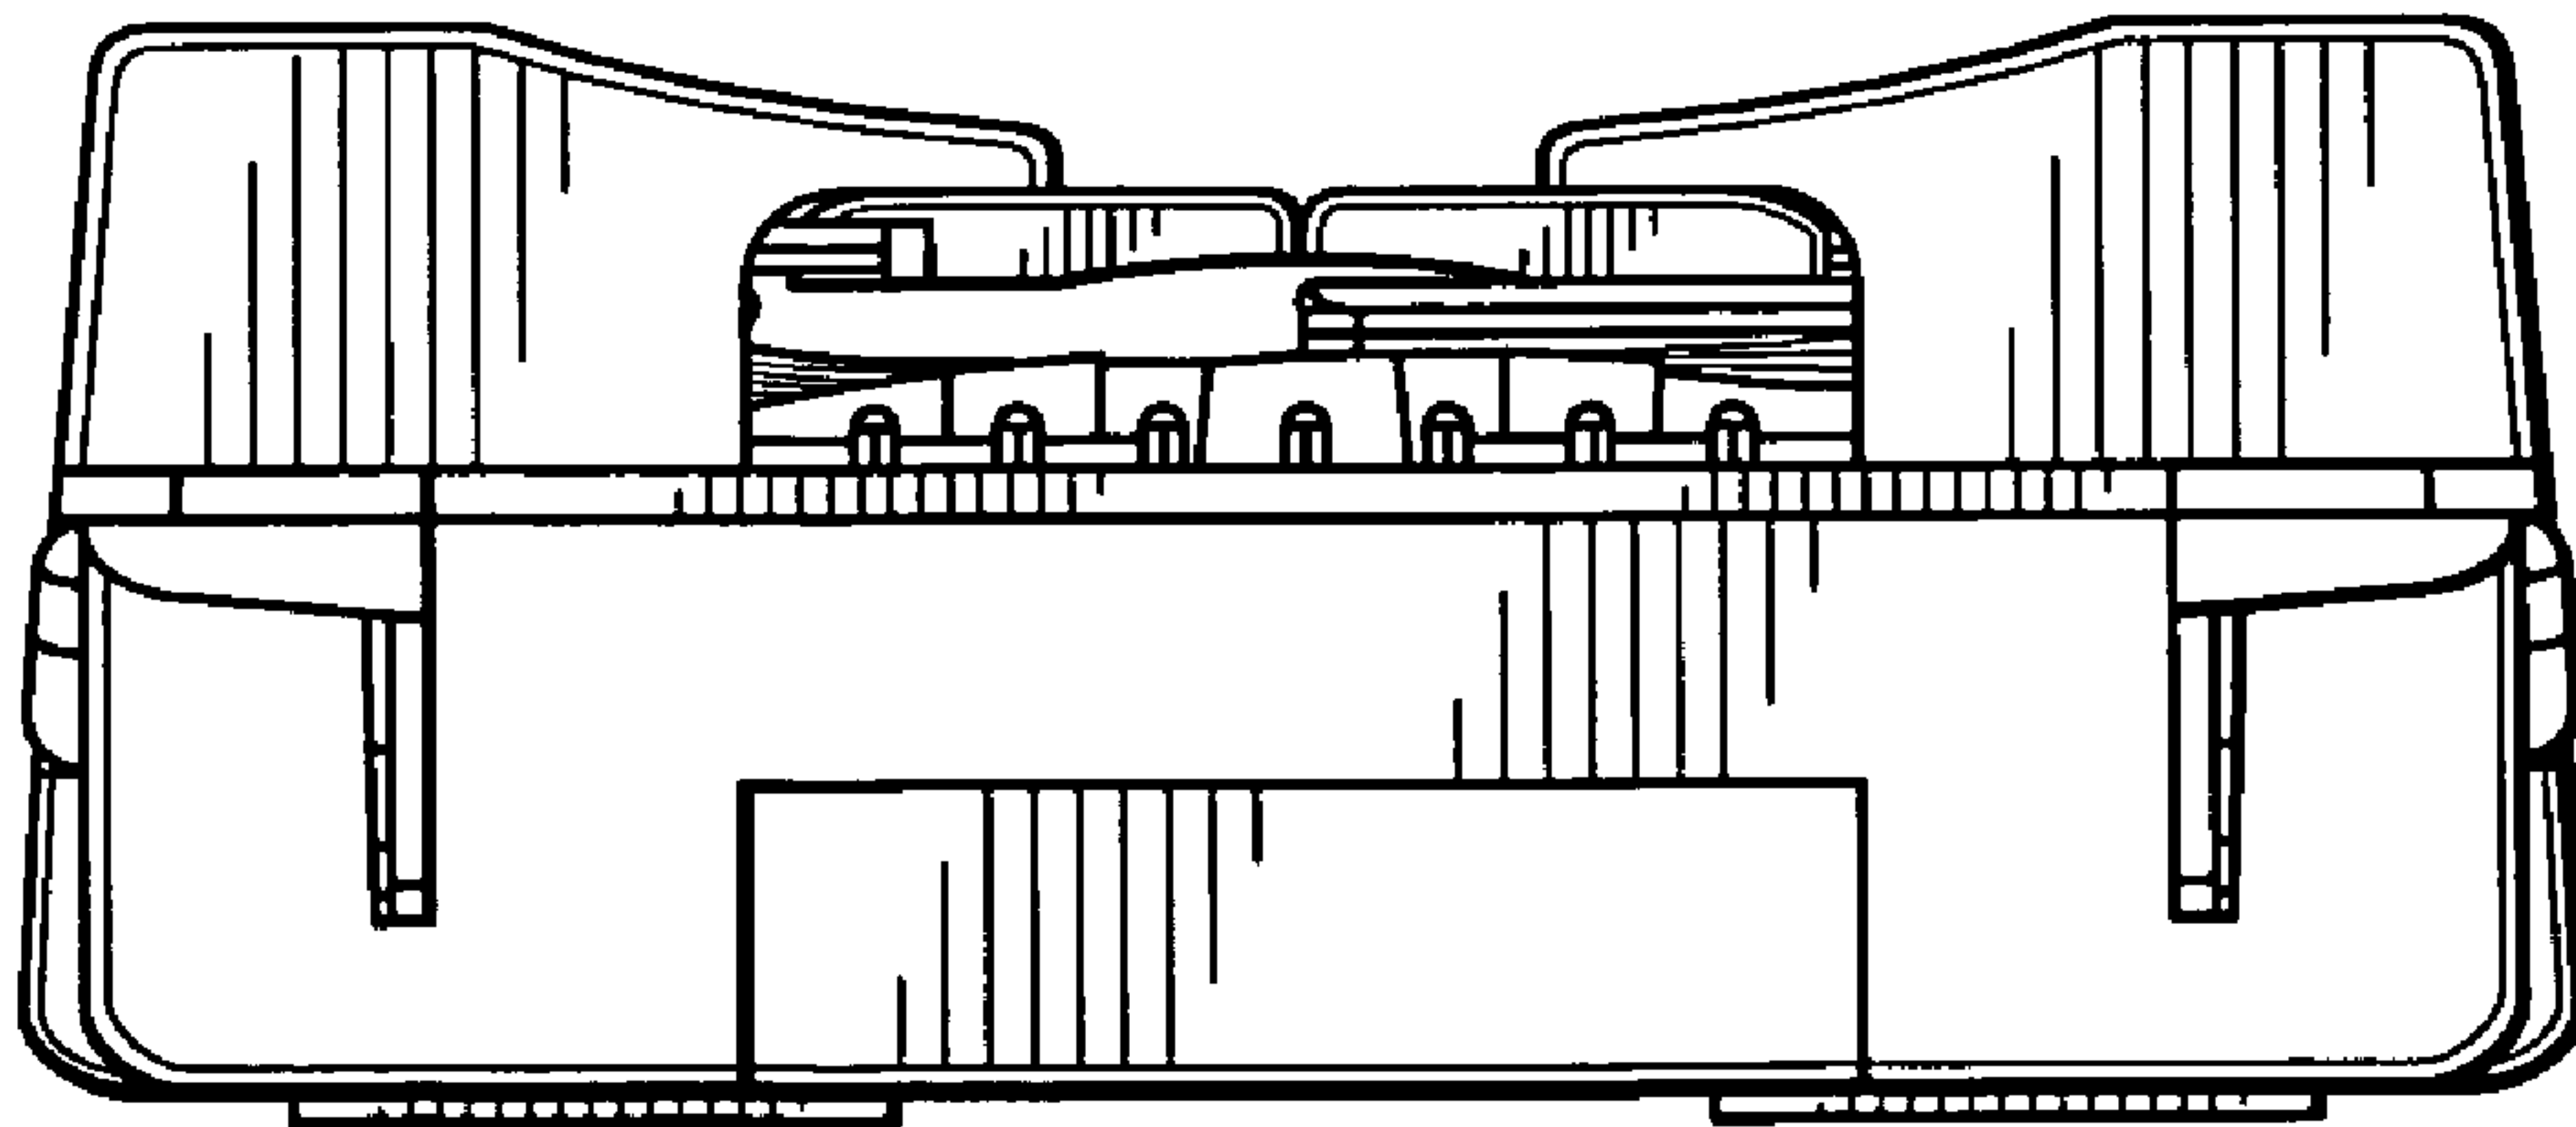


FIG. 6

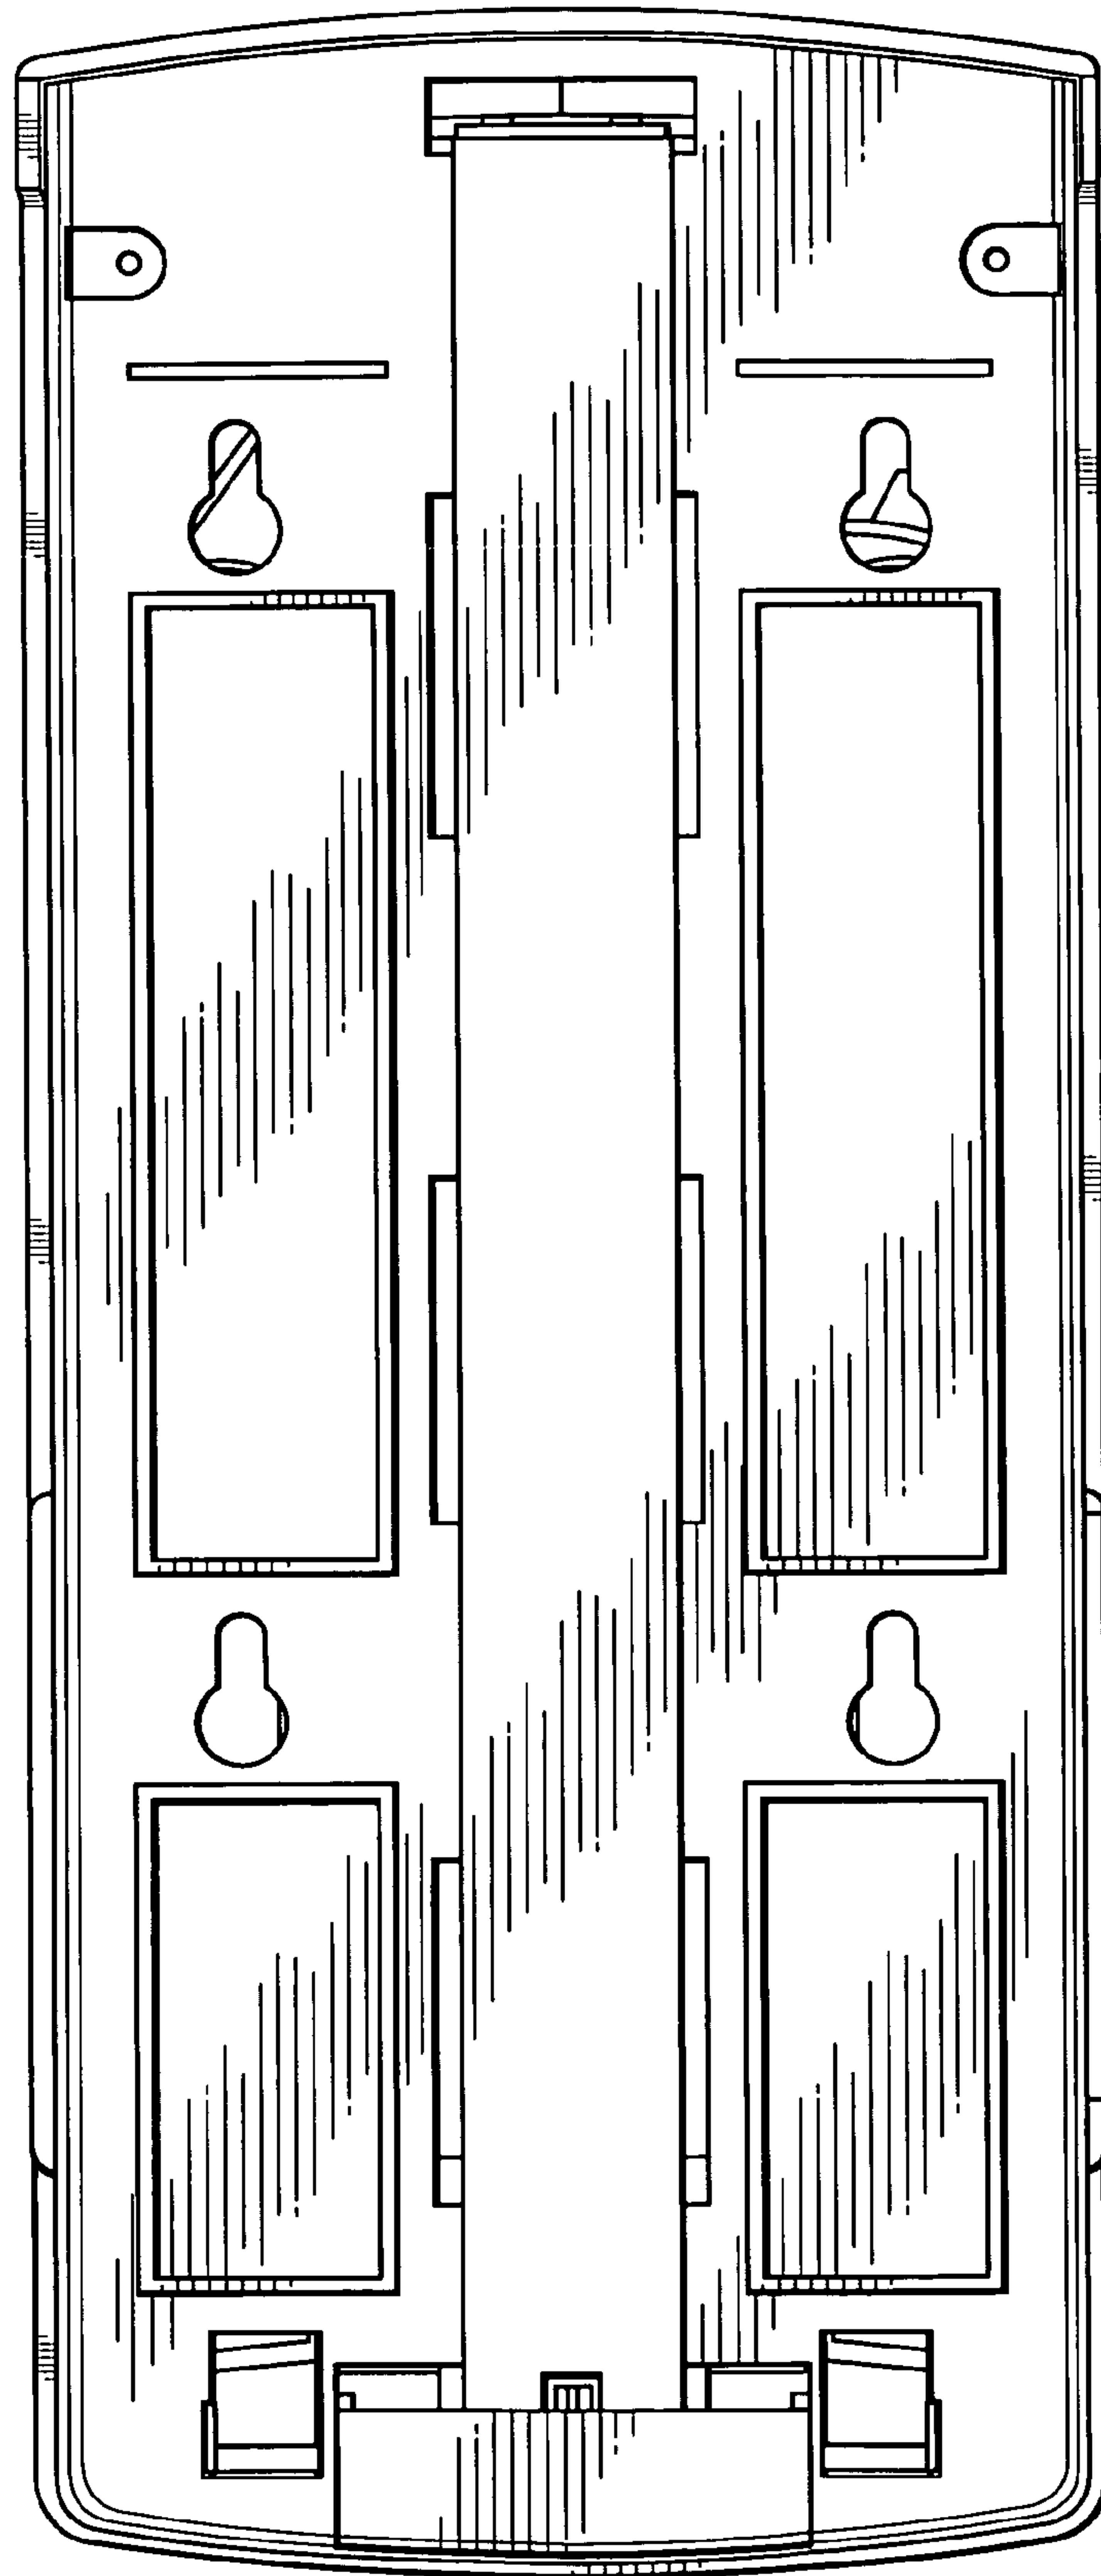


FIG. 7

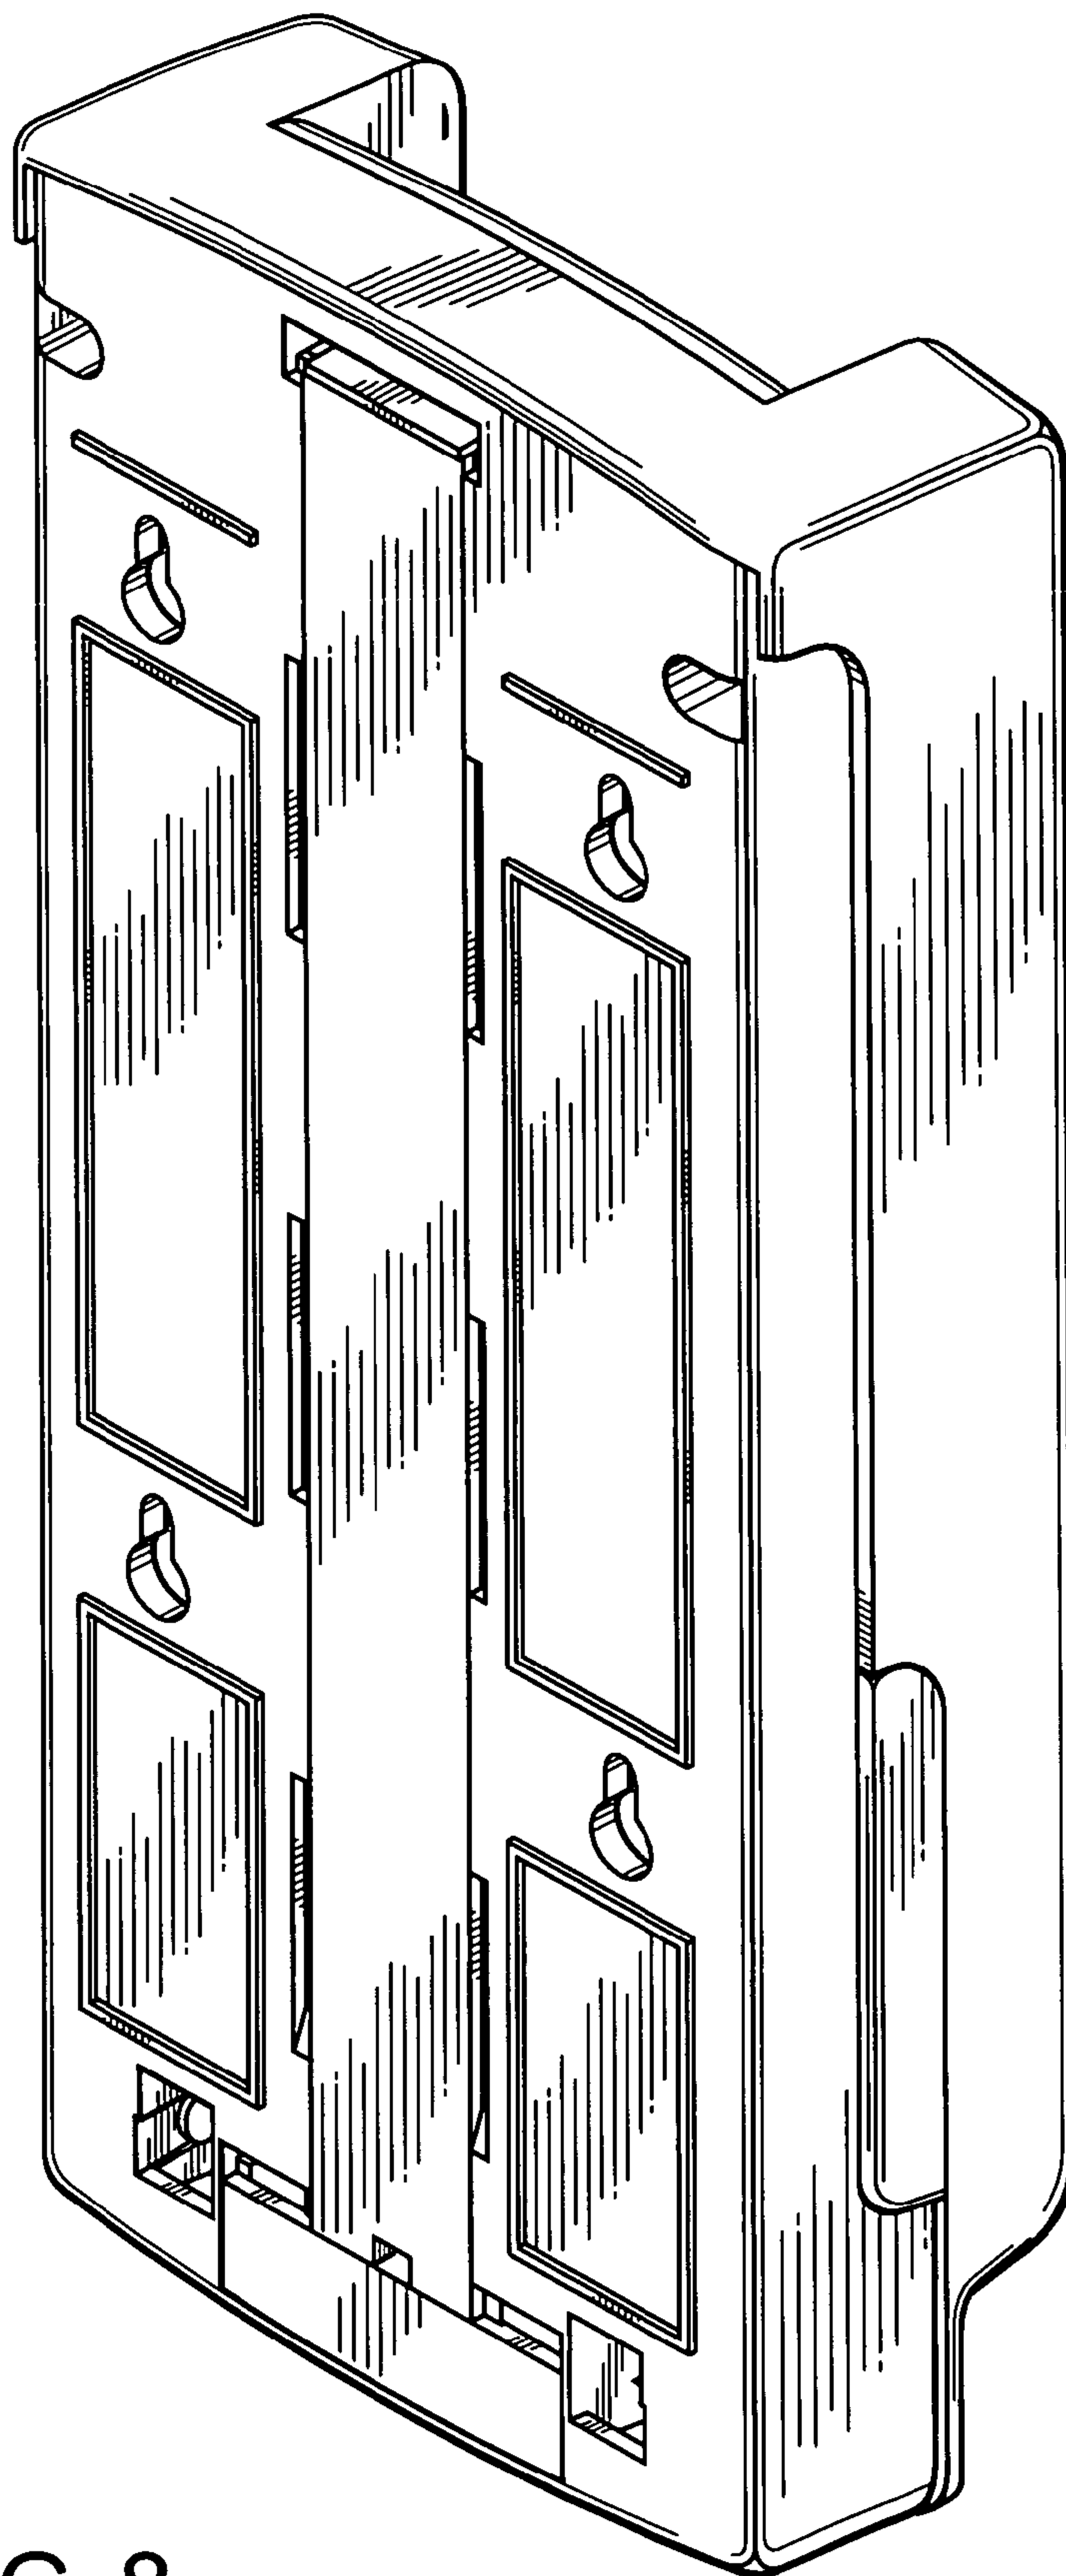


FIG. 8