



US00D622374S

(12) **United States Design Patent**
Julian et al.

(10) **Patent No.:** **US D622,374 S**

(45) **Date of Patent:** **** *Aug. 24, 2010**

(54) **AUTOMATIC INJECTION DEVICE**

WO WO-08/005315 A2 1/2008

(75) Inventors: **Joseph F. Julian**, Libertyville, IL (US);
Steven Rolfe, Bischester (GB)

OTHER PUBLICATIONS

U.S. Appl. No. 29/265,646, filed Sep. 6, 2006.

(73) Assignee: **Abbott Biotechnology Ltd.**, Hamilton
(BM)

(Continued)

(*) Notice: This patent is subject to a terminal disclaimer.

Primary Examiner—T. Chase Nelson

Assistant Examiner—David G Muller

(74) *Attorney, Agent, or Firm*—McCarter & English, LLP;
David R. Burns; Ishna Neamatullah

(**) Term: **14 Years**

(57) **CLAIM**

(21) Appl. No.: **29/265,691**

The ornamental design for an automatic injection device, as shown and described.

(22) Filed: **Sep. 6, 2006**

(51) **LOC (9) Cl.** **24-02**

DESCRIPTION

(52) **U.S. Cl.** **D24/113**

(58) **Field of Classification Search** D24/114,
D24/113, 133, 112, 130, 147; 604/232, 187,
604/163, 207, 208, 227, 229, 132, 22, 19;
606/181, 185

FIG. 1 is a perspective view of the design with a top removable cap covering an activator button and a bottom removable cap covering an injection opening;

FIG. 2 is a front view of the design with the removable caps for the activator button and injection opening in covering positions;

See application file for complete search history.

FIG. 3 is a rear view of the design;

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,637,403	A *	1/1987	Garcia et al.	D24/147
D322,479	S *	12/1991	Miyaguchi	D24/147
D343,897	S *	2/1994	Rand et al.	D24/112
D346,219	S *	4/1994	Fardigh	D24/133
5,378,233	A *	1/1995	Haber et al.	D24/112
5,645,534	A *	7/1997	Chanoch	604/187
5,744,360	A *	4/1998	Hu et al.	604/22
5,993,421	A *	11/1999	Kriesel	604/132
6,221,044	B1 *	4/2001	Greco	604/232
6,277,099	B1 *	8/2001	Strowe et al.	604/207
D461,555	S *	8/2002	Binet et al.	D24/114

FIG. 4 is a right side view of the assembled design. The left side view is a mirror image of the right side, with the exception of the numbers "1" and "2", which are not symmetric.

FIG. 5 is a top view of the design, illustrating the activator button;

FIG. 6 is a bottom view of the design; and,

FIG. 7 is a front view of the design with a top removable cap covering an activator button removed and a bottom removable cap covering an injection opening removed.


The broken line showing of parts of the drawings is included for the purpose of illustrating use and environment and forms no part of the claimed design.

(Continued)

FOREIGN PATENT DOCUMENTS

WO WO-06/000785 A1 1/2006

1 Claim, 4 Drawing Sheets

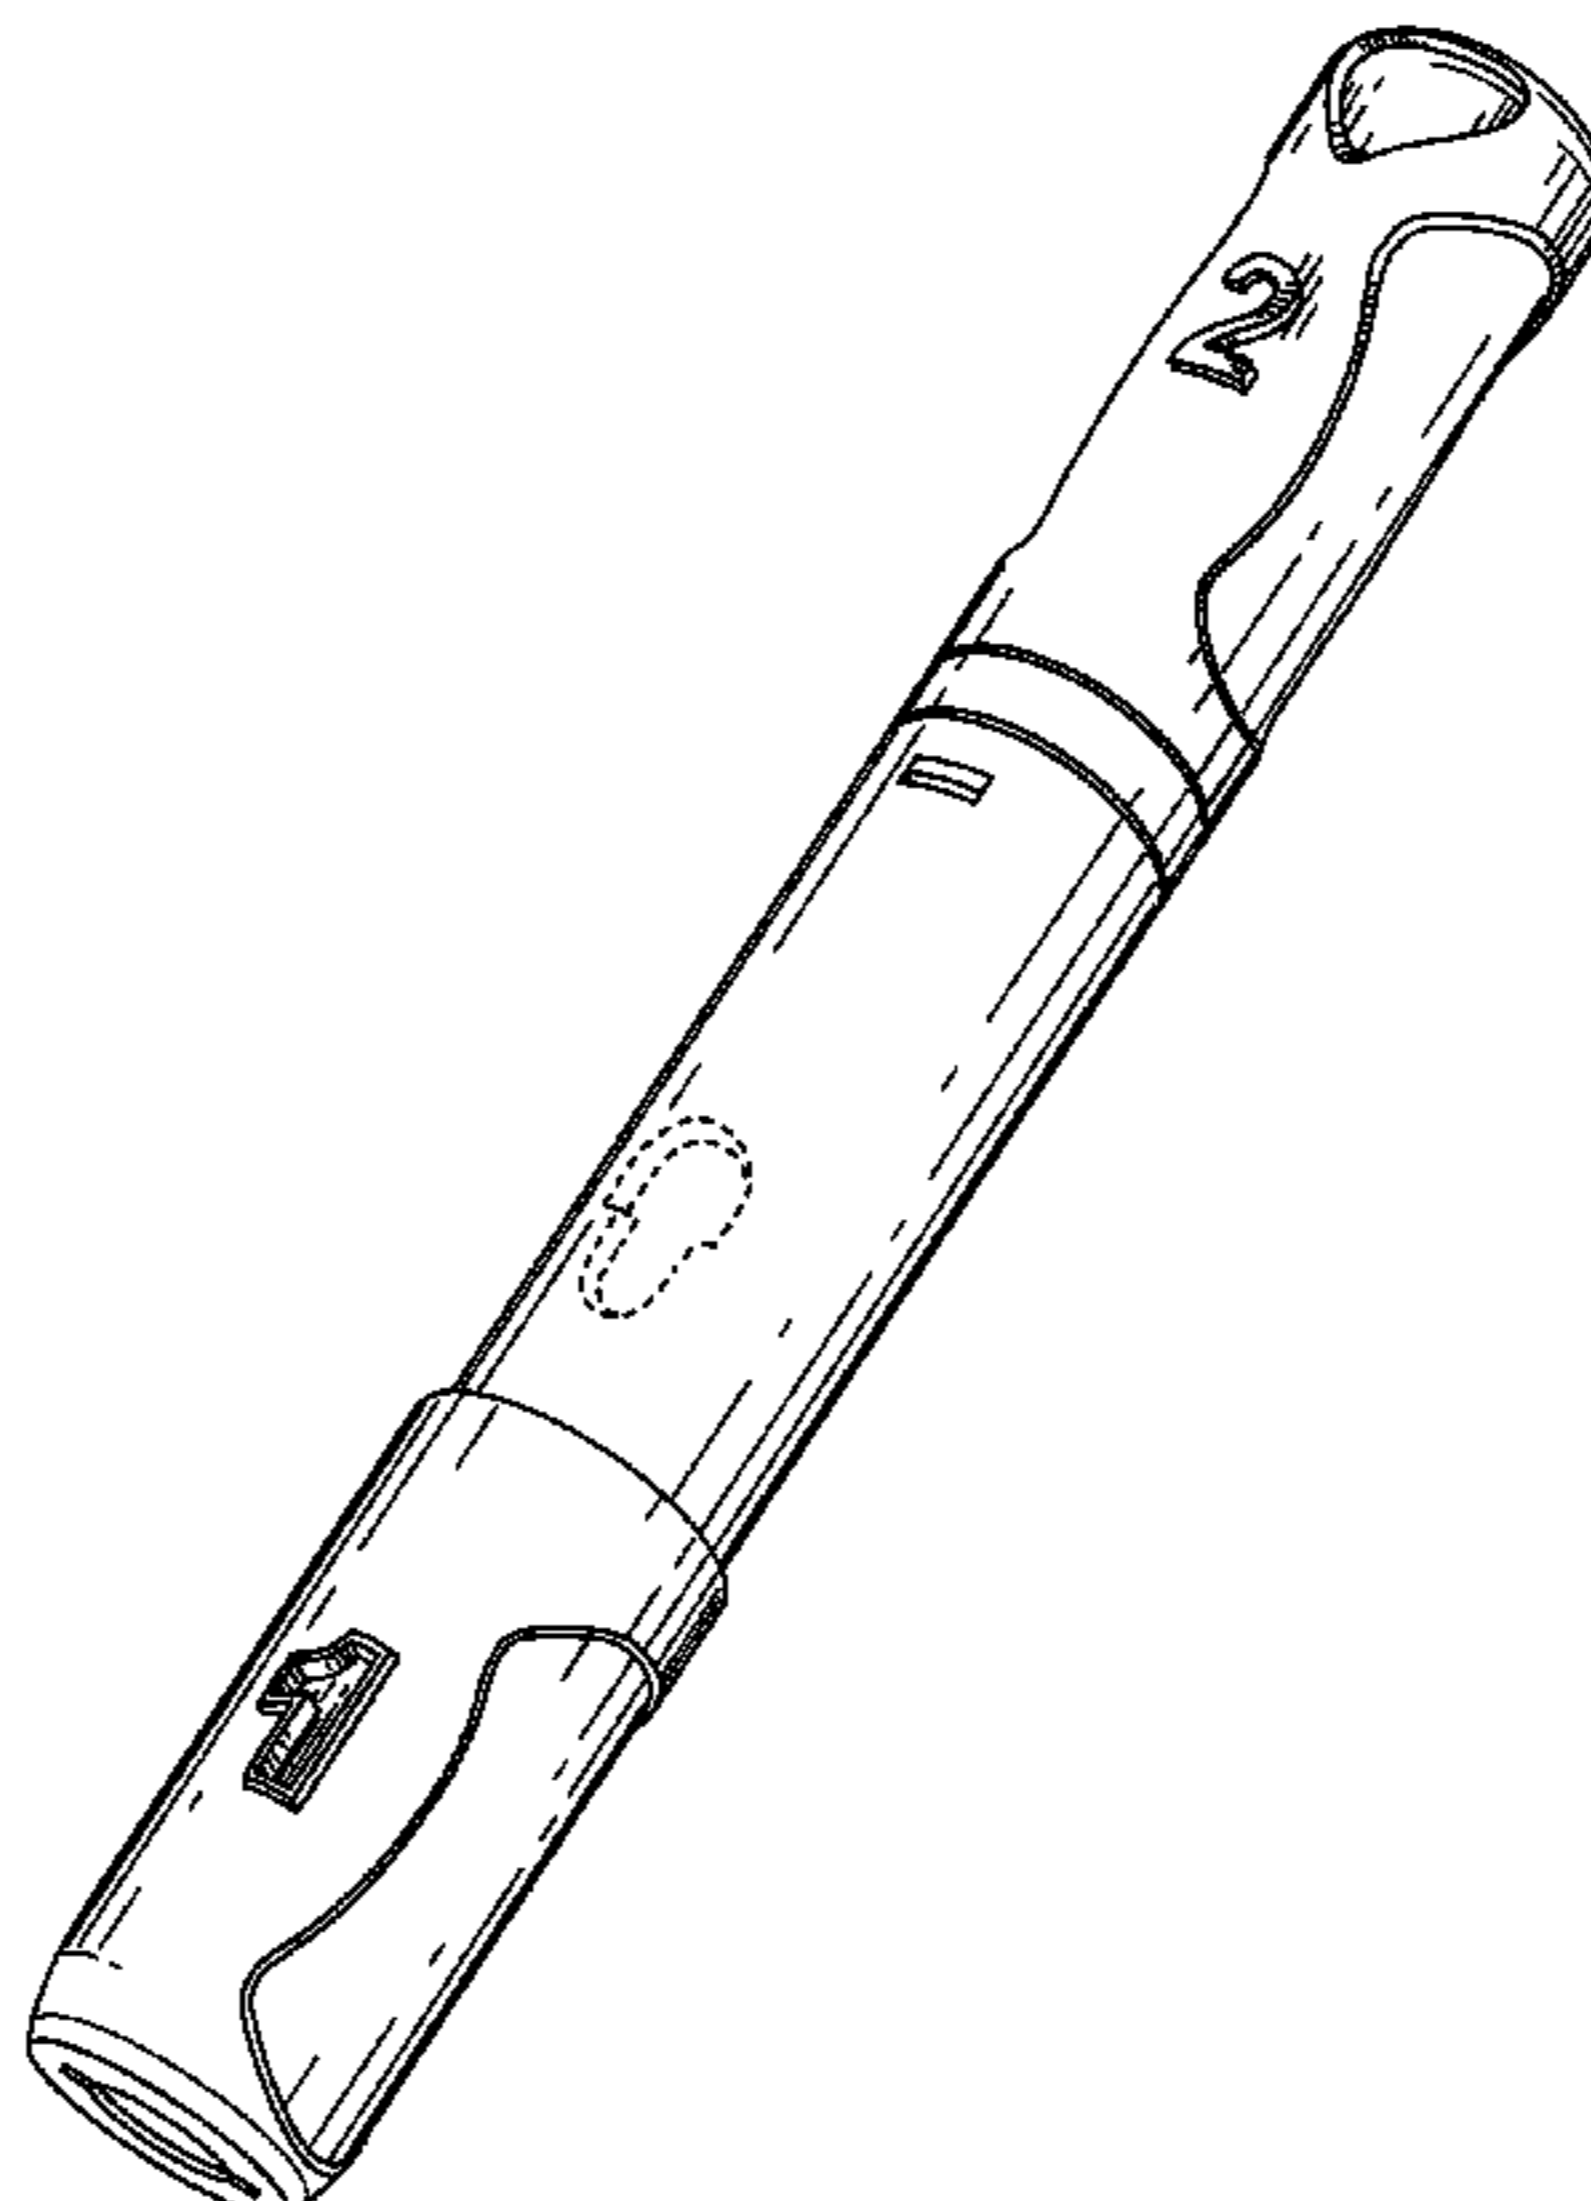

US D622,374 S

Page 2

U.S. PATENT DOCUMENTS

D494,270 S * 8/2004 Reschke D24/133
D518,175 S * 3/2006 Hardin et al. D24/133
2002/0002344 A1* 1/2002 Douglas et al. 606/181
2002/0169408 A1* 11/2002 Beretta et al. 604/19
2006/0047250 A1* 3/2006 Hickingbotham et al. ... 604/187
2006/0167413 A1 7/2006 Marshall et al.

2007/0161960 A1* 7/2007 Chen et al. 604/187

OTHER PUBLICATIONS

“Abbott Receives FDA Approval for New Humira® Delivery Device,” Press Release (Jun. 26, 2006) (Color).

* cited by examiner

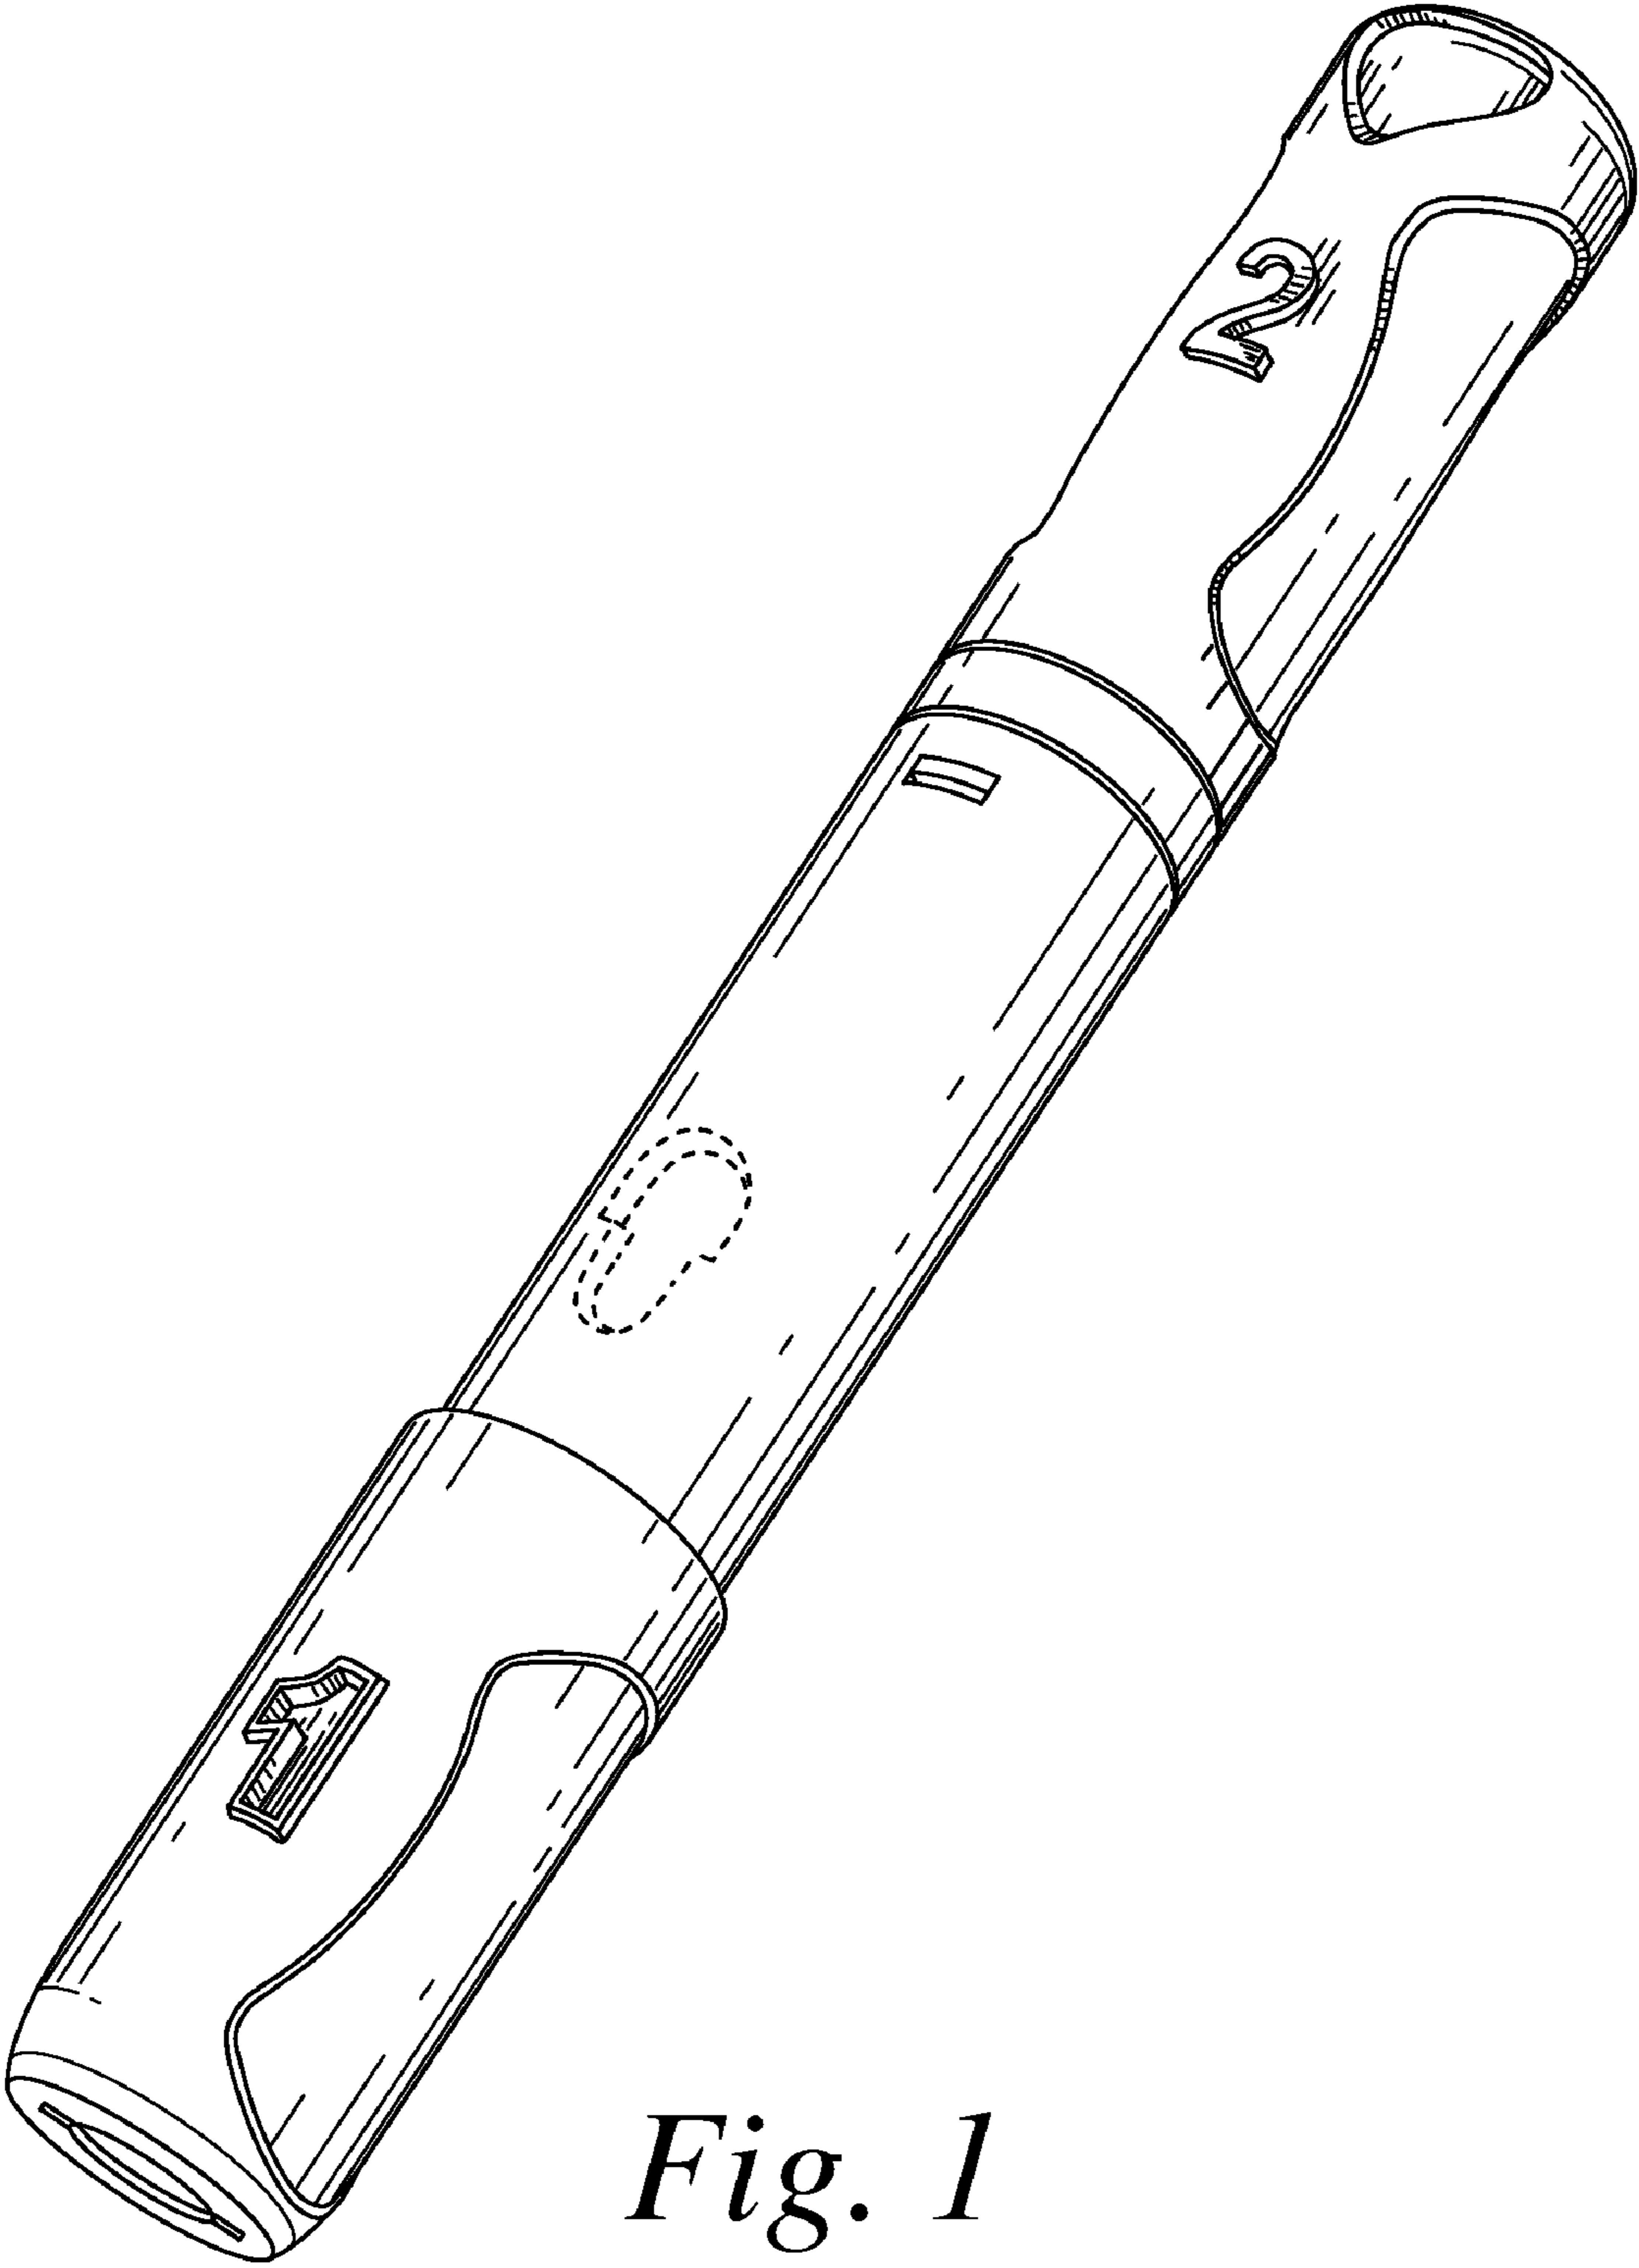


Fig. 1

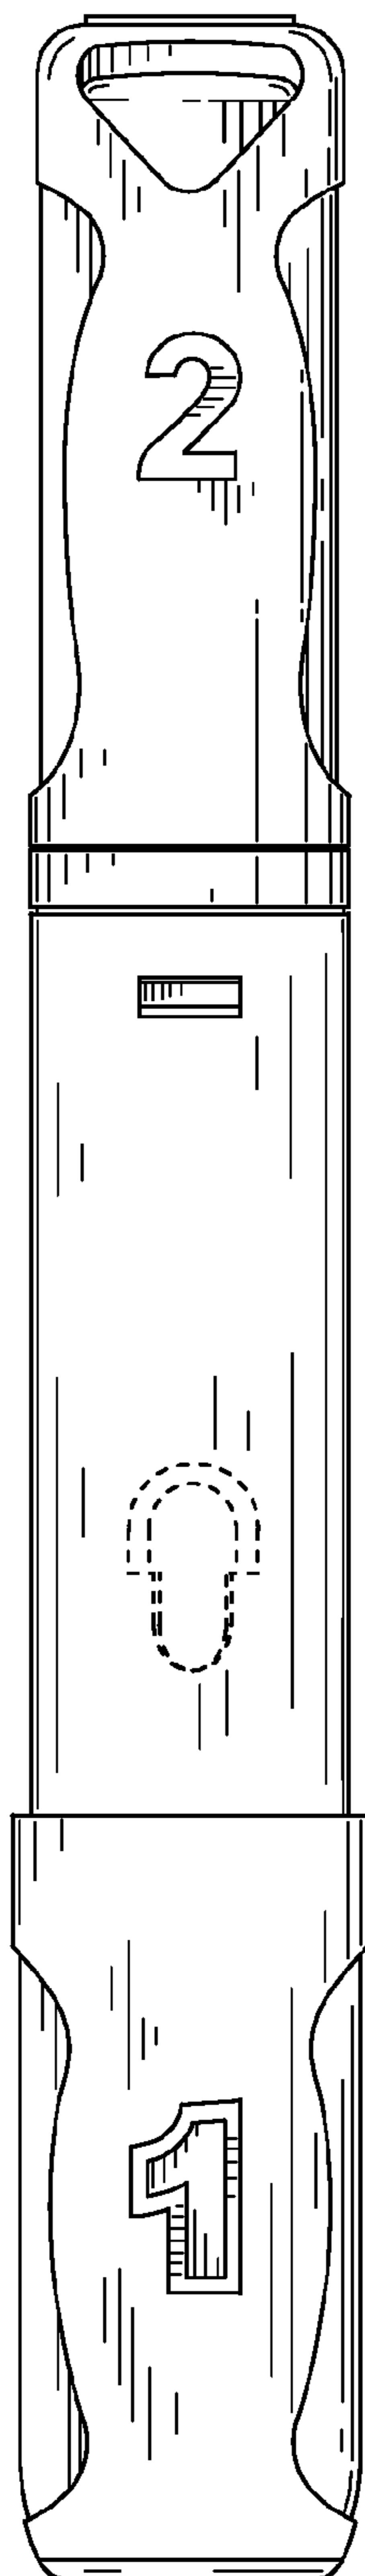


Fig. 2

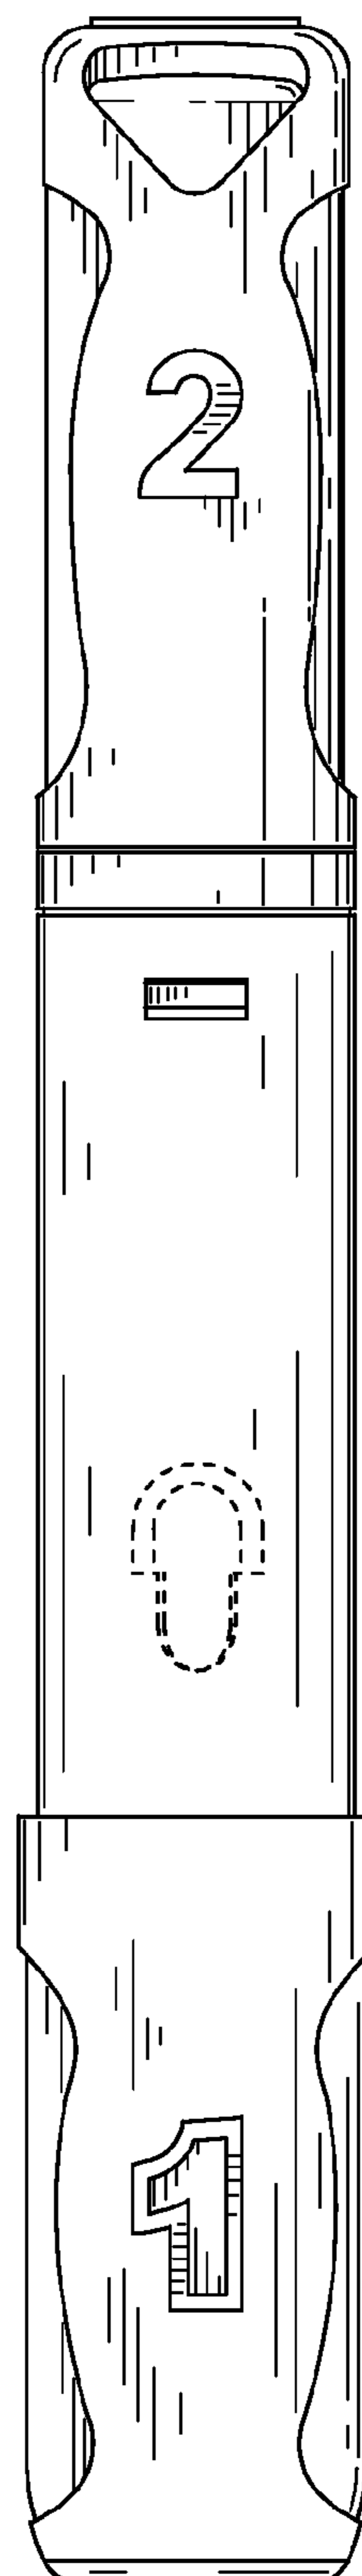


Fig. 3

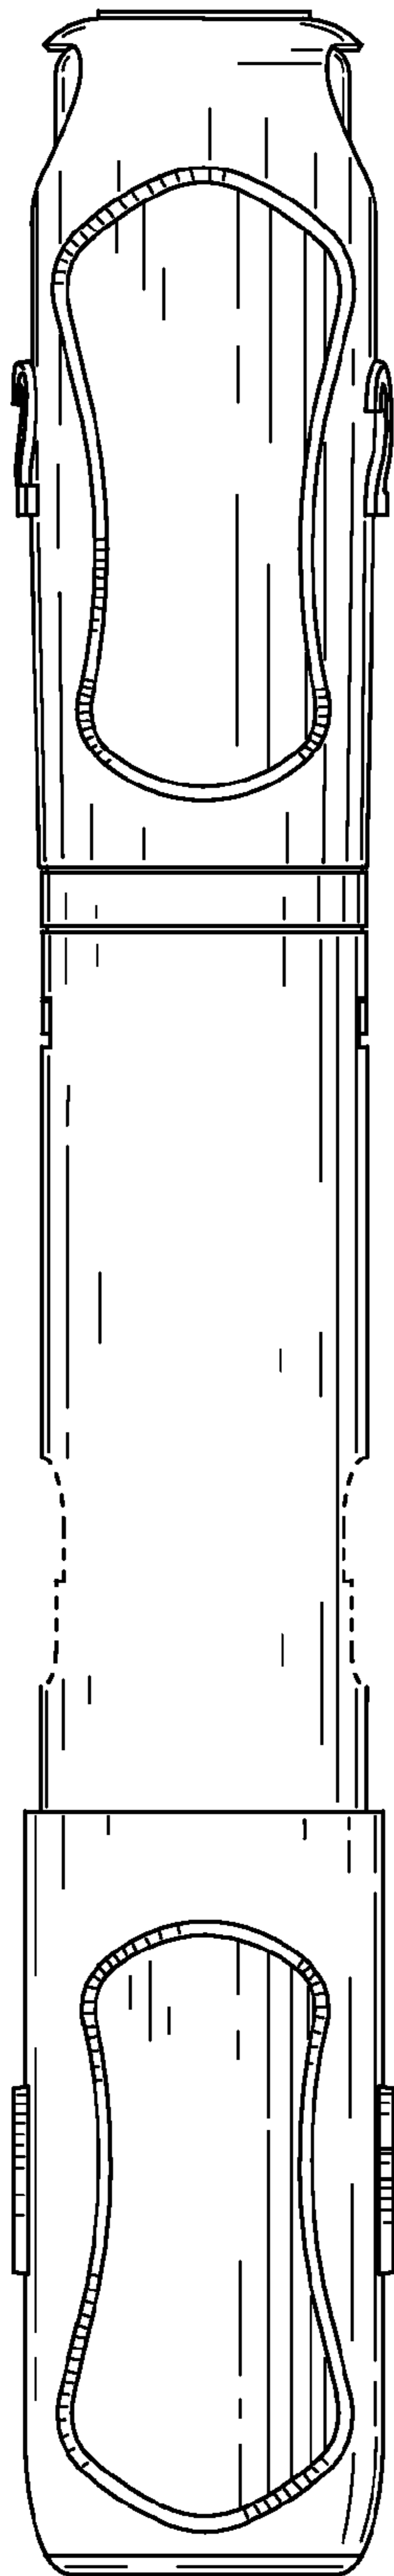


Fig. 4

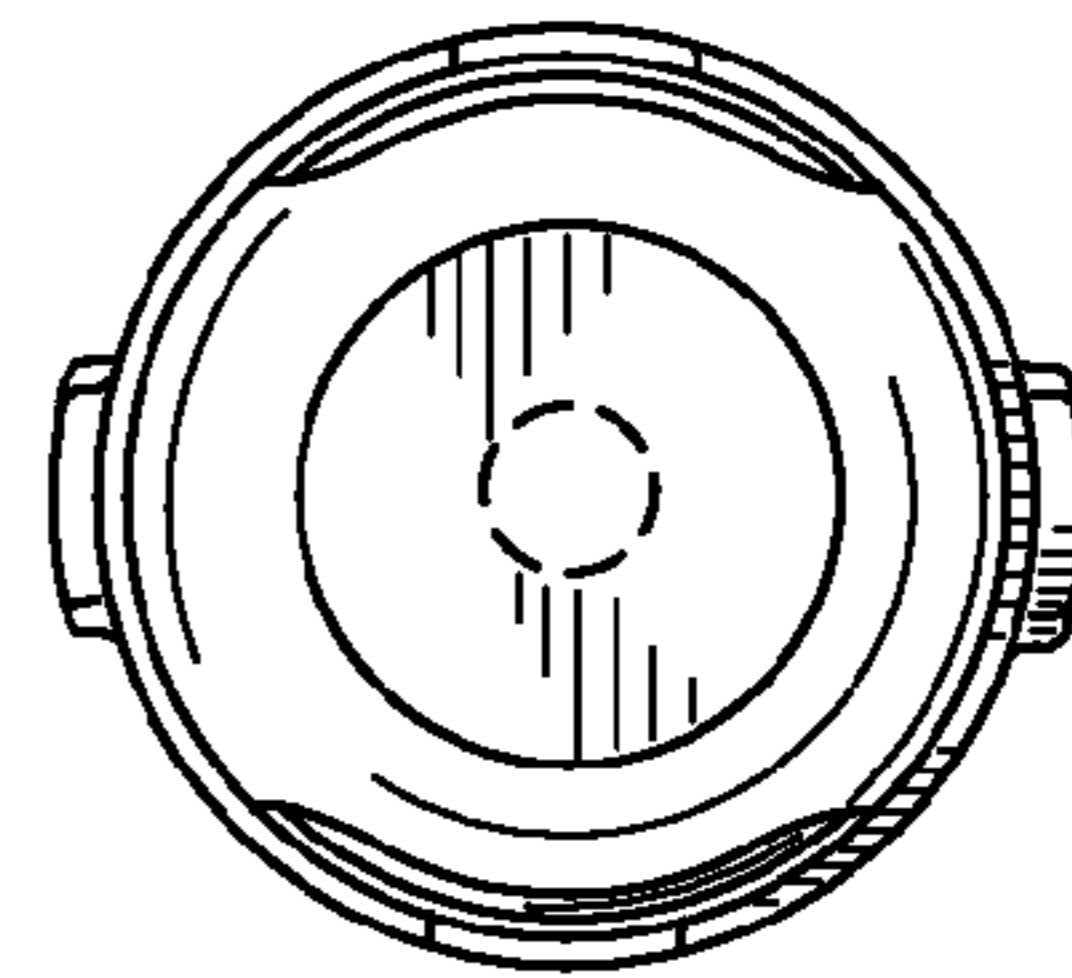


Fig. 5

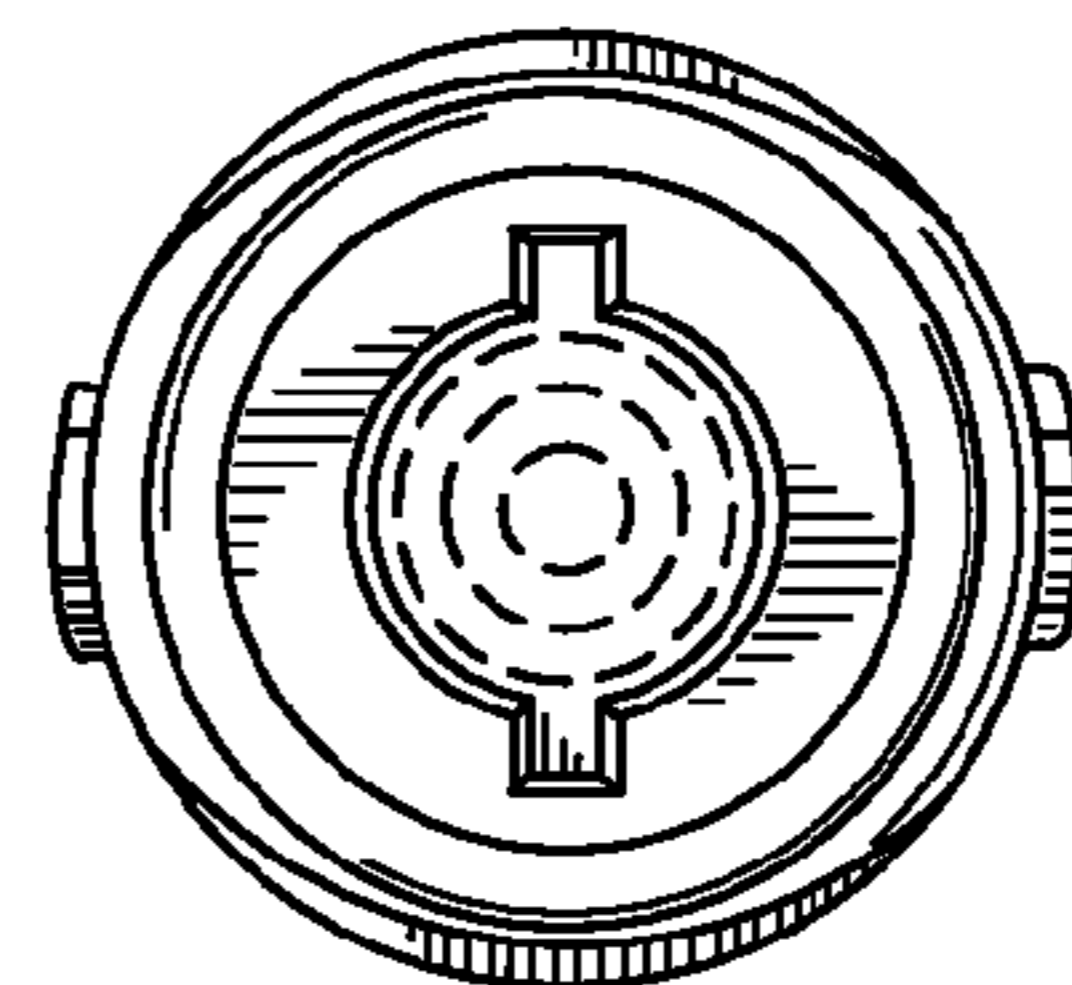


Fig. 6

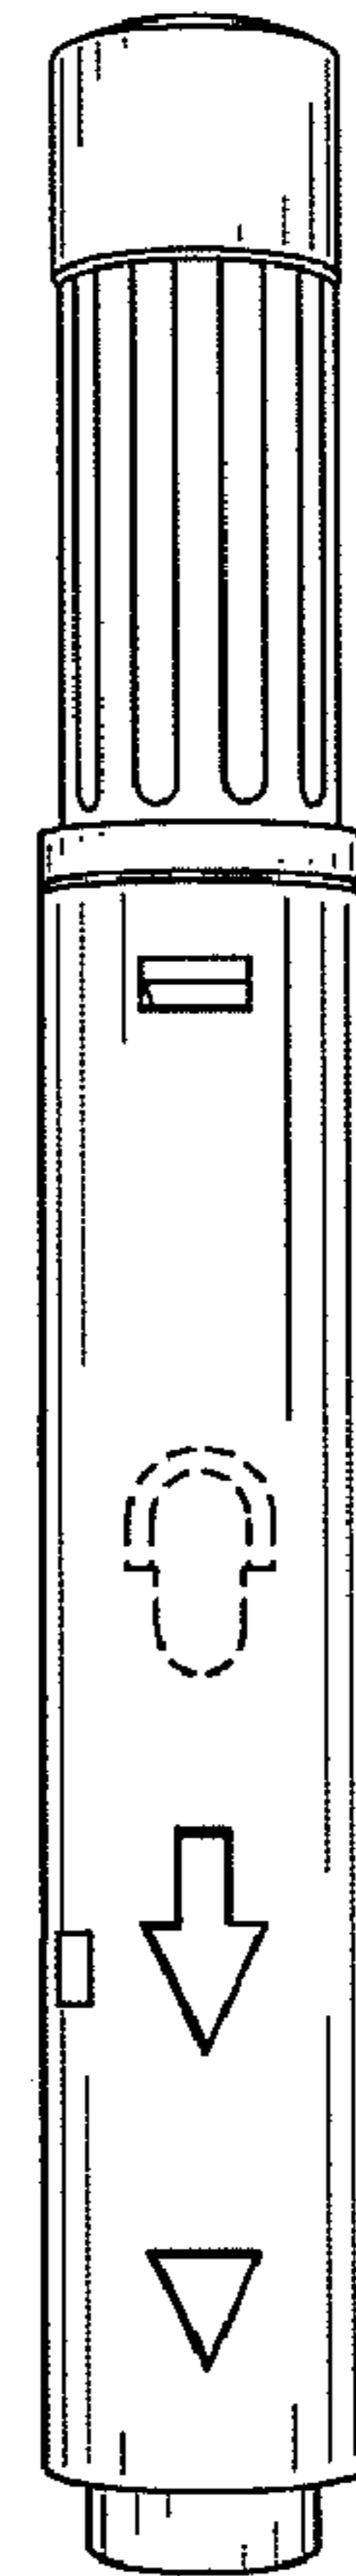
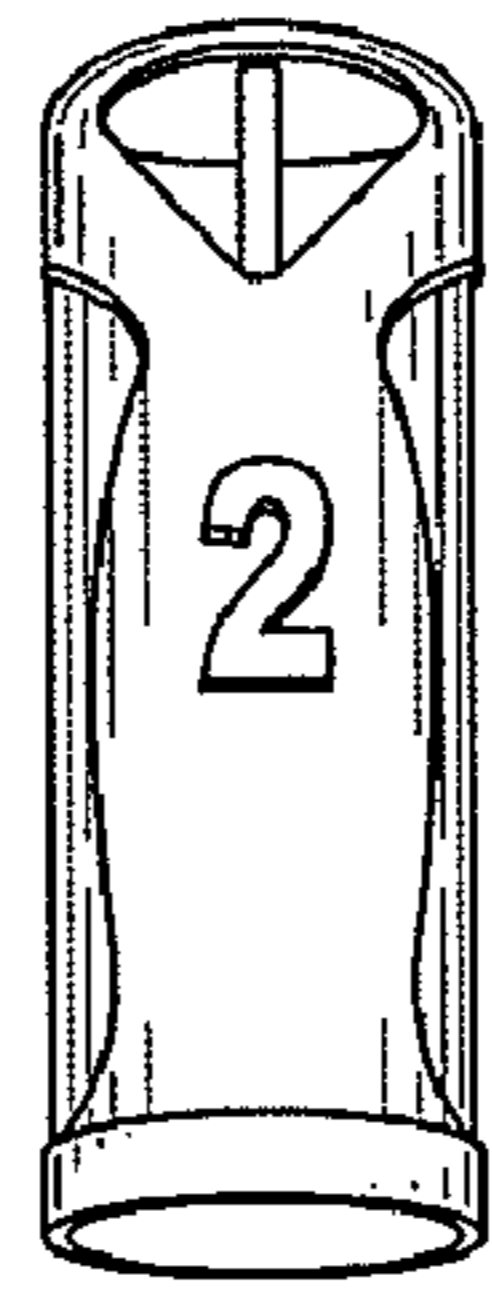


Fig. 7