



US00D626216S

(12) **United States Design Patent**
Tyce

(10) **Patent No.:** **US D626,216 S**

(45) **Date of Patent:** **** Oct. 26, 2010**

(54) **MEDICAL INJECTOR**

(75) Inventor: **Daniel Paul Charles Tyce,**
Warwickshire (GB)

(73) Assignee: **Sanofi-Aventis Deutschland GmbH,**
Frankfurt (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/274,154**

(22) Filed: **Mar. 30, 2007**

(30) **Foreign Application Priority Data**

Oct. 30, 2006 (EM) 000620851

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/114**

(58) **Field of Classification Search** D19/35,
D19/36, 41, 43, 44, 45, 46, 47, 48, 49, 50,
D19/51, 54, 55, 56, 57; D24/108, 112, 113,
D24/114, 130, 133, 138, 146, 147; 604/187,
604/188, 189, 197, 198, 207, 208, 227, 229,
604/232; 606/181, 182, 185

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,398,544 A * 4/1946 Lockhart 604/68
3,045,593 A * 7/1962 Petterson 101/368
3,254,836 A * 6/1966 Corpian 235/64
4,637,403 A * 1/1987 Garcia et al. 600/583

(Continued)

OTHER PUBLICATIONS

SoloStar disposable pen injector by DCA Design International for Sanofi Aventis GmbH, as shown on www.effective design.org.uk, dated Oct. 22, 2009 (3 pages).*

(Continued)

Primary Examiner—Elizabeth A Albert
Assistant Examiner—Karen E Eldridge Powers

(74) *Attorney, Agent, or Firm*—Finnegan, Henderson, Farabow, Garrett & Dunner, L.L.P.

(57) **CLAIM**

The ornamental design for the a medical injector, as shown and described.

DESCRIPTION

The file of this patent contains at least one photograph executed in color. Copies of this patent with color photographs will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front plan view of the first embodiment of a medical injector of my new design;

FIG. 2 is a left side view thereof,

FIG. 3 is a rear view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a bottom view thereof;

FIG. 6 is a top view thereof;

FIG. 7 is a front plan view of a second embodiment of a medical injector of my new design;

FIG. 8 is a left side view thereof,

FIG. 9 is a rear view thereof;

FIG. 10 is a right side view thereof;

FIG. 11 is a bottom view thereof; and,

FIG. 12 is a top view thereof.

The colors of the first embodiment of the design are as follows:


Body/Cap: Pantone: 16-3802 TPX (corresponds to light gray);

Dose dial grip: Pantone 18-4005 TPX (corresponds to dark gray);

Dose button/border of the label: Pantone 2645 (corresponds to violet blue); and

Surface of the label: no color (white).

1 Claim, 6 Drawing Sheets
(3 of 6 Drawing Sheet(s) Filed in Color)

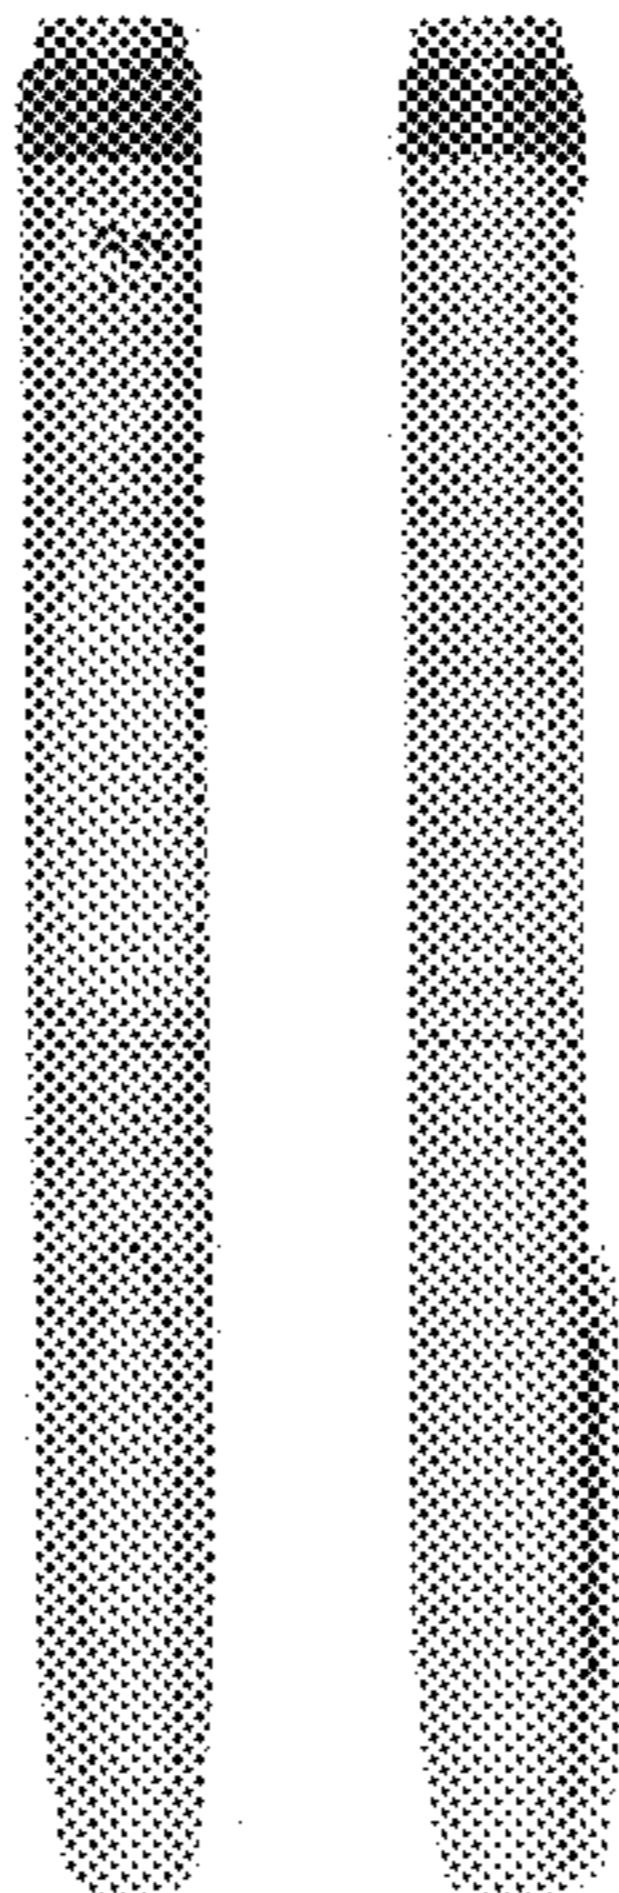

US D626,216 S

Page 2

U.S. PATENT DOCUMENTS

D289,424	S *	4/1987	Huang	D19/36
4,973,318	A *	11/1990	Holm et al.	604/208
D324,070	S *	2/1992	Suzuki	D19/51
5,334,144	A *	8/1994	Alchas et al.	604/68
5,569,214	A *	10/1996	Chanoch	604/246
D390,872	S *	2/1998	Sunaga	D19/36
D414,201	S *	9/1999	Larson et al.	D19/36
D426,299	S *	6/2000	Bydlon et al.	D24/112
D426,572	S *	6/2000	Salemme et al.	D19/47
6,110,149	A *	8/2000	Klitgaard et al.	604/209
D451,138	S *	11/2001	Rosenbaum	D19/36
D462,760	S *	9/2002	Ahlgrim et al.	D24/114
6,454,746	B1 *	9/2002	Bydlon et al.	604/227
D479,602	S *	9/2003	Bainton	D24/114
D479,747	S *	9/2003	Bainton	D24/114
D479,748	S *	9/2003	Tyce	D24/114
D483,067	S *	12/2003	Takanashi	D19/43
D492,027	S *	6/2004	Tyce et al.	D24/114
D492,405	S *	6/2004	Bainton	D24/114
D501,253	S *	1/2005	Bainton	D24/114
D502,739	S *	3/2005	Shova et al.	D19/66
D503,797	S *	4/2005	Tyce	D24/114
D505,490	S *	5/2005	Tyce	D24/114
6,932,794	B2 *	8/2005	Giambattista et al.	604/207
7,018,364	B2 *	3/2006	Giambattista et al.	604/207
D540,465	S *	4/2007	Bainton	D24/114
D567,939	S *	4/2008	Mattigka	D24/114
7,534,222	B2 *	5/2009	Sugita et al.	604/82
D599,009	S *	8/2009	Tyce	D24/113
D599,010	S *	8/2009	Tyce	D24/113
D600,794	S *	9/2009	Tyce	D24/113
D600,795	S *	9/2009	Tyce	D24/113
7,621,891	B2 *	11/2009	Wyrick	604/117
2004/0106895	A1 *	6/2004	Slate et al.	604/68
2004/0236284	A1 *	11/2004	Hoste et al.	604/198
2005/0187523	A1 *	8/2005	Giambattista et al.	604/207
2005/0234492	A1 *	10/2005	Tsai et al.	606/181
2005/0251103	A1 *	11/2005	Steffen et al.	604/500
2006/0155246	A1 *	7/2006	Higuchi et al.	604/165.01
2006/0229570	A1 *	10/2006	Lovell et al.	604/218
2007/0123829	A1 *	5/2007	Atterbury et al.	604/207
2007/0129687	A1 *	6/2007	Marshall et al.	604/207
2009/0076458	A1 *	3/2009	Nielsen et al.	604/189

OTHER PUBLICATIONS

DCA brochure for SoloStar disposable pen injector for insulin, as found on www.effectivedesign.org.uk, as indicated at arrow on Item "U" above, dated Jun. 2, 2009 (10 pages). Reference to date of product launch (2007) on p. 2, last paragraph.*

Article on www.diabeteshealth.com about FDA approval of Lantus SoloStar disposable insulin pen, with a picture of the product, dated May 4, 2007 (5 pages).*

* cited by examiner

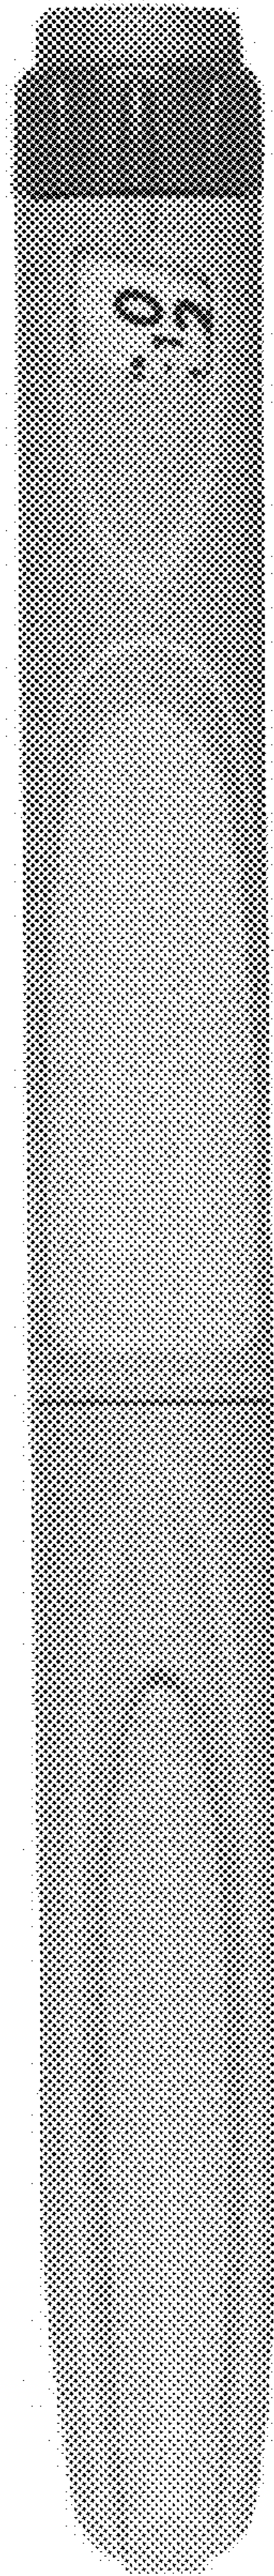


FIG. 1

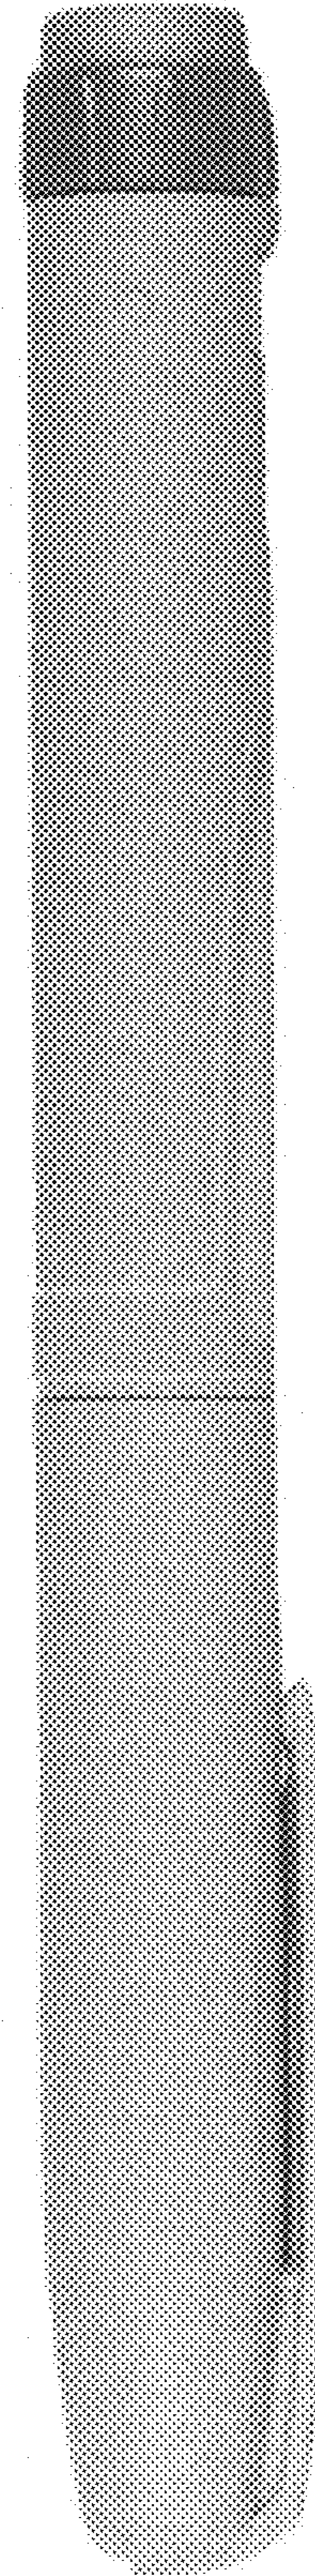


FIG. 2

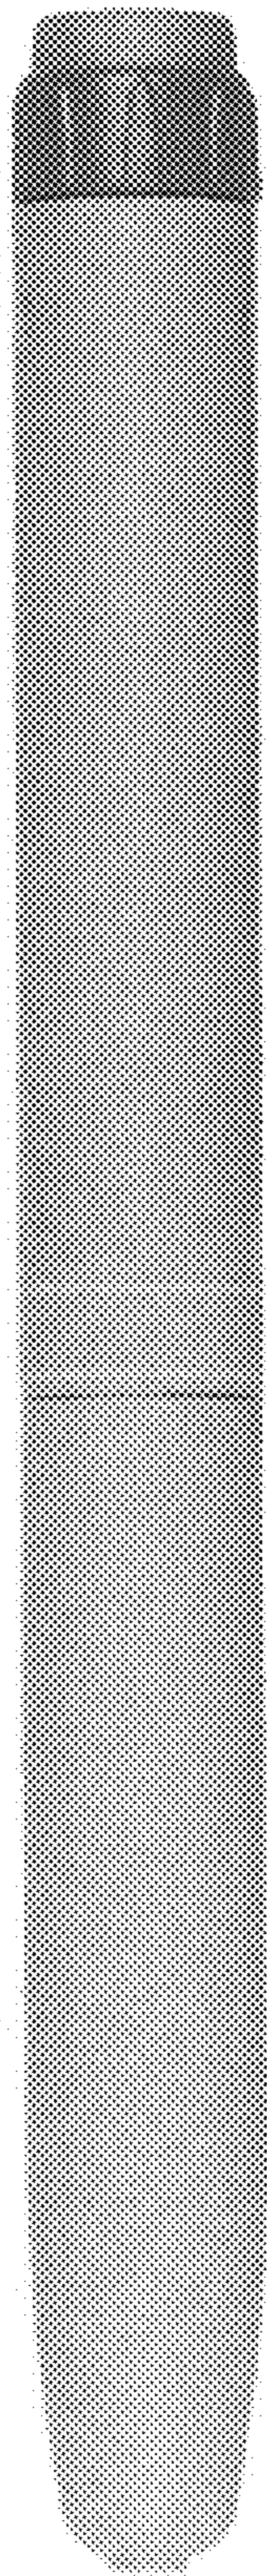


FIG. 3

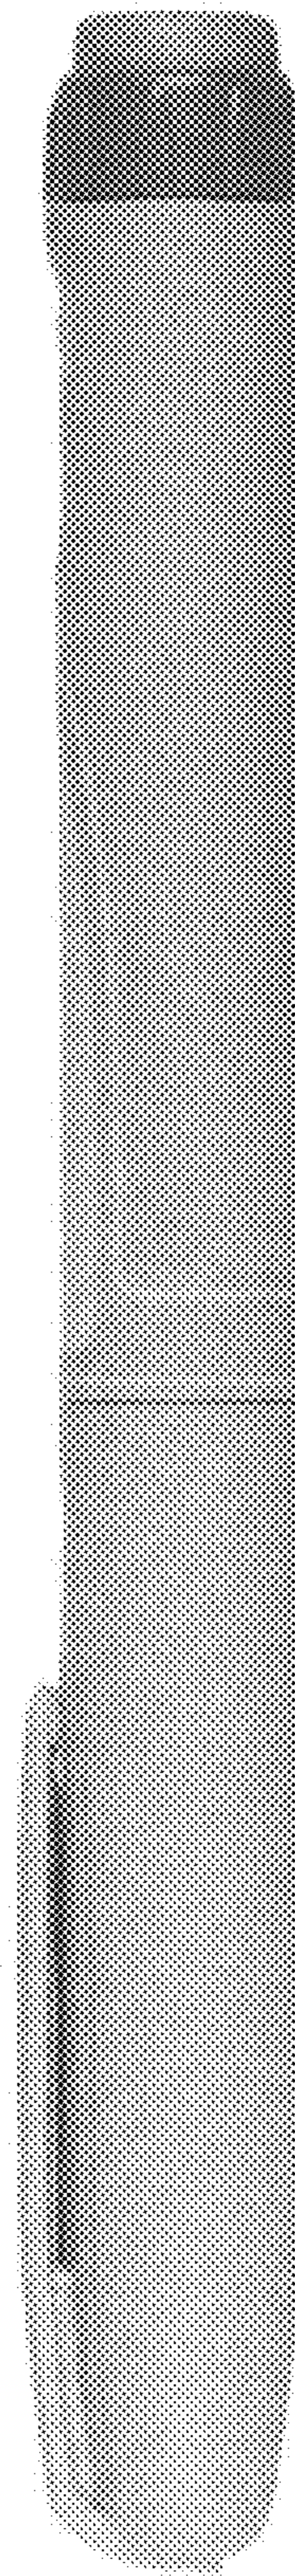


FIG. 4

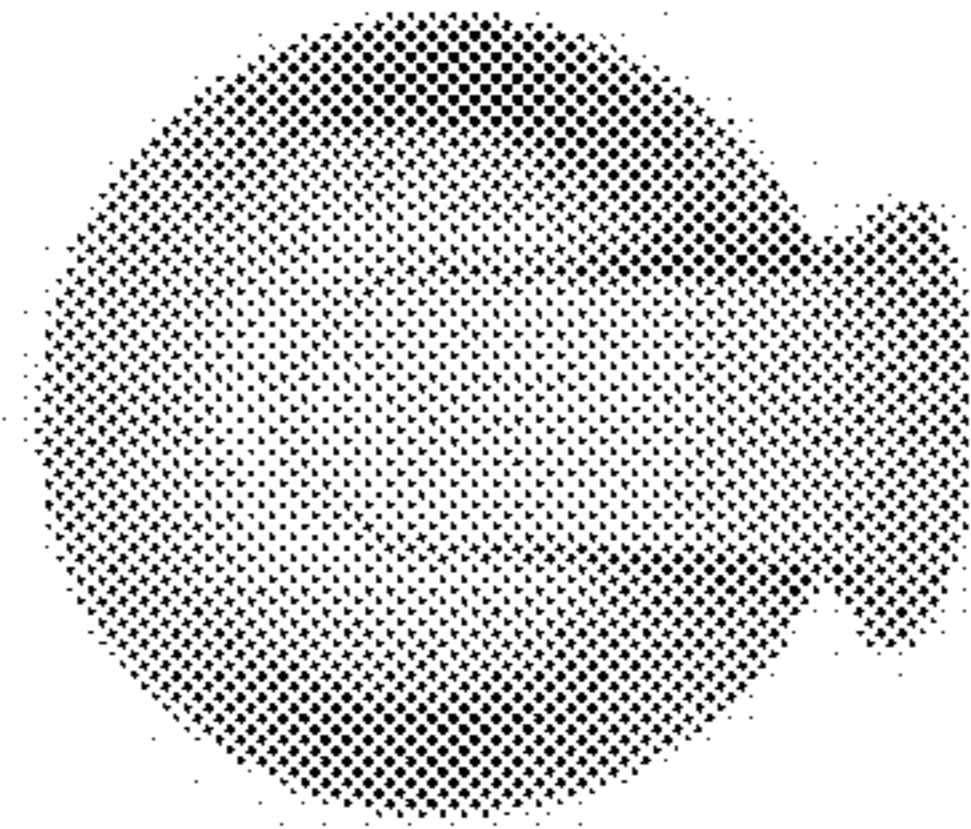


FIG. 5

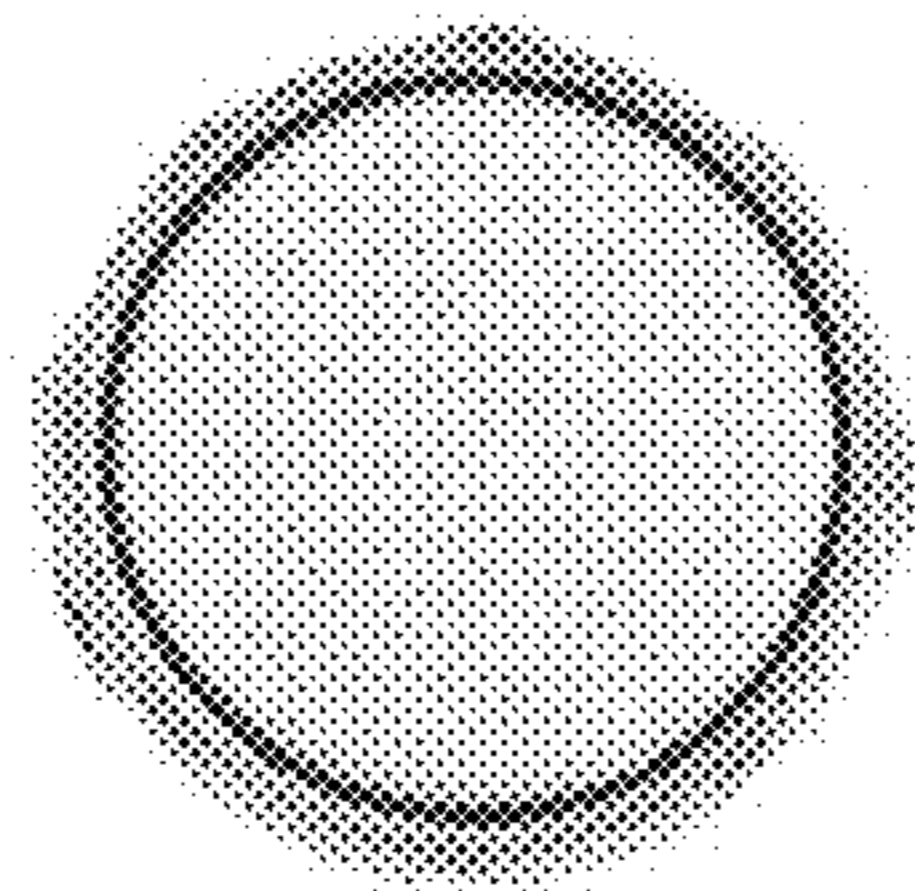


FIG. 6

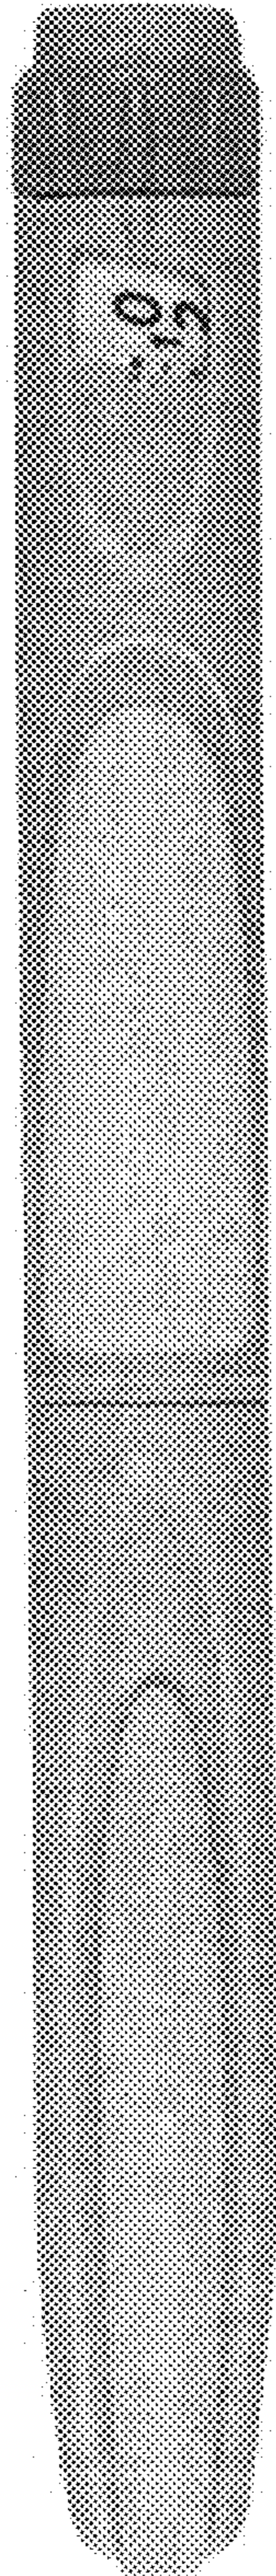


FIG. 7

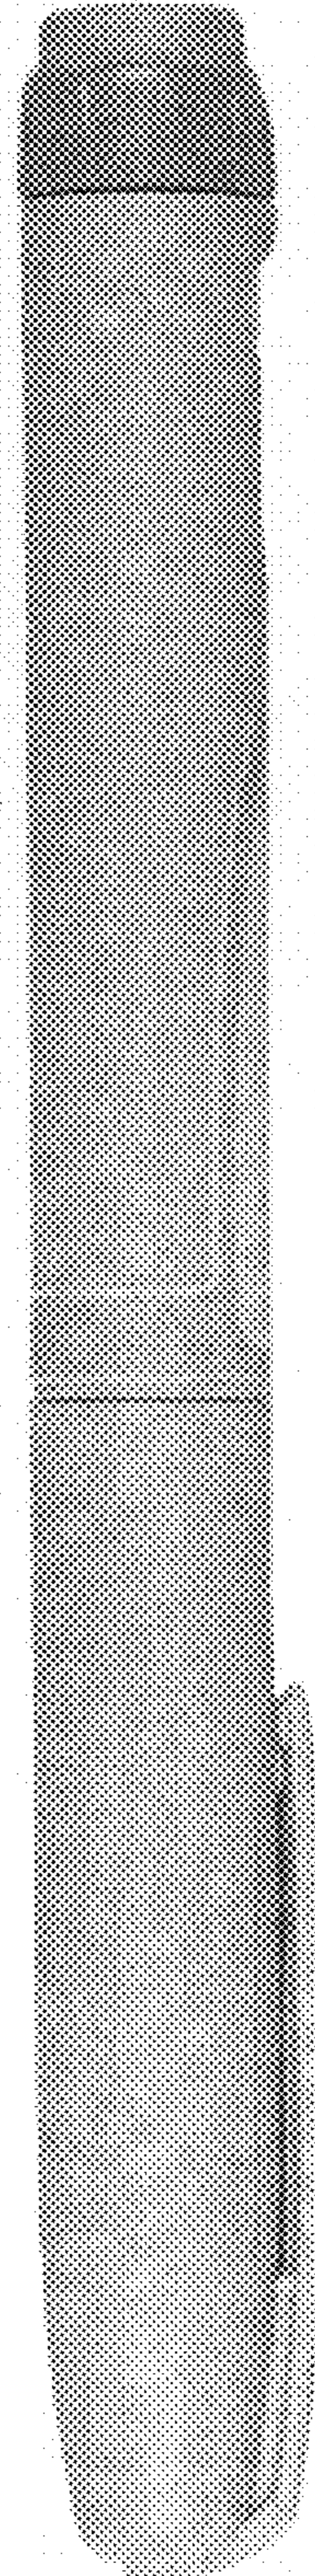


FIG. 8

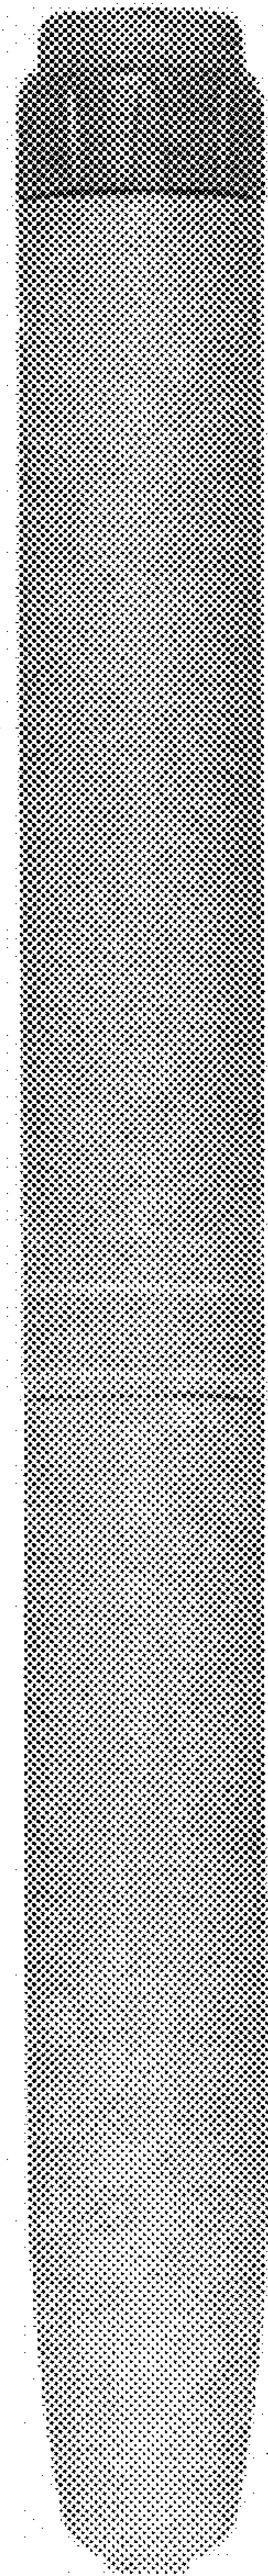


FIG. 9

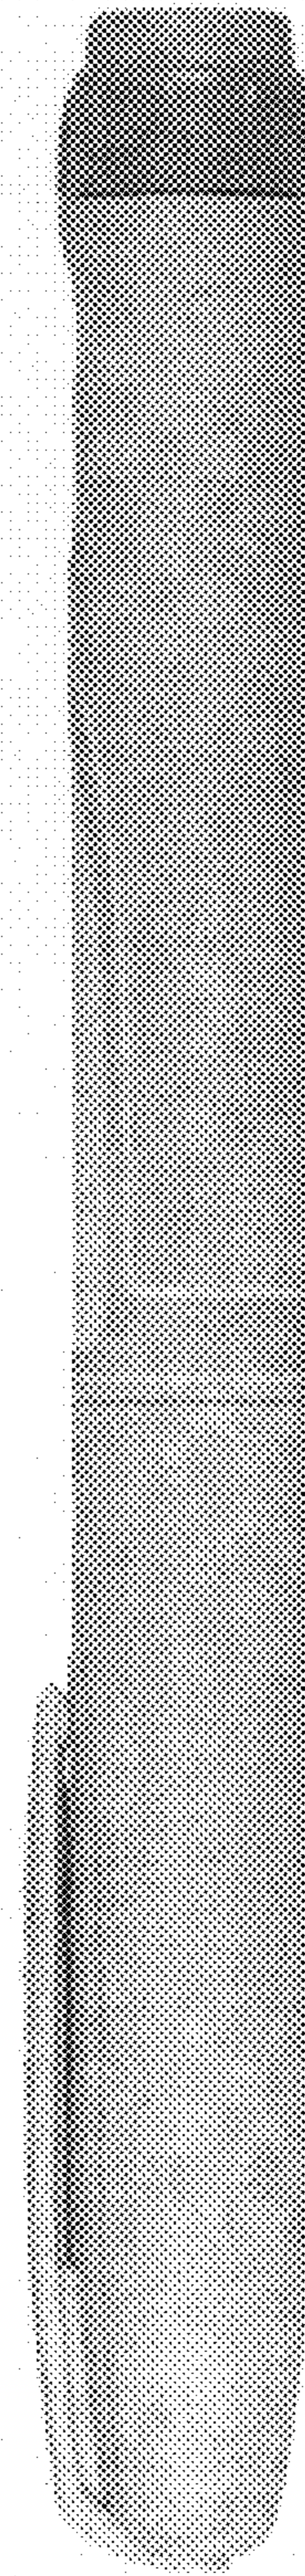


FIG. 10

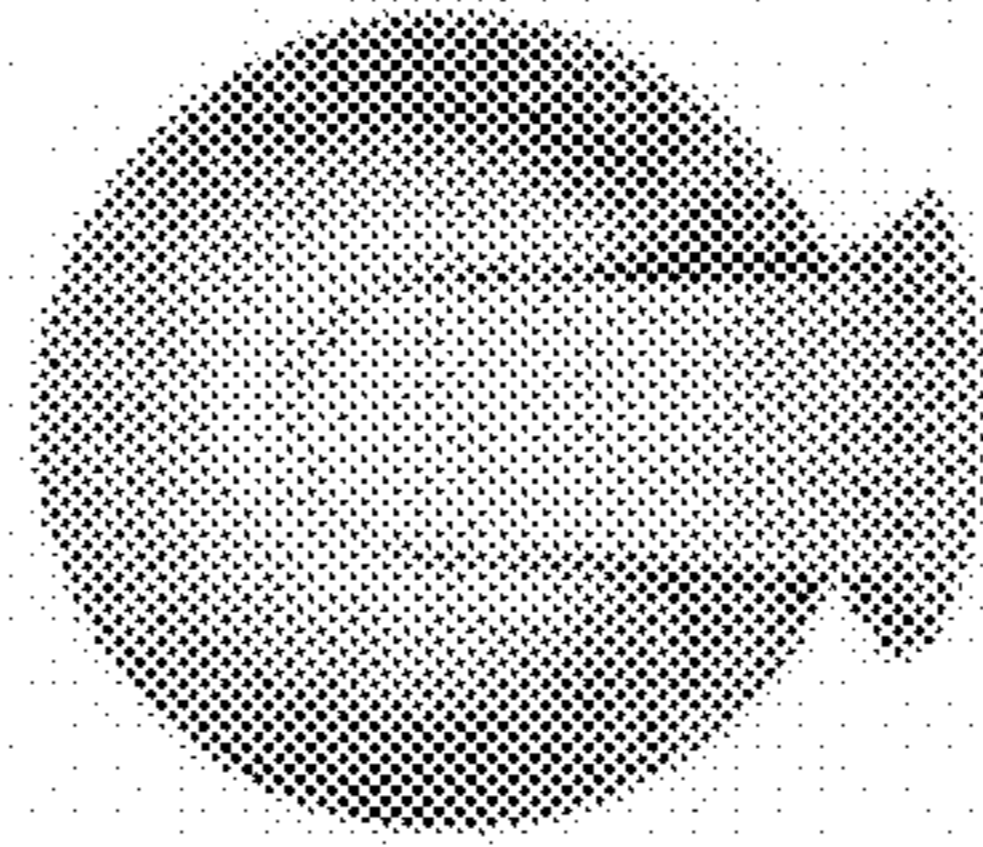


FIG. 11

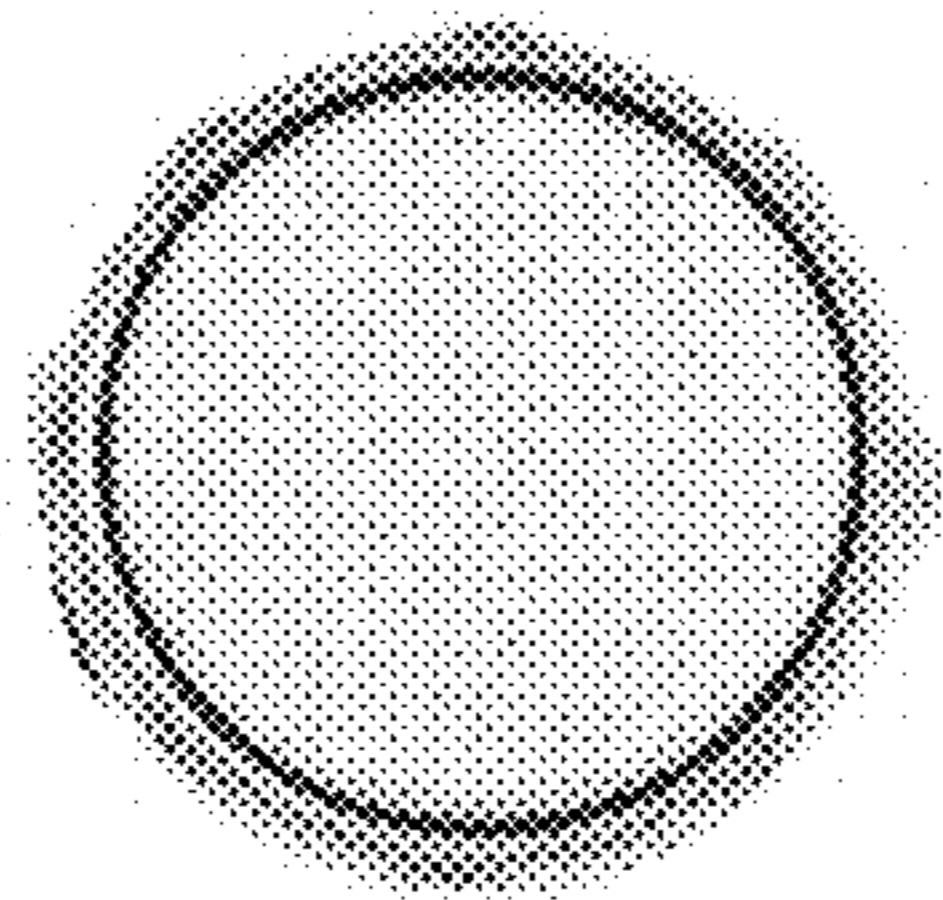


FIG. 12