

US00D626236S

(12) **United States Design Patent**
Ninomiya et al.

(10) **Patent No.:** **US D626,236 S**
(45) **Date of Patent:** **** Oct. 26, 2010**

(54) **ULTRASOUND DIAGNOSIS APPARATUS**

(75) Inventors: **Atsushi Ninomiya**, Tokyo (JP); **Yoshimi Kasai**, Tokyo (JP); **Kasanami Tsuneo**, Tokyo (JP); **Masaru Inoue**, Tokyo (JP)

(73) Assignee: **Hitachi Medical Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/309,857**

(22) Filed: **Oct. 28, 2008**

(30) **Foreign Application Priority Data**

Apr. 28, 2008 (JP) 2008-010824

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/185**

(58) **Field of Classification Search** D24/158,
D24/160, 183-186, 231; D13/163; 128/916,
128/922; 248/918; 312/209, 223.1; 600/442,
600/443, 437

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D300,241 S * 3/1989 LaCelle et al. D24/160
D318,919 S * 8/1991 Takaki et al. D24/160
D360,690 S * 7/1995 Murakami D24/160
D365,148 S * 12/1995 Murakami et al. D24/160

6,648,825 B1 * 11/2003 Mesaros et al. 600/437
6,709,391 B2 * 3/2004 Mesaros et al. 600/437
D512,508 S * 12/2005 Mesaros D24/185
7,044,568 B2 * 5/2006 Olivera et al. 312/209
D529,611 S * 10/2006 Gumisawa et al. D24/158
D560,807 S * 1/2008 Kitayama et al. D24/158
D571,011 S * 6/2008 Otoha et al. D24/158
2004/0036386 A1 * 2/2004 Olivera 312/209
2004/0046487 A1 * 3/2004 Olivera et al. 312/209

* cited by examiner

Primary Examiner—Mary Ann Calabrese

(74) *Attorney, Agent, or Firm*—Antonelli, Terry, Stout & Kraus, LLP.

(57) **CLAIM**

We claim the ornamental design for an ultrasound diagnosis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a front, top and right side perspective view of a ultrasound diagnosis apparatus showing our new design;

FIG. 3 is a rear side elevation view thereof;

FIG. 4 is a top side elevational view thereof;


FIG. 5 is a bottom plan view thereof;

FIG. 6 is a right plan view thereof; and,

FIG. 7 is a left side elevational view thereof.

The broken lines indicate portions of the ultrasound diagnosis apparatus which form no part of the claimed design.

1 Claim, 5 Drawing Sheets

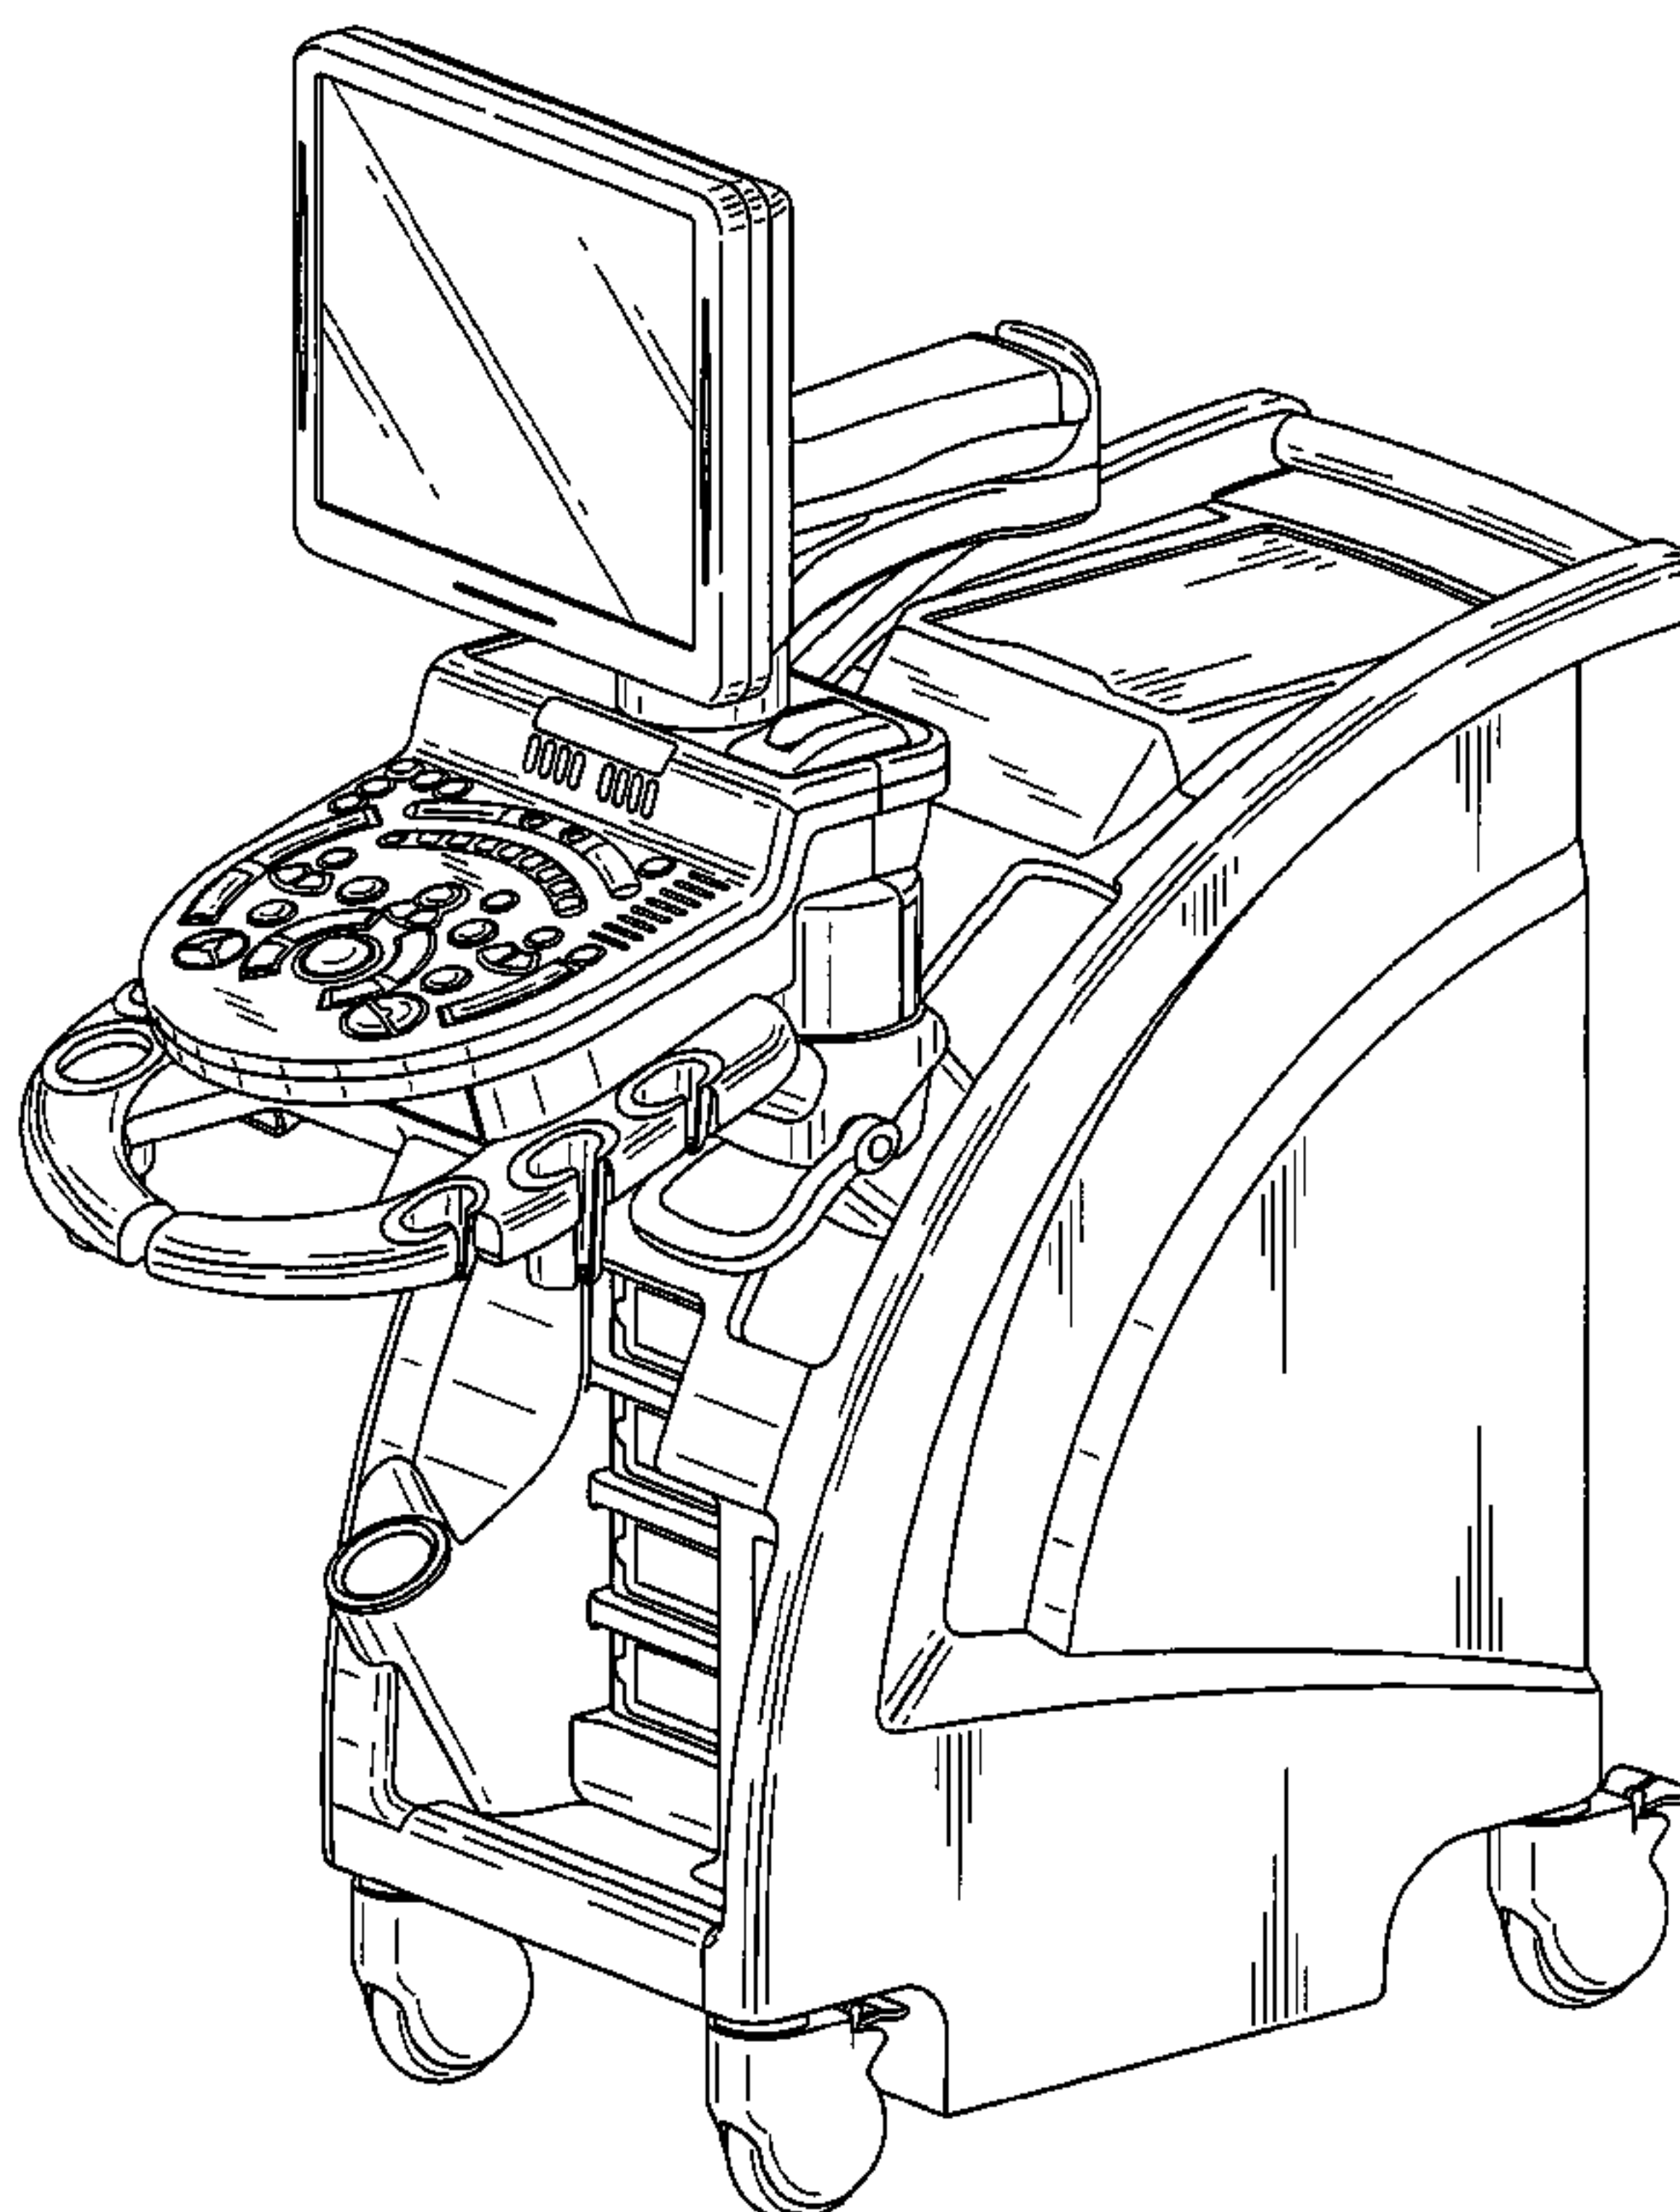

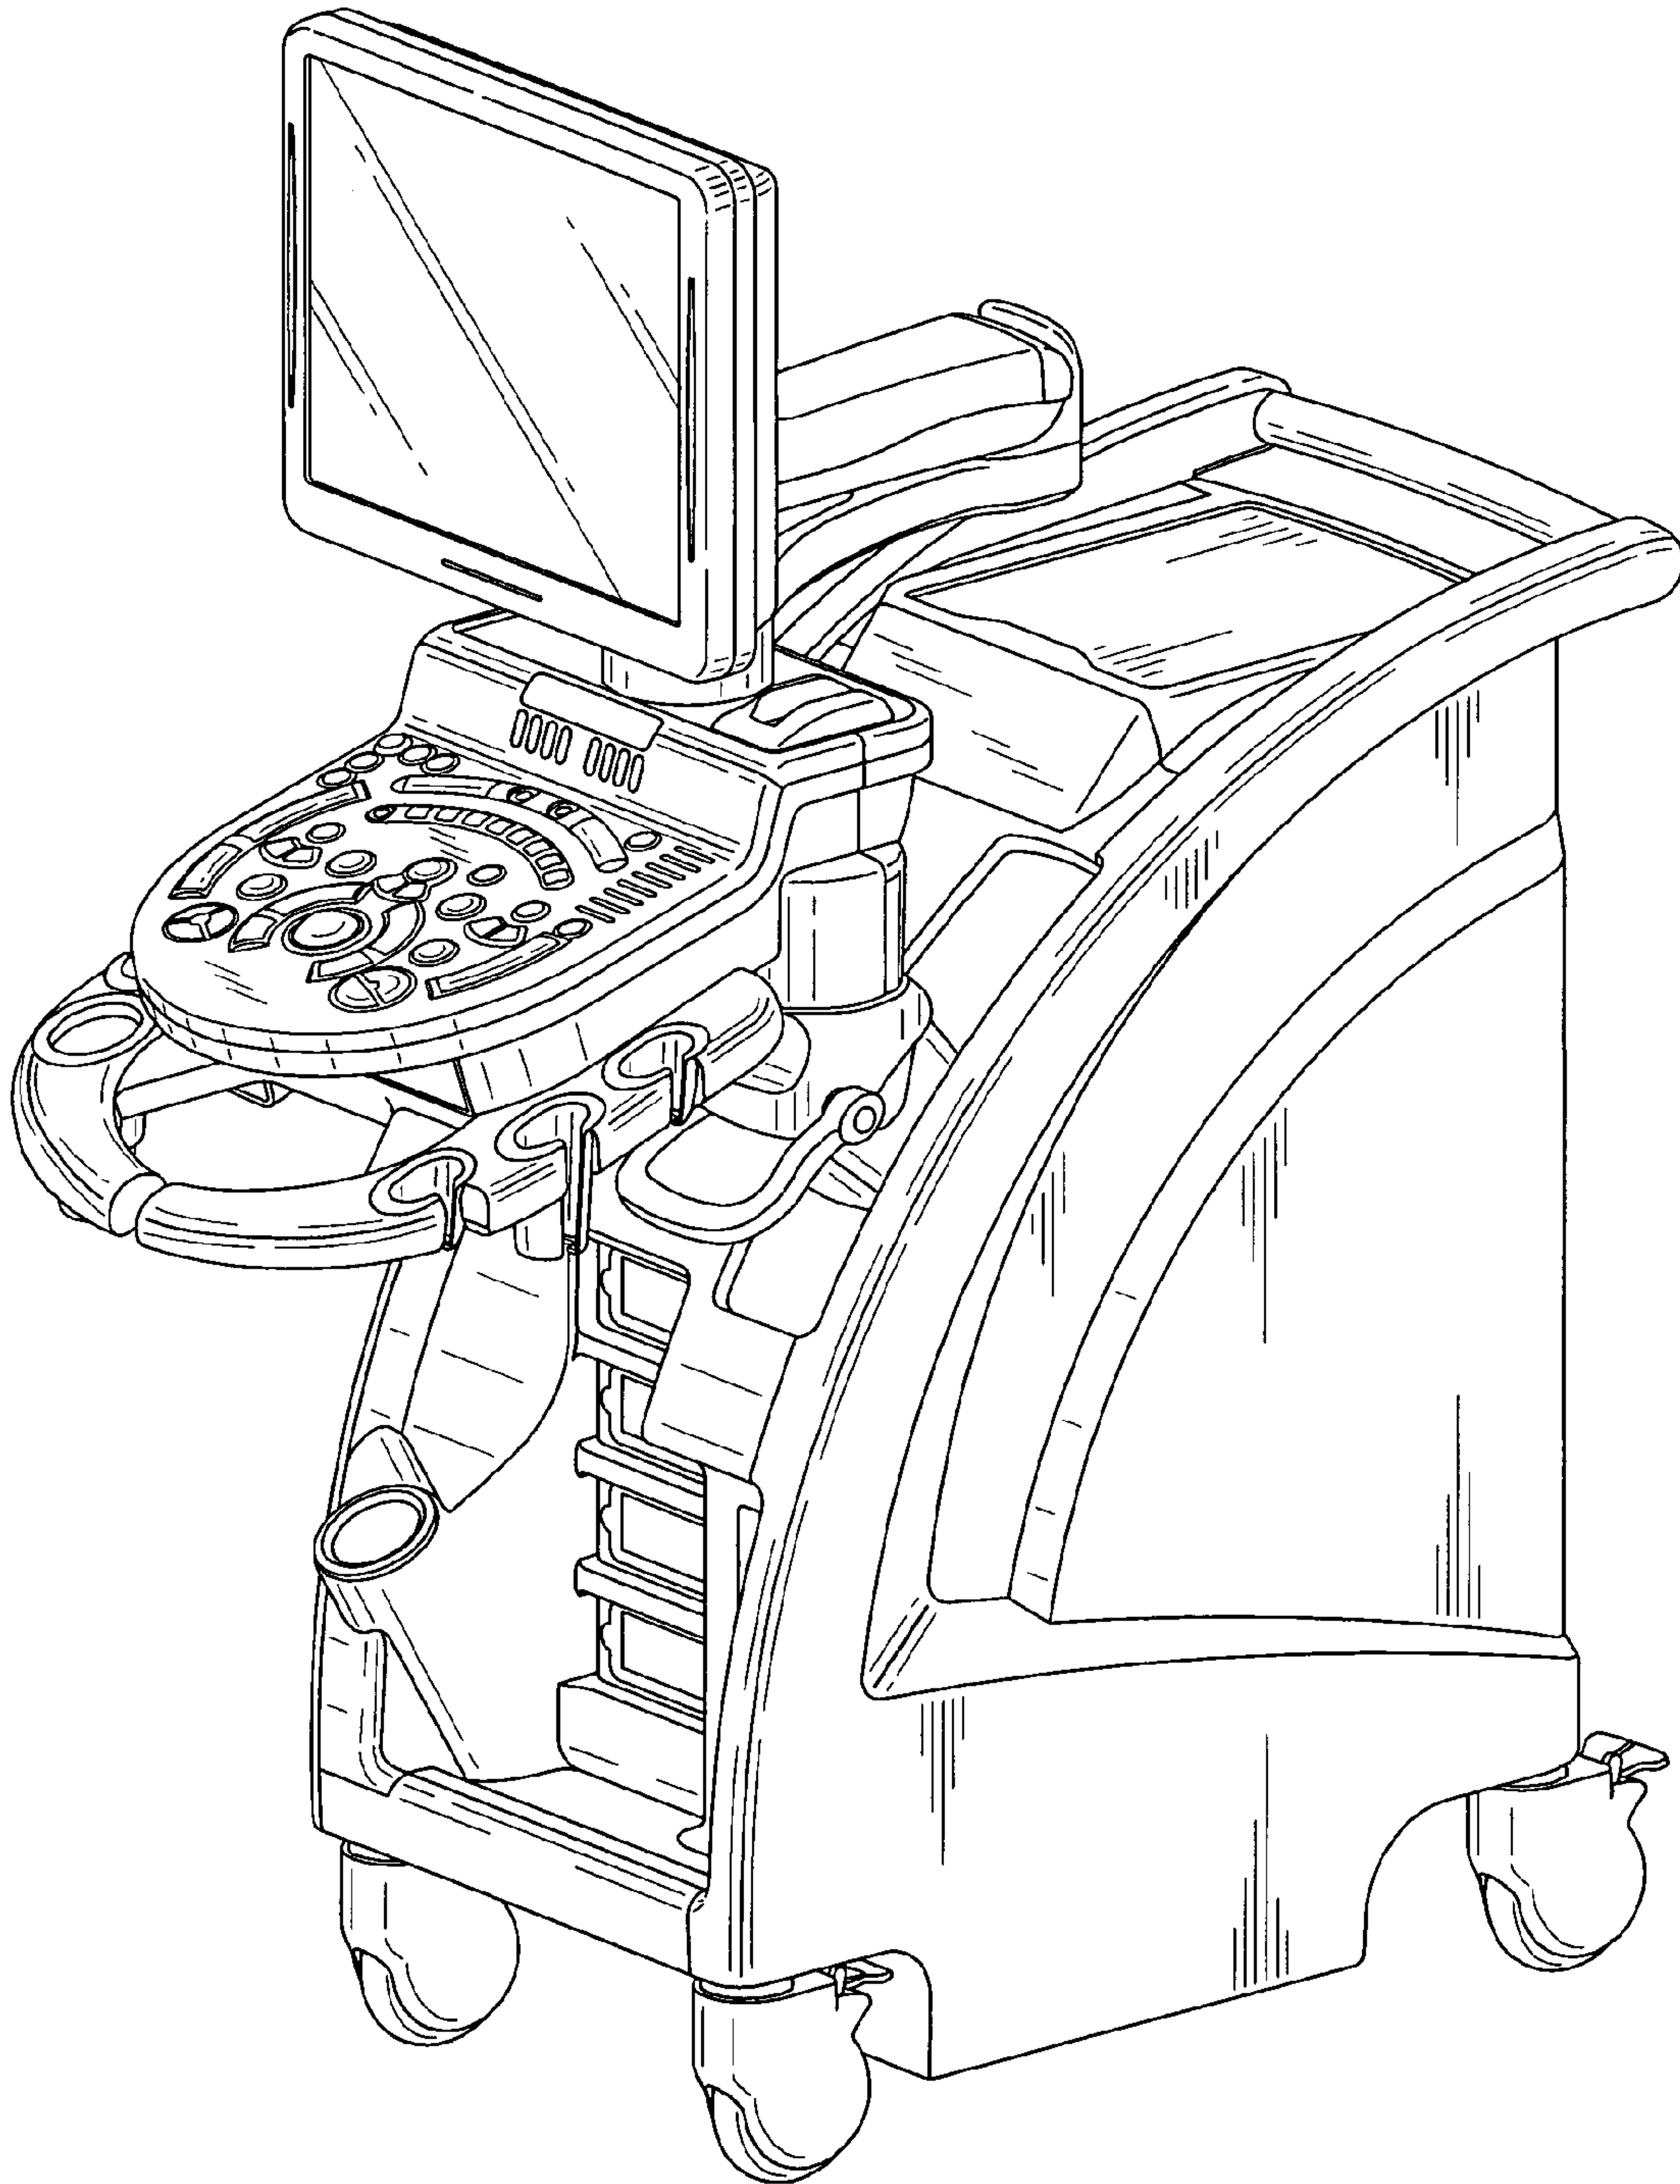


FIG. 1

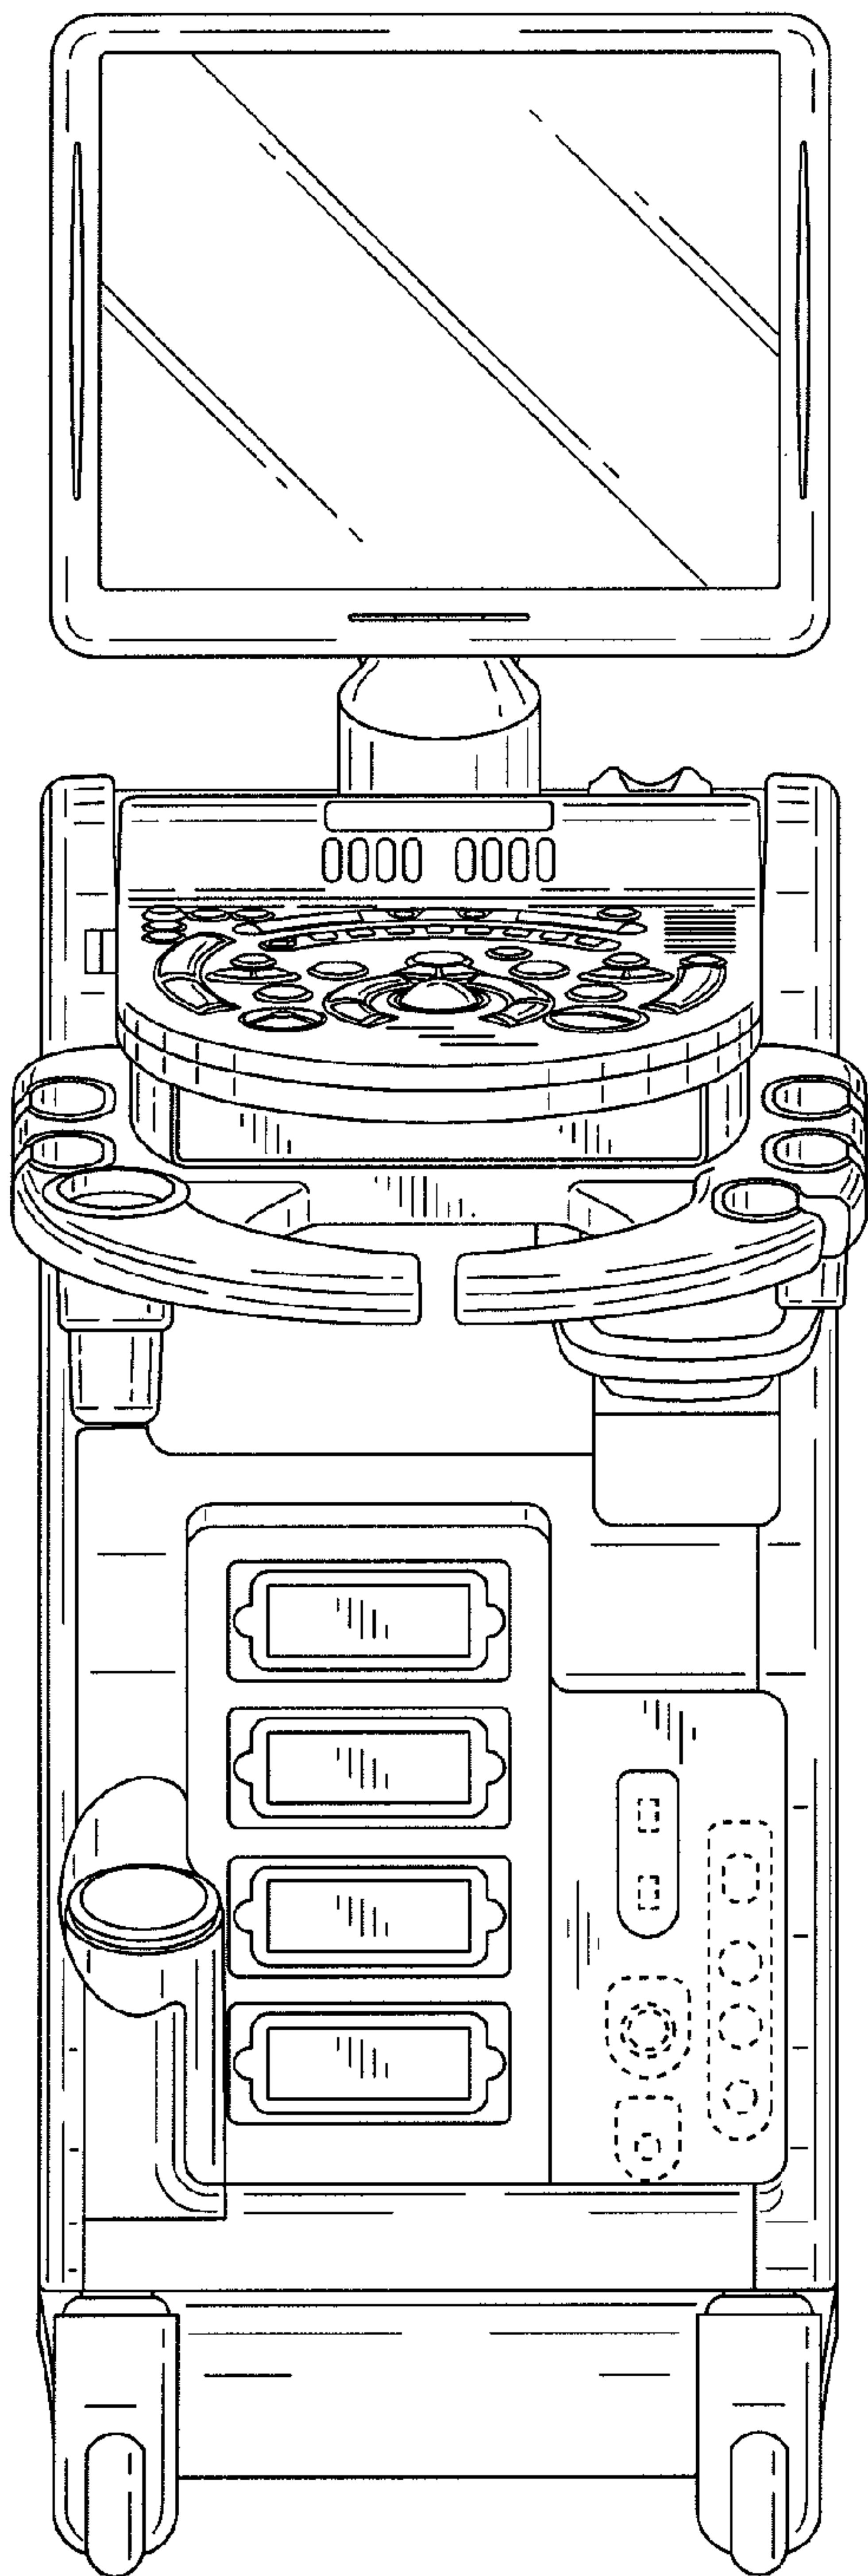


FIG. 2

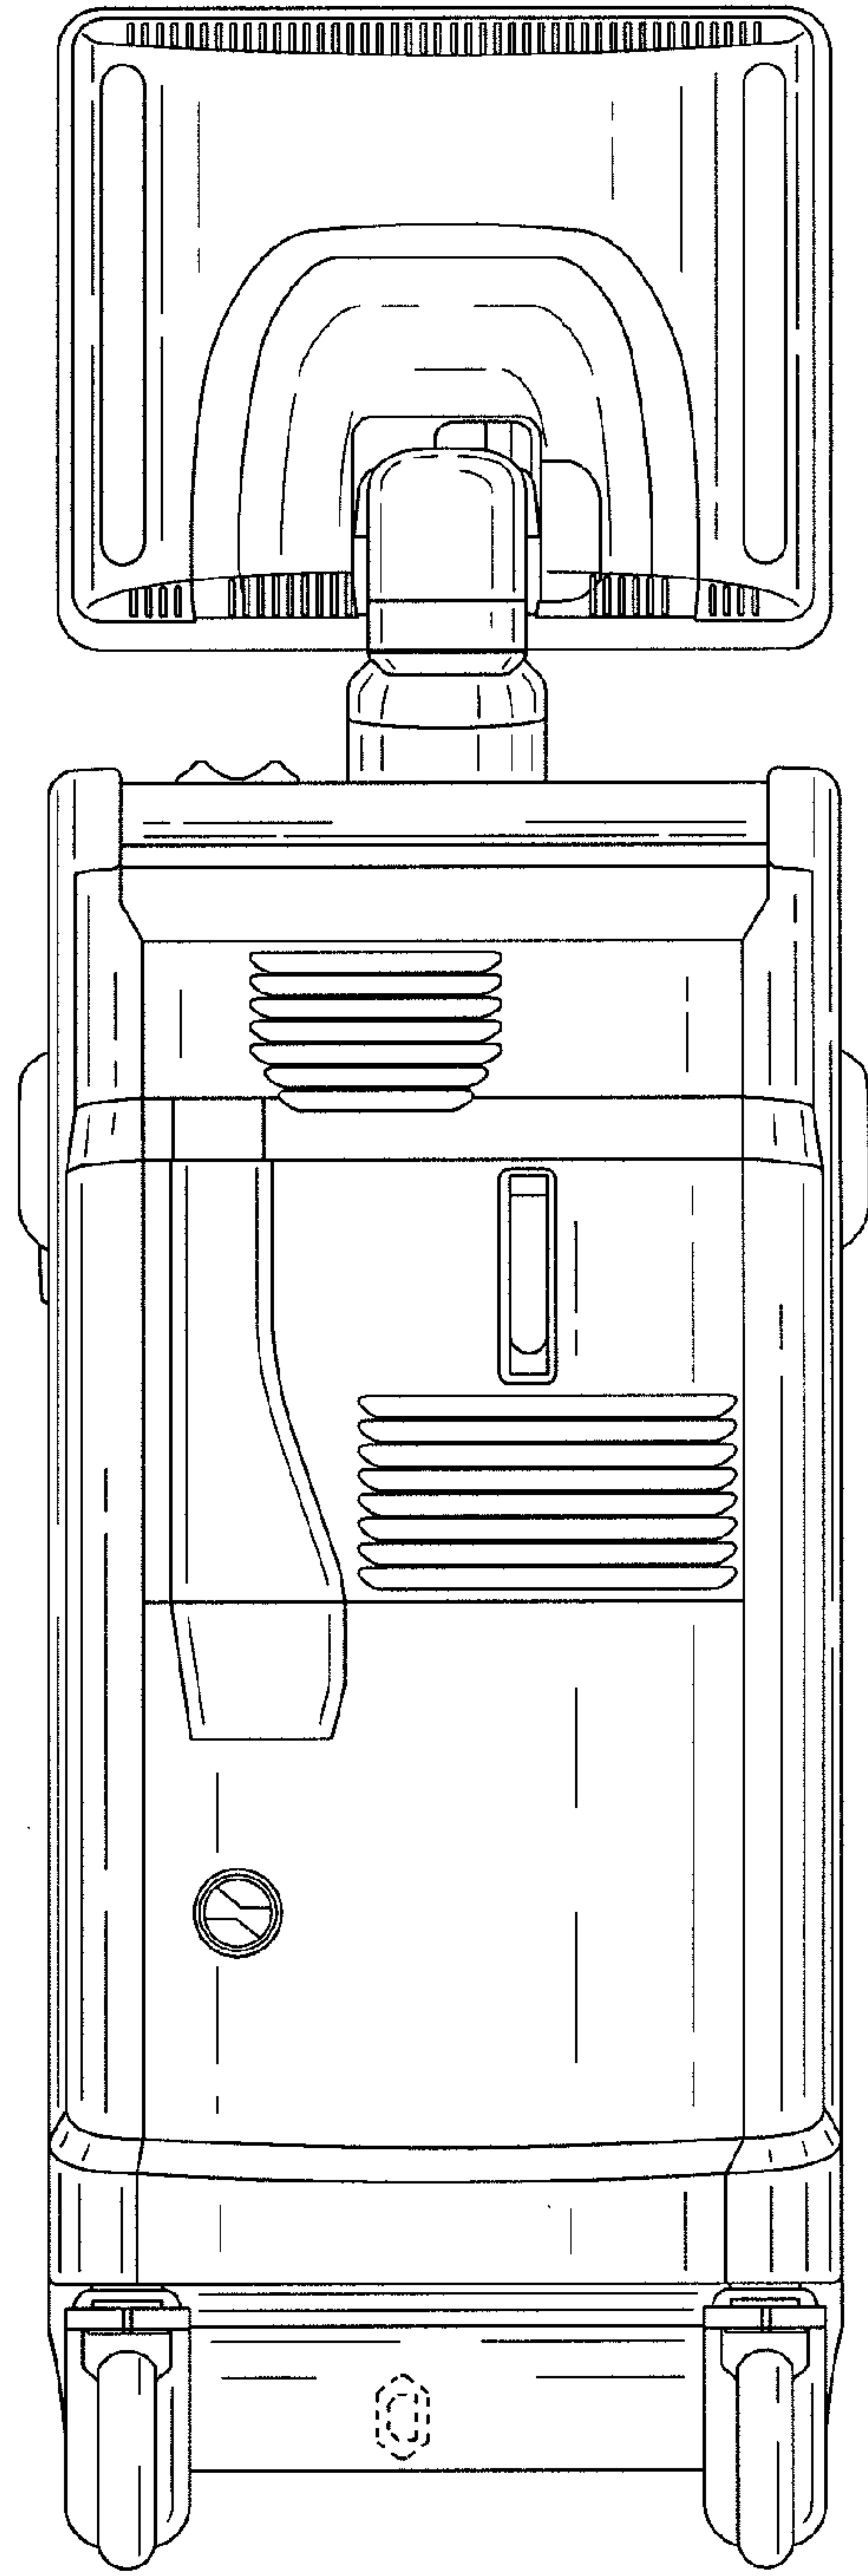


FIG. 3

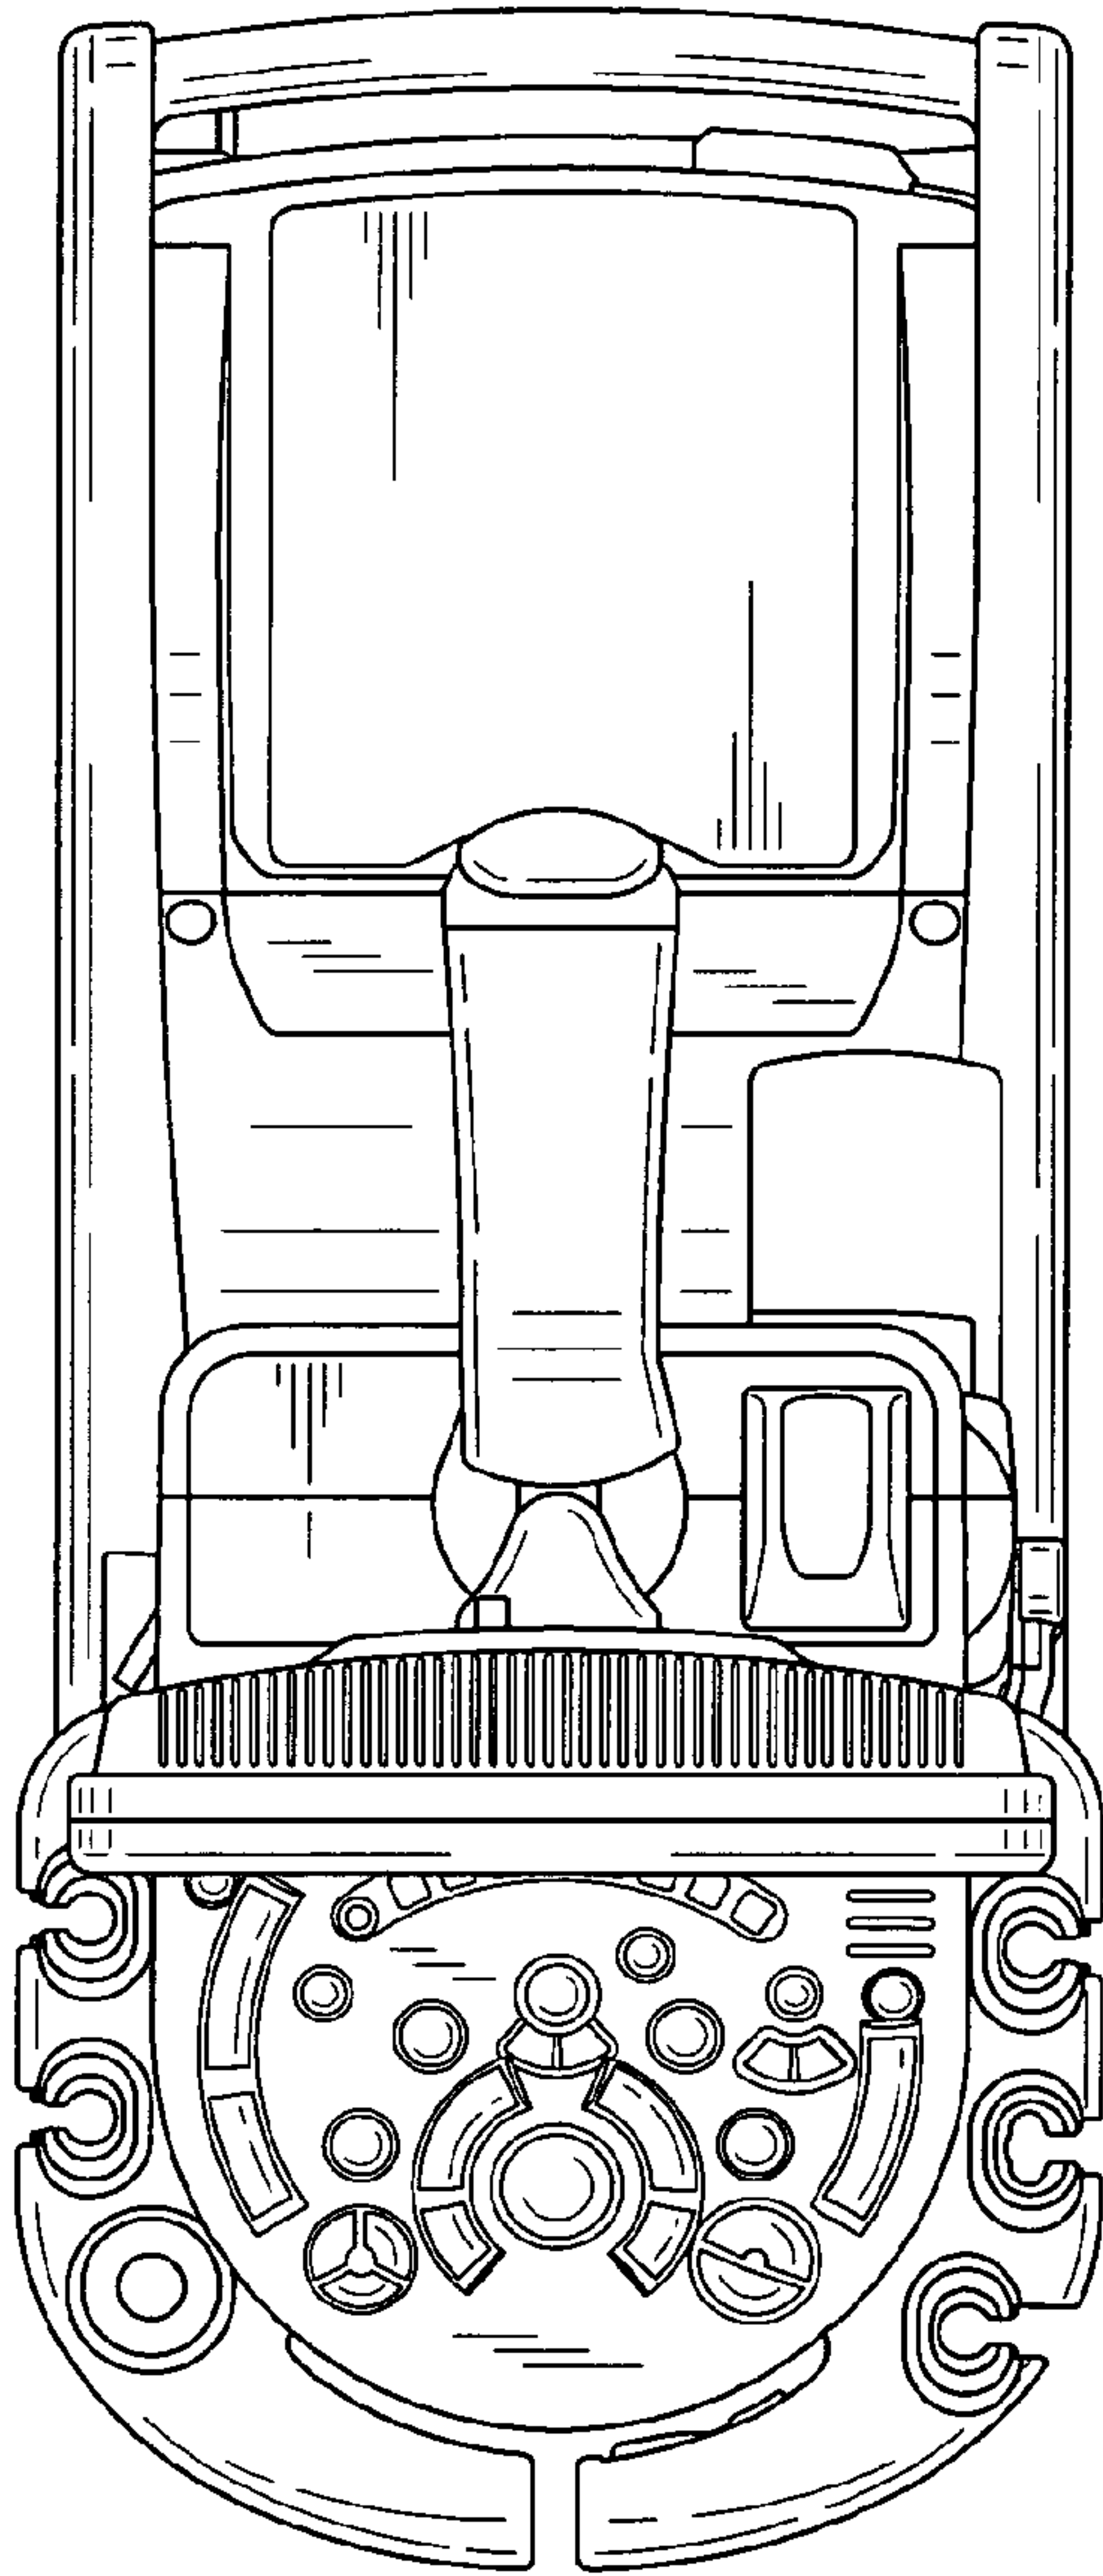


FIG. 4

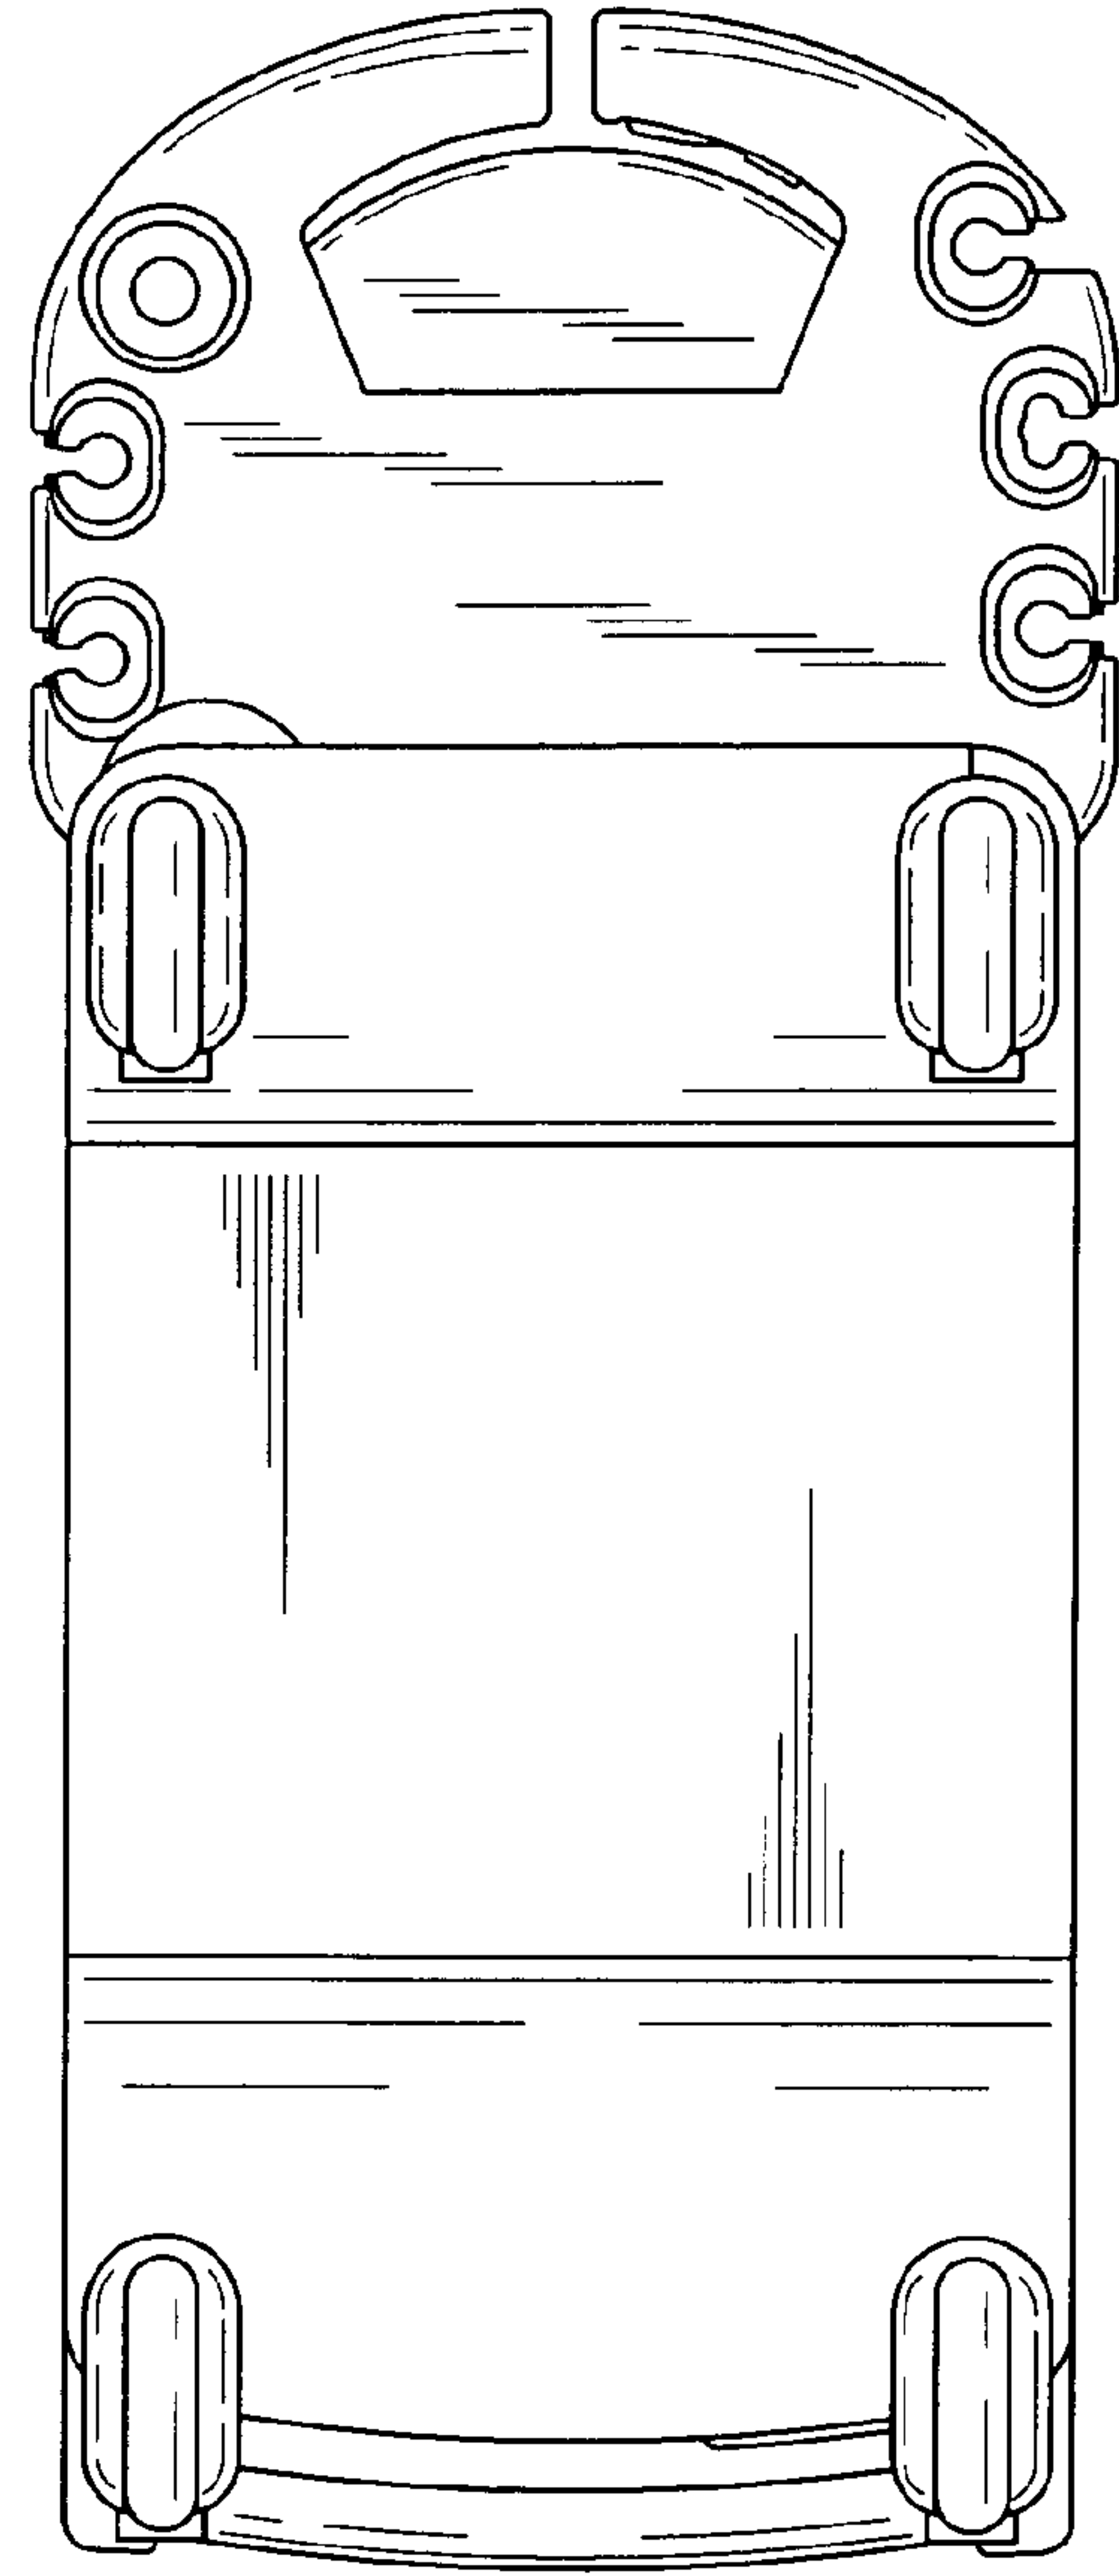


FIG. 5

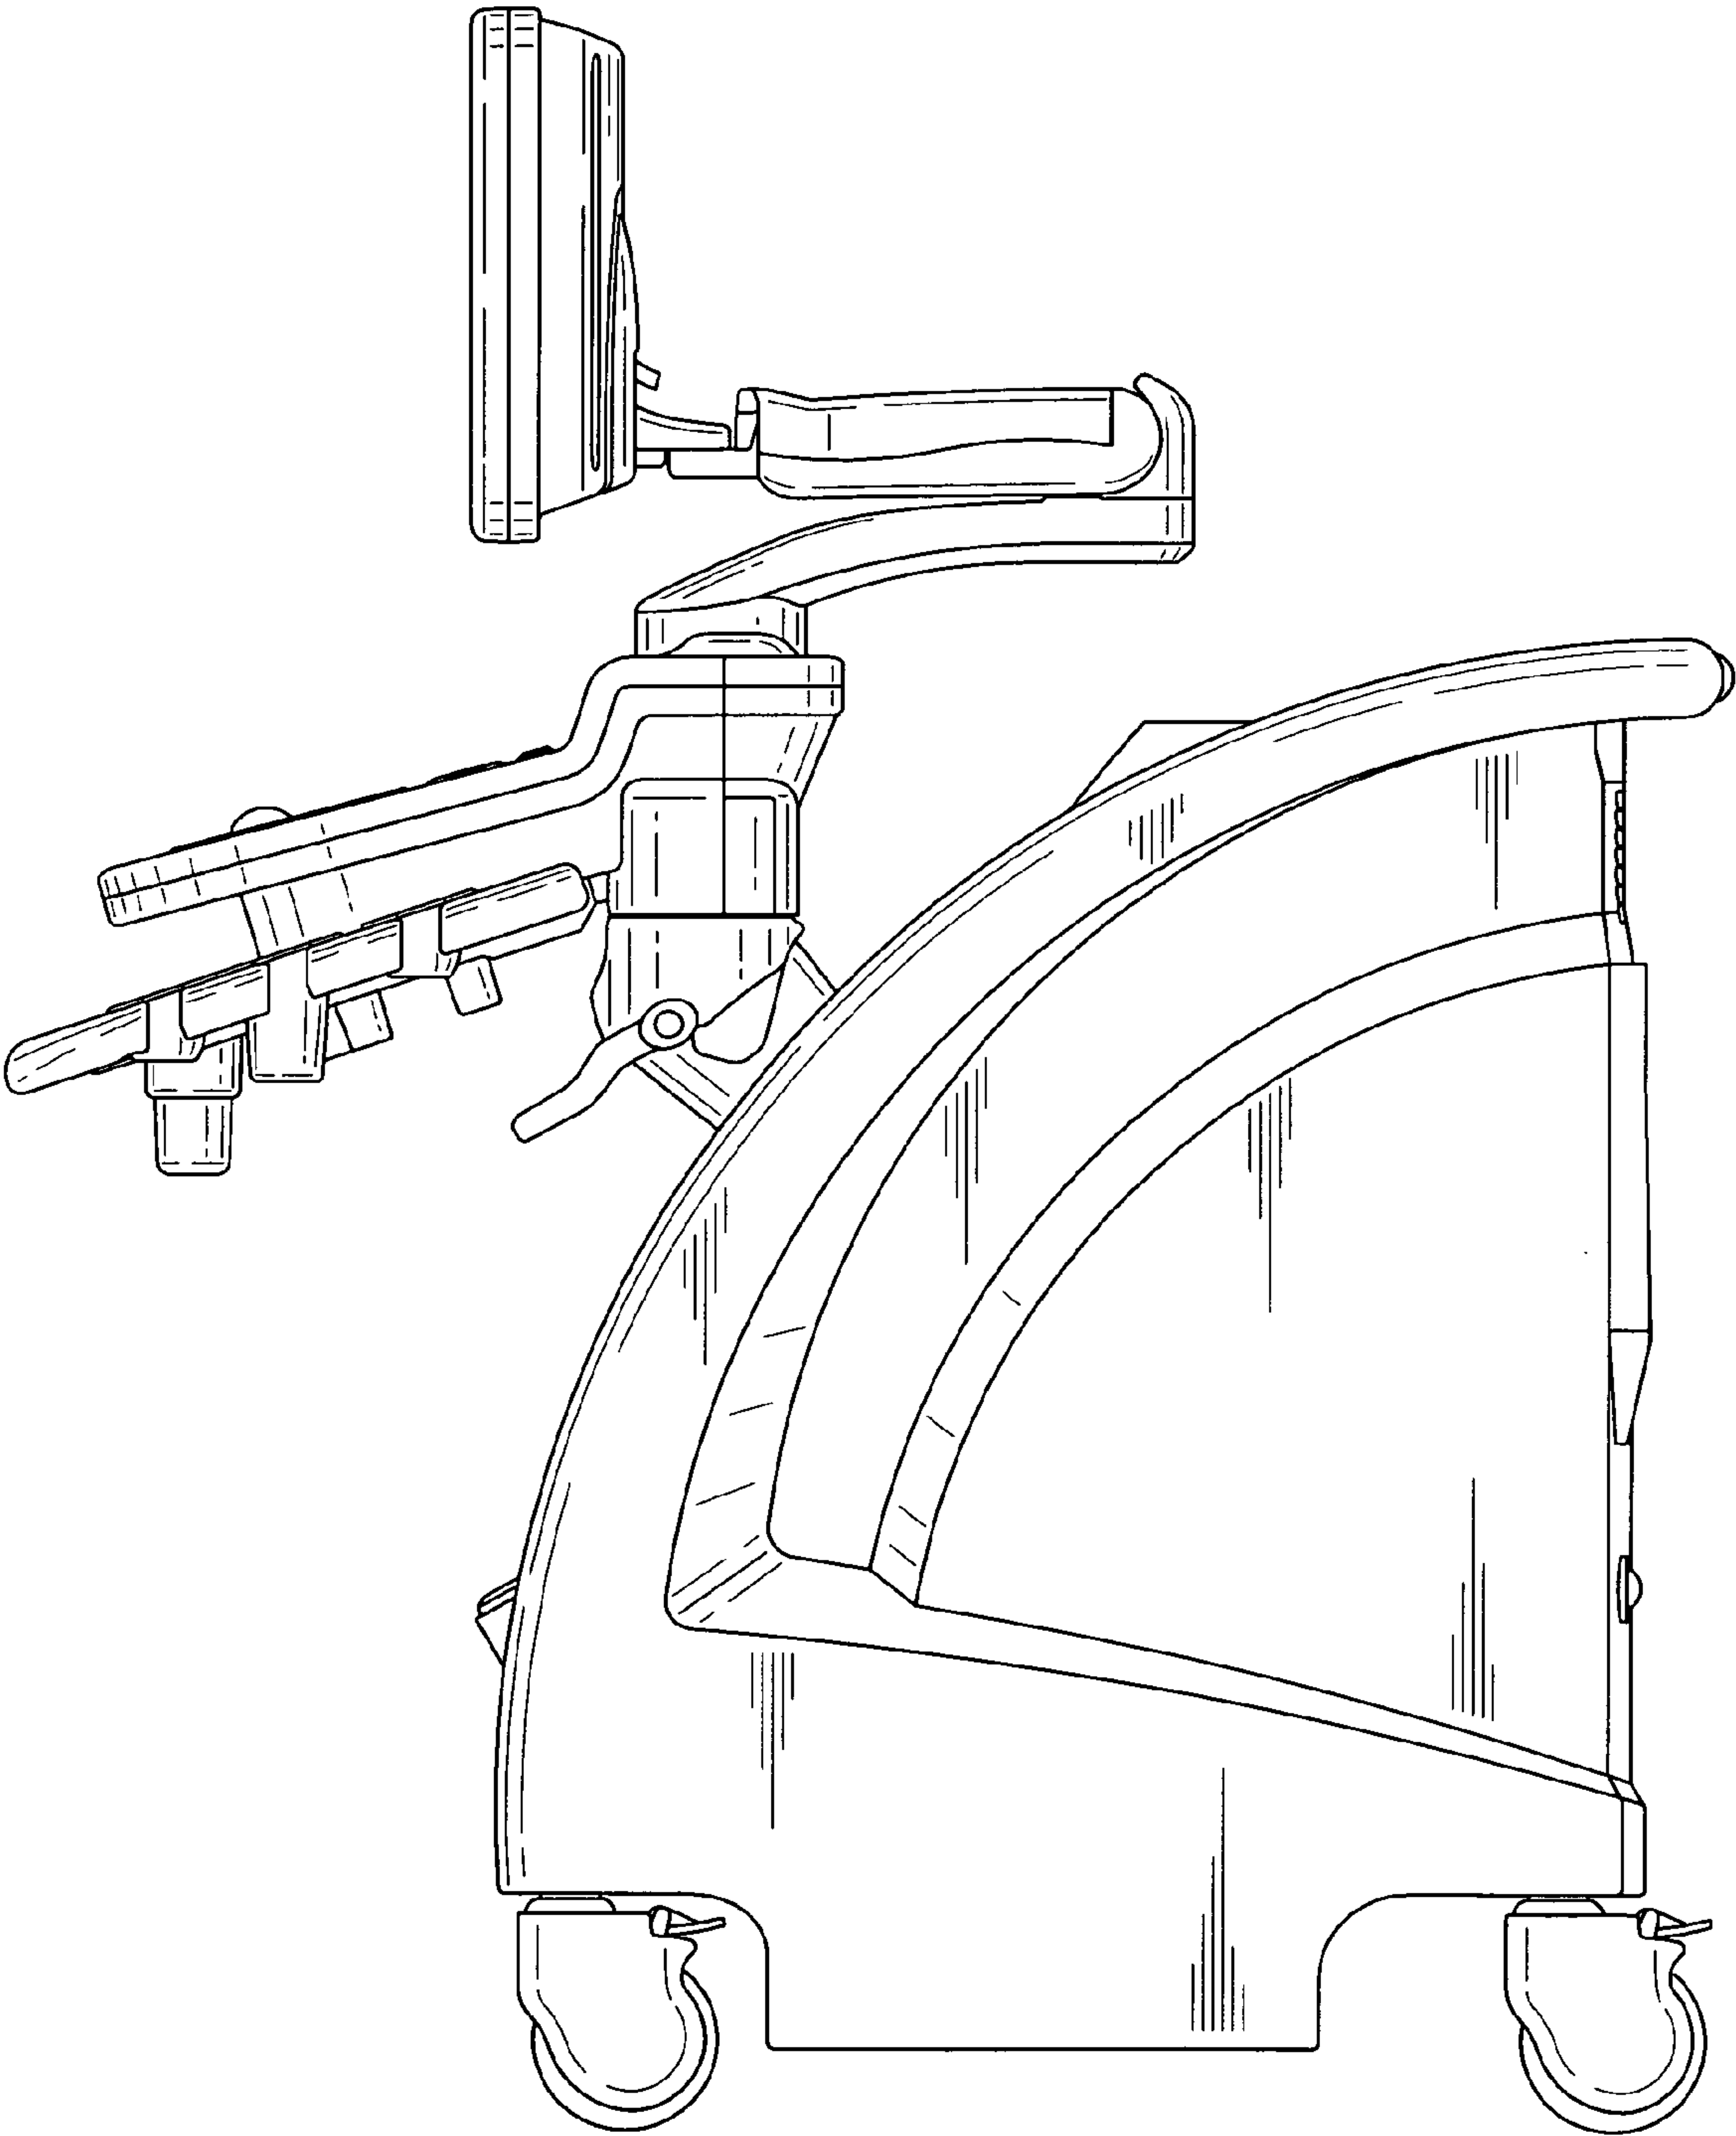


FIG. 6

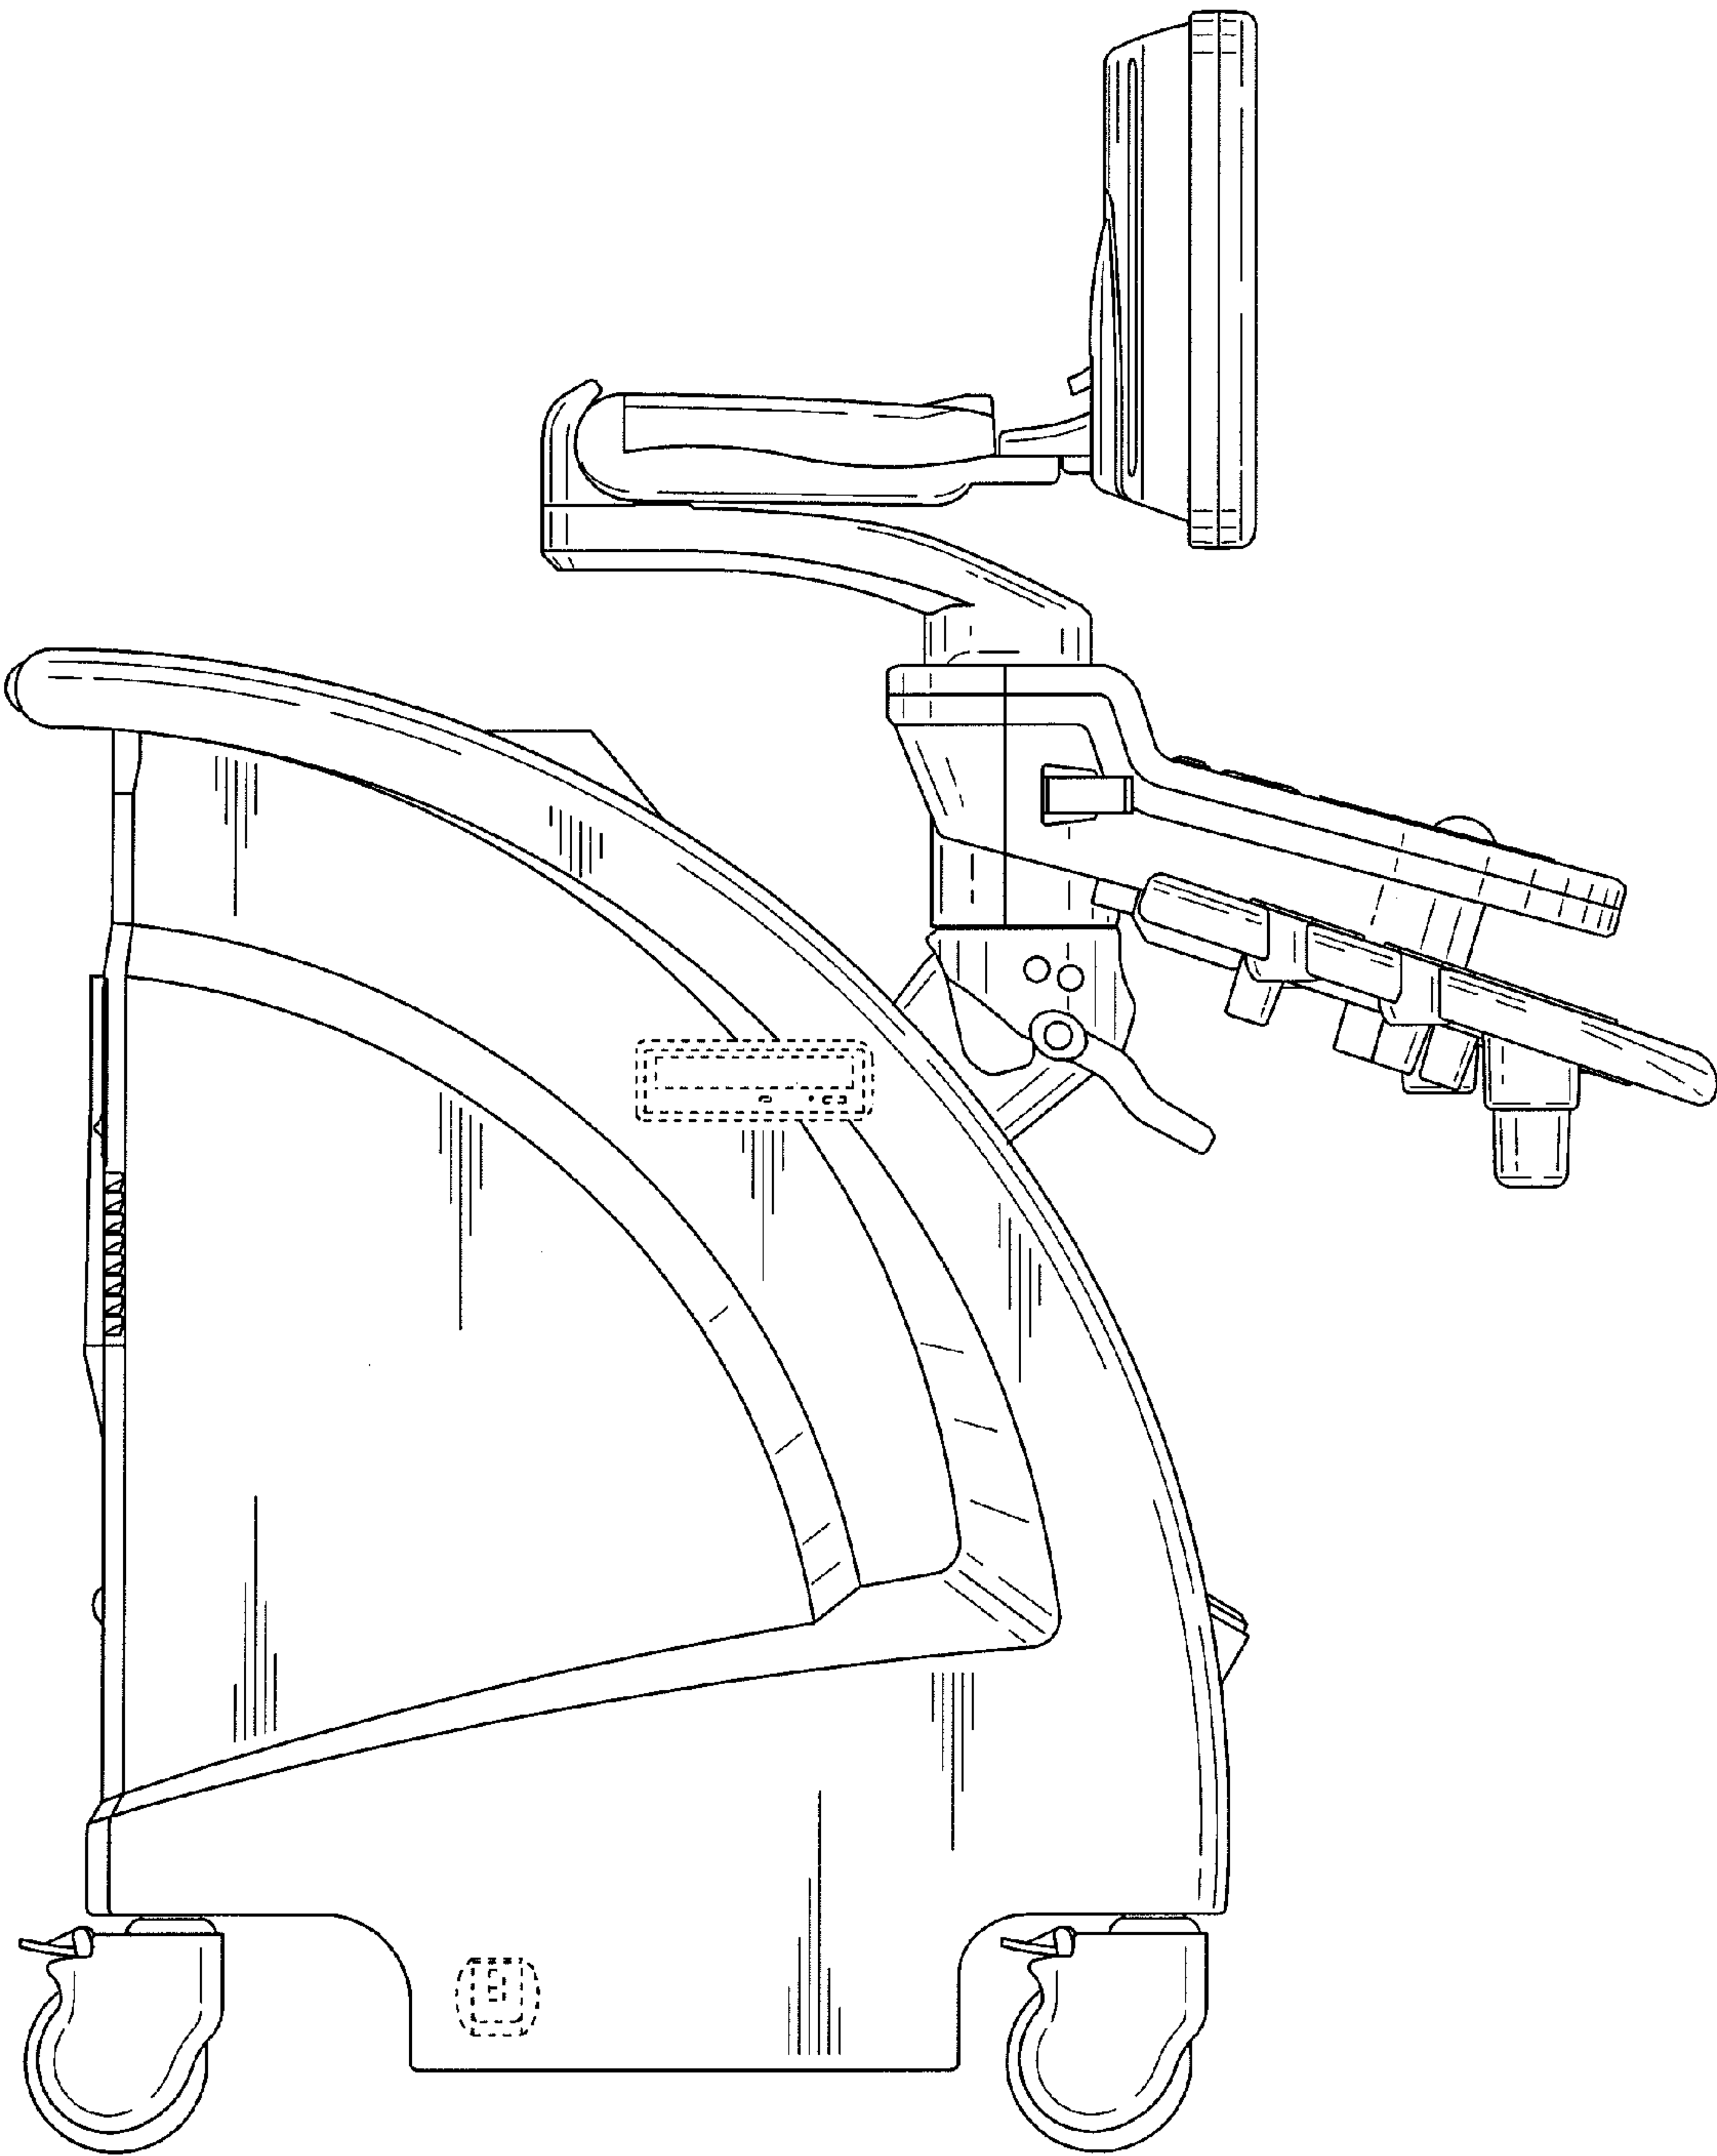


FIG. 7