



US00D628212S

(12) **United States Design Patent**
Molden

(10) **Patent No.:** **US D628,212 S**

(45) **Date of Patent:** **** Nov. 30, 2010**

(54) **GRAPHICAL USER INTERFACE FOR A DISPLAY SCREEN**

(75) Inventor: **Mathias Molden**, Stavanger (NO)

(73) Assignee: **Laerdal Medical AS**, Stavanger (NO)

(**) Term: **14 Years**

(21) Appl. No.: **29/324,110**

(22) Filed: **Sep. 5, 2008**

(30) **Foreign Application Priority Data**

Mar. 7, 2008 (NO) 20080161

(51) **LOC (9) Cl.** **14-04**

(52) **U.S. Cl.** **D14/489**

(58) **Field of Classification Search** D14/485–95;
D18/24–33; D19/6, 52, 9, 10; D20/11; D21/324–33;
715/700–867, 973–77

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D253,490 S	11/1979	Reiser	
D263,740 S	4/1982	Rogers et al.	
4,797,104 A	1/1989	Laerdal et al.	434/265
5,241,302 A	8/1993	Thong	340/701
D354,811 S	1/1995	Tsushi	
D378,414 S	3/1997	Allen et al.	
D425,080 S *	5/2000	Cappa et al.	D14/492
6,390,996 B1	5/2002	Halperin et al.	601/41
D462,696 S *	9/2002	Sturm	D14/489
D466,215 S	11/2002	Lindseth et al.	
D468,323 S *	1/2003	Schmitt	D14/489
D482,042 S *	11/2003	Peters	D14/492
D550,244 S *	9/2007	Nijima	D14/491
D562,985 S	2/2008	Brefka et al.	
D572,726 S *	7/2008	Guimaraes et al.	D14/495
D579,569 S	10/2008	Strawn et al.	
D585,910 S *	2/2009	Chen et al.	D14/492
D588,607 S *	3/2009	O'Donnell et al.	D14/489
D590,509 S	4/2009	Costa	
D590,837 S *	4/2009	Dawson et al.	D14/492

D593,127 S *	5/2009	Hosokawa et al.	D14/492
2004/0157199 A1	8/2004	Eggert et al.	
2008/0145827 A1	6/2008	Strand et al.	434/265
2008/0146973 A1	6/2008	Lund et al.	601/40
2008/0146974 A1	6/2008	Lund et al.	601/41

FOREIGN PATENT DOCUMENTS

DE	102004007077	9/2005
EP	1609453	11/1999

(Continued)

OTHER PUBLICATIONS

Abella, Benjamin S. et al., "Quality of Cardiopulmonary Resuscitation During In-Hospital Cardiac Arrest," (Reprinted) JAMA. 2005; vol. 293, No. 3.

(Continued)

Primary Examiner—Melanie H Tung
(74) *Attorney, Agent, or Firm*—Dorsey & Whitney LLP

(57) **CLAIM**


The ornamental design for a graphical user interface for a display screen, as shown and described.

DESCRIPTION

The single FIGURE is a front view of a graphical user interface for a display screen showing my new design.

The broken line showing of a display screen is not part of the claimed design.

1 Claim, 1 Drawing Sheet

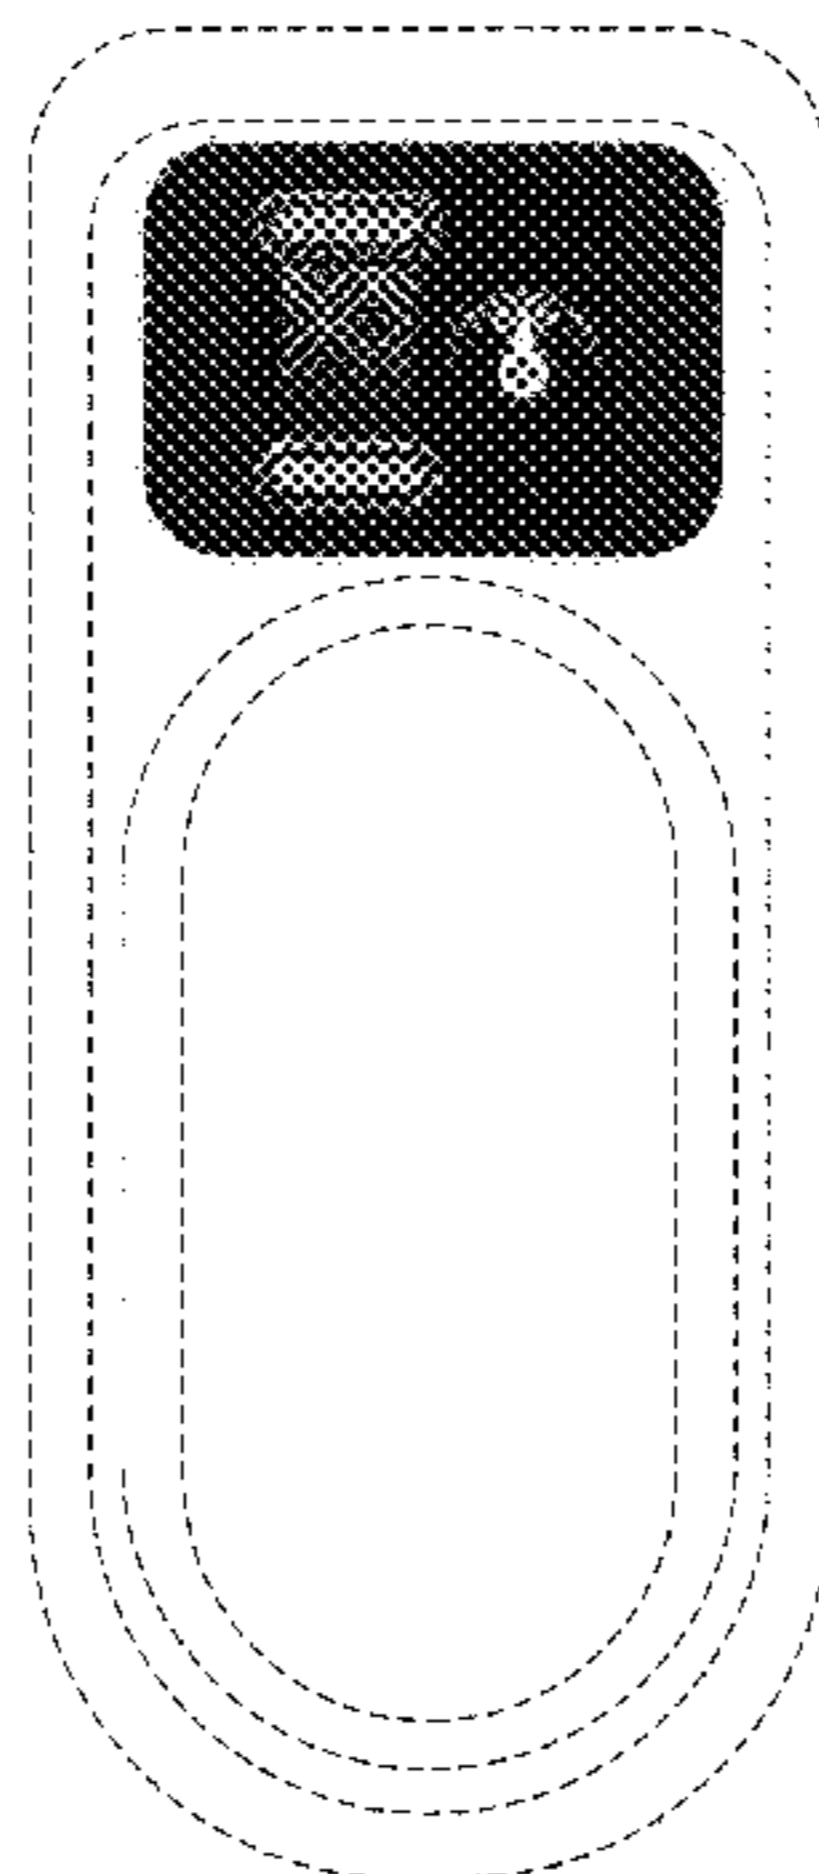

FOREIGN PATENT DOCUMENTS

EP	1057451	5/2000
EP	1578340	7/2004
EP	1491176	12/2004
GB	1425833	4/1973
WO	WO2006/083882	8/2006
WO	WO2006/088373	8/2006

OTHER PUBLICATIONS

American Heart Association, "Guidelines 2000 for Cardiopulmonary Resuscitation and Emergency Cardiovascular Care," *Circulation*. 2000; 102 (suppl. I): I-95-I-104., available online at www.circulationaha.org.

Aufderheide, Tom P. et al., "Hyperventilation-Induced Hypotension During Cardiopulmonary Resuscitation," *Circulation*. 2004; 109, available online at www.circulationaha.org.

van Alem, Anouk P. et al., "Interruption of Cardiopulmonary Resuscitation With the Use of the Automated External Defibrillator in Out-of-Hospital Cardiac Arrest," *Annals of Emergency Medicine*. Oct. 2003; 42:4.

Wik, Lars et al., "Quality of Cardiopulmonary Resuscitation During Out-of-Hospital Cardiac Arrest," (Reprinted) *JAMA*. 2005; vol. 293, No. 3.

* cited by examiner

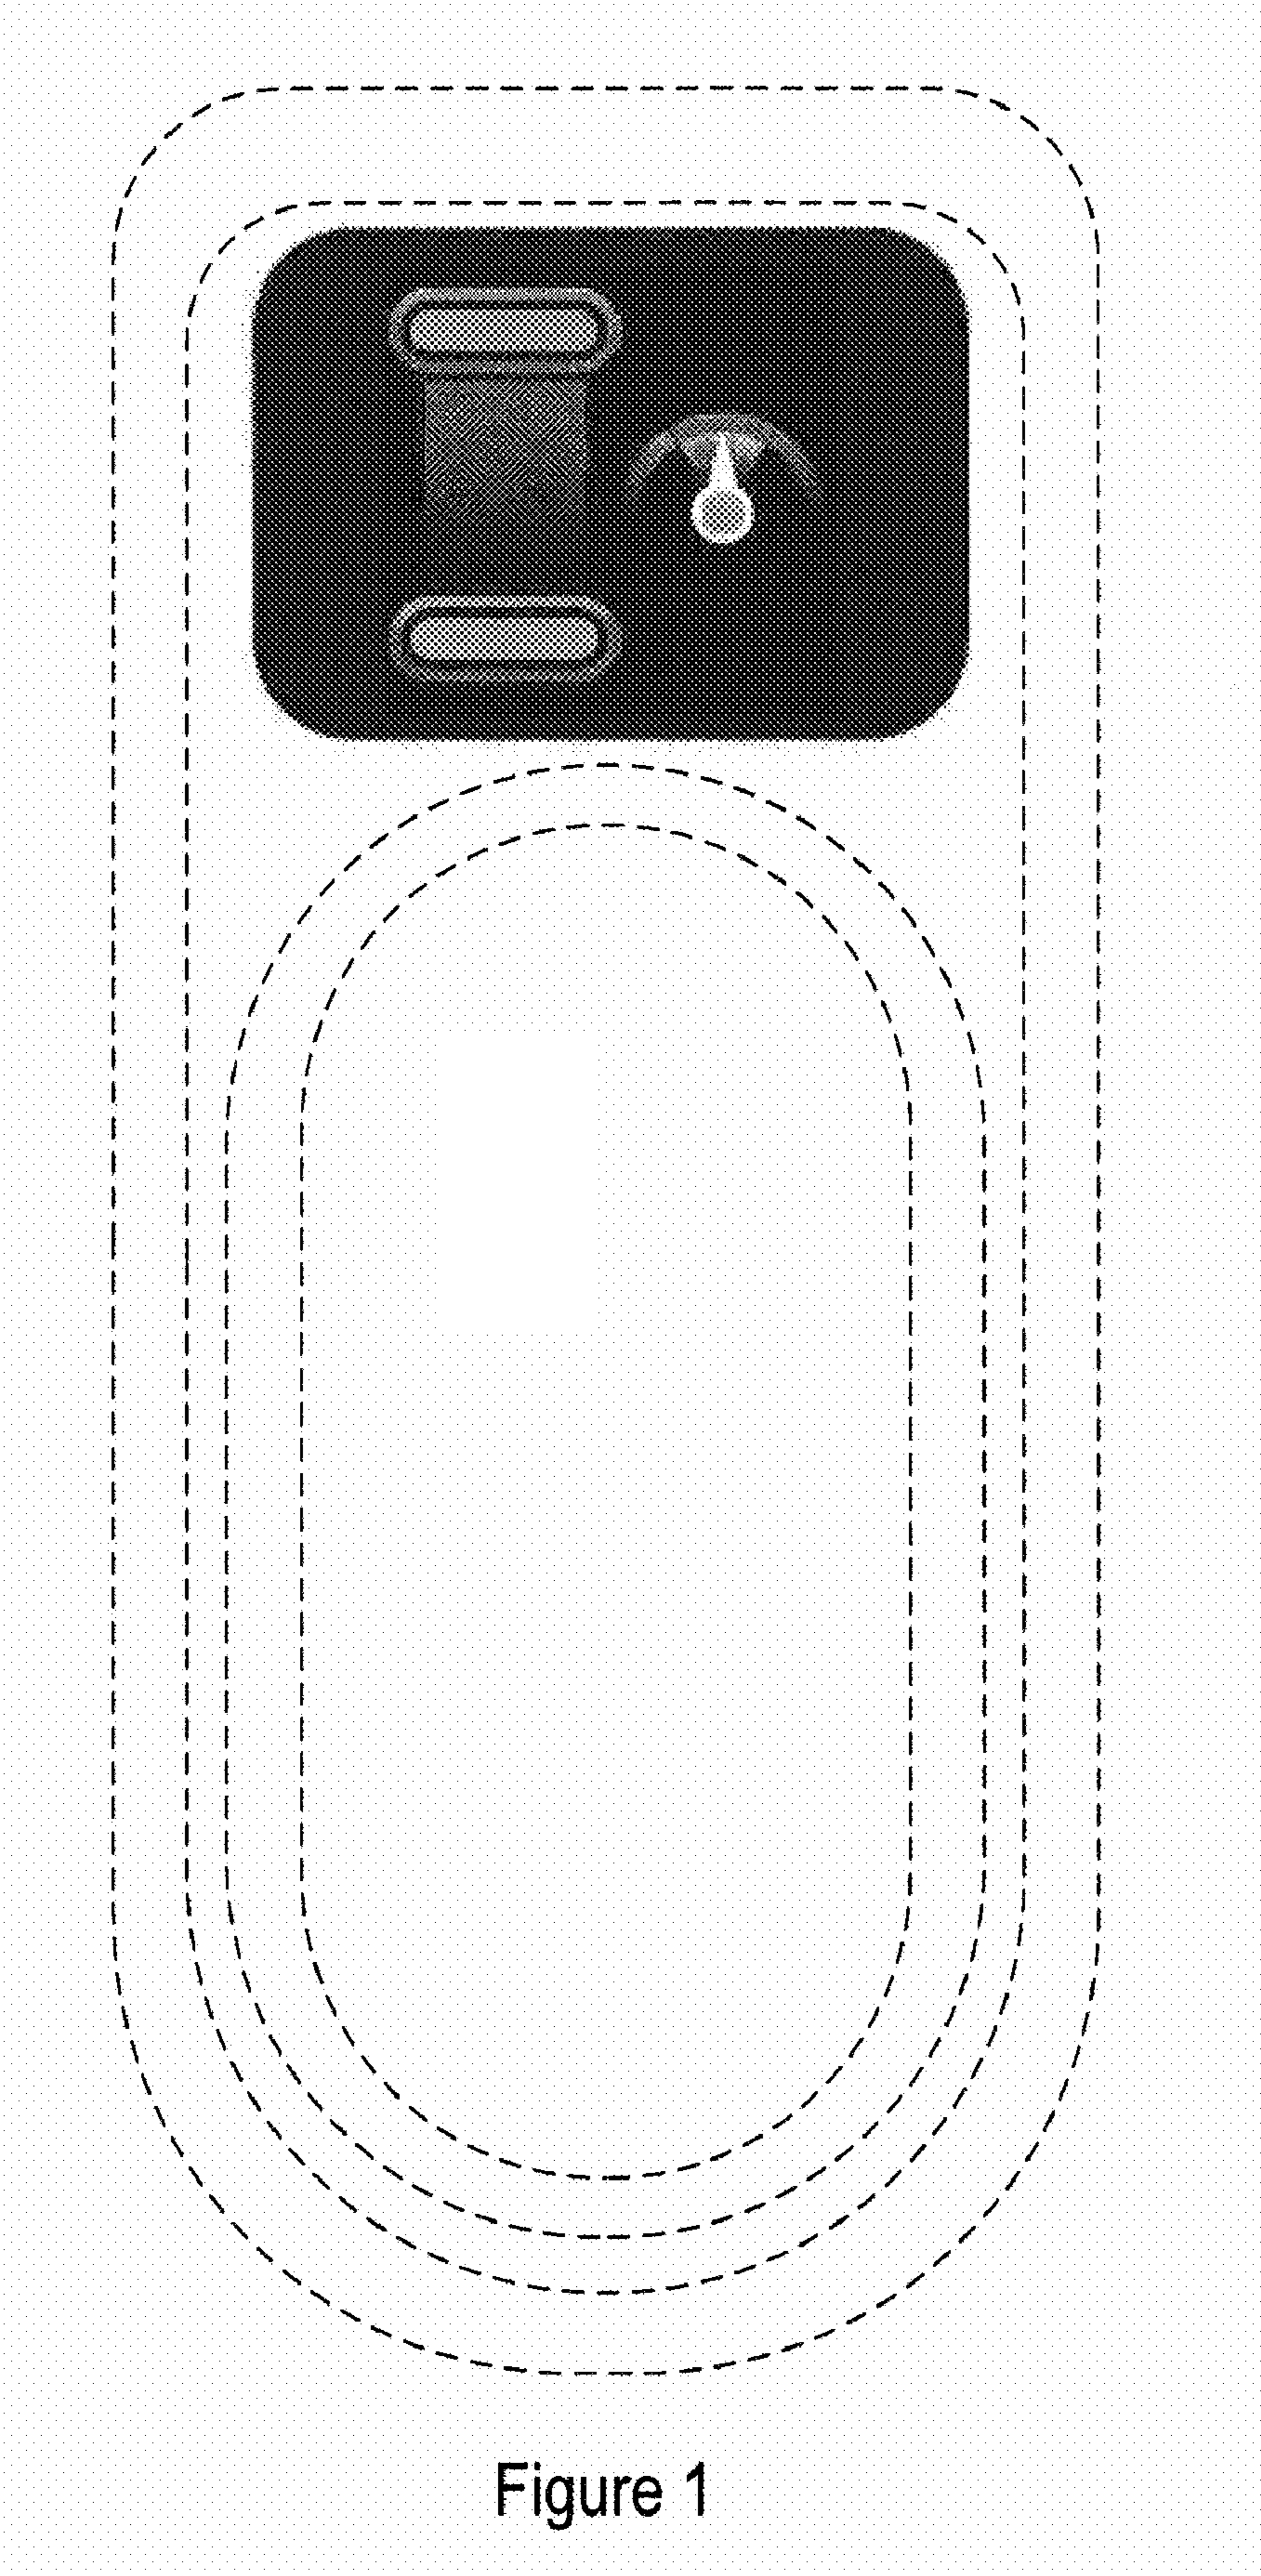


Figure 1