



US00D628307S

(12) **United States Design Patent**
Krause-Bonte

(10) **Patent No.:** **US D628,307 S**

(45) **Date of Patent:** **** Nov. 30, 2010**

(54) **MEDICAL LOUPE WITH HEAD SET**

6,667,832 B2 * 12/2003 Caplan et al. 359/409

(75) Inventor: **Margit Krause-Bonte**, Aalen (DE)

(73) Assignee: **Carl Zeiss Surgical GmbH**,
Oberkochen (DE)

(Continued)

(**) Term: **14 Years**

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Walter Ottesen

(21) Appl. No.: **29/287,399**

(22) Filed: **Aug. 1, 2007**

(57) **CLAIM**

(30) **Foreign Application Priority Data**

The ornamental design for a medical loupe with head set, as shown and described.

Feb. 7, 2007 (EM) 000666359

(51) **LOC (9) Cl.** **24-01**

DESCRIPTION

(52) **U.S. Cl.** **D24/231**

(58) **Field of Classification Search** D24/137,
D24/150, 160, 186, 231; D26/24, 27, 39,
D26/51, 113, 120; D29/103; D16/311, 133,
D16/135–136, 309; 362/105–106, 573, 804;
600/249, 111, 109; 359/409

FIG. 1 is a perspective front view of a medical loupe with head set of my new design;

FIG. 2 is a top plan view of said medical loupe with head set of FIG. 1;

See application file for complete search history.

FIG. 3 is a bottom plan view of said medical loupe with head set of FIG. 1;

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | |
|-----------|-----|---------|------------------|---------|
| 3,285,242 | A * | 11/1966 | Wallace | 600/249 |
| 3,745,993 | A * | 7/1973 | Feinbloom | 600/249 |
| 3,830,230 | A * | 8/1974 | Chester | 362/105 |
| D238,958 | S * | 2/1976 | Bliel | D26/39 |
| D266,192 | S * | 9/1982 | Feinbloom et al. | D26/39 |
| 4,593,683 | A * | 6/1986 | Blaha | 362/804 |
| 4,621,283 | A * | 11/1986 | Feinbloom | 600/109 |
| D296,337 | S * | 6/1988 | Caplan | D16/133 |
| 4,797,736 | A * | 1/1989 | Kloots et al. | 600/109 |
| D333,828 | S * | 3/1993 | Baldassarre | D16/133 |
| D383,229 | S * | 9/1997 | Kiichiro | D26/39 |
| 5,667,291 | A * | 9/1997 | Caplan et al. | 362/105 |
| D398,403 | S * | 9/1998 | Bishop et al. | D24/231 |
| D399,580 | S * | 10/1998 | Feinbloom | D26/39 |
| D406,371 | S * | 3/1999 | Van Der Bel | D26/39 |
| D441,111 | S * | 4/2001 | Van Der Bel | D24/231 |
| D441,886 | S * | 5/2001 | Beck | D24/231 |
| D472,998 | S * | 4/2003 | Paris et al. | D26/39 |

FIG. 4 is a right side elevational view of said medical loupe with head set of FIG. 1;

FIG. 5 is a left side elevational view of said medical loupe with head set of FIG. 1;


FIG. 6 is a front elevational view of said medical loupe with head set of FIG. 1; and,

FIG. 7 is a rear elevational view of said medical loupe with head set of FIG. 1.

The broken lines are included for the purpose of illustrating portions of the medical loupe with head set that form no part of the claimed design.

The adjusting knob at the back of the head set and the lock knob at the front end as well as the accessory plate at the top of the head set and the base of the switch are shaded to represent the color blue.

1 Claim, 7 Drawing Sheets

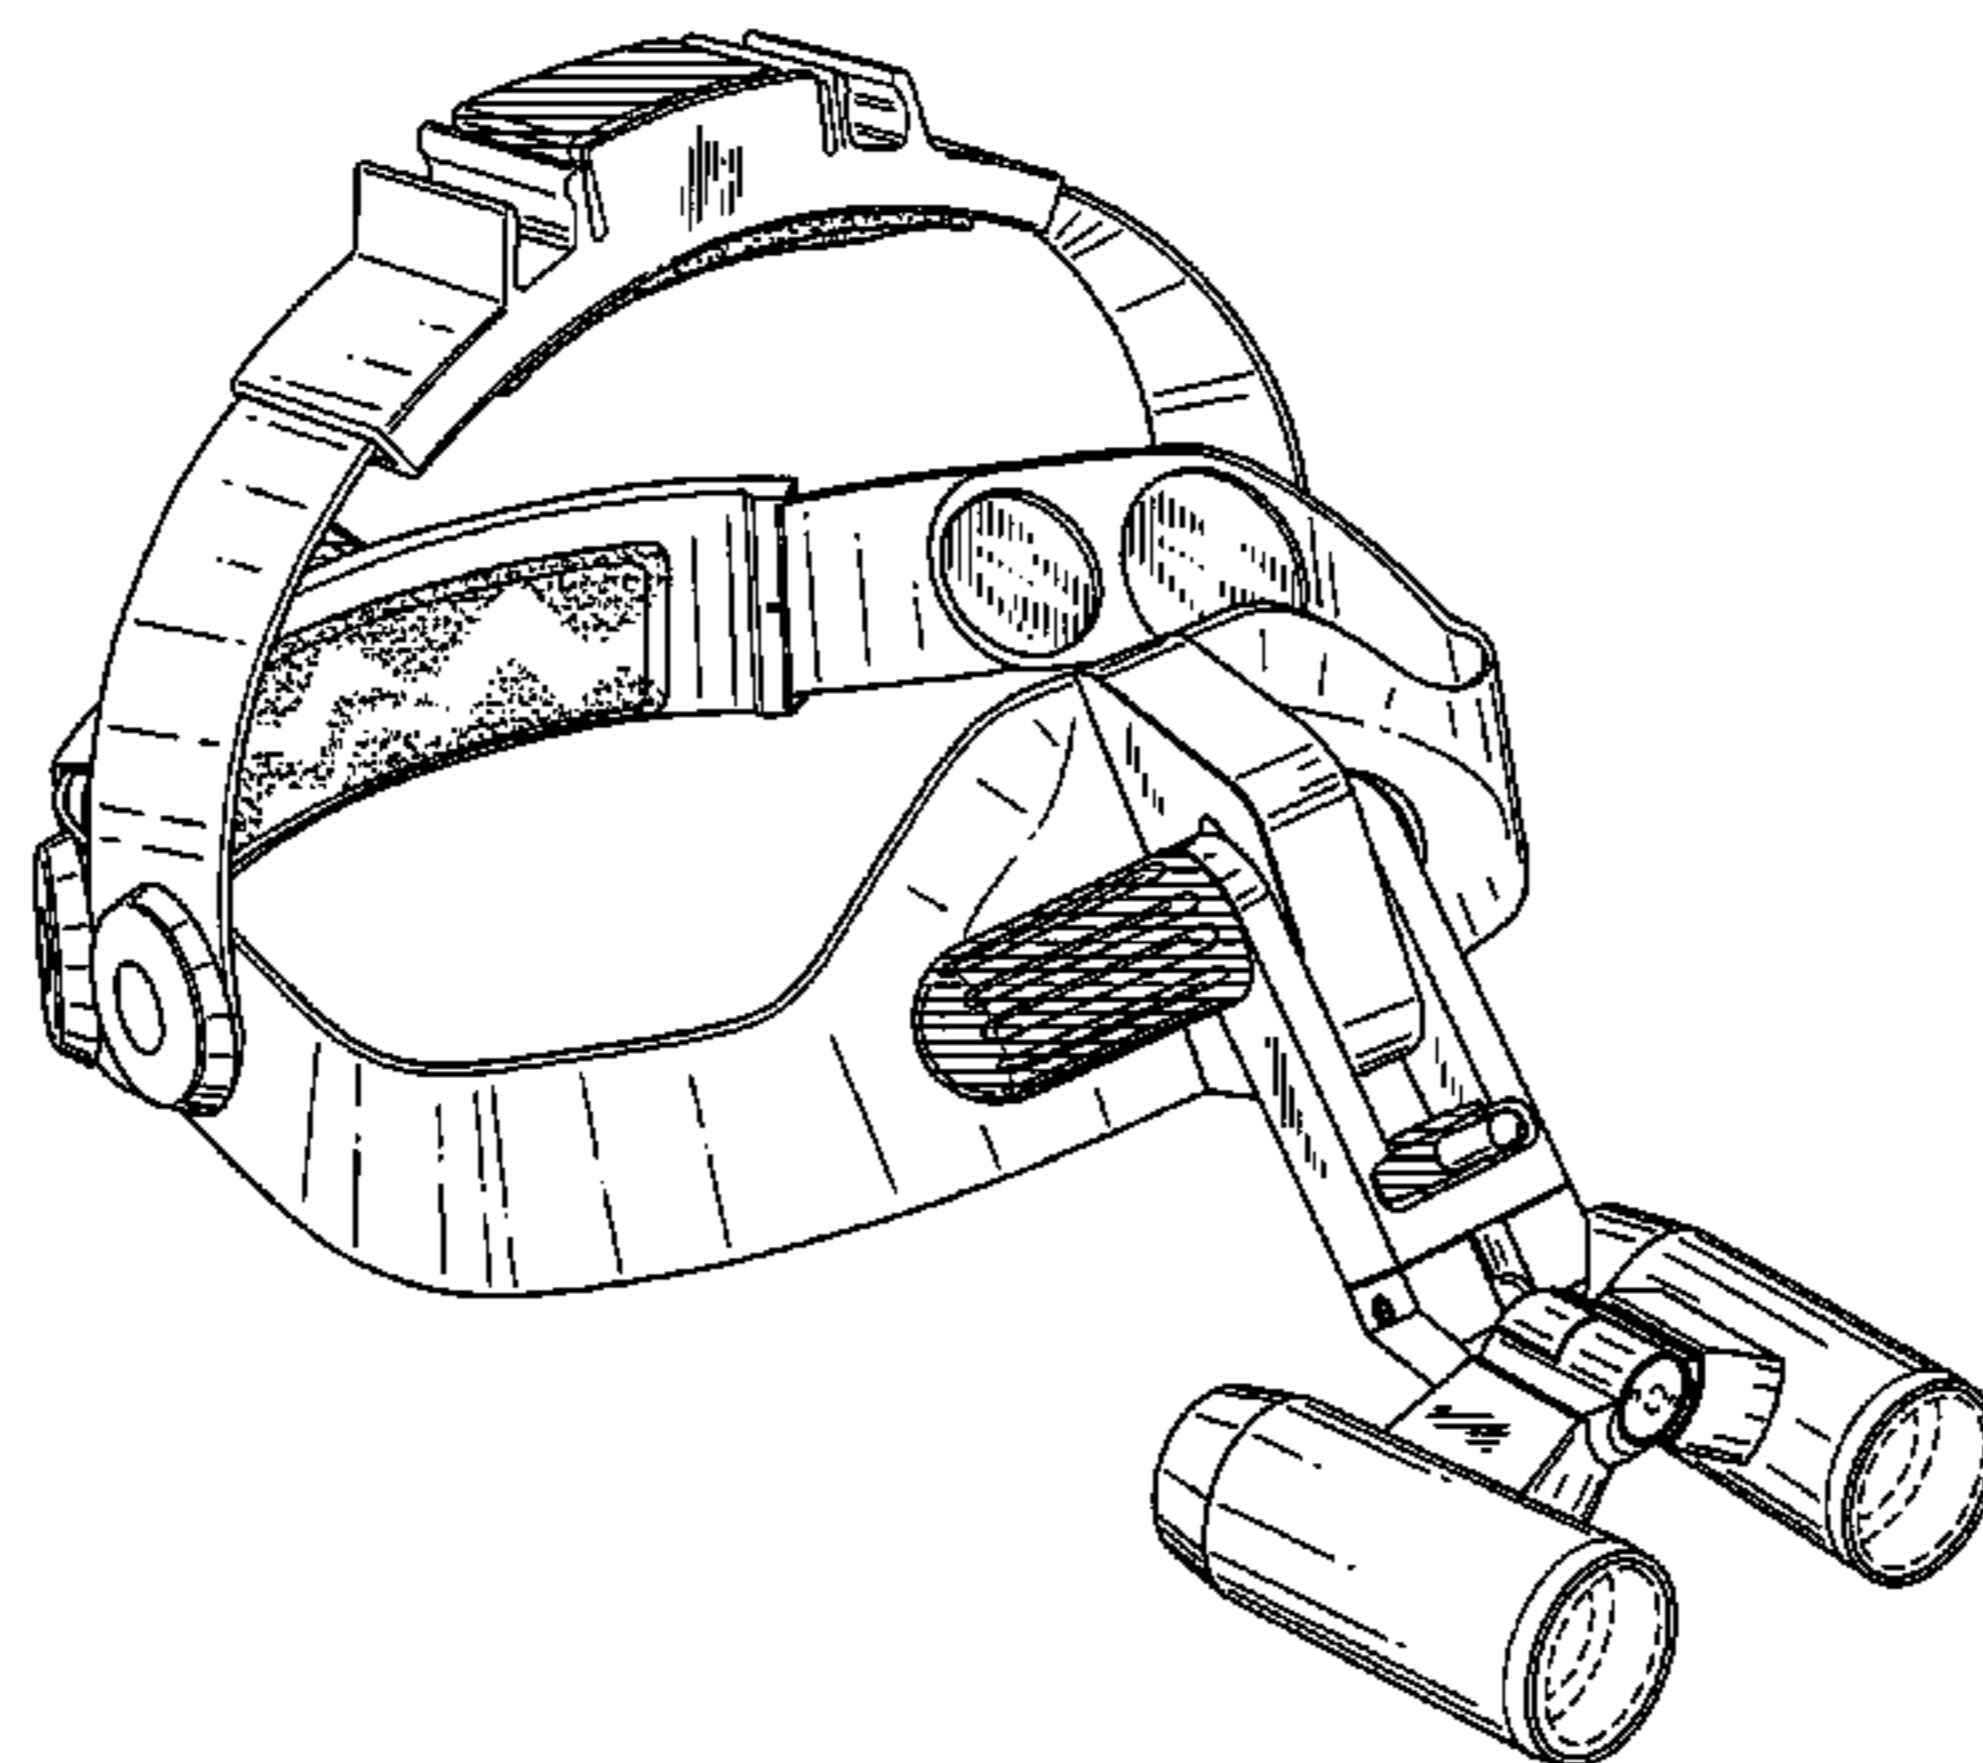

US D628,307 S

Page 2

U.S. PATENT DOCUMENTS

| | | | | | | | |
|----------------|---------|----------------------|---------|-------------------|---------|-----------------------|---------|
| D489,838 S * | 5/2004 | Opolka | D26/39 | D586,932 S * | 2/2009 | Feinbloom et al. | D26/39 |
| 6,955,444 B2 * | 10/2005 | Gupta | 362/105 | D591,327 S * | 4/2009 | Krause-Bonte | D16/309 |
| D531,335 S * | 10/2006 | Garrity | D26/39 | D592,691 S * | 5/2009 | Chang | D16/309 |
| D539,952 S * | 4/2007 | Iranyi et al. | D26/39 | D592,692 S * | 5/2009 | Chang | D16/309 |
| 7,210,810 B1 * | 5/2007 | Iversen et | 362/105 | D592,693 S * | 5/2009 | Chang | D16/309 |
| D552,278 S * | 10/2007 | Spartano et al. | D26/39 | D608,479 S * | 1/2010 | Heine et al. | D24/231 |
| D564,011 S * | 3/2008 | Beate et al. | D16/309 | 2006/0245175 A1 * | 11/2006 | Heine et al. | 362/105 |
| | | | | 2008/0239707 A1 * | 10/2008 | Feinbloom et al. | 362/105 |

* cited by examiner

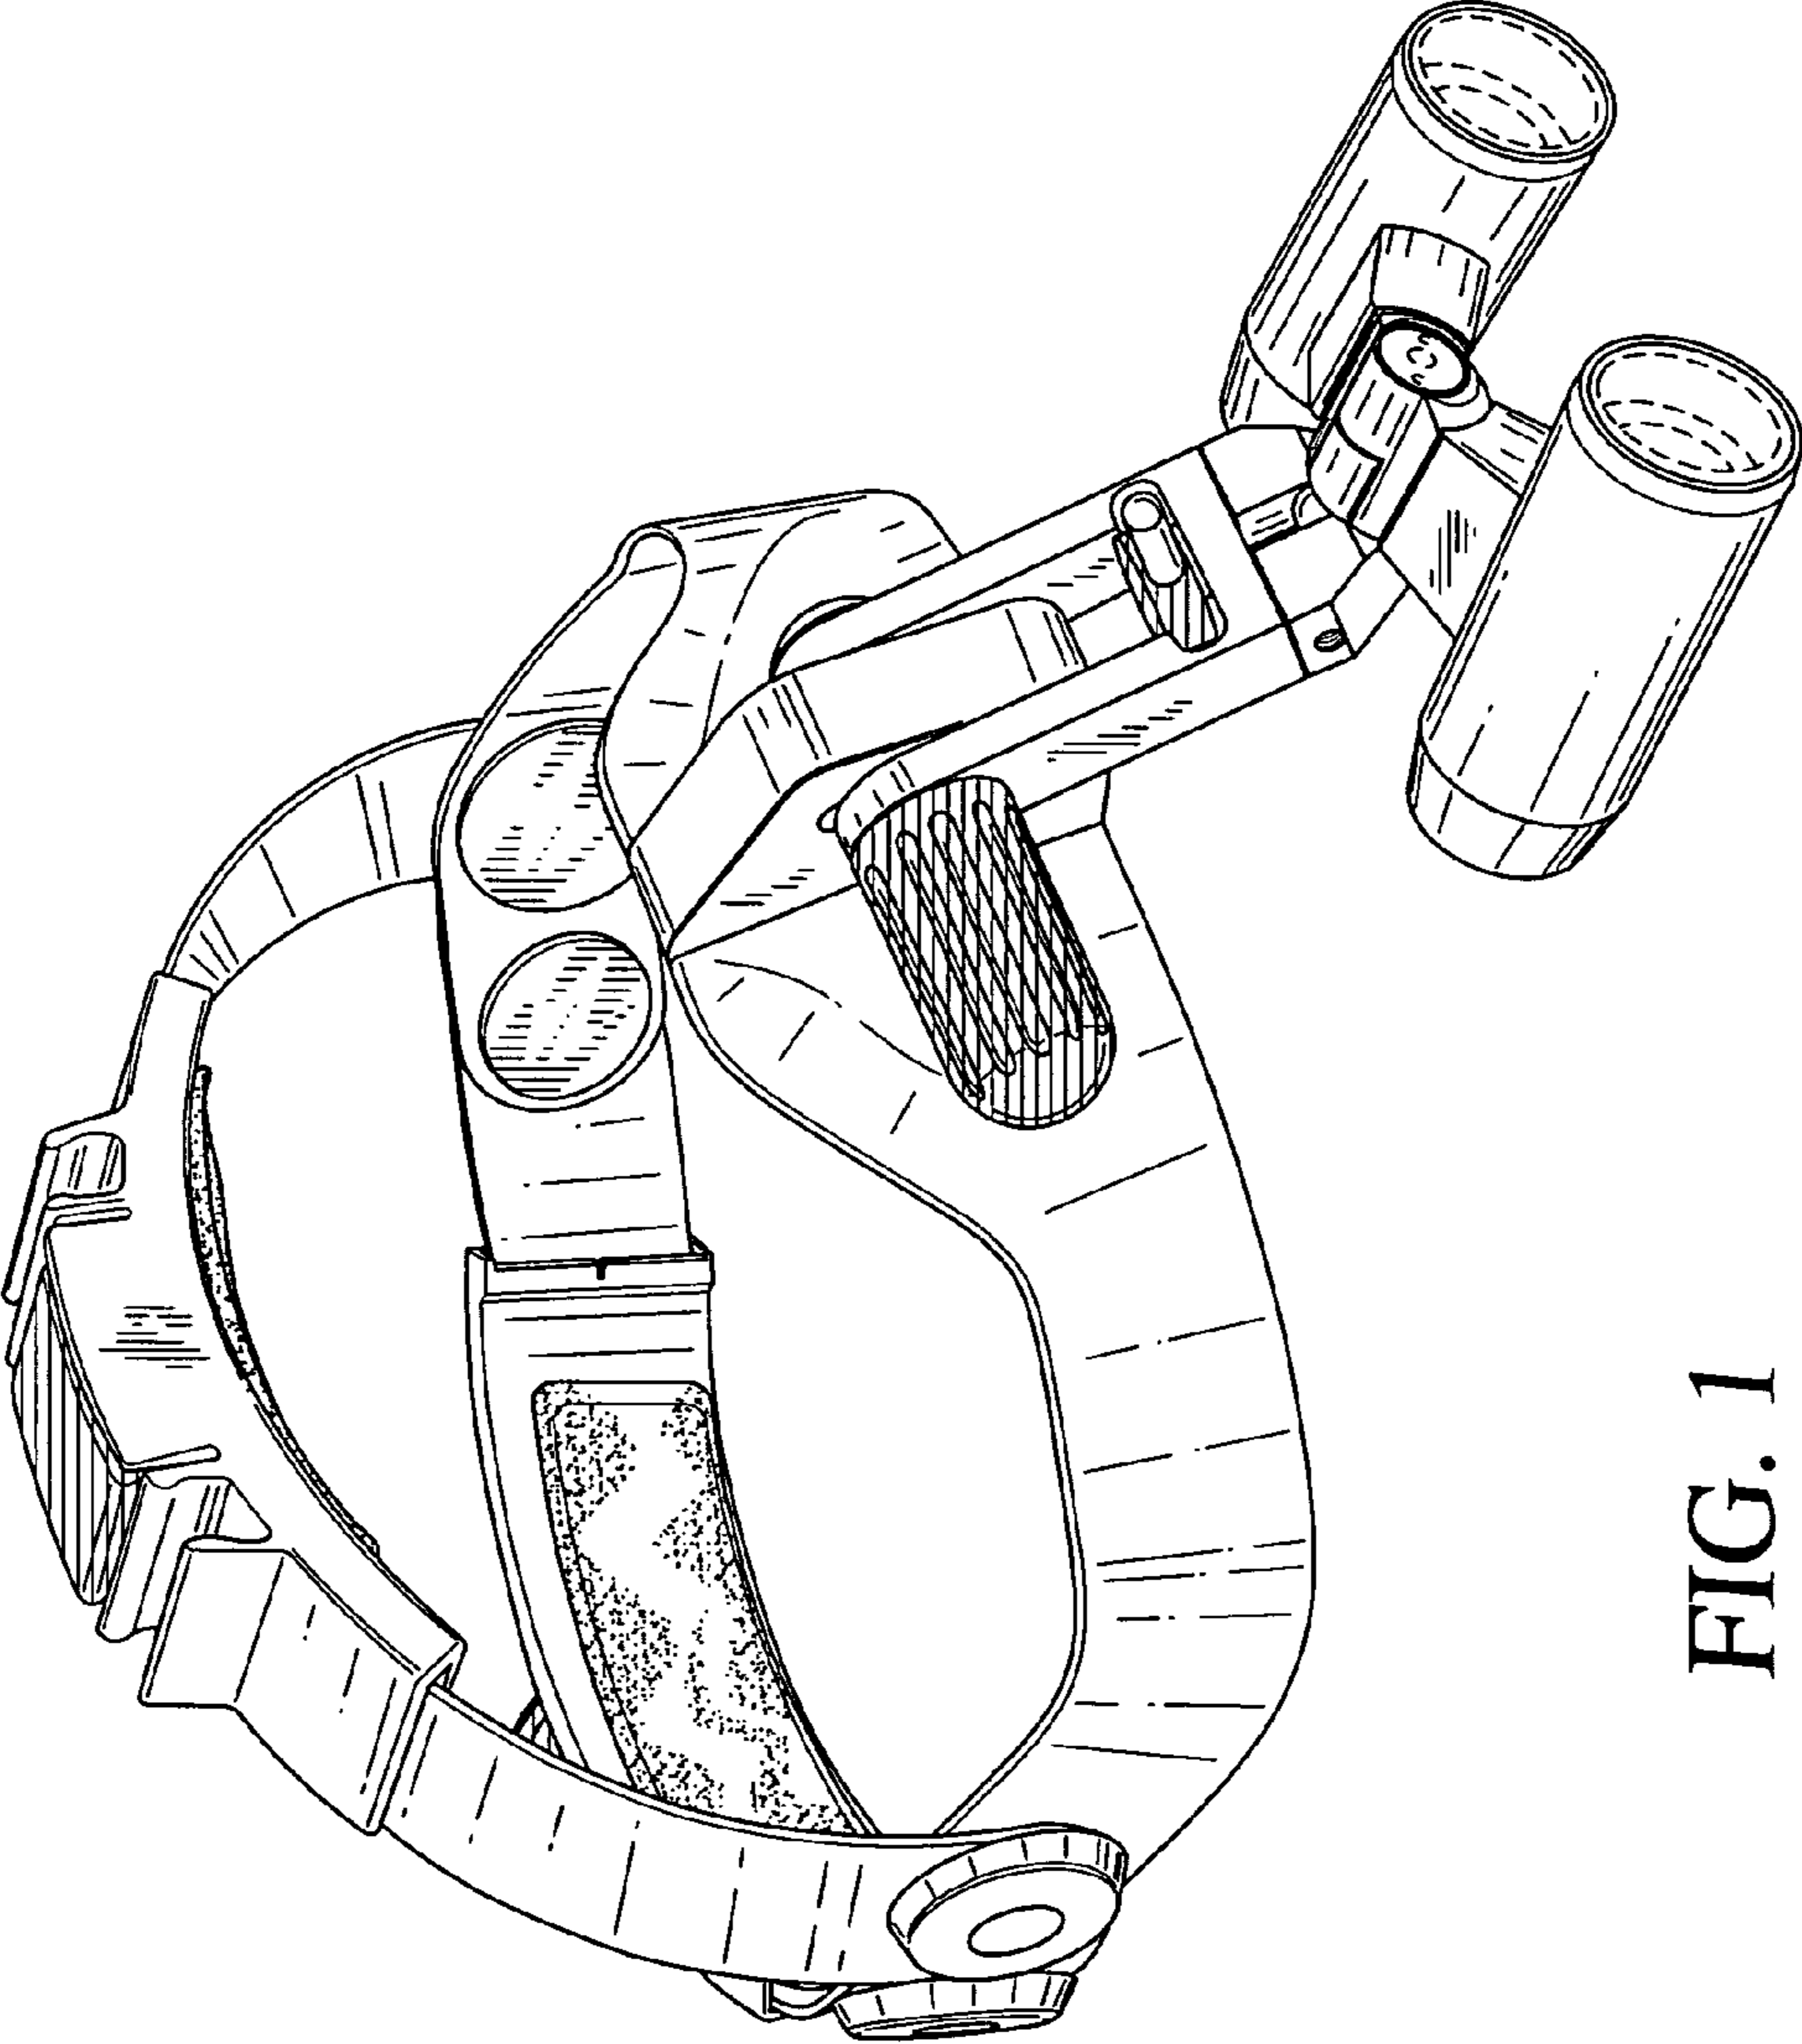


FIG. 1

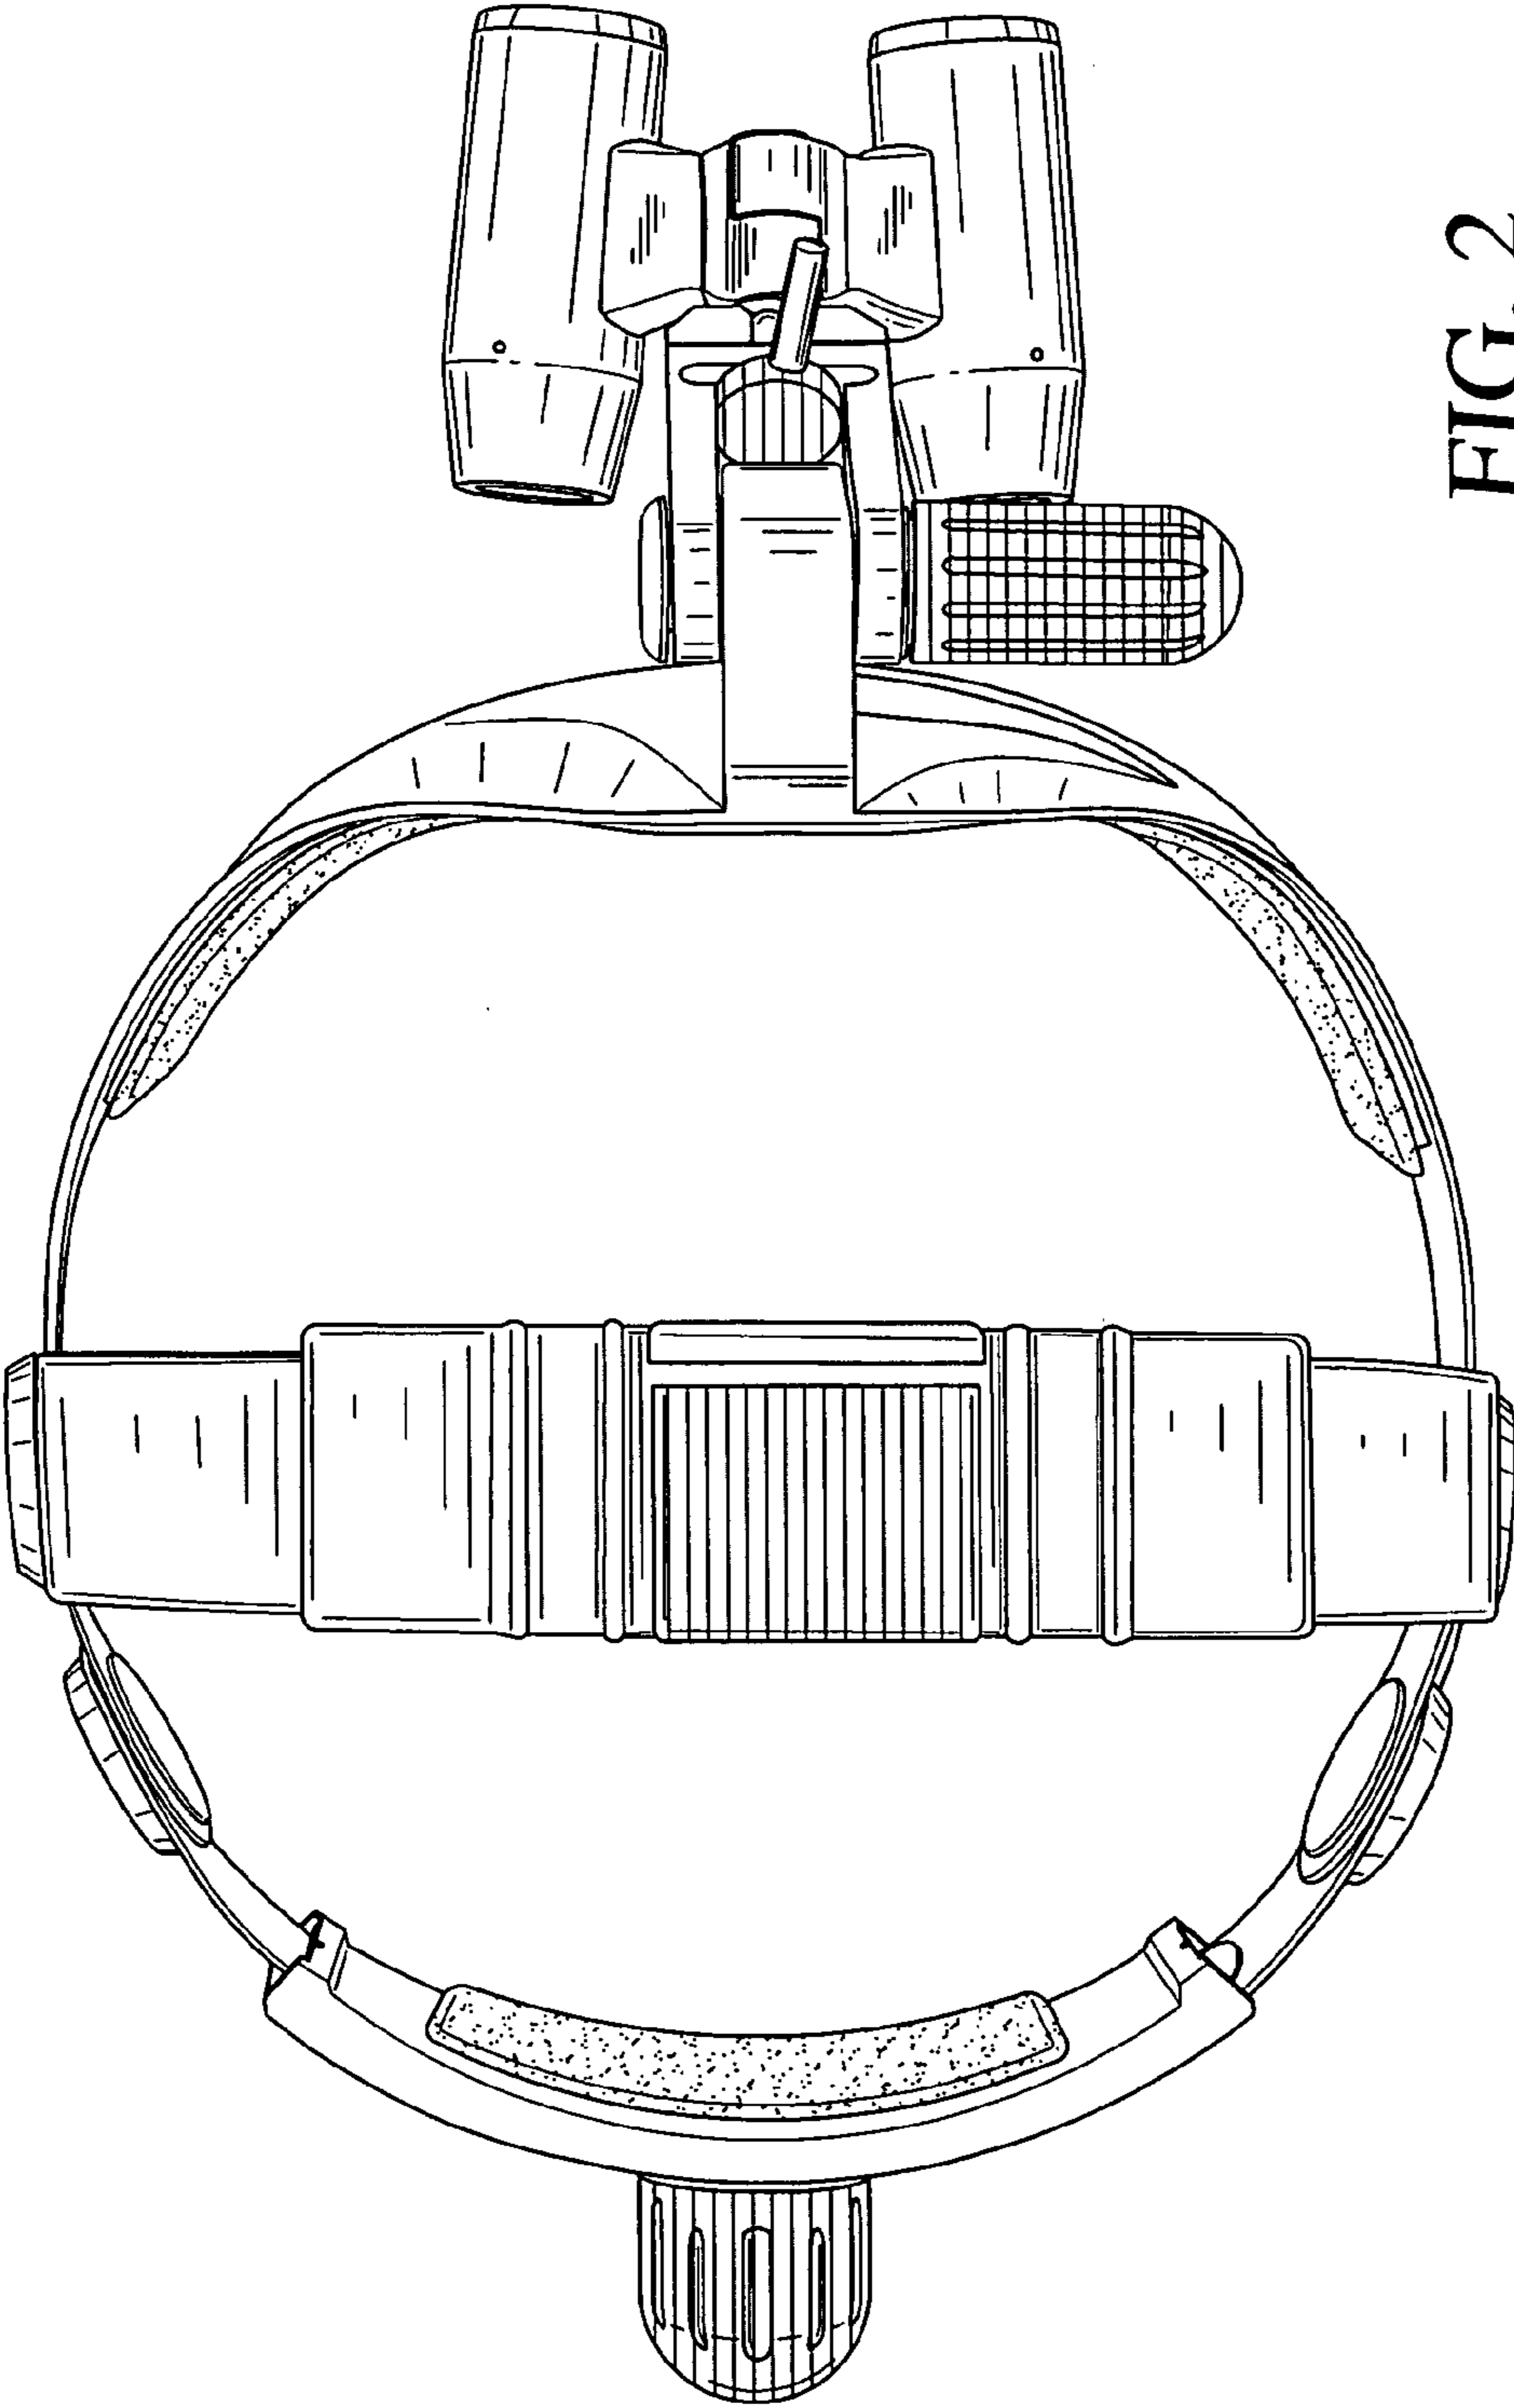


FIG. 2

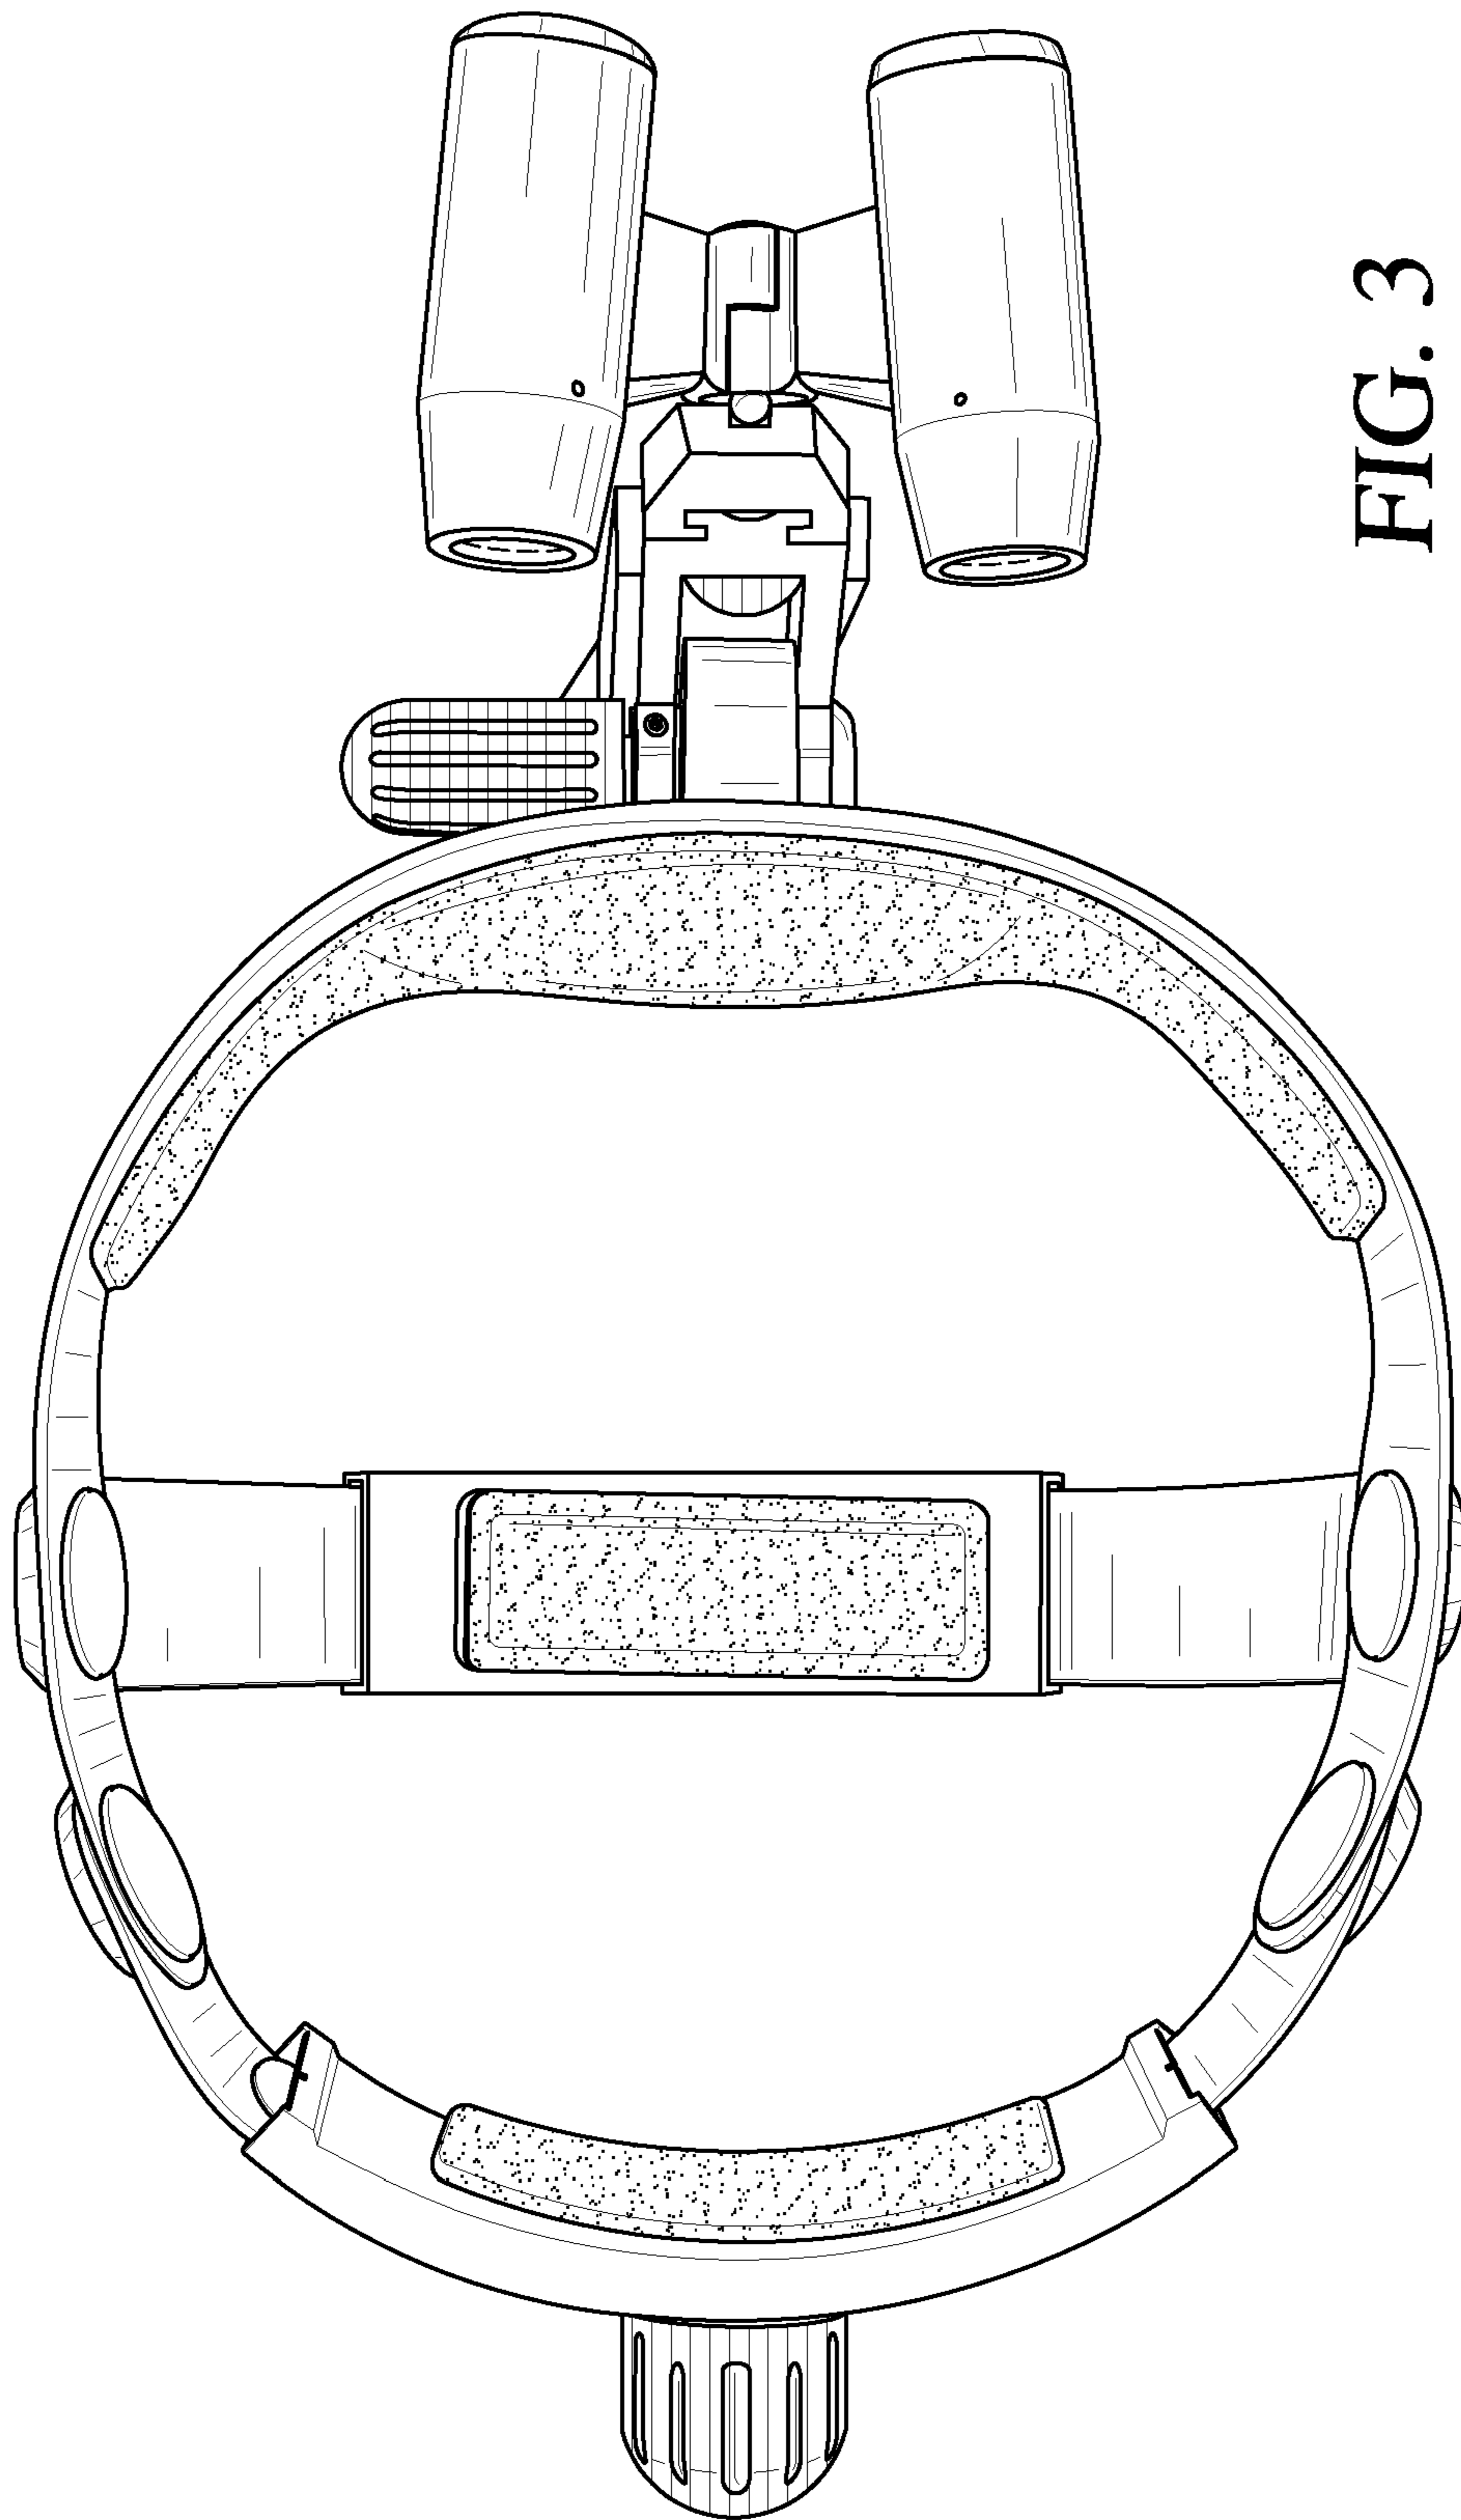


FIG. 3

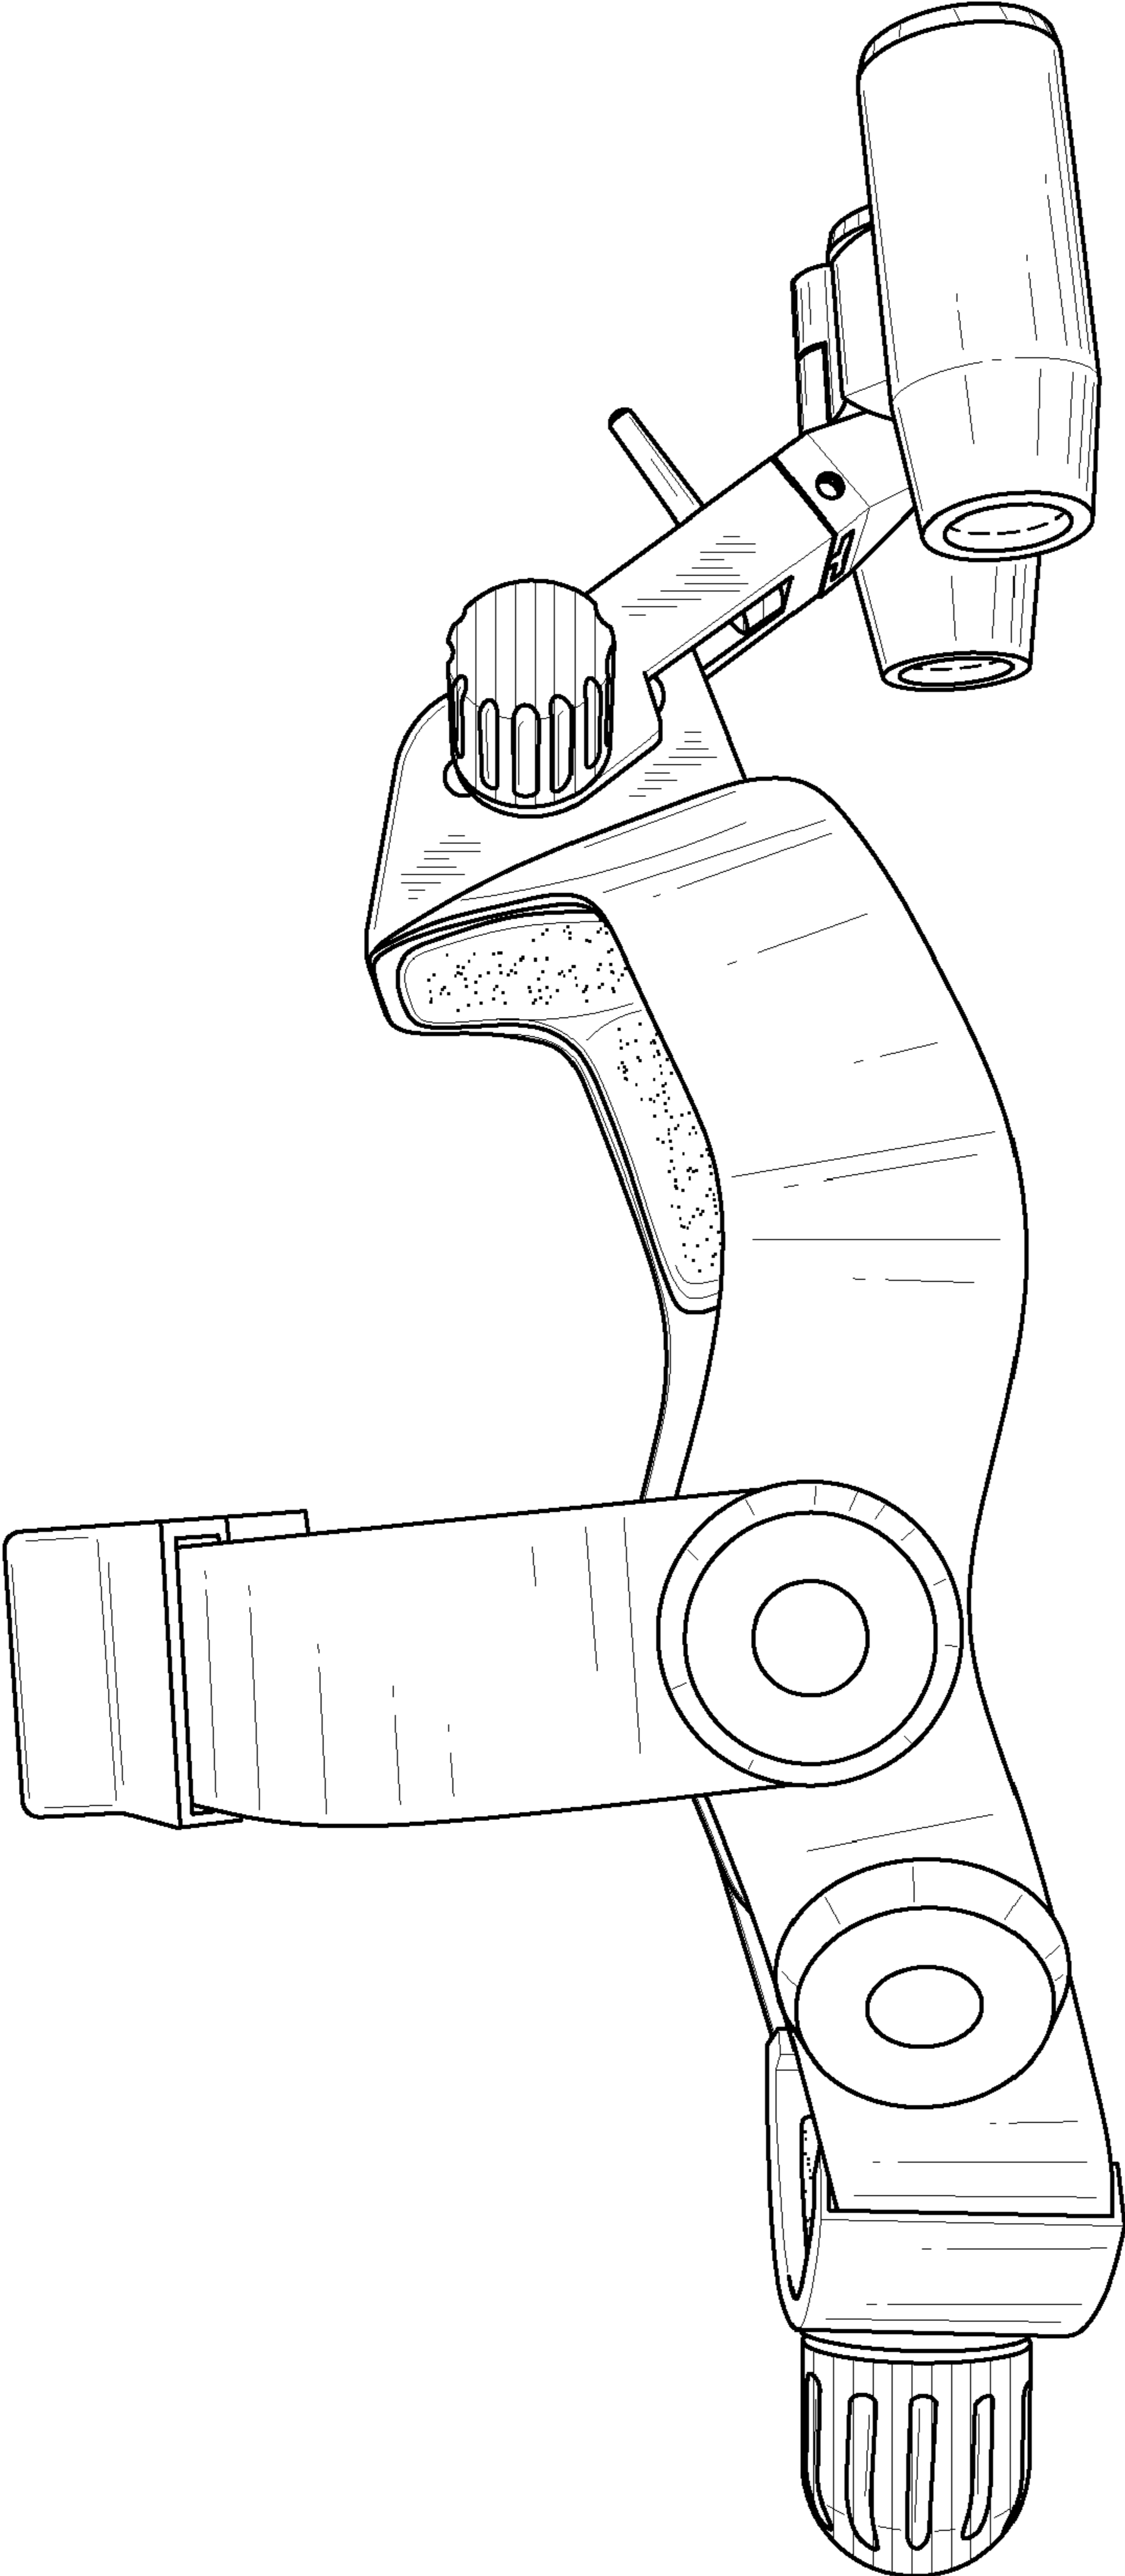


FIG. 4

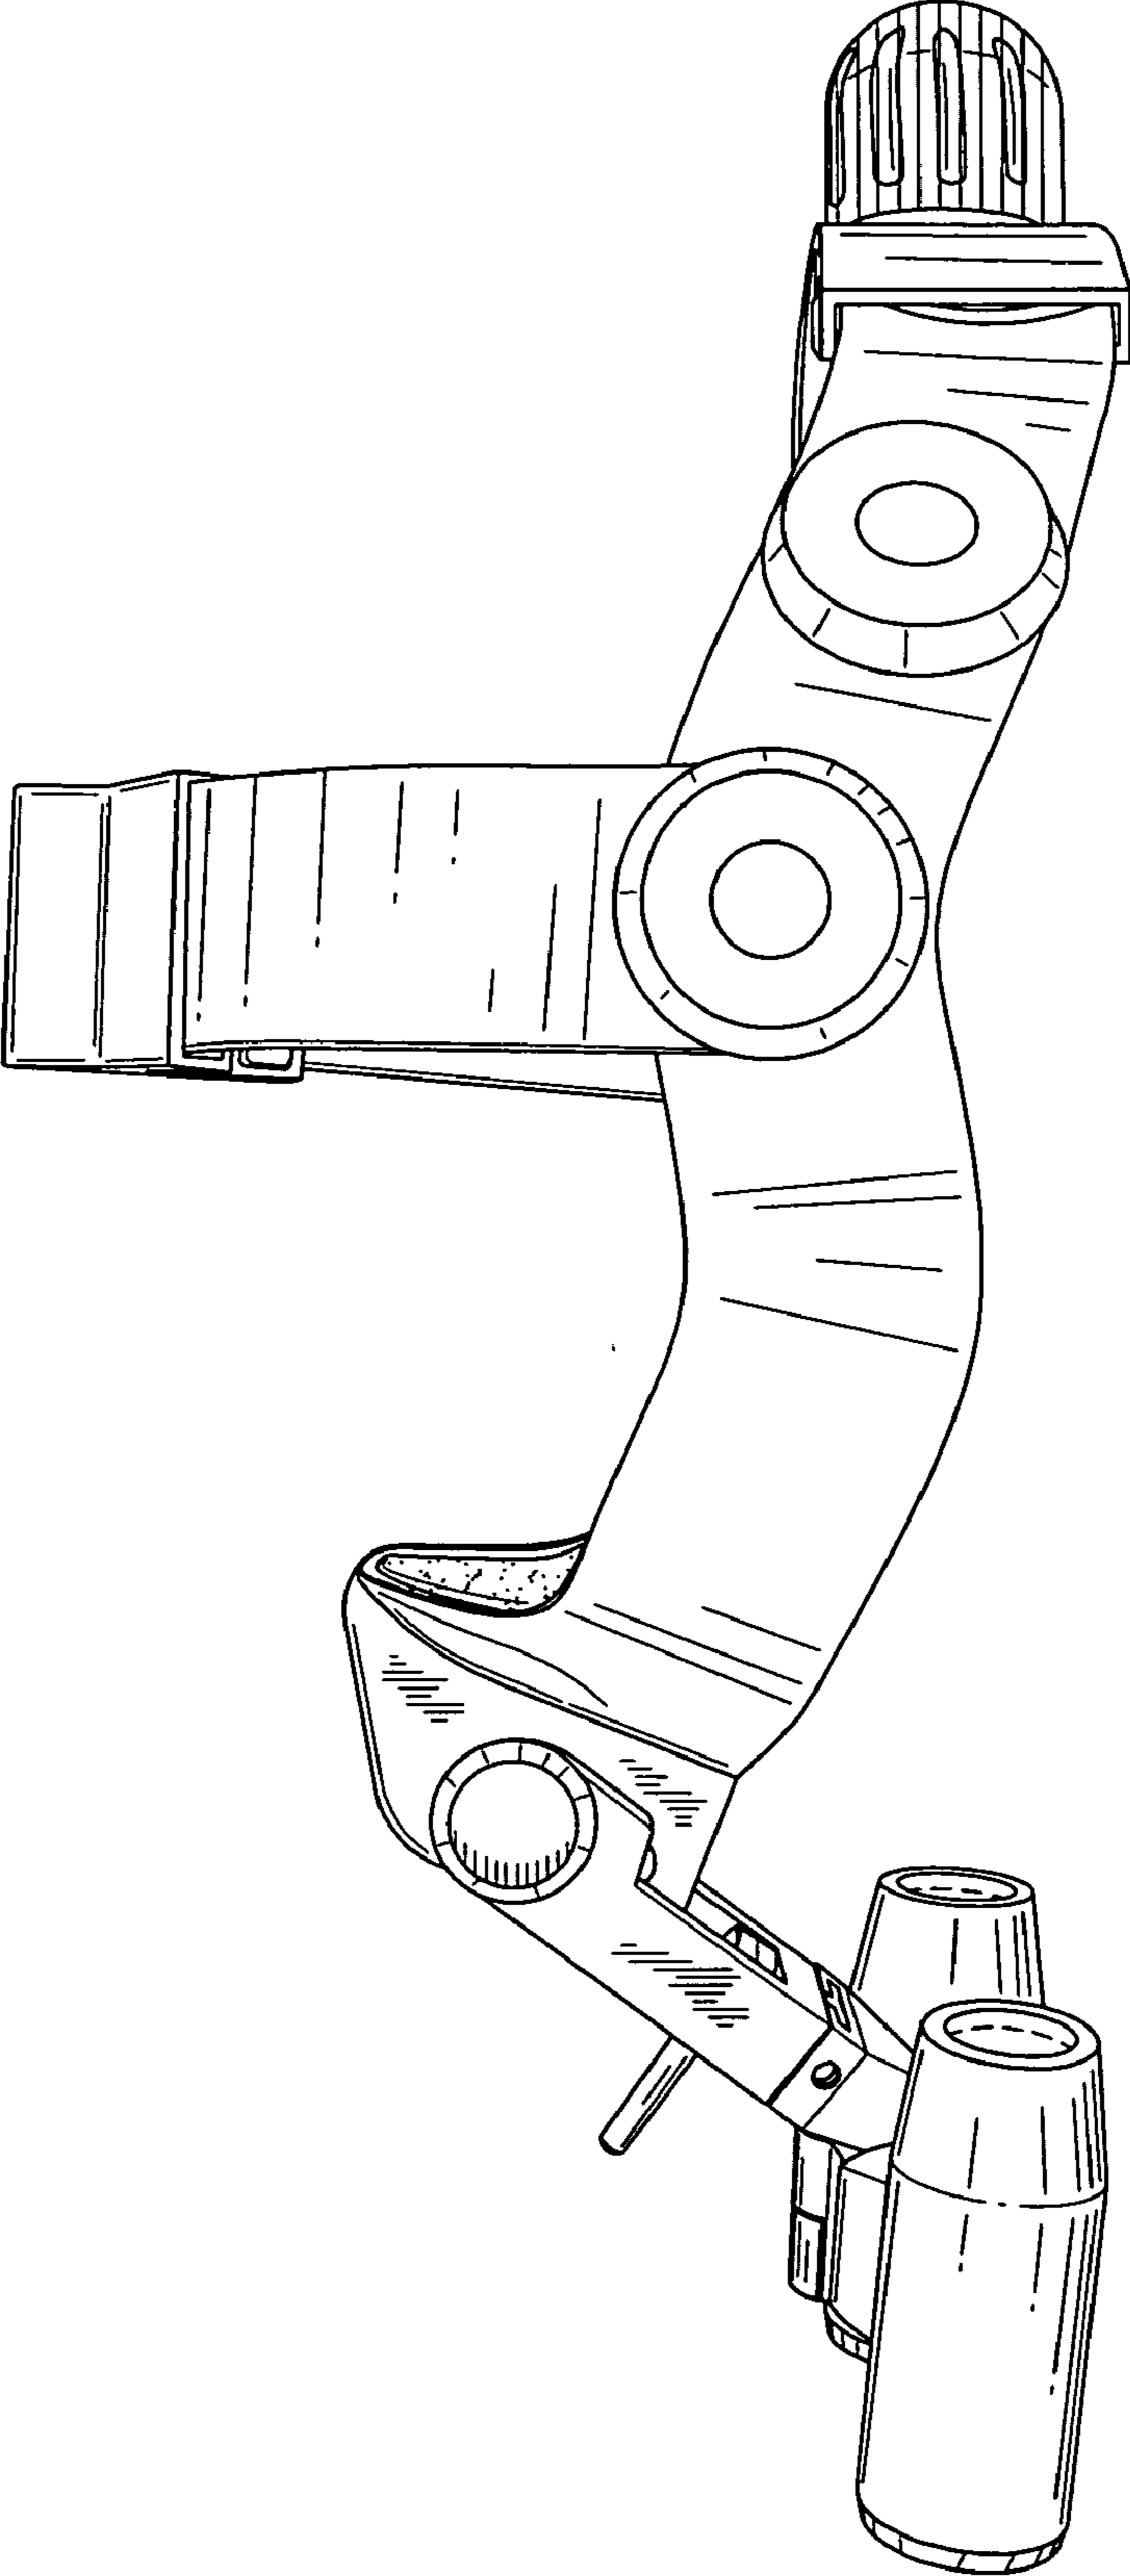


FIG. 5

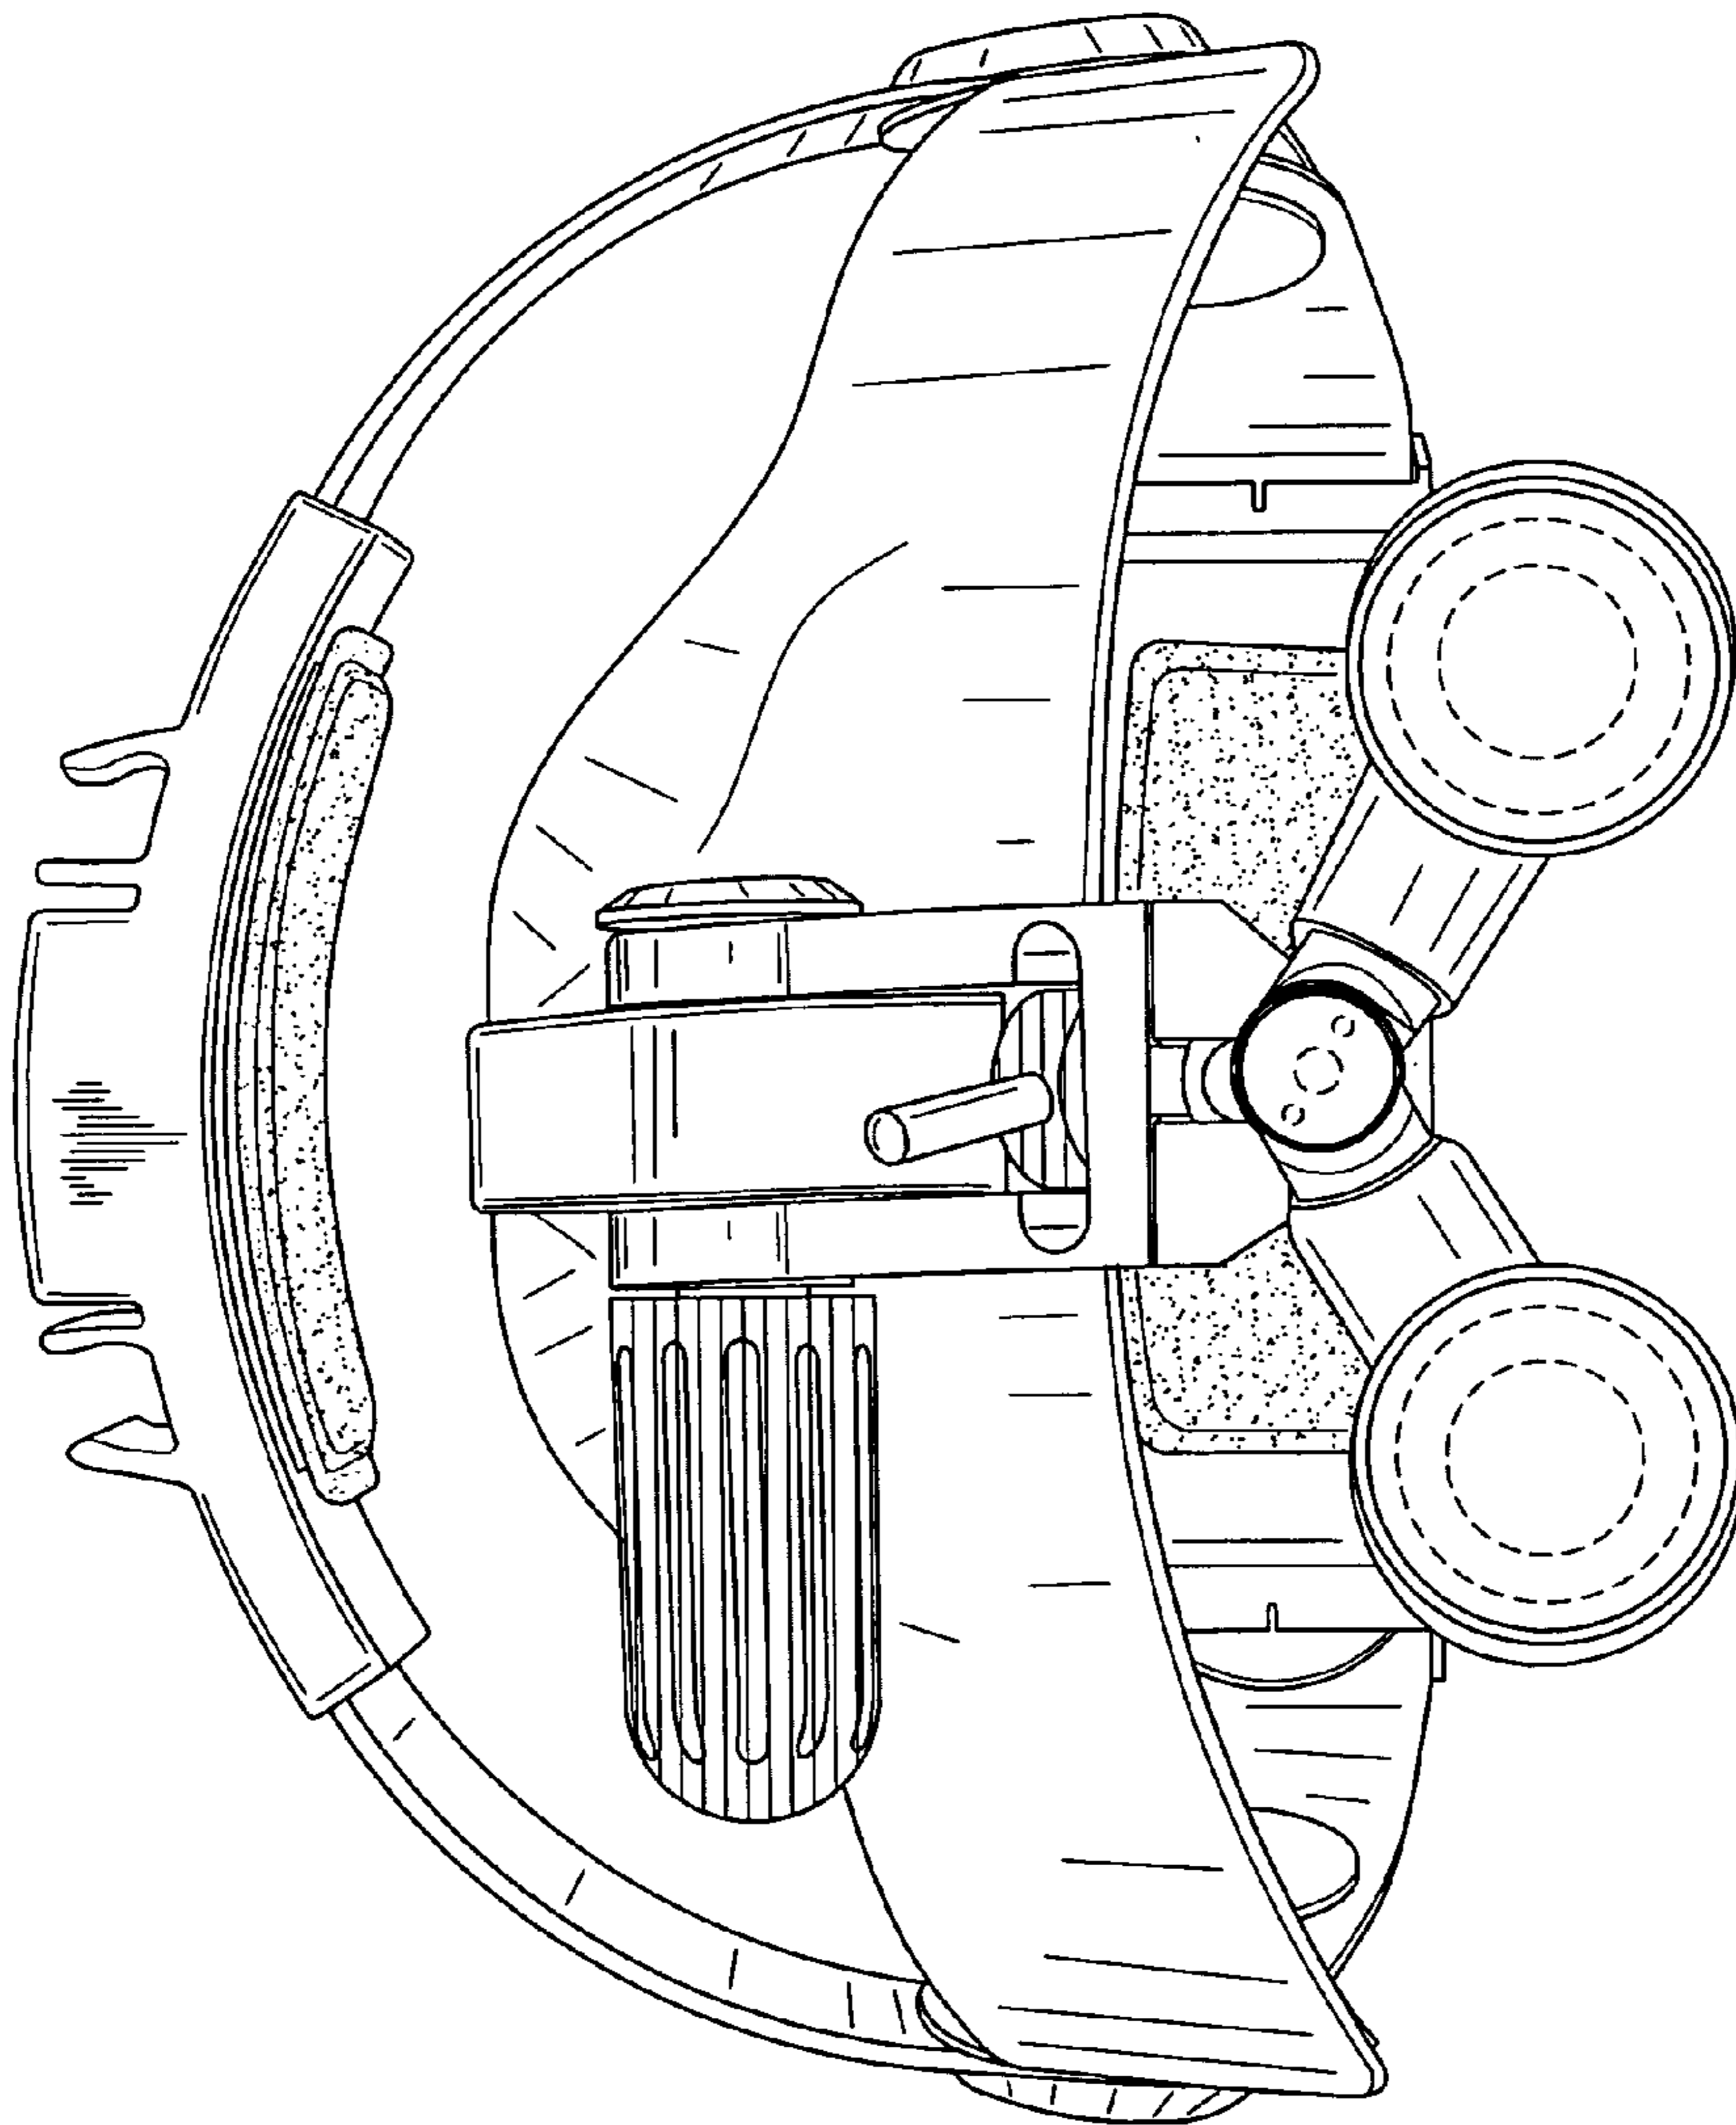


FIG. 6

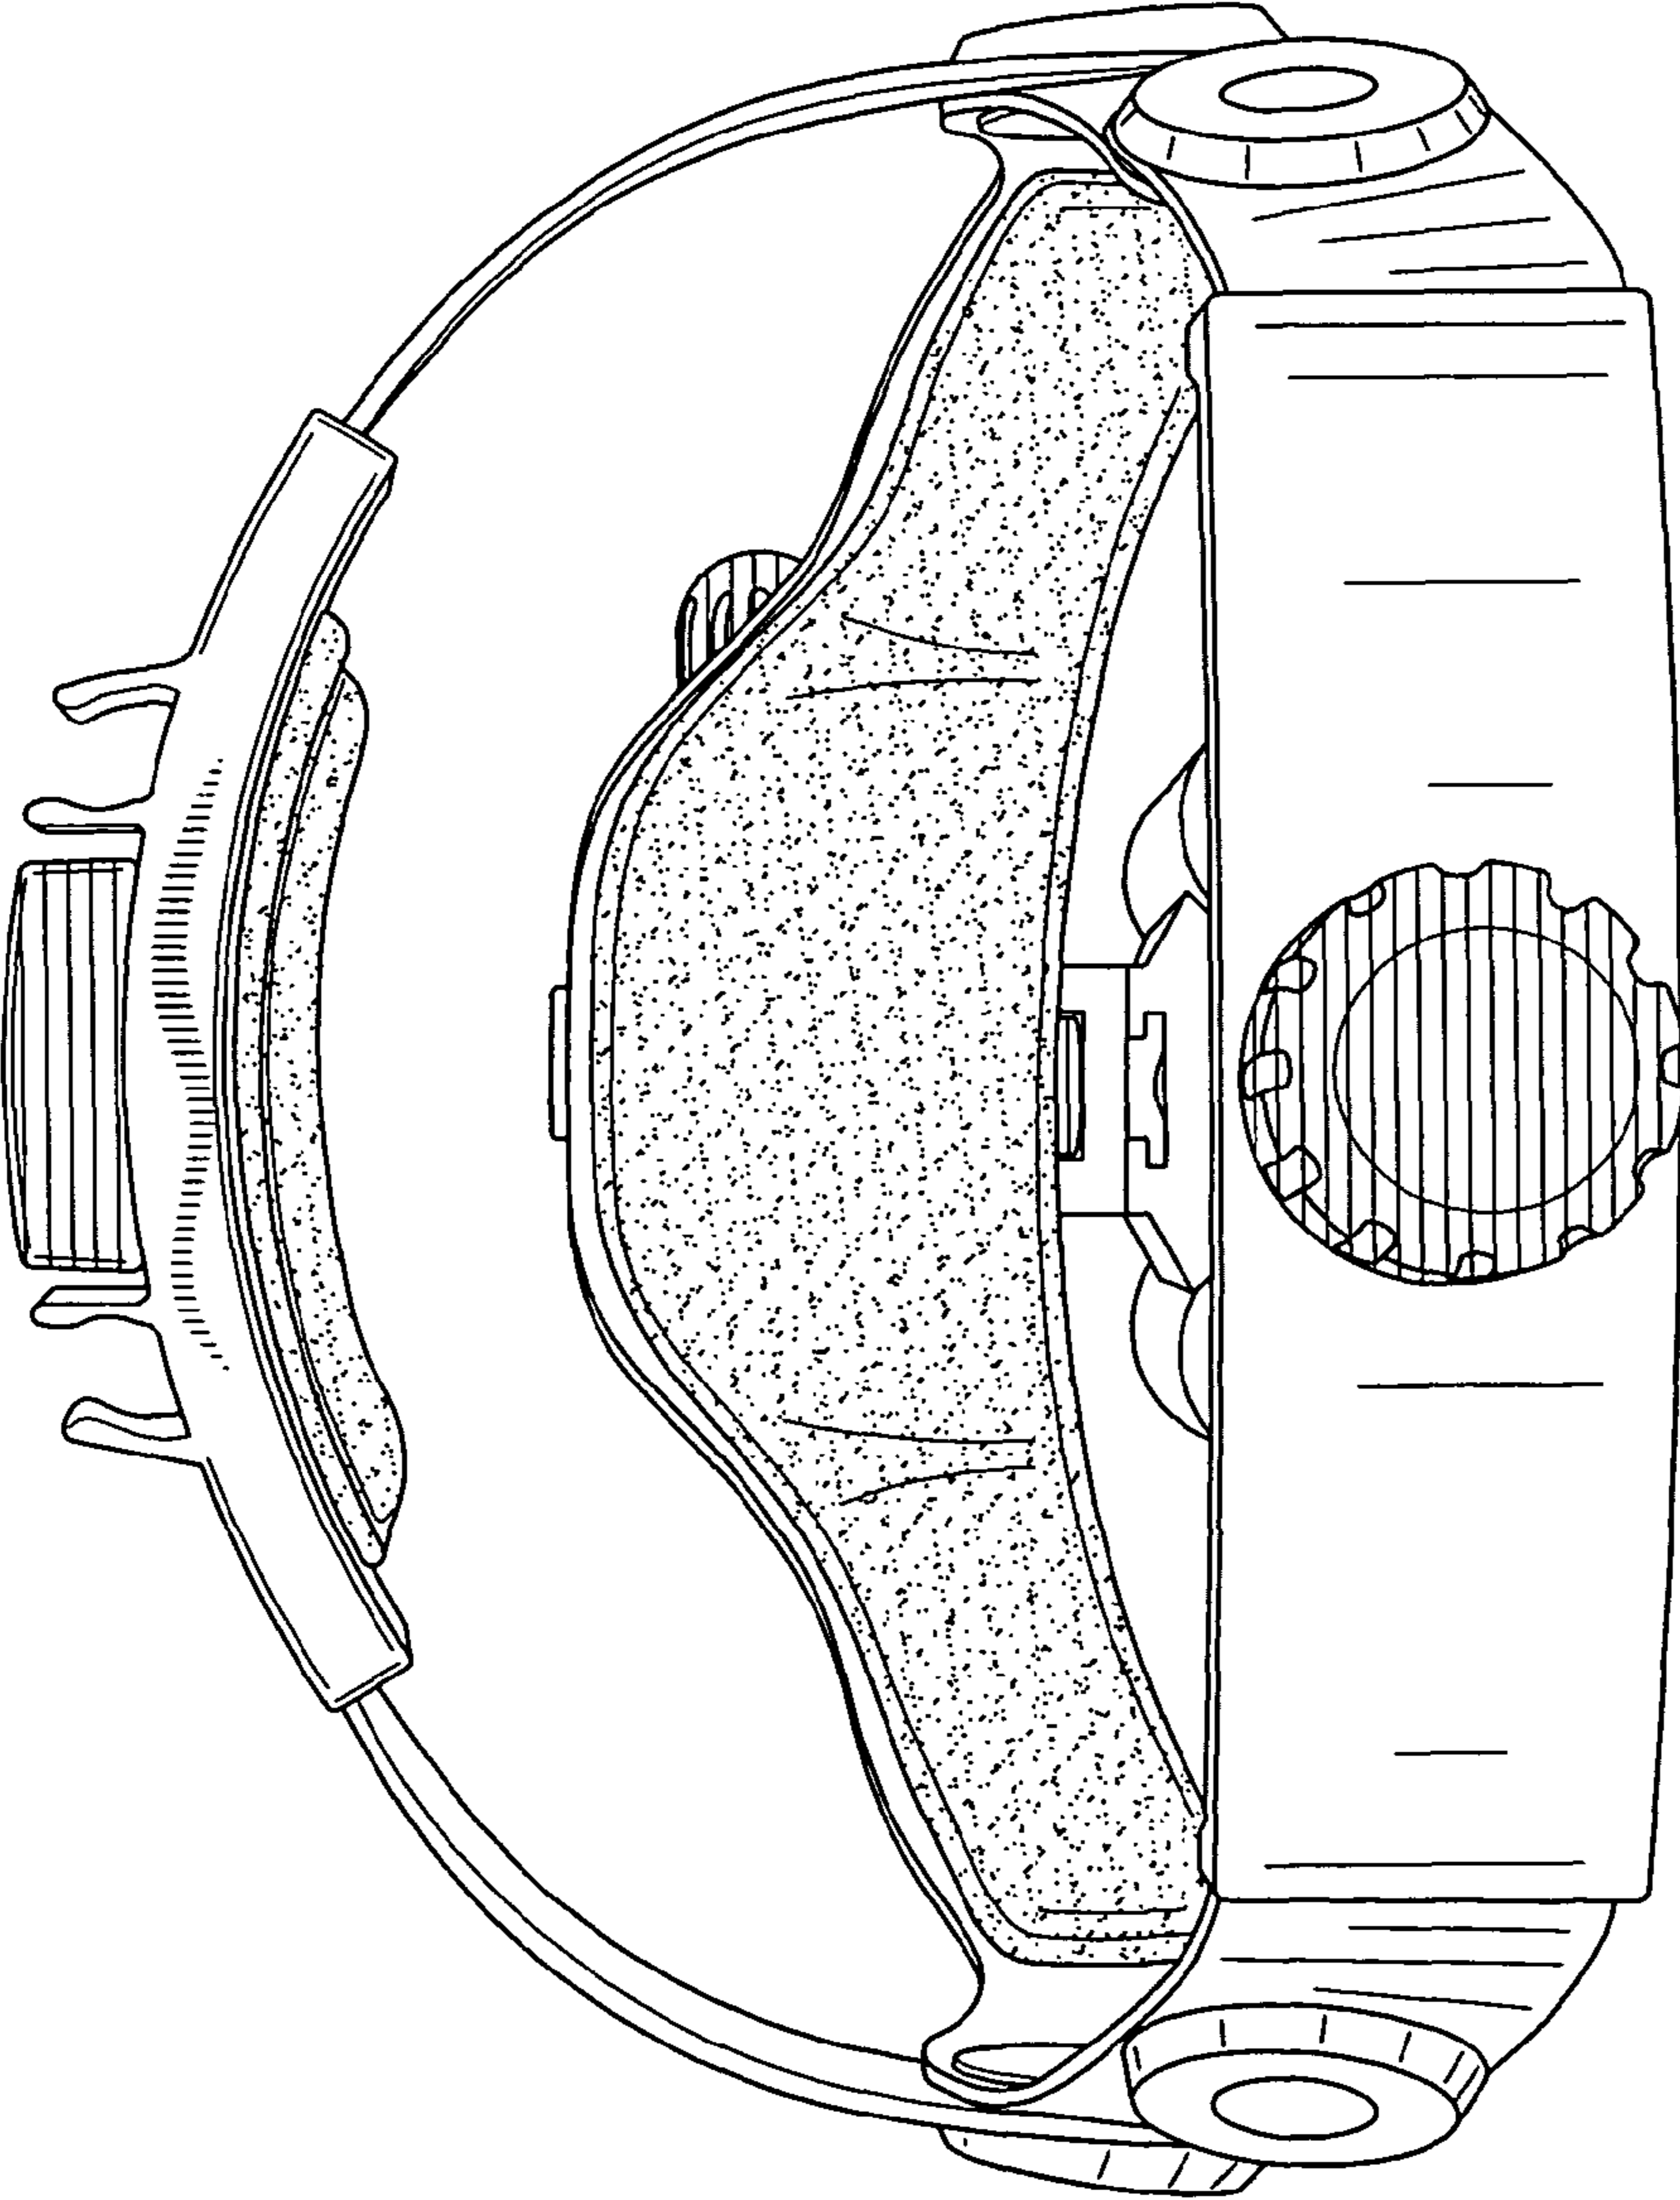


FIG. 7