



US00D628395S

(12) **United States Design Patent**
Henry

(10) **Patent No.:** **US D628,395 S**
(45) **Date of Patent:** **** Dec. 7, 2010**

(54) **MEDICAL CERTIFICATE DISPLAY MAT**

(76) Inventor: **Jeffrey J. Henry**, 337 Oakwood Dr.,
Geneva, IL (US) 60134

(**) Term: **14 Years**

(21) Appl. No.: **29/315,446**

(22) Filed: **Jun. 26, 2009**

(51) **LOC (9) Cl.** **06-07**

(52) **U.S. Cl.** **D6/302**

(58) **Field of Classification Search** D6/300–304,
D6/308–314; D20/10, 40; 40/700, 711,
40/718, 729–730, 735, 744, 745, 765, 768–770,
40/780, 790, 798; D11/132

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D385,708 S *	11/1997	Key et al.		D6/302
6,119,386 A	9/2000	Henry et al.		
D431,909 S	10/2000	Henry et al.		
D437,121 S	2/2001	Henry et al.		
D438,019 S *	2/2001	Carlson		D6/302
D438,020 S *	2/2001	Carlson		D6/302
D439,223 S *	3/2001	Sheckler		D14/125
6,536,149 B1 *	3/2003	Phillips		40/768
D502,005 S	2/2005	Henry		
D540,547 S *	4/2007	Barnhorn		D6/303

* cited by examiner

Primary Examiner—Philip S Hyder

Assistant Examiner—Sydney R Buffalow

(74) *Attorney, Agent, or Firm*—Meroni & Meroni, P.C.;
Charles F. Meroni, Jr.; Christopher J. Scott

(57) **CLAIM**

The ornamental design for a medical certificate display mat,
as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of my medical certificate display
mat showing my new design;

FIG. 2 is a rear view thereof of my medical certificate display
mat;

FIG. 3 is a bottom end view of my medical certificate display
mat;

FIG. 4 is a top end view of my medical certificate display mat;


FIG. 5 is a left side view of my medical certificate display mat

FIG. 6 is a right side view of my medical certificate display
mat; and,

FIG. 7 is another perspective view of my medical certificate
display mat showing my new design similar to FIG. 1 only
with the dash lines at the edges of the mat illustrating the
location of a frame and the dash lines over mat windows
indicating glass reflections when assembled with the frame.

The broken lines at the edge of the medical certificate display
mat and over the mat windows in FIG. 7 illustrate a frame and
glass reflections which form no part of the claimed design.

1 Claim, 3 Drawing Sheets

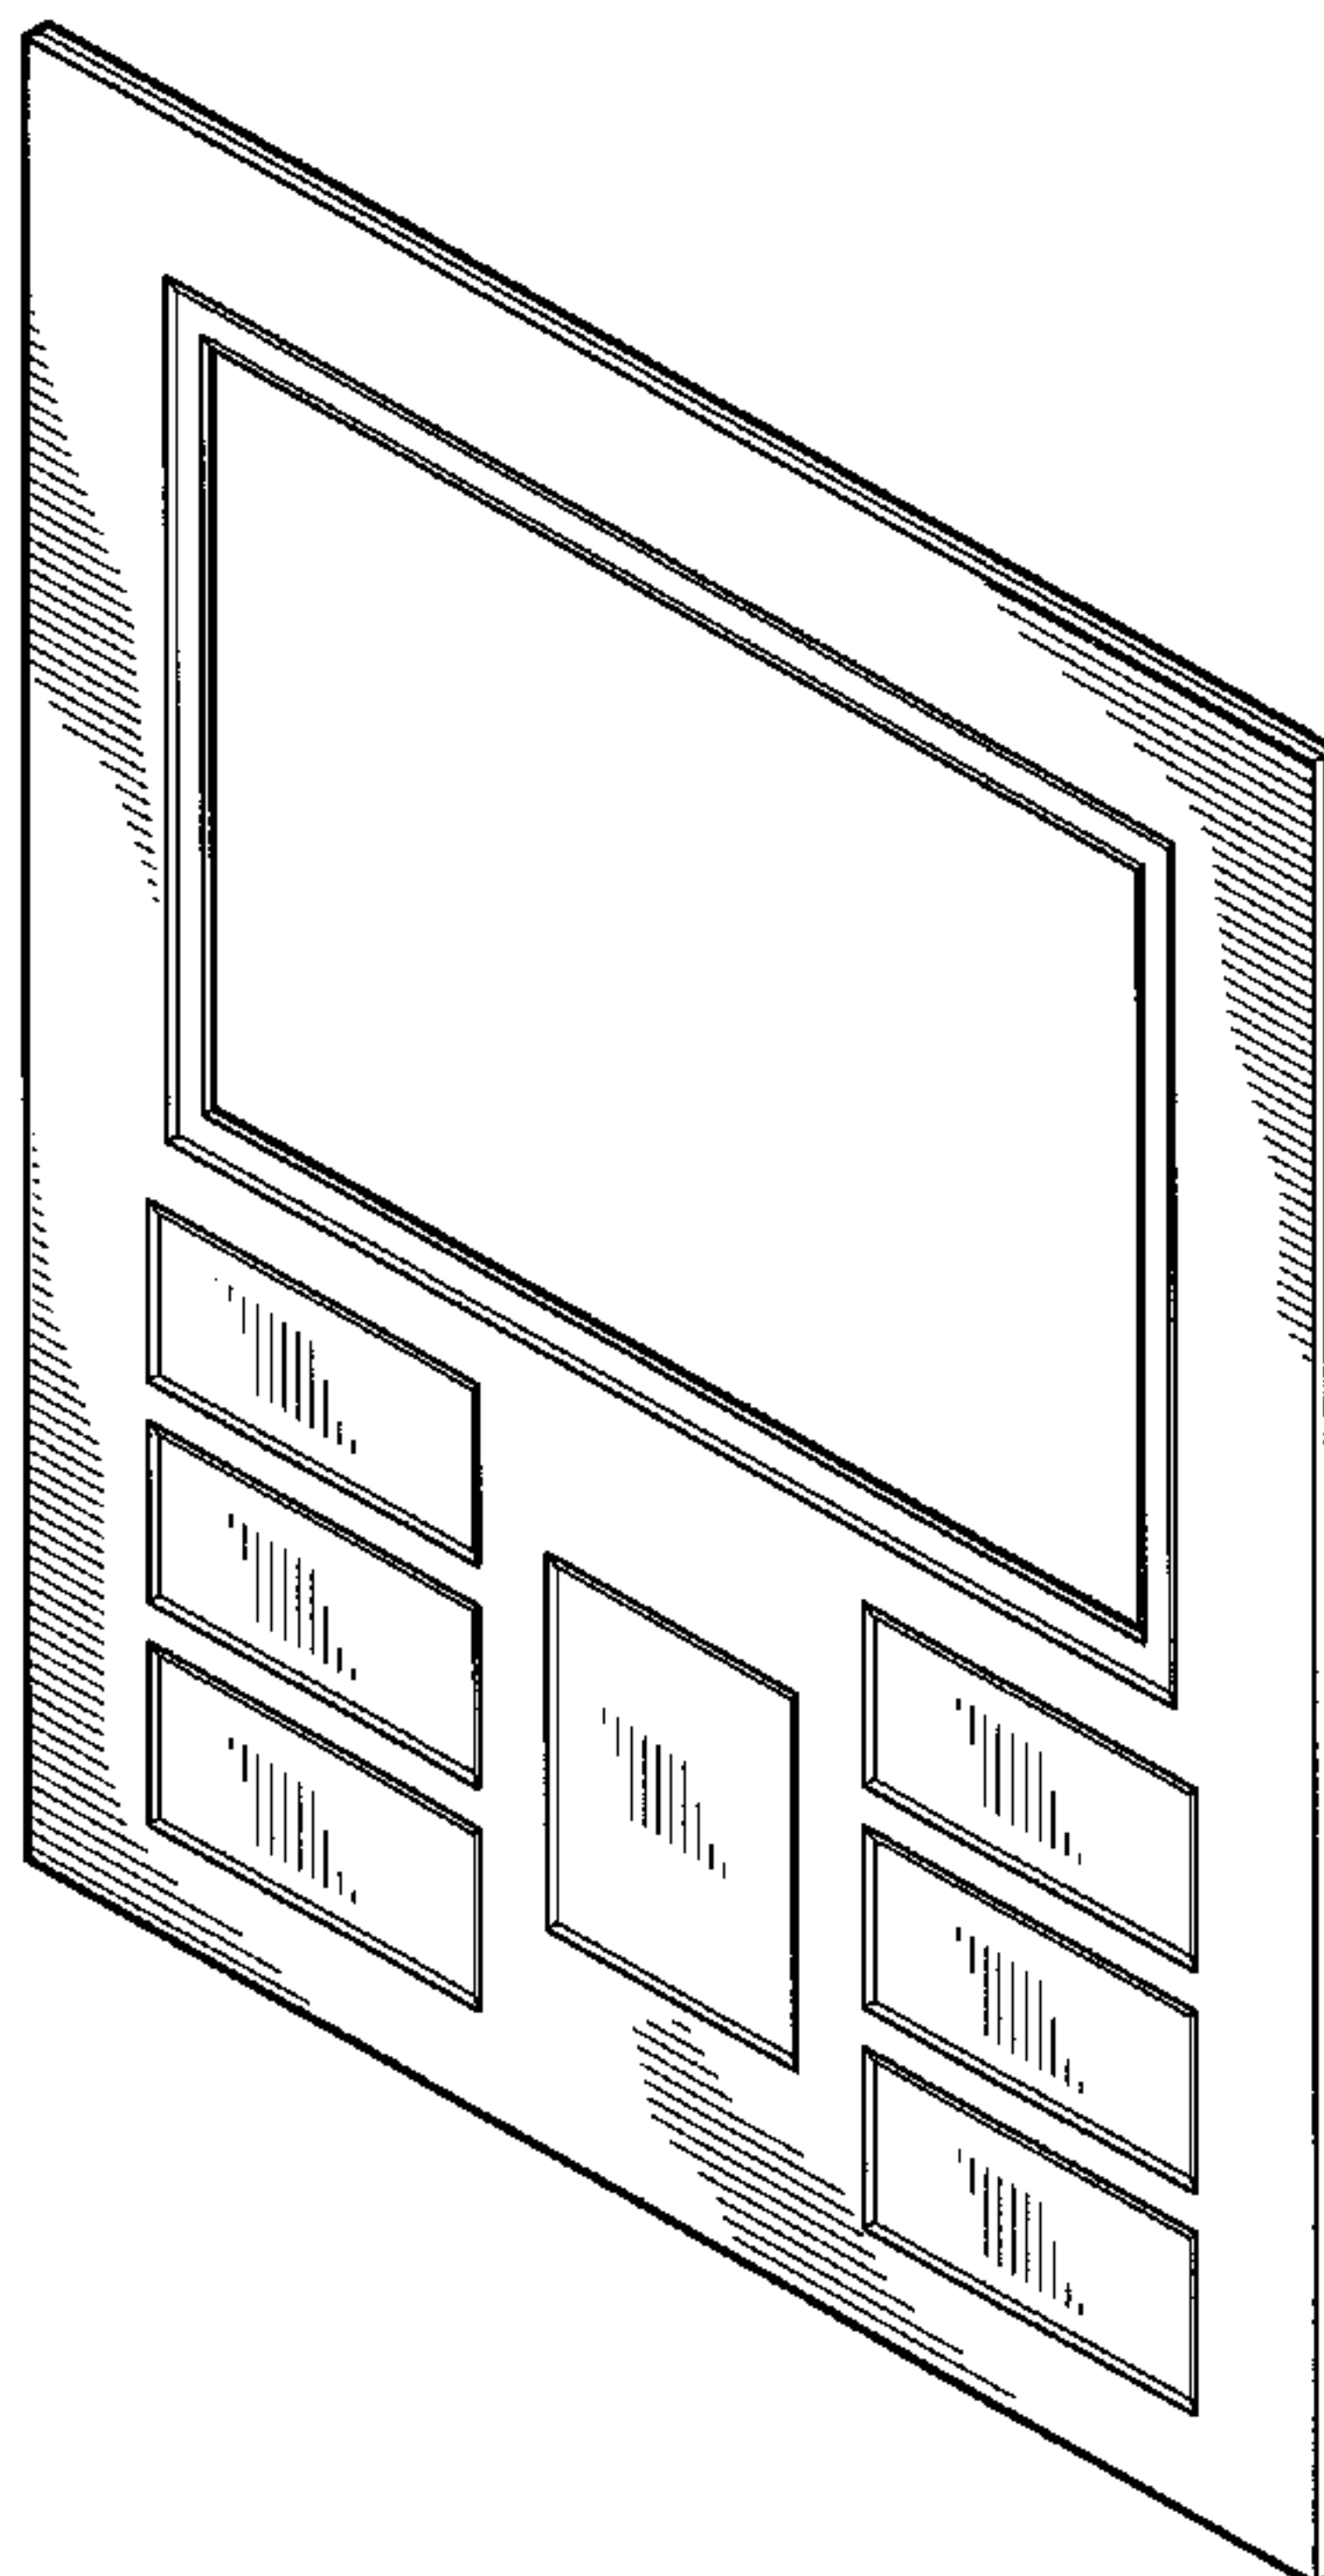

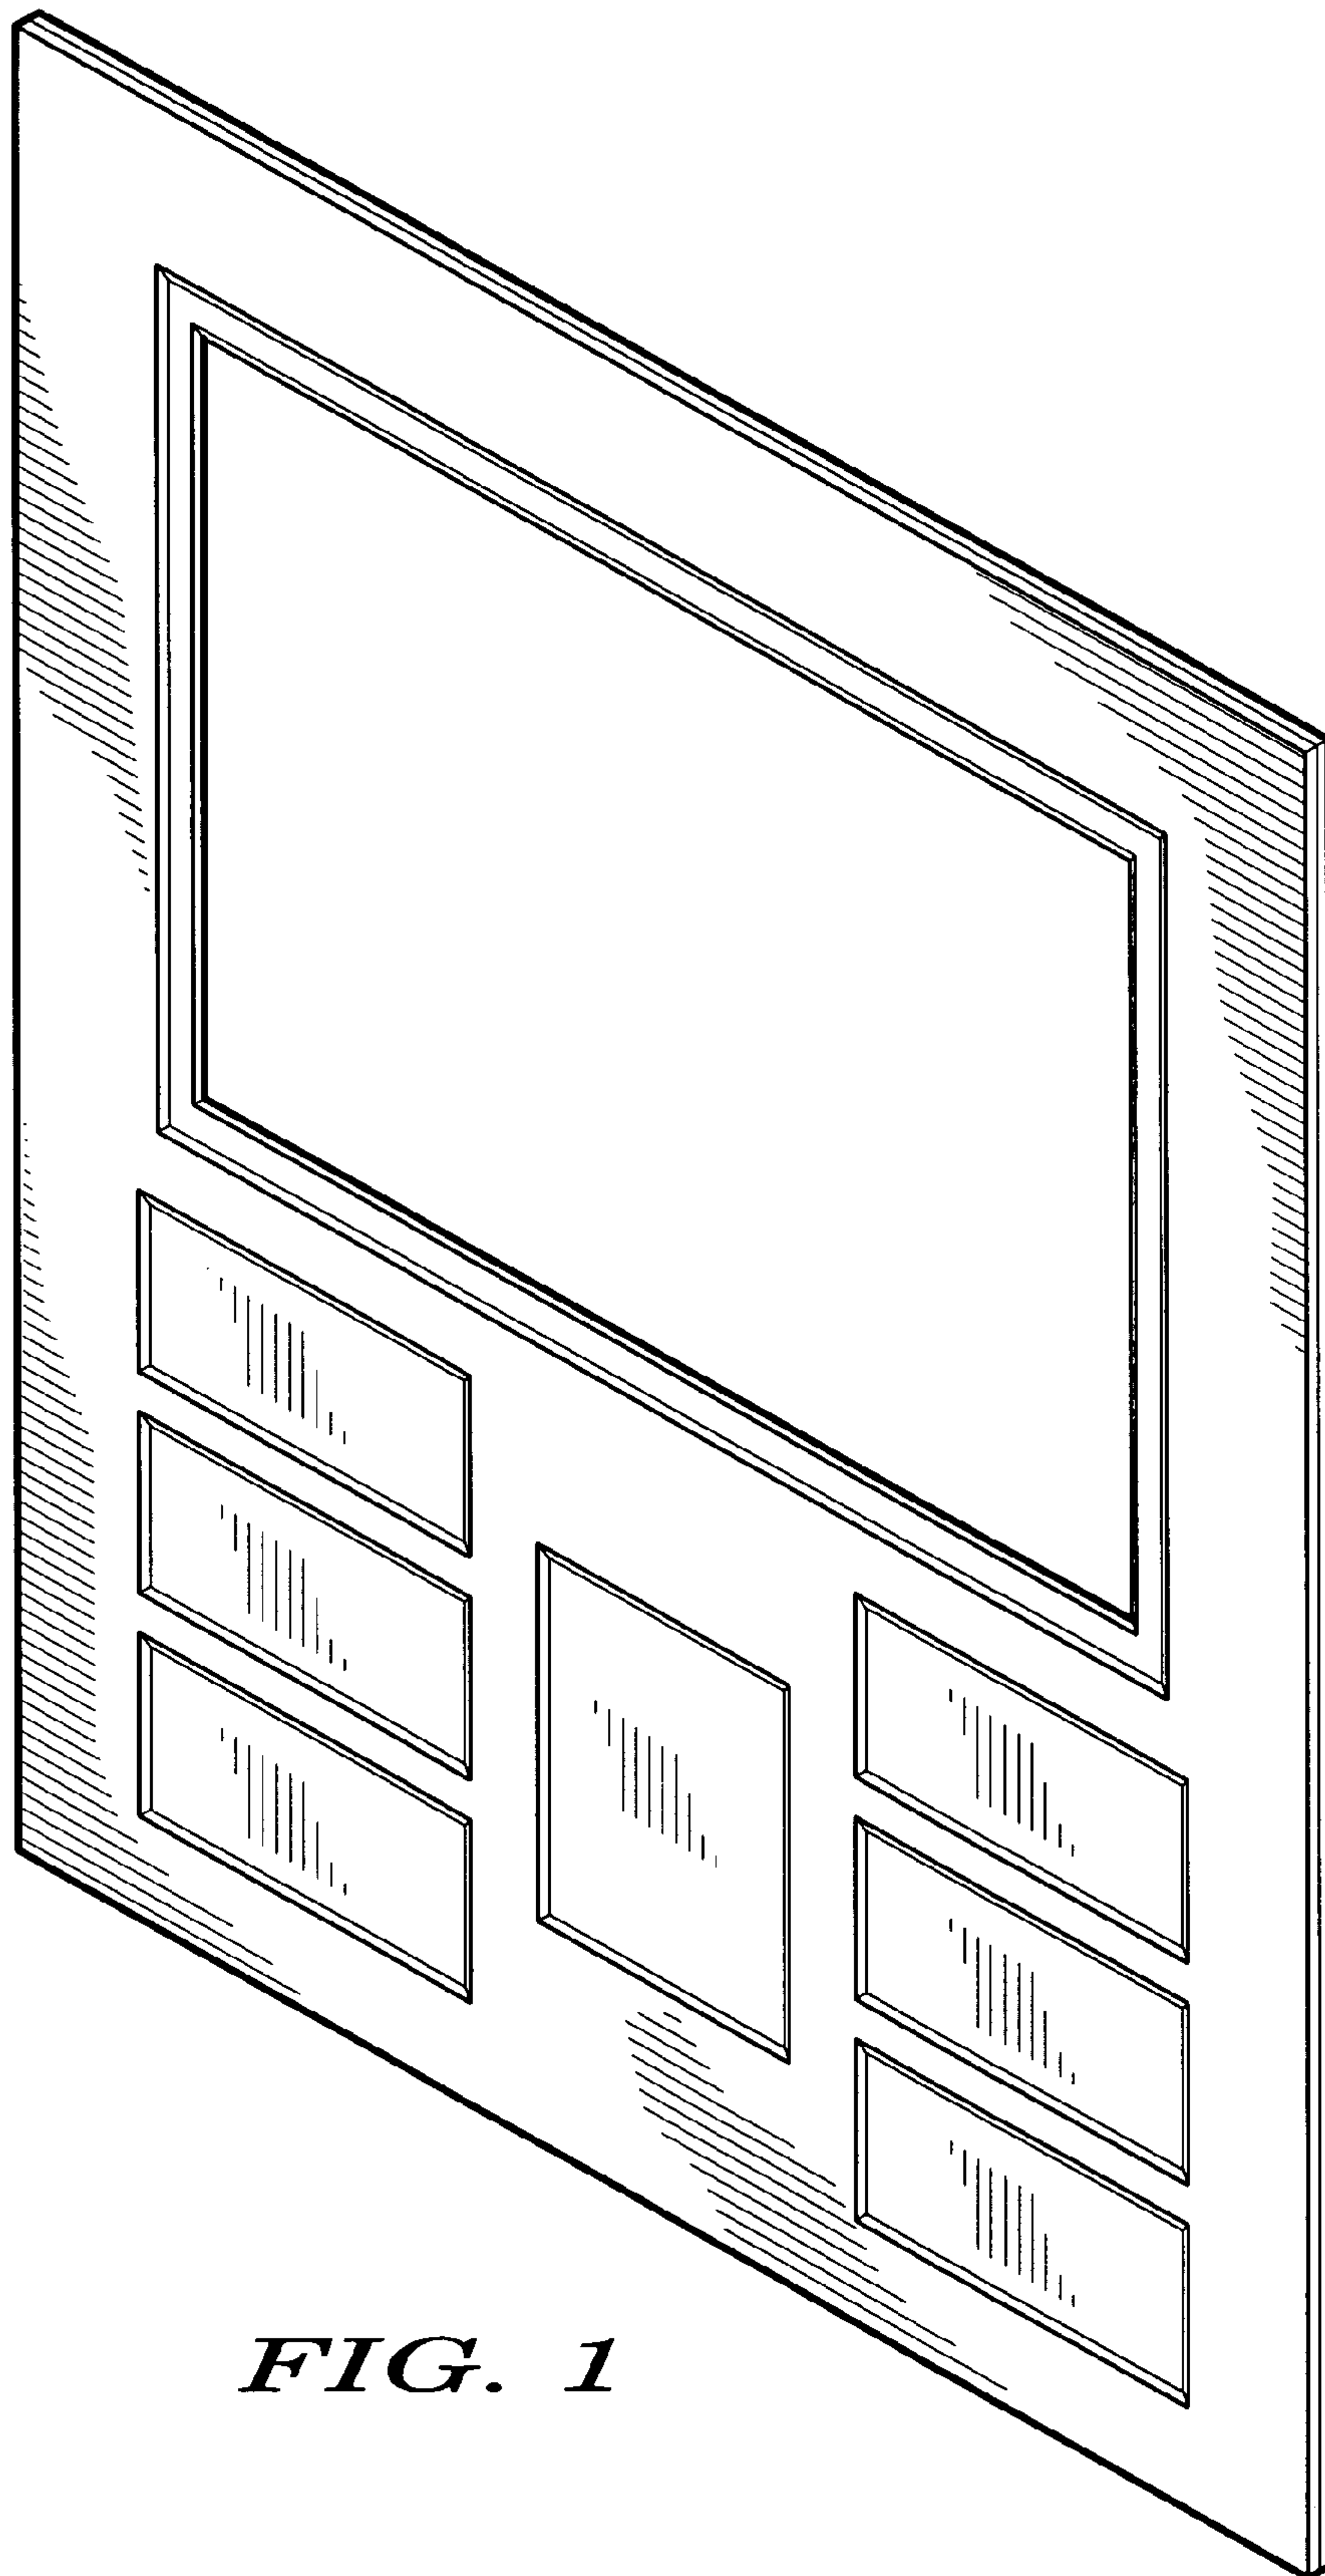


FIG. 1

FIG. 4




FIG. 5

FIG. 6

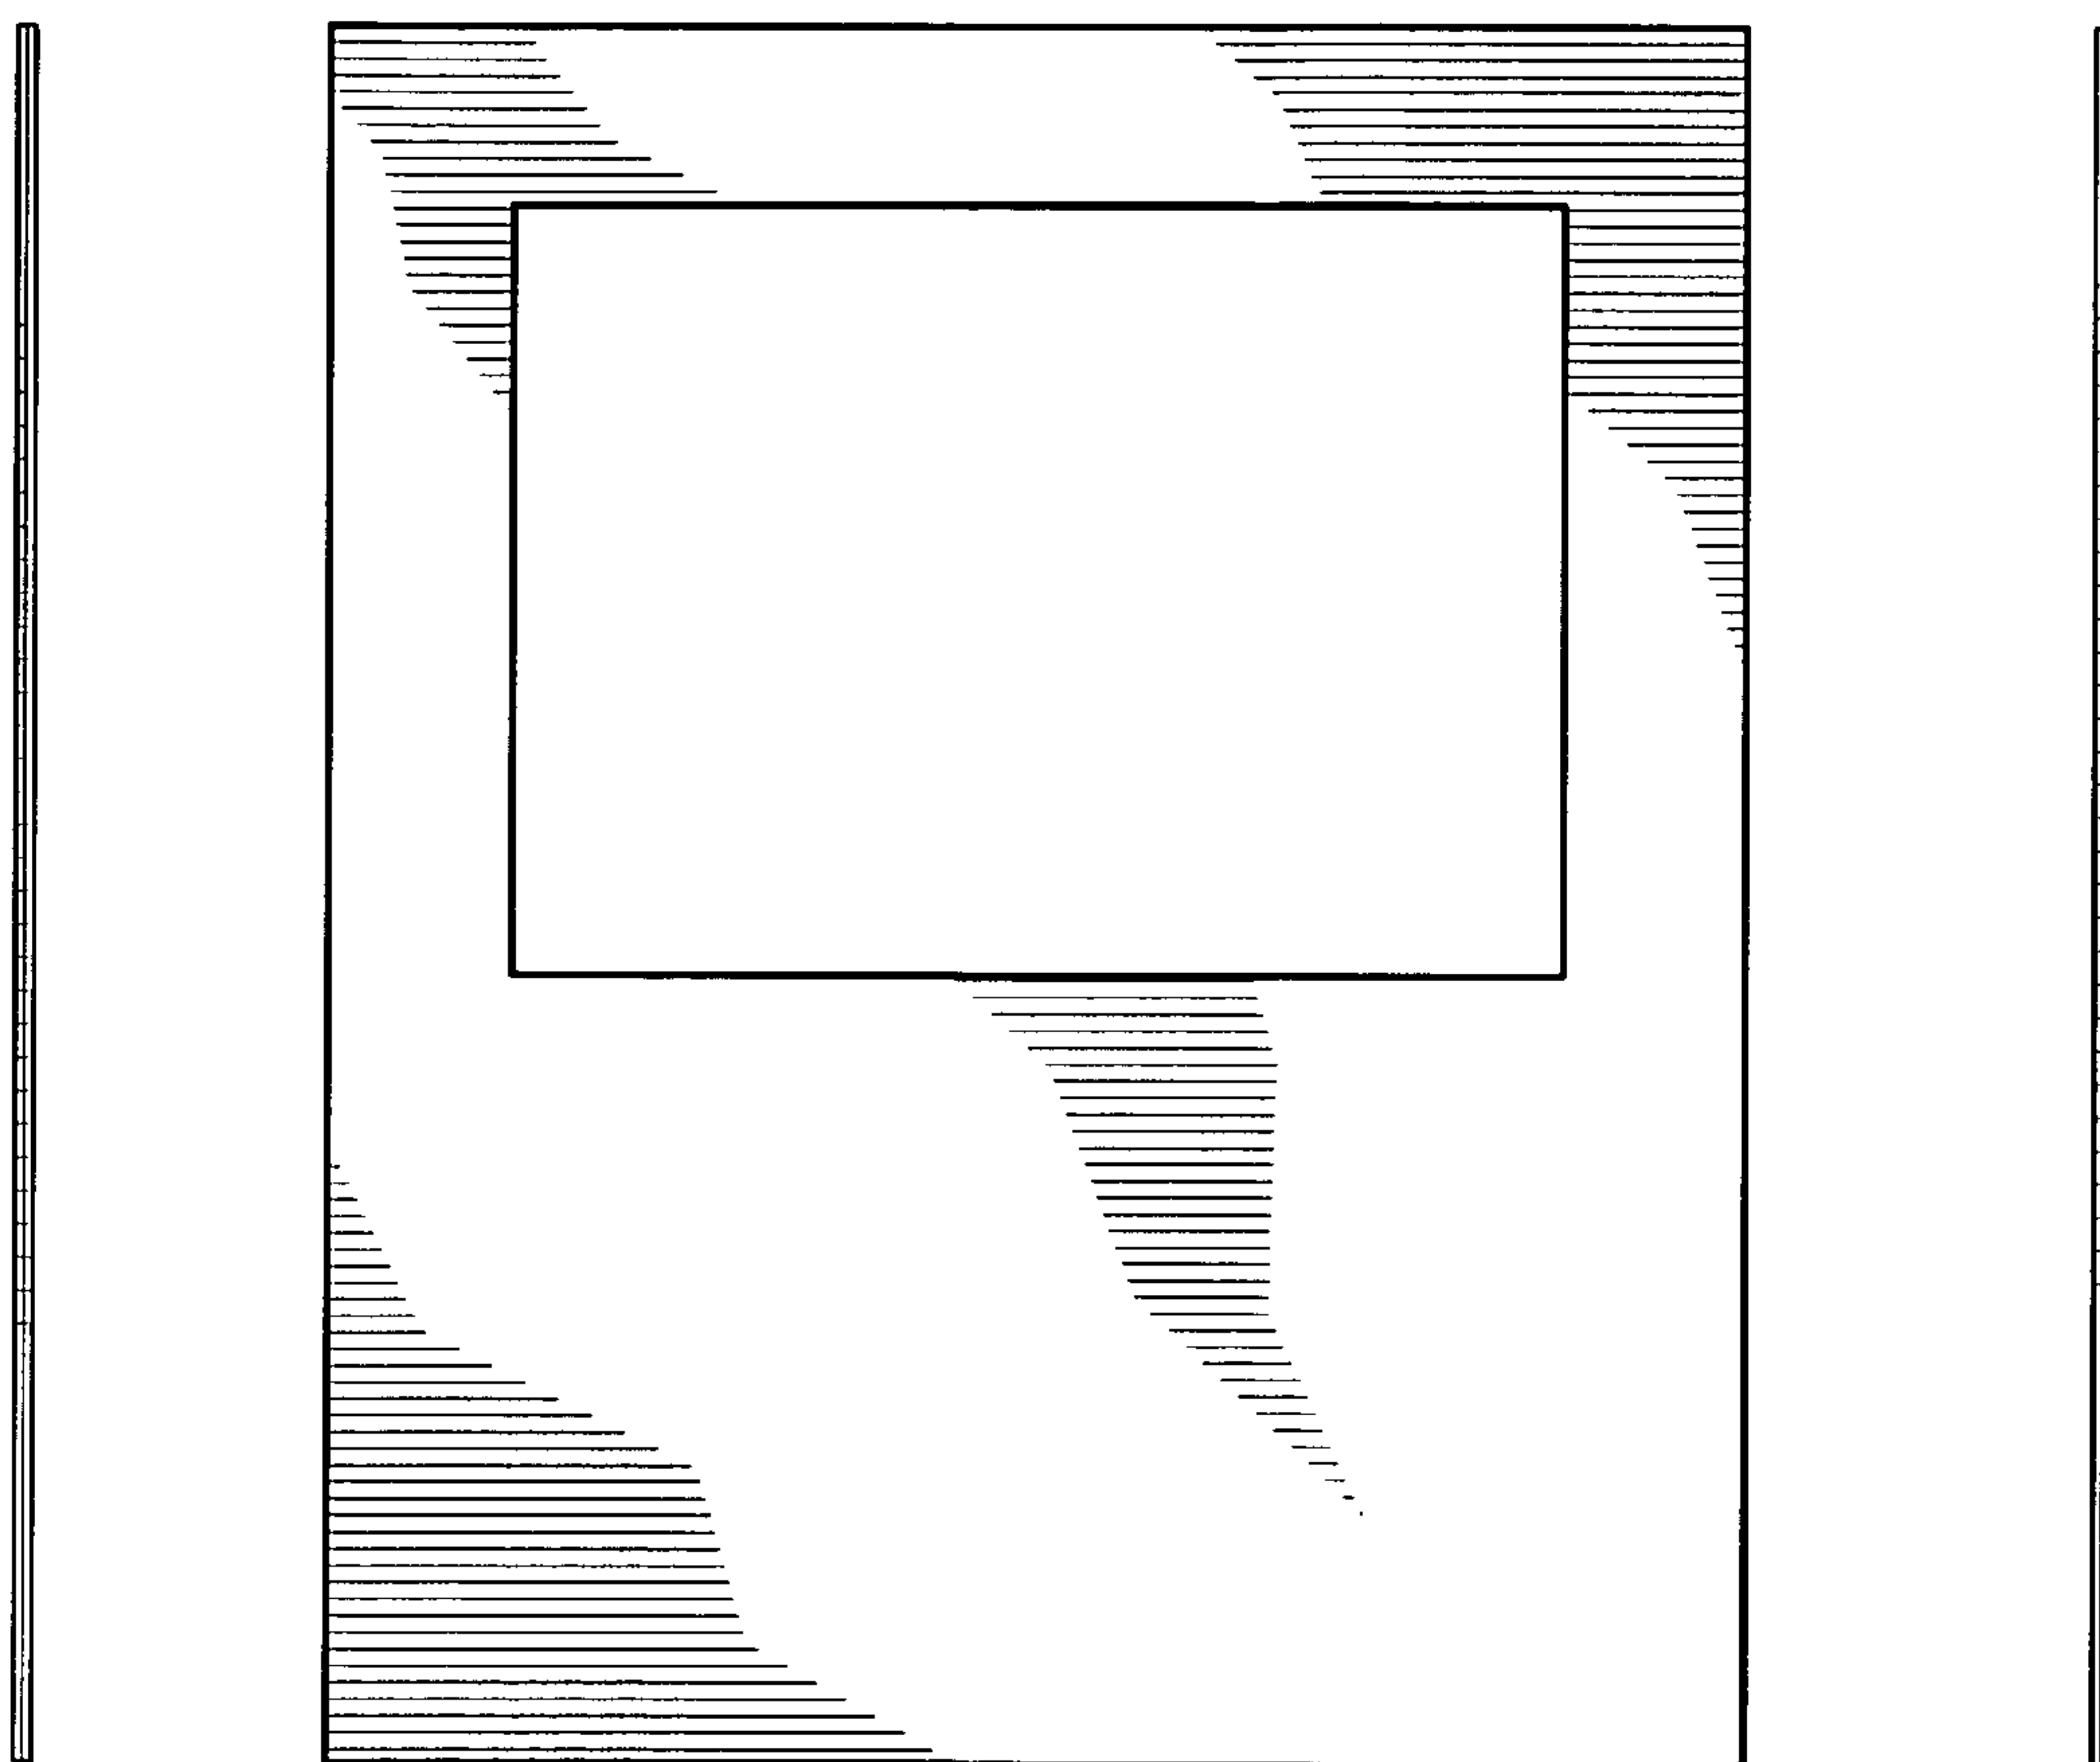


FIG. 2



FIG. 3

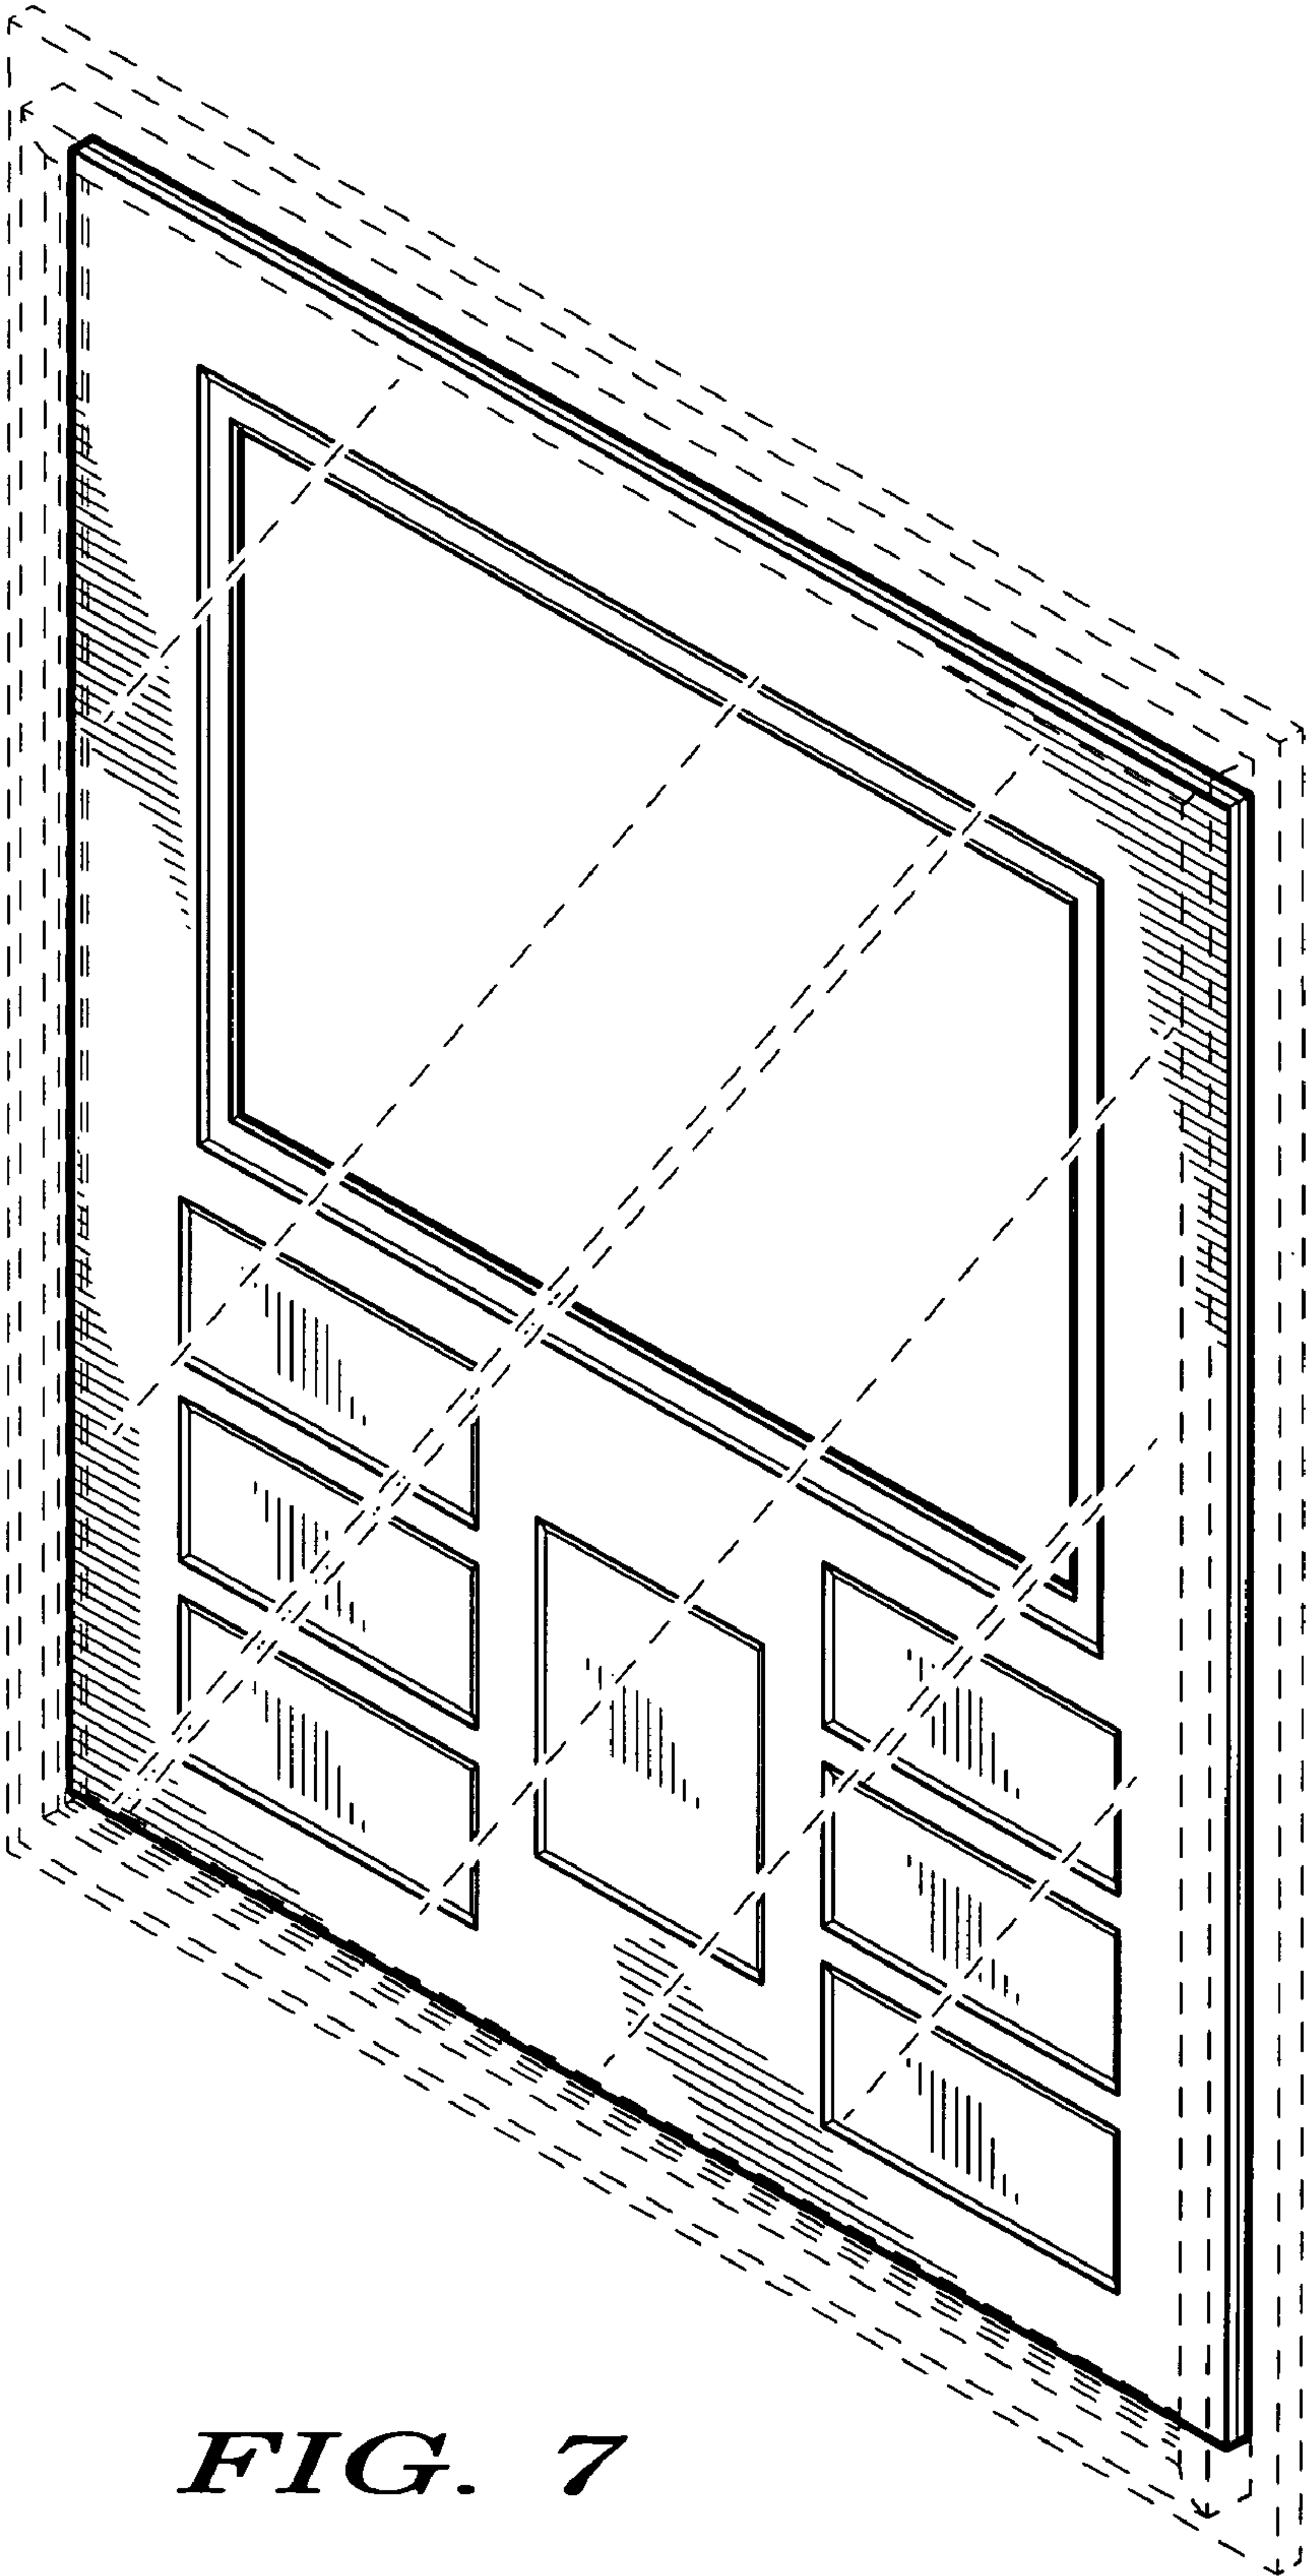


FIG. 7