



US00D629112S

(12) **United States Design Patent**
Immekus

(10) **Patent No.:** **US D629,112 S**

(45) **Date of Patent:** **** Dec. 14, 2010**

(54) **MEDICAL DEVICE ASSEMBLY**

(75) Inventor: **Claudio Immekus**, Emmendingen (DE)

(73) Assignee: **Rudolf Medical GmbH & Co. KG**,
Friedingen (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/279,227**

(22) Filed: **Apr. 24, 2007**

(30) **Foreign Application Priority Data**

Oct. 24, 2006 (EM) 000610001

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/186**

(58) **Field of Classification Search** D24/107,
D24/111, 138, 144, 165, 170, 186, 231, 232;
D14/203.01, 363, 498; 128/900, 902; 422/119;
600/301, 306, 483, 508, 523; D10/46; D13/101
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D286,280 S *	10/1986	Holtman et al.	D24/107
D287,052 S *	12/1986	Avoy et al.	D24/165
D300,359 S *	3/1989	Lee et al.	D10/46
D310,120 S *	8/1990	Wickham et al.	D24/186
D311,062 S *	10/1990	Nelson	D24/186
D330,768 S *	11/1992	Yoshikawa et al.	D24/165
D412,977 S *	8/1999	Hayamizu	D24/144
D481,123 S *	10/2003	Hayamizu	D24/138
D523,806 S *	6/2006	Symanzik et al.	D13/101
D574,961 S *	8/2008	Kitahara et al.	D24/186
D582,044 S *	12/2008	Hacker et al.	D24/170
D584,812 S *	1/2009	Ries	D24/111
D598,098 S *	8/2009	Tanaka	D24/138
D598,100 S *	8/2009	Tanaka	D24/138

* cited by examiner

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Bachman & LaPointe, P.C.

(57) **CLAIM**

The ornamental design for a medical device assembly, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the top portion of a medical device assembly shown separately for clarity showing the new design;

FIG. 2 is a front view thereof;

FIG. 3 is a right side view thereof;

FIG. 4 is a left side view thereof;

FIG. 5 is a rear view thereof;

FIG. 6 is a top view thereof;

FIG. 7 is a bottom view thereof;

FIG. 8 is a perspective view of the bottom portion of a medical device assembly shown separately for clarity;

FIG. 9 is a front view thereof;

FIG. 10 is a right side view thereof;

FIG. 11 is a left side view thereof;

FIG. 12 is a rear view thereof;

FIG. 13 is a top view thereof;

FIG. 14 is a bottom view thereof;

FIG. 15 is a perspective view of both portions of a medical device assembly shown stacked in condition of use;

FIG. 16 is a front view thereof;

FIG. 17 is a right side view thereof;

FIG. 18 is a left side view thereof;

FIG. 19 is a rear view thereof;


FIG. 20 is a top view thereof; and,

FIG. 21 is a bottom view thereof.

The broken lines are included for the purpose of illustrating a portion of the medical device assembly that forms no part of the claimed design.

The name Rudolf and the R Design displayed on the medical device assembly are trademarks owned by Rudolf Medical GmbH & Co. KG.

1 Claim, 17 Drawing Sheets

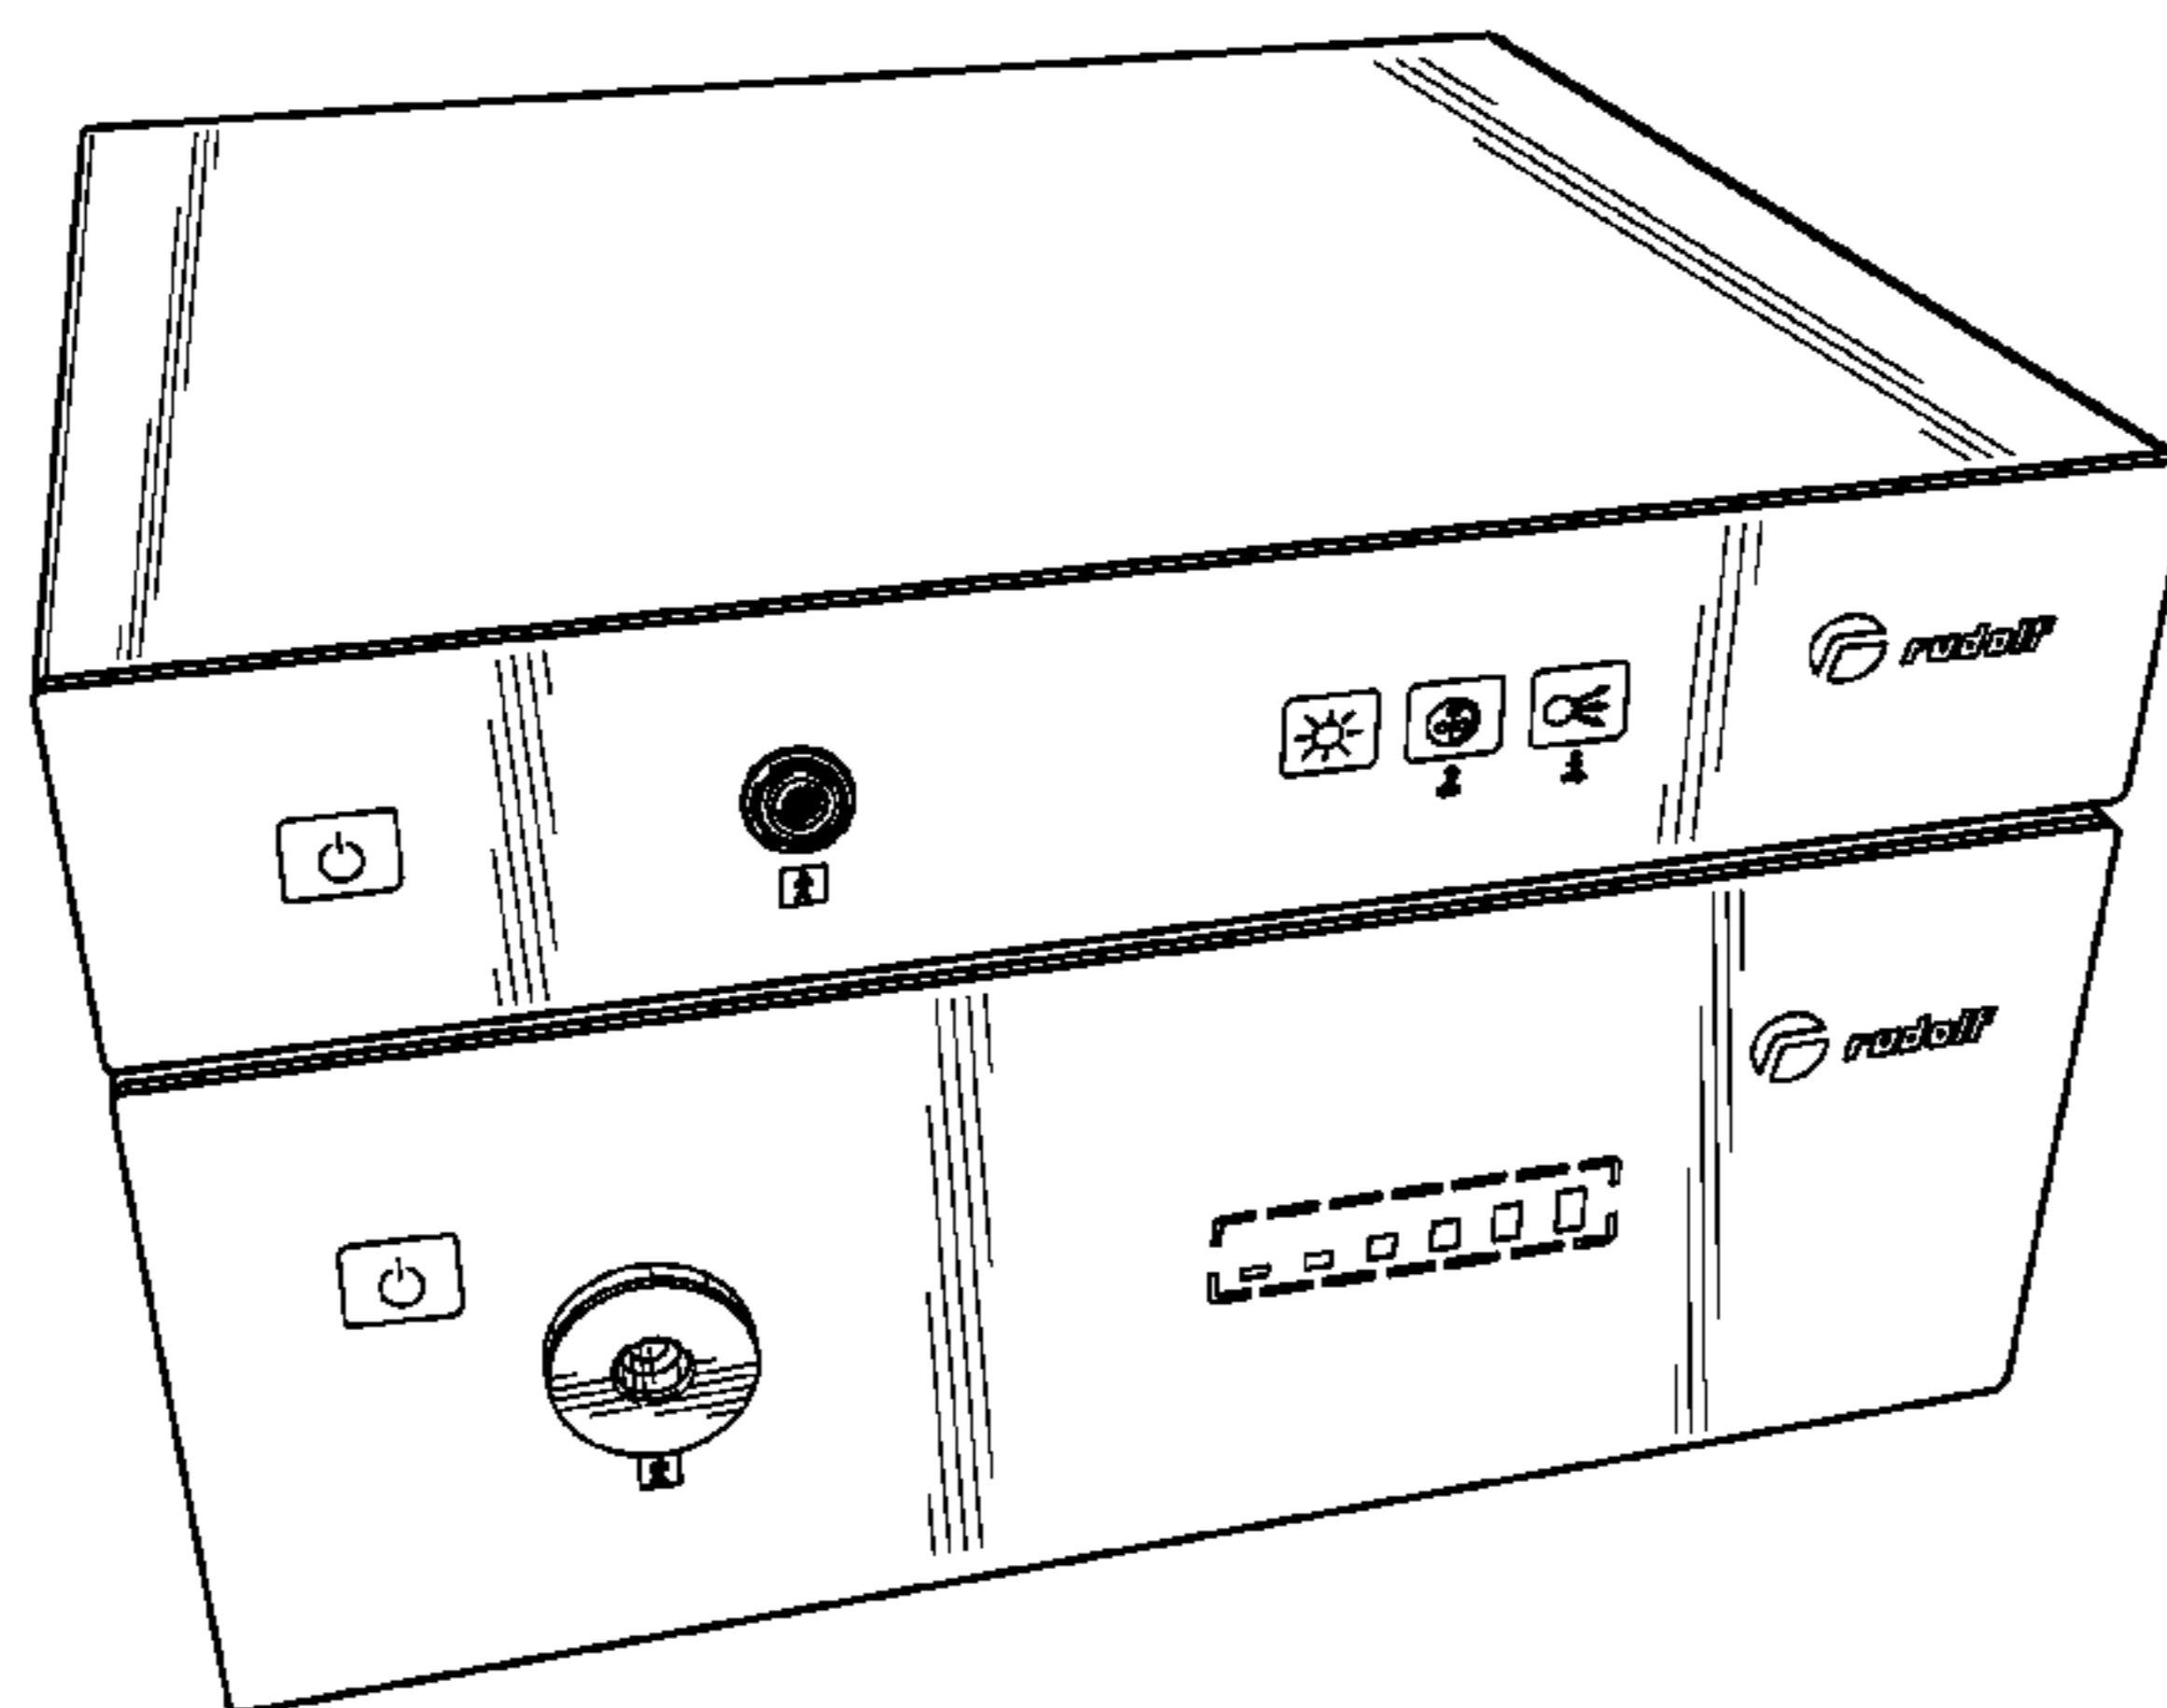

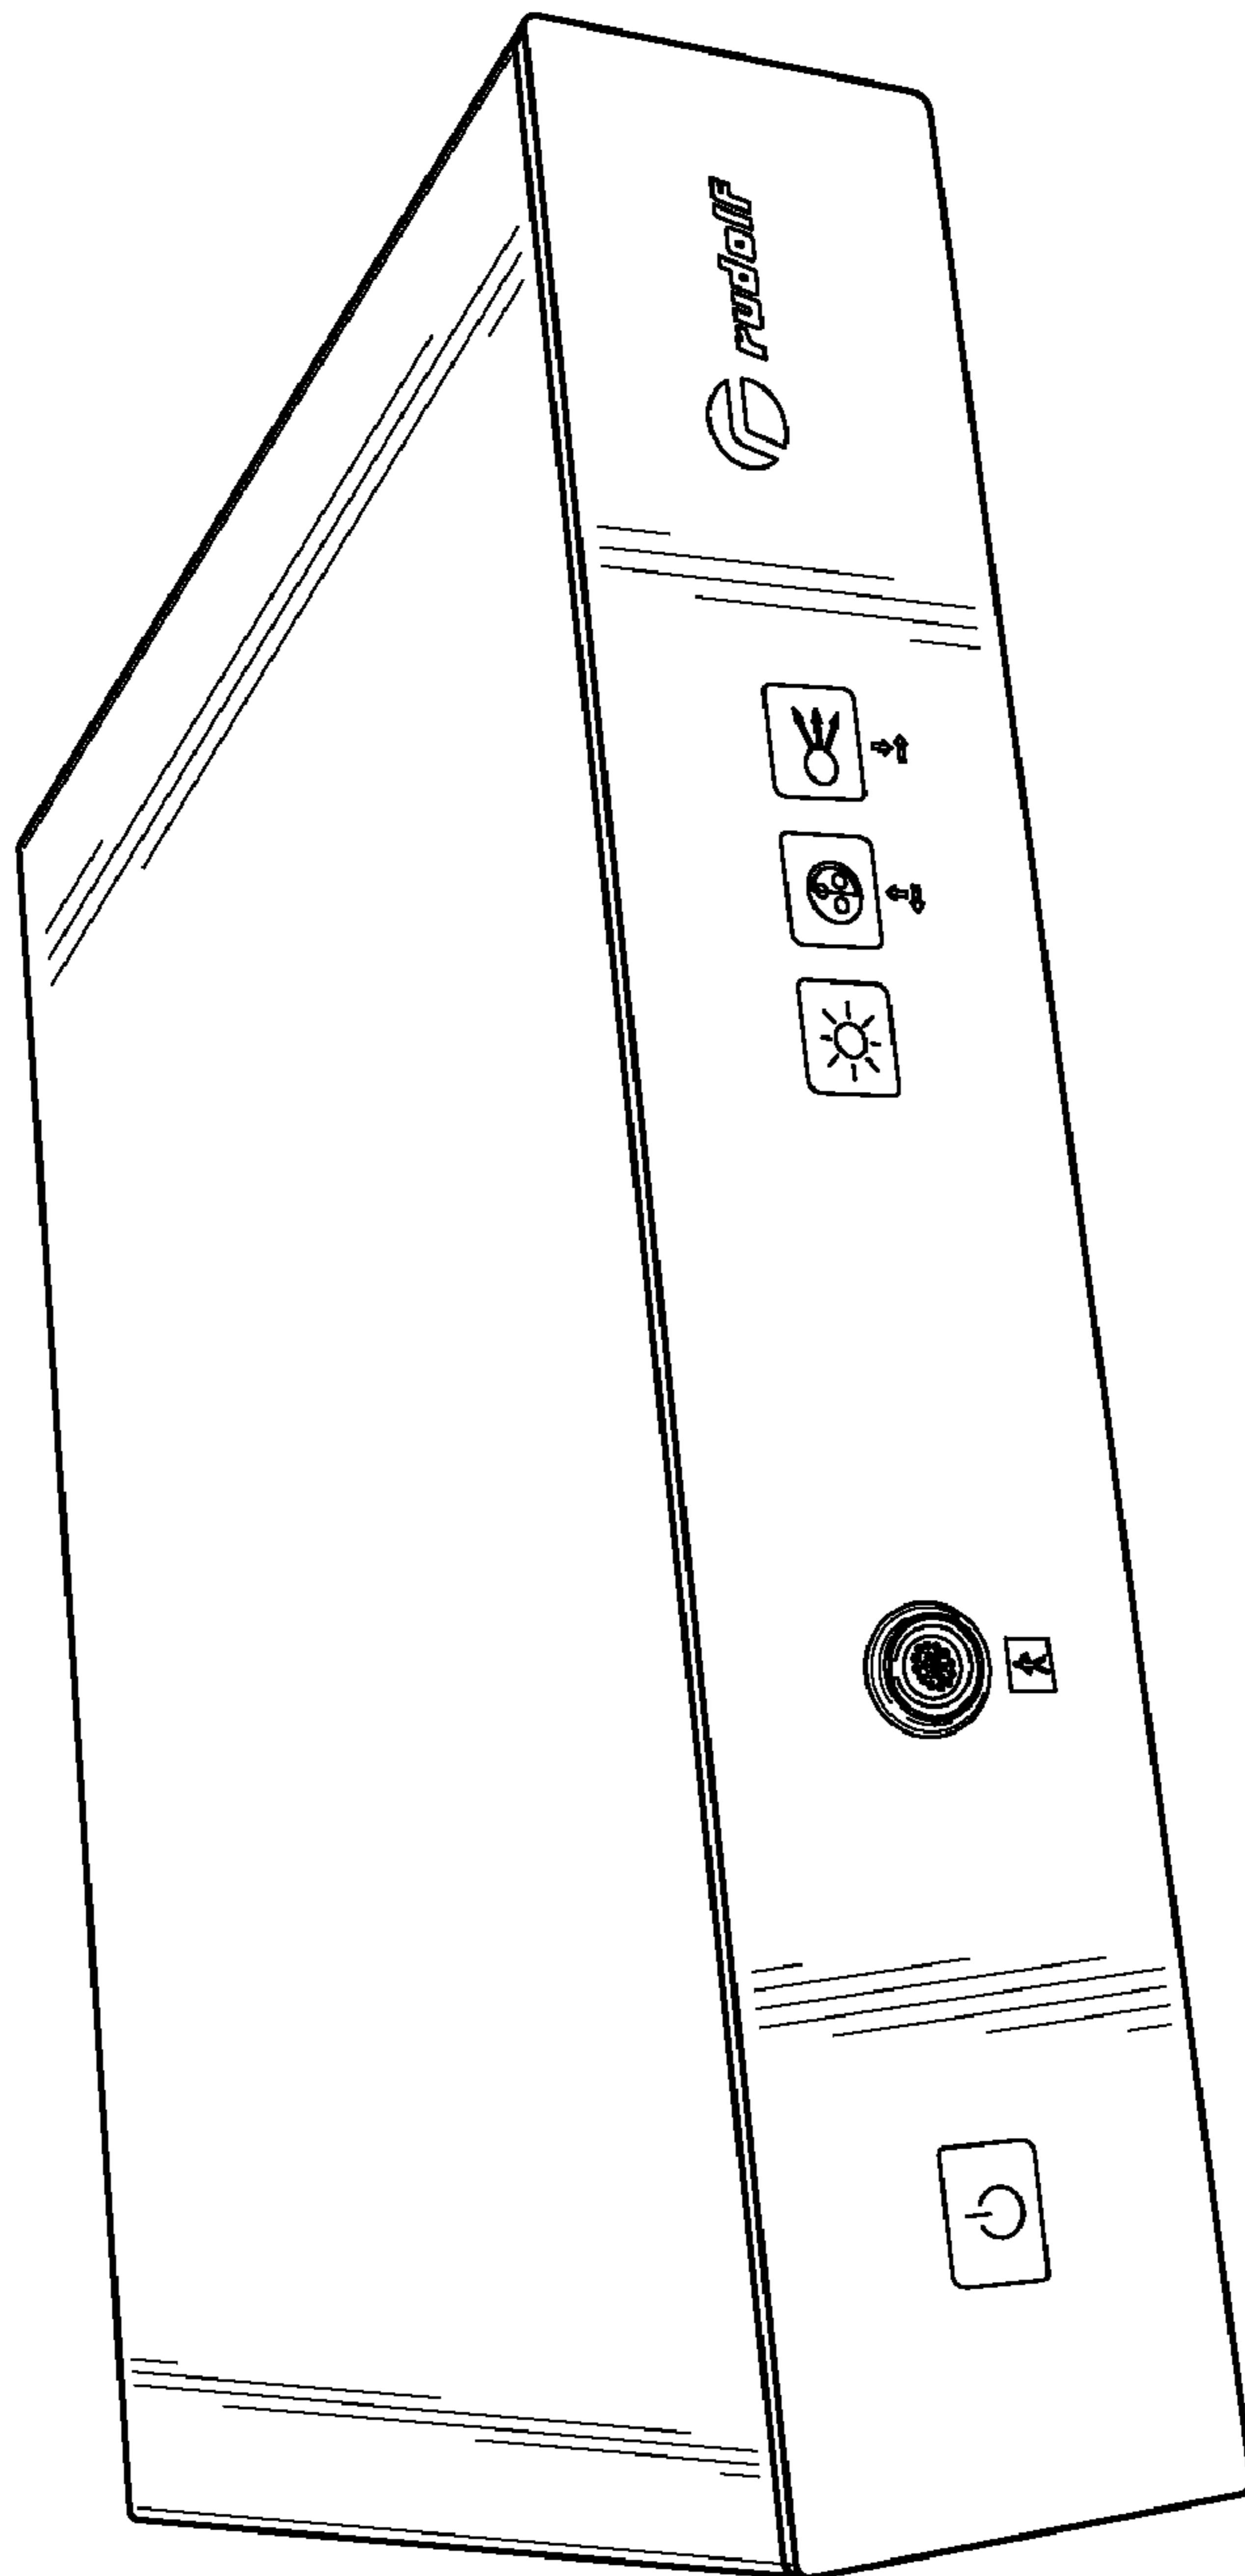


FIG. 1

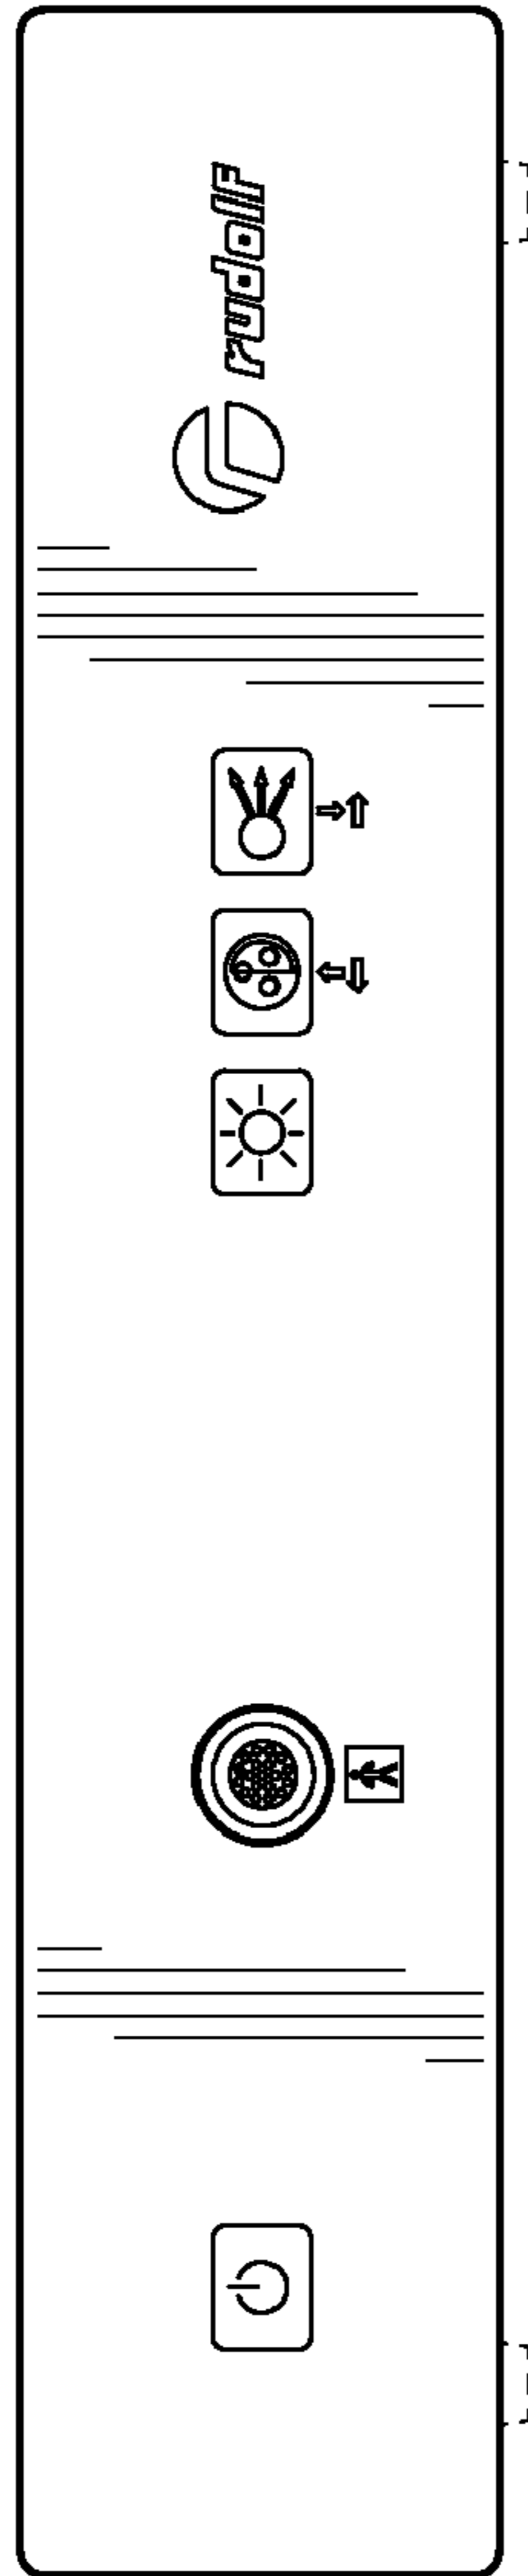


FIG. 2

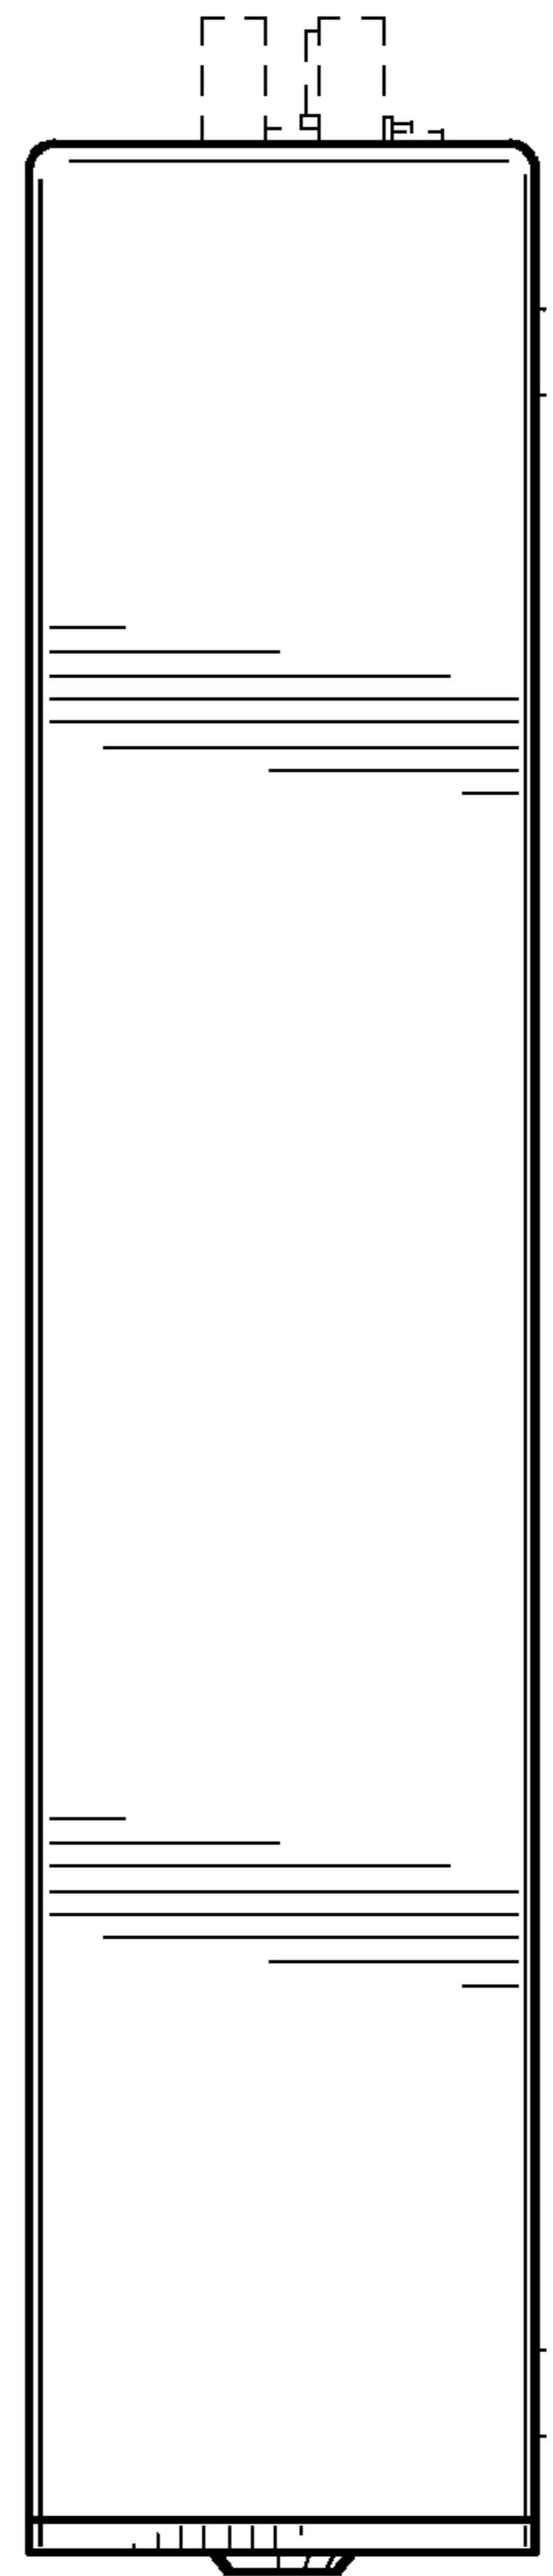


FIG. 3

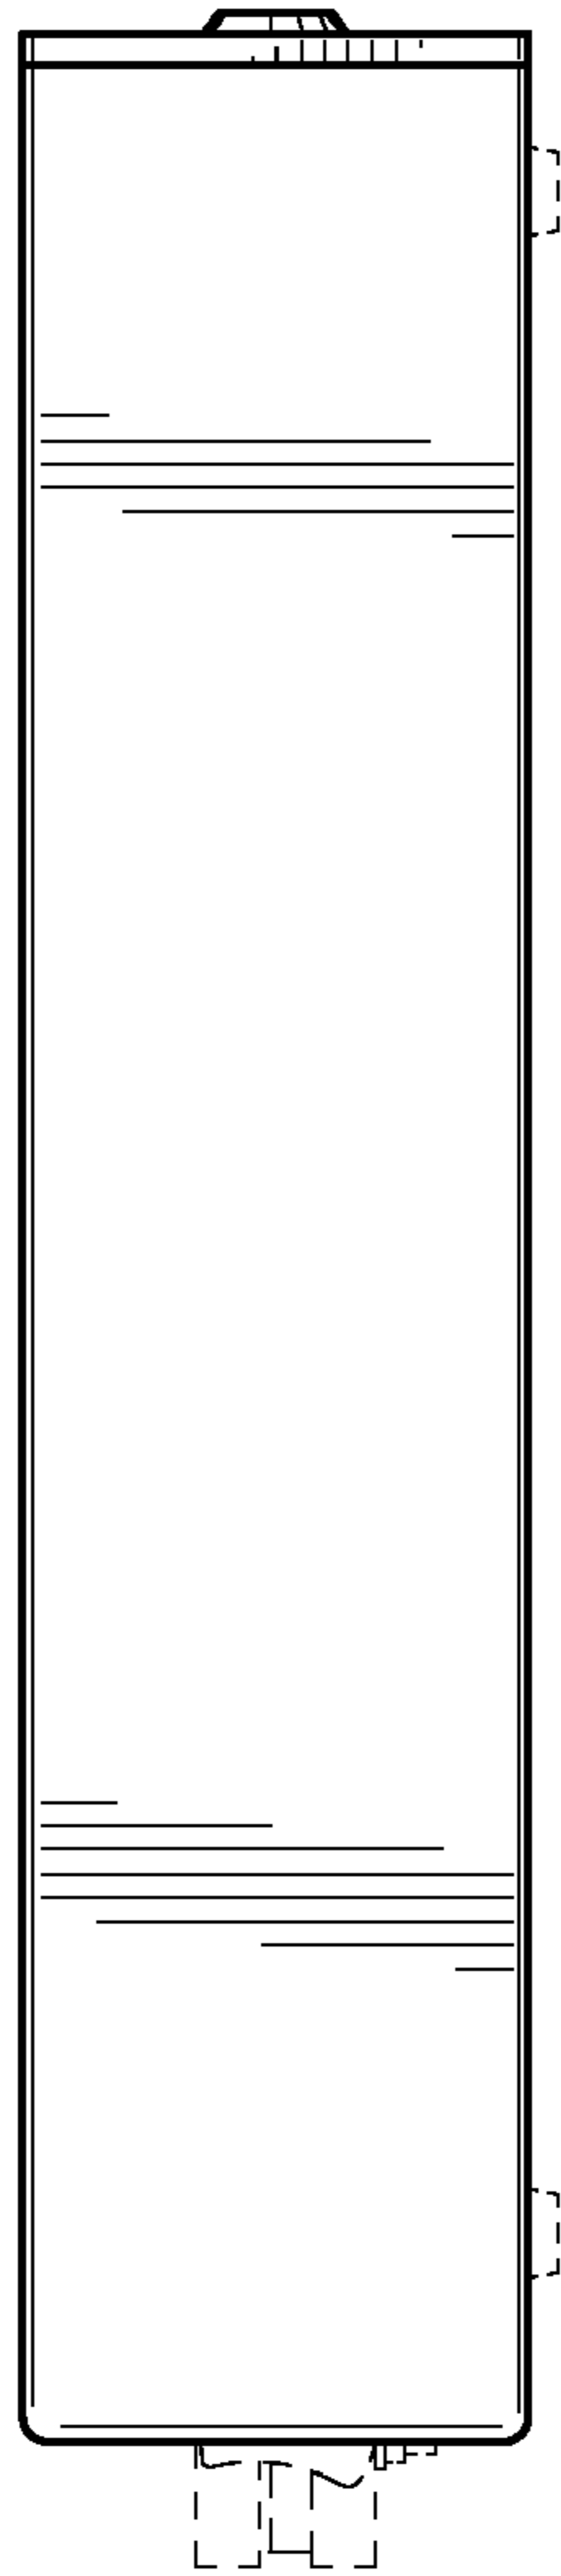


FIG. 4

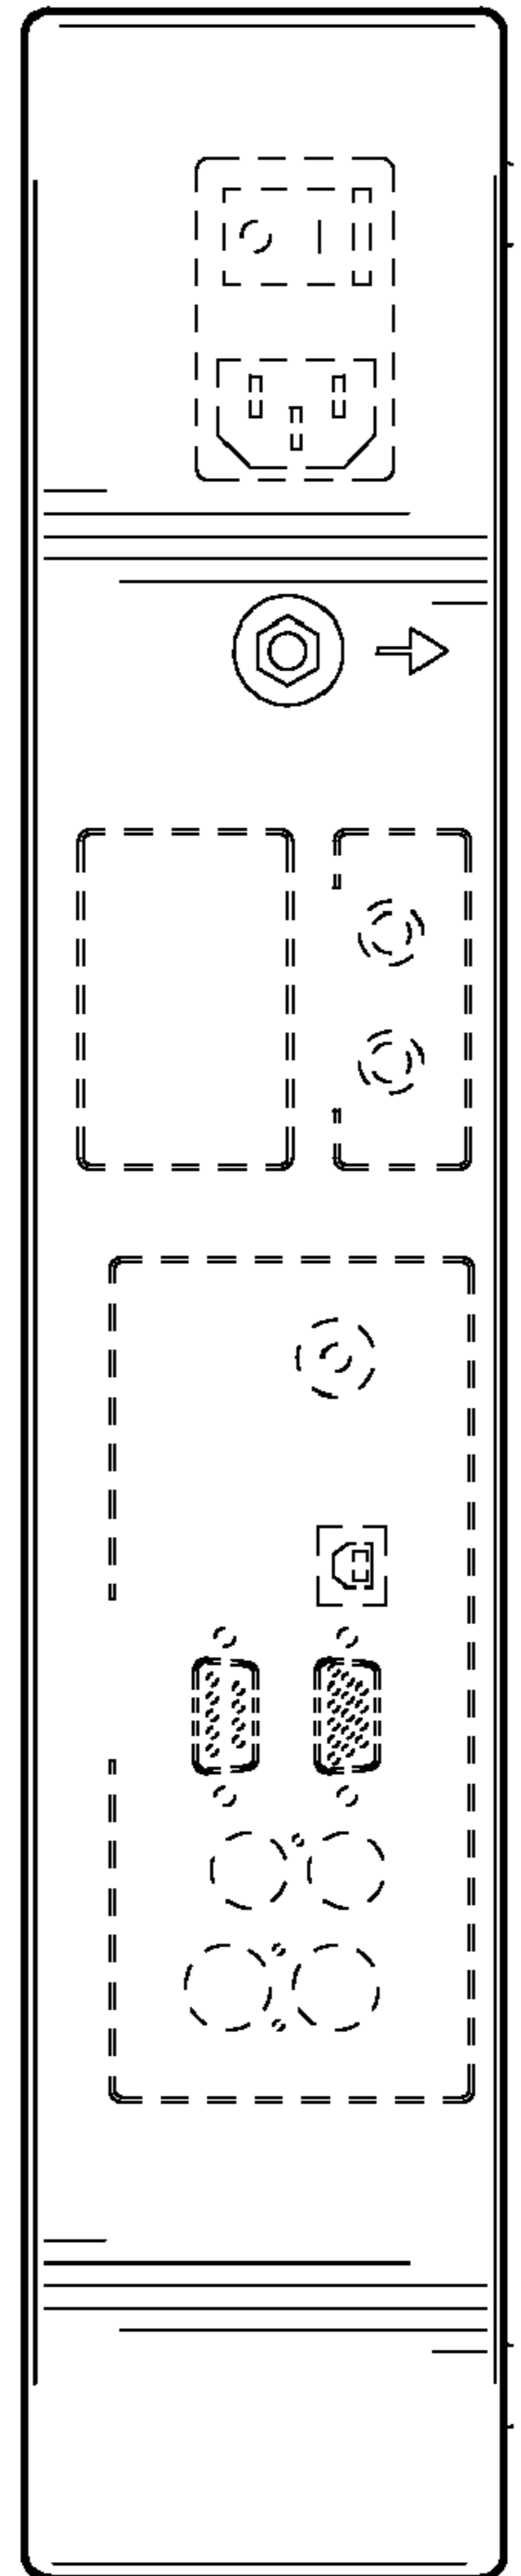


FIG. 5




FIG. 6

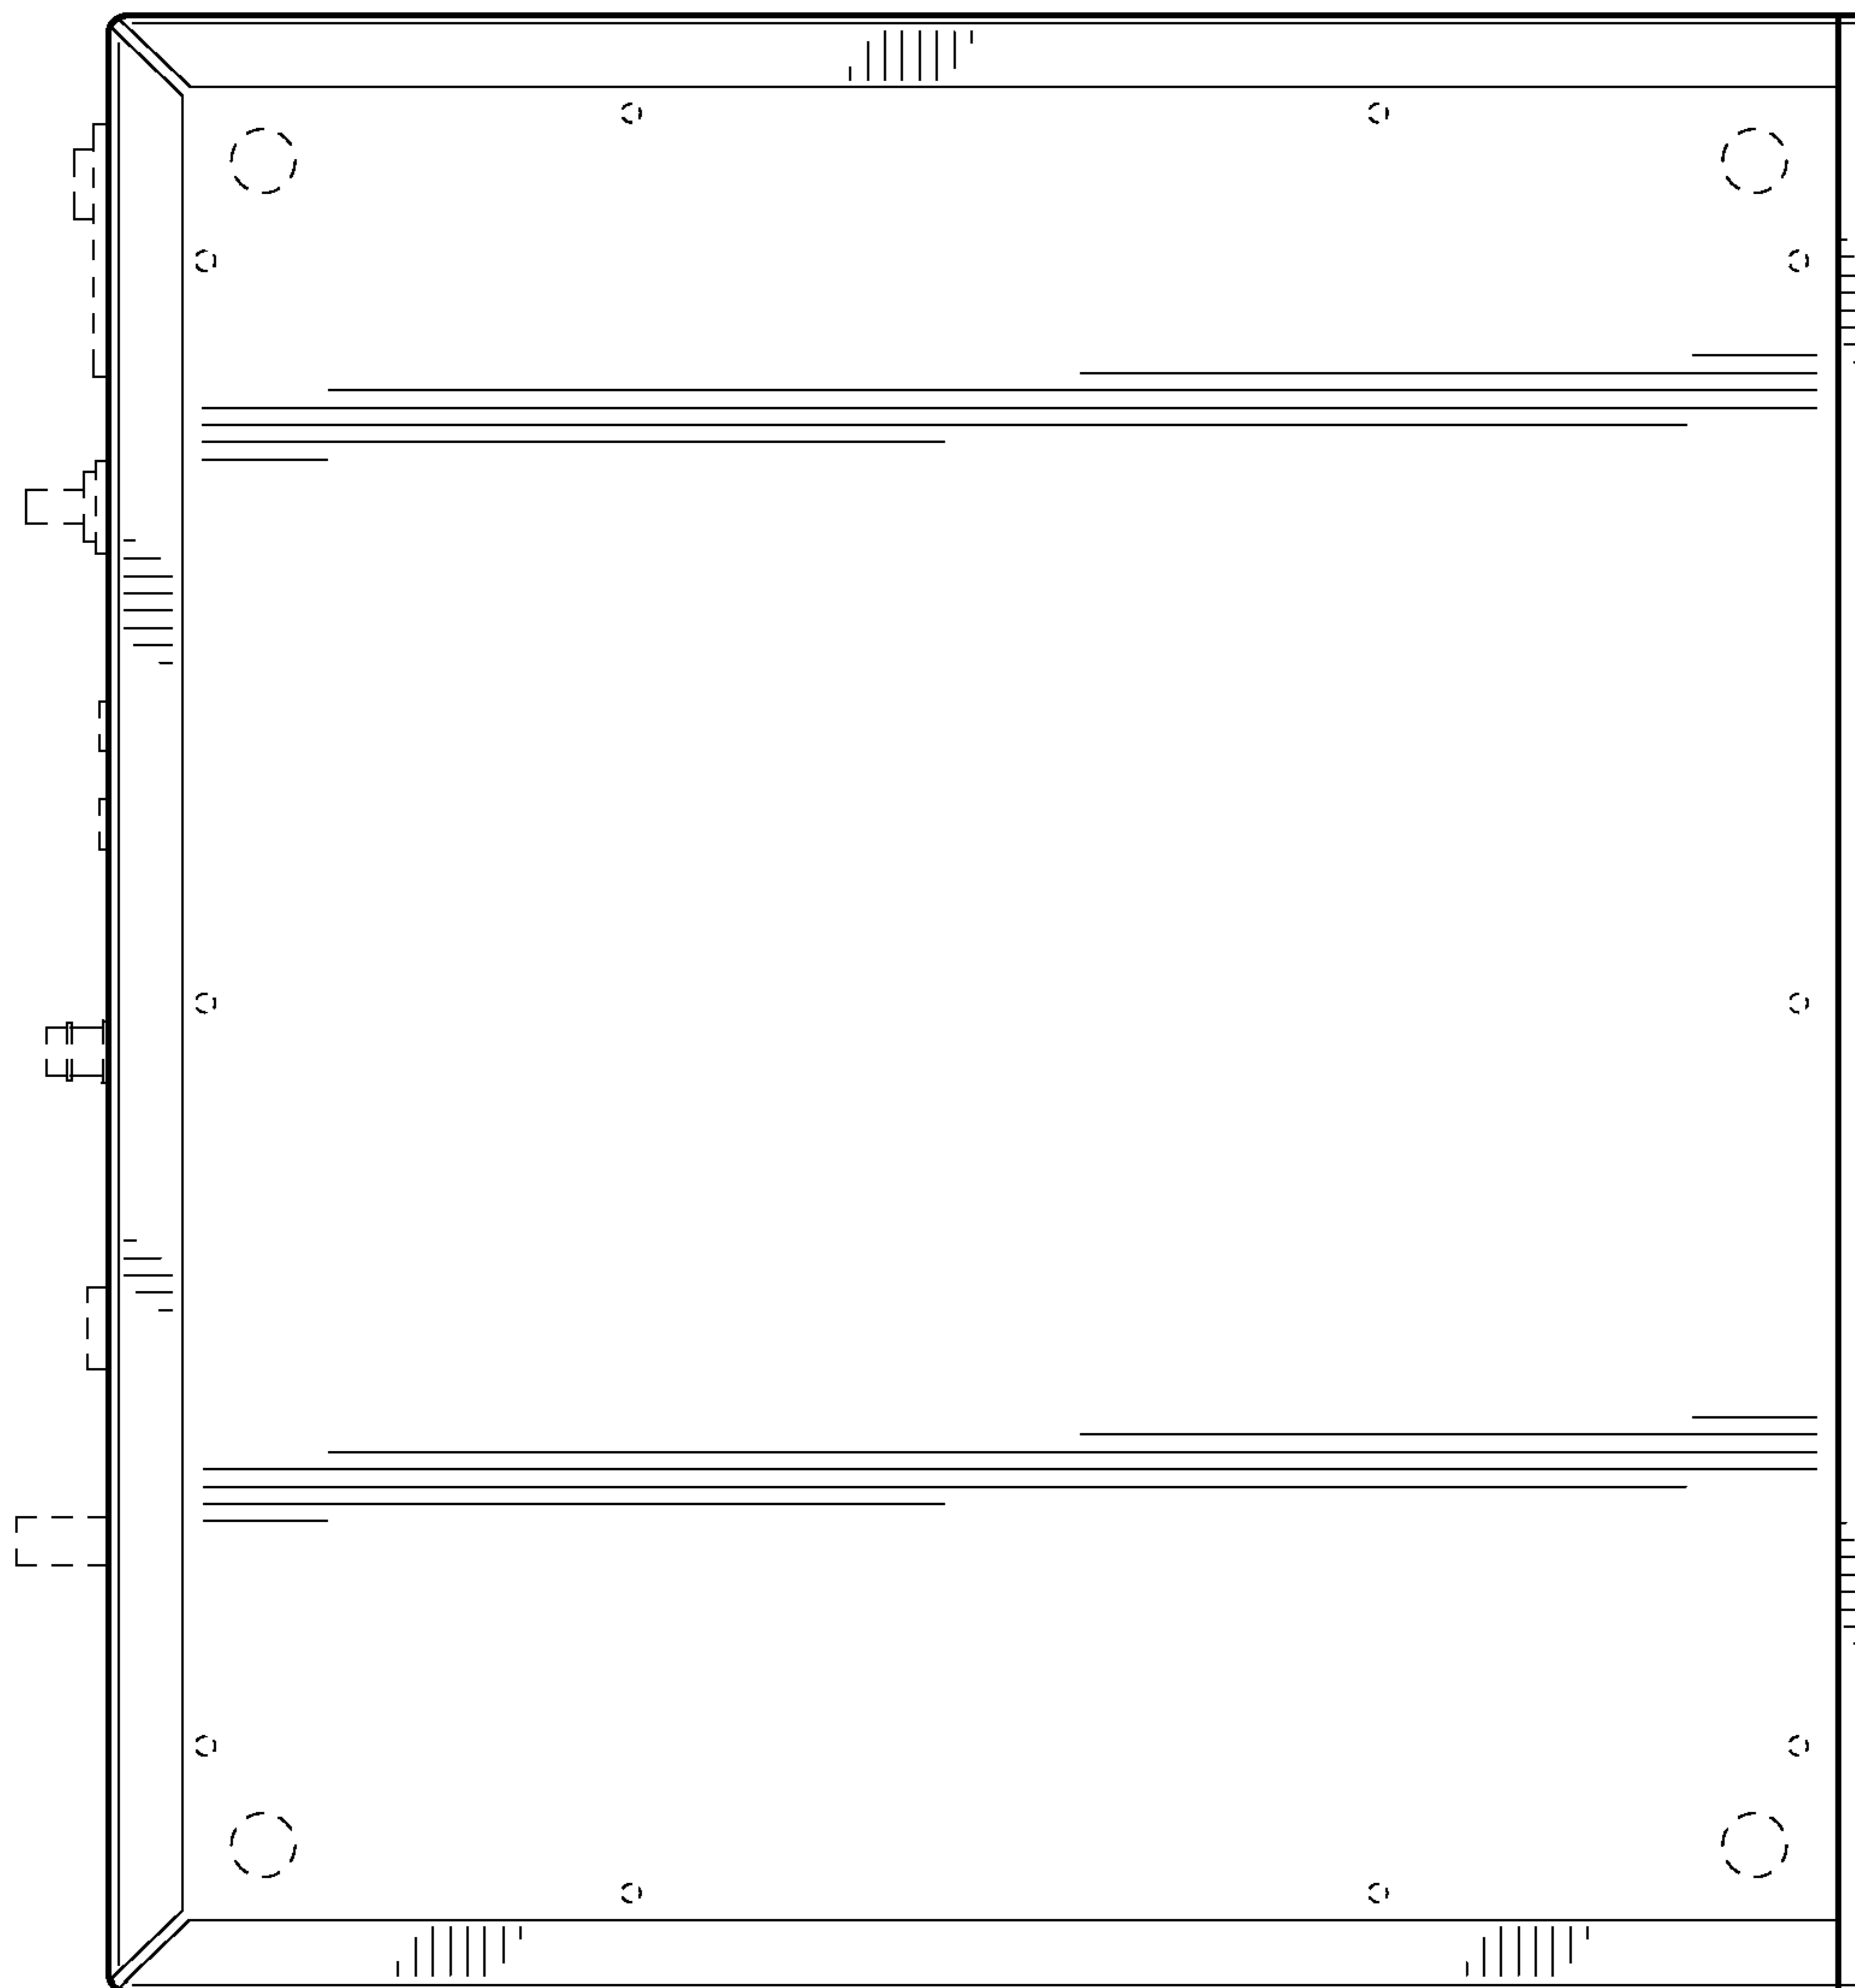


FIG. 7

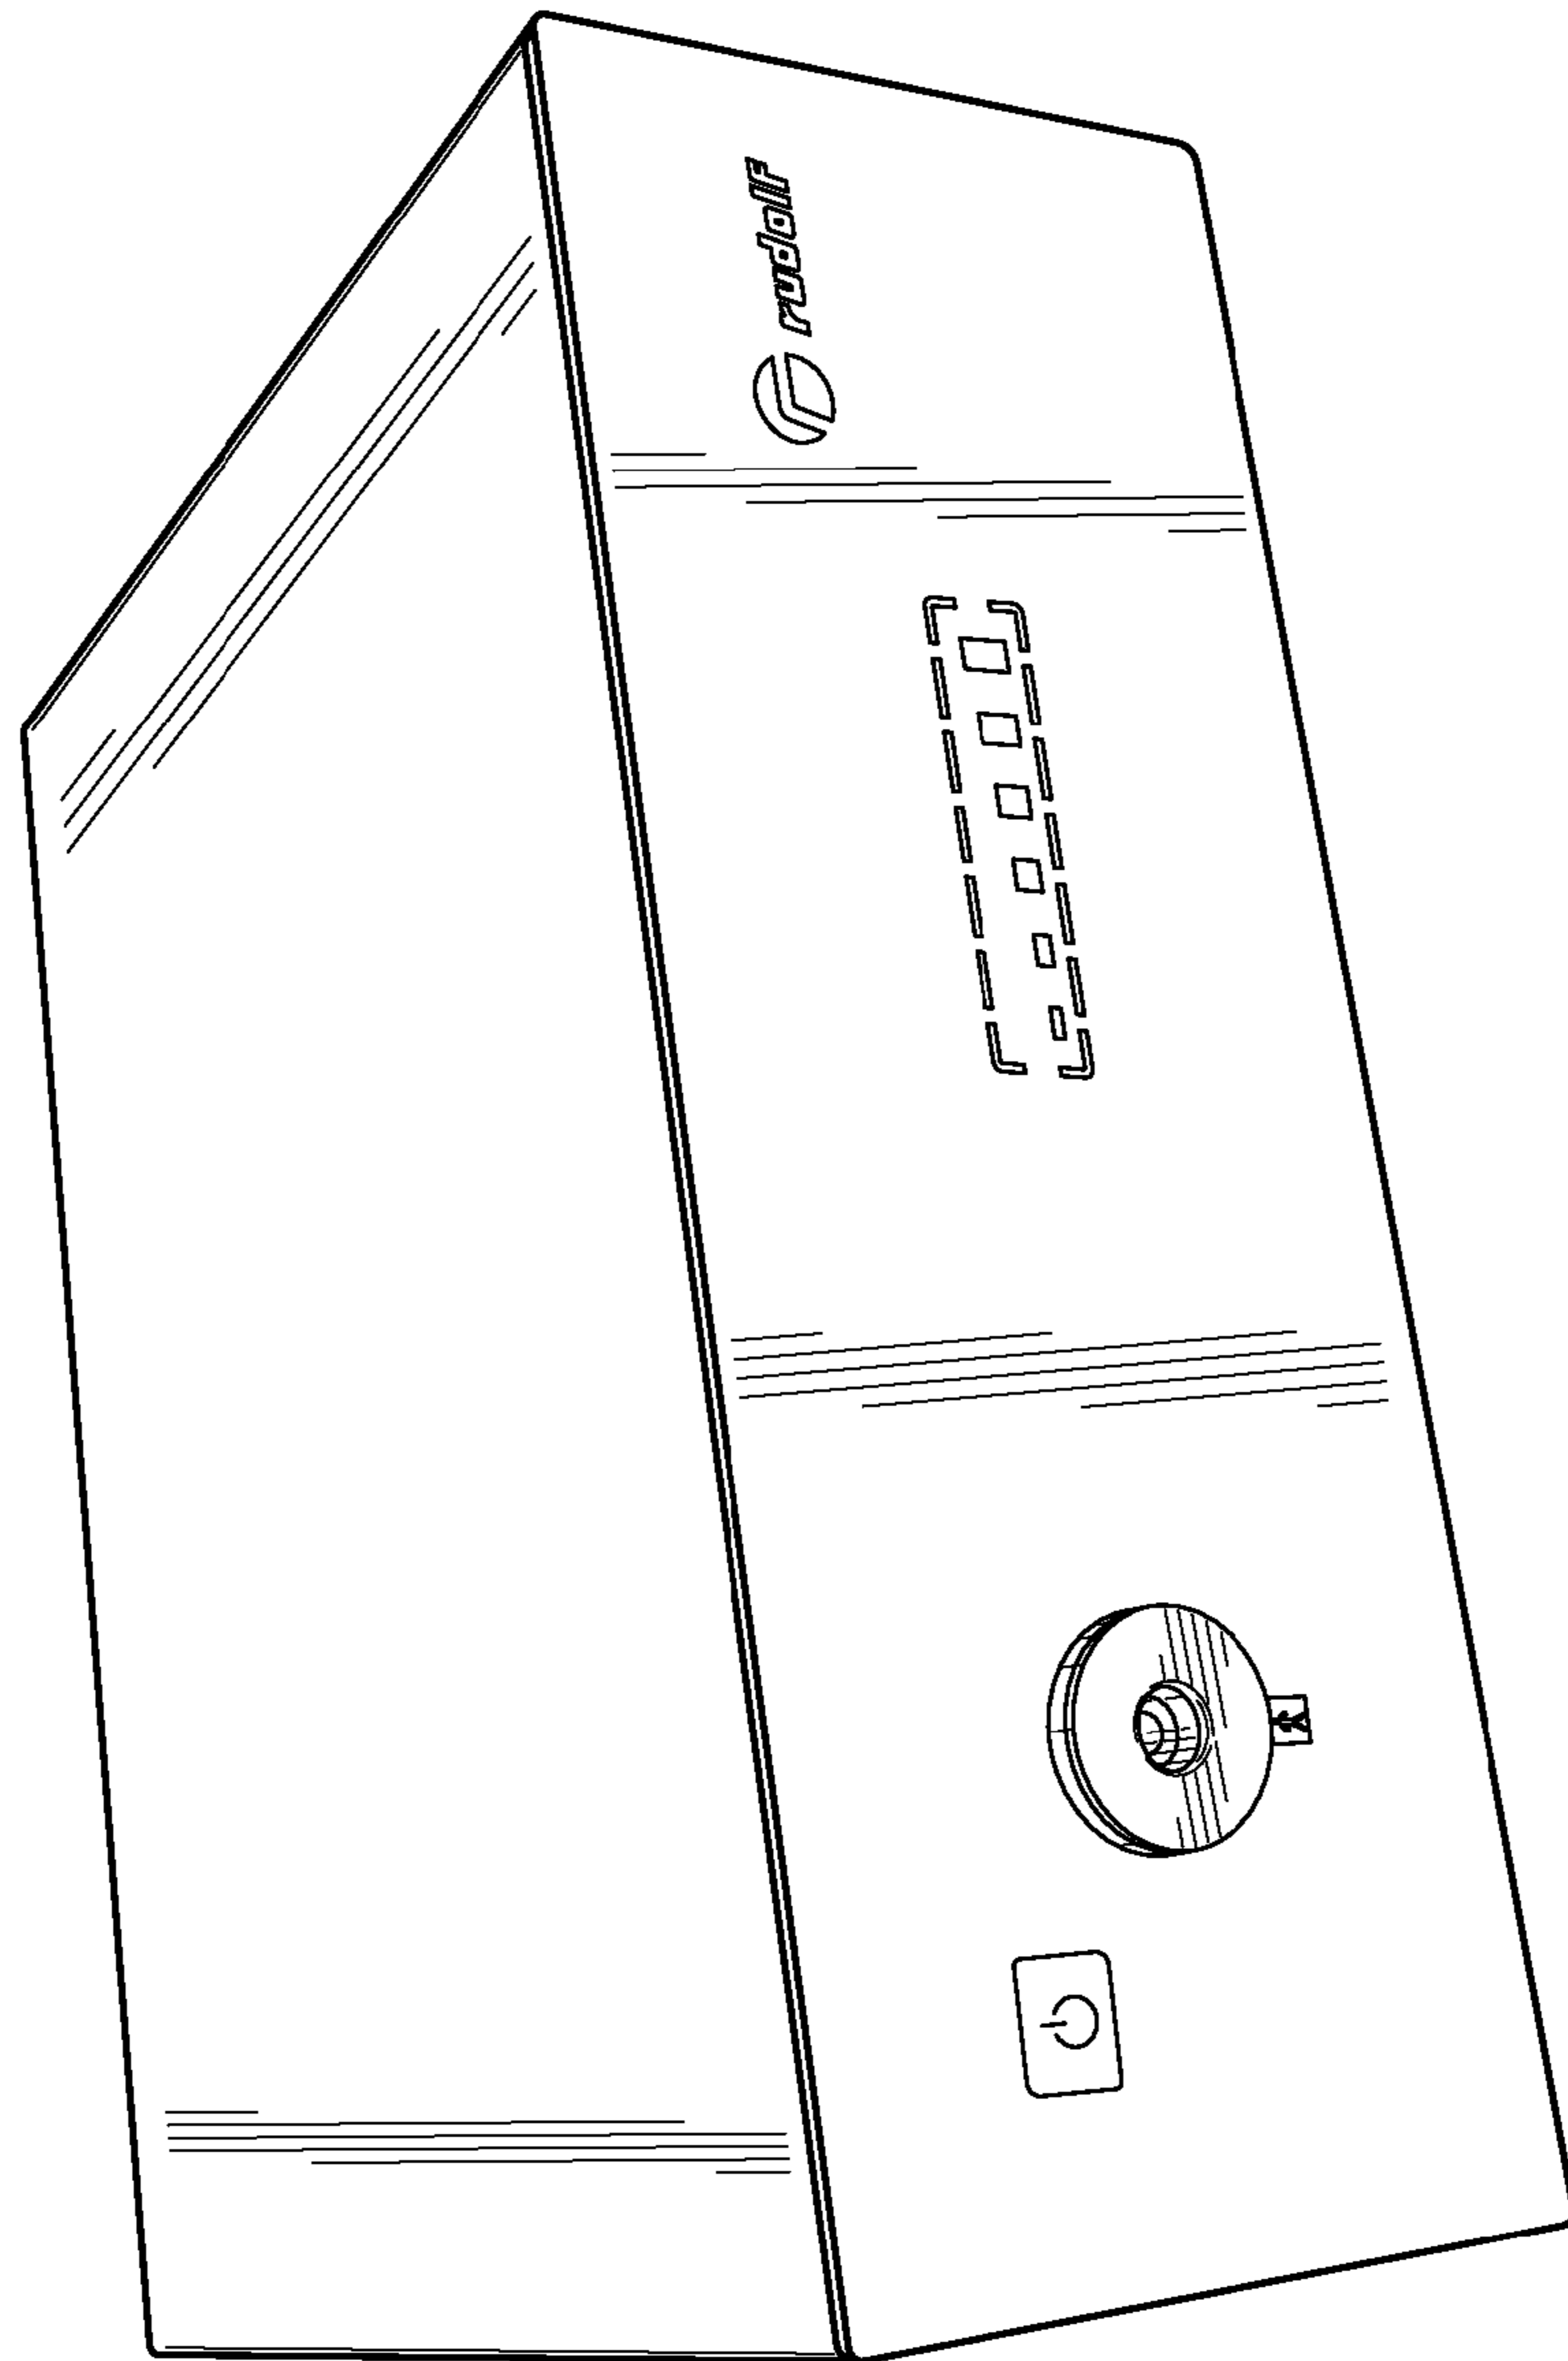


FIG. 8

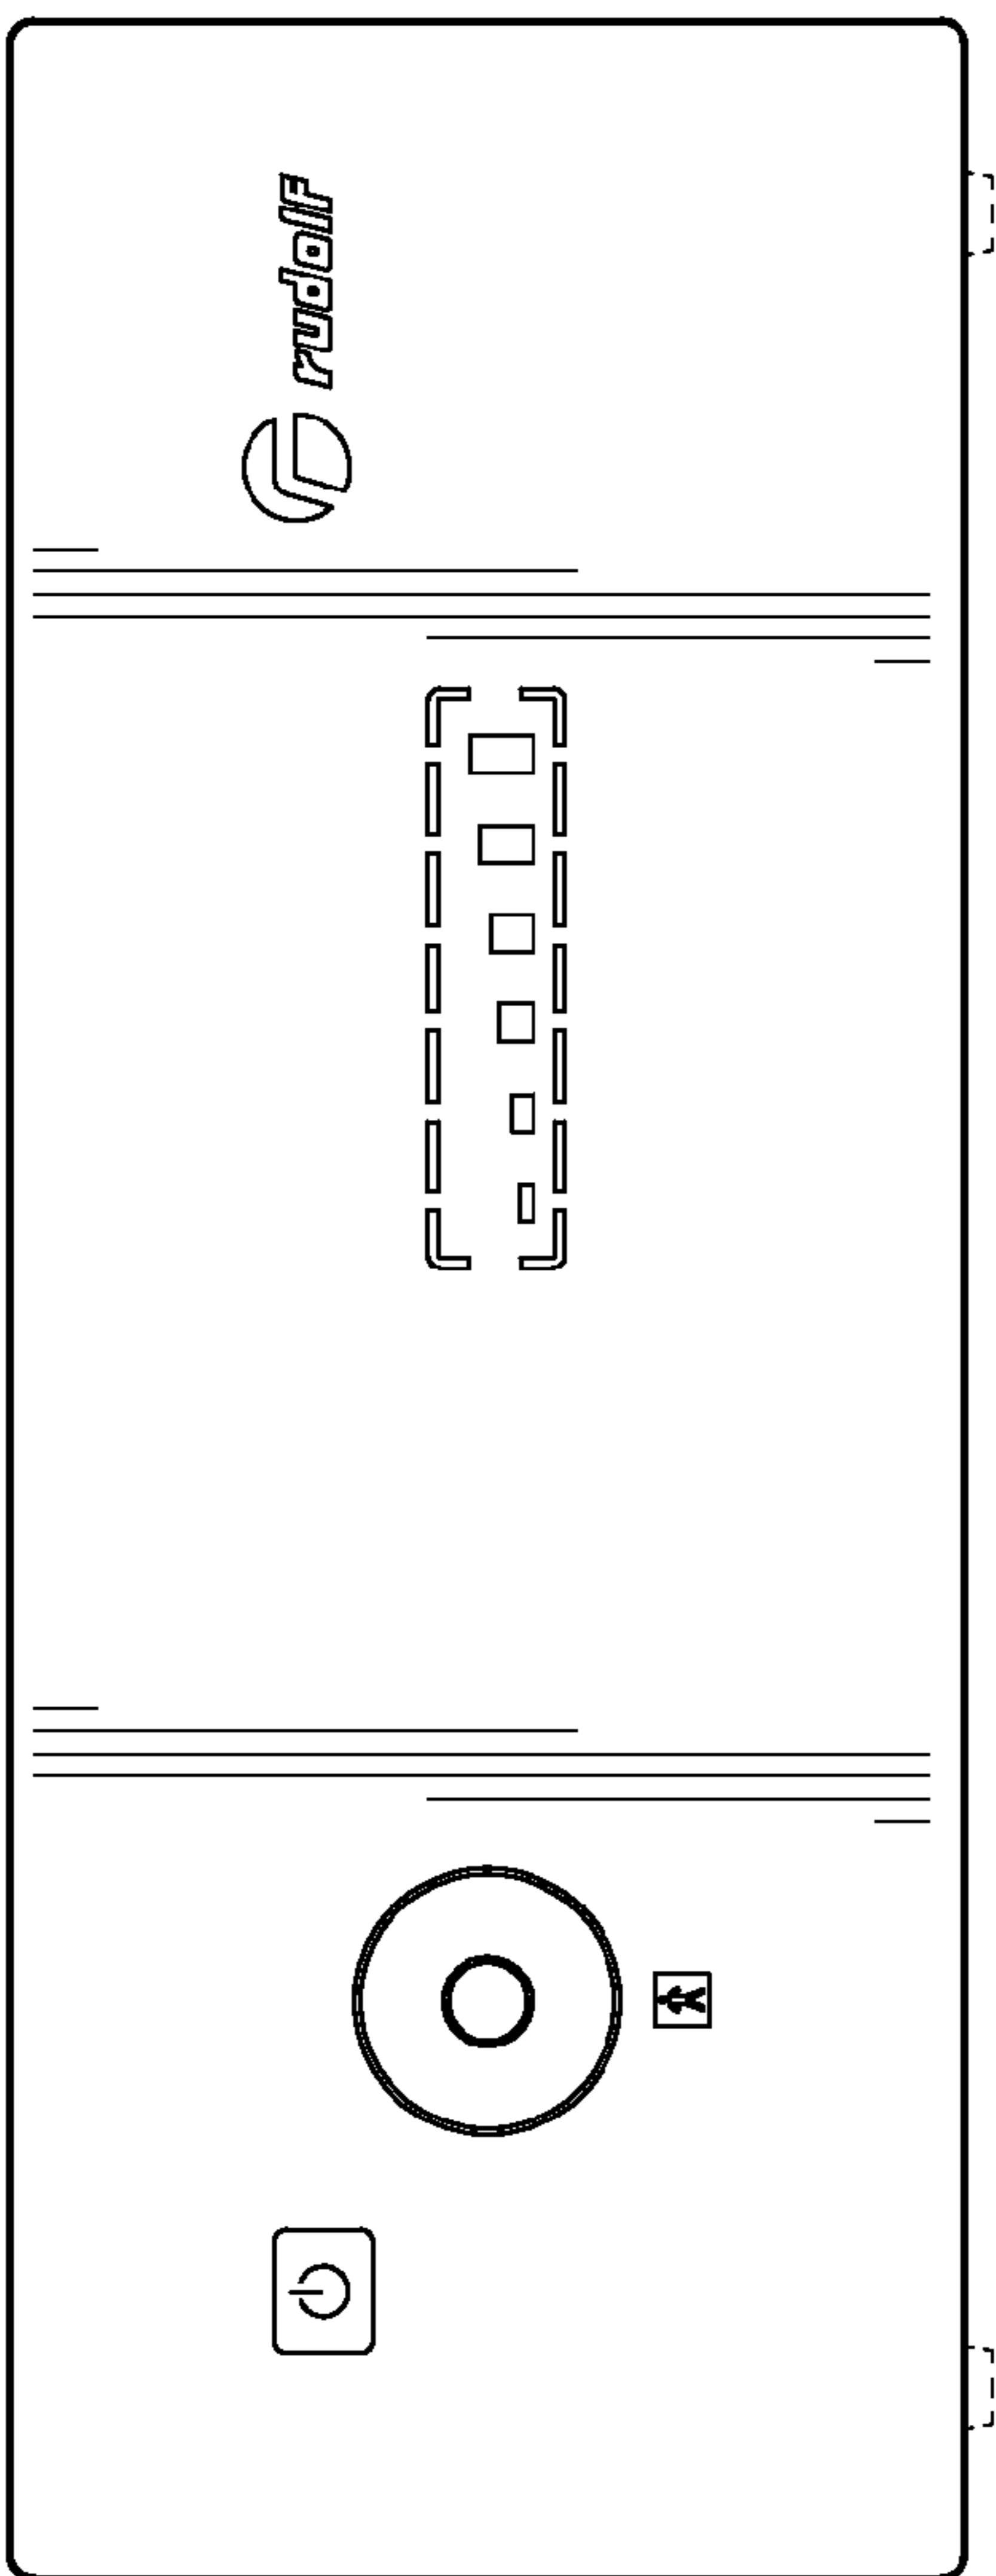


FIG. 9




FIG. 10




FIG. 11

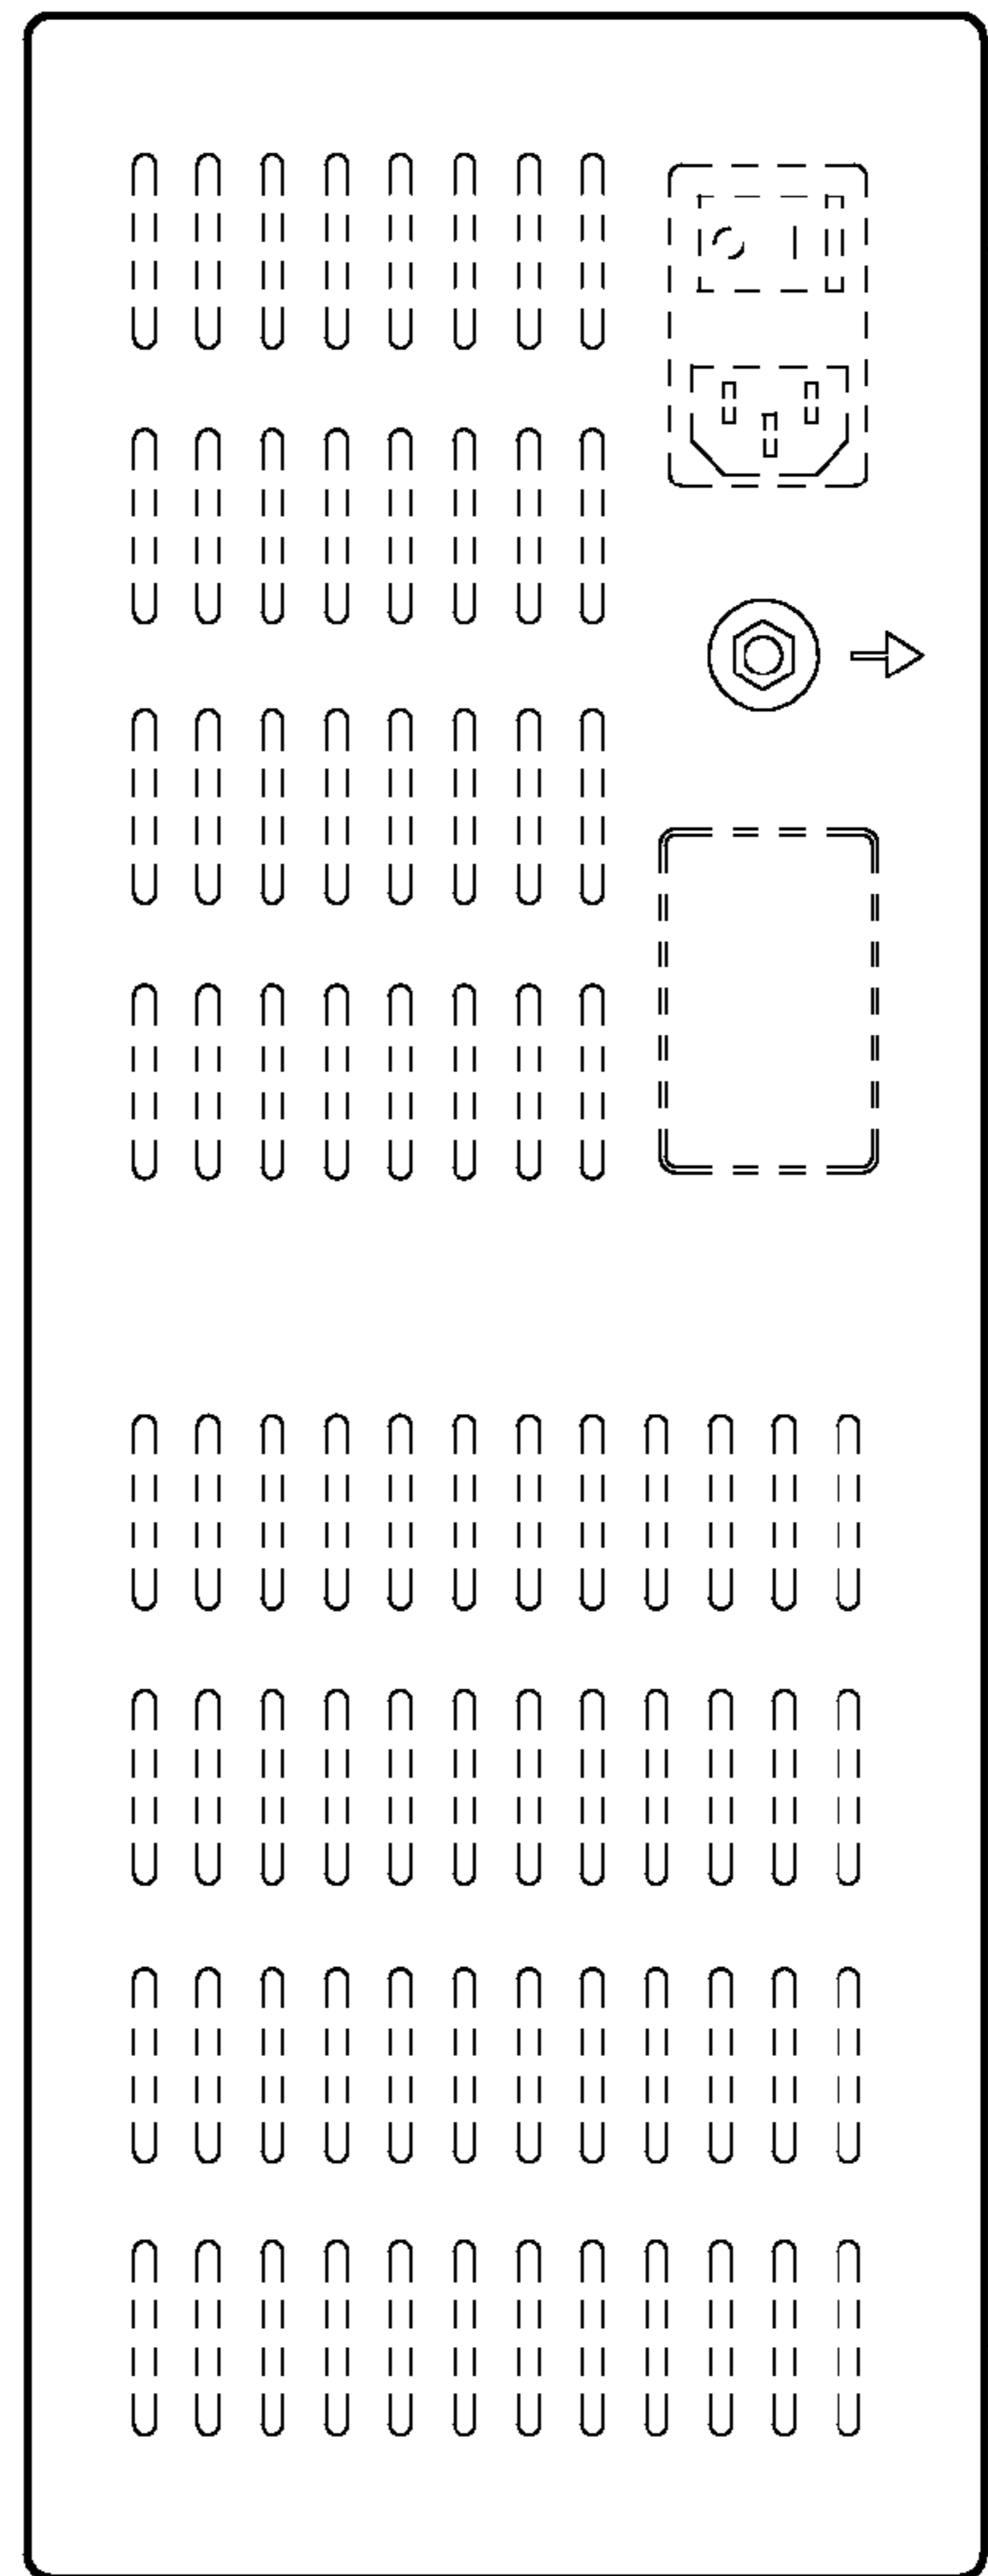


FIG. 12




FIG. 13

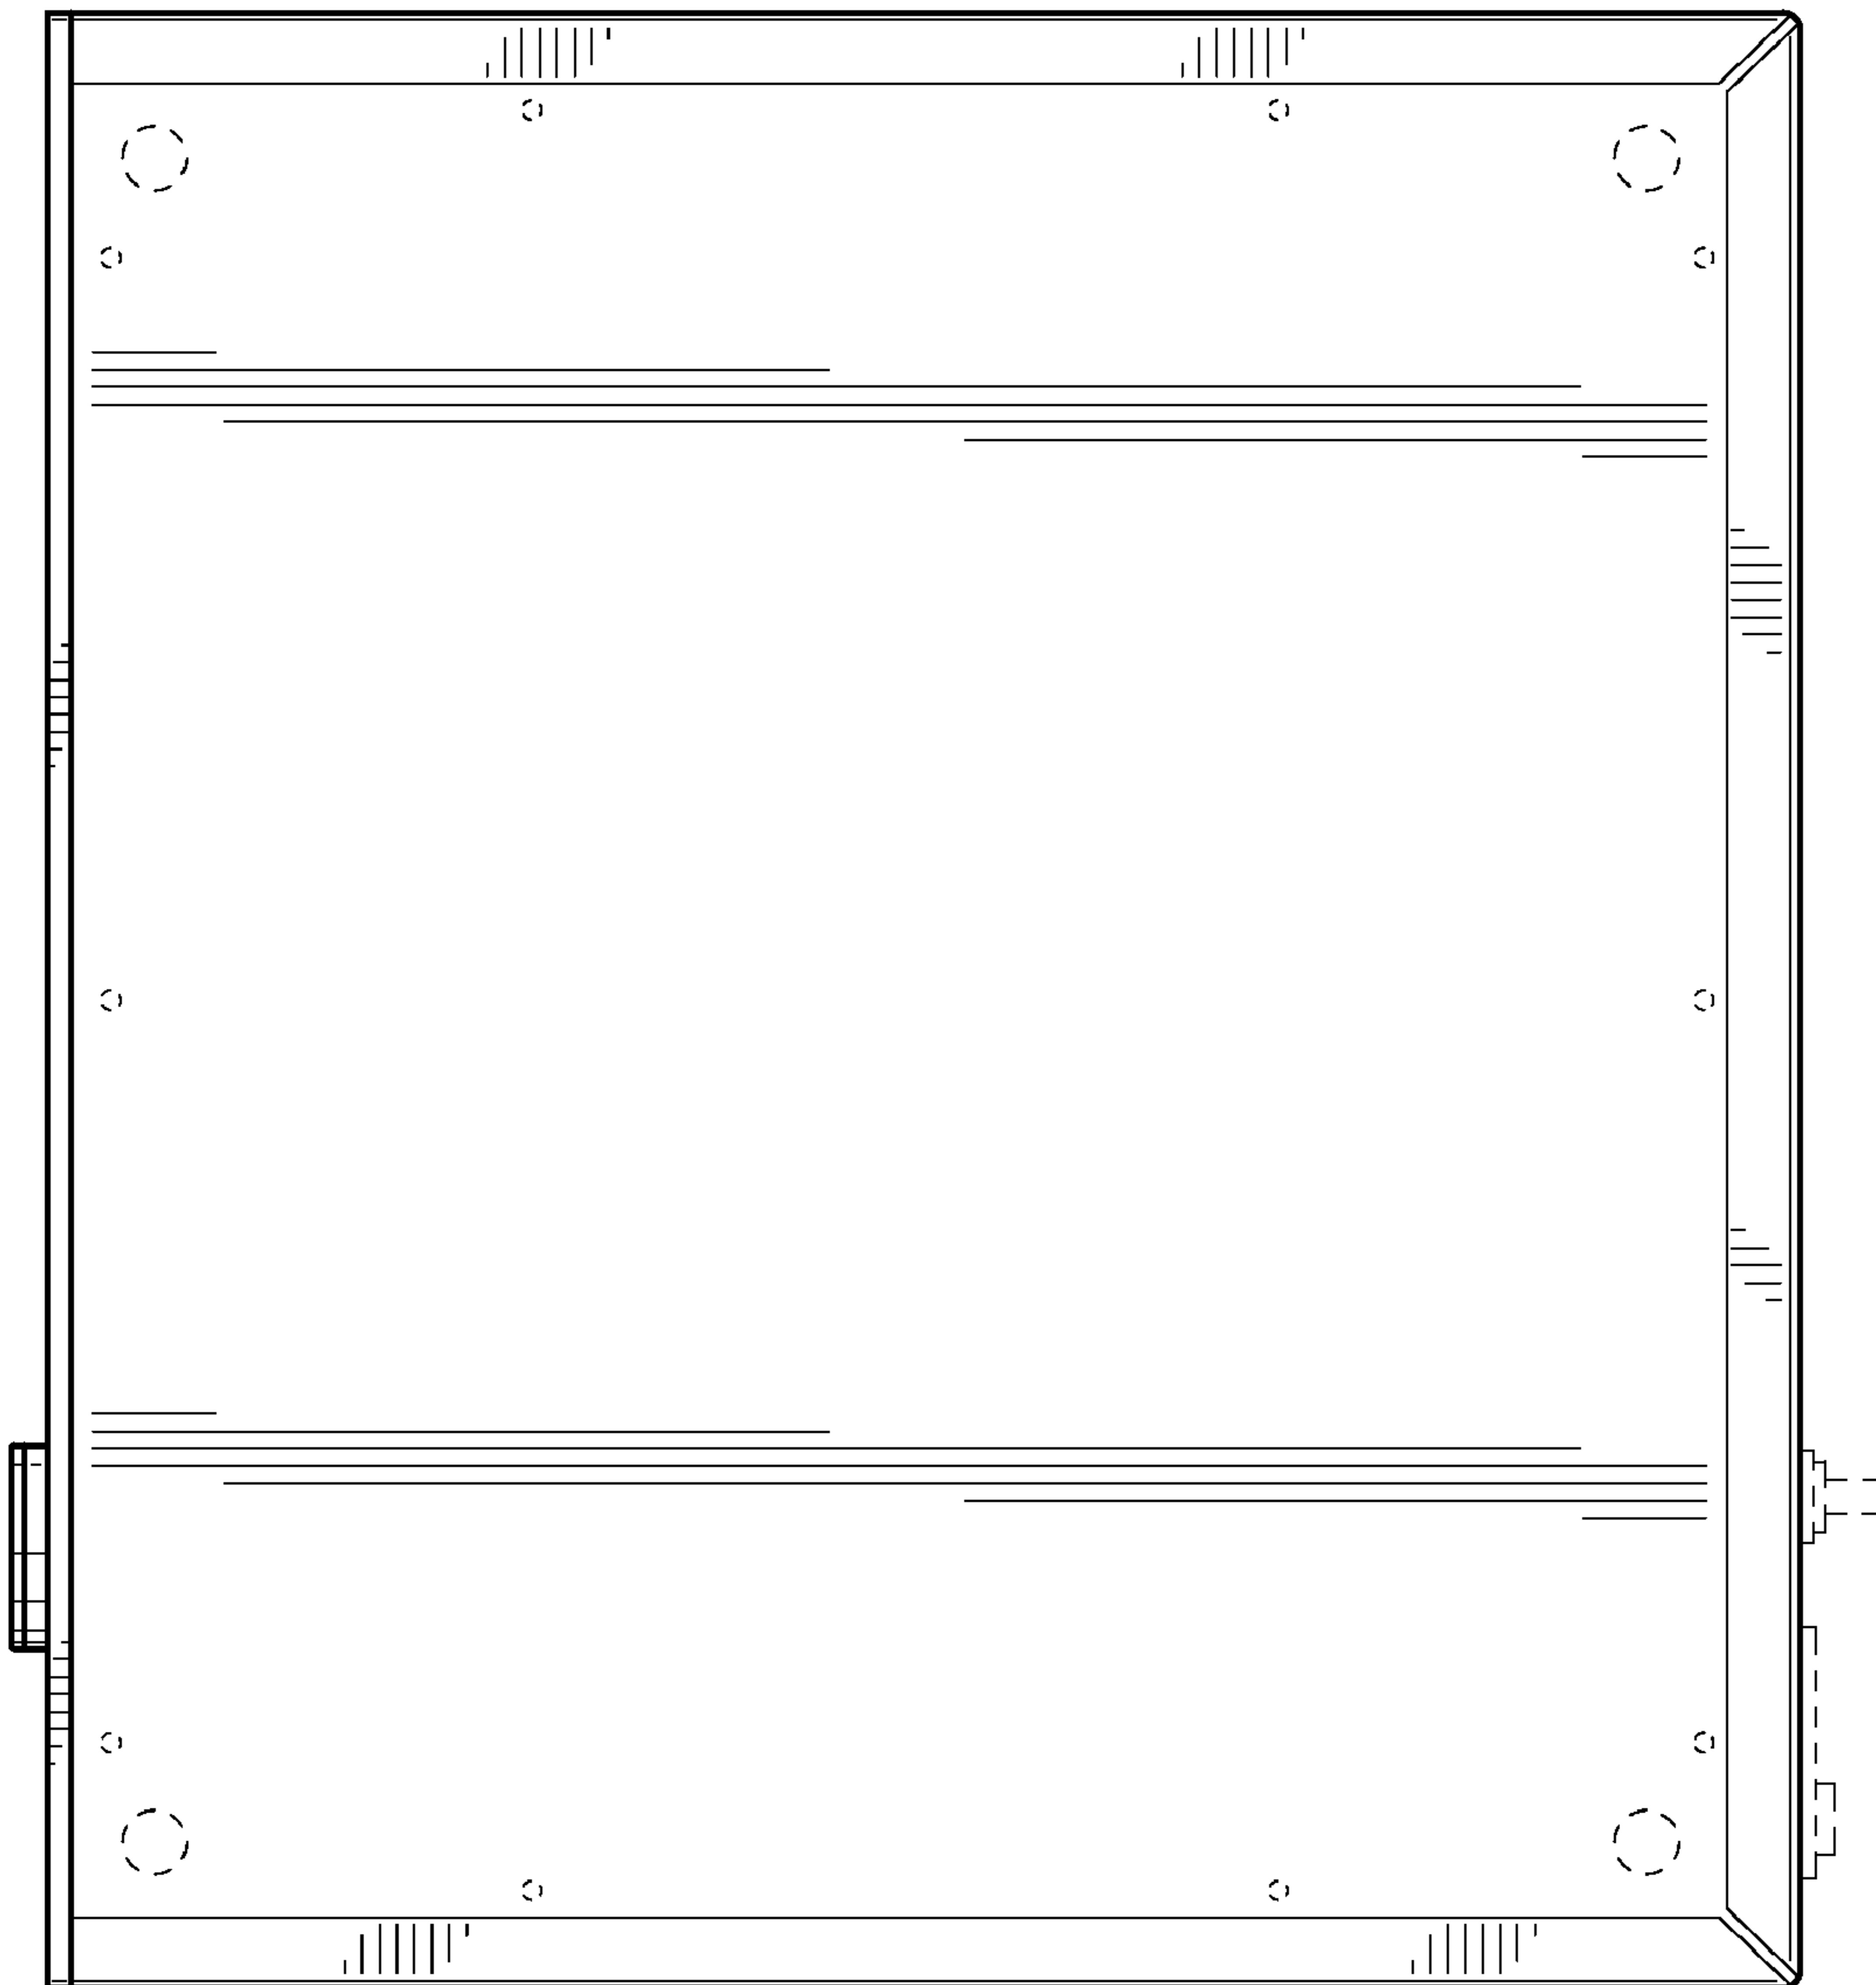


FIG. 14

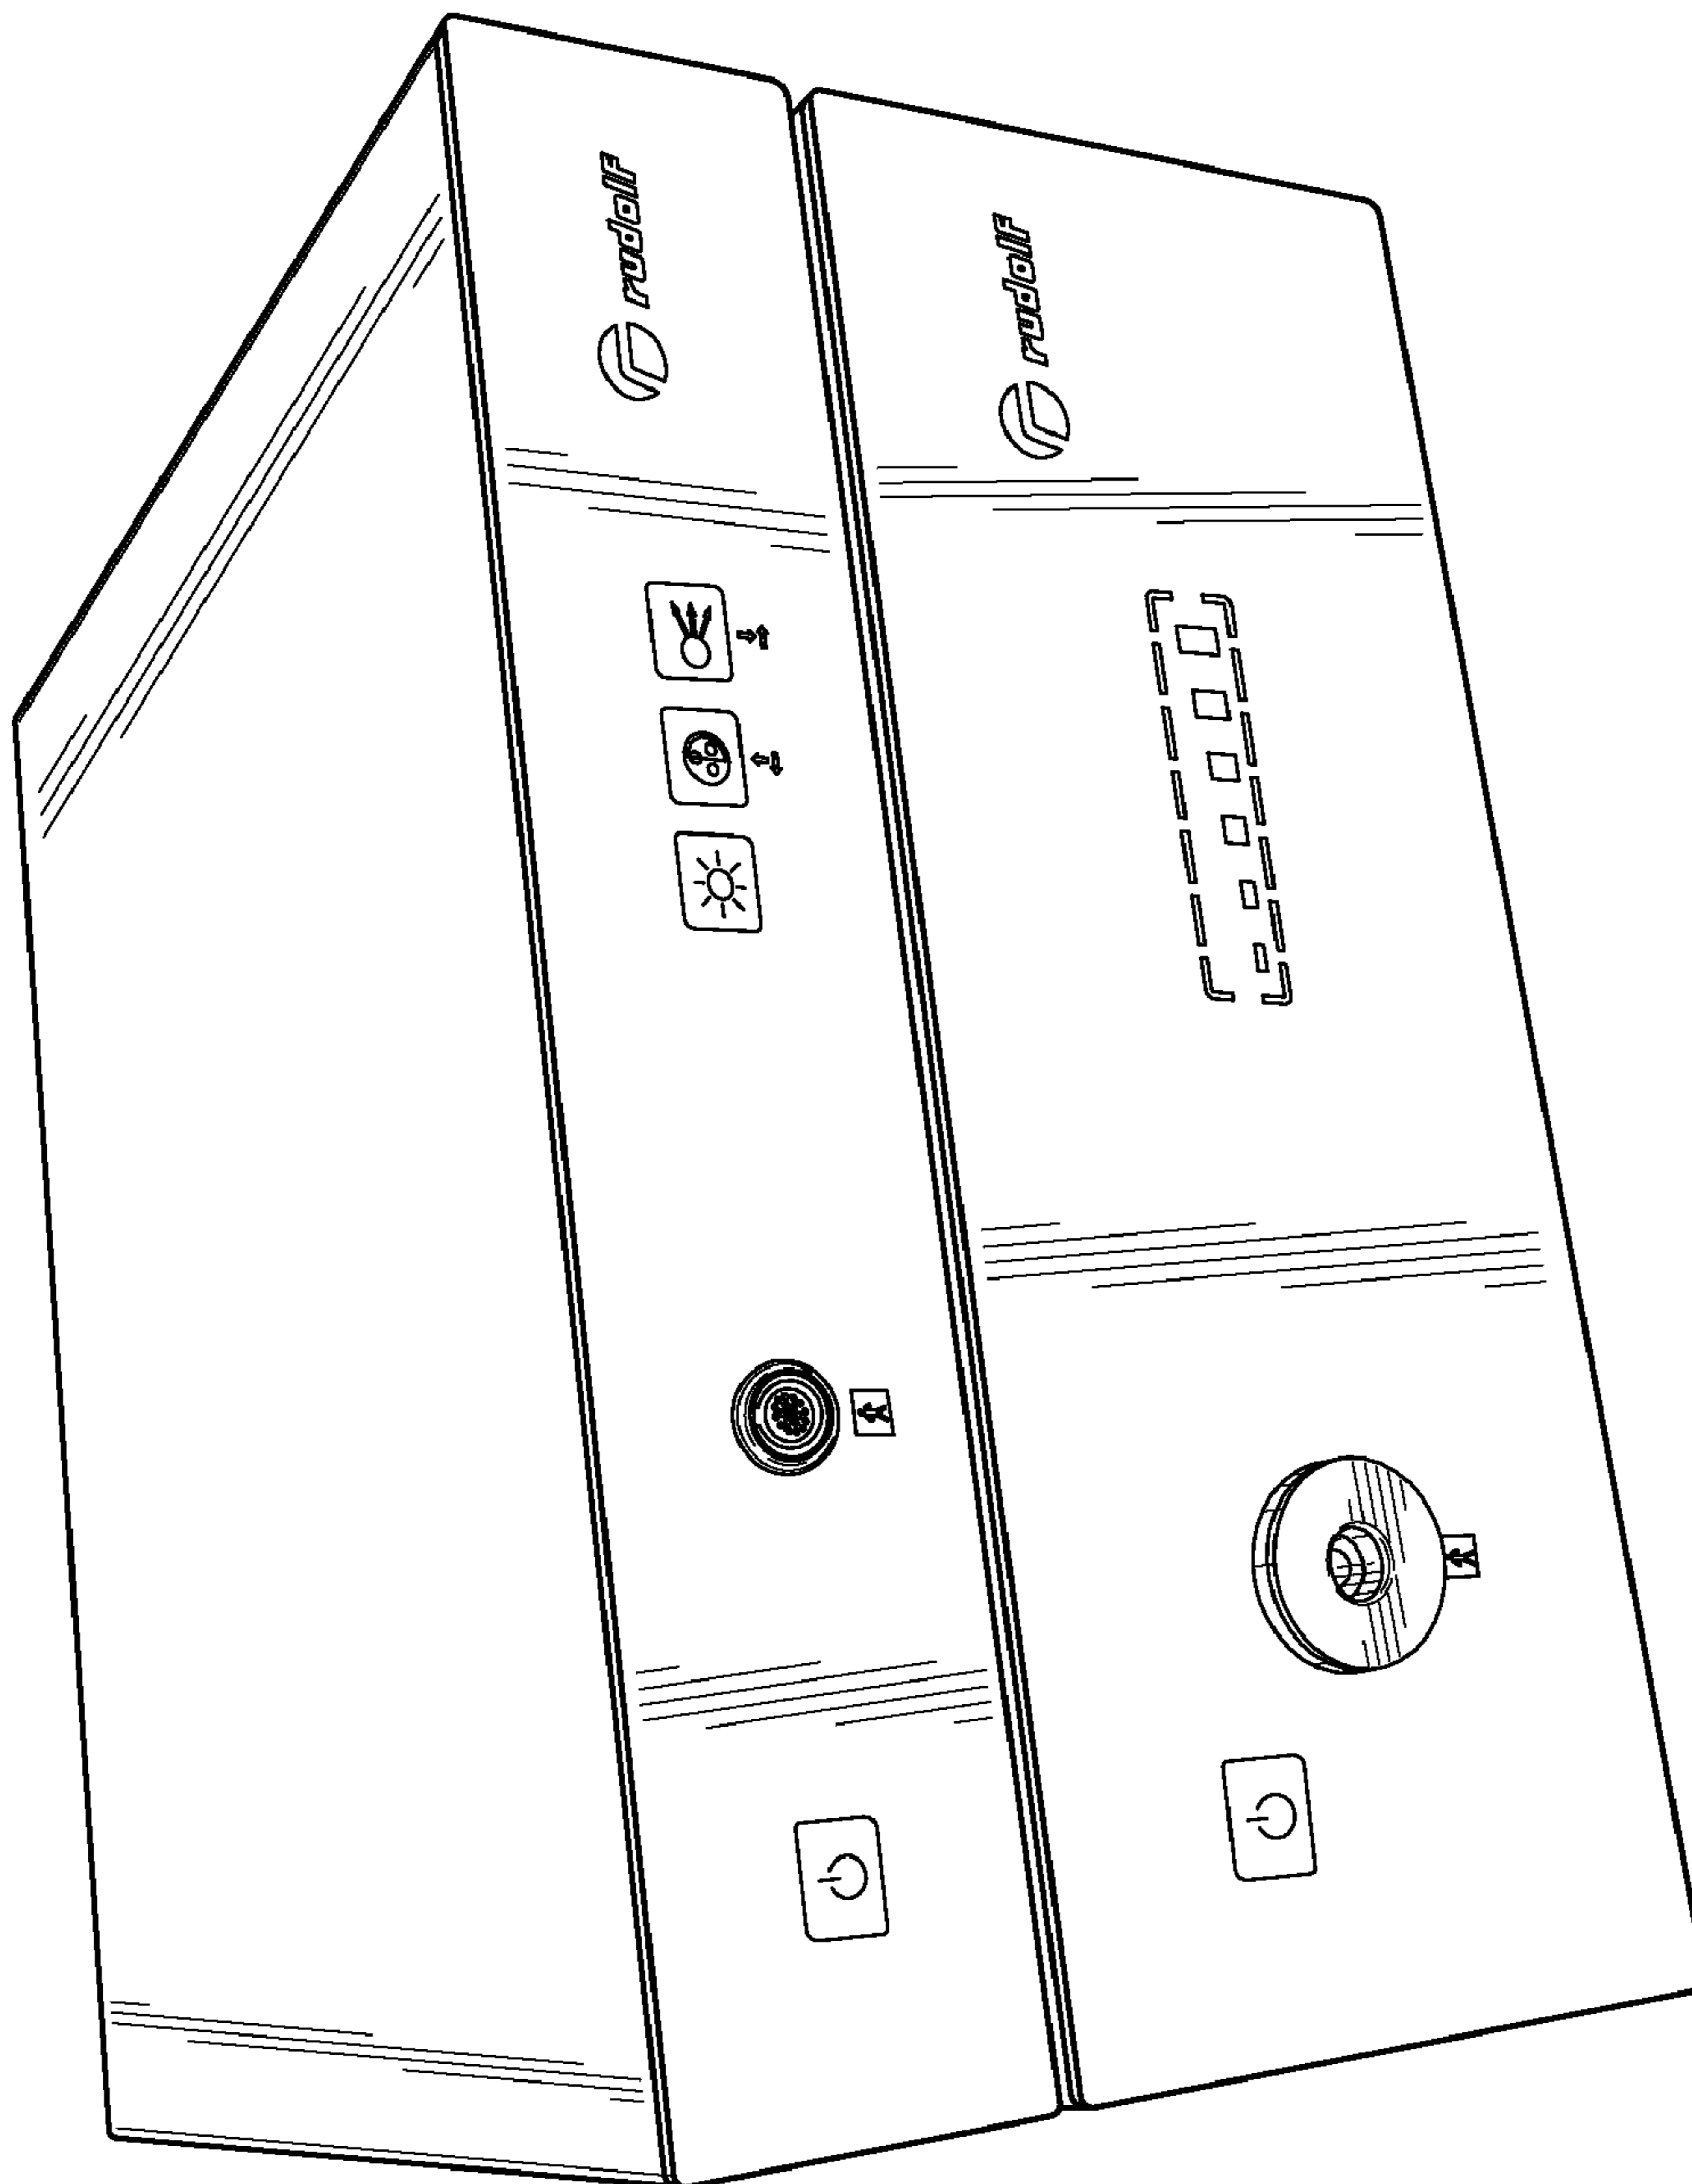


FIG. 15

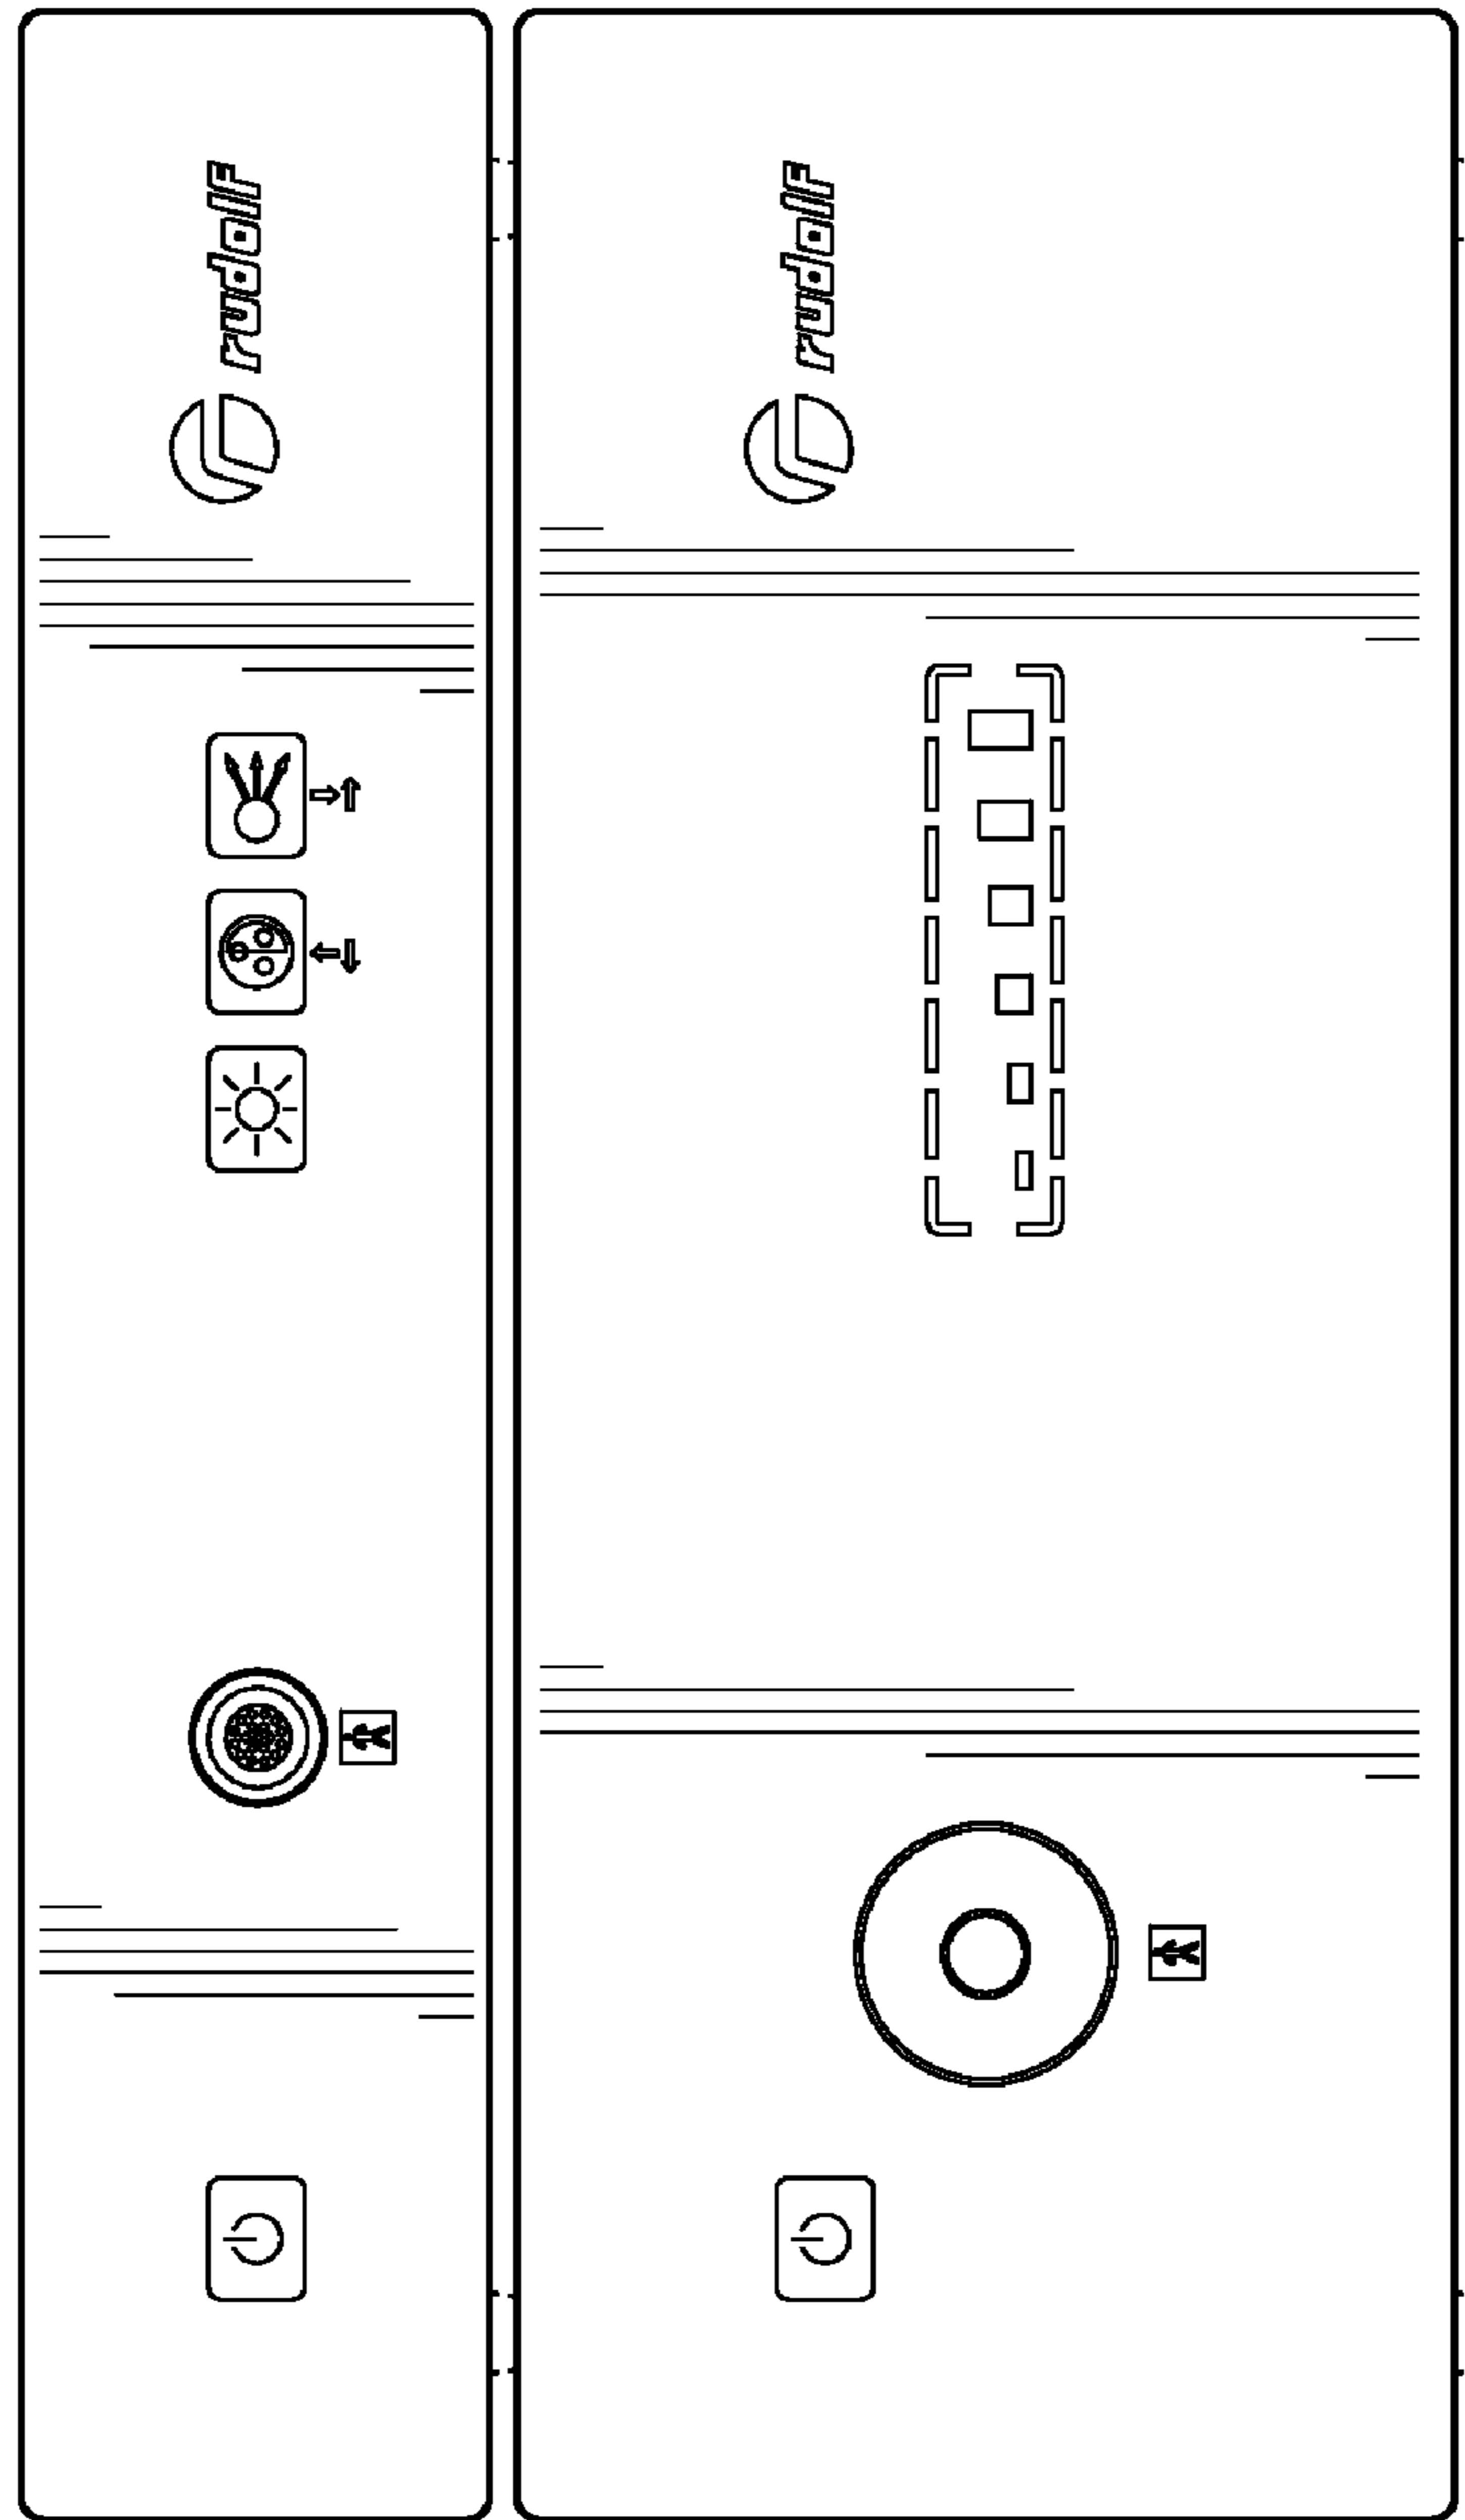


FIG. 16

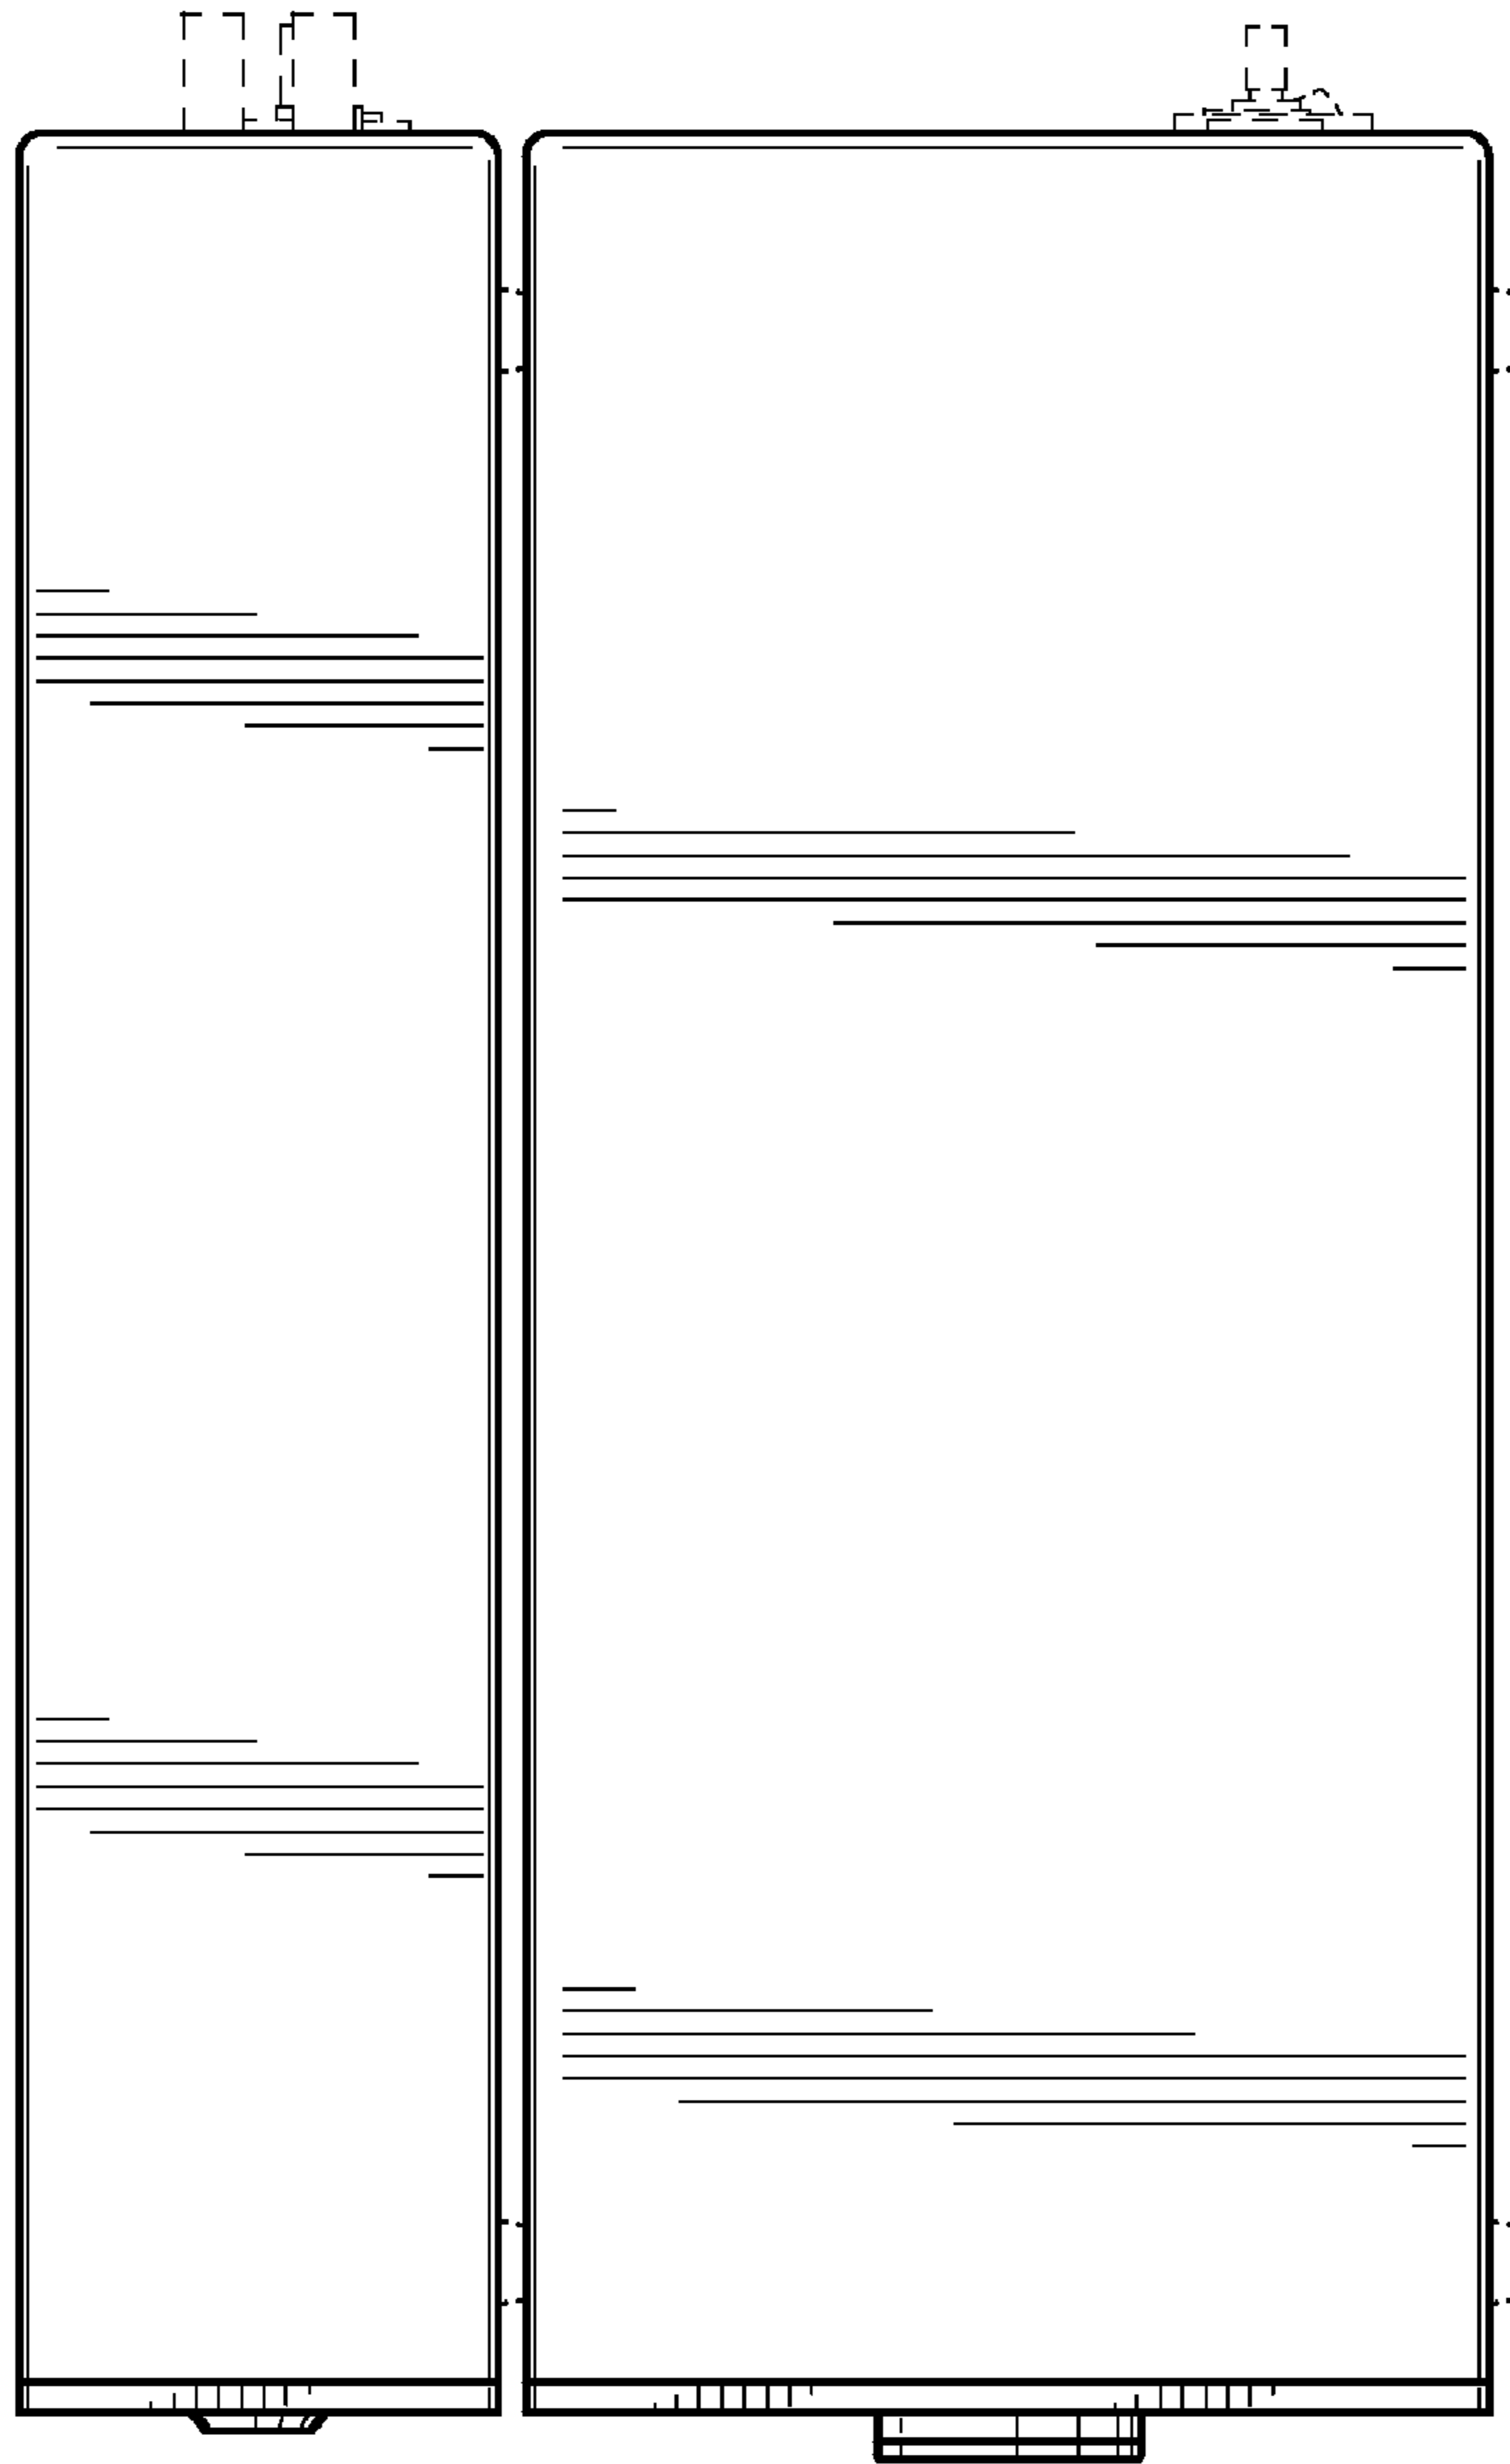


FIG. 17

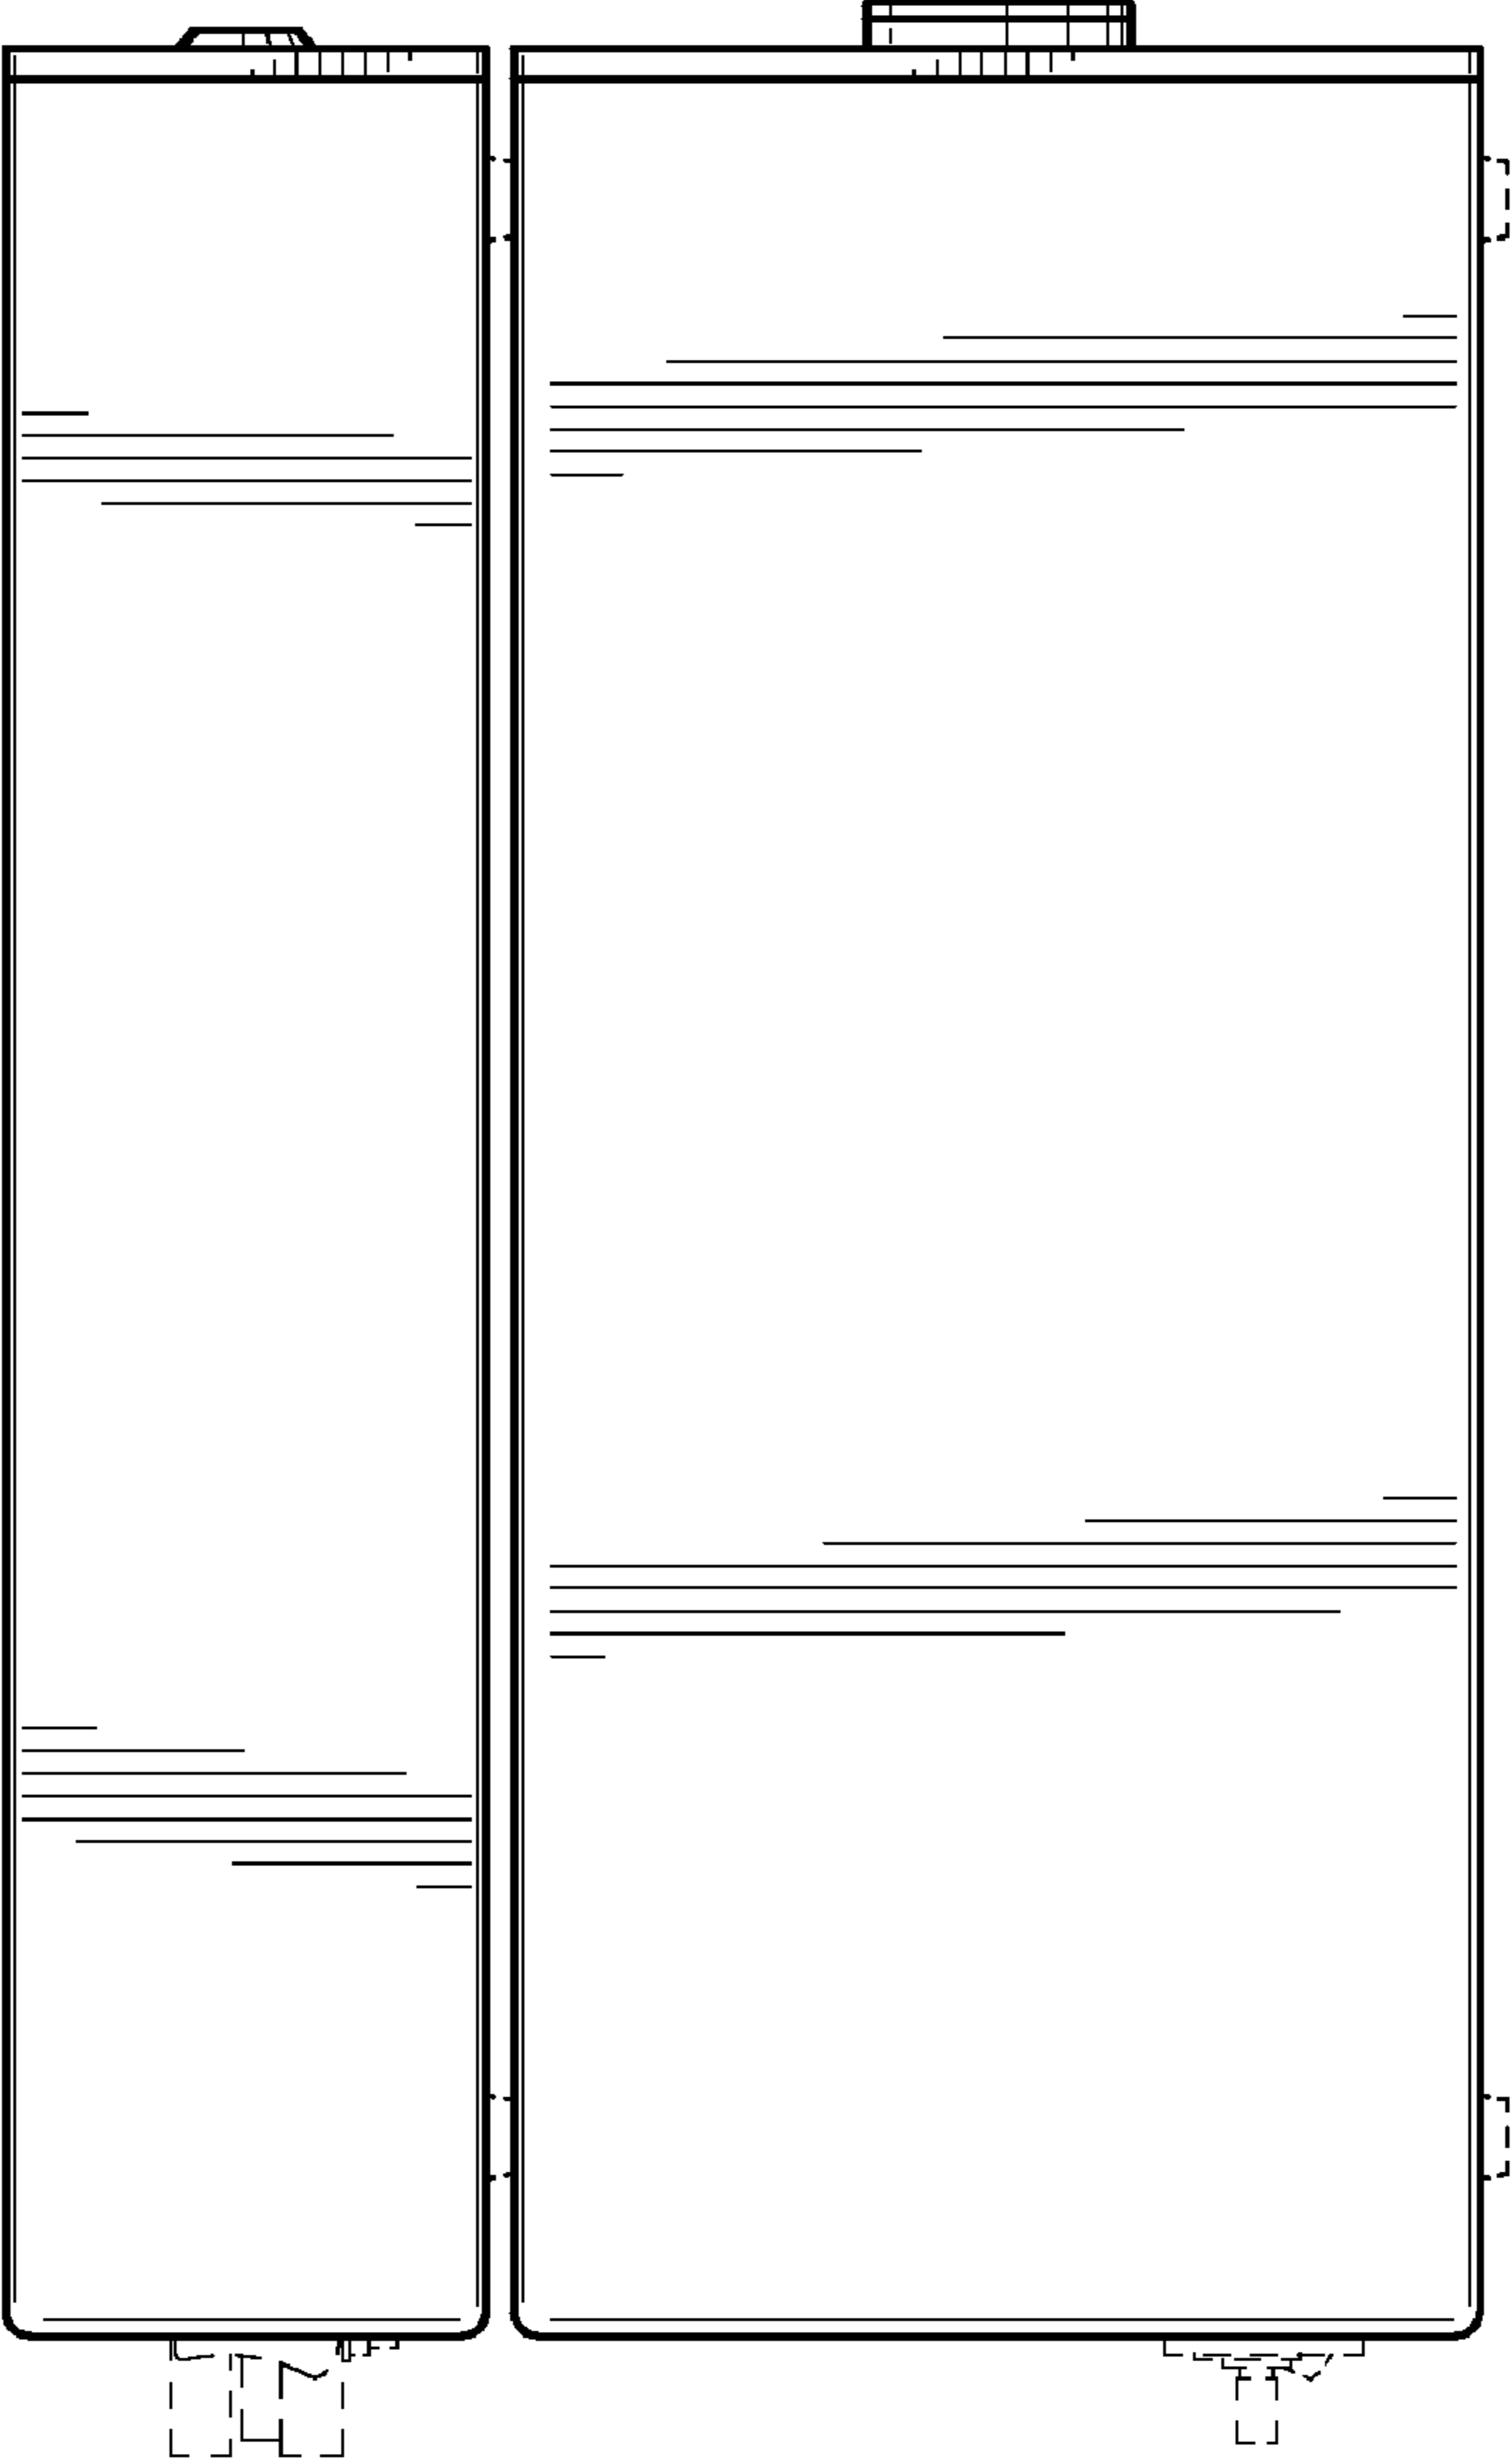


FIG. 18

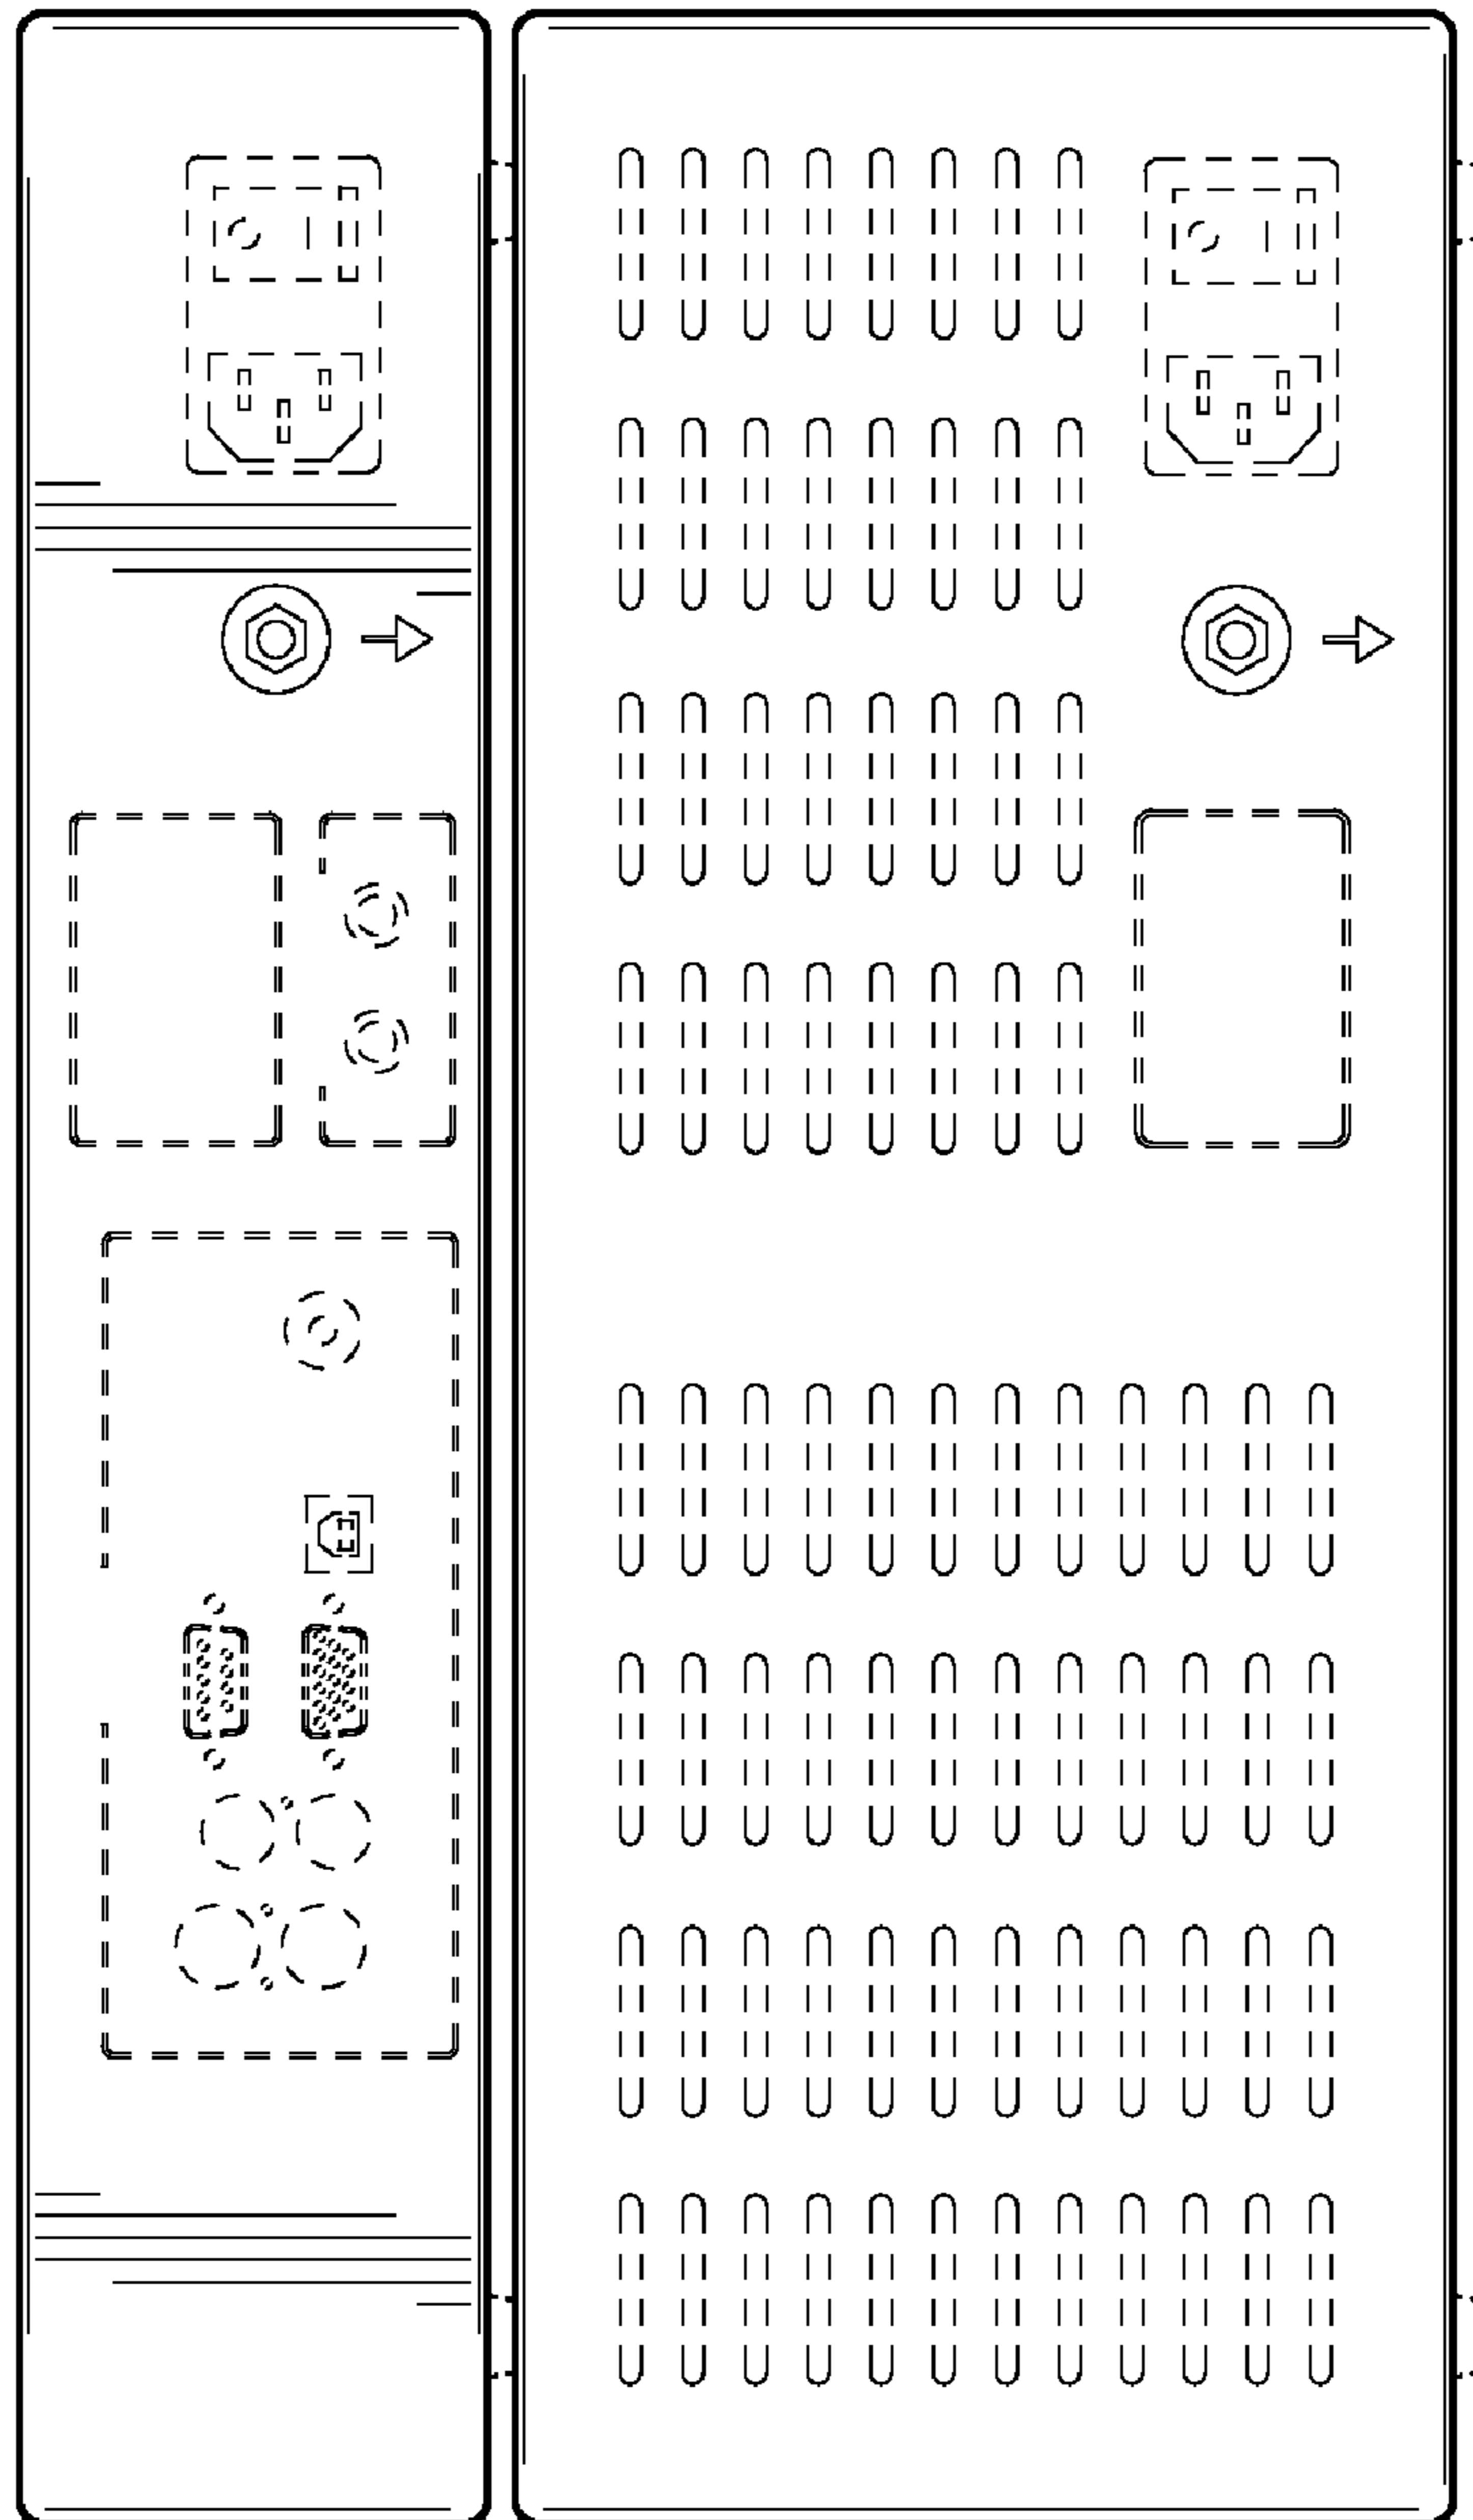


FIG. 19




FIG. 20

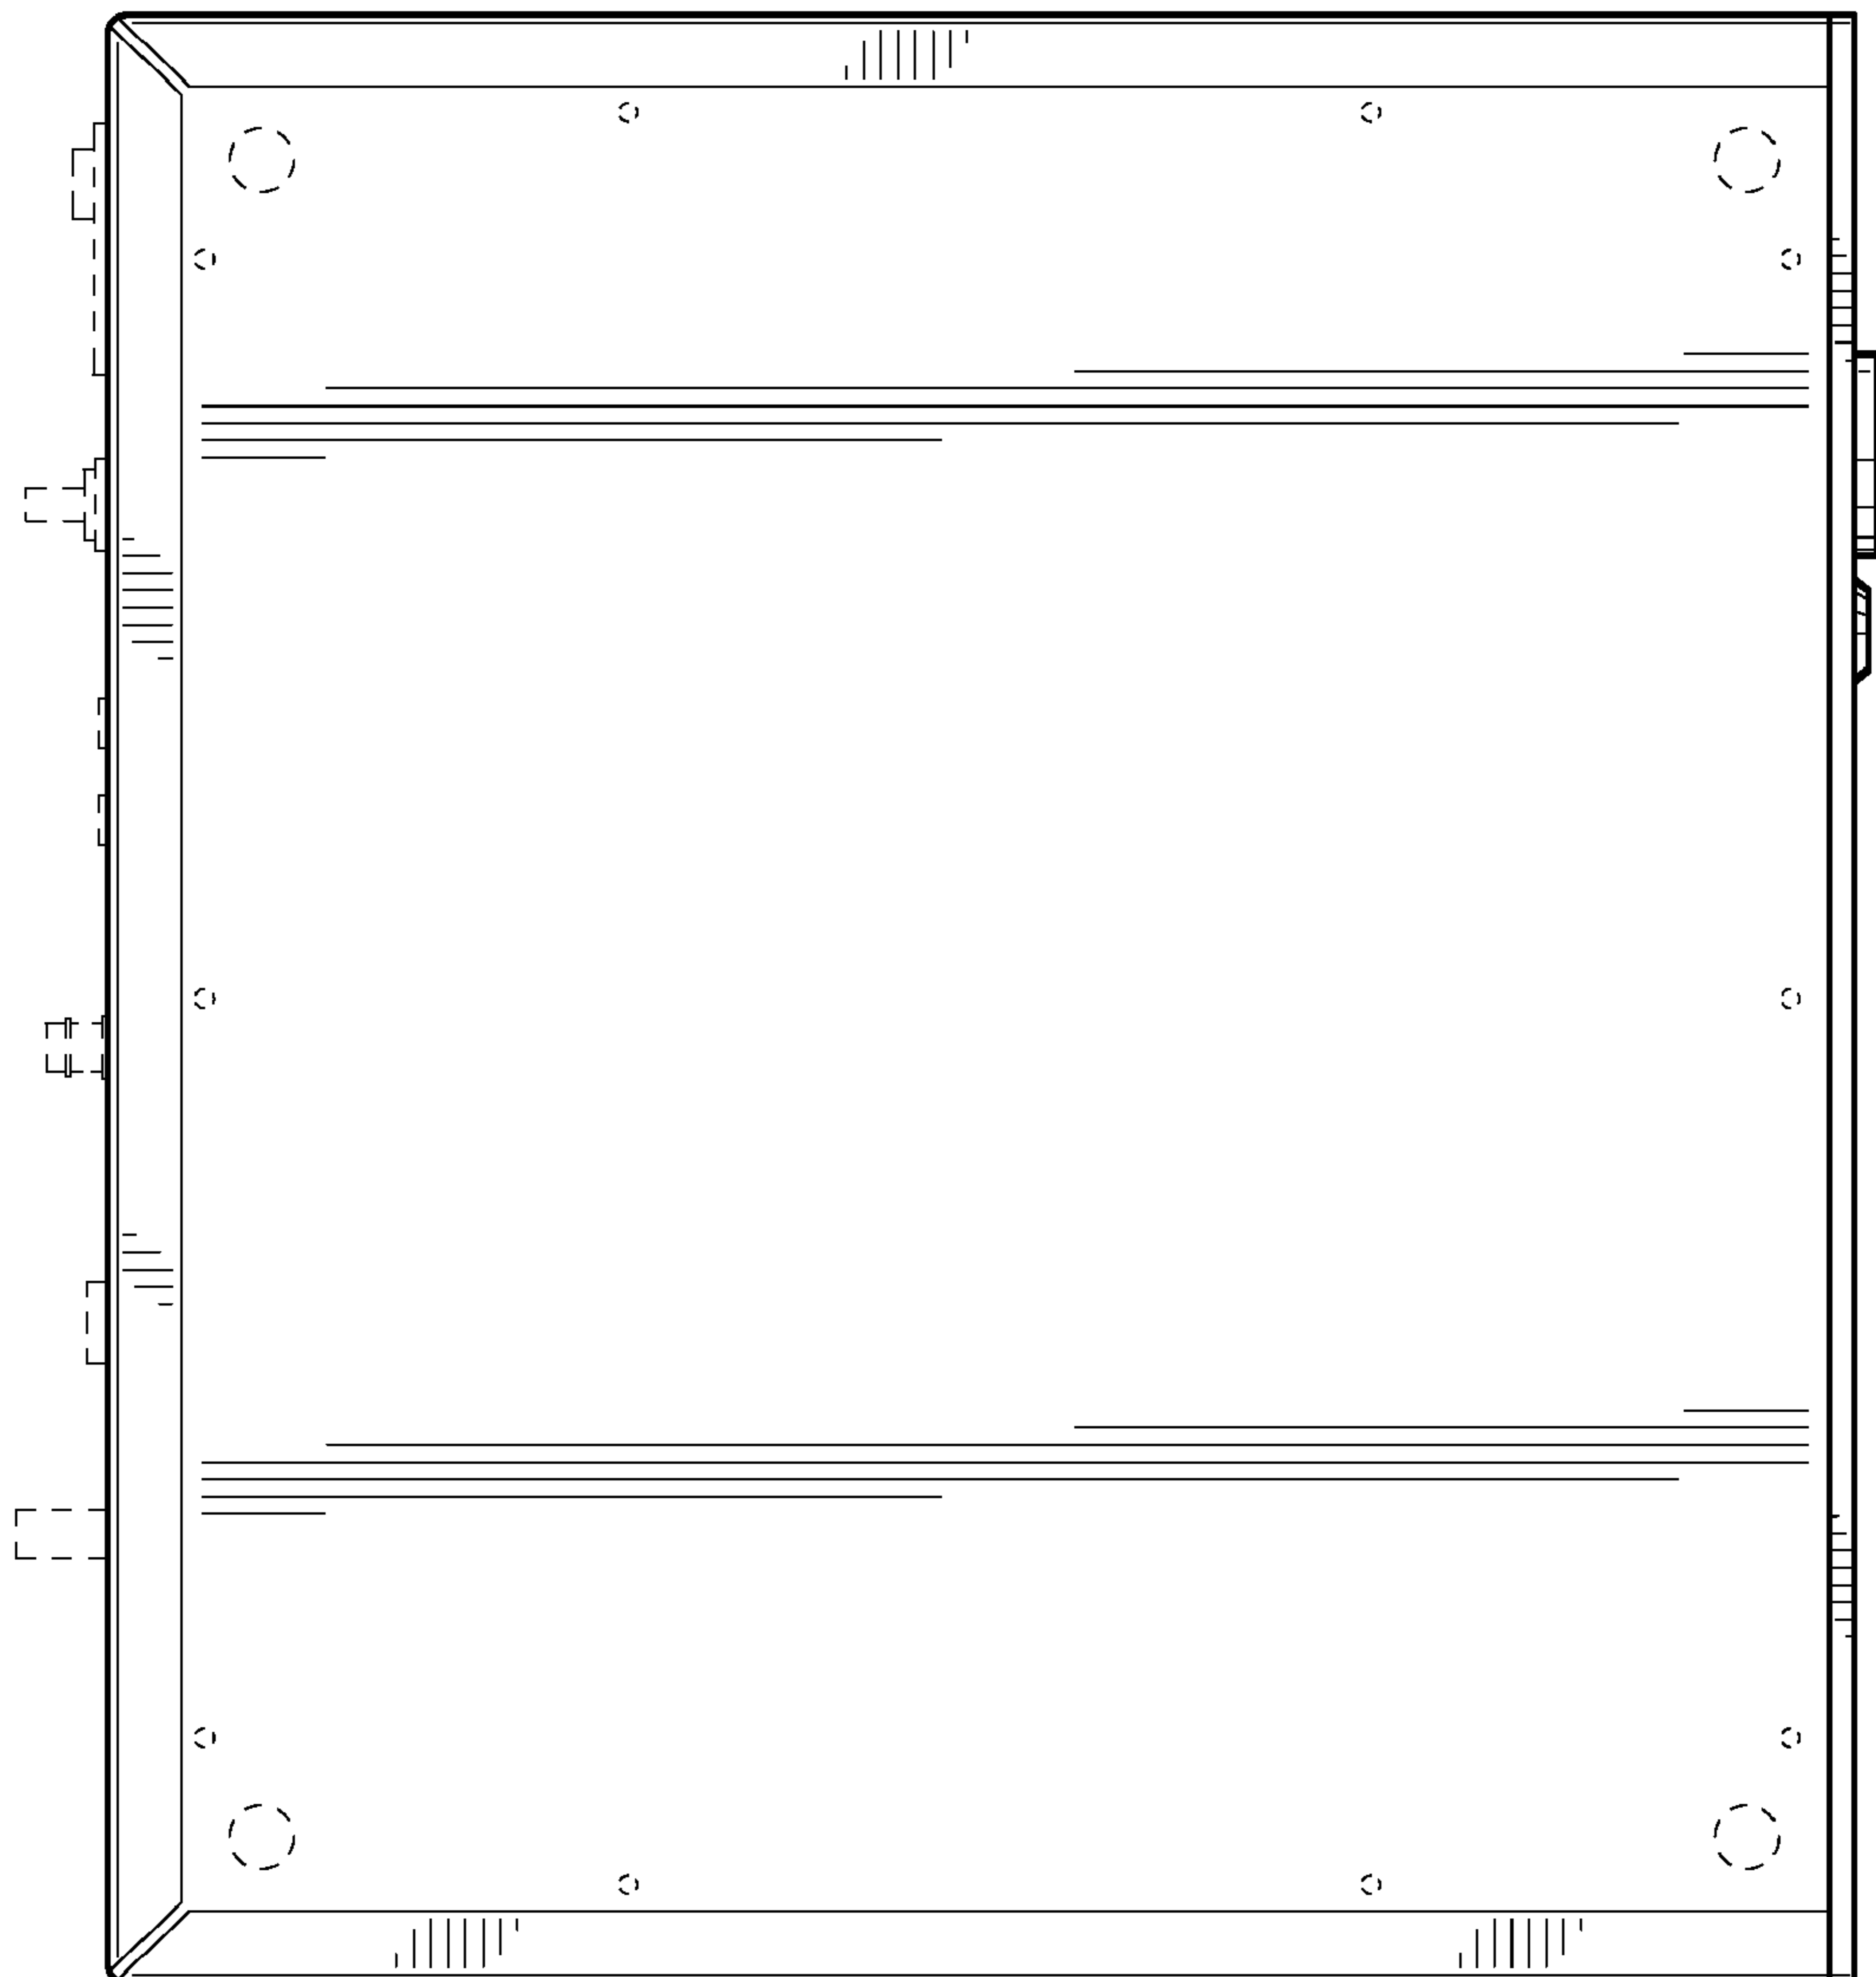


FIG. 21