



US00D630322S

(12) **United States Design Patent**
Speiser

(10) **Patent No.:** **US D630,322 S**

(45) **Date of Patent:** **** Jan. 4, 2011**

(54) **MEDICAL INSTRUMENT**

(75) Inventor: **Bjoern Speiser**, Rottweil (DE)

(73) Assignee: **Karl Storz GmbH & Co. KG**,
Tuttlingen (DE)

(**) Term: **14 Years**

(21) Appl. No.: **29/350,534**

(22) Filed: **Nov. 18, 2009**

(30) **Foreign Application Priority Data**

May 18, 2009 (EM) 001516550-0017

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/133**

(58) **Field of Classification Search** D24/133,
D24/134, 135, 136, 137, 138, 139, 140, 141,
D24/142, 143, 146, 150, 152, 144, 145, 147,
D24/148, 149, 151, 153, 154, 127, 128, 129,
D24/130, 106-108, 112, 111, 200; D23/233,
D23/235; D8/40, 47, 57, 60, 67, 68, 69,
D8/80, 82, 83, 84, 93, 94, 97, 107; 600/184,
600/201-203, 210-218, 220-223, 224, 225-227;
606/7, 86 A, 86 B, 119

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D274,096 S * 5/1984 Shutt D24/143
D289,437 S * 4/1987 Honkanen D24/148
D308,576 S * 6/1990 Iversen D24/129
D338,065 S * 8/1993 Rose D24/143
5,342,381 A * 8/1994 Tidemand 606/174
D357,980 S * 5/1995 Ek et al. D24/143
D362,908 S * 10/1995 Shutt et al. D24/143
5,562,699 A * 10/1996 Heimberger et al. 606/205
5,613,977 A * 3/1997 Weber et al. 606/170

5,658,281 A * 8/1997 Heard 606/48
6,139,563 A * 10/2000 Cosgrove et al. 606/205
6,340,365 B2 * 1/2002 Dittrich et al. 606/205

(Continued)

FOREIGN PATENT DOCUMENTS

EM 000324074-0001 * 4/2005

(Continued)

Primary Examiner—Bridget L Eland

(74) *Attorney, Agent, or Firm*—Muncy, Geissler, Olds &
Lowe, PLLC

(57) **CLAIM**

The ornamental design for a medical instrument, as shown
and described.

DESCRIPTION

FIG. 1 is a left side perspective view of a medical instrument
the present invention.

FIG. 2 is a right side perspective view of the medical instru-
ment of FIG. 1.

FIG. 3 is a top perspective view of the medical instrument of
FIG. 1.

FIG. 4 is a bottom perspective view of the medical instrument
of FIG. 1.


FIG. 5 is a front perspective view of the medical instrument of
FIG. 1.

FIG. 6 is a rear perspective view of the medical instrument of
FIG. 1; and,

FIG. 7 is a three-quarter perspective view of the medical
instrument of FIG. 1.

The broken lines shown at the end of the cord and at the end
of the tubular shaft represent the bounds of the claimed
design; the broken lines form no part of the claimed design.

1 Claim, 7 Drawing Sheets

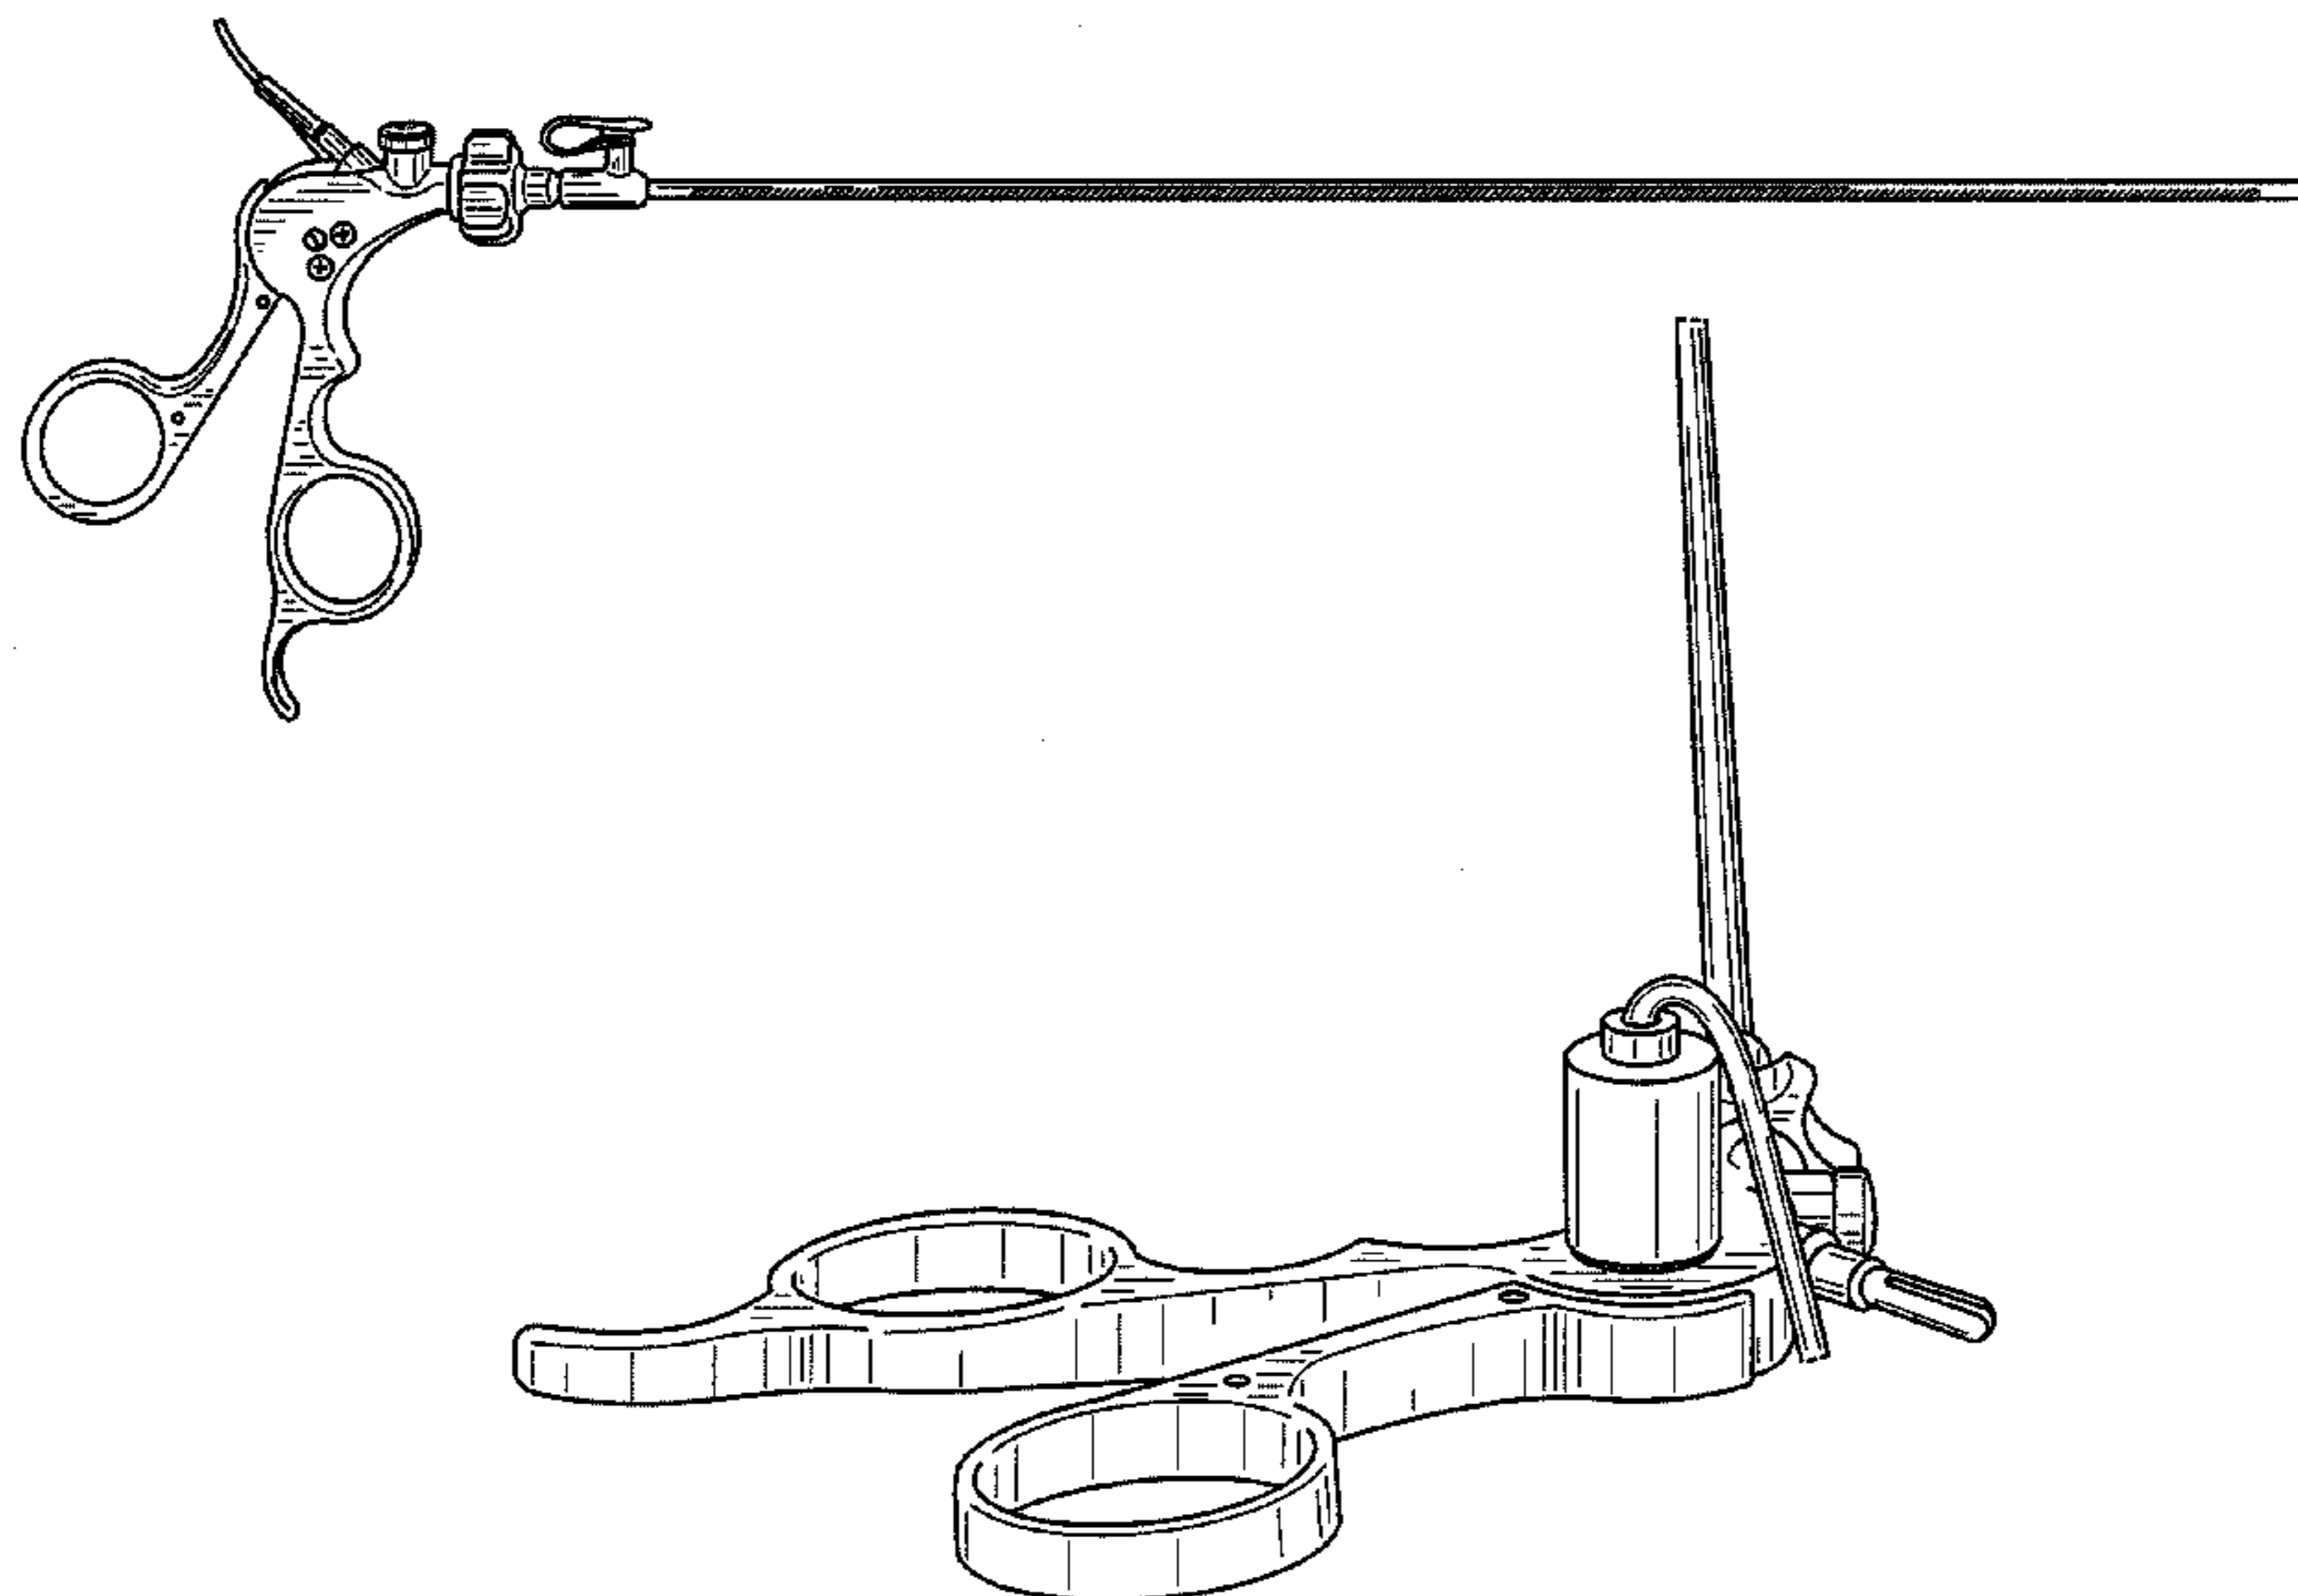

US D630,322 S

Page 2

U.S. PATENT DOCUMENTS

D465,281 S * 11/2002 Lang D24/147
6,752,823 B2 * 6/2004 Prestel 606/208
D498,300 S * 11/2004 Karl-Heinz D24/146
6,896,686 B2 * 5/2005 Weber 606/145
D535,398 S * 1/2007 Stammberger D24/146
D541,416 S * 4/2007 Baehr et al. D24/133
D548,836 S * 8/2007 Lang et al. D24/146
D557,415 S * 12/2007 Bacher D24/133
D583,941 S * 12/2008 Leroy D24/135
D594,982 S * 6/2009 Stefan D24/133

D605,761 S * 12/2009 Stefan D24/143
2005/0143626 A1 * 6/2005 Prescott 600/162
2009/0036745 A1 * 2/2009 Bonadio et al. 600/208
2009/0076521 A1 * 3/2009 Hansen 606/129

FOREIGN PATENT DOCUMENTS

EM 000324074-0003 * 4/2005
EM 001516550-0017 * 5/2009
WO DM/060711 * 6/2002

* cited by examiner

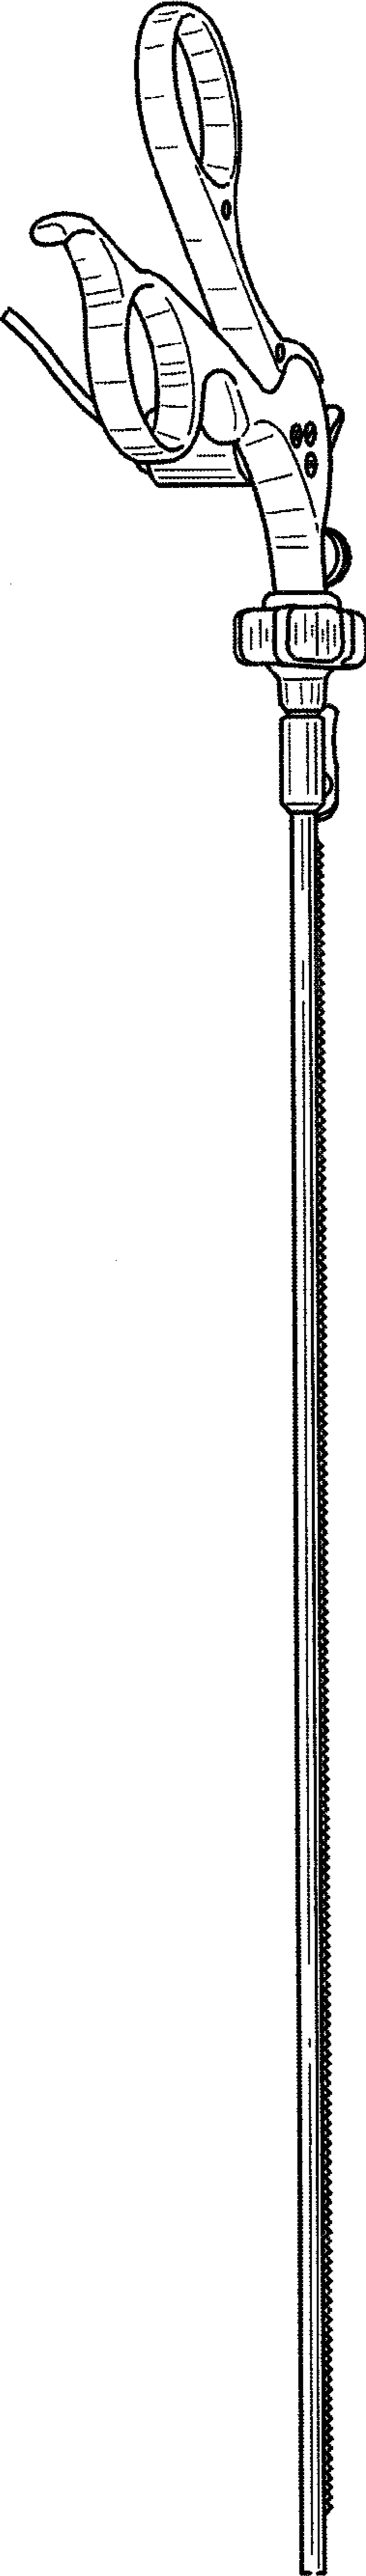


FIG. 1

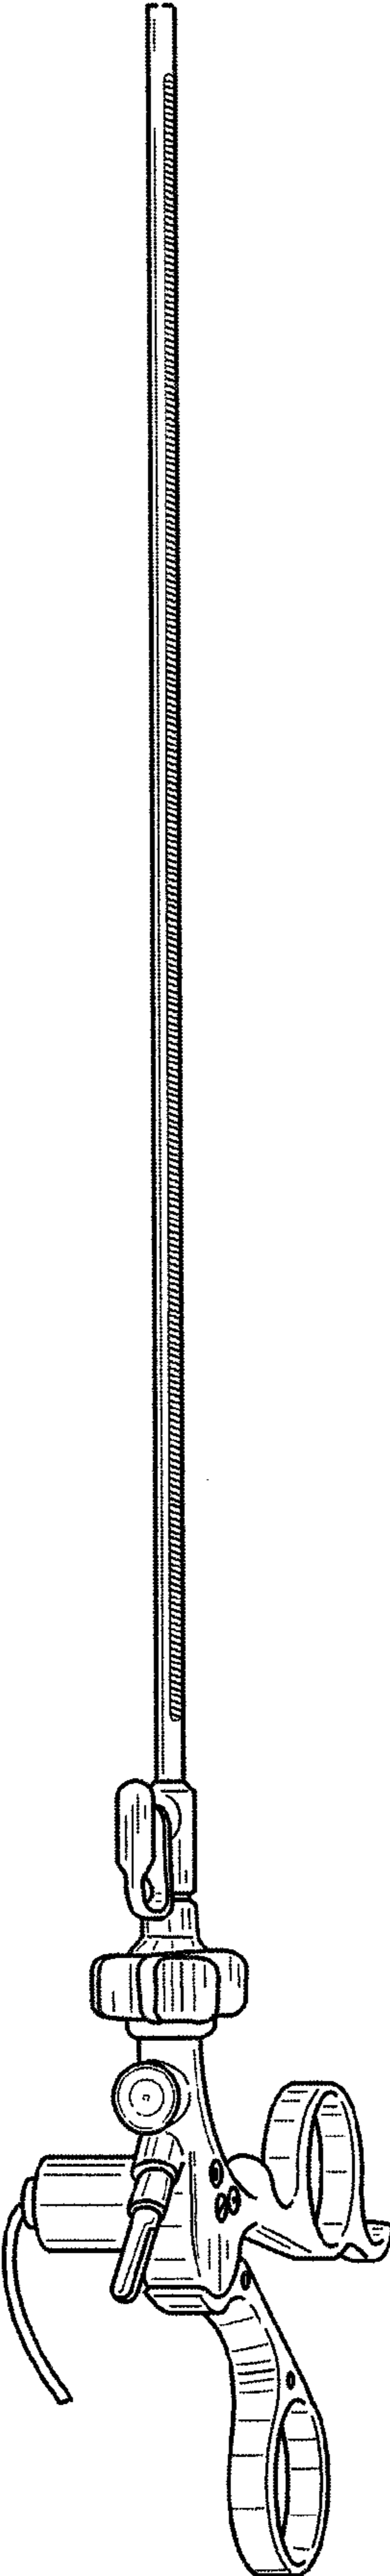


FIG. 2

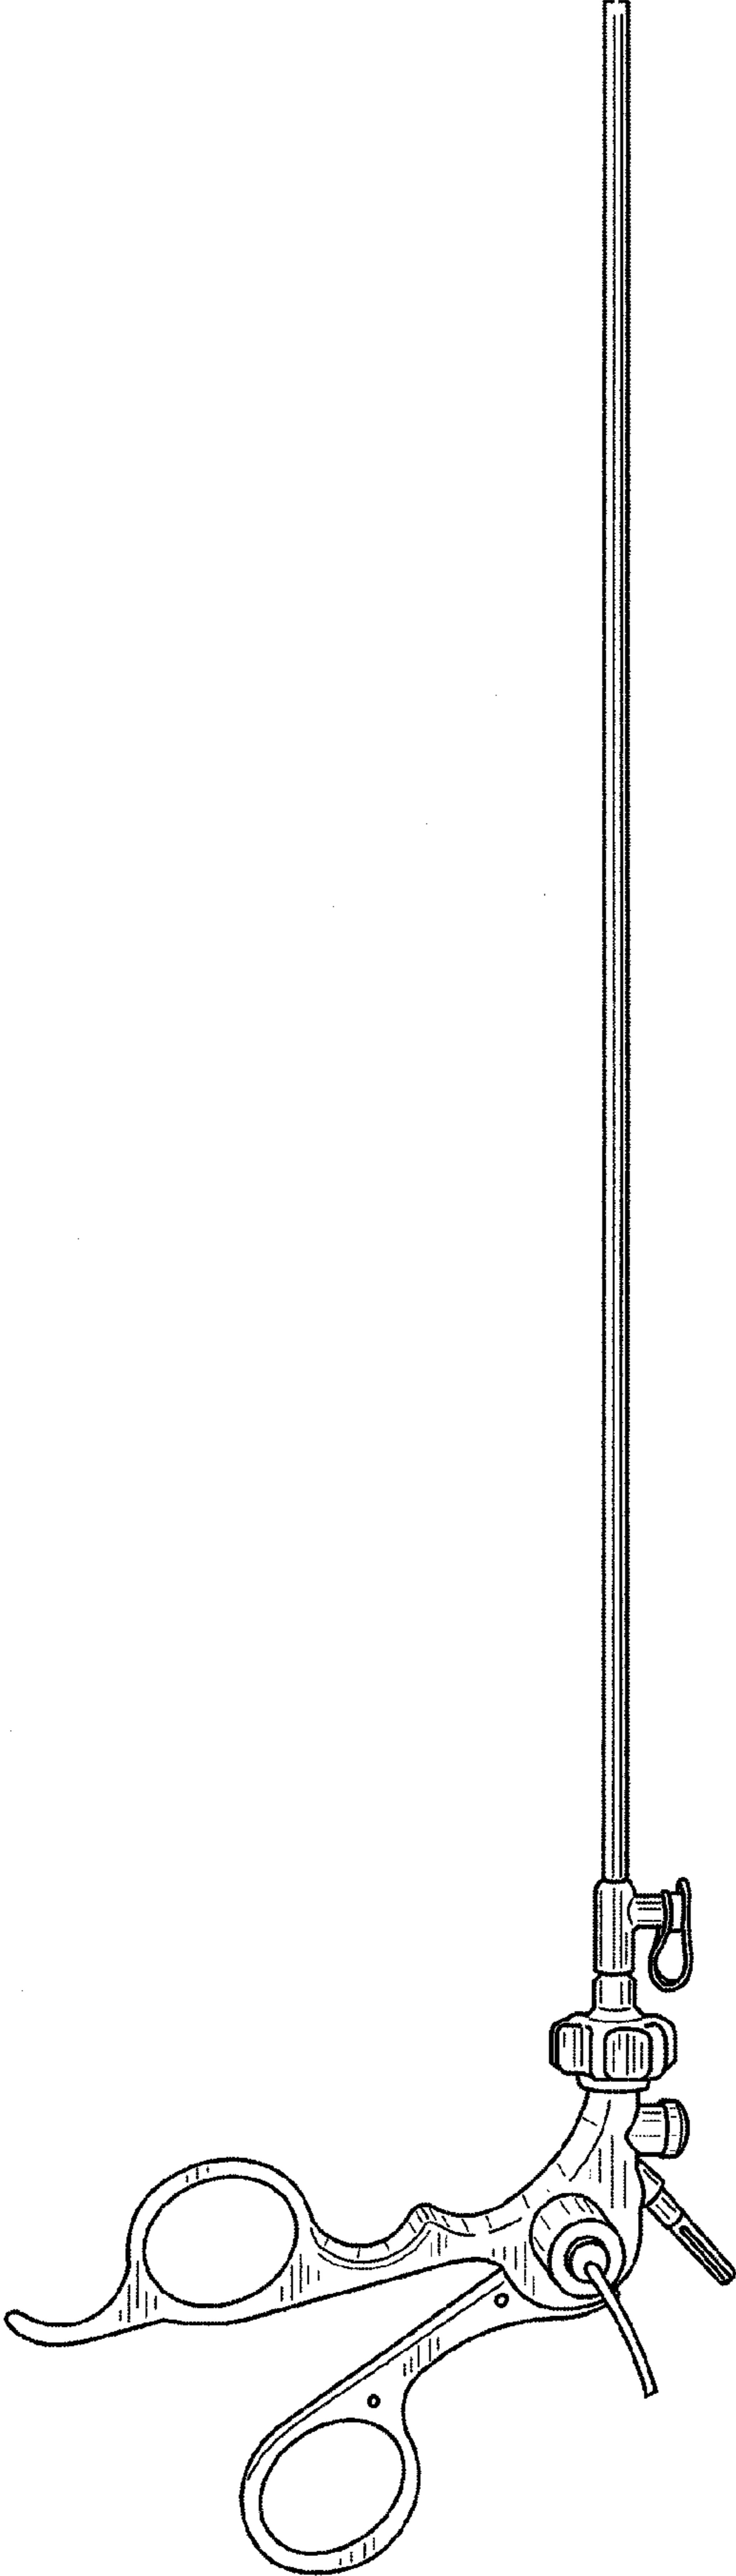


FIG. 3

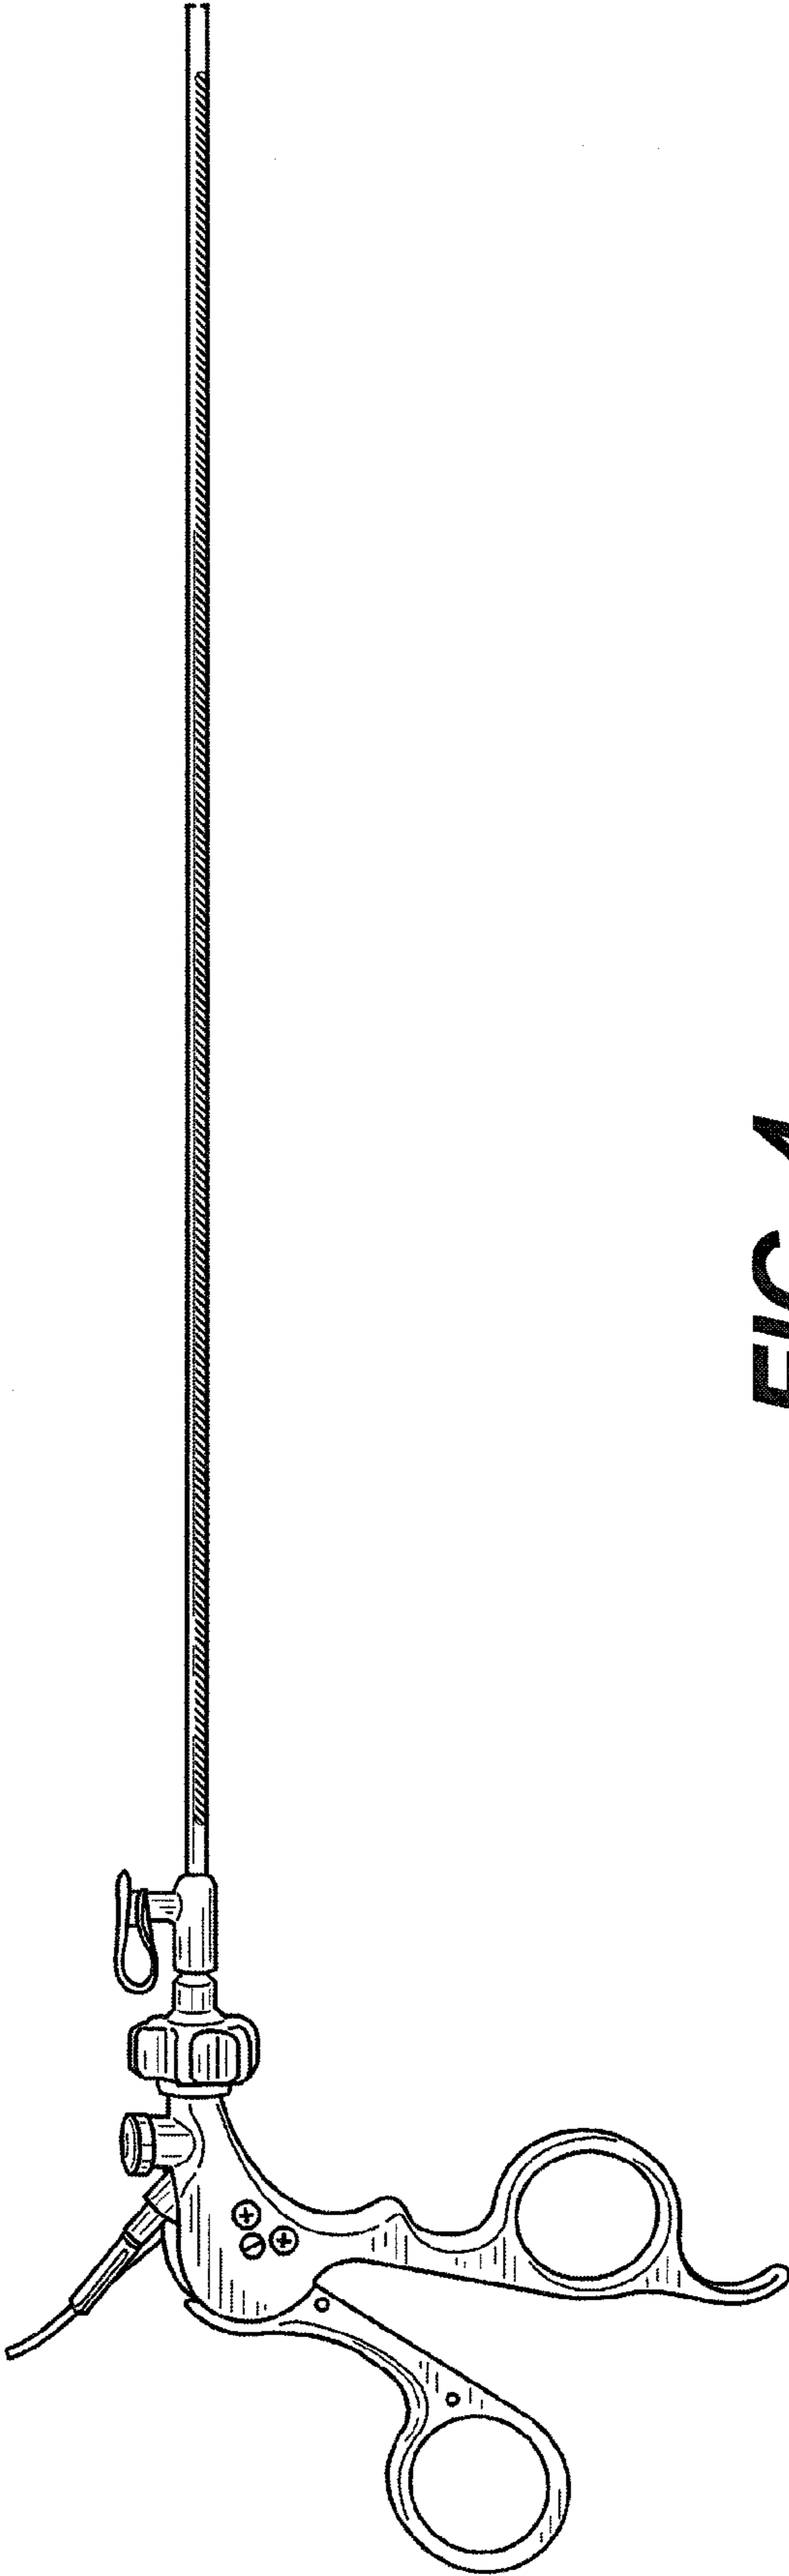


FIG. 4

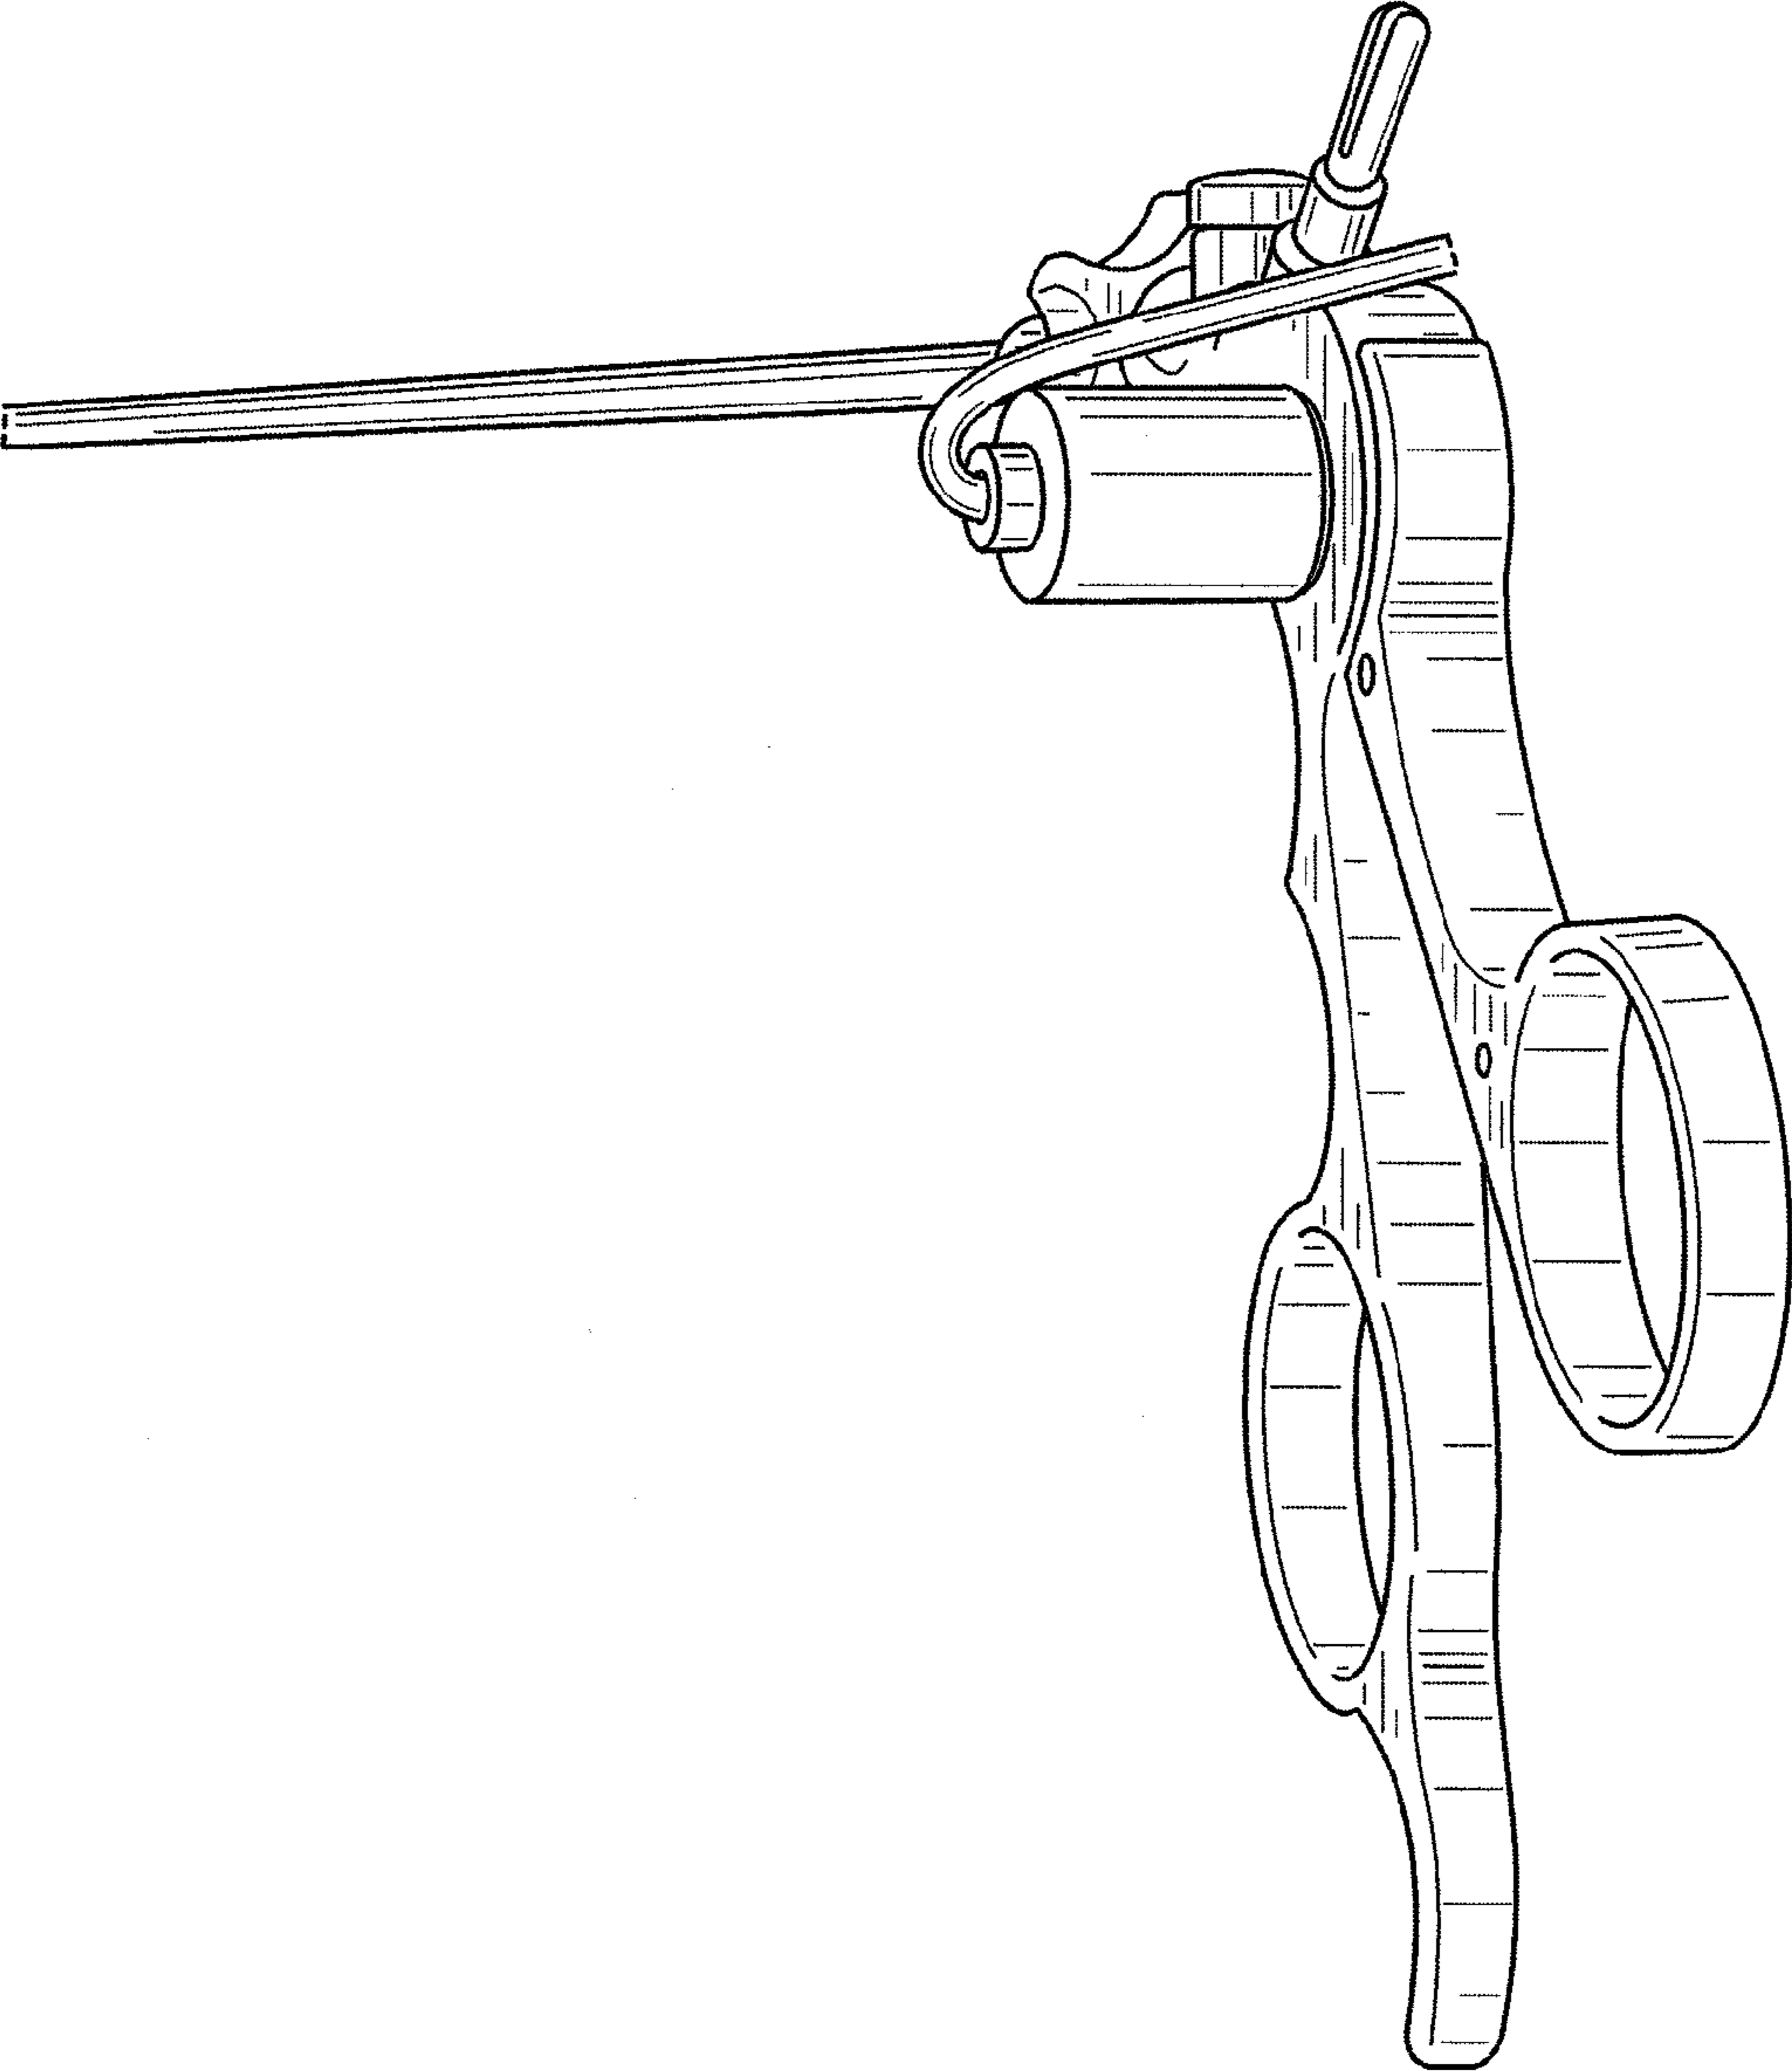


FIG. 5

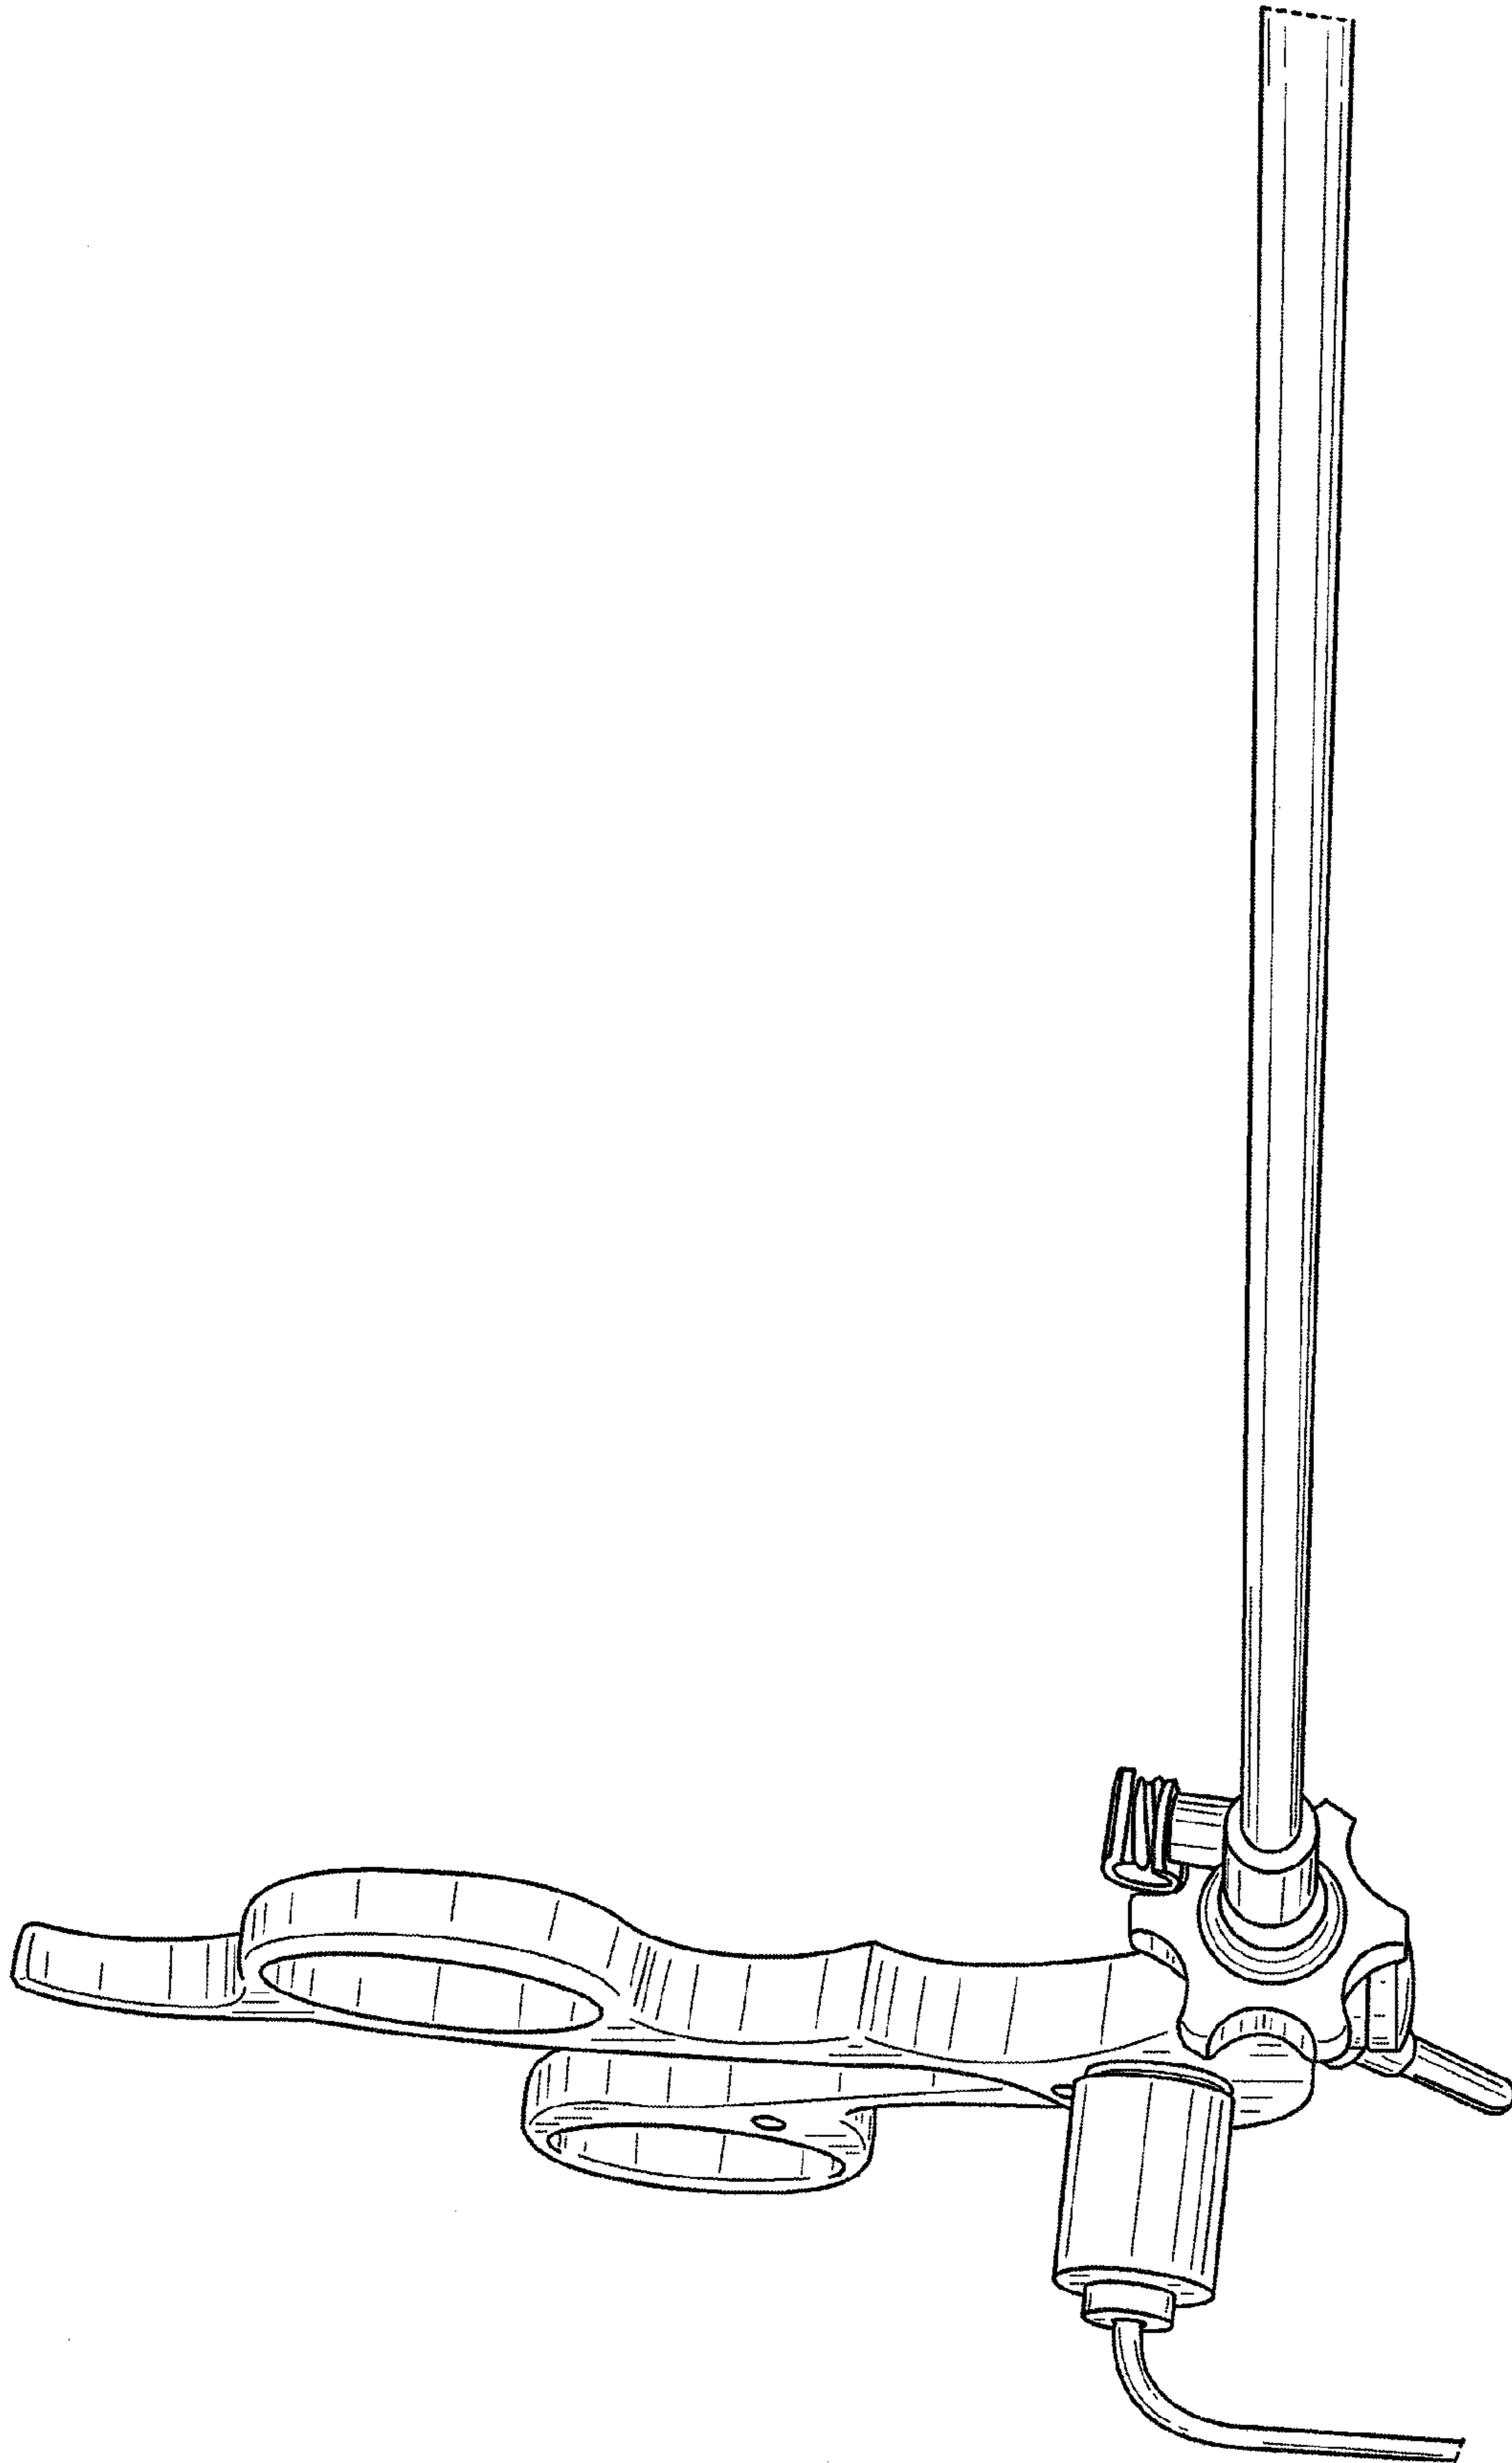


FIG. 6

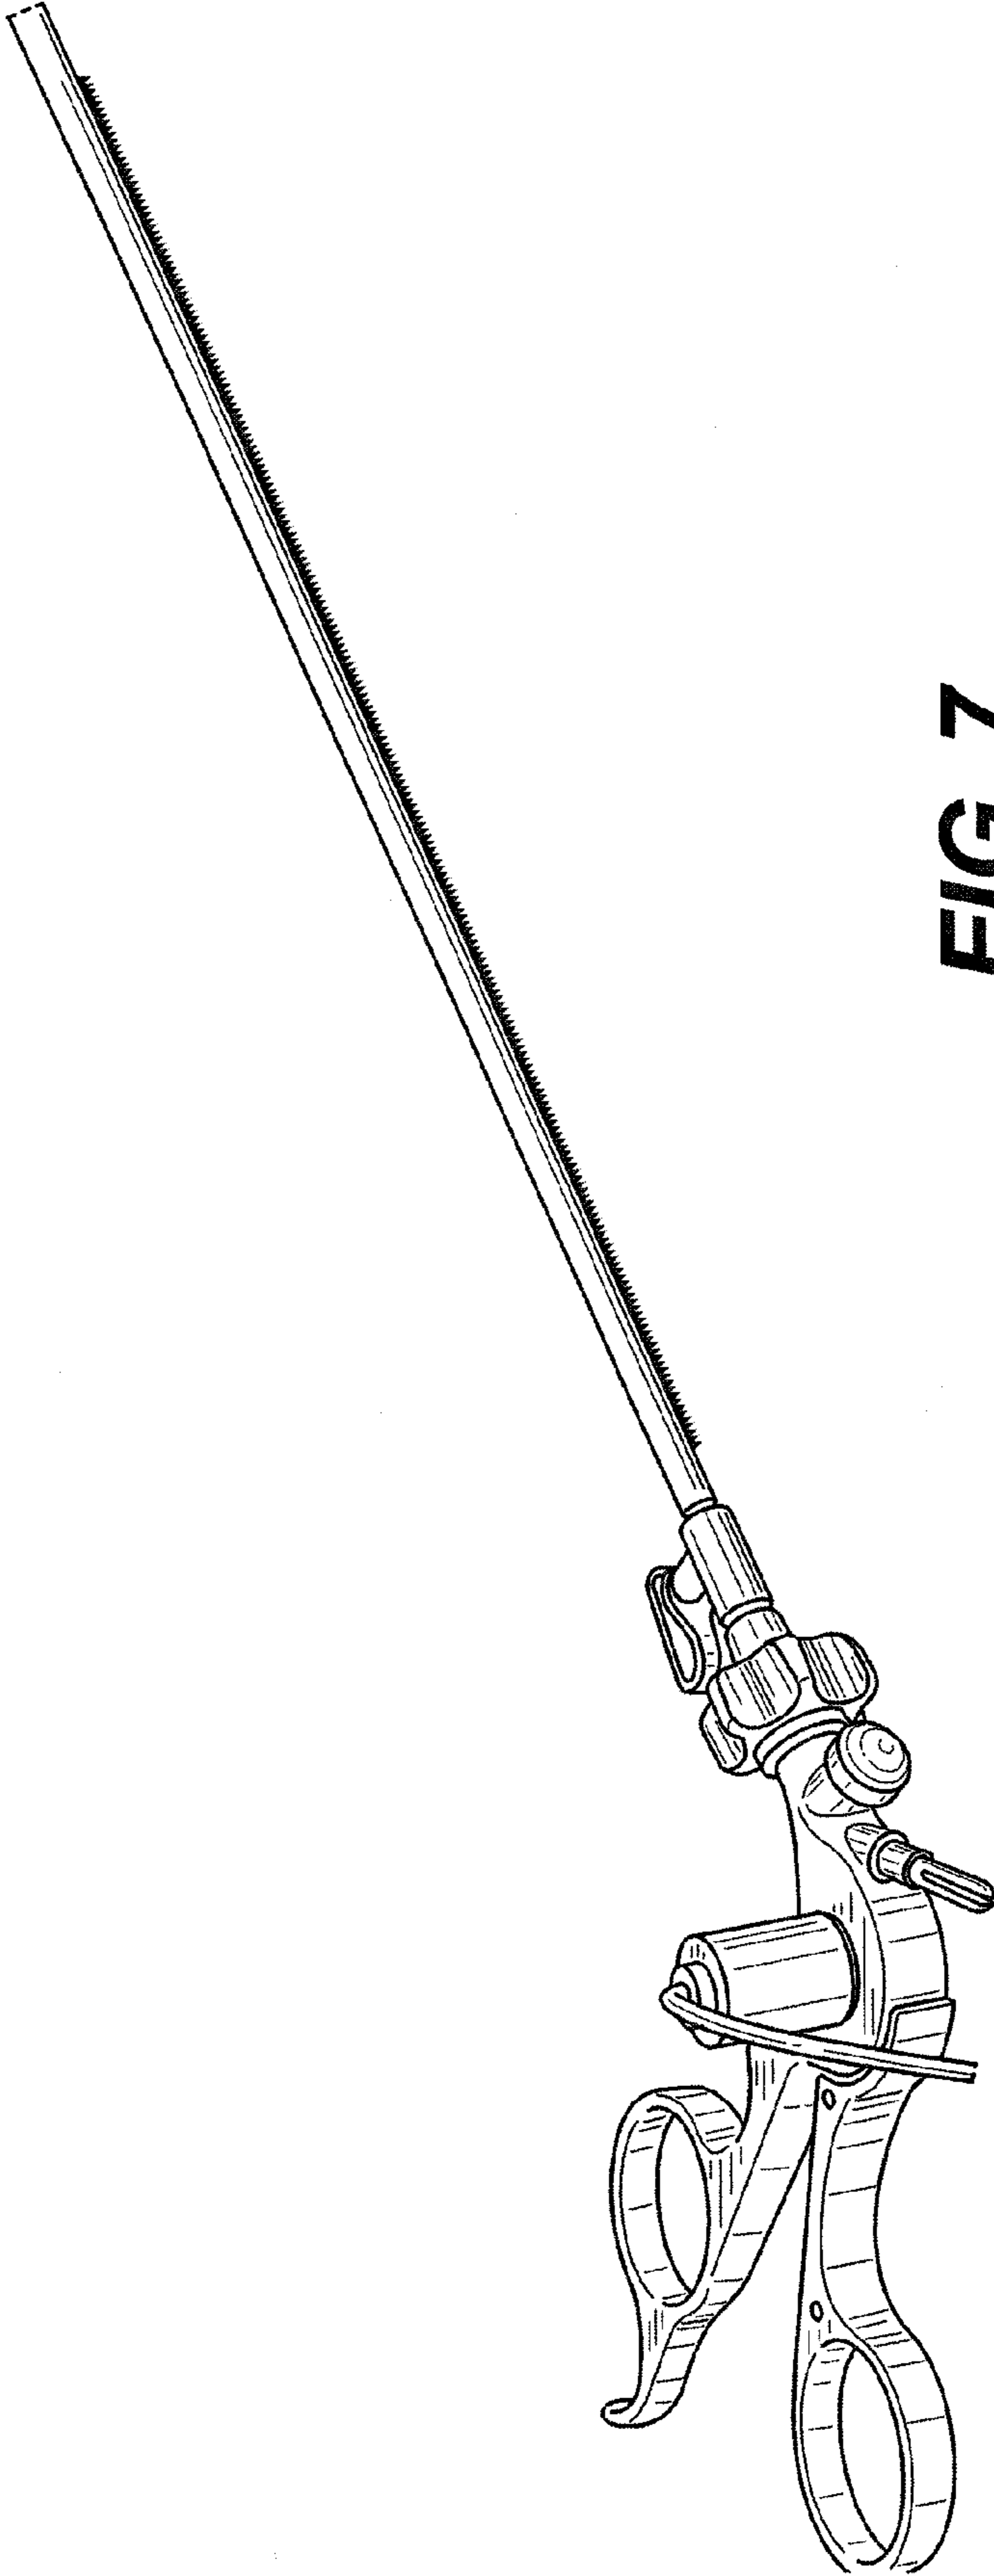


FIG. 7