



US00D630322S

(12) **United States Design Patent**  
**Speiser**

(10) **Patent No.:** **US D630,322 S**

(45) **Date of Patent:** **\*\* Jan. 4, 2011**

(54) **MEDICAL INSTRUMENT**

(75) Inventor: **Bjoern Speiser**, Rottweil (DE)

(73) Assignee: **Karl Storz GmbH & Co. KG**,  
Tuttlingen (DE)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/350,534**

(22) Filed: **Nov. 18, 2009**

(30) **Foreign Application Priority Data**

May 18, 2009 (EM) ..... 001516550-0017

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/133**

(58) **Field of Classification Search** ..... D24/133,  
D24/134, 135, 136, 137, 138, 139, 140, 141,  
D24/142, 143, 146, 150, 152, 144, 145, 147,  
D24/148, 149, 151, 153, 154, 127, 128, 129,  
D24/130, 106-108, 112, 111, 200; D23/233,  
D23/235; D8/40, 47, 57, 60, 67, 68, 69,  
D8/80, 82, 83, 84, 93, 94, 97, 107; 600/184,  
600/201-203, 210-218, 220-223, 224, 225-227;  
606/7, 86 A, 86 B, 119

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D274,096 S *	5/1984	Shutt	.....	D24/143
D289,437 S *	4/1987	Honkanen	.....	D24/148
D308,576 S *	6/1990	Iversen	.....	D24/129
D338,065 S *	8/1993	Rose	.....	D24/143
5,342,381 A *	8/1994	Tidemand	.....	606/174
D357,980 S *	5/1995	Ek et al.	.....	D24/143
D362,908 S *	10/1995	Shutt et al.	.....	D24/143
5,562,699 A *	10/1996	Heimberger et al.	.....	606/205
5,613,977 A *	3/1997	Weber et al.	.....	606/170

5,658,281 A *	8/1997	Heard	.....	606/48
6,139,563 A *	10/2000	Cosgrove et al.	.....	606/205
6,340,365 B2 *	1/2002	Dittrich et al.	.....	606/205

(Continued)

**FOREIGN PATENT DOCUMENTS**

EM 000324074-0001 \* 4/2005

(Continued)

*Primary Examiner*—Bridget L Eland

(74) *Attorney, Agent, or Firm*—Muncy, Geissler, Olds & Lowe, PLLC

(57) **CLAIM**

The ornamental design for a medical instrument, as shown and described.

**DESCRIPTION**

FIG. 1 is a left side perspective view of a medical instrument the present invention.

FIG. 2 is a right side perspective view of the medical instrument of FIG. 1.

FIG. 3 is a top perspective view of the medical instrument of FIG. 1.

FIG. 4 is a bottom perspective view of the medical instrument of FIG. 1.


FIG. 5 is a front perspective view of the medical instrument of FIG. 1.

FIG. 6 is a rear perspective view of the medical instrument of FIG. 1; and,

FIG. 7 is a three-quarter perspective view of the medical instrument of FIG. 1.

The broken lines shown at the end of the cord and at the end of the tubular shaft represent the bounds of the claimed design; the broken lines form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

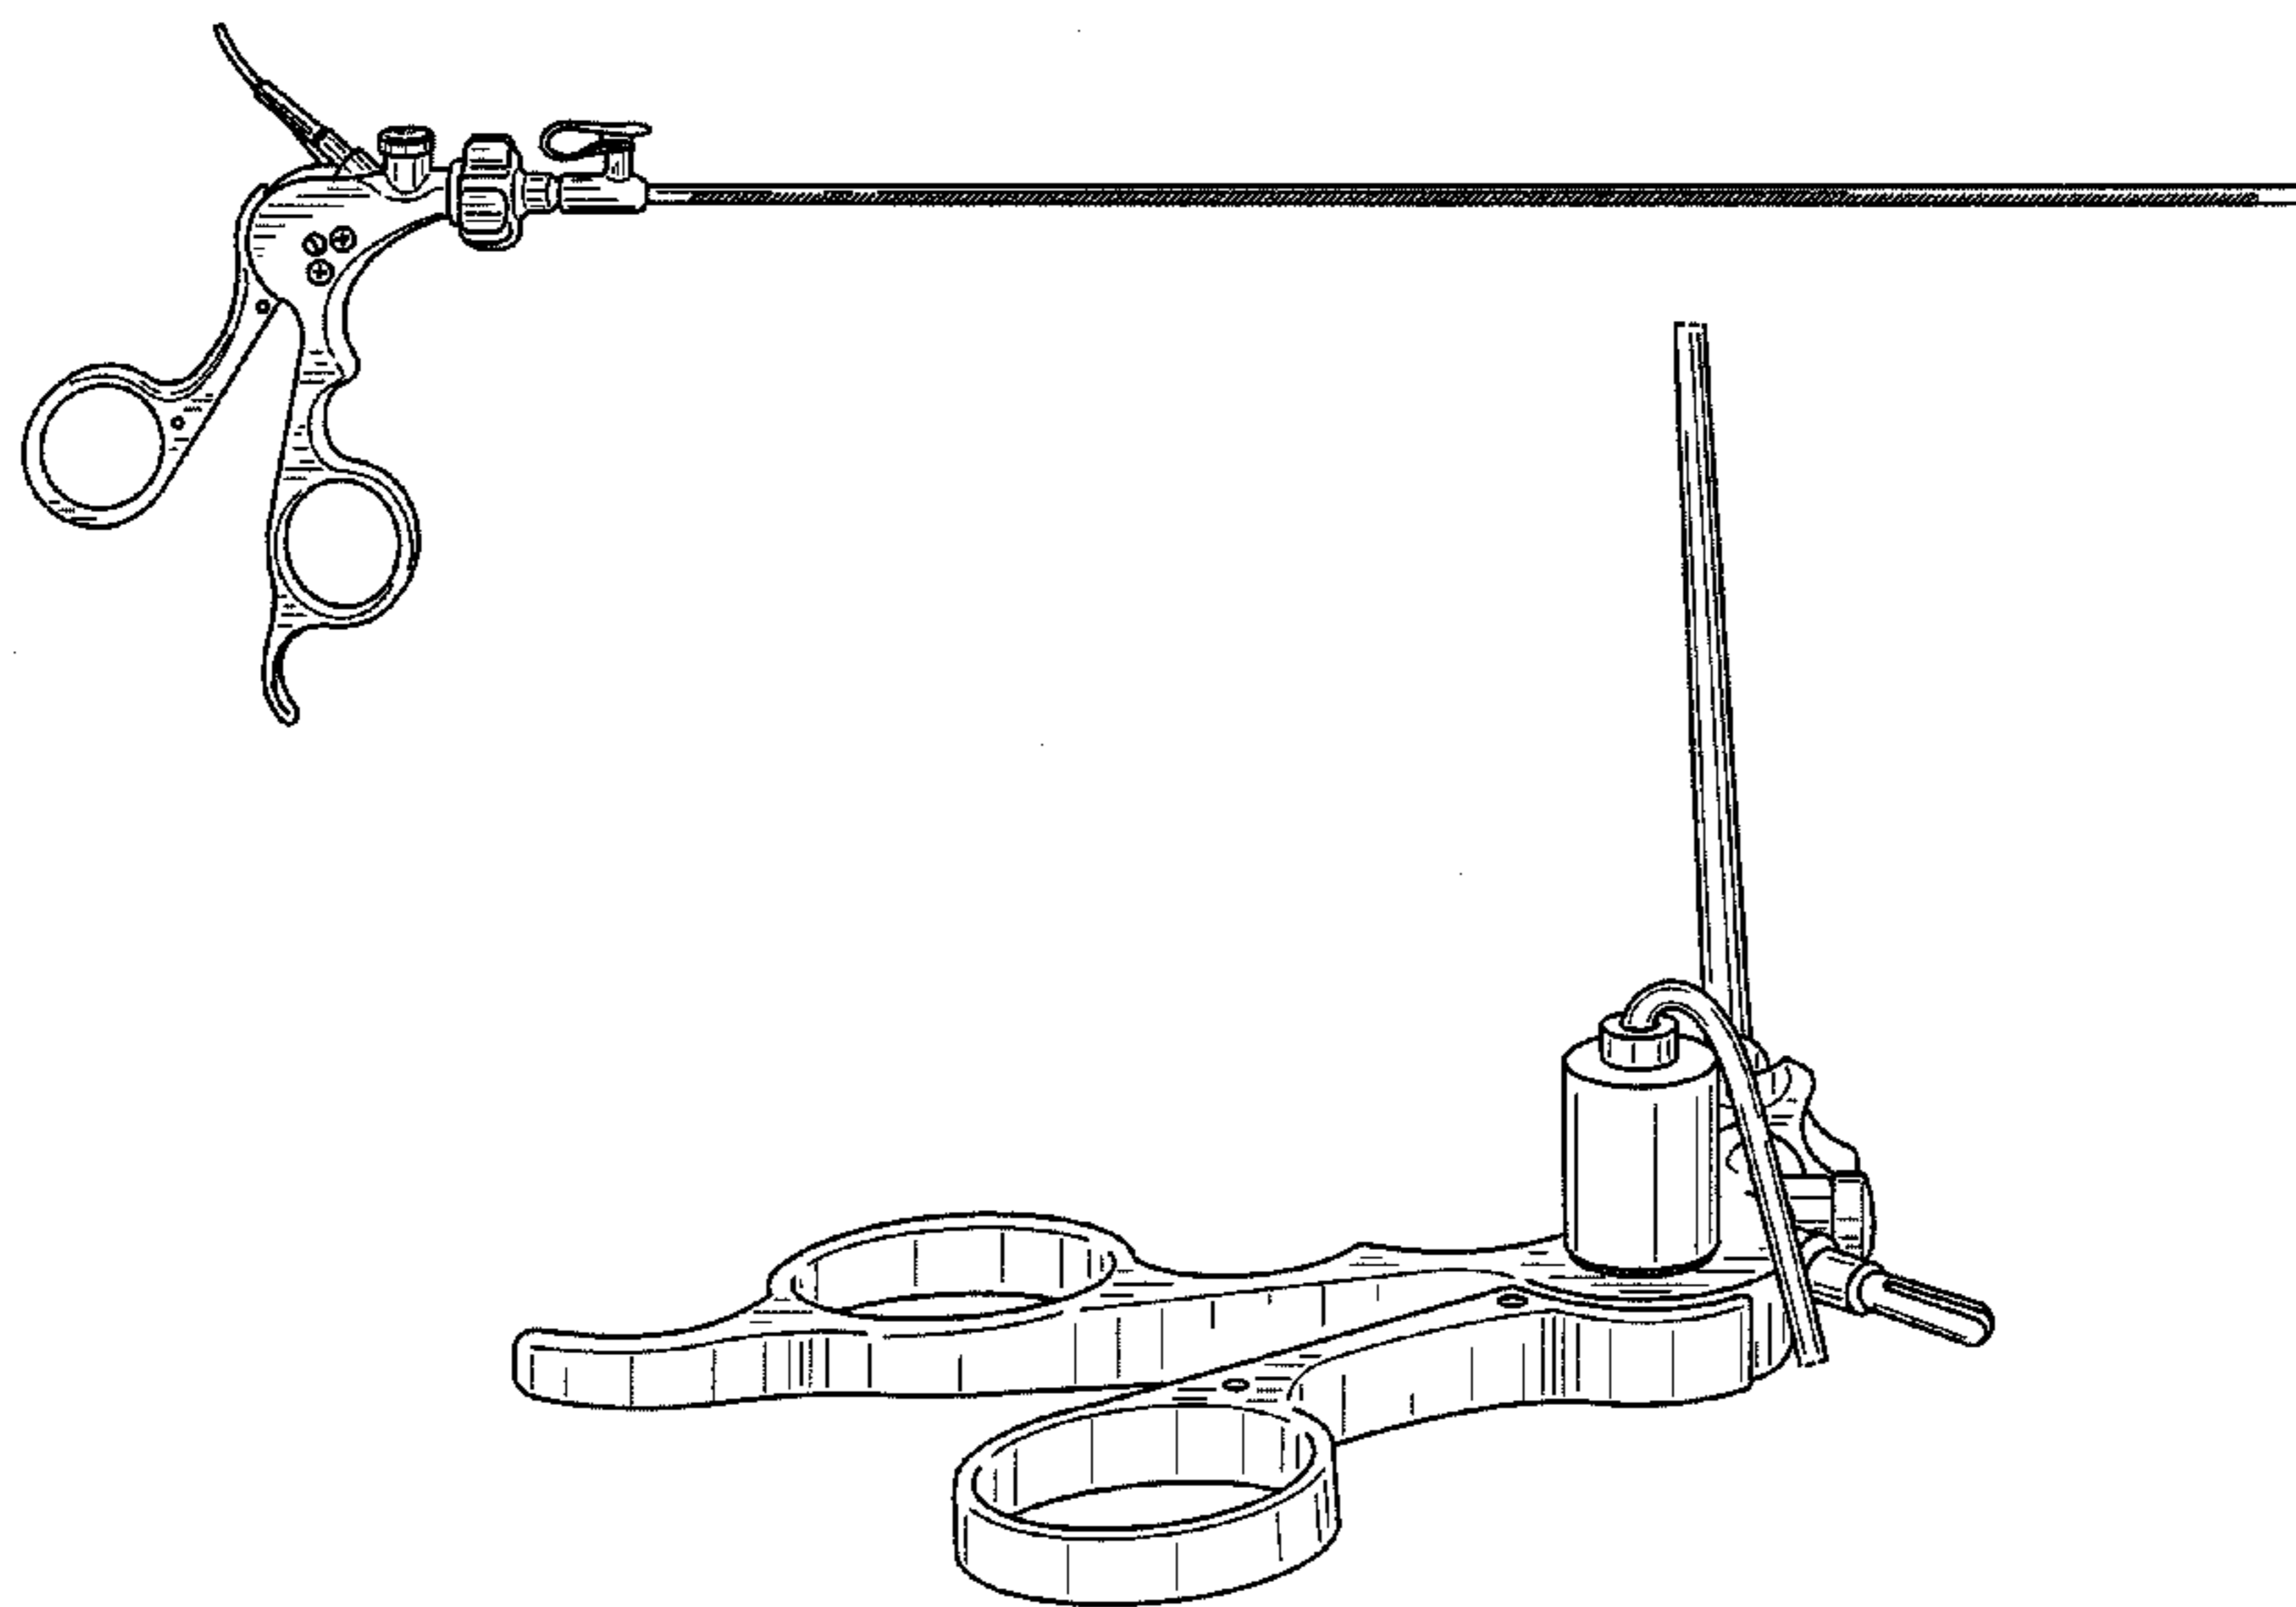

# US D630,322 S

Page 2

---

## U.S. PATENT DOCUMENTS


D465,281 S \* 11/2002 Lang ..... D24/147  
6,752,823 B2 \* 6/2004 Prestel ..... 606/208  
D498,300 S \* 11/2004 Karl-Heinz ..... D24/146  
6,896,686 B2 \* 5/2005 Weber ..... 606/145  
D535,398 S \* 1/2007 Stammberger ..... D24/146  
D541,416 S \* 4/2007 Baehr et al. .... D24/133  
D548,836 S \* 8/2007 Lang et al. .... D24/146  
D557,415 S \* 12/2007 Bacher ..... D24/133  
D583,941 S \* 12/2008 Leroy ..... D24/135  
D594,982 S \* 6/2009 Stefan ..... D24/133

D605,761 S \* 12/2009 Stefan ..... D24/143  
2005/0143626 A1 \* 6/2005 Prescott ..... 600/162  
2009/0036745 A1 \* 2/2009 Bonadio et al. .... 600/208  
2009/0076521 A1 \* 3/2009 Hansen ..... 606/129


## FOREIGN PATENT DOCUMENTS

EM 000324074-0003 \* 4/2005  
EM 001516550-0017 \* 5/2009  
WO DM/060711 \* 6/2002


\* cited by examiner

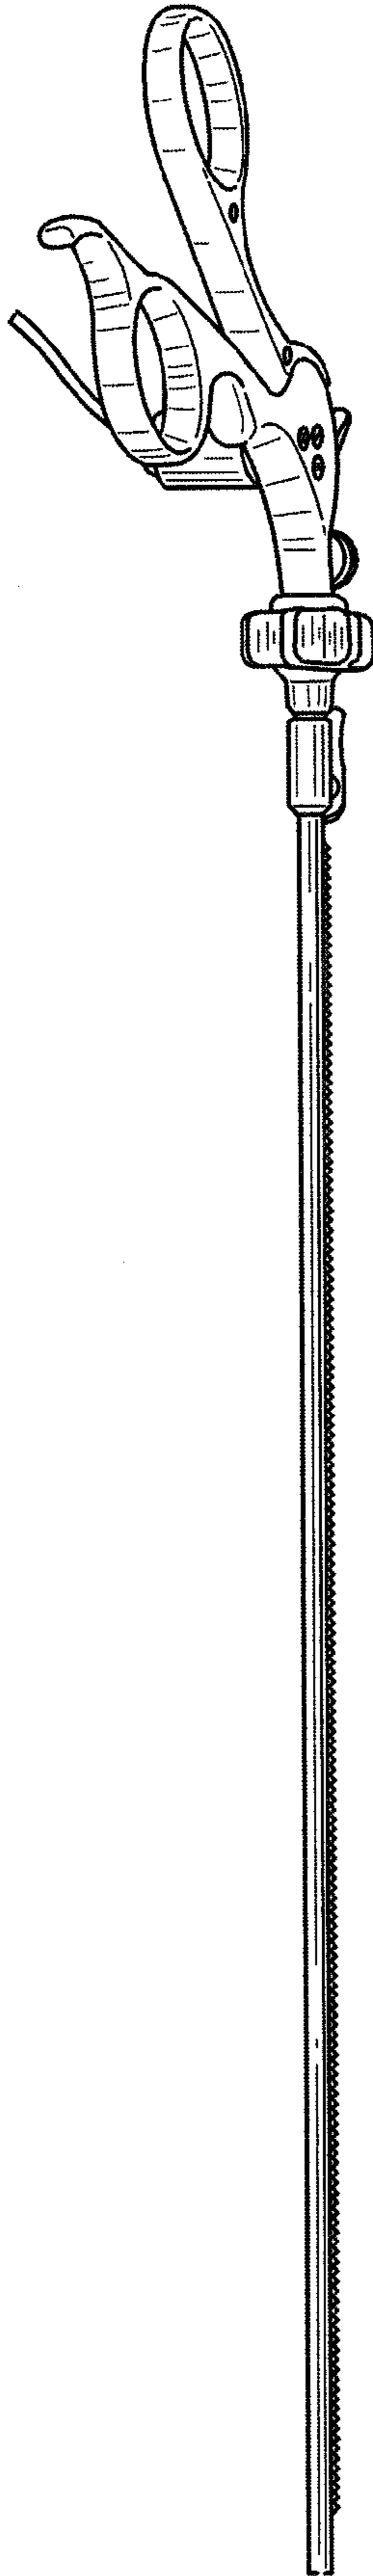


**FIG. 1**

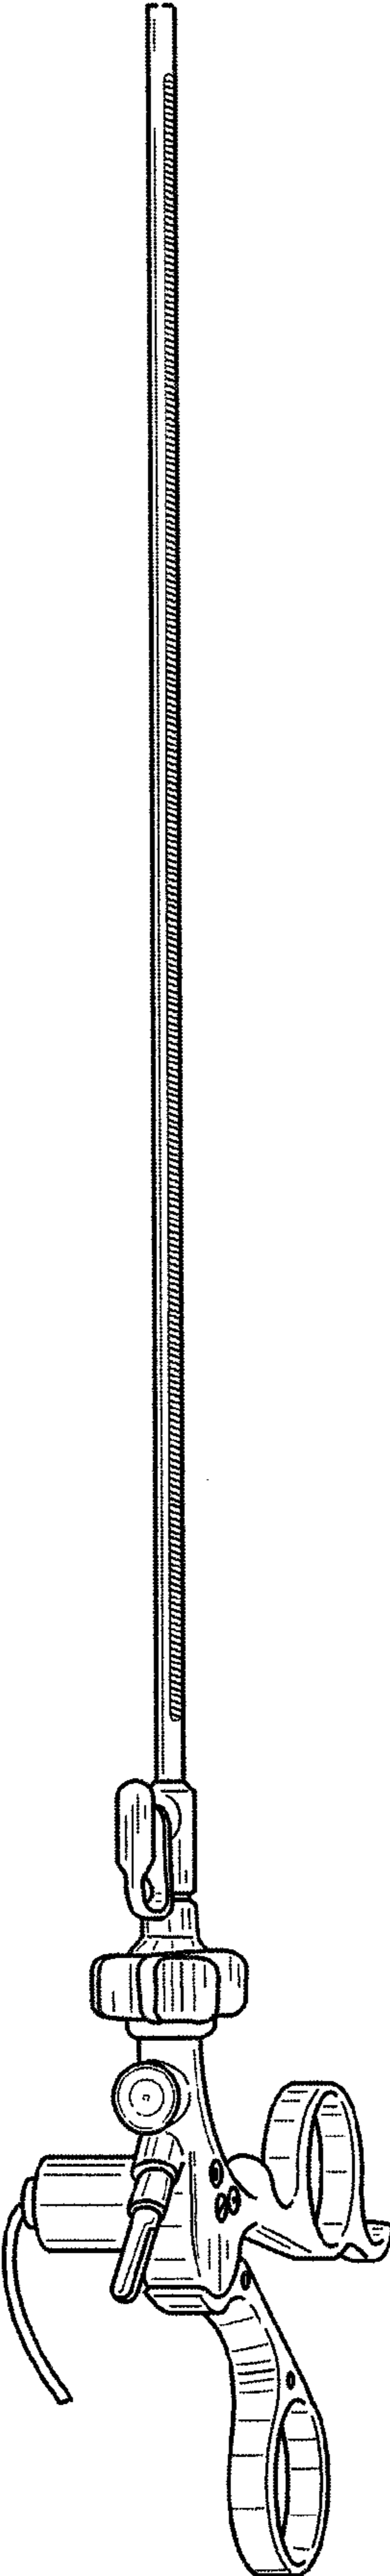


**FIG. 2**

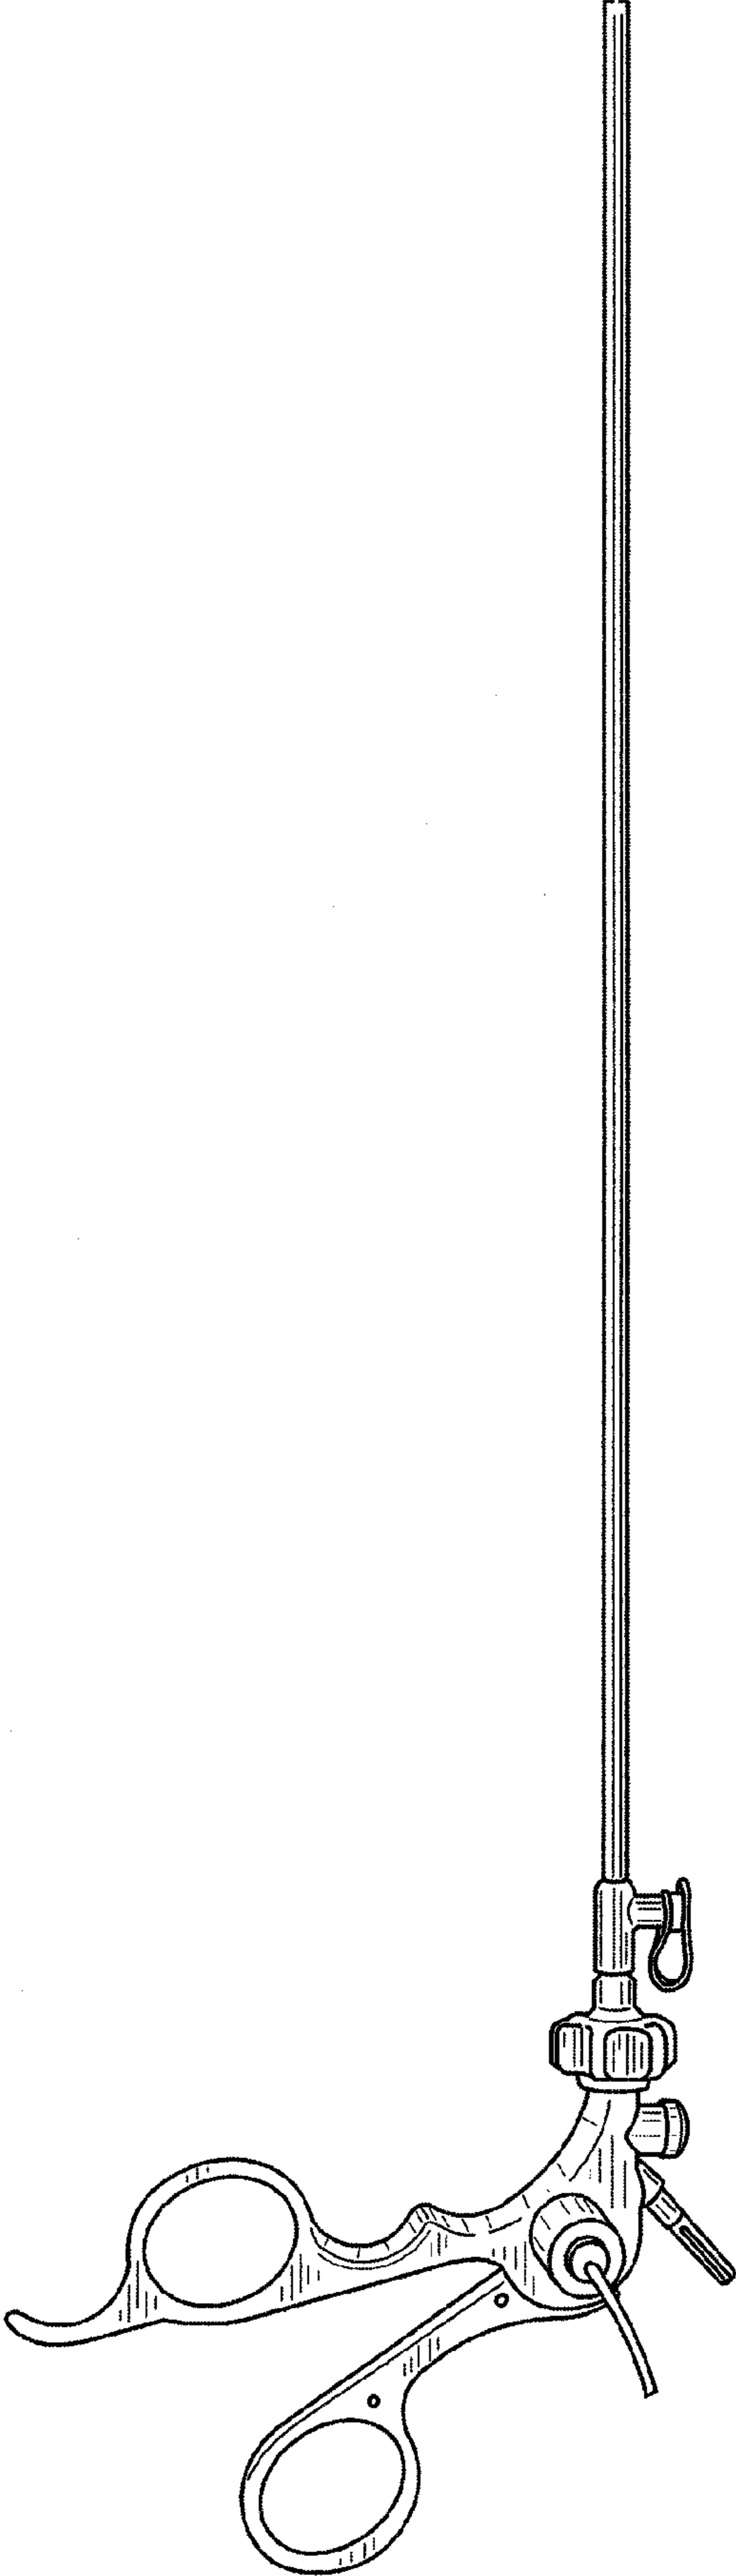


**FIG. 3**

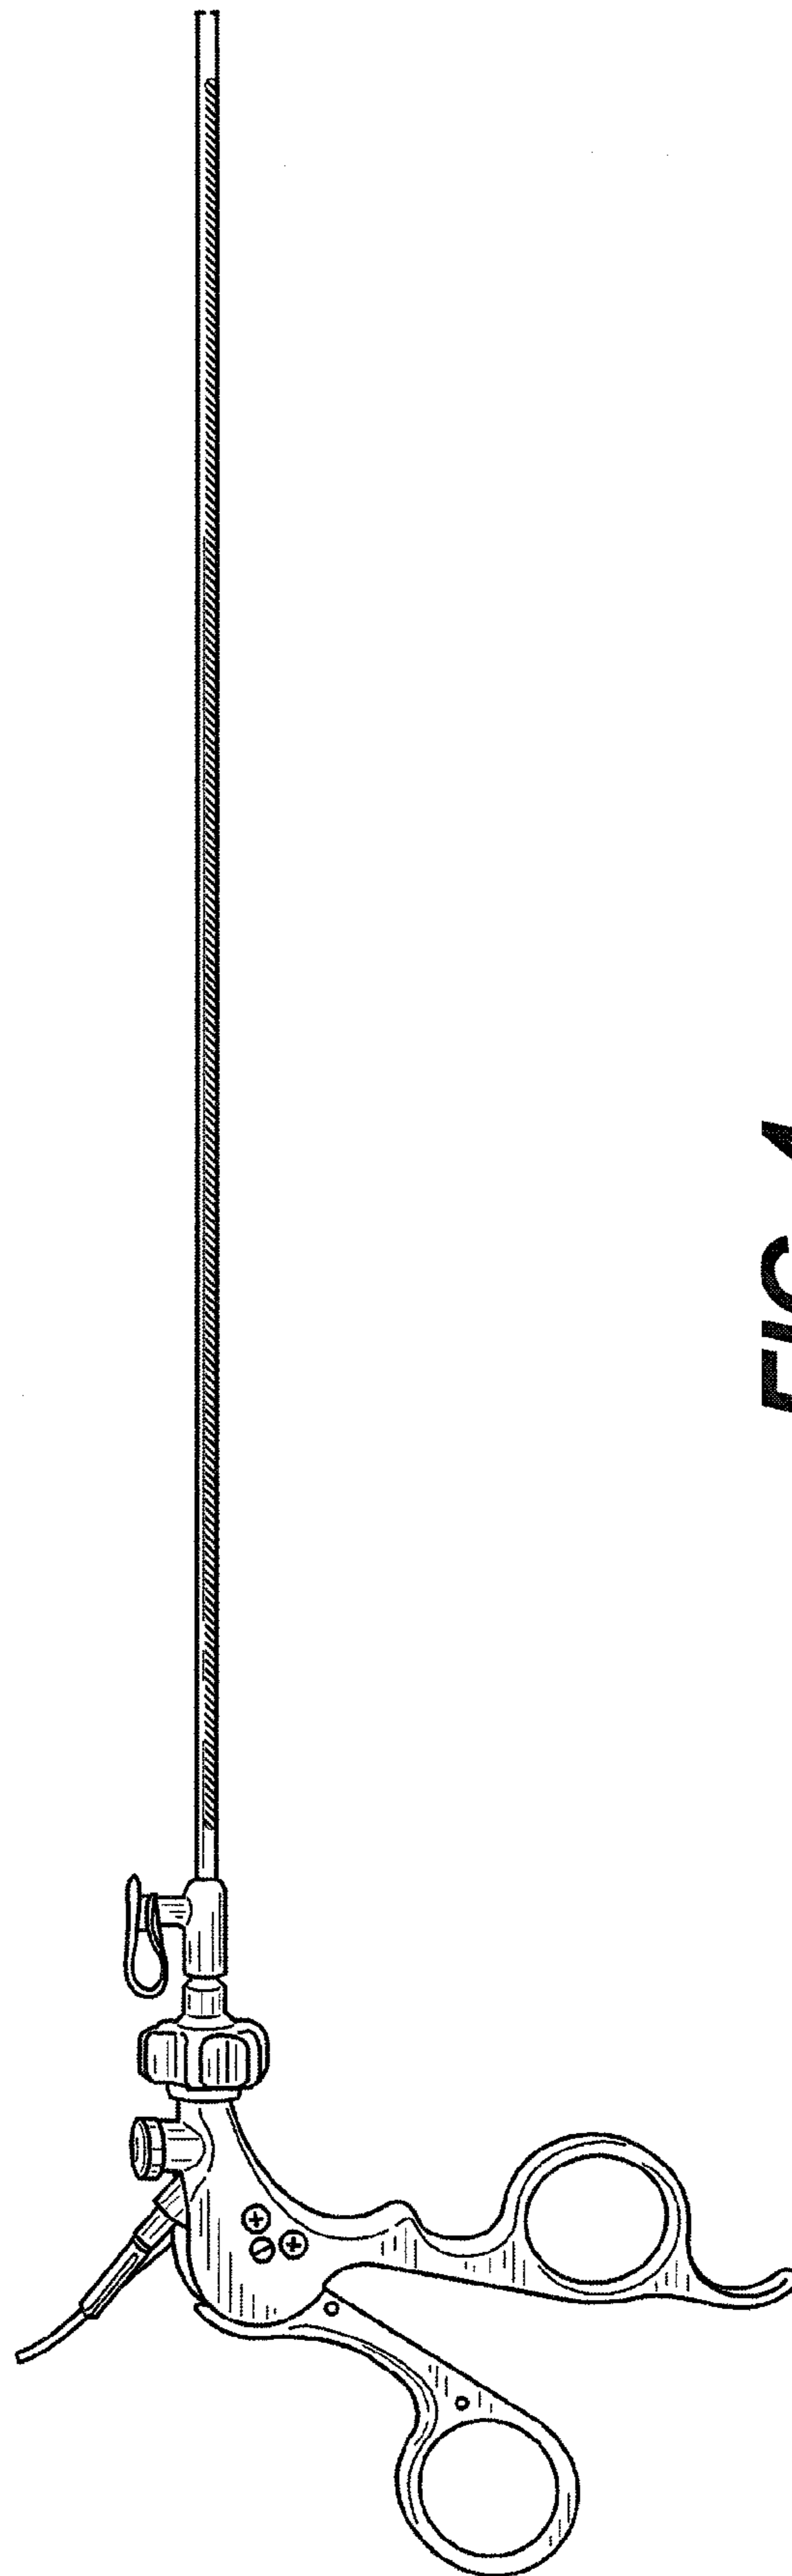

**FIG. 4**

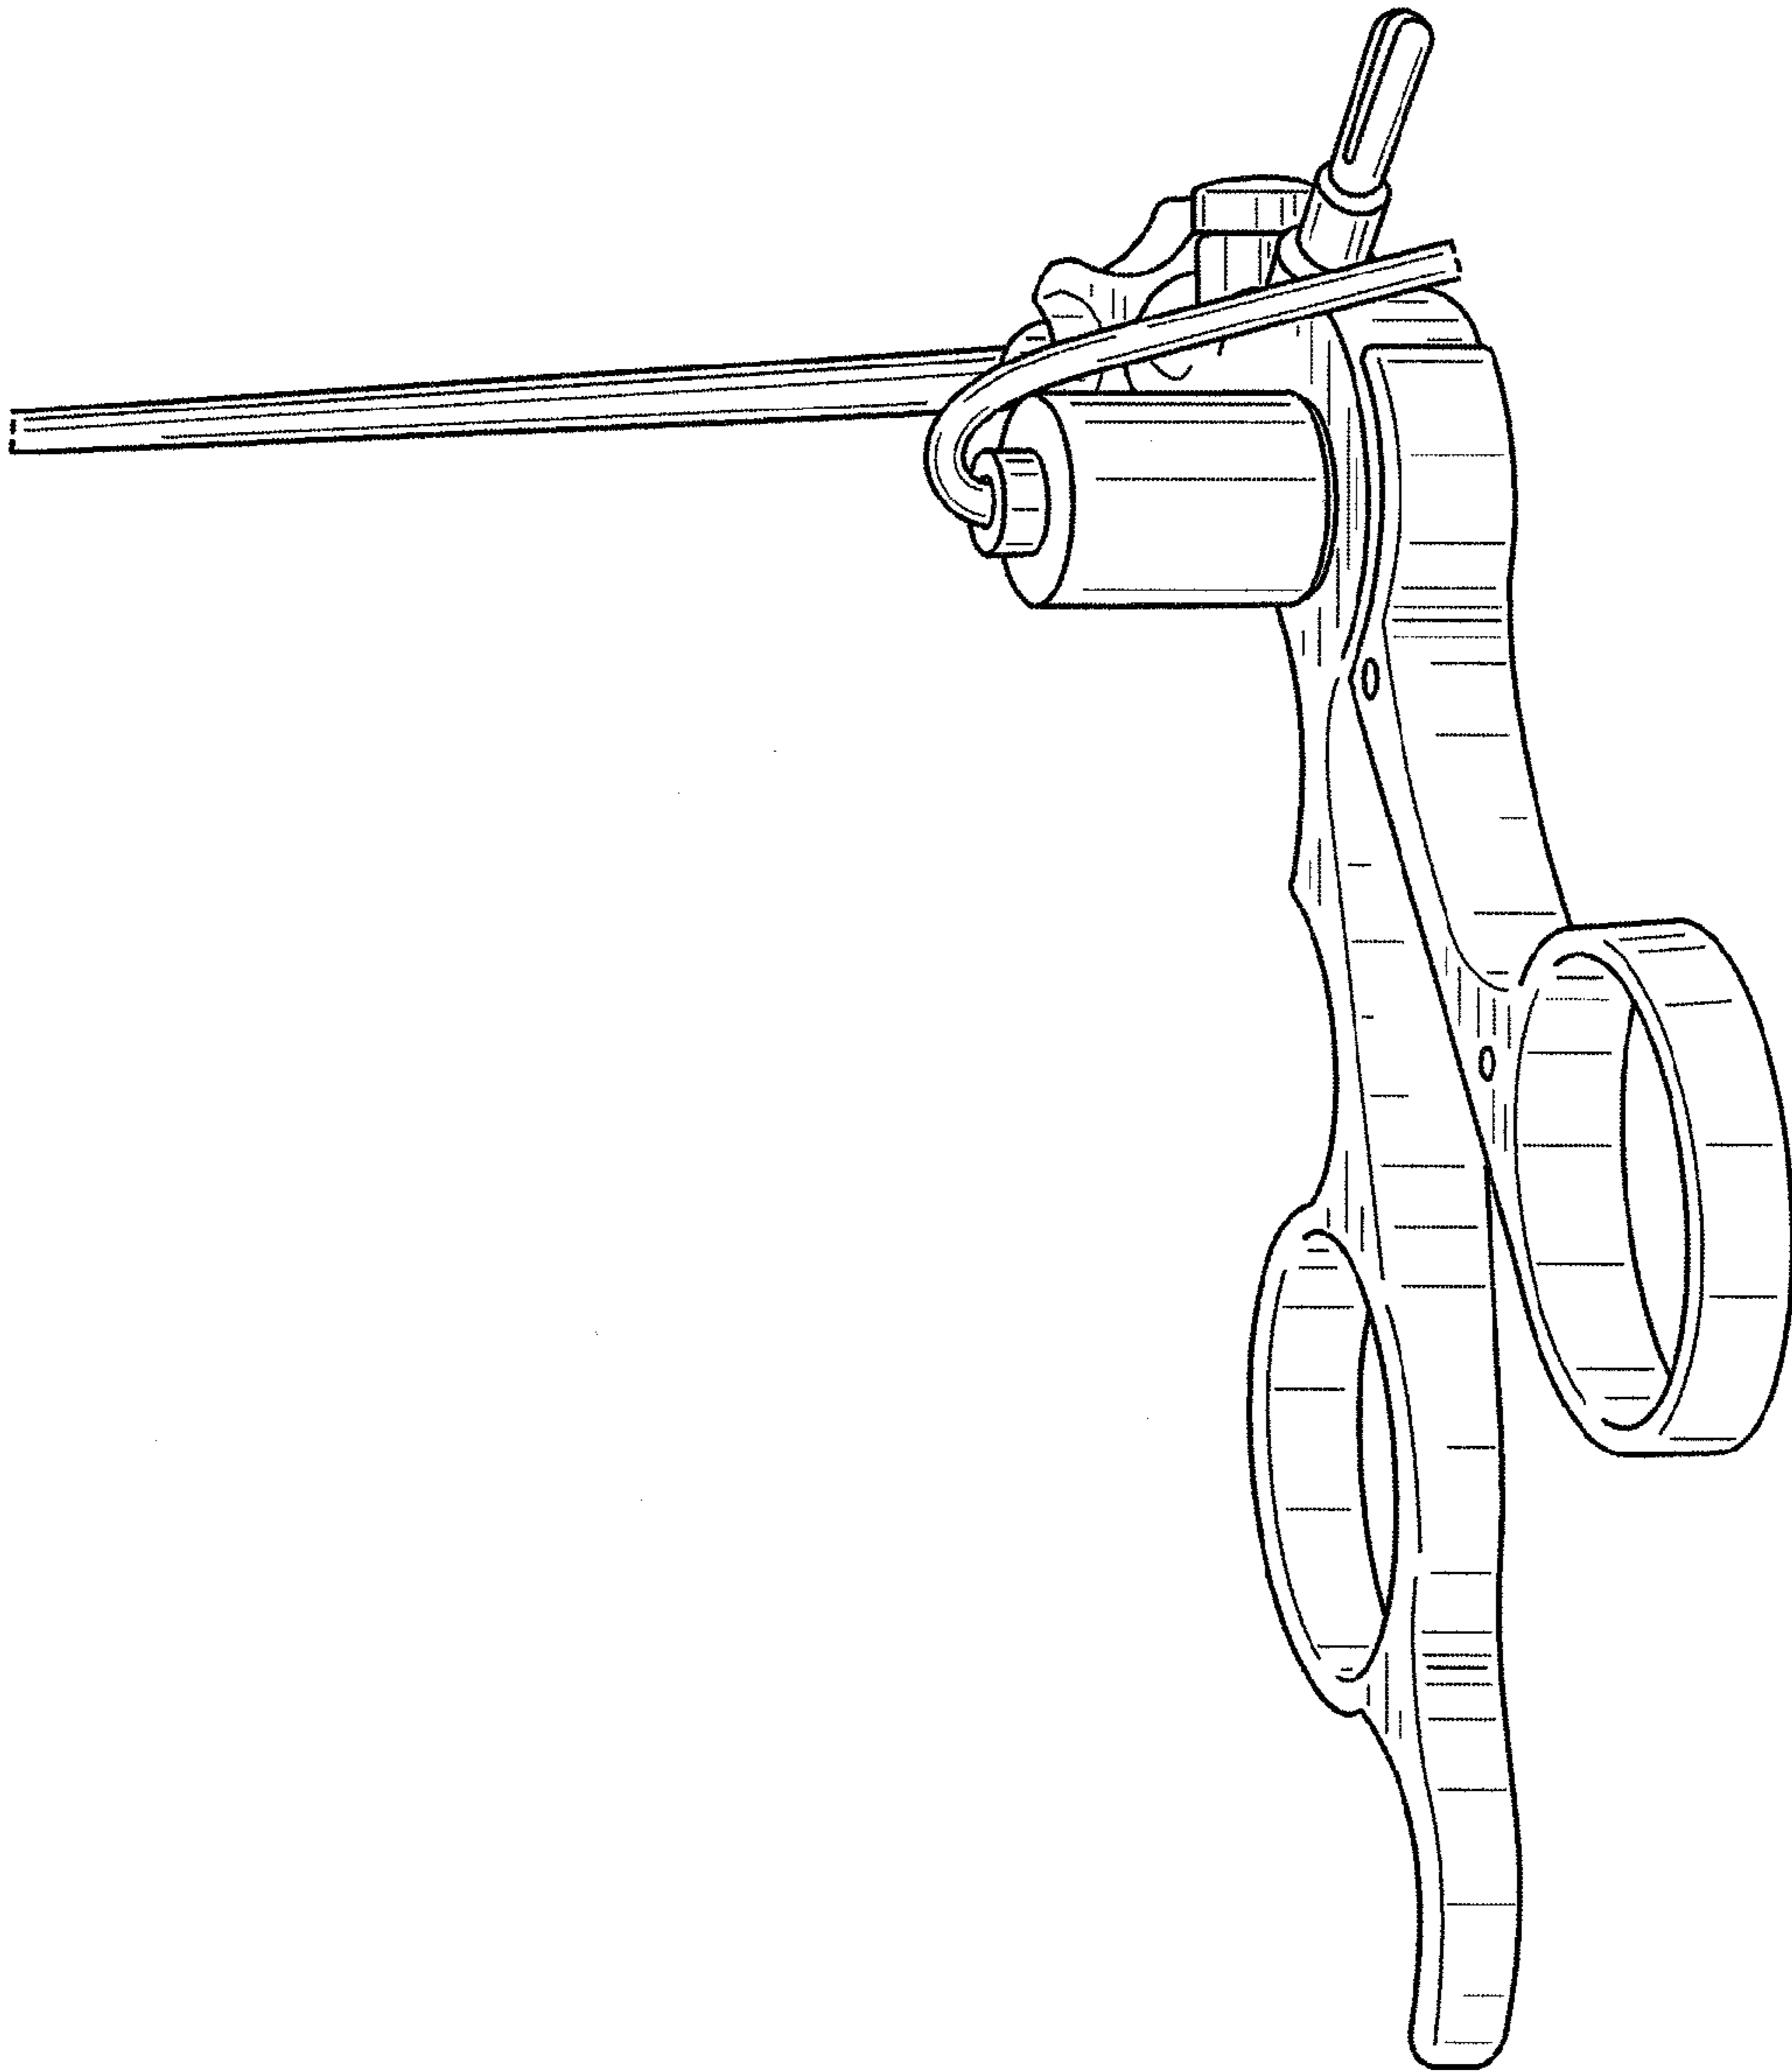


**FIG. 5**

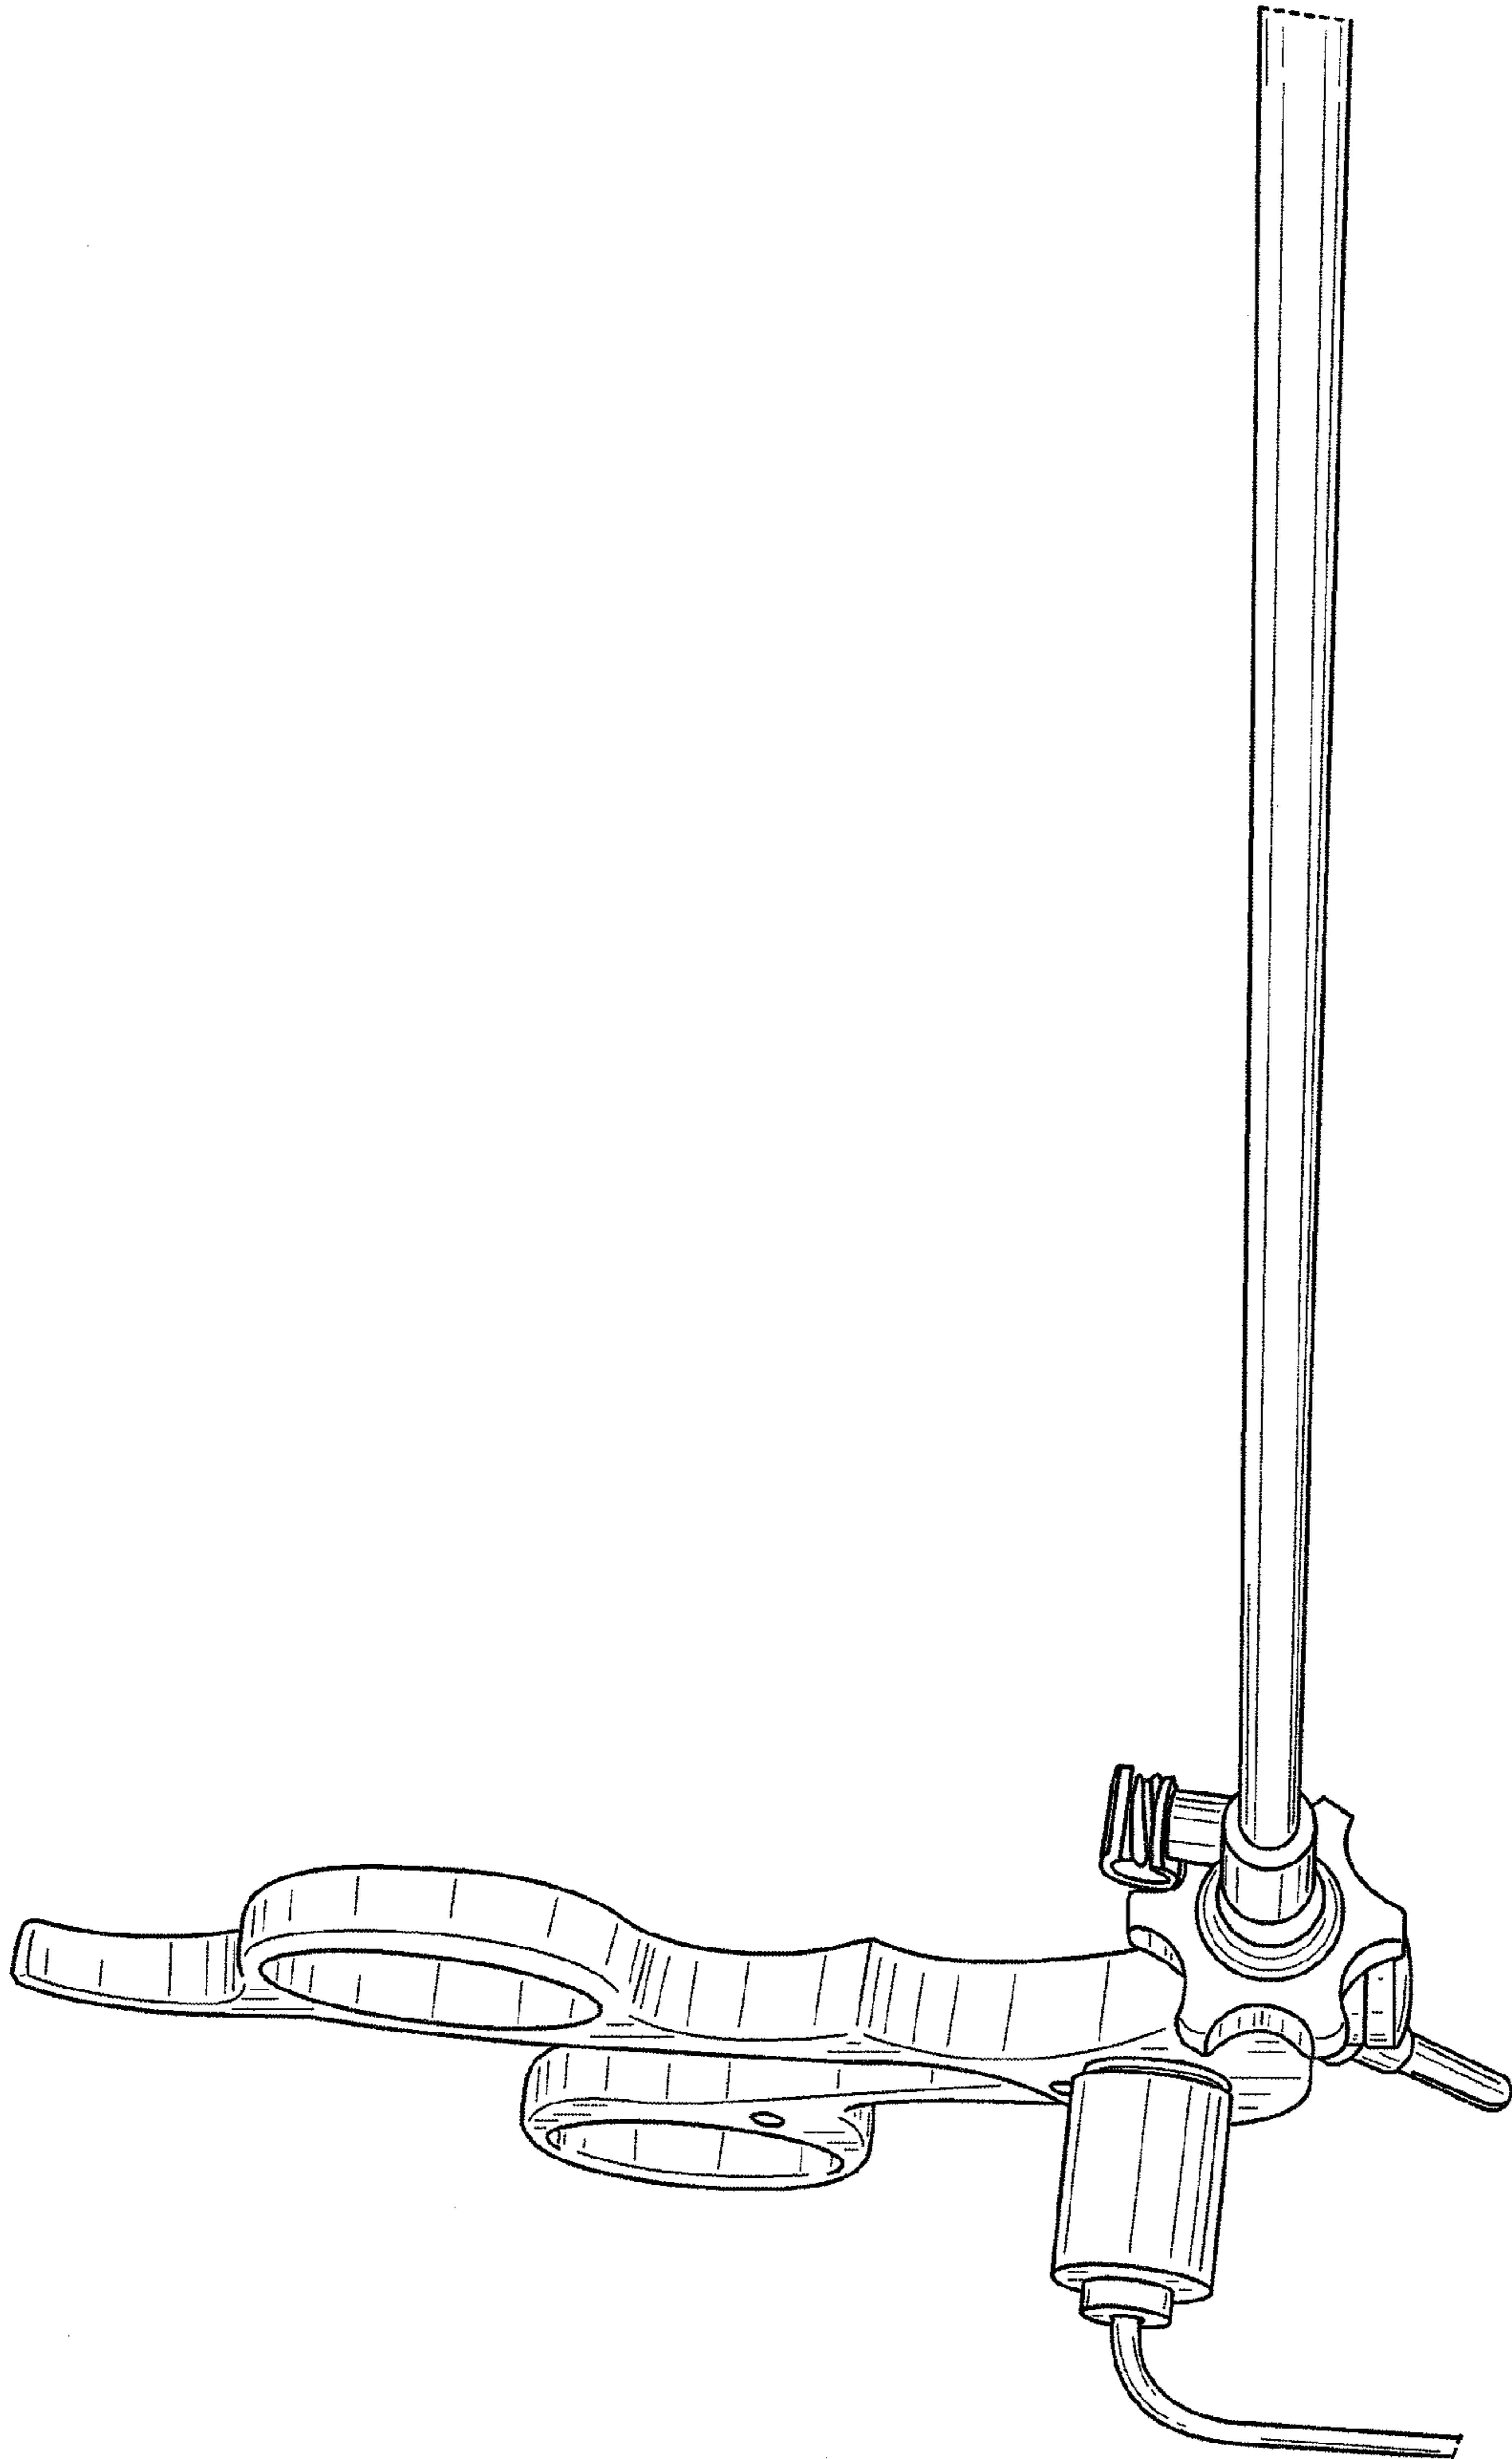

**FIG. 6**



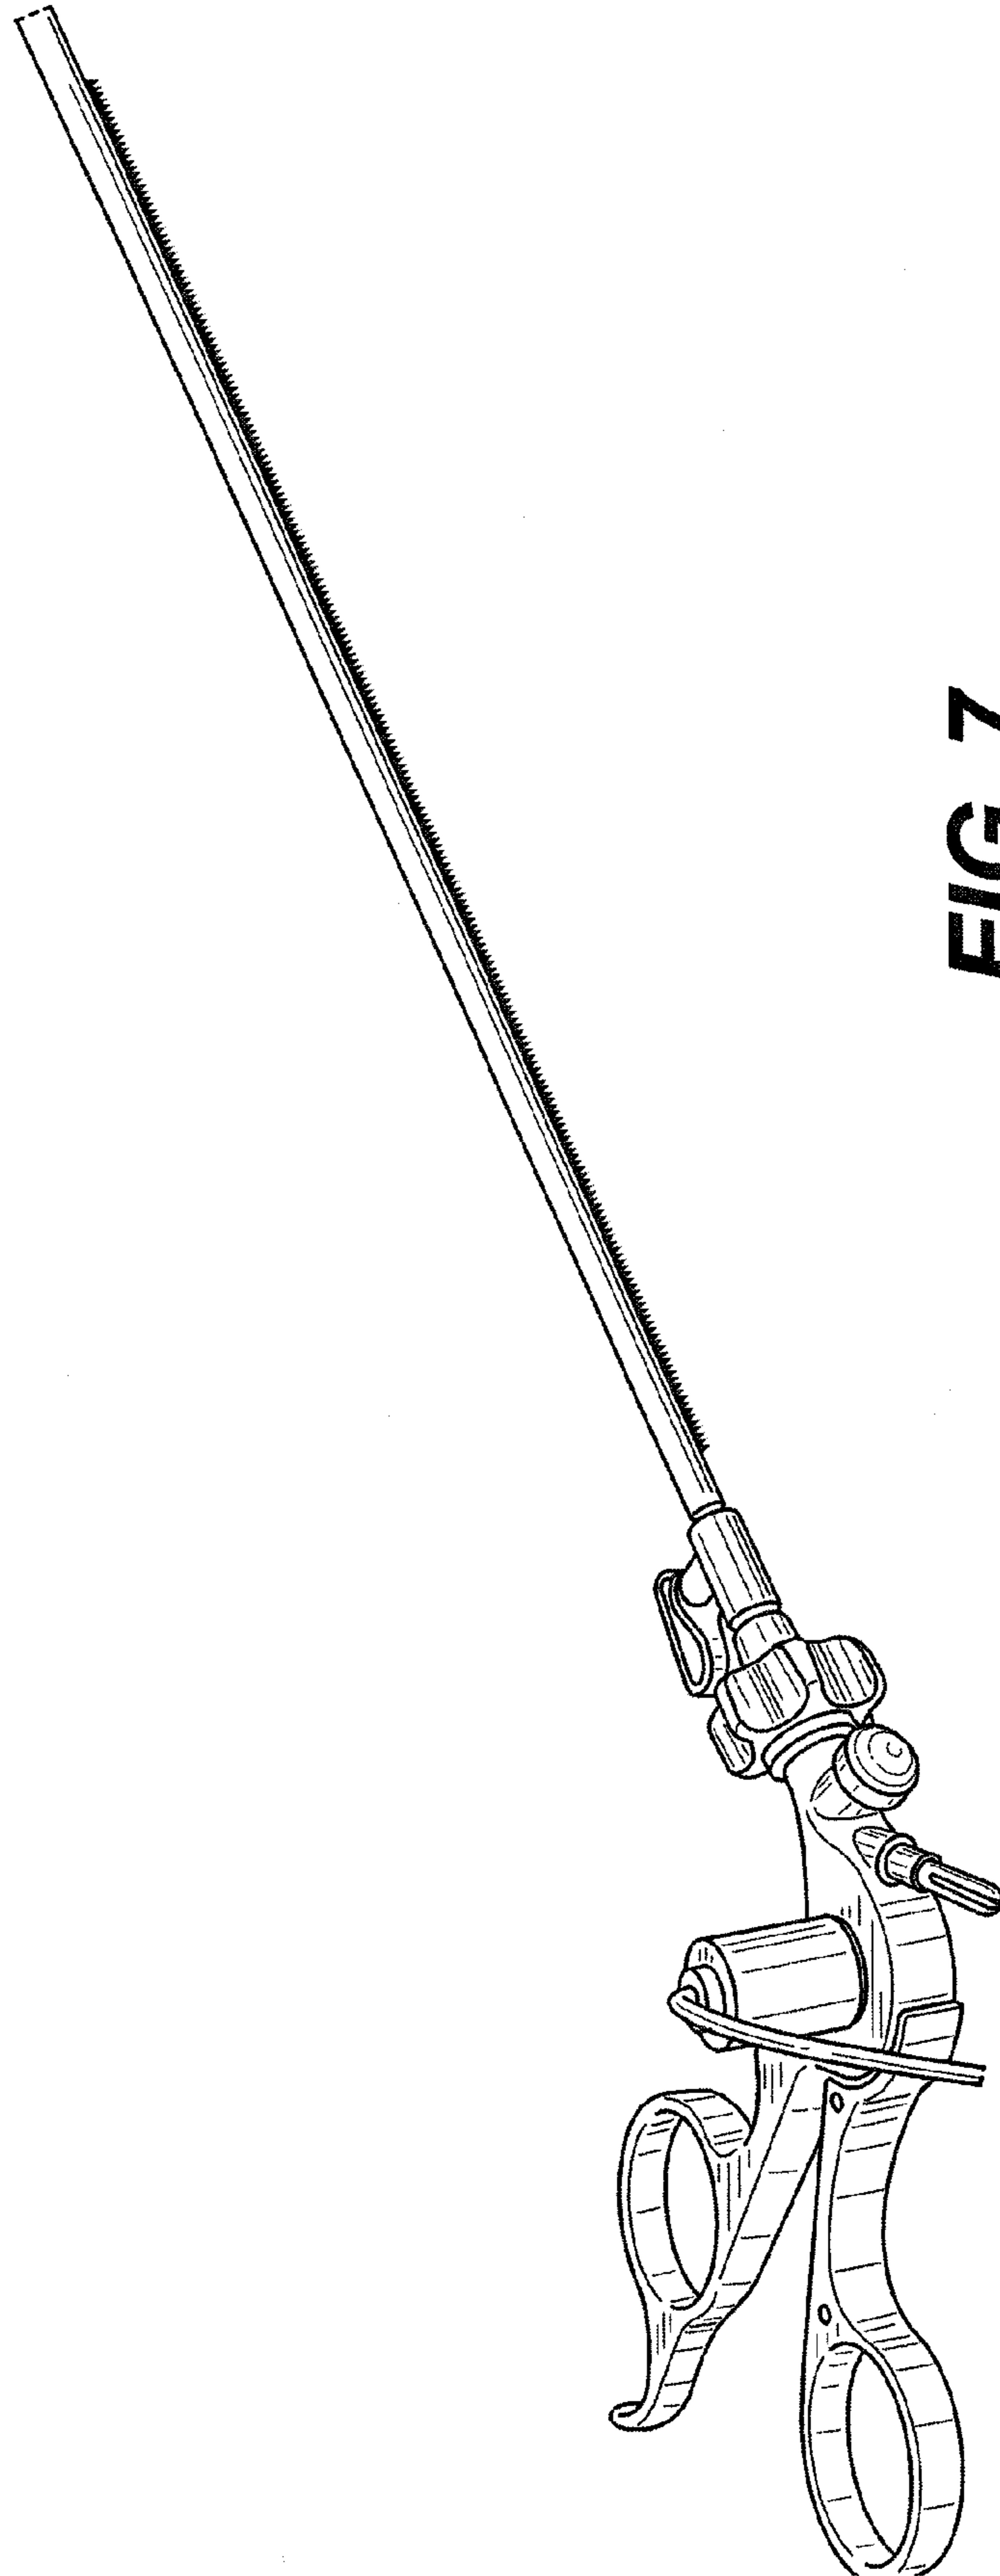

**FIG. 7**