



US00D630766S

(12) **United States Design Patent**
Harbin

(10) **Patent No.:** **US D630,766 S**
(45) **Date of Patent:** **** Jan. 11, 2011**

(54) **MEDICAL LOUPE HEAD SET**

(75) Inventor: **Daniel Harbin**, West Midlands (GB)

(73) Assignee: **Birmingham City University** (GB)

(**) Term: **14 Years**

(21) Appl. No.: **29/340,945**

(22) Filed: **Jul. 28, 2009**

(30) **Foreign Application Priority Data**

Jan. 29, 2009	(EM)	001081715-0001
Jan. 29, 2009	(EM)	001081715-0002
Jan. 29, 2009	(EM)	001081715-0003
Jan. 29, 2009	(EM)	001081715-0004
Jan. 29, 2009	(EM)	001081715-0005
Jan. 29, 2009	(EM)	001081715-0006

D399,580	S *	10/1998	Feinbloom	D26/39
D406,371	S *	3/1999	Van Der Bel	D26/39
D441,111	S *	4/2001	Van Der Bel	D24/231
D441,886	S *	5/2001	Beck	D24/231
D472,998	S *	4/2003	Paris et al.	D26/39
6,667,832	B2 *	12/2003	Caplan et al.	359/409
D489,838	S *	5/2004	Opolka	D26/39
6,955,444	B2 *	10/2005	Gupta	362/106
D531,335	S *	10/2006	Garrity	D26/39
D539,952	S *	4/2007	Iranyi et al.	D26/39
7,210,810	B1 *	5/2007	Iversen et	362/105
D552,278	S *	10/2007	Spartano et al.	D26/39
D564,011	S *	3/2008	Beate et al.	D16/309
D586,932	S *	2/2009	Feinbloom et al.	D26/39
D591,327	S *	4/2009	Krause-Bonte	D16/309
D592,691	S *	5/2009	Chang	D16/309
D592,692	S *	5/2009	Chang	D16/309
D592,693	S *	5/2009	Chang	D16/309
D608,479	S *	1/2010	Heine et al.	D24/231
2006/0245175	A1 *	11/2006	Heine et al.	362/105
2008/0239707	A1 *	10/2008	Feinbloom et al.	362/105

(51) **LOC (9) Cl.** **24-01**

(52) **U.S. Cl.** **D24/231**

(58) **Field of Classification Search** D24/137,
D24/150, 160, 186, 231; D26/24, 27, 39,
D26/51, 113, 120; D29/103; D16/311, 133,
D16/135-136, 309; 362/105-106, 573, 804;
600/249, 111, 109; 359/409

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,285,242	A *	11/1966	Wallace	362/105
3,745,993	A *	7/1973	Feinbloom	600/249
3,830,230	A *	8/1974	Chester	600/249
D238,958	S *	2/1976	Feinbloom	D26/39
D266,192	S *	9/1982	Feinbloom et al.	D26/39
4,593,683	A *	6/1986	Blaha	362/106
4,621,283	A *	11/1986	Feinbloom	600/109
D296,337	S *	6/1988	Caplan	D16/133
4,797,736	A *	1/1989	Kloots et al.	600/109
D333,828	S *	3/1993	Baldassarre	D16/133
D383,229	S *	9/1997	Kiichiro	D26/39
5,667,291	A *	9/1997	Caplan et al.	362/105
D398,403	S *	9/1998	Bishop et al.	D24/231

* cited by examiner

Primary Examiner—T. Chase Nelson

Assistant Examiner—Mark Cavanna

(74) *Attorney, Agent, or Firm*—Barnes & Thornburg LLP

(57) **CLAIM**

The ornamental design for a medical loupe head set, as shown and described.

DESCRIPTION

FIG. 1 is side isometric view of a medical loupe head set;
FIG. 2 is an isometric view of the medical loupe head set;
FIG. 3 is a rear isometric view of the medical loupe head set;
FIG. 4 is a side isometric view of the medical loupe head set;
FIG. 5 is a front isometric view of the medical loupe head set;
FIG. 6 is a top isometric view of the medical loupe head set;
FIG. 7 is a bottom isometric view of the medical loupe head set;
FIG. 8 is side isometric view of the head gear component;
FIG. 9 is an isometric view of the head gear component;

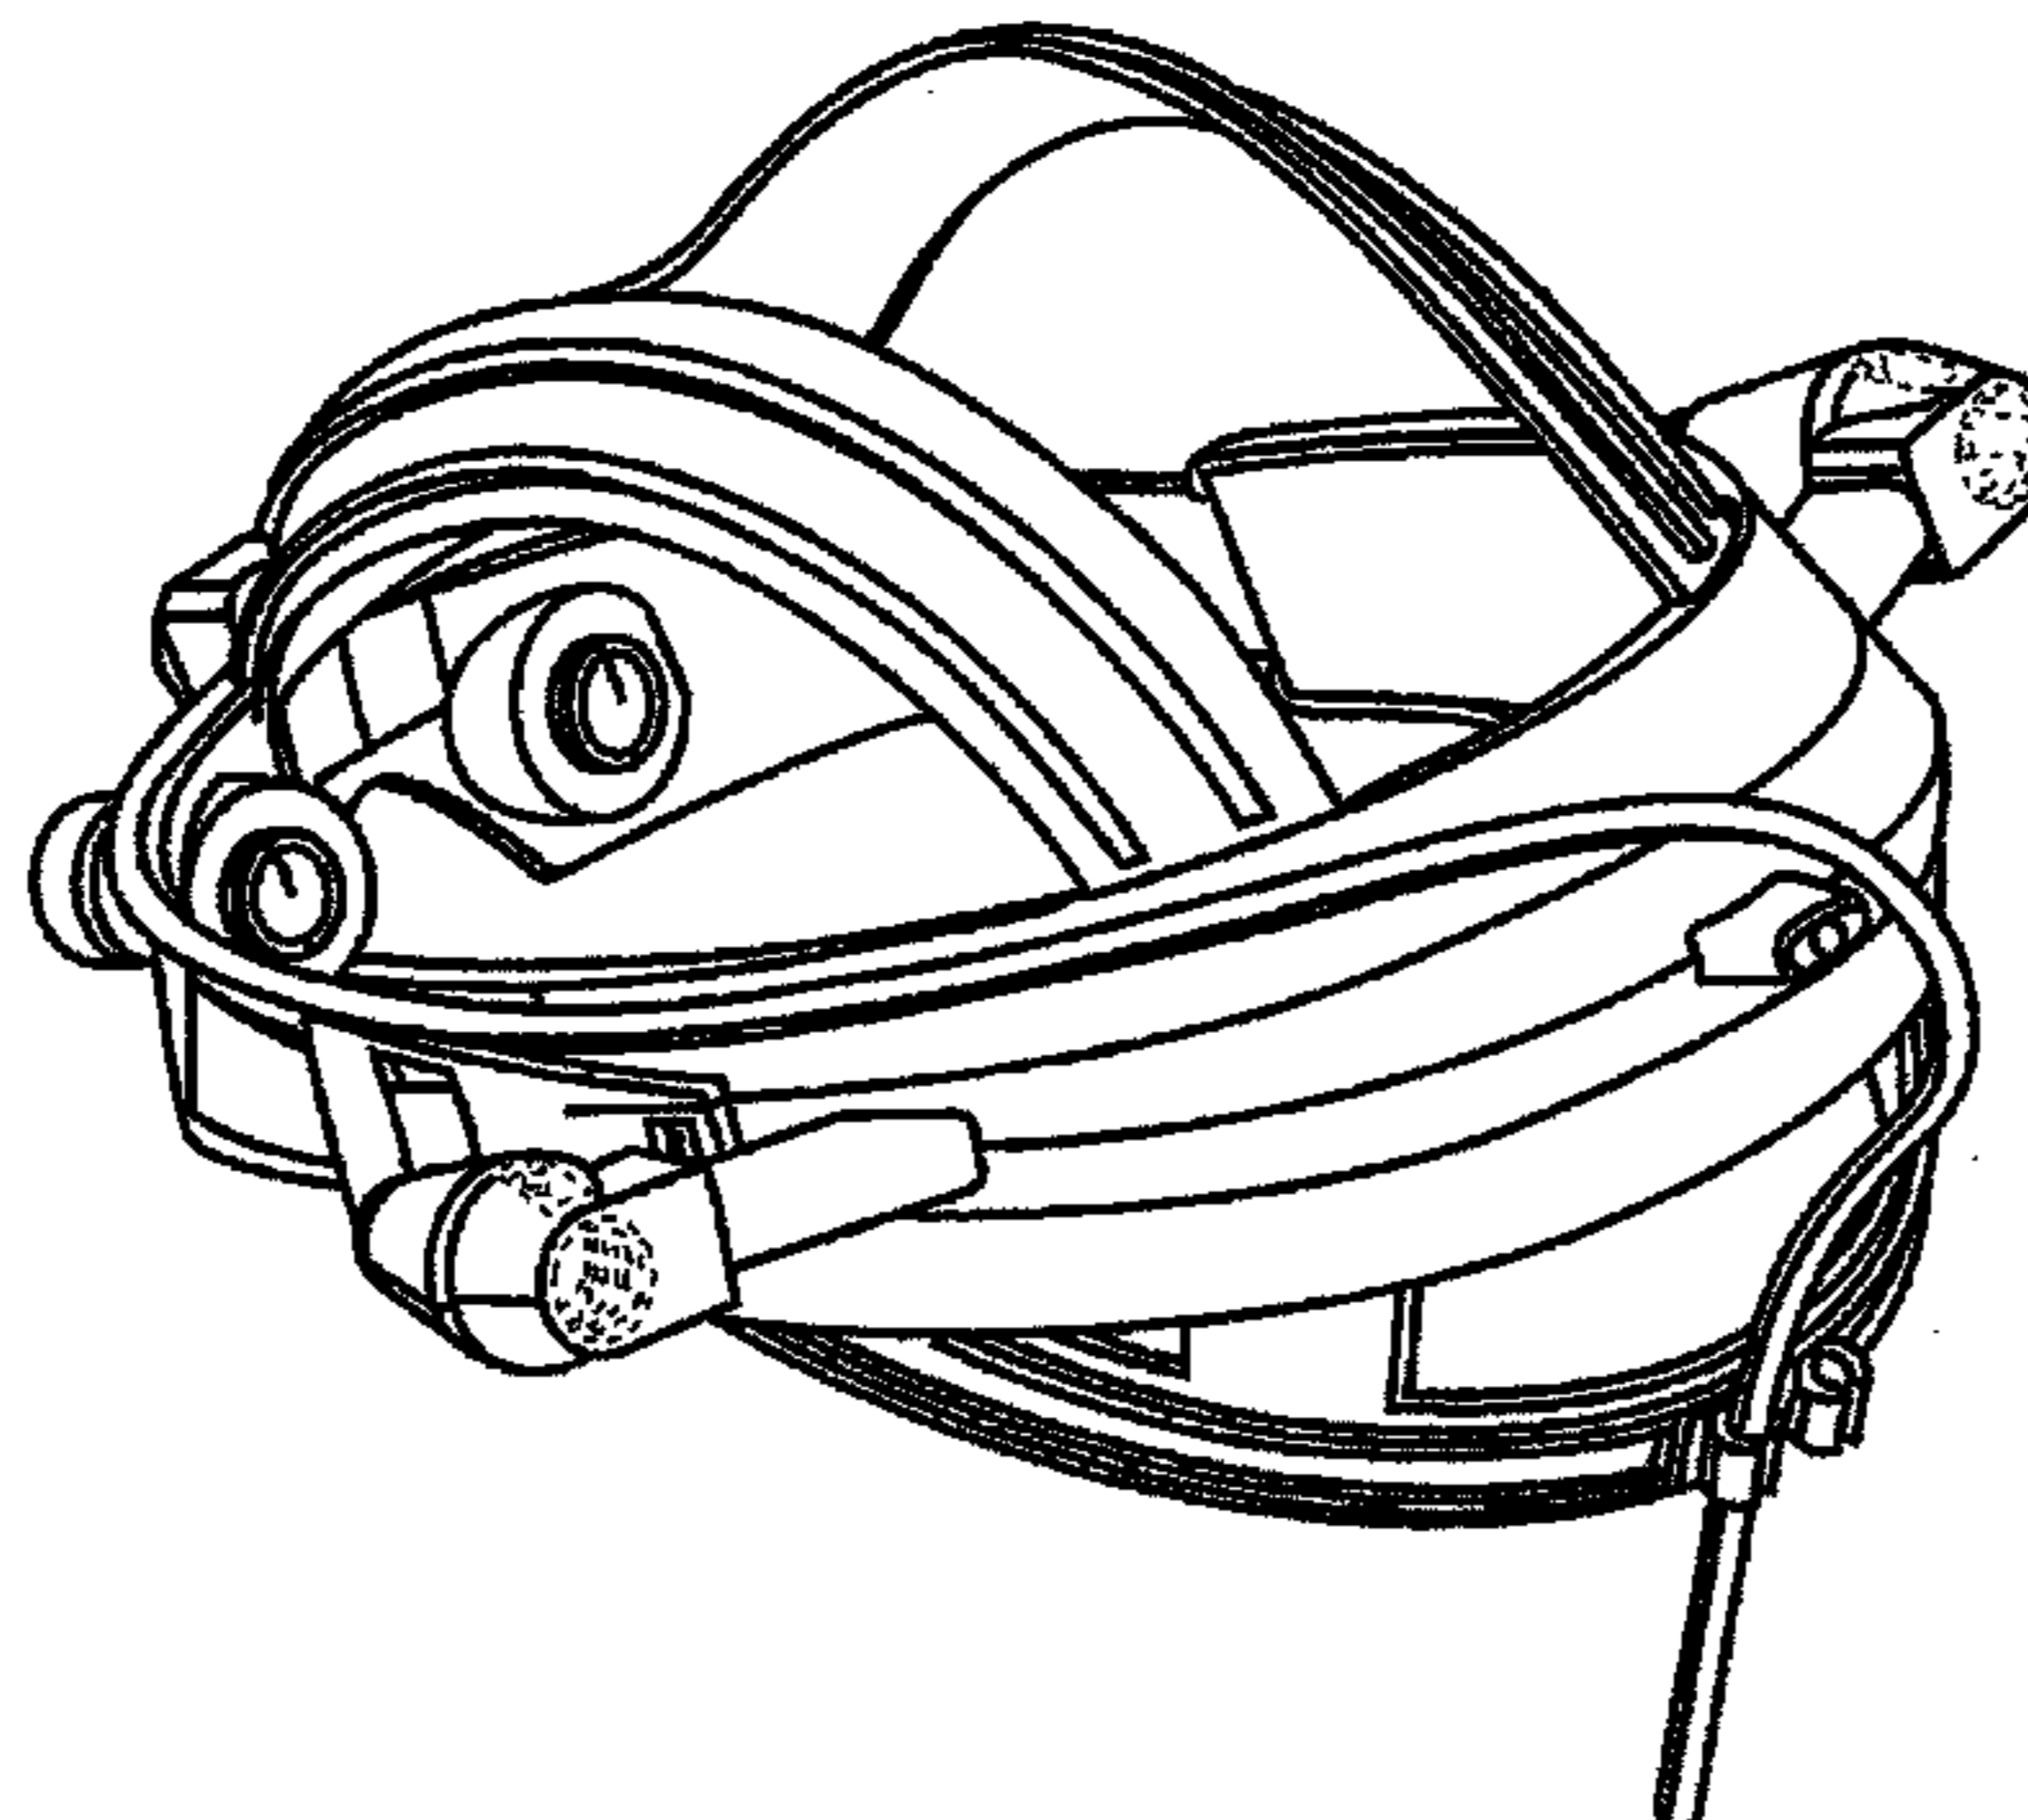


FIG. 10 is a rear isometric view of the head gear component;
FIG. 11 is a side isometric view of the head gear component;
FIG. 12 is a front isometric view of the head gear component;
FIG. 13 is a top isometric view of the head gear component;
FIG. 14 is a side isometric view of the optical loupe component;
FIG. 15 is a rear isometric view of the optical loupe component;
FIG. 16 is a front isometric view of the optical loupe component;
FIG. 17 is a side isometric view of the optical loupe component;
FIG. 18 is a side isometric view of the optical loupe component;
FIG. 19 is a top isometric view of the optical loupe component;
FIG. 20 is a bottom isometric view of the optical loupe component;
FIG. 21 is a side isometric view of the lighting component;
FIG. 22 is a rear isometric view of the lighting component;
FIG. 23 is a front isometric view of the lighting component;
FIG. 24 is a bottom isometric view of the lighting component;
FIG. 25 is a top isometric view of the lighting component;
FIG. 26 is a side isometric view of the lighting component;
FIG. 27 is a rear isometric view of the lighting component;
FIG. 28 is a side isometric view of the head gear component with the optical loupe component;
FIG. 29 is a rear isometric view of the head gear component with the optical loupe component;

FIG. 30 is another rear isometric view of the head gear component with the optical loupe component;
FIG. 31 is a side isometric view of the head gear component with the optical loupe component;
FIG. 32 is a front isometric view of the head gear component with the optical loupe component;
FIG. 33 is a top isometric view of the head gear component with the optical loupe component;
FIG. 34 is an enlarged isometric view of the head gear component with the optical loupe component;
FIG. 35 is a side isometric view of the head gear component with the lighting component;
FIG. 36 is a rear isometric view of the head gear component with the lighting component;
FIG. 37 is another rear isometric view of the head gear component with the lighting component;
FIG. 38 is a side isometric view of the head gear component with the lighting component;
FIG. 39 is a front isometric view of the head gear component with the lighting component;
FIG. 40 is a top isometric view of the head gear component with the lighting component; and,
FIG. 41 is an enlarged isometric view of the head gear component with the lighting component.

The broken lines are included for the purpose of illustrating a portion of the medical loupe head set that forms no part of the claimed design.

1 Claim, 21 Drawing Sheets

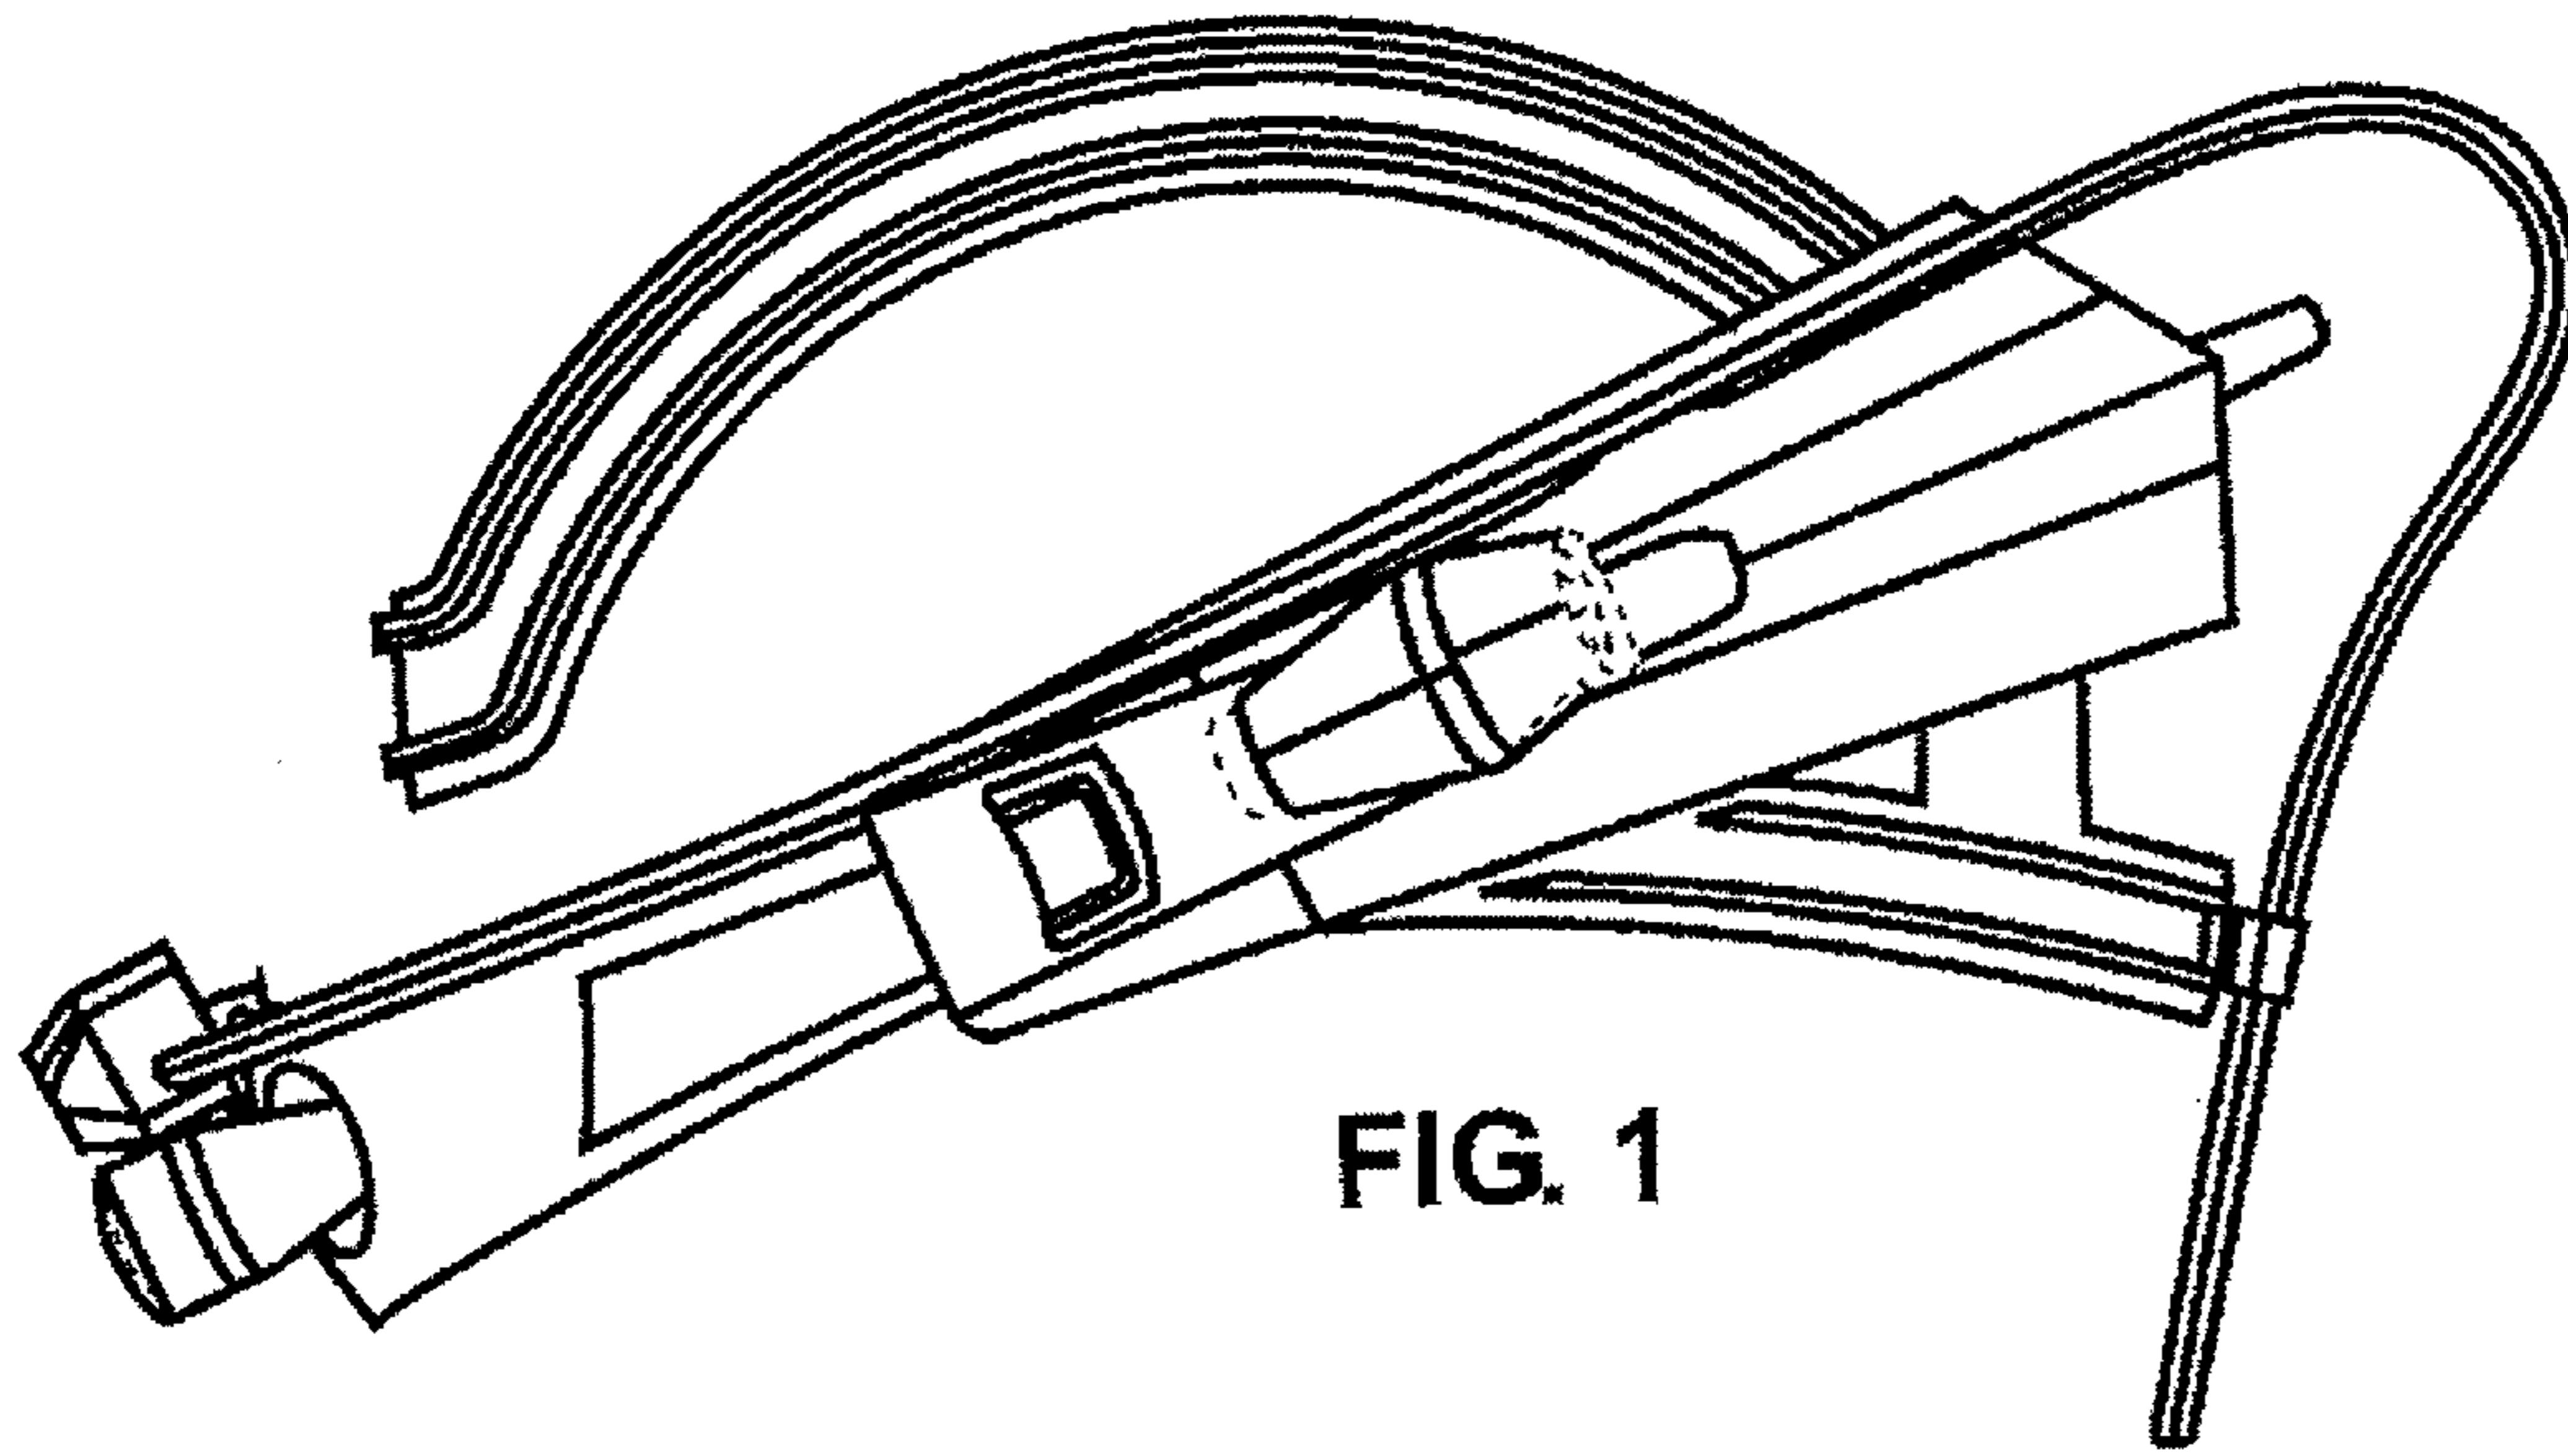


FIG. 1

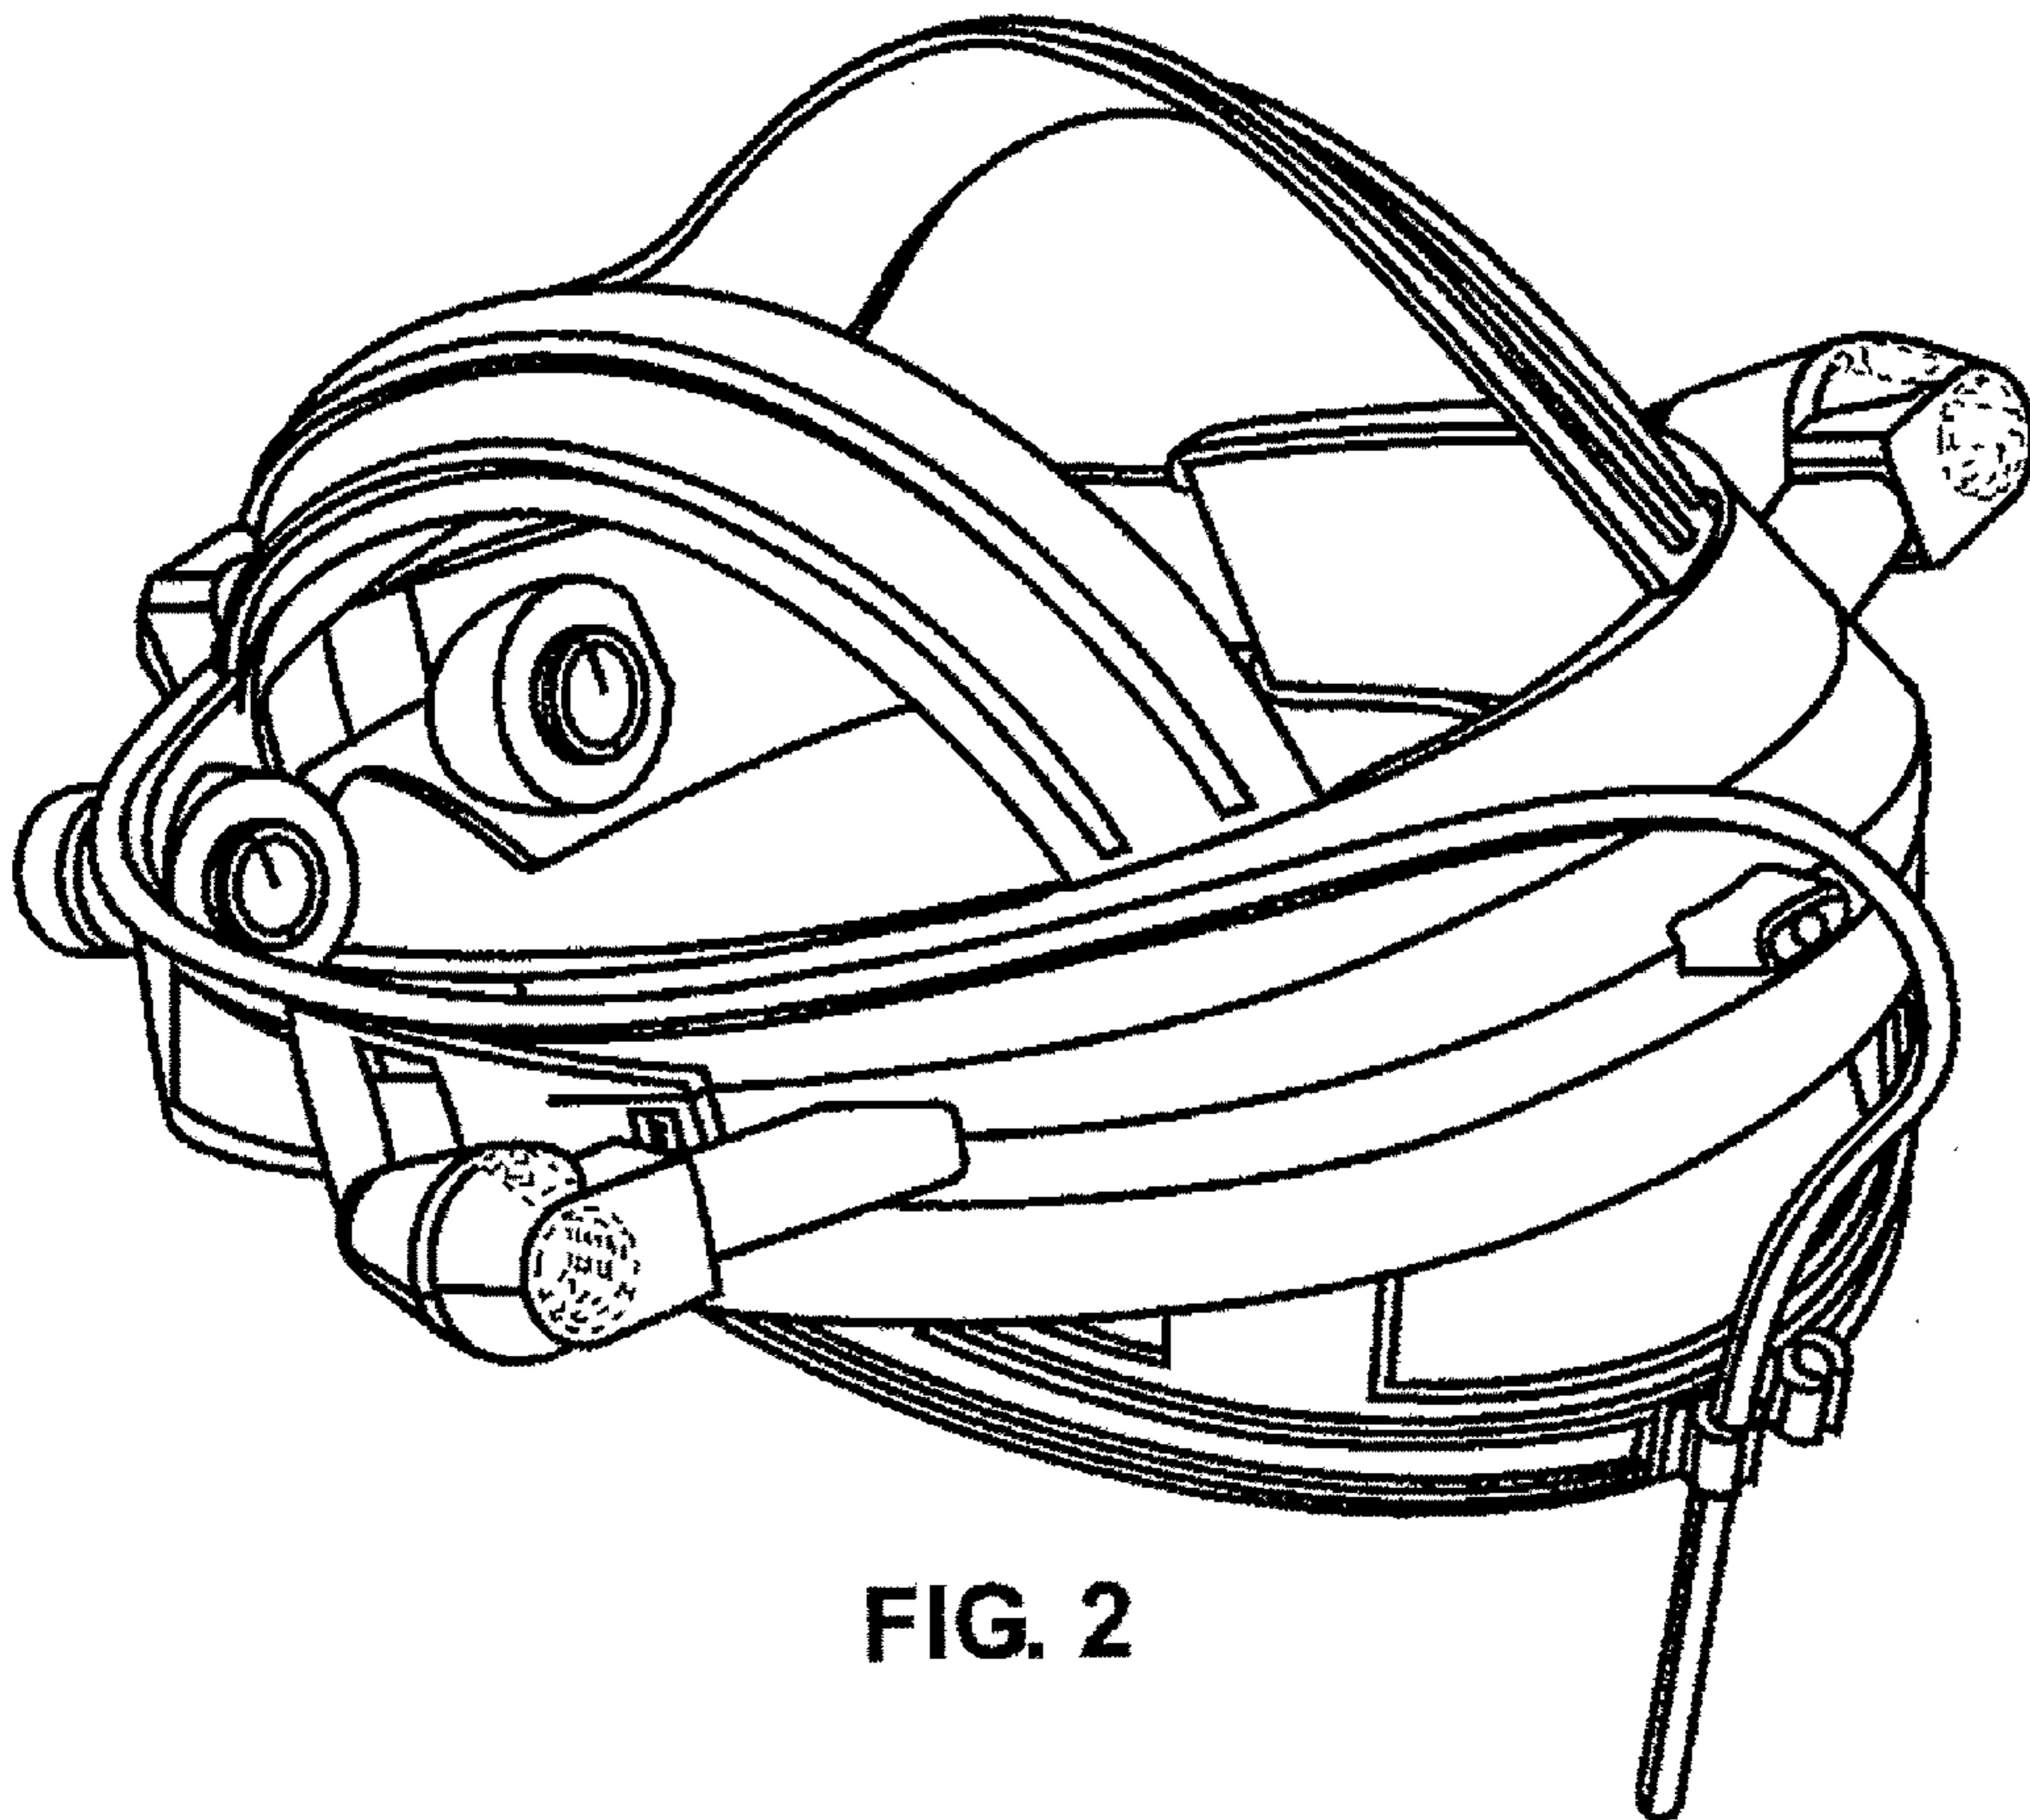
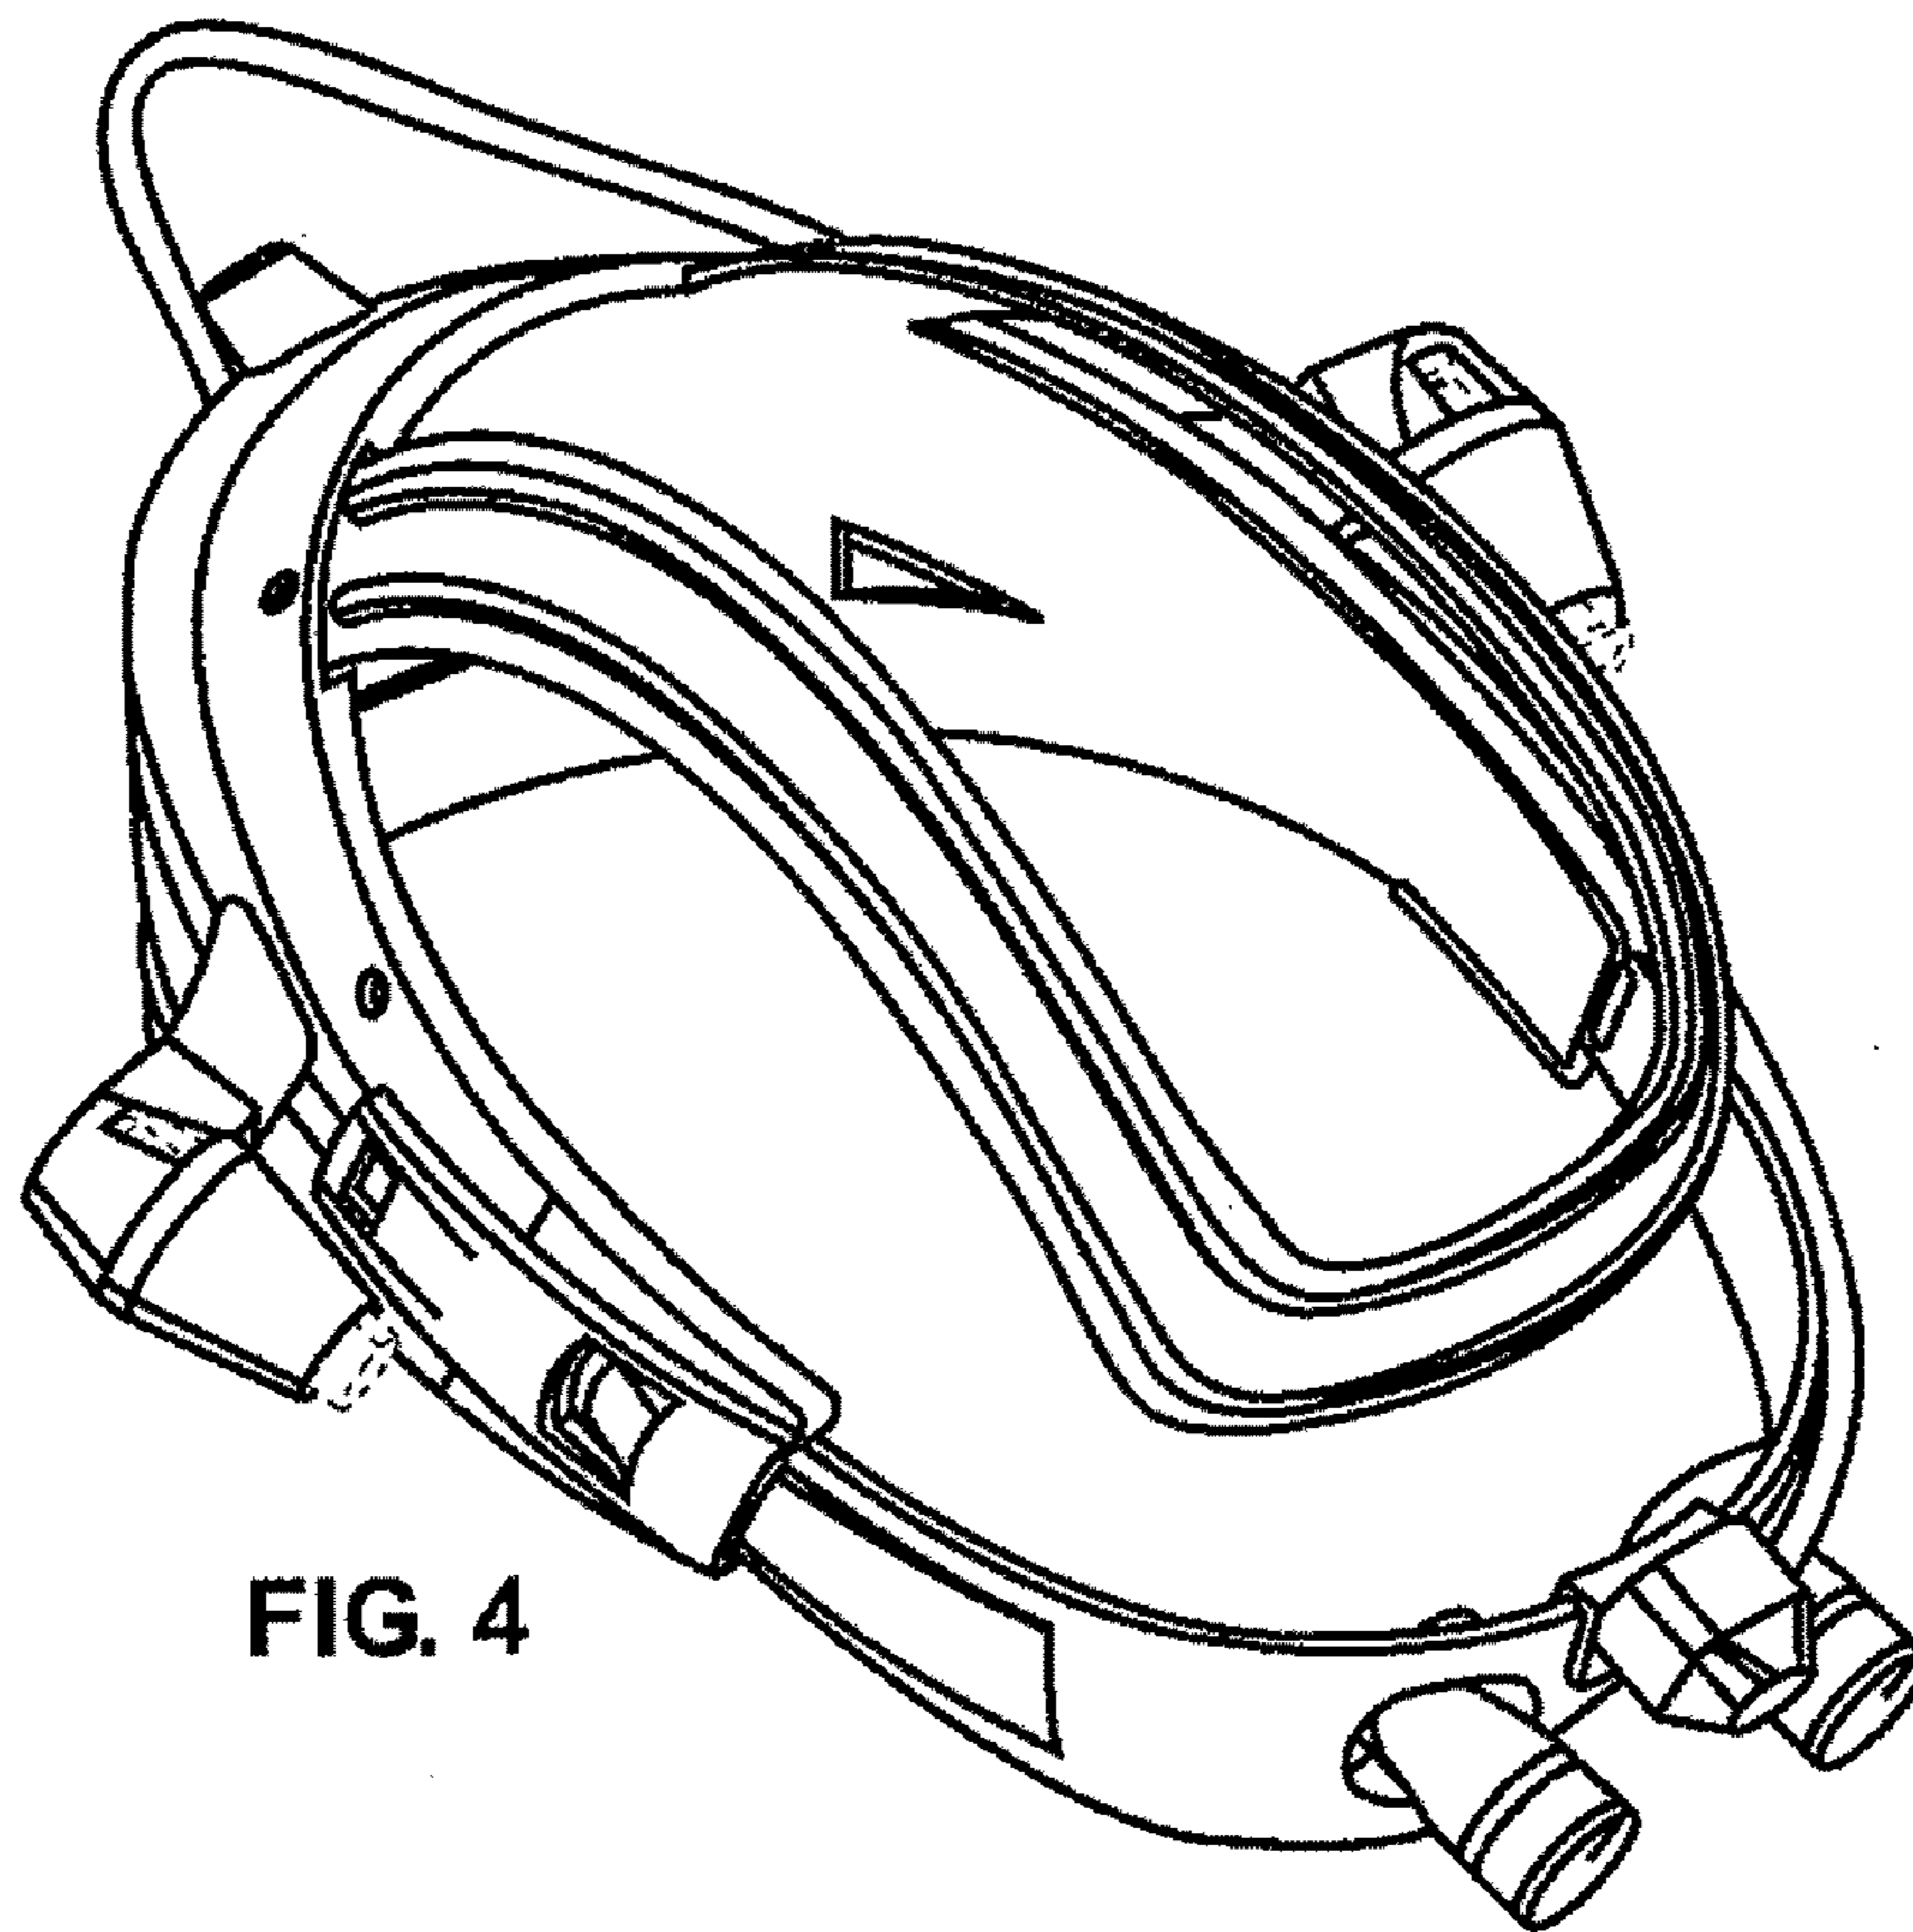
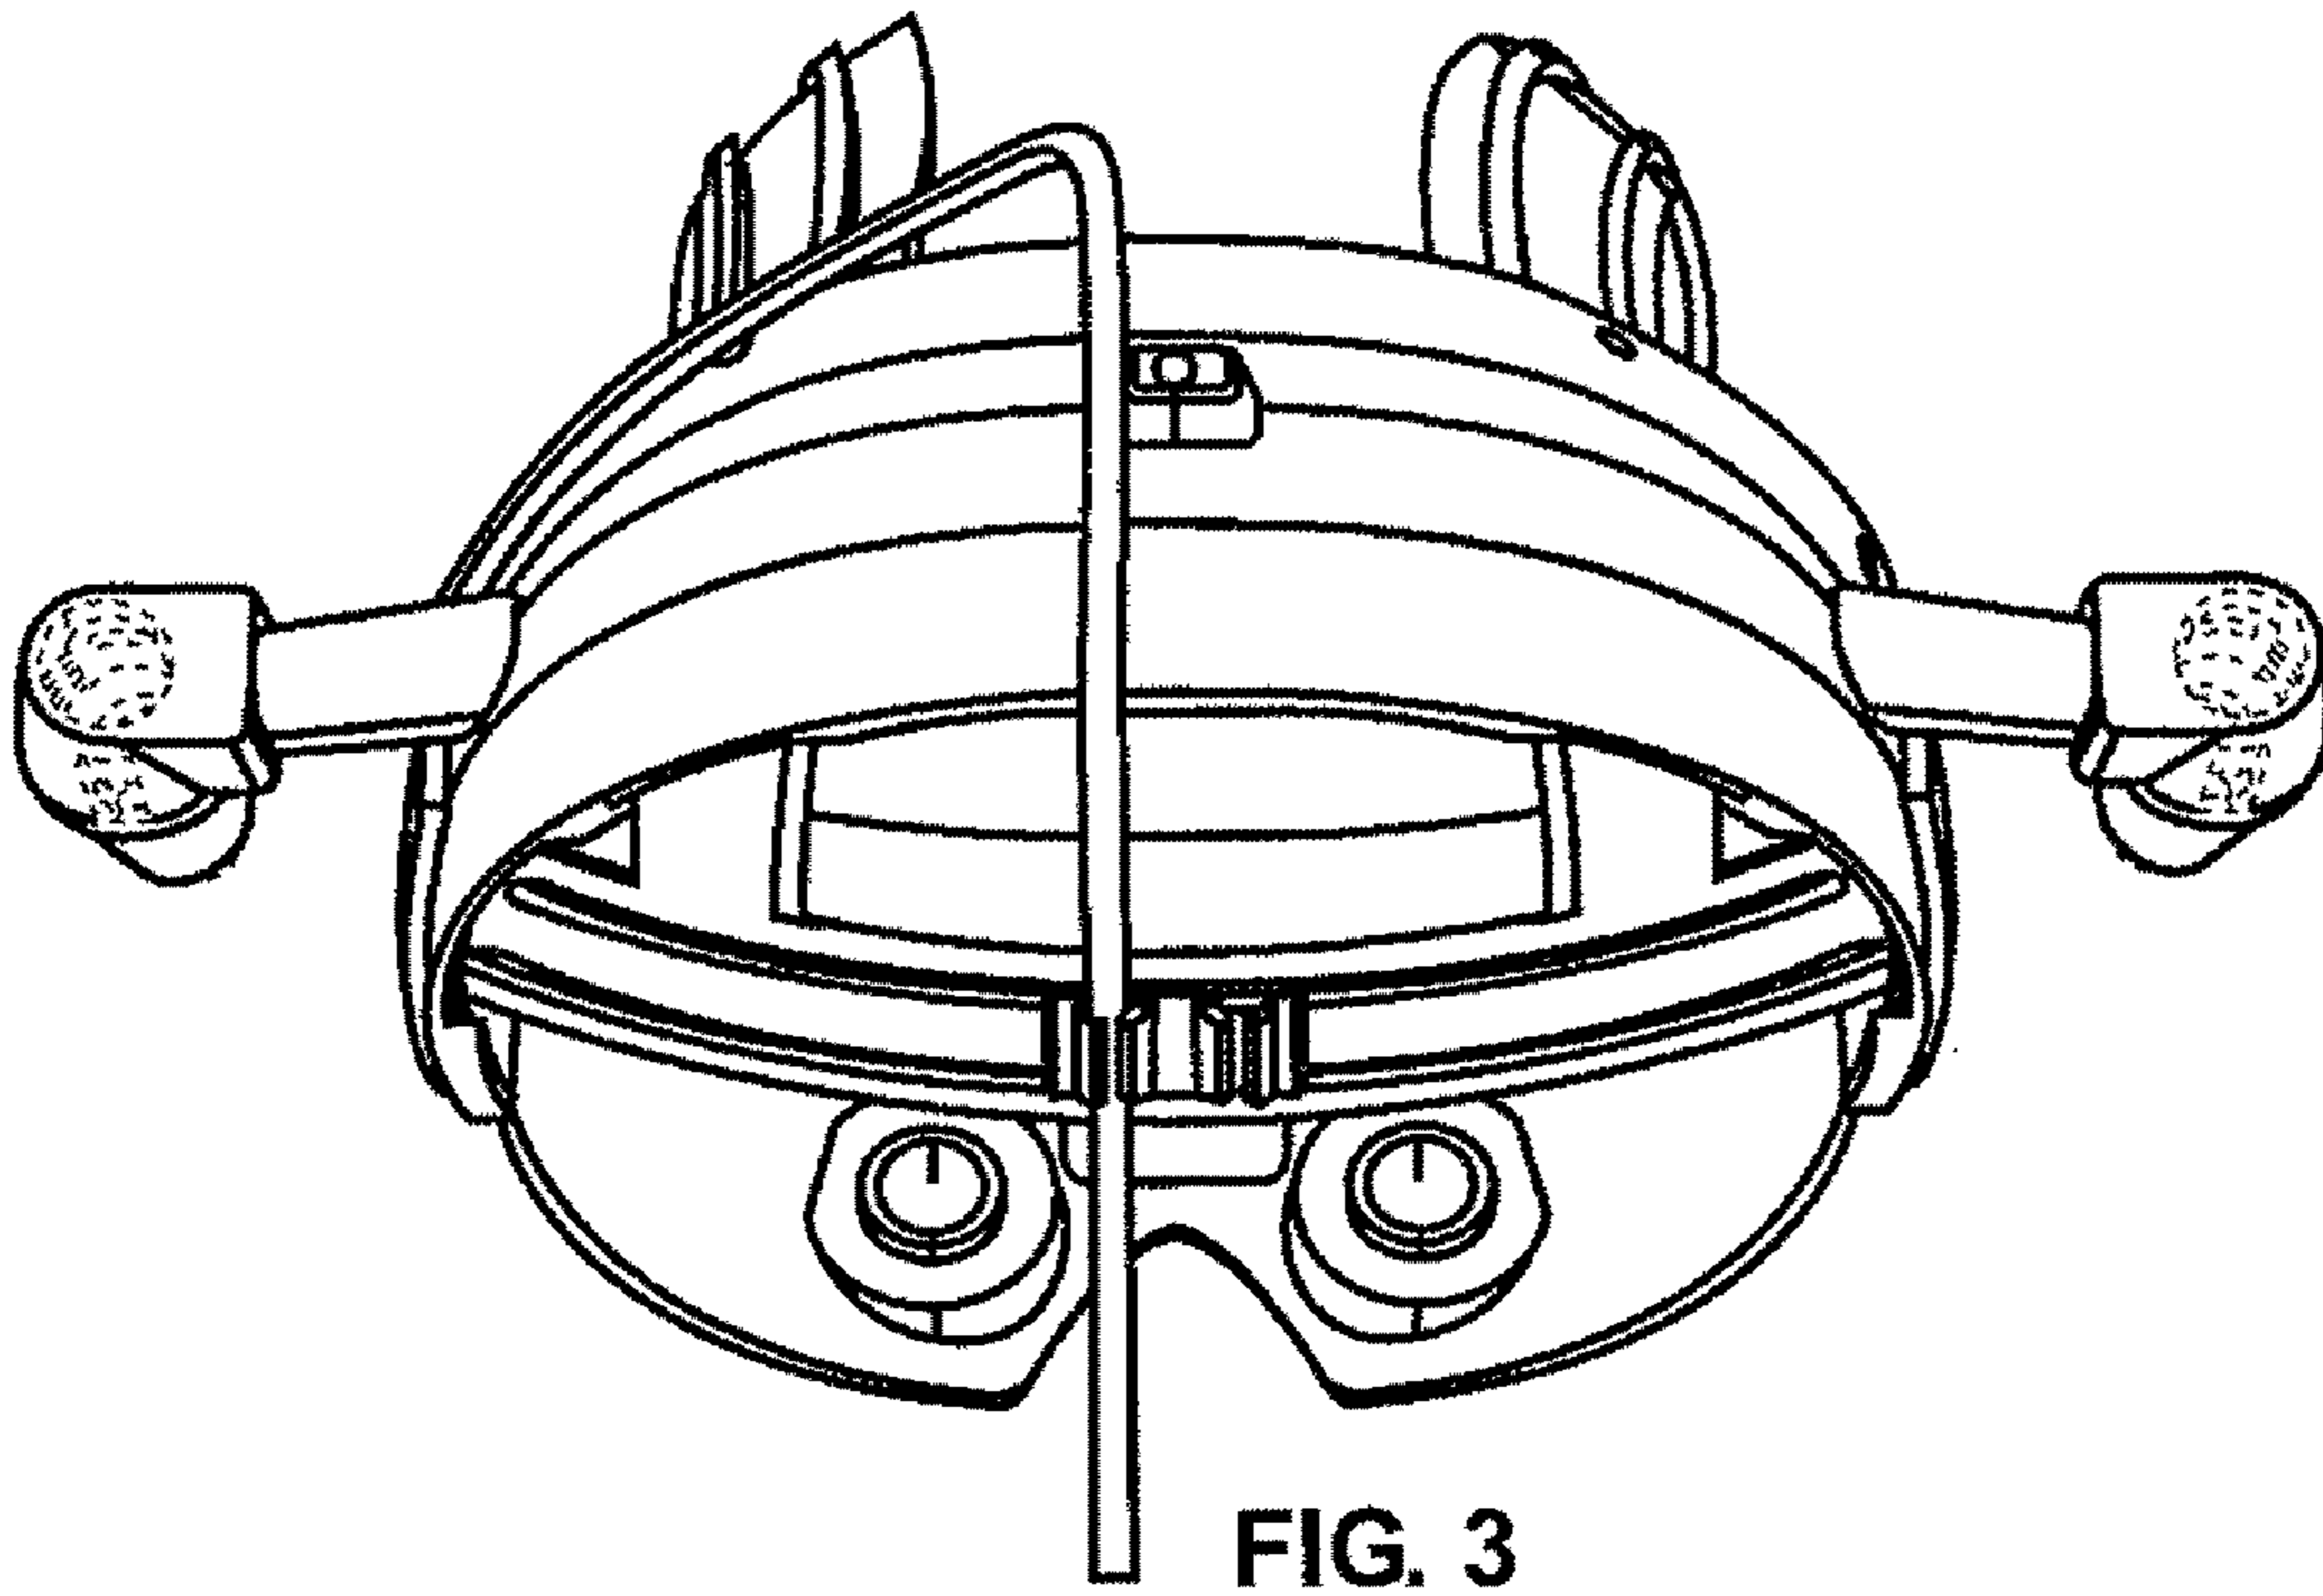
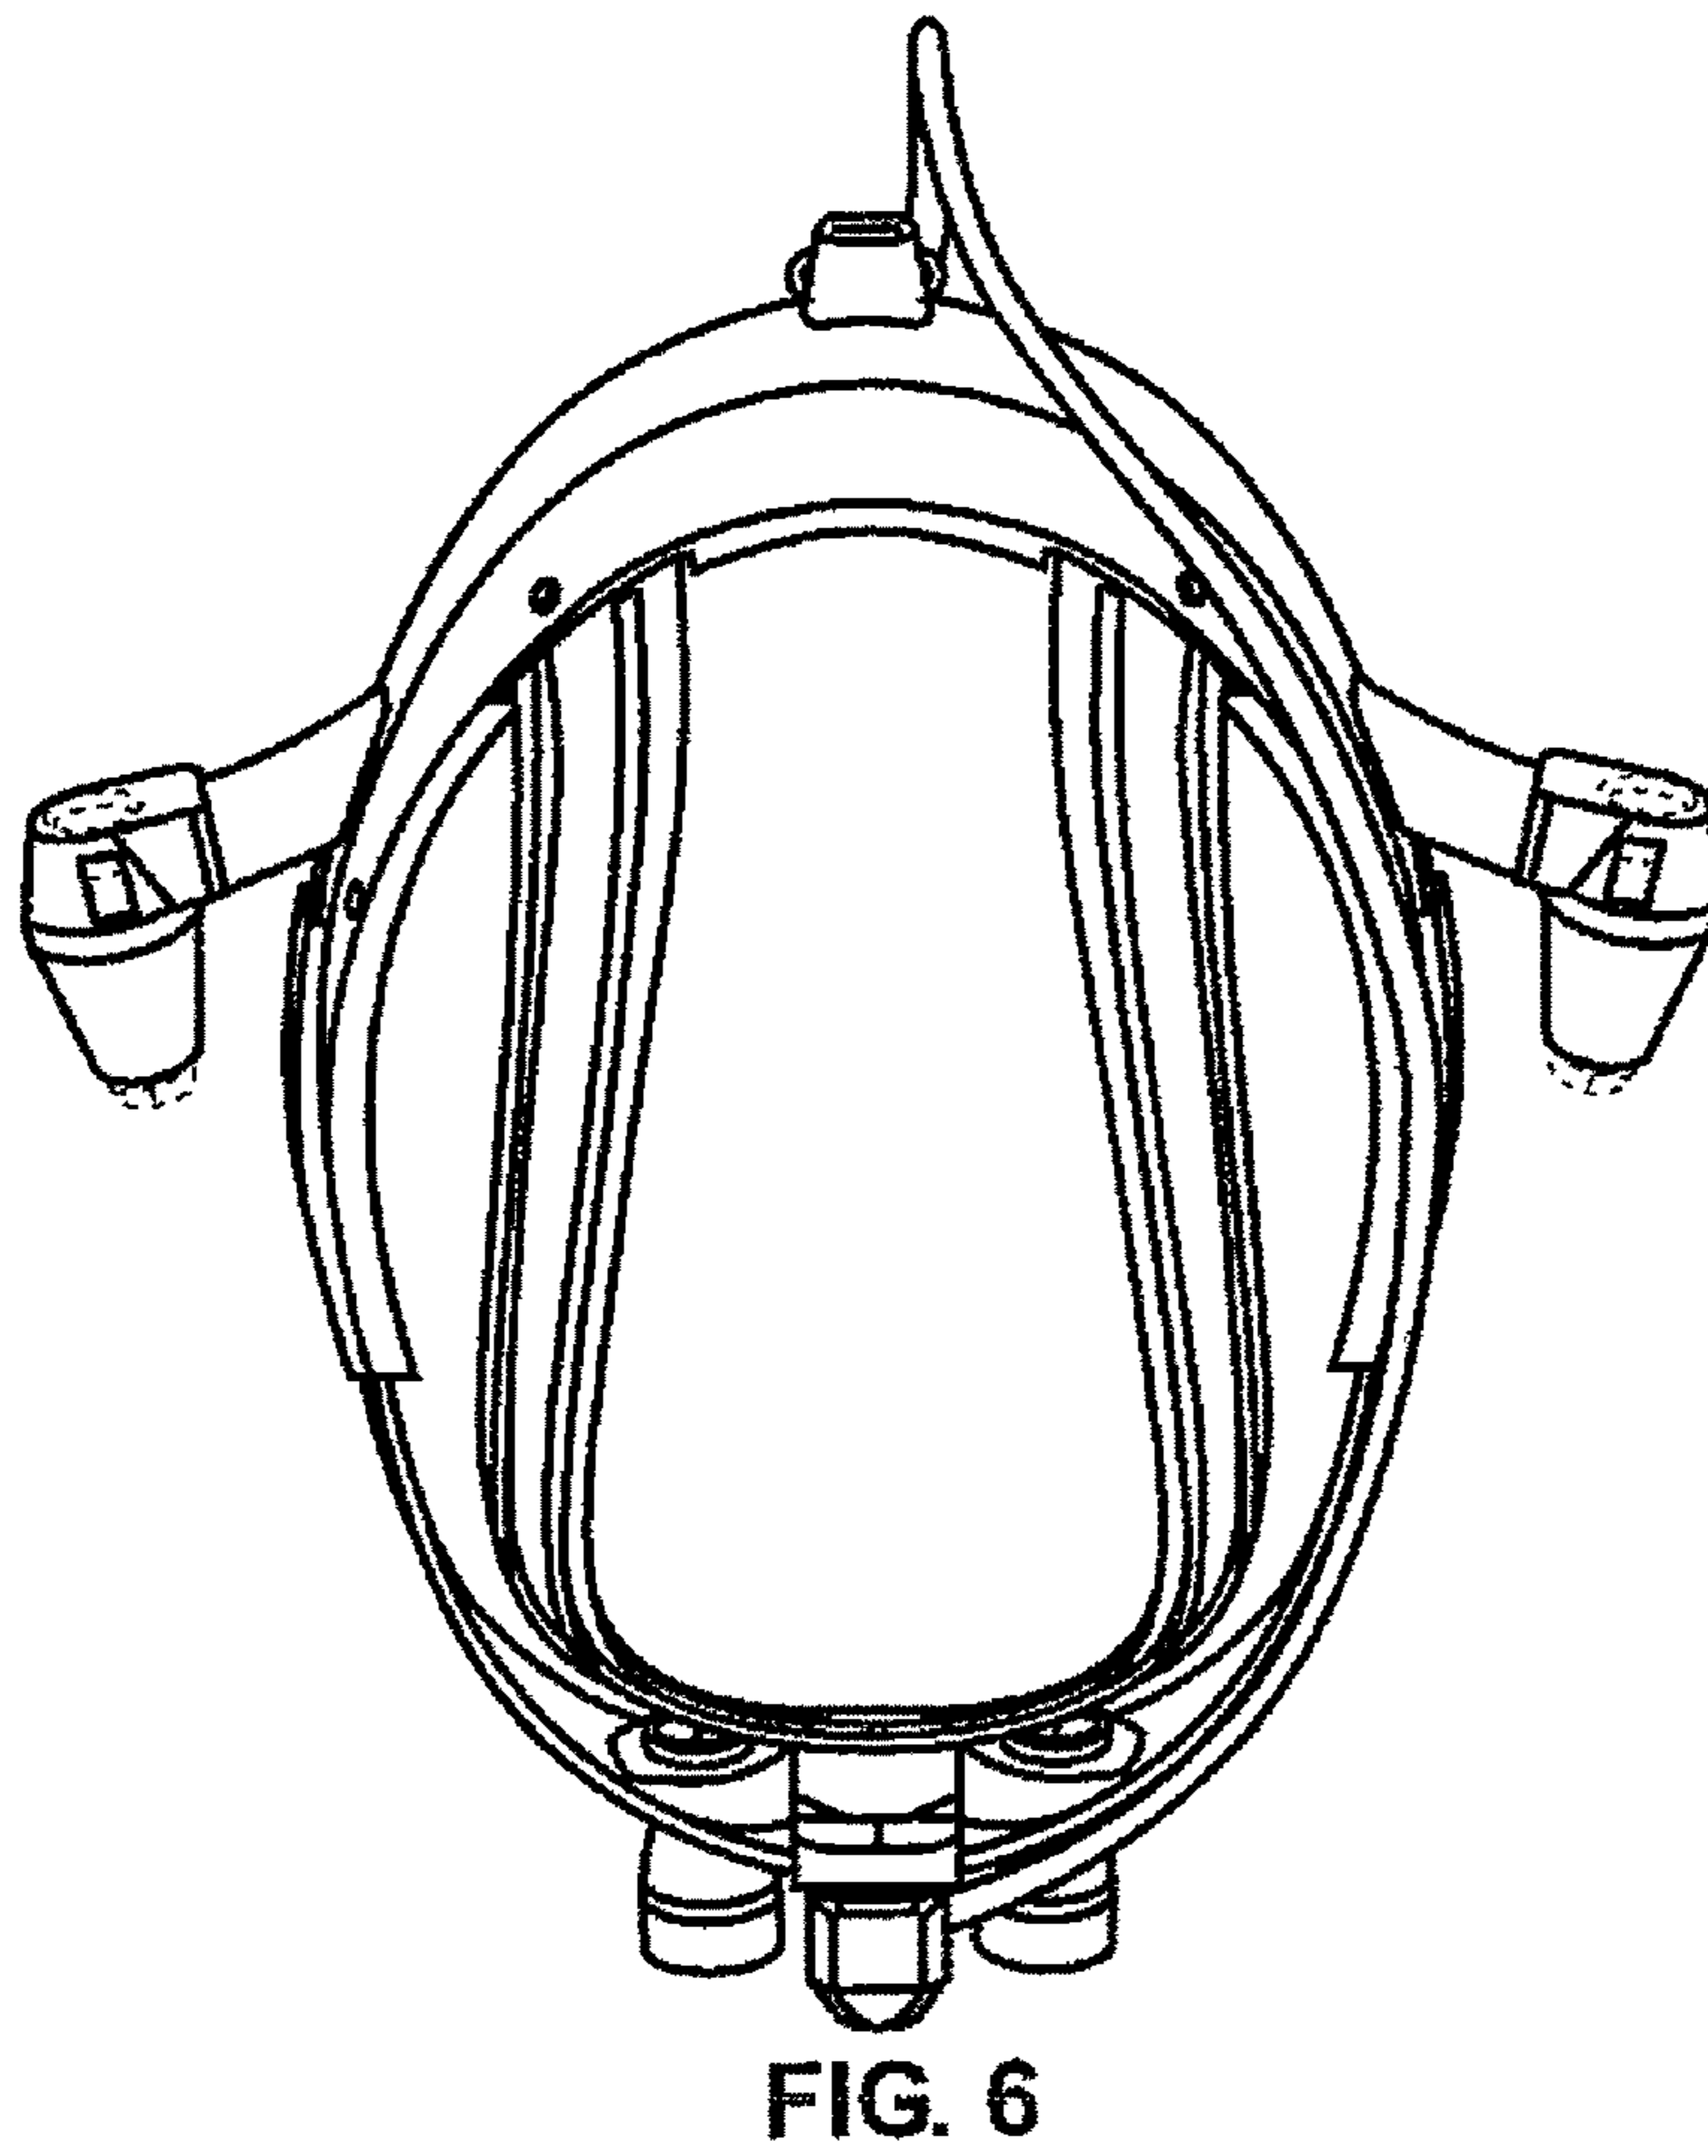
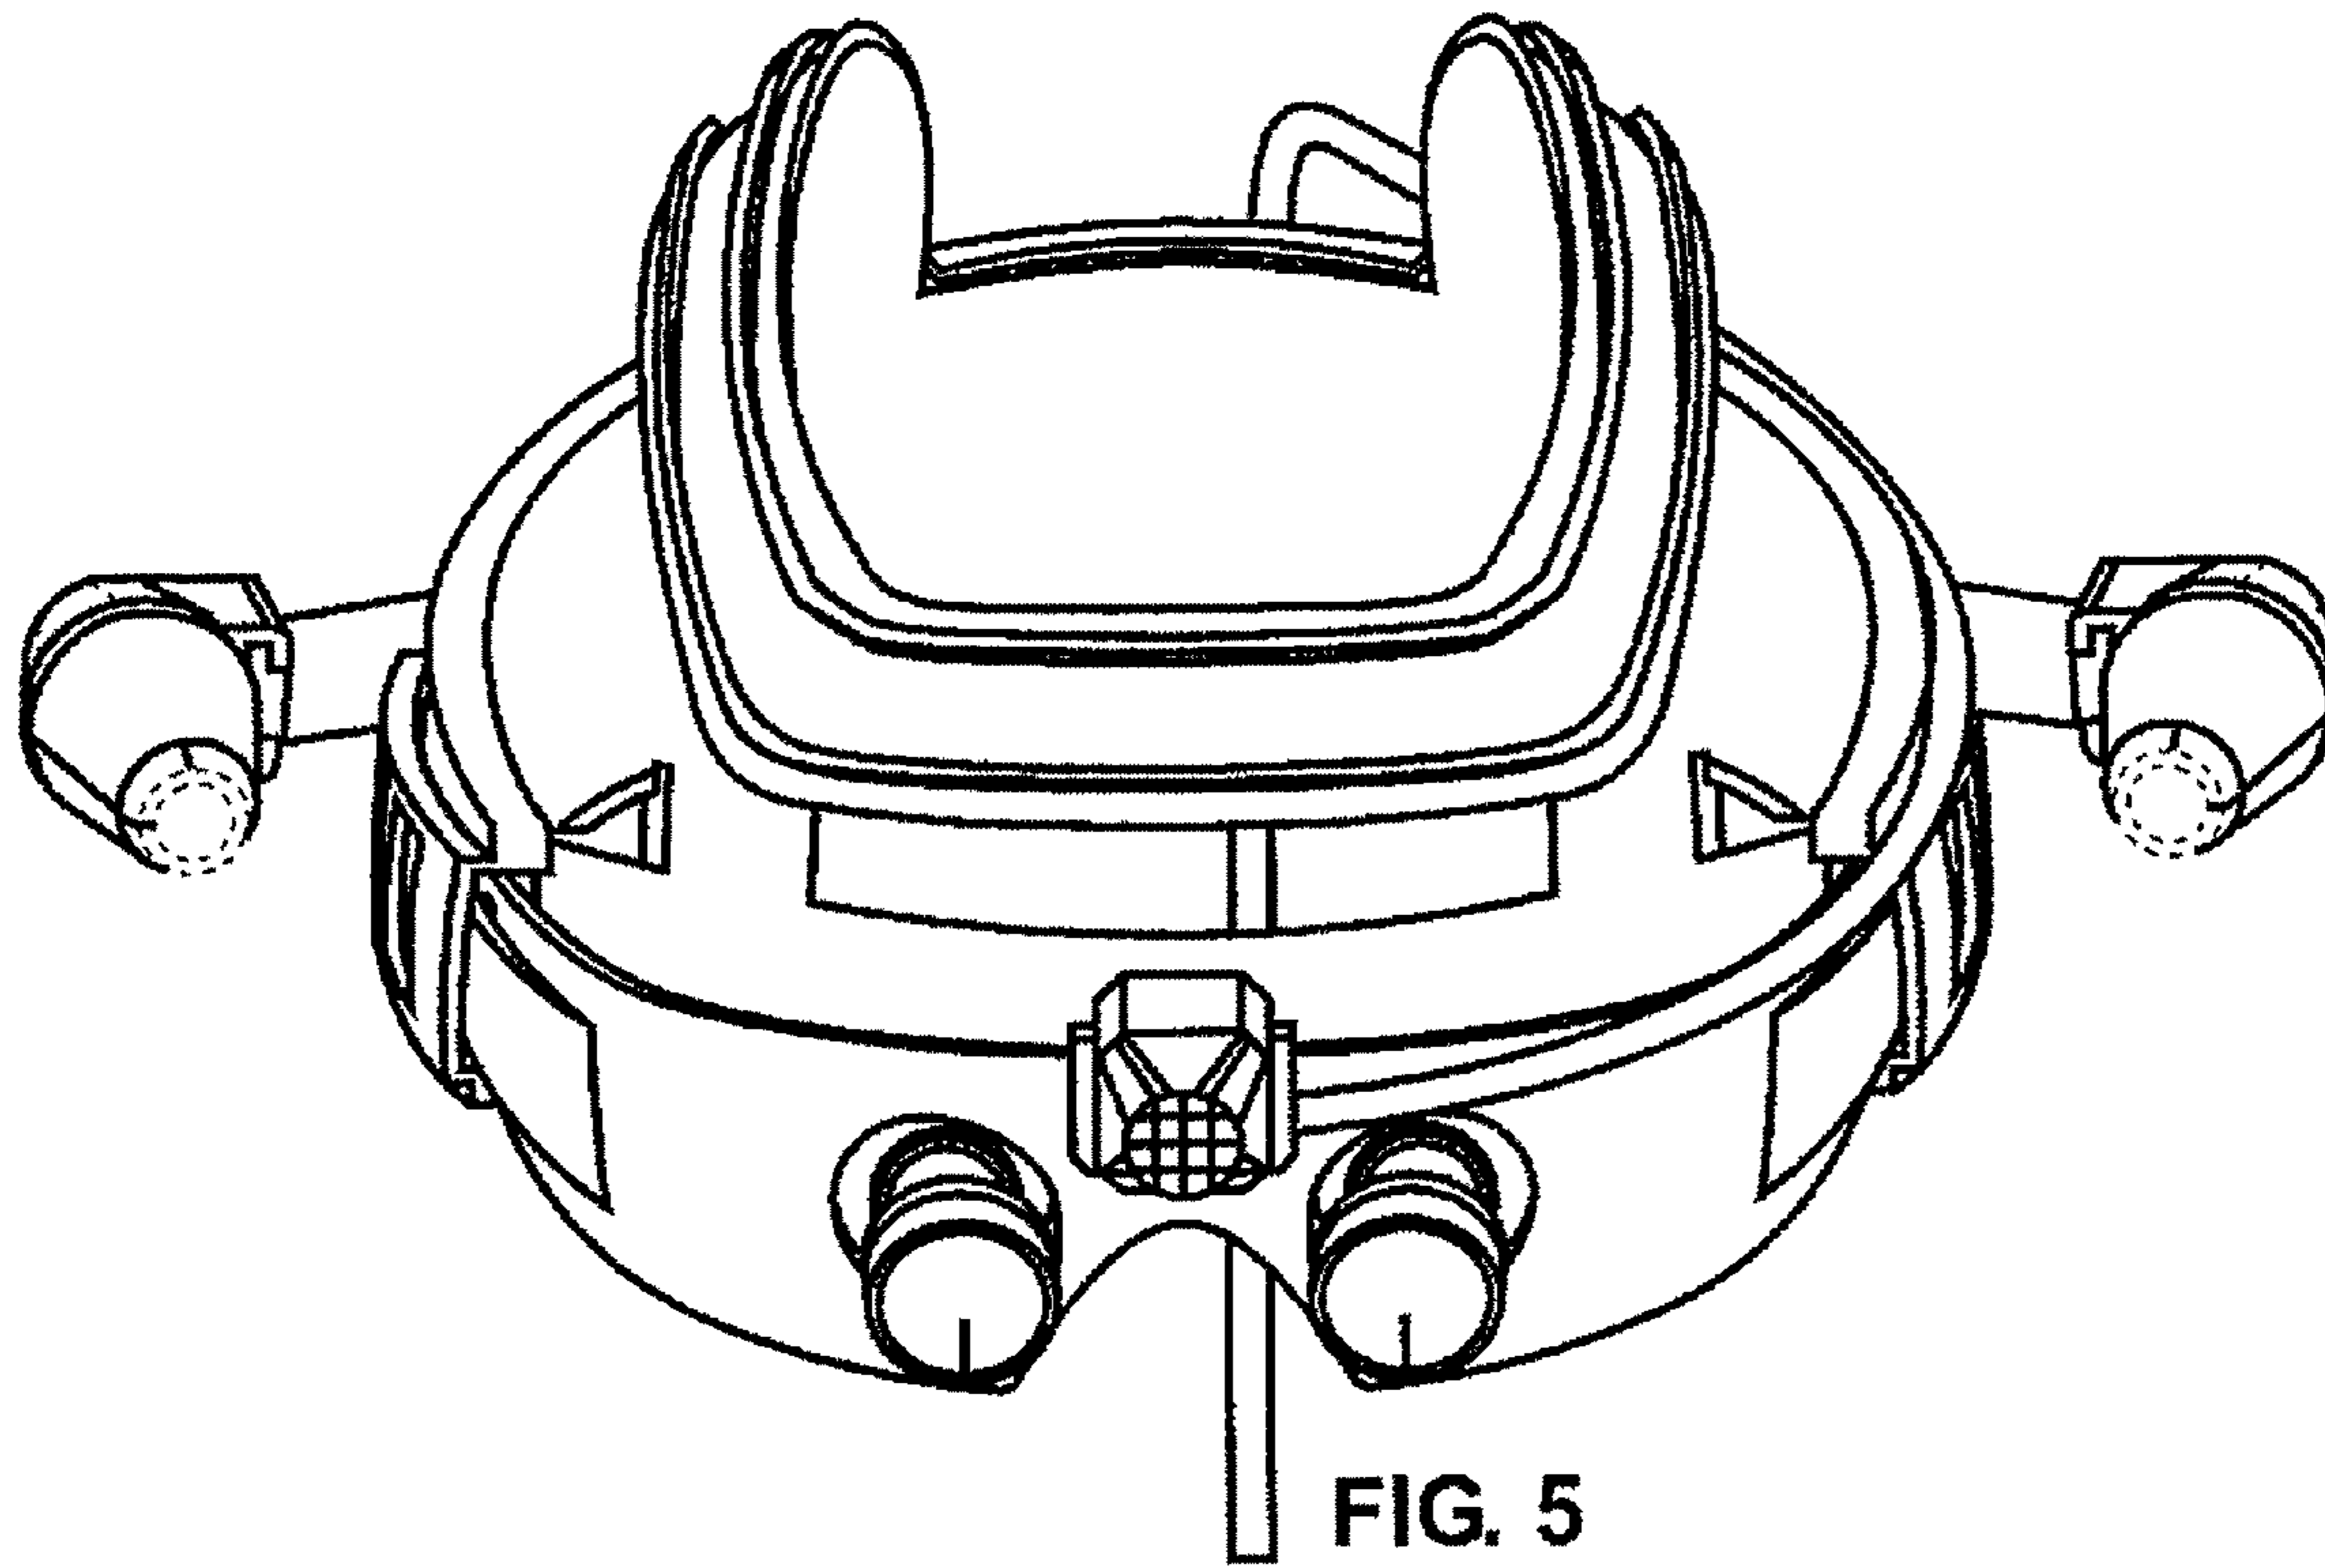
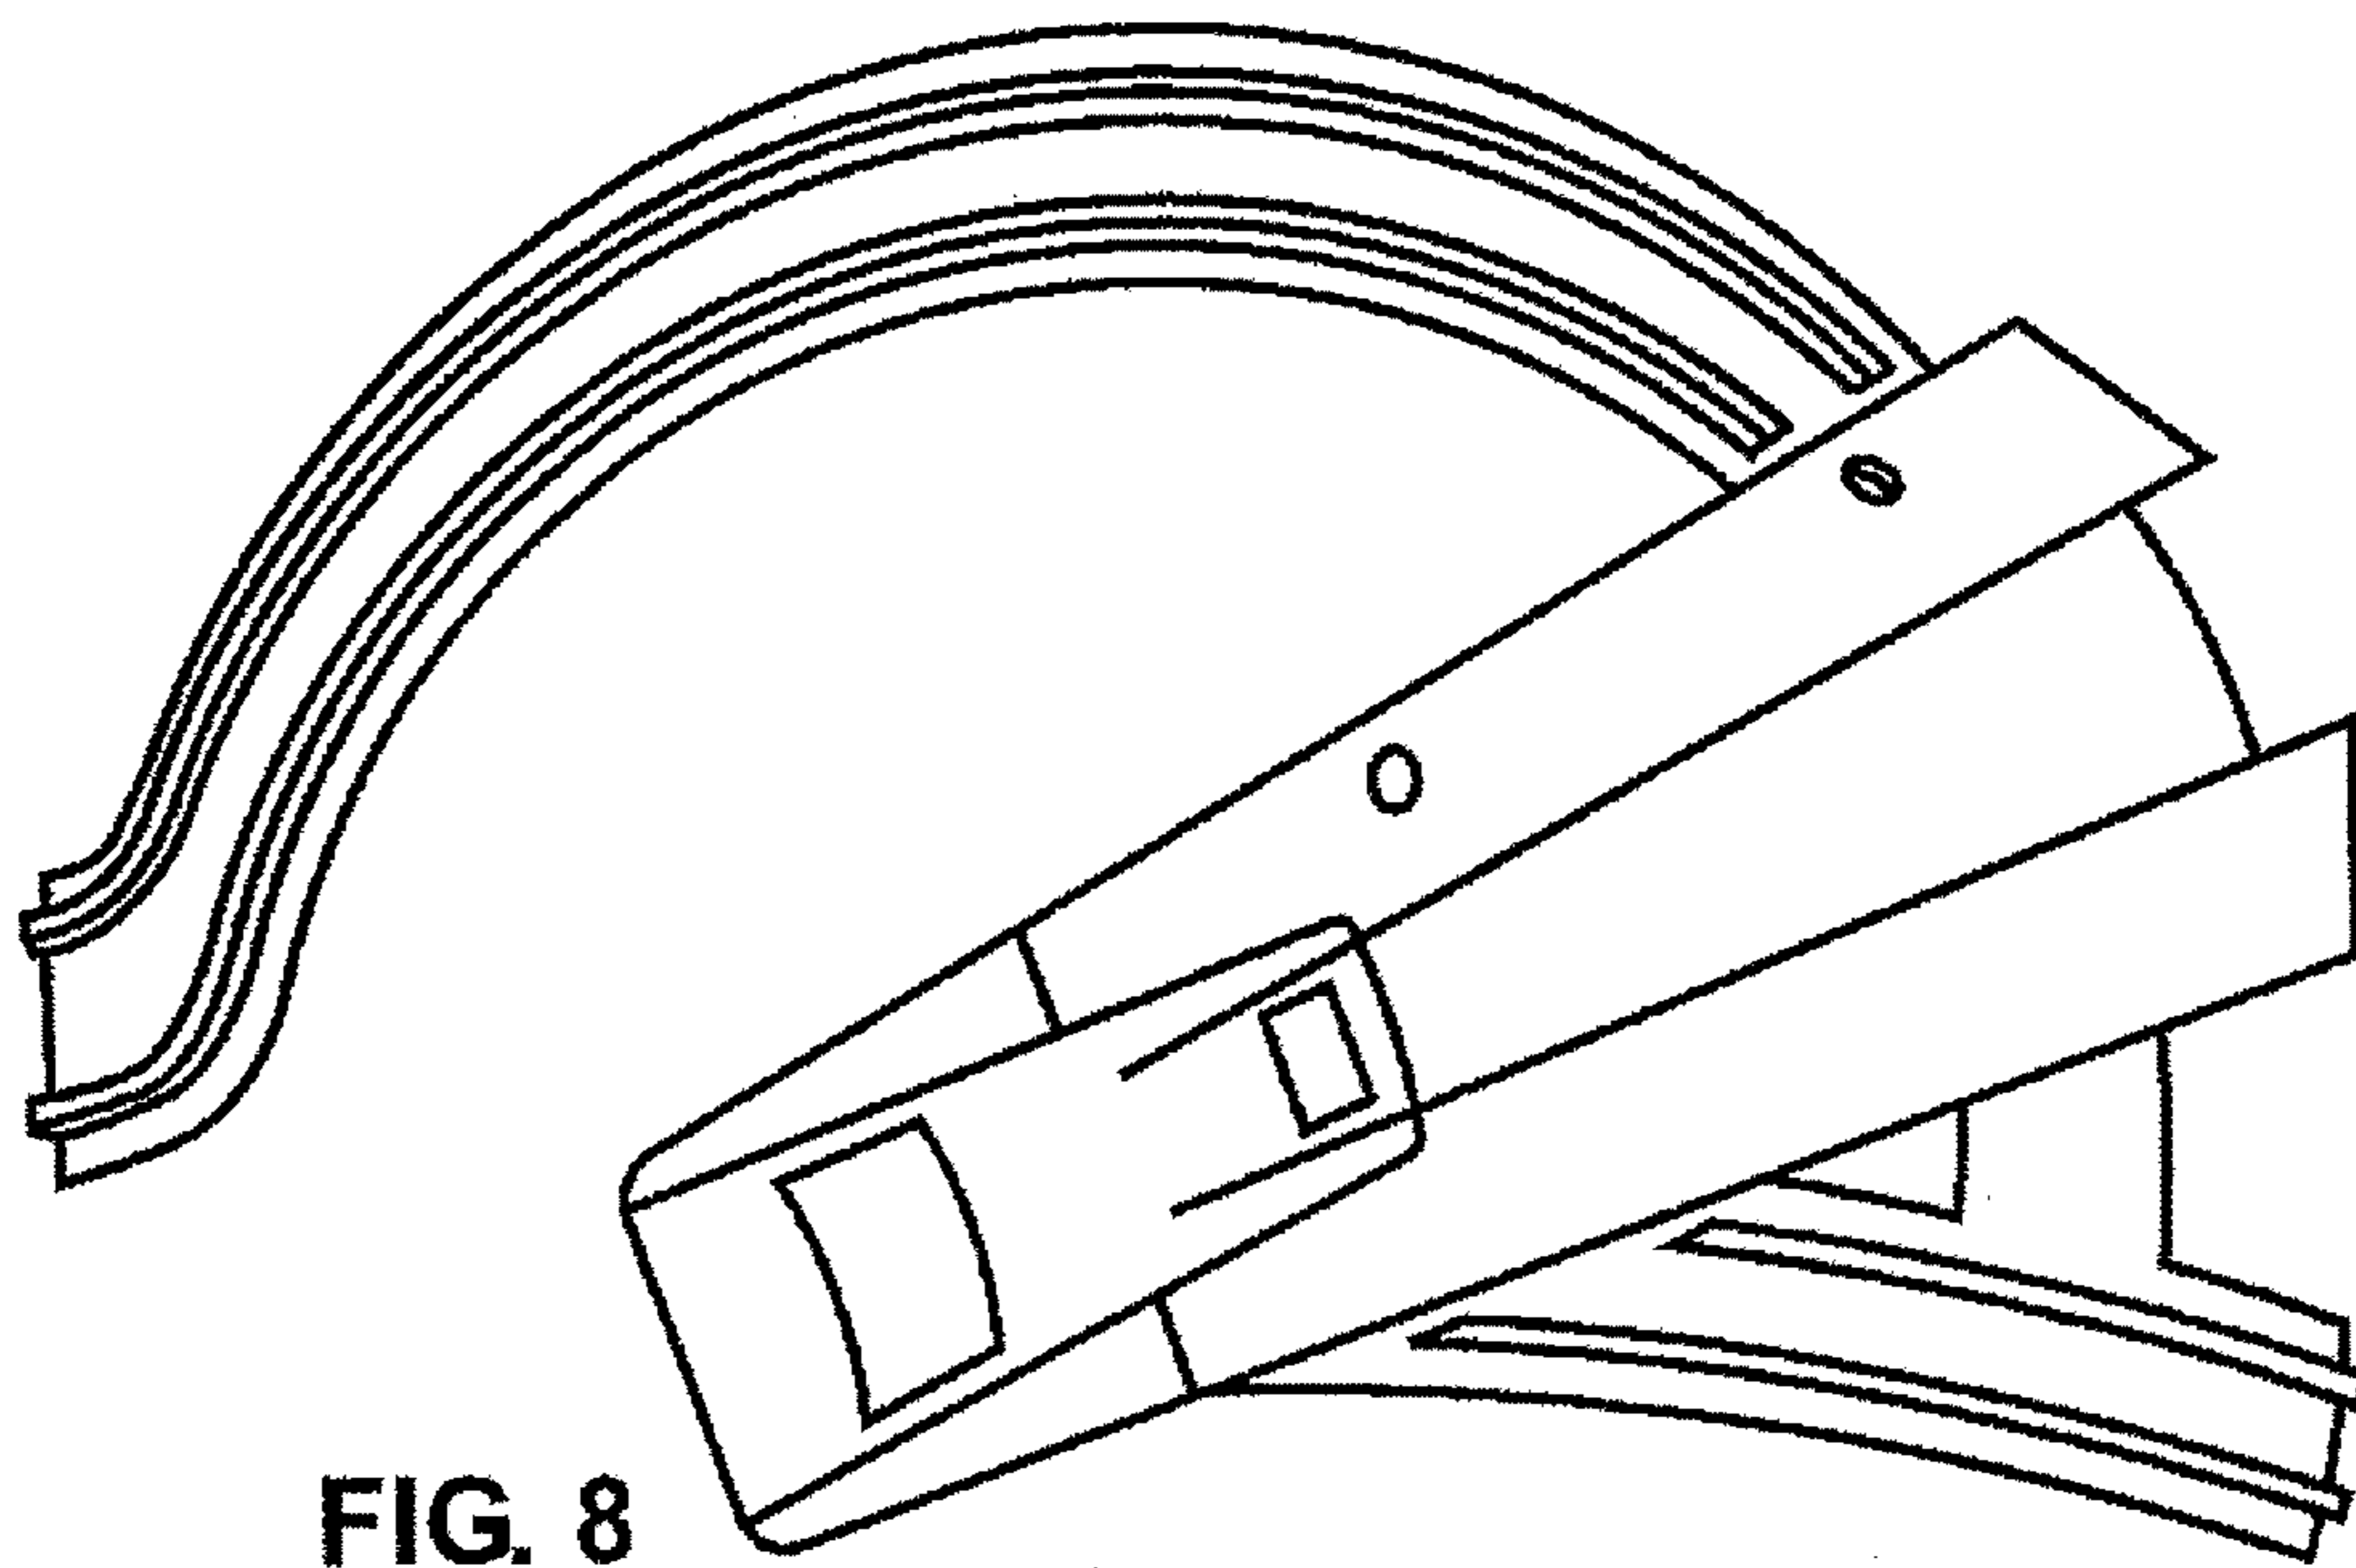
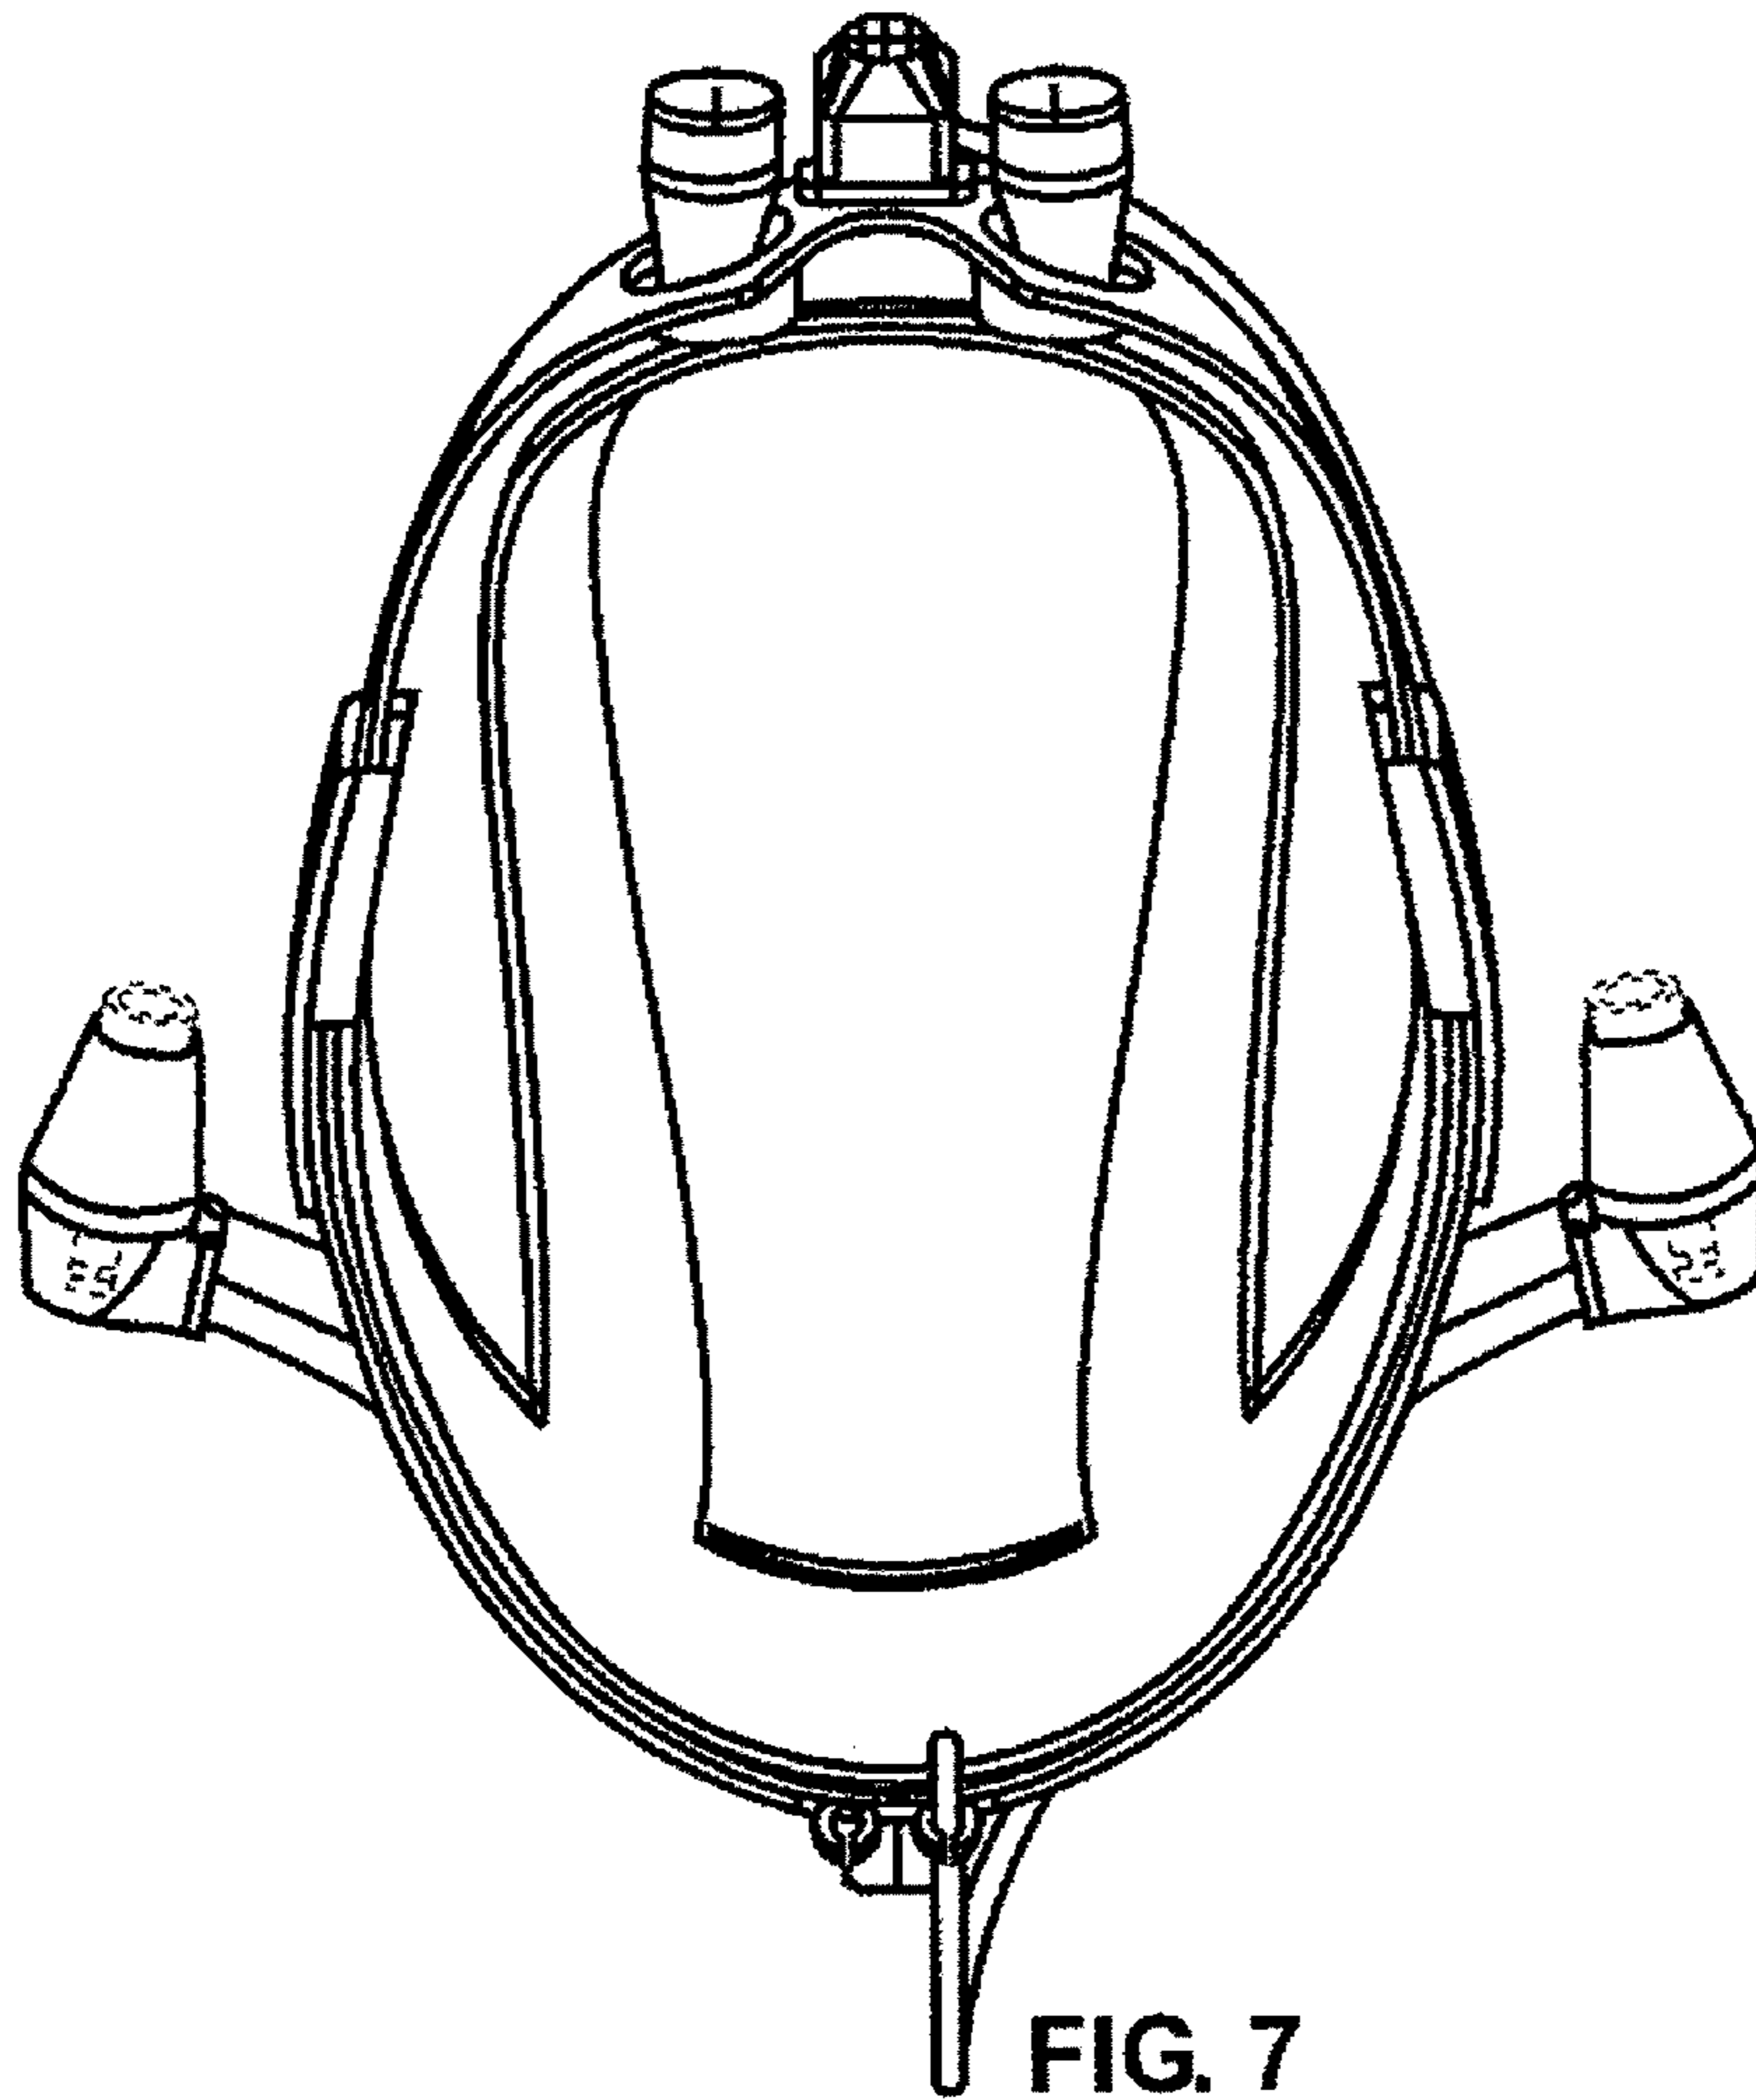


FIG. 2







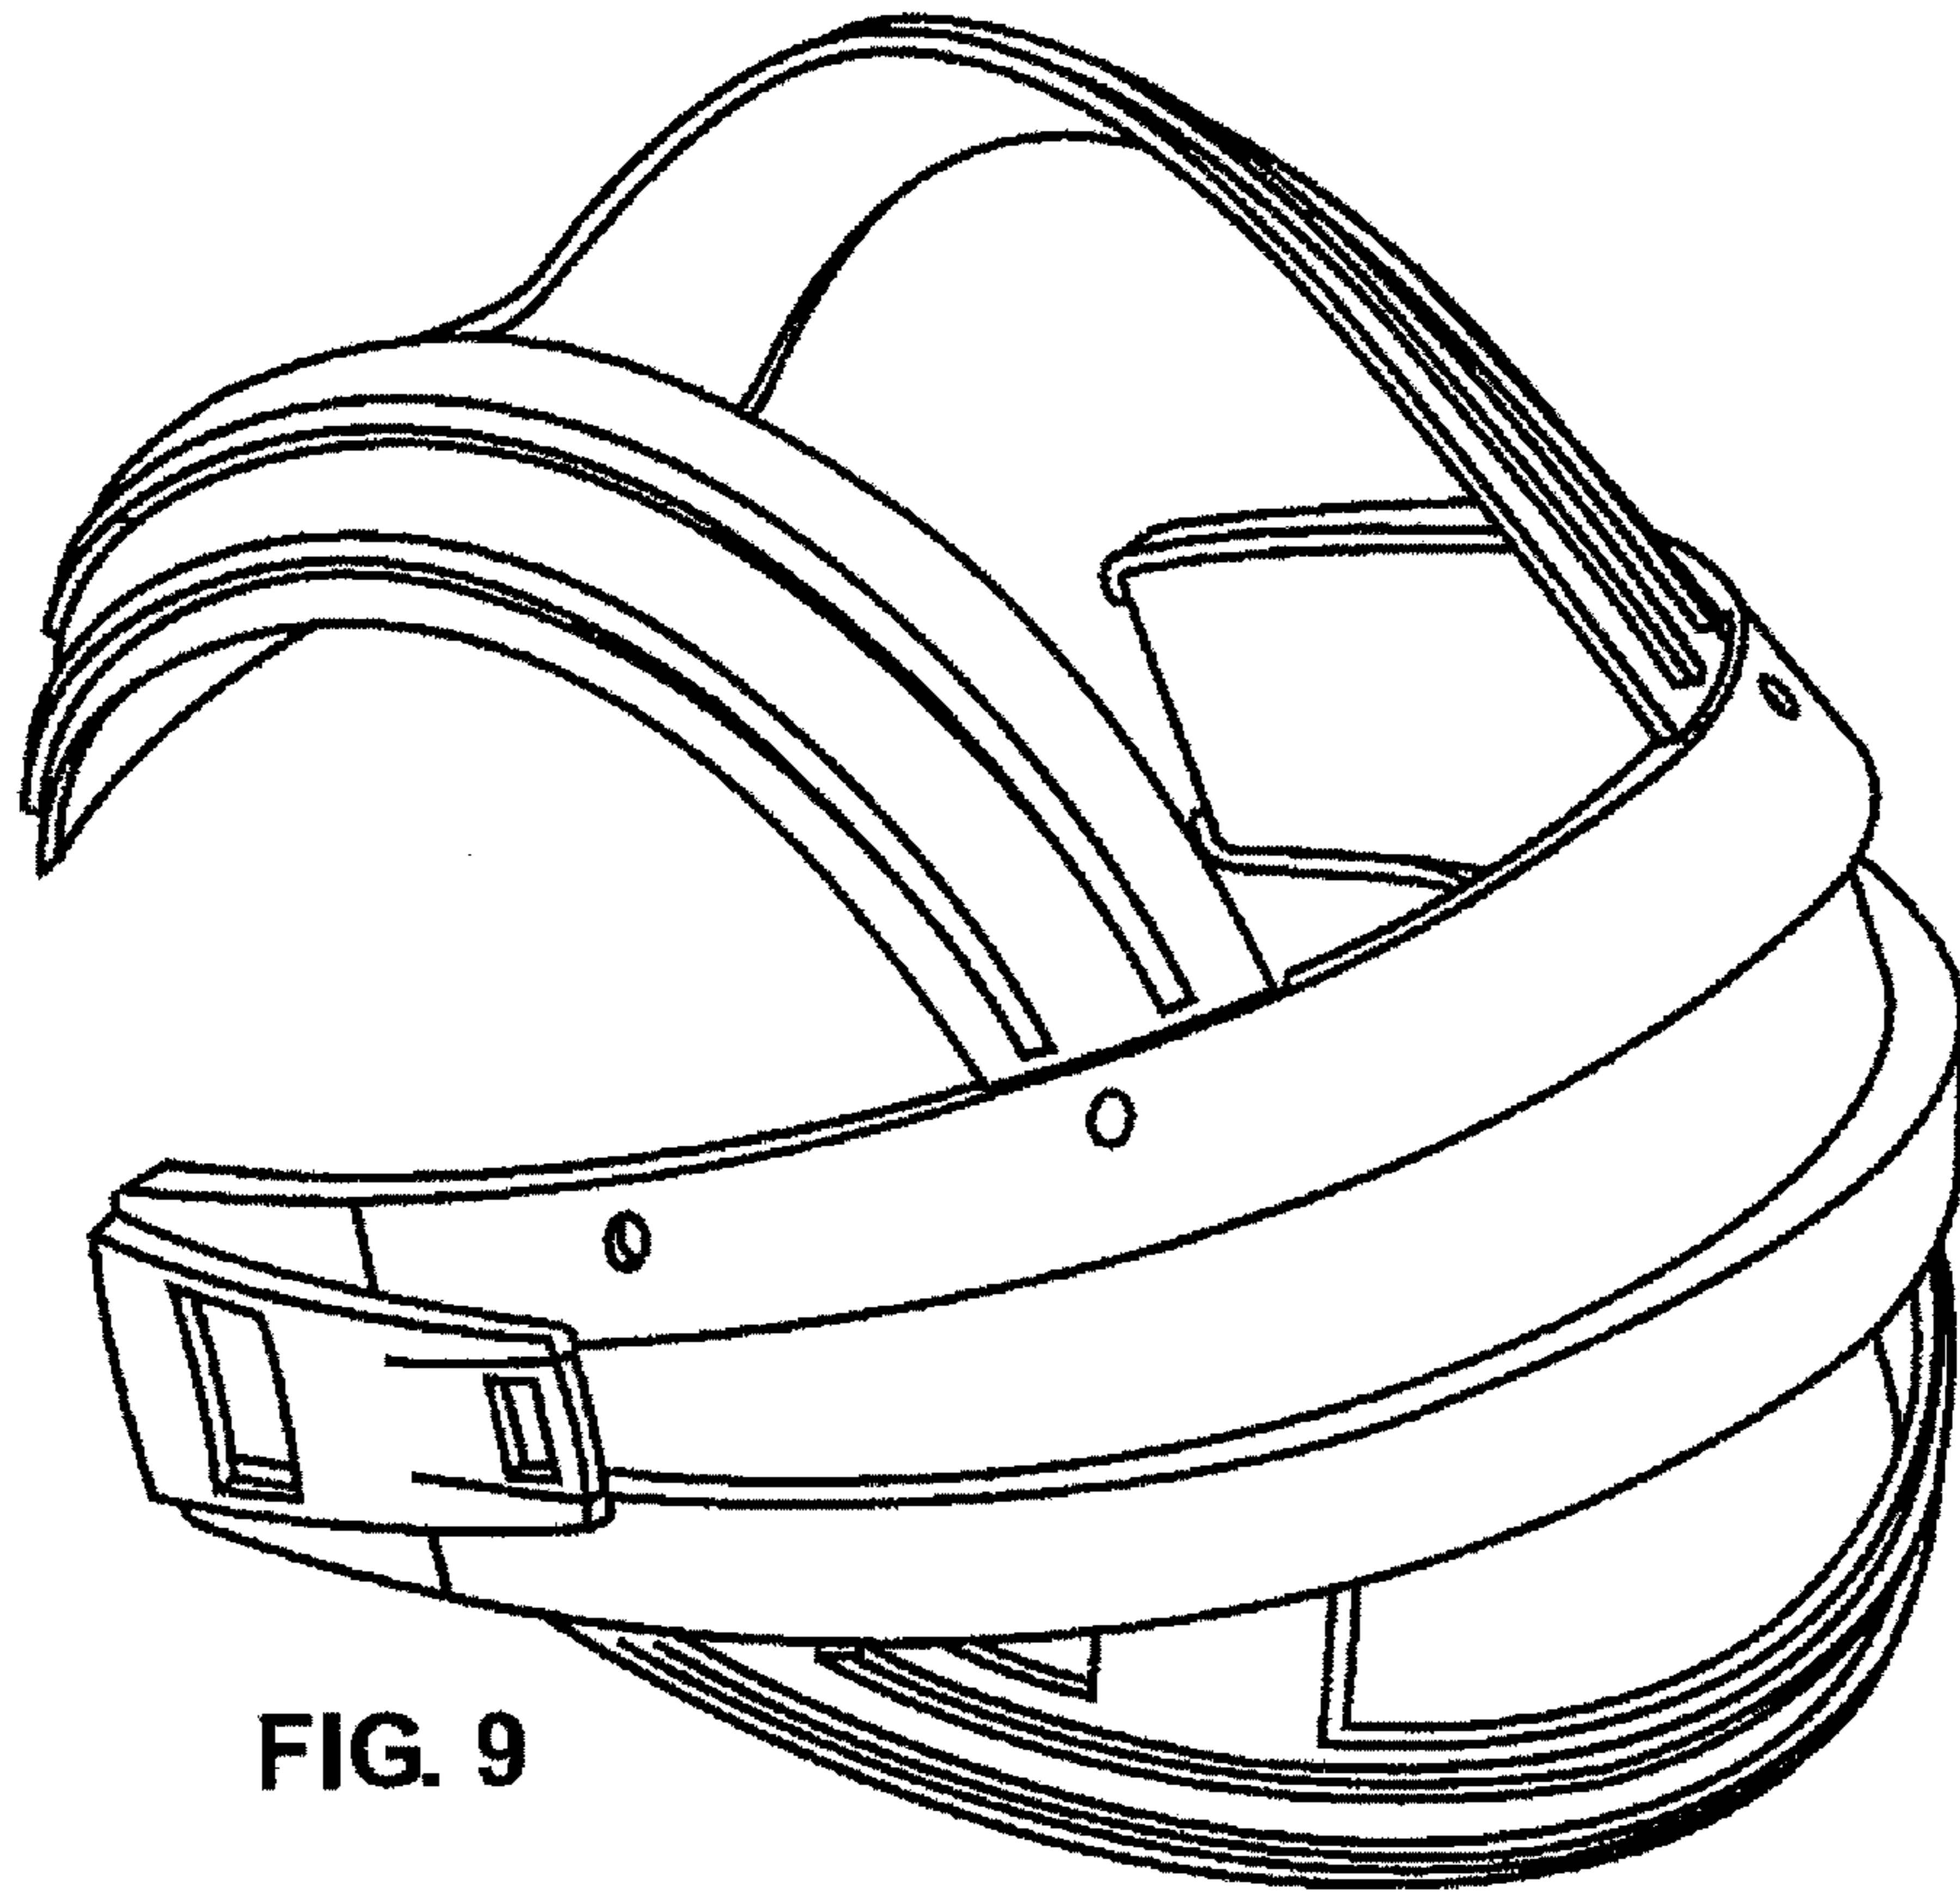


FIG. 9

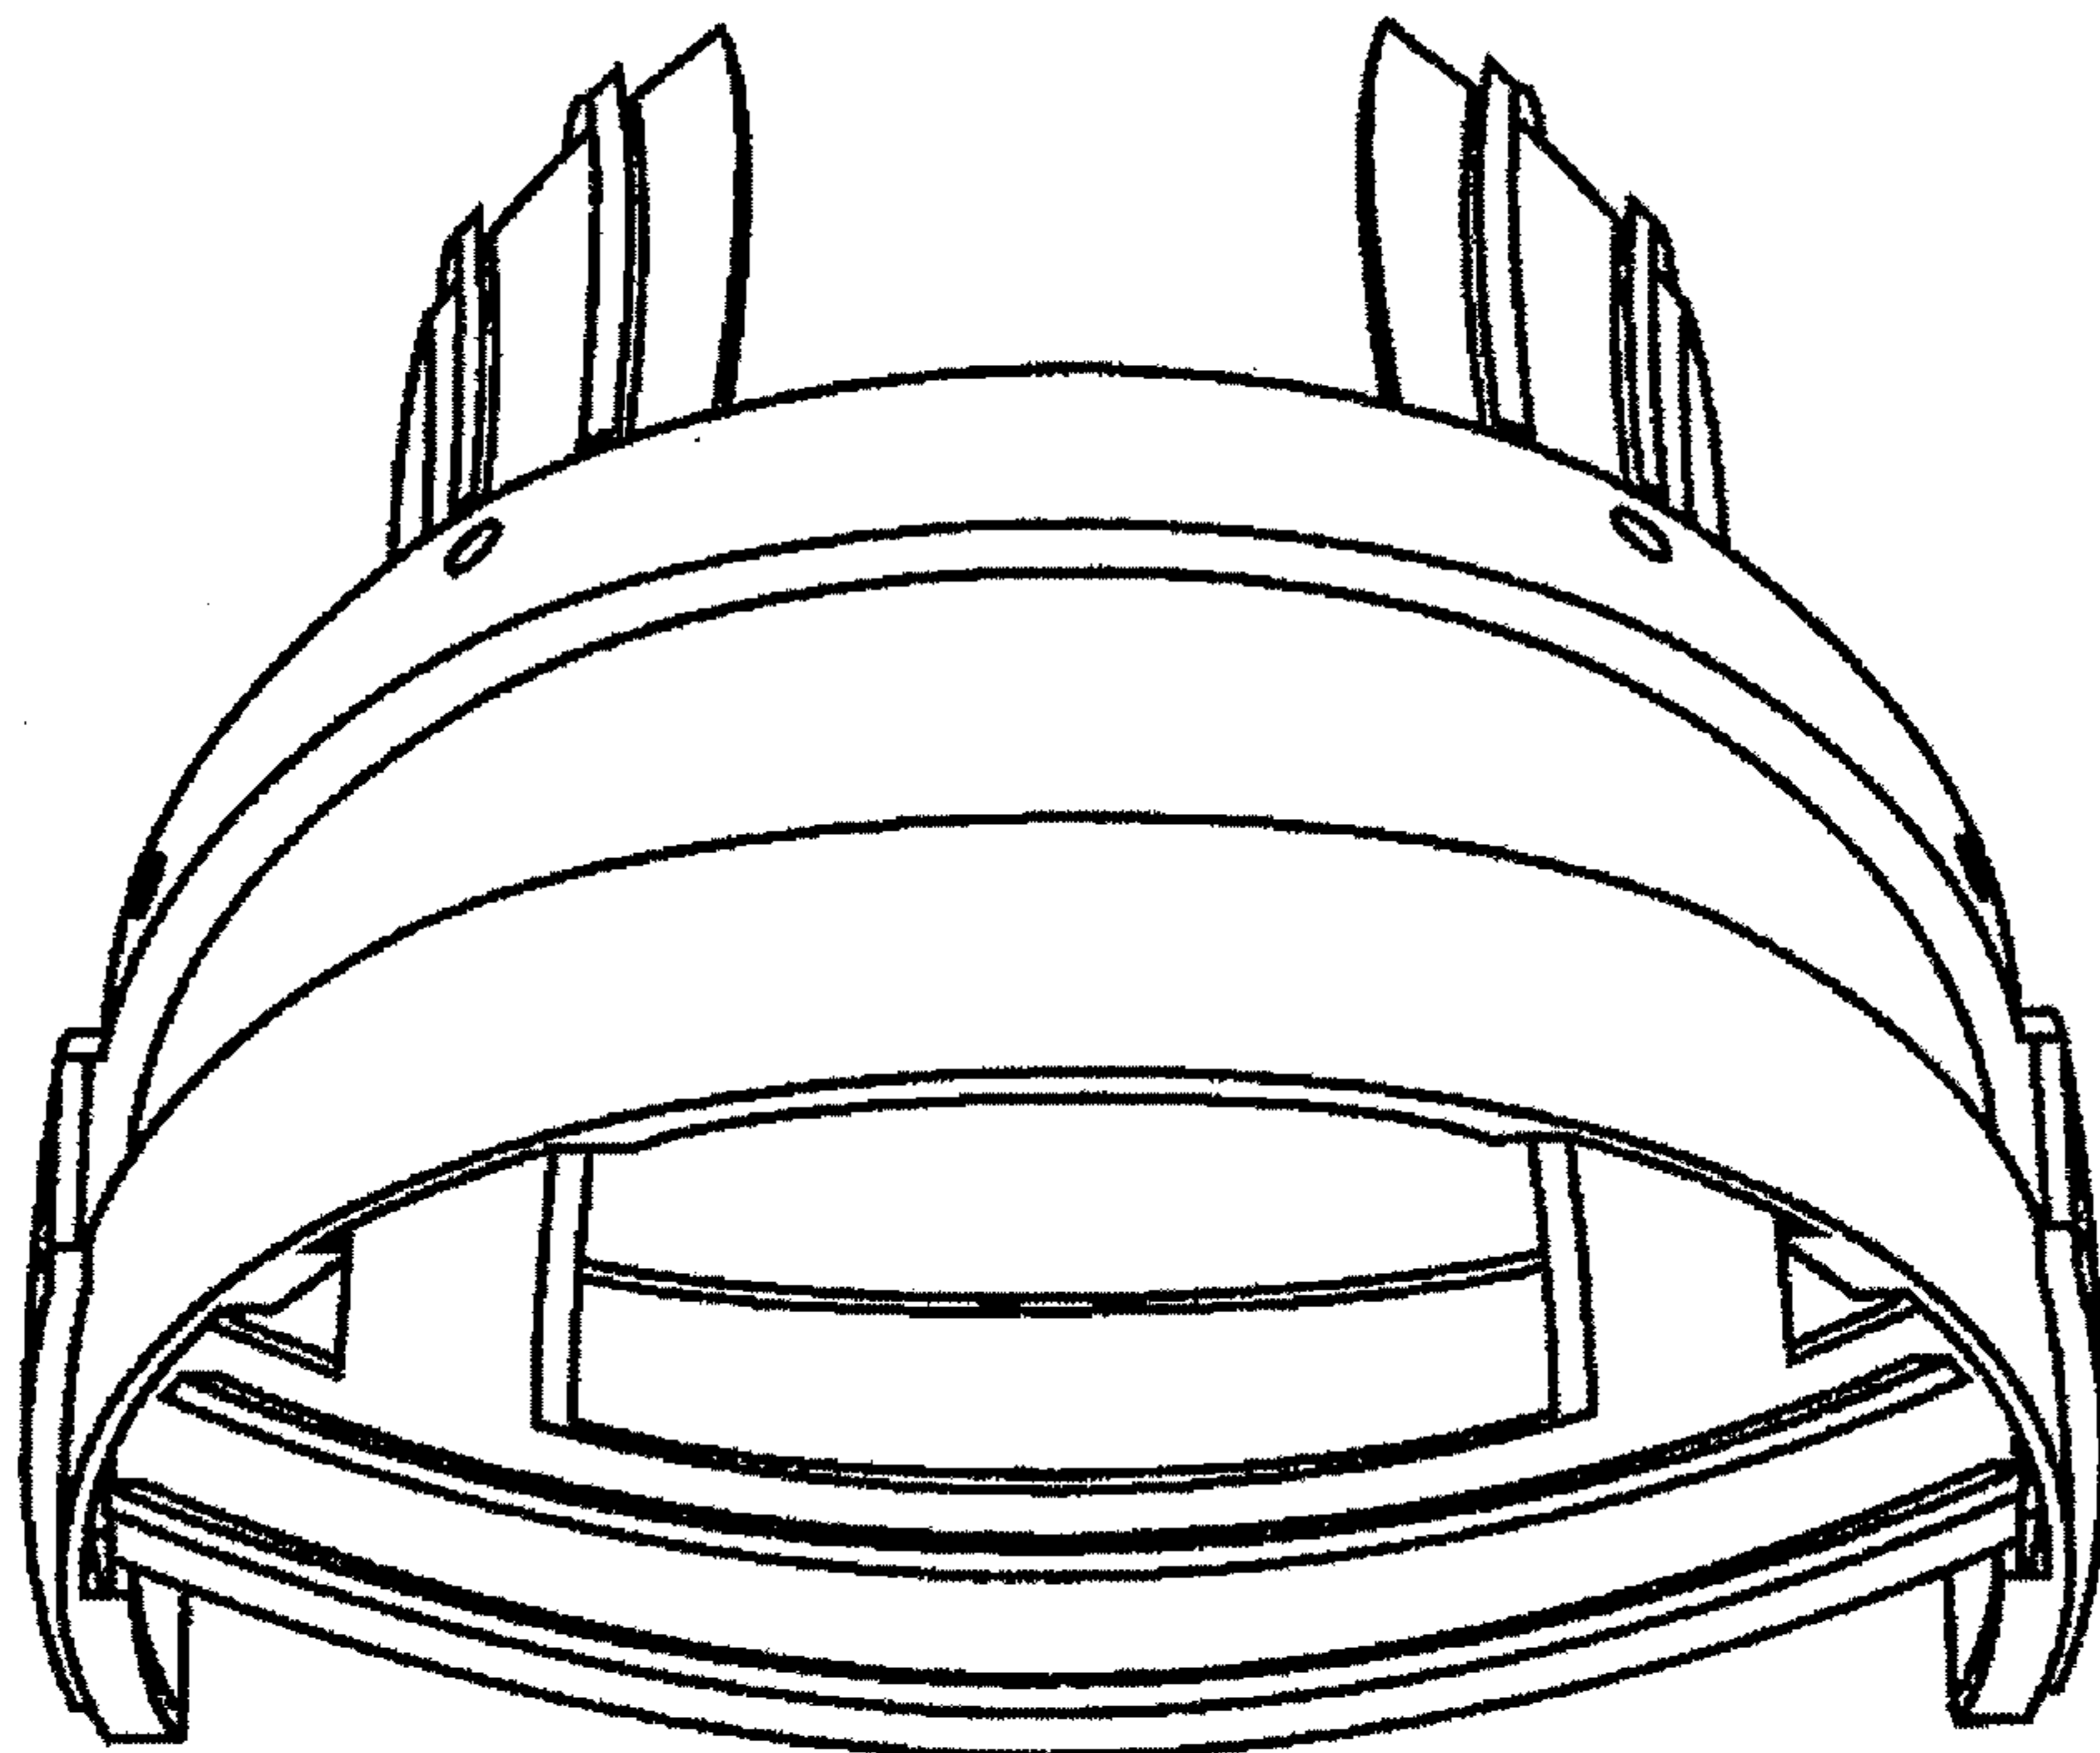


FIG. 10

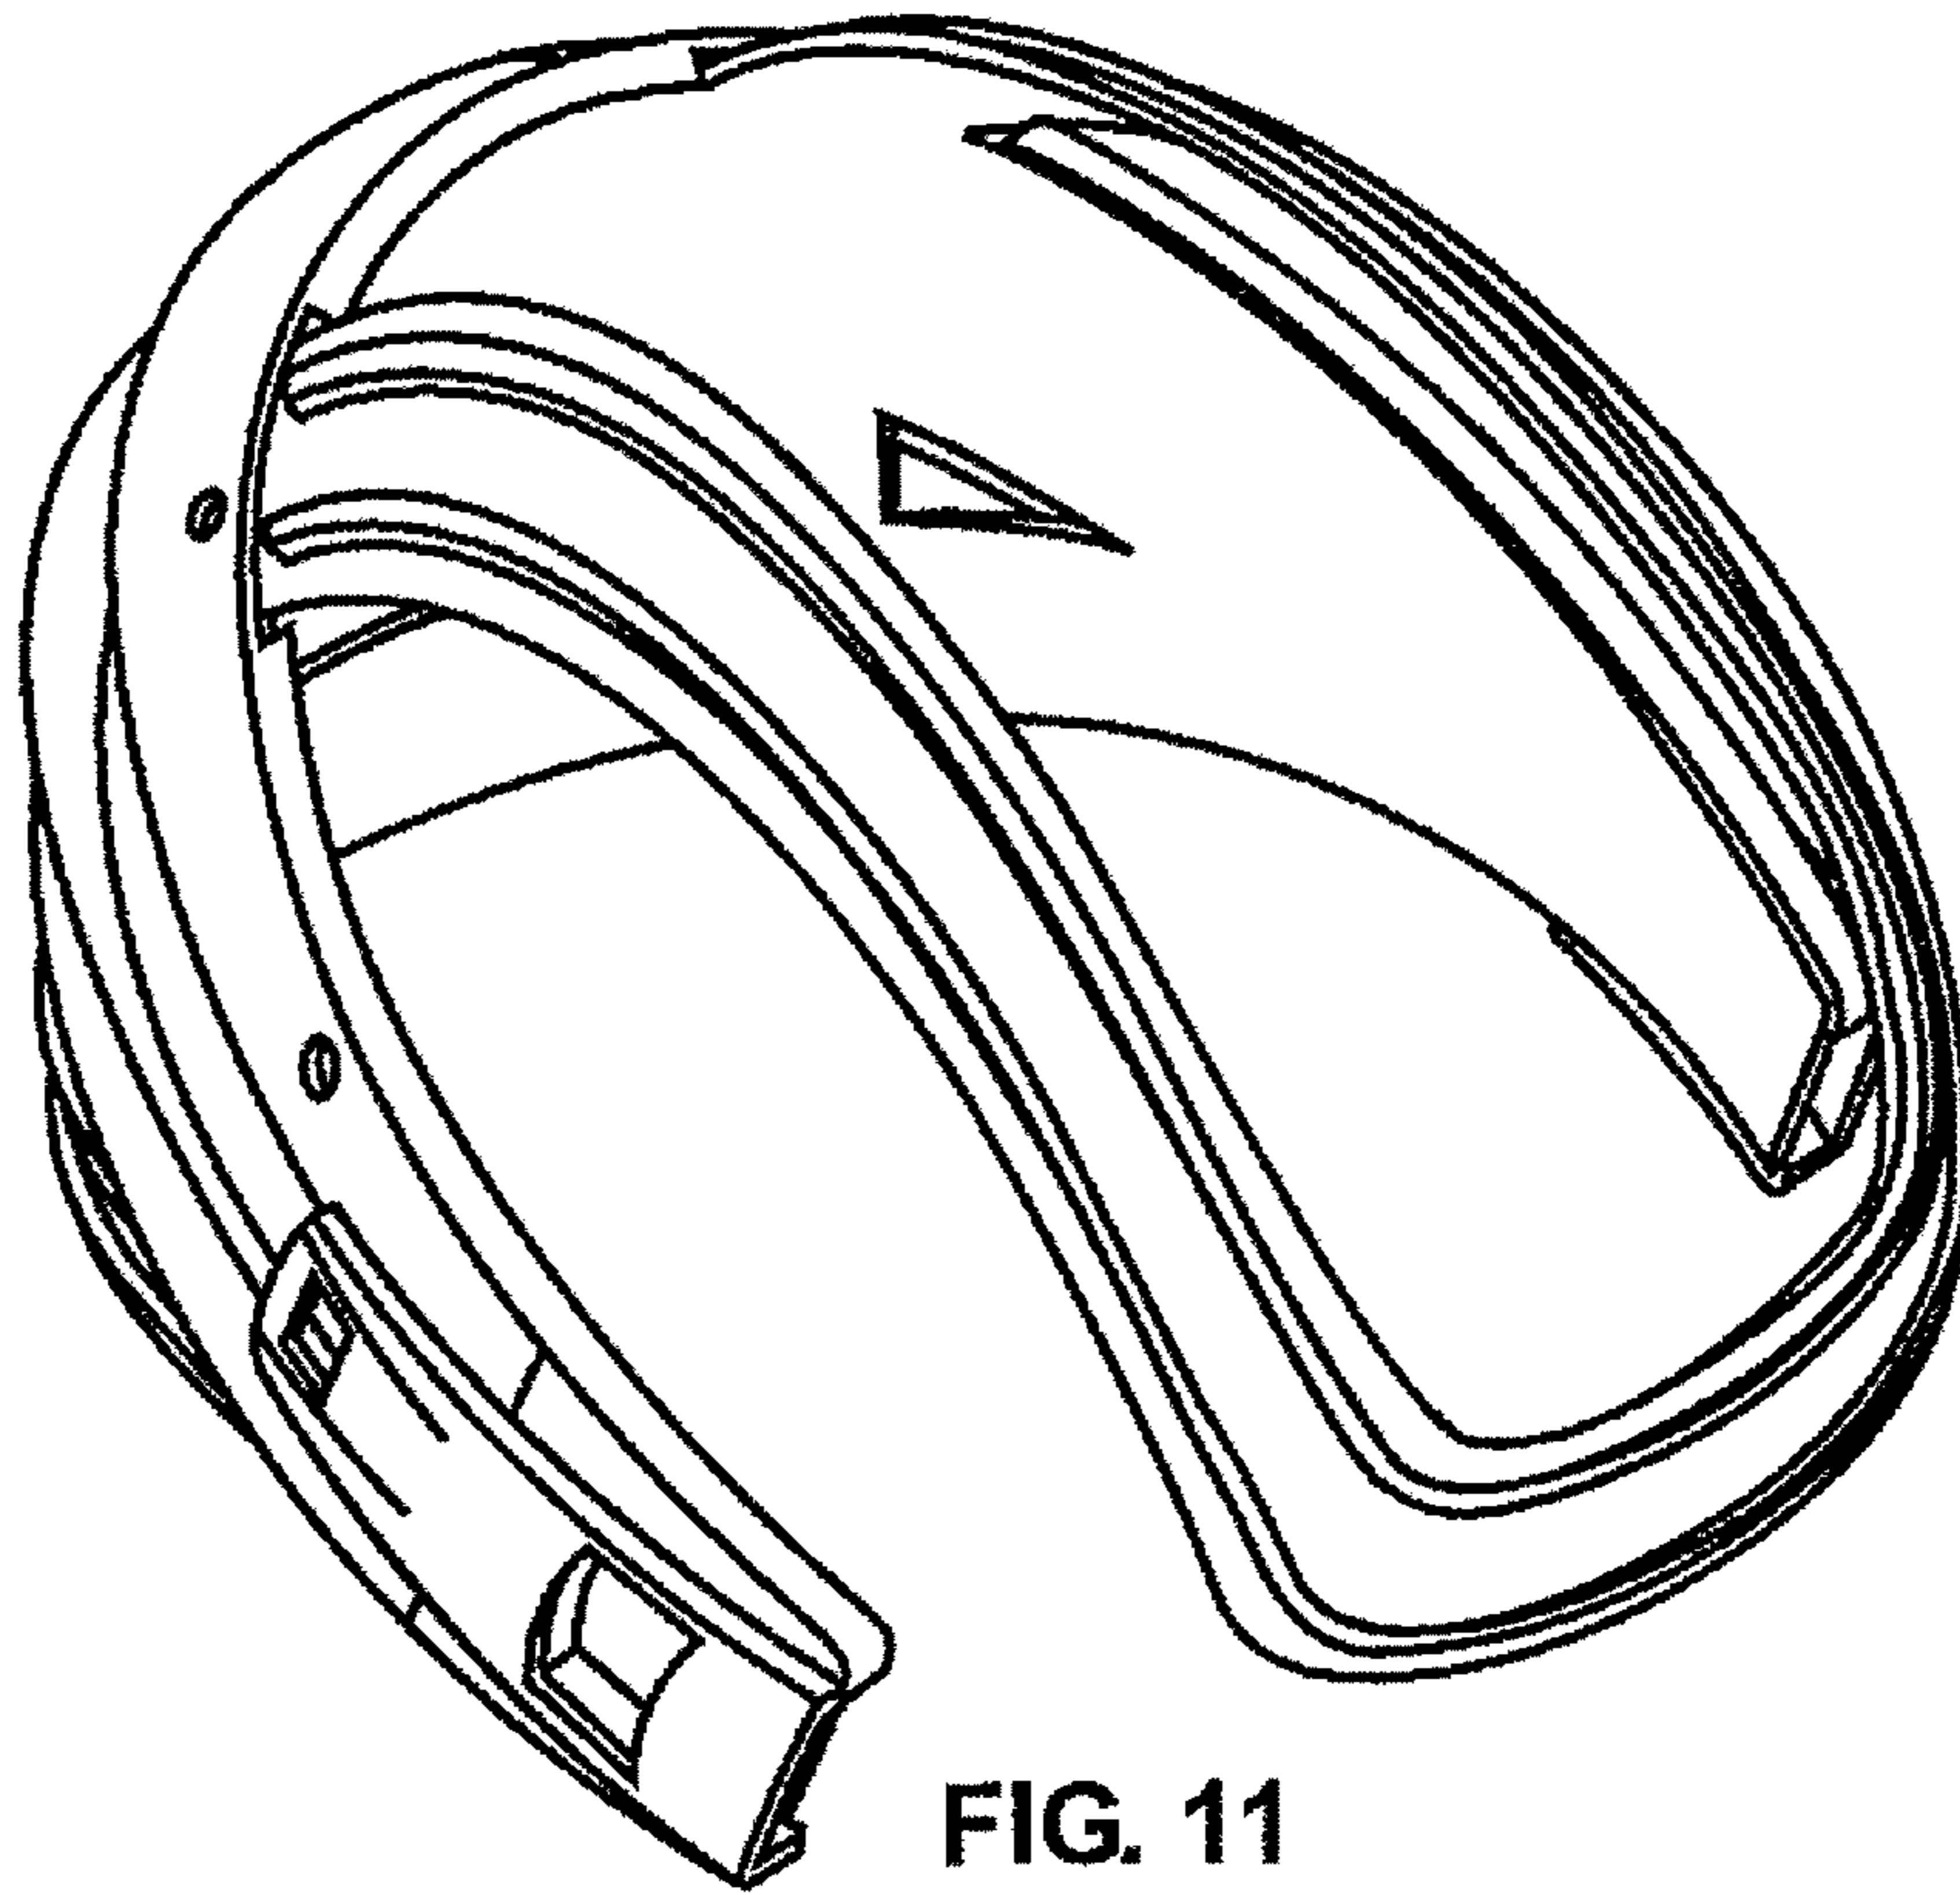


FIG. 11

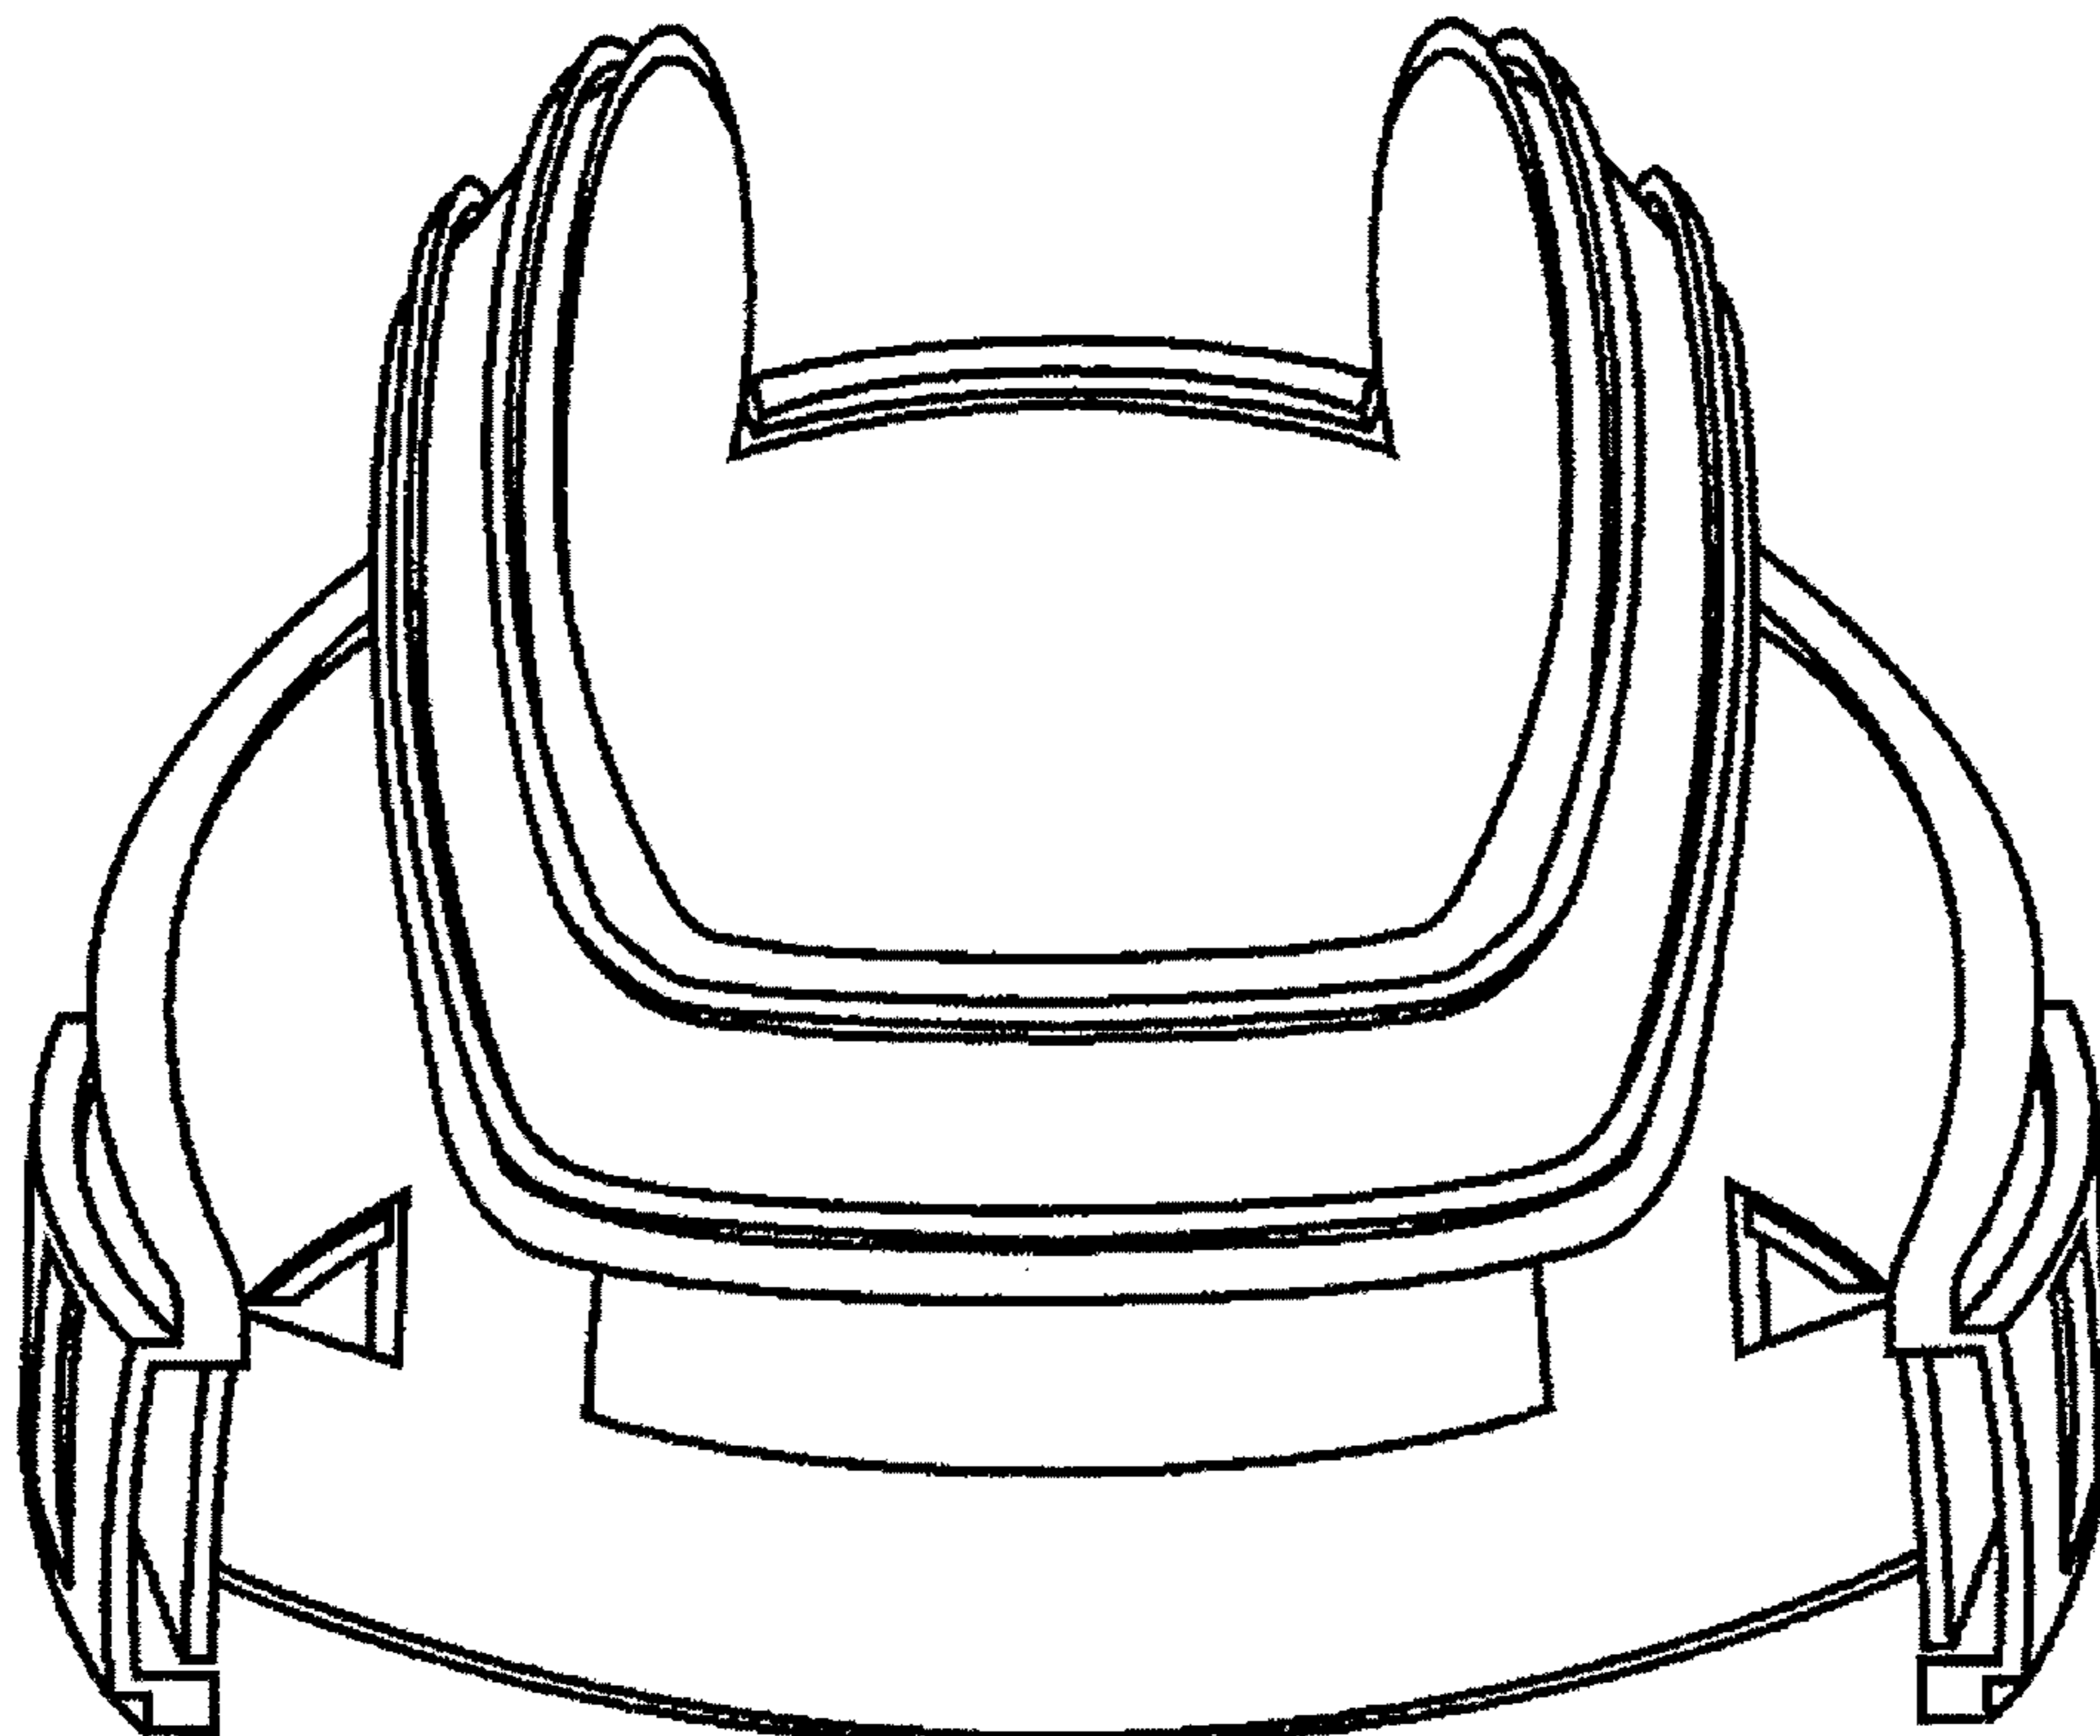


FIG. 12

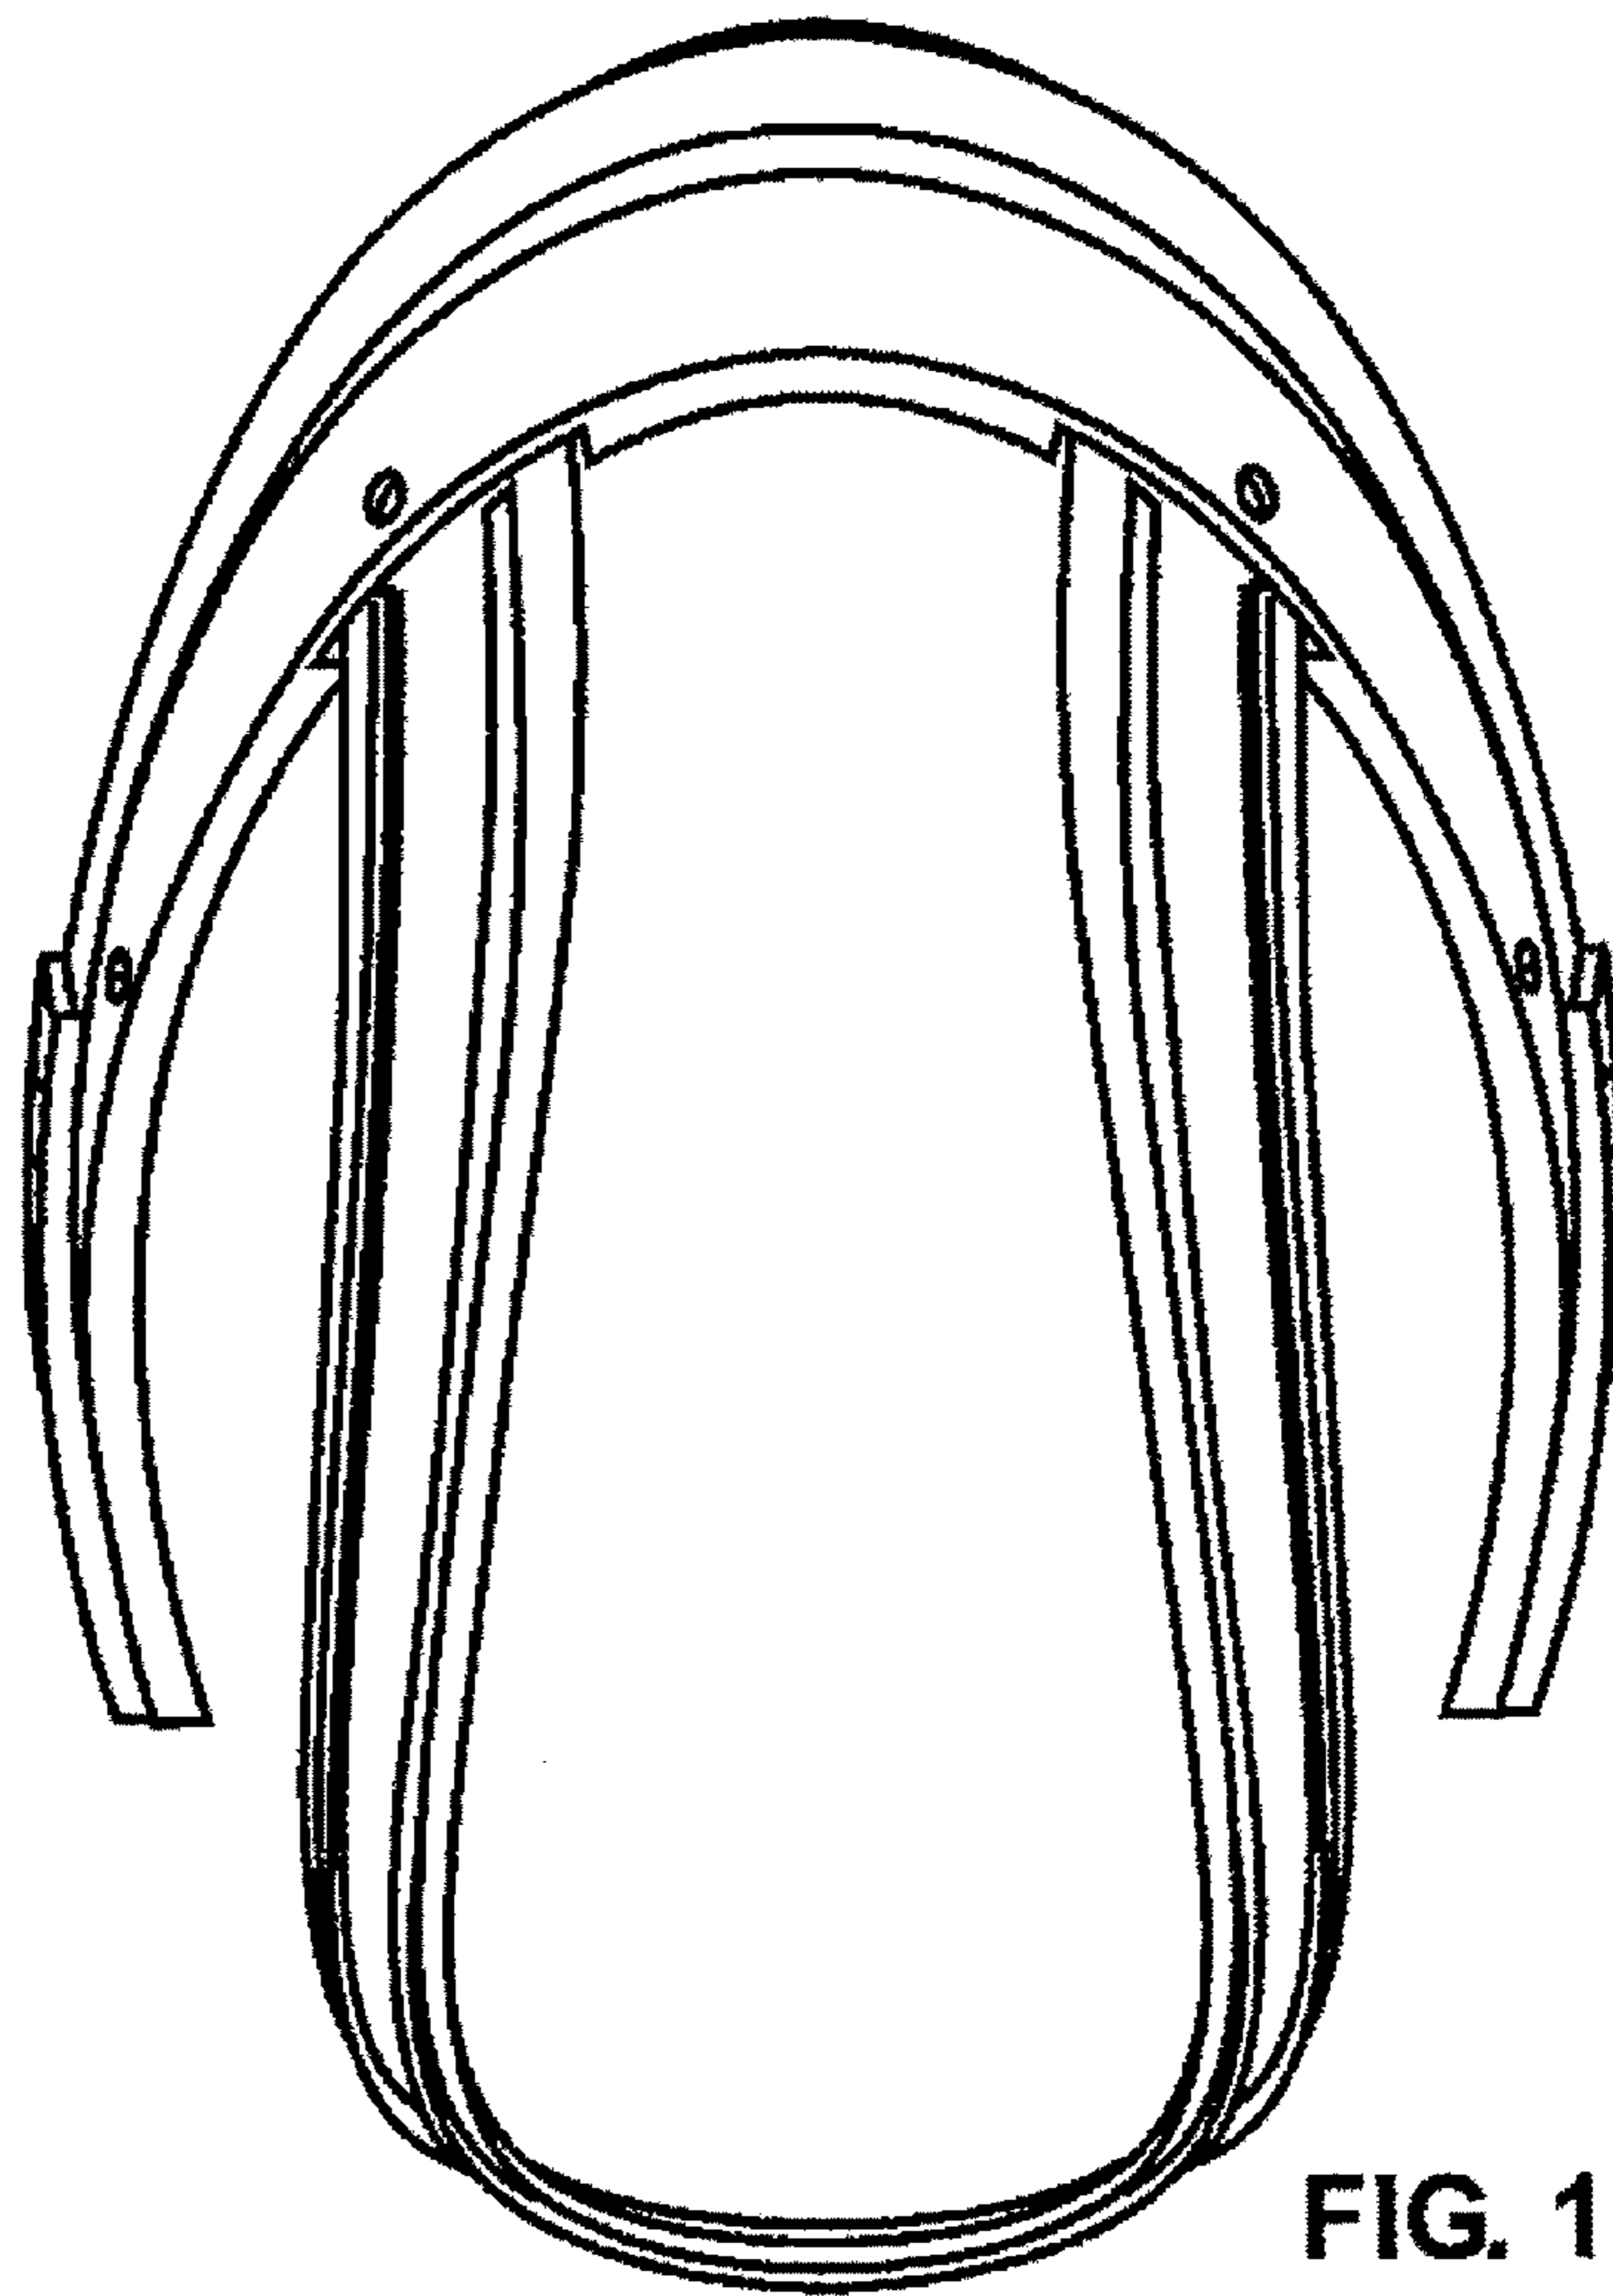


FIG. 13

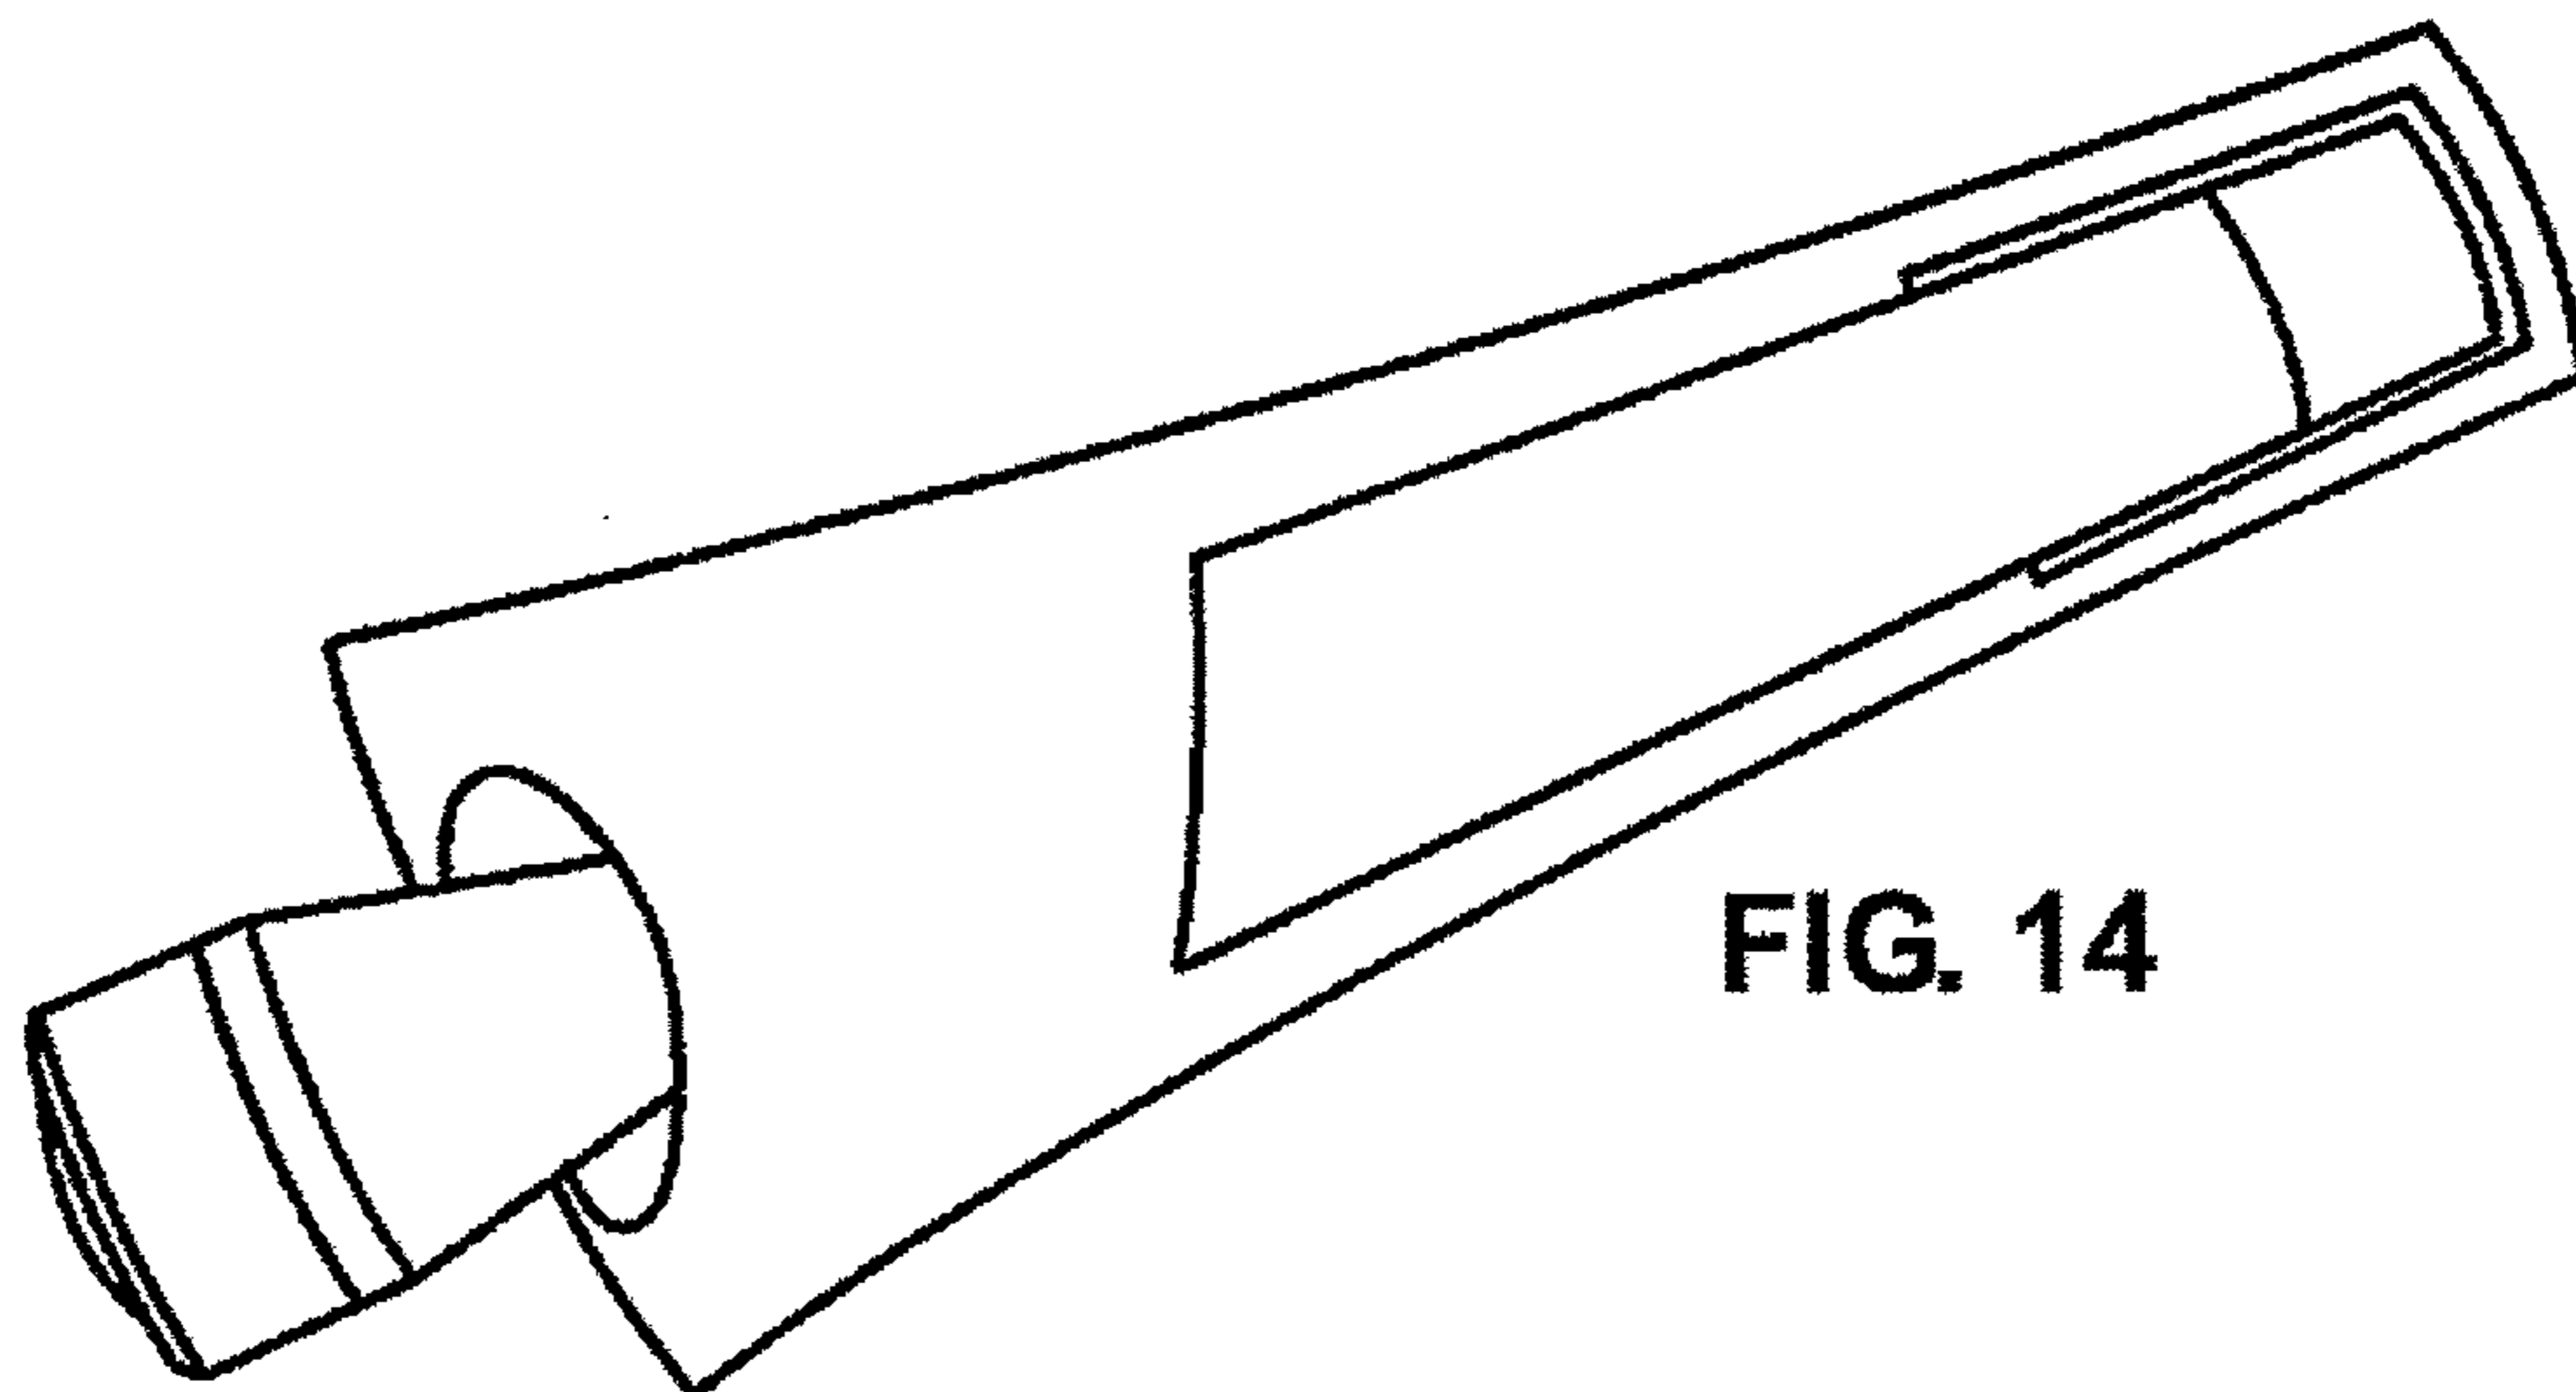


FIG. 14

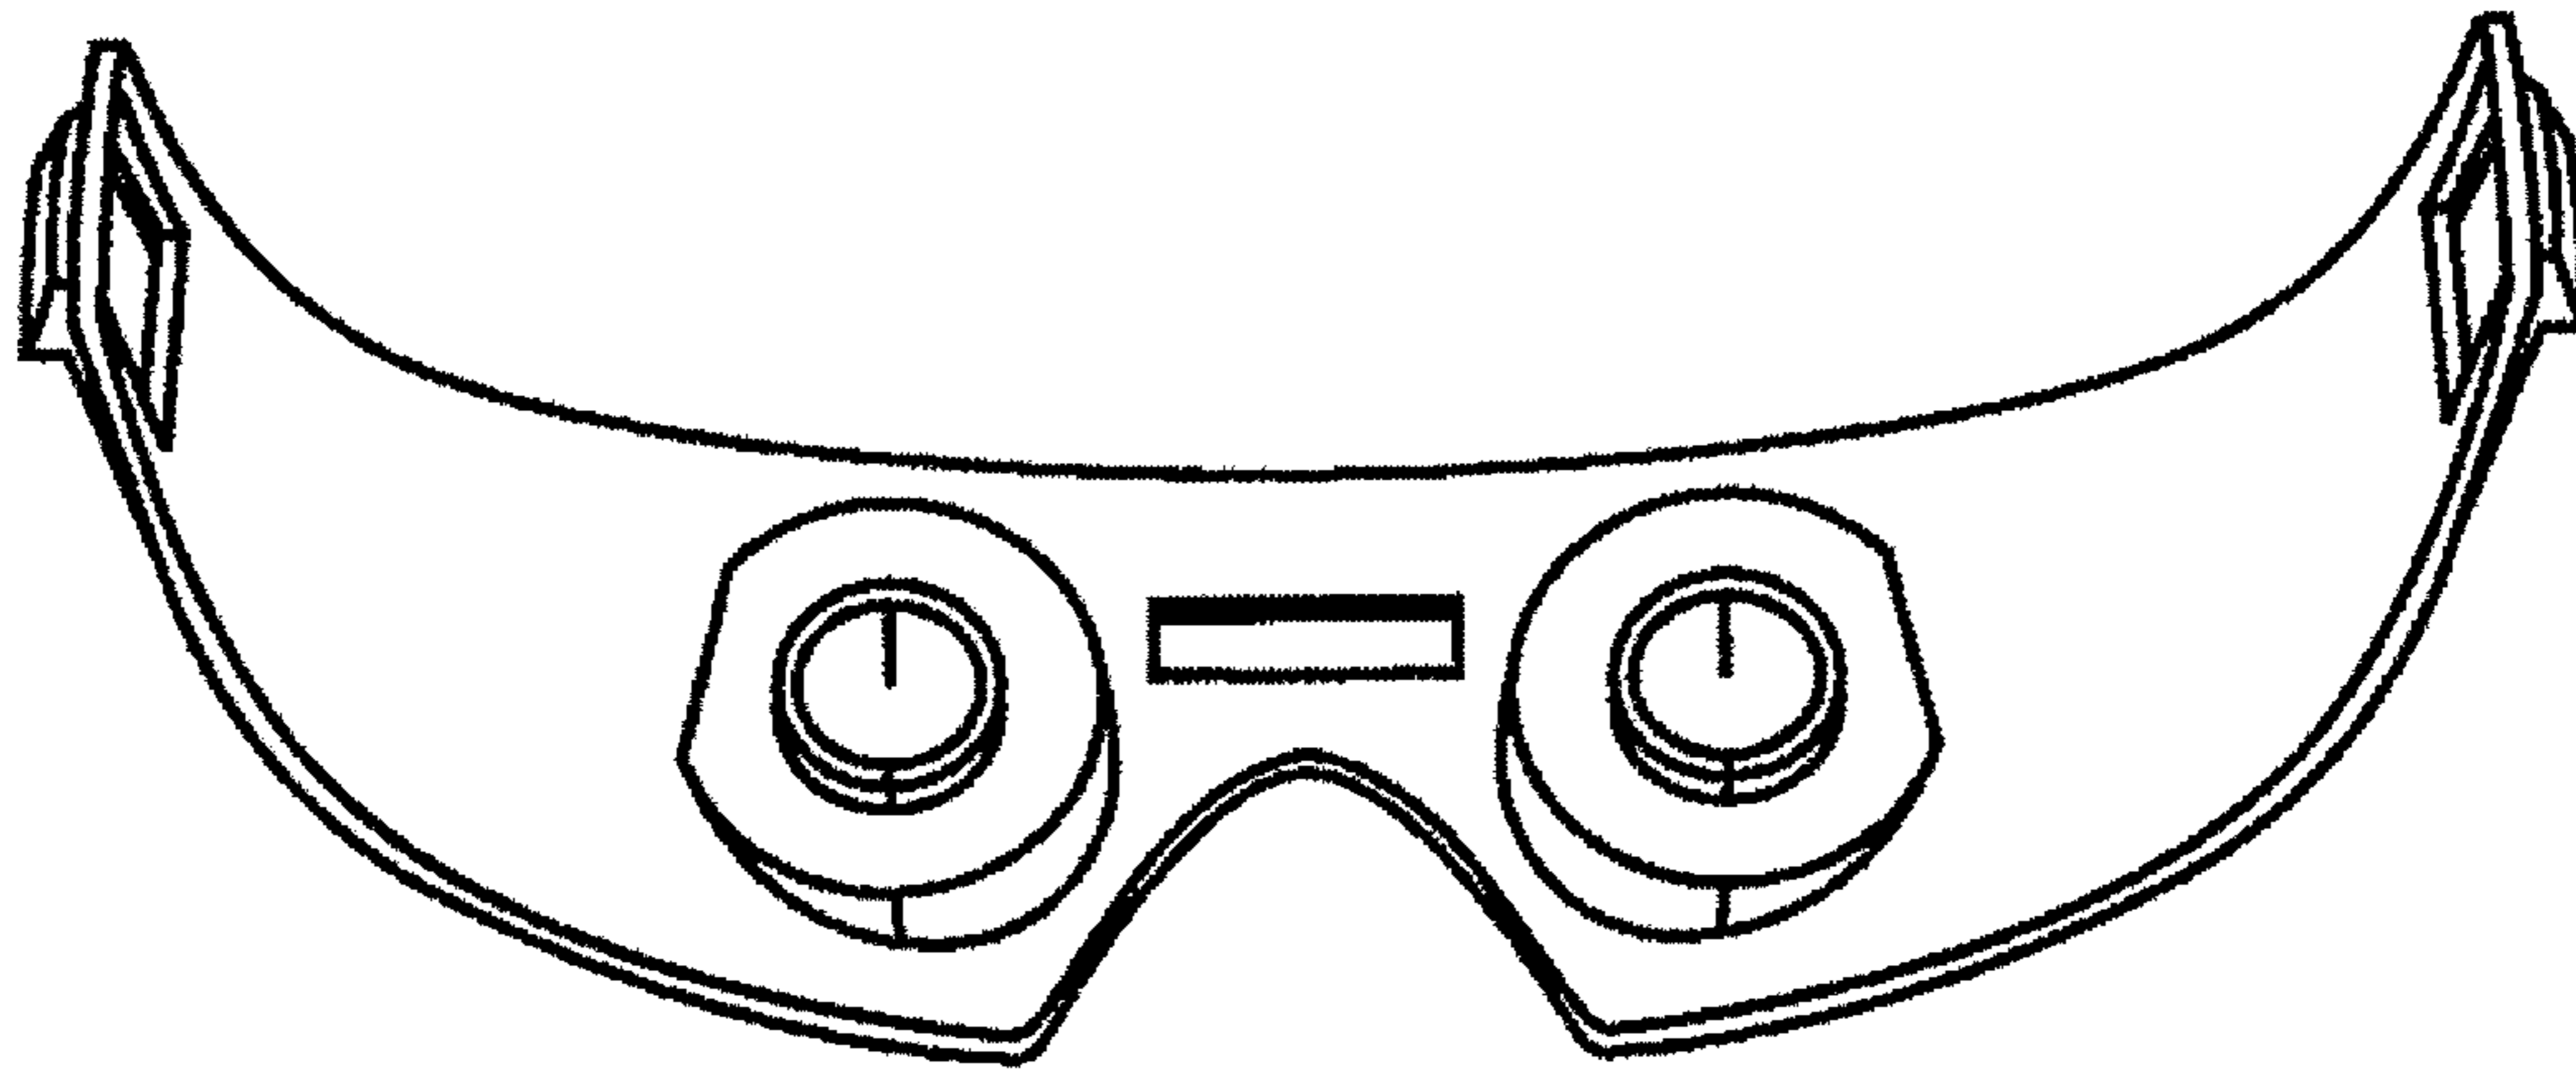


FIG. 15

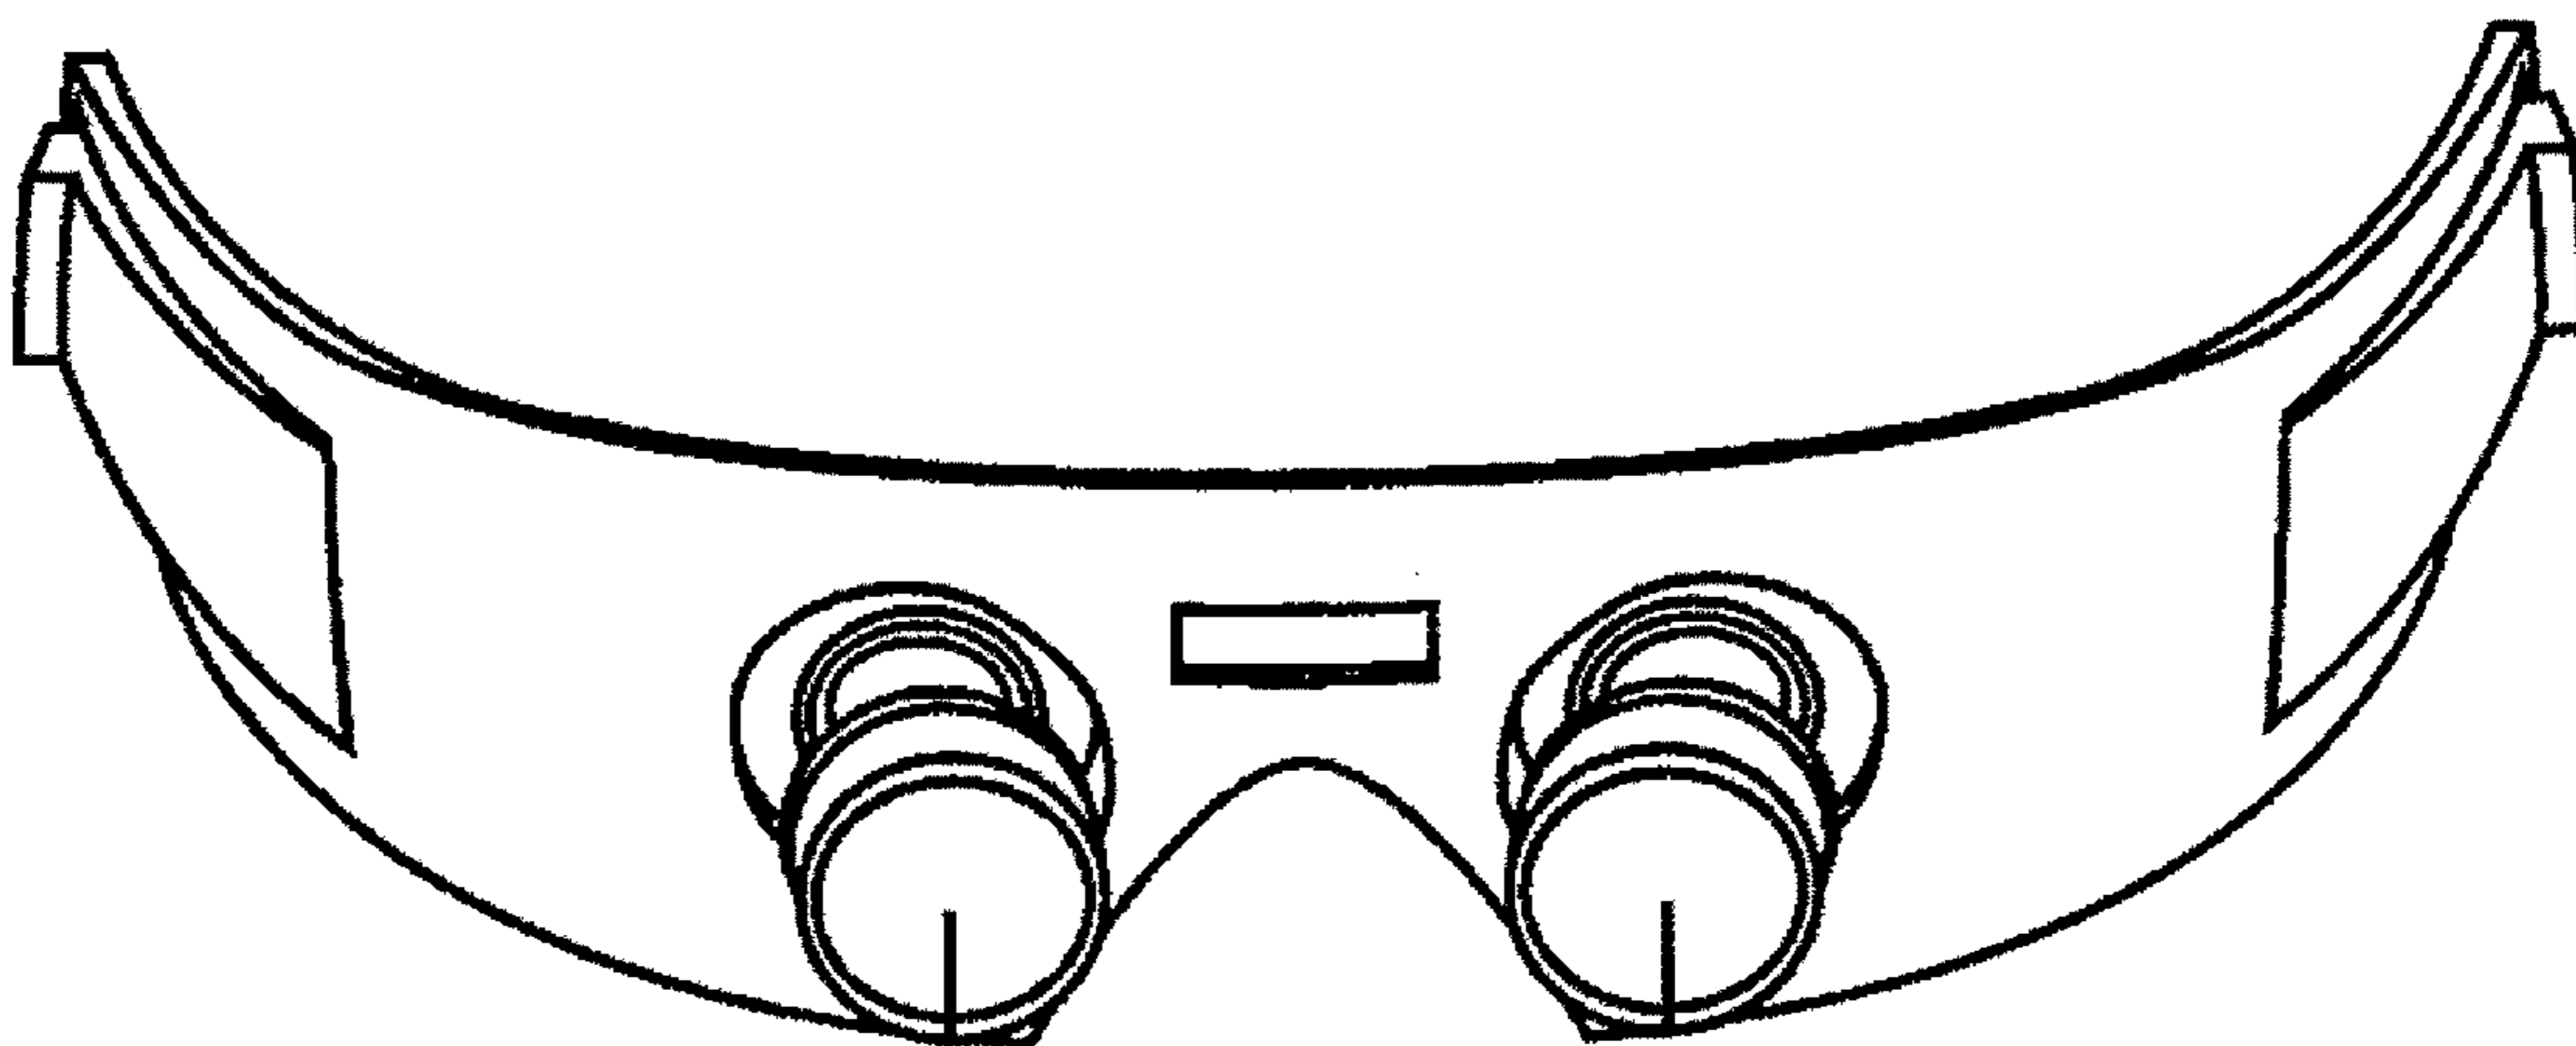


FIG. 16

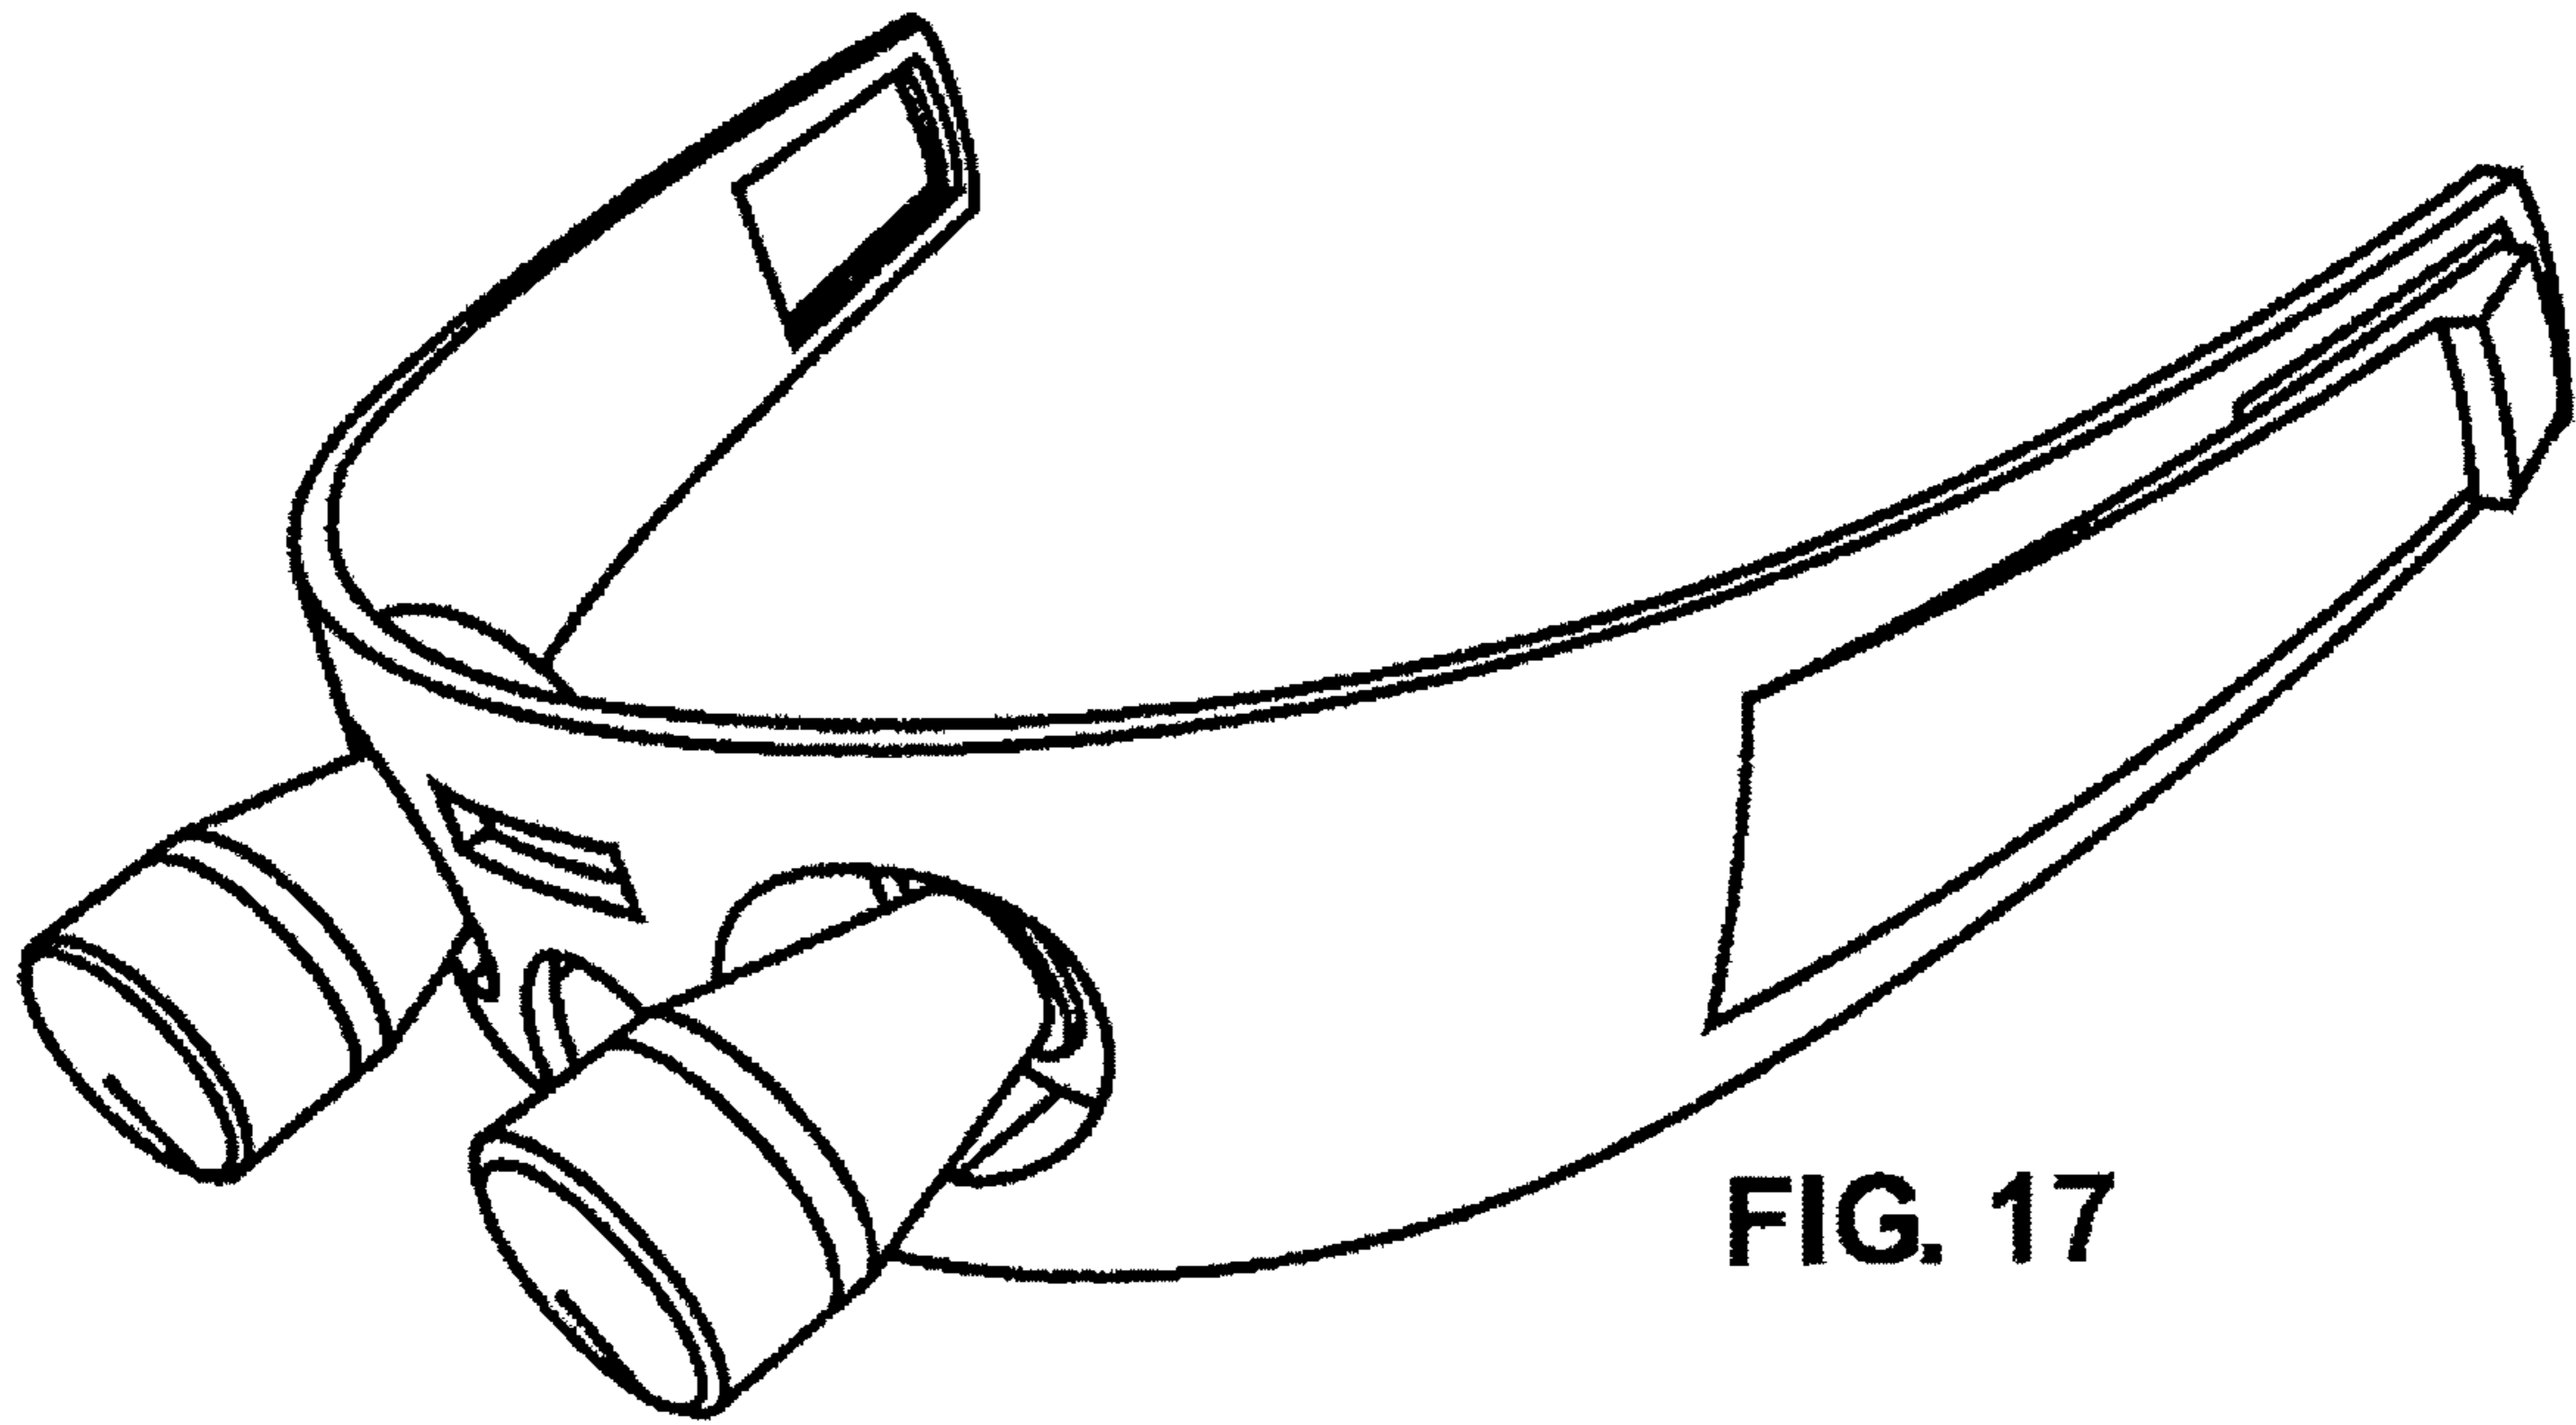


FIG. 17

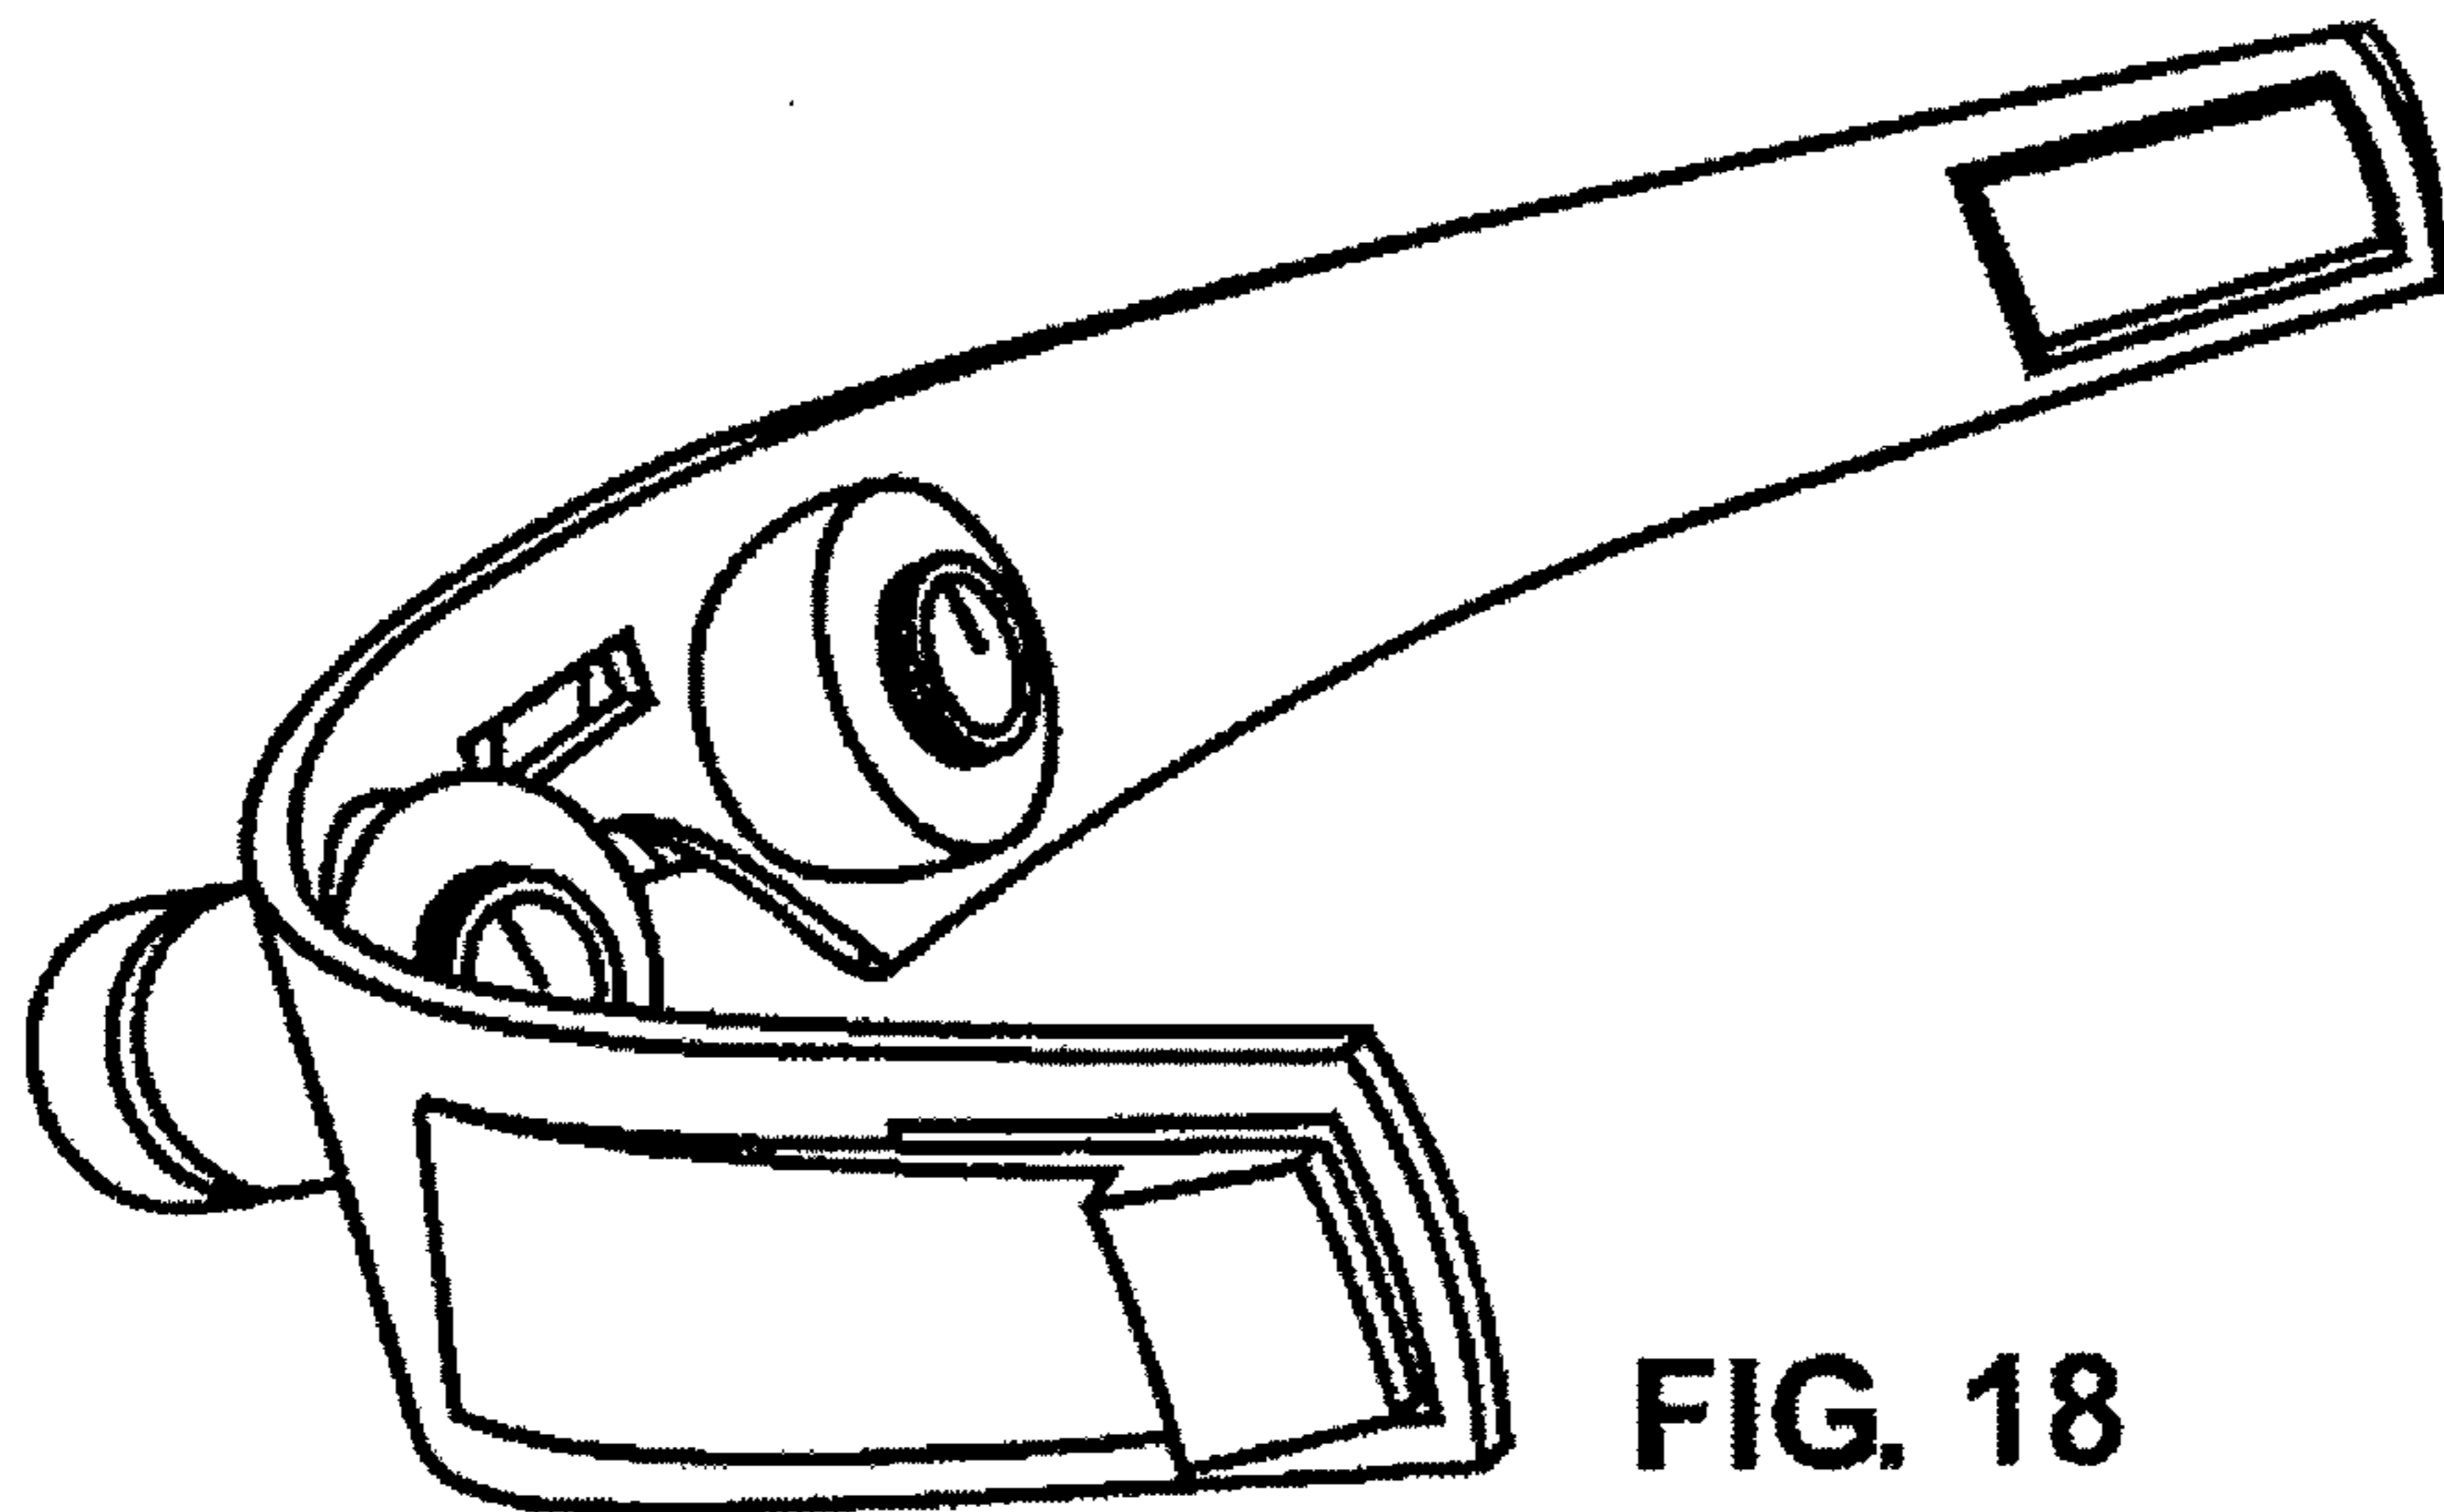


FIG. 18

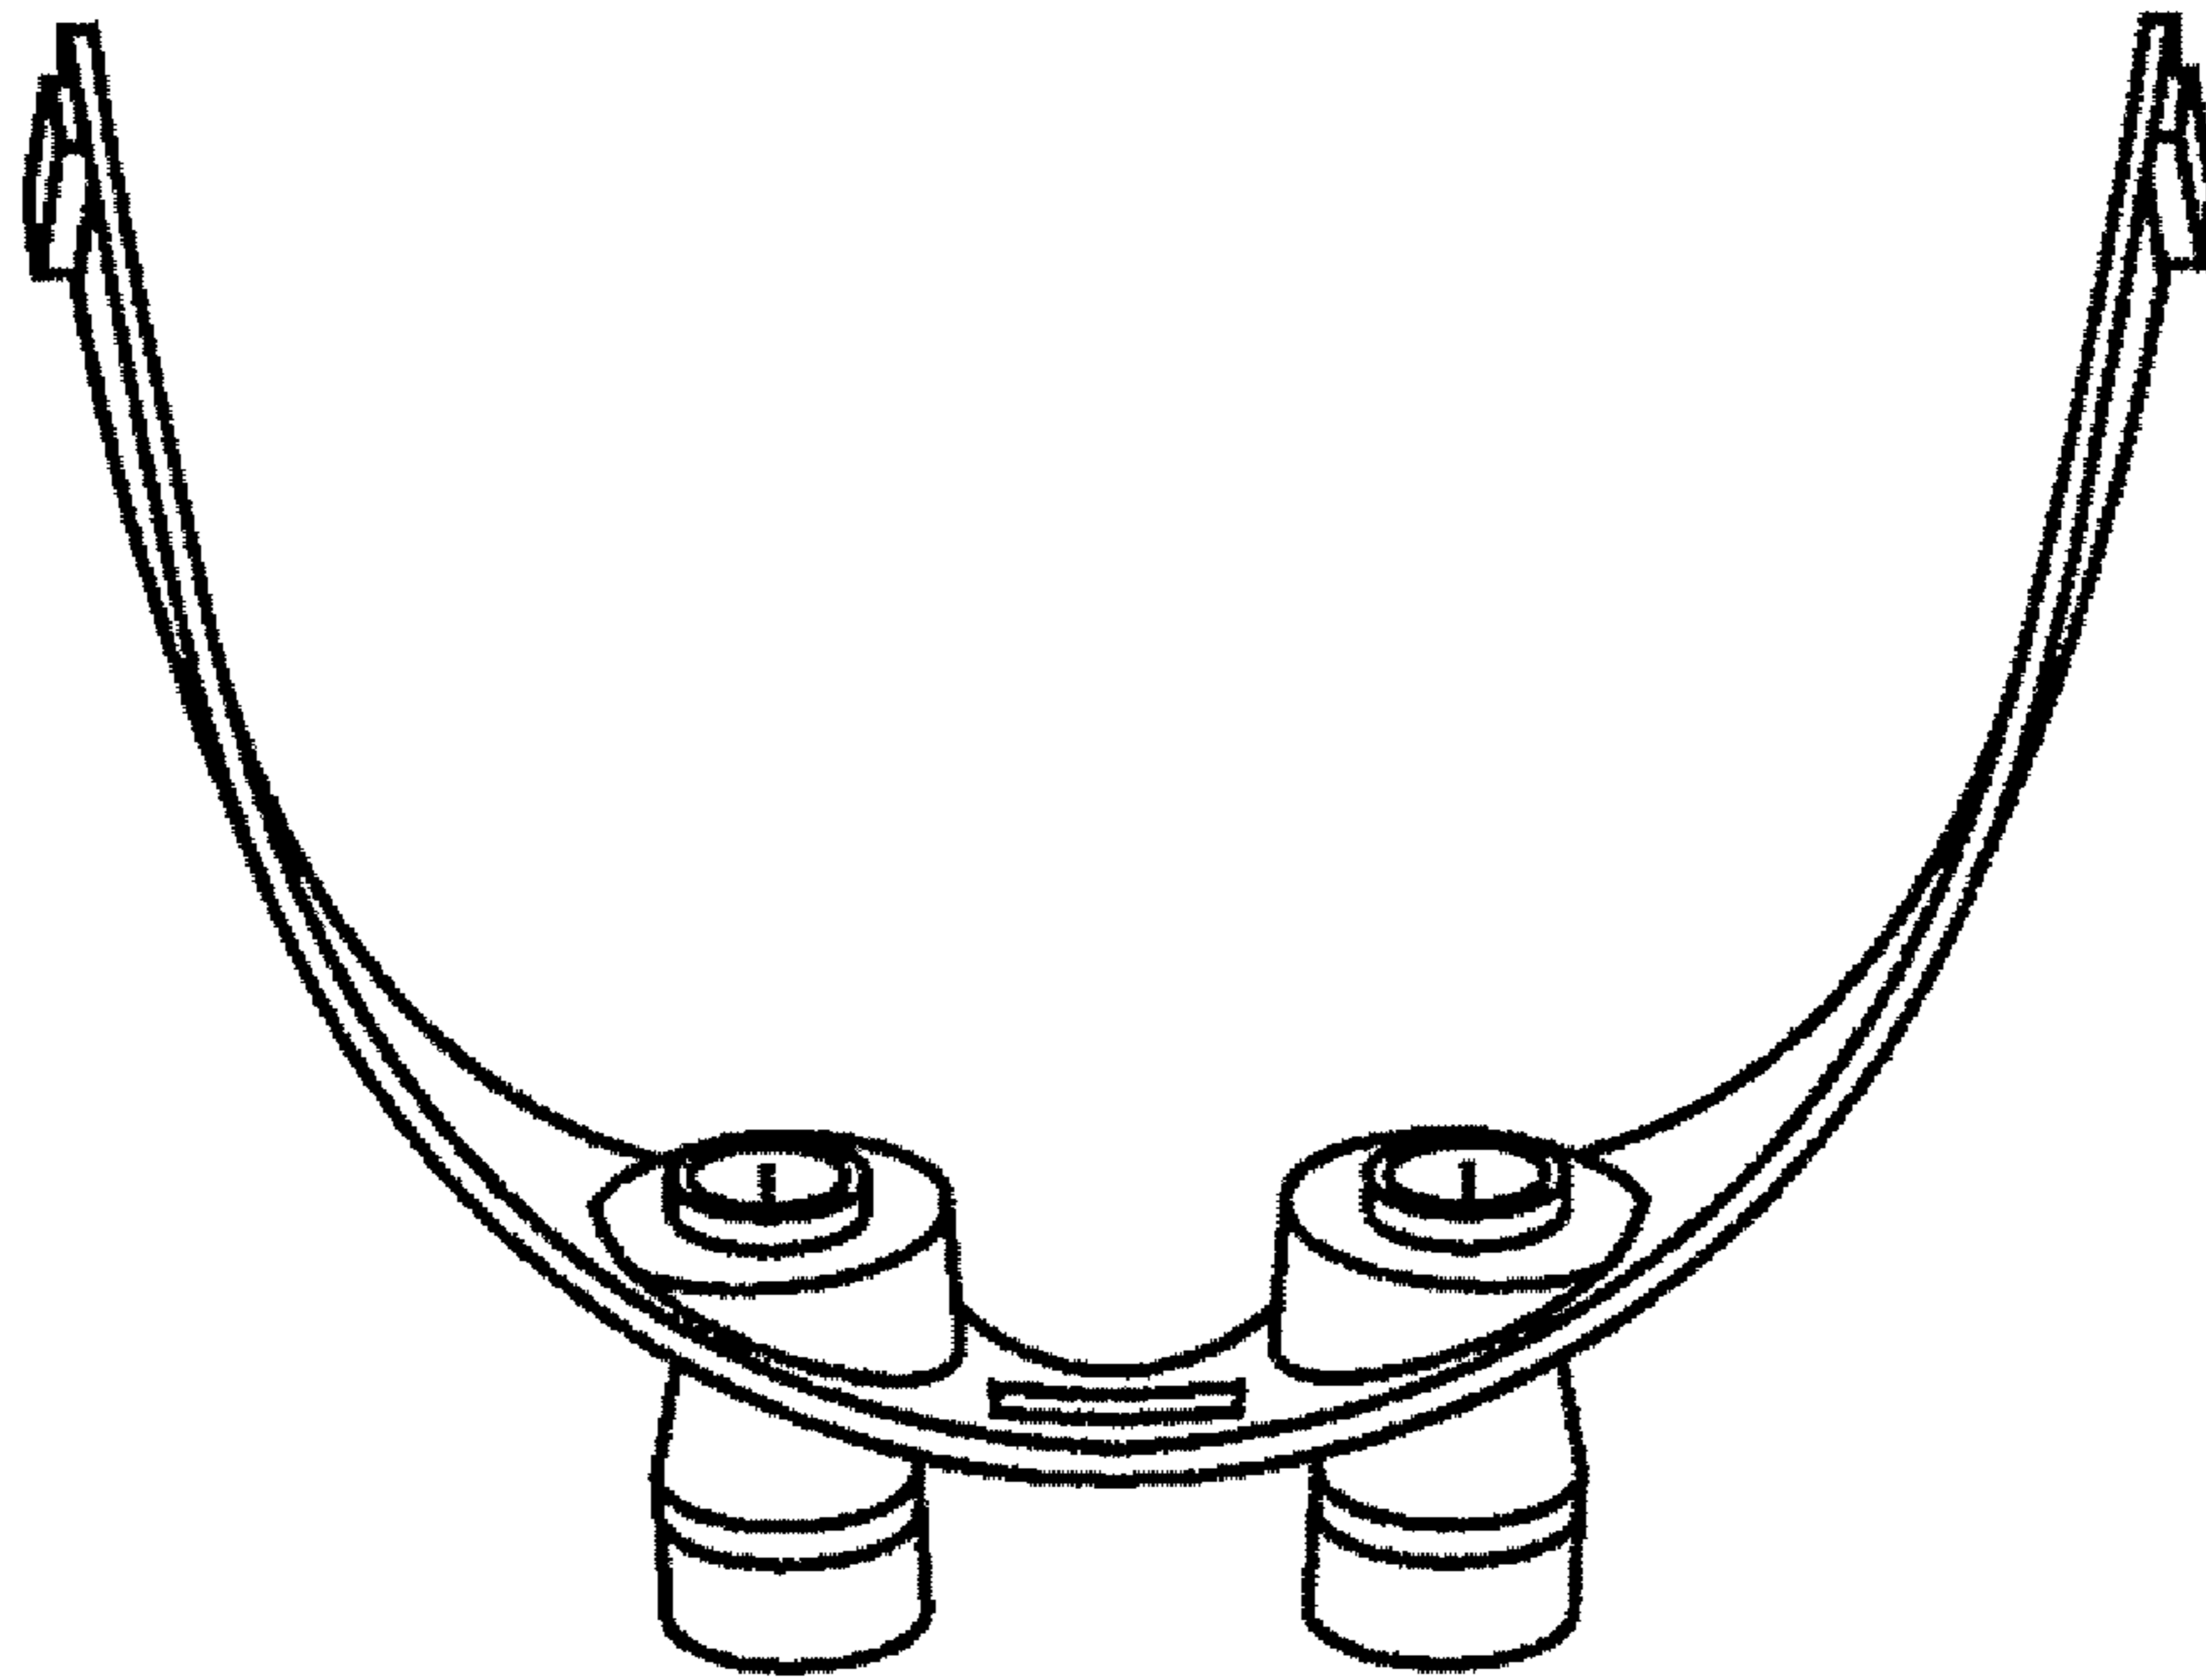


FIG. 19

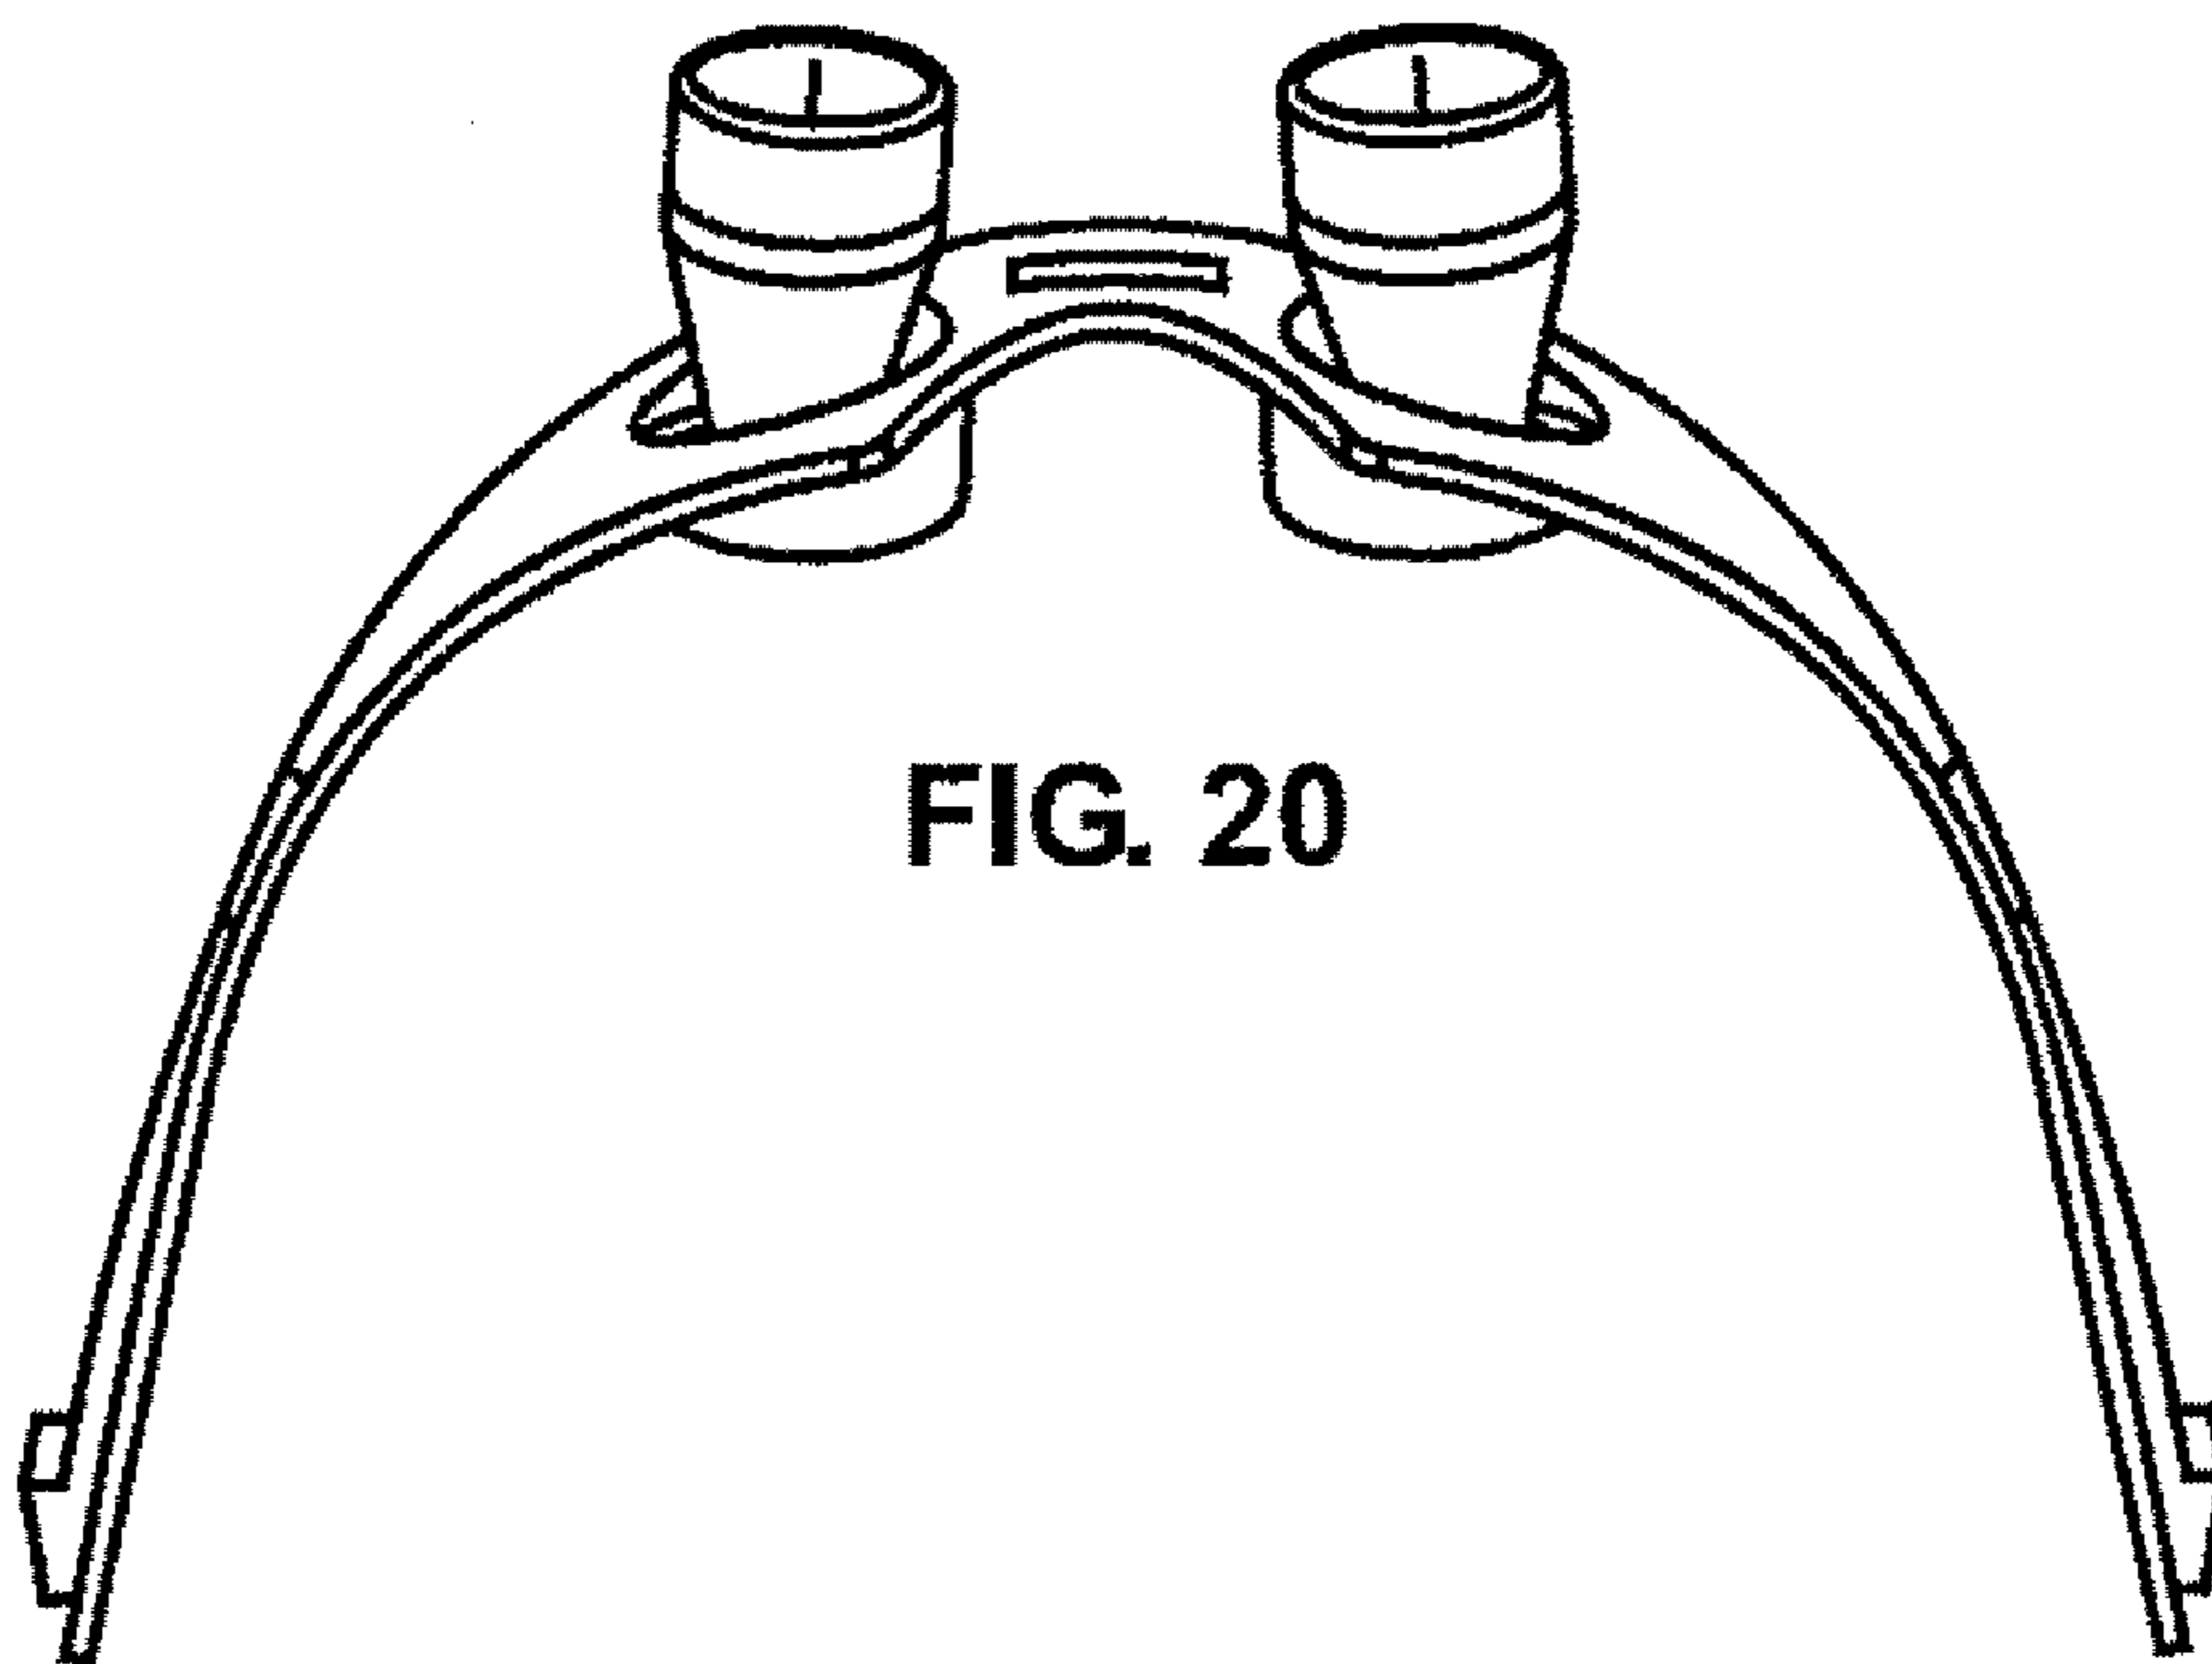


FIG. 20

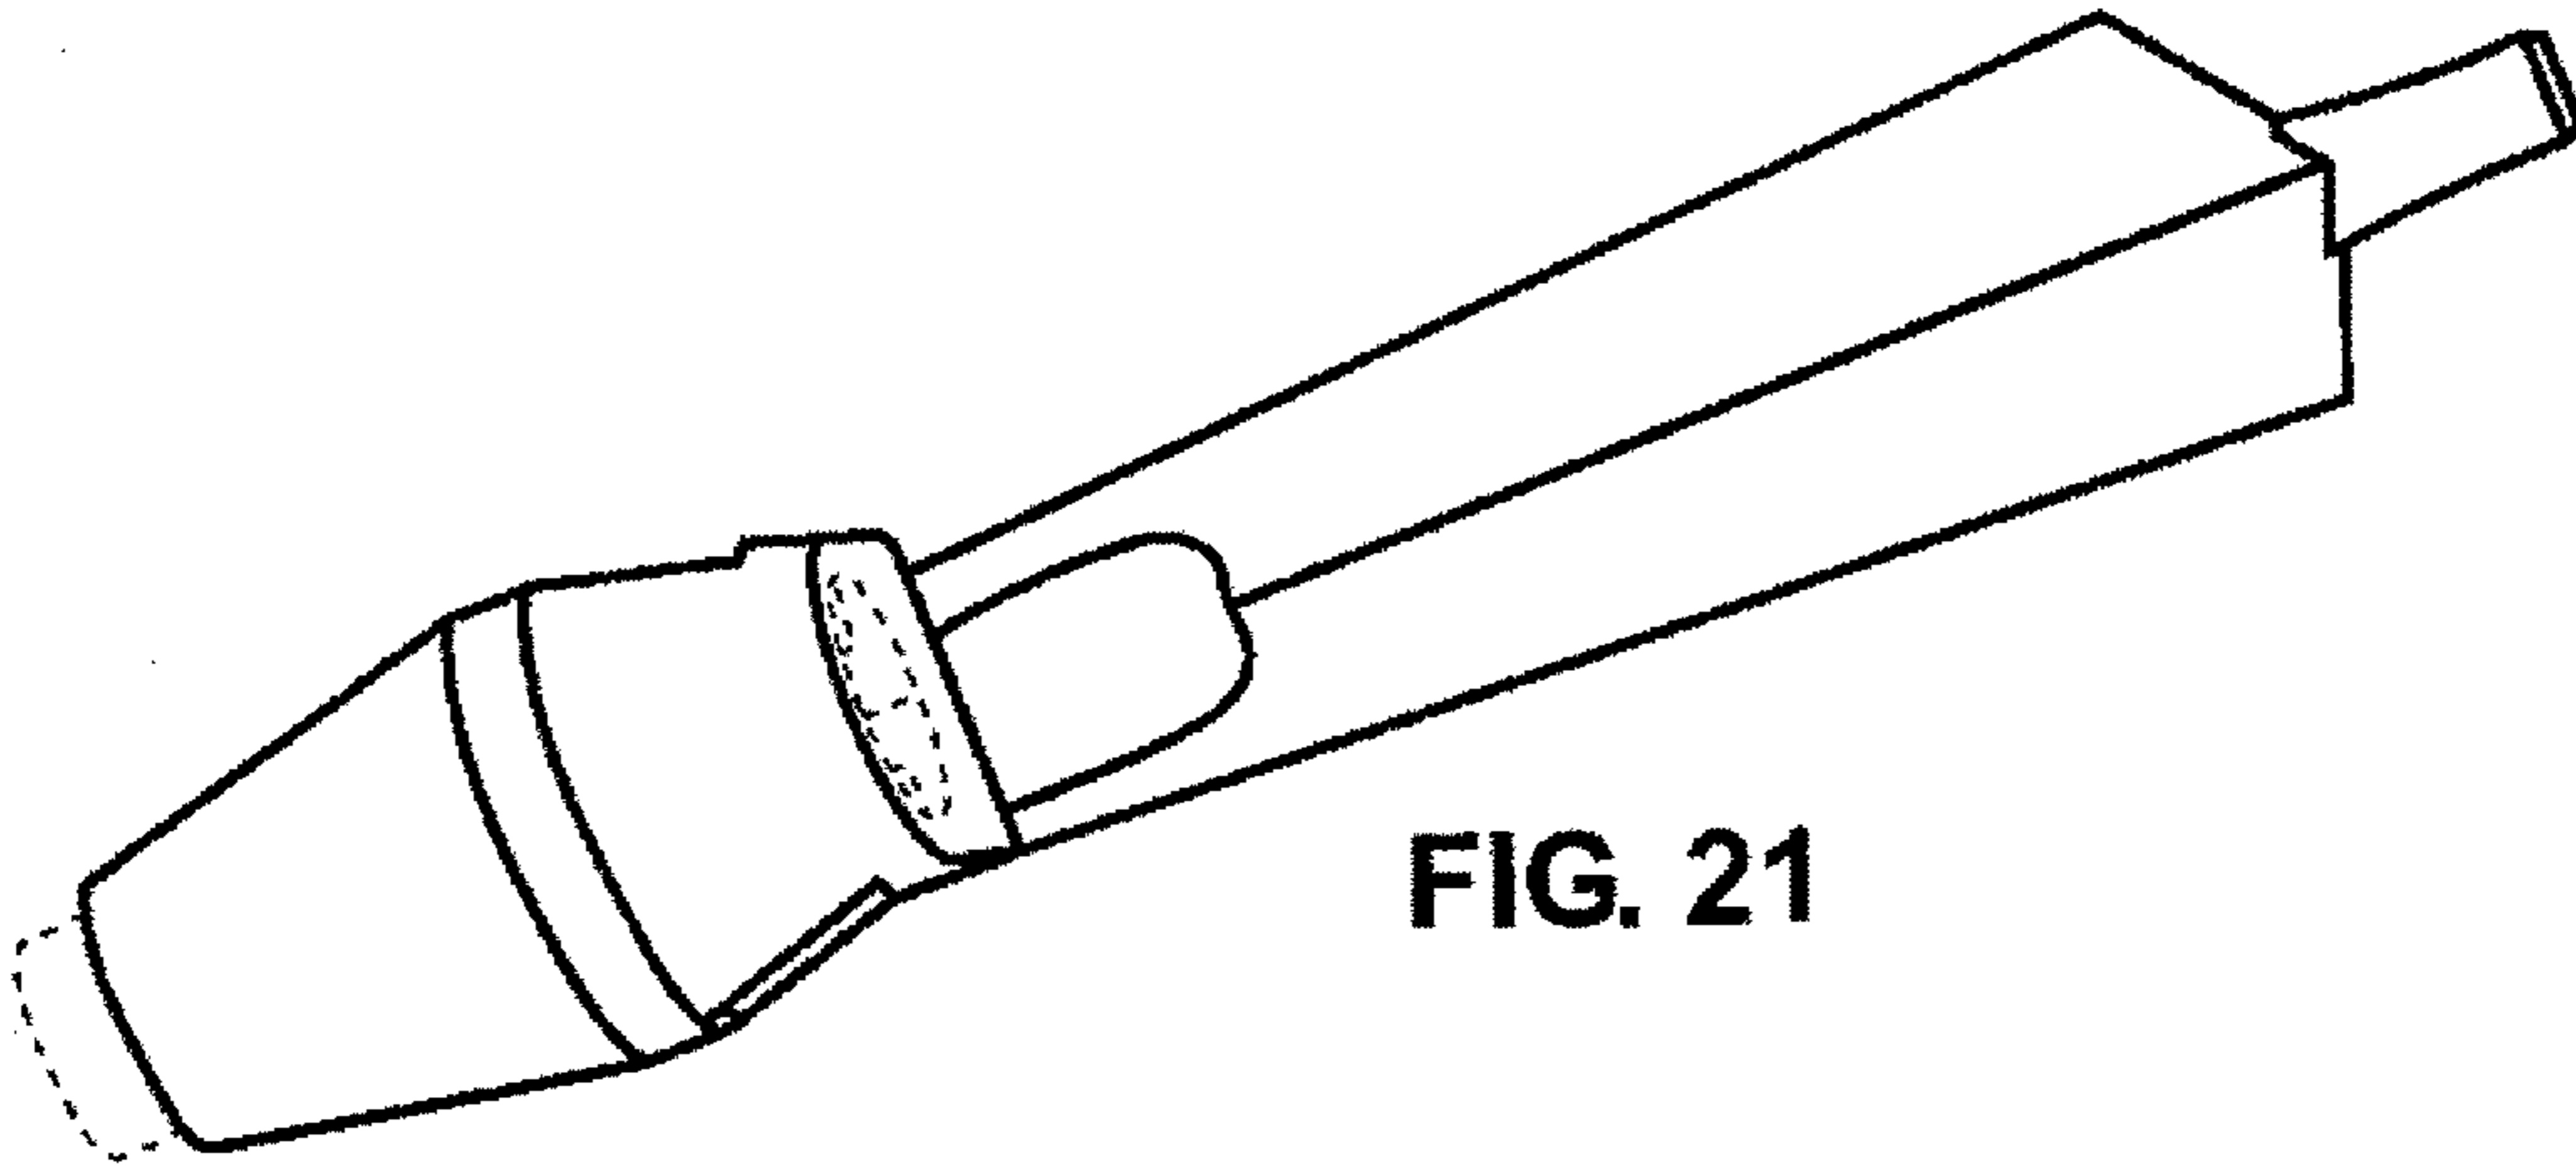


FIG. 21

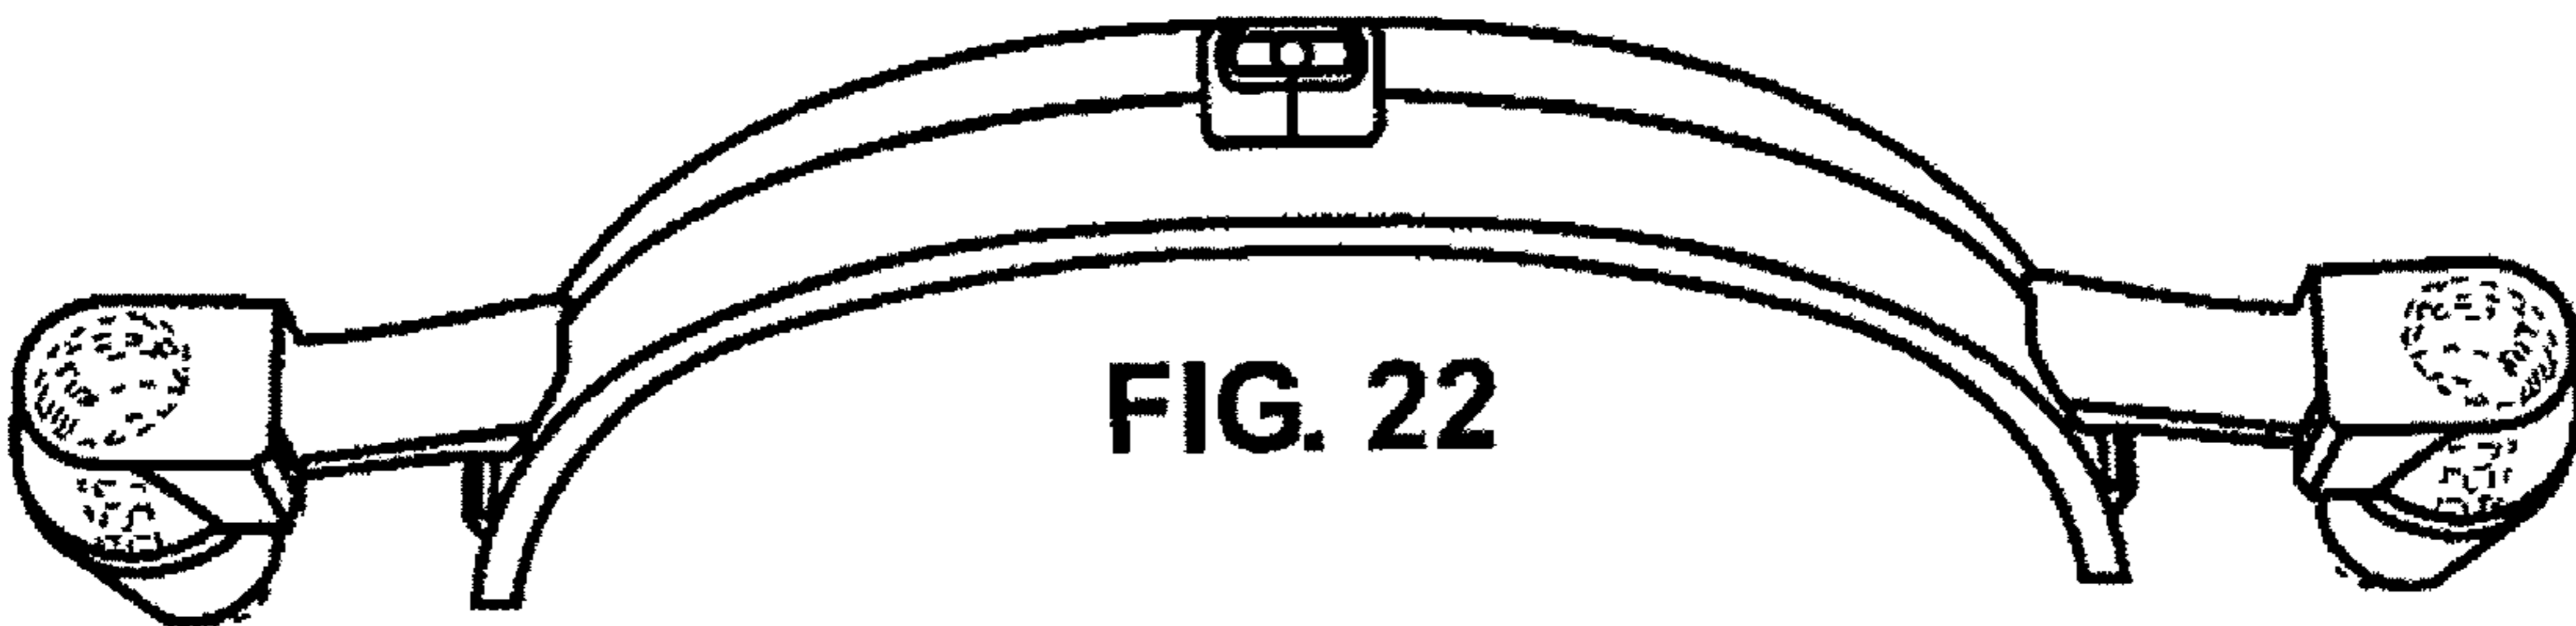


FIG. 22

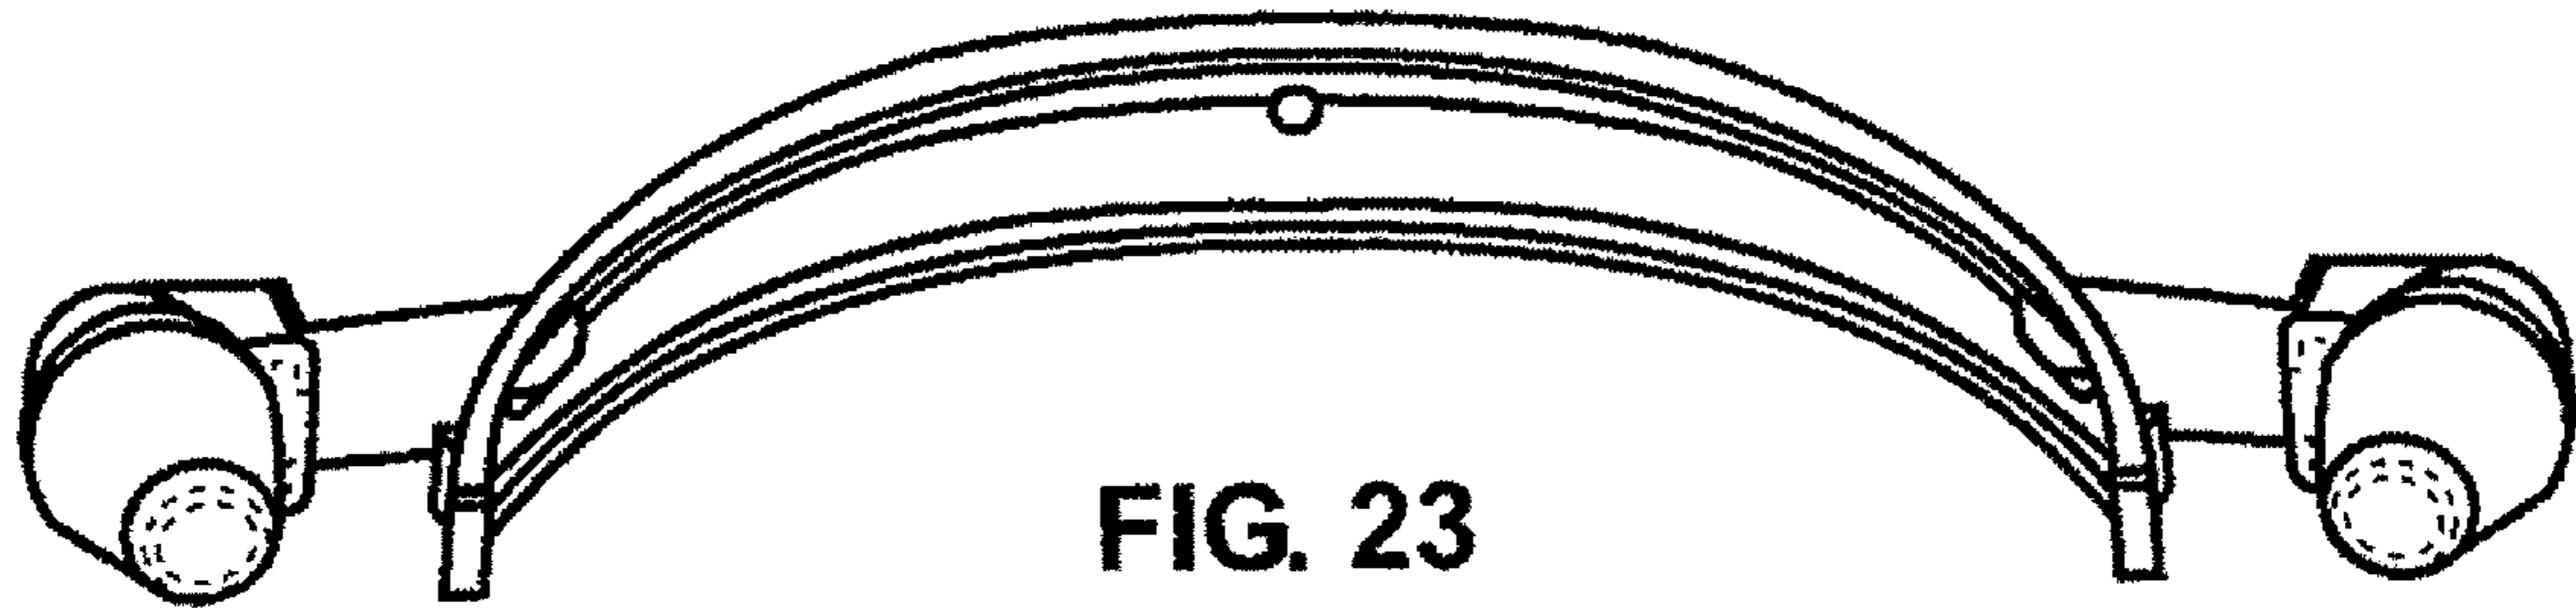


FIG. 23

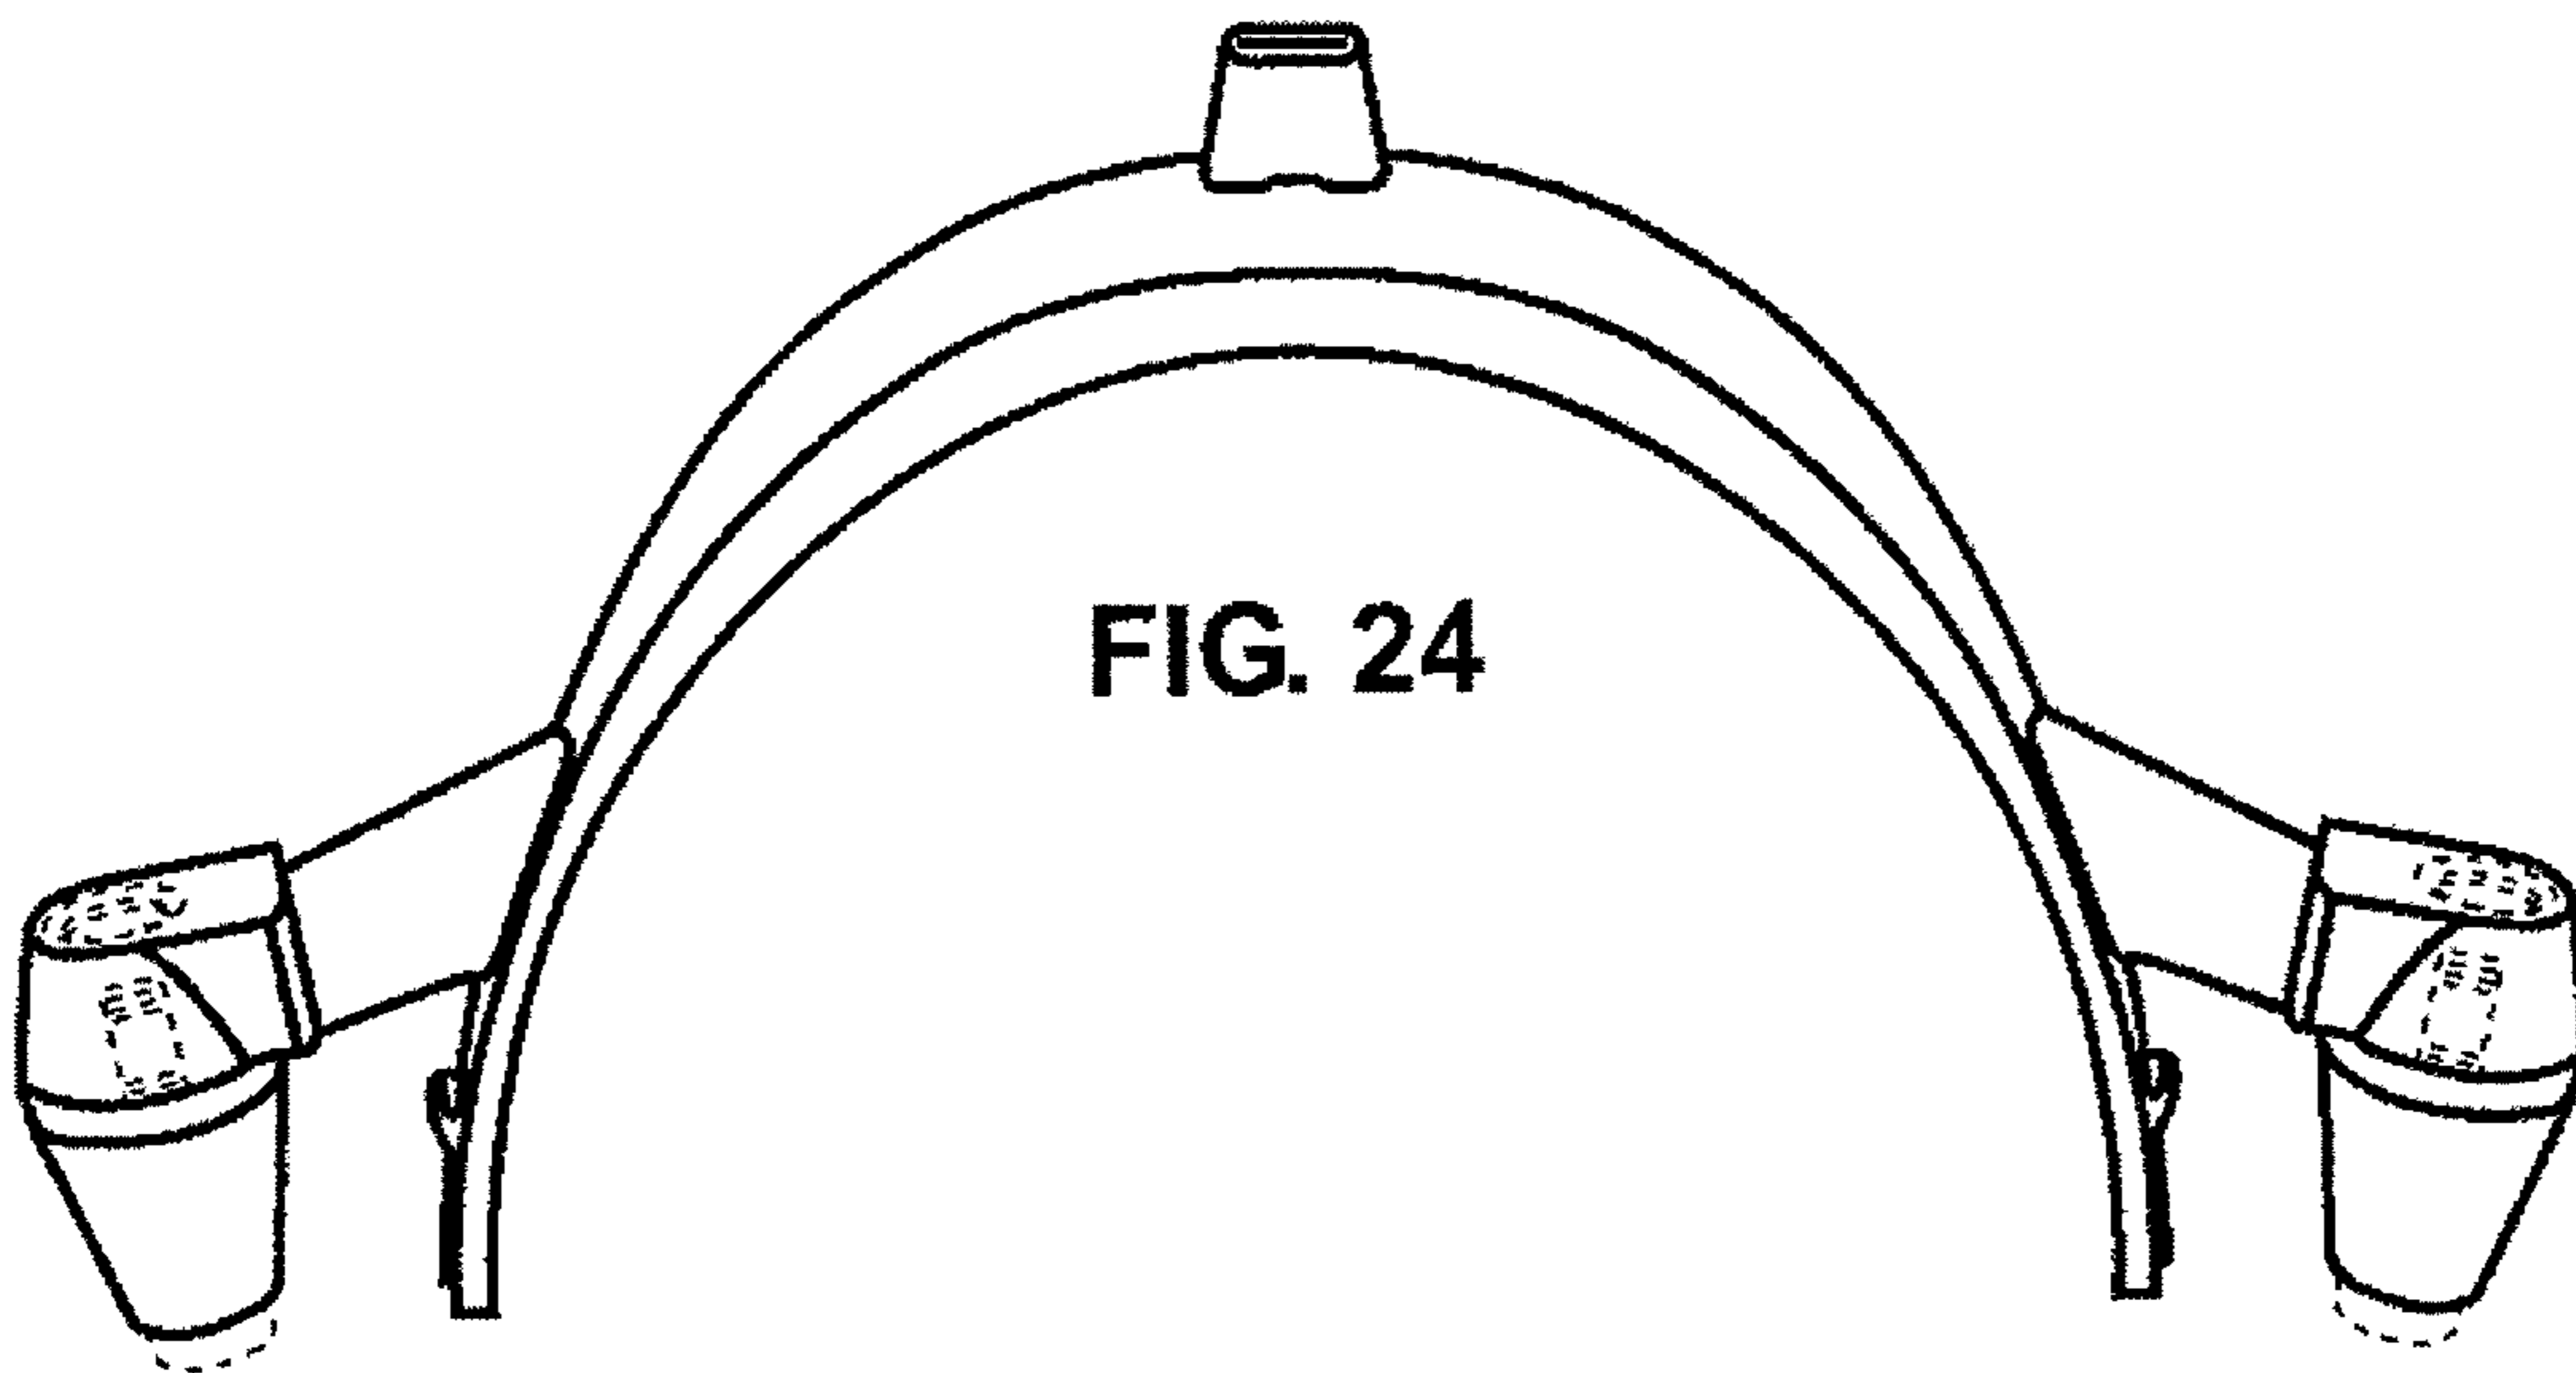


FIG. 24

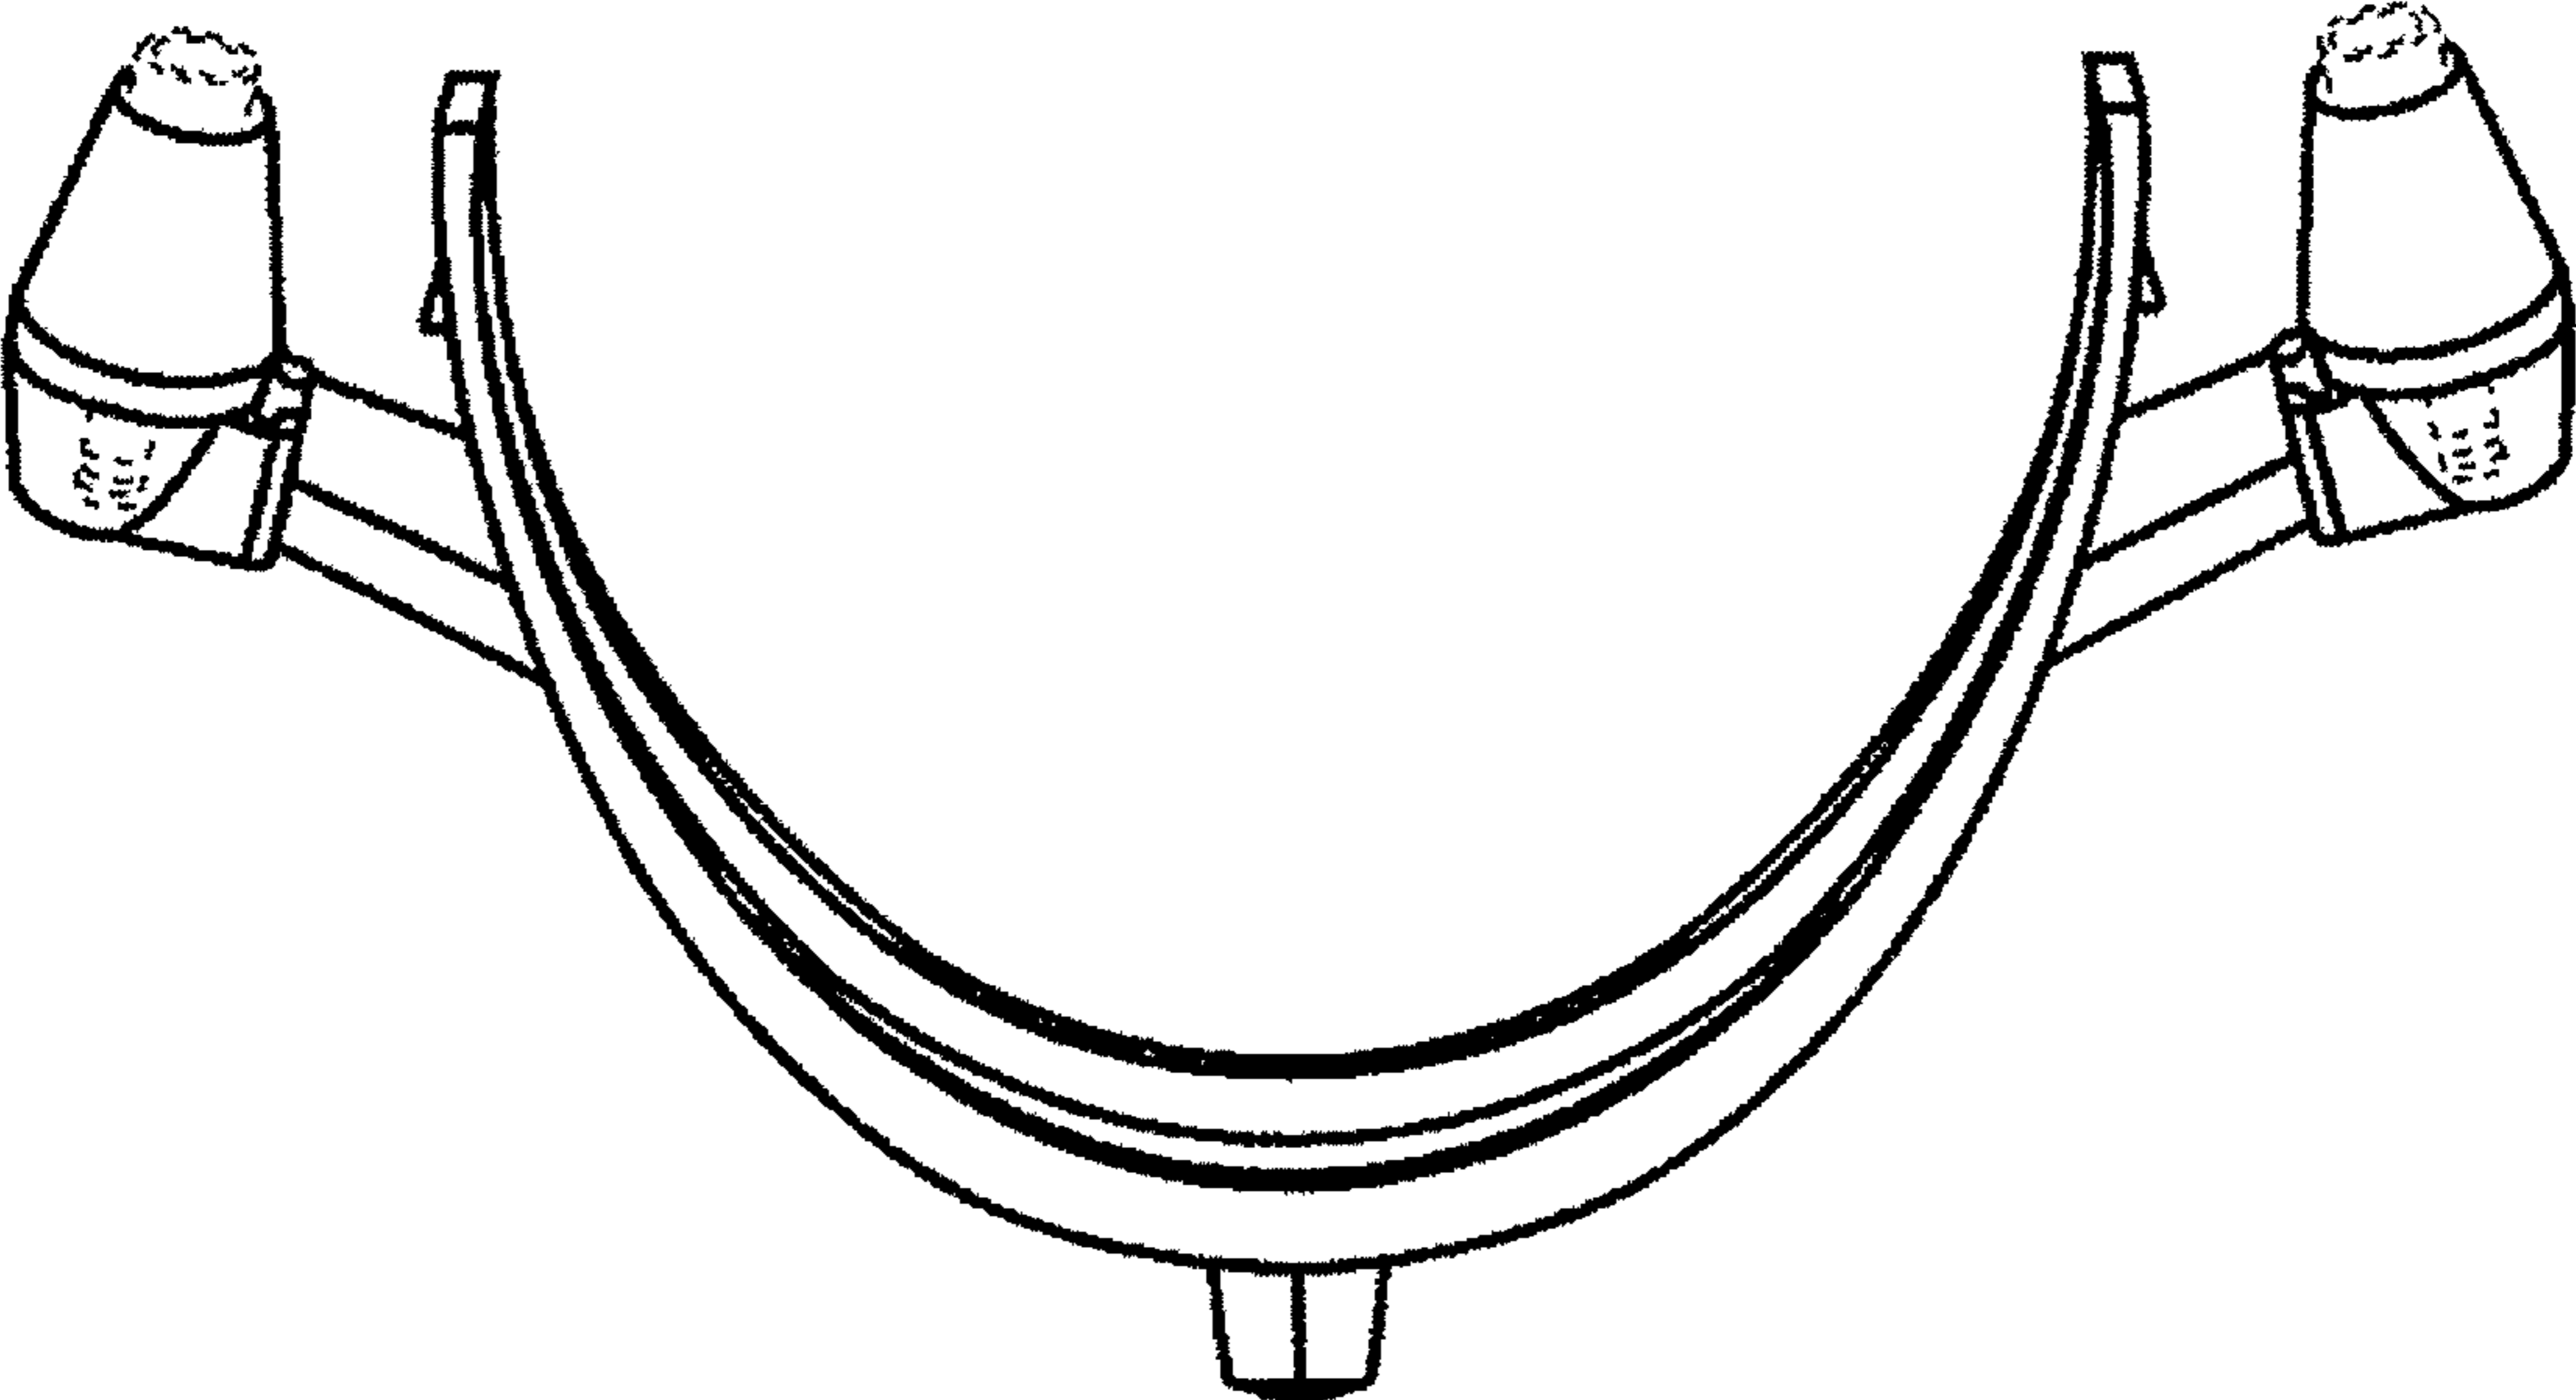


FIG. 25

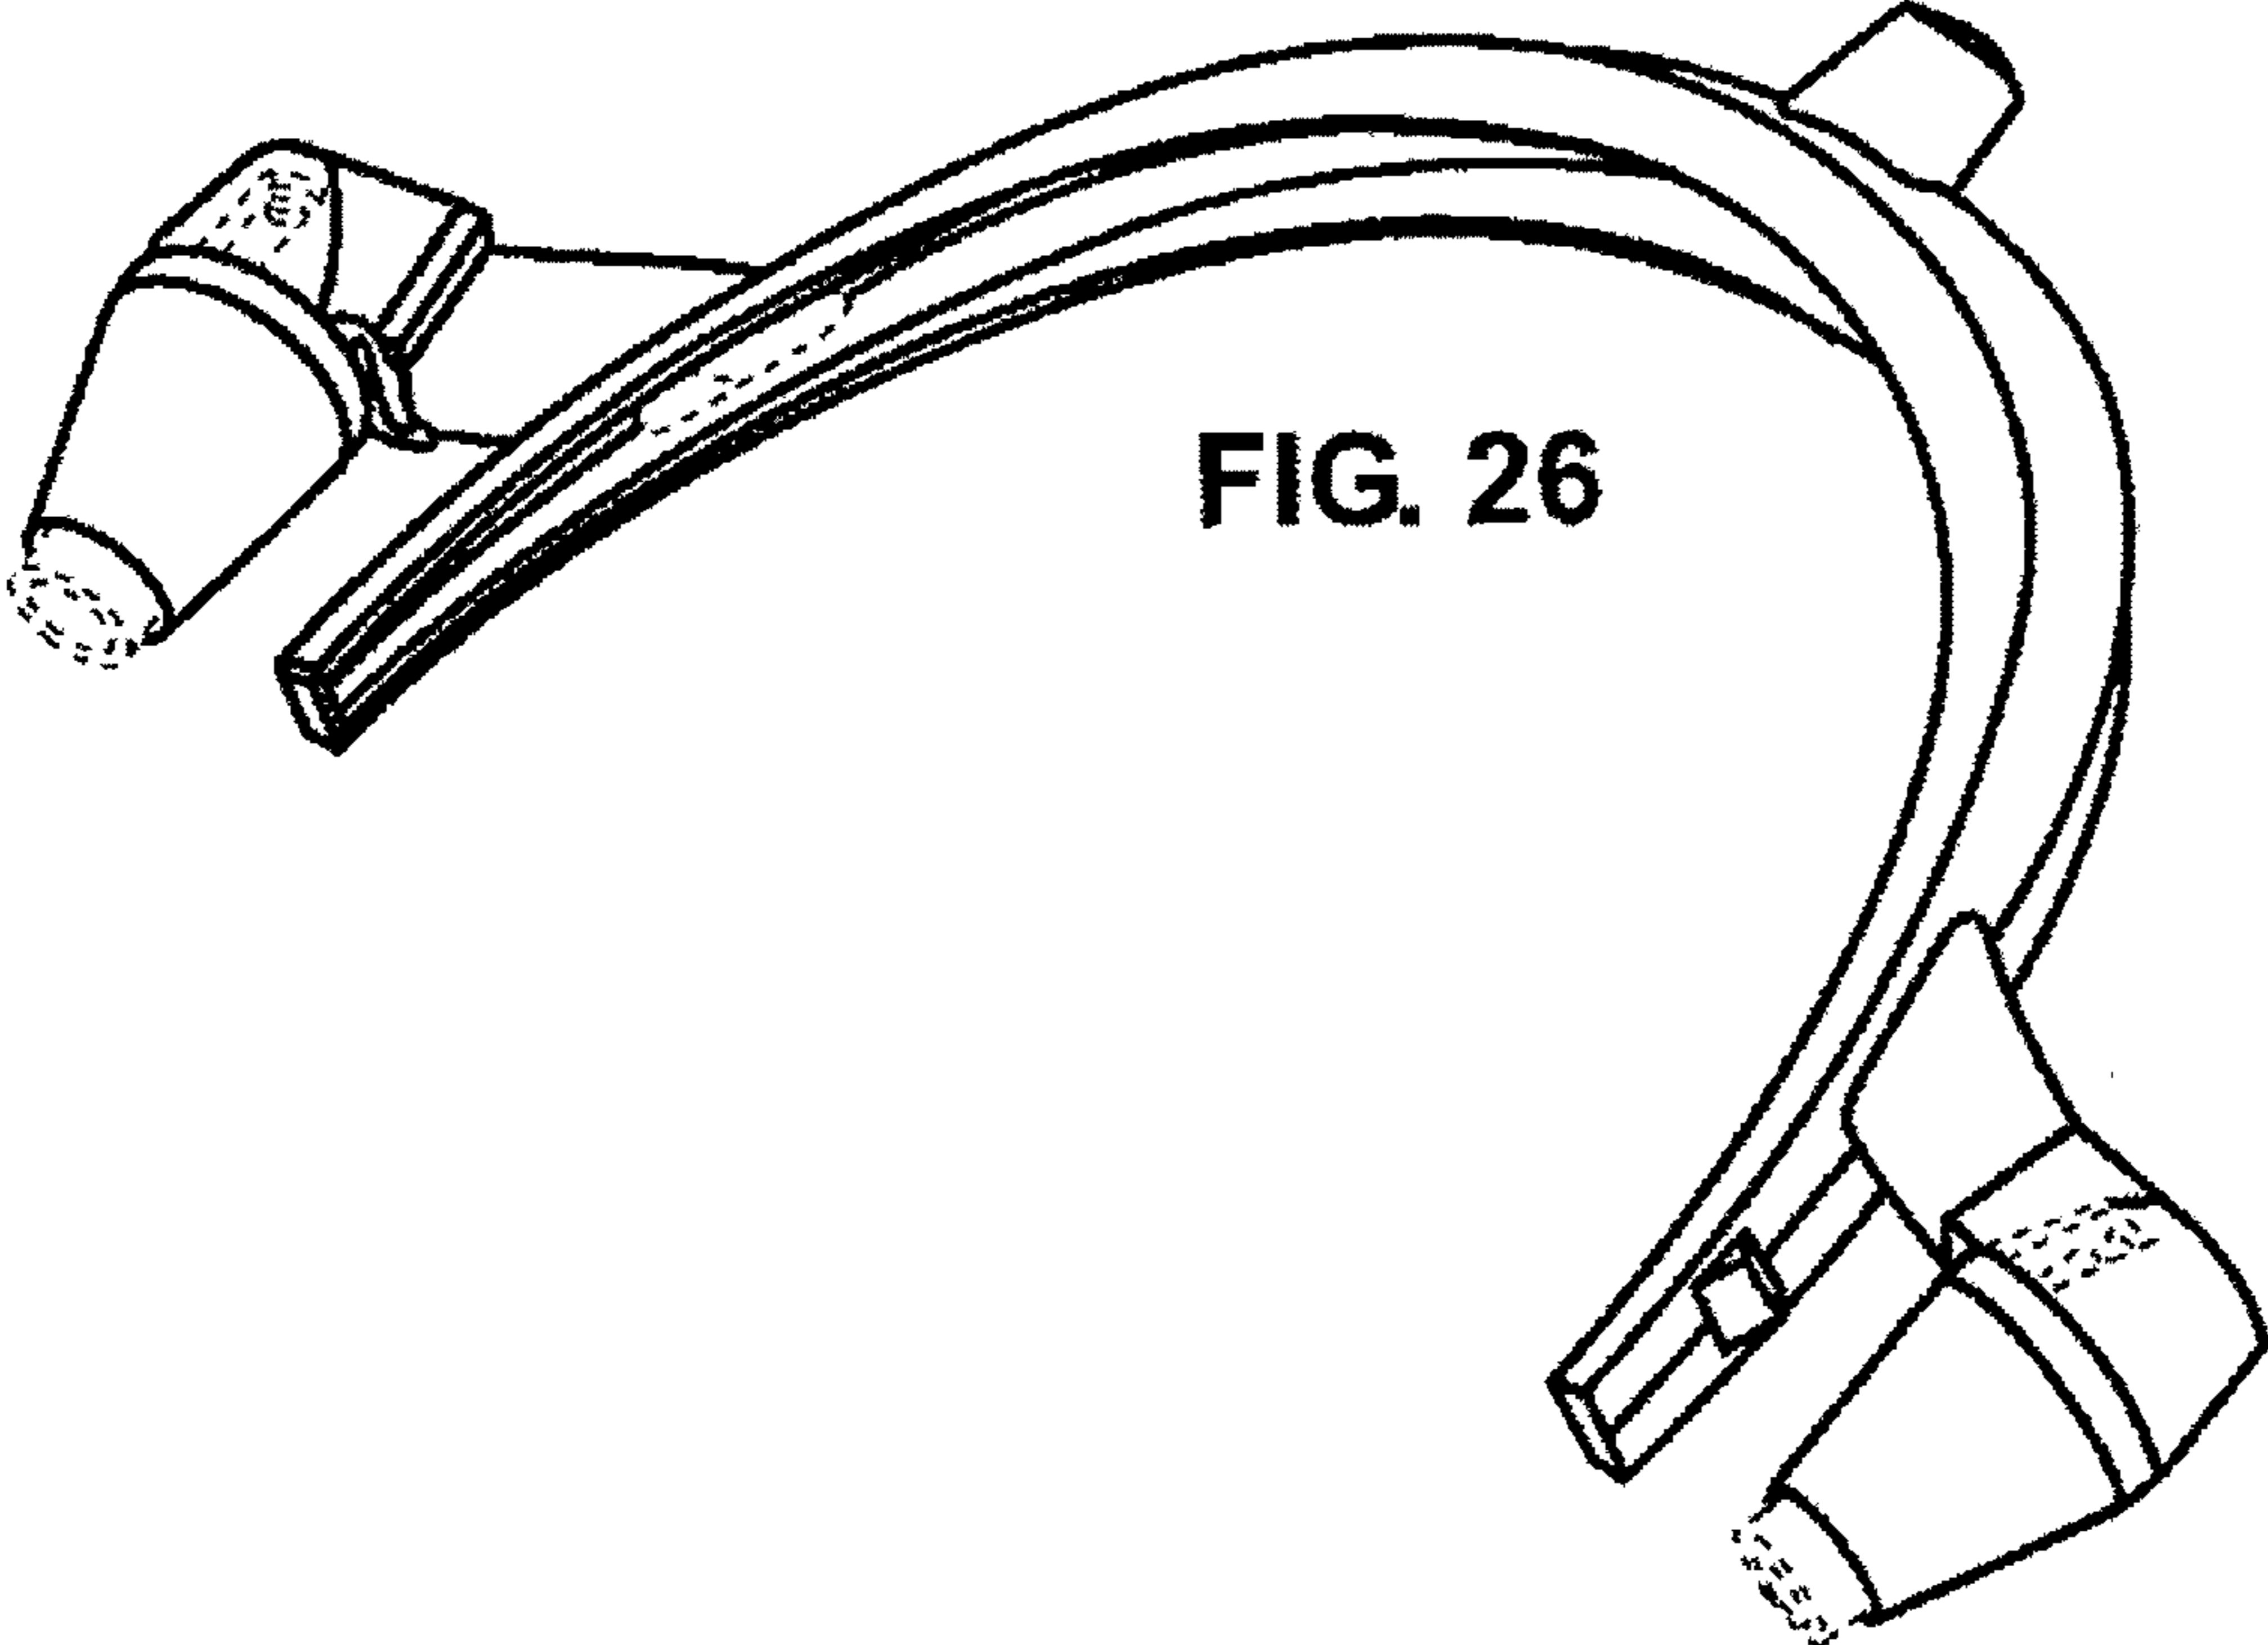


FIG. 26

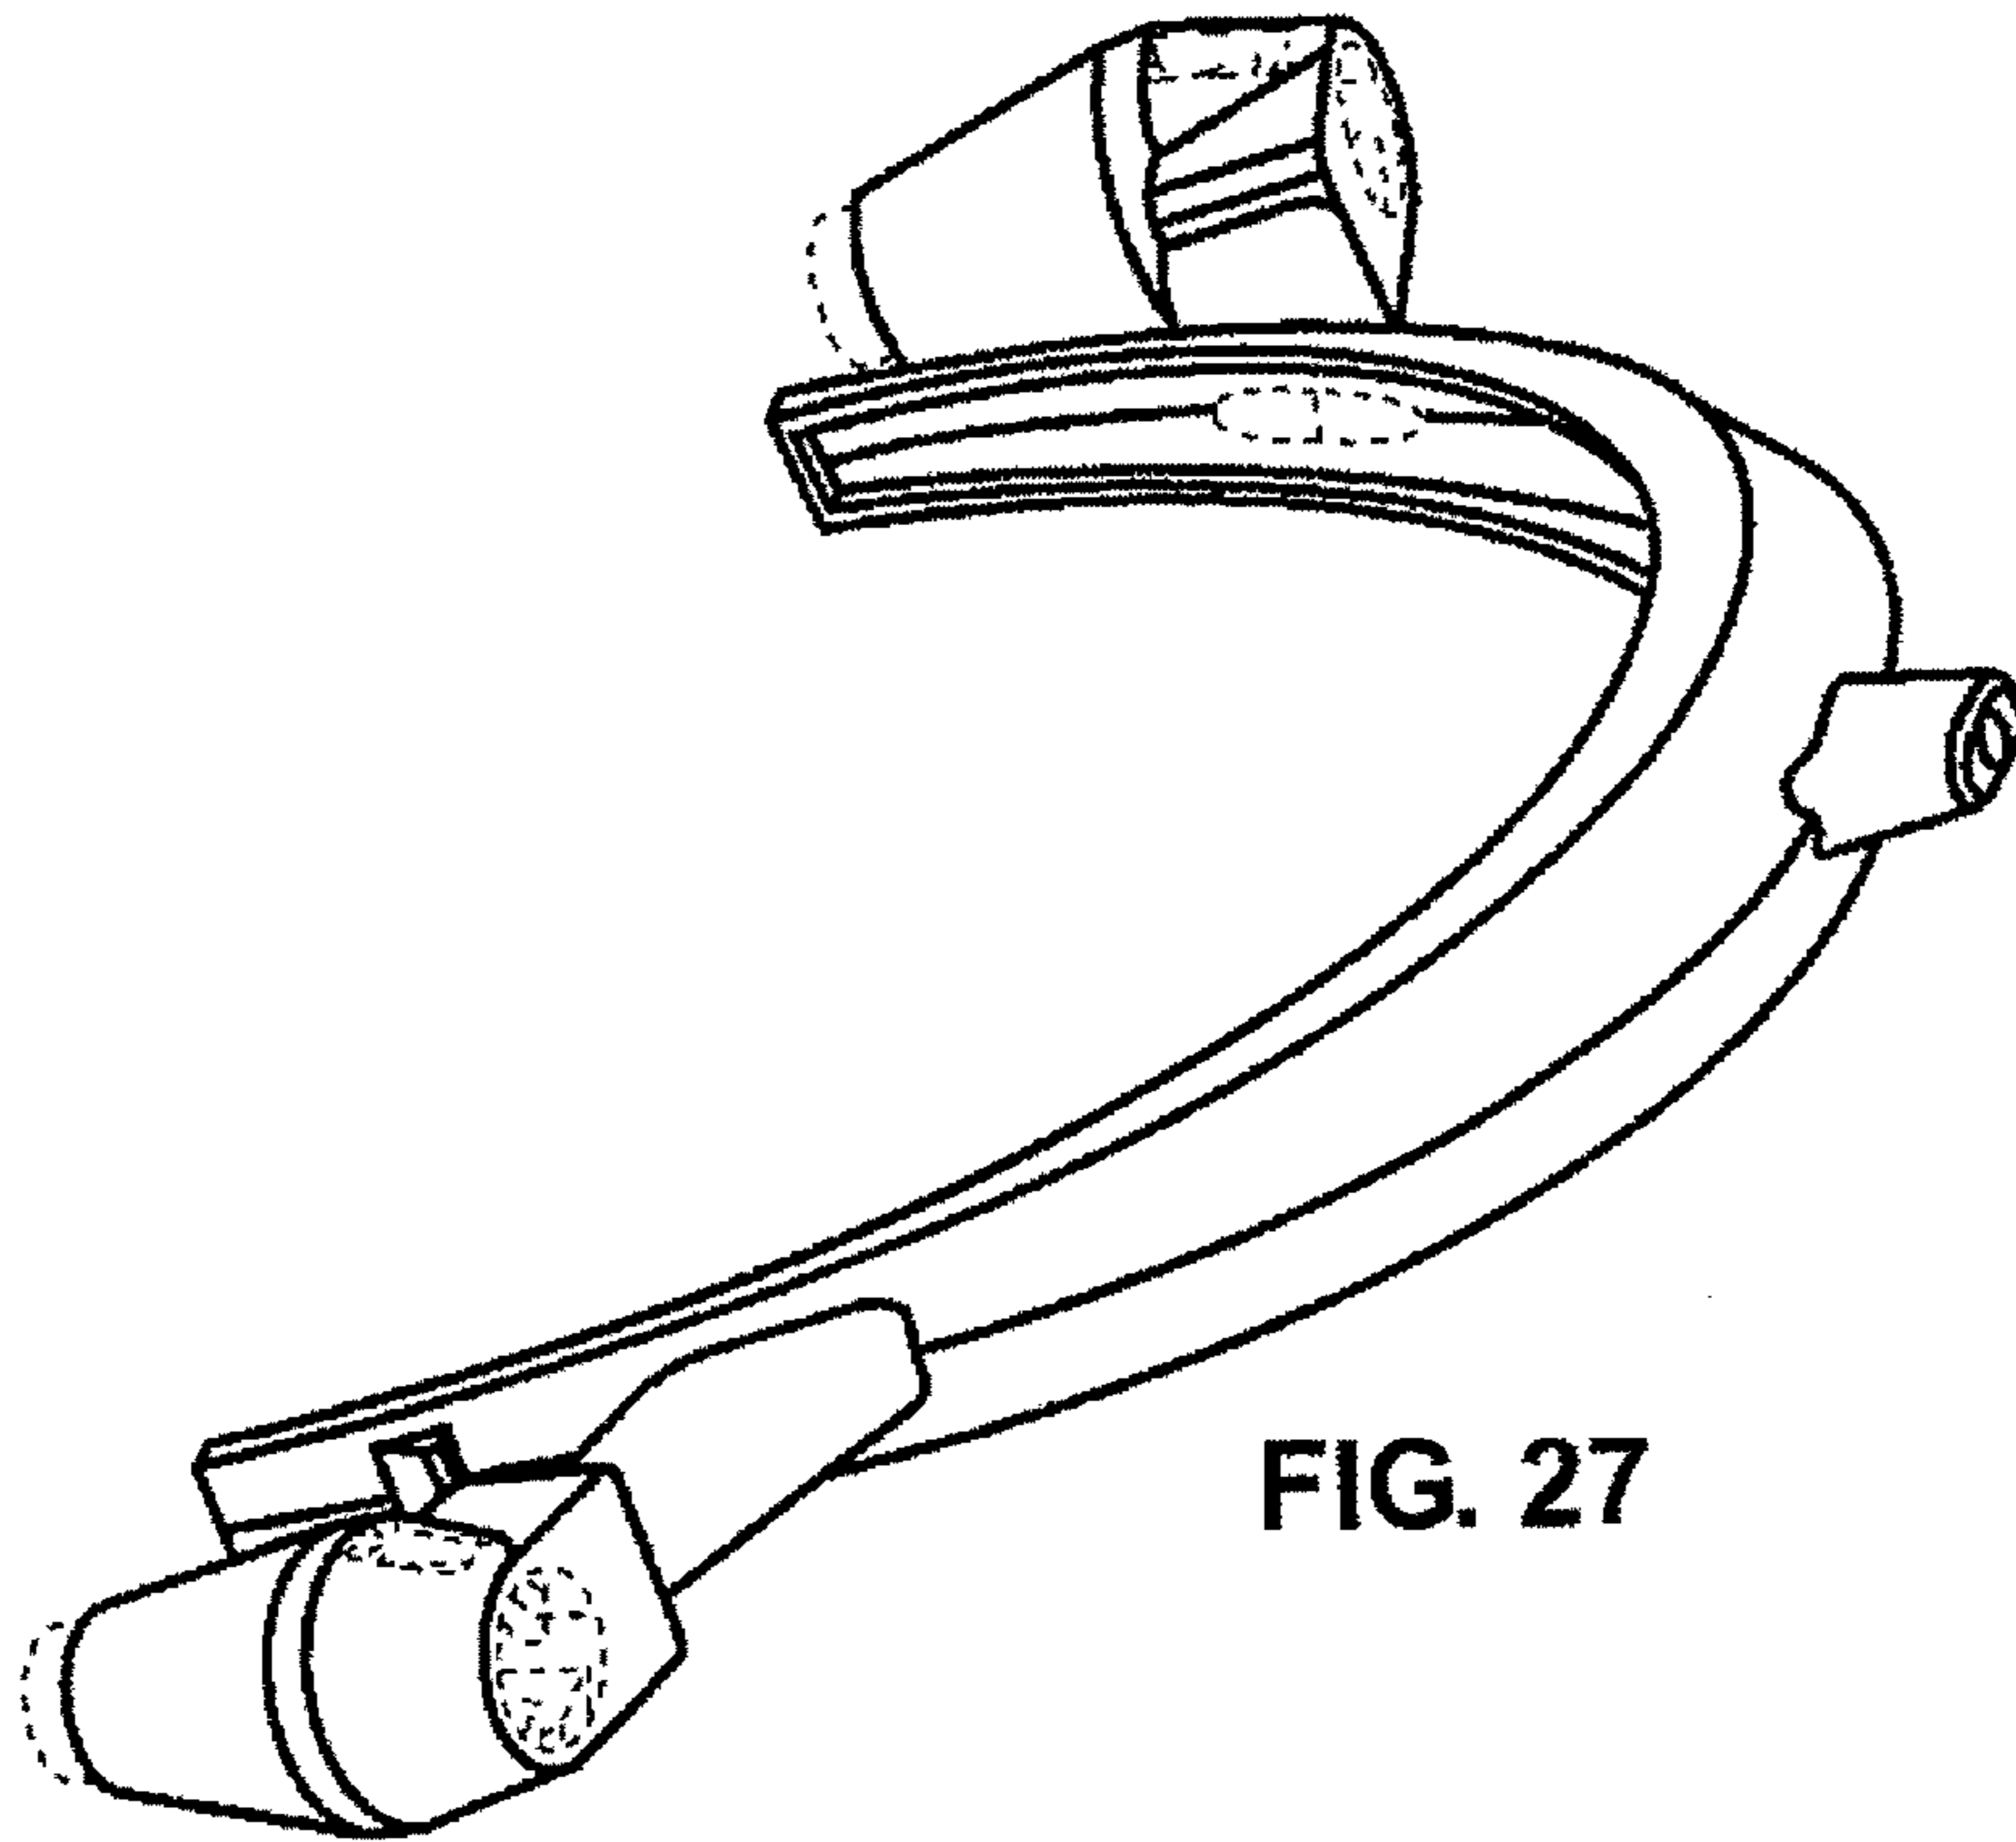


FIG. 27

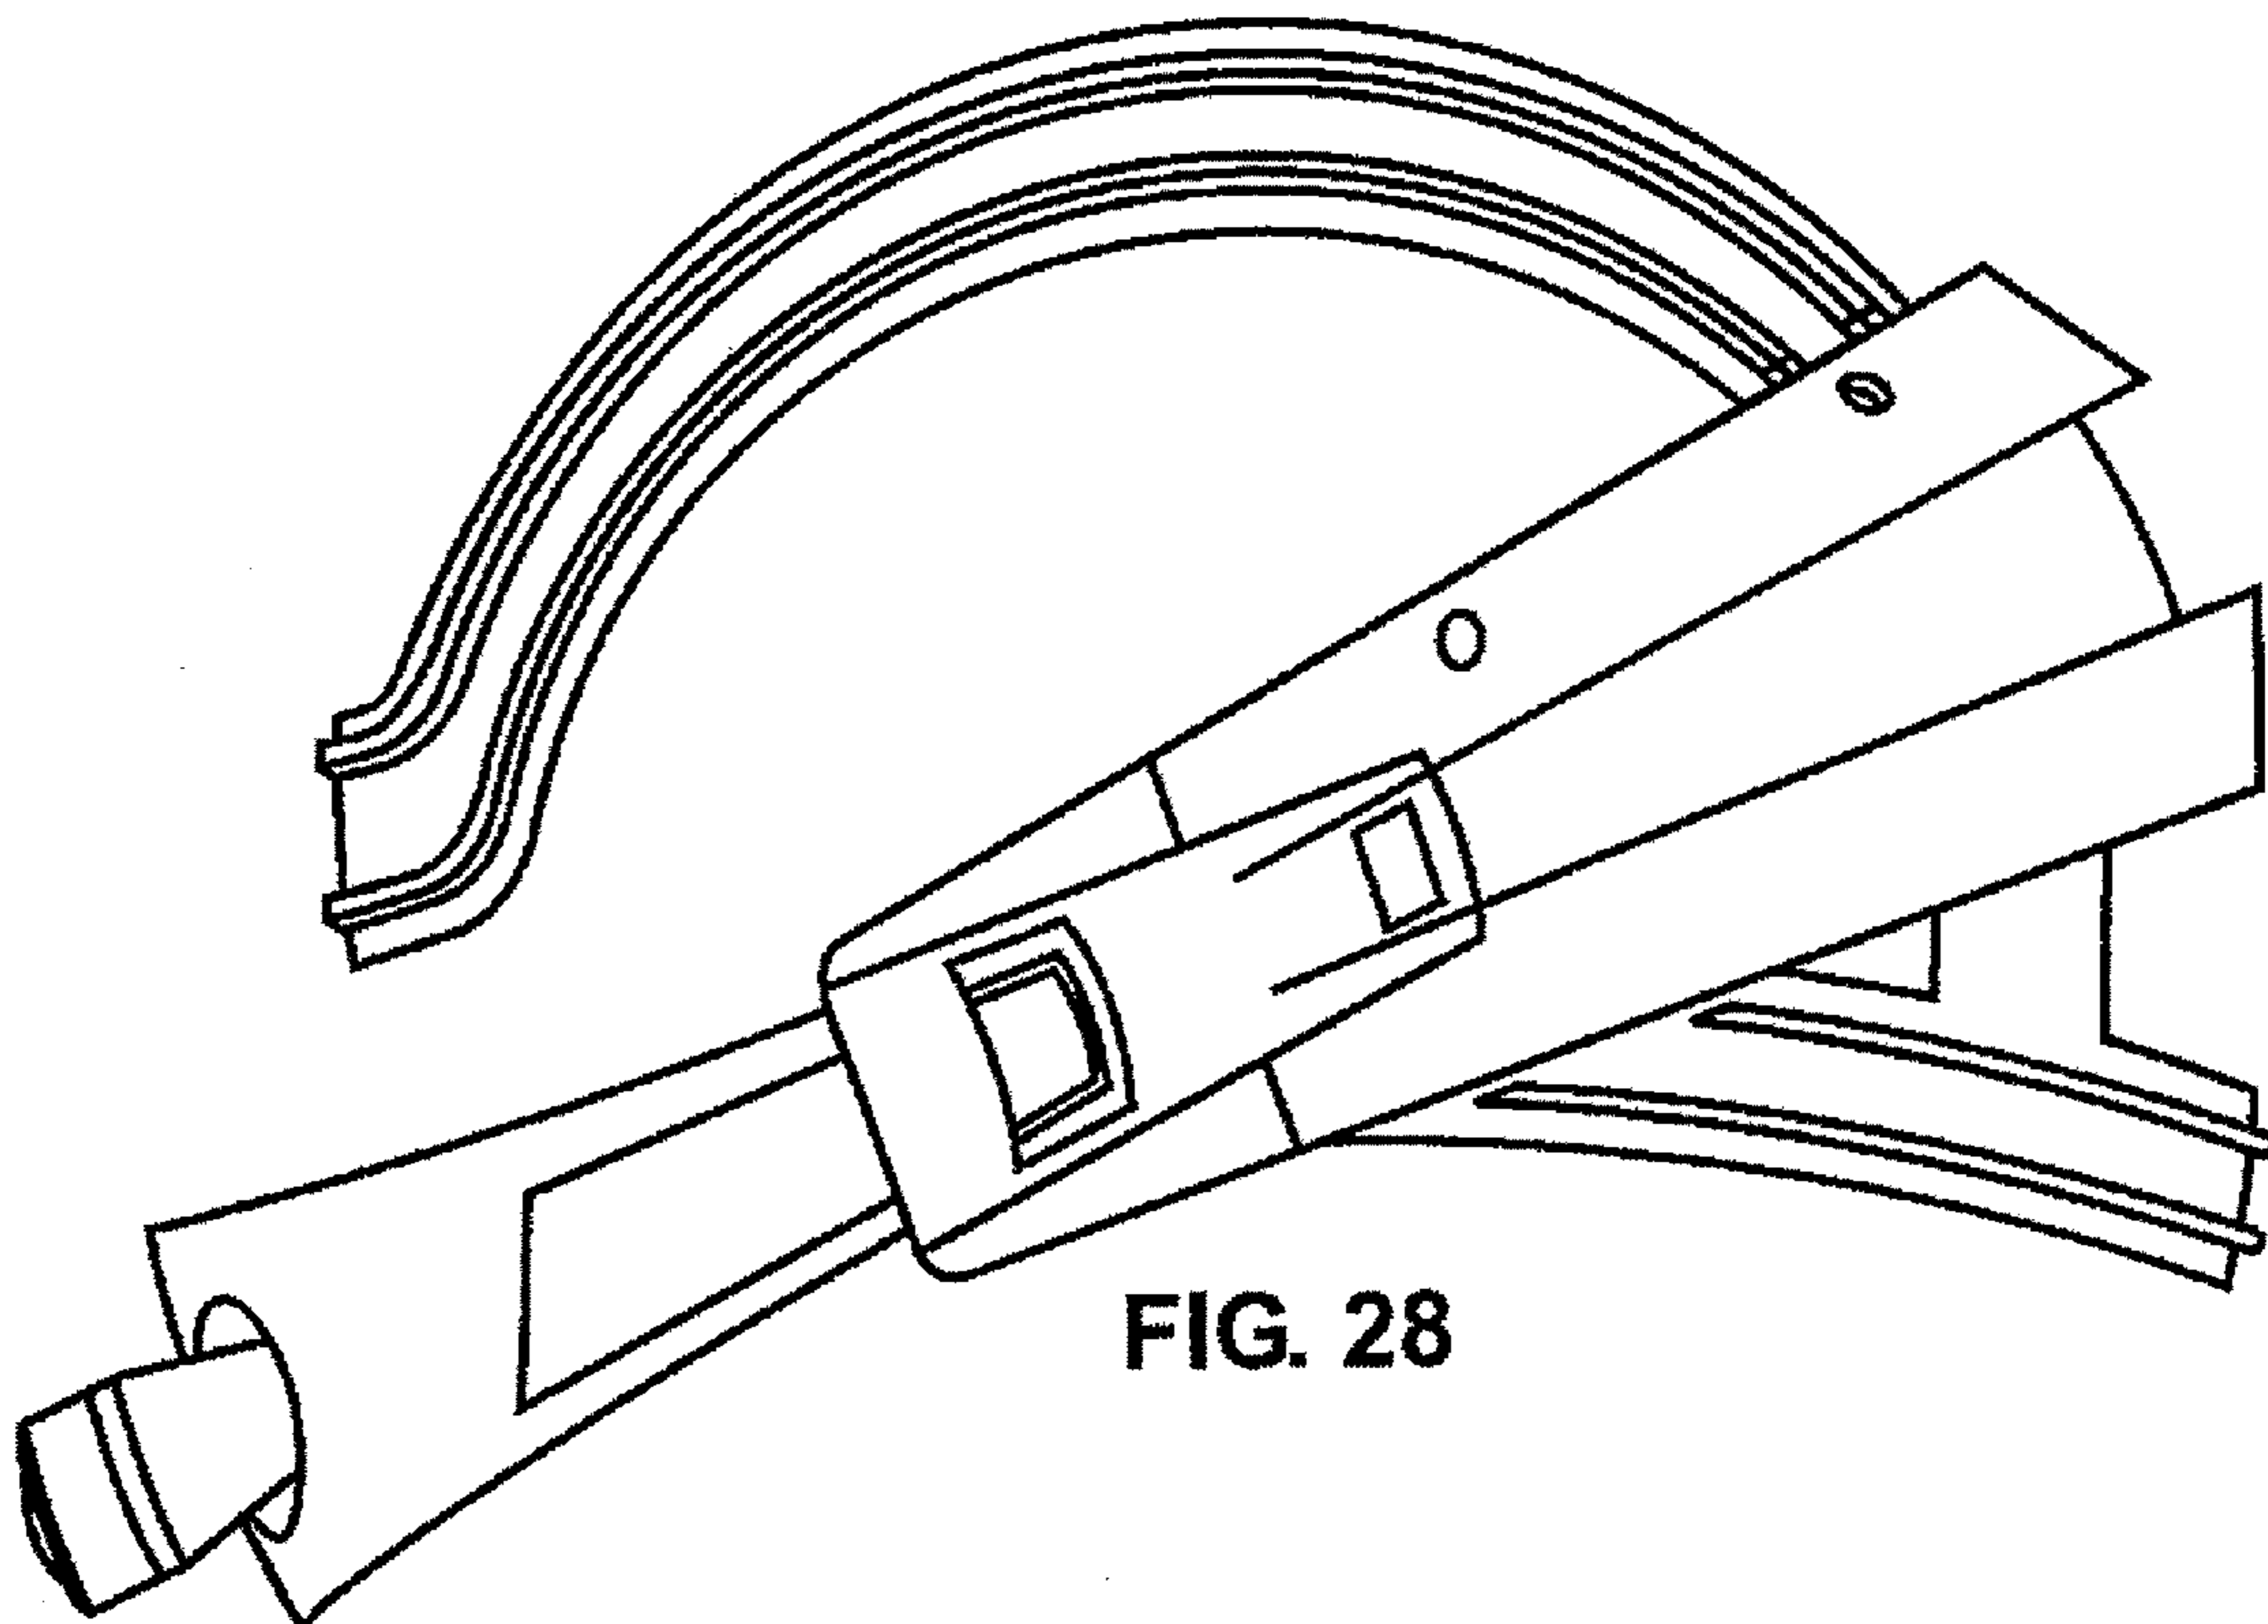


FIG. 28

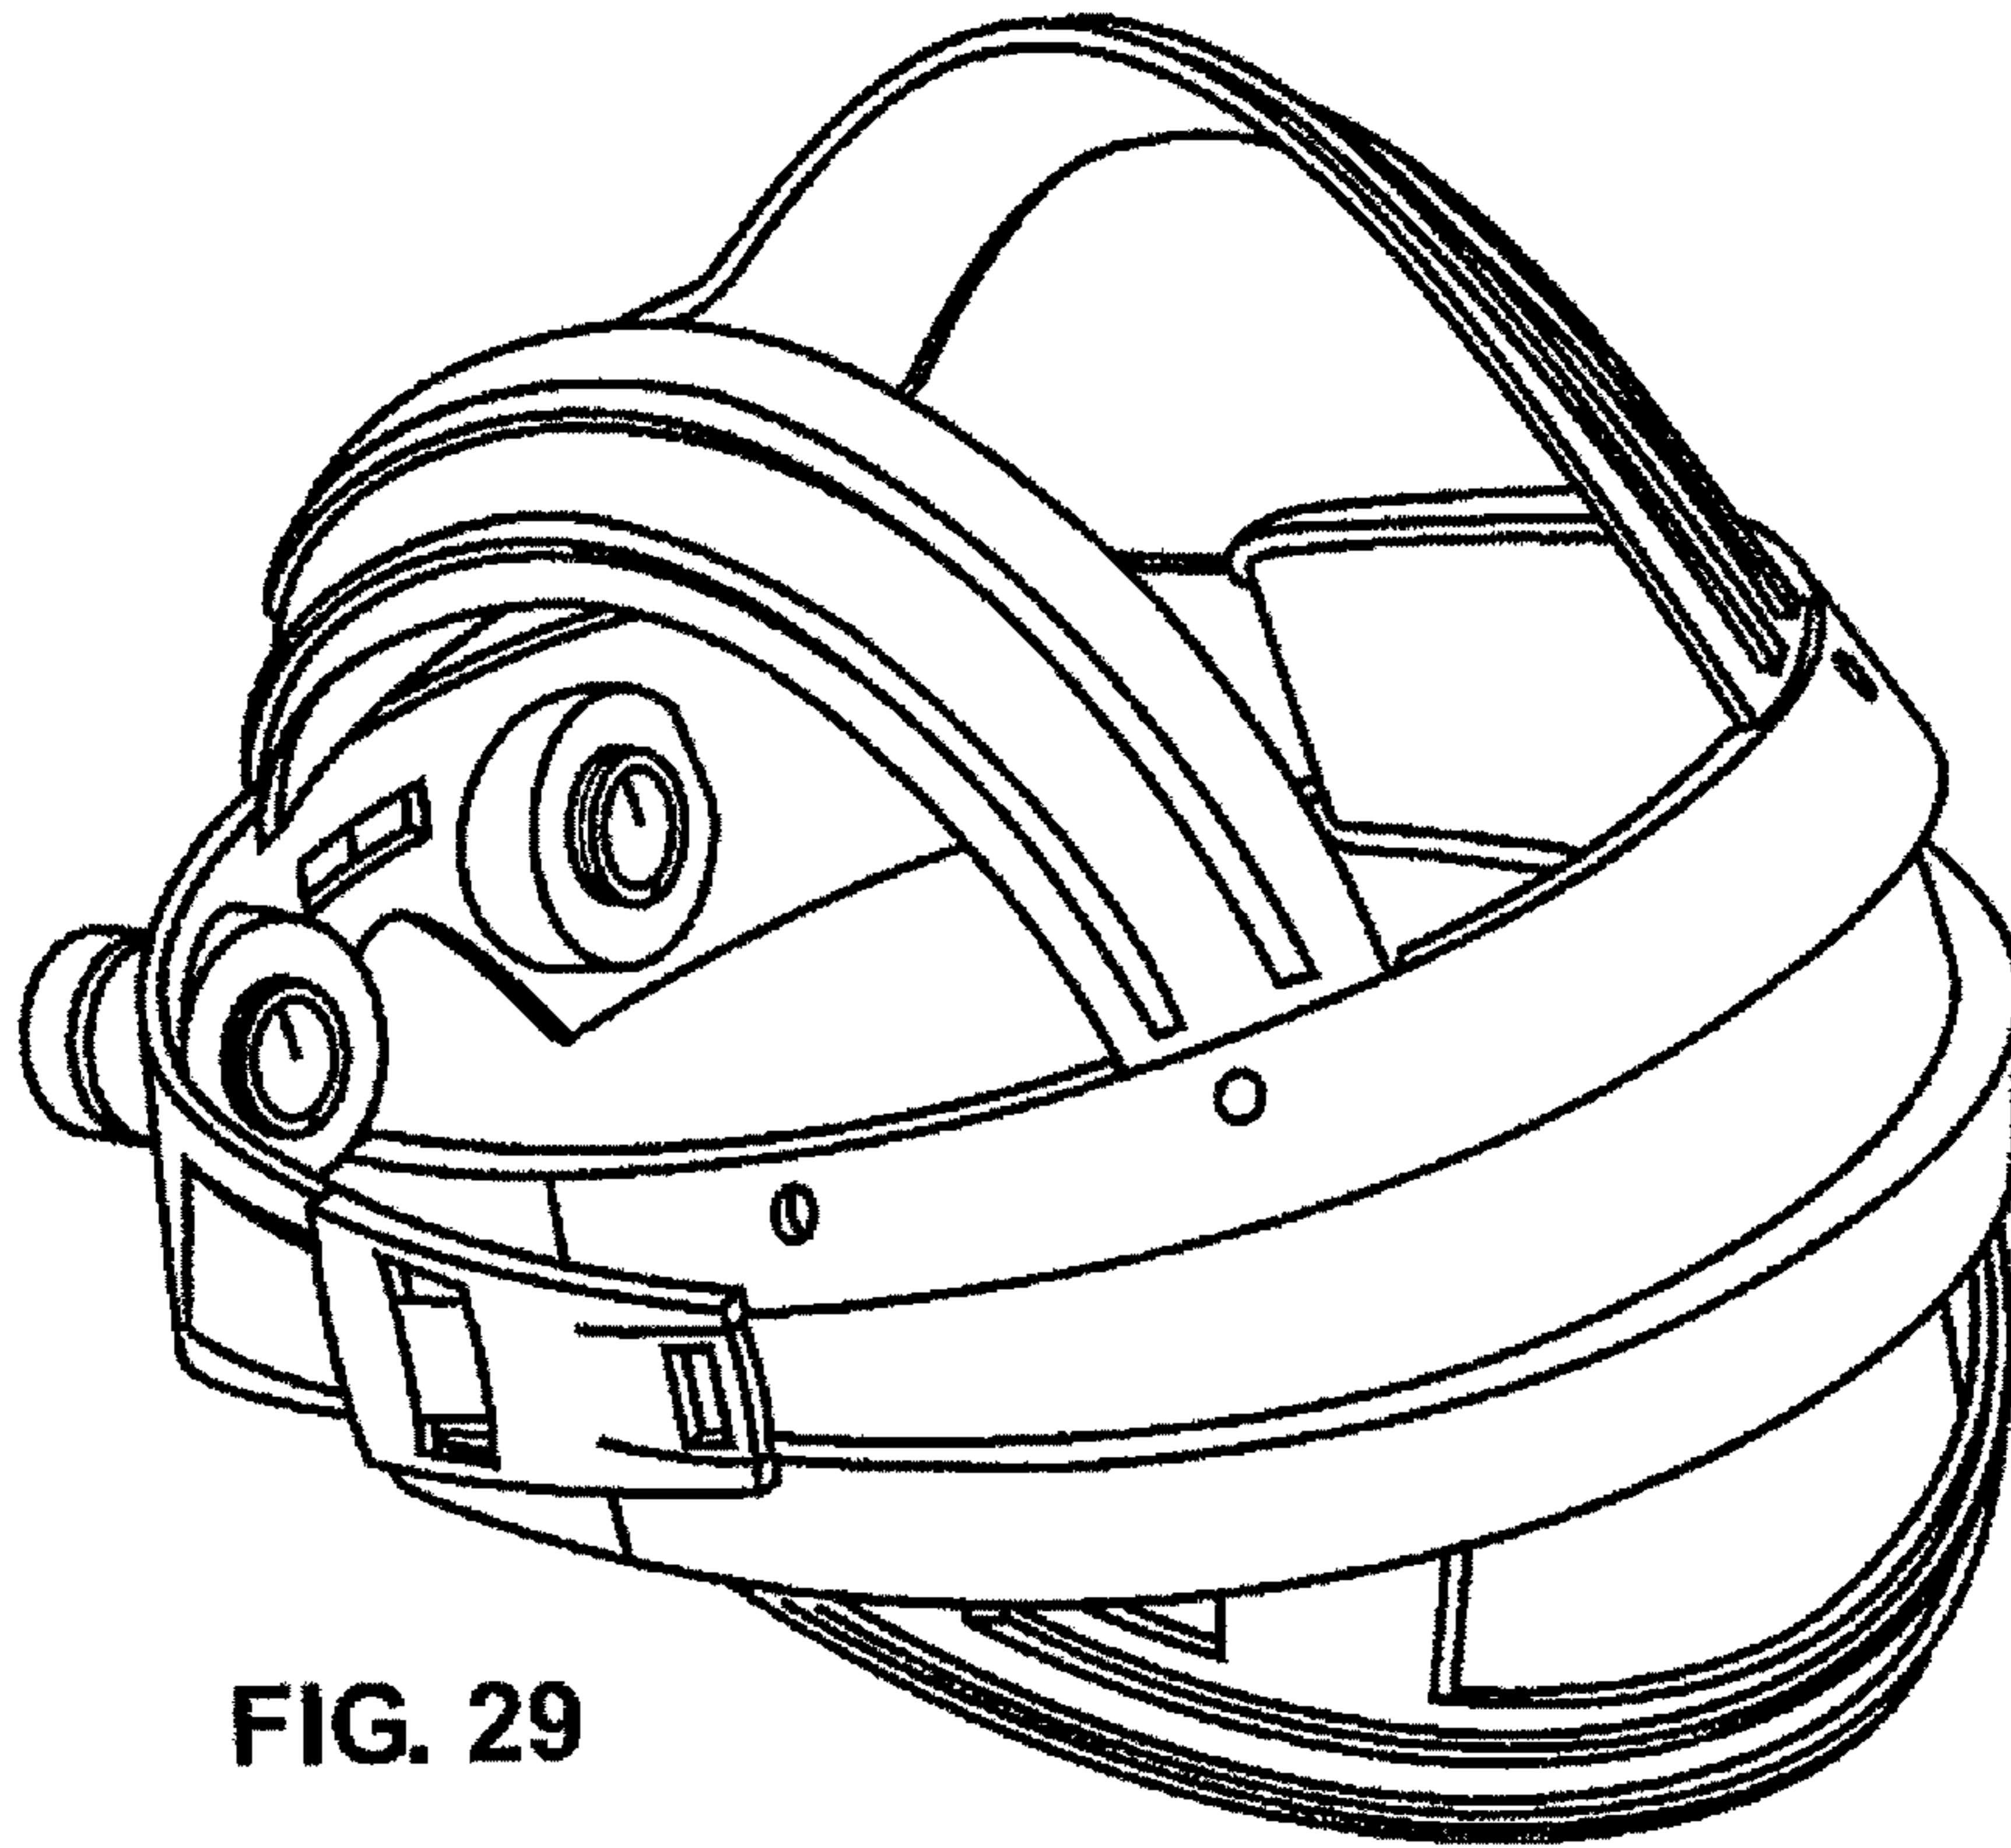


FIG. 29

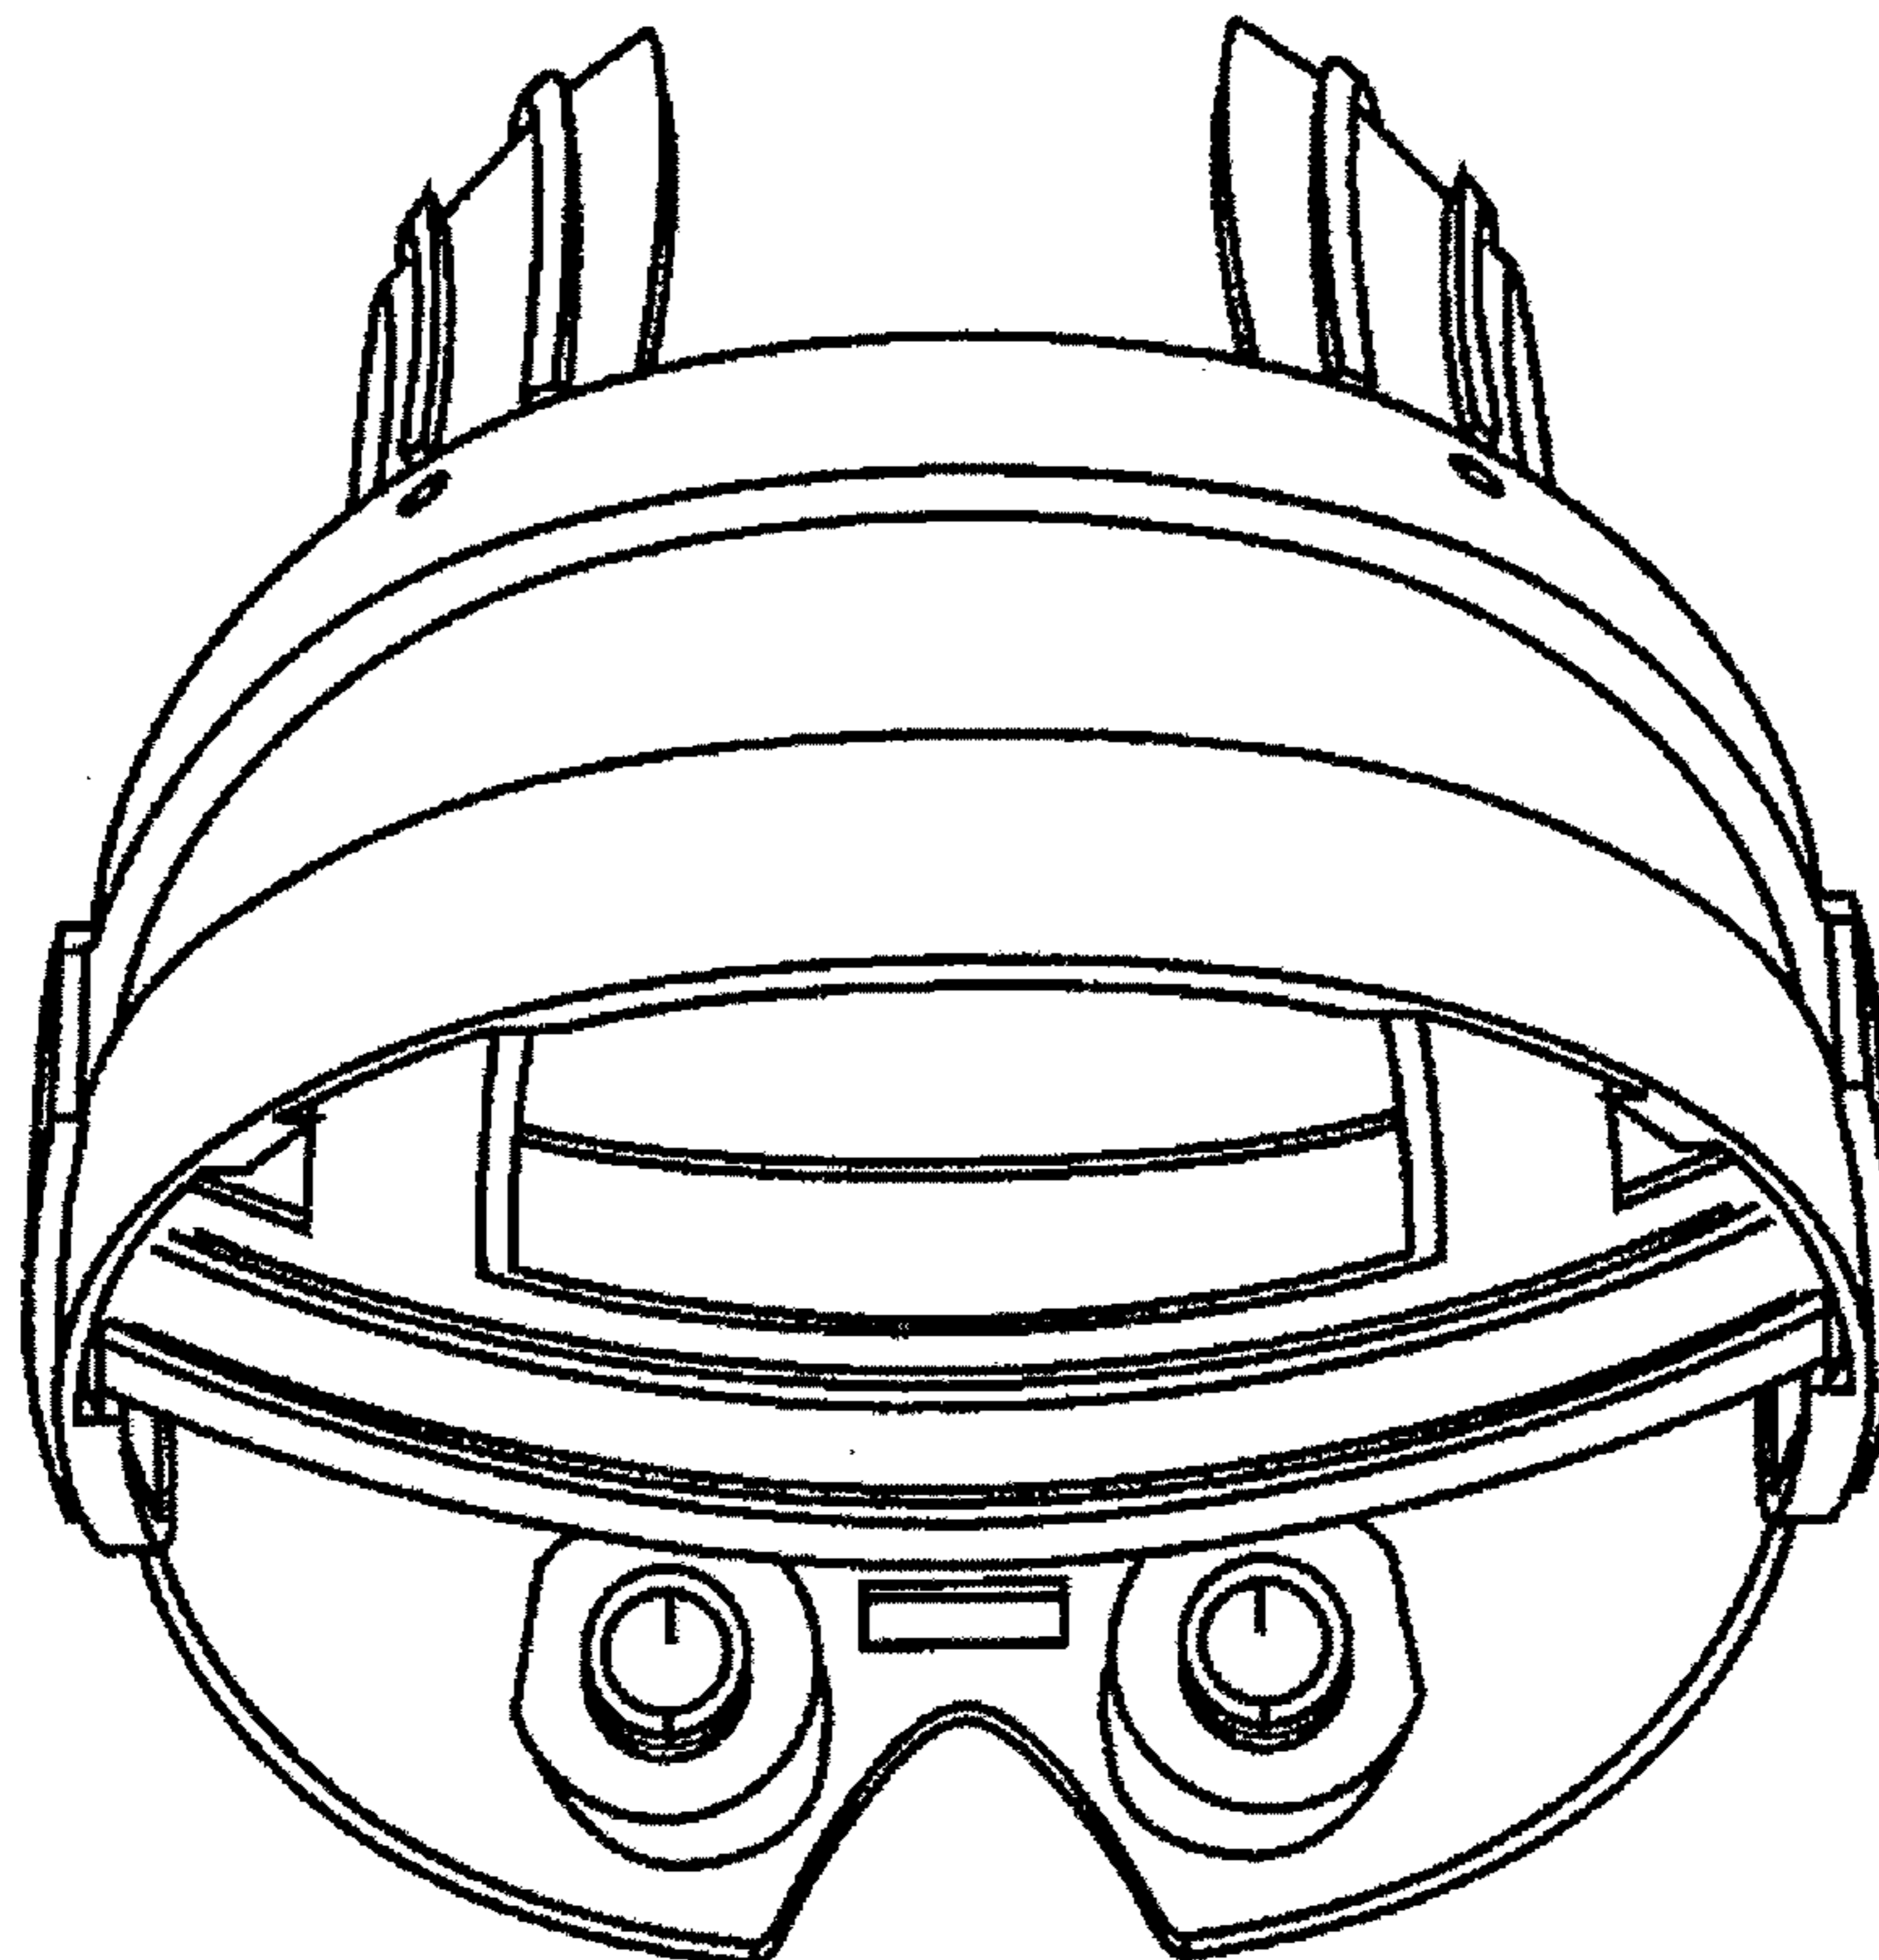


FIG. 30

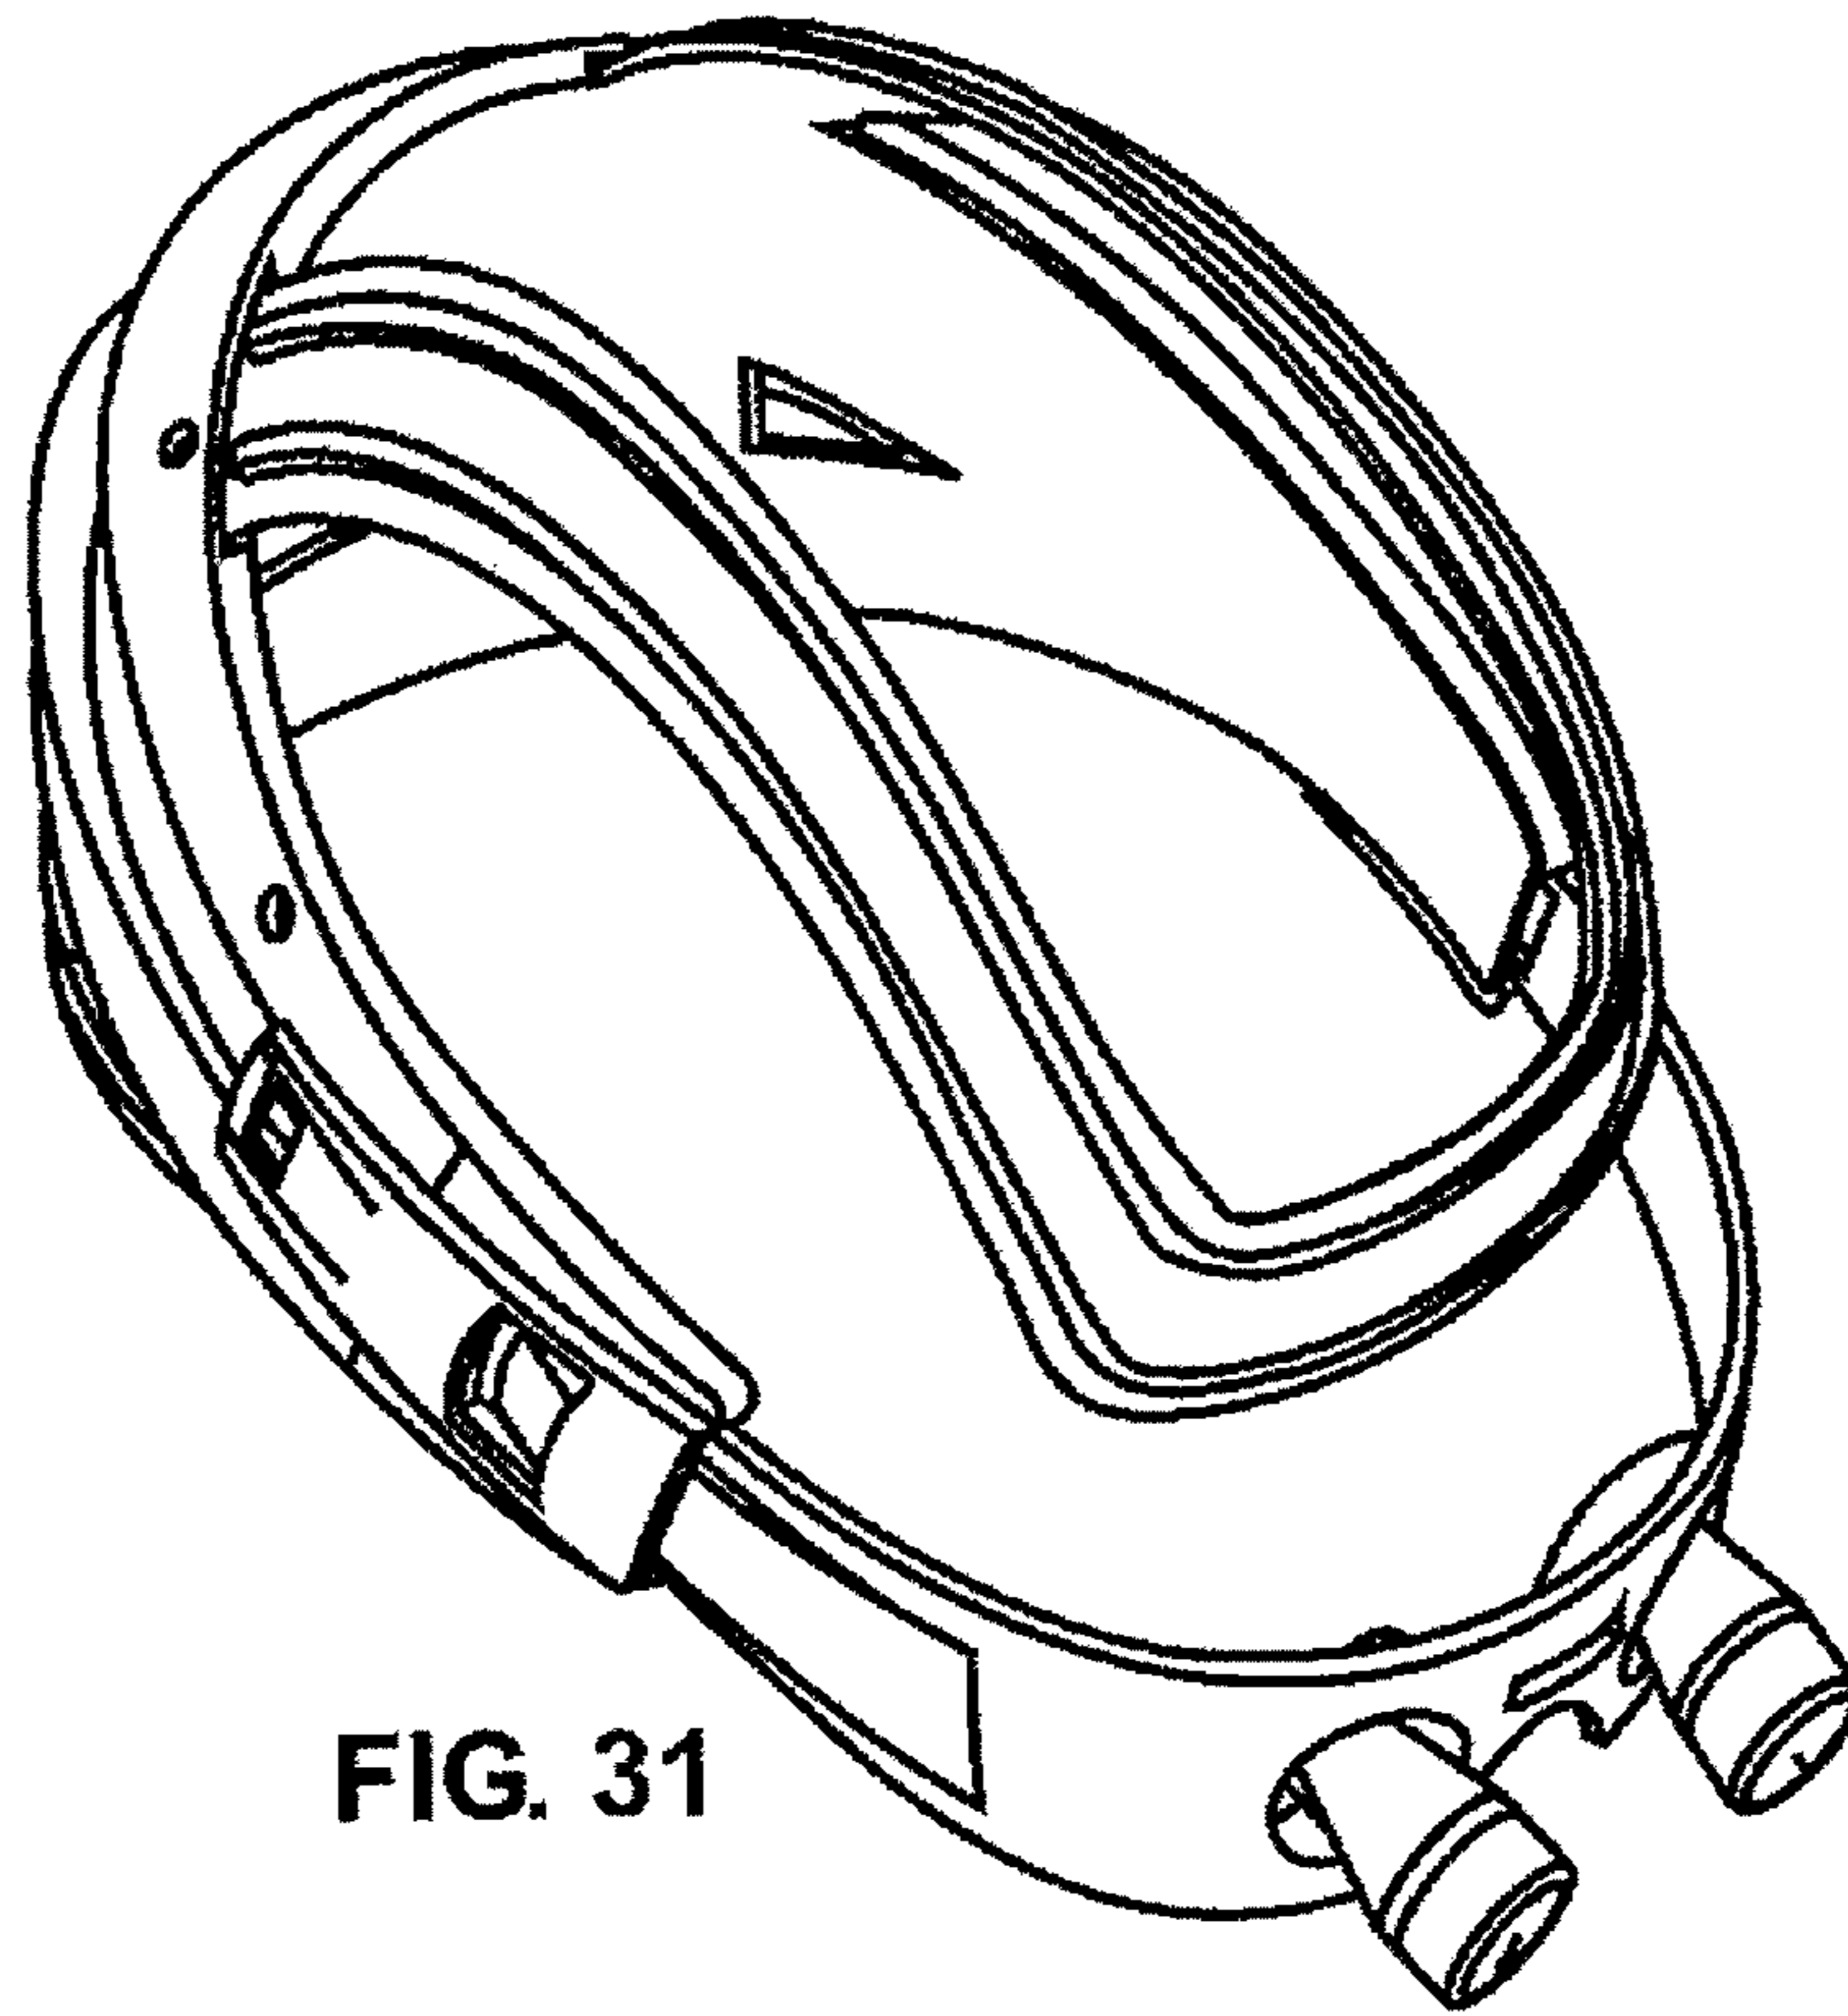


FIG. 31

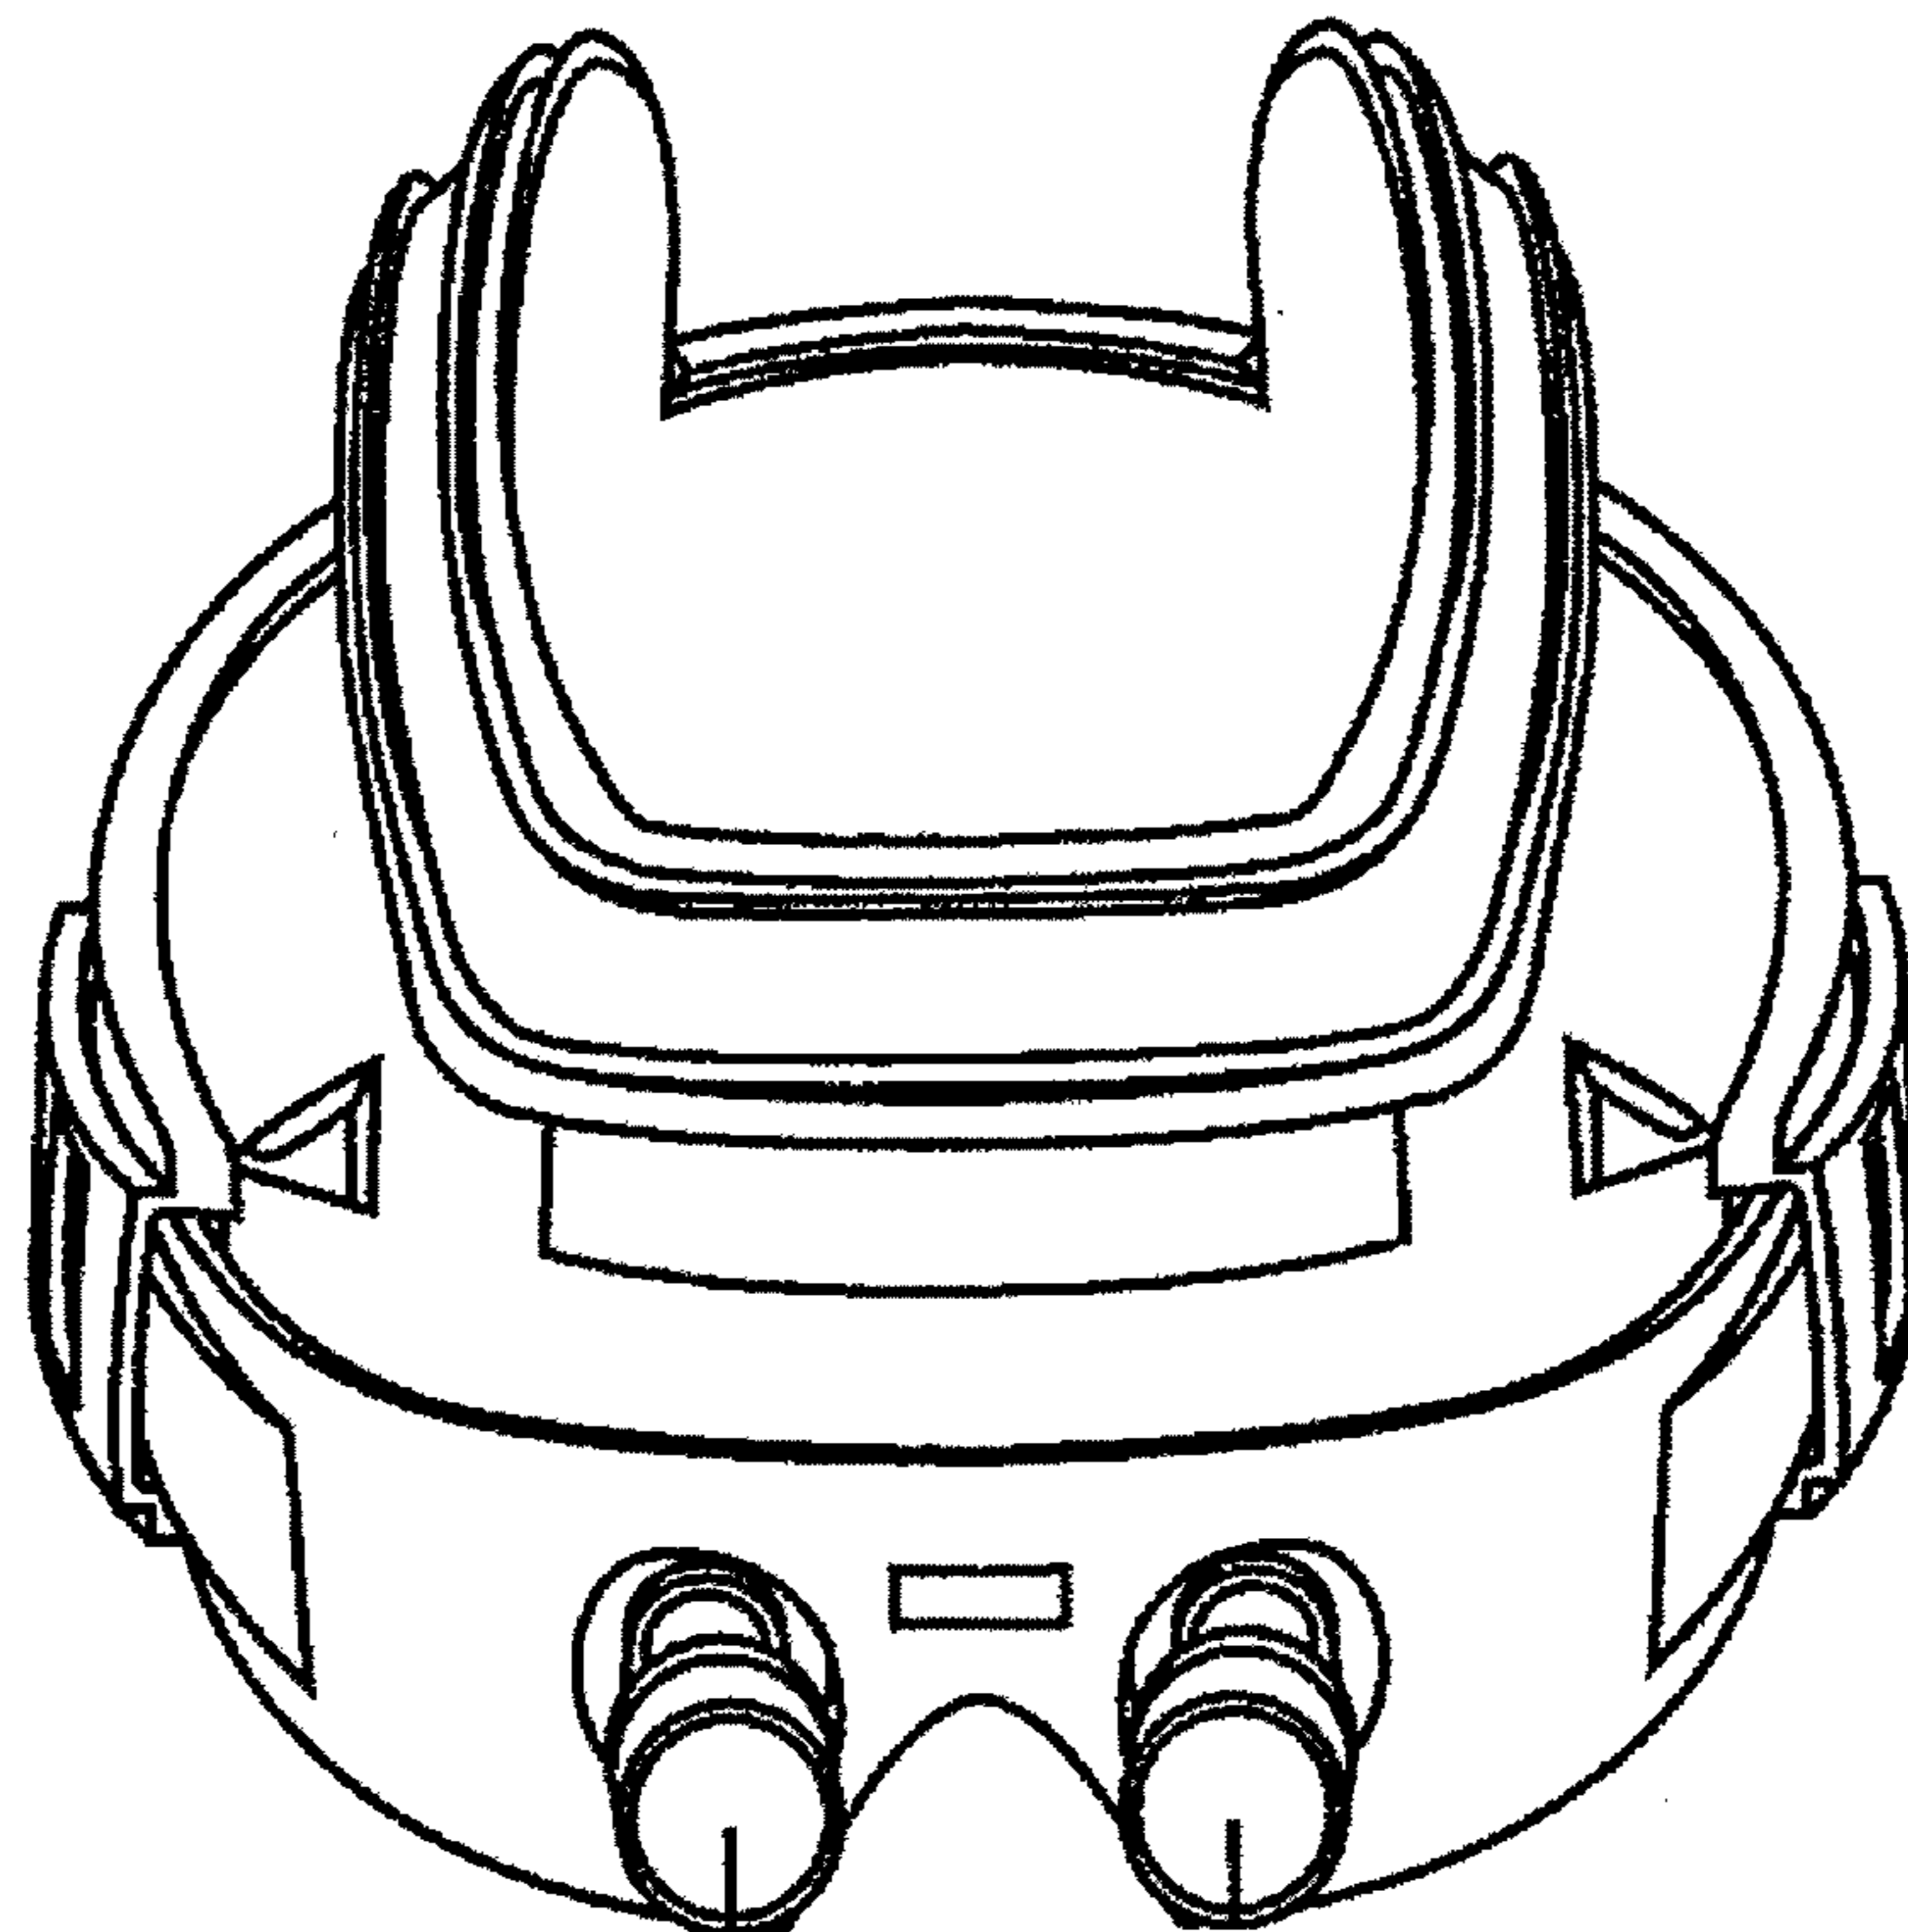


FIG. 32

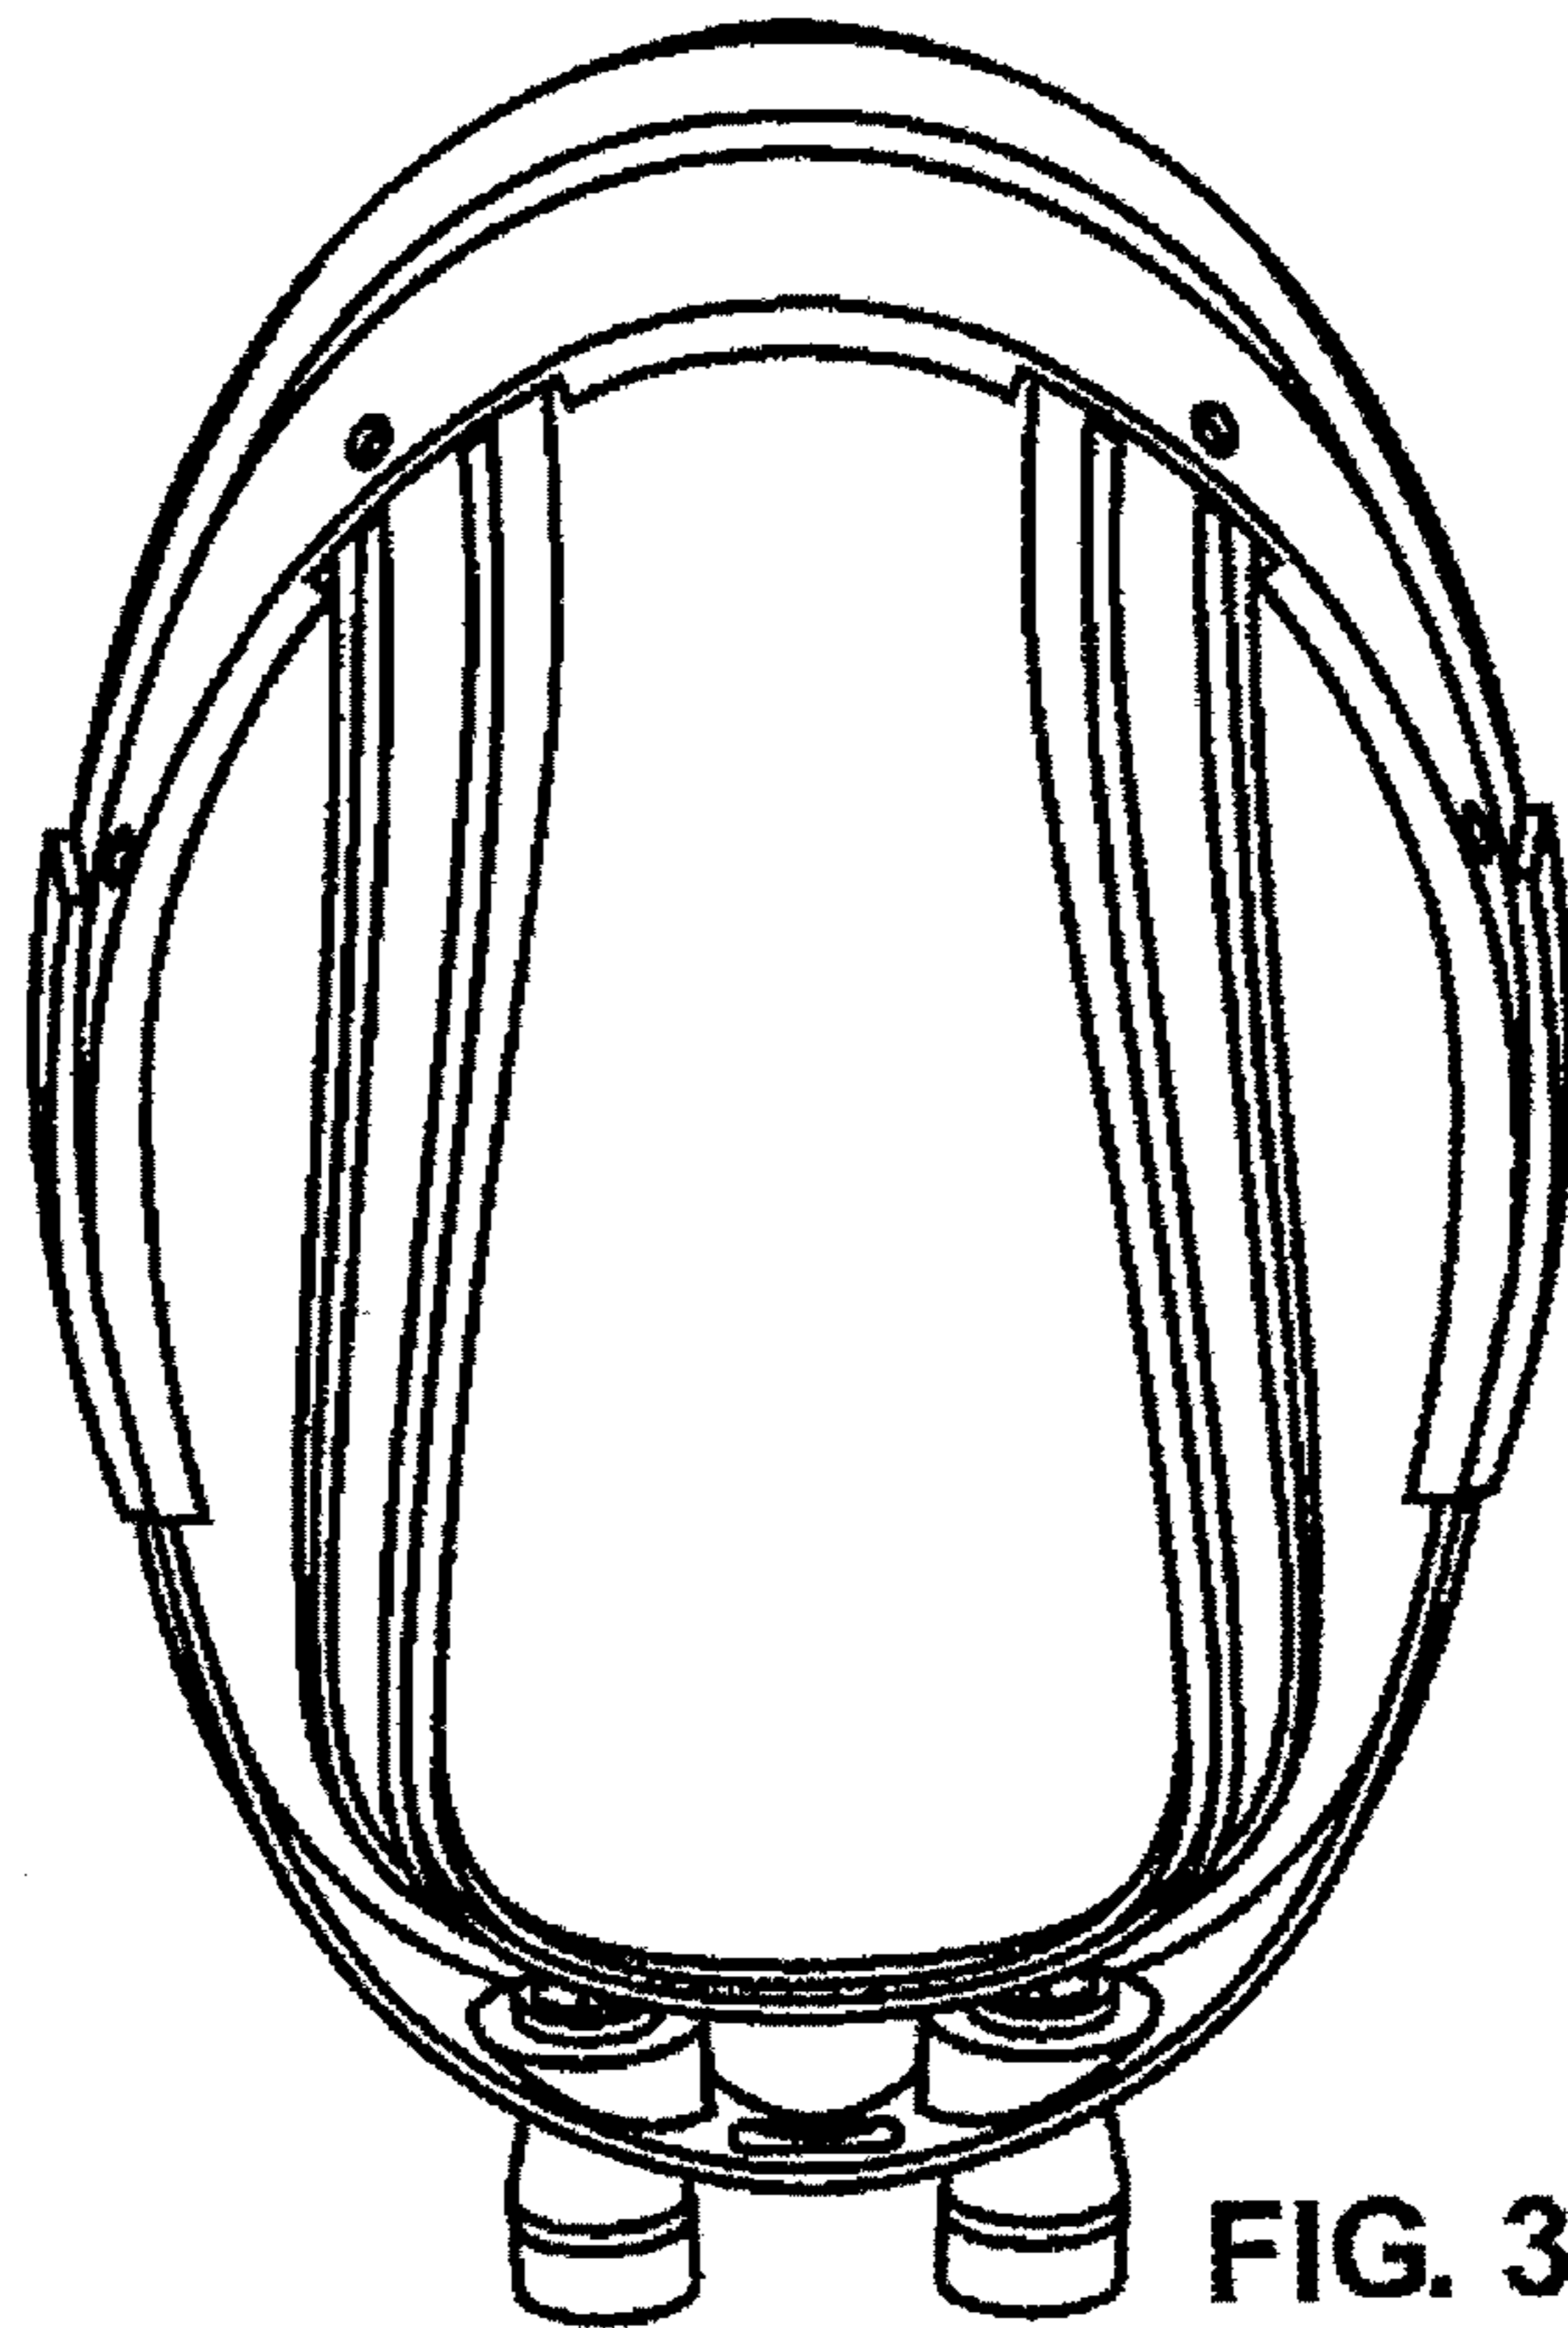


FIG. 33

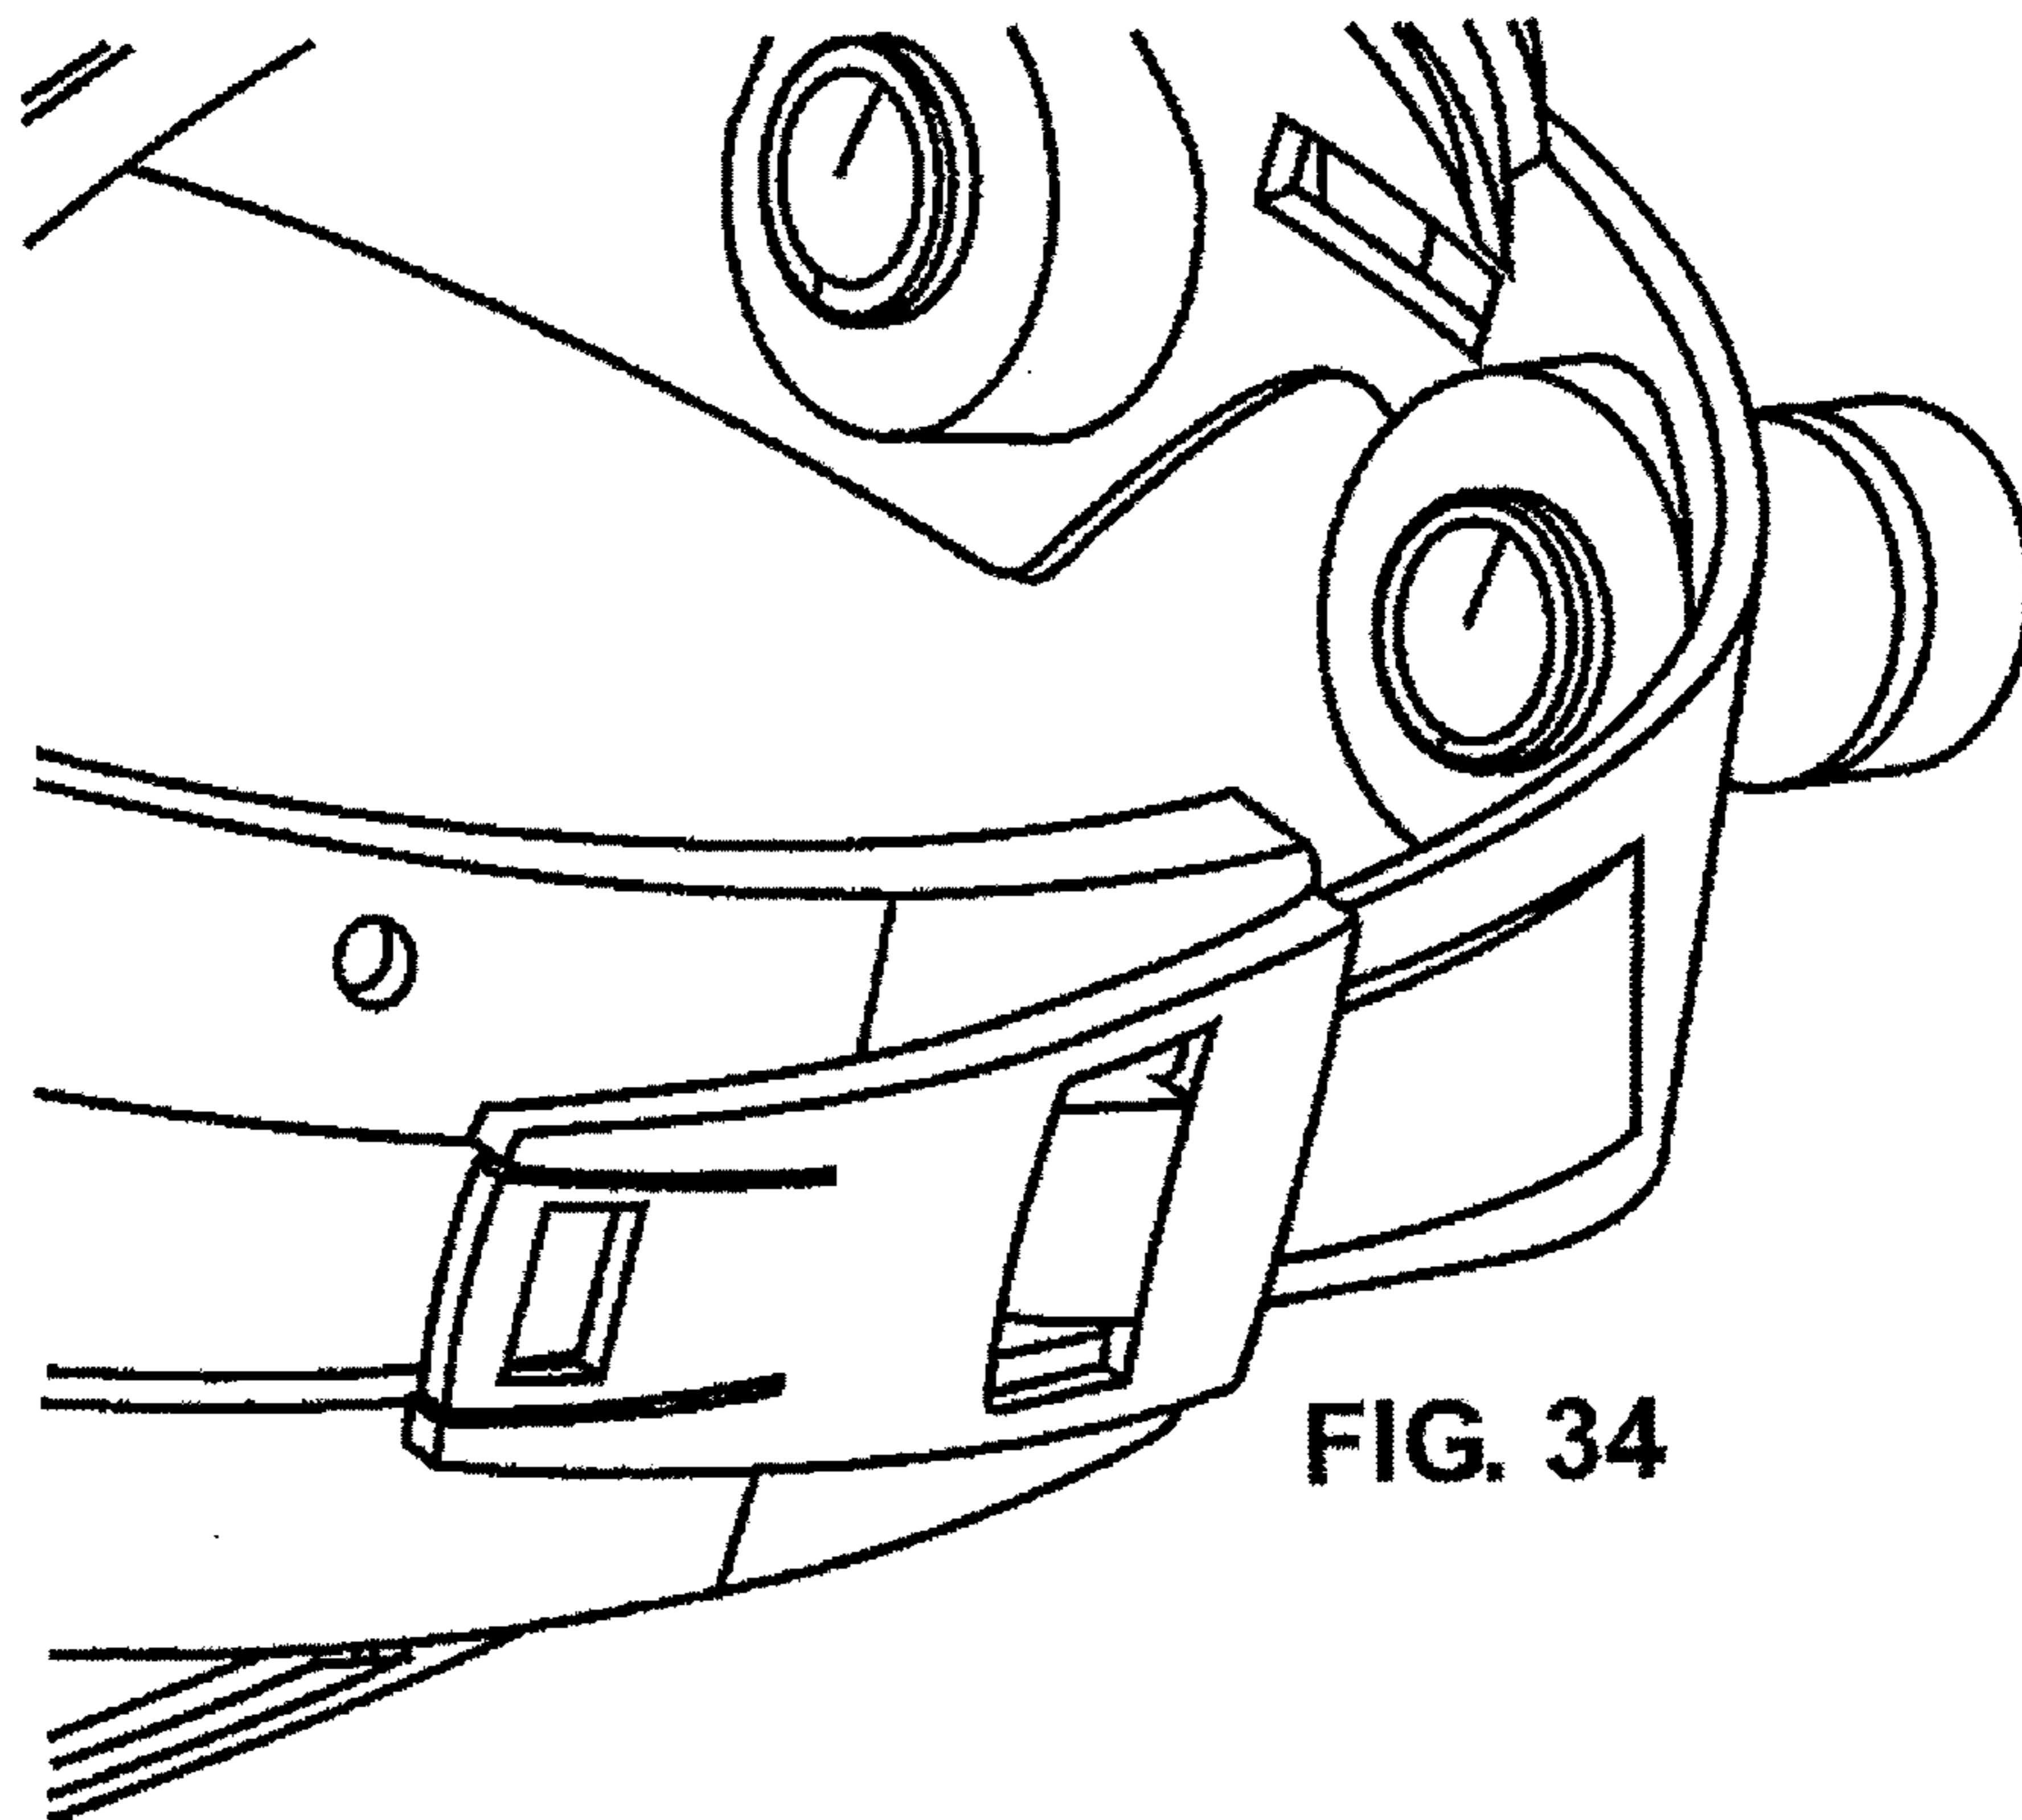


FIG. 34

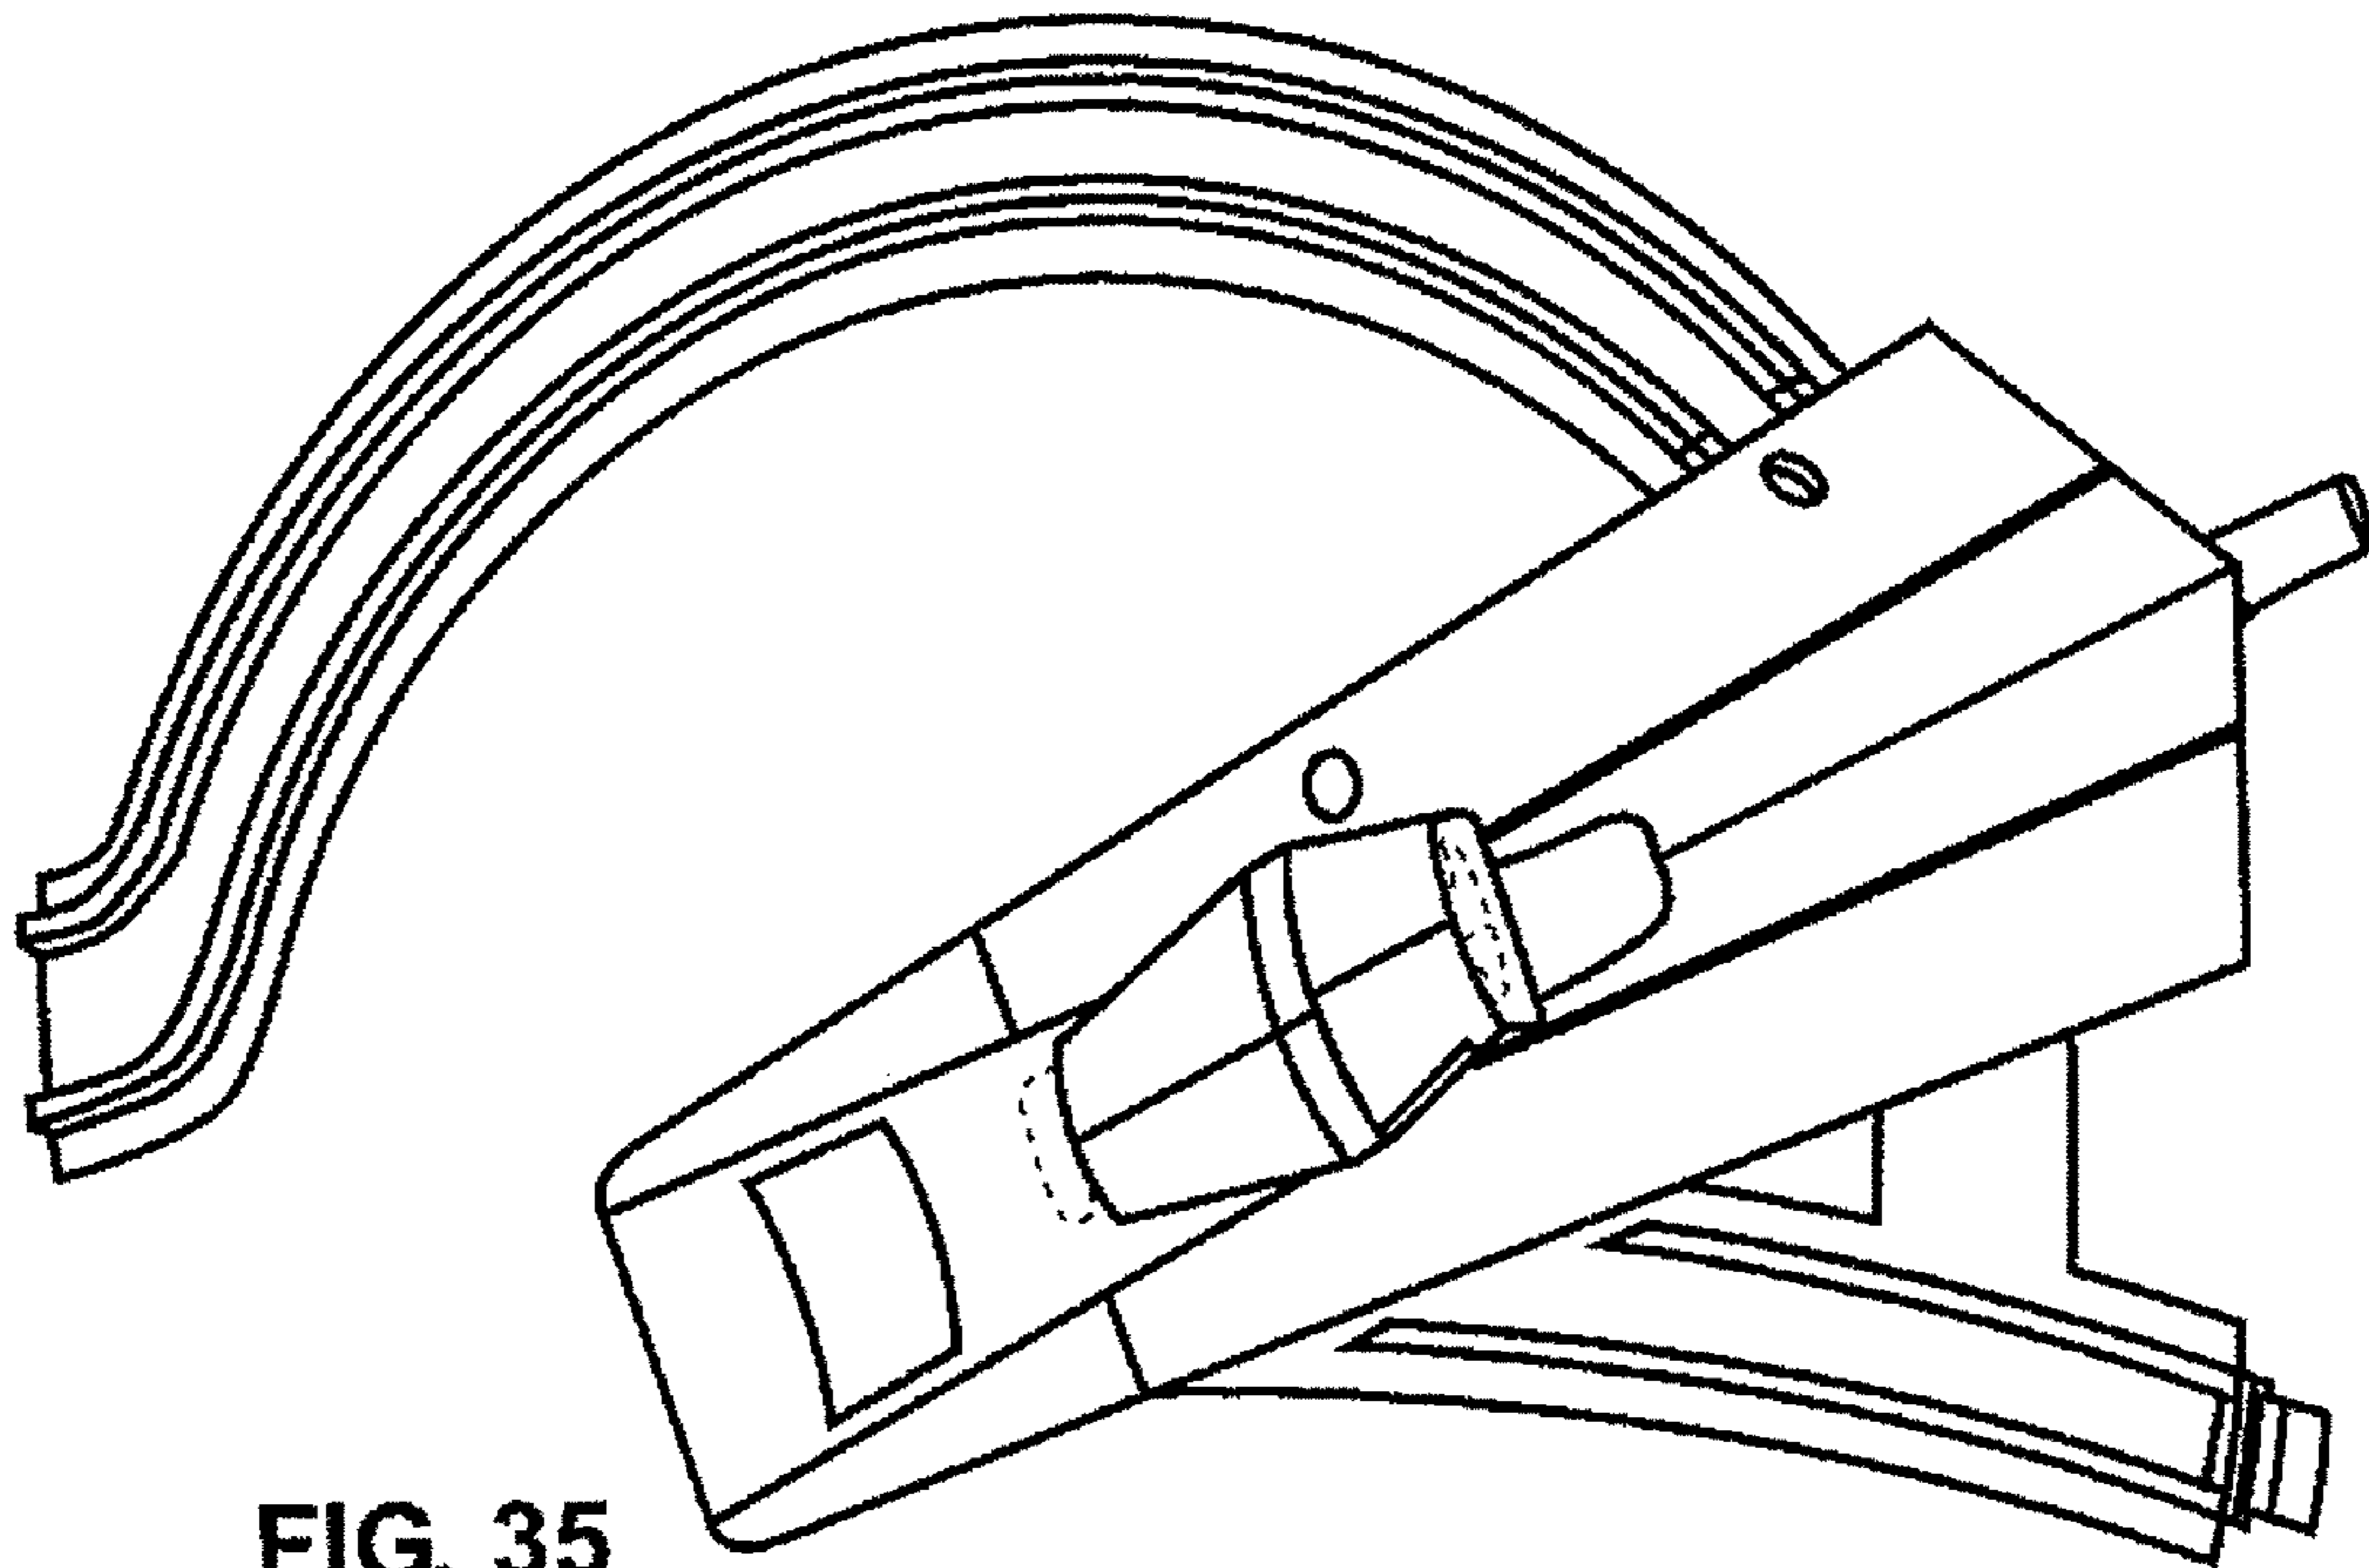


FIG. 35

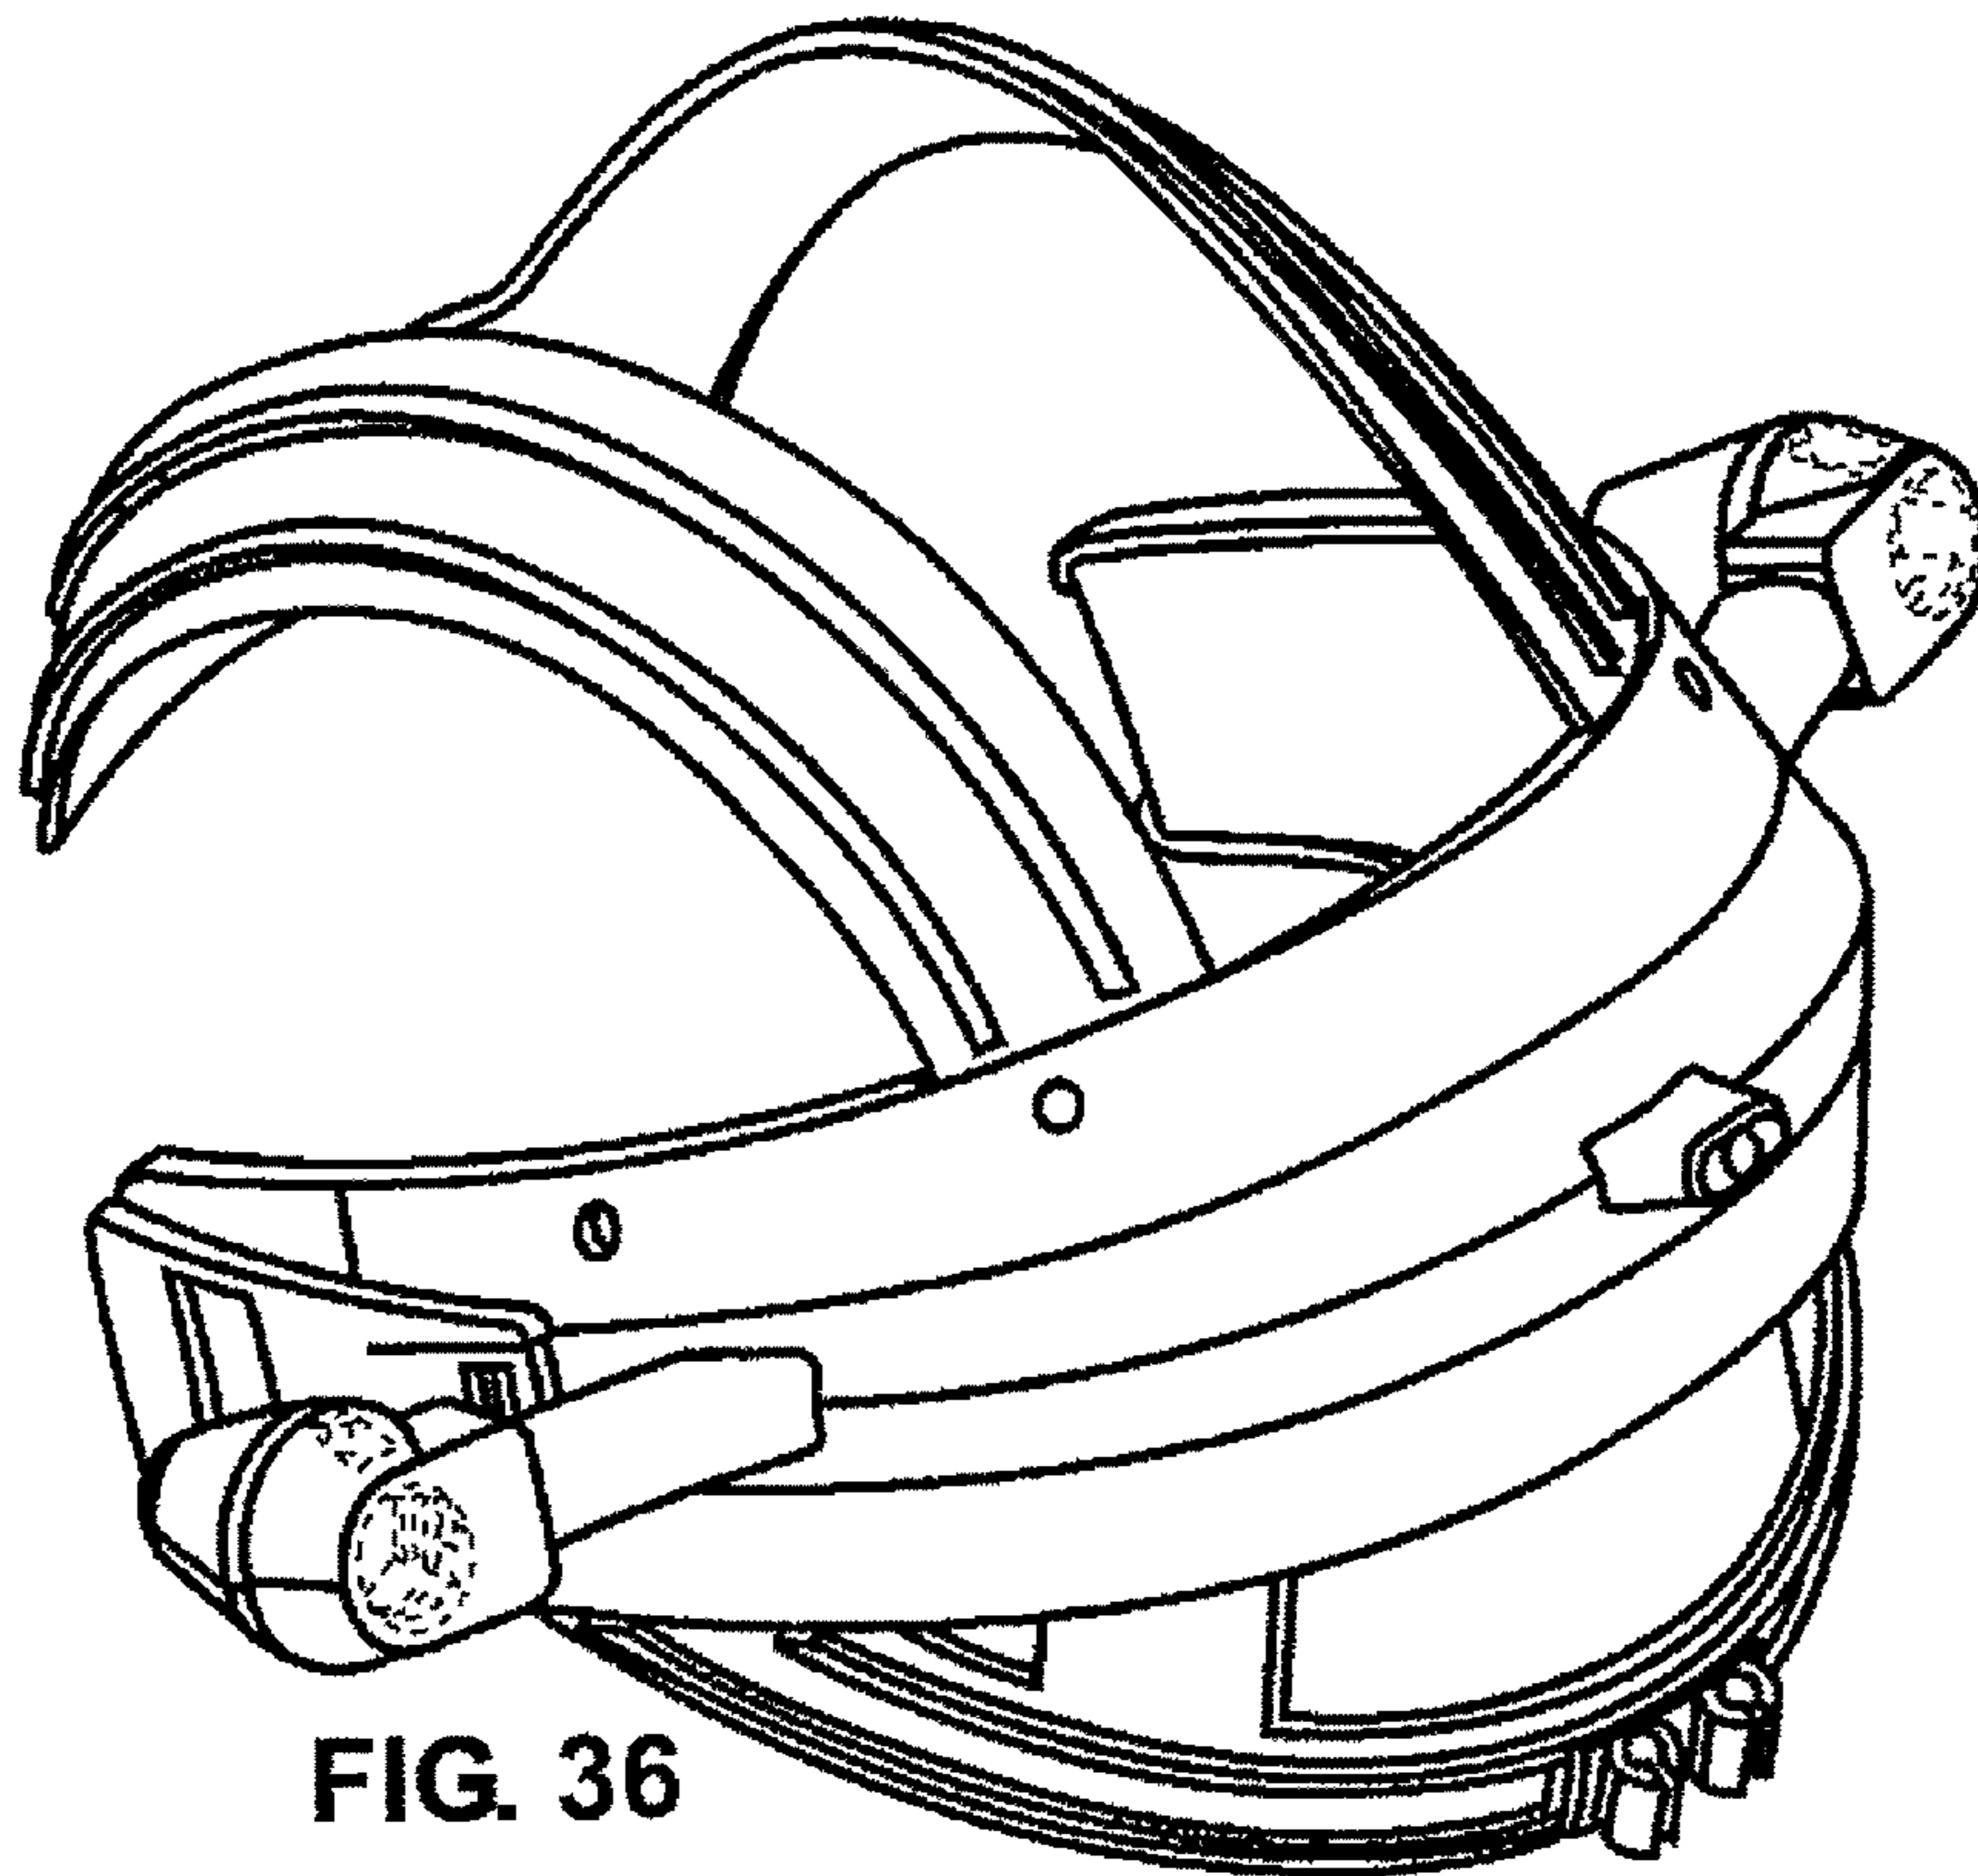


FIG. 36

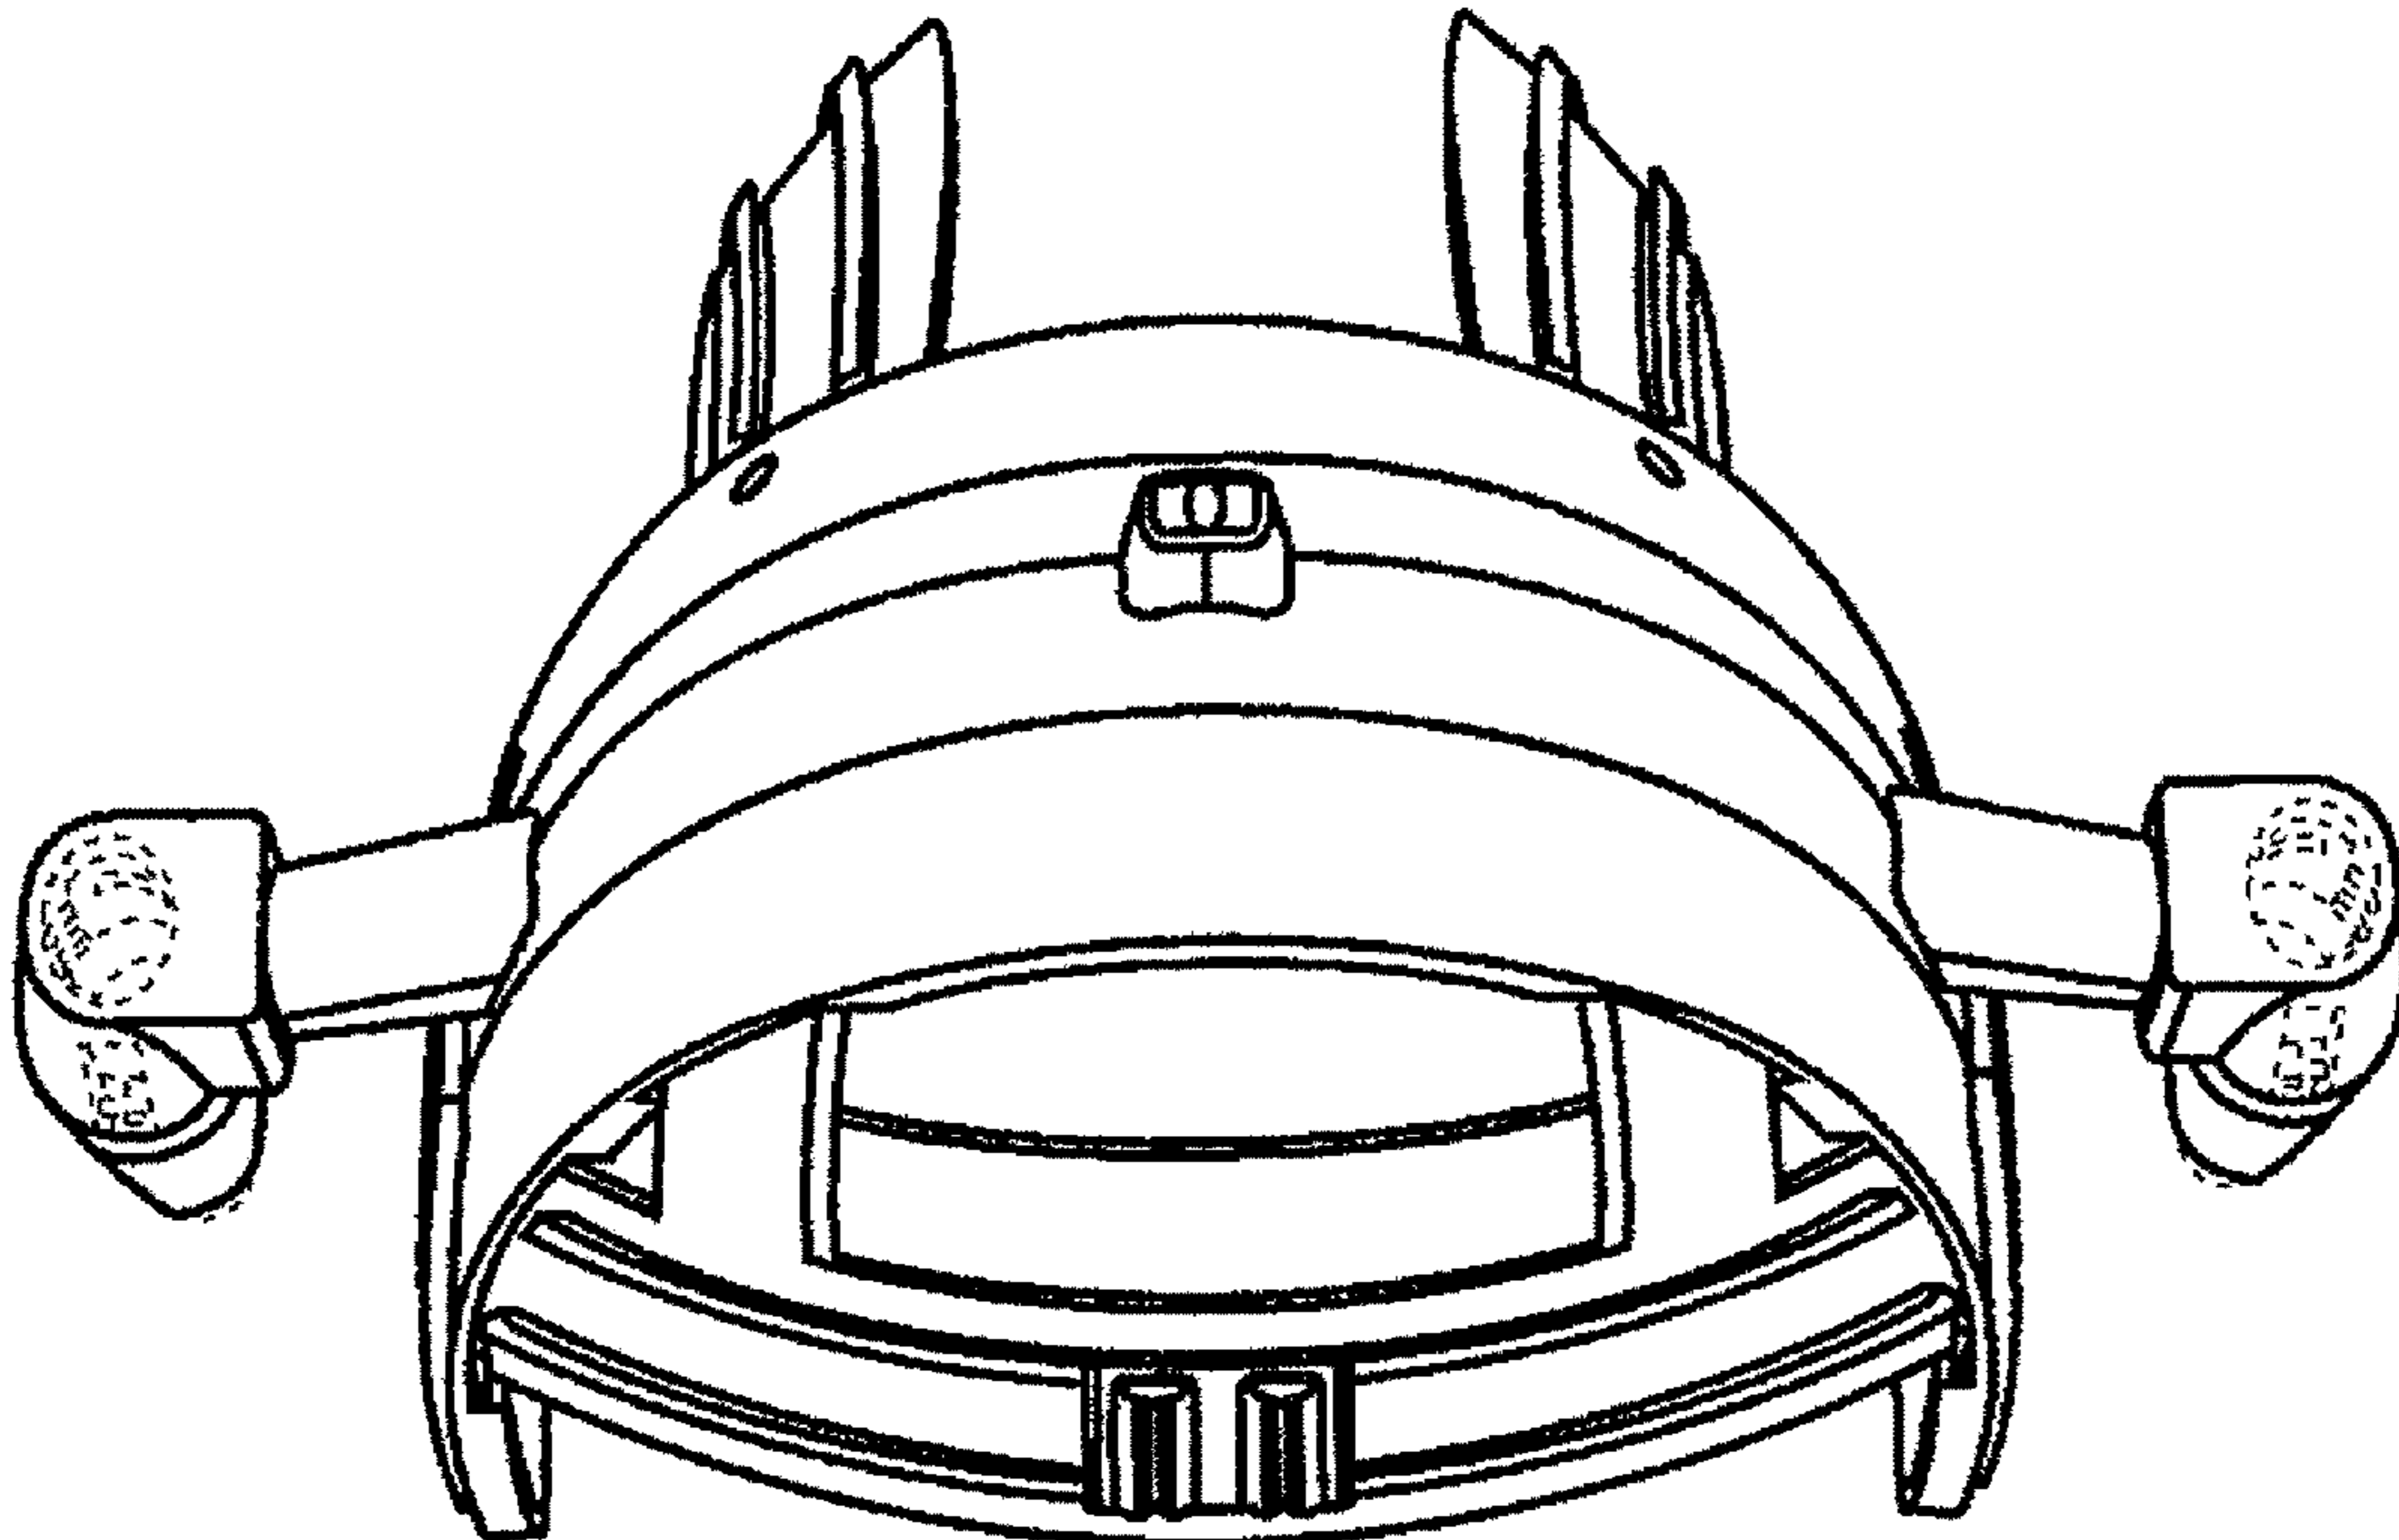


FIG. 37

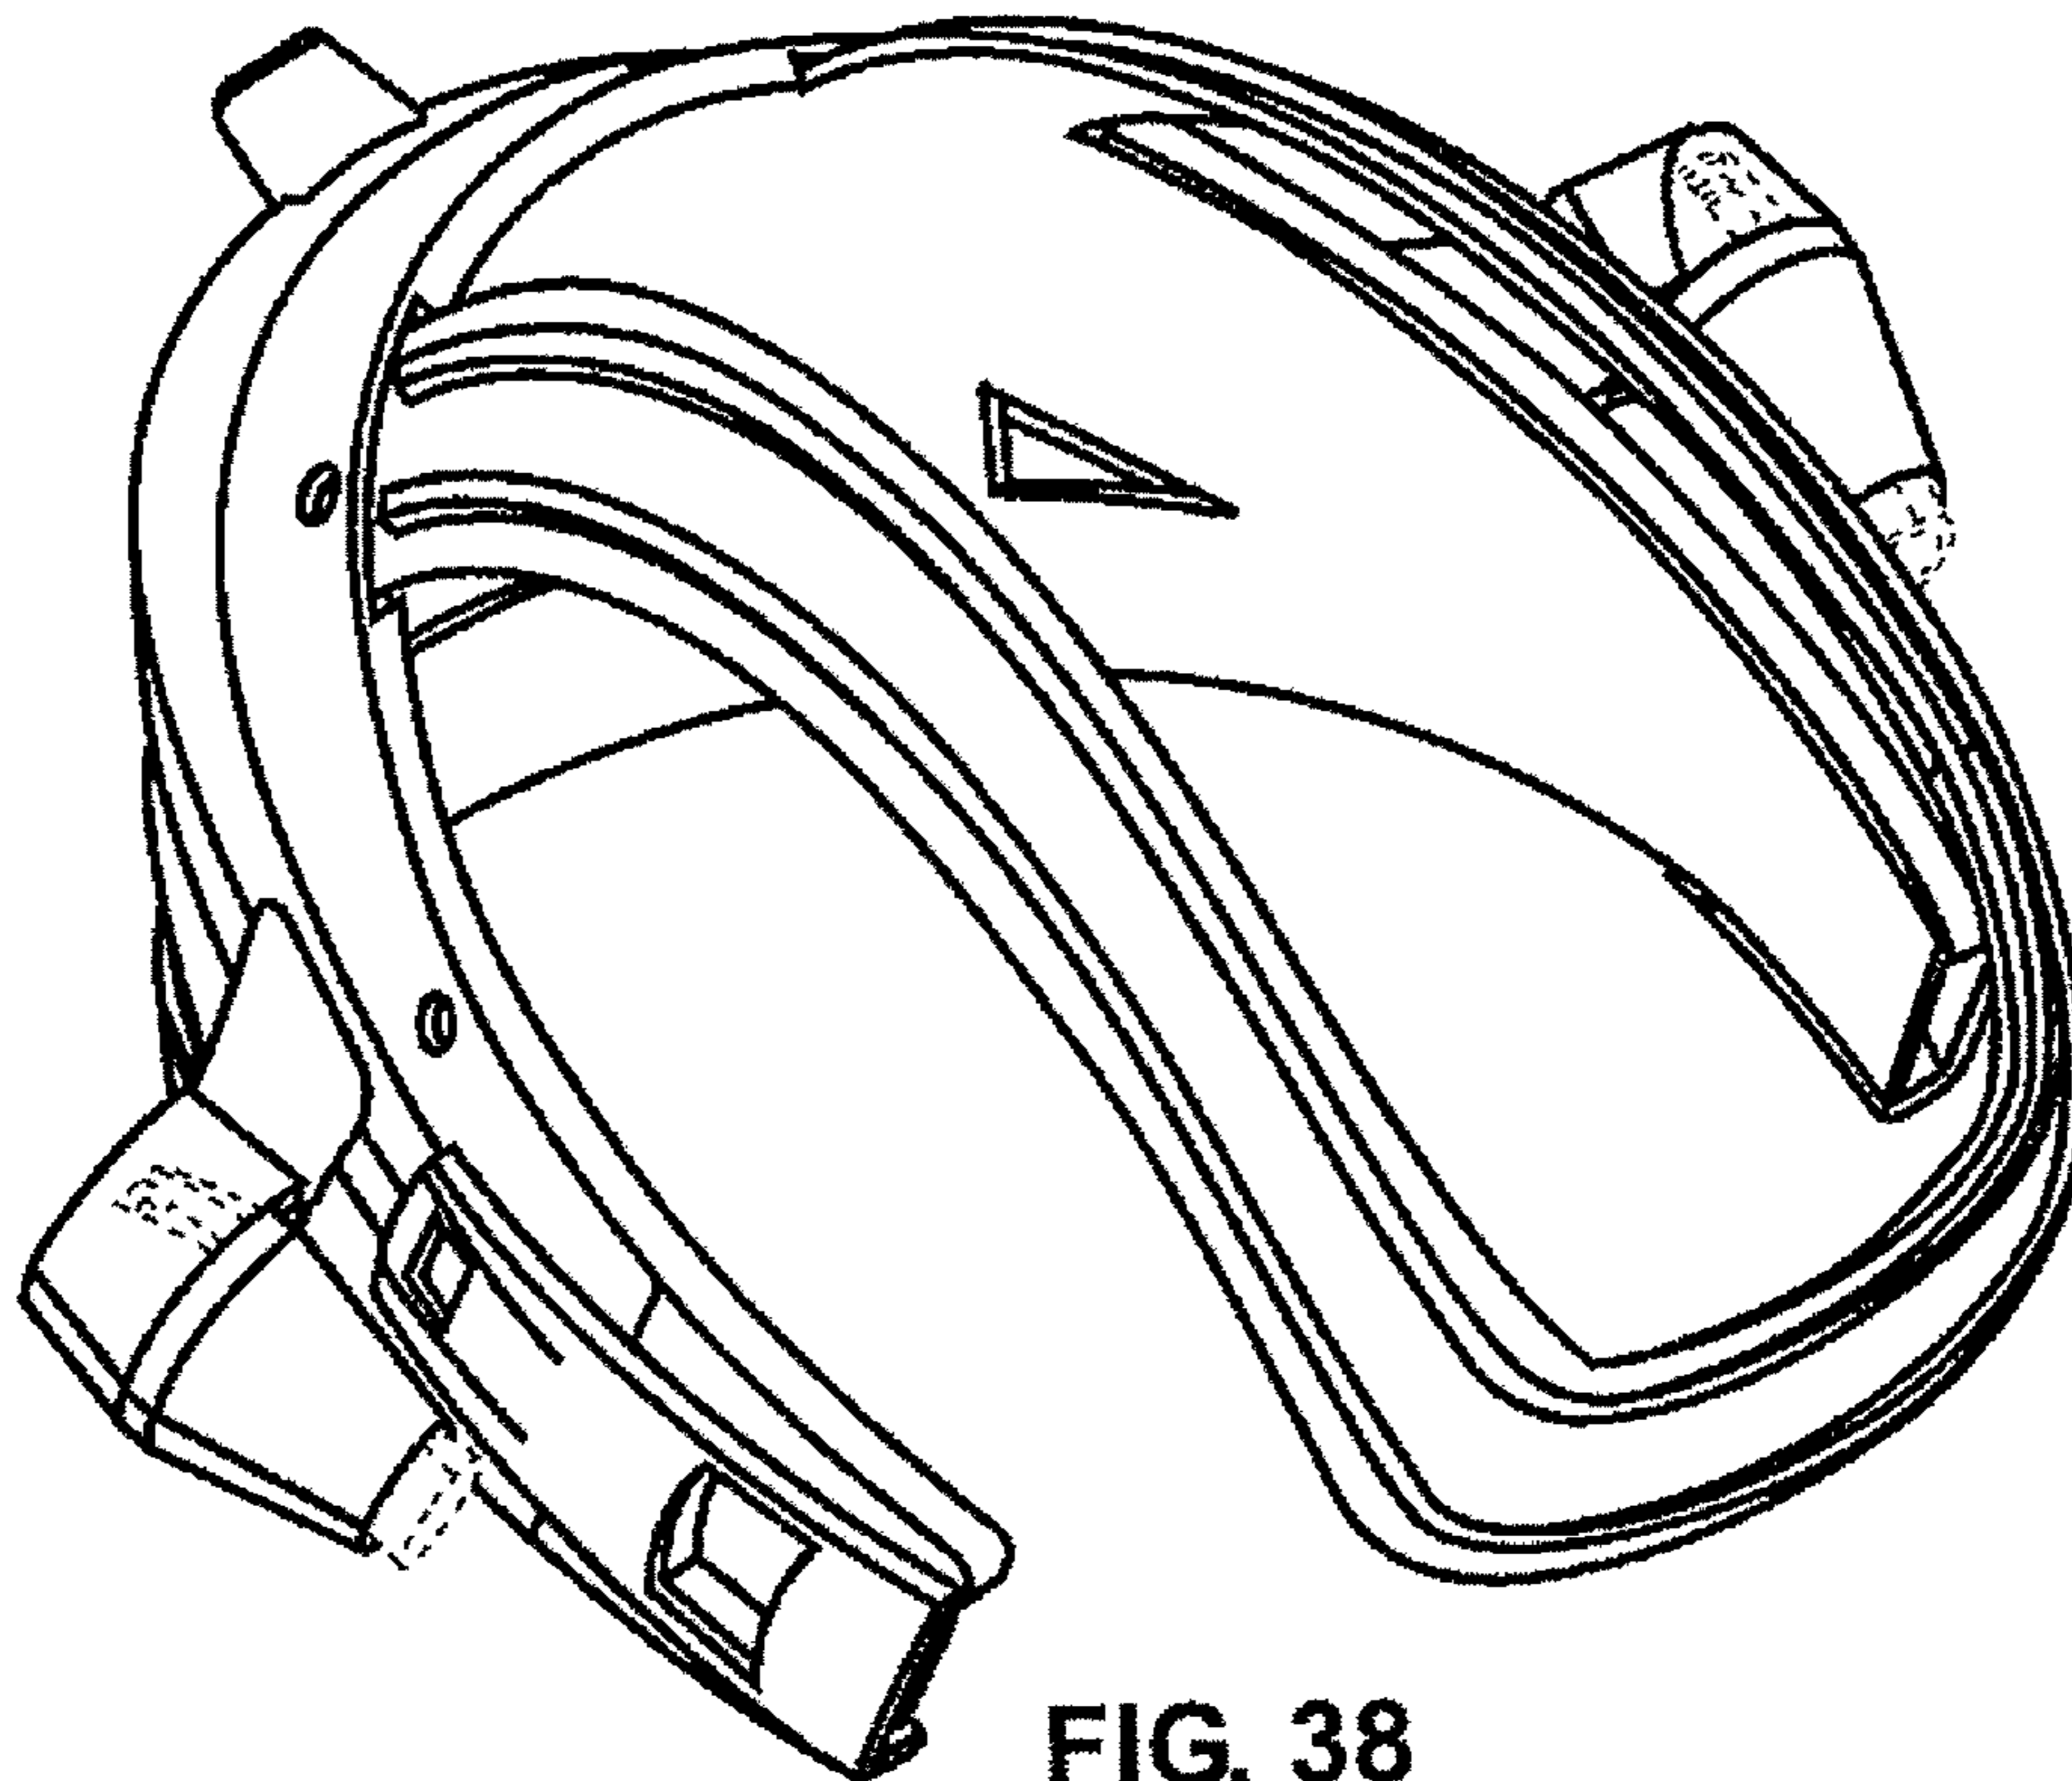


FIG. 38

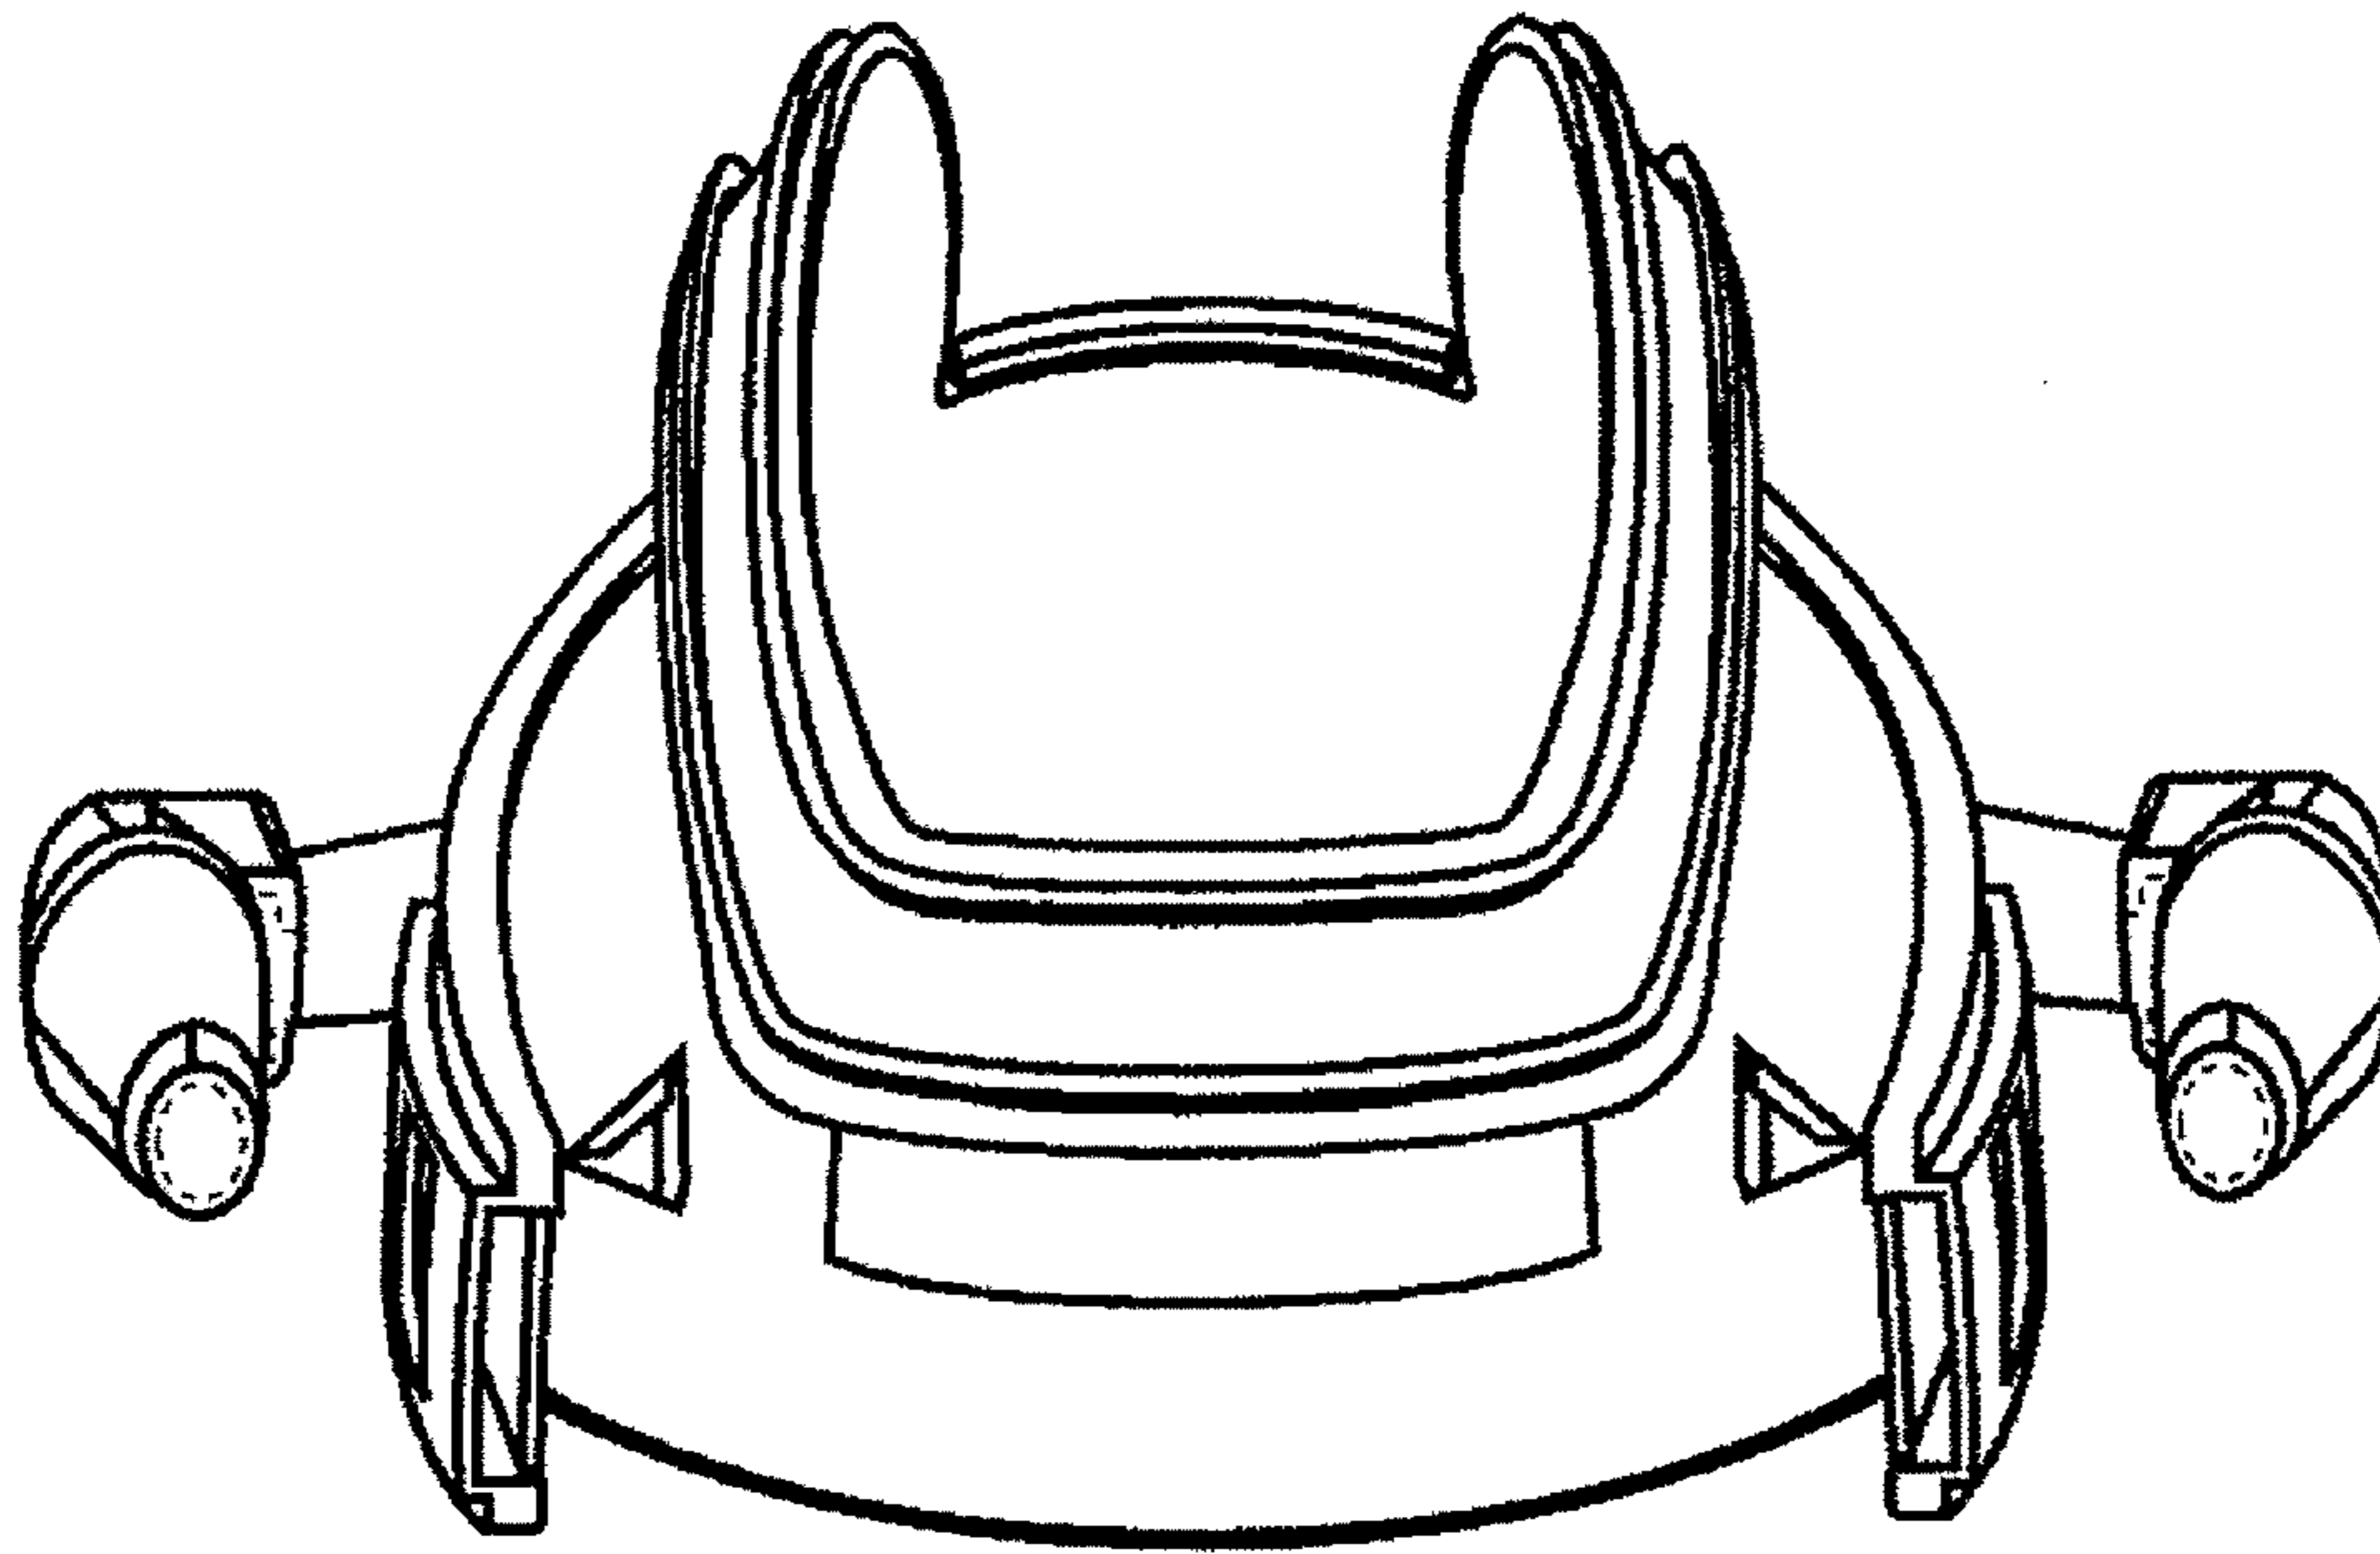


FIG. 39

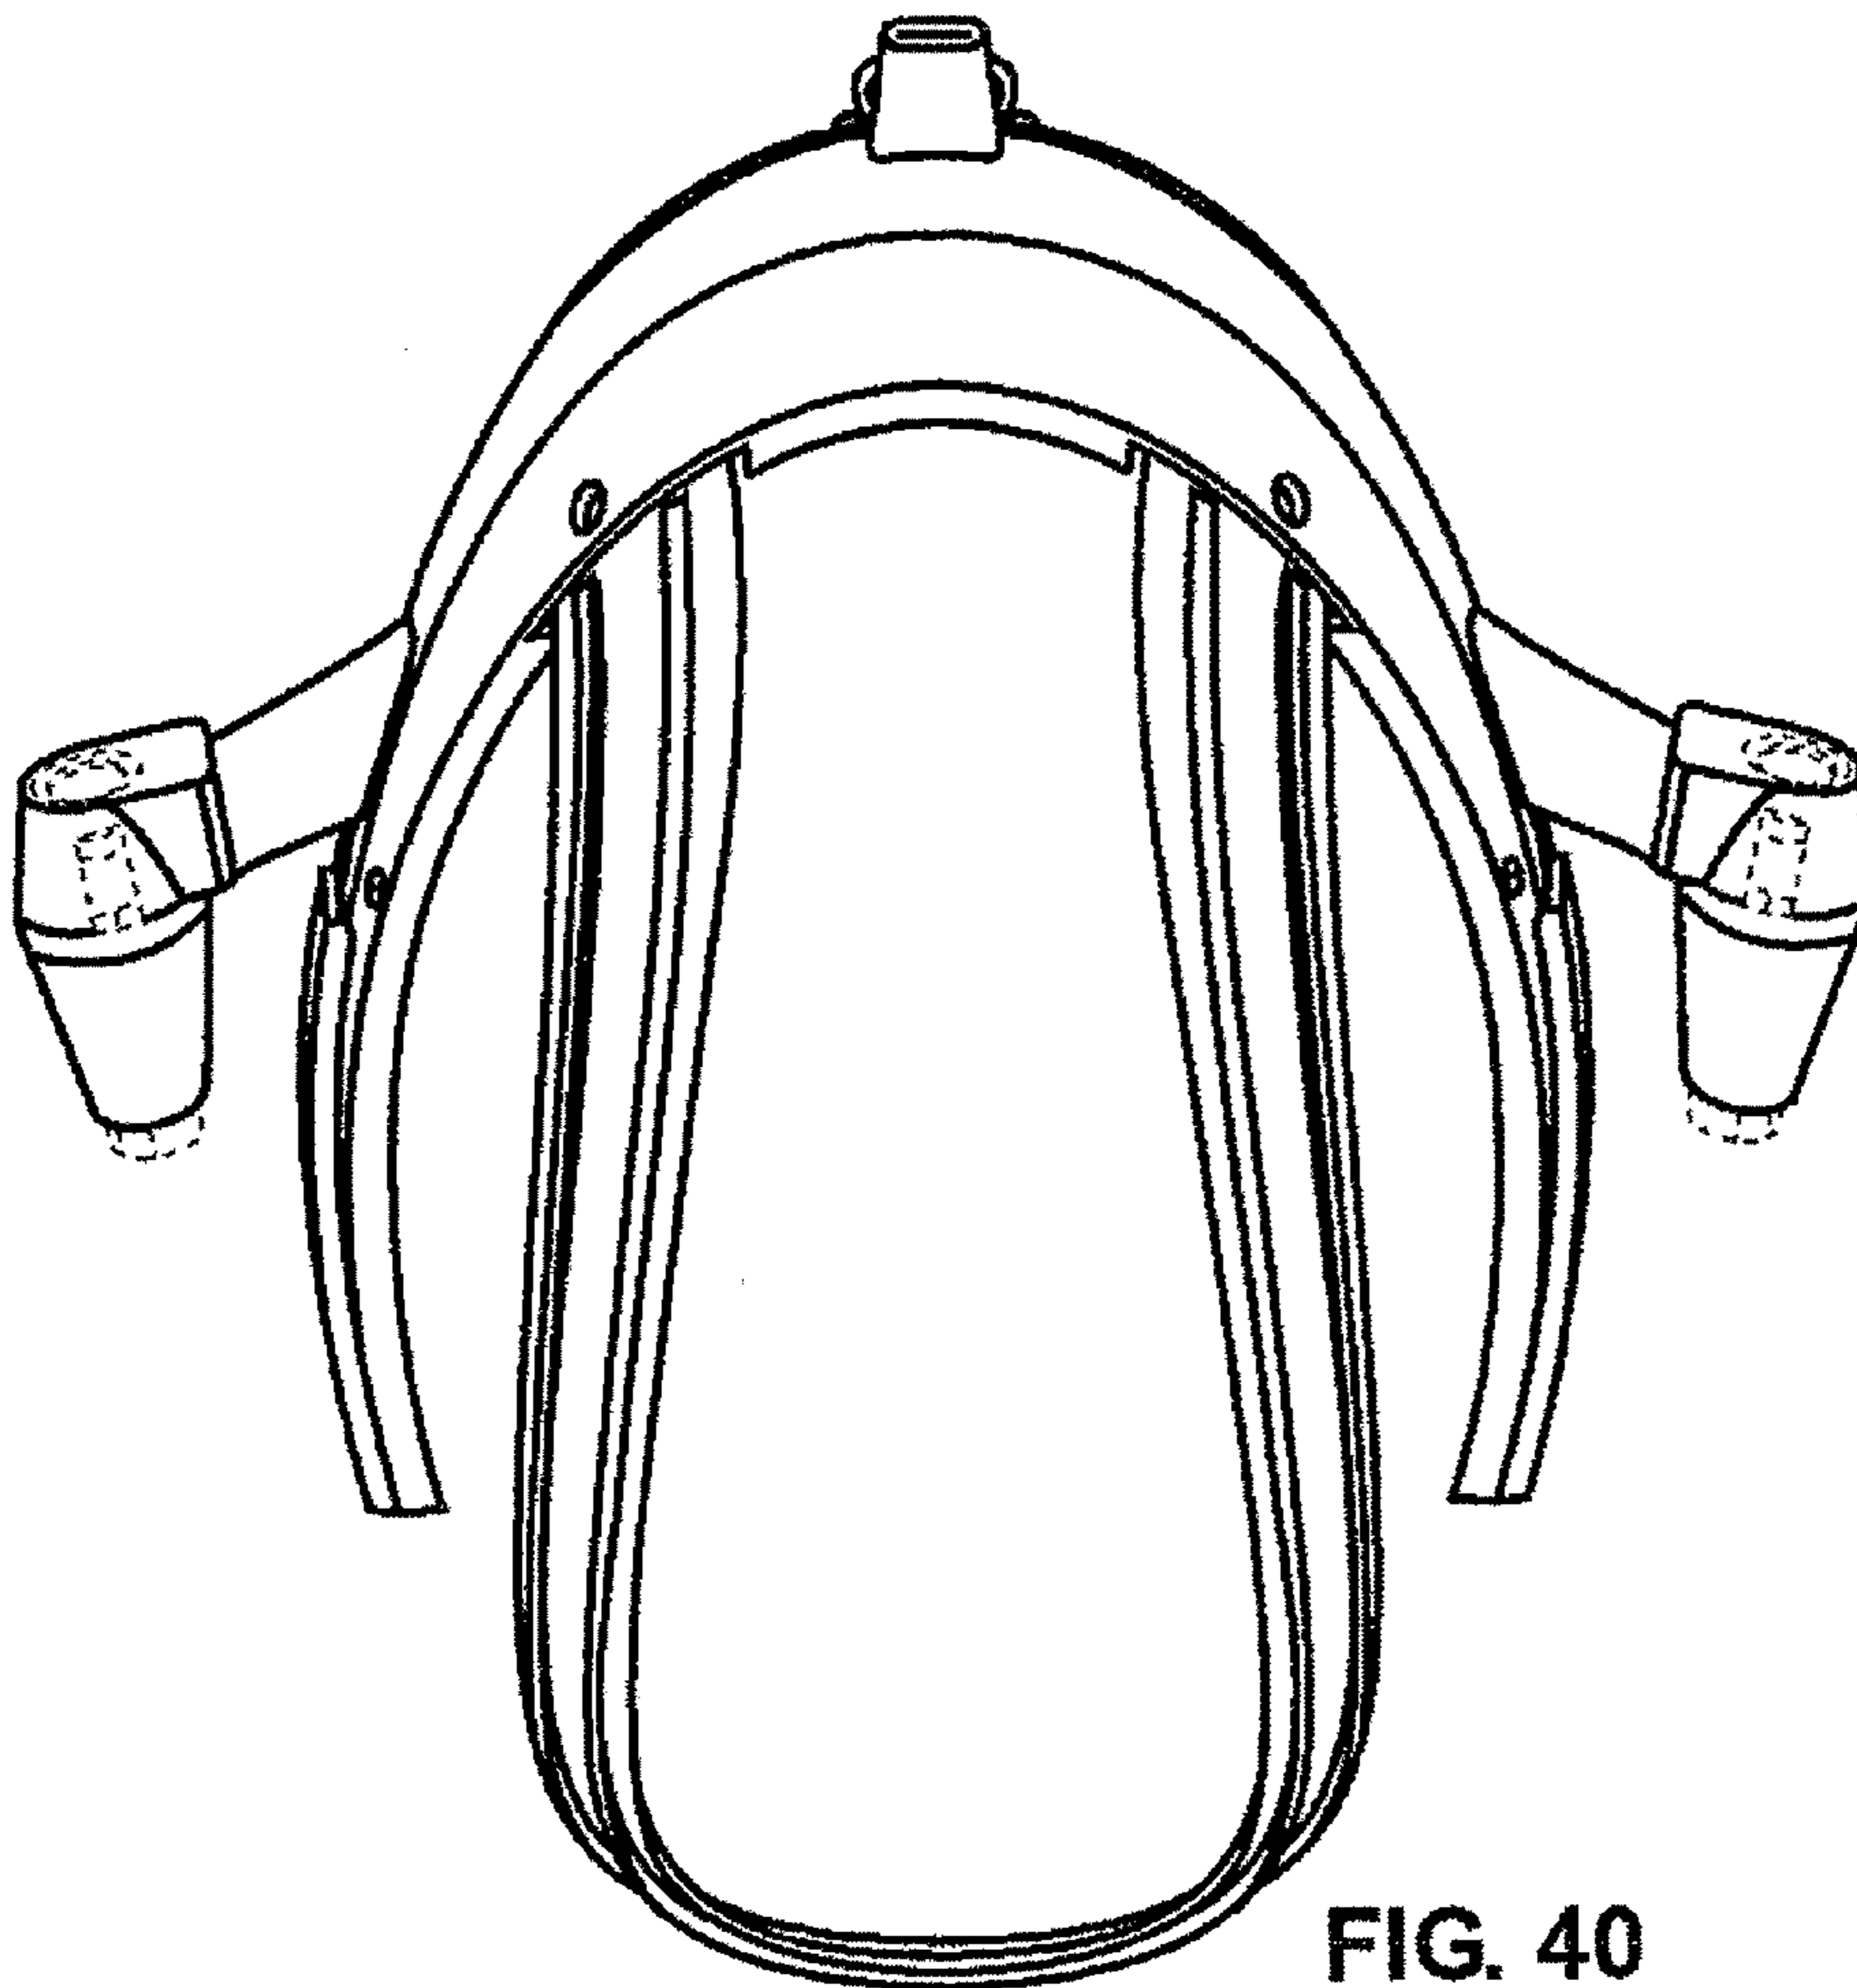


FIG. 40

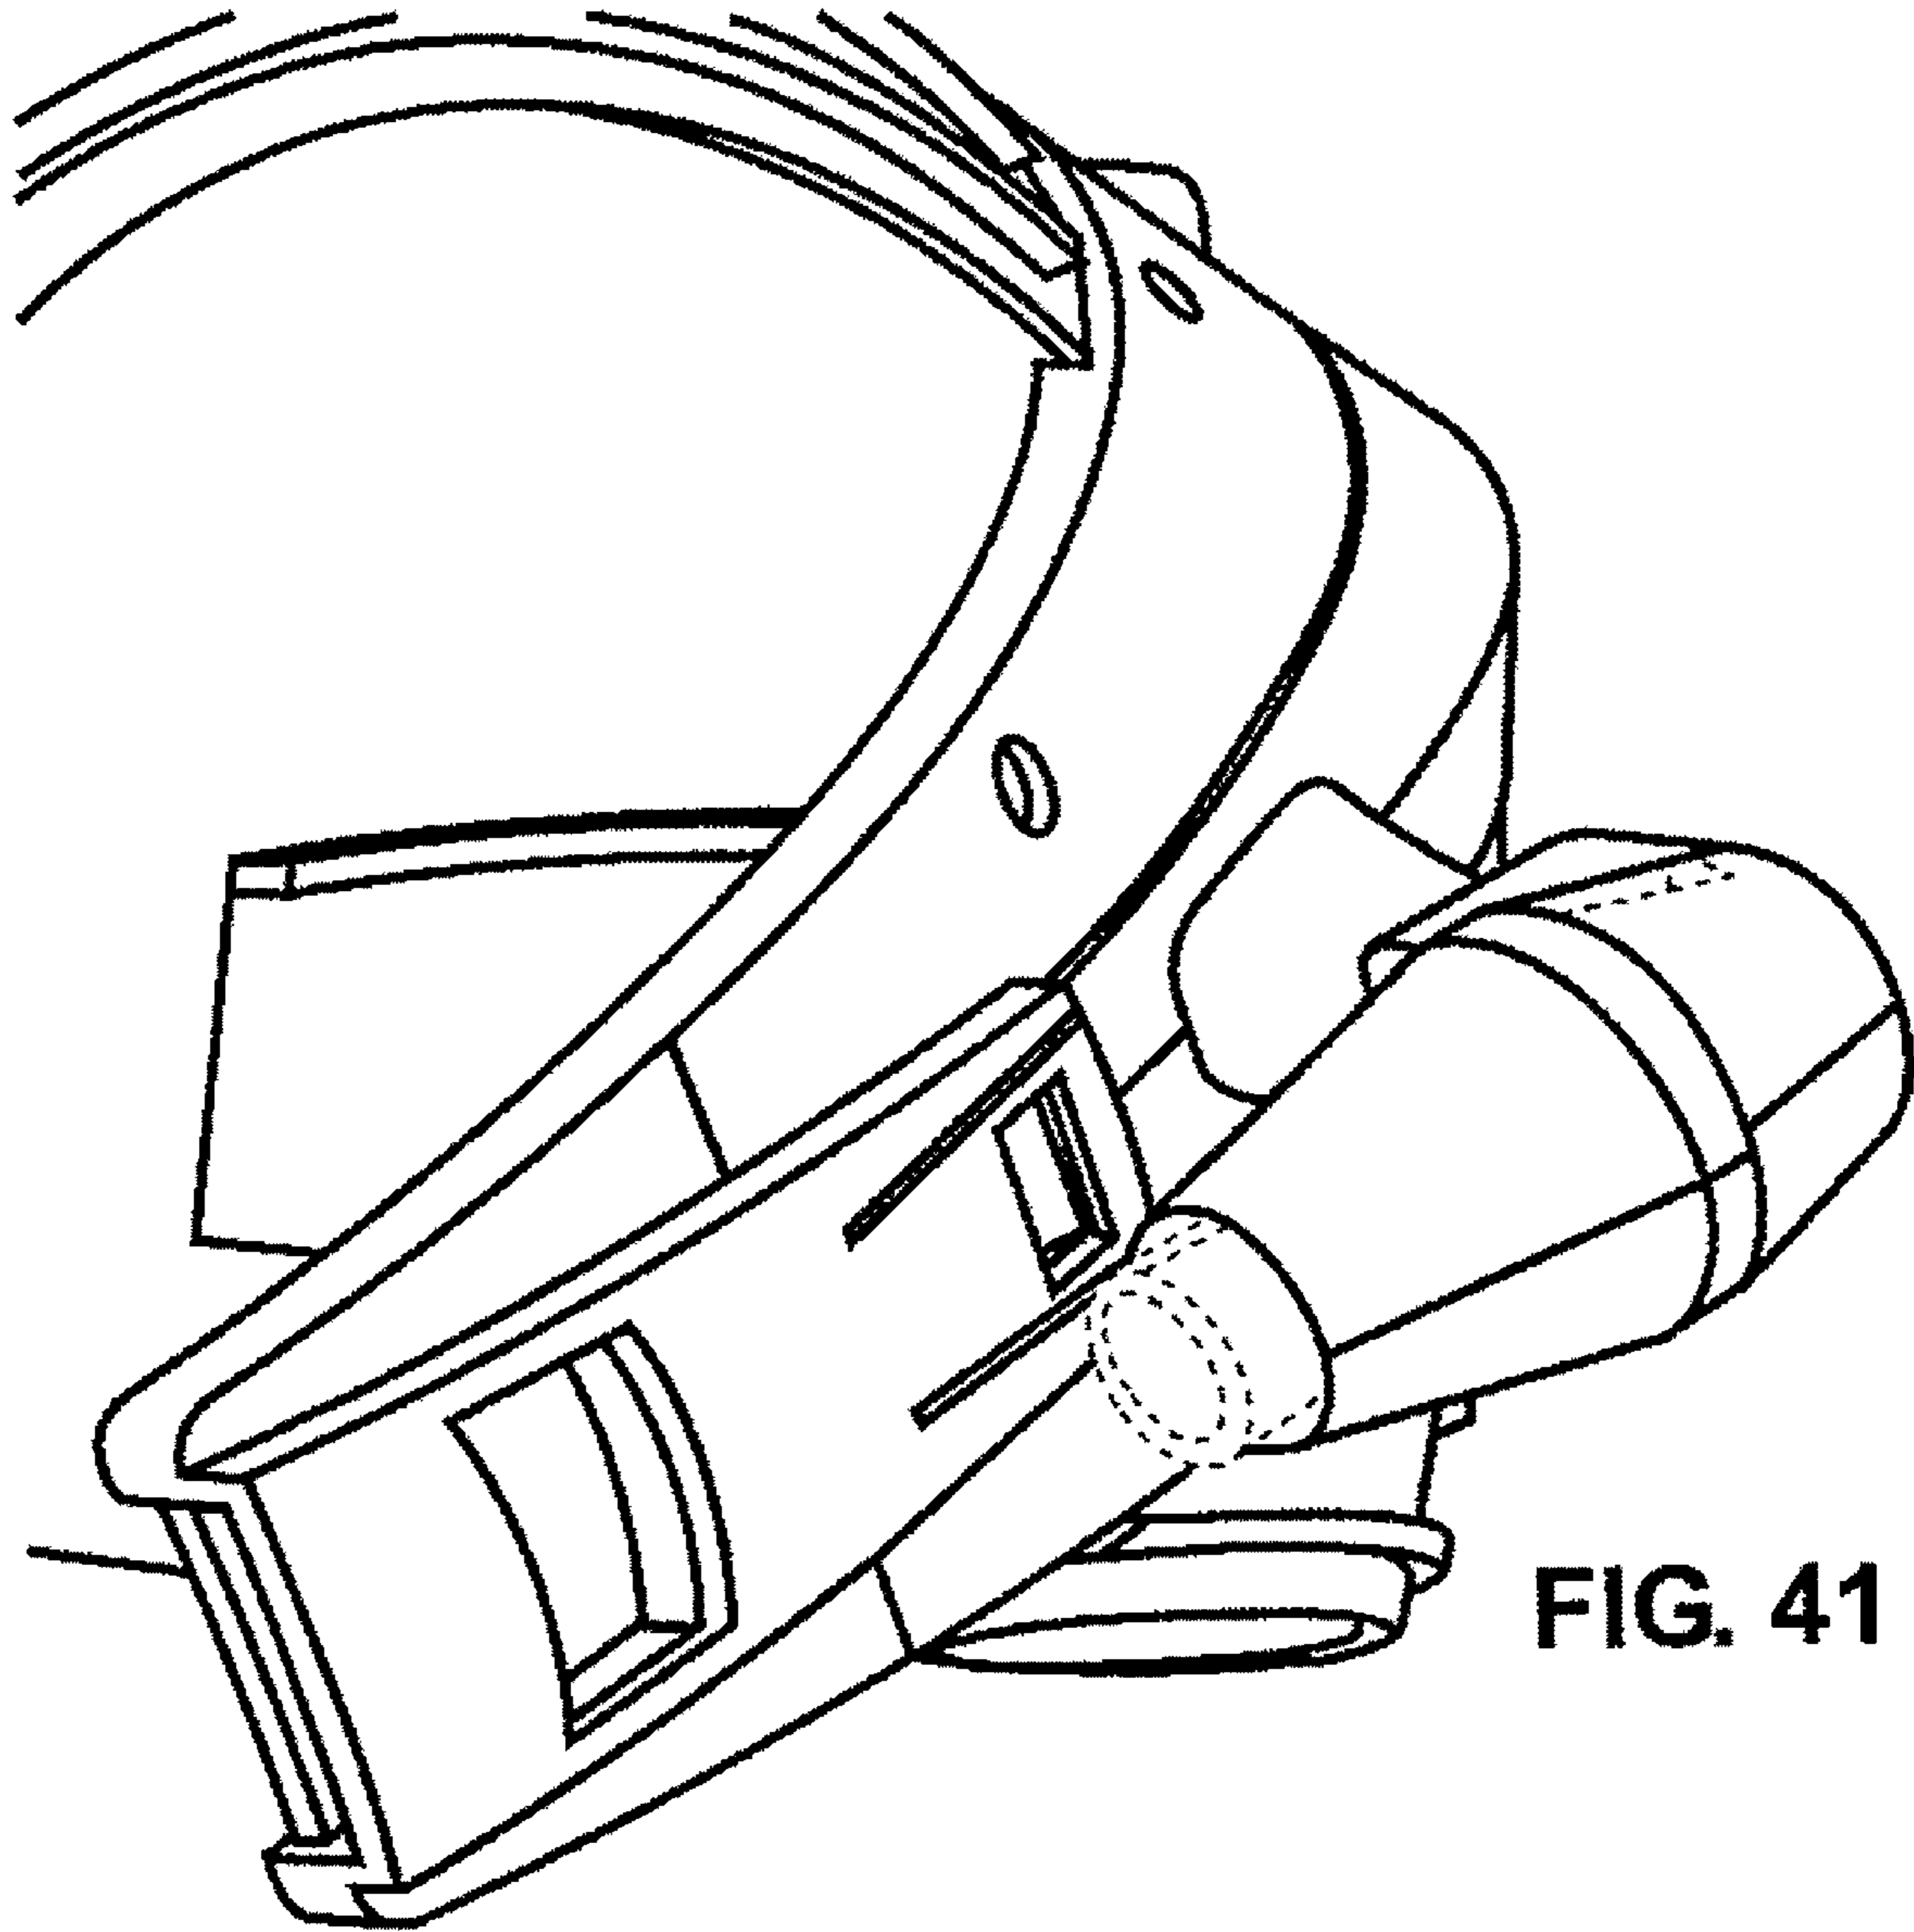


FIG. 41