



US00D631165S

(12) **United States Design Patent**
Fisher et al.

(10) **Patent No.:** **US D631,165 S**
(45) **Date of Patent:** **** Jan. 18, 2011**

- (54) **ELECTRONIC READER FOR MEDICAL ENVIRONMENTS**
- (75) Inventors: **Stanley Fisher**, Durham, NC (US);
Stephen S. Jackson, Chapel Hill, NC (US)
- (73) Assignee: **RadarFind Corporation**, Morrisville, NC (US)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/359,700**
- (22) Filed: **Apr. 14, 2010**
- (51) **LOC (9) Cl.** **23-01**
- (52) **U.S. Cl.** **D24/186; D13/162**
- (58) **Field of Classification Search** D24/185–186;
D10/104, 106, 109, 40, 15; D13/158, 162,
D13/164, 165, 168, 170, 177, 160, 154, 137.1,
D13/137.2, 137.3, 137.4, 139.1, 139.2, 139.8;
340/573.4, 555–556, 600; 250/353, 349,
250/342, 370; 600/473; 439/105, 535; 174/66;
363/146

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D301,868 S * 6/1989 Schwartz D13/158
- D309,890 S * 8/1990 Cheng D13/168
- D310,063 S * 8/1990 Cheng D13/168
- D310,814 S * 9/1990 Rosenbaum et al. D13/158
- D314,368 S * 2/1991 Schwartz D13/165
- D323,297 S * 1/1992 Zeller D10/15
- D324,670 S * 3/1992 Ferraro D13/137.4
- D325,370 S * 4/1992 Belcher D13/137.3
- D325,562 S * 4/1992 Smith, Sr. D13/139.2
- D329,422 S * 9/1992 Fujiyoshi D13/139.1
- D354,943 S * 1/1995 Williams et al. D13/137.1
- D357,460 S * 4/1995 Lovett D13/139.8
- D361,315 S * 8/1995 Wedell et al. D13/160
- D399,495 S * 10/1998 Bachschmid D13/177
- D401,555 S * 11/1998 Tam D13/137.3
- D405,760 S * 2/1999 Yu D13/139.3
- 6,045,374 A * 4/2000 Candeloro 439/105
- 6,049,281 A * 4/2000 Osterweil 600/473

- D431,027 S * 9/2000 Armstrong D13/162
- D435,523 S * 12/2000 Ciornei et al. D13/164
- D436,082 S * 1/2001 Jilani D13/158
- D443,589 S * 6/2001 Tong et al. D13/137.2
- D455,406 S * 4/2002 Pinchuk D13/158
- D486,126 S * 2/2004 Aromin D13/137.2
- D500,686 S * 1/2005 Stekelenburg D10/40
- D500,687 S * 1/2005 Morrison et al. D10/40
- D514,067 S * 1/2006 Lee D13/137.2
- D523,397 S * 6/2006 Maglionico et al. D13/137.2
- D535,204 S * 1/2007 Bender et al. D10/104
- D543,939 S * 6/2007 Burke D13/137.2
- D547,272 S * 7/2007 Ng D13/137.2
- D567,950 S * 4/2008 Savage, Jr. D24/186
- D568,253 S * 5/2008 Gorman D13/154
- D581,870 S * 12/2008 Zhou D13/137.2
- D582,346 S * 12/2008 Zhou D13/137.2

(Continued)

Primary Examiner—T. Chase Nelson
Assistant Examiner—Mark Cavanna
(74) *Attorney, Agent, or Firm*—Myers Bigel Sibley & Sajovec, P.A.


(57) **CLAIM**

The ornamental design for electronic reader for medical environments, as shown and described.

DESCRIPTION

FIG. 1 is a front perspective view of an electronic reader for medical environments showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a side view thereof;
FIG. 4 is an opposing side view thereof;
FIG. 5 is a rear view of the side thereof;
FIG. 6 is a top end view thereof;
FIG. 7 is a bottom end view thereof; and,
FIG. 8 is a front perspective environmental view thereof illustrating the electronic reader for medical environments in an exemplary clinical use environment.

1 Claim, 5 Drawing Sheets

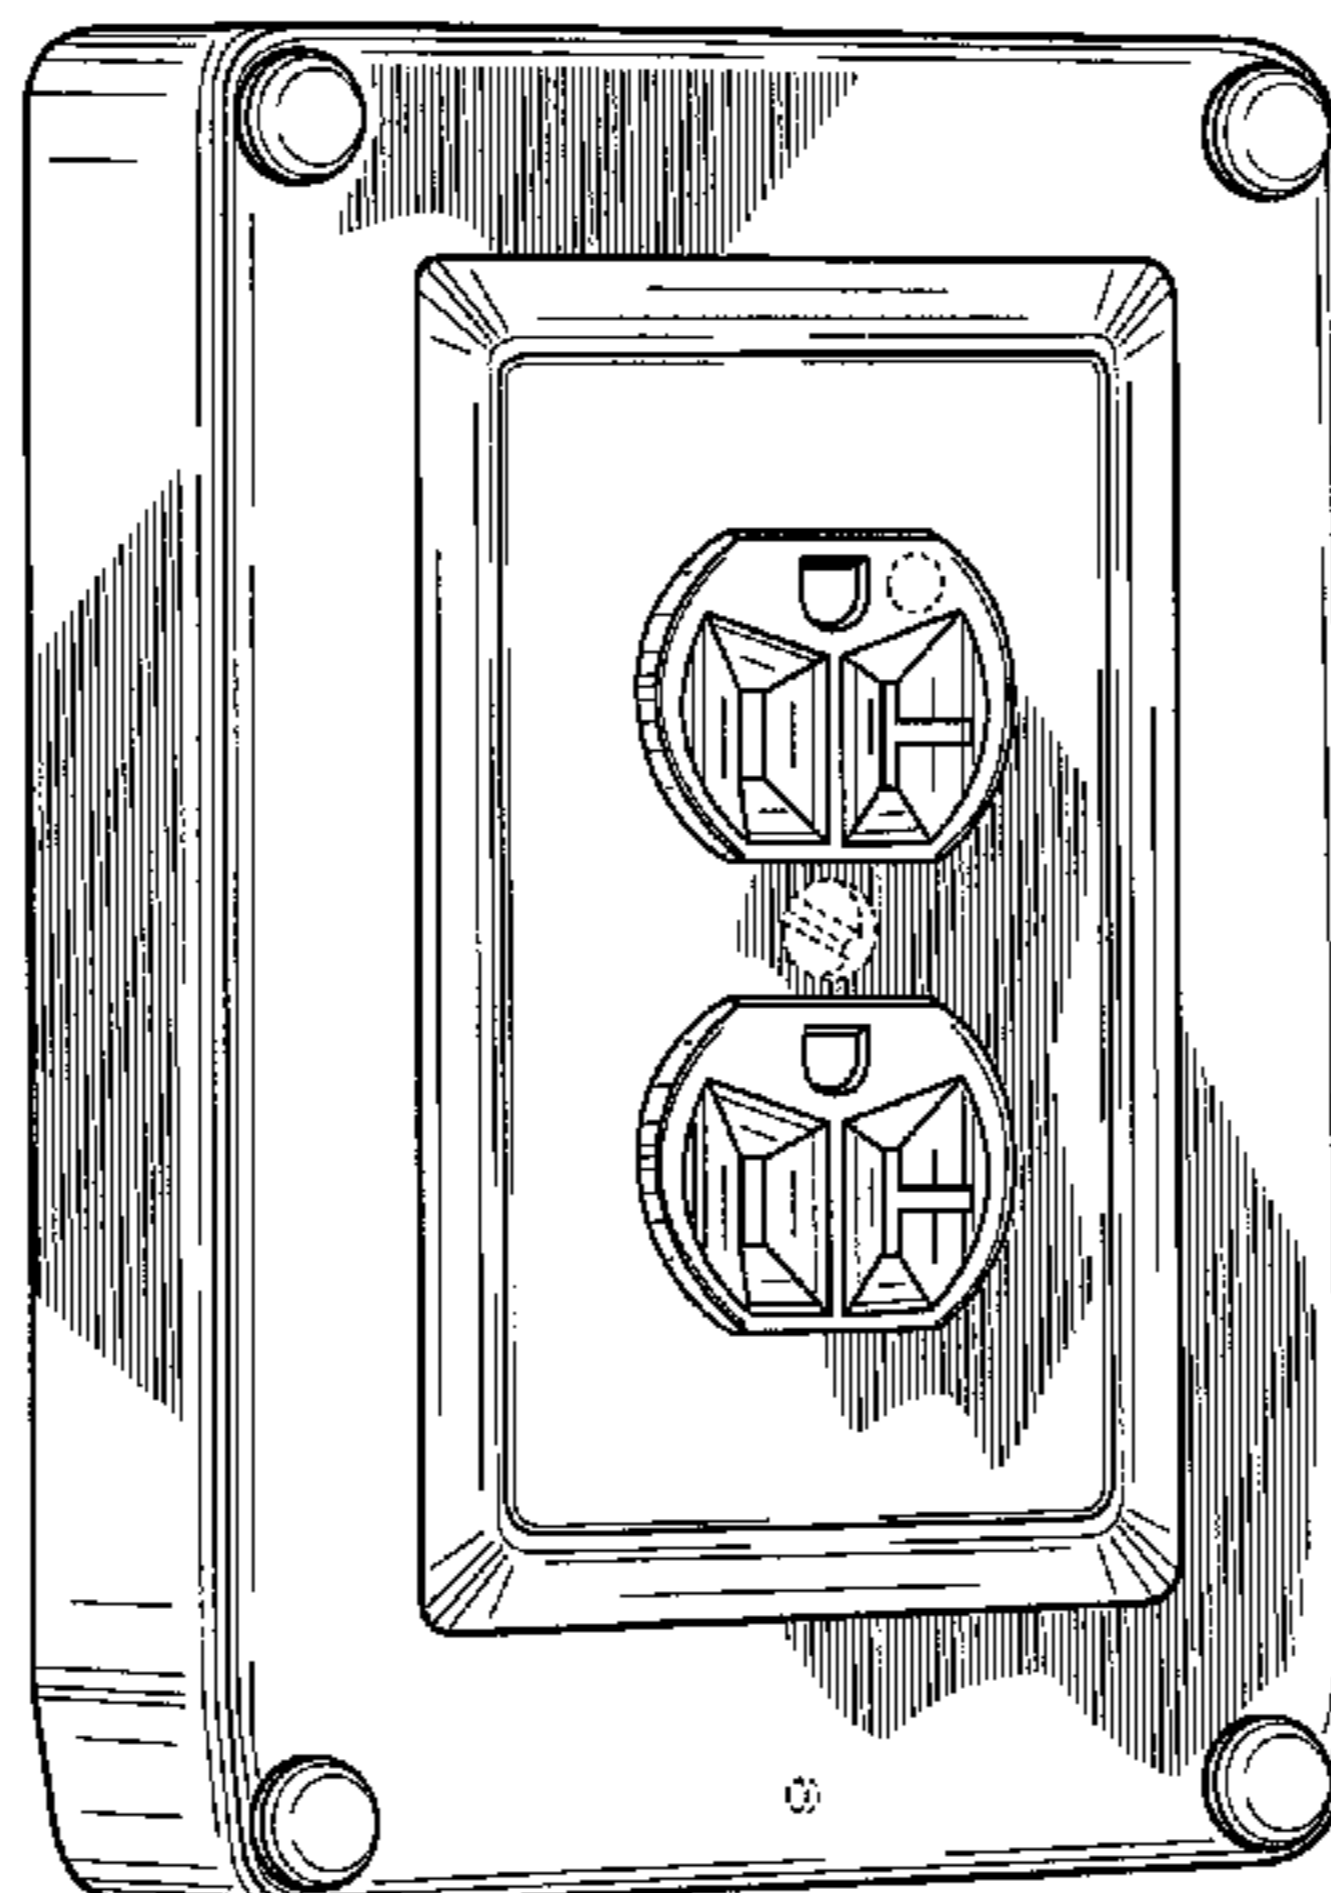

US D631,165 S

Page 2

U.S. PATENT DOCUMENTS

D588,076 S *	3/2009	Ollila	D13/168	D608,302 S *	1/2010	Liu	D13/164
D590,352 S *	4/2009	Jacoby et al.	D13/164	D610,554 S *	2/2010	Lanfear et al.	D13/162
D595,229 S *	6/2009	LaGrotta	D13/137.2	D611,005 S *	3/2010	Lanfear et al.	D13/162
D595,604 S *	7/2009	Schmalz et al.	D10/104	2002/0072272 A1 *	6/2002	King	439/535
D596,140 S *	7/2009	Hollner	D13/164	2003/0151938 A1 *	8/2003	Liao	363/146
D603,346 S *	11/2009	Murray et al.	D13/162	2004/0121648 A1 *	6/2004	Voros	439/535
				2008/0289844 A1 *	11/2008	Dutton, Jr.	174/66

* cited by examiner

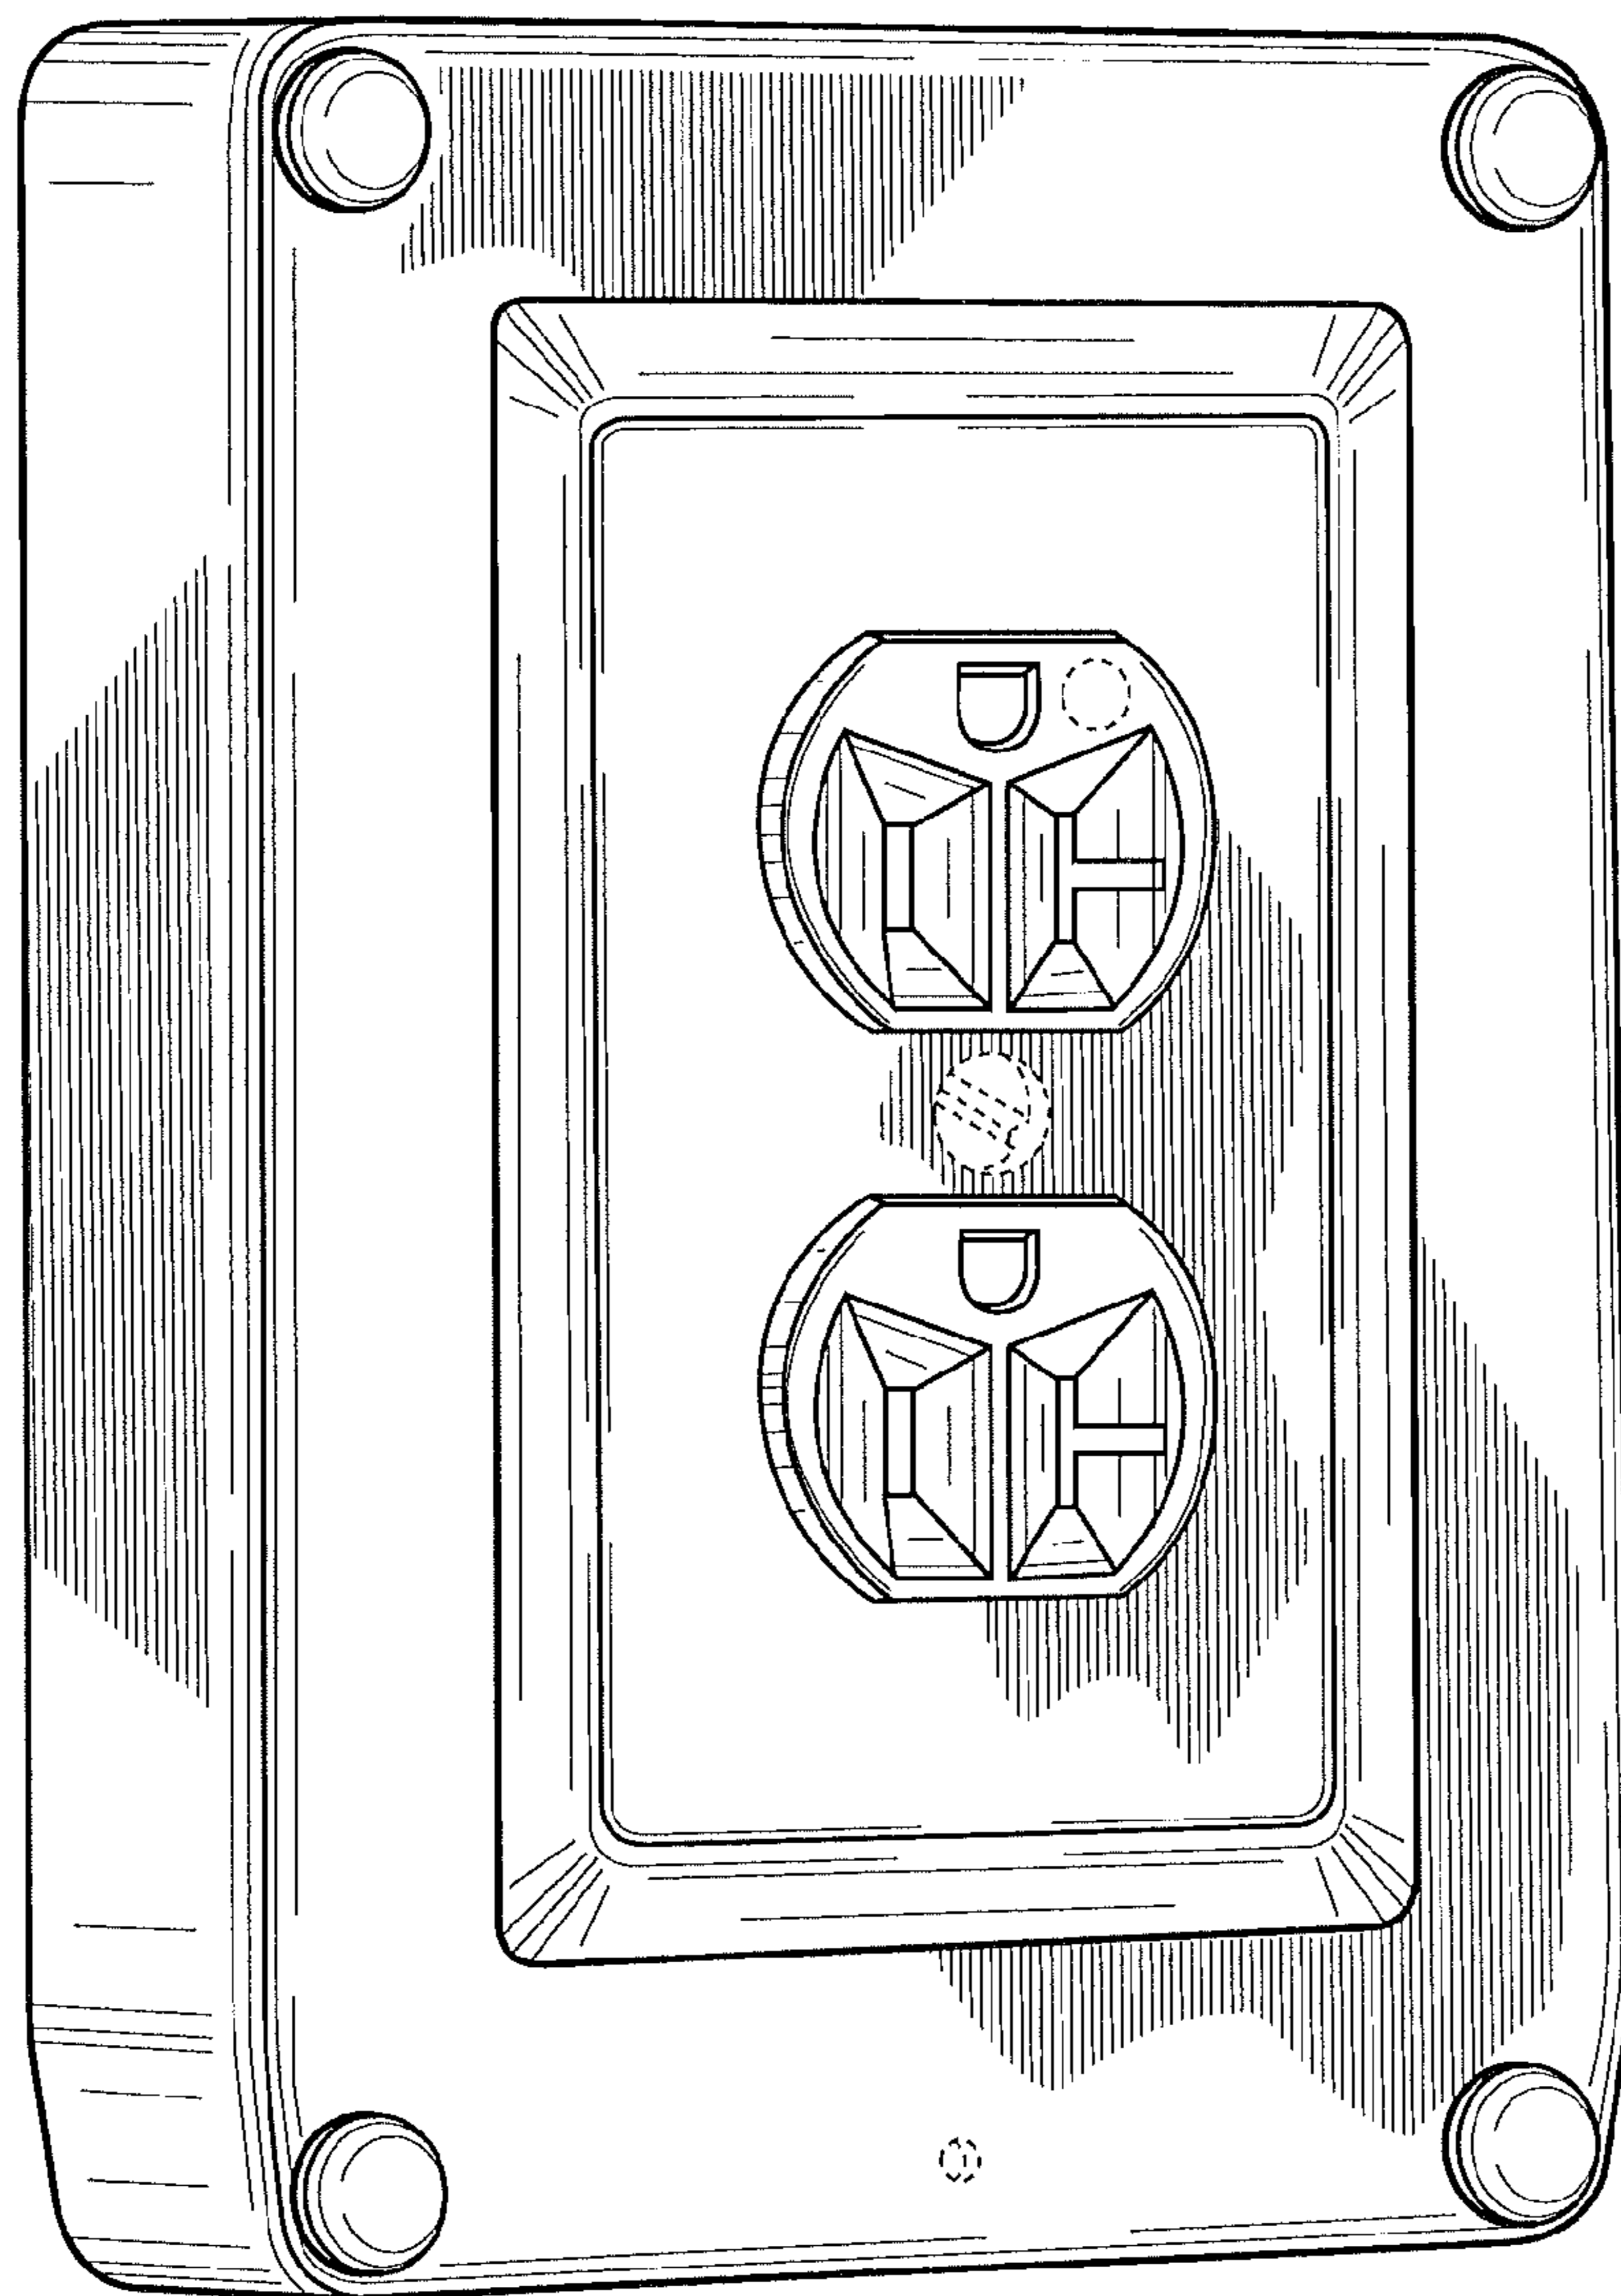


FIG. 1

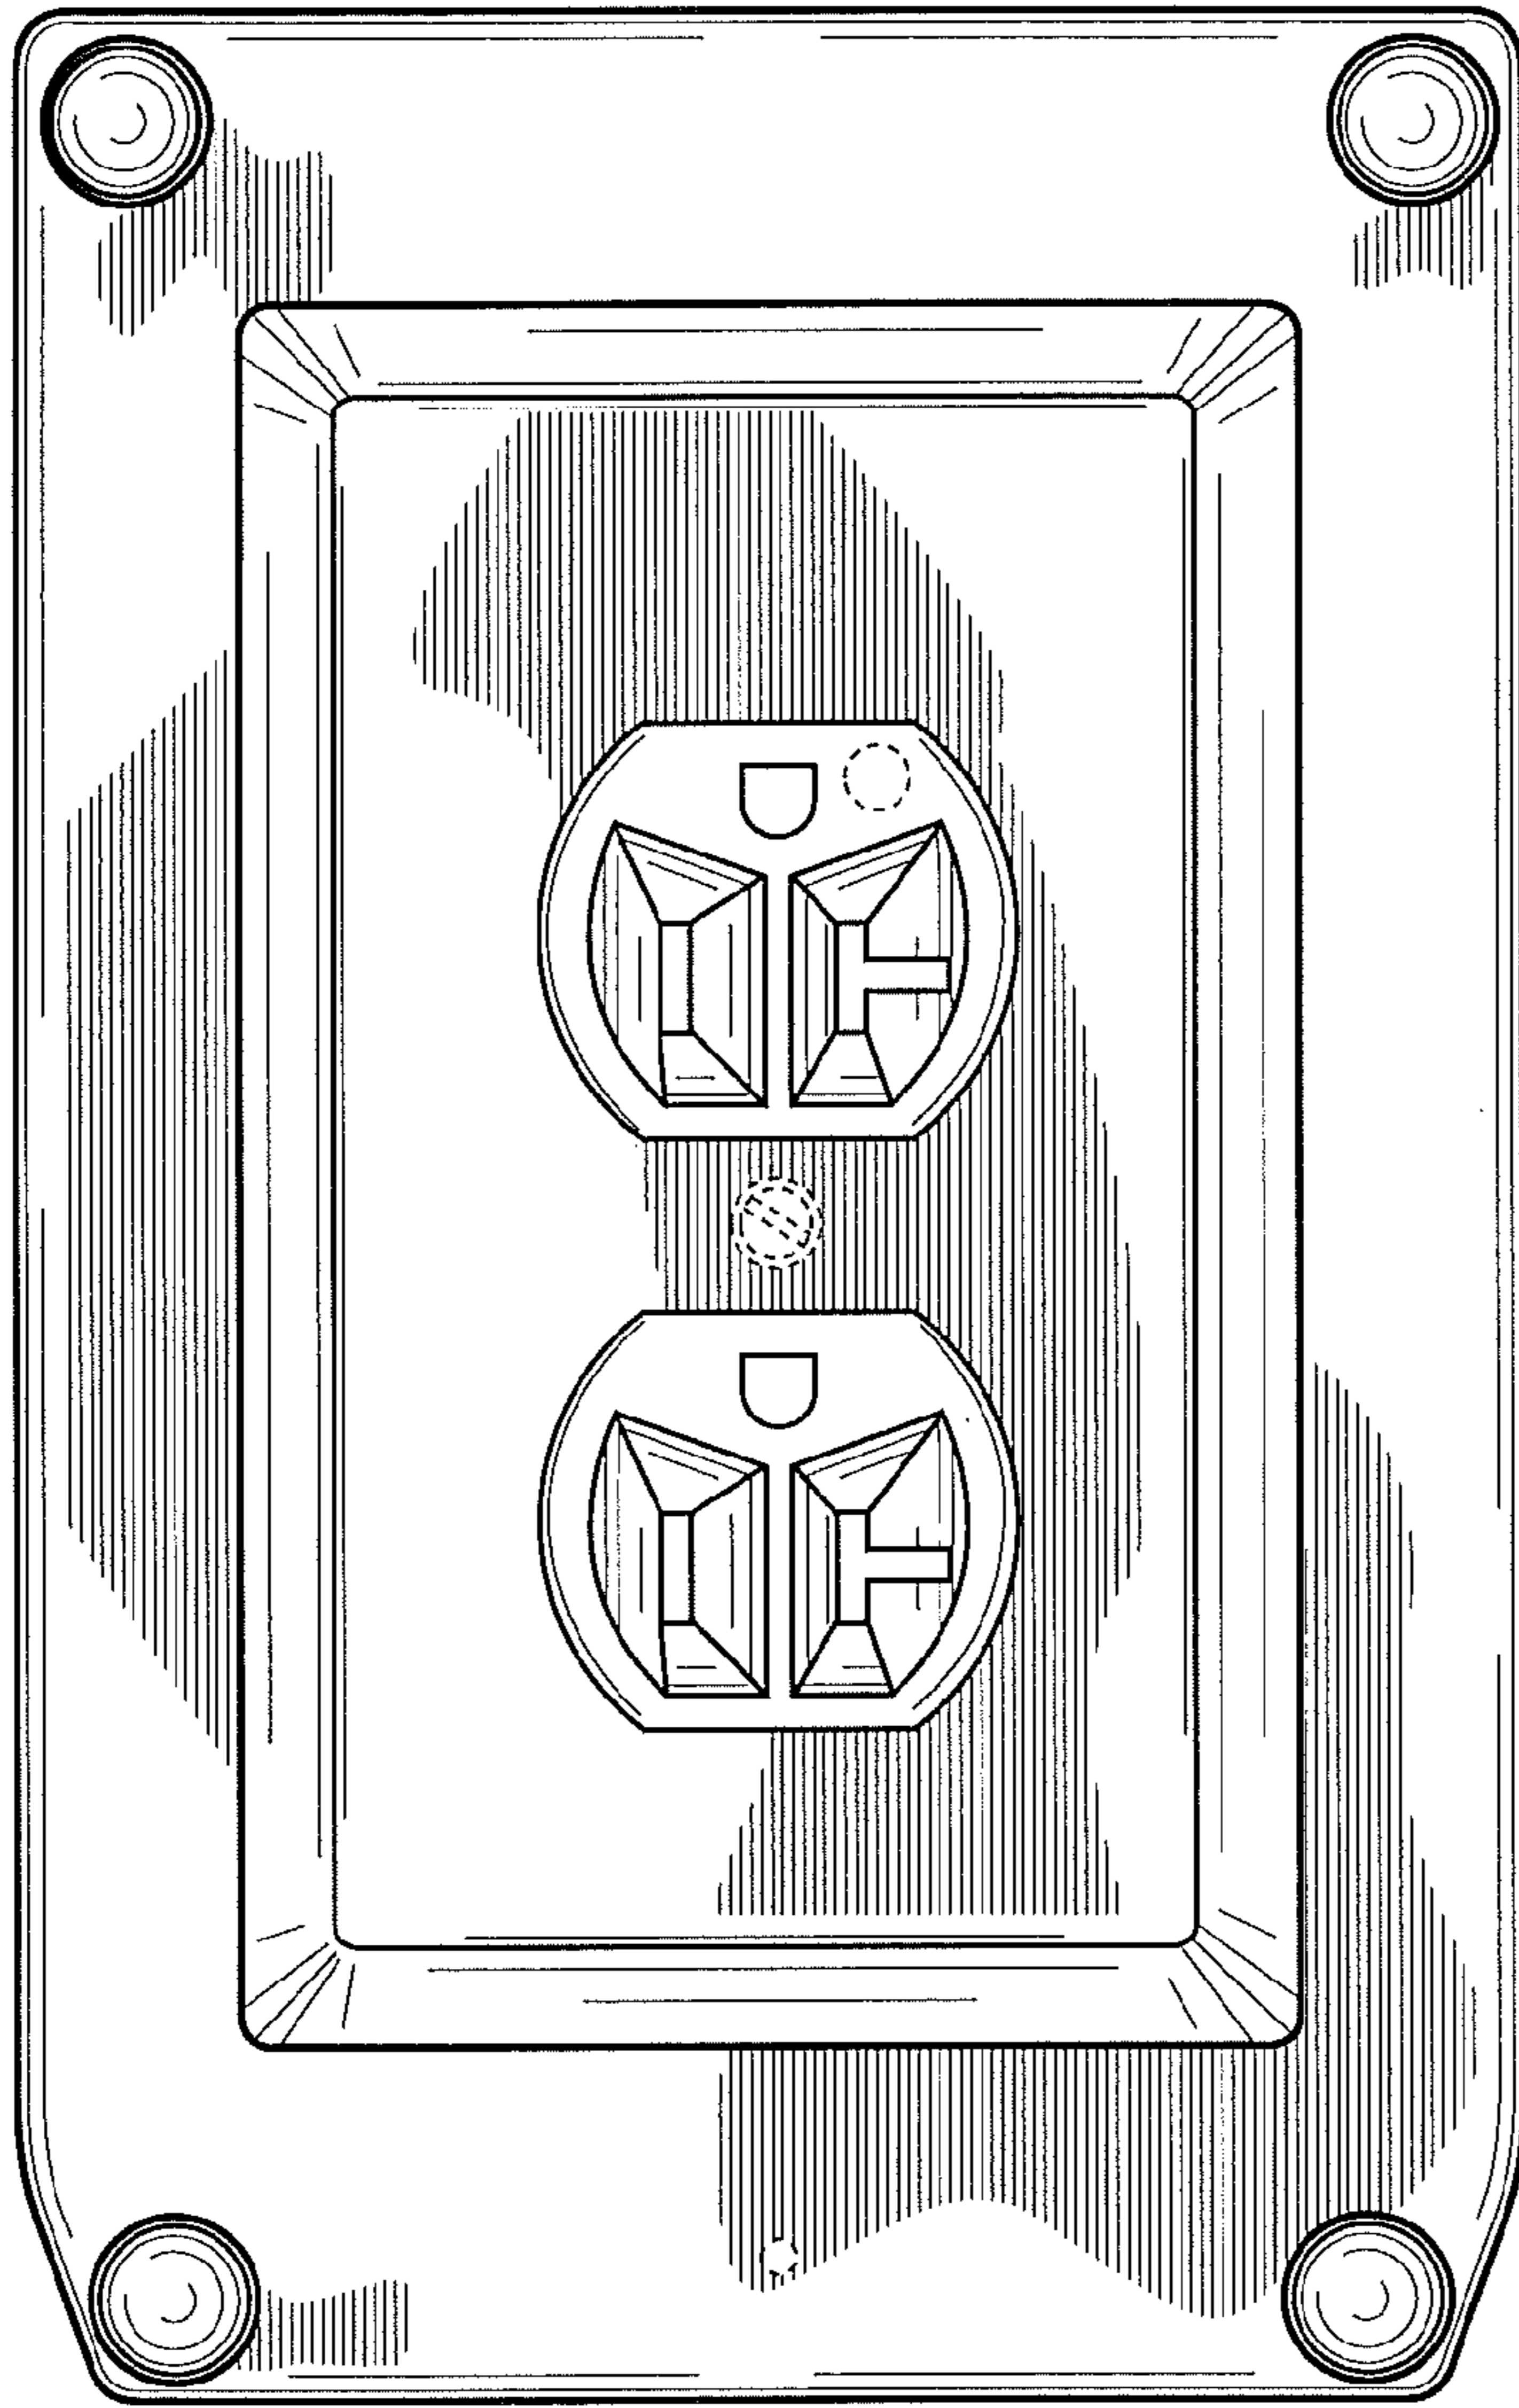


FIG. 2

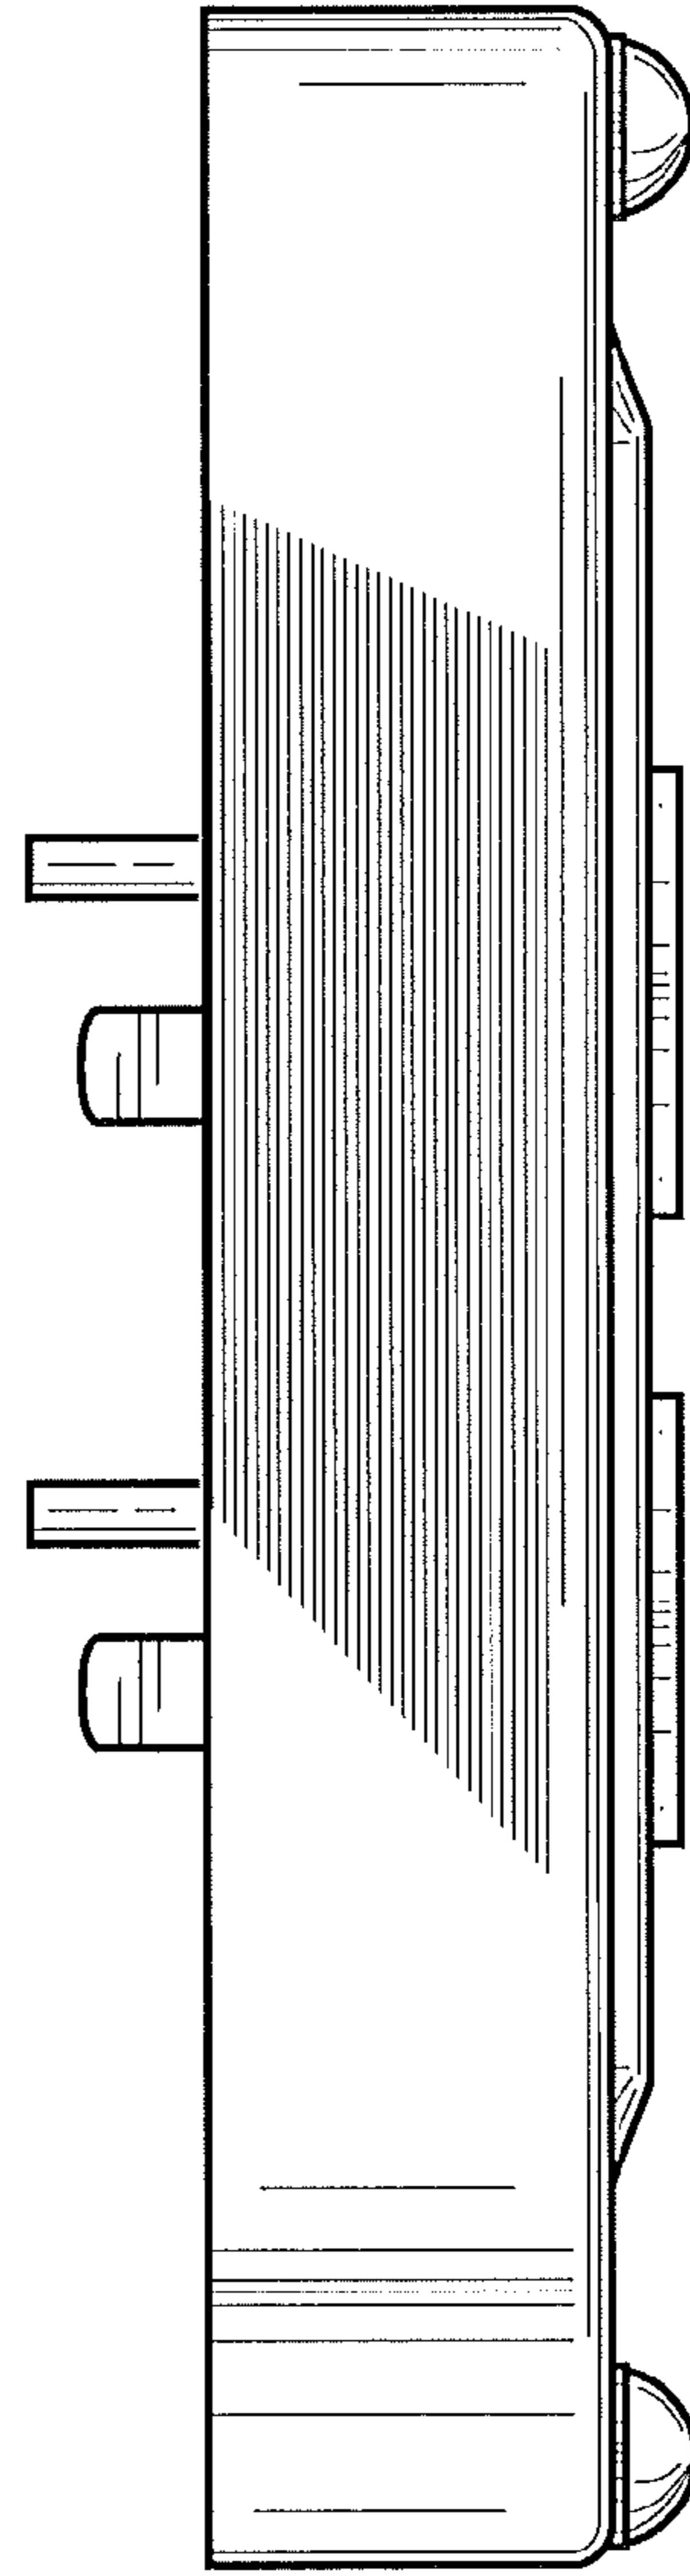


FIG. 3

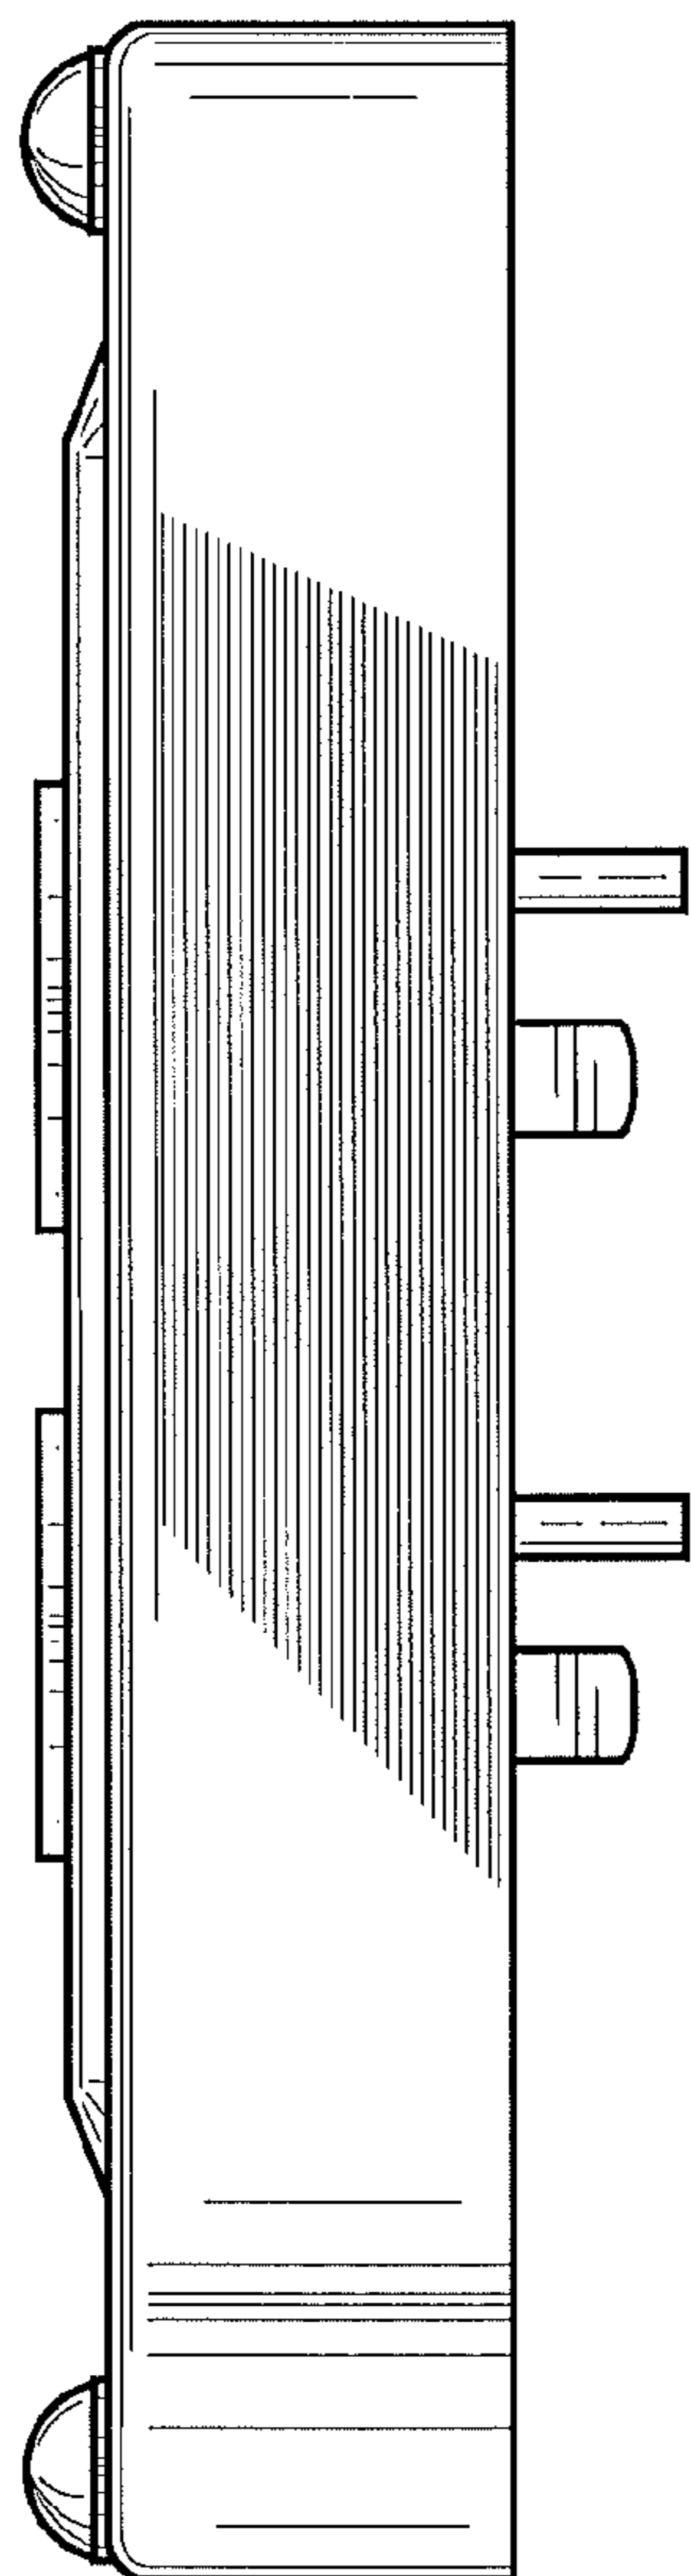


FIG. 4

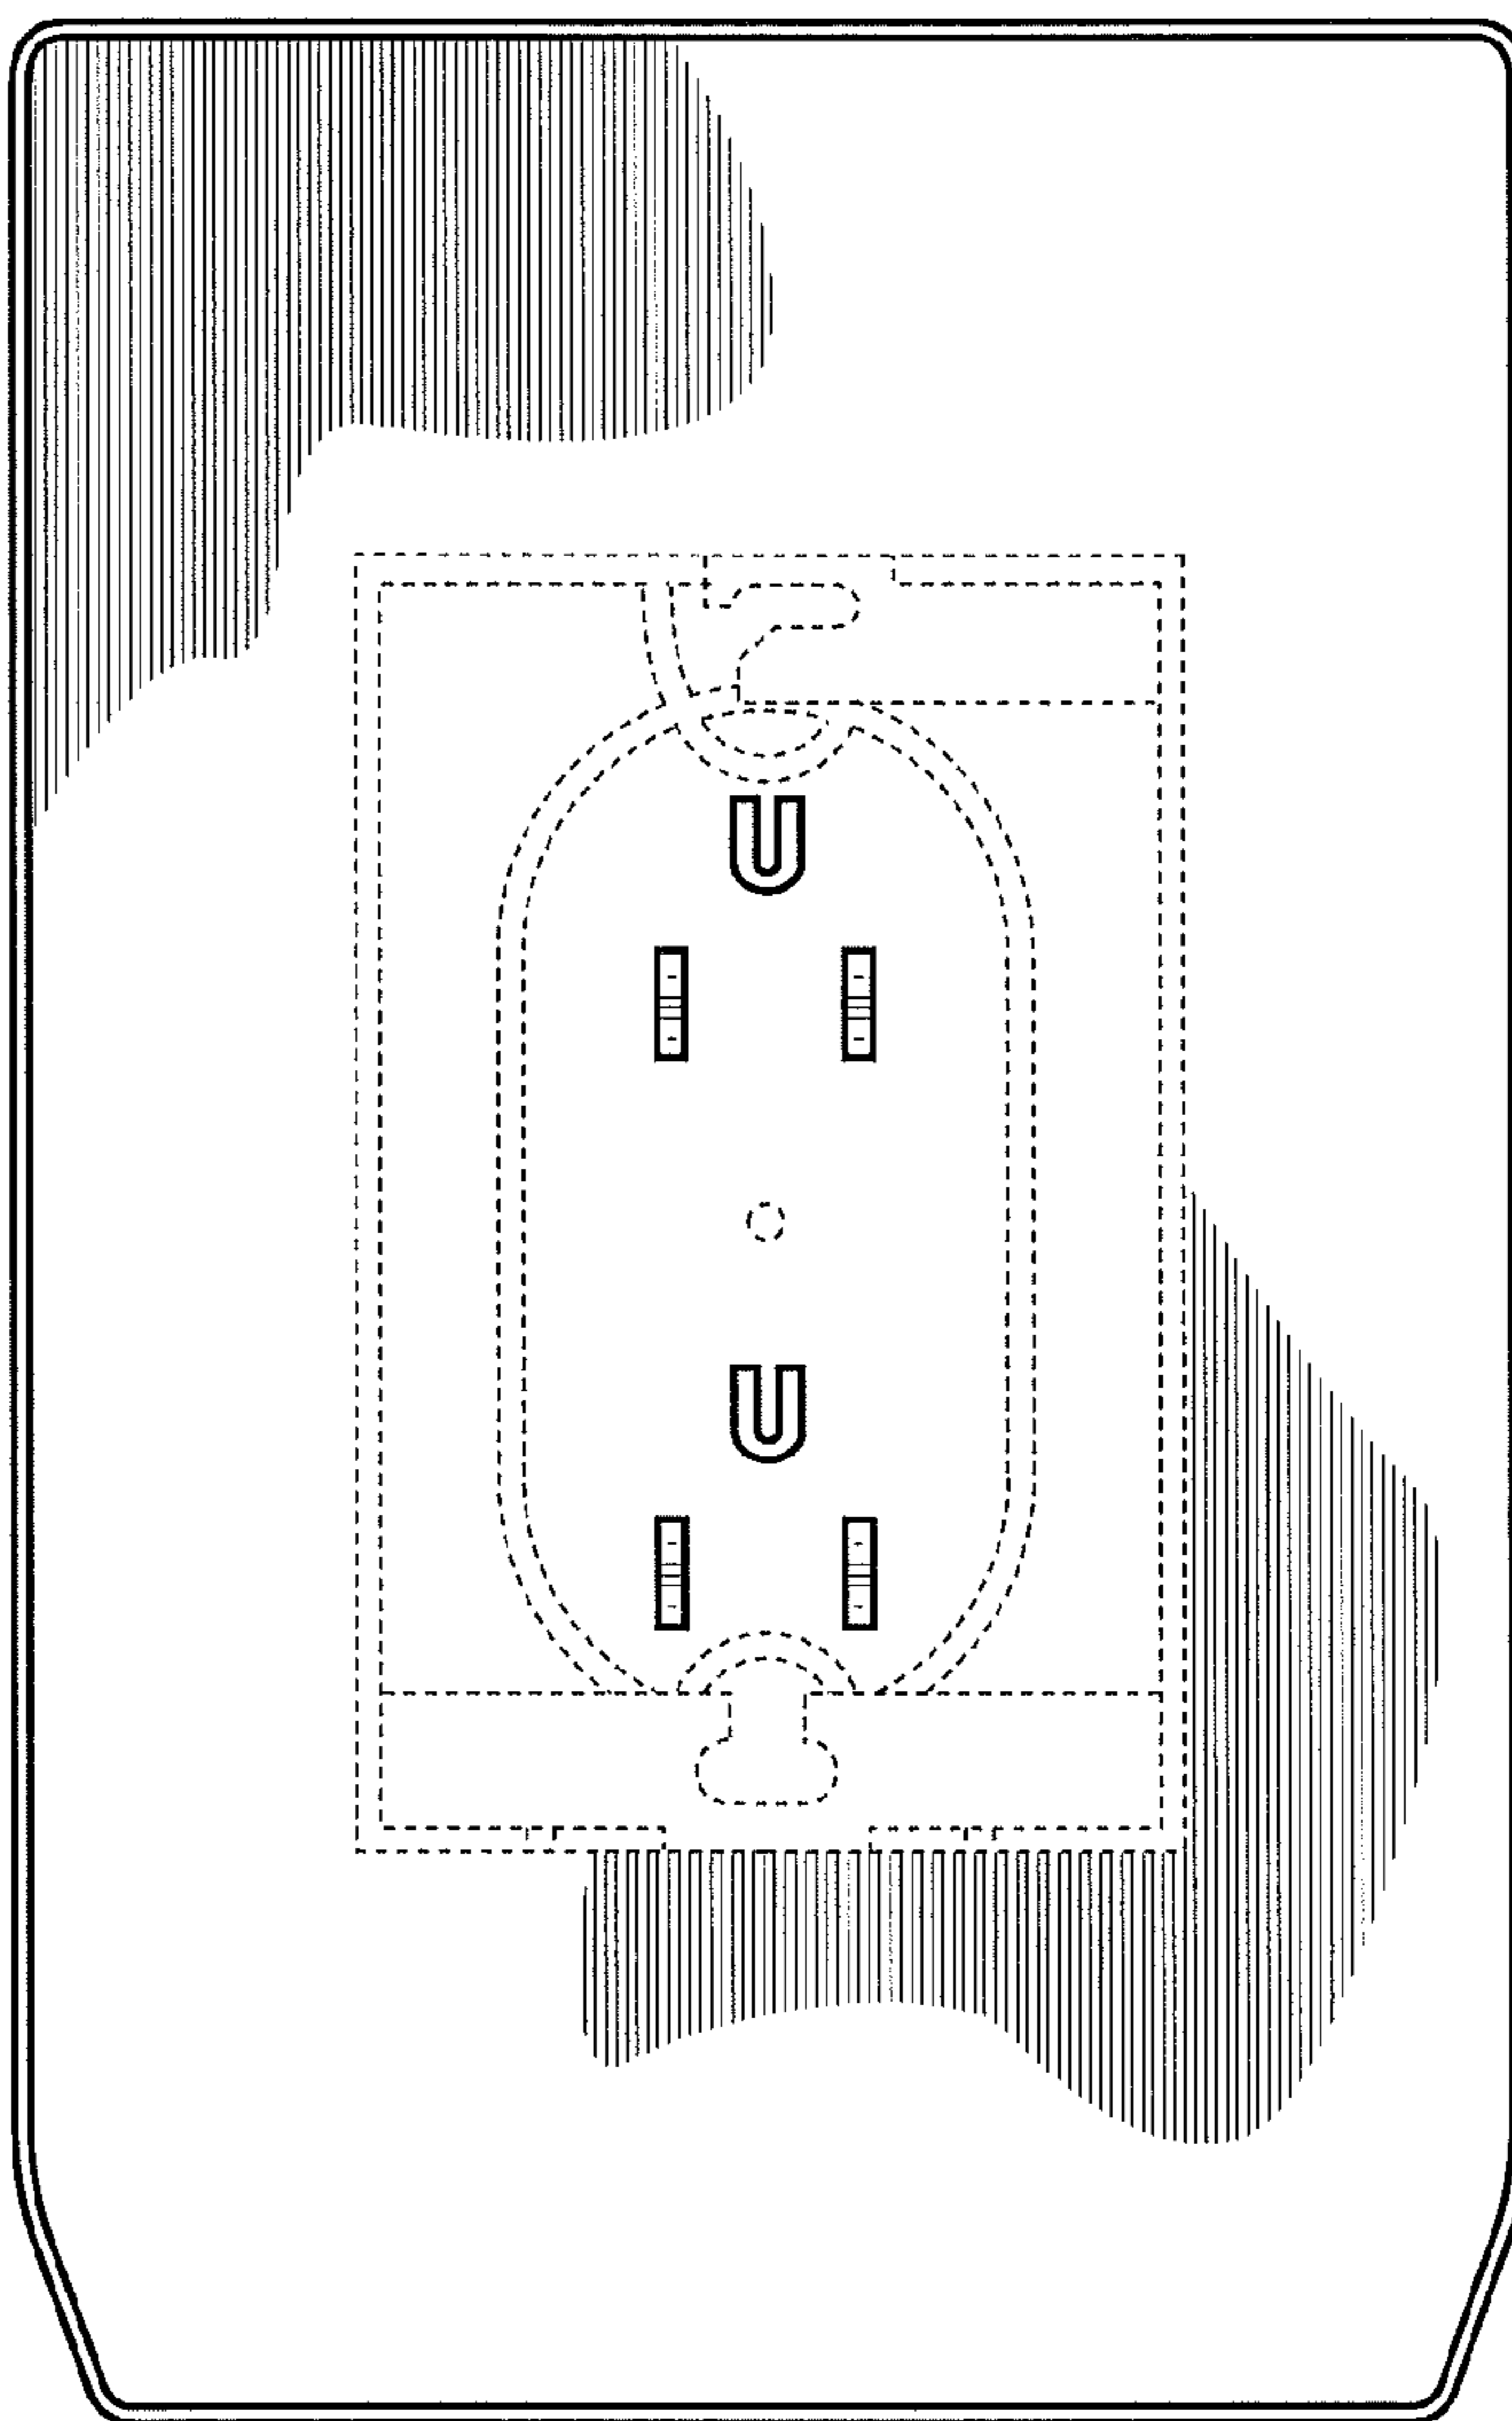


FIG. 5

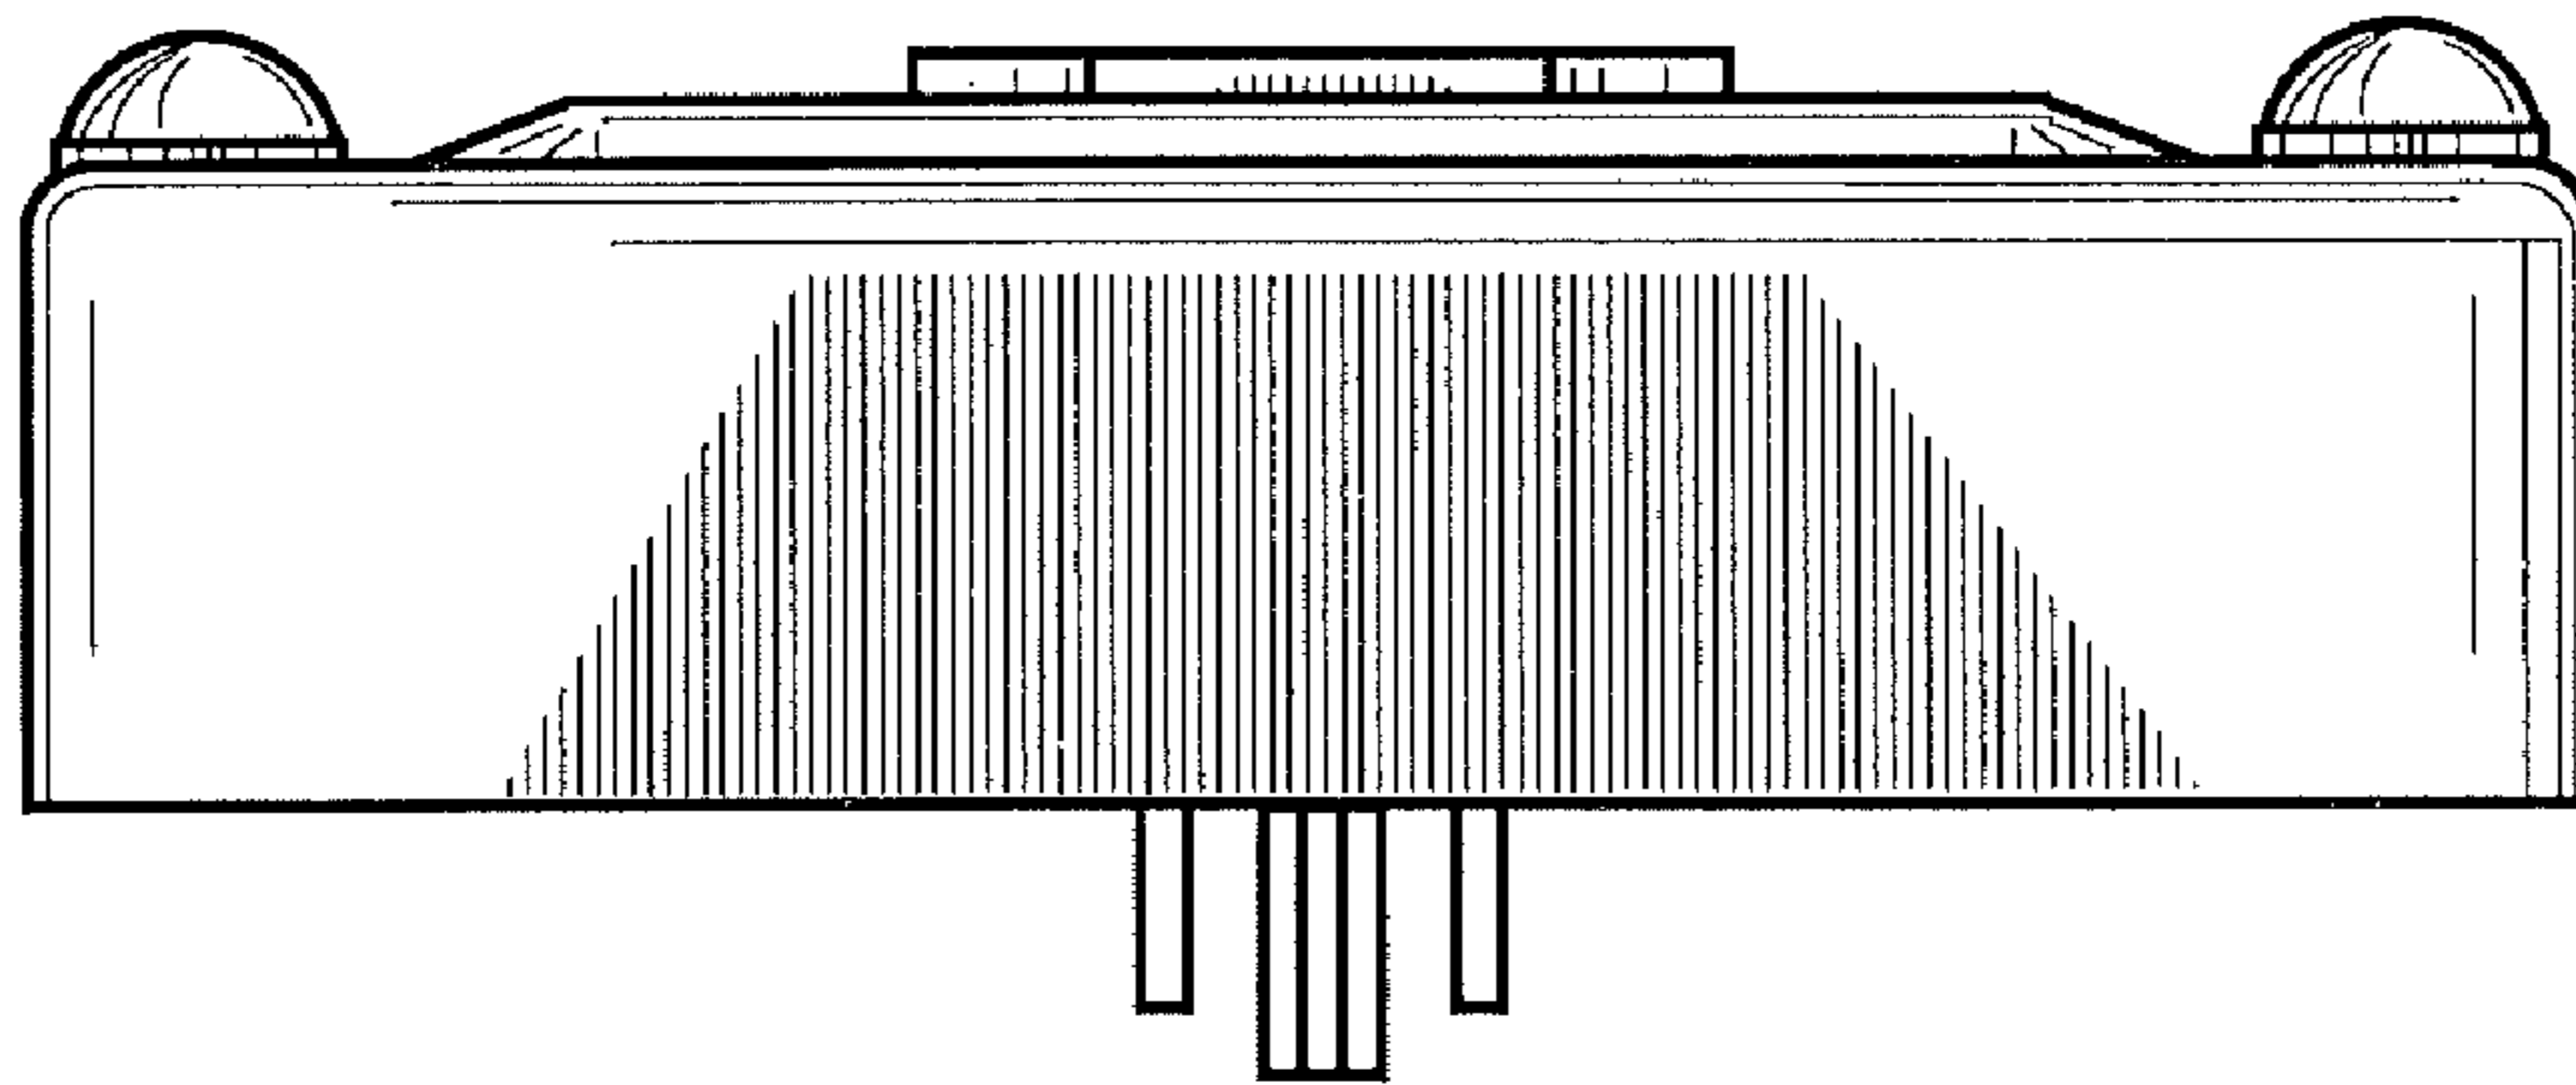


FIG. 6

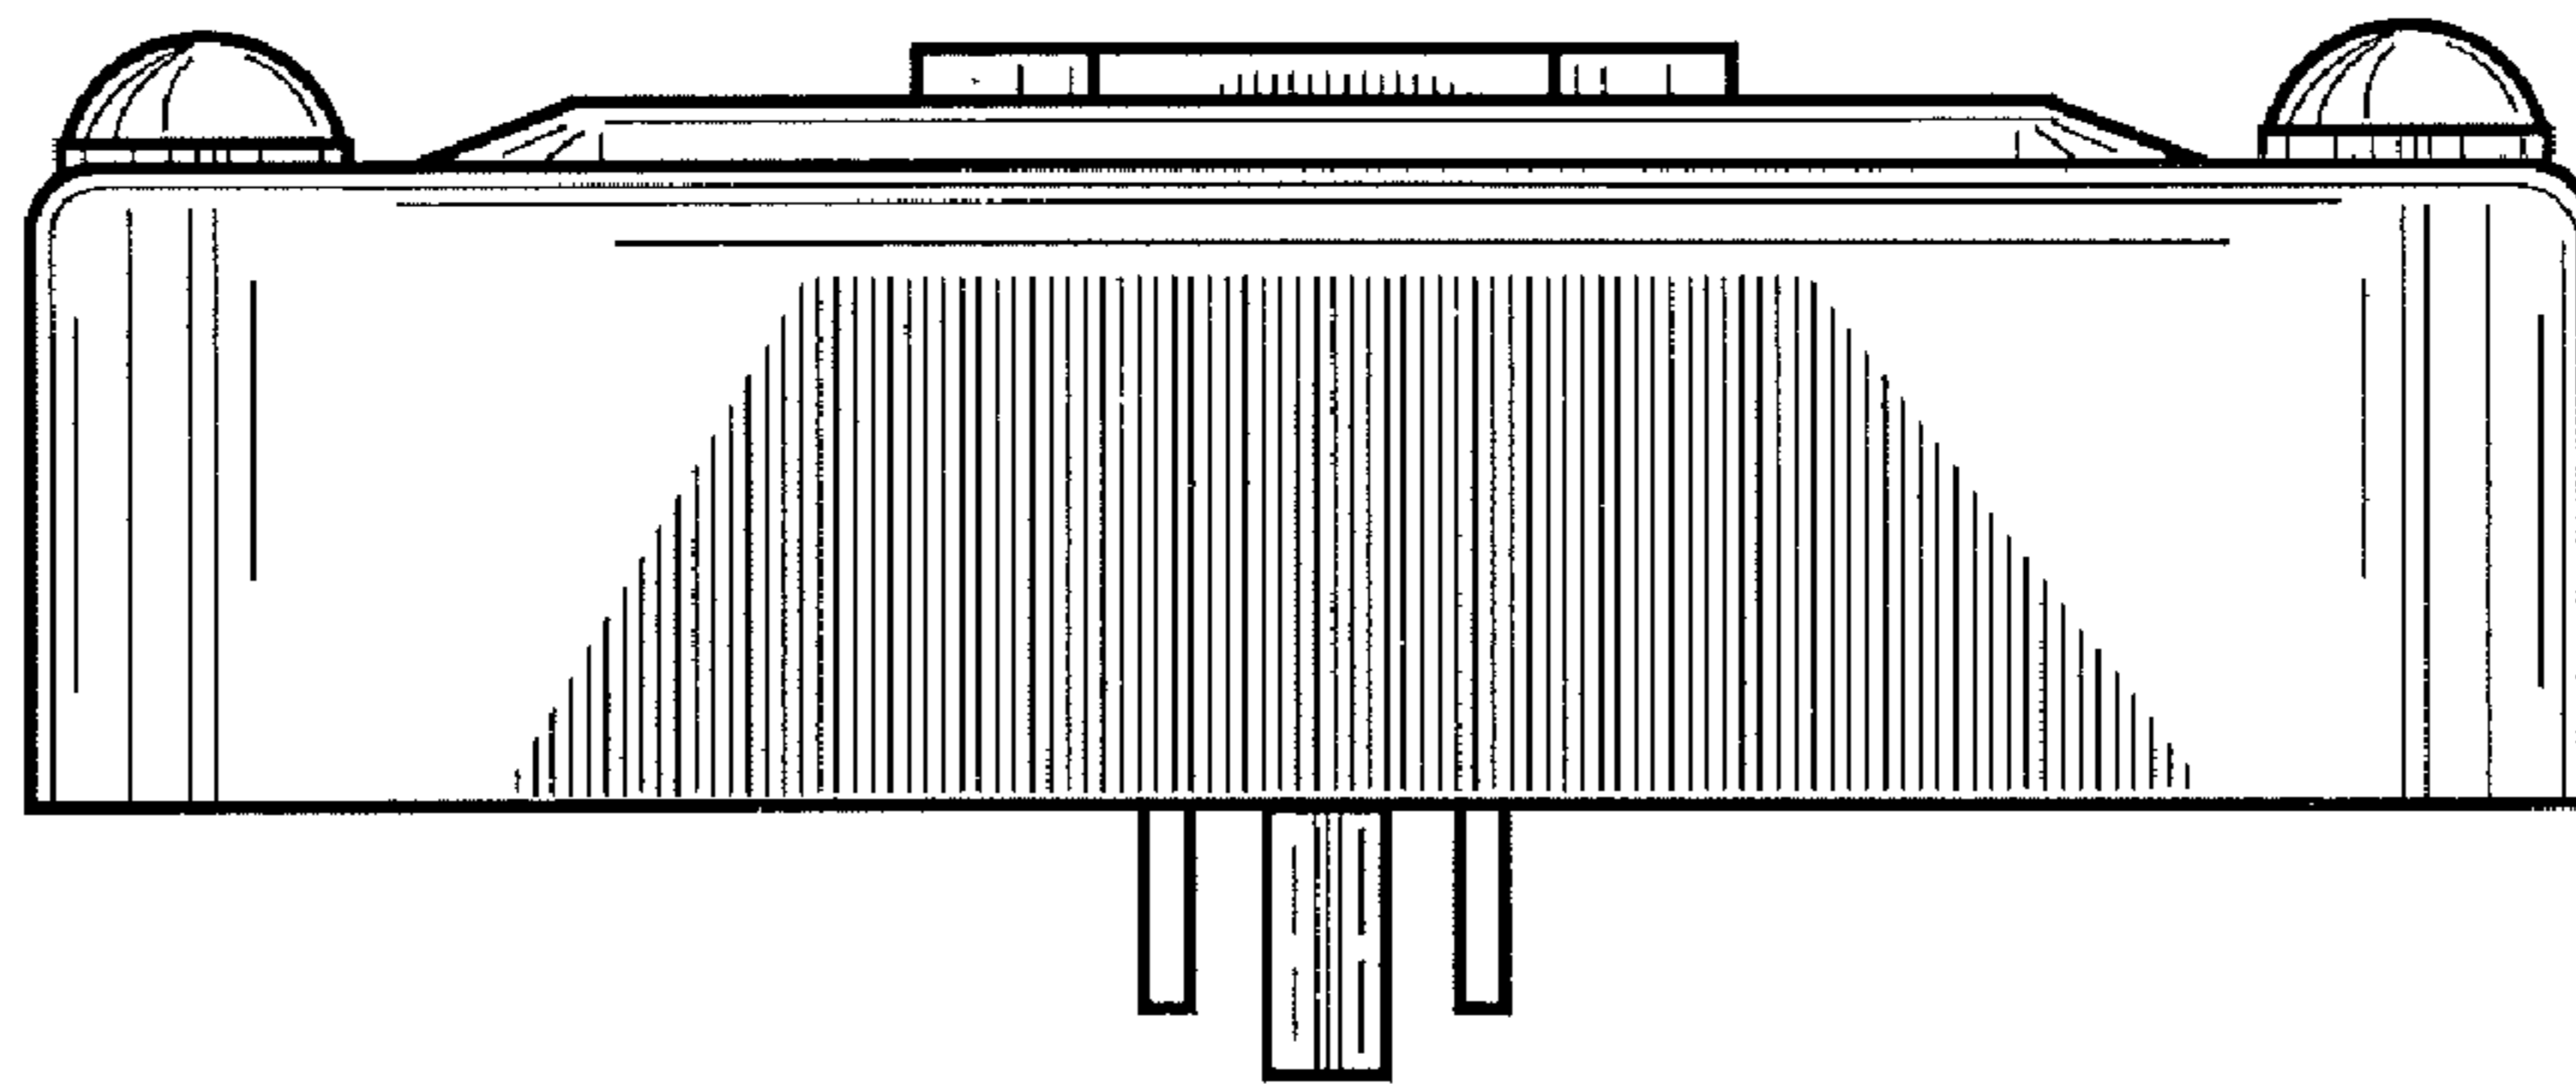


FIG. 7

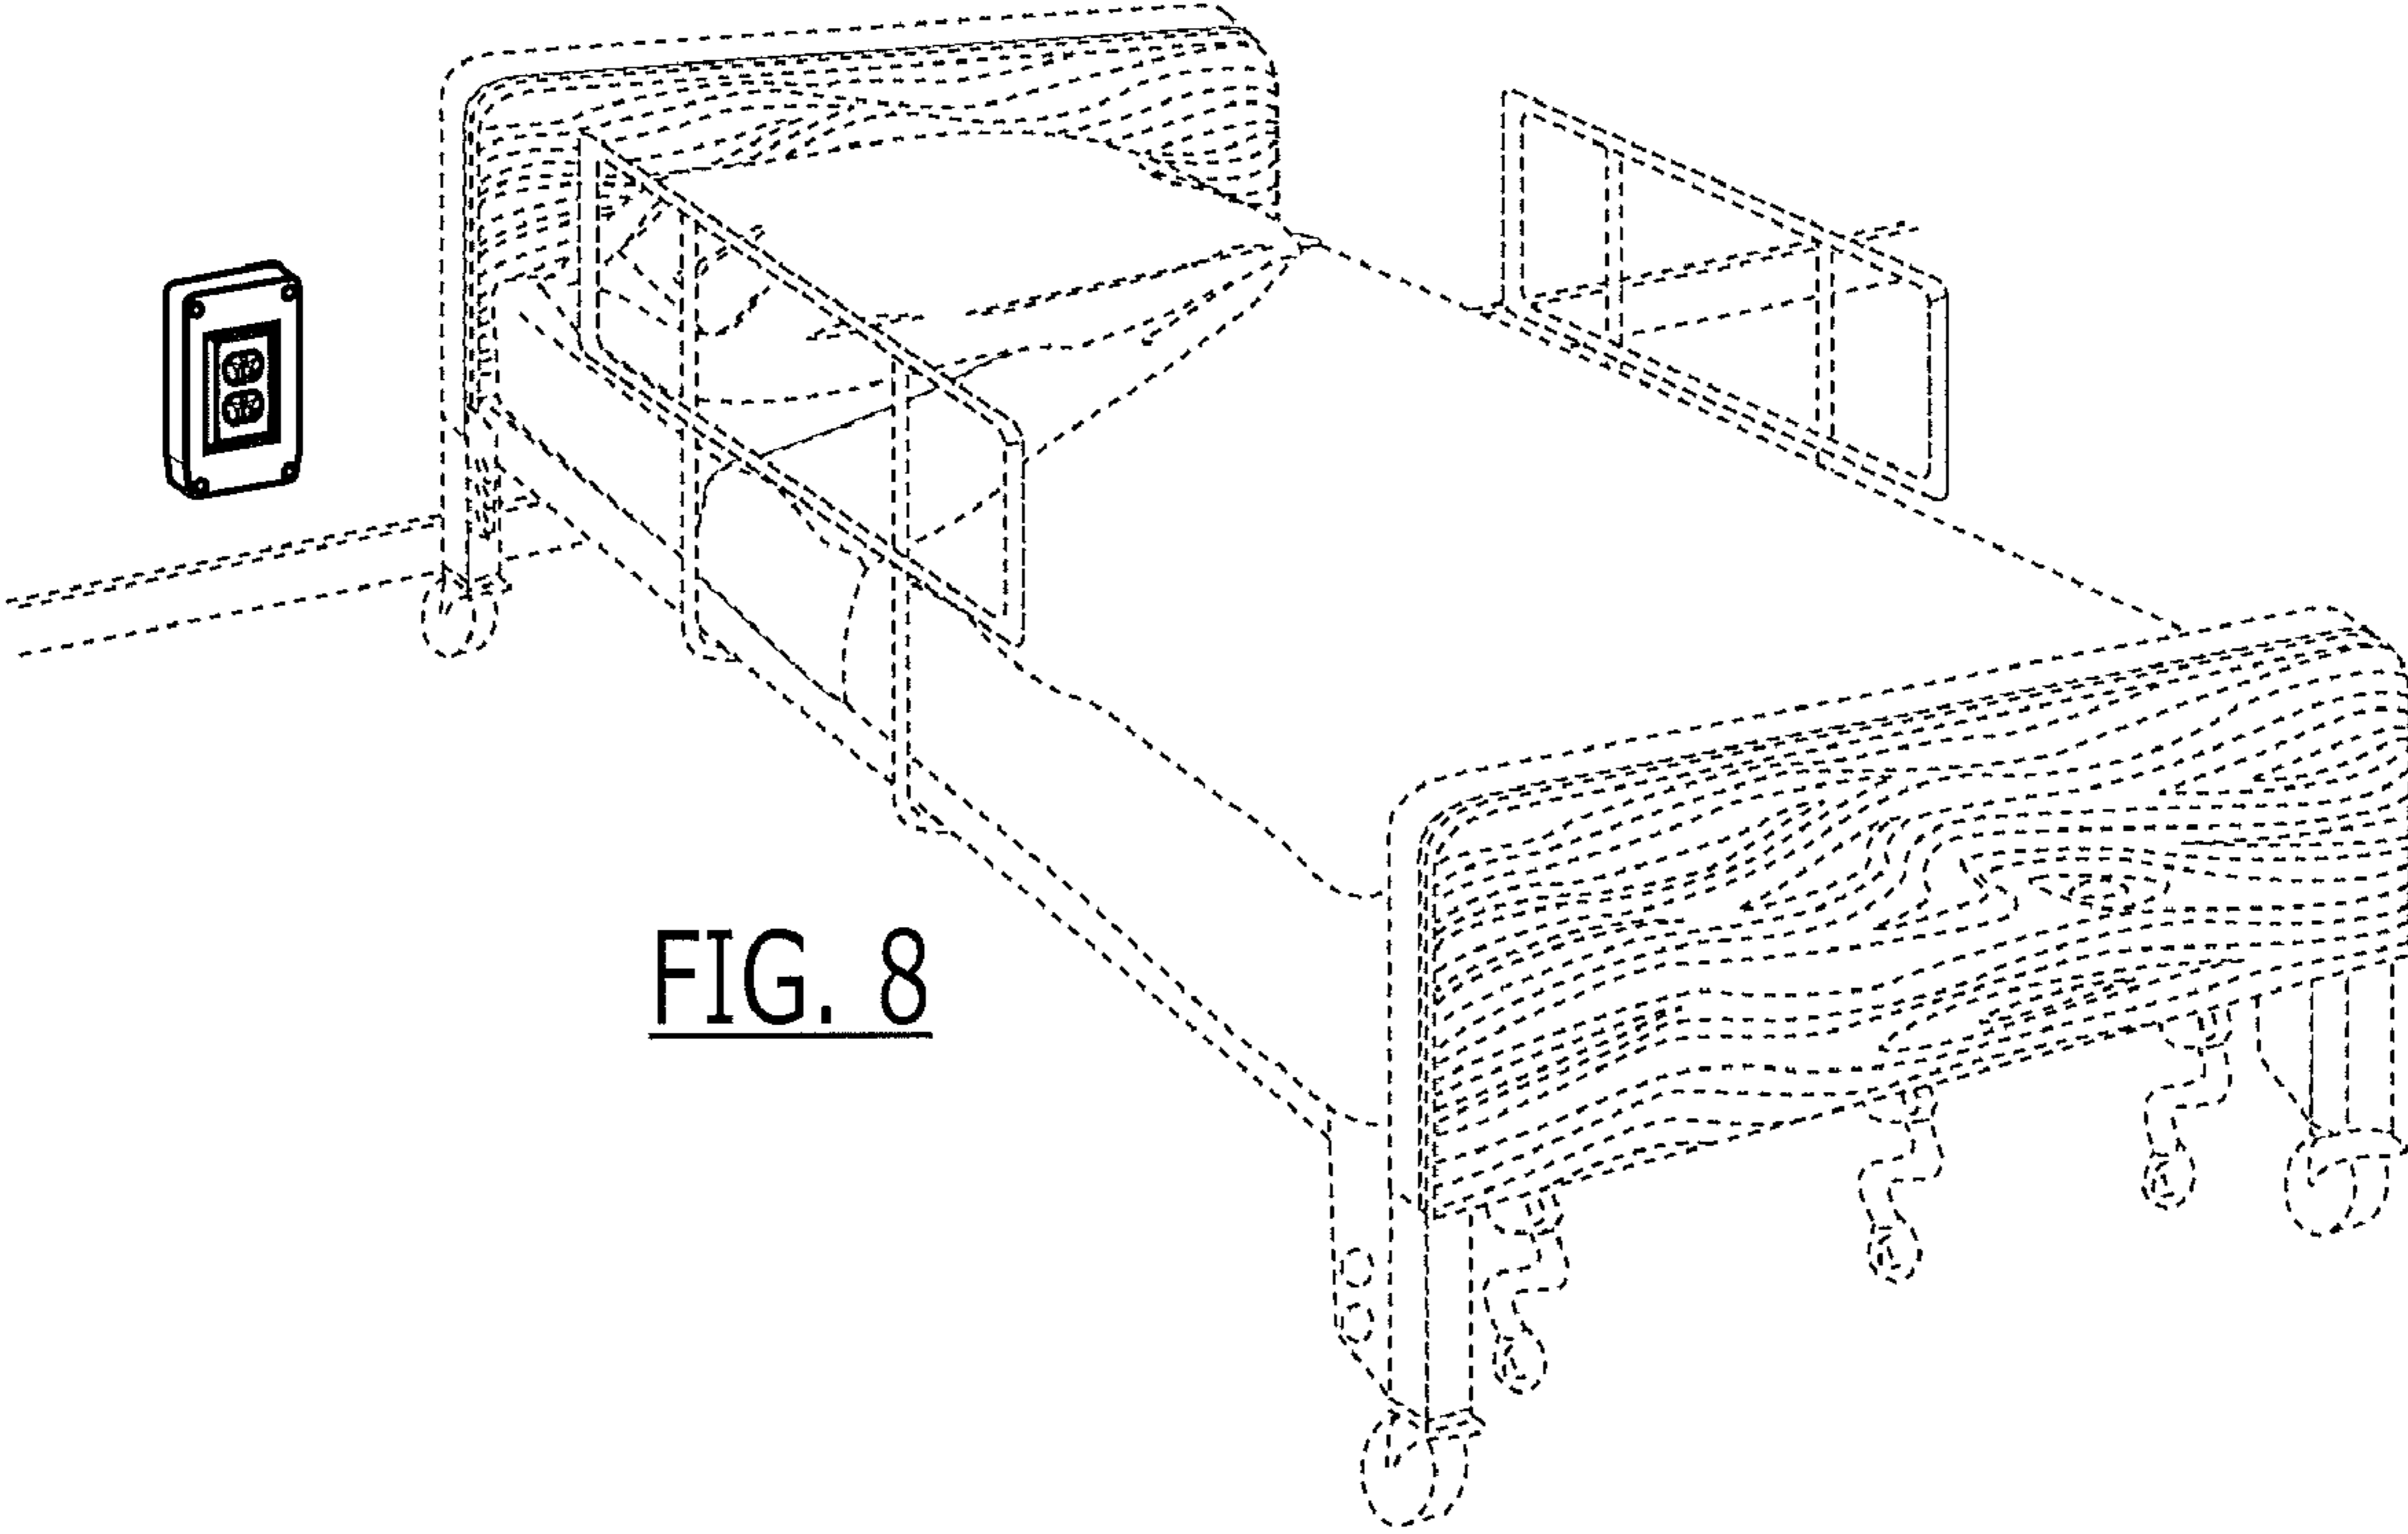


FIG. 8