



US00D631976S

(12) **United States Design Patent**  
**Oonuma et al.**

(10) **Patent No.:** **US D631,976 S**  
(45) **Date of Patent:** **\*\* Feb. 1, 2011**

(54) **SAMPLER UNIT FOR CLINICAL ANALYZER**

(75) Inventors: **Mitsuru Oonuma**, Tokyo (JP); **Hitoshi Tokieda**, Hitachinaka (JP); **Yoshimitsu Takagi**, Hitachinaka (JP); **Takeshi Shibuya**, Hitachinaka (JP)

(73) Assignee: **Hitachi High-Technologies Corporation**, Tokyo (JP)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/354,619**

(22) Filed: **Jan. 27, 2010**

(30) **Foreign Application Priority Data**

Aug. 25, 2009 (JP) ..... 2009-019398

(51) **LOC (9) Cl.** ..... **24-01**

(52) **U.S. Cl.** ..... **D24/216**

(58) **Field of Classification Search** ..... D24/216,  
D24/222-226, 231, 232, 169; D10/81; 422/100,  
422/62-67, 68.1; 436/47, 48  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D330,770 S \* 11/1992 Rodomista et al. .... D24/216  
D339,639 S \* 9/1993 Ohnuma et al. .... D24/232  
D380,551 S \* 7/1997 Ohnuma et al. .... D24/186  
6,521,183 B1 \* 2/2003 Burri et al. .... 422/65  
D474,416 S \* 5/2003 Oonuma et al. .... D10/81  
D482,796 S \* 11/2003 Oyama et al. .... D24/232  
6,841,126 B2 \* 1/2005 Oonuma et al. .... 422/64  
D508,999 S \* 8/2005 Fanning et al. .... D24/216

D523,153 S \* 6/2006 Akashi et al. .... D24/232  
D554,551 S \* 11/2007 Ouchi et al. .... D10/81  
D560,131 S \* 1/2008 Hu ..... D10/81  
2007/0110617 A1 \* 5/2007 Nagai et al. .... 422/65

**FOREIGN PATENT DOCUMENTS**

JP D1036951 4/1999  
JP D1060387 2/2000

\* cited by examiner

*Primary Examiner*—T. Chase Nelson

*Assistant Examiner*—Anhdao Doan

(74) *Attorney, Agent, or Firm*—Antonelli, Terry, Stout & Kraus, LLP.

(57) **CLAIM**

We claim the ornamental design for a sampler unit for clinical analyzer, as shown and described.

**DESCRIPTION**

FIG. 1 is a front, top and right side perspective view of a sampler unit for clinical analyzer showing our new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a rear elevational view thereof;

FIG. 4 is a left side elevational view thereof;


FIG. 5 is a right side elevational view thereof;

FIG. 6 is a top plan view thereof; and,

FIG. 7 is a bottom plan view thereof.

The broken lines in the drawing views are included for the purpose of illustrating portions of the sampler unit for clinical analyzer that form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

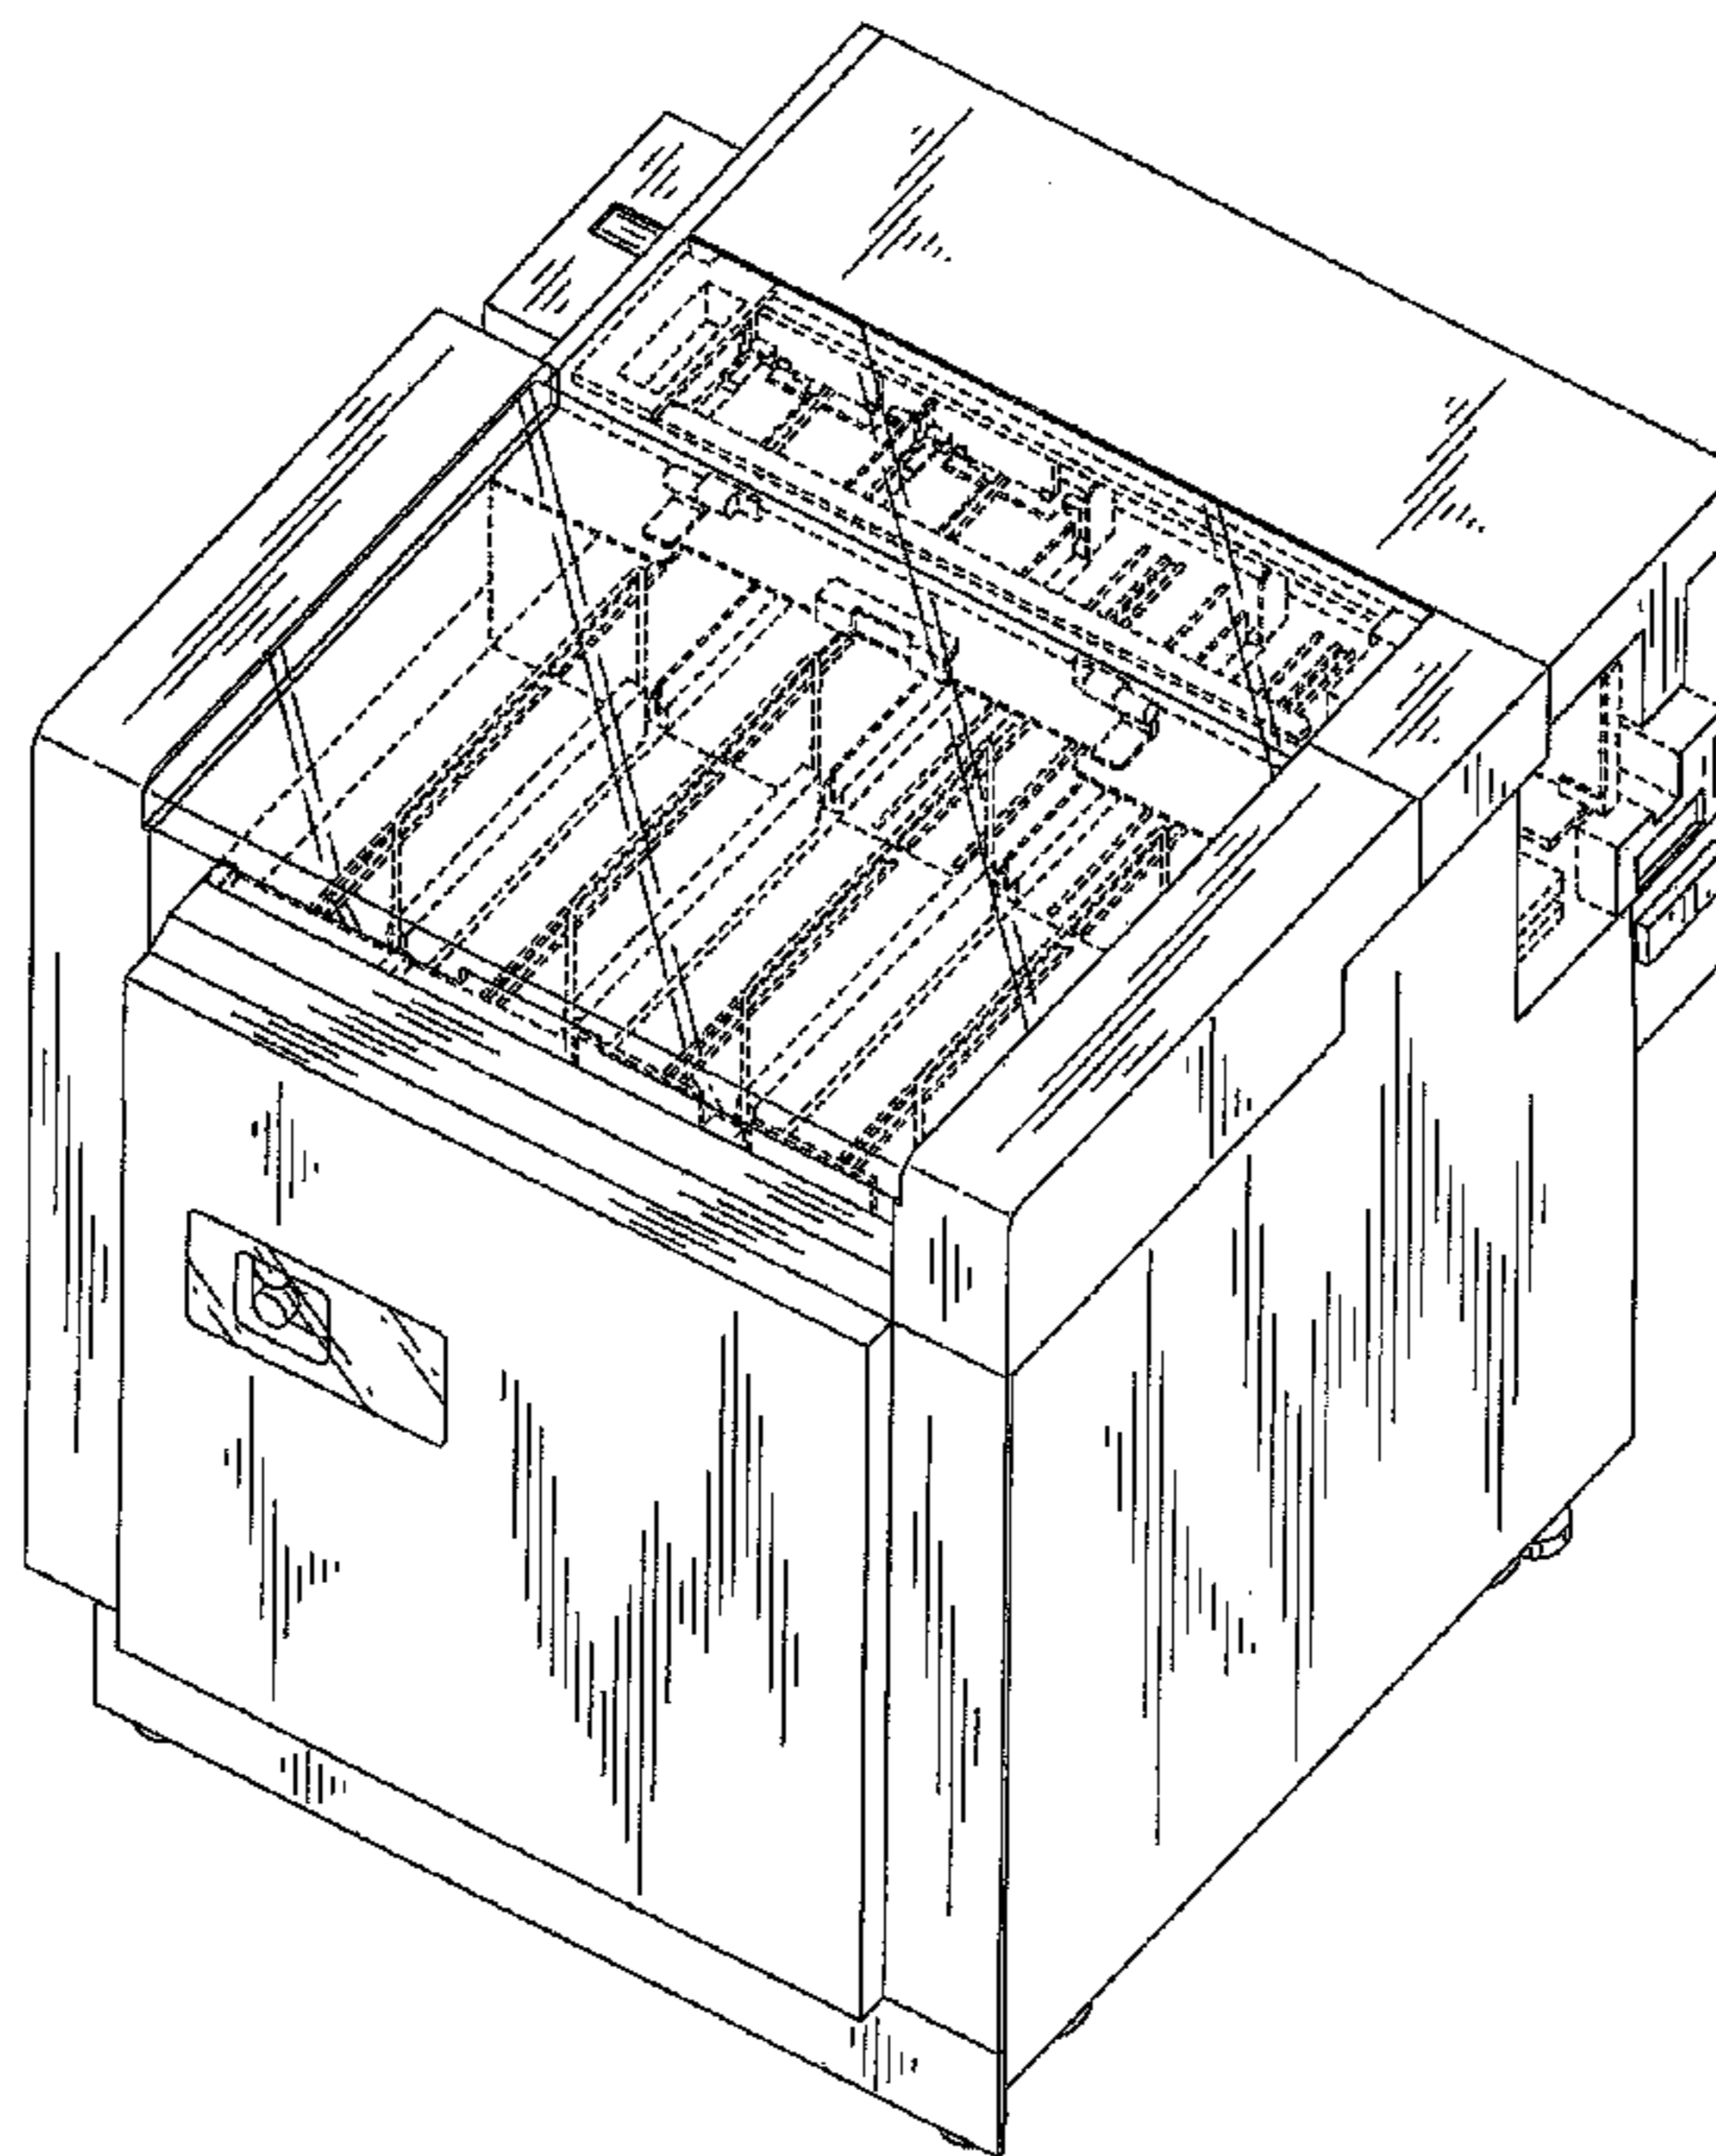

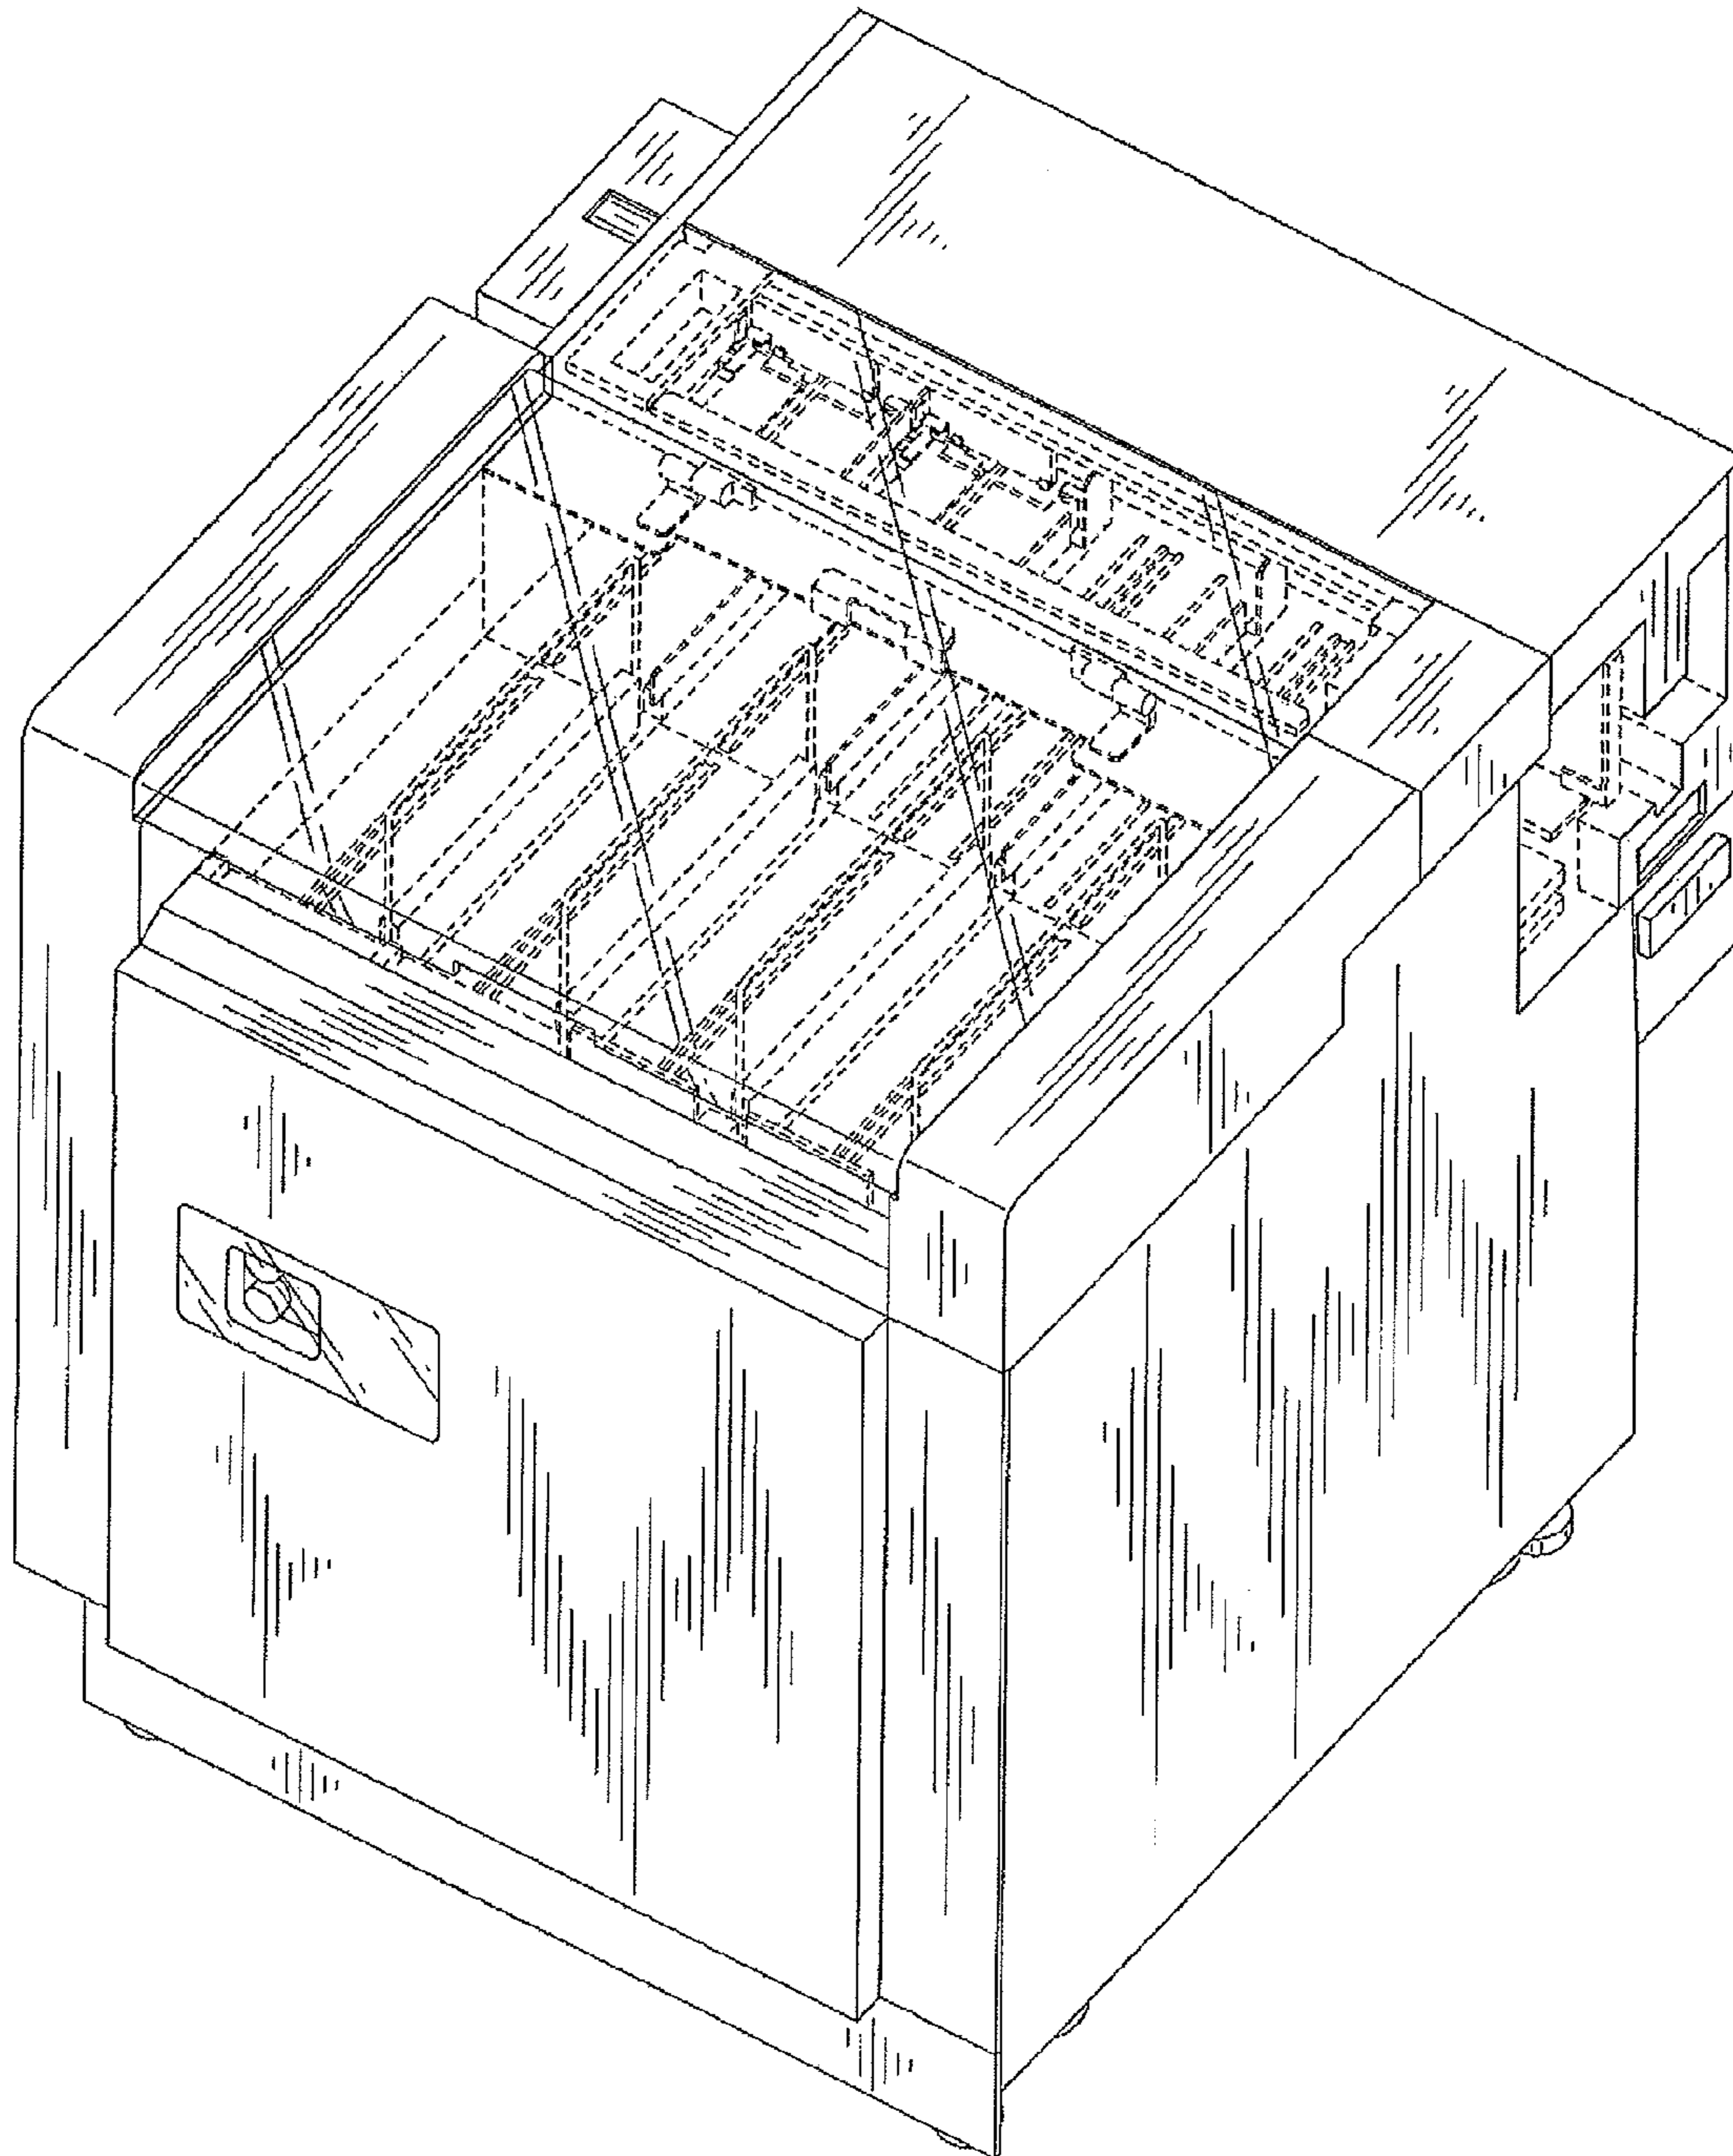


FIG. 1

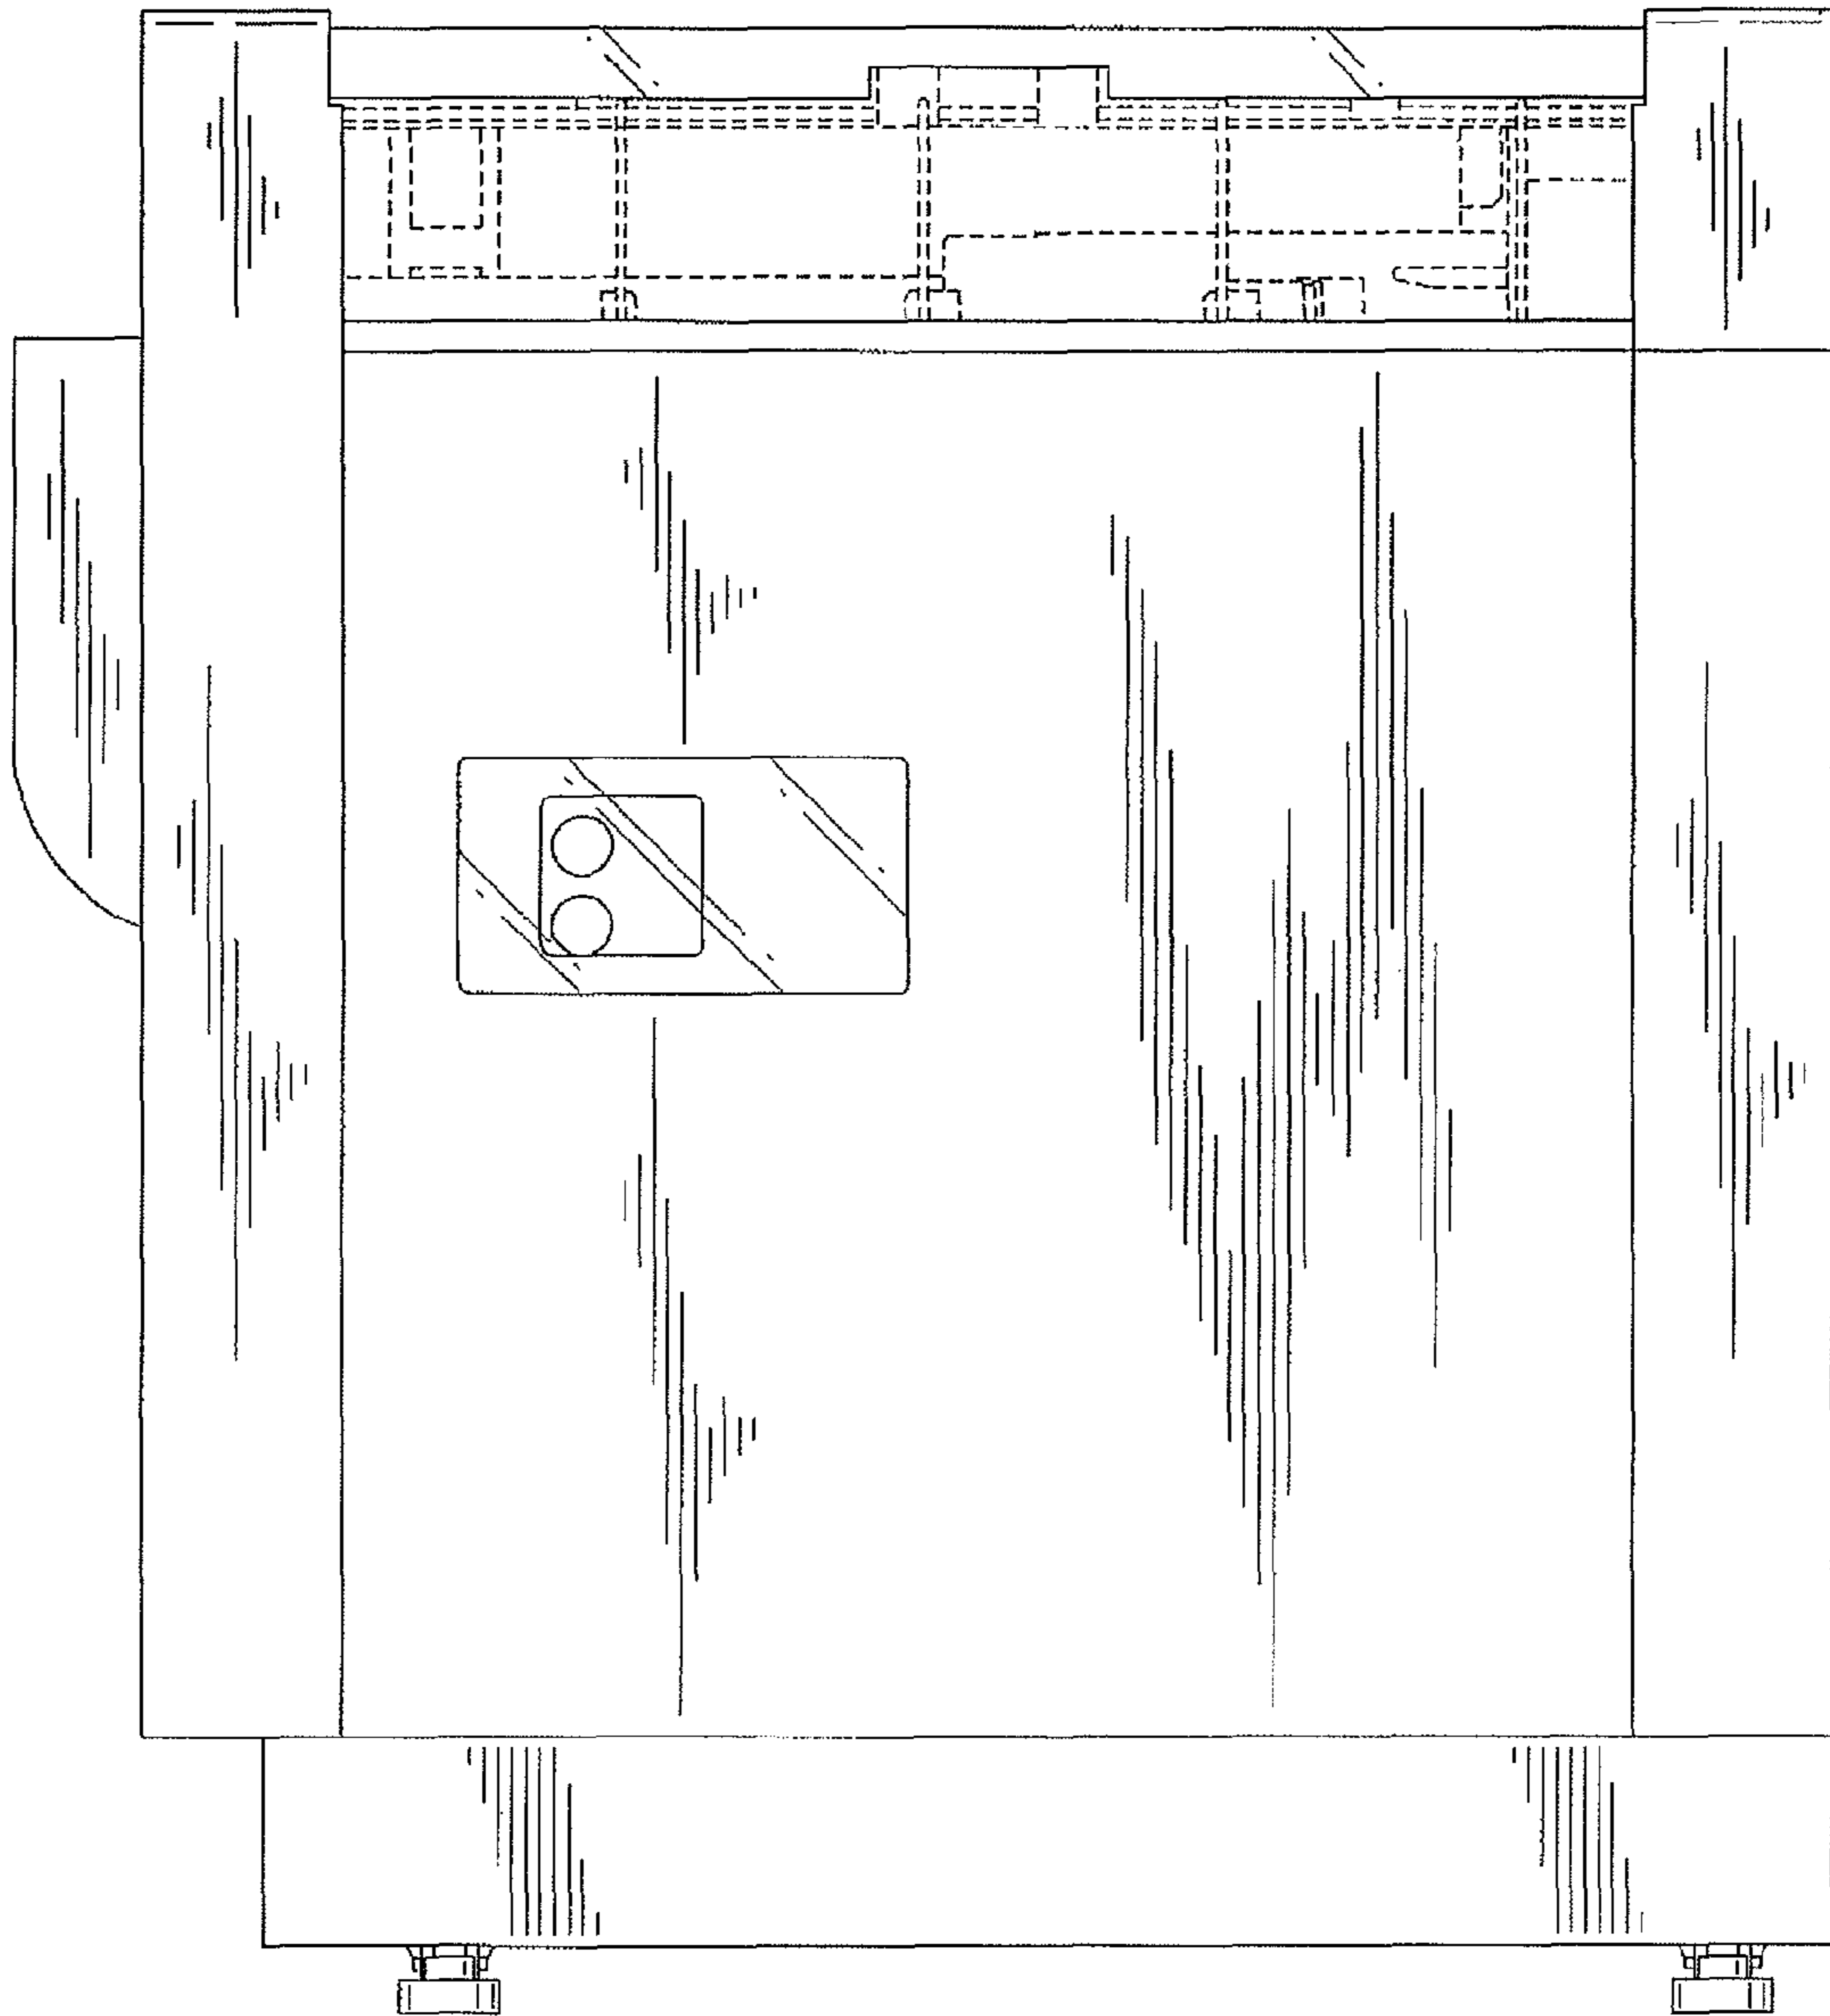


FIG. 2

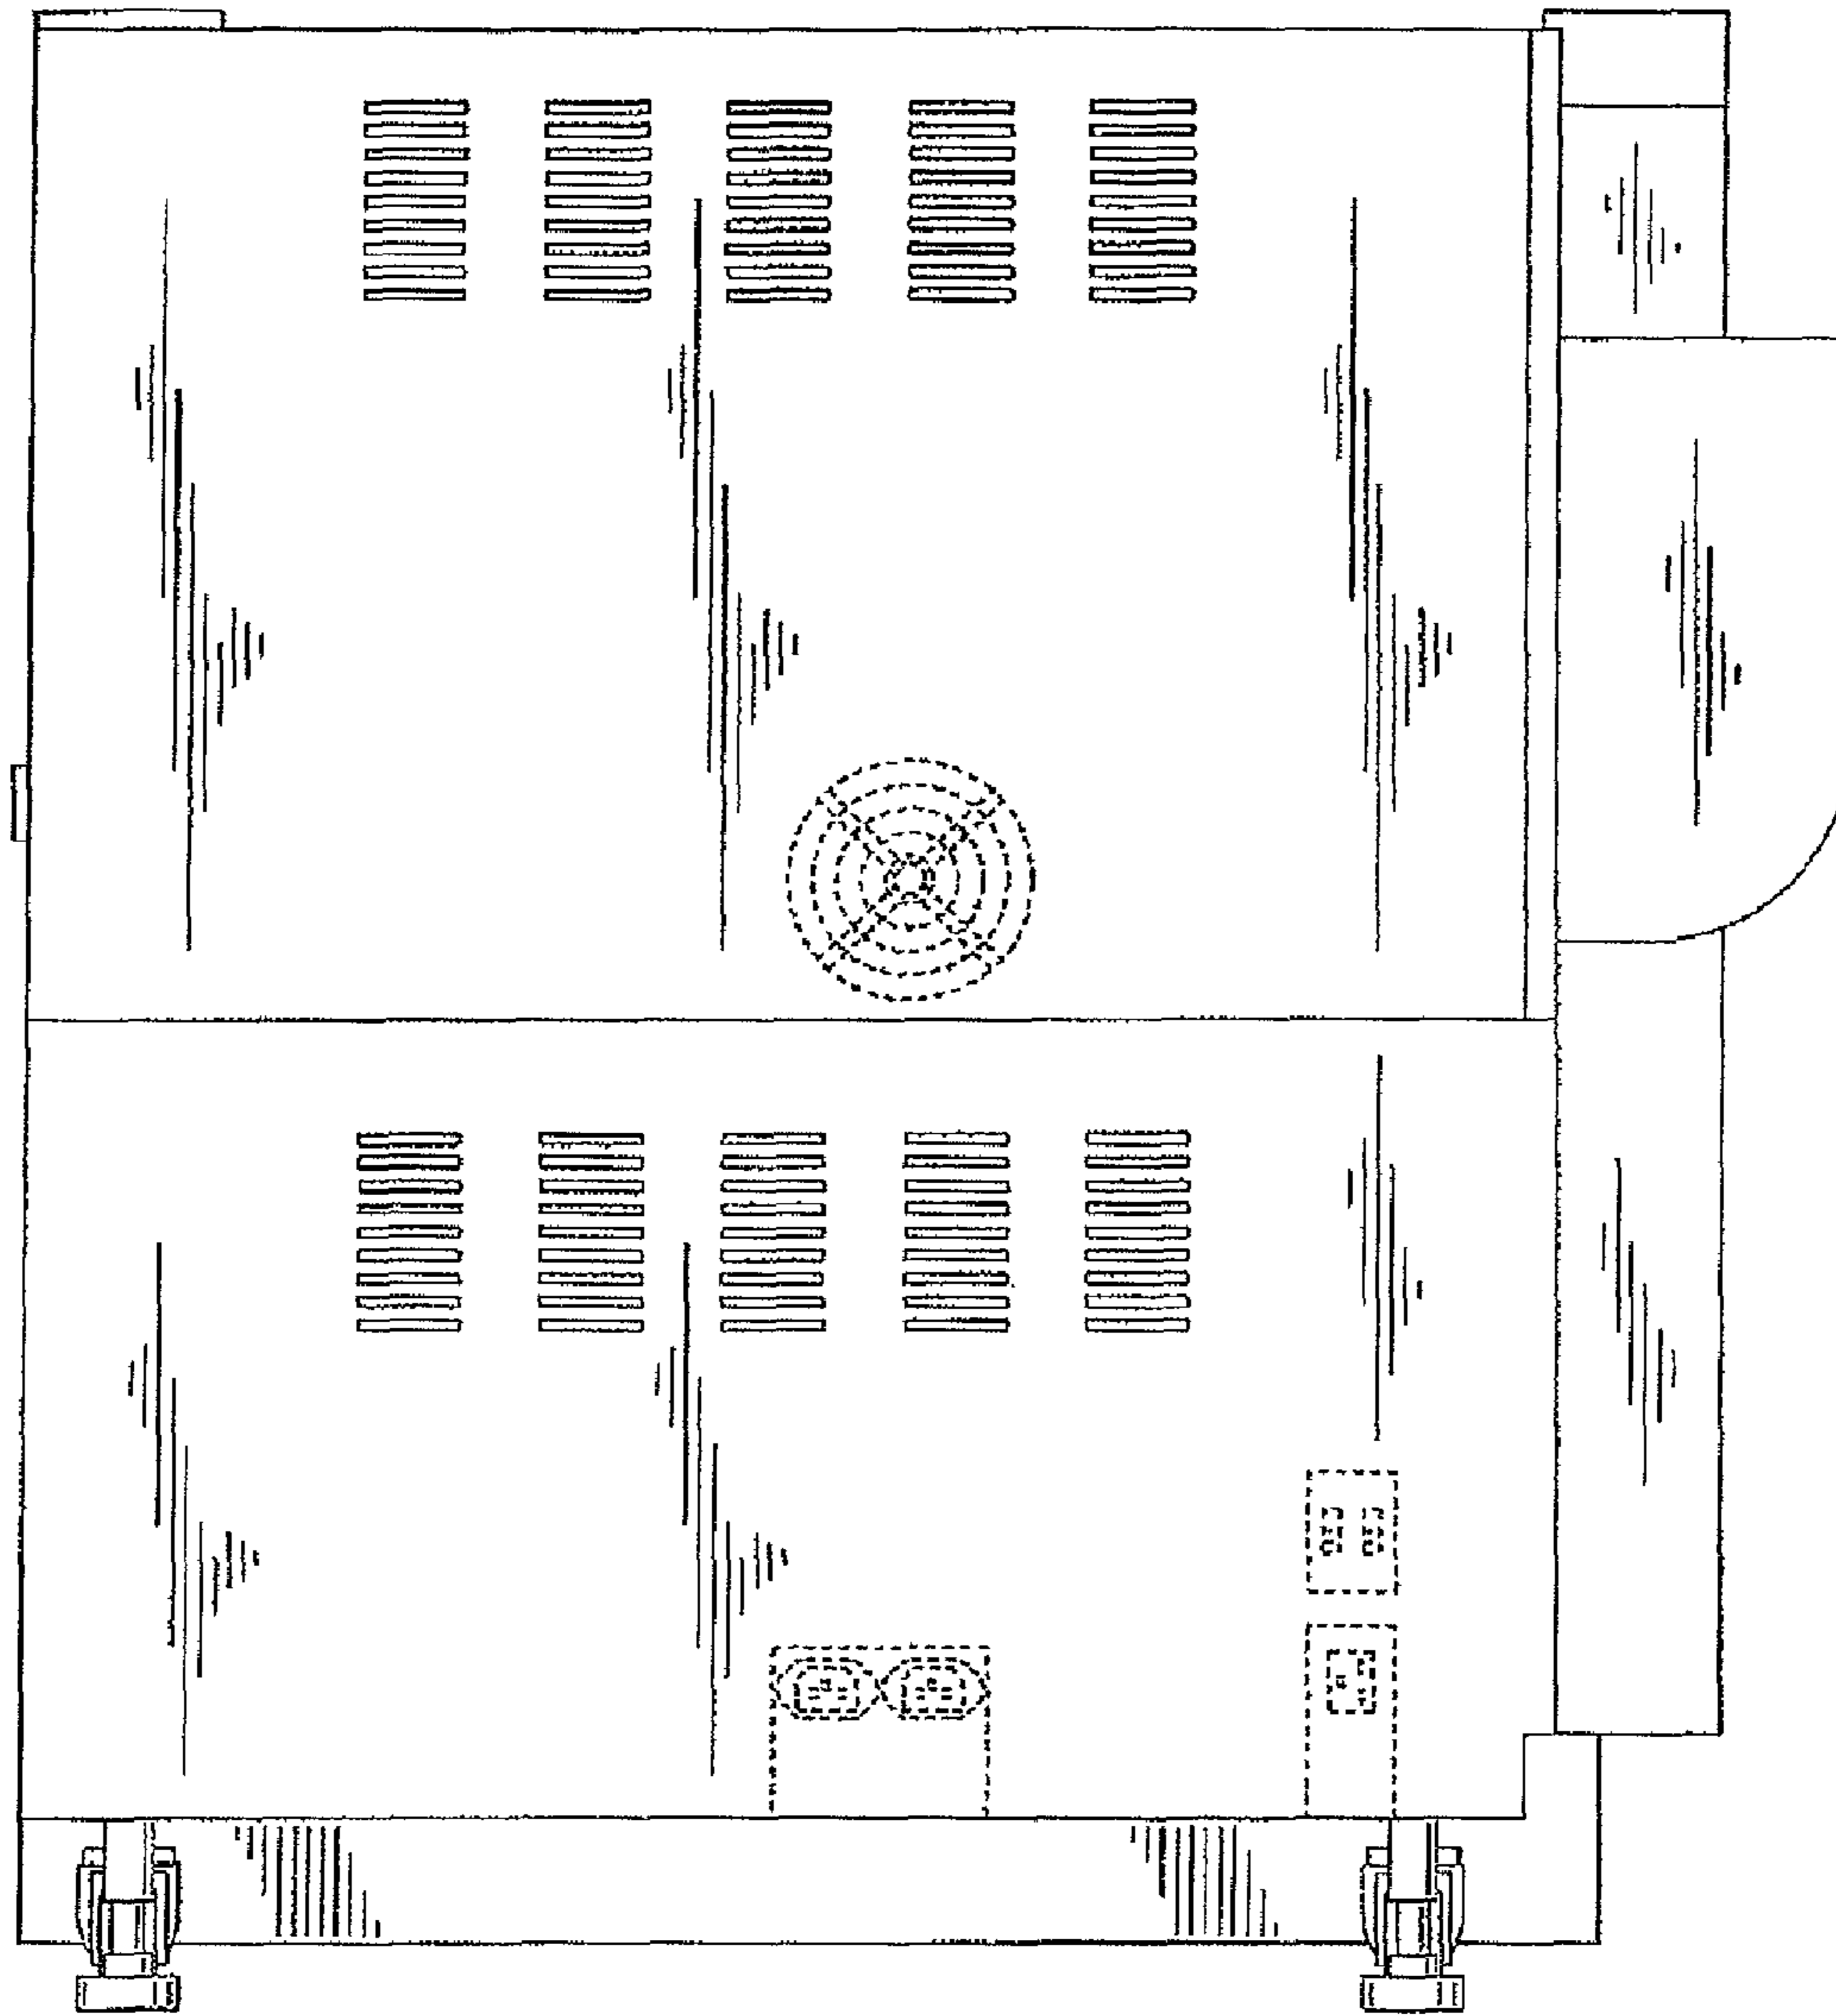


FIG. 3

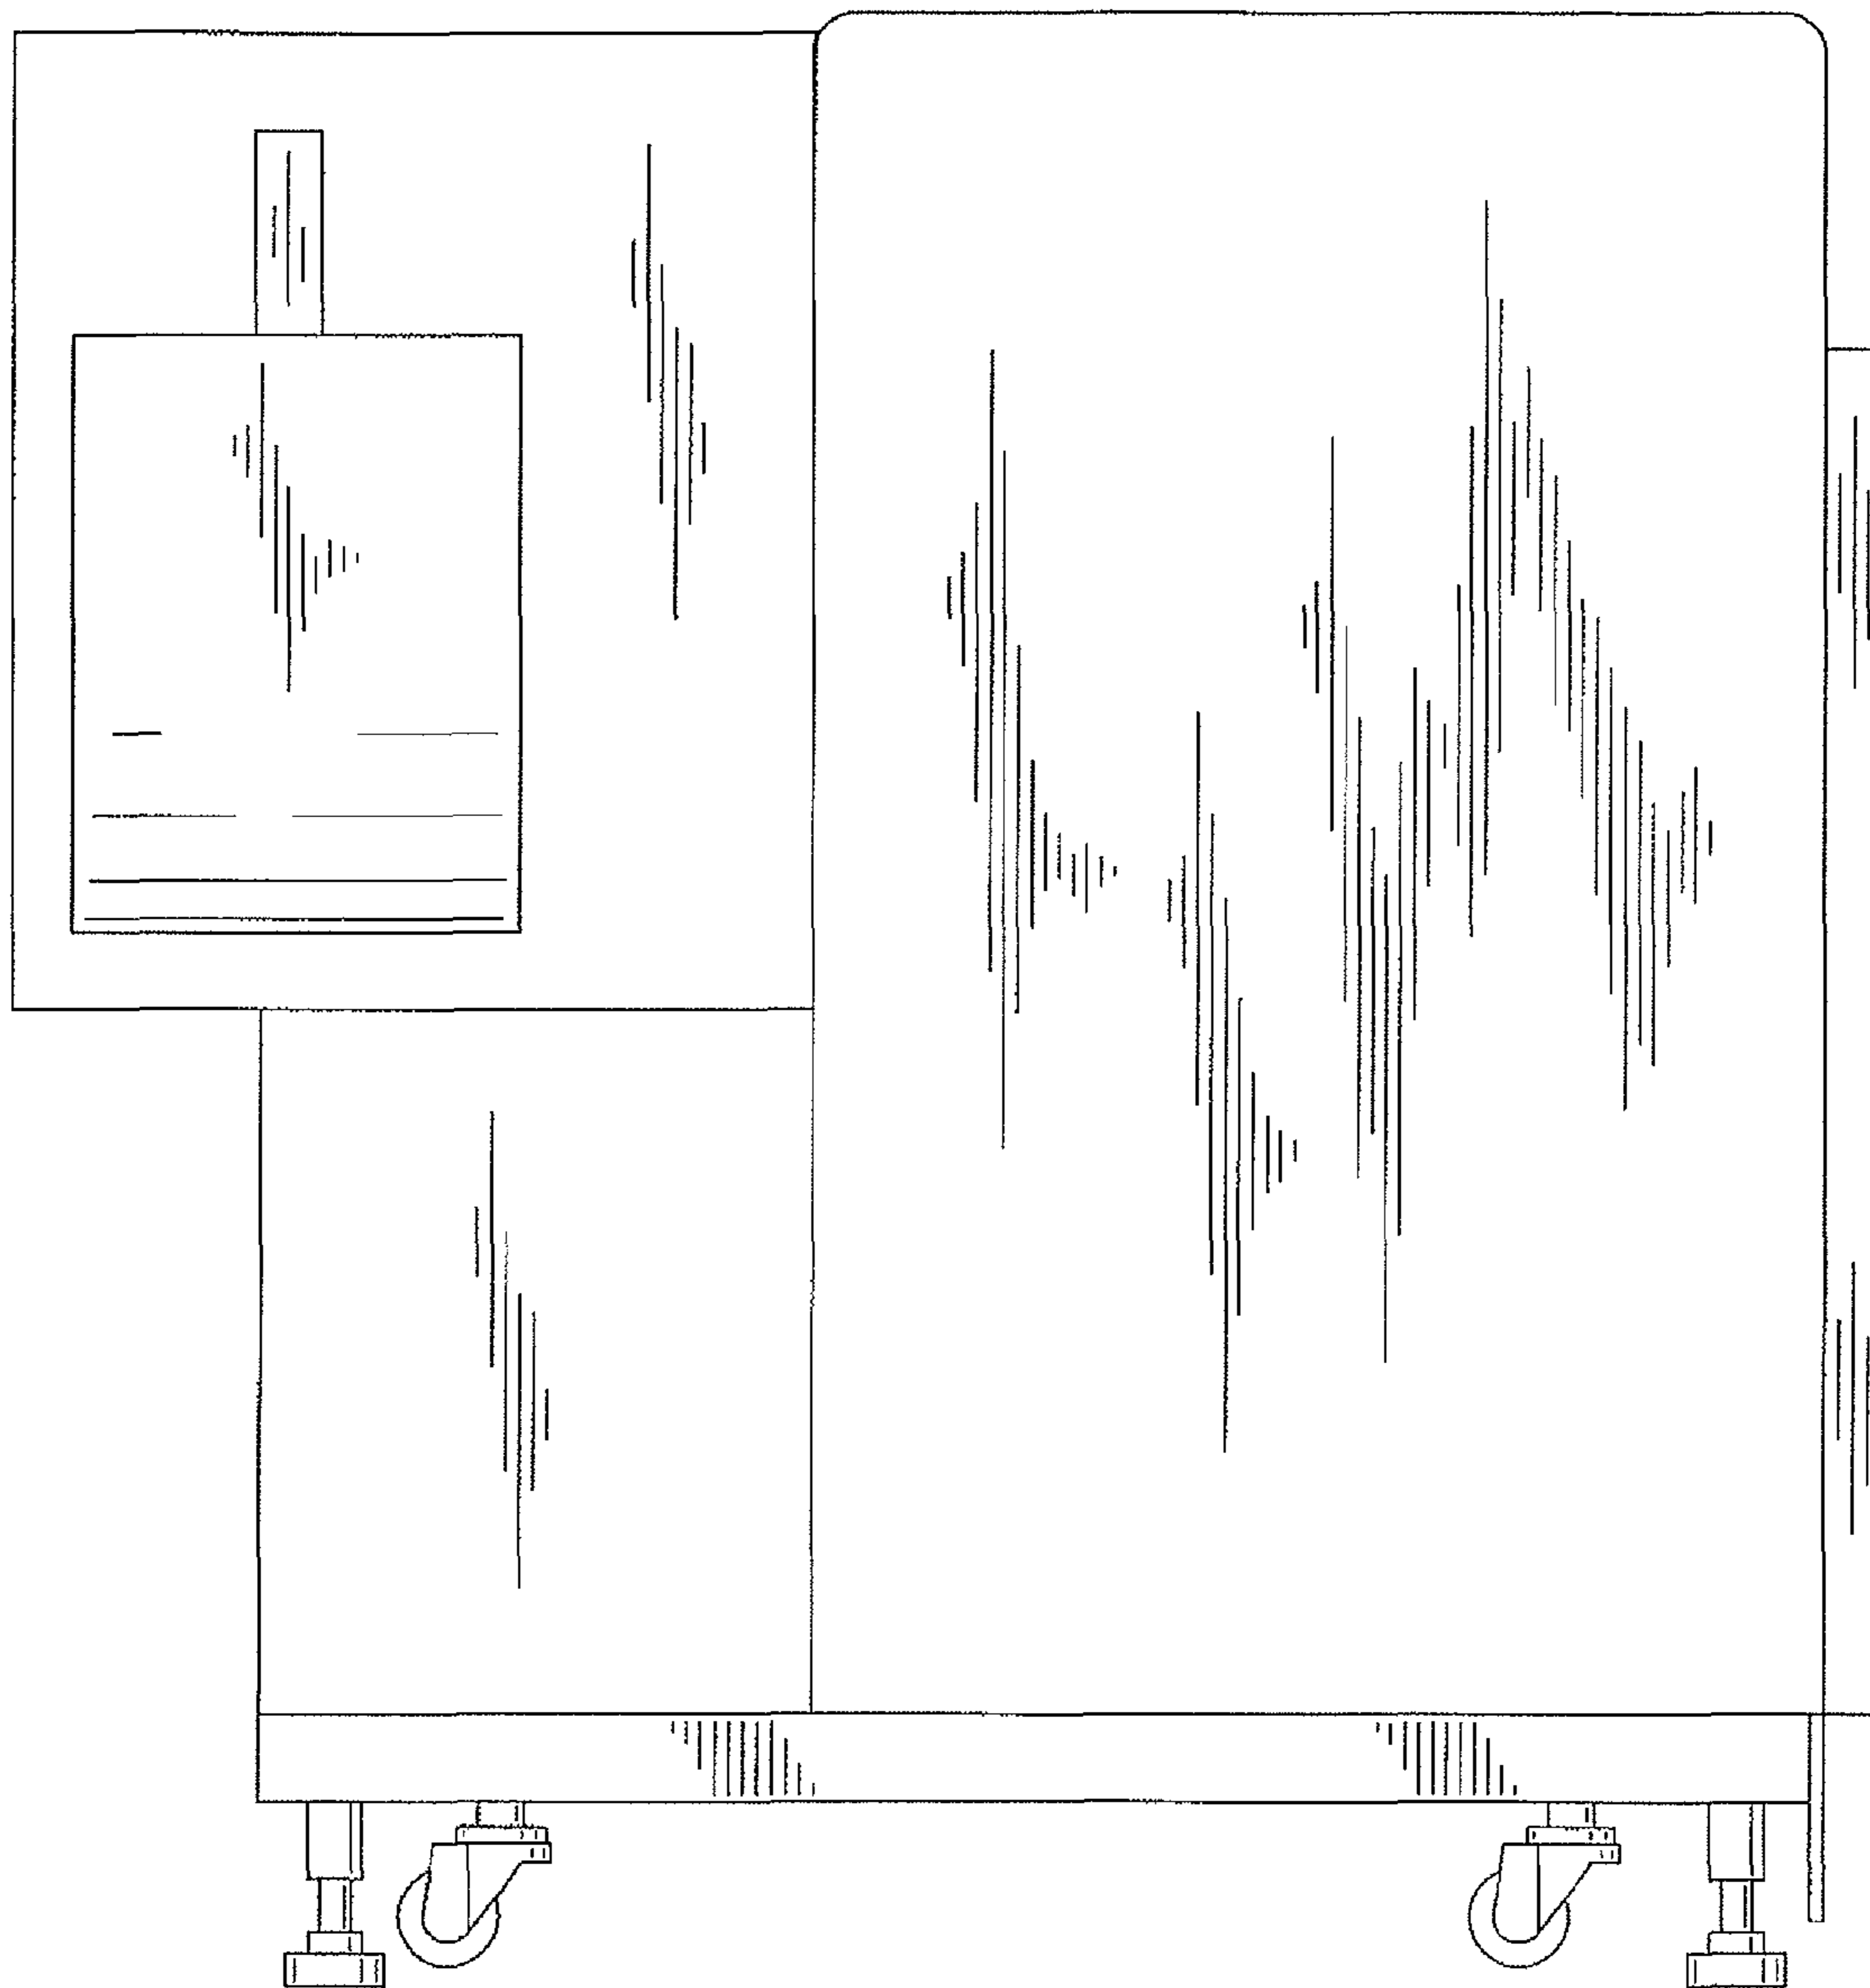


FIG. 4

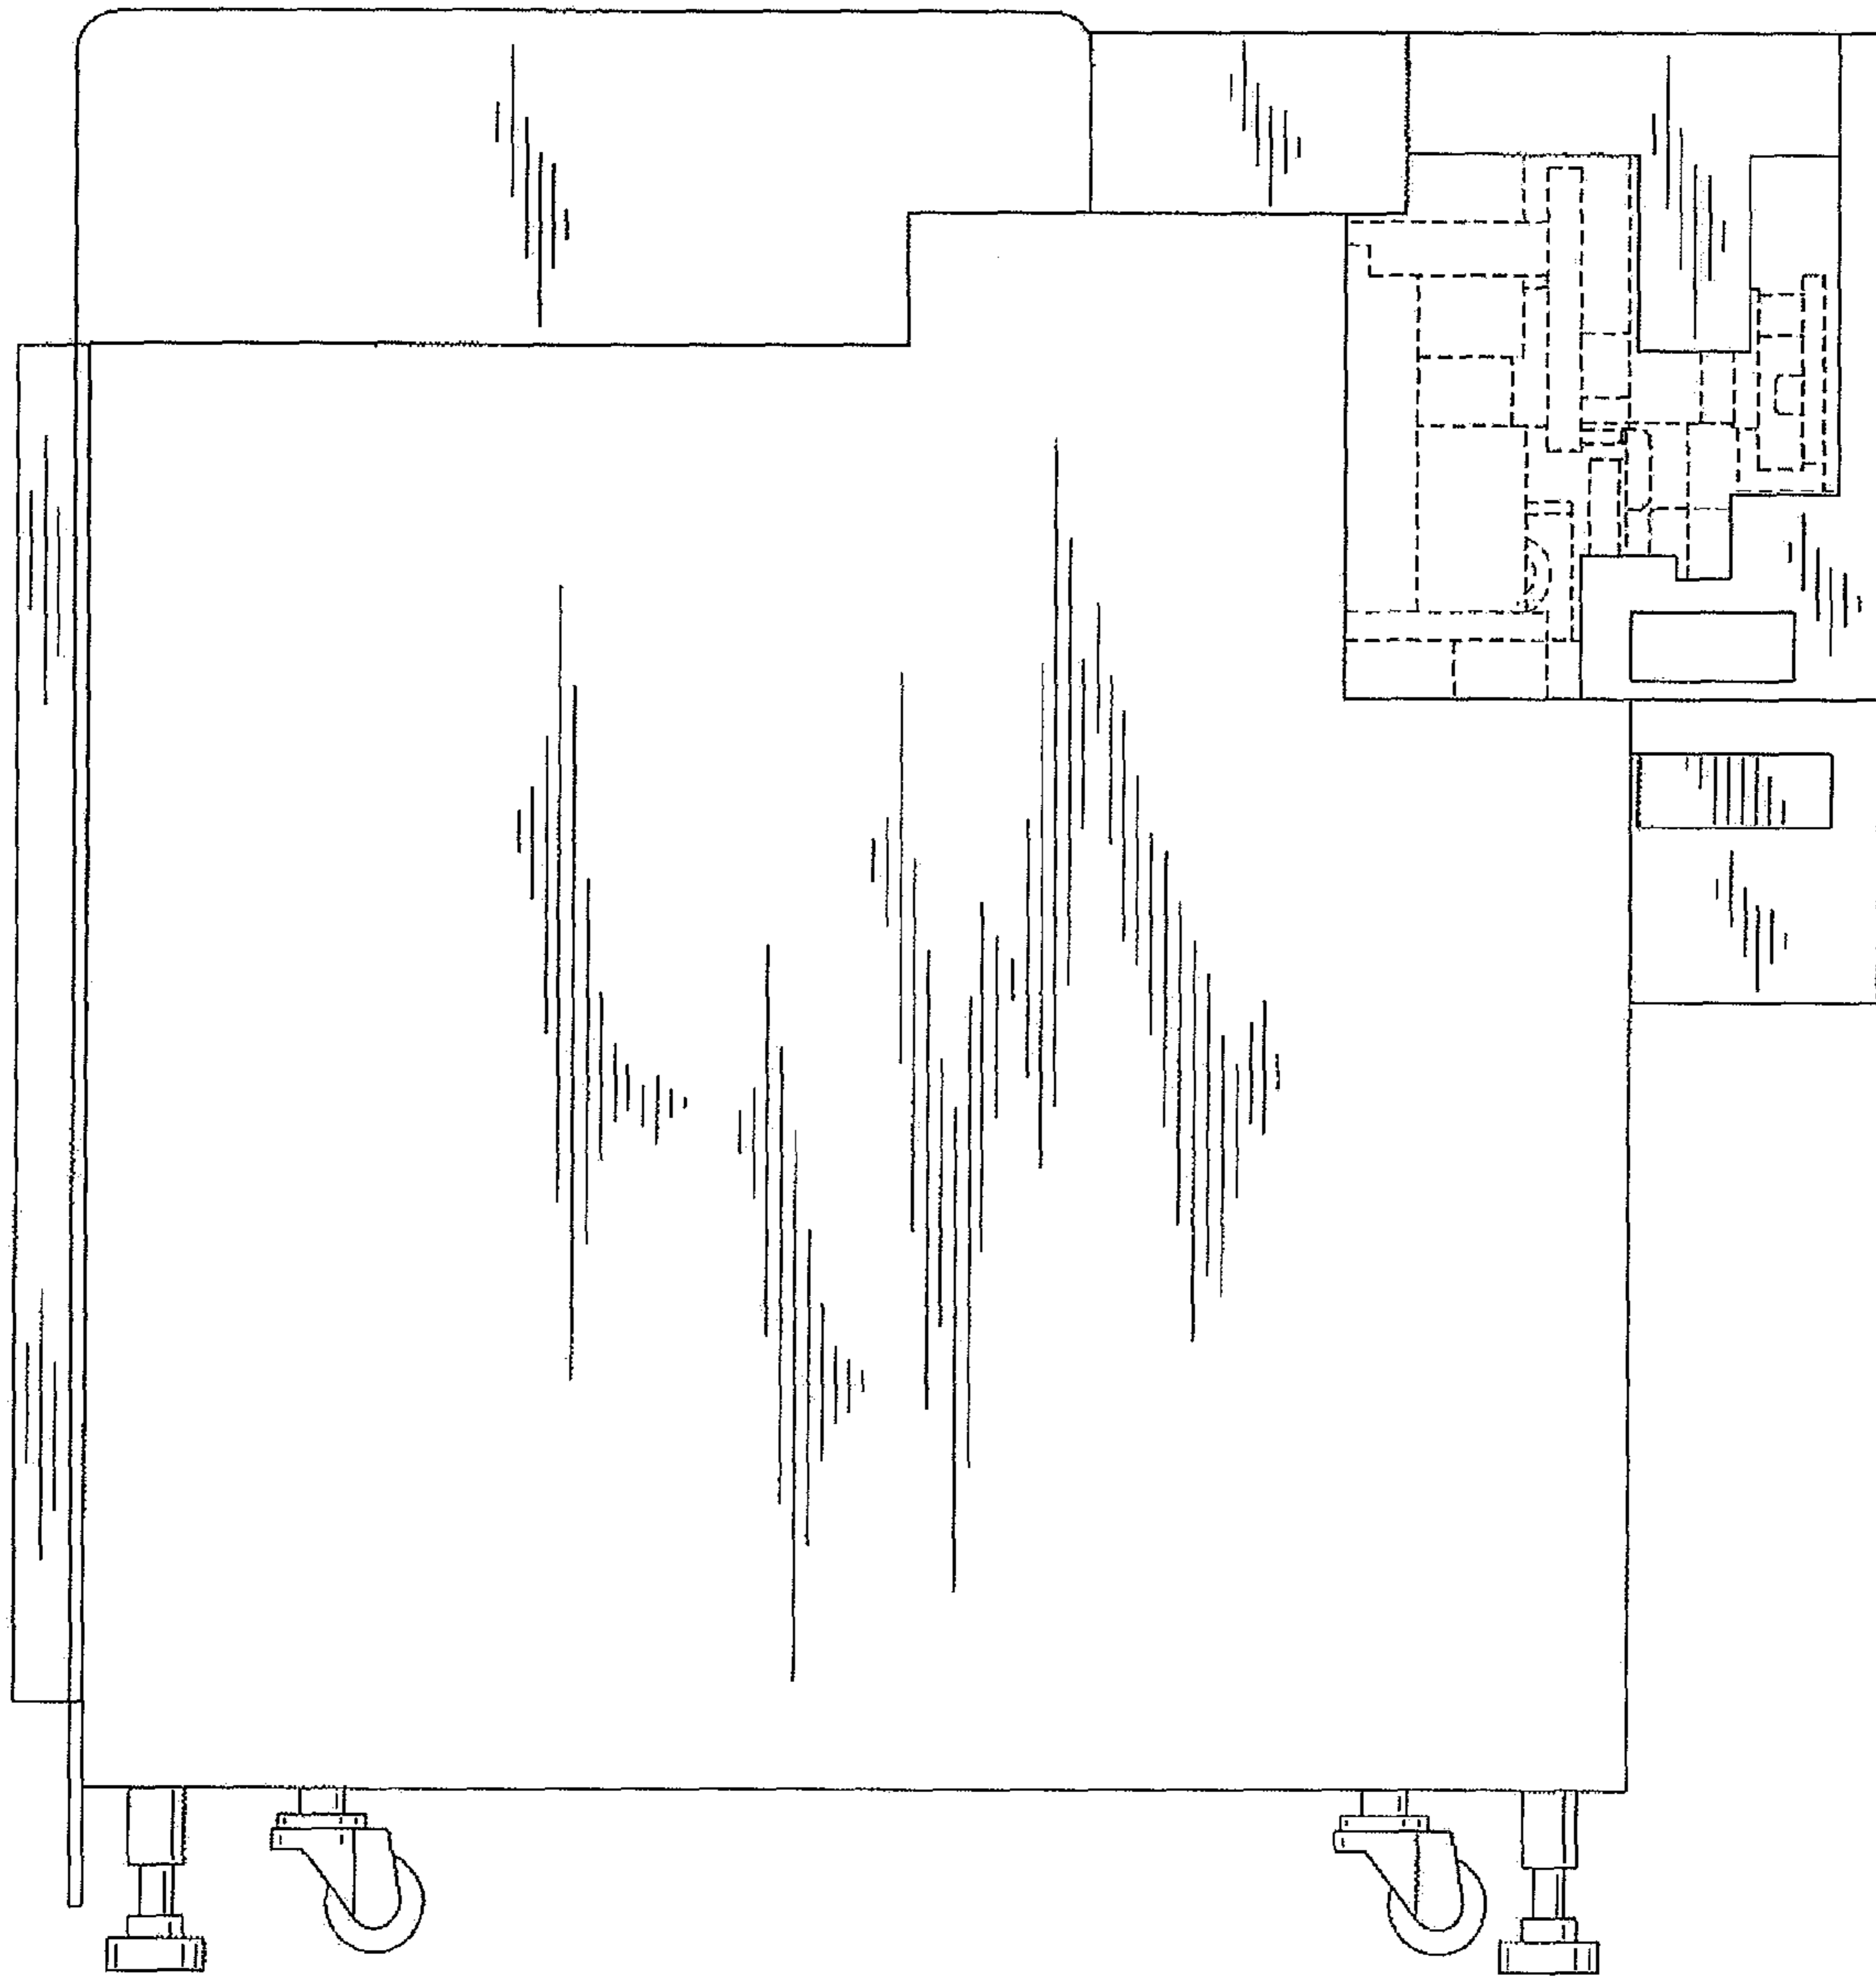


FIG. 5

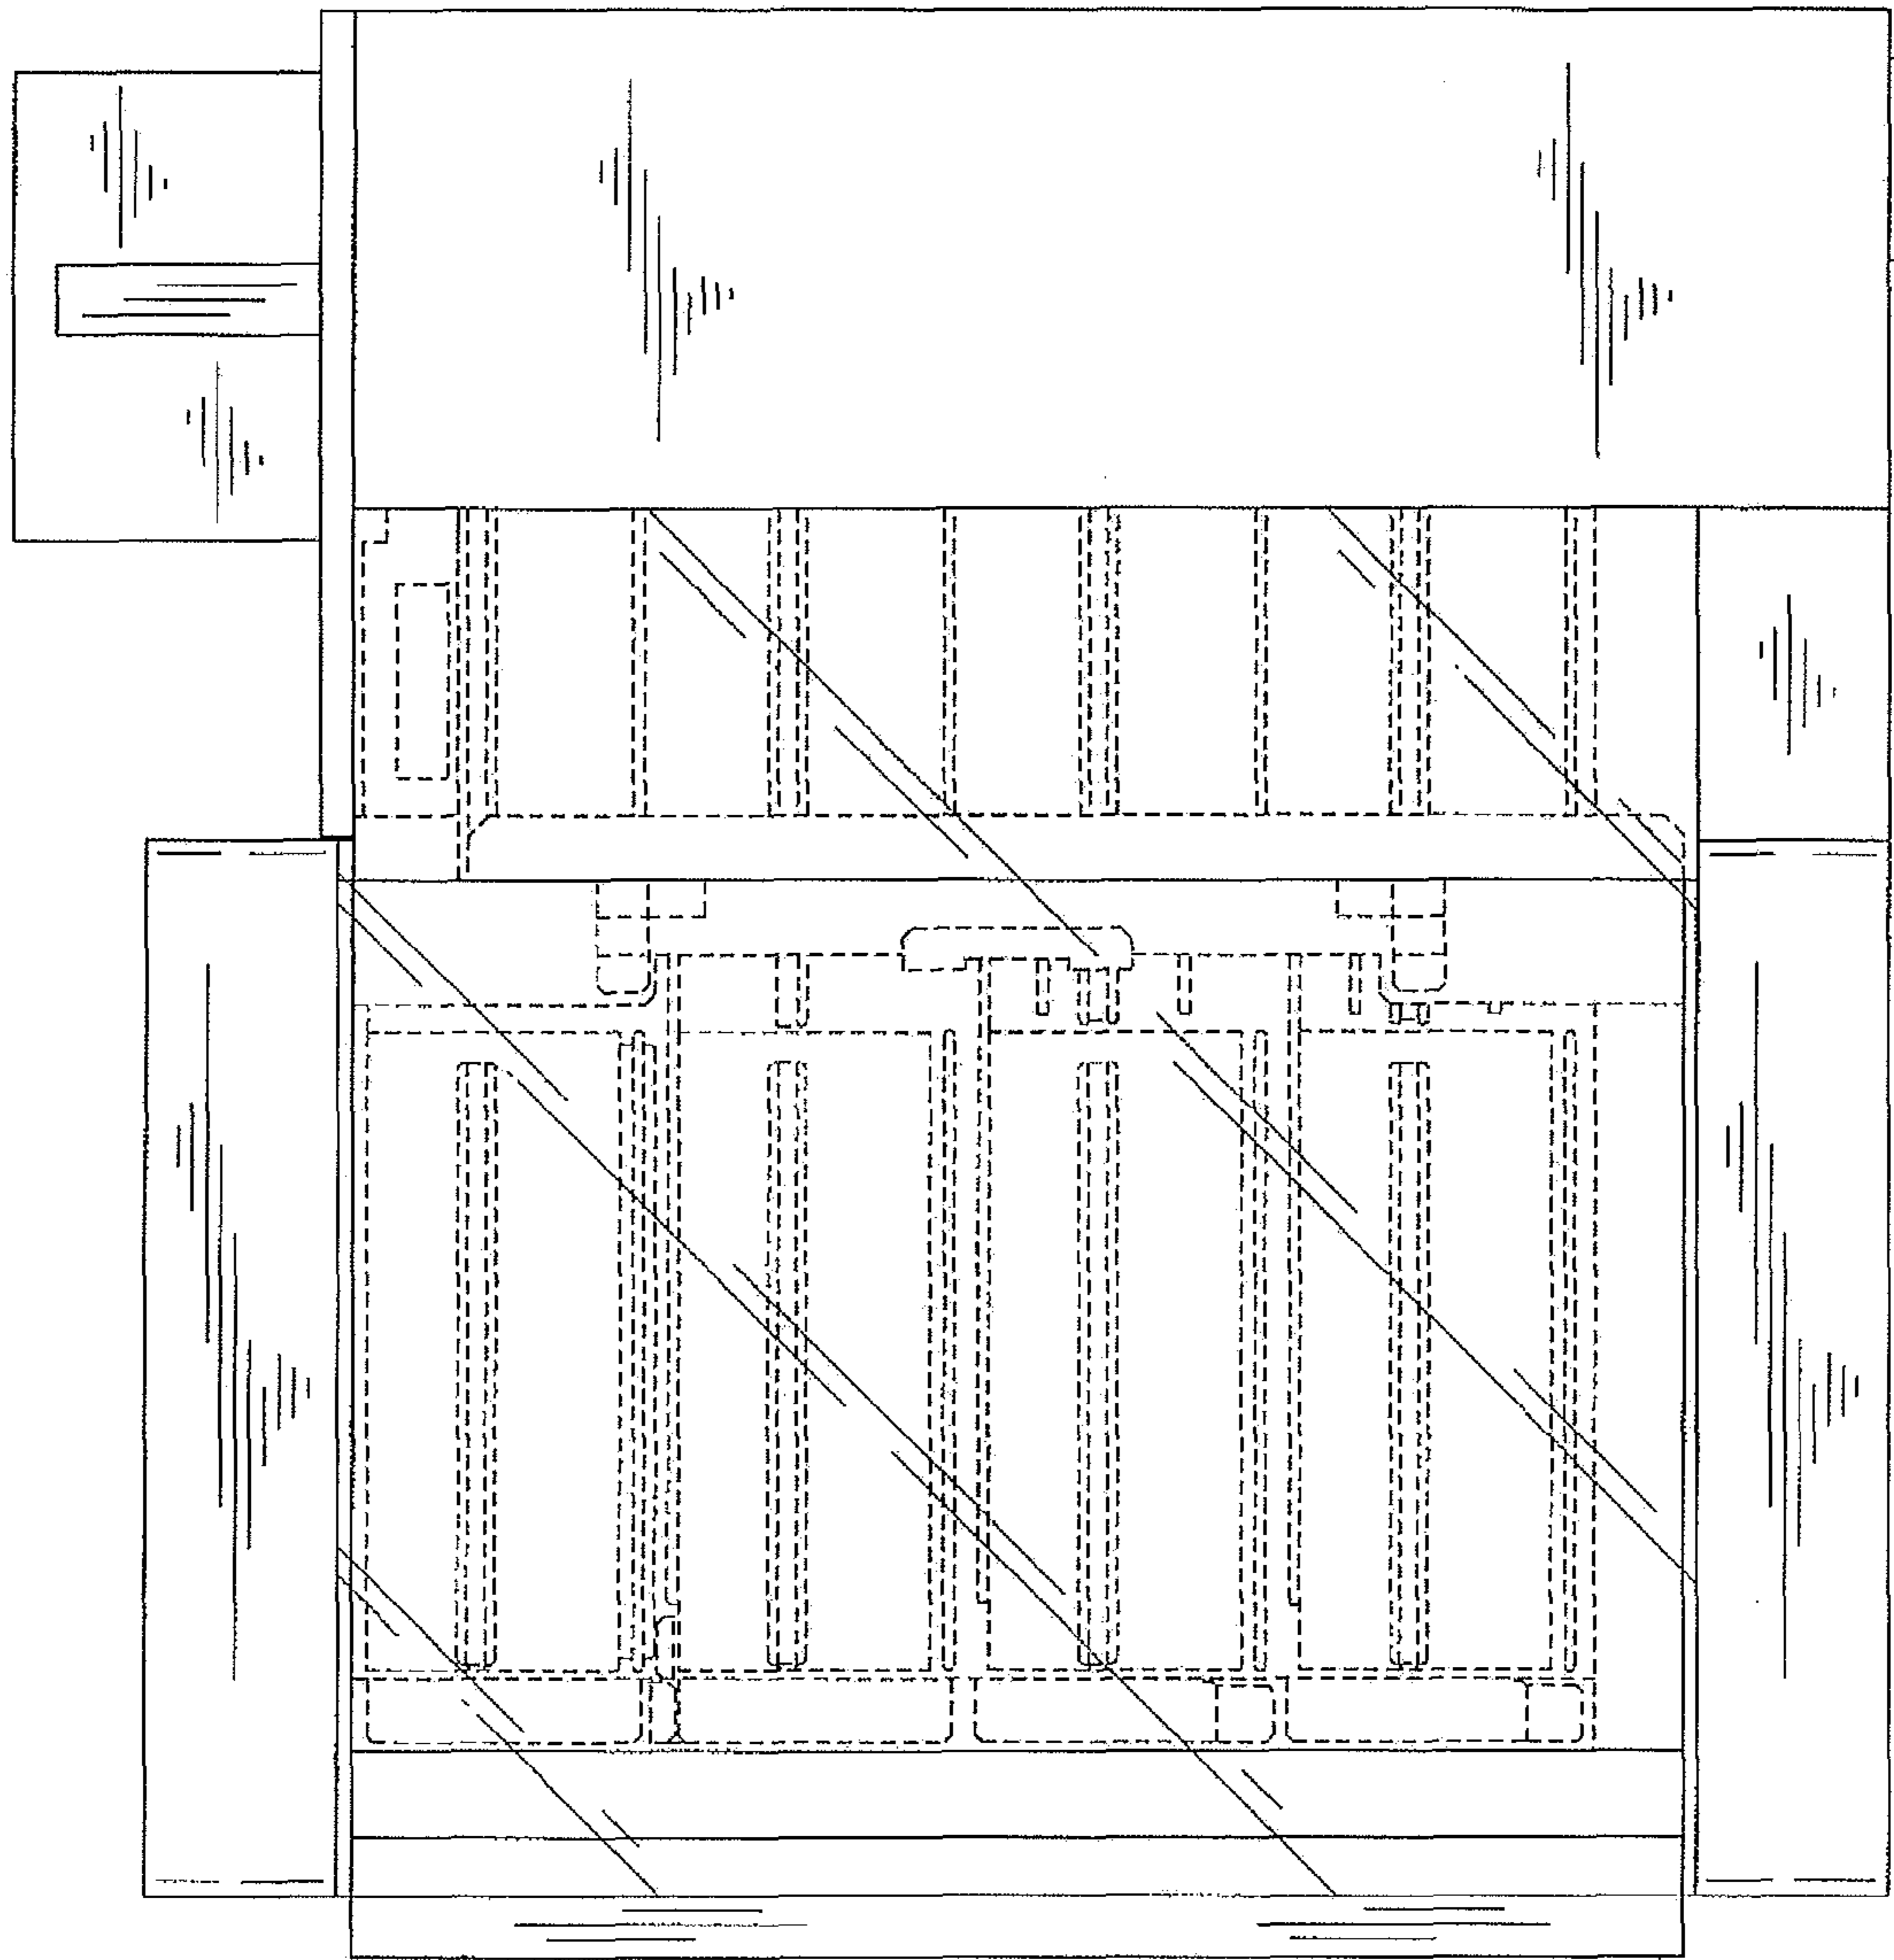


FIG. 6

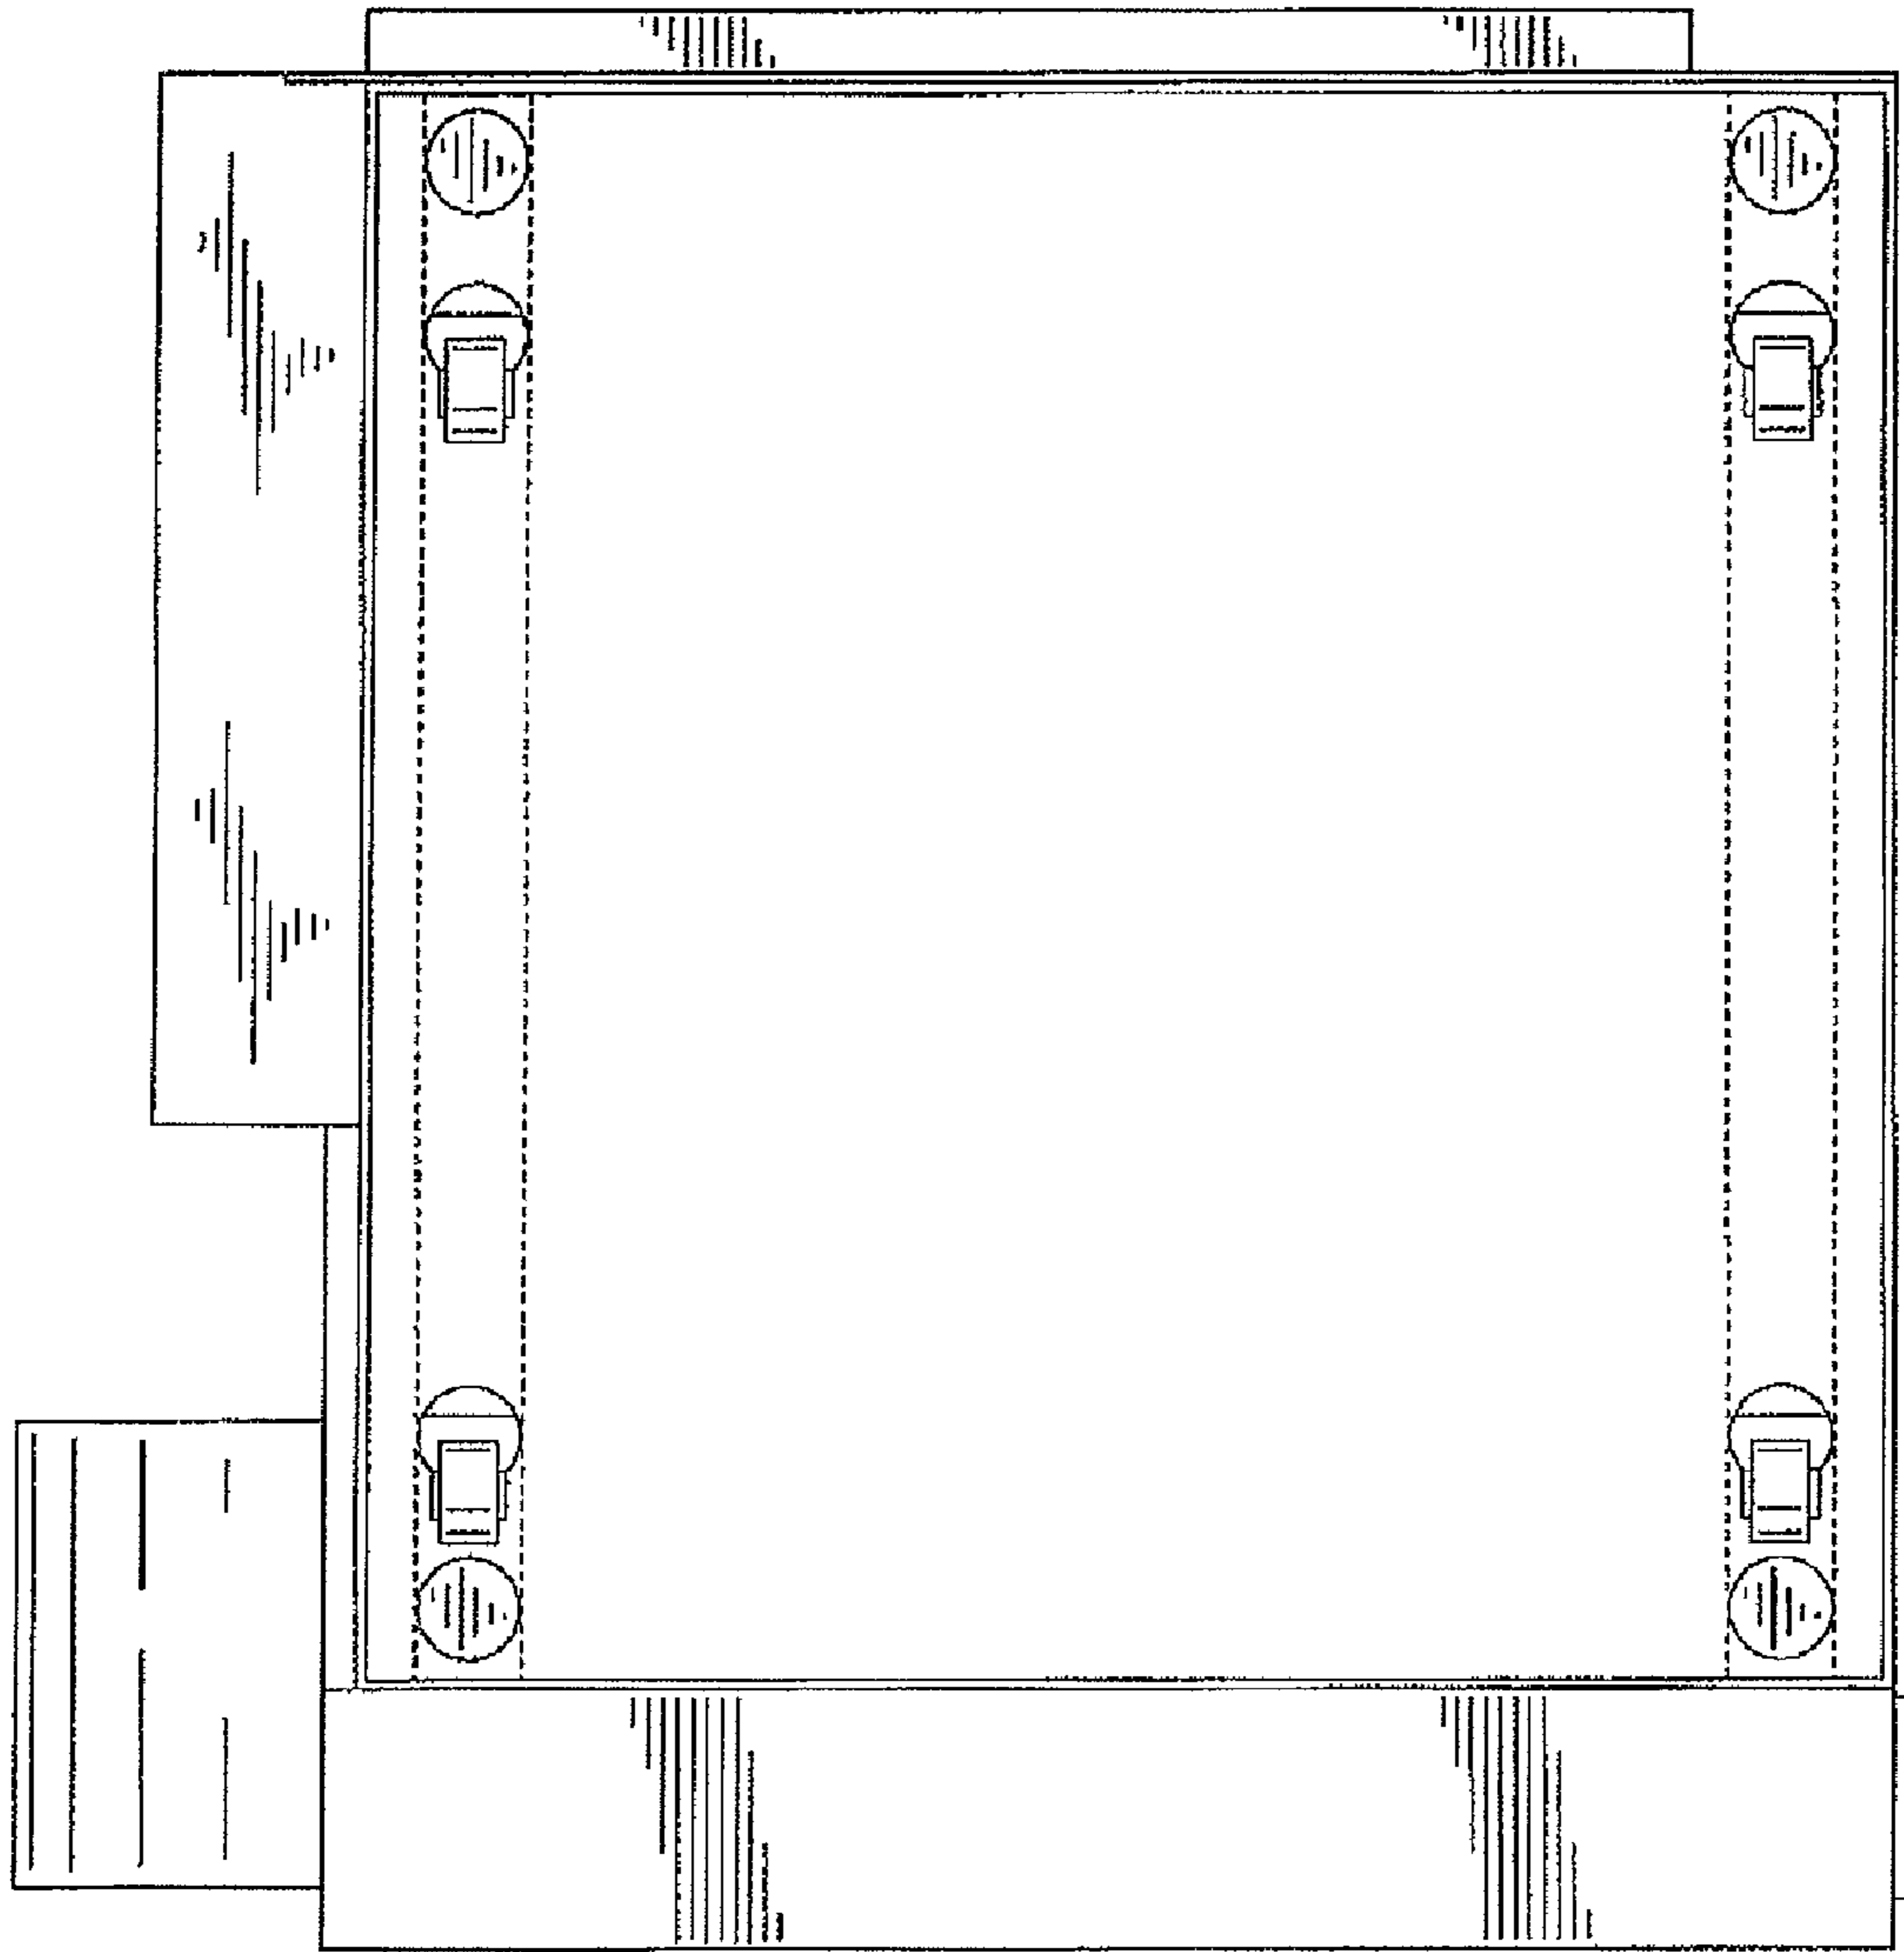


FIG. 7