



US00D634631S

(12) **United States Design Patent**
Taylor

(10) **Patent No.:** **US D634,631 S**
(45) **Date of Patent:** **** Mar. 22, 2011**

- (54) **NOZZLE AND COLLAR**
 - (75) Inventor: **Kurt M. Taylor**, Fort Collins, CO (US)
 - (73) Assignee: **Water Pik, Inc.**, Fort Collins, CO (US)
 - (**) Term: **14 Years**
 - (21) Appl. No.: **29/352,101**
 - (22) Filed: **Dec. 16, 2009**
 - (51) **LOC (9) Cl.** **09-07**
 - (52) **U.S. Cl.** **D9/447**
 - (58) **Field of Classification Search** D9/724,
D9/454, 453, 449, 448, 447, 435, 434, 418;
D28/7; D24/129, 115; 604/414, 411, 403;
422/103; 239/327; 222/522, 211, 209, 109;
221/63; 220/254.1-254.4; 215/247; 206/824;
141/329
- See application file for complete search history.

- D314,702 S * 2/1991 Gonzalez D9/667
- D317,940 S * 7/1991 Brenner D19/41
- 5,316,054 A 5/1994 Hall et al.
- 5,330,634 A 7/1994 Wong et al.
- 5,354,849 A 10/1994 Schoefberger
- 5,806,723 A 9/1998 DuBose
- D405,525 S 2/1999 Barrett et al.
- 5,897,872 A 4/1999 Picciano

(Continued)

FOREIGN PATENT DOCUMENTS

DE 29602605 4/1996

(Continued)

OTHER PUBLICATIONS

Author Unknown, "NasaFlo Neti Pot," <http://www.neilmed.com/usa/nasaflo.php>, 1 page, at least as early as Dec. 9, 2009.

(Continued)

Primary Examiner — Susan Bennett Hattan

(74) *Attorney, Agent, or Firm* — Dorsey & Whitney LLP

(56) **References Cited**

U.S. PATENT DOCUMENTS

- 2,115,959 A 5/1938 Lewis
- 2,571,921 A 10/1951 Morris
- 2,578,864 A 12/1951 Tupper
- D169,996 S * 7/1953 Vuilleumet D24/115
- 2,811,283 A 10/1957 Bowen
- 3,363,808 A 1/1968 Gorman
- 3,847,145 A 11/1974 Grossan
- 4,083,840 A 4/1978 Schoefberger
- D250,546 S 12/1978 Pick et al.
- D250,601 S 12/1978 Pick et al.
- 4,356,941 A 11/1982 McRoskey et al.
- D271,028 S * 10/1983 Adams D19/55
- 4,439,206 A 3/1984 Hildebrand et al.
- 4,489,535 A 12/1984 Veltman
- 4,513,891 A 4/1985 Hain et al.
- 4,555,469 A 11/1985 Erdmann et al.
- D305,262 S 12/1989 Nichols
- 4,925,128 A 5/1990 Brody

(57) **CLAIM**

The ornamental design for a nozzle and collar, as shown and described.

DESCRIPTION


FIG. 1 is a front isometric view of a nozzle and collar of the present invention;

FIG. 2 is a top plan view of the nozzle and collar of FIG. 1; FIG. 3 is a side elevation view of the nozzle and collar of FIG. 1, with the front, back and other side elevation views being the same; and,

FIG. 4 is a bottom plan view of the nozzle and collar of FIG. 1.

The broken lines in the drawings depict environmental subject matter only and form no part of the claimed design.

1 Claim, 3 Drawing Sheets

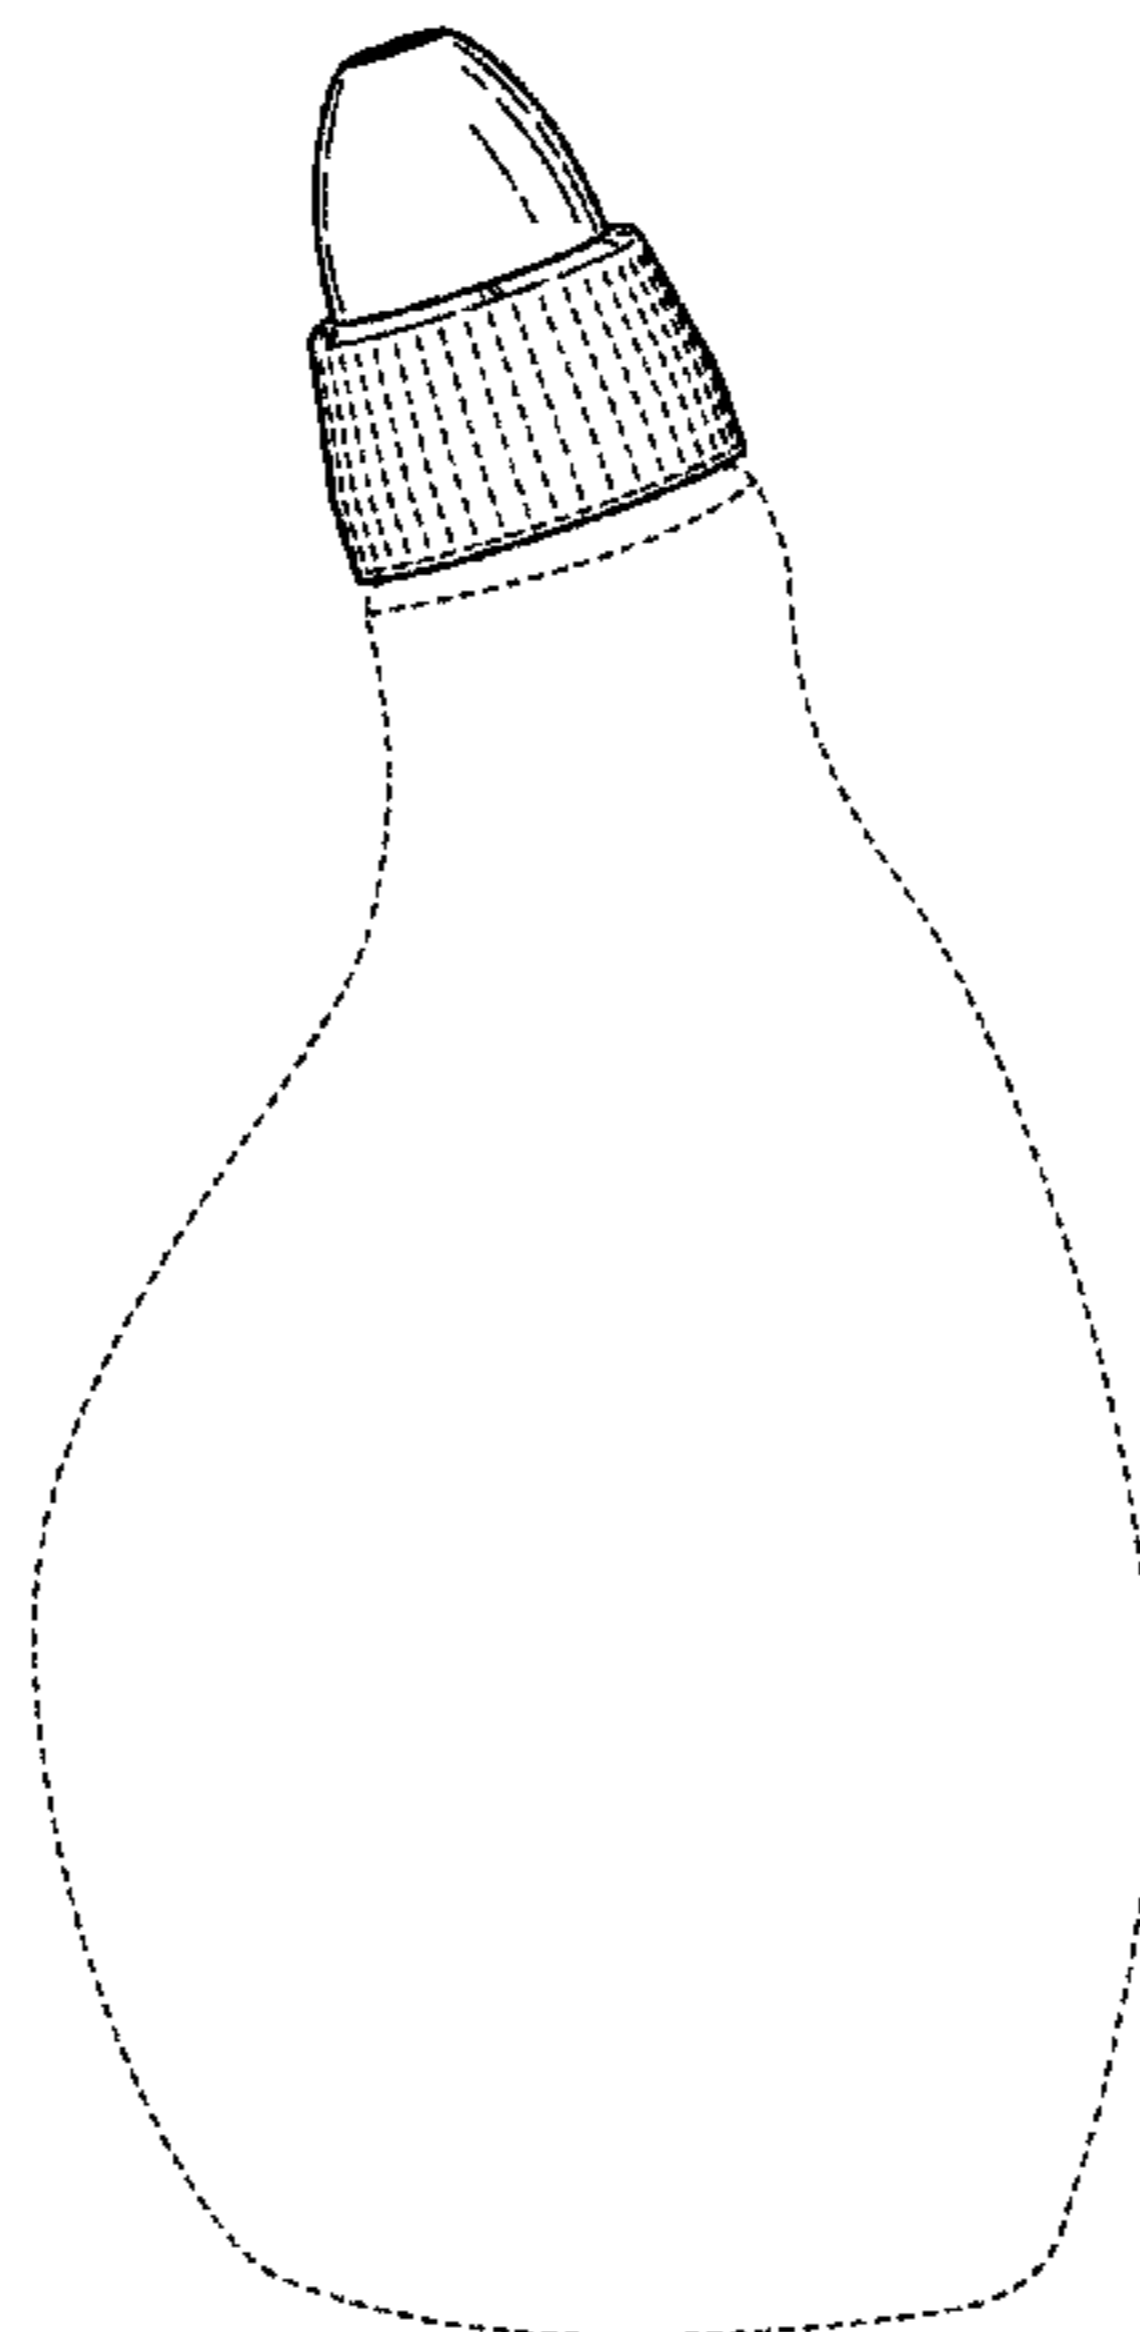

US D634,631 S

Page 2

U.S. PATENT DOCUMENTS

5,899,878 A 5/1999 Glassman
5,967,377 A 10/1999 Glynn
D424,197 S 5/2000 Sydlowski et al.
D426,300 S 6/2000 Conforti
6,238,377 B1 5/2001 Liu
6,293,436 B2 9/2001 Faughnder et al.
6,520,384 B2 2/2003 Mehta
6,669,059 B2 12/2003 Mehta
6,688,497 B2 2/2004 Mehta
6,736,792 B1 5/2004 Liu
D490,896 S 6/2004 Bogazzi
D493,888 S 8/2004 Reschke
D495,954 S 9/2004 Solomon
D497,107 S 10/2004 Hama et al.
7,306,121 B2 12/2007 Ophardt et al.
D562,404 S 2/2008 Jansen et al.
D584,151 S * 1/2009 Murphy D9/453
D590,493 S 4/2009 Harlan et al.
D608,645 S 1/2010 Handy et al.
2003/0062367 A1 * 4/2003 Robinson et al. 220/254.1
2008/0294124 A1 11/2008 Mehta

FOREIGN PATENT DOCUMENTS

GB 881807 10/1958
WO WO9629044 9/1996

OTHER PUBLICATIONS

Author Unknown, "SinuFlo Ready Rinse," <http://www.neilmed.com/usa/sinuflo.php>, 1 page, at least as early as Dec. 9, 2009.
Author Unknown, "Sinus Rinse Nasal Wash," <http://www.neilmed.com/usa/sinusrinse.php>, 3 pages, at least as early as Dec. 9, 2009.
Papsin et al., "Saline Nasal Irrigation," *Canadian Family Physician*, vol. 49, pp. 168-173, Feb. 2003.
Rabago et al., "Efficacy of Daily Hypertonic Saline Nasal Irrigation Among Patients with Sinusitis: A Randomized Controlled Trial," *The Journal of Family Practice*, vol. 51, No. 12, pp. 1049-1055, Dec. 2002.
Schumann et al., "Patients Insist on Antibiotics for Sinusitis? Here is a Good Reason to Say 'No'," *The Journal of Family Practice*, vol. 57, No. 7, pp. 464-468, Jul. 2008.

* cited by examiner

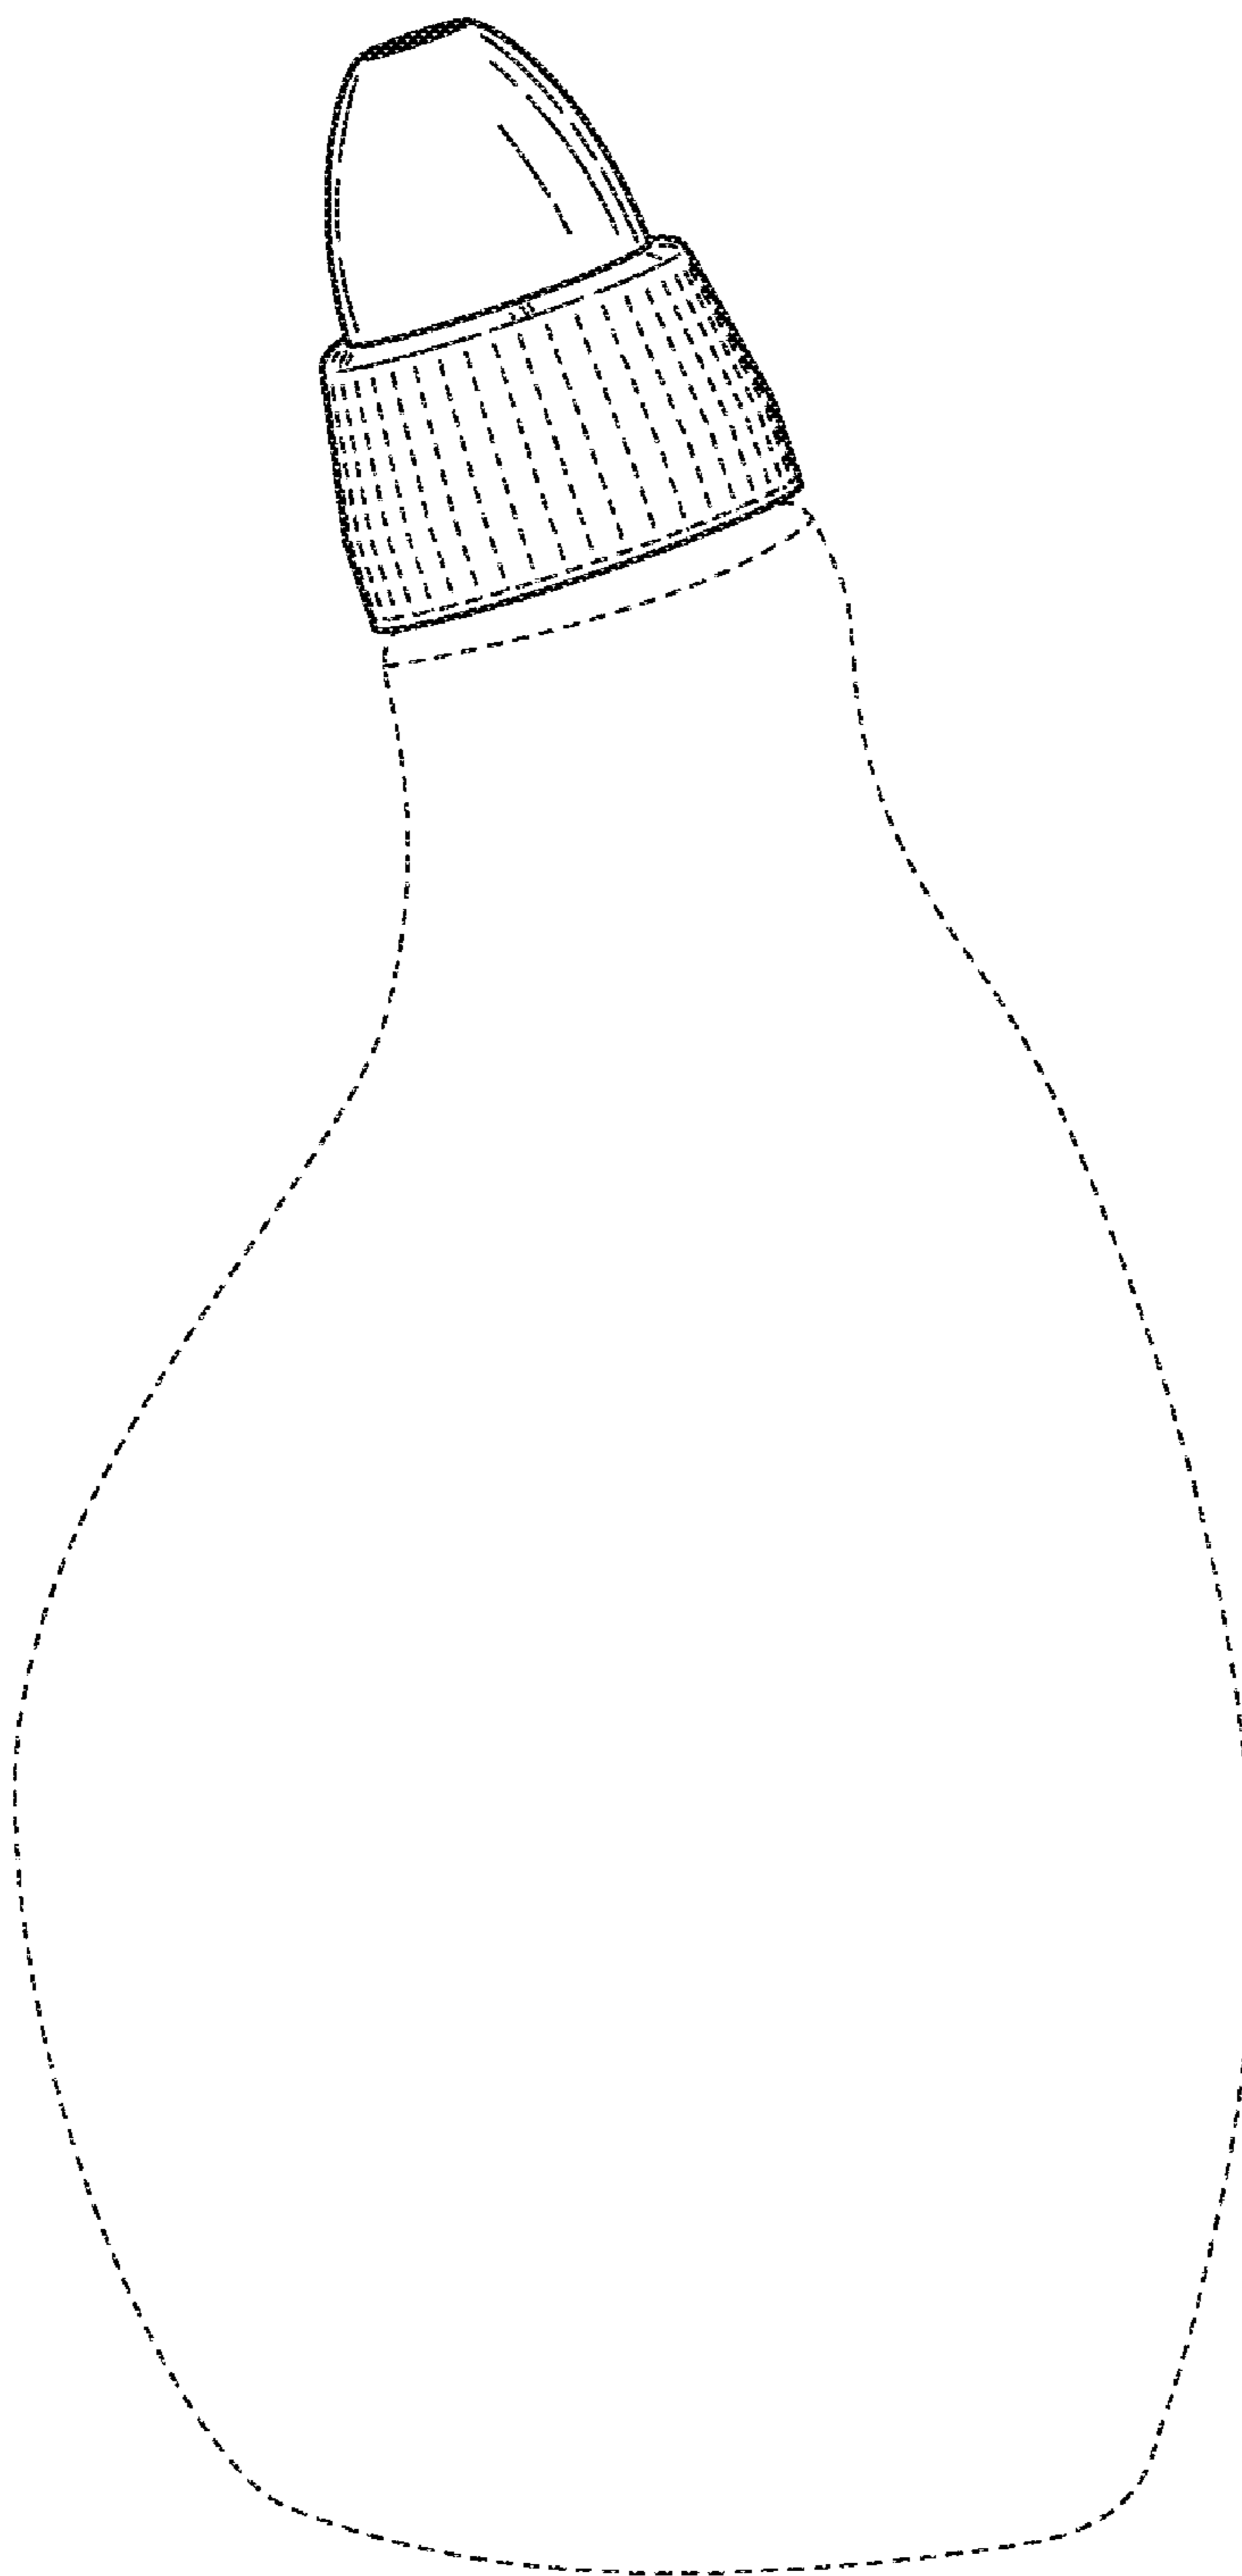


FIG. 1

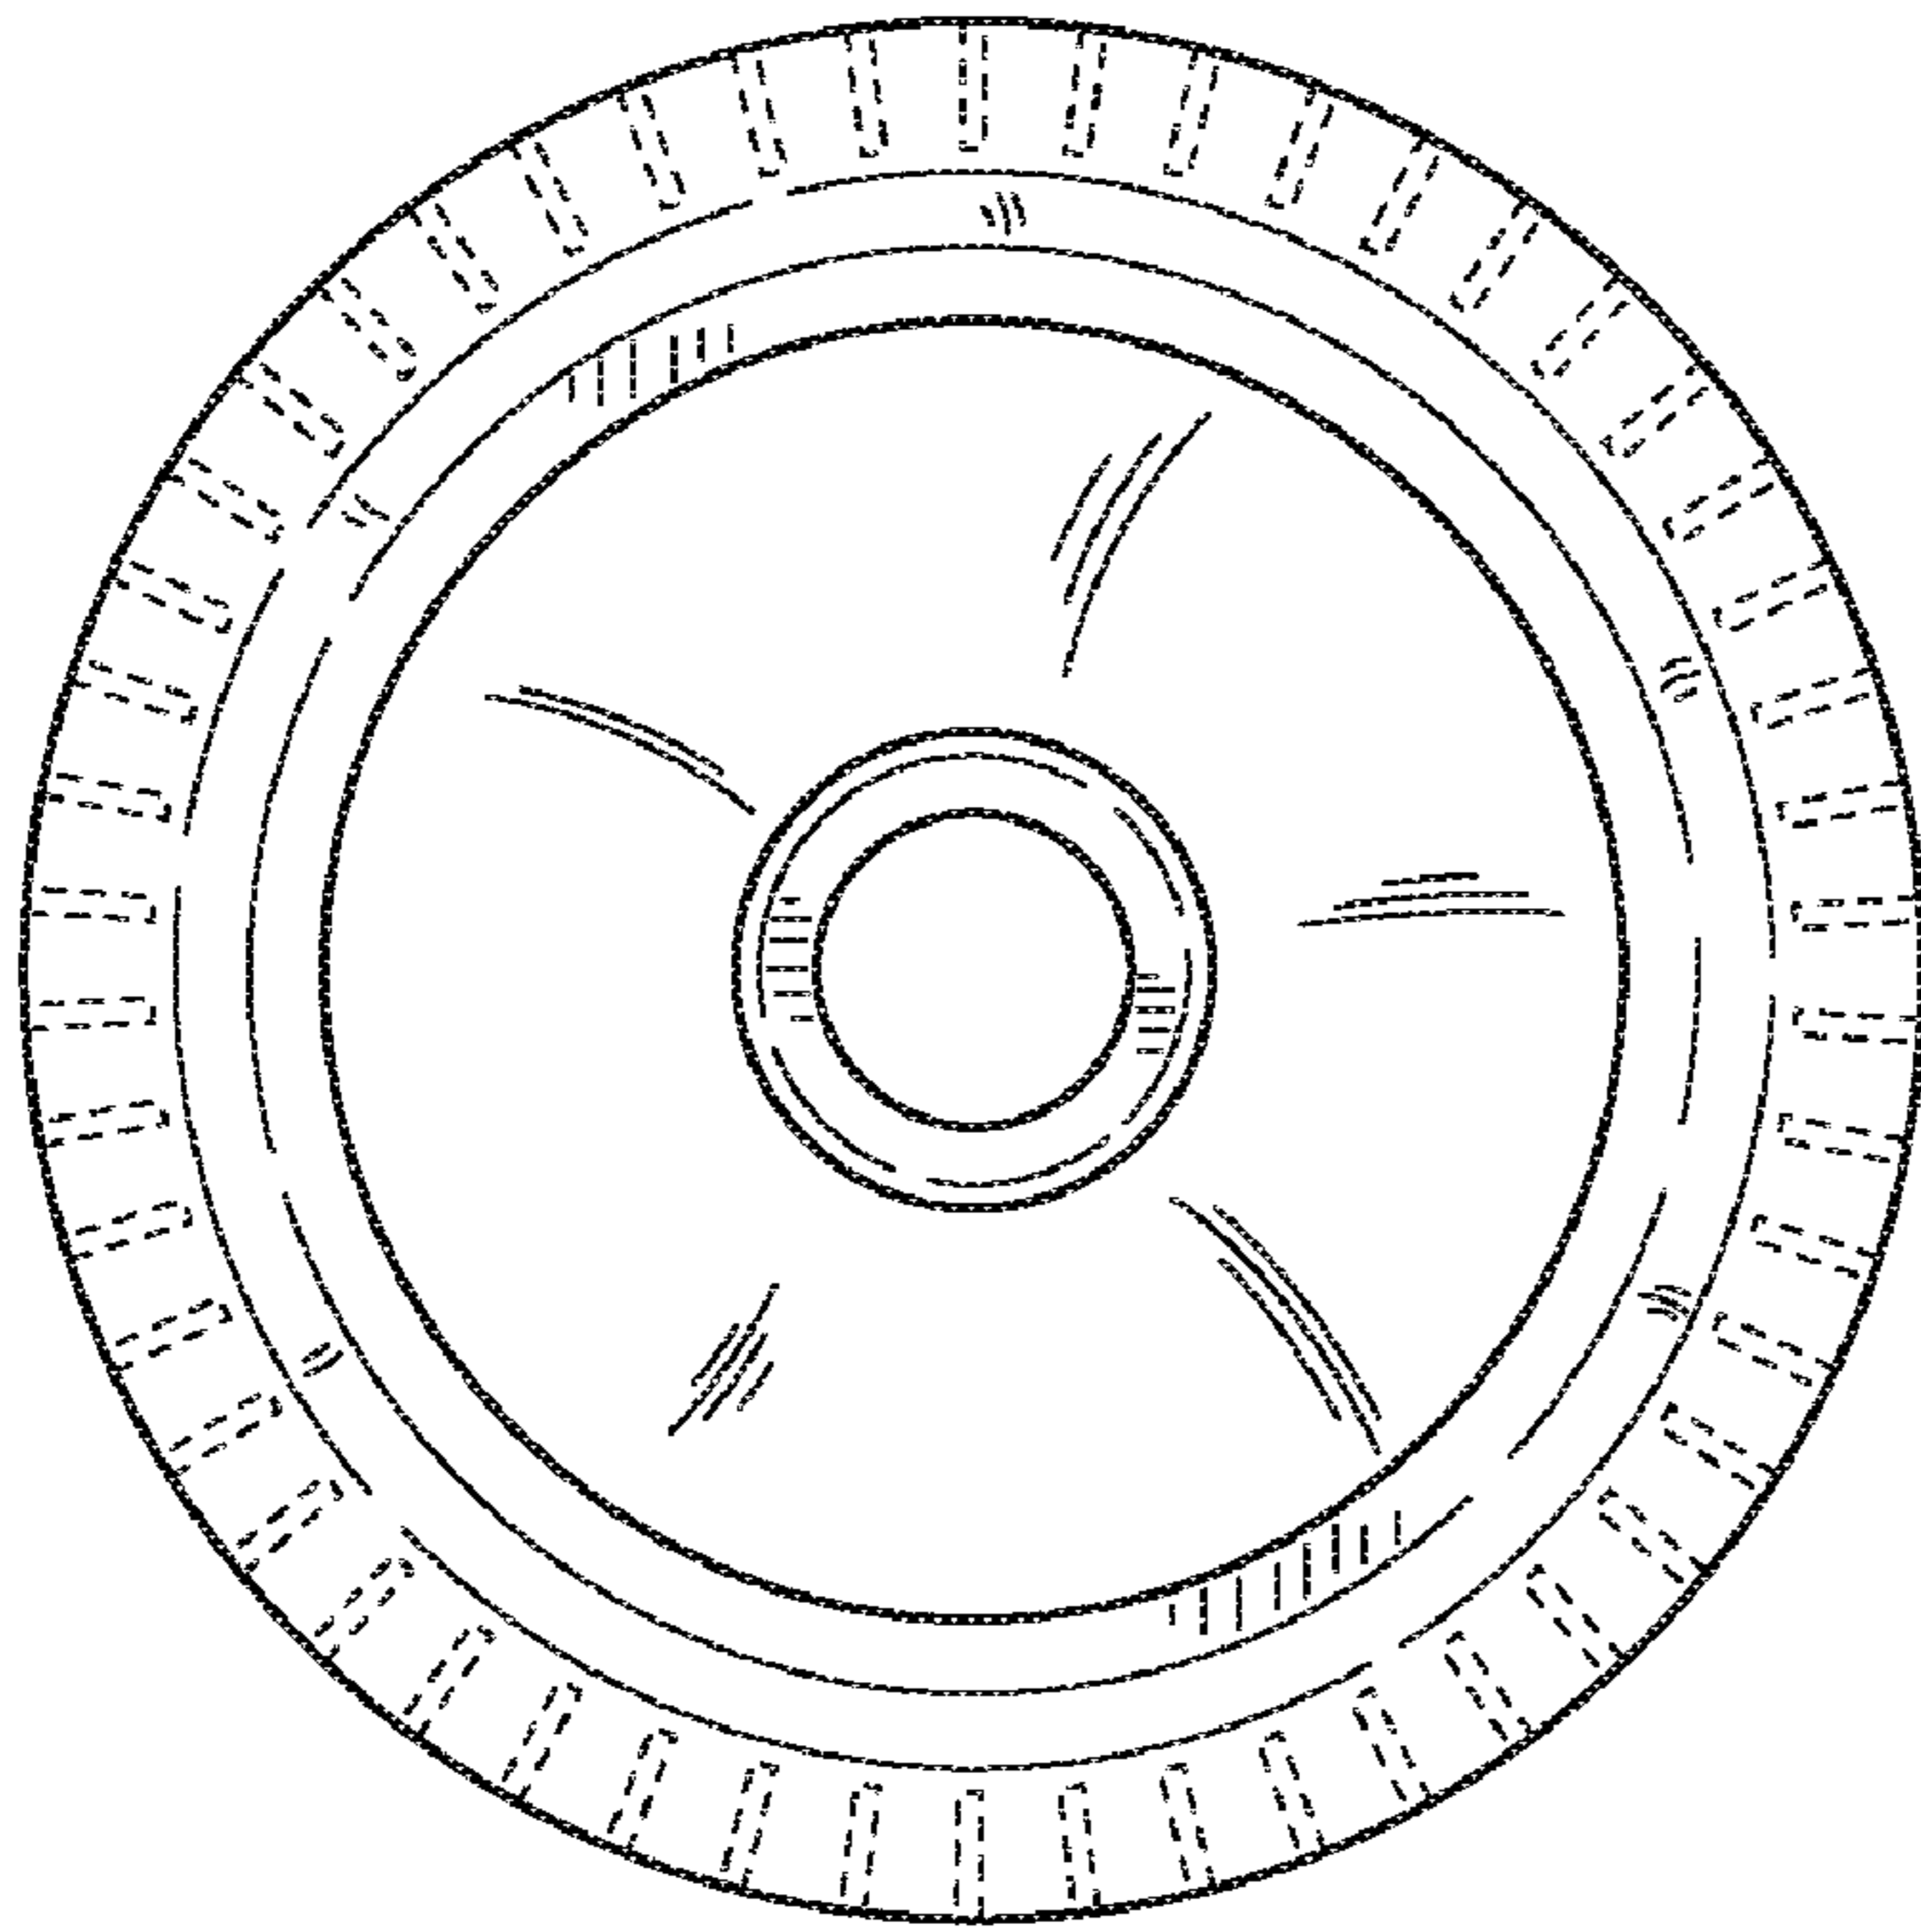


FIG. 2

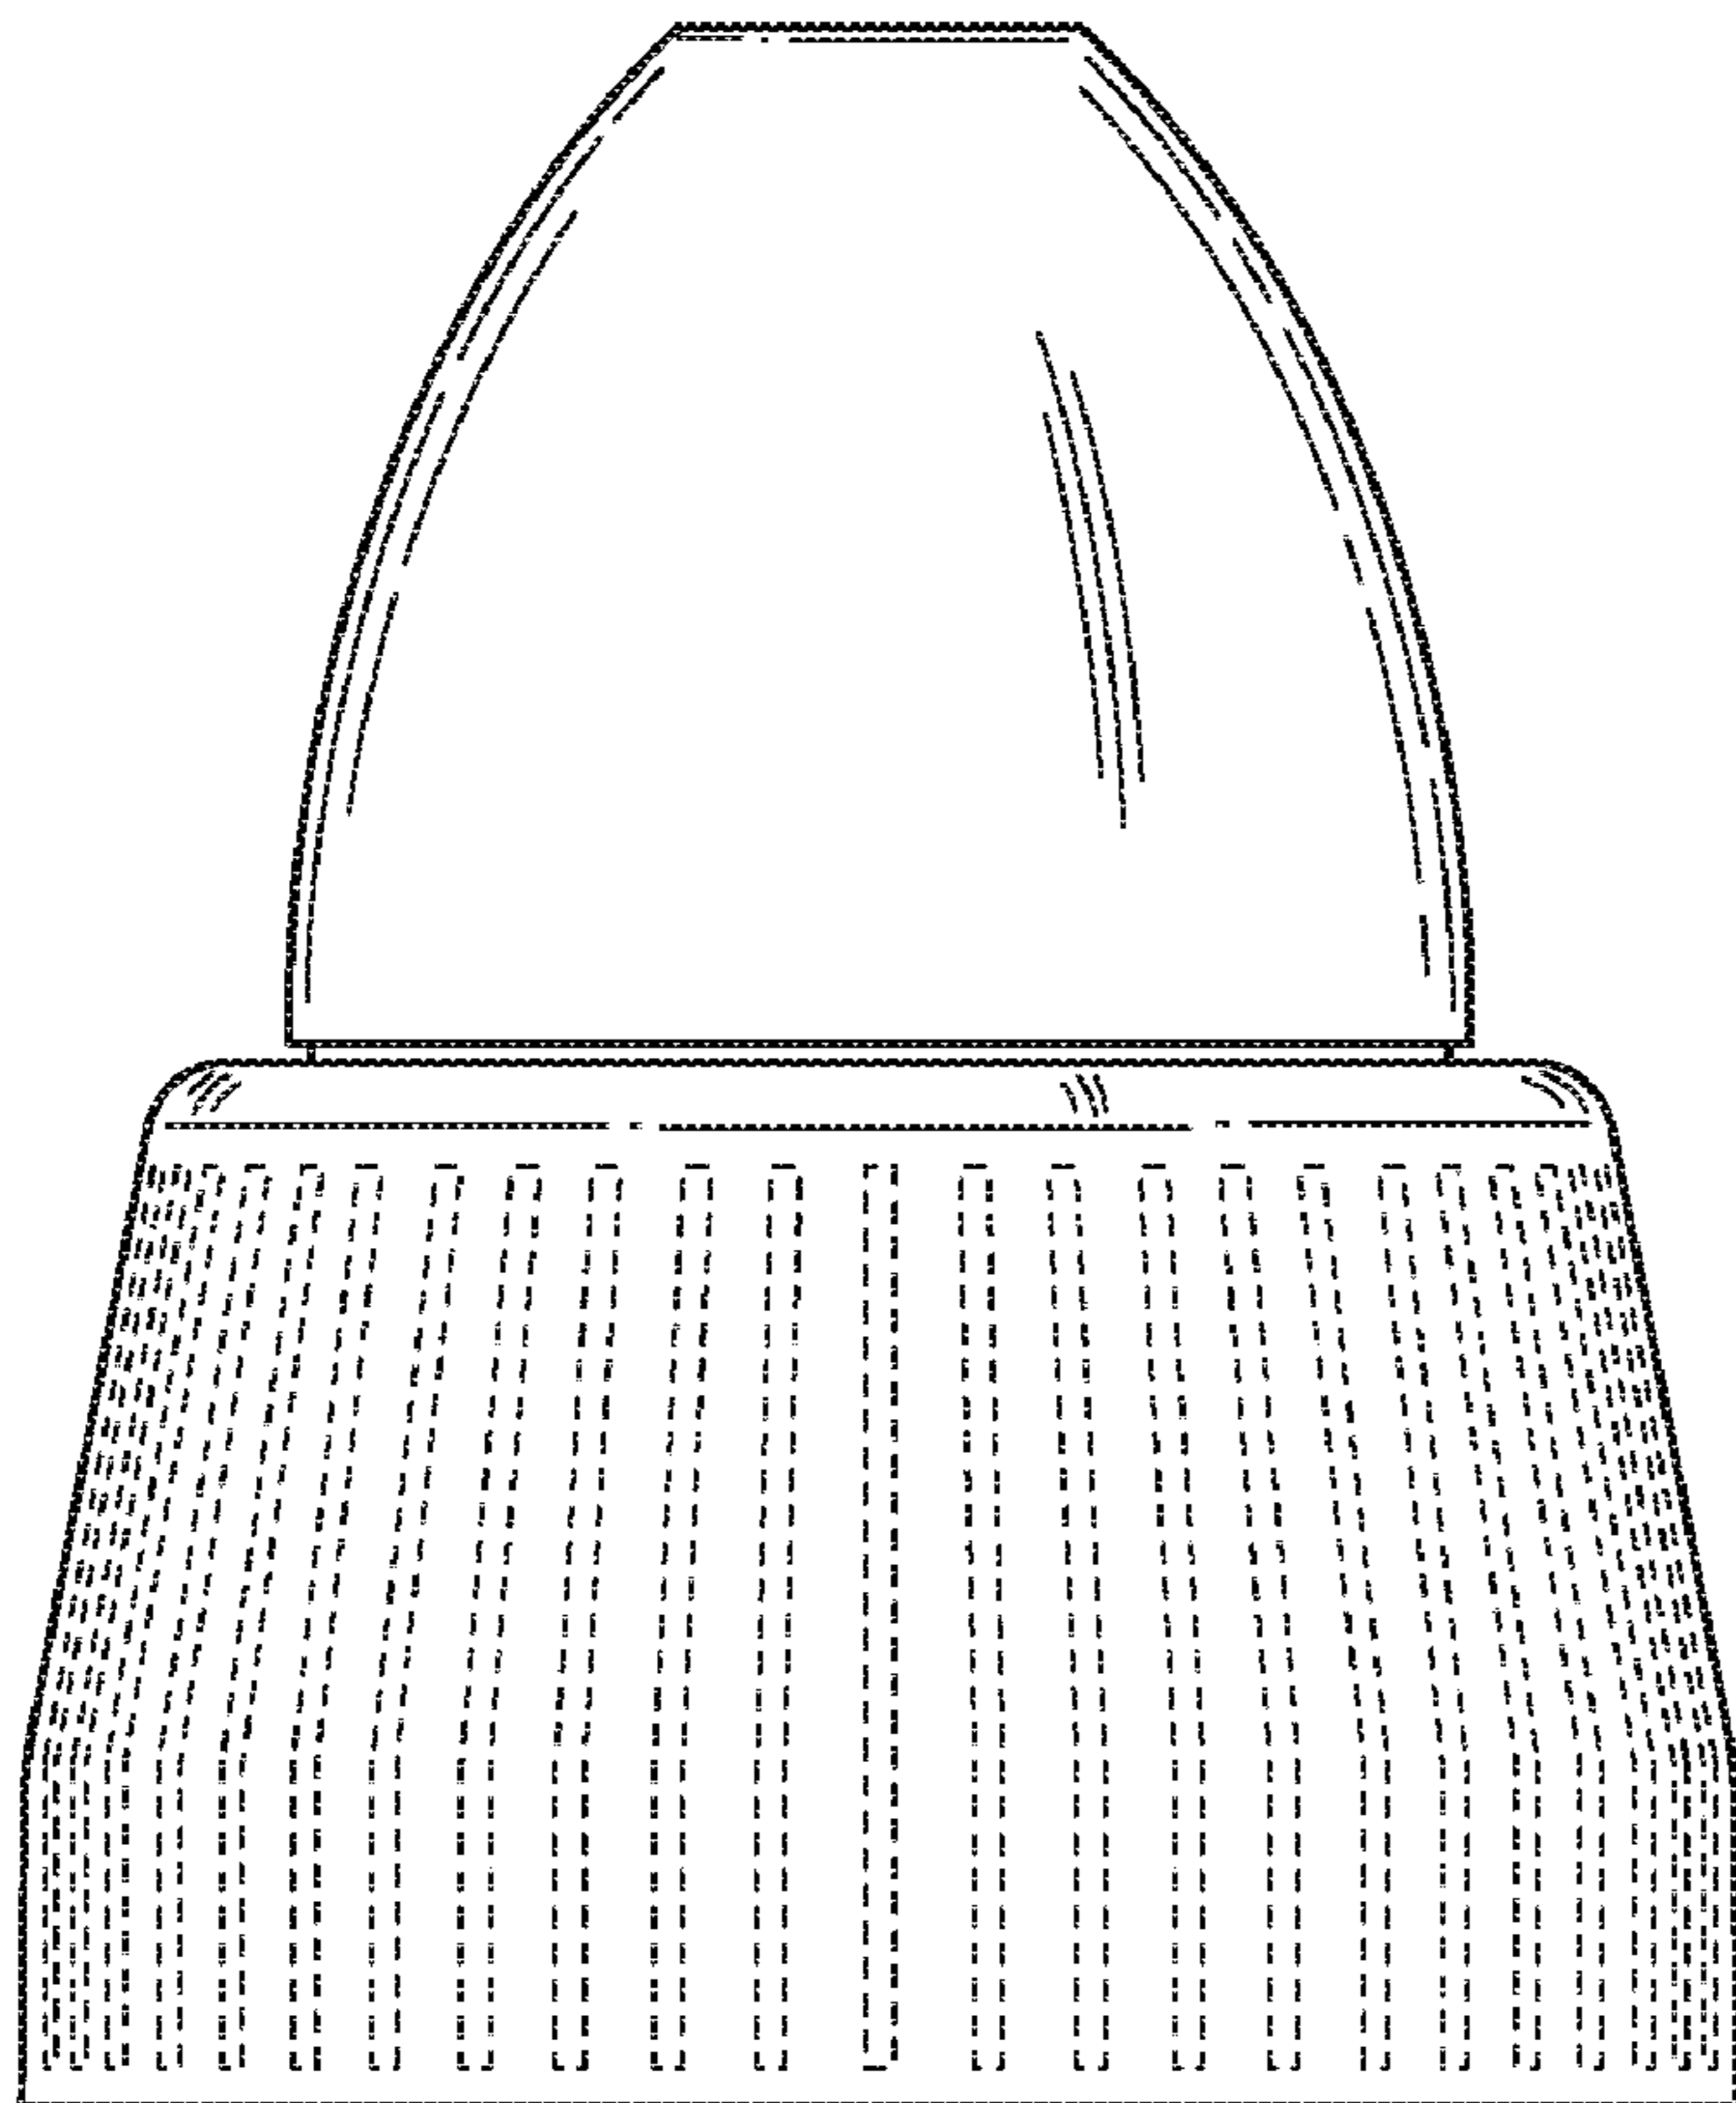


FIG. 3

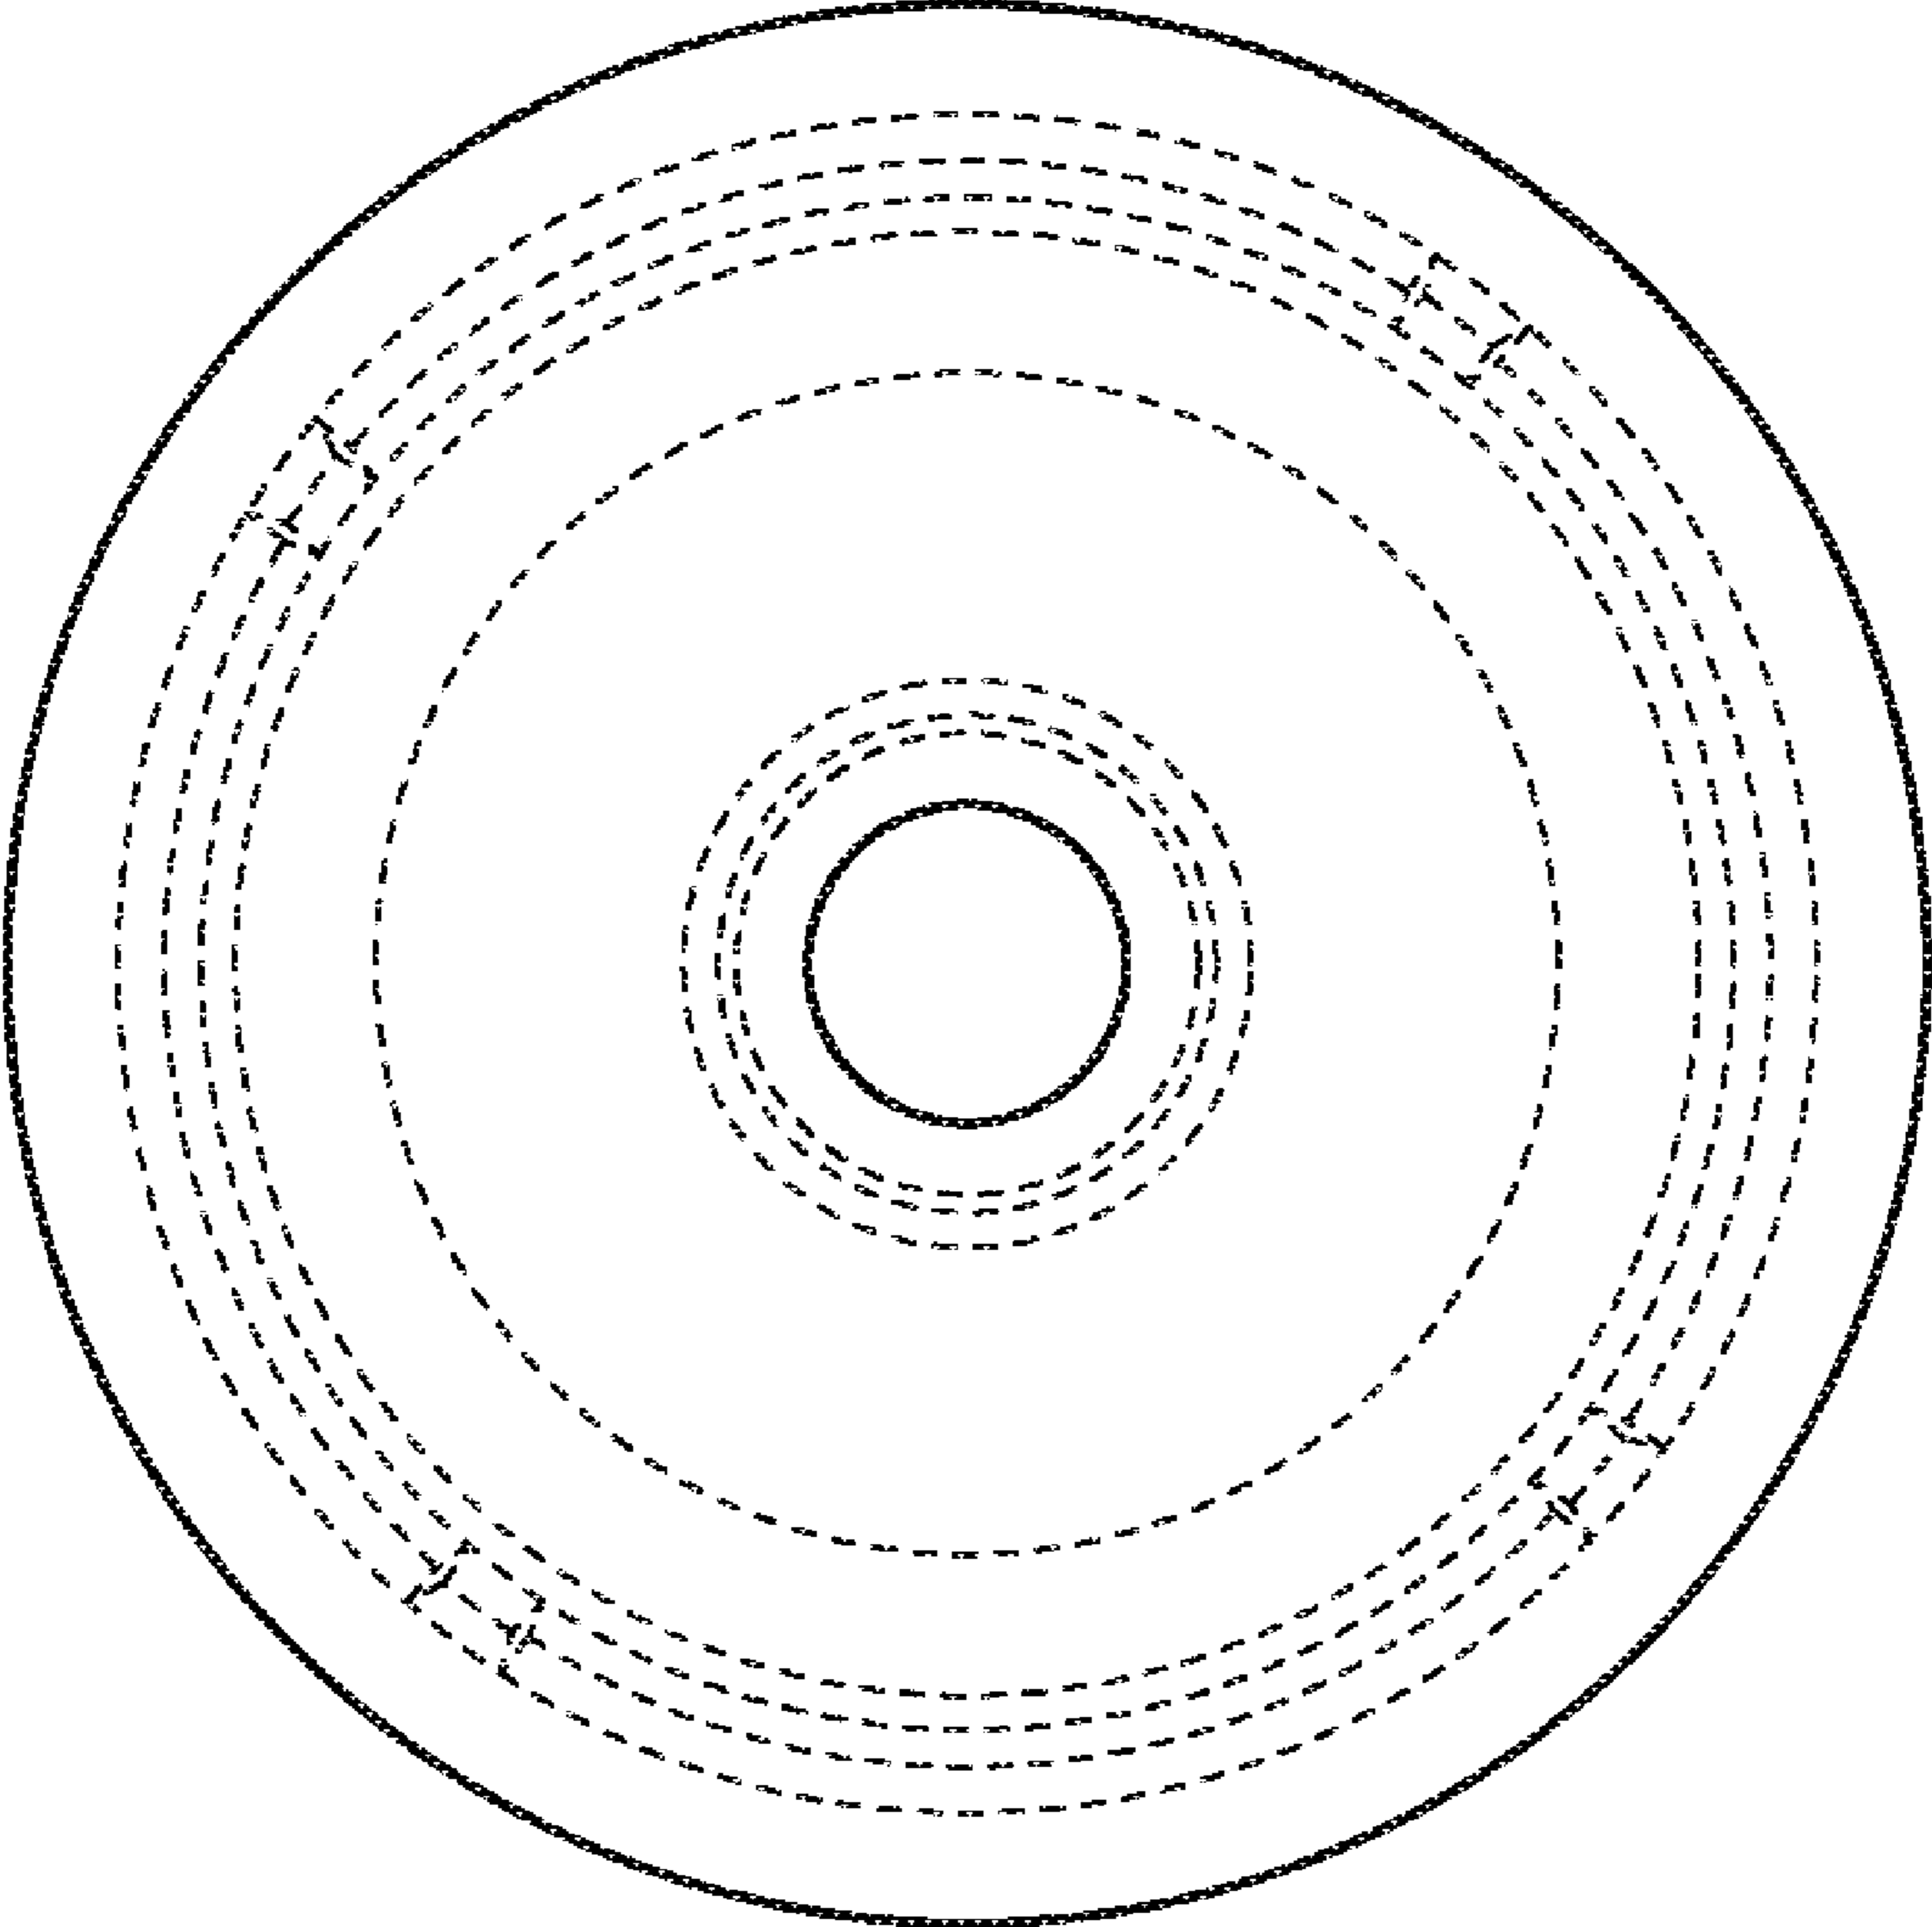


FIG.4