



US00D634849S

(12) **United States Design Patent**
Kanokogi et al.

(10) **Patent No.:** **US D634,849 S**
(45) **Date of Patent:** **** Mar. 22, 2011**

(54) **PROBE OF ULTRASOUND DIAGNOSIS APPARATUS**

(75) Inventors: **Tomoki Kanokogi**, Tokyo (JP); **Osamu Mori**, Tokyo (JP)

(73) Assignee: **Hitachi Medical Corporation**, Tokyo (JP)

(**) Term: **14 Years**

(21) Appl. No.: **29/365,823**

(22) Filed: **Jul. 15, 2010**

(30) **Foreign Application Priority Data**

Jan. 18, 2010 (JP) 2010-000955

(51) **LOC (9) Cl.** **24-02**

(52) **U.S. Cl.** **D24/187**

(58) **Field of Classification Search** D24/107,
D24/141, 158, 164, 165, 167, 170, 186-187,
D24/231; D10/57, 60, 78, 80; 600/407,
600/461, 459; 378/98.7, 98.8, 189
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

| | | | | | | |
|----------|---|---|---------|------------------|-------|---------|
| D245,513 | S | * | 8/1977 | Kopel | | D24/187 |
| D316,376 | S | * | 4/1991 | Dubut | | D10/80 |
| D319,793 | S | * | 9/1991 | Dubut | | D10/60 |
| D387,867 | S | * | 12/1997 | Henderson et al. | | D24/187 |
| D389,918 | S | * | 1/1998 | Ninomiya et al. | | D24/186 |
| D389,919 | S | * | 1/1998 | Ninomiya et al. | | D24/186 |

| | | | | | | |
|-----------|---|---|---------|-----------------|-------|---------|
| D390,959 | S | * | 2/1998 | Mesaros et al. | | D24/186 |
| D392,044 | S | * | 3/1998 | Mesaros et al. | | D24/186 |
| 5,897,503 | A | * | 4/1999 | Lyon et al. | | 600/459 |
| D545,433 | S | * | 6/2007 | Messerly et al. | | D24/186 |
| D546,460 | S | * | 7/2007 | Hasegawa | | D24/186 |
| D555,252 | S | * | 11/2007 | Kitayama et al. | | D24/186 |
| D596,299 | S | * | 7/2009 | Han et al. | | D24/186 |
| D596,300 | S | * | 7/2009 | Han et al. | | D24/186 |
| D598,108 | S | * | 8/2009 | Hasegawa | | D24/186 |
| D609,352 | S | * | 2/2010 | Kitayama | | D24/186 |
| D622,401 | S | * | 8/2010 | Suzuki | | D24/187 |

* cited by examiner

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Antonelli, Terry, Stout & Kraus, LLP.

(57) **CLAIM**



The ornamental design for probe of ultrasound diagnosis apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a front, top and right side perspective view of console showing our new design;
FIG. 2 is a front elevational view thereof;
FIG. 3 is a rear side elevational view thereof;
FIG. 4 is a top plan view thereof;
FIG. 5 is a bottom plan view thereof;
FIG. 6 is a left side elevational view thereof; and,
FIG. 7 is a right side elevational view thereof.

The broken lines shown are included for the purpose of illustrating a portion of the probe of ultrasound diagnosis apparatus that forms no part of the claimed design.

1 Claim, 3 Drawing Sheets

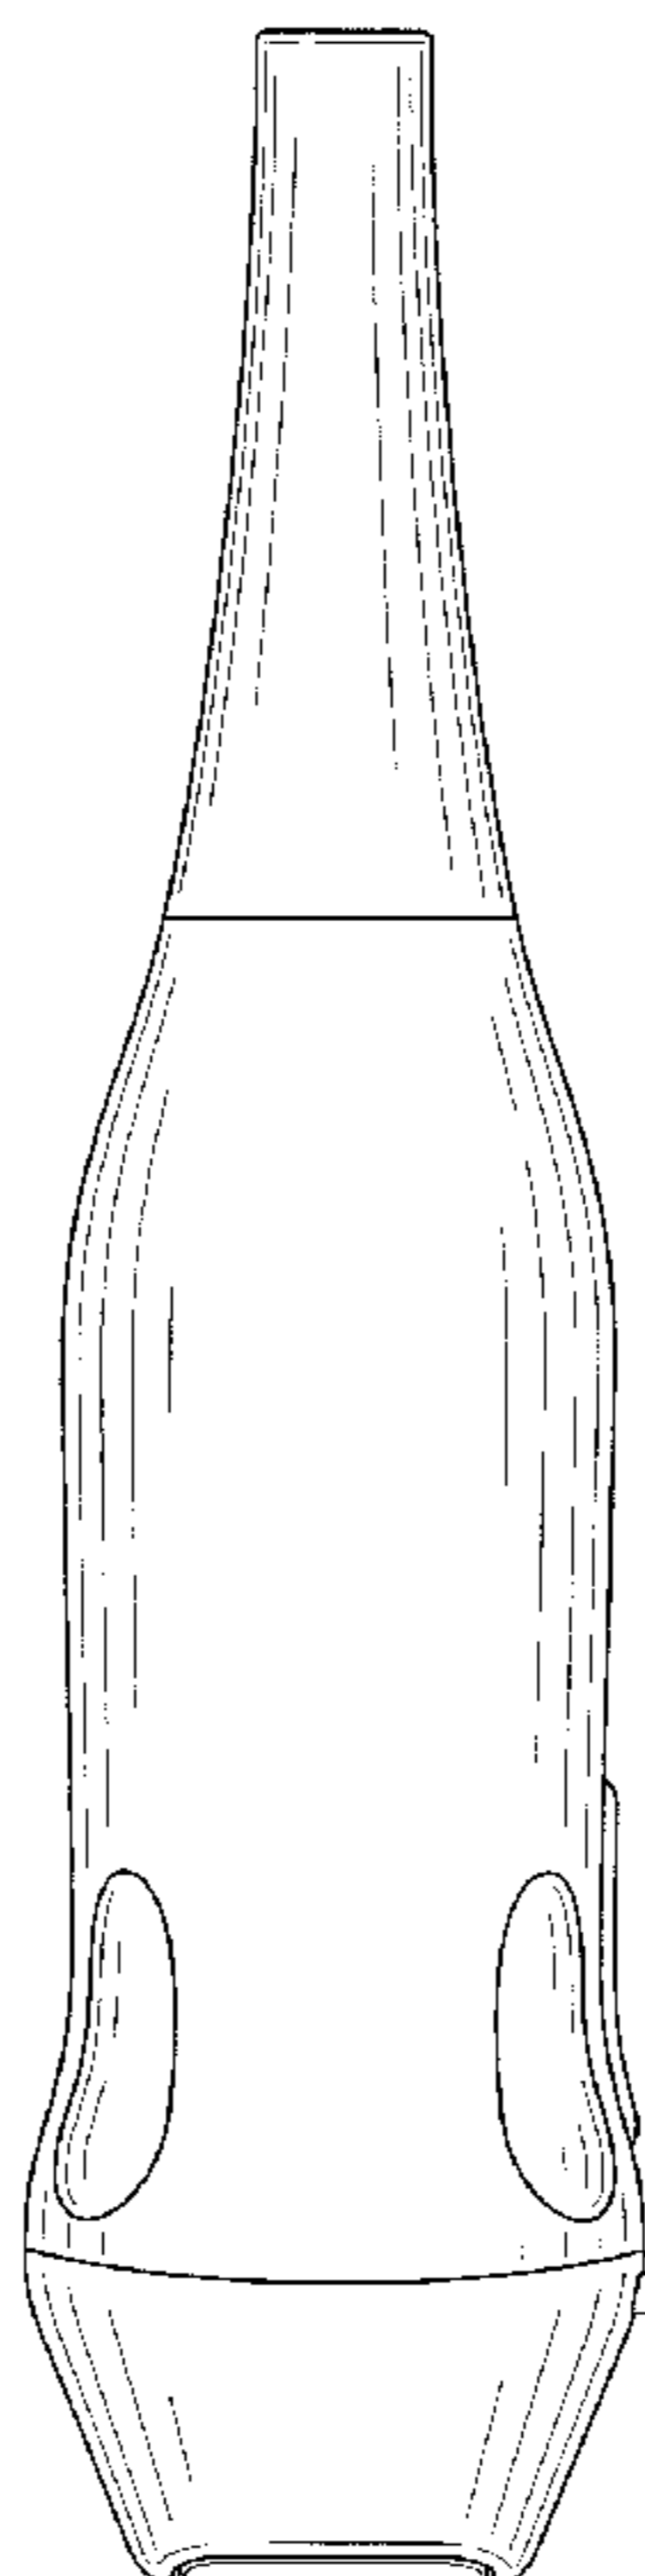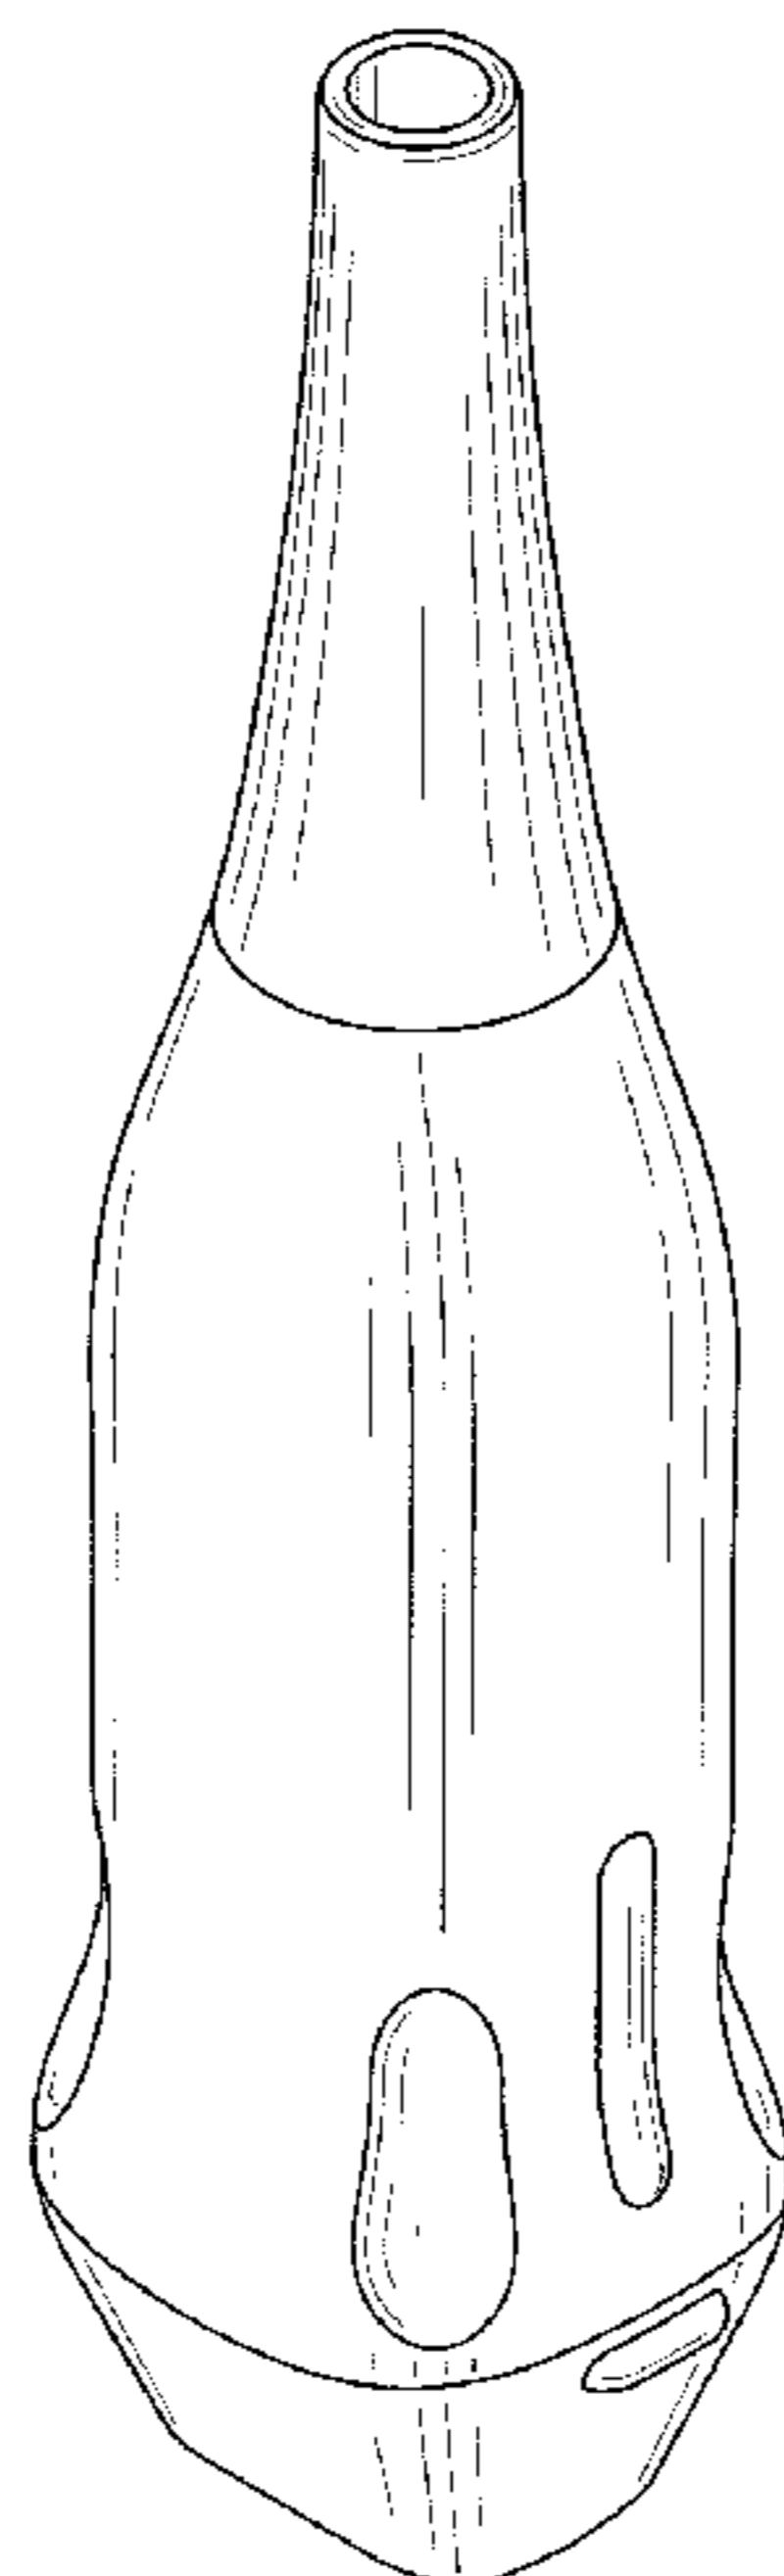

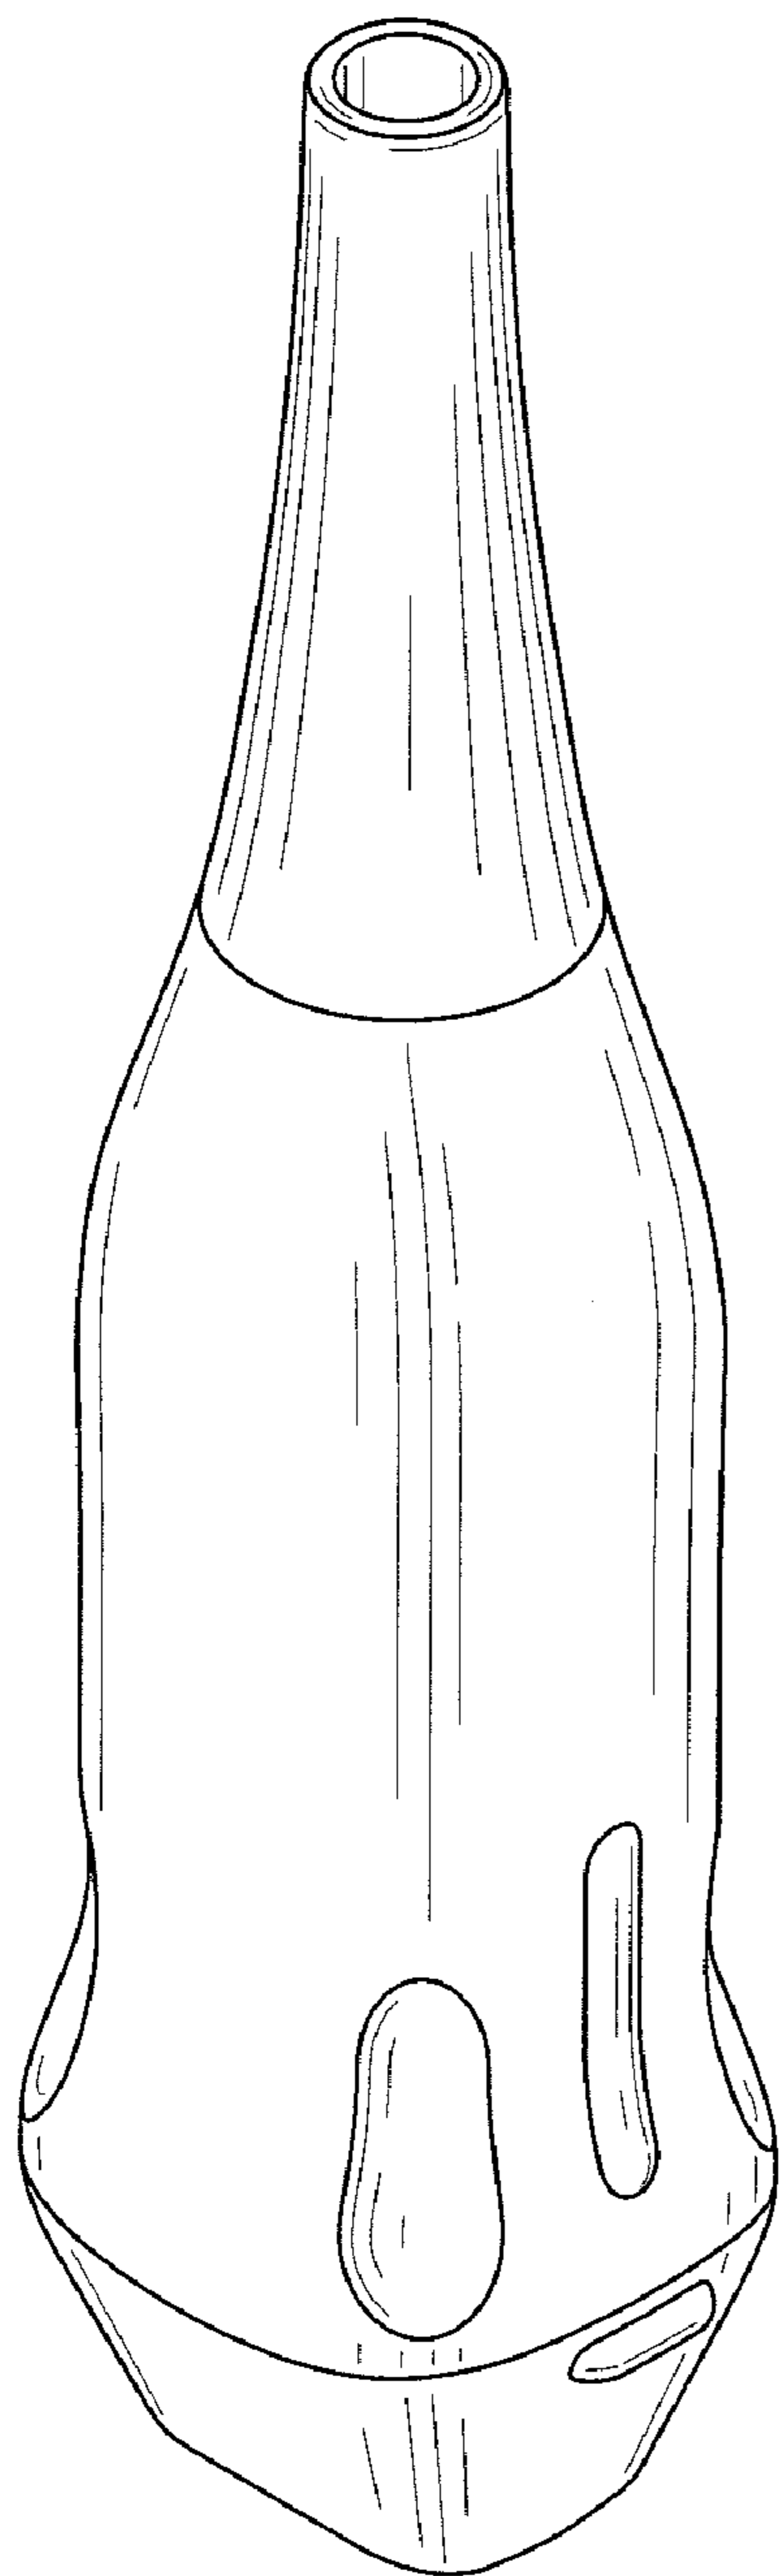


FIG. 1

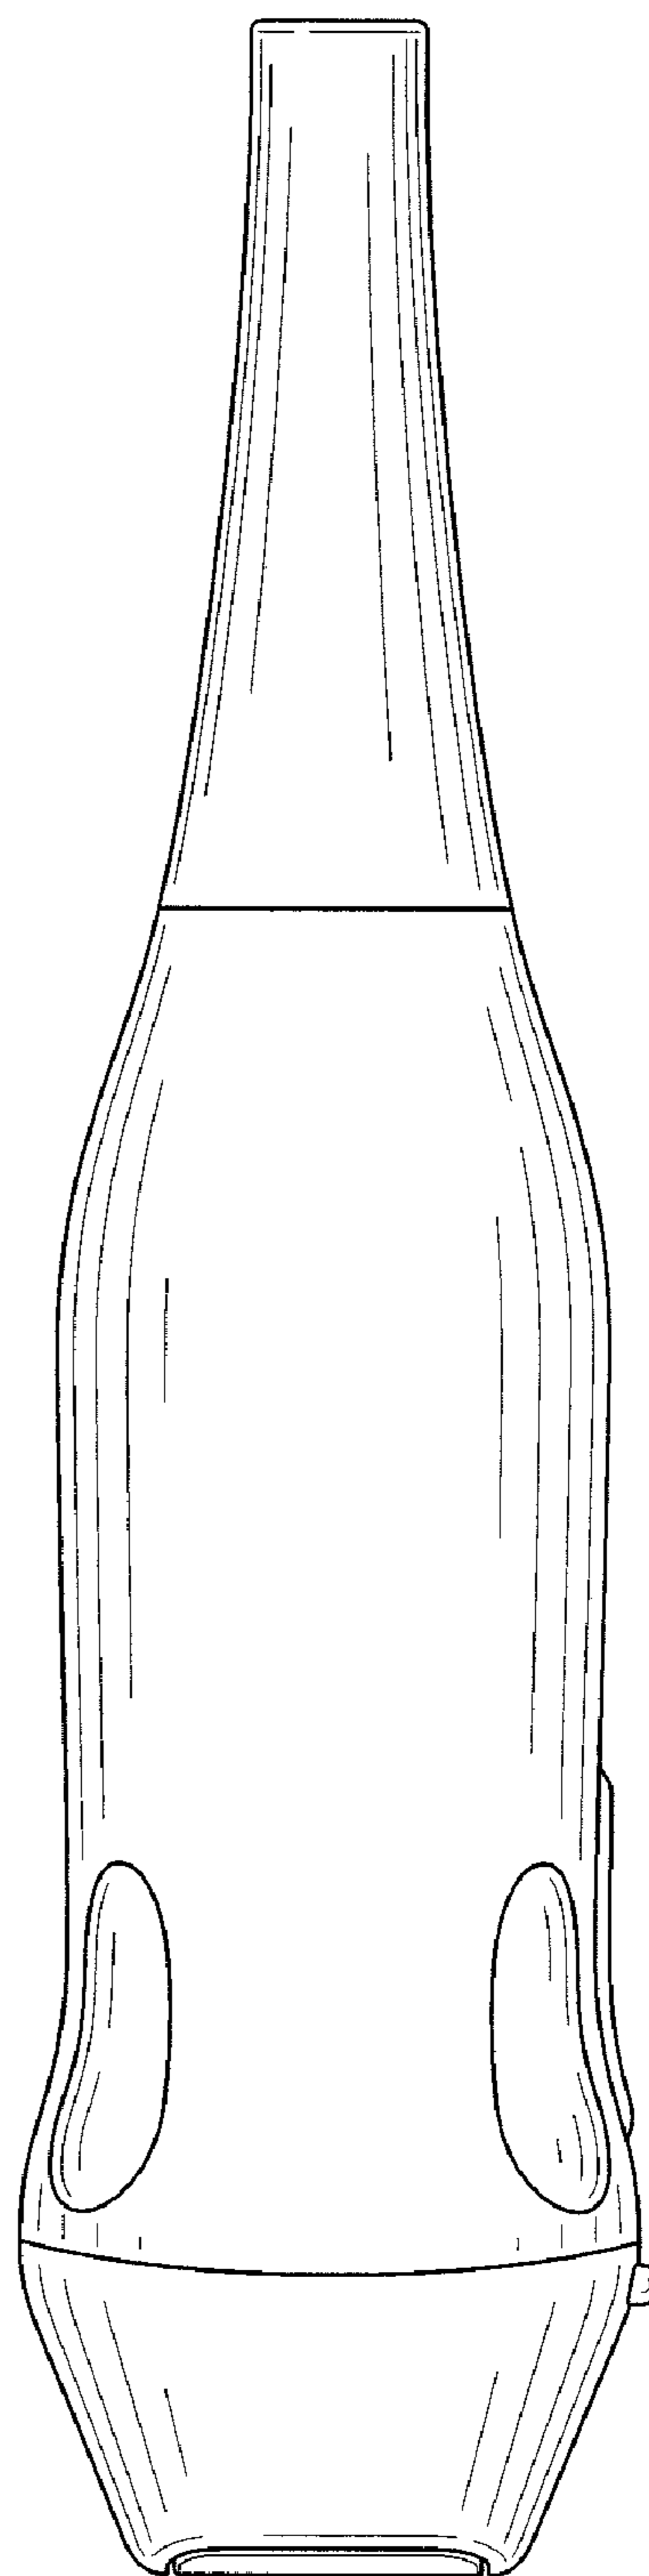


FIG. 2

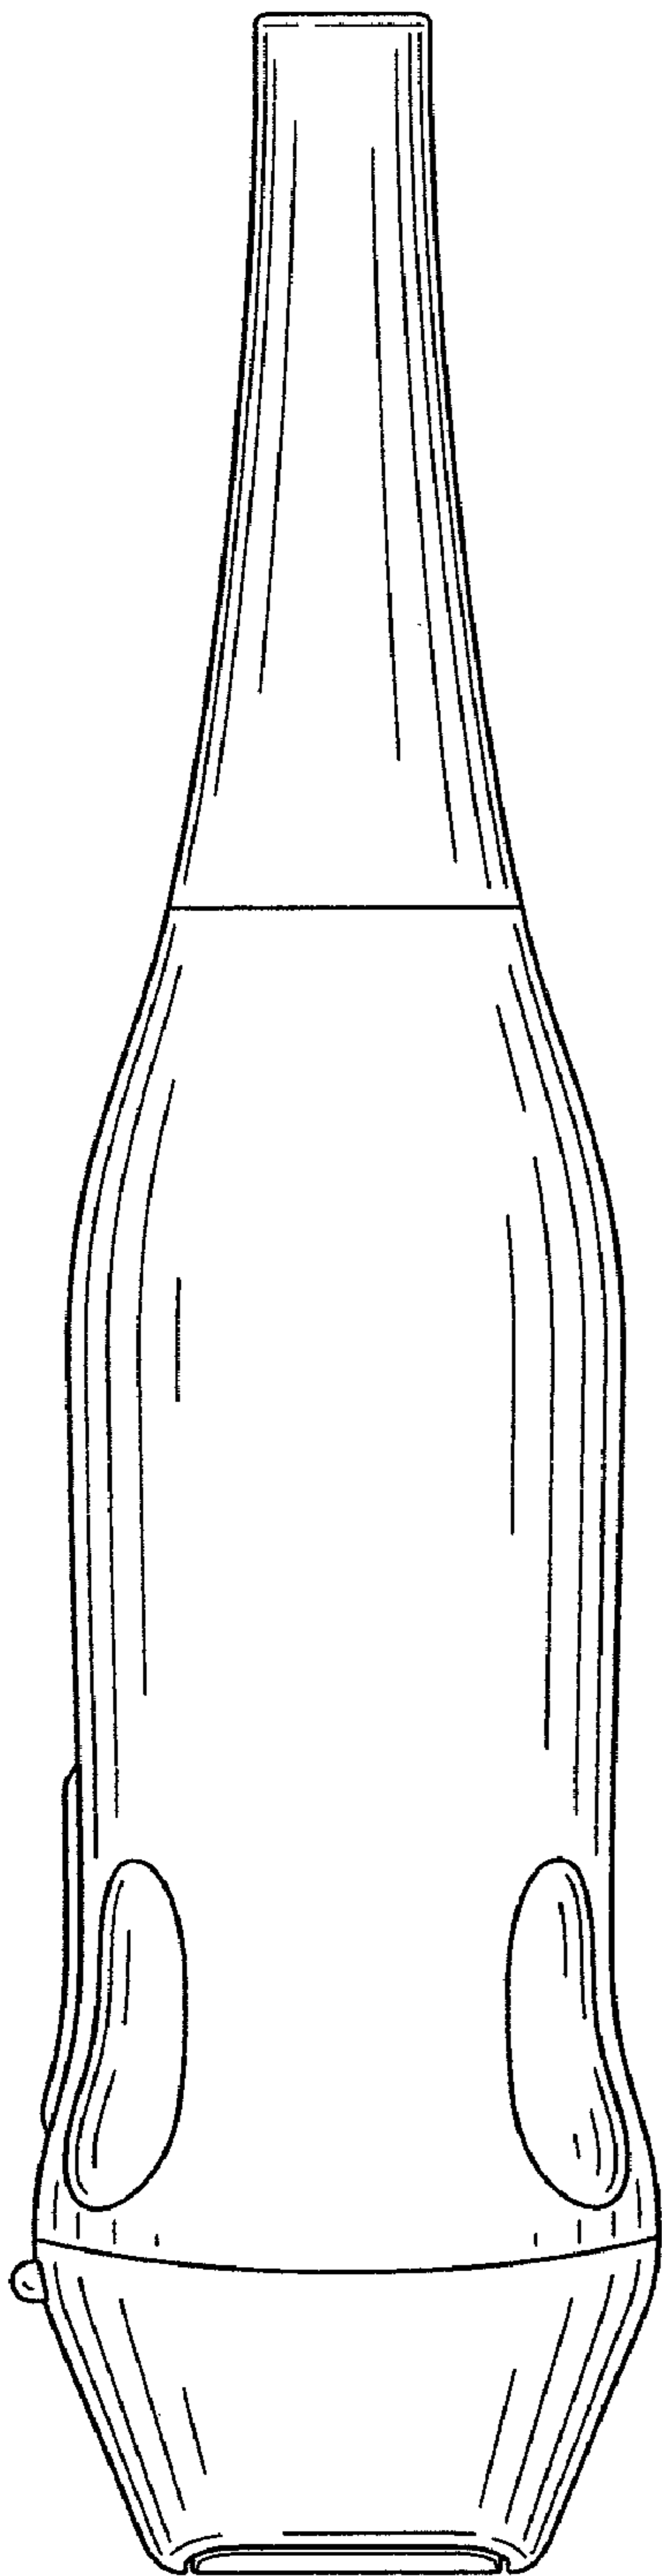


FIG. 3

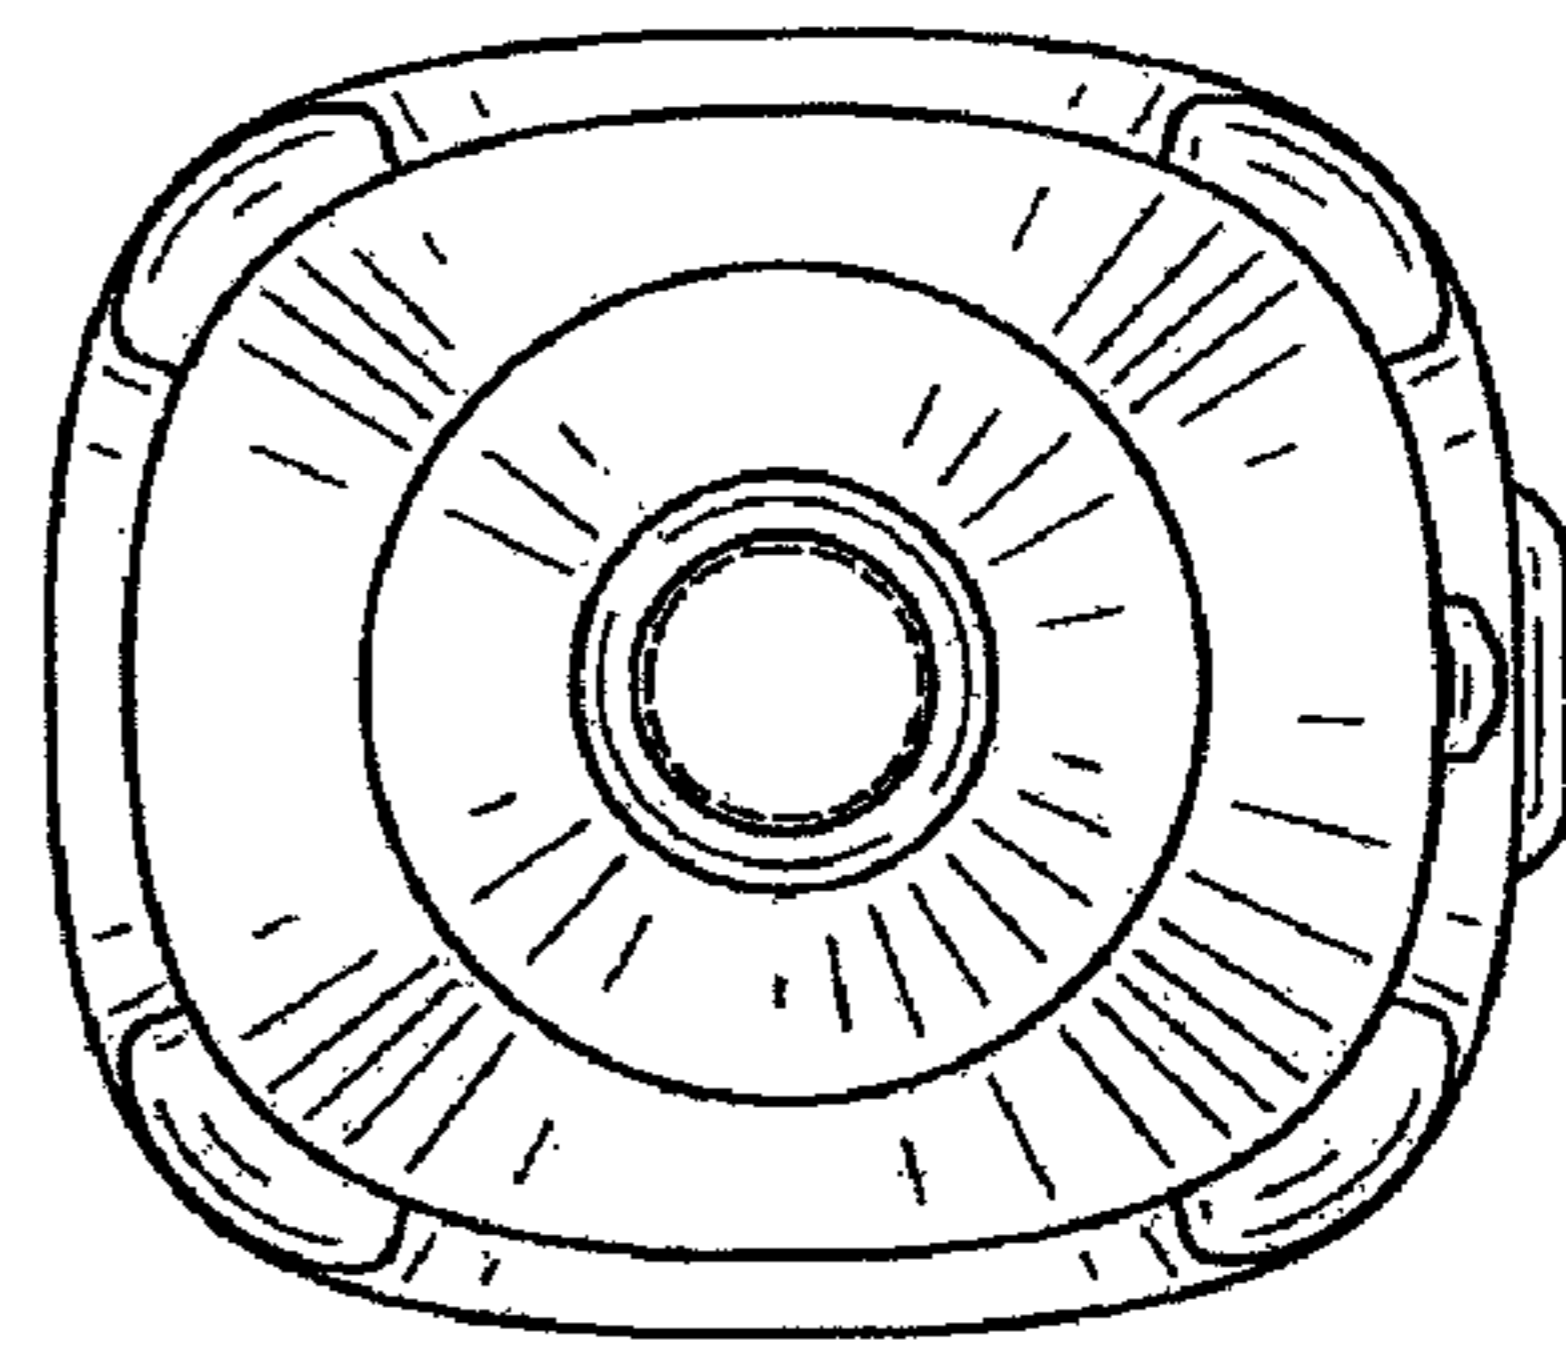


FIG. 4

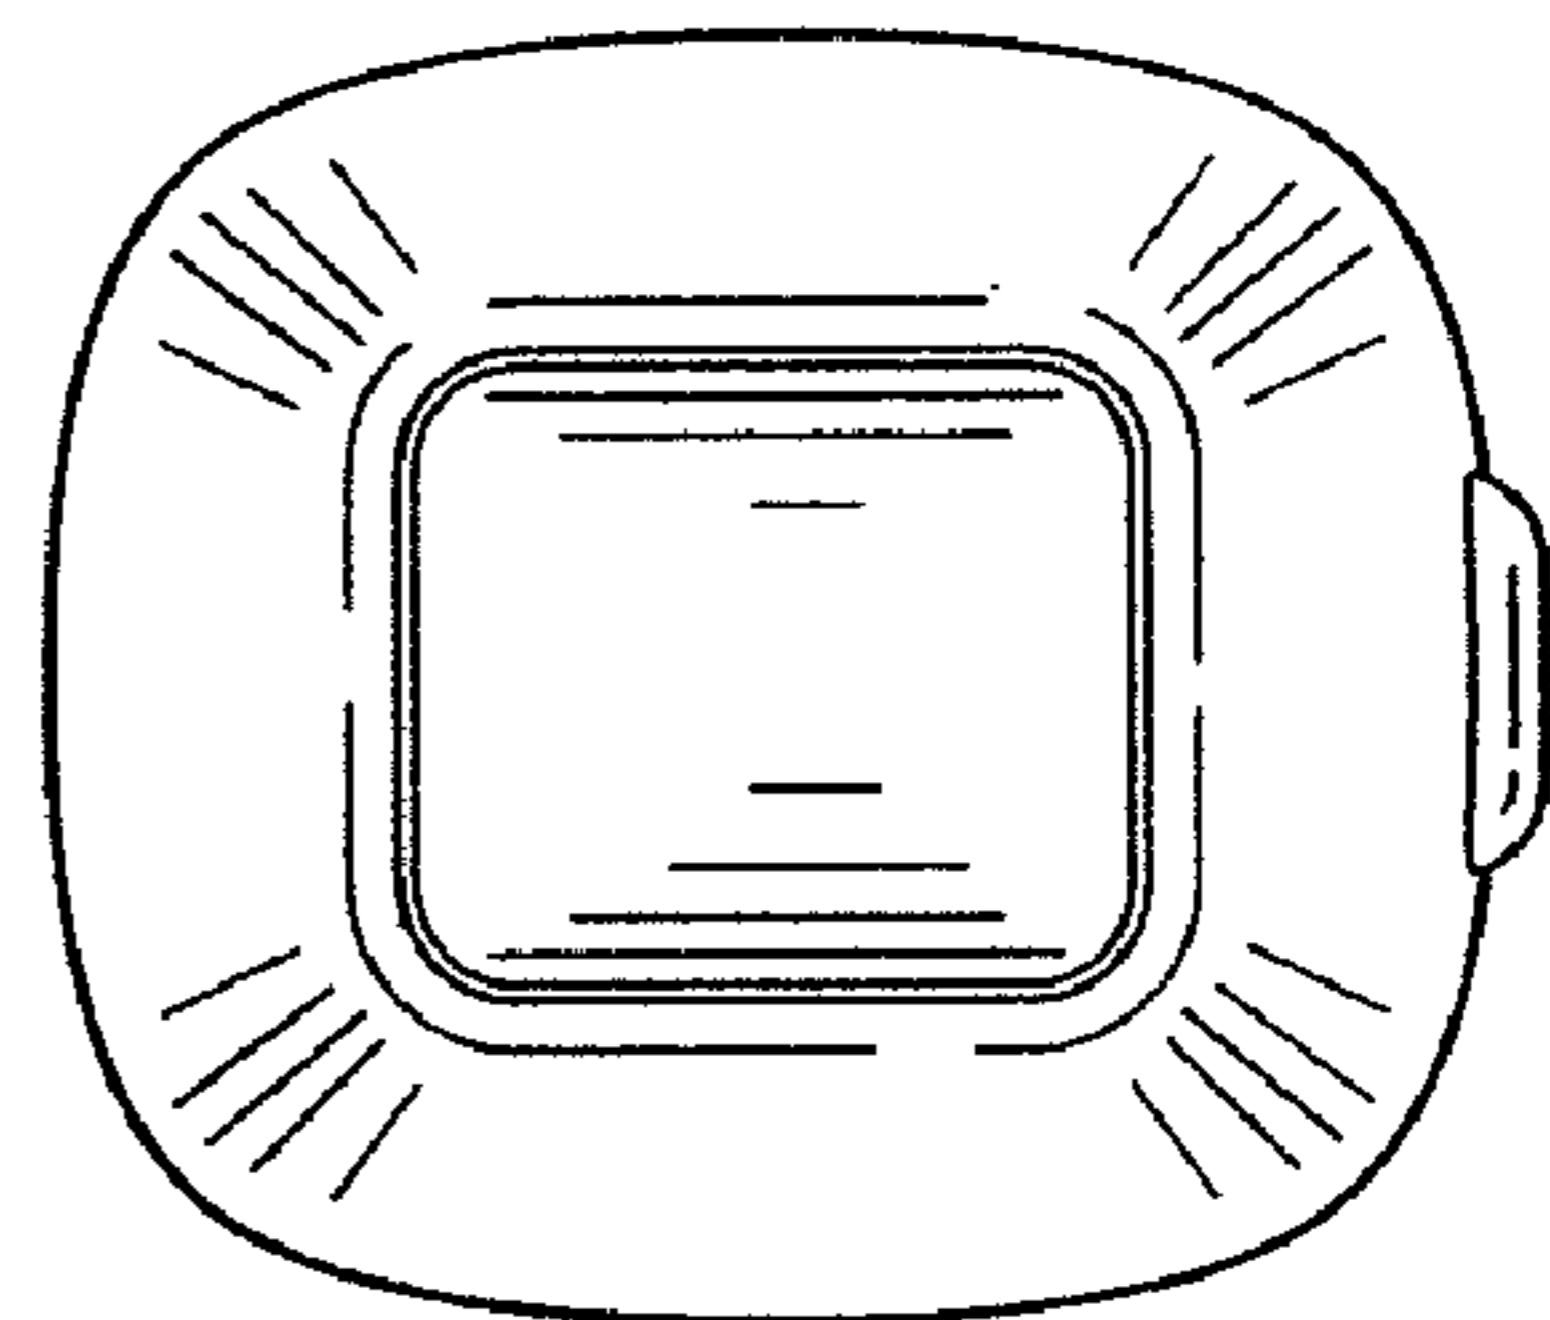


FIG. 5

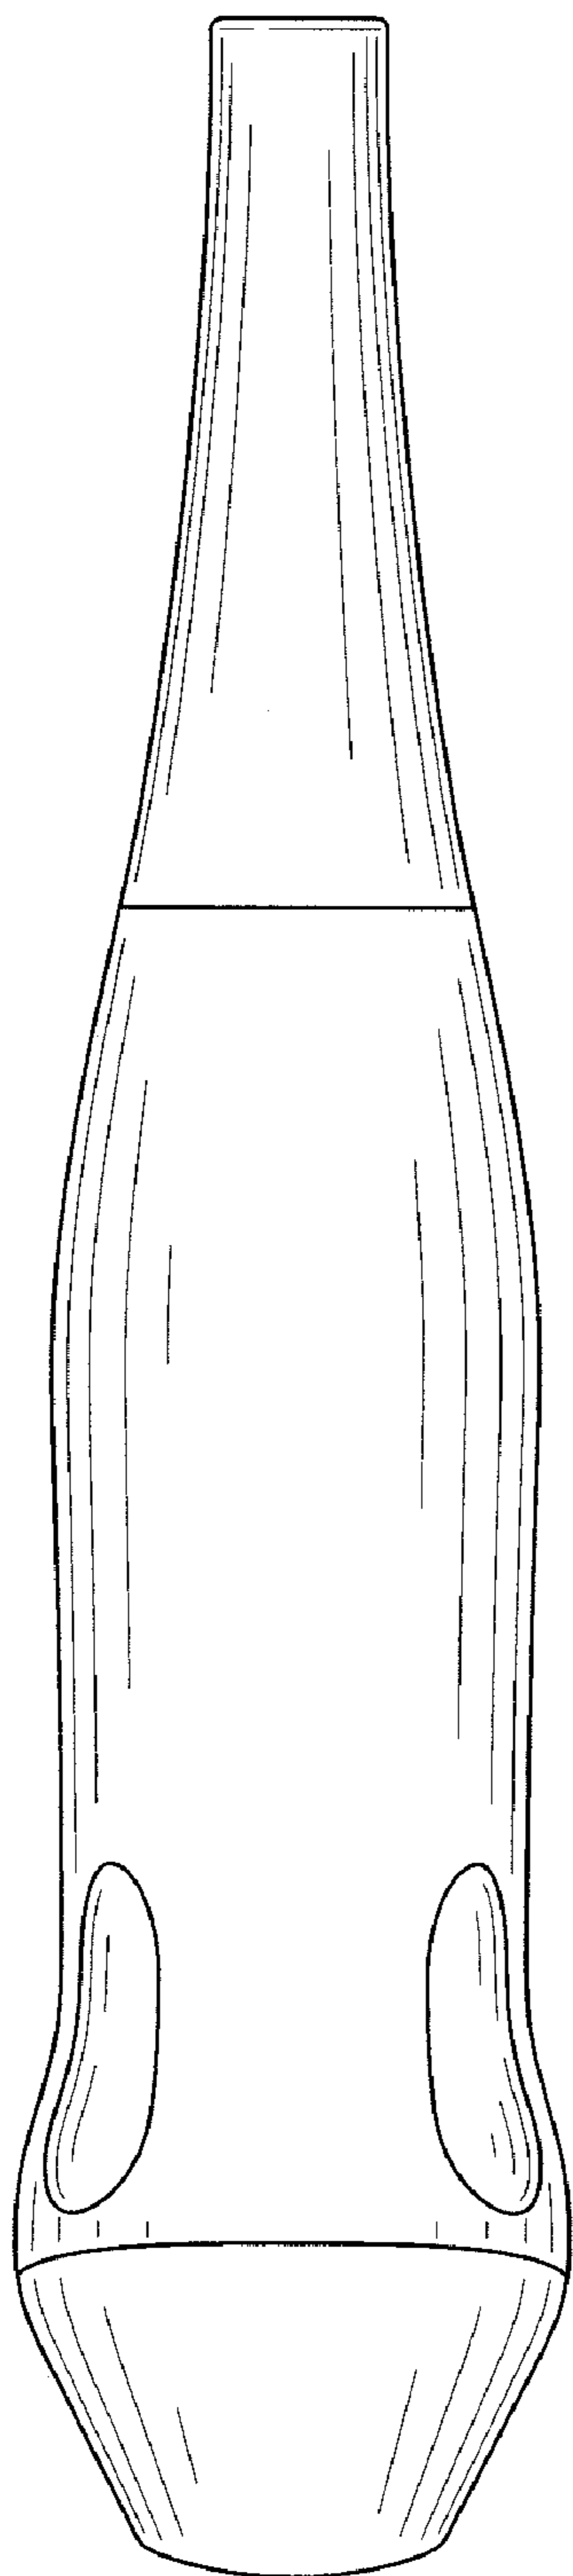


FIG. 6

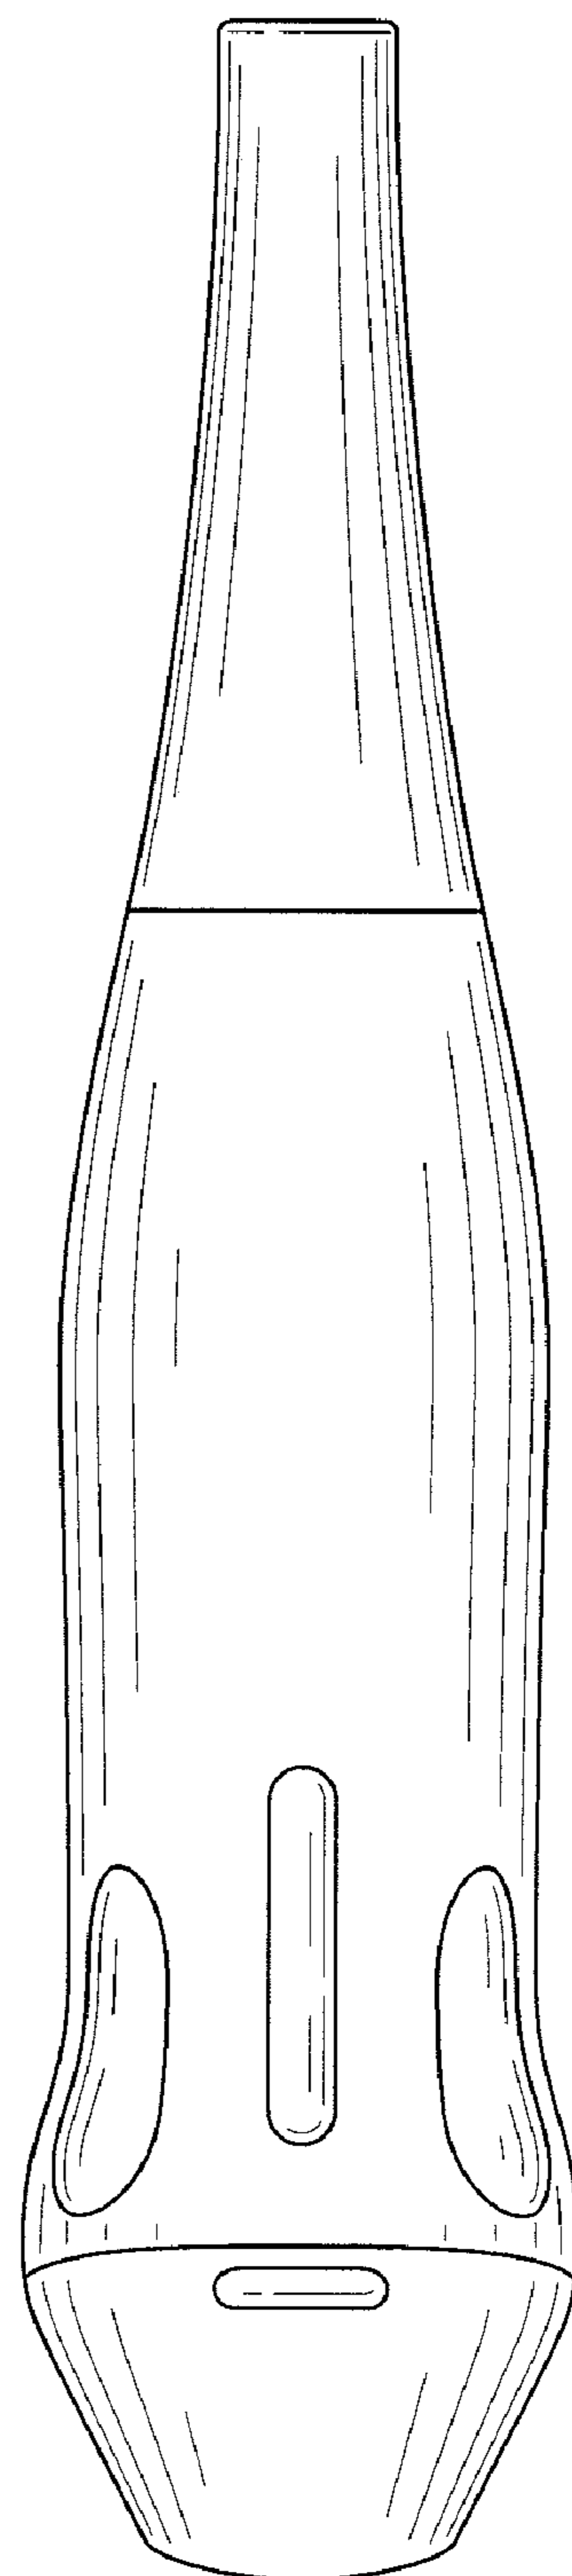


FIG. 7