



US00D635256S

(12) **United States Design Patent**
Huang

(10) **Patent No.:** **US D635,256 S**
(45) **Date of Patent:** **** Mar. 29, 2011**

- (54) **MEDICAL INSPECTION DEVICE**
- (75) Inventor: **Tzai-Kun Huang**, Taipei (TW)
- (73) Assignee: **Apple Biomedical Inc.**, Taipei (TW)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/345,750**
- (22) Filed: **Oct. 21, 2009**
- (51) **LOC (9) Cl.** **24-02**
- (52) **U.S. Cl.** **D24/137; D24/151**
- (58) **Field of Classification Search** **D24/137,**
D24/138, 151; 600/200, 559
See application file for complete search history.

7,269,262 B2 * 9/2007 Iseberg et al. 381/60
 7,670,287 B2 * 3/2010 Roberts et al. 600/200
 2010/0191063 A1 * 7/2010 Hsu 600/200
 * cited by examiner

Primary Examiner — Ian Simmons
Assistant Examiner — Carissa C Fitts
 (74) *Attorney, Agent, or Firm* — Roger H. Chu

(57) **CLAIM**
 The ornamental design for a medical inspection device, as shown and described.


DESCRIPTION

FIG. 1 is a perspective view of a medical inspection device showing my new design;
 FIG. 2 is a front elevation view thereof;
 FIG. 3 is a rear elevation view thereof;
 FIG. 4 is a right side elevation view thereof;
 FIG. 5 is a left side elevation view thereof;
 FIG. 6 is a top view thereof; and,
 FIG. 7 is a bottom view thereof.

The broken lines shown in the drawings are included for the purpose of illustrating portions of the medical inspection device that forms no part of the claimed design.

- (56) **References Cited**
- U.S. PATENT DOCUMENTS
- 3,110,304 A * 11/1963 Hartman 600/200
- D207,372 S * 4/1967 Pulos D24/137
- D221,109 S * 7/1971 Heine D24/137
- 4,567,881 A * 2/1986 Heller 600/200
- D288,960 S * 3/1987 Riester D24/137
- 4,688,582 A * 8/1987 Heller et al. 600/559

1 Claim, 4 Drawing Sheets

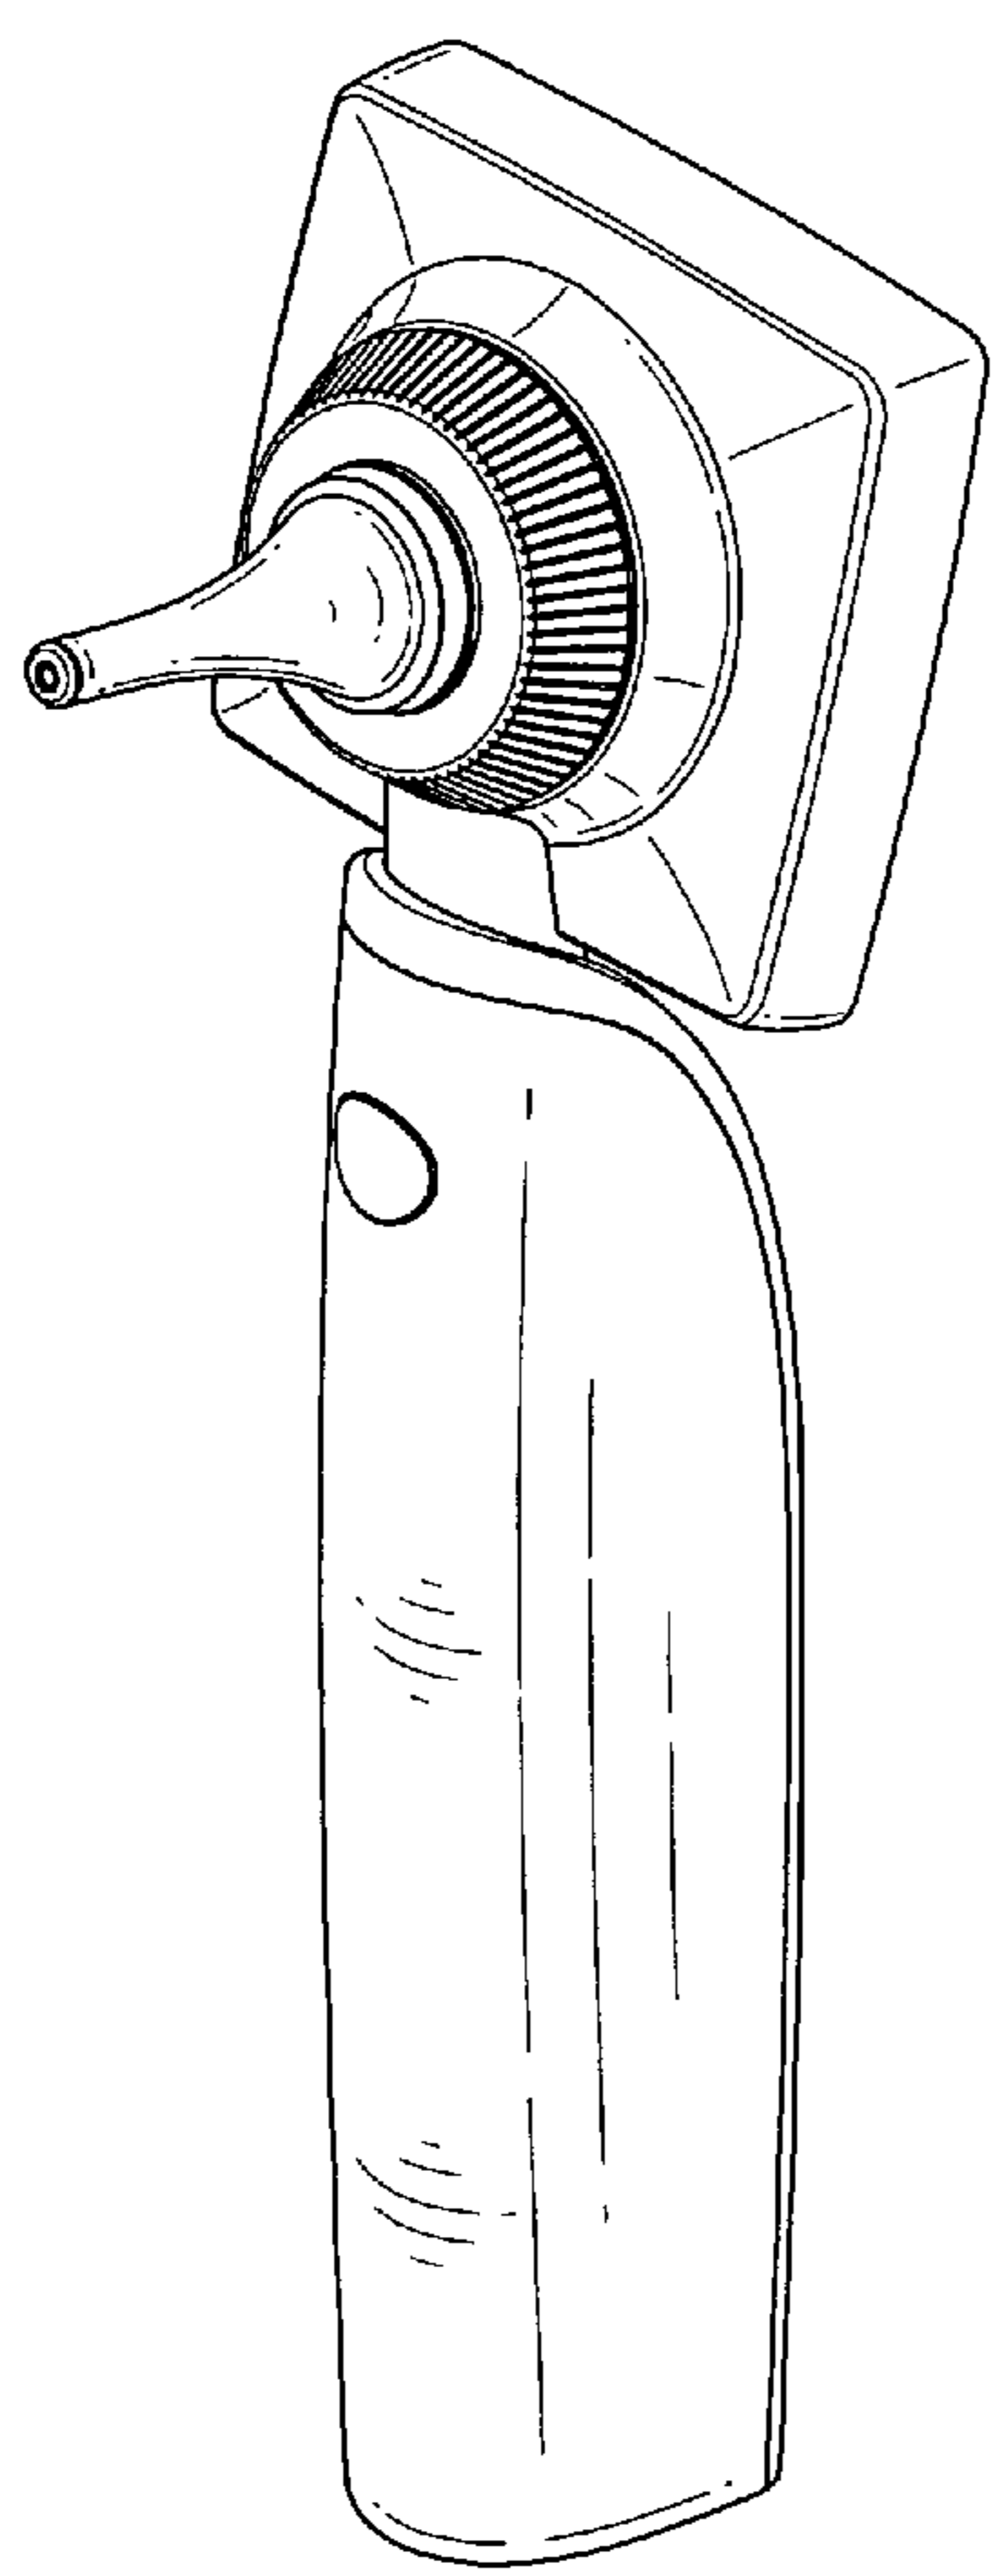

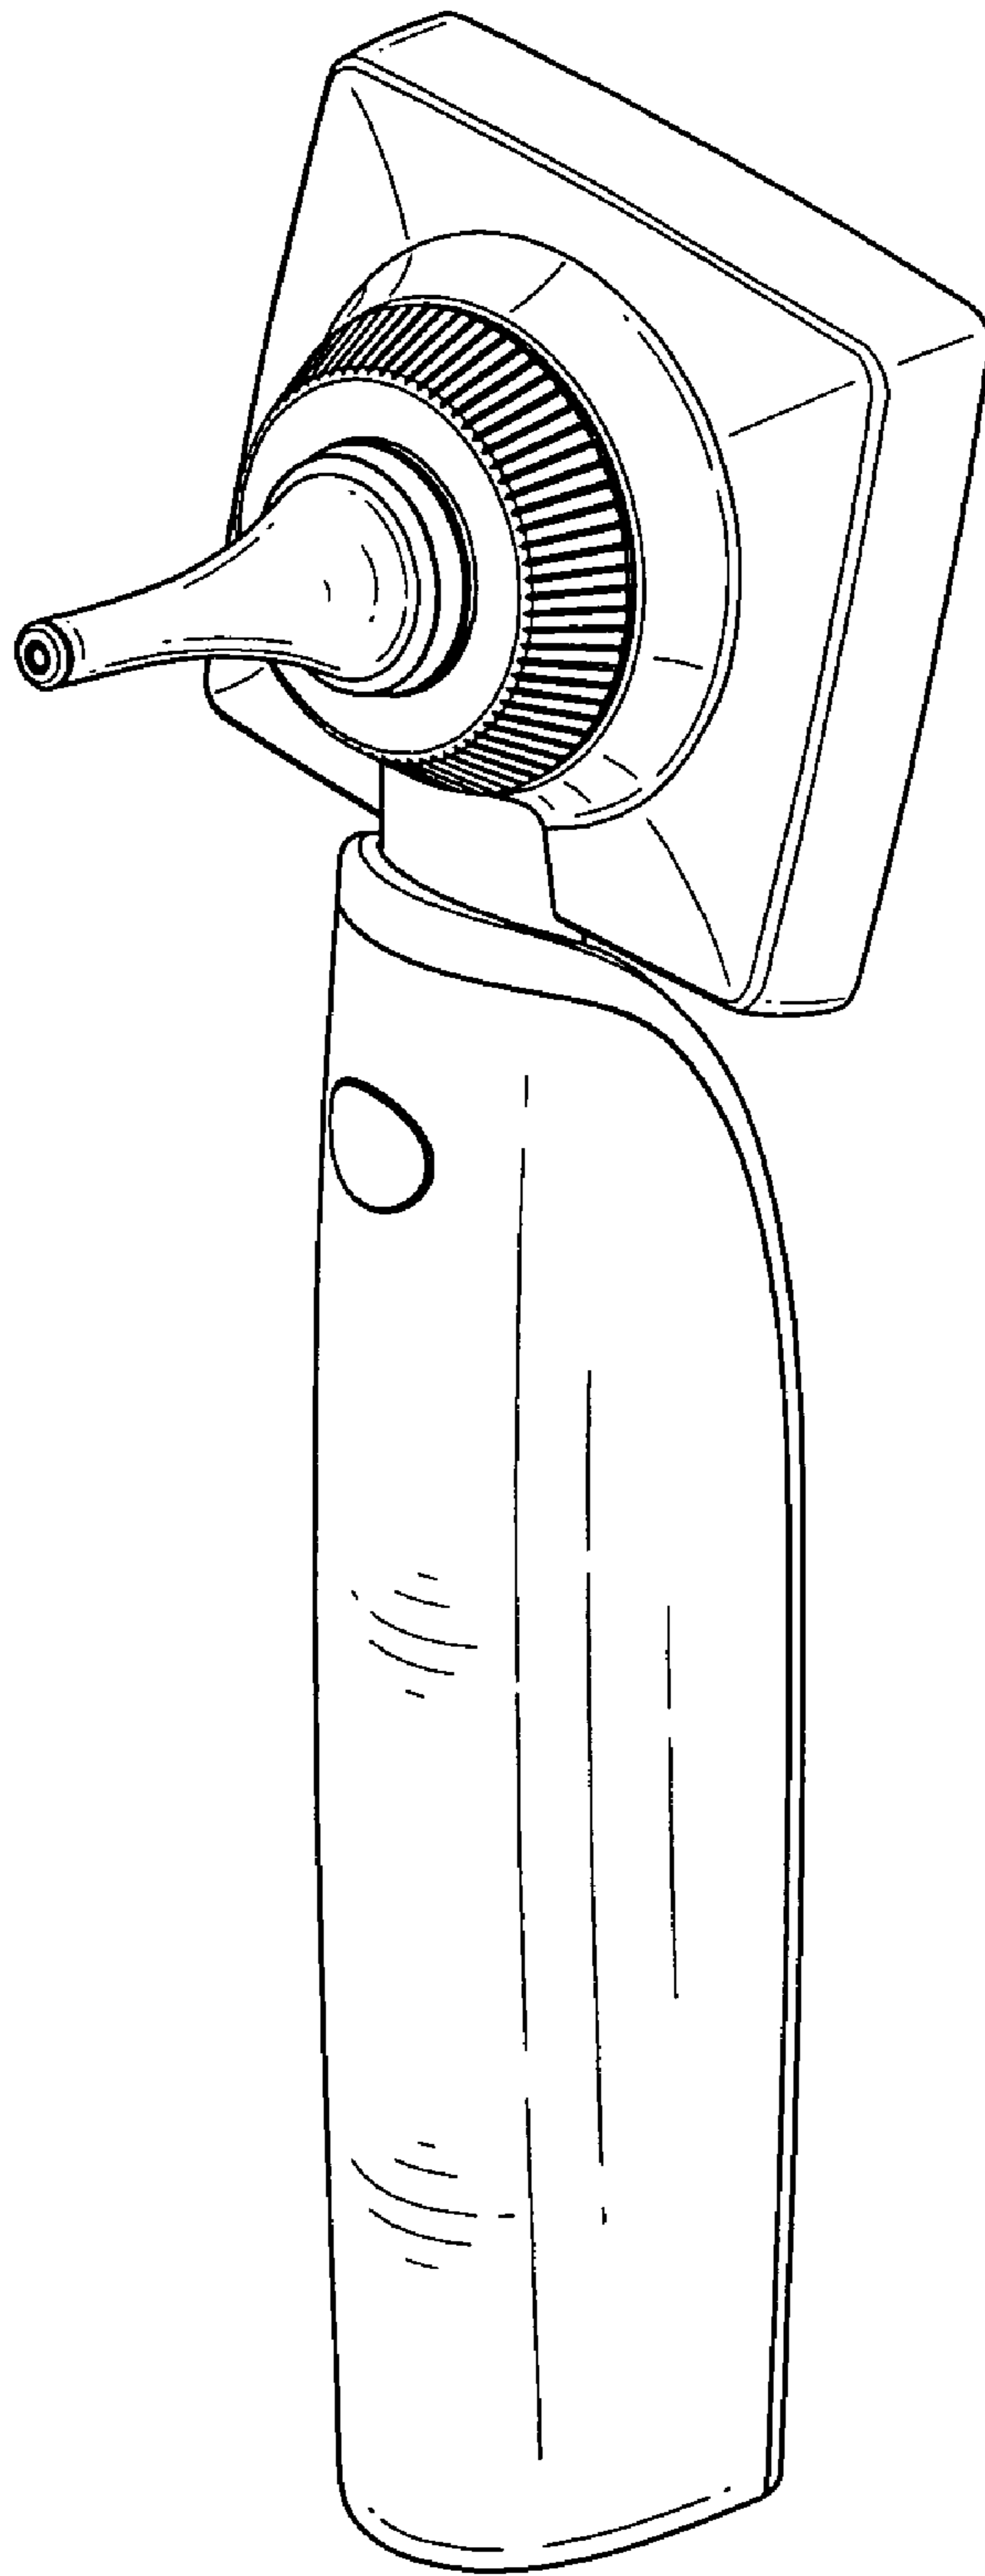


FIG. 1

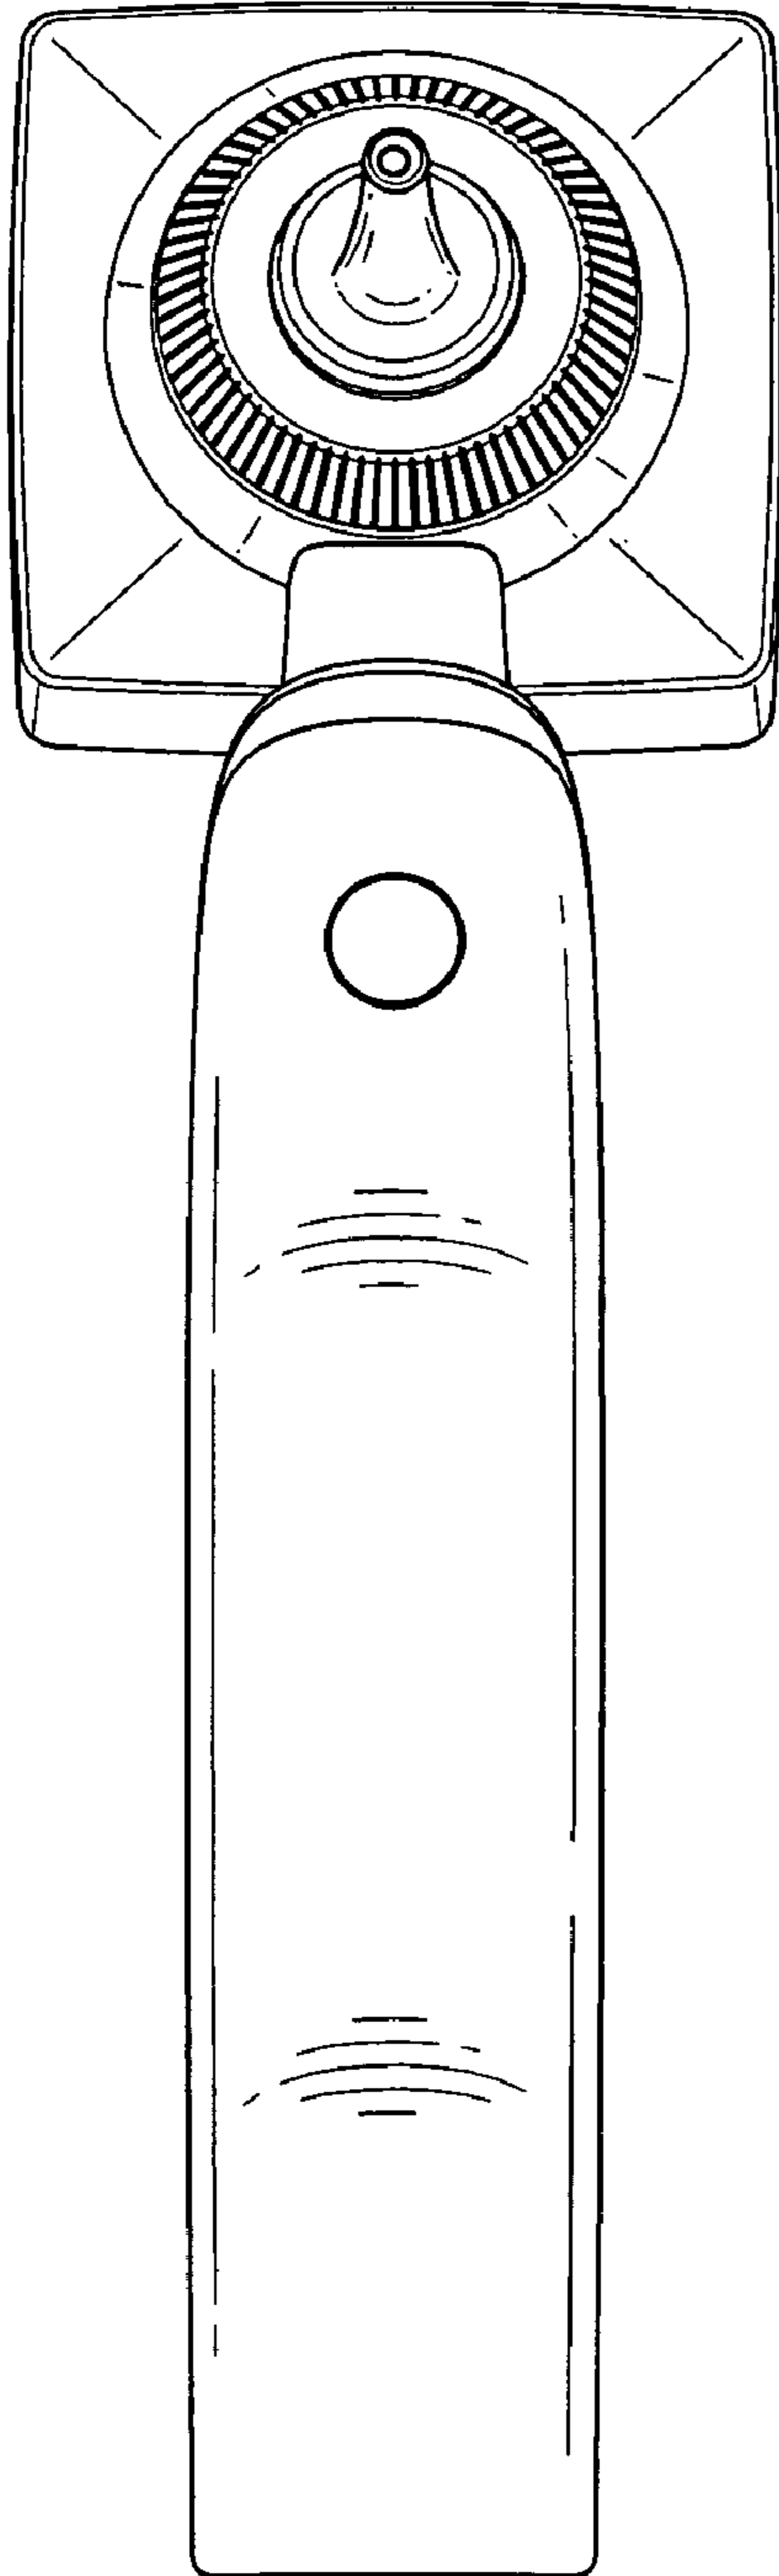


FIG. 2

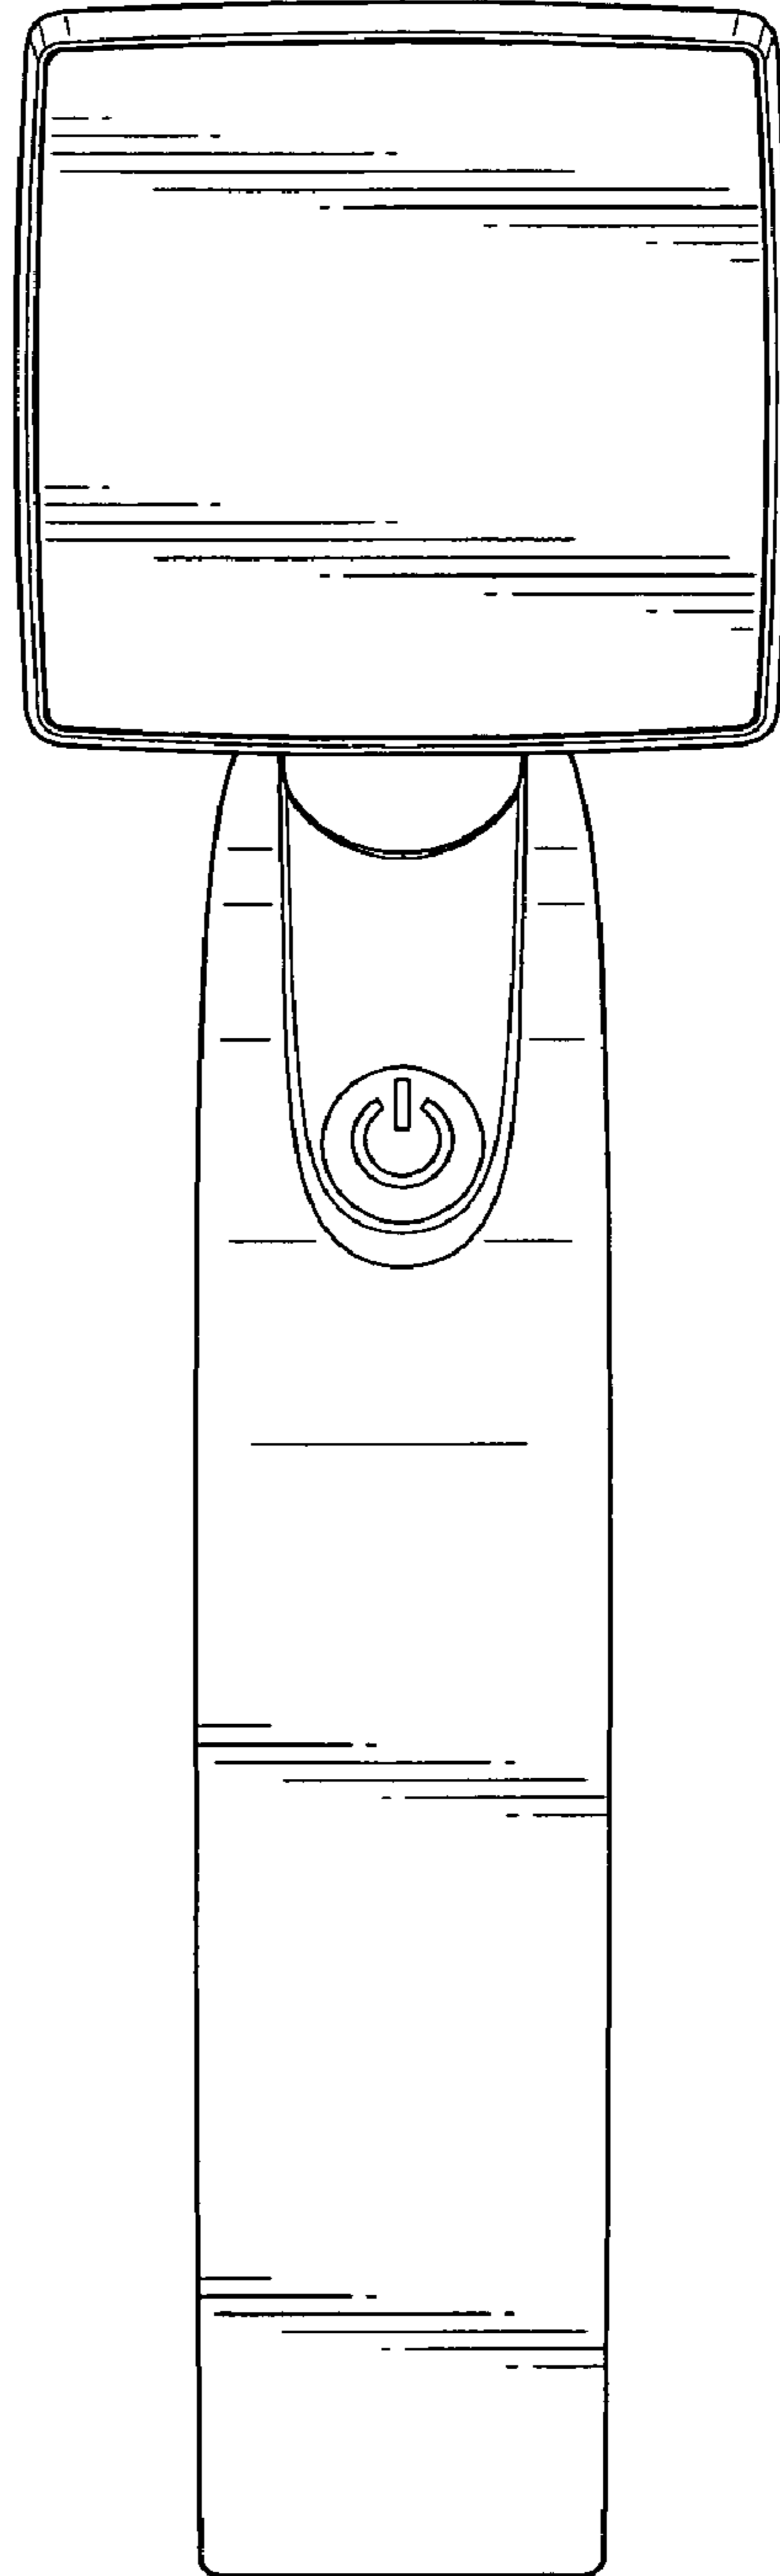


FIG. 3

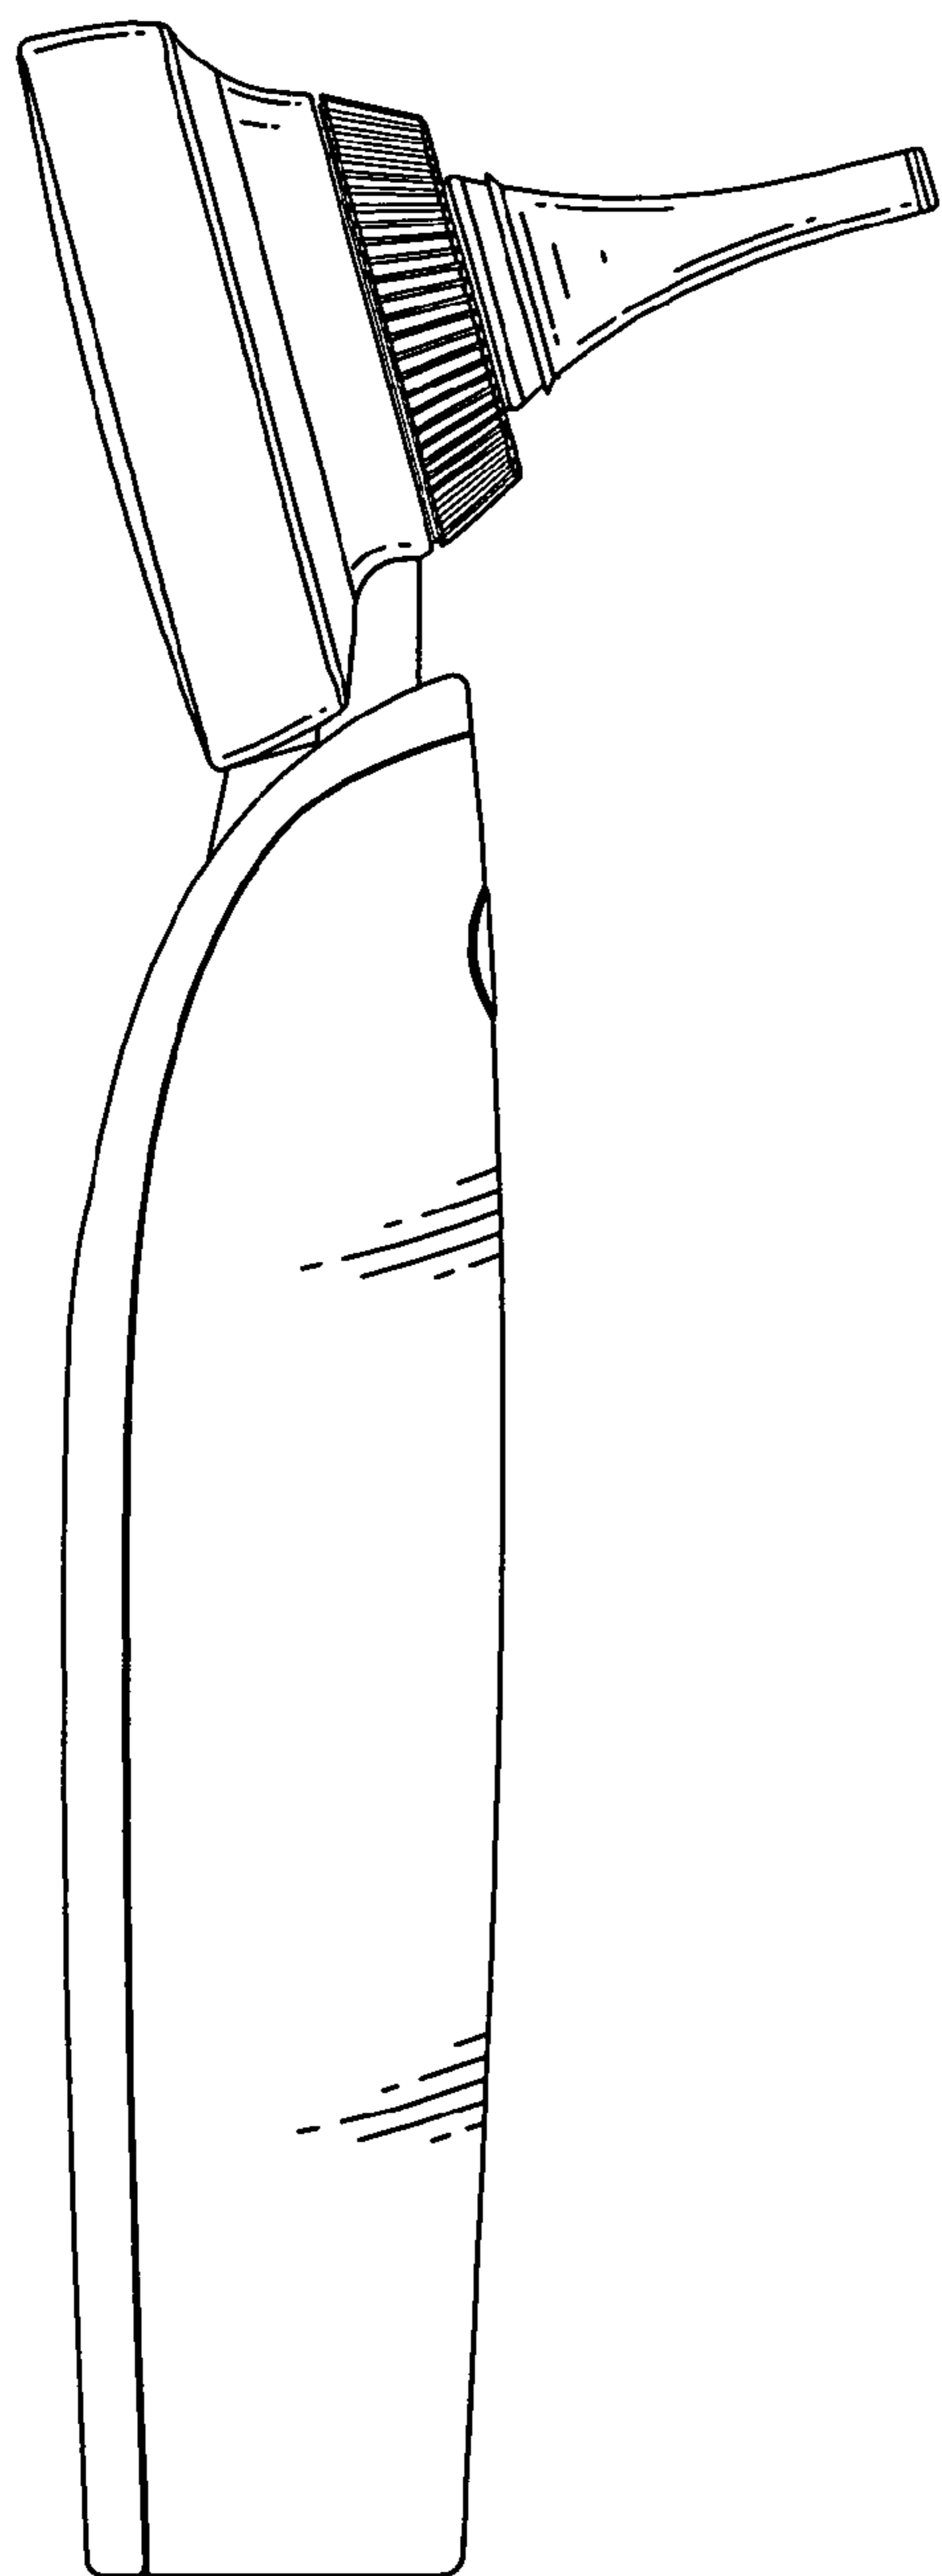


FIG. 4

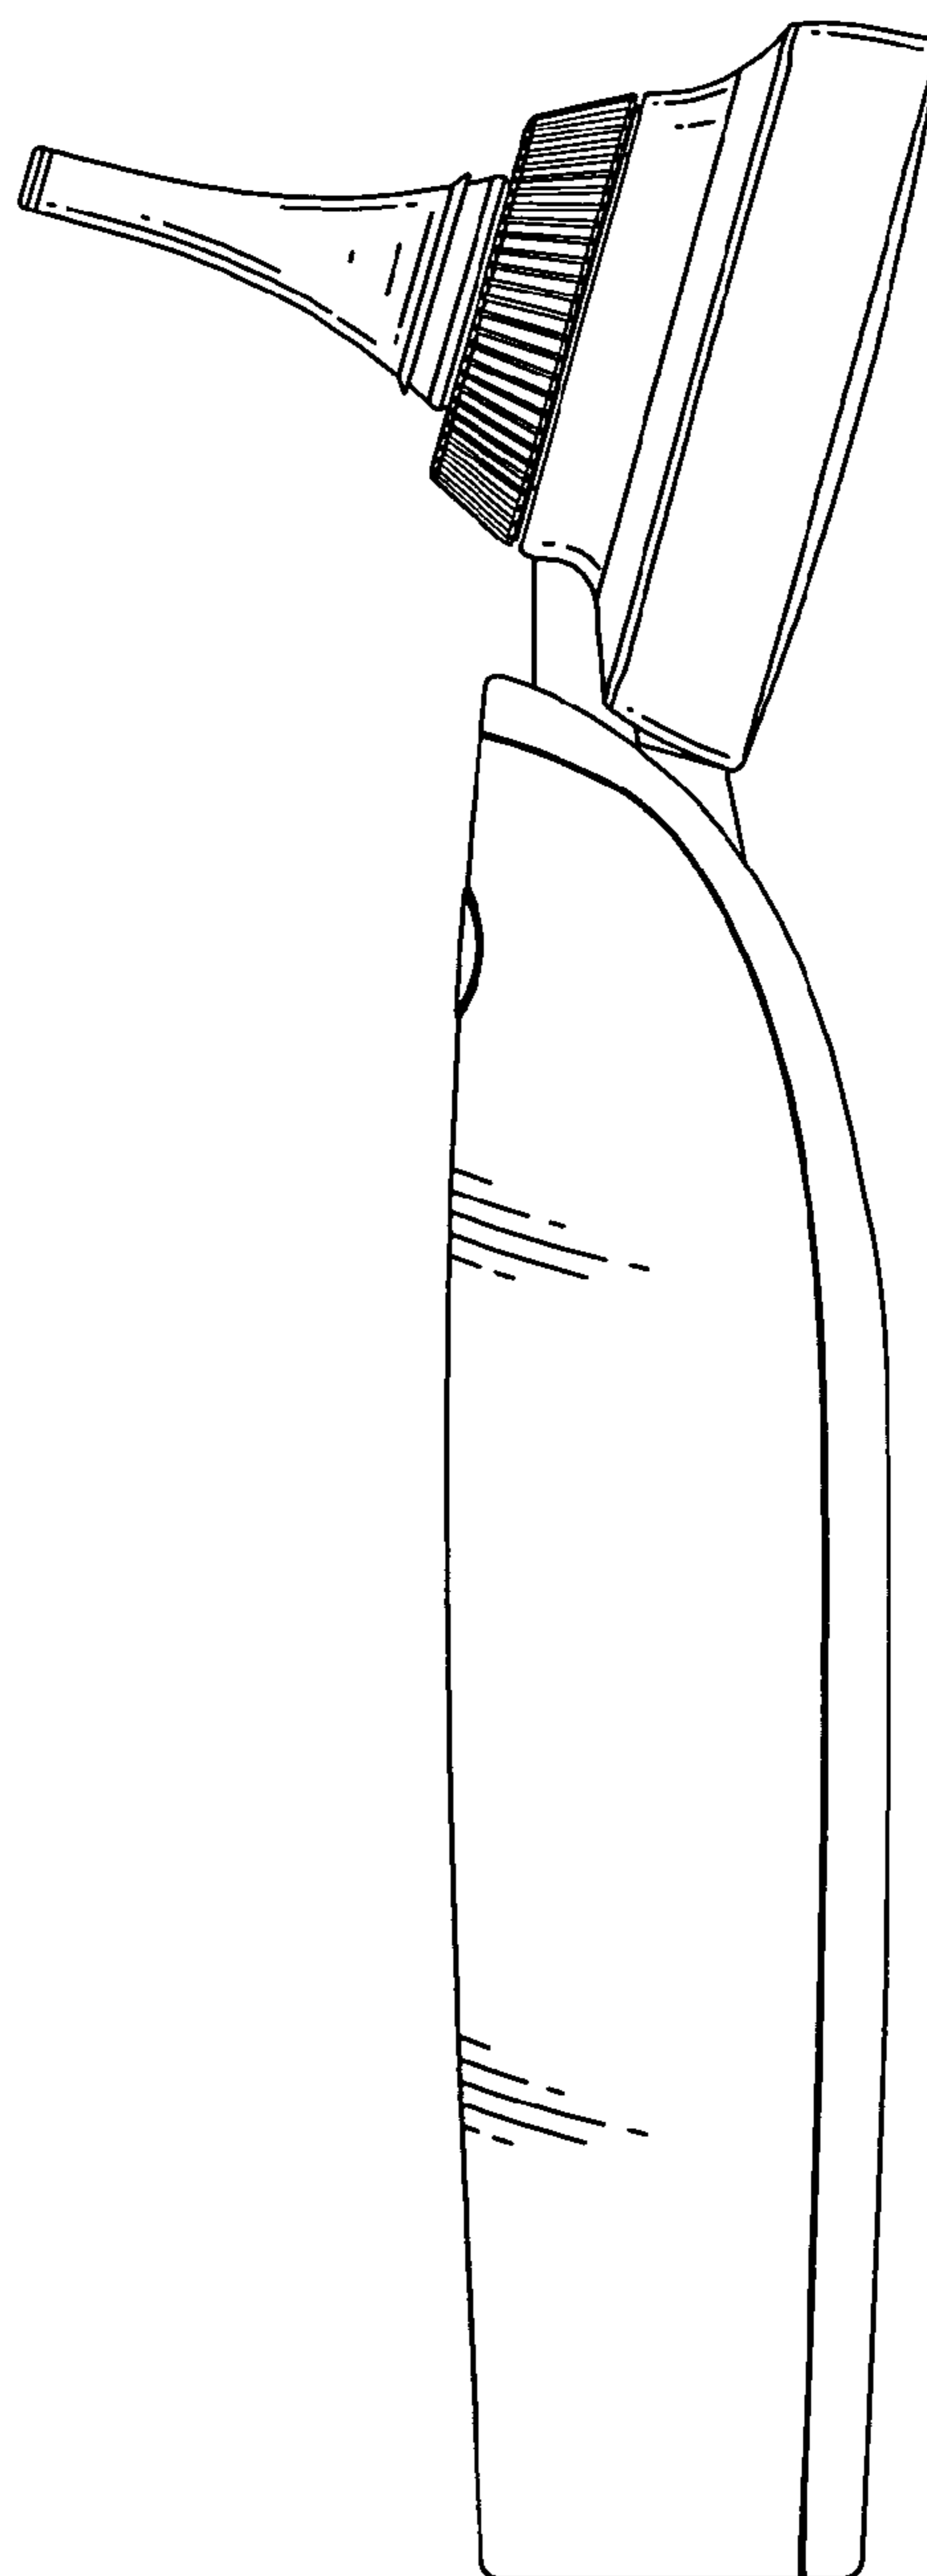


FIG. 5

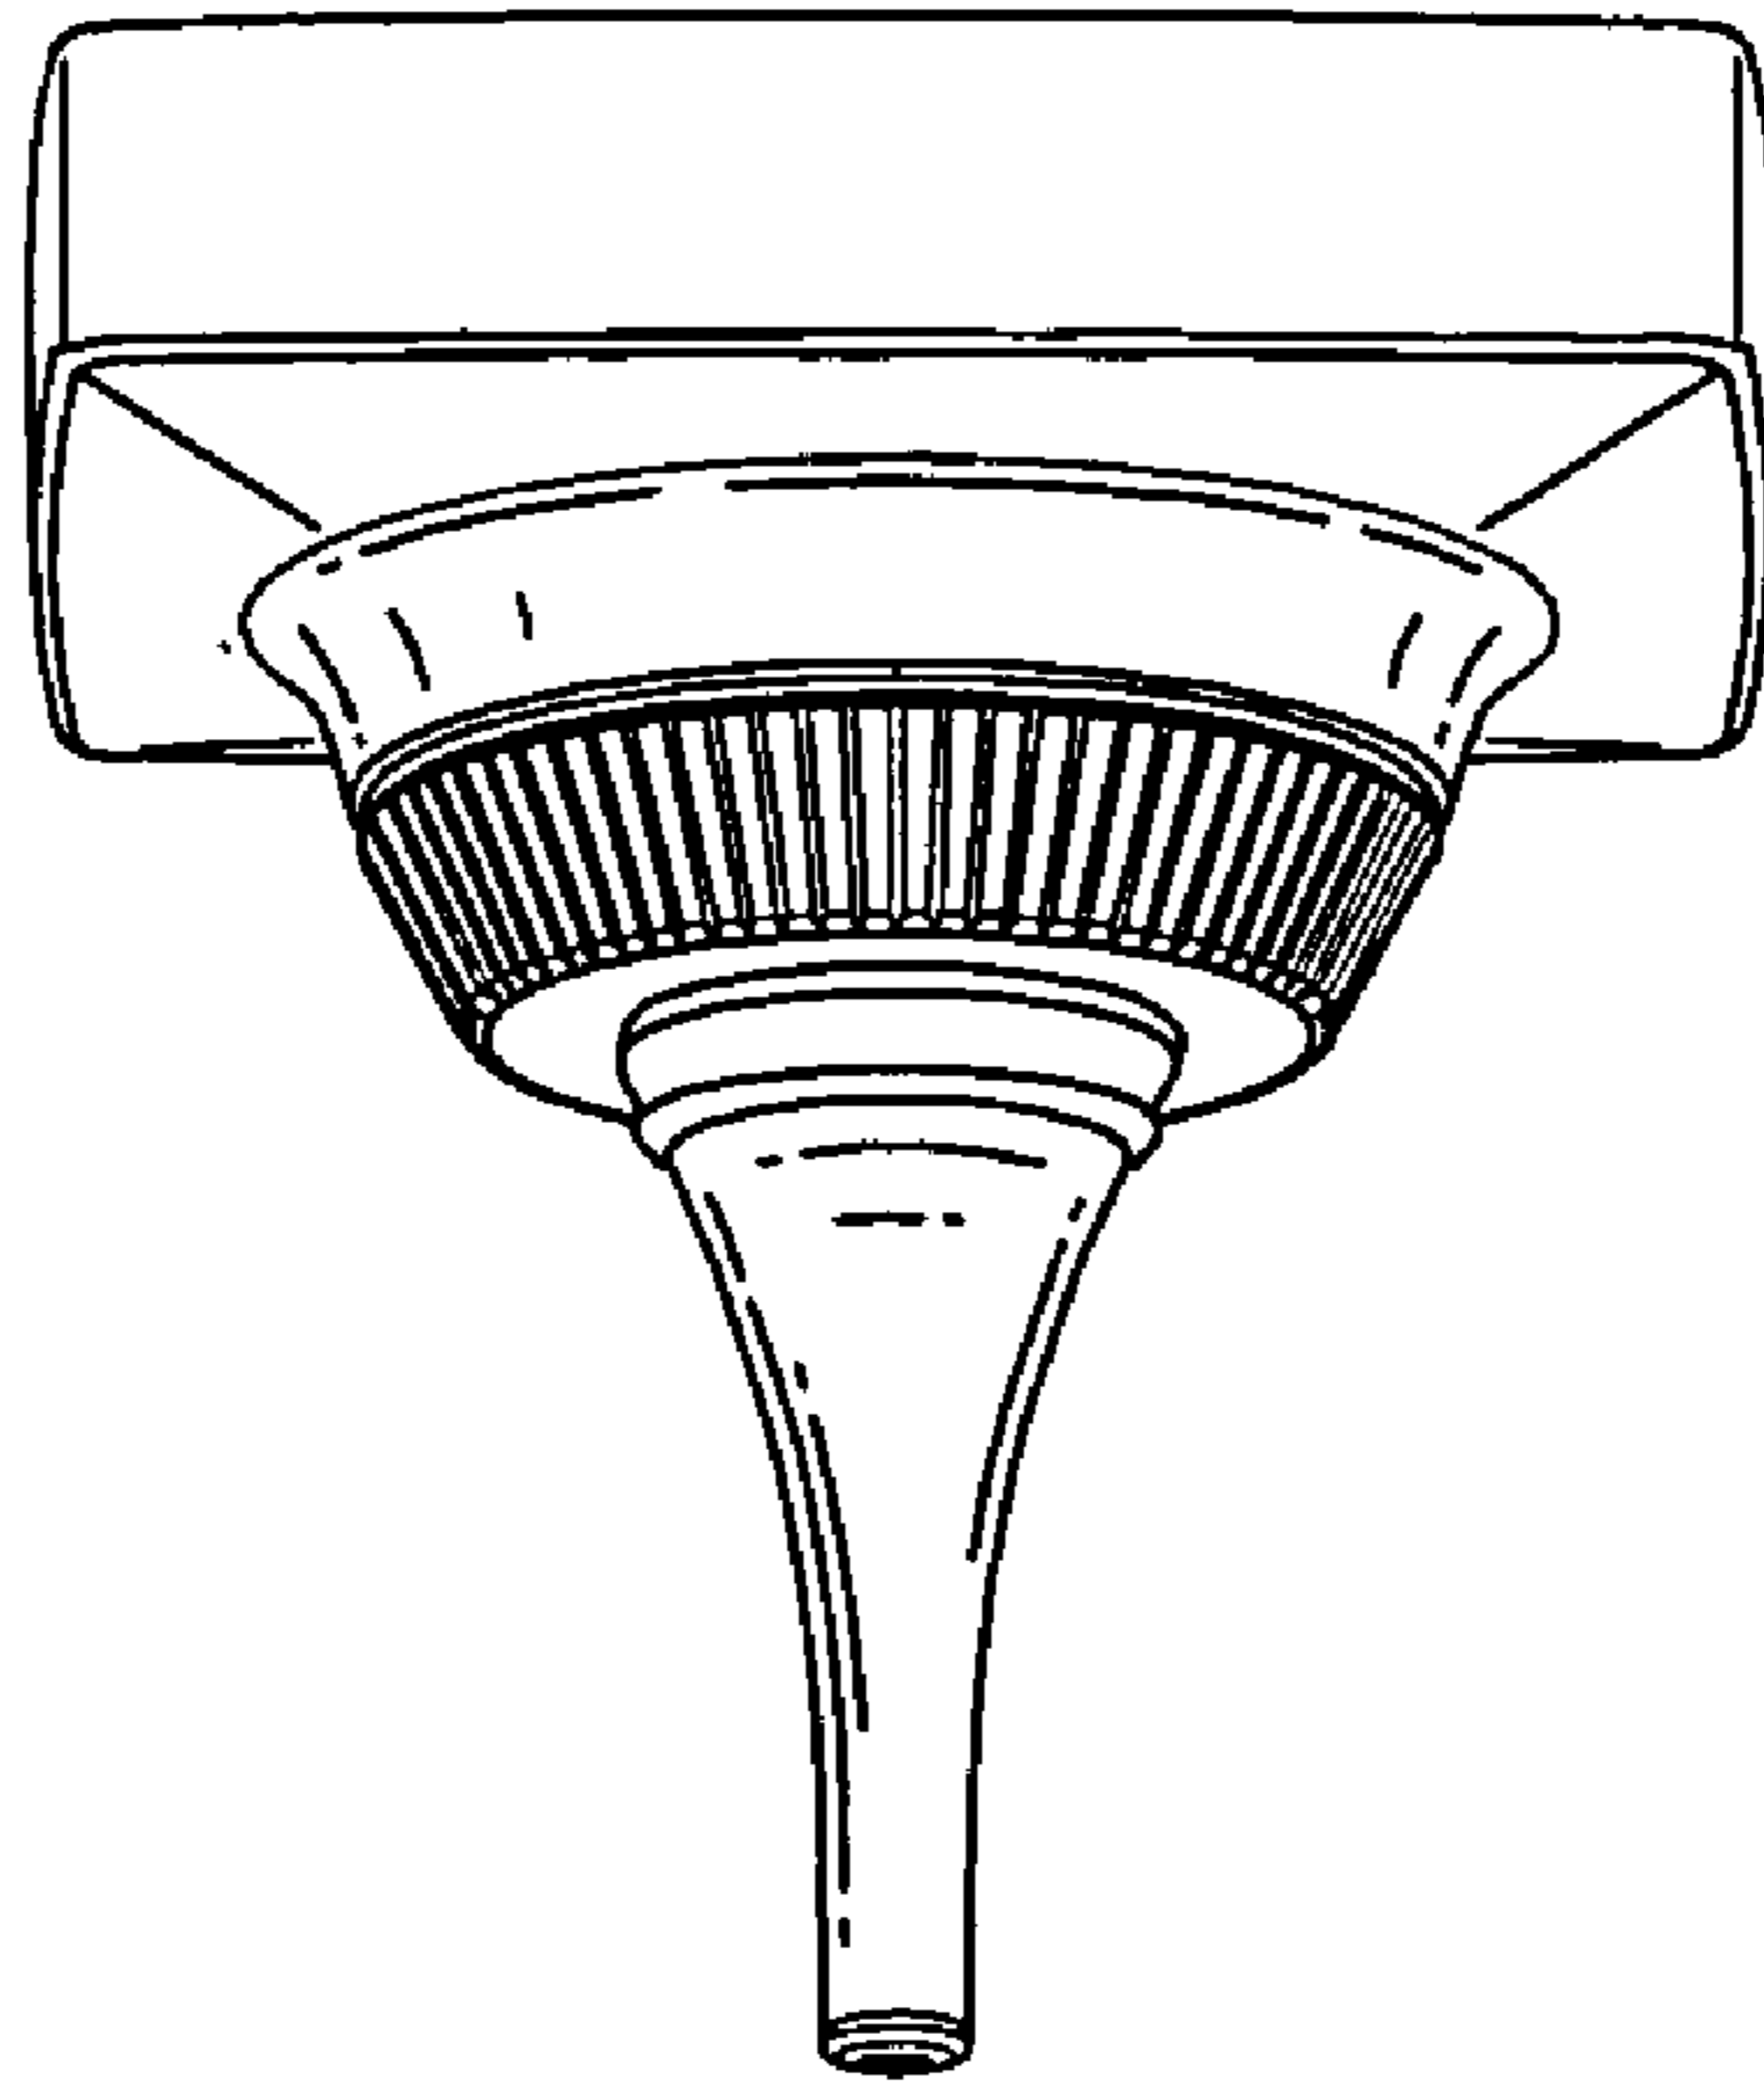


FIG. 6

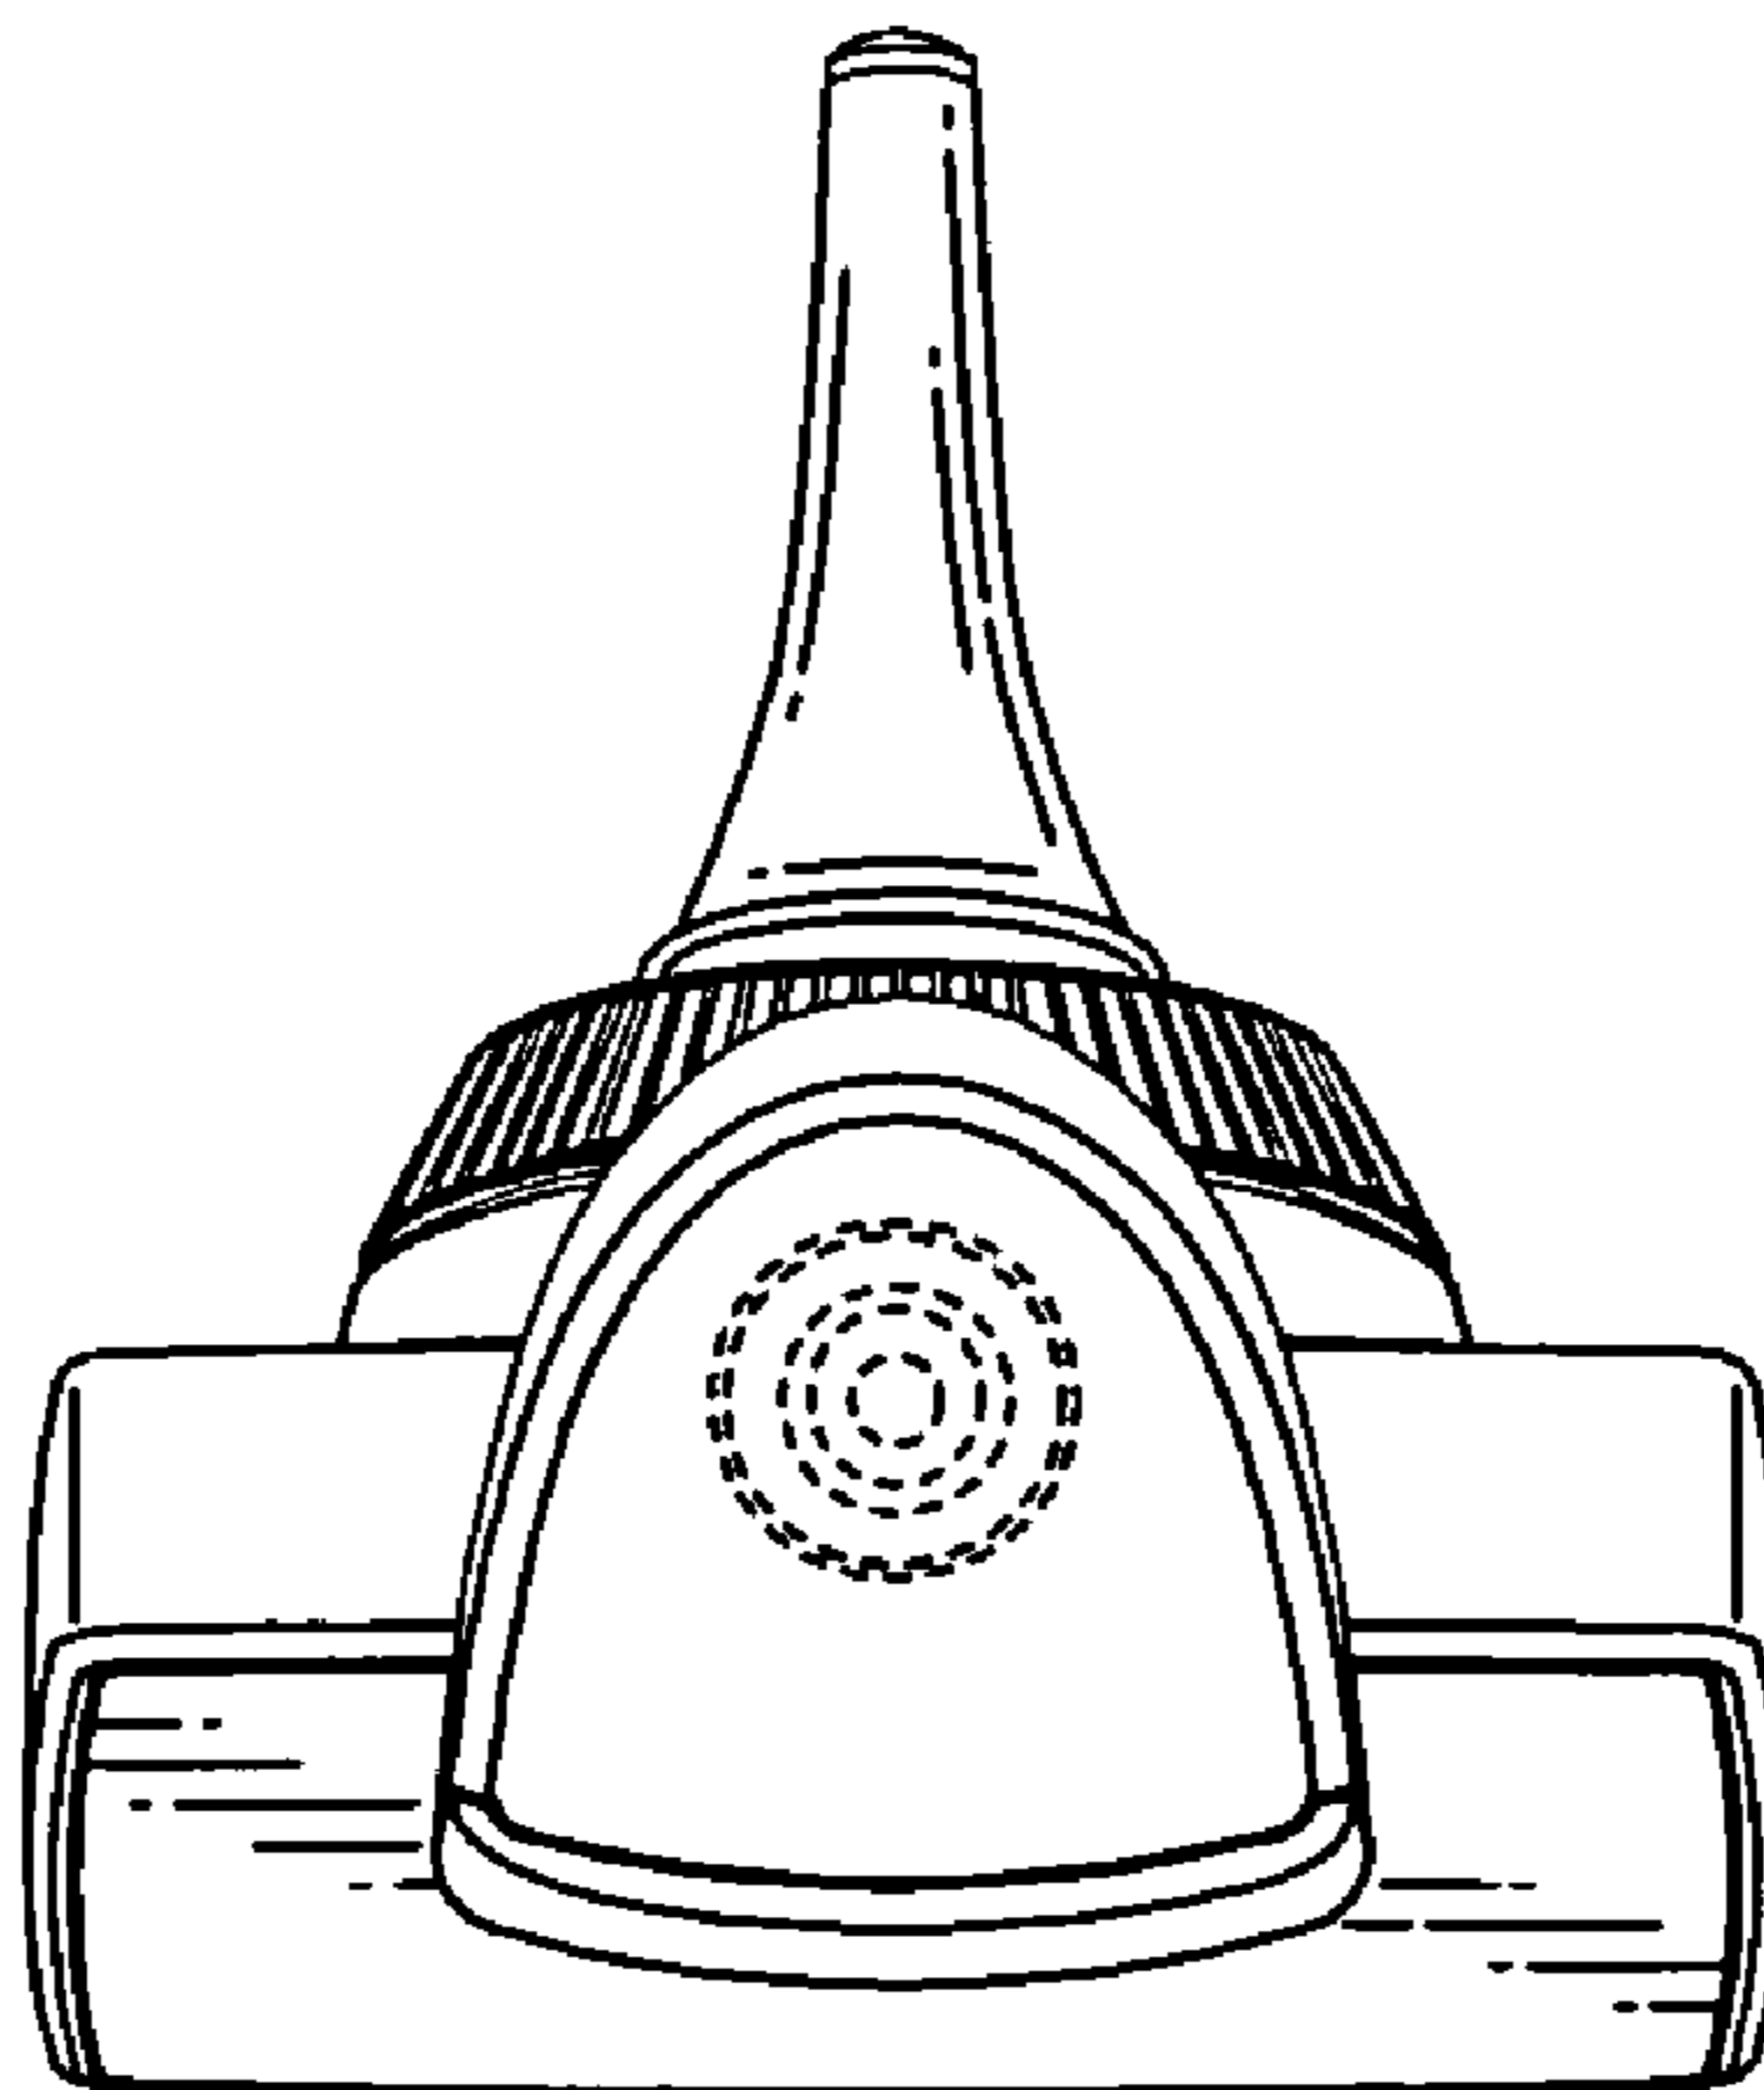


FIG. 7