

US00D635257S

(12) **United States Design Patent**
Ellman

(10) **Patent No.:** **US D635,257 S**
(45) **Date of Patent:** **** Mar. 29, 2011**

- (54) **OPHTHALMOSCOPE**
- (75) Inventor: **Marc Ellman**, El Paso, TX (US)
- (73) Assignee: **EyeQuick, LLC**, El Paso, TX (US)
- (**) Term: **14 Years**
- (21) Appl. No.: **29/365,664**
- (22) Filed: **Jul. 13, 2010**

- 6,112,114 A 8/2000 Dreher
 - D441,076 S 4/2001 Cooper et al.
 - 6,275,718 B1 8/2001 Lempert
 - 6,432,046 B1 8/2002 Yarush et al.
 - 6,511,420 B1 1/2003 Farrell et al.
- (Continued)

FOREIGN PATENT DOCUMENTS

WO WO/2006/086269 8/2006

OTHER PUBLICATIONS

“AMD-2020 Direct Ophthalmoscope”, AMD Global Telemedicine, available at <http://www.amdtelemedicine.com/telemedicine-equipment/ophthalmology/amd-2020-direct-ophthalmoscope.html>, last visited May 26, 2010.

(Continued)

Primary Examiner — Bridget L Eland

(74) *Attorney, Agent, or Firm* — Adam R. Stephenson, Ltd.

Related U.S. Application Data

- (62) Division of application No. 29/337,776, filed on May 29, 2009, now Pat. No. Des. 619,708.
- (51) **LOC (9) Cl.** **24-02**
- (52) **U.S. Cl.** **D24/137; D24/150**
- (58) **Field of Classification Search** D24/137, D24/138, 150, 172; 351/218, 221, 205, 206; 606/4

See application file for complete search history.

(57) **CLAIM**

The ornamental design for an ophthalmoscope, as shown and described.

(56) **References Cited**

U.S. PATENT DOCUMENTS


- D189,554 S 1/1961 Armbruster
- D207,371 S 4/1967 Pulos
- D221,255 S 7/1971 Heine
- D231,949 S 6/1974 Pulos
- 3,861,789 A * 1/1975 Heine 351/218
- D238,100 S 12/1975 Pulos
- 4,208,107 A 6/1980 Oharek
- 4,265,518 A 5/1981 Matsumura
- 4,304,483 A 12/1981 Whitten
- 4,742,819 A 5/1988 George
- 4,938,584 A 7/1990 Suematsu et al.
- 5,200,772 A * 4/1993 Perkins et al. 351/213
- 5,459,535 A * 10/1995 Cleveland et al. 351/218
- 5,599,276 A 2/1997 Hauptli et al.
- D379,514 S 5/1997 Laun et al.
- 5,658,235 A 8/1997 Priest et al.
- 5,885,214 A 3/1999 Monroe et al.
- D426,920 S 6/2000 Georgescu

DESCRIPTION

FIG. 1 is a rear perspective view of an ophthalmoscope; FIG. 2 is a left side view thereof; FIG. 3 is a right side view thereof; FIG. 4 is a front view thereof; FIG. 5 is a rear view thereof; FIG. 6 is a top view thereof; and, FIG. 7 is a bottom view thereof.

The broken lines immediately adjacent the shaded areas that define unshaded regions represent the bounds of the claimed design while all other broken lines are directed to environment and are for illustrative purposes only; the broken lines form no part of the claimed design.

1 Claim, 6 Drawing Sheets

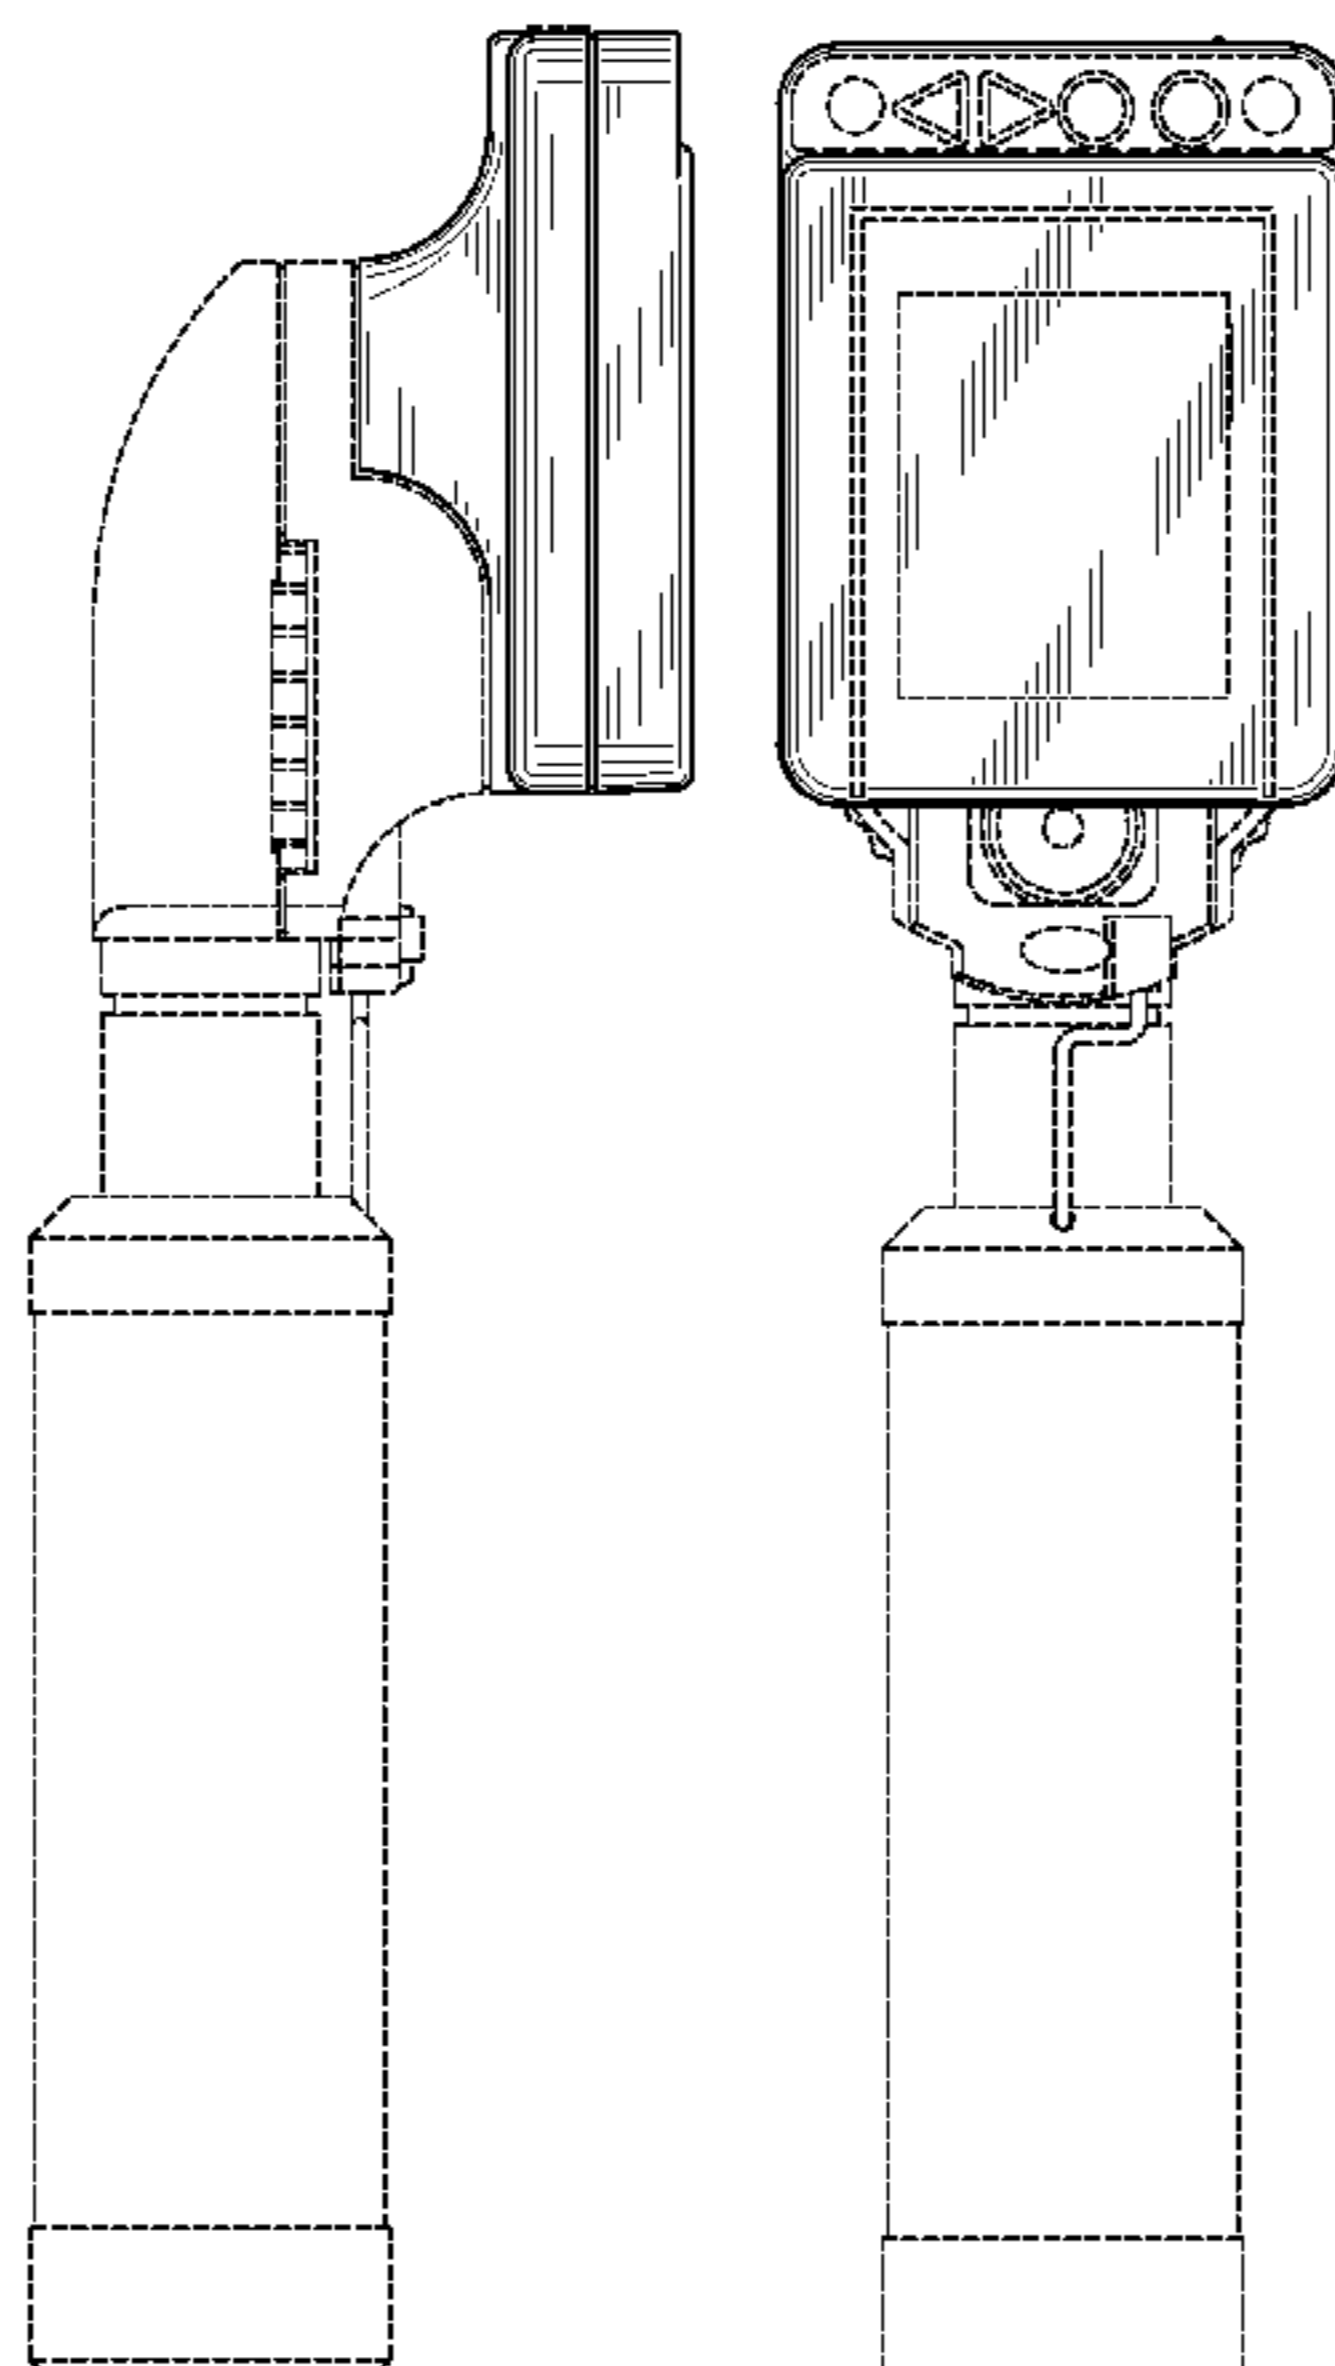

US D635,257 S

Page 2

U.S. PATENT DOCUMENTS

6,554,765 B1 4/2003 Yarush et al.
6,743,168 B2 6/2004 Luloh et al.
6,761,561 B2 7/2004 Mandelkern et al.
6,862,036 B2 3/2005 Adair et al.
7,086,859 B2 8/2006 Gregorio et al.
7,211,042 B2 5/2007 Chatenever et al.
7,237,896 B2 7/2007 Silverbrook et al.
D550,842 S 9/2007 Koch et al.
7,290,882 B2 11/2007 Collins et al.
7,364,297 B2 4/2008 Goldfain et al.
D618,346 S * 6/2010 Sisko et al. D24/137

D618,794 S * 6/2010 Onuma D24/137
2005/0110949 A1 5/2005 Goldfain et al.
2005/0171399 A1 8/2005 Rich et al.
2007/0106117 A1 5/2007 Yokota
2008/0002152 A1 1/2008 Collins et al.

OTHER PUBLICATIONS

James Tyrrell, "Ophthalmoscope Goes Digital", optics.org (Jul. 30, 2004) <http://optics.org/cws/article/research/19973>, last visited Jun. 24, 2010.

* cited by examiner

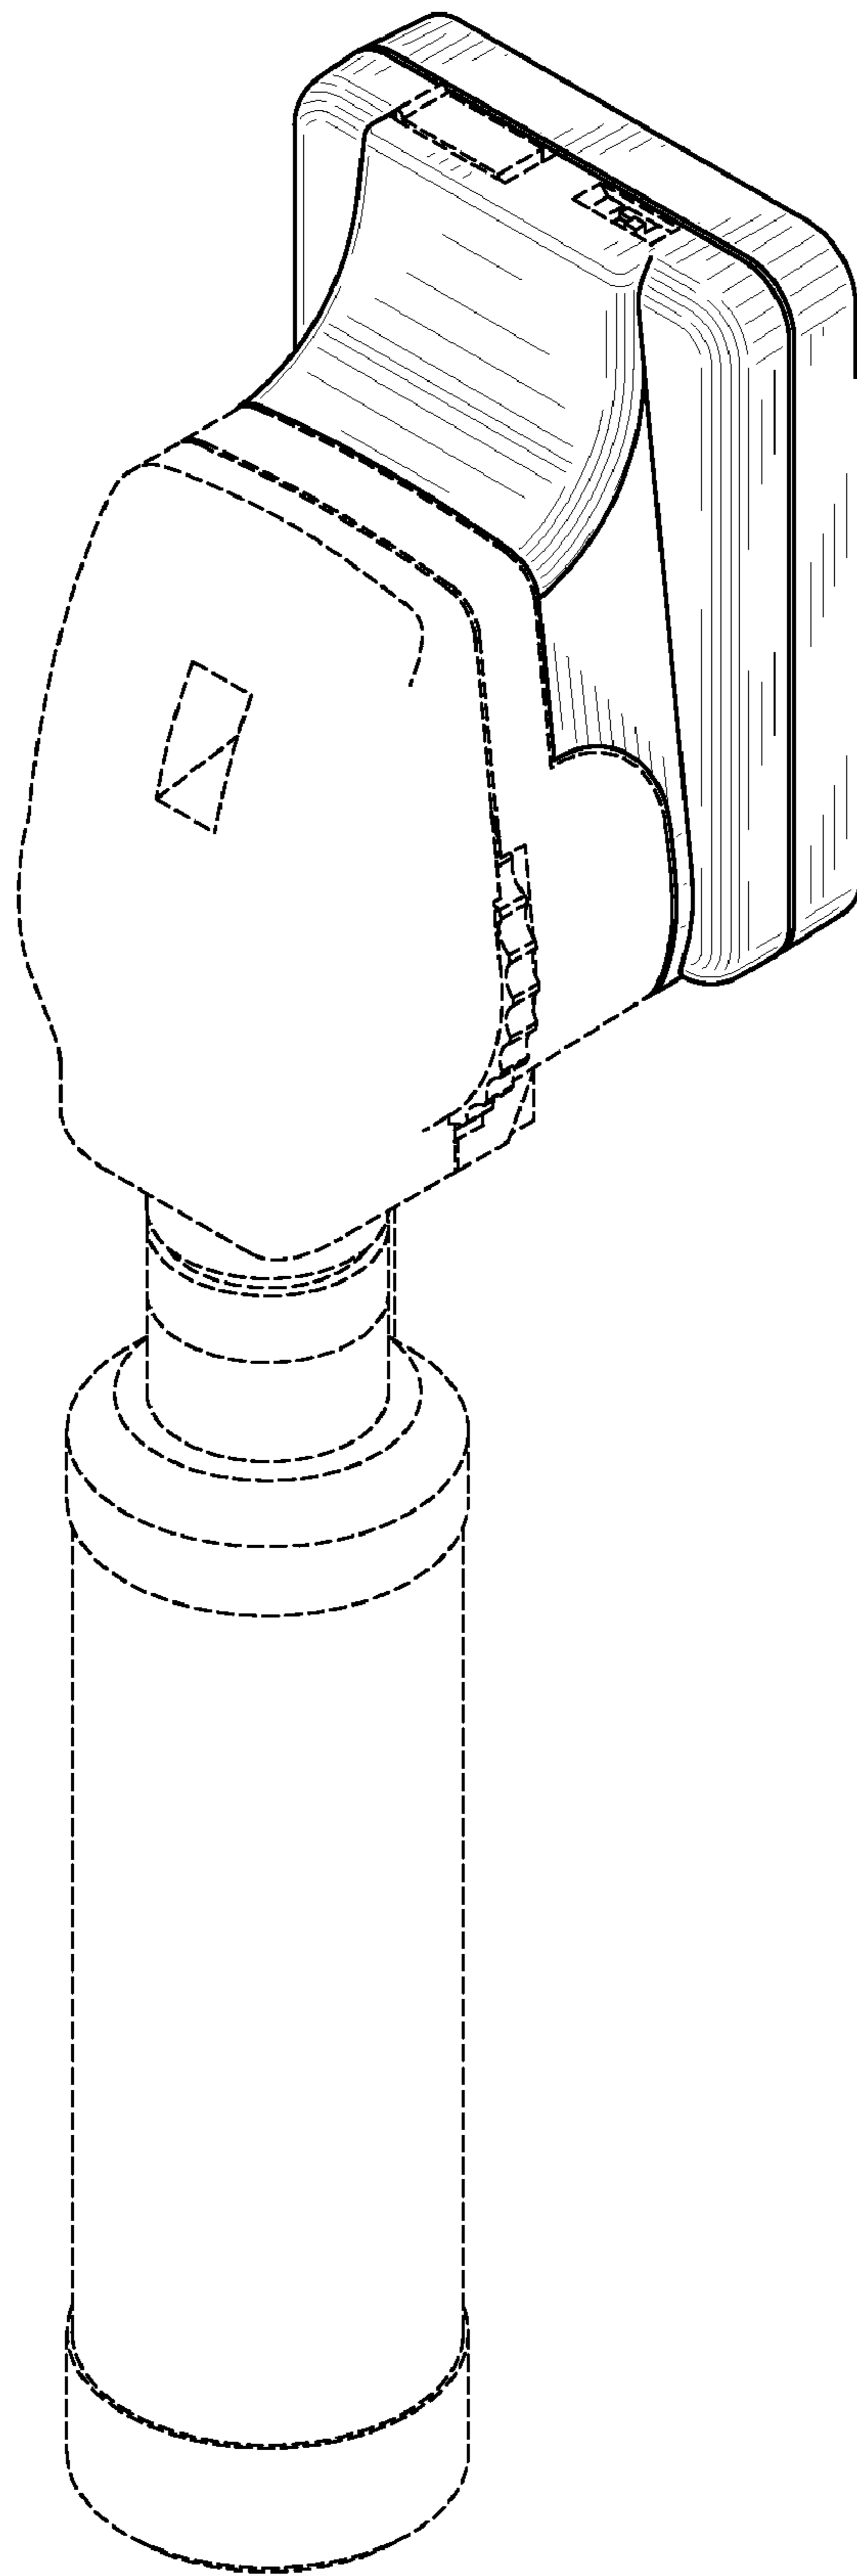


FIG. 1

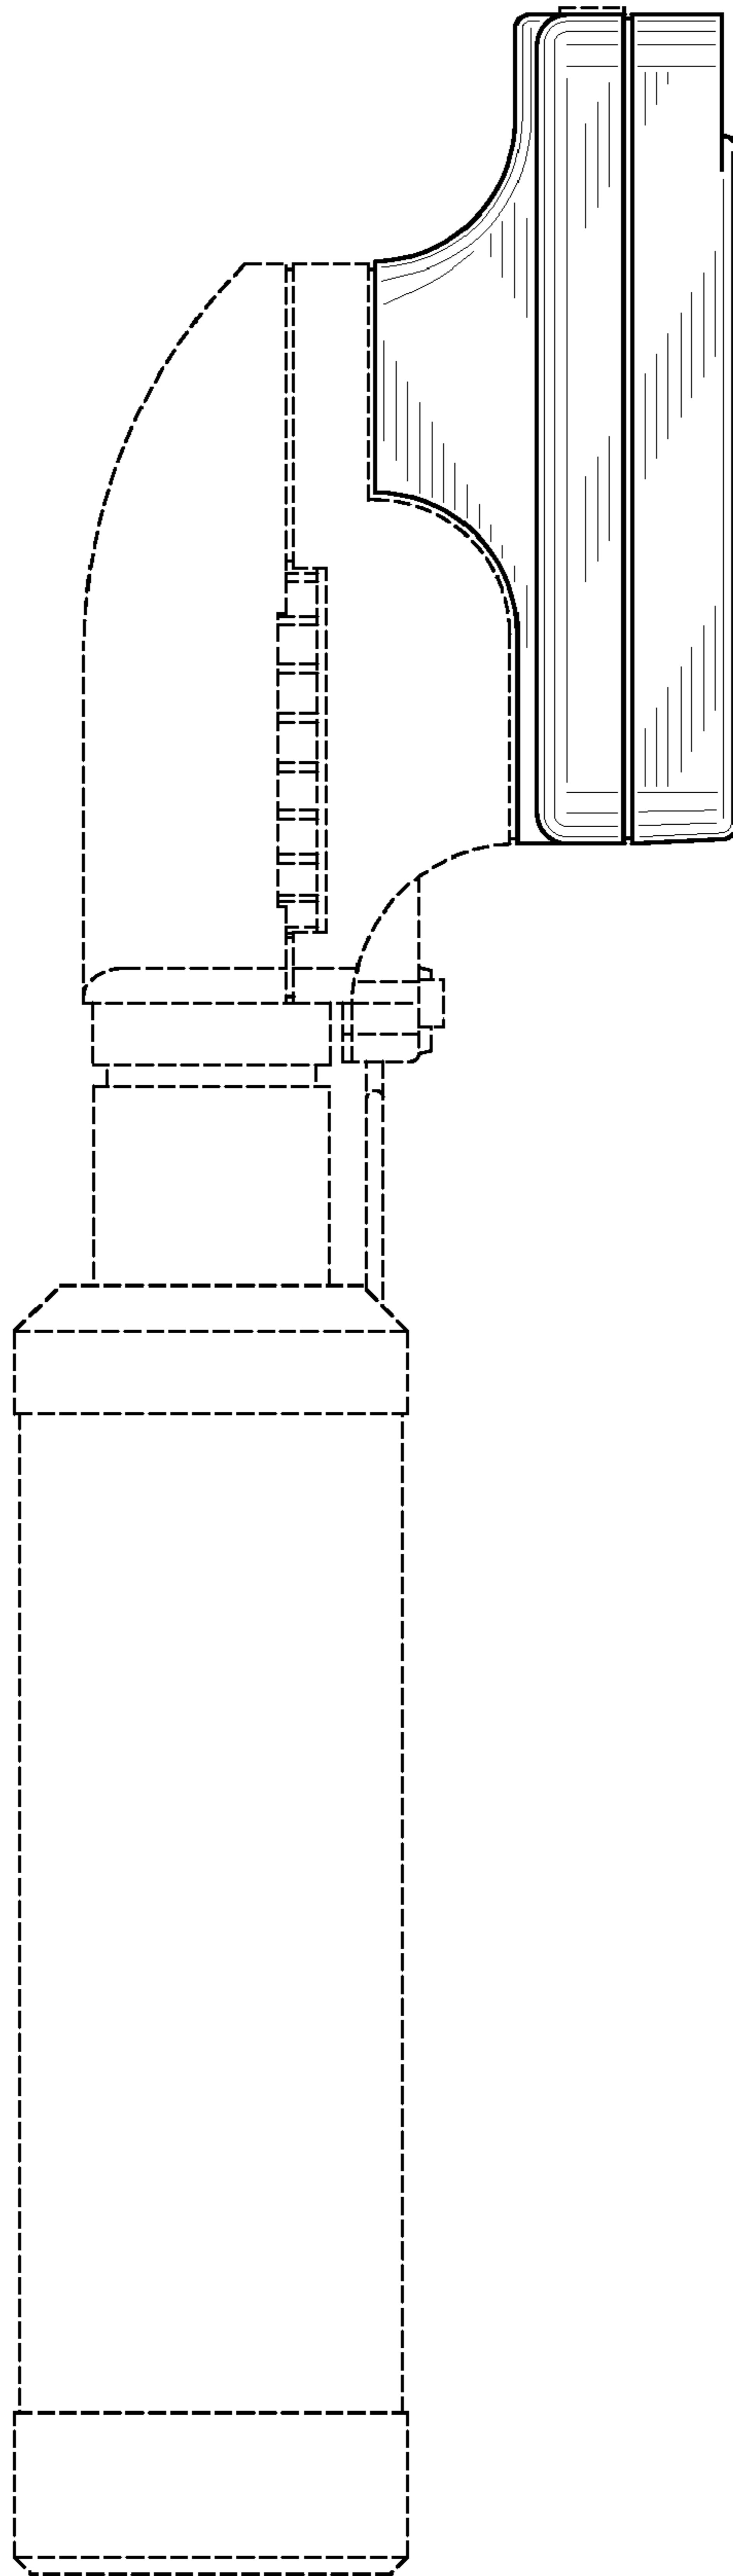


FIG. 2

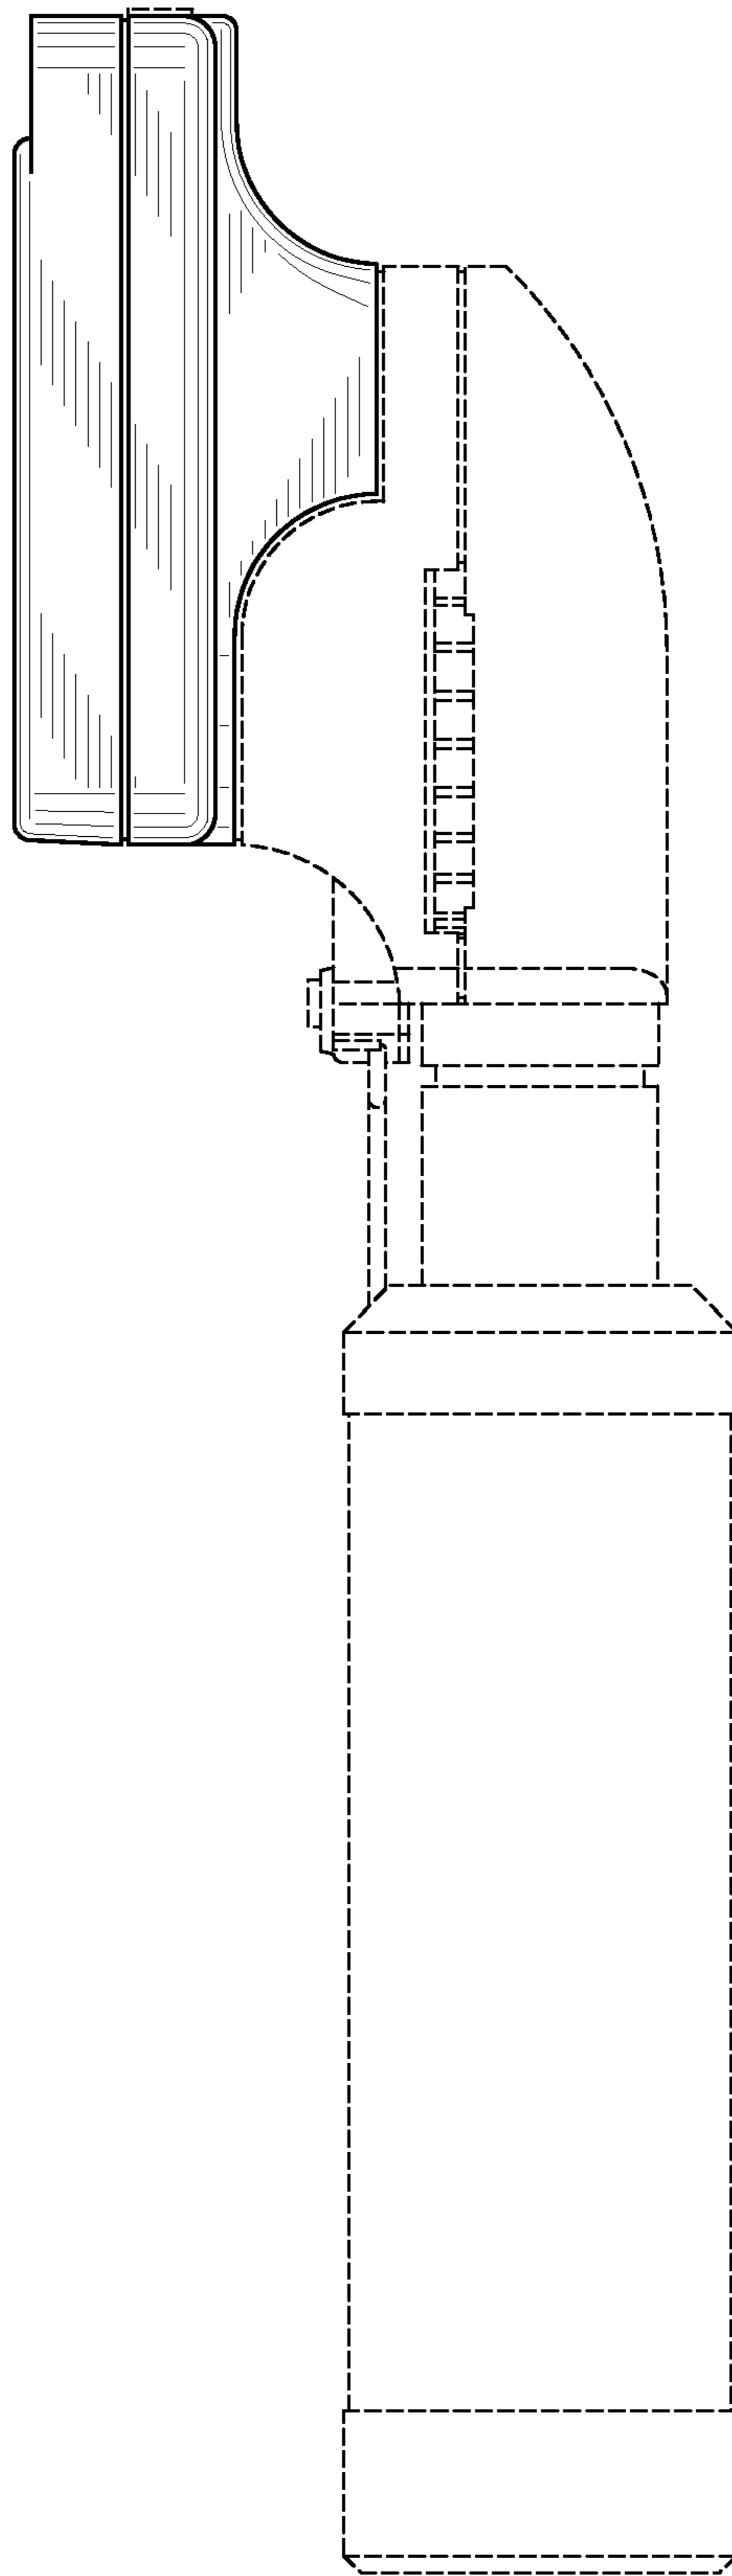


FIG. 3

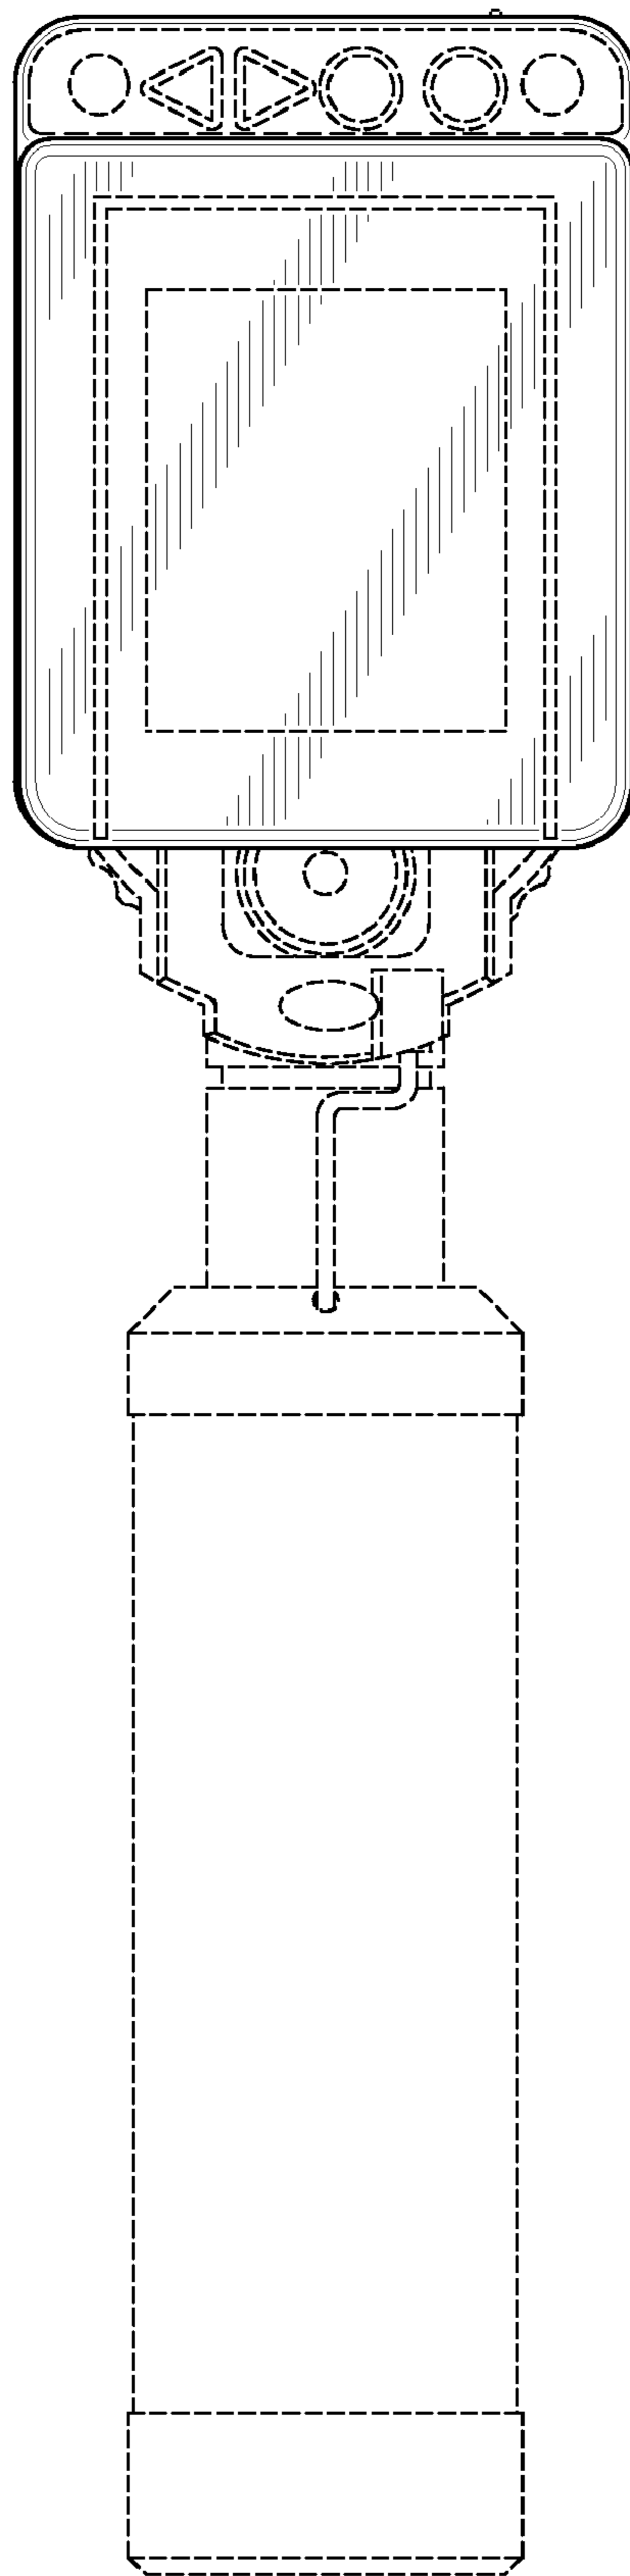


FIG. 4

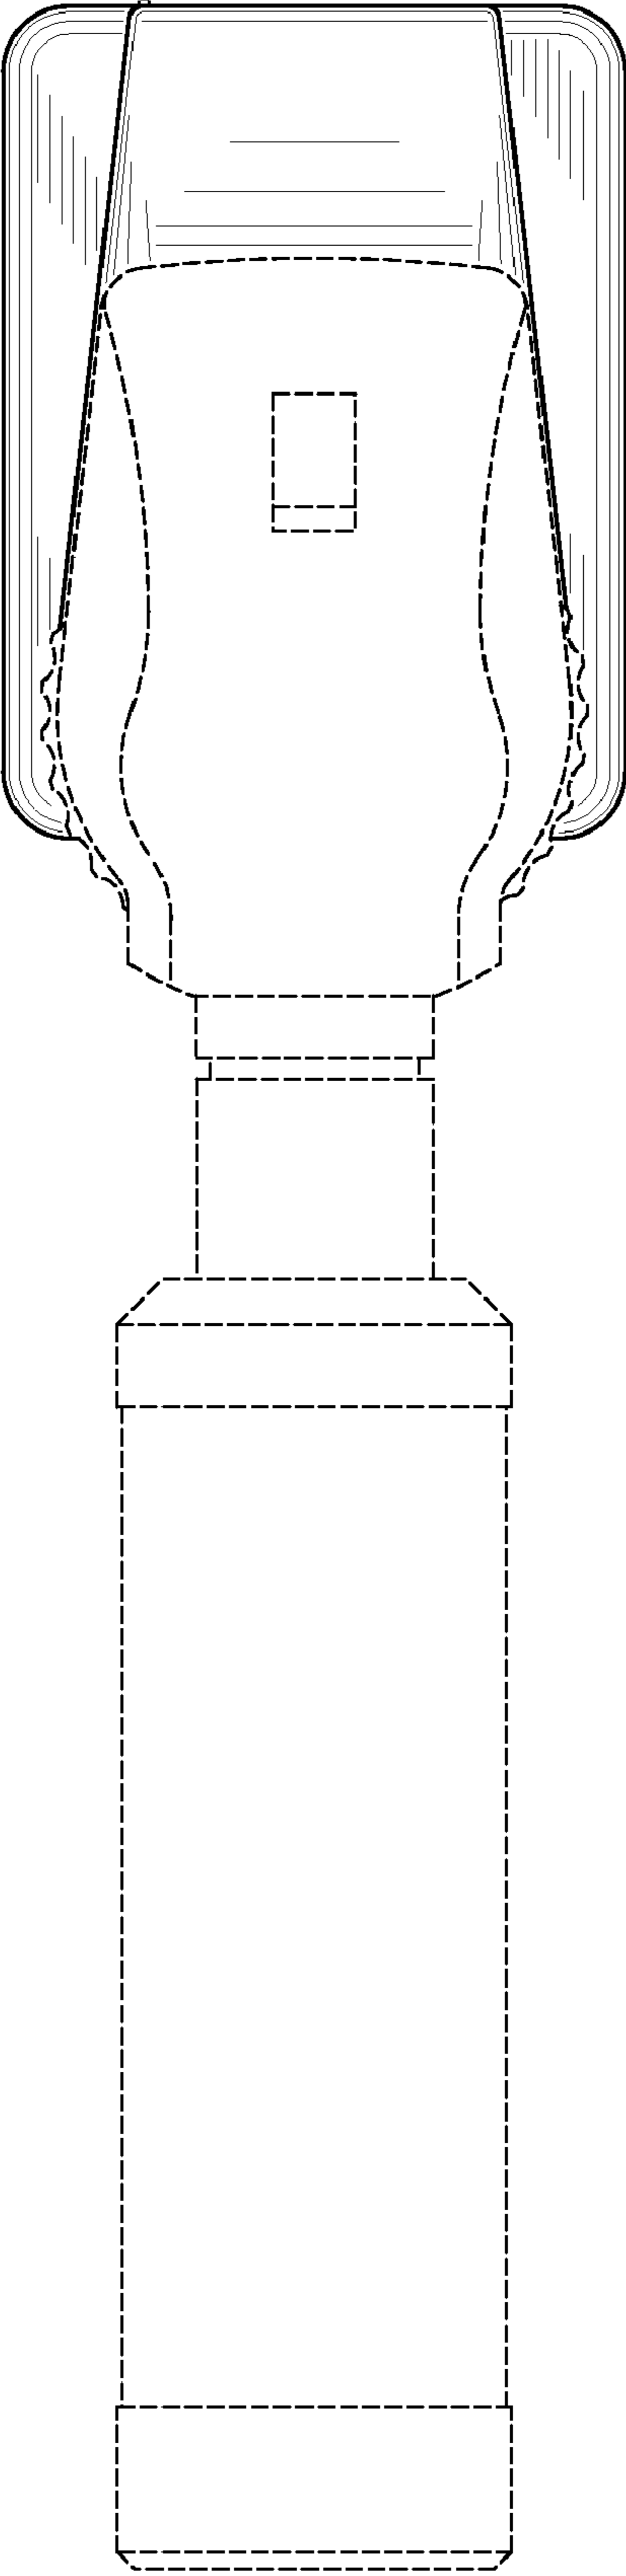


FIG. 5

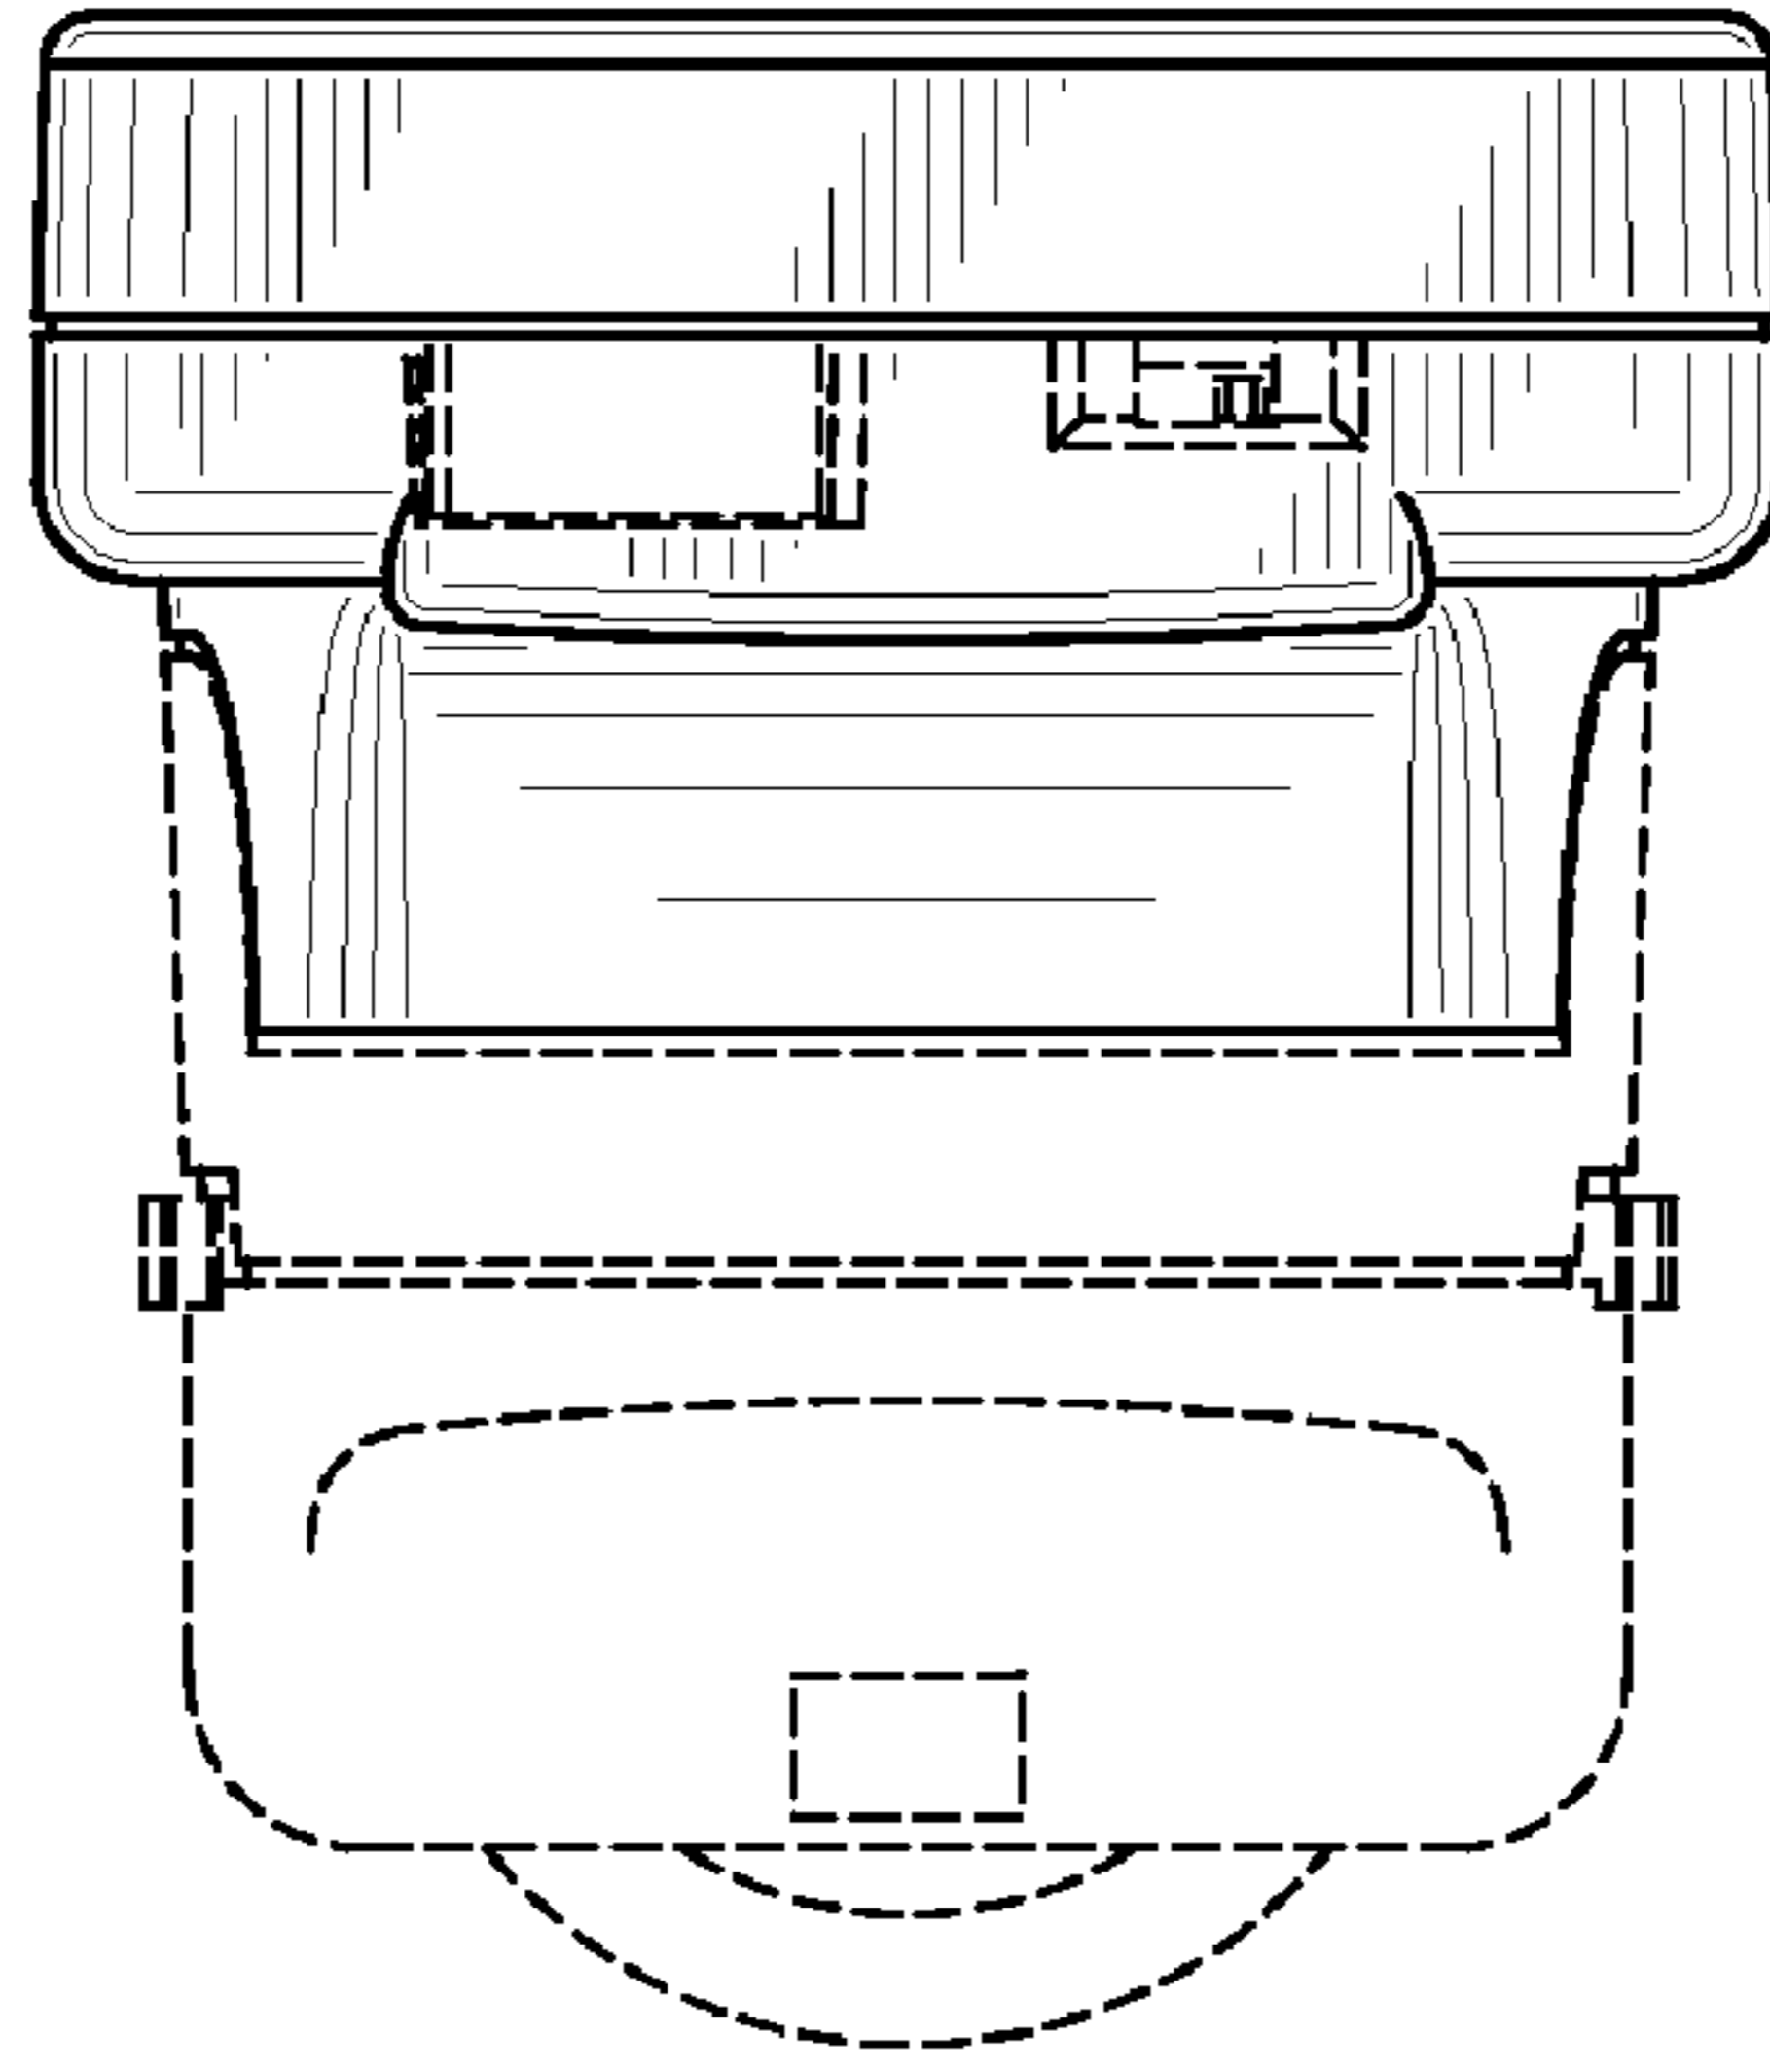


FIG. 6

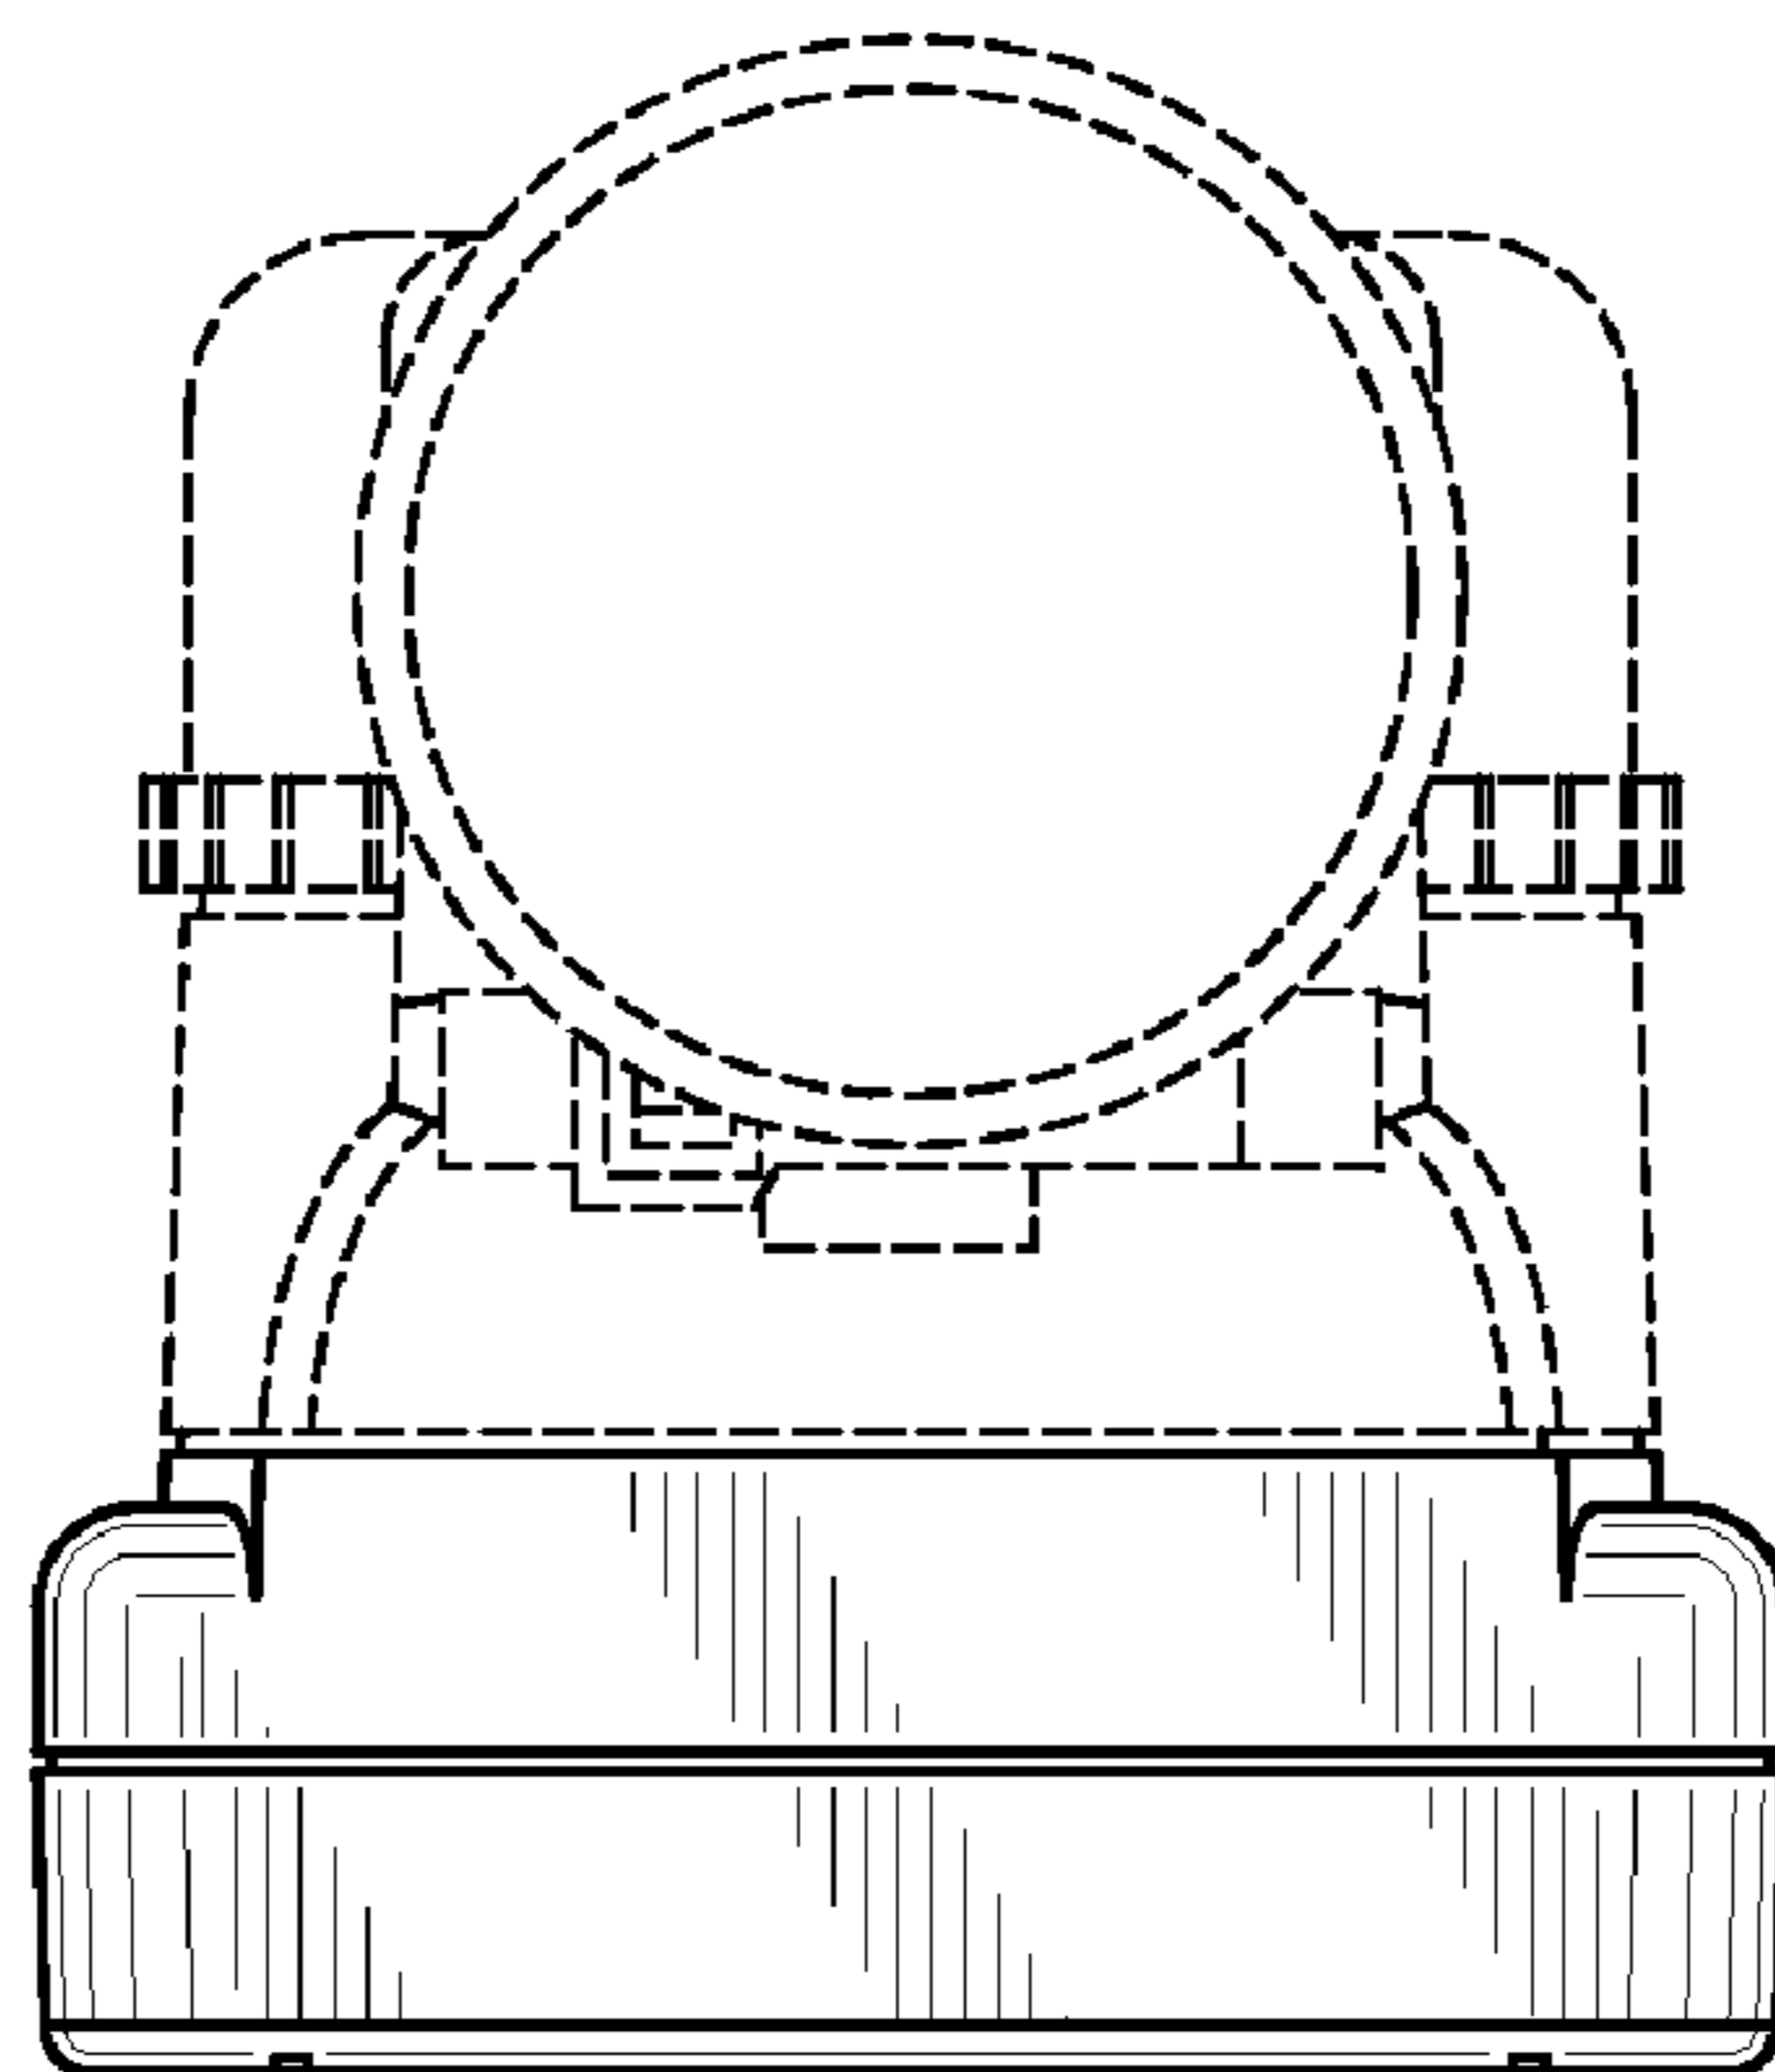


FIG. 7