



US00D636082S

(12) **United States Design Patent**  
**Cote et al.**

(10) **Patent No.:** **US D636,082 S**

(45) **Date of Patent:** **\*\* Apr. 12, 2011**

(54) **SURGICAL BLADE TIP ADAPTOR WITH  
SIDE CHANNELS**

(75) Inventors: **Dana Cote**, Boxford, MA (US);  
**Gregory P. Halloran**, Grafton, MA  
(US); **Thomas F. Walsh**, Stoneham, MA  
(US); **Jessica Chiappone**, Boston, MA  
(US)

(73) Assignee: **Beaver-Visitec International (US), Inc.**,  
Waltham, MA (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/361,324**

(22) Filed: **May 10, 2010**

(51) **LOC (9) Cl.** ..... **24-02**

(52) **U.S. Cl.** ..... **D24/147**

(58) **Field of Classification Search** ..... D24/130,  
D24/133, 146, 147; D19/55; 30/162, 329;  
606/167, 170, 172; D8/98-100, 103, 107

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D261,678	S	*	11/1981	Mann	.....	D24/144
4,569,133	A	*	2/1986	Schmidt	.....	606/172
D285,835	S	*	9/1986	Hanses	.....	D24/152
D338,955	S	*	8/1993	Gresl et al.	.....	D24/130
D609,810	S	*	2/2010	Cote et al.	.....	D24/146

\* cited by examiner

*Primary Examiner* — Charles A Rademaker

*Assistant Examiner* — Carissa C Fitts

(74) *Attorney, Agent, or Firm* — Hoffmann & Baron, LLP


(57) **CLAIM**

The ornamental design for a surgical blade tip adaptor with side channels, as shown and described.

**DESCRIPTION**

FIG. 1 is a top perspective view of a surgical blade tip adaptor with side channels;  
FIG. 2 is a top plan view thereof, the bottom plan view being identical thereto;  
FIG. 3 is a left elevational view thereof, the right elevational view being identical thereto;  
FIG. 4 is a front elevational view thereof; and,  
FIG. 5 is a rear elevational view thereof.  
The broken line showings in FIGS. 1-5 illustrate environmental matter and form no part of the claimed invention.

**1 Claim, 2 Drawing Sheets**

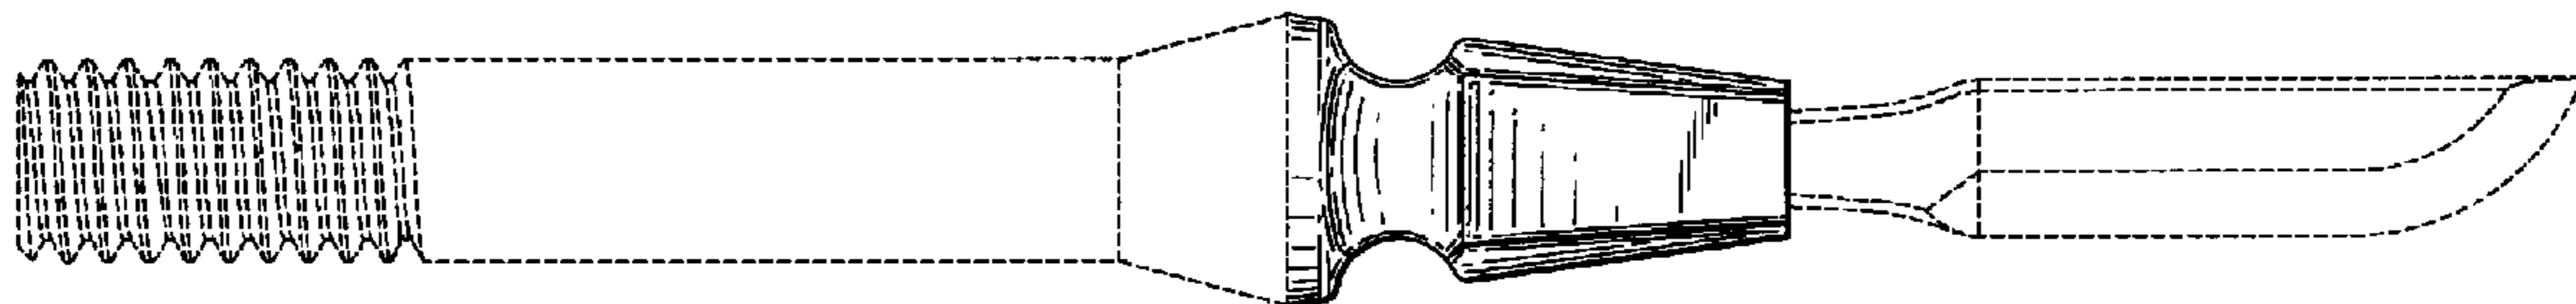

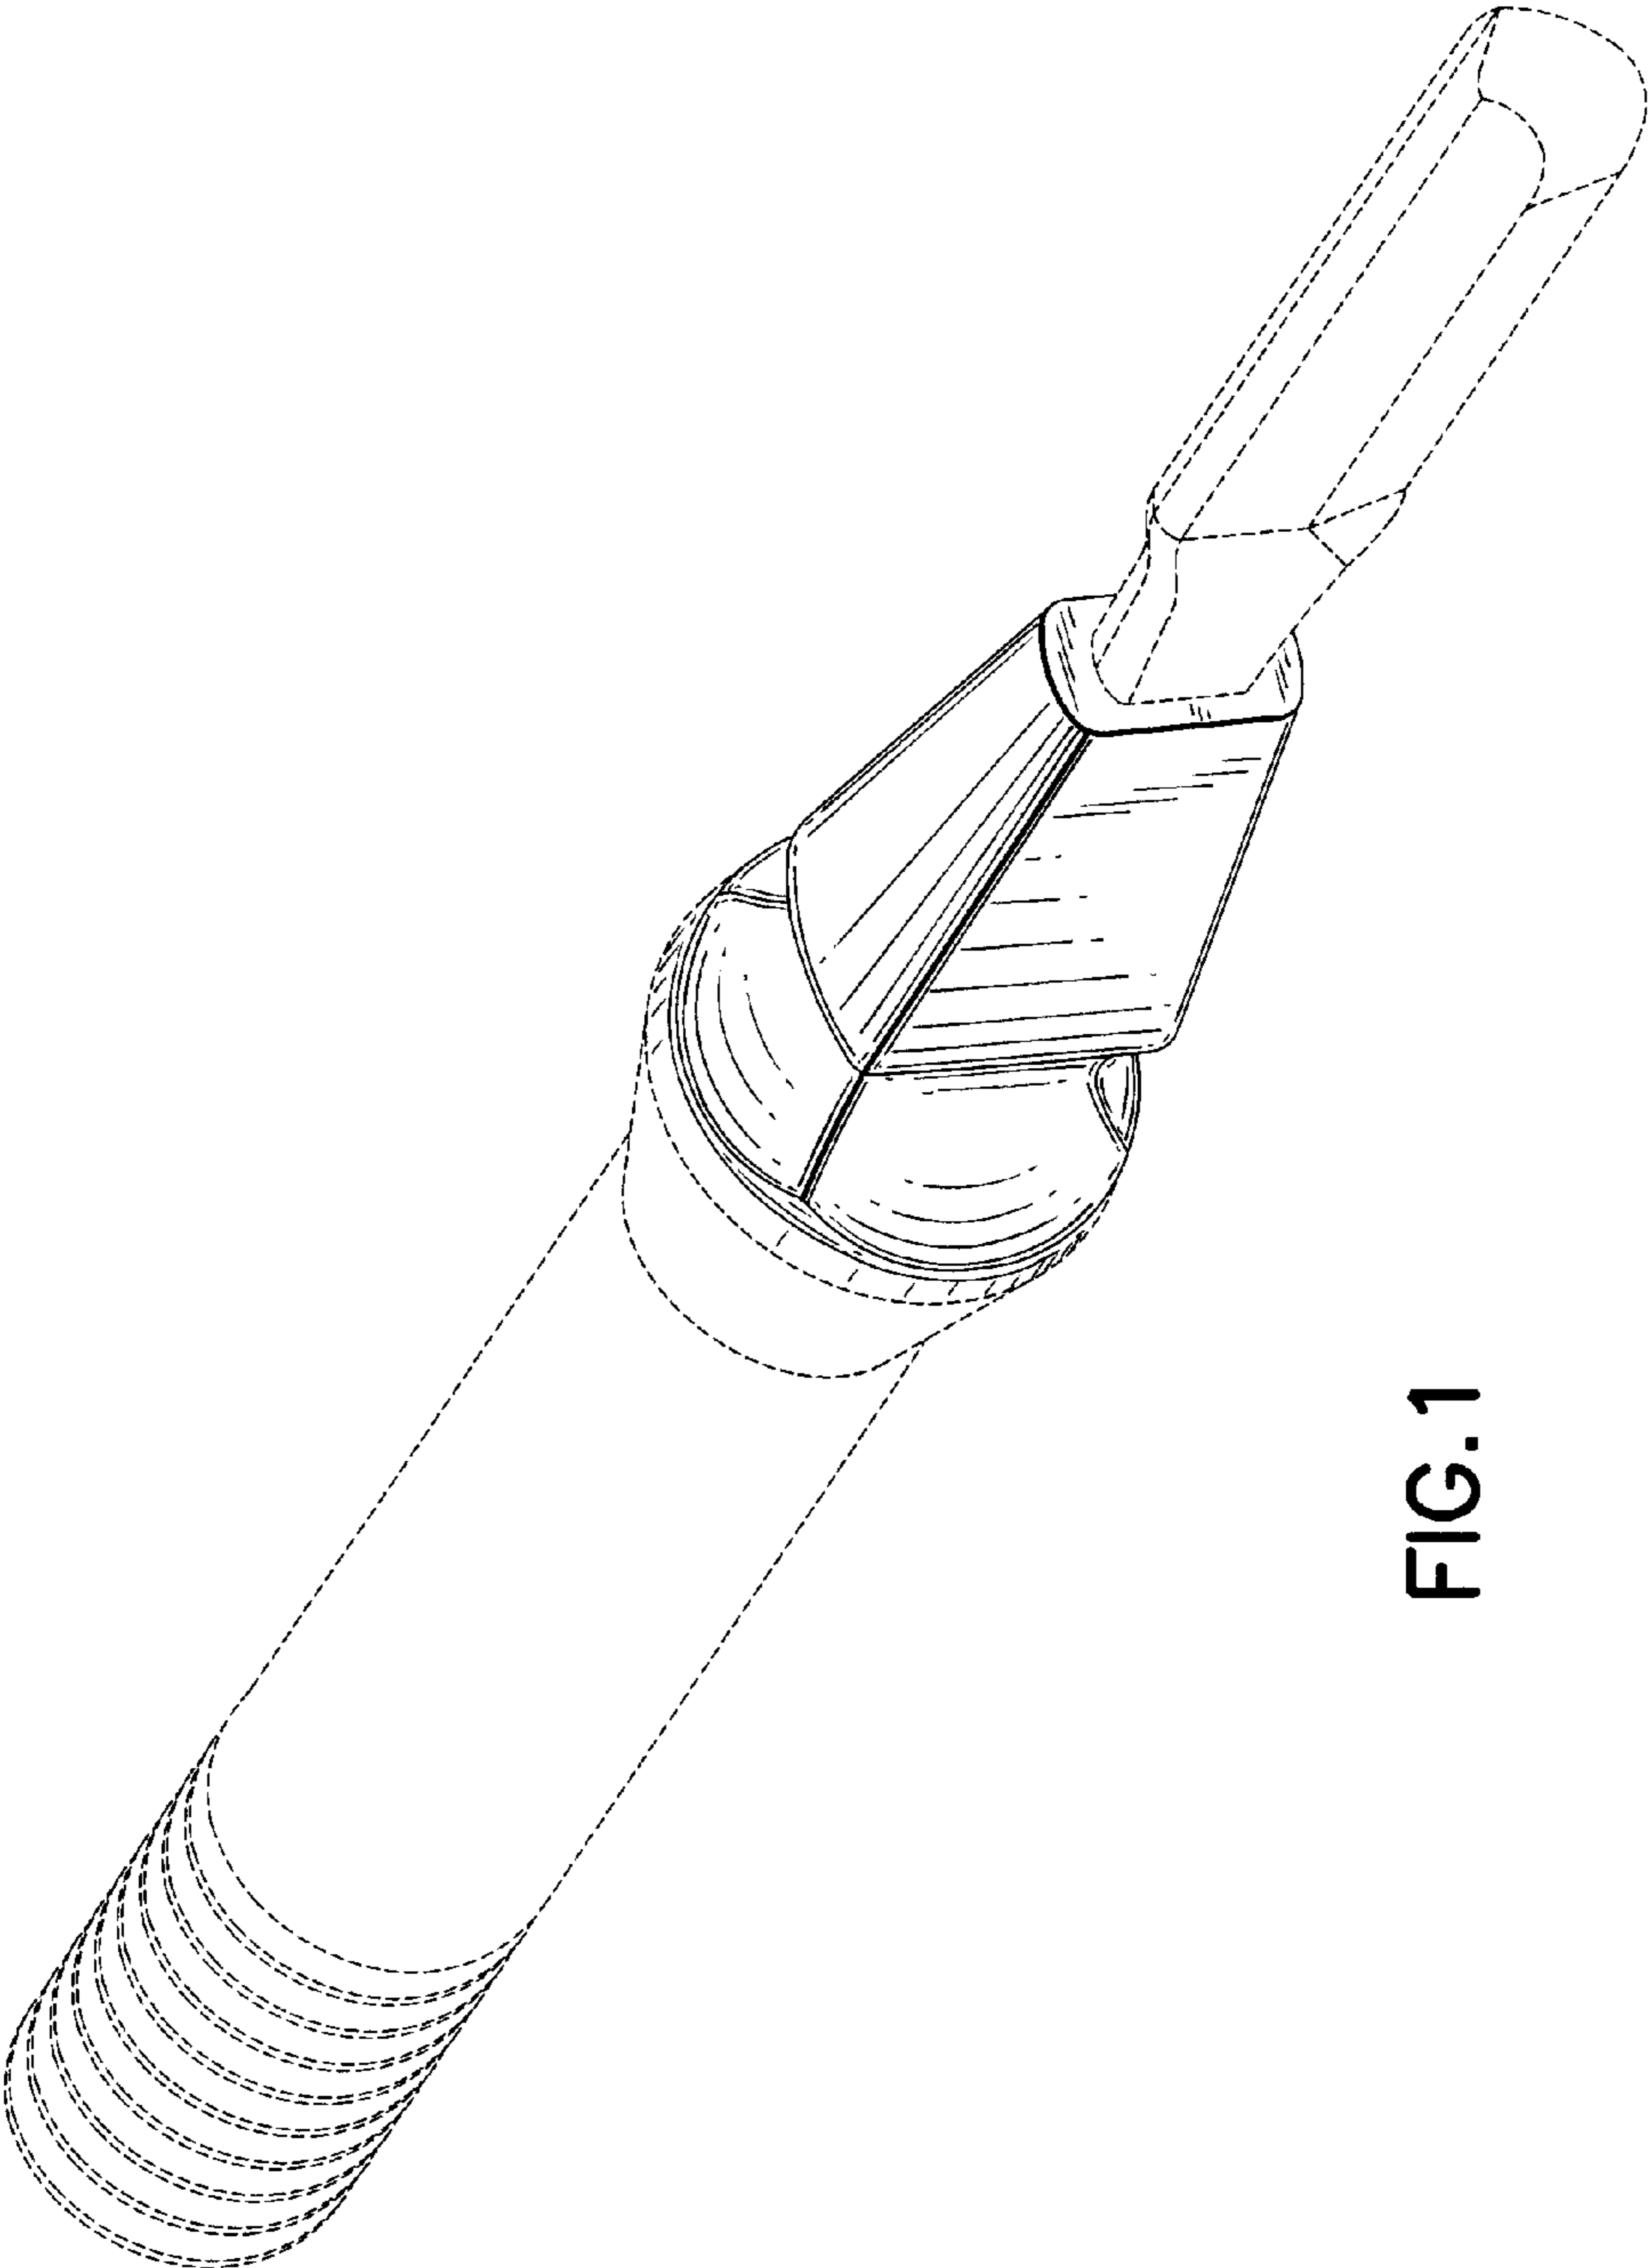


FIG. 1

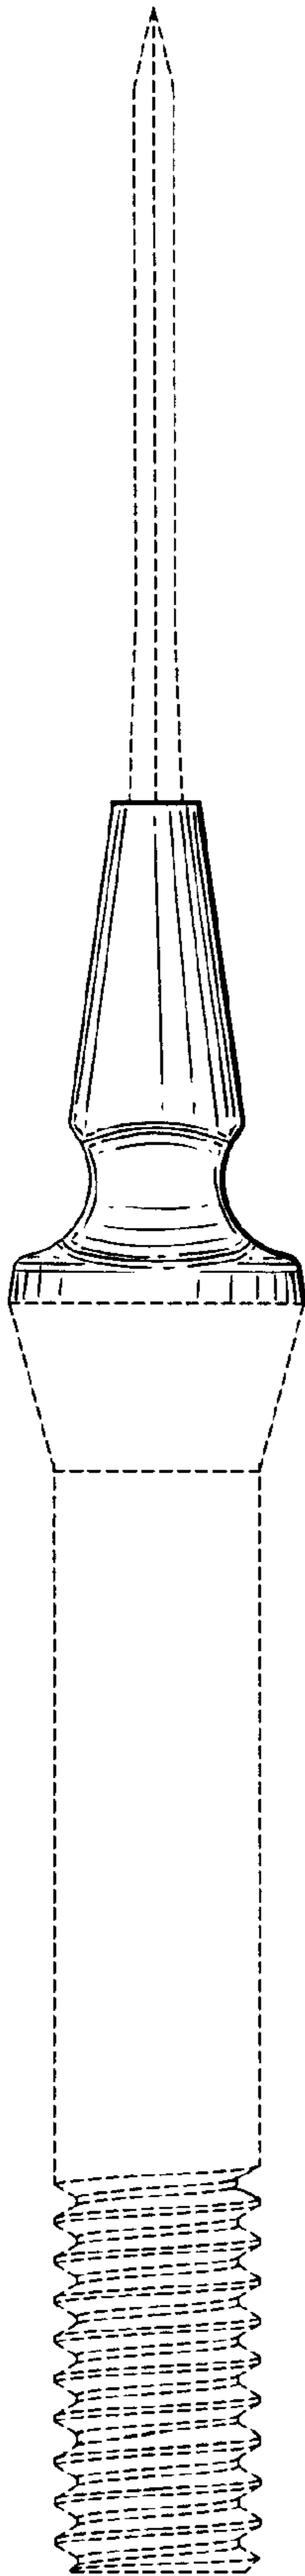


FIG. 2

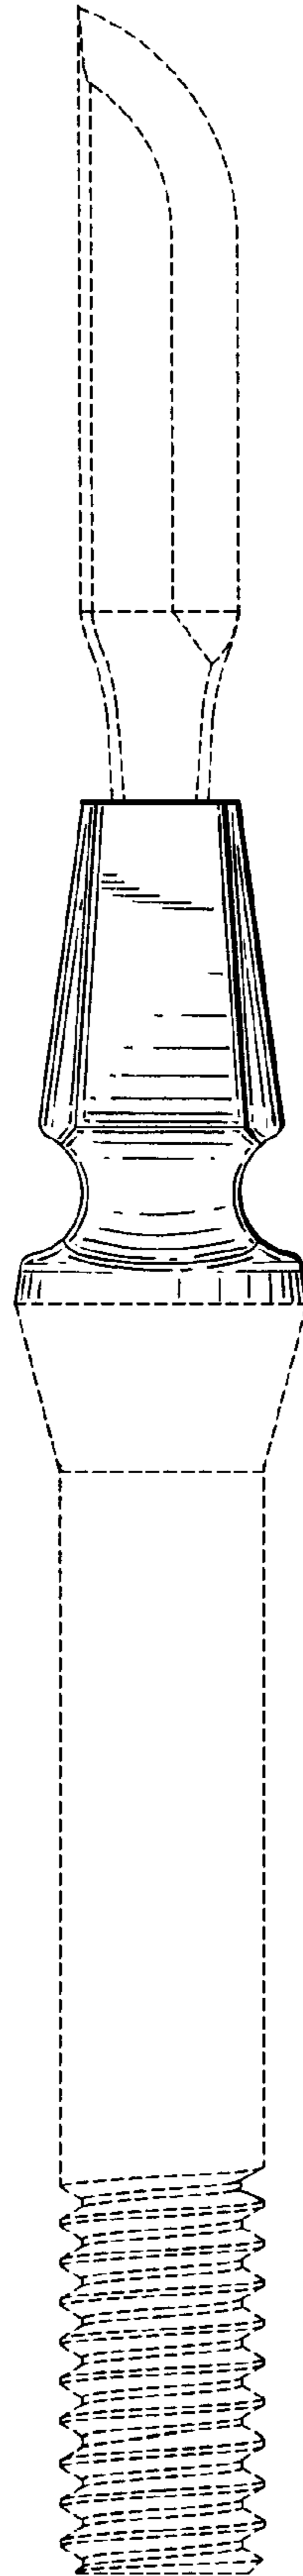


FIG. 3

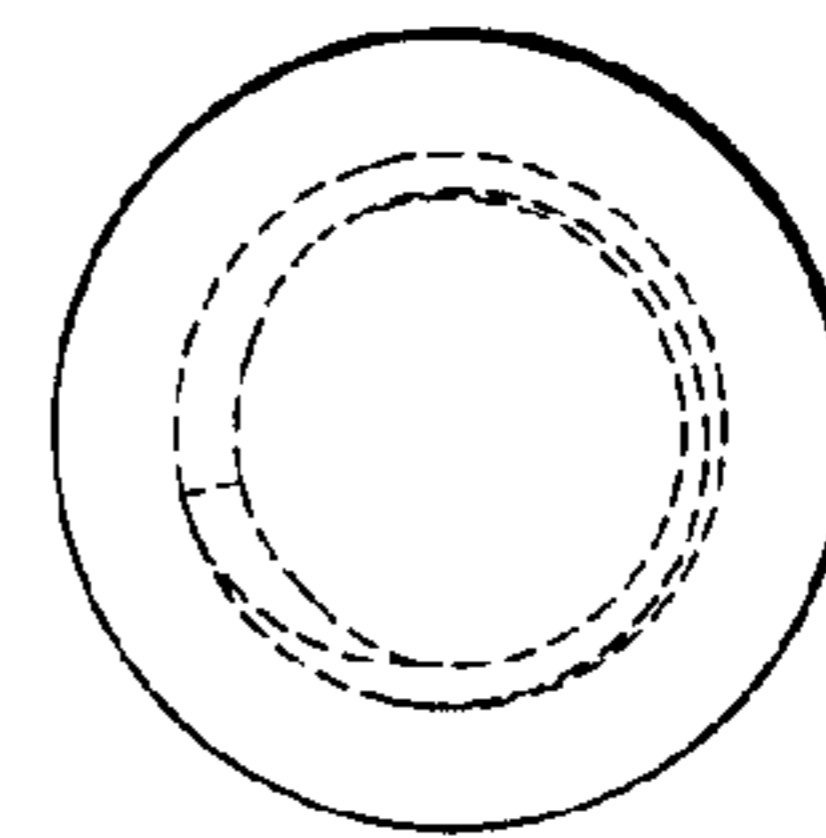


FIG. 4

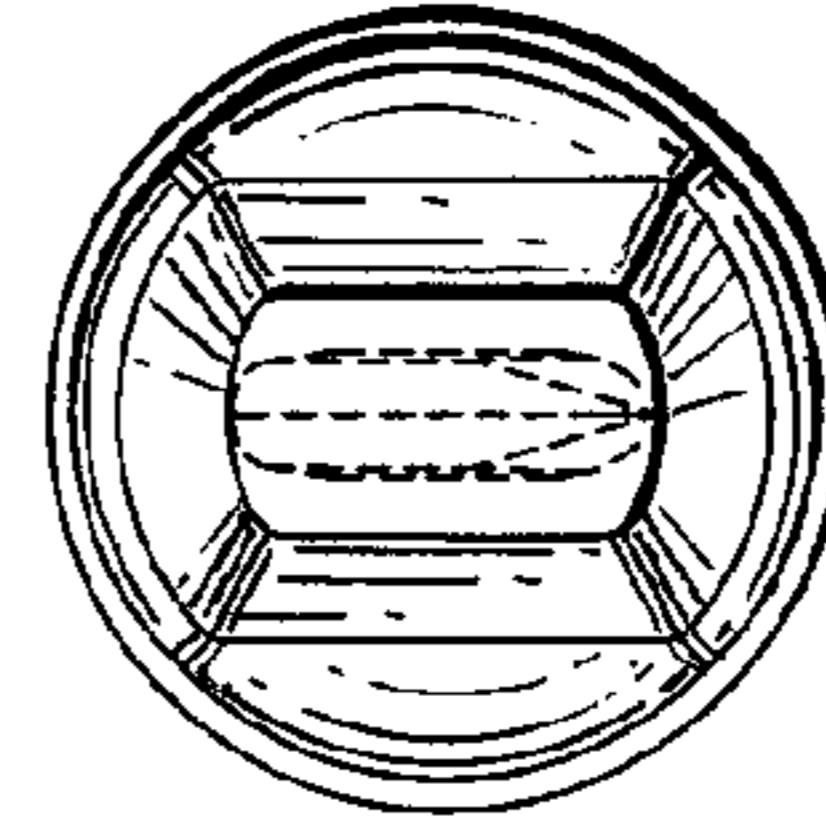


FIG. 5