



US00D638171S

(12) **United States Design Patent**  
**Goranov et al.**

(10) **Patent No.:** **US D638,171 S**

(45) **Date of Patent:** **\*\* May 17, 2011**

(54) **PROTECTIVE AIR FILTRATION DEVICE**

(75) Inventors: **Konstantin Goranov**, Atkinson, NH (US); **Albena Milencheva**, Atkinson, NH (US)

(73) Assignee: **Salutaris, LLP**, Atkinson, NH (US)

(\*\*) Term: **14 Years**

(21) Appl. No.: **29/378,576**

(22) Filed: **Nov. 5, 2010**

(51) **LOC (9) Cl.** ..... **29-02**

(52) **U.S. Cl.** ..... **D29/108**

(58) **Field of Classification Search** ..... D29/108-110, D29/122; D24/110.1; 128/858, 863, 201.23, 128/206.12, 206.13, 206.16, 206.19, 206.28, 128/206.11; 2/9, 206, 5, 6.6, 411-414, 424, 2/425

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D248,497	S *	7/1978	Slosek	.....	D24/110.1
D267,985	S *	2/1983	Huber	.....	D24/110.1
D273,145	S *	3/1984	Ponsi	.....	D24/110.1
D287,649	S *	1/1987	Zdrok et al.	.....	D24/110.1
5,374,458	A *	12/1994	Burgio	.....	428/36.1
5,419,318	A	5/1995	Tayebi		
D368,960	S *	4/1996	Lanford	.....	D24/110.1
5,558,089	A *	9/1996	Castiglione	.....	128/206.24
5,561,863	A	10/1996	Carlson, II		
5,611,938	A	3/1997	Smolik et al.		
D390,652	S *	2/1998	Parker	.....	D24/110.1
6,041,782	A *	3/2000	Angadjivand et al.	...	128/206.19
6,116,236	A *	9/2000	Wyss	.....	128/200.24
6,224,579	B1	5/2001	Modak et al.		
D443,927	S *	6/2001	Chen	.....	D24/110.1
D464,726	S *	10/2002	Wolfe	.....	D24/110.1
6,585,989	B2	7/2003	Herbst et al.		
6,596,906	B2	7/2003	Baumann et al.		
6,843,784	B2	1/2005	Modak et al.		

D511,209	S *	11/2005	Callan	.....	D24/110.1
7,131,442	B1 *	11/2006	Kronzer et al.	.....	128/205.27
7,171,967	B2	2/2007	Brunell et al.		
7,185,653	B2	3/2007	Lee		
7,210,482	B2	5/2007	Huang et al.		
7,290,545	B2	11/2007	Kleman et al.		
7,559,968	B2	7/2009	Bolduc		
7,802,572	B2	9/2010	Hahne		
2001/0010016	A1	7/2001	Modak et al.		

(Continued)

**FOREIGN PATENT DOCUMENTS**

CA 2170112 8/1996

(Continued)

**OTHER PUBLICATIONS**

“Safety & Industrial 2009 Buyer’s Guide,” *LSS*, Disposable Respirators, pp. 142-151, 340, 851 (Jan. 2009).

(Continued)

*Primary Examiner* — Ruth McInroy

(74) *Attorney, Agent, or Firm* — Greenberg Traurig, LLP; David J. Dykeman; Roman Fayerberg



(57) **CLAIM**

The ornamental design for a protective air filtration device, as shown and described.

**DESCRIPTION**

FIG. 1 is a front view of the protective air filtration device of the present invention;  
FIG. 2 is a rear view thereof;  
FIG. 3 is a top view thereof;  
FIG. 4 is a bottom view thereof;  
FIG. 5 is a right side view thereof;  
FIG. 6 is a left side view thereof; and,  
FIG. 7 is a perspective view thereof.  
The portions of the design depicted in broken lines form no part of the claimed design.

**1 Claim, 7 Drawing Sheets**

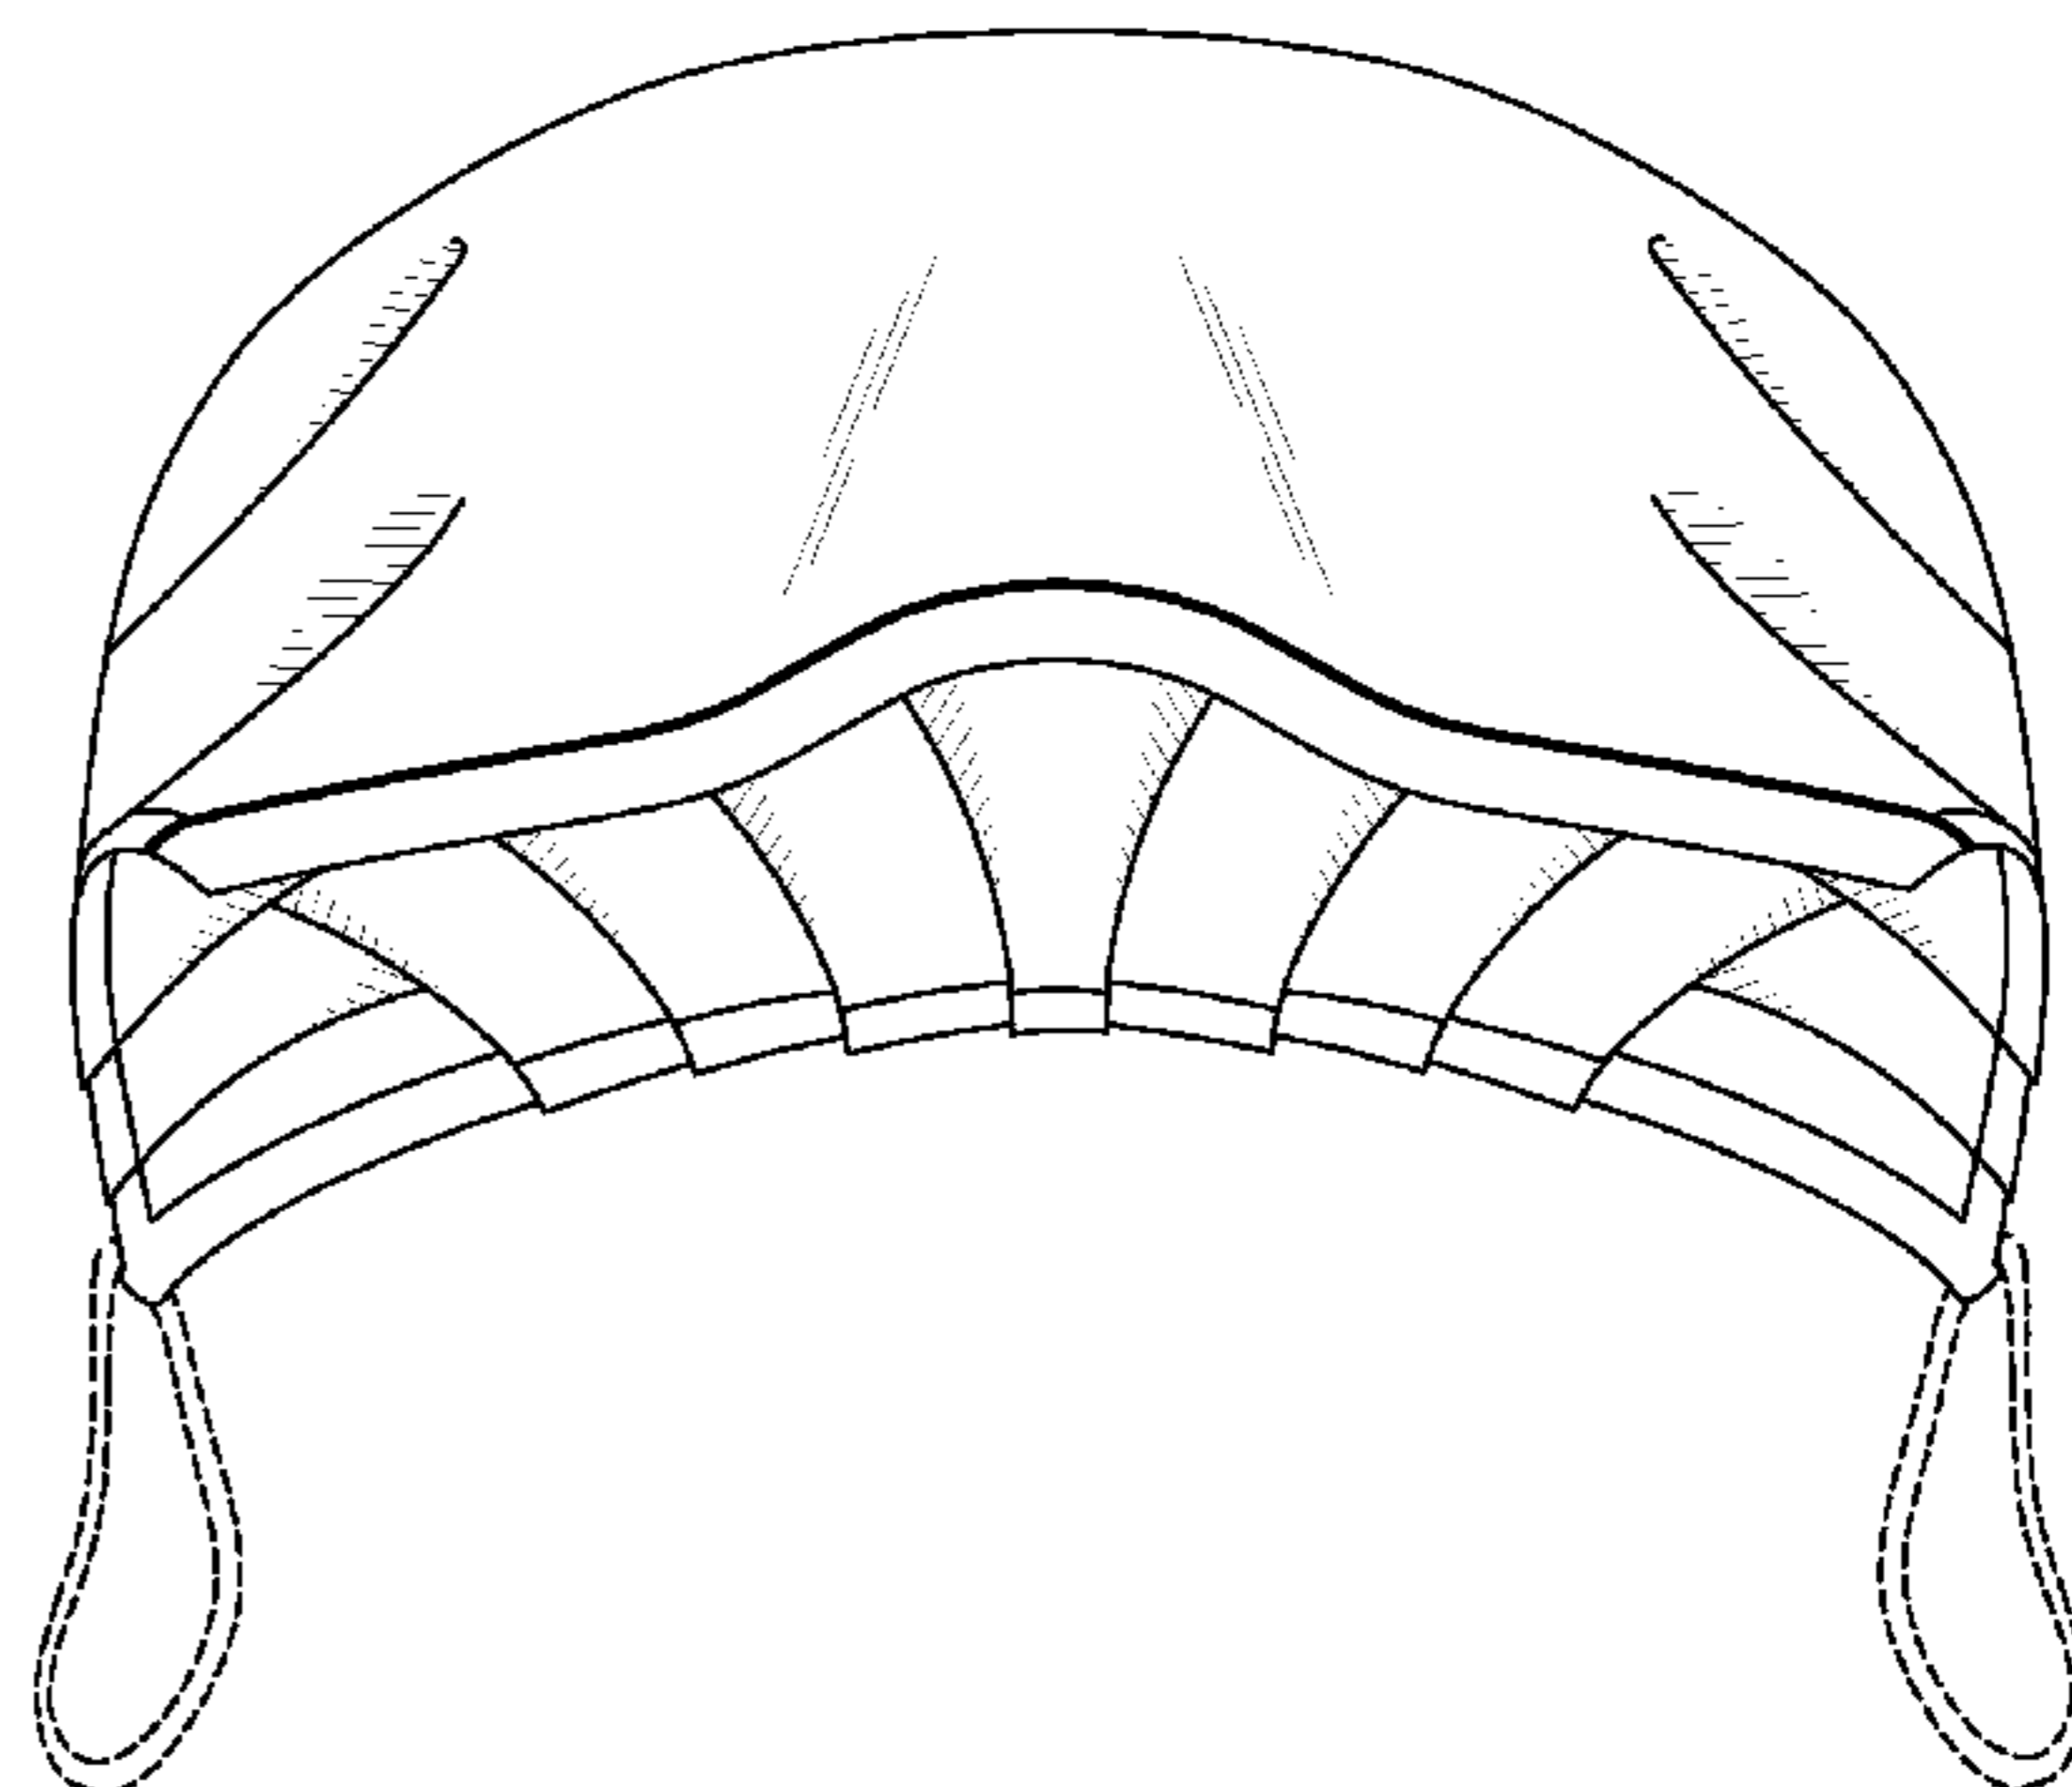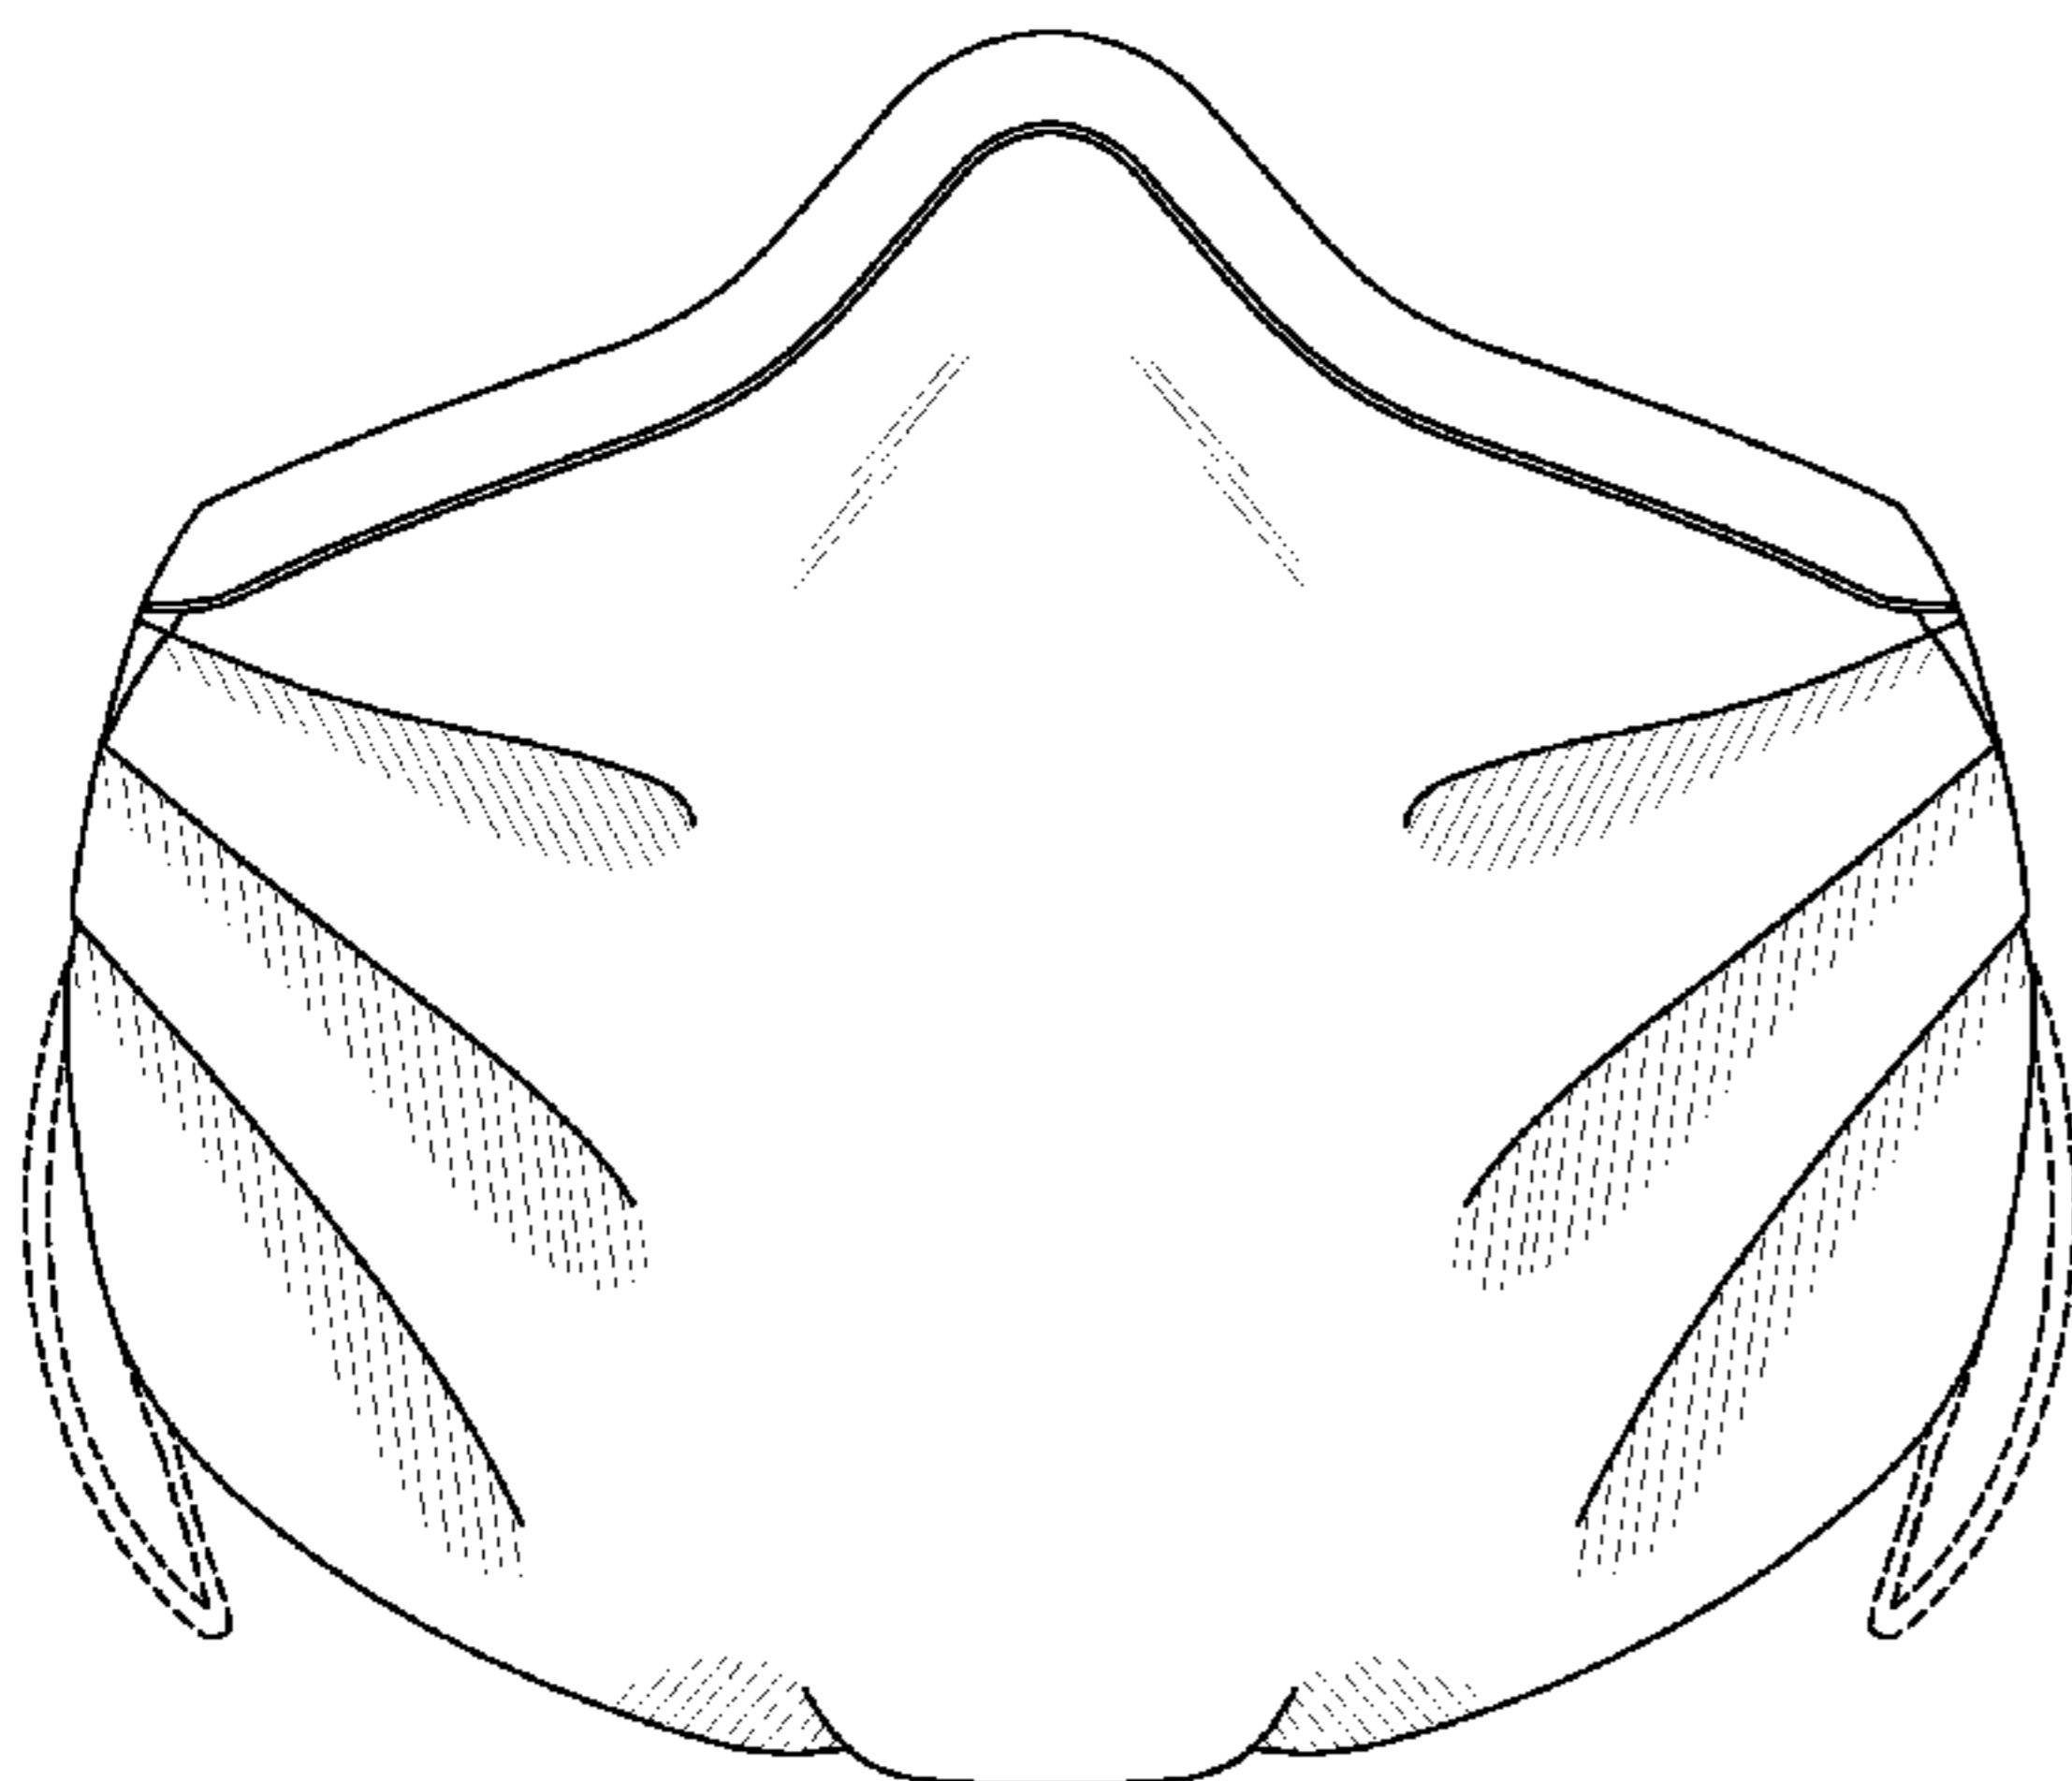

U.S. PATENT DOCUMENTS

2002/0038055	A1	3/2002	Baumann et al.	
2002/0106413	A1	8/2002	Herbst et al.	
2003/0125413	A1	7/2003	Herbst et al.	
2003/0125583	A1	7/2003	Baumann et al.	
2005/0124725	A1	6/2005	Modak et al.	
2005/0131100	A1	6/2005	Herbst et al.	
2007/0048344	A1	3/2007	Yahiahoui et al.	
2007/0231391	A1	10/2007	Bracken et al.	
2008/0295843	A1*	12/2008	Haas .....	128/205.27
2010/0218774	A1*	9/2010	Flaherty .....	128/863

FOREIGN PATENT DOCUMENTS

CA	2366380	10/2000
EP	1 190 622	3/2002
WO	WO 2005/067895	7/2005
WO	WO 2006/034227	3/2006
WO	WO 2009/026725	3/2009

OTHER PUBLICATIONS

“2009-2010 Buyer’s Guide: Hard Hats, Safety Glasses, Ear Plugs, Respirators, Faceshields . . .” R3 *Safety*, Respiratory Protection: Disposables, pp. 104-112 (Jan. 2009).  
 “Product Catalog: Total Solutions to Health Care,” *INTCO Healthcare, FIME Expo*, Nonwoven Disposables, pp. 5-10 (Aug. 2010).

“2010-2011 Catalogue of Plus Medical,” *Foshan Nanhai Plus Medical Co., Ltd., FIME Expo*, pp. 17 (Aug. 2010).  
 “Weini Product Brochure,” *Weinida Nonwoven Textiles Co., Ltd., NSC Congress & Expo* (Oct. 2009).  
 “MaskEnomics—A Reference Guide to Proper Mask Selection,” *Crosstex* (Apr. 2010).  
 “3M VFlex Particulate Respirators 9105 and 9105S, N95,” *3M, NSC Congress & Expo* (Oct. 2010).  
 “Dashengmask: Health Talisman,” *Shanghai Dasheng Health Products Manufacture Co., Ltd., NSC Congress & Expo*, pp. 27-31 (Oct. 2010).  
 “Fitseal FS300, FS400 & FS500 Series Respirators,” *Wein Products, Inc., NSC Congress & Expo* (Oct. 2010).  
 “Kimberly-Clark PFR95 N95 Particulate Filter Respirators,” *Kimberly-Clark* (Mar. 2007).  
 “Moldex Hearing & Respiratory Protection Product Catalog 9700-748,” *Moldex-Metric, Inc.*, pp. 2-7 (Sep. 2009).  
 “Gerson Smart-Mask Particulate Respirators: A New Level of Design, Function and Performance,” *Gerson Co., Inc.* (Jan. 2007).  
 “Gateway Safety, Inc.: Where Safety Meets Style,” *Gateway Safety, Inc., Respiratory Protection Disposable Respirators*, pp. 26-27 (Jan. 2009).  
 “Respiratory Protection: Product Guide 2008 01/10 SPR670031,” *NSC Congress & Expo*, Disposable Respirators, pp. 3-15 (Jan. 2010), “Sperian”.

\* cited by examiner

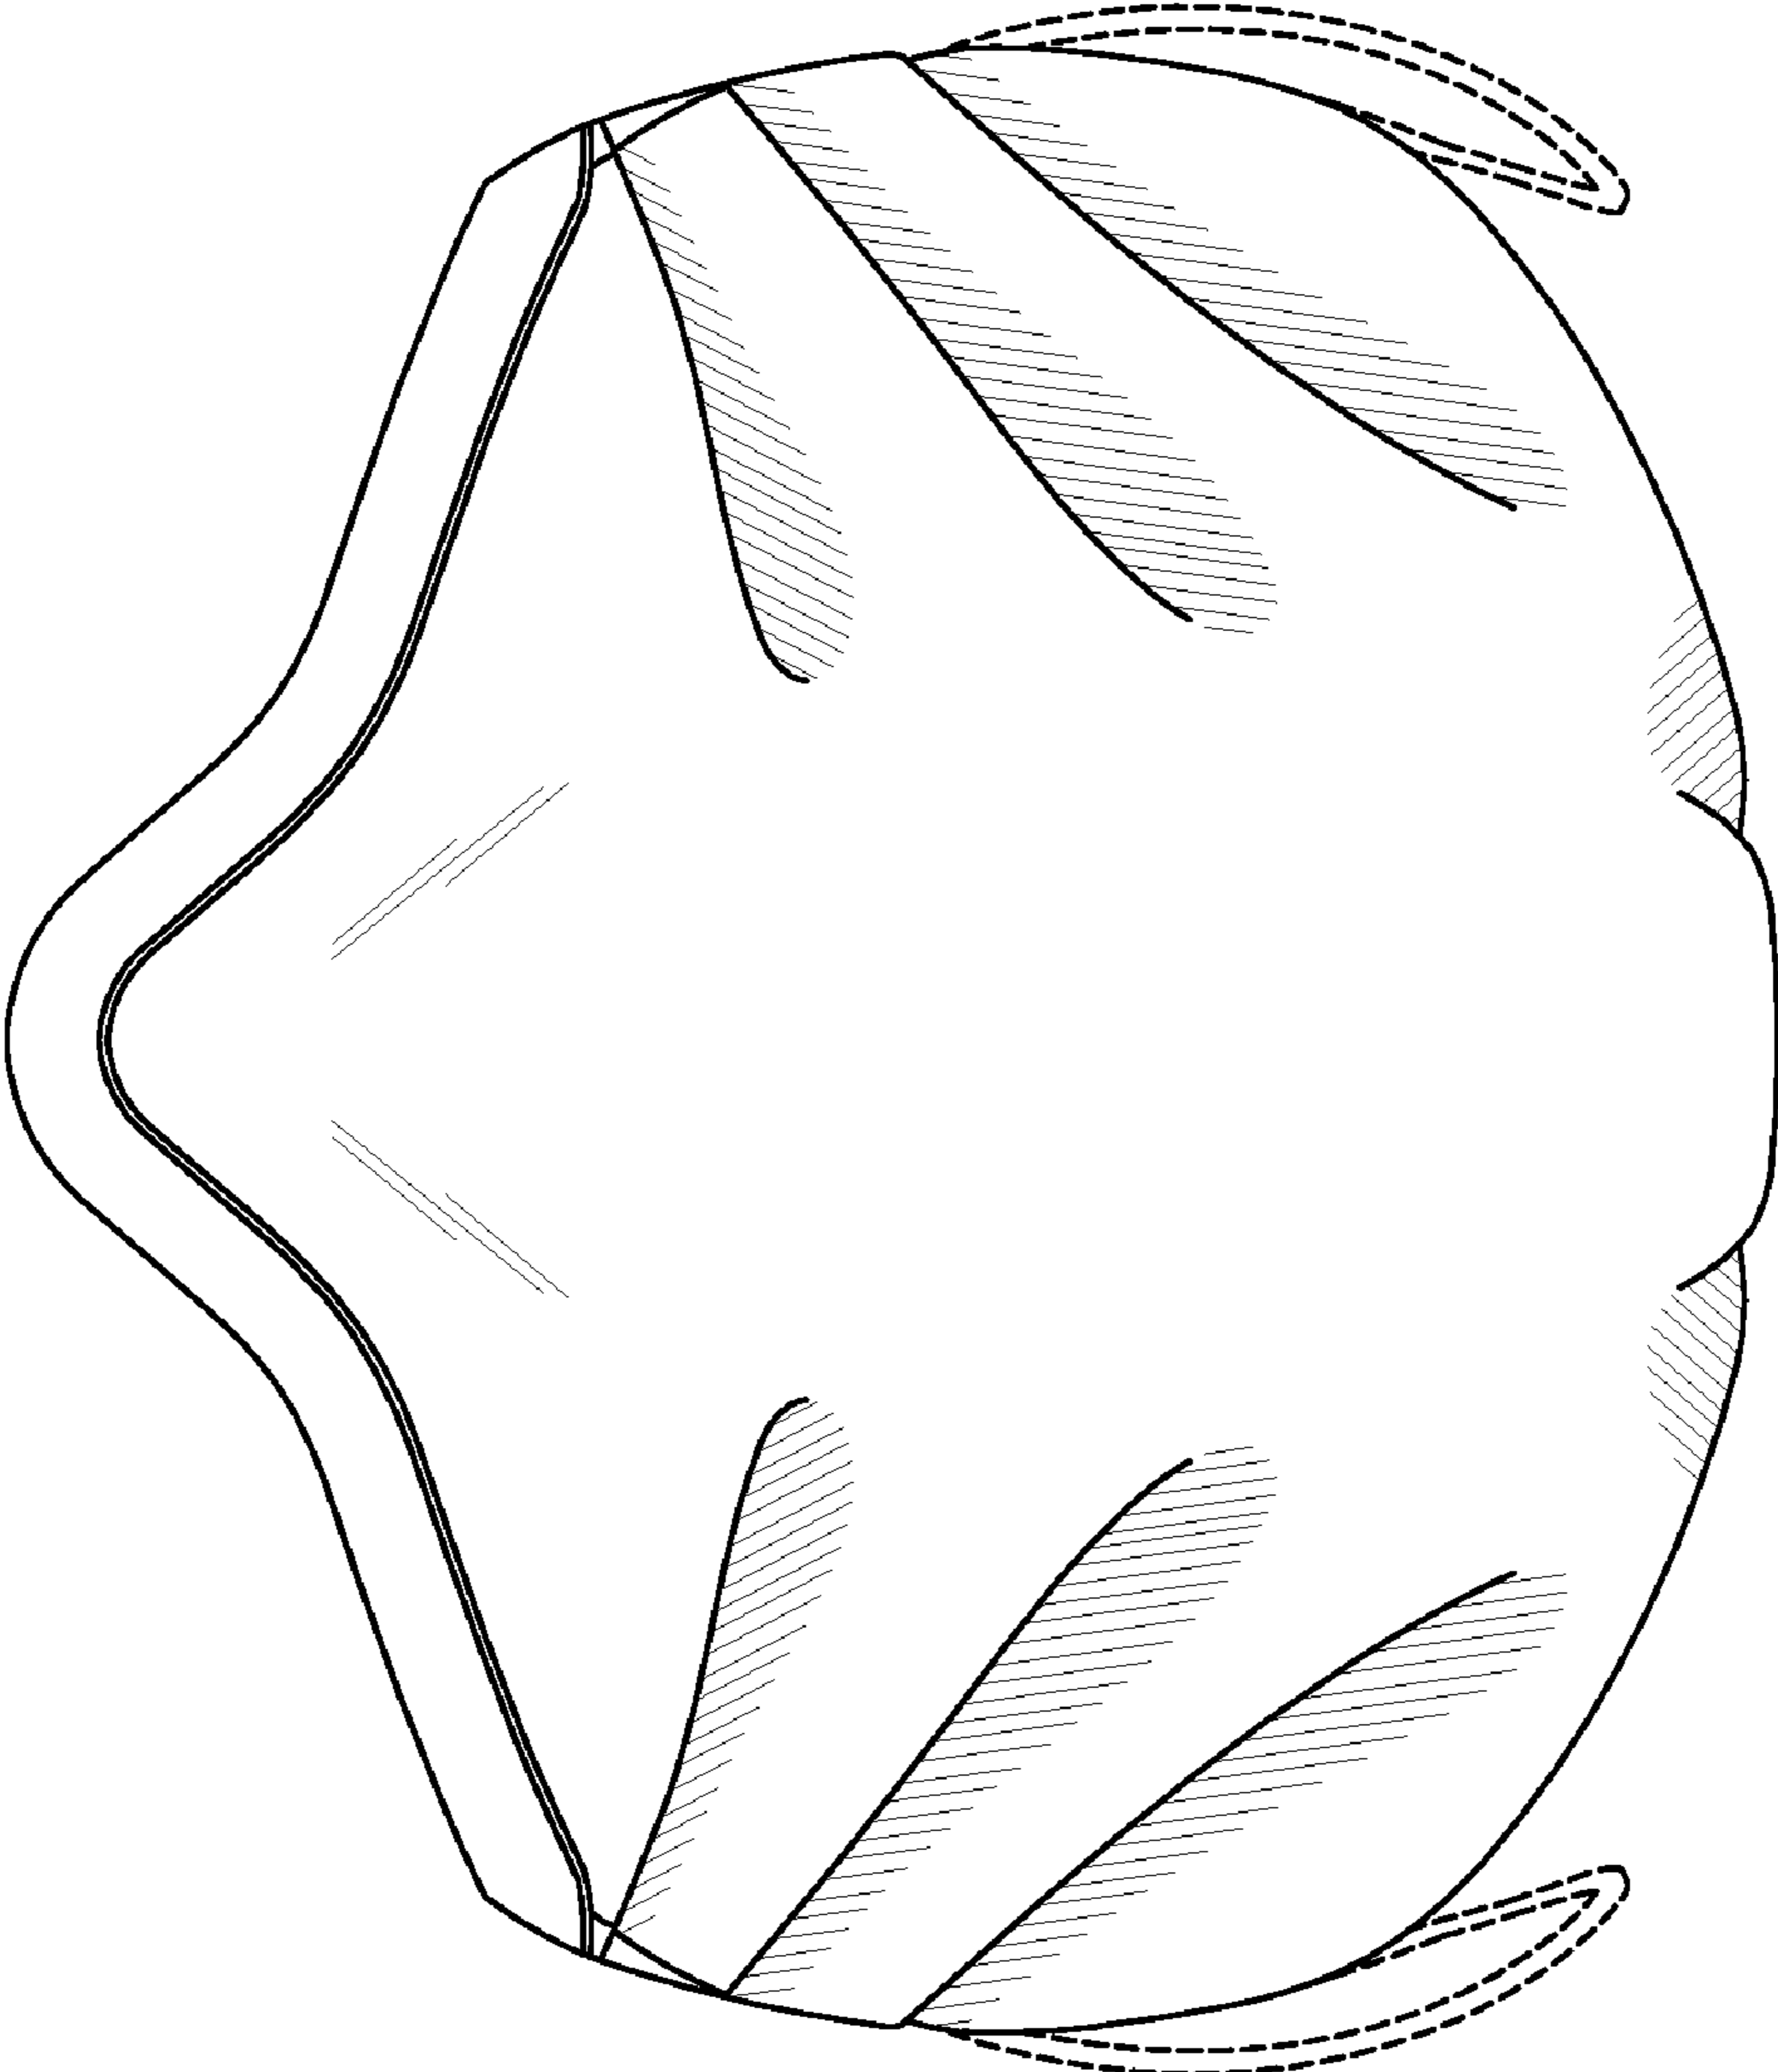


FIG. 1

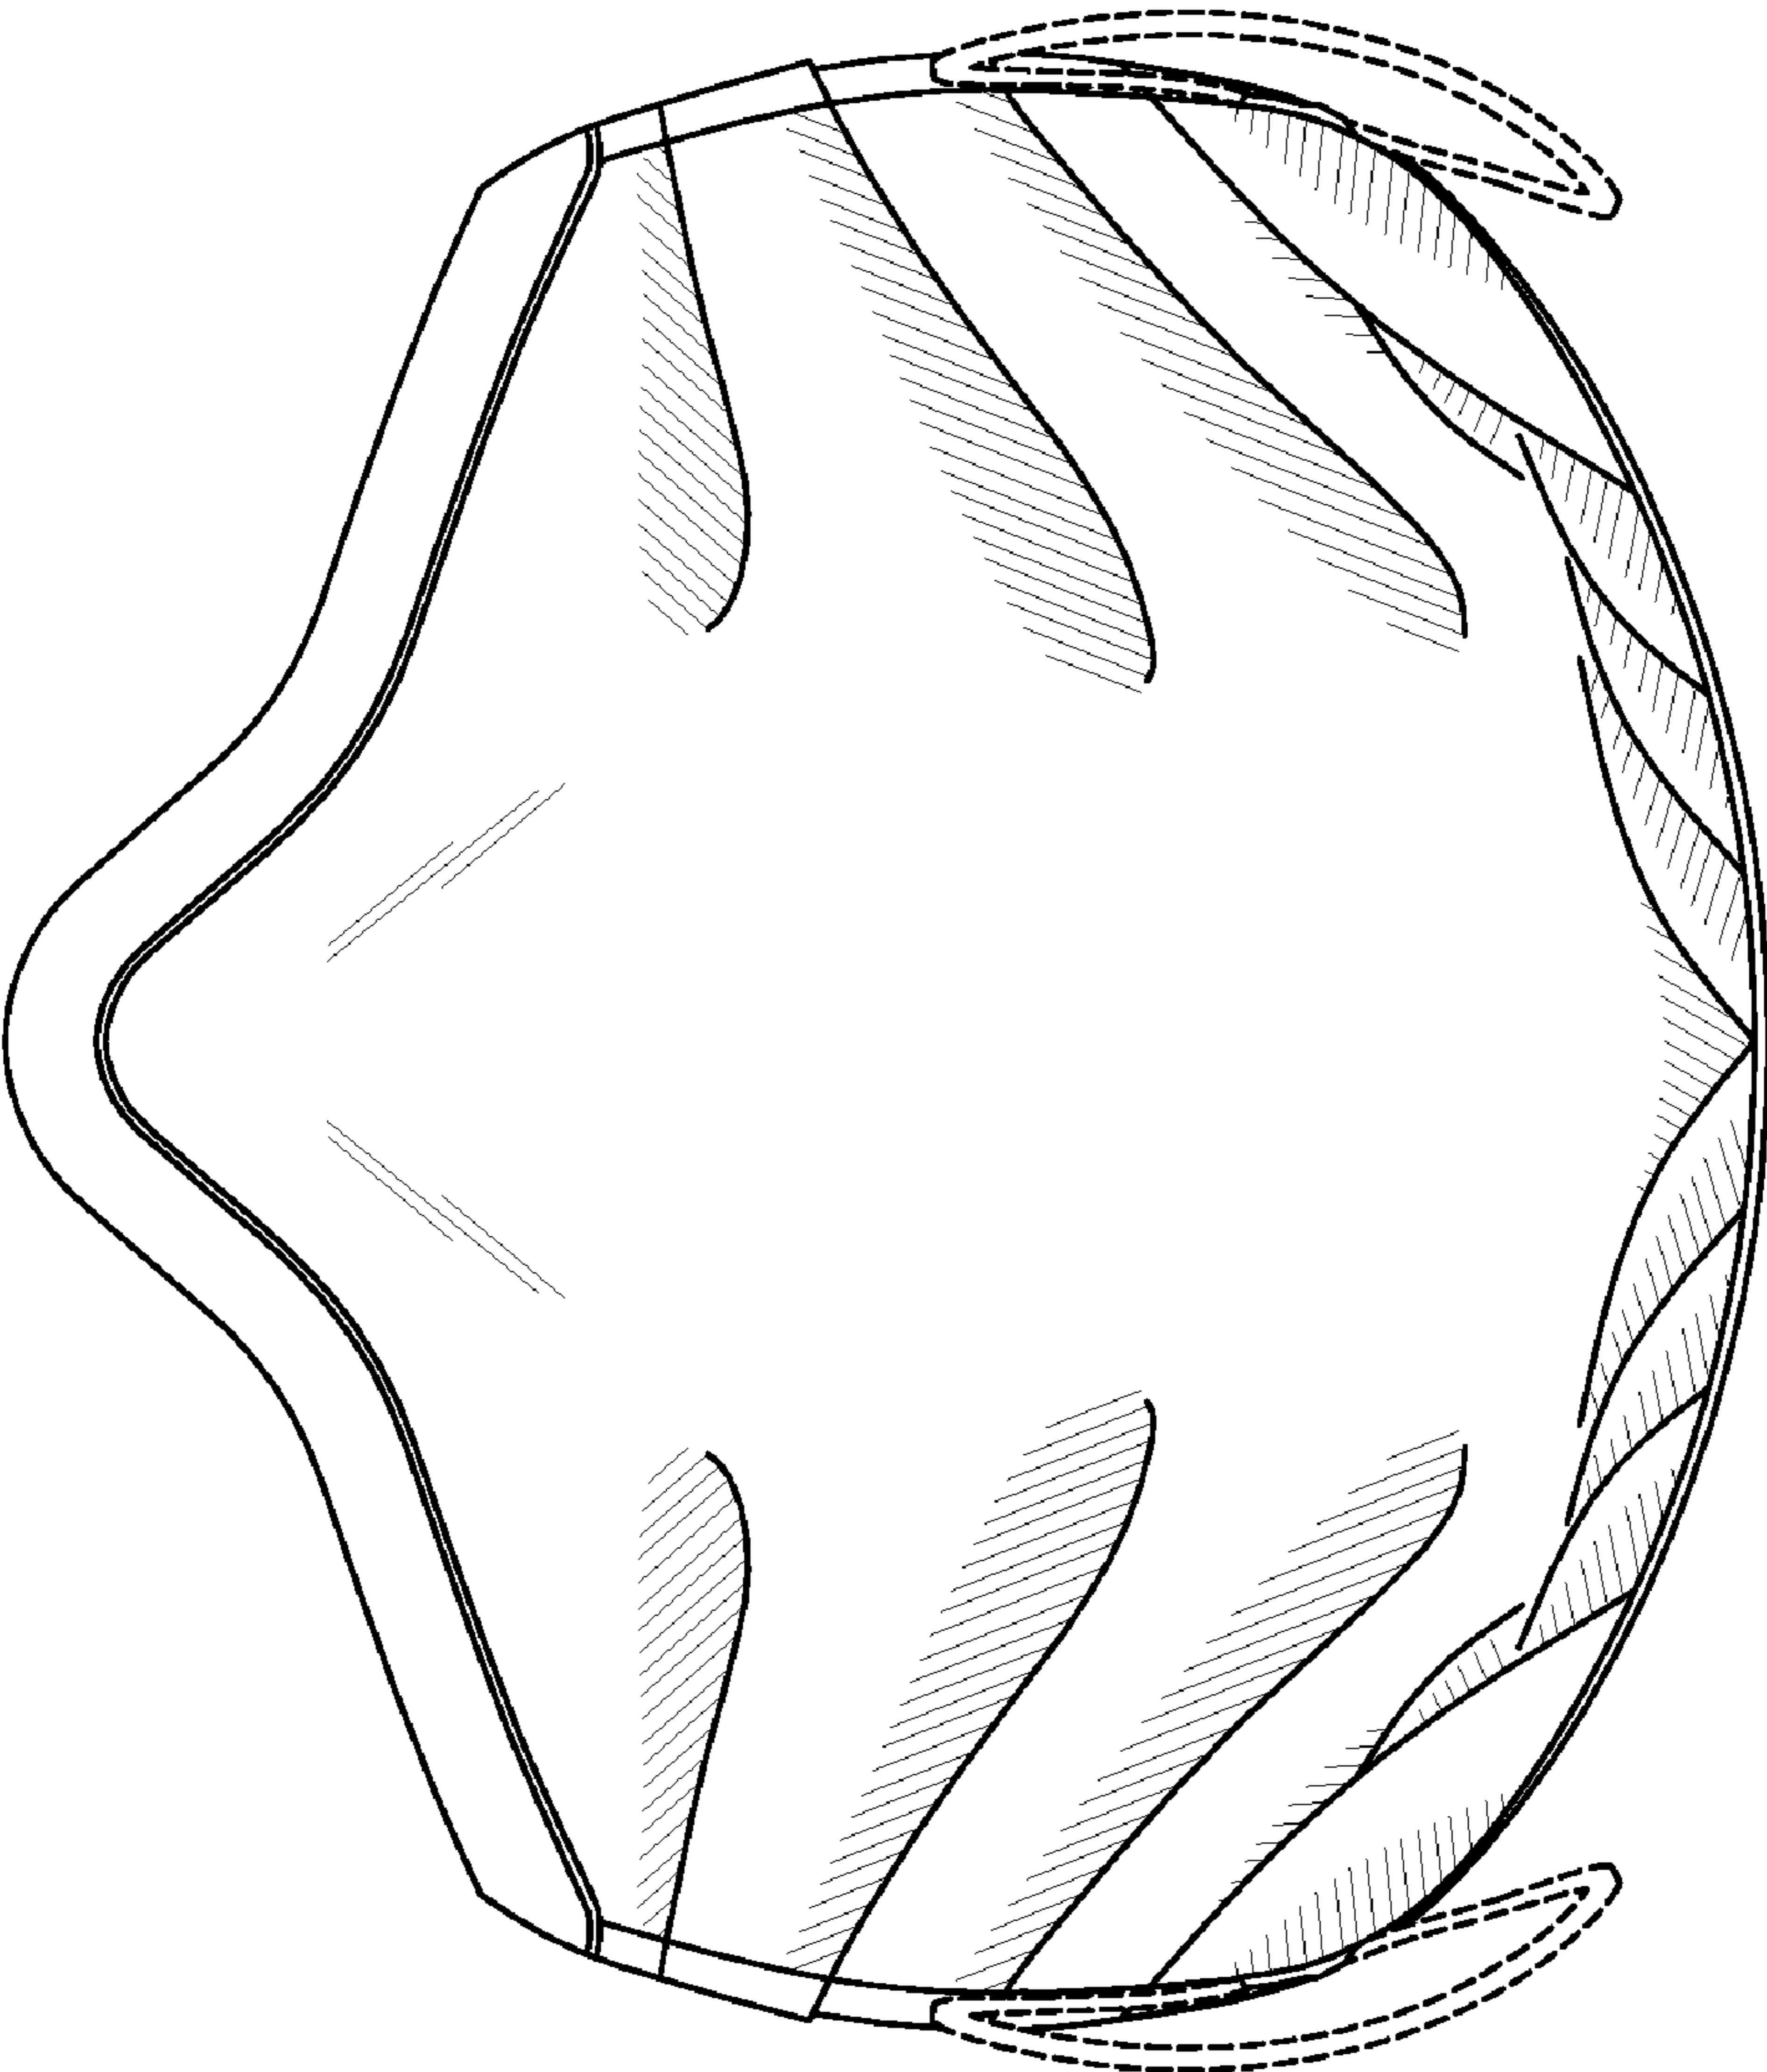


FIG. 2

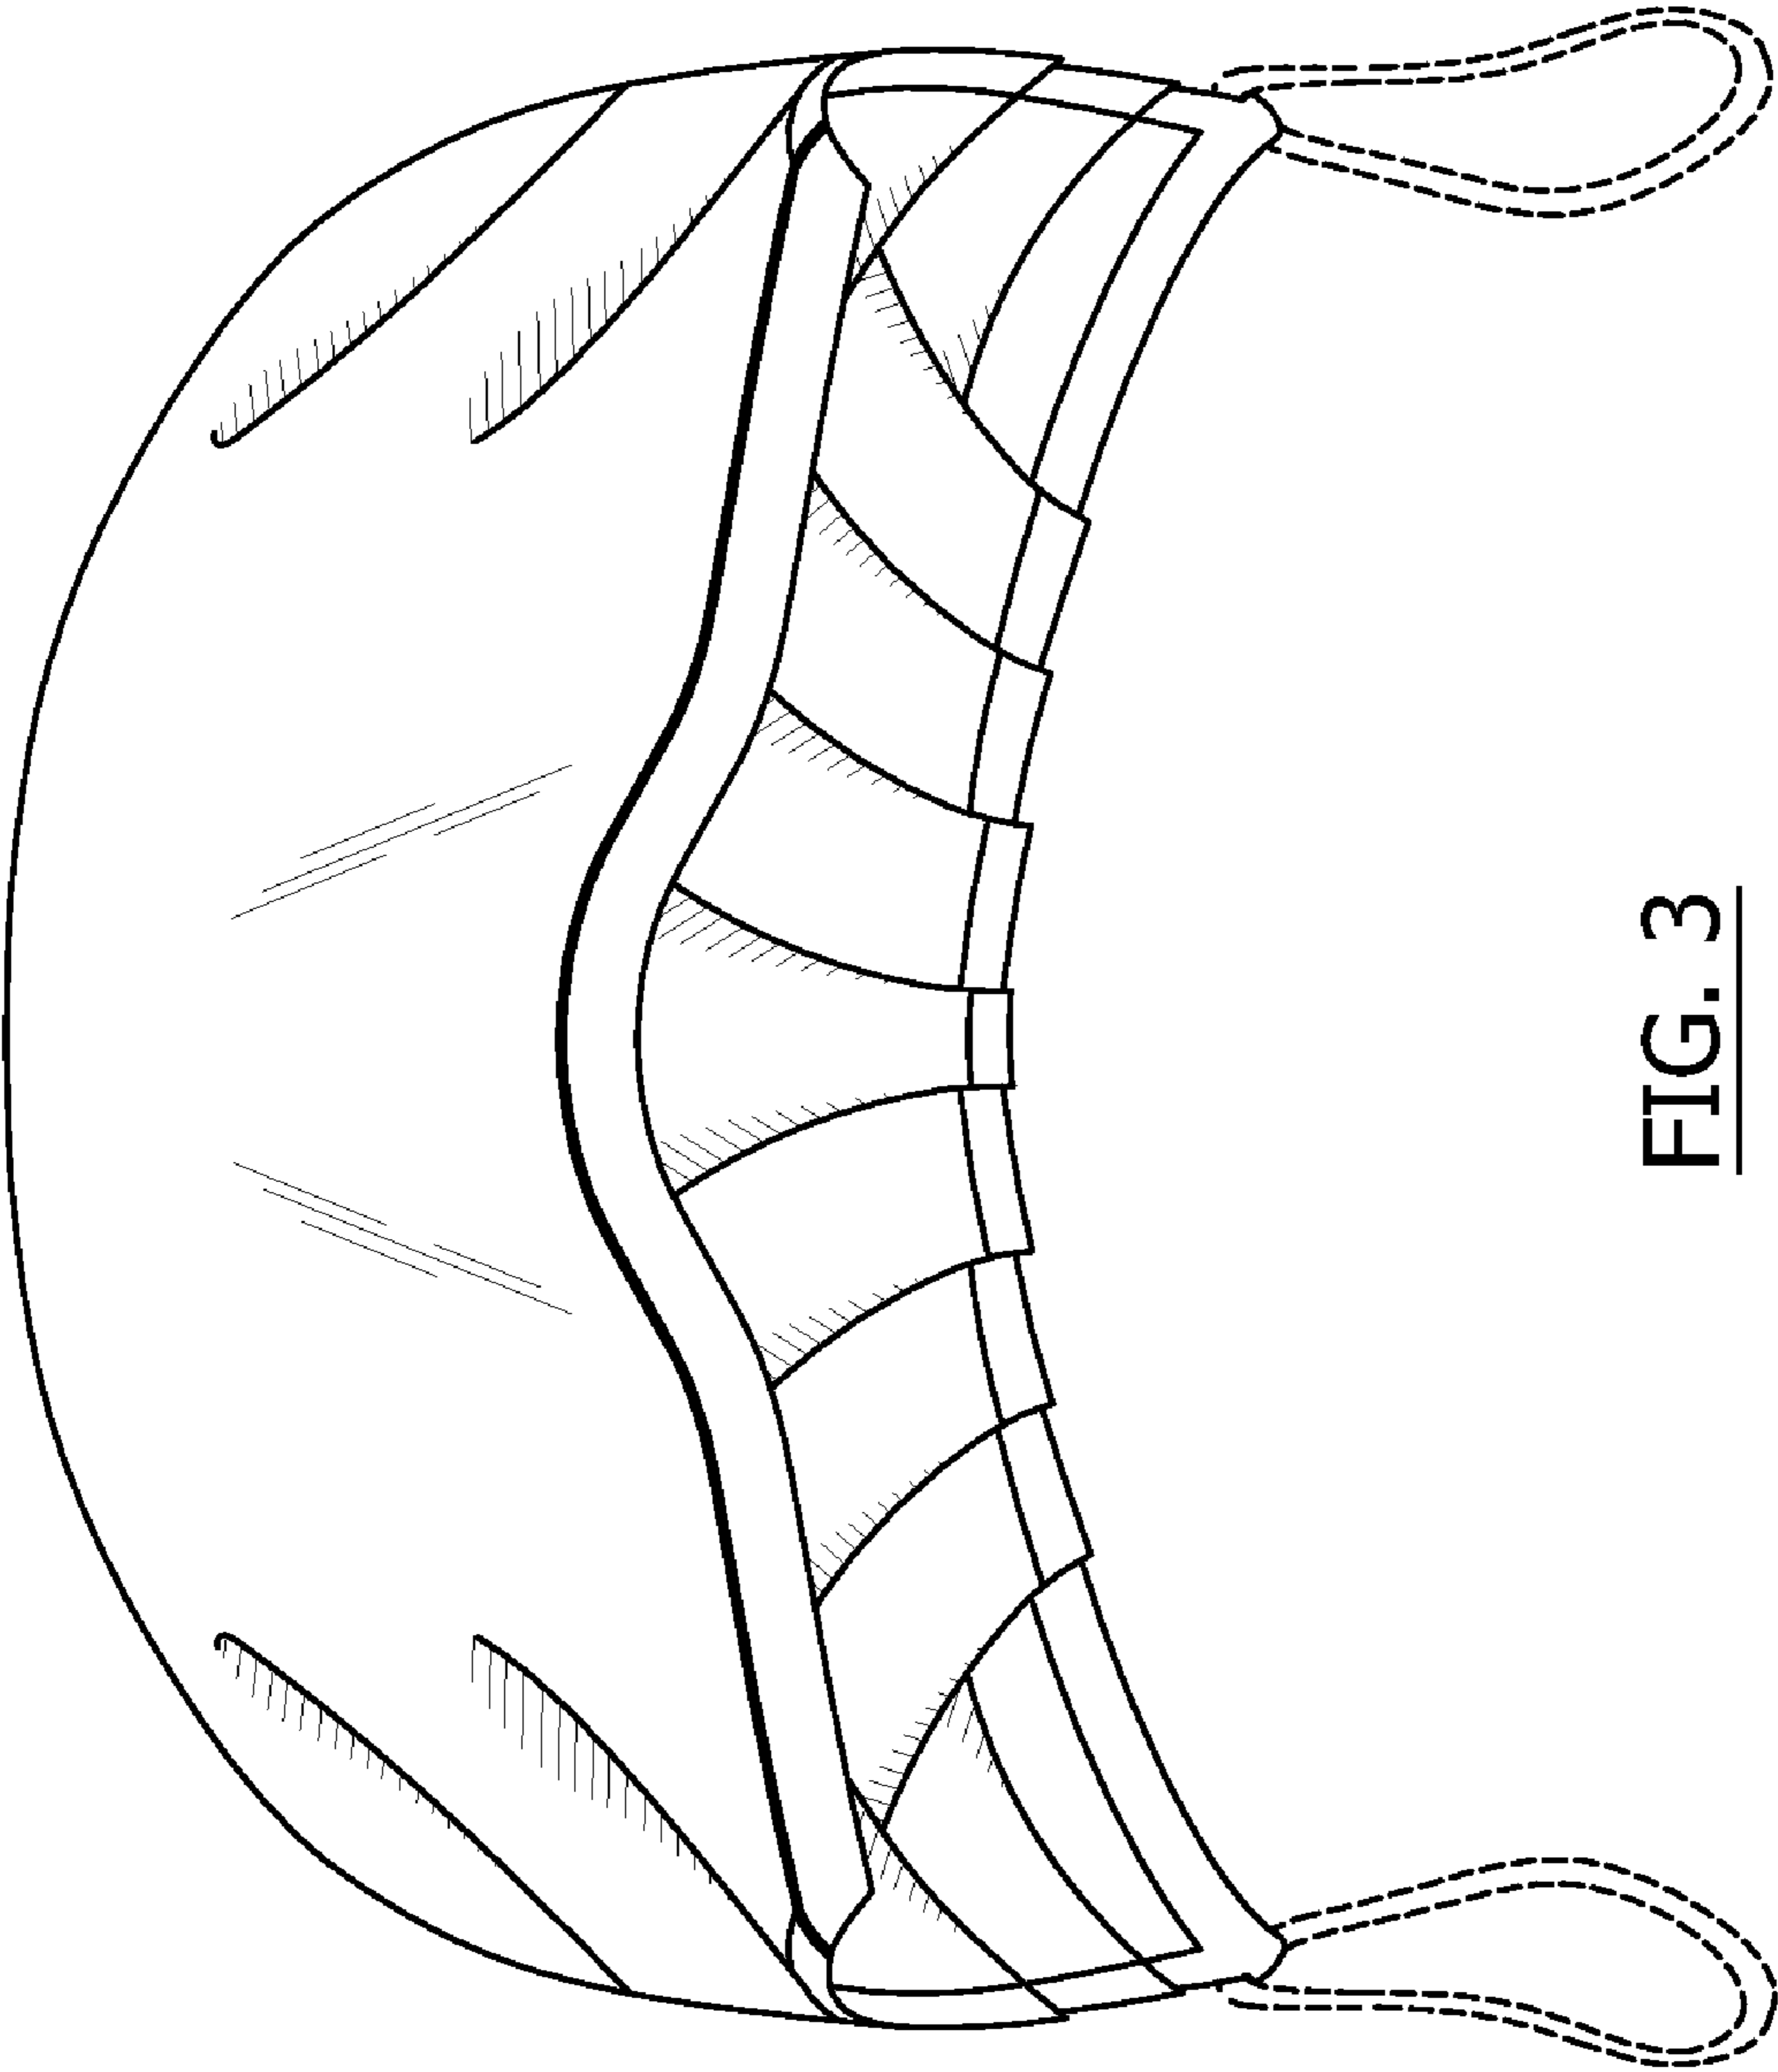


FIG. 3

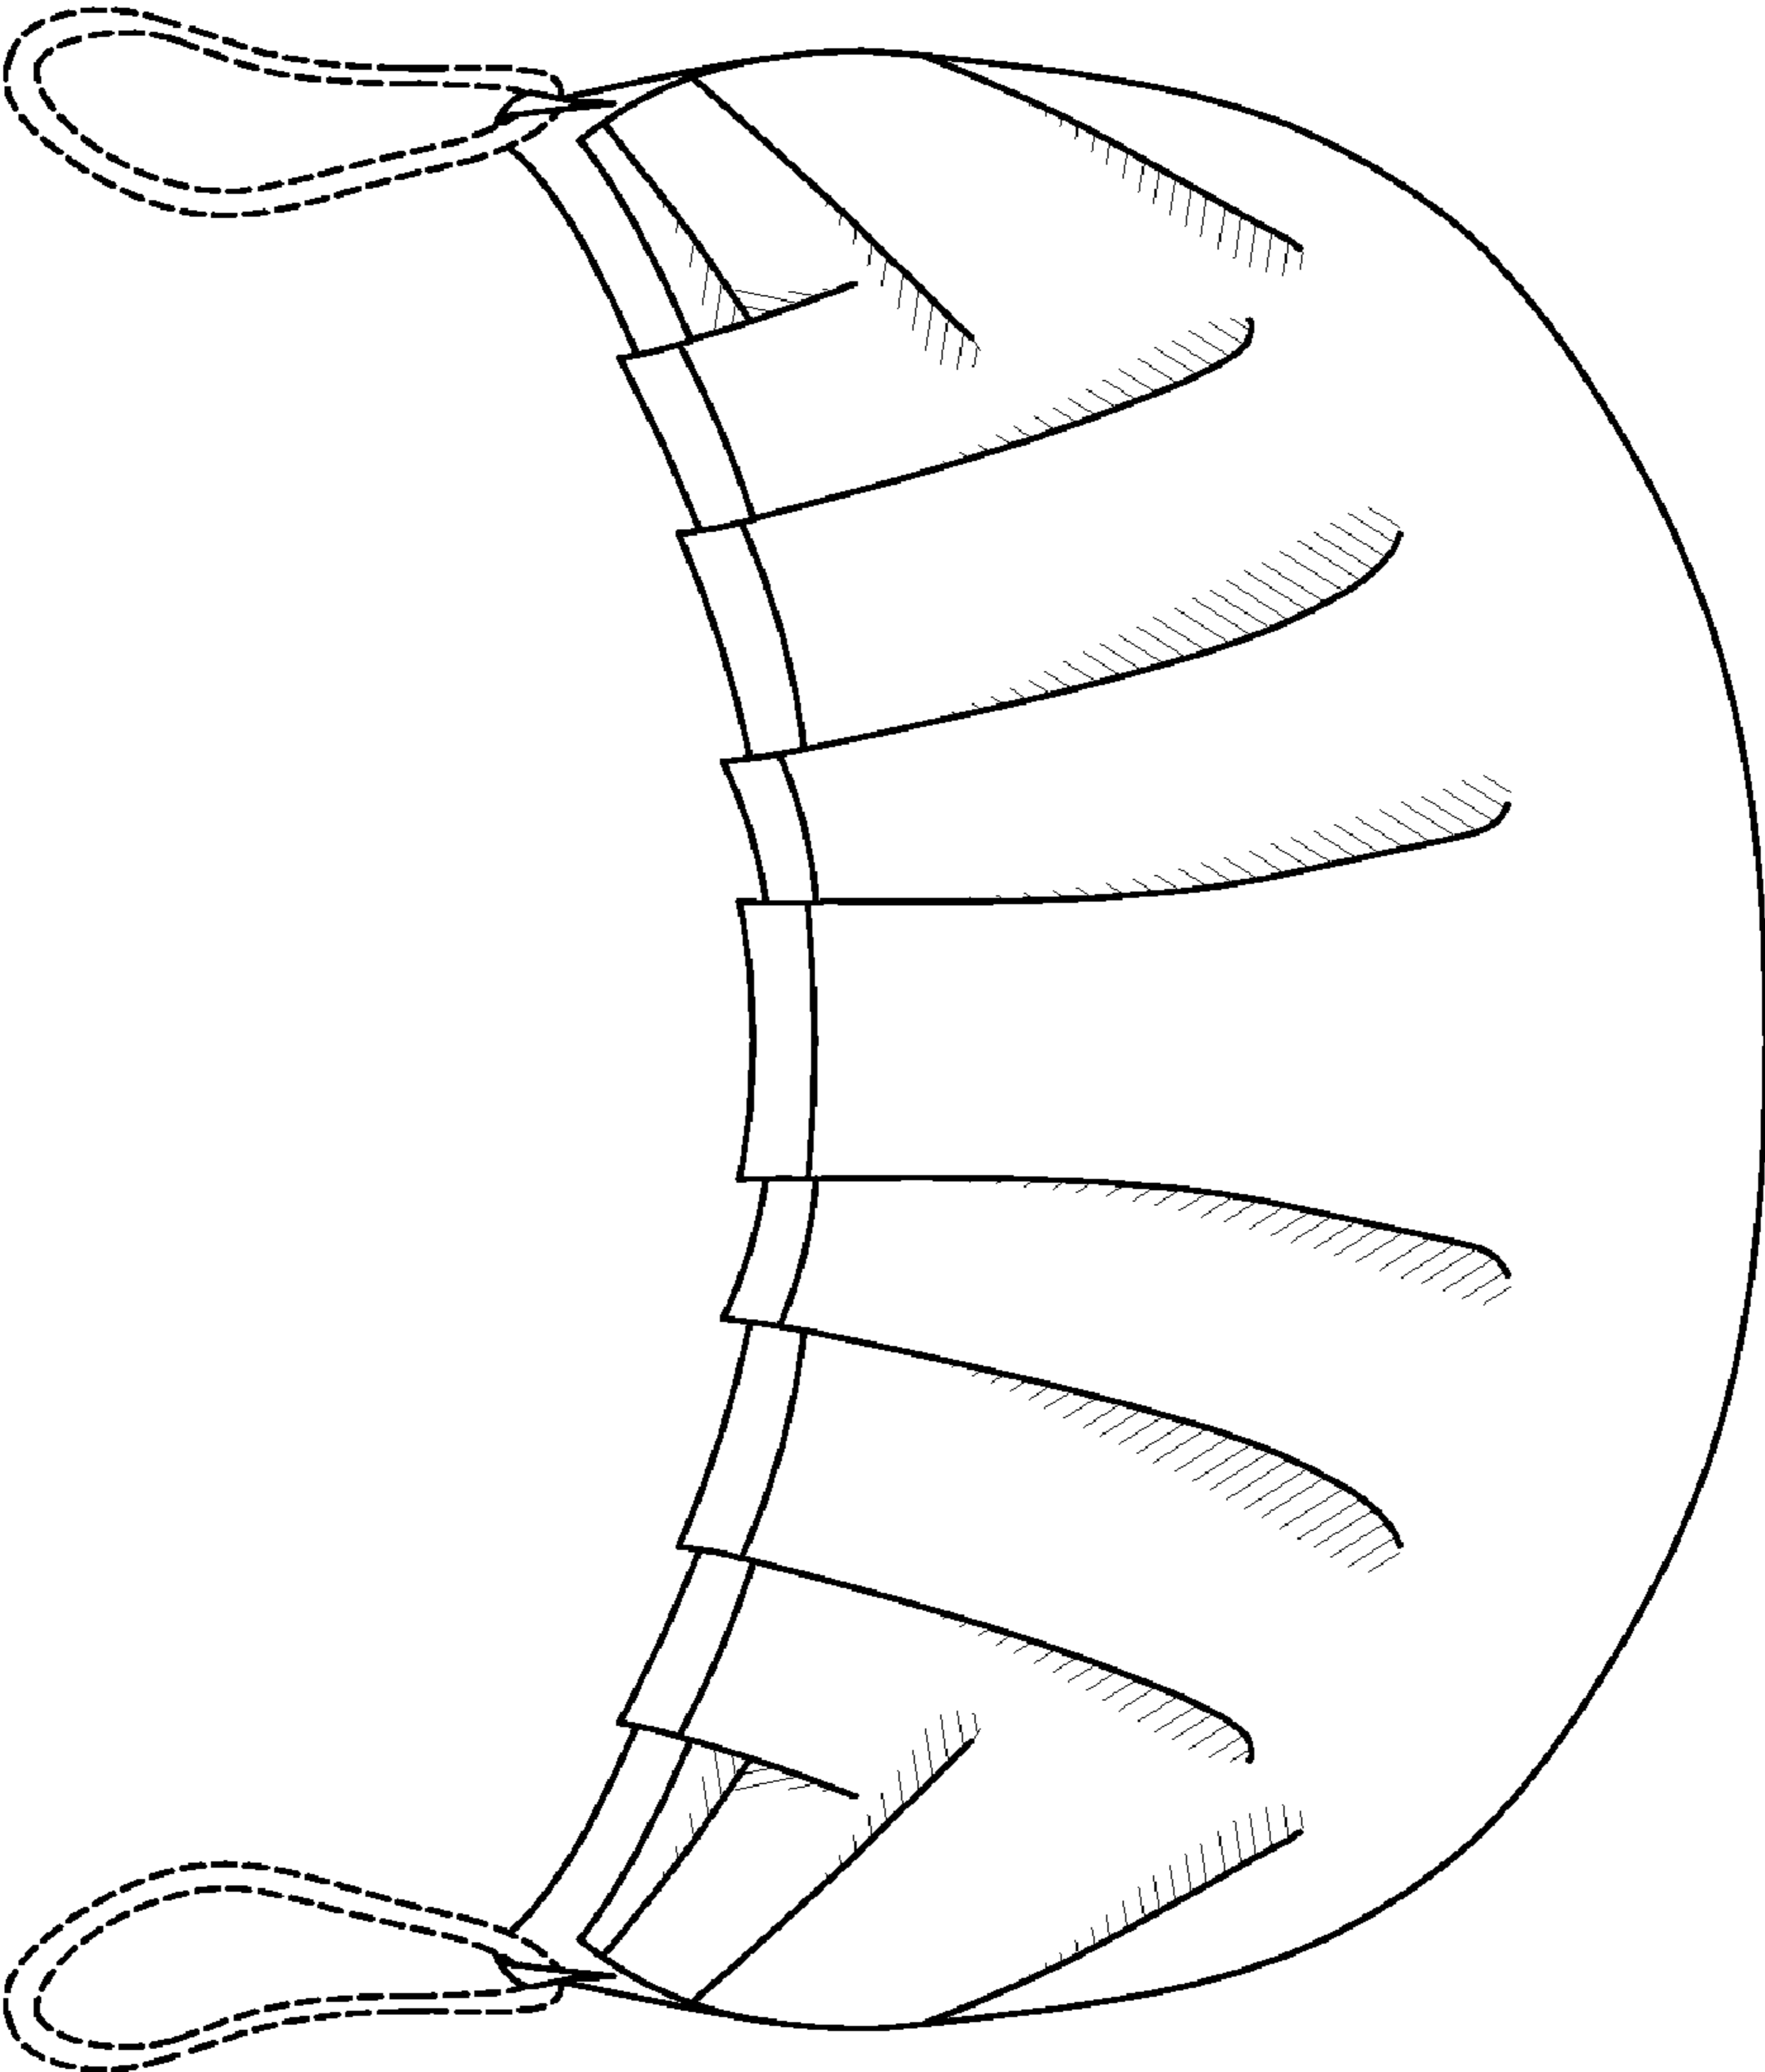


FIG. 4

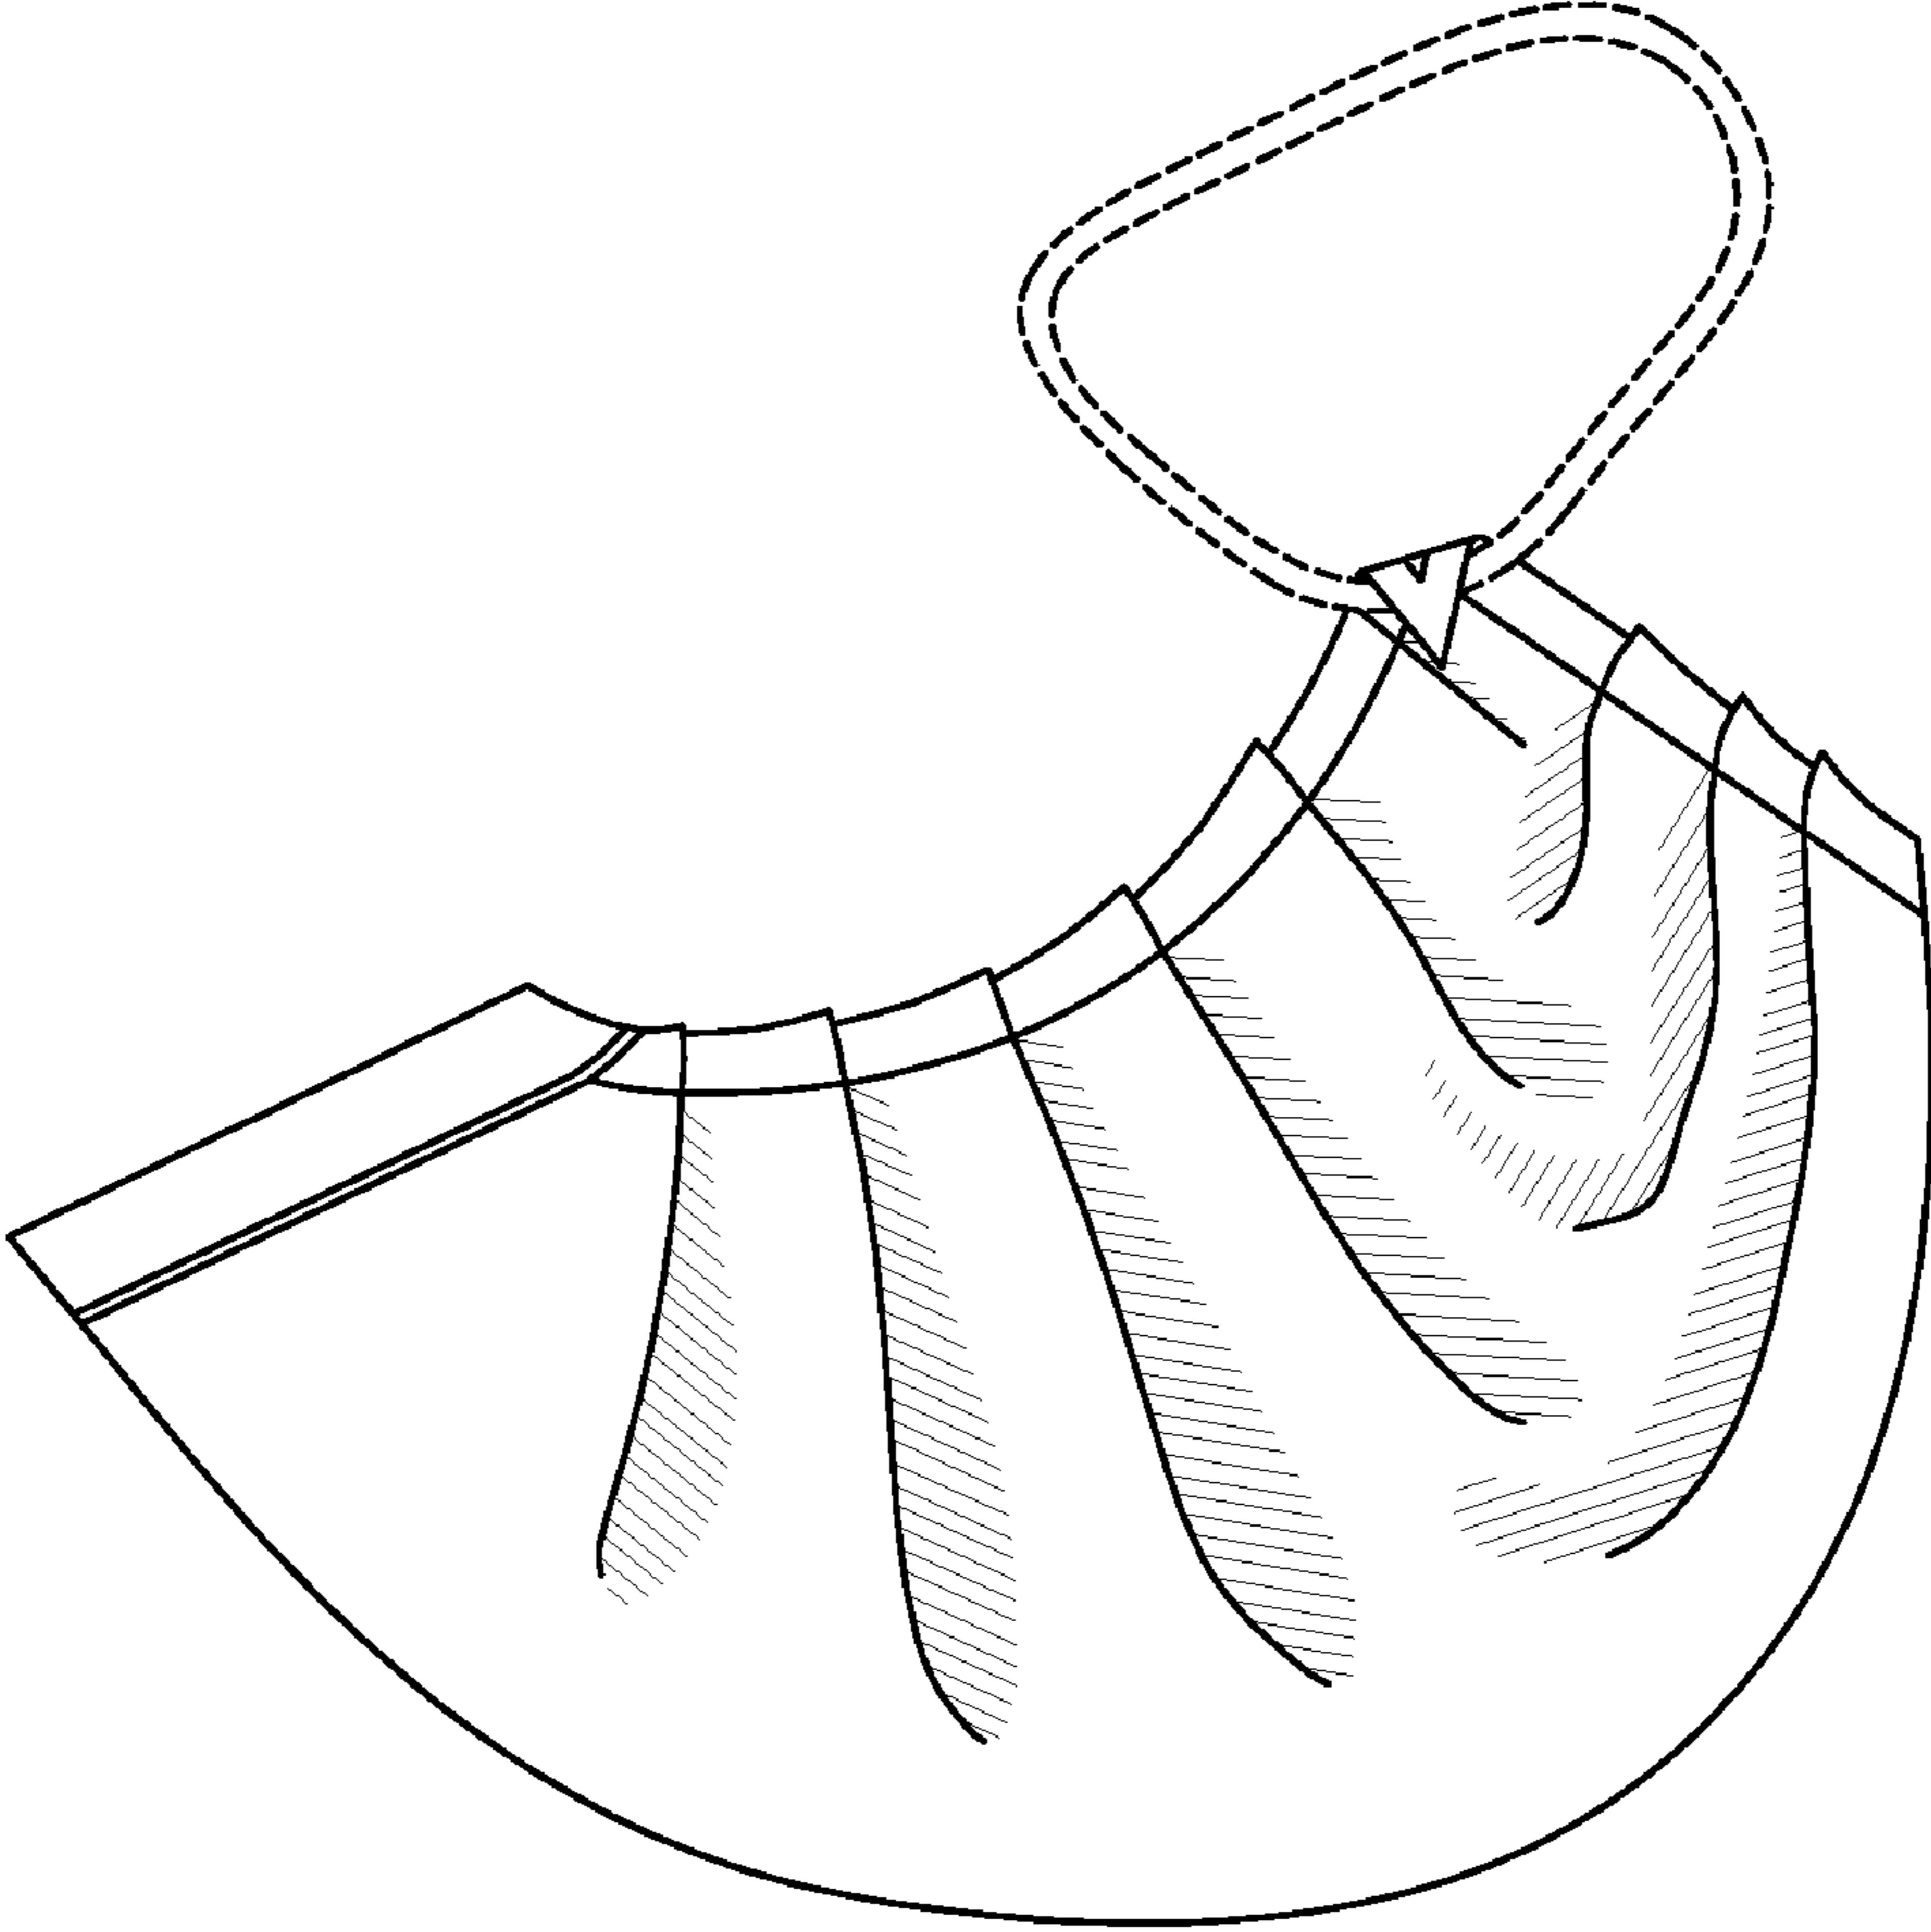


FIG. 5

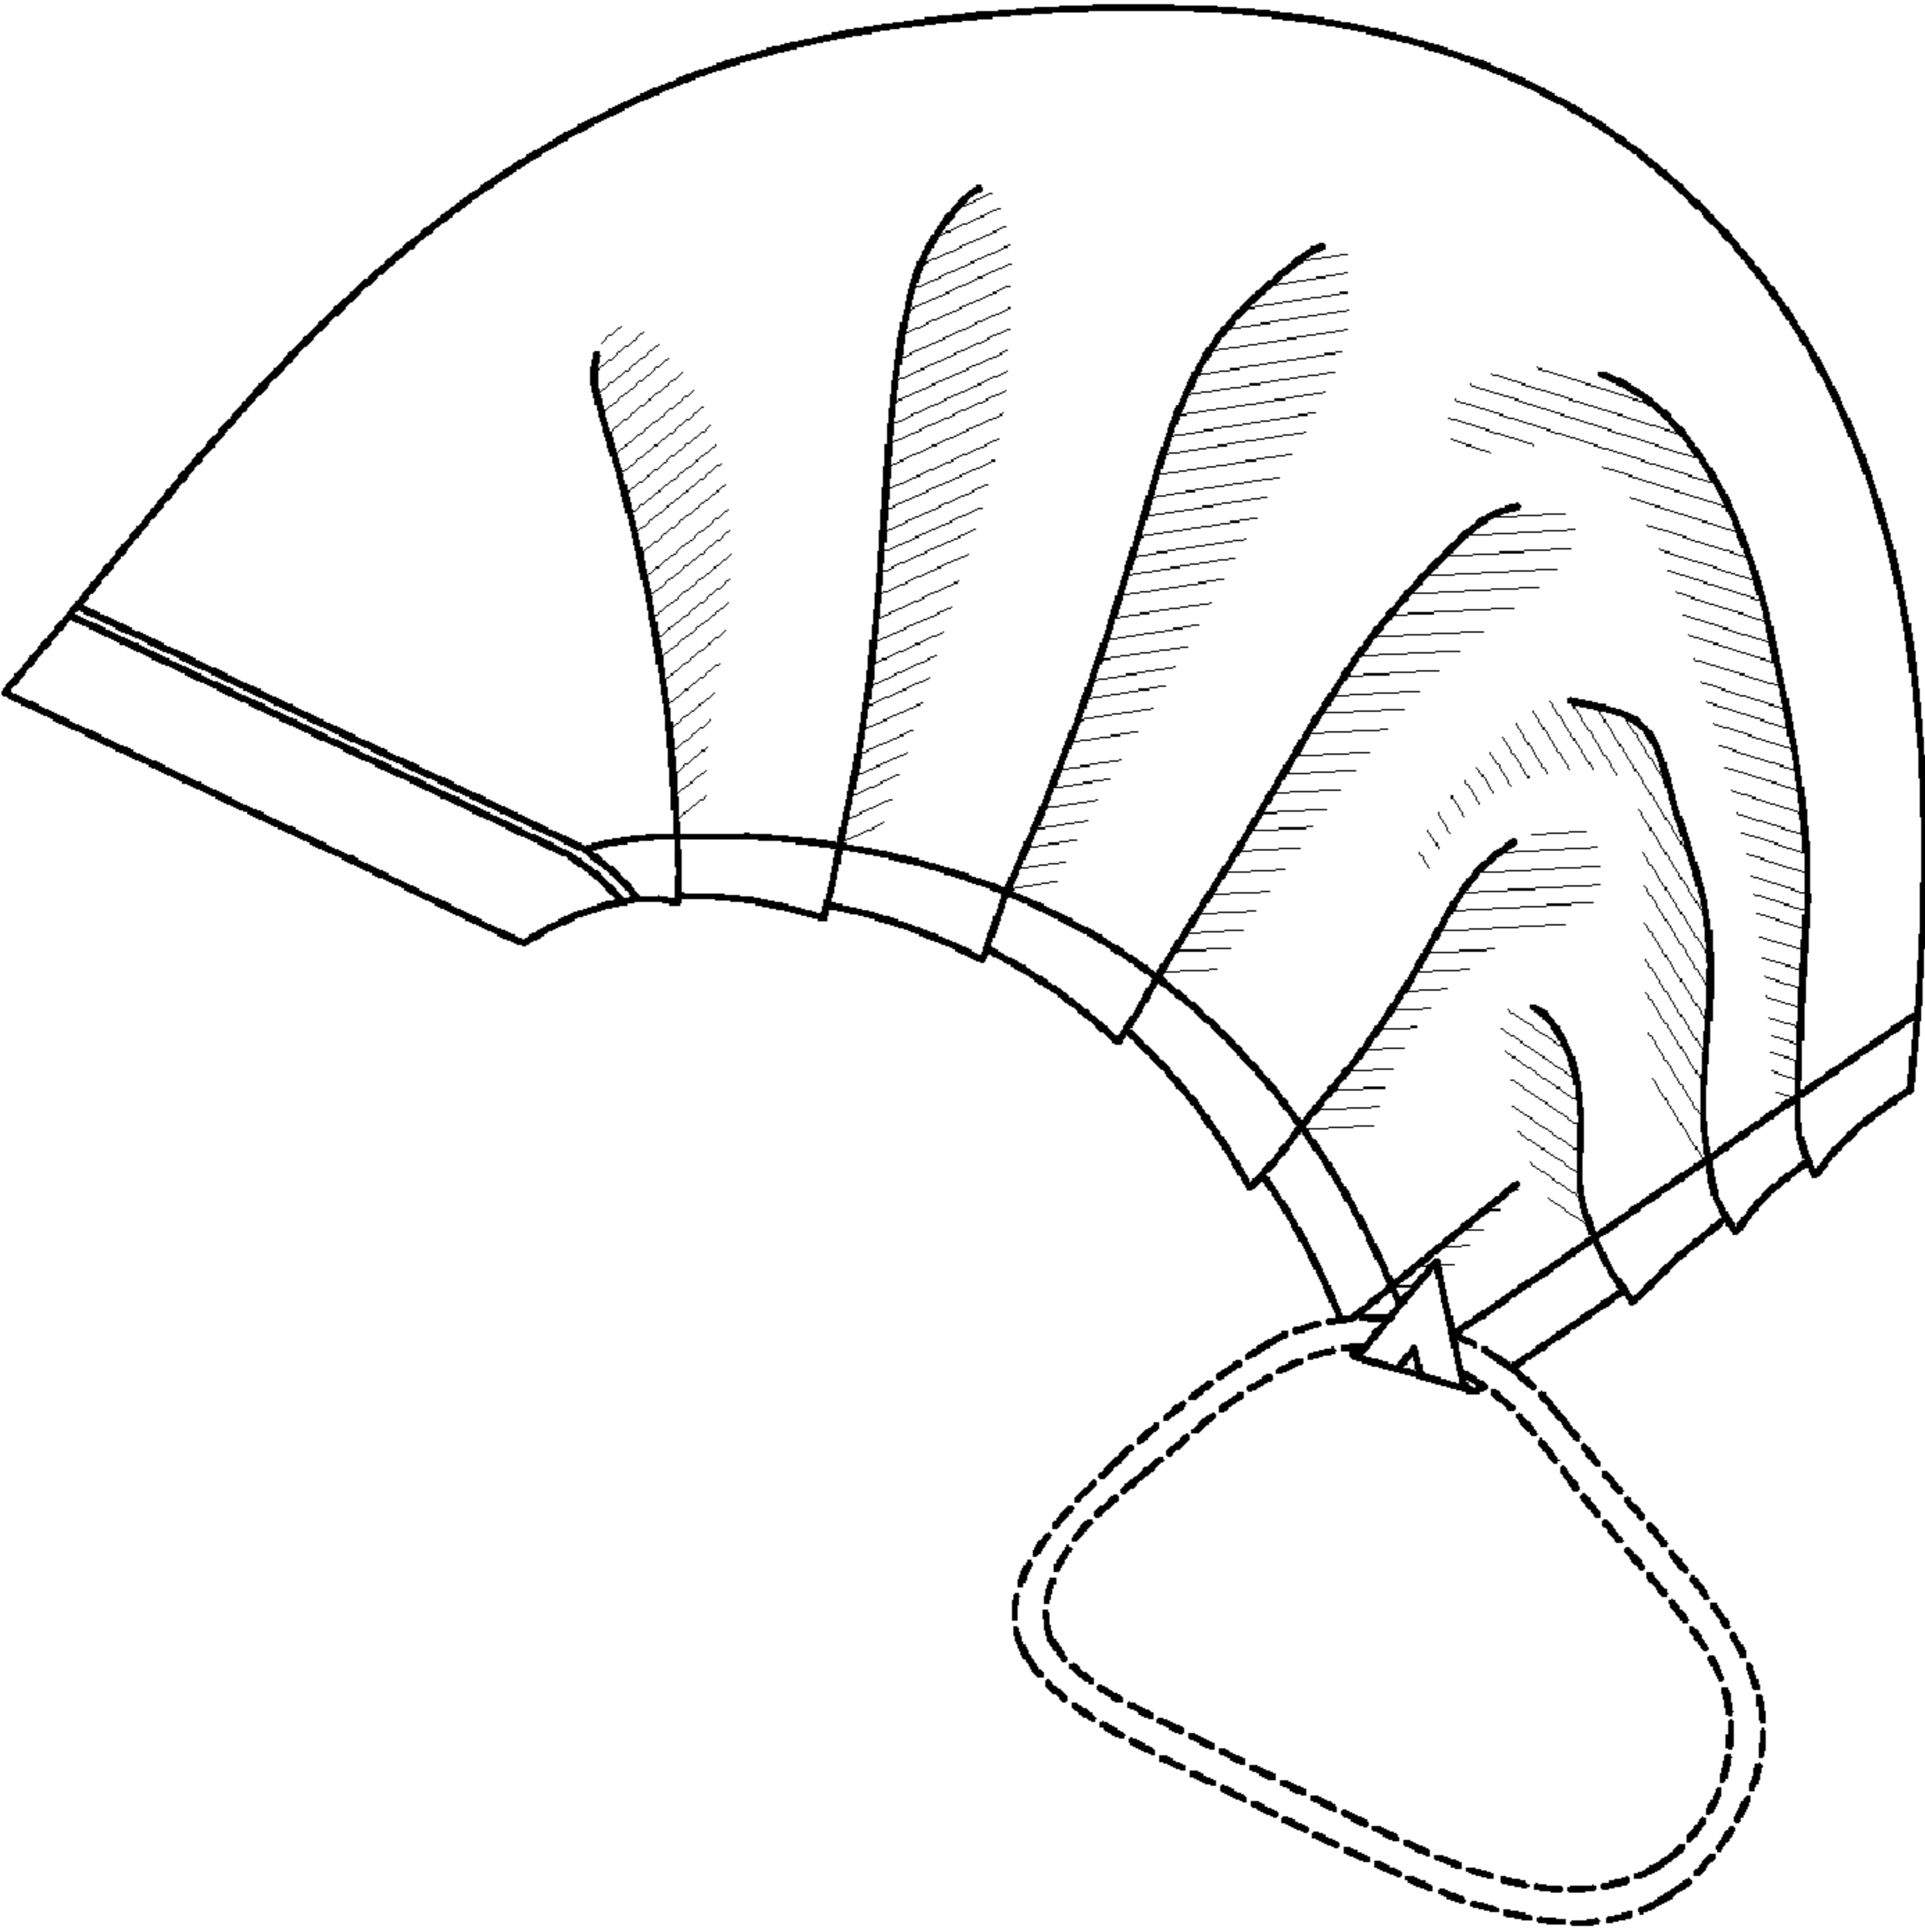


FIG. 6



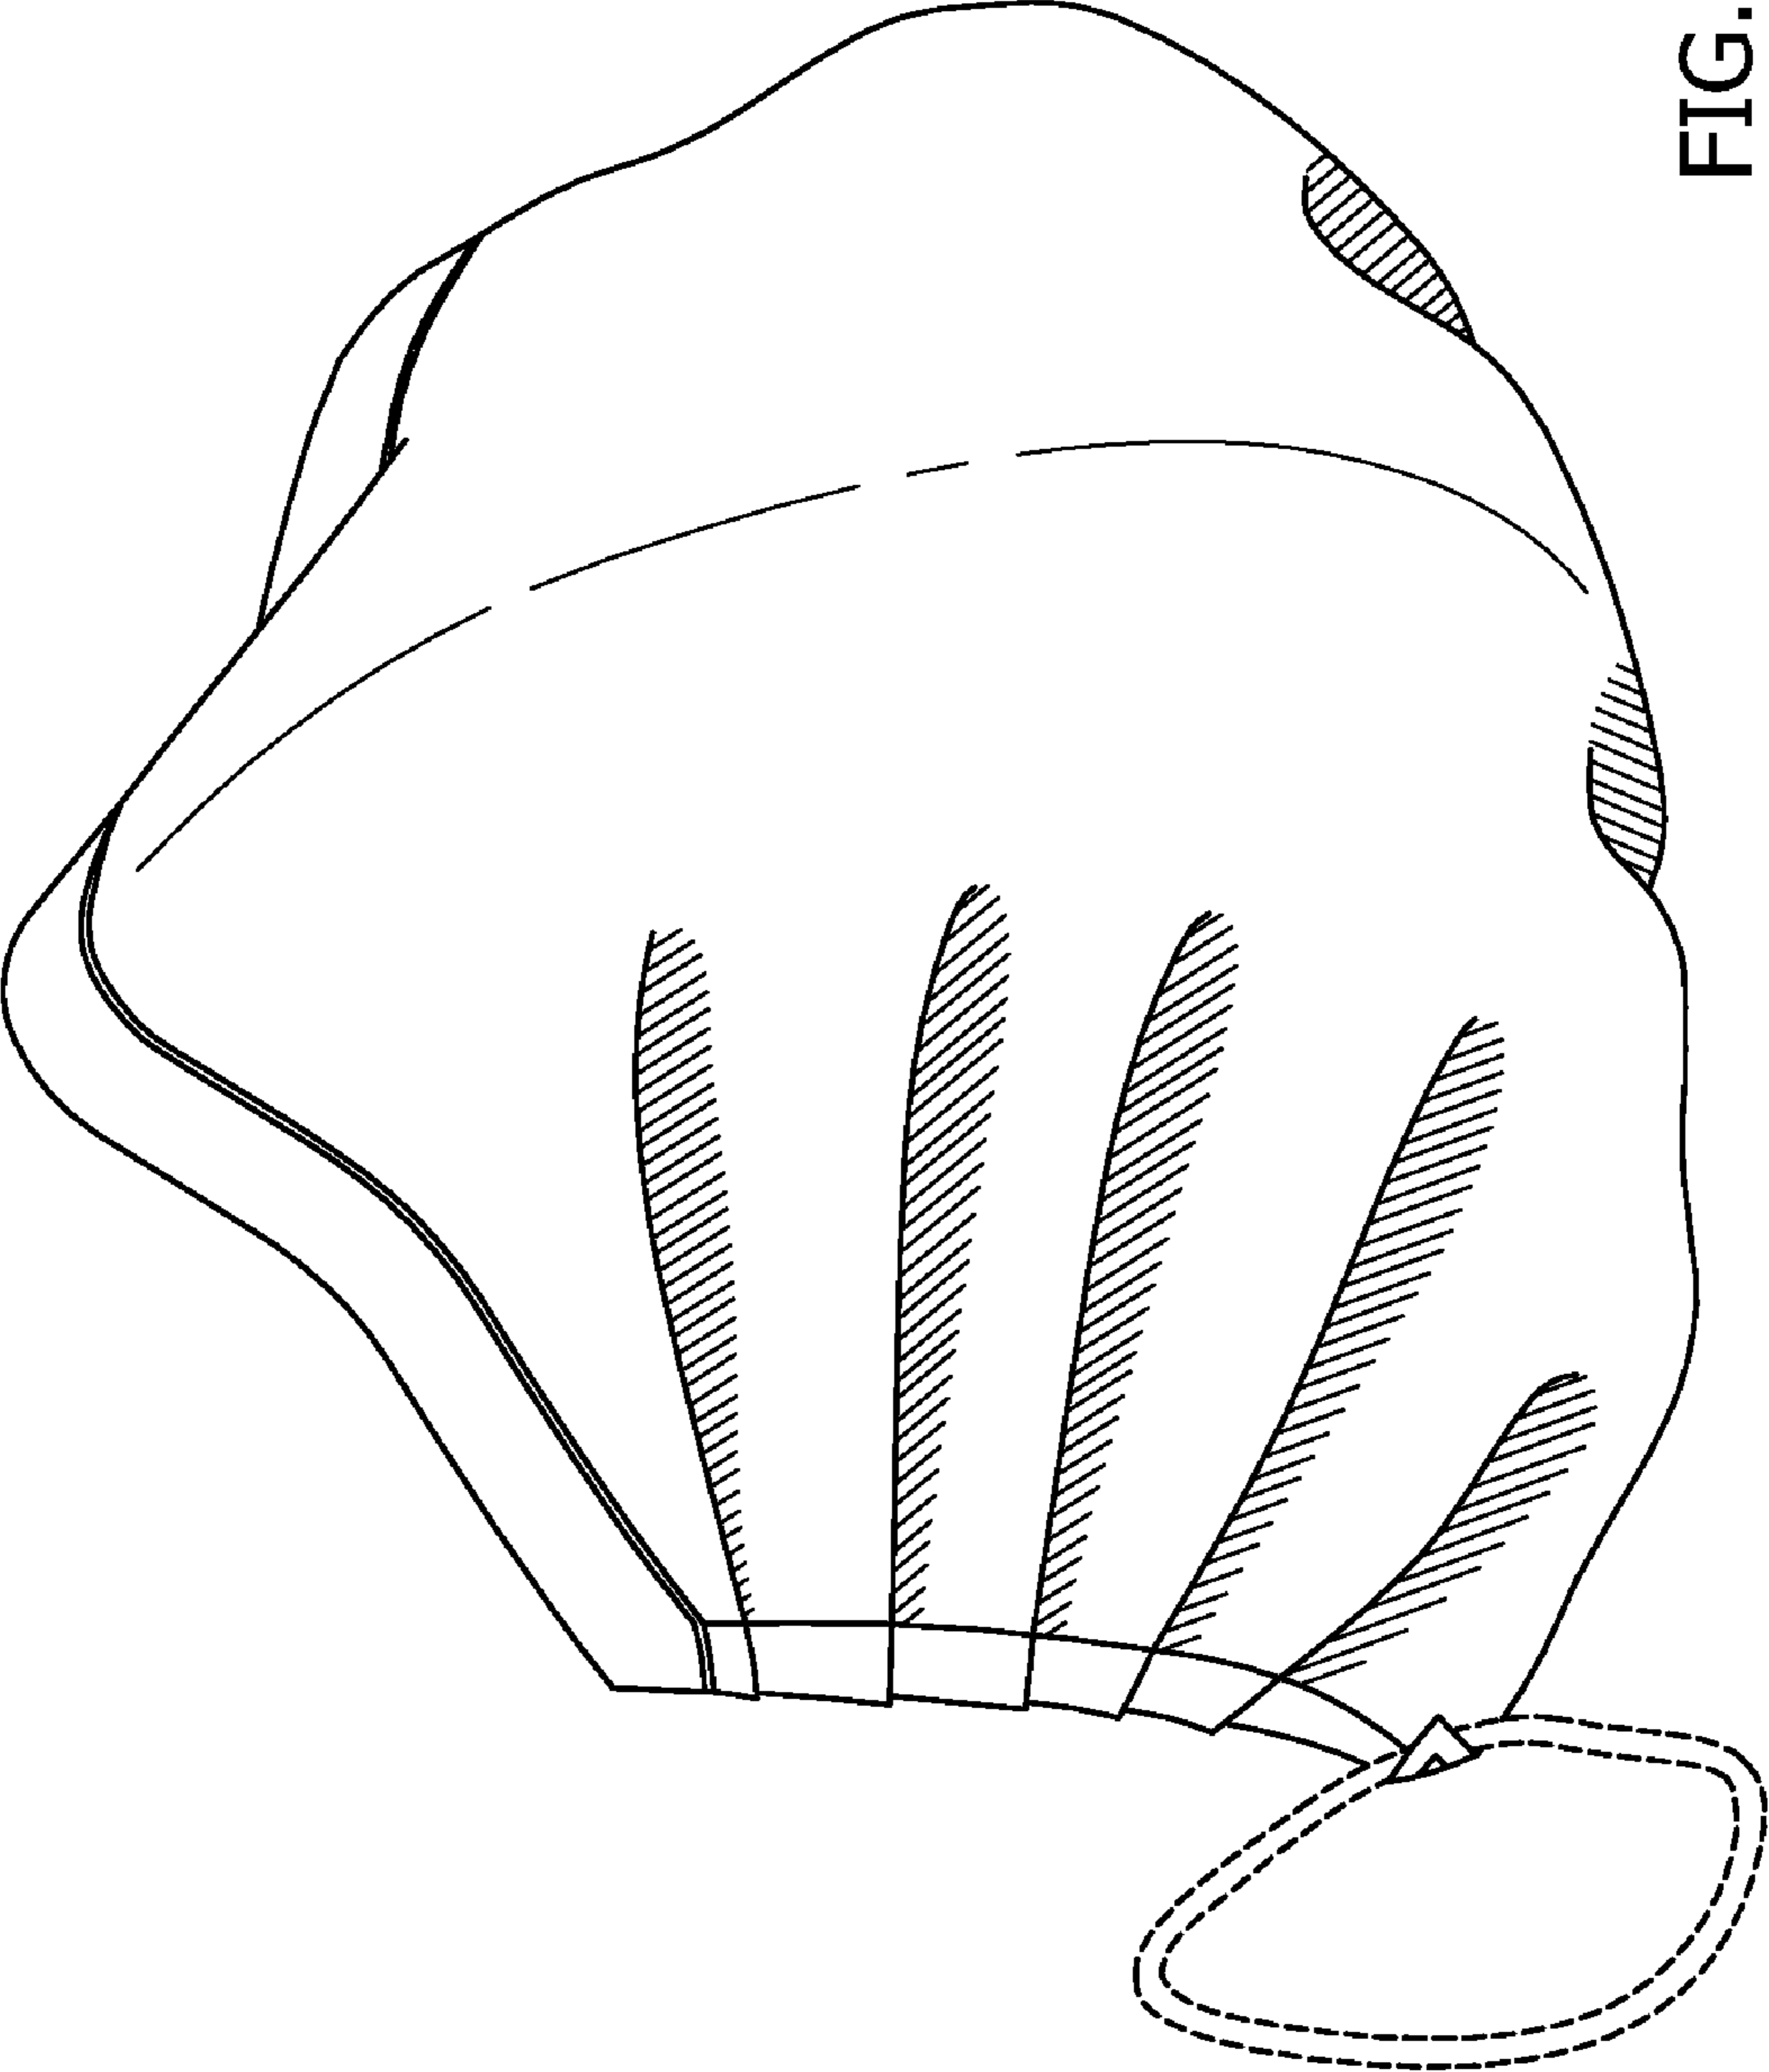


FIG. 7